



Correction: Tumor-targeting, enzyme-activated nanoparticles for simultaneous cancer diagnosis and photodynamic therapy

Huaxia Shi,^a Wucheng Sun,^a Changbing Liu,^a Guiying Gu,^b Bo Ma,^b Weili Si,^c Nina Fu,^a Qi Zhang,^{*b} Wei Huang^{*ac} and Xiaochen Dong^{*c}

Cite this: *J. Mater. Chem. B*, 2023, 11, 5922

DOI: 10.1039/d3tb90090h

rsc.li/materials-b

Correction for 'Tumor-targeting, enzyme-activated nanoparticles for simultaneous cancer diagnosis and photodynamic therapy' by Huaxia Shi *et al.*, *J. Mater. Chem. B*, 2016, 4, 113–120, <https://doi.org/10.1039/C5TB02041G>.

The authors regret that due to a figure compilation error, the representative tumor image on day 7 for the DBHA-NPs without light group was incorrect in Fig. 6b. The corrected version of Fig. 6 is provided below.

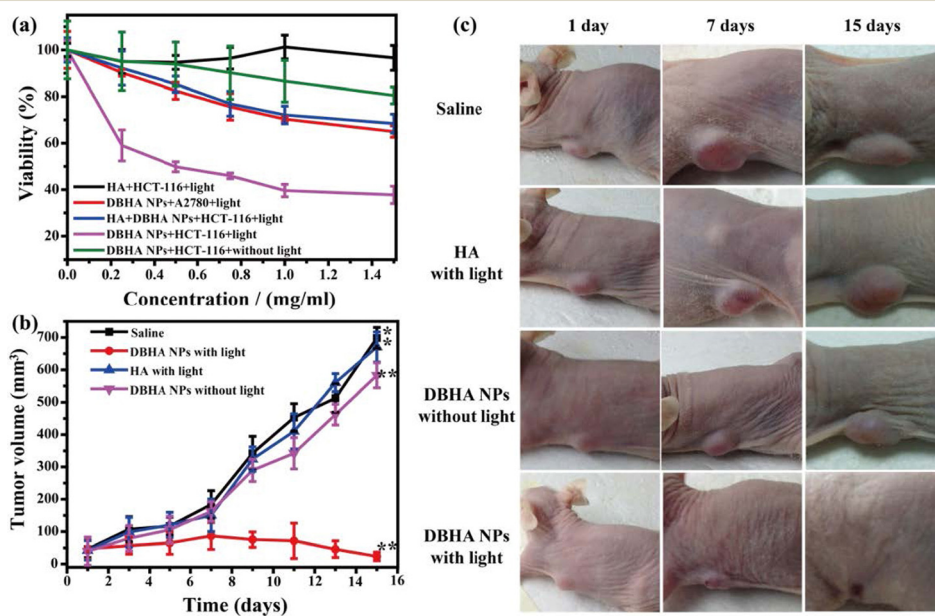


Fig. 6 (a) Comparison of cell viabilities by MTT assay ($\lambda > 600$ nm). (b) The relationship between tumor volume and treatment time for the DBHA-NPs in the HCT-116 mouse model tumor cells via tail vein injection. Twenty-four mice were randomly assigned into four groups (6 mice per group), including saline with light, HA with light, DBHA-NPs without light and DBHA-NPs with light. (c) Typical photographs of tumor-bearing mice treated at different times. Note, * $p < 0.05$, ** $p < 0.01$.

The Royal Society of Chemistry apologises for these errors and any consequent inconvenience to authors and readers.

^a Key Laboratory for Organic Electronics & Information Displays (KLOEID), Nanjing University of Posts and Telecommunications, Nanjing 210023, China

^b School of Pharmaceutical Science, Nanjing Tech University (NanjingTech), 30 South Puzhu Road, Nanjing 211816, China. E-mail: zhangqi@njtech.edu.cn

^c Key Laboratory of Flexible Electronics (KLOFE) & Institute of Advanced Materials (IAM), Jiangsu National Synergetic Innovation Center for Advanced Materials (SICAM), NanjingTech University (NanjingTech), 30 South Puzhu Road, Nanjing 211816, China. E-mail: iamxcdong@njtech.edu.cn, iamwhuang@njtech.edu.cn

