

JAAS

Accepted Manuscript



This is an *Accepted Manuscript*, which has been through the Royal Society of Chemistry peer review process and has been accepted for publication.

Accepted Manuscripts are published online shortly after acceptance, before technical editing, formatting and proof reading. Using this free service, authors can make their results available to the community, in citable form, before we publish the edited article. We will replace this *Accepted Manuscript* with the edited and formatted *Advance Article* as soon as it is available.

You can find more information about *Accepted Manuscripts* in the [Information for Authors](#).

Please note that technical editing may introduce minor changes to the text and/or graphics, which may alter content. The journal's standard [Terms & Conditions](#) and the [Ethical guidelines](#) still apply. In no event shall the Royal Society of Chemistry be held responsible for any errors or omissions in this *Accepted Manuscript* or any consequences arising from the use of any information it contains.

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

Improving Accuracy of Single particle ICPMS for Measurement of Size Distributions and Number Concentrations of Nanoparticles by Determining Analyte Partitioning During Nebulisation[†]

Jani Tuoriniemi¹, Geert Cornelis¹, Martin Hassellöv^{1,}*

¹Department of Chemistry and Molecular Biology, University of Gothenburg, SE-412 96


Gothenburg, Sweden

*CORRESPONDING AUTHOR: martin.hasselov@chem.gu.se, tel. +46-31-786 9050, fax
+46-31-77227856.

[†]Electronic supplementary information (ESI) available.

TOC entry

The analyte is redistributed between the waste and plasma flows. These analyte partitioning effects need to be corrected for to obtain the most accurate size calibration of spICPMS.

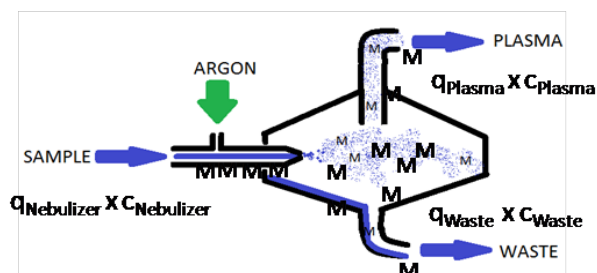

Abstract Application of single particle ICP-MS (spICPMS) for measurement of size and number concentration, c_p of nanoparticles is currently hampered by insufficient accuracy. The relative contributions of different types of noise to the overall uncertainty during spICPMS measurements of Ag and Au nanoparticle dispersions were quantified showing that the accuracy of spICPMS is mainly limited by the uncertainty in nebulization efficiency (f_{neb}). This uncertainty was improved by correcting f_{neb} for analyte partitioning effects during nebulization, and the calculated Ag and Au nanoparticle sizes were in close agreement with sizes determined by scanning electron microscopy. The duration of the particle events was measured, which allowed to correct for incomplete particle events, detector dead time, and to determine the effective dwell time for particle counting. The c_p measured with spICPMS agreed with that measured by counting particles deposited on filters, and calculated from the mass concentration of analyte.

1
2
3 **Introduction** The increased use of nanoparticles (NP) demands improved methods for their
4
5 characterization.¹ Of particular concern is the lack of validated methods for measurement of
6
7 particle number concentration, and number based size distributions in liquid samples at
8
9 relevant concentrations.² Proposed EU legislation has adopted a particle number based
10
11 definition of NPs. Enforcing regulations based on such definition would require accurate,
12
13 sensitive and rapid particle counting techniques. These methods would find use in a range of
14
15 applications such as environmental monitoring, characterization of samples for toxicological
16
17 tests, industrial quality control, and improved characterization and studies of colloid
18
19 dynamics.
20
21
22
23
24

25
26 Electron microscopy is time-consuming and is not capable of measuring particles in
27
28 dispersion. Size fractionation with *e.g.* centrifugation or field flow fraction (FFF), followed by
29
30 optical detection result in intensity weighted distributions that can be recalculated to number
31
32 based ones, provided that the particles' optical properties are known. Such approaches are
33
34 however limited to simple, and already well-characterized samples. Coupling FFF to
35
36 techniques such as ICP-MS or ICP-OES³ enables characterization of the mass as a function
37
38 of, *e.g.*, hydrodynamic diameter of target inorganic nanoparticles in complex matrices.
39
40 However, techniques for counting and sizing individual particles are required in order to also
41
42 measure the number concentration, c_p .
43
44
45
46
47

48 The need for sensitive and selective methods for characterization of environmental colloids
49
50 has led to development of single particle inductively coupled plasma mass spectrometry
51
52 (spICPMS). When a particle enters the plasma it produces a burst of ions. If the dwell time is
53
54 reduced to a level comparable to the duration of such pulses, the particle events appear as
55
56 spikes in the continuous signal. It was shown by Degueldre *et al.*⁴⁻⁸ and Laborda *et al.*⁹ that
57
58 the frequency of such spikes is proportional to the particle number concentration. The
59
60 intensities depend on the mass of analyte in the particle. If the chemical composition is

1
2
3 known, the intensities can, provided suitable calibration, be calculated to spherical volume
4 equivalent diameters. spICPMS can measure both size distributions and number
5
6 concentrations of particles at extremely low concentrations ($\sim 10^2$ particles mL⁻¹).¹⁰ Since the
7
8 technique is element-specific, particles of interest can be characterized in complex samples in
9
10 the presence of orders of magnitude higher background particle concentrations, provided
11
12 these particles consist of other elements. The measured diameters have been shown to be
13
14 comparable to those measured using differential centrifugal sedimentation (DCS) analysis
15
16 (Ag),¹¹ scanning electron microscopy (SEM) (SiO₂),¹² and nanoparticle tracking analysis
17
18 (NTA) (Ag).¹³ The number concentrations were in agreement with values calculated from
19
20 mass concentrations of Au dispersions.¹⁴ spICPMS has also potential to achieve an excellent
21
22 size resolution because the mass of particles is proportional to the cube of their diameter.
23
24
25
26
27
28
29

30 To be able to develop spICPMS into a standard technique for regulations purposes it is
31
32 necessary to identify the factors limiting its accuracy, because the particle size distributions
33
34 analysed using spICP-MS are broadened relative to distributions analyzed with other
35
36 techniques.¹⁴ Therefore it was the aim of this study to evaluate the influence of parameters
37
38 critical for both size and number concentration measurements, quantify the contributions of
39
40 different types of noise affecting the size resolution, and to provide suggestions for further
41
42 improvements.
43
44
45

46
47 One of the main factors limiting accuracy of both particle sizing and concentration
48
49 determination is the uncertainty in the nebulization efficiency (f_{neb}).¹⁰ It is the percentage of
50
51 analyte, dissolved or nanoparticulate that is injected into the plasma. More than 80 % of the
52
53 sample is redirected to waste from most conventional nebulizers, because the spray chamber
54
55 only allows the finest droplets to reach the plasma, because these can be most easily dried,
56
57 atomized and ionized. For conventional nebulizer-spraychamber systems, the only method for
58
59 measuring the f_{neb} while the plasma is ignited is the waste collection (WC) method.¹⁵ The
60

1
2
3 concentration of analyte ions in the aerosol droplets is lower in the vicinity of surfaces than in
4
5 the bulk liquid. As the sample break up into droplets of decreasing size during the
6
7 nebulization process, the smaller droplets that preferentially pass on to the plasma are formed
8
9 primarily from this analyte depleted surface layer. These aerosol ion redistribution (AIR)
10
11 effects¹⁶ cause redistribution of the analyte between the waste and plasma flows so that the
12
13 ratio of analyte to solvent in the stream going to the plasma is different than the ratio in the
14
15 sample. The laborious procedure and disappointing results with the WC method have led to
16
17 suggestions of using reference materials with known diameter, or number concentrations for
18
19 determination of f_{neb} .¹¹ There are however neither reference materials with certified particle
20
21 number concentrations nor validated methods for accurately measuring number
22
23 concentrations for NPs. The use of reference materials with certified diameters adds cost and
24
25 does not further the development of spICPMS into an independent method. In addition, any
26
27 uncertainty in diameter is propagated cubed to the f_{neb} . For instance the ~ 5 % discrepancies
28
29 among certified diameters for the NIST 60 nm Au particles would result in ~ 15 %
30
31 uncertainty in f_{neb} .¹¹ It has also not been verified that nebulization efficiency is independent of
32
33 the size and concentration of the reference nanoparticles. Validation and even modest
34
35 improvements to f_{neb} determination methods are therefore likely to render spICPMS as
36
37 accurate as many established particle sizing techniques.
38
39
40
41
42
43
44
45

46
47 In this article, methods to improve the accuracy of size distribution determinations using
48
49 spICPMS or at least an alternative to presently used methods are presented. First, the
50
51 magnitude of partitioning effects for the WC method are estimated by including dissolved In,
52
53 and Au standards during waste collection. Correcting for dissolved analyte partitioning allows
54
55 determining an analyte based f_{neb} ¹⁵ that takes AIR effects into account. The duration of
56
57 particle events was measured using ultrafast acquisition times of 0.1 ms. It allowed estimation
58
59 of the role of error sources such as incomplete measurement time and dead time error¹² at
60

1
2
3 higher acquisition times by computing the fraction of ions that are detected in each situation.
4
5 Acquisition time is in this article referred to as dwell time (t_{dwell}). The levels of different types
6
7 of noise in the particle signals are evaluated to estimate the resolution in particle sizes. The
8
9 effective dwell time for particle counting is determined, and the combined effects of counting
10
11 statistics, variation in particle flux, and uncertainty in f_{neb} for the accuracy of particle number
12
13 concentration determination are discussed. The spICPMS c_p of Au colloids were compared
14
15 with results obtained by counting particles on filters to assess the accuracy of particle number
16
17 determination, and calculating it from the mass concentration and diameter. A list of symbols
18
19 used in this article is found in table 1.
20
21
22
23
24

25 **Experimental**

26 **Methods**

27
28
29 **Chemicals** The citrate coated silver nanoparticles (AgNP) had a nominal diameter of 80 nm,
30
31 and the also citrate stabilized gold nanoparticles (AuNP) were nominally 50, 100, and 250 nm
32
33 (British biocell international, UK). Ultrapure water (Millipore MilliQ) was used as dilution
34
35 media for all samples. Dissolved Ag, Au, and In standards were diluted from 1 gL⁻¹ 2% HNO₃
36
37 solutions provided by Ultra Scientific in ultrapure water.
38
39
40
41
42
43
44

45 **spICPMS** A Thermo Element2 sector field ICP-MS was used in all experiments. The method,
46
47 particle detection algorithm, and data acquisition of the used instrument are discussed in an
48
49 earlier publication.¹⁰ Data acquisition with 0.1 ms time resolution was achieved for the 80 nm
50
51 Ag particles by using the following settings in the method file of the instrument software:
52
53 Resolution: *low*, Samples per peak: *1000*, Integration window: *10*. As the instruments scans
54
55 through the mass range set in the integration window, 100 consecutive dwells having 0.1 ms
56
57 t_{dwell} are acquired without any time gap between them. The instrument parameters given in
58
59 table 2 were optimized using dissolved In standards.
60

Determination of nebulization efficiency and calibrating for particle mass The nebulization efficiency was measured with 7 (Ag), and 8 (Au) replicates using the waste collection method.^{15,10} Spray chamber waste flow (q_{waste}) was collected and weighted while the flow into the nebulizer ($q_{nebulizer}$) was monitored using a flow meter (Glass Expansion ``truflow``). The waste flow was driven by a peristaltic pump (Perimax 12). To investigate and correct for analyte partitioning between plasma and waste flows in the spray chamber, In ($1\mu\text{g L}^{-1}$) and Au ($10\mu\text{g L}^{-1}$) was added to the sample flow and its concentration was measured both in the collected waste (c_{waste}), and inflow to the nebulizer ($c_{nebulizer}$). The In concentration that effectively reaches the plasma (c_{plasma}) can be calculated from the mass-balance:

$$q_{plasma}c_{plasma} + q_{waste}c_{waste} = q_{nebulizer}c_{nebulizer} \quad (1)$$

The analyte-based nebulization efficiency f_{neb} then equals $c_{plasma} \times q_{plasma} / (c_{nebulizer} \times q_{nebulizer})^{-1}$, whereas the more commonly used sample mass-based nebulization efficiency equals $q_{plasma}/q_{nebulizer}$. Note that in order to be able to calculate the analyte based f_{neb} it is enough to measure the ratio of the ICPMS signal intensities in the sample and collected waste. To calibrate for mass 0, 4, and 6 $\mu\text{g L}^{-1}$ dissolved Ag standards and 1, 5, and 10 $\mu\text{g L}^{-1}$ Au were measured using a dwell time of 10 ms.

Measurement of particle size distribution and concentration The AgNP stock dispersion was initially diluted 10^5 times using ultrapure water, and then further to a 10^7 times dilution in 20 replicates for size distribution and number concentration measurements. 10 000 consequent analyses (dwells) with a 10 ms t_{dwell} were measured on each replicate to obtain a total number of dwells (D) of 200 000, and to count 986 particle events. The Au particles were measured at 10^6 (50 nm), 10^5 (100 nm), and 10^4 (250 nm) times dilution and the number of particle events counted, N were 1250, 485, and 133 respectively. The total Au

1
2
3 concentrations in NP suspensions were measured in three replicates after digestion with *aqua*
4
5 *regia*. To determine the effective dwell time and quantify bias due to incomplete particle
6
7 events, the AgNP containing samples were diluted $1-2 \times 10^6$ times and were then measured
8
9 using varying dwell times between 2 ms and 6 ms. In these experiments more than 500
10
11 particle events were counted for each dwell time.
12
13

14
15
16 To reduce the number of false positives, *i.e.* measurements of dissolved ions only that are
17
18 recognized as particles, to a negligible level an iterative algorithm with an 8σ detection limit¹⁰
19
20 was used for discriminating between particle events and the dissolved background. The mean
21
22 value of the background signal was subtracted from the particle event signals. The signal
23
24 intensity (I_{part} , ion counts) of a frequency-intensity diagram with bin width of 50 counts was
25
26 recalculated to diameter, and the frequency (F, ND^{-1}) of the signals within each bin was
27
28 recalculated to c_p using the formulas below.
29
30
31

$$32 \quad d = [6(I_{part} - r)(\pi \rho s)^{-1}]^{1/3} \quad c_p = F(f_{neb} t_{dwell} q_{nebulizer})^{-1} \quad (2)$$

33
34
35 r (ion counts) is the recipient on the intensity axis of the calibration curve, ρ is the density of
36
37 the NP material, s is the sensitivity or slope of the calibration curve (ion counts g^{-1}).
38
39
40
41

42
43 **Deposition of particles on filters** The number concentrations of AuNP dispersions were
44
45 measured by depositing the particles in a volume of dispersion on filters, and then using SEM
46
47 to determine their surface concentration (particles m^{-2}). Knowing the total area of the filter
48
49 that was exposed to the dispersion and the area that was imaged using SEM allowed
50
51 calculation of the c_p (particles mL^{-1}) in the liquid sample. The Au colloids were diluted to
52
53 4×10^6 particles mL^{-1} , 9×10^7 particles mL^{-1} , and 6×10^9 particles mL^{-1} for the 250, 100, and 50
54
55 nm particles respectively. The filters were placed on glass frit supports giving an effective
56
57 filtration area of 9.6 cm^2 , and 10 mL of the dispersions were forced through by vacuum
58
59 suction. The filters used for the 250 nm AuNP were the 100 nm nominal cut off cellulose
60

1
2
3 ester membranes from Millipore, while Corning 50 nm nominal cut off nuclepore track etched
4
5 polycarbonate filters were used for the 100 and 50 nm samples. The experiments were
6
7 performed in three replicates. The efficiency of retaining the particles was assessed by
8
9 measuring total Au concentrations in the filtrate.
10
11

12
13 **SEM** A droplet of undiluted Ag colloid was placed on a silicon wafer, spread on the surface
14
15 and left to dry in air. The sample preparation was done the same day as the spICPMS
16
17 measurements. Secondary electron images with 40 000 – 50 000 times magnification were
18
19 acquired with FEI quanta 200 FEG variable pressure SEM using 20 kV acceleration voltage.
20
21 The Au particles were analyzed on the filters. A few small pieces were cut from each filter
22
23 and placed on SEM stubs. Several backscattered electron images were taken at random
24
25 locations on each piece, using again 20 kV acceleration voltage. The number of AuNP was
26
27 counted in each image and the surface concentration was obtained by dividing with the
28
29 imaged area. The instrument was operated in the high vacuum mode for Ag, while the non
30
31 conducting filter substrates necessitated the use of low vacuum (~ 0.6 Torr) for imaging the
32
33 Au particles.
34
35
36
37
38
39

40
41 For determining the surface concentration of AuNP, at least 700 particles were counted for
42
43 each replicate. The magnifications were 3000 – 5000 times for the 100 and 250 nm AuNP,
44
45 and around 20000 times for the 50 nm AuNP, except for some images used for counting only
46
47 where ~ 8000 times magnification was sufficient. Images of the AuNP are shown in ESI-1.
48
49

50
51 Projected area diameters of 616 Ag particles were determined by fitting the particles with
52
53 ellipses in the imageJ (National institute of health, <http://imagej.nih.gov/ij>) software. The
54
55 automatic particle identification and sizing routine of the software was used to measure
56
57 projected area diameters of 518, (50 nm), 531 (100 nm), 837 (250 nm) Au particles.
58
59
60

Results and discussion

1
2
3 **Calibration for mass** Uncertainties on numbers given are always 95% confidence intervals
4 of the mean calculated from replicate measurements, unless stated otherwise. When
5 measuring the Ag particles the f_{neb} based on sample mass was 6.7 ± 2.2 %. The In
6 concentration ratio between nebulizer ($c_{nebulizer}$) and waste flows (c_{waste}) was 0.76 ± 0.14 ,
7 resulting in an analyte-based f_{neb} of 4.7 ± 1.8 %. The Au particles were measured in a second
8 session where the ratio of Au concentration between nebulizer and waste flows were
9 0.53 ± 0.05 and the mass and analyte based f_{neb} were 8.7 ± 0.49 %, and 4.7 ± 0.26 % respectively.
10 Dissolved analyte thus appear to partition preferentially to the waste. The AIR effects are not
11 necessarily the same for NP as for dissolved analytes, but previous studies¹⁷⁻¹⁸ found no
12 significant differences when quantifying the total mass of NP with or without prior digestion.
13 This suggests that dissolved analytes and NP similarly pass the sample introduction system.
14 The nebulization efficiencies and size calibration parameters are listed in table 3.

15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32 **Measurement of ion burst duration** Data acquisition with 0.1 ms time resolution enabled to
33 measure the durations of 16 particle events of 80 nm Ag (Fig. 1). The ion bursts appear to be
34 Gaussian distributed as a function of time, with an average time-dependent standard
35 deviation, σ_b of 0.08 ± 0.01 ms, but in many cases a tail could be observed because the cloud
36 of ions expands while they are extracted through the sampler cone.¹⁹ As 99.7% of the ions
37 arrive within $3\sigma_b$ of the peak of the ion plume, $6\sigma_b$ can be used as a measure of the duration, t_b
38 from the beginning to the end of the ion burst which is 0.48 ± 0.06 ms. The duration of such ion
39 plumes seems not to be dramatically different for varying materials and spectrometers, as in
40 previous studies the t_b of ion bursts due to SiO₂ particles¹² were ~ 0.20 - 0.4 ms, while droplets
41 containing dissolved analyte²⁰ gave bursts lasting between ~ 0.3 and 0.5 ms for the 20
42 different isotopes investigated, with a t_b of ~ 0.45 for silver.

43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60 **SEM and spICPMS size distributions** The majority of the Ag, and 50 nm Au particles were
spheroidal (Fig. 2) with occasional rod- or triangular-shaped particles. The particles were

1
2
3 fitted with ellipses in order to calculate their projected area diameters. The average ratio of the
4 major and minor axis of the particles was 1.29, and 2.08 respectively, wherefore the projected
5 area and volume equivalent diameters are not necessarily equal. The imaged AgNP were
6
7
8 mostly part of aggregates. Care was taken to not measure particles that were obscured by their
9
10
11 neighbors, since their diameters would appear smaller than their actual values. The spICPMS
12
13 size detection limit, DL_s is the smallest ion burst that is distinguished as a particle event. The
14
15 DL_s were 52, and 35 ion counts for the Ag and Au particles, which correspond to diameters of
16
17
18 ~ 24 and 19 nm respectively. The DL_s for Ag is similar to that calculated in a previous
19
20
21 publication.¹⁰ The mean particle signals, I_{part} were 597, and 2017 ion counts for the Ag and
22
23
24 Au particles respectively. The SEM and spICPMS size distributions are shown in Fig.3. For
25
26
27 the AuNP, the spICPMS diameter obtained using analyte-based f_{neb} (61.06 nm) nearly
28
29
30 coincided with the SEM diameter (63.48 nm), while the diameter seems to be overestimated
31
32 using the mass-based f_{neb} (76.16 nm). For AgNP, the differences in diameters obtained by
33
34
35 spICPMS using the analyte-based f_{neb} (56.24 nm), or the sample mass-based f_{neb} (60.74 nm)
36
37
38 are smaller, and they are both in relatively close agreement with that calculated using SEM
39
40
41 data, (61.99 nm). The accuracy of these size distributions are discussed further below. Note
42
43
44 that the SEM size distribution of AuNP appears to be wider than that measured by spICPMS
45
46
47 which is probably because of varying orientation of these asymmetric particles on the filter
48
49
50 surface.

Accuracy of particle sizing A statistically significant number of particles were examined
51
52 both with SEM, and spICPMS. The size distributions of the Au and Ag particles are by a
53
54 good approximation Gaussian (r^2 of Gaussian fit is 0.96 and 0.95 for the Au and Ag particles
55
56 respectively.). Therefore the uncertainty (95 % confidence interval) due to finite particle
57
58 count can be approximated by $\pm 1.96 * e_{std}$, where e_{std} is the standard error of the mean
59
60 diameter; $e_{std} = \sigma_{Size\ distribution} / (N)^{0.5}$. This uncertainty for spICPMS diameters (analyte-based

1
2
3 f_{neb}) were 0.32 nm and 0.57 nm for Ag and Au particles respectively, while it was 0.39 nm,
4
5 and 1.54 nm for SEM.
6
7

8
9 The dwell time is one of the most important parameters in spICPMS. The intensity of a
10 dissolved signal per dwell decreases when using a shorter t_{dwell} , but particle event intensities
11 do not decrease. Decreasing the t_{dwell} thus increases the ratio between signals due to particles
12 and dissolved analytes, allowing smaller particles to be detected. At the same time, the
13 probability that a particle event does not completely coincide with t_{dwell} increases. The
14 incompletely measured particle events broaden the distribution of particle signals and cause
15 bias towards smaller particle sizes. However, when t_b is known, this error can be corrected
16 for.
17
18
19
20
21
22
23
24
25
26

27
28 An average $t_b = 0.48$ ms was in this study obtained for 80 nm AgNP (Figure 1). The fraction
29 of the ions from a particle event that is detected on average, f_d and the coefficient of variation
30 for the spread in signal, $cv_{incomplete}$ is calculated as a function of dwell time in Fig. 4. It was
31 assumed that the spread and bias are proportional to the signal intensity. The calculations
32 were performed numerically by integrating the signal in a Gaussian having the same I_{part} , and
33 t_b as obtained here in a moving window of width t_{dwell} . The distribution of signal intensities
34 was obtained by sliding the window across the ion burst in steps of 0.001 ms. Such
35 distributions were calculated both without assuming any detection threshold, and setting the
36 DL_s to the values observed here. Experimental values are shown for a few different values of
37 t_{dwell} . For this data, the f_d for 10 ms was assumed to be what was calculated, and f_d for shorter
38 dwell times, $t_{dwell} = x$ ms was calculated from $I_{part\ 10ms}/I_{part\ x\ ms} = f_{d\ 10\ ms}/f_{d\ x\ ms}$. In the case of
39 $DL_s = 0$, and $t_{dwell} > t_b$ the f_d is given by (Derivation in ESI-2):
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57

$$58 \quad f_d = \frac{t_{dwell}}{t_{dwell} + t_b} \quad (3)$$

59
60

1
2
3 Eqn.3 is plotted in Fig.4. It agrees with the results obtained by numerical calculations for the
4 case $DL_s = 0$. Fig.4 shows that f_d increases as t_{dwell} increases, because the change that the ion
5 burst occurs completely within dwell increases. Eqn.3 can be used to correct for incomplete
6 particle events, but as is evident in Fig.4, the bias is seemingly reduced with increasing DL_s as
7 a larger fraction of the produced ions needs to be detected to exceed the detection limit, and a
8 part of the incomplete particle events are thus not detected. Eqn. 3 under estimates f_d because
9 the particle signals always need to exceed DL_s . However, the deviation from true values will
10 be small for particle signals considerably higher than the DL_s . Because the variation in burst
11 duration is small between different types of ions the calculations for Ag presented in Fig 4 are
12 useful for estimating the bias for other analytes as well.
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27

28 The incomplete particle events reduce the apparent particle mass of the Ag particles on
29 average approximately ~3.1 % lower than its actual value when measured using a 10 ms dwell
30 time. This reduces the calculated average diameter by ~ 1.2%.
31
32
33
34
35

36 Multiple particle event scan give rise to a spurious tail of large particles. However, according
37 to Poisson statistics, only 0.234 % of the Ag particle events were due to more than one
38 particle for the F of 0.00493. During a particle event the signal may momentarily reach high
39 count rates while the automatic dead time correction is based on the average count rate during
40 the whole duration of the dwell.¹² If 597 Ag ions are delivered as a Gaussian pulse with
41 duration of t_b ($\sigma=0.08$ ms), the average ion flux during the particle event will be 10^6 cps.
42
43
44
45
46
47
48
49
50 Given that the detector has a dead time of 25 ns, only ~2.7 % of the ions are on average
51 omitted from counting, resulting in ~ 0.9 % smaller size. For larger particles dead time could
52 be a significant source of error, and it is advised that it should be evaluated for each
53 measurement situation whether sensitivity should be reduced or if analogue ion detection is a
54 more suitable option.
55
56
57
58
59
60

1
2
3 Finally, the error in f_{neb} is propagated to the s . The sensitivity can be can be rewritten as
4
5 $I_{diss}(q_{nebulizer}t_{dwell}C_{nebulizer}f_{neb})^{-1}$, where the I_{diss} is the dissolved signal intensity. When this
6
7 expression is substituted into Eqn 2 it becomes clear that the error is reduced to its third root
8
9 when calculating the diameter. The percent uncertainty in particle diameter can be expressed
10
11 as:
12
13

$$100\% \times \sqrt[3]{\frac{f_{neb} \pm \Delta f_{neb}}{f_{neb}}} = \Delta \% d \quad (4)$$

14
15
16
17
18
19
20
21 In the case of Ag the 95% confidence interval in f_{neb} translates to an uncertainty in particle
22
23 diameter ranging from -12.6 % to 10.0 %, and -15.1 % to 11.5 % for mass and analyte-based
24
25 f_{neb} respectively. The uncertainty in nebulization efficiency is thus dominating source of error
26
27 in these measurements, because other error sources are small or can be at least partially
28
29 corrected for. The average particle diameter (analyte based f_{neb}) corrected for incomplete
30
31 particle events and dead time becomes thus 57.4 with a 95% confidence interval ranging from
32
33 48.8 to 64.0 nm (Table 4). For comparison, the corresponding confidence interval for the
34
35 diameter obtained with sample mass based f_{neb} without correction for analyte partitioning
36
37 would be 53.1 – 66.8 nm. Regardless of if correction for analyte partitioning is applied or not,
38
39 the SEM diameter is included in the confidence interval. The data do therefore not allow
40
41 drawing any conclusions regarding the validity of the proposed correction scheme.
42
43
44
45
46

47
48 The data for AuNP demonstrates more clearly the feasibility of correcting for analyte
49
50 partitioning. The frequency of multiple particle events is insignificantly low (1.3 % of the
51
52 particle events), and the uncertainty in diameter due to f_{neb} is only $\pm \sim 2$ %. Correction for dead
53
54 time and incompletely measured particle event error was also performed assuming that t_b is
55
56 equal to that for Ag particles. The corrected diameter is equal to the size measured by SEM,
57
58
59
60

and has a confidence interval whose width is comparable to the accuracy of many established particle sizing methods²¹ (Table 4).

Noise in particle signals The ability of spICPMS to resolve differing sizes is limited by the noise in particle signals. The standard deviation of particle event signals, σ_{total} , is due to both noise and polydispersity. It can be written as a sum of squares of its components:

$$\sigma_{Polydispersity}^2 + \sigma_{Ion\ Count}^2 + \sigma_{Proportional}^2 + \sigma_{Background}^2 + \sigma_{Incomplete}^2 = \sigma_{total}^2 \quad (5)$$

where $\sigma_{Ion\ count}$ is shot noise, *i.e.* the random error of the ion count. The signal during a particle event is the sum of ions originating from the particle, and those from the background levels of dissolved analyte. The mean intensity of background signal is subtracted from ion count to obtain I_{part} but its noise, $\sigma_{Background}$ remain in the particle signals. $\sigma_{Proportional}$ is flicker noise proportional to the signal intensity given by $\sigma_{Proportional} = I_{part} * cv_{pr}$, where cv_{pr} is called the flicker factor. Flicker noise of dissolved ions is mainly caused by random sizes and arrival times of nebulized droplets, but also by varying trajectories of ions in the plasma and ion diffusion during transport from the plasma to the detector.²² In the case of the noise on particle events, noise sources prior to atomization and ionization of particles in the plasma are irrelevant. The remaining flicker noise originates in varying trajectory lines of ions relative to the cone axis, and the distance from sampler cone to the point of vaporization and subsequently diffusion during transport to the detector.²³ The $\sigma_{Incomplete}$ is noise due incompletely measured particle events, $\sigma_{Incomplete} = I_{part} * cv_{Incomplete}$. The spread in particle signals increases sharply when t_{dwell} approaches the particle event duration (Fig.4).

The levels of different type of noise for the Ag particles are listed in table 5. For this sample any spurious spread in SEM size distribution is likely to be small, and $\sigma_{Polydispersity}$ was estimated by using Eqn. 2 to recalculate the SEM diameters to their corresponding I_{part} values. The $\sigma_{Background}$ was obtained from the signal variation in dwells where there were no

1
2
3 particles. The $\sigma_{Incomplete}$ was taken from Fig.4. To calculate $\sigma_{Ion\ count}$ it was assumed that this
4
5 noise is given by $(\beta I_{part})^{0.5}$ where β is the shot noise coefficient.²⁴ The β was determined to
6
7 22.64 along with the flicker noise in dissolved signals in ESI-3. The remaining variation in
8
9 particle signals was attributed to $\sigma_{Proportional}$.
10
11

12
13 The shot, flicker and noise due to incompletely measured particle events are dominating for
14
15 these ~ 60 nm particles. The flicker noise appears to be smaller for particles (5.7 % RSD) than
16
17 for dissolved analyte (10.2 % RSD). The background noise amplitude is most likely only
18
19 quantitatively relevant close to the size detection limit. It is instructive to calculate the
20
21 resolution in particle size to facilitate comparison with other methods. The resolution in
22
23 particle mass, R_m can be defined as three times the standard deviation in I_{part} due to noise,
24
25 which is divided by the sensitivity in order to convert the units to mass, $R_m = 3 * \sigma_{noise} * s^{-1}$. For
26
27 the Ag particles that are measured here the R_m is ~ 0.95 fg which corresponds to ~ 12 nm
28
29 difference in diameter. This falls short from *e.g.* the sub nanometer resolution obtainable by
30
31 analytical ultracentrifugation,²⁵ and the so far most sensitive suspended nano channel
32
33 resonator device²⁶ that weighs Ag nanoparticles as small as 20 nm with an R_m of 0.027 fg.
34
35 However, efforts to reduce the $\sigma_{Incomplete}$ by fast data acquisition²⁷ or correction using a known
36
37 t_b as outlined above are likely to result in significant improvements in resolution.
38
39
40
41
42
43
44

45 **Effective dwell time** Decreasing t_{dwell} introduces also bias in particle number concentration.

46
47 Large particles producing signals well above the DL_s may be detected even if the peak of the
48
49 ion burst occurs a time t_p before the dwell starts, or after it ends. Fig.5 shows that the effective
50
51 dwell time for determination of particle number concentration is in this case $t_{eff} = t_{dwell} + 2t_p$. If
52
53 more than 50 % of the ions produced by a particle needs to be detected for I_{part} to exceed DL_s ;
54
55 the peak of the ion burst must occur during a dwell (Fig.5). In this case the effective dwell
56
57 time becomes shorter than the set dwell time, *i.e.* t_p becomes negative. For the Ag particles
58
59
60

investigated here, an average t_p of 0.15 ms was calculated from I_{part} , t_b , and DL_s . An experimental value was determined using a procedure developed by Heithmar.²⁸ Using $t_{dwell} + 2t_p$ instead of t_{dwell} , equation 2 can be rearranged to:

$$\frac{F}{c_p} = f_{neb}q_{nebuliser}t_{dwell} + 2t_p f_{neb}q_{nebuliser} \quad (6)$$

In Fig. 6 Fc_p^{-1} is plotted against t_{dwell} , and a t_p of 0.31 ± 0.24 ms is obtained by dividing the intercept ($2t_p f_{neb}q_{nebuliser}$) with the slope ($f_{neb}q_{nebuliser}$) using equation (6). The confidence interval magnitude expresses the uncertainty in the fit parameters, a value that is high because the value of the intercept is sensitive to random error in F that scatters the data points. This method should consequently be used with caution.

Accuracy of particle number concentration determination The random uncertainty in c_p , $\Delta c_{p Random}$ is given by the root sum of squares of the counting statistics confidence interval, $\Delta c_{p Particle count}$ and uncertainty in nebulization efficiency, $\Delta c_{p f_{neb}}$. It is also possible that the particle frequency is not constant during the measurements due to *e.g.* fluctuations in sample flow rate. In this case uncertainty due to short term fluctuations in F , $\Delta c_{p F}$ should also be taken into consideration.

To calculate the $\Delta c_{p Particle count}$ it is assumed that the number of particles that are detected in a sequence of D dwells with a particle frequency $F = ND^{-1}$ is given by the binomial distribution. For such distribution, there exists several ways of approximating the confidence interval in F as a function of F and D .²⁹ The fact that N is given by $N = DF$ allows to express these confidence intervals as a function of particle count. An approximation for the ΔF as function of particle count was derived previously using the Wald confidence interval.¹⁰ Here the more reliable Wilson confidence interval was used instead, because the confidence intervals calculated by the Wald equation may be significantly shorter than their true values for small

values of D .²⁹ An approximation to the relative width of the 95 % confidence interval, ΔFF^{-1} as a function of N was calculated according to equation 4 in Ref.29, and shown in Fig7.

To investigate if there were significant fluctuations in F , a bootstrap method³⁰ was applied to estimate the uncertainty as a function of N based on experimental data. Dwells were chosen randomly with repetition and inspected for particle events from the set of 200 000 measured dwells. This was repeated D^* times, until the desired number of particle events were found. 2000 D^* values were acquired, and a 95% confidence interval for D^* was calculated by ordering the set of D^* and considering the values of the 100: th and 1900: th elements as the confidence interval boundaries. The confidence interval in D^* is for a given particle frequency proportional to the uncertainty in c_p , which is here denoted $\Delta c_{p \text{ Bootstrap}}$. The relative width of $\Delta c_{p \text{ Bootstrap}}$ is shown as a function of N in Fig. 7.

The $\Delta c_{p \text{ Particle count}}$ and $\Delta c_{p \text{ Bootstrap}}$ follow each other closely; however the bootstrap technique seems to slightly underestimate the width of the confidence interval for most values of N . Note also that the bootstrap confidence interval does not follow a smooth curve due to the random nature of the calculations. These results suggest that the contribution from Δc_{pF} was not significant here. The total random uncertainty is therefore given by:

$$\Delta c_{p \text{ Random}} = \sqrt{\Delta^2 c_{p \text{ Particle count}} + \Delta^2 c_{p f_{neb}}} \quad (7)$$

The relative width of $\Delta c_{p \text{ Random}}$ is plotted in figure 7. The random uncertainty in this case decreases initially rapidly with increasing particle count to reach a level determined mainly by $\Delta c_{p f_{neb}}$ at ~300 particle events. The c_p in the Ag dispersion was measured to 528 particles mL⁻¹ with a 95 % confidence interval ranging from 380 to 976 particles mL⁻¹ using the calculated t_{eff} of 10.3 ms. Correction for effective dwell time is unlikely important when using 10 ms t_{dwell} , because t_{eff} is not more than a few percent longer than the set dwell time. The

1
2
3 relative importance of dwell time correction increases for shorter dwell times, and when t_{dwell}
4 approaches the duration of the ion burst ($t_{dwell} \sim < 2$ ms) it might become significant in
5
6 comparison with the random error.
7
8

9
10 To evaluate the magnitude of non random error, the number concentrations of AuNP
11 measured by spICPMS are compared in Fig.8 with those measured by counting particles on
12 filters (Filter deposition), and calculated from analyte mass concentration and diameter
13 assuming a spherical shape (Total Au mass). The SEM diameters, aspect ratios, and
14 concentrations measured by spICPMS are listed in table 6. Note that the sizes for 100 and 250
15 nm AuNP differ significantly from their nominal values. This is probably due to Ostwald
16 ripening because these dispersions were old. After using the bootstrap method to confirm that
17 there were no significant fluctuations in F , the uncertainties in c_p were calculated according to
18 Eqn. 7 and are shown in Fig. 8. The frequencies of multiple particle events were not
19 significant for the larger AuNP either, with 0.47 %, and 0.13 % of the particle events for 100
20 nm, and 250 nm AuNP being due to more than one particle.
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37

38 The c_p calculated from mass concentration is not necessary equal to the true value because
39 these particles are not completely spherical. Based on analysis of the filtrate, more than 99.99
40 % of the mass of Au in the 250, and 100 nm dispersions, and 91 % of that in the 50 nm
41 dispersions were retained on the filters. However, the accuracy of the filter deposition method
42 is reduced due to aggregation, and because the examined areas are not necessarily fully
43 representative as the surface concentration varied over the filter area.
44
45
46
47
48
49
50
51
52

53 The shortcomings of the methods of comparison result in a large spread in the c_p values, that
54 nevertheless agree relatively well with spICPMS. The average ratio of reference c_p , and
55 spICPMS c_p for each of the 6 reference values for the three samples was 1.27 ± 0.64 . More
56 accurate reference methods are required to assess subtle error sources such as analyte
57
58
59
60

1
2
3 partitioning, off axis trajectories of particles in plasma, and adsorption of particles to tubing
4
5 and container walls.
6
7

8
9 **Conclusions and outlook** The accuracy of both particle diameter and c_p are ultimately
10
11 limited by the uncertainty in f_{neb} . It was found that systematic errors in the WC method could
12
13 be significantly reduced by correcting f_{neb} for analyte partitioning between plasma and sample
14
15 flows, however further work is necessary in order to develop this approach into an fully
16
17 reliable analytical method. Among other things, it should be investigated whether size
18
19 fractionation occurs in the spray chamber. The other identified error sources are small, and
20
21 can be at least partially corrected for, if proper care is taken during measurements. If f_{neb}
22
23 would be known precisely, the sizing accuracy of spICPMS would rival *e.g.* the 3 %
24
25 achievable by electrospray scanning mobility particle sizer (ES-SMPS),³¹ and the 5 %
26
27 accuracy of magnification calibration in SEM, which is nominally reached by following
28
29 American society for testing materials (ASTM) standard procedures.³²
30
31
32
33

34
35
36 The size resolution is limited by the noise in particle signals. The noise in particle signals is
37
38 dominated by that due to shot, incomplete particle events, and flicker noise, which could be
39
40 reduced by proper measurement settings and sample introduction respectively. For instance,
41
42 when measuring ion bursts from a train of droplets containing dissolved analyte introduced by
43
44 a monodisperse dried microparticle injector (MDMI) device and acquiring data with fast time
45
46 resolution using an oscilloscope, the coefficient of variation was reduced to 5 %.¹⁹ However,
47
48 the magnitudes of noise in the measurements made in this article are still low enough for
49
50 polydispersity to dominate the spread in sizes for most samples that are encountered in
51
52 practice.
53
54
55

56
57
58 No systematic bias in number concentration that exceeds the margin of uncertainty of the
59
60 reference methods was observed. Further improvements in accuracy of spICPMS in terms of

1
2
3 particle counting are difficult due to the lack of accurate and validated reference methods.
4
5 Counting particles on filters could be developed to such high accuracy technique. Particle
6
7 populations can be quantitatively retained on filters, and if filtration devices utilizing small
8
9 enough filter areas ($< 1 \text{ mm}^2$) were used, sampling error could be eliminated by counting all
10
11 of the particles in a volume of dispersion. The aggregation on filter surfaces could be reduced
12
13 by decreasing the concentration in the filtered dispersion.
14
15

16
17
18 A completely different approach to determine f_{neb} would be to add particles quantifiable by
19
20 optical means to the sample flow. An accurate method for particle counting using
21
22 fluorescence spectrometry is being developed for micron sized particles.³³ If it could be
23
24 extended to fluorescent quantum dots, rapid and accurate determination of a particle based f_{neb}
25
26 would be possible by passing the sample flow through a fluorescence detector. Besides the
27
28 possibility to create an internal standard for nebulization efficiency, such hyphenated system
29
30 would allow straight forward quantification of possible losses due to adsorption on surfaces
31
32 and trajectories lying off the sampler cone axis.
33
34
35
36
37

38 **SUPPLEMENTARY INFORMATION** Electronic supplementary information (ESI) is
39
40 available as indicated in text.
41
42

43 **ACKNOWLEDGEMENT**

44
45
46 We thank the following funding agencies for support: European Commission FP7 projects
47
48 NANOFATE (Ref#: 247739, 2010-2014) and MARINA (Ref#: 263215, 2011-2015), the
49
50 Swedish Environmental Research Council FORMAS and the Gothenburg graduate school
51
52 Environment and Health.
53
54
55
56
57
58
59
60

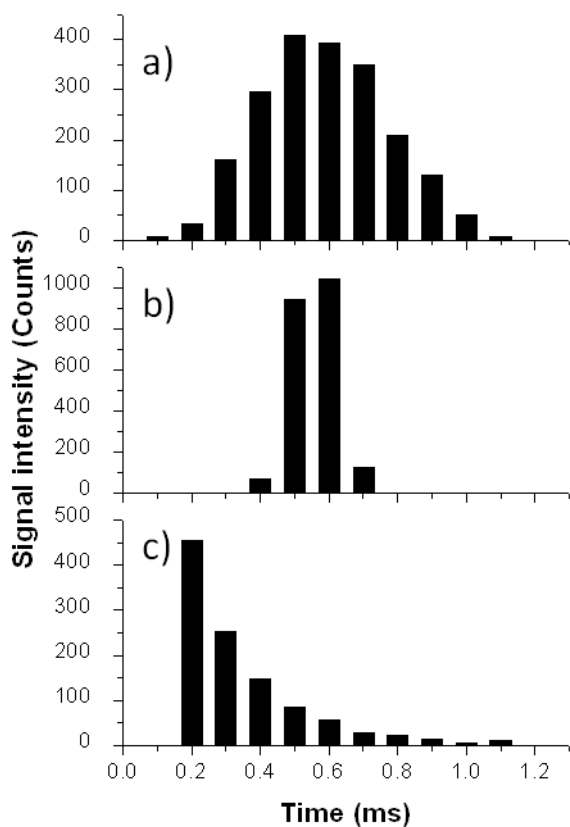


Fig. 1 Particle events of 80 nm Ag particles measured using fast data acquisition with 0.1 ms time resolution. a) A particle event that is a) broader, and b) narrower than average. c) An extreme case of the occasionally observed tailing effect.

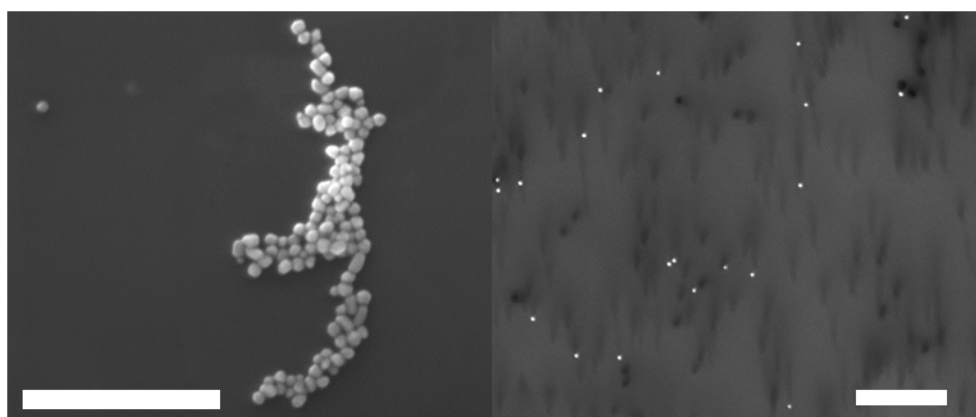


Fig. 2 Images of 80 nm AgNP (Left), and 50 nm AuNP (Right). The scale bars are 1 μm.

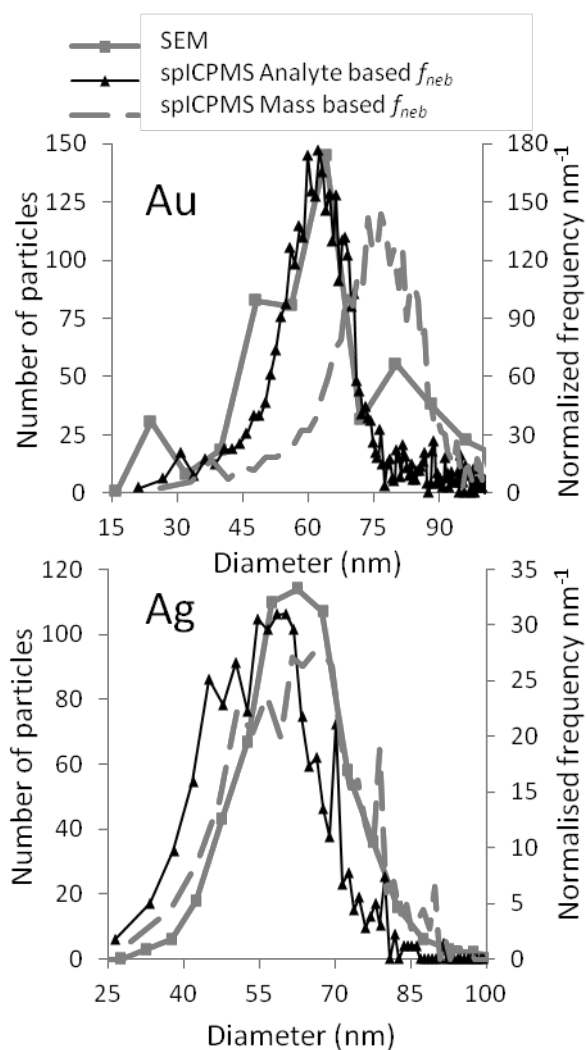


Fig.3 SEM and spICPMS size distributions of the 80 nm AgNP and 50 nm AuNP. The spICPMS size distributions were calculated using both mass and analyte based f_{neb} .



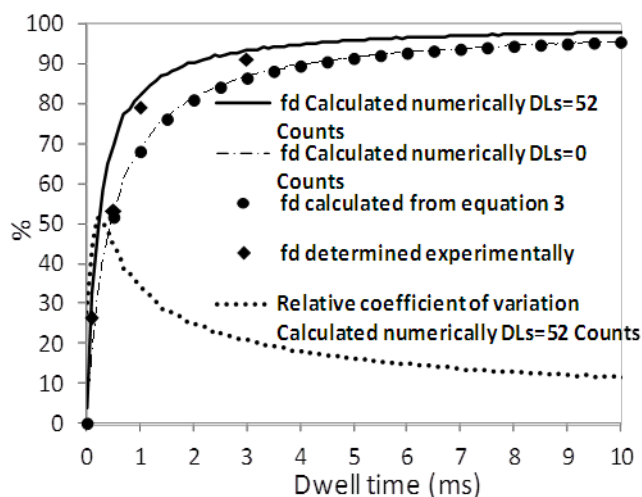


Fig.4 The average fraction of ions in the particle events with an ion burst duration $t_b = 0.48$ ms that are appearing in each dwell, f_d , as a function of dwell time for both theoretical and experimental data. Theoretical calculations using two different size detection limits are shown. The relative coefficient of variation (spread) of particle signal intensities due to incomplete particle events is also included.

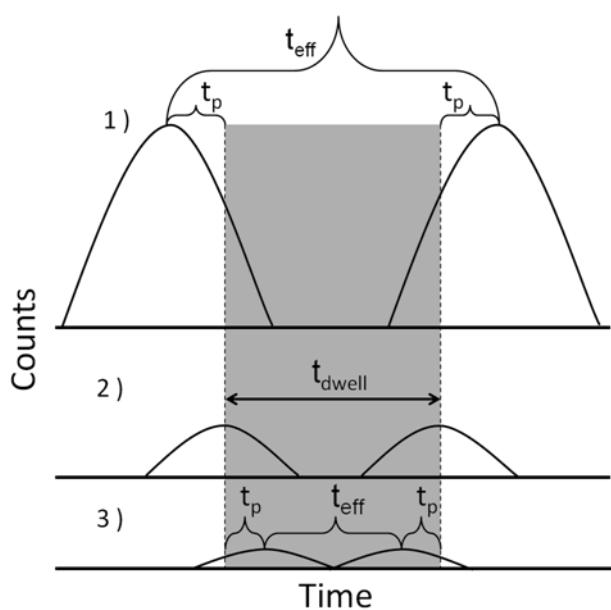

1
2
3 **Fig.5** Illustration explaining the concepts particle time, t_p effective dwell time, t_{eff} , and set
4 dwell time, t_{dwell} . 1) The effective dwell time is longer than t_{dwell} for a large particle where
5 only the tails of ion bursts need to coincide with the dwell time for it to be detected. 2) When
6 half of the ions have to be detected to exceed the detection threshold, DL_s , the t_{eff} is equal to
7 the set dwell time. 3) In order to detect a small particle, most of the ions must arrive during
8 t_{dwell} . In this case, the effective dwell time for particle detection becomes shorter, *i.e.* t_p is
9 negative.

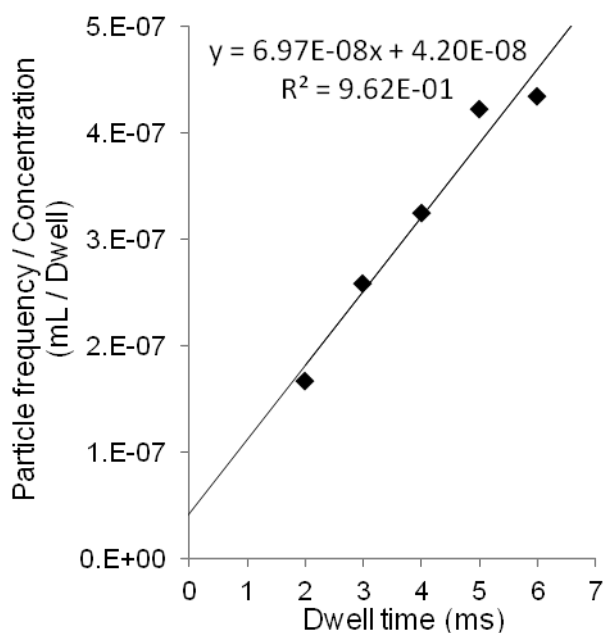

20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47 **Fig.6** The concentration normalized particle frequency as a function of dwell time. The slope
48 and intercept of the fitted line was used for determination of t_{eff} .

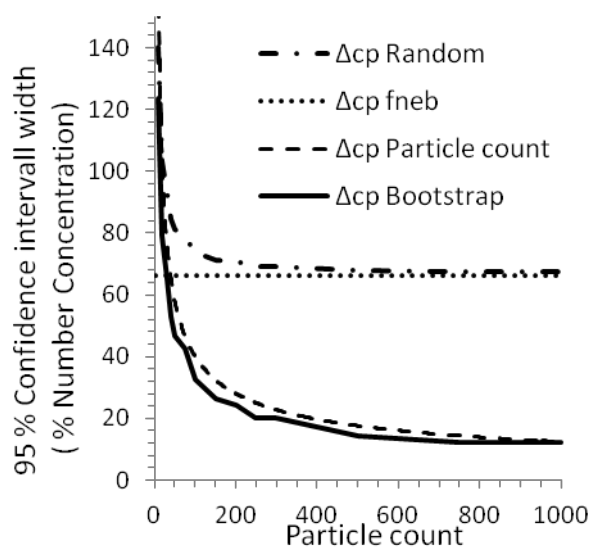


Fig.7 The width of confidence intervals of c_p as a function of particle count: The confidence interval of c_p due to total random uncertainty calculated from Eqn. 7 (Δc_p Random). The confidence interval of c_p due to the uncertainty in f_{neb} (Δc_p fneb). The Wilson confidence interval of c_p due to counting statistics (Δc_p Particle count). The uncertainty calculated using the bootstrap method (Δc_p Bootstrap).

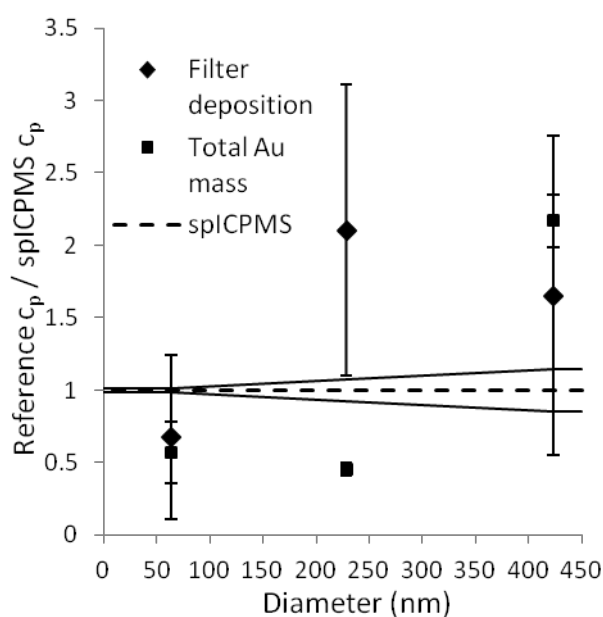


Fig.8 The ratio of number concentrations measured by the reference methods and spICPMS. The lines indicating spICPMS error show the uncertainty due to inaccurate nebulization efficiency, and stochastic error in particle count determined according to equation 7. The uncertainty for the filter counting data is due to variation among replicate experiments, while that of the analyte mass is due to combined effects of uncertainty in particle diameter, and variation among replicate ICPMS measurements.

Table 1. List of symbols.

Symbol	
c_p	Number concentration (Particles V^{-1})
D	Number of dwells
N	Number of particles
F	Particle frequency ($N D^{-1}$)
DL_s	Detection limit (Counts)
I_{part}	Particle signal intensity (Counts)
I_{diss}	Dissolved signal intensity (Counts)
s	Sensitivity (Counts g^{-1})
q	Flow rate ($V s^{-1}$)
c	Concentration (gV^{-1})
f_{neb}	Nebulization efficiency (%)
Δ	Confidence interval
σ	Standard deviation
t_{dwell}	Dwell time (s)
t_b	Duration of ion burst (s)
t_p	Particle time (s)
t_{eff}	Effective dwell time (s)
cv	Coefficient of variation (RSD %)
f_d	Fraction of ions measured

R_m	Resolution in particle mass (g)
d	Particle diameter (m)
e_{std}	Standard error of the mean (m)

Table 2. Massspectrometer tune parameters and sample introduction components.

Sample gas flow rate (L min ⁻¹)	~1.370
Auxiliary gas flow rate (L min ⁻¹)	~0.96
Cool gas flow rate (L min ⁻¹)	15.02
Sample uptake rate (ml min ⁻¹)	~0.523
RF power (W)	1158
Nebulizer	Micromist 0.4 ml/min uptake rate concentric nebulizer (Glass expansion)
Spray chamber	Cyclonic (Glass expansion)
Torch	Fassel type (Thermo Finnigan)
Sample cone	Nickel 1.0 mm orifice diameter
Skimmer cone	Nickel 0.8 mm orifice diameter

Table 3. Nebulization efficiency and particle size calibration parameters.

Sample	$q_{nebulizer}$	q_{waste}	Mass based f_{neb}	Analyte based f_{neb}	Sensitivity	Recipient
Ag 80 nm	0.53 ± 0.012 mL / min	0.49 ± 0.017 mL / min	6.7 ± 2.2 %	4.7 ± 1.8 %	4.99 * 10 ¹⁷ Counts g ⁻¹	123 Counts
Au 50 nm	0.56 ± 0.0055 mL / min	0.51 ± 0.0037 mL / min	8.7 ± 0.49 %	4.7 ± 0.26 %	5.08 * 10 ¹⁷ Counts g ⁻¹	739 Counts

Table 4. SEM and spICPMS diameters of AgNP, and 50 nm AuNP showed together with the magnitudes of bias and uncertainty in the spICPMS measurements. The spICPMS diameters were corrected for bias, and the corrected values are given with the 95 % confidence interval due to Δf_{neb} .

Particles	spICPMS d^{\dagger}	Dead time ‡	Incomplete particle events ‡	Δf_{neb}	Corrected spICPMS d	SEM d
AgNP	56.24 nm	-0.9 %	-1.2 %	-15.1 % +11.5 %	48.8 - 64.0 nm	61.99 \pm 0.39 nm
50 nm AuNP	61.06 nm	-3.3 %	-1.2 %	-1.9 % +1.8 %	62.6 - 65.0 nm	63.48 \pm 1.54 nm

† Measured using analyte based f_{neb} . ‡ It was assumed that the t_b of Au particles equaled that measured for Ag.

Table 5. Contributions of sample polydispersity and noise to the spread in particle signals (Relative standard deviation, RSD).

σ_{\dagger} Polydispersity	σ_{\dagger} Ion Count	σ_{\dagger} Proportionality	σ_{\dagger} Incomplete	σ_{\dagger} Background	σ_{\dagger} total
51 % RSD	18.9 % RS	5.7 % RSD	12 % RSD	1 % RSD	56 % RSD

† Determined from SEM

data. ‡ The contribution from incomplete particle events was estimated from figure 4.

Table 6. Properties of the AuNP dispersions.

Sample	Aspect ratio	SEM diameter †	spICPMS Concentration ‡
Au 50 nm	2.08	63.48 \pm 1.54 nm	5631 particles mL $^{-1}$
Au 100 nm	1.58	228.1 \pm 16 nm	2185 particles mL $^{-1}$
Au 250 nm	1.68	423.0 \pm 13.6 nm	599 particles mL $^{-1}$

† The uncertainty was calculated from the e_{std} . ‡ The concentration in the dispersions diluted for measurement.

References

1. P.J.J. Alvarez, V. Colvin, J. R Lead, V. Stone, *ACS Nano* 2009, **3**, 1616-1619
2. K. Ehara, H. Sakurai, H. Metrologia 2010, **47**, S83-S90

3. S. Dubascoux, I. L. Hecho, M. Hasselov, F. V. D. Kammer, M. P. Gautier. G. Lespes, *J. Anal. At. Spectrom.* 2010, **25**, 613-623.
4. C. Degueldre, P. Y. Favarger, *Colloids Surf. A* 2003, **217**, 137-142.
5. C. Degueldre, P. Y. Favarger, *Talanta*, 2004, **62**, 1051-1054.
6. C. Degueldre, P. Y. Favarger, C. Bitea, *Anal. Chim. Acta*, 2004, **518**, 137-142.
7. C. Degueldre, P. Y. Favarger, S. Wold, *Anal. Chim. Acta*, 2006, **555**, 263-268.
8. C. Degueldre, P. Y. Favarger, S. Wold, *Talanta*, 2006, **68**, 623-628.
9. F. Laborda, J. Jimenez-Lamana, E. Bolea, J. R. Castillo, *J. Anal. At. Spectrom.* 2011, **26**, 1362-1371.
10. J. Tuoriniemi, G. Cornelis, M. Hassellöv, *Anal.chem.* 2012, **84**, 3965-3972.
11. H. E. Pace, N. J. Rogers, C. Jarolimek, V. A. Coleman, C. P. Higgins, J. F. Ranville, *Anal.chem.* 2011, **83**, 9361-9369
12. J. W. Olesik, P. J. Gray, *J. Anal. At. Spectrom.* 2012, **27**, 1143-1155
13. H. E. Pace, N. J. Rogers, C. Jarolimek, V.A. Coleman, C. P. Higgins, E. P. Gray, J. F. Ranville, *Env. Sci. Tech.* 2012, **46**, 12272-12280.
14. F. Laborda, J. Jimenez-Lamana, E. Bolea, J.R. Castillo, *J. Anal. At. Spectrom.* 2013, **28**, 1220-1232.
15. D. Smith, R. Browner, *Anal. Chem.* 1982, **54**, 533-537.
16. J. A. Boroweic, A. W. Boorn, J. H. Dillard, M. S. Cresser, R. F. Browner, *Anal. Chem.* 1980, **52**, 1054-1059.
17. D. M. Mitrano, E. K. Leshner, A. Bednar, J. Monserud, C. P. Higgins, J. F. Ranville, *Environ. Toxicol. Chem.* 2012, **3**, 115-121.
18. R. Allabashi, W. Stach, A. de la Escosura-Muniz, A. L. Liste-Calleja, A. Merkoci, *J. nanopart. Res.* **2009**, 11, 2003-2011.
19. I. I. Stewart, J. W. Olesik, *J. Am. Soc. mass spec.* 1999, **10**, 159-174.
20. O. Borovinskaya, B. Hattendorf, M. Tanner, S. Gschwind, D. Günther, *J. Anal. At. Spectrom.* 2013, **28**, 226-233.
21. A. Lamberty, K. Franks, A. Braun, V. Kestens, G. Roebben, T. P. J. Linsinger, *J. nanopart. Res.* 2011, **13**, 7317-7329
22. J. W. Olesik, J. A. Kinzer, G. J. McGowan, *Appl. Spectrosc.* 1997, **51**, 607-617.

- 1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60
23. M. P. Dziwiatkoski, L.B. Daniels, J.W. Olesik. *Anal.Chem.* 1996, **68**, 1101-1109.
24. G. Cornelis, M. Hassellöv, *J. Anal. At. Spectrom.* 2013 Accepted for publication
DOI: 10.1039/C3JA50160D
25. K. L. Planken, and H. Cölfen, *Nanoscale*, 2010, **2**, 1849-1869.
26. J. Lee, W. Shen, K. Payer, T. Burg, S. Manalis, *Nano lett*2010, **10**, 2537–2542
27. S. Gschwind, L. Flamigni, J. Koch, O. Borovinskaya, S. Groh, K. Niemax, D.
Gunther, *J.Anal. At.Spectrom.* 2011, **26**, 1166-1174.
28. E. M. Heithmar, *237th ACS National meeting*; abstracts of papers of the American
chemical society: Salt lake city, UT USA, **2009**; Vol. 237, pp 58-COLL
29. L.D. Brown, T.T. Cai, A. DasGupta, *Stat.Sci.*, 2001, **16**, 101-133.
30. J. Carpenter, J. Bithell, *Statist. Med.* 2000, **19**, 1141-1164.
31. D. P. Kinney, D. Y. HPui, G. W. Mulholland, N.P. Bryner, *Journal of Research of the
National Institute of Standards and Technology* 1991,**96**, 147-176.
32. ASTM E766:98 American society of testing materials **2008**
33. T. Sakaguchi, K. Ehara, *Proceedings SPIE 5856 Optical Measurement Systems for
Industrial Inspection IV*, 994 (August 03, 2005); **DOI:**10.1117/12.612472