

Analytical Methods

Accepted Manuscript



This is an *Accepted Manuscript*, which has been through the Royal Society of Chemistry peer review process and has been accepted for publication.

Accepted Manuscripts are published online shortly after acceptance, before technical editing, formatting and proof reading. Using this free service, authors can make their results available to the community, in citable form, before we publish the edited article. We will replace this *Accepted Manuscript* with the edited and formatted *Advance Article* as soon as it is available.

You can find more information about *Accepted Manuscripts* in the [Information for Authors](#).

Please note that technical editing may introduce minor changes to the text and/or graphics, which may alter content. The journal's standard [Terms & Conditions](#) and the [Ethical guidelines](#) still apply. In no event shall the Royal Society of Chemistry be held responsible for any errors or omissions in this *Accepted Manuscript* or any consequences arising from the use of any information it contains.

Technical Note

Cyanide Detection in Gastric Juice with Corrin-based Chemosensors

Christine Aebersold,^a Beat Amstutz,^b Andrea E. Steuer,^b Thomas Kraemer^b and Felix Zelder^{a*}

^aDepartment of Chemistry, University of Zurich, Winterthurerstrasse 190, 8057 Zurich, Switzerland. Fax: +41 44 635 6803; E-mail: felix.zelder@chem.uzh.ch, www.felix-zelder.com.

^bDepartment of Forensic Pharmacology and Toxicology, Zurich Institute of Forensic Medicine, University of Zurich, Zurich, Switzerland

Abstract:

This Technical Note describes the detection of cyanide in artificial gastric juice with corrin-based chemosensors. The application of this method in authentic human samples is demonstrated in a proof-of-principle forensic investigation.

1. Introduction

Cyanide (CN⁻) is highly toxic to humans and most forms of life because of its strong binding to biologically active transition metal ions.^{1, 2} In particular, it effectively blocks the vacant coordination sites of ferri-(Fe^{III}) containing heme complexes and thereby inactivates cellular respiration.³⁻⁵ Cyanide intoxications may occur from intentional and accidental cyanide uptake and are most frequently encountered in industrialized countries after smoke inhalations from fires.⁶ Indeed, more than 80 % of fire victims die from smoke gas intoxications and not from burns.⁷ One of the most toxic combustion products of nitrogen containing organic products is hydrogen cyanide (HCN; pK_a = 9.04⁸),⁹ the conjugated acid of cyanide. Testing for cyanide intoxication is therefore required in clinical diagnostics and forensic investigations.^{1, 2, 10, 11} For this purpose, different types of body fluids such as blood,¹²⁻¹⁷ saliva^{18, 19} and gastric acid^{20, 21} are usually analysed. Most methods require sample pre-treatment, sophisticated technical equipment (e.g. GC-MS,²² ESI-MS-MS²³) as well as specialised users and hence, the analysis of cyanide is not yet routine in hospital and forensic settings.² Recent developments indicate that low-cost and straightforward test-kits with colorimetric and fluorometric indicators may overcome these limitations.^{12, 17, 24-29} In this context, vitamin B₁₂ based chemosensors are currently representing one of the most promising systems for detecting cyanide in biological samples in terms of handling, selectivity, sensitivity and response time.^{4, 26, 28-34} Based on earlier pioneering investigations of our group,³⁴⁻³⁷ we describe herein the detection of cyanide in artificial gastric juice with corrin-based chemosensors and

1
2
3 solid phase extraction (SPE).^{24, 38} The applicability of the method is demonstrated in
4 a proof-of-concept forensic investigation.
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

2. Materials and methods

2.1 Materials and general information

Chromabond C18ec polypropylene columns (100 mg), Chromafix C18ec columns (s) (270 mg), shorty (5 mg) and Chromabond adapter PP were obtained from Macherey-Nagel AG, Switzerland. The columns were pre-conditioned prior use with MeOH (1 mL) and water (5 mL).

UV-vis spectra were measured at $T = 21 \pm 1$ °C with a Cary 50 spectrometer (Varian, Switzerland) using quartz cells with a path length of 1 cm.

2.2 Preparation of solutions

The desired pH value of the stock solution of the buffer Ches (0.25 mol L^{-1} ; pH 9.6) was adjusted by the addition of 2 mol L^{-1} NaOH and 1 mol L^{-1} HCl solutions. The pH values were measured with a Metrohm 827 pH lab (Metrohm, Switzerland).

The cyanide stock solution ($10^{-3} \text{ mol L}^{-1}$) was freshly prepared every day.

Artificial gastric juice (AGJ) was obtained by dissolving pepsin (32 mg, 89 μmol), NaCl (20 mg, 0.34 mmol) and HCl (32 %, 0.07 mL) in 10 mL water.³⁹

2.3 Preparation of the chemosensor aquacyanocobyric acid heptamethylester (ACCbs)⁴⁰

The corrin-based chemosensor aquacyanocobyric acid heptmethylester (ACCbs) was synthesized as described elsewhere.^{36, 40}

2.4 Artificial gastric juice cyanide detection

Artificial gastric juice (AGJ; 500 μL) was spiked with cyanide ($[\text{CN}^-] = 0 - 160 \mu\text{mol L}^{-1}$). Fifteen minutes later, the gastric juice sample was diluted to 972 μL with Ches buffer (0.25 mol L^{-1} ; pH 9.6; 392 – 472 μL , depending on the volume of CN^- added) and ACCbs (28 μL ; 1.5 mmol L^{-1} ; 42 nmol) was added.

Cyanide was either detected directly in solution (A) or after solid-phase extraction (B).

A: The solution was transferred to a quartz cuvette and analyzed with UV-vis spectroscopy.

B: After one minute, the sample was passed through a pre-conditioned C18ec column and subsequently washed with water (3 mL) to remove adhering gastric juice from the C18ec material. The chemosensor was subsequently eluted from the C18ec column with MeOH (0.4 mL). The eluate volume was adjusted to 0.5 mL with MeOH,

transferred to a quartz cuvette and analysed with UV-vis. The cyanide content was determined with the help of a calibration curve.

2.5 Calibration curves

Homogenous conditions:

UV-vis spectra of AGJ samples spiked with different amounts of cyanide ($[\text{CN}^-] = 0 - 160 \mu\text{mol L}^{-1}$) were analysed. The calibration curve was obtained by plotting the absorptions at 583 nm against CN^- concentrations. Each experiment was repeated three times to assign mean values and standard deviations. A linear equation ($y = a + b \cdot x$) was obtained by fitting the linear range with OriginPro2015.

Solid-phase extraction:

UV-vis spectra of AGJ samples spiked with different amounts of cyanide ($[\text{CN}^-] = 0 - 160 \mu\text{mol L}^{-1}$) were analysed after eluting the reagent from the C18ec cartridge with MeOH ($V = 0.4 \text{ mL}$). The eluate volume was adjusted to 0.5 mL with MeOH and the UV-vis spectra were recorded. The calibration curve was obtained by plotting the absorptions at 583 nm against CN^- concentrations. Each experiment was performed three times in order to determine the mean value and standard deviations. A linear equation ($y = a + b \cdot x$) was obtained by fitting the linear range with OriginPro2015.

2.6 Artificial gastric juice cyanide detection at different incubation times

The influence of incubation time (defined as time between spiking and analysis) was determined for AGJ samples stored at room temperature ($T = 23 \pm 1 \text{ }^\circ\text{C}$). Samples spiked with cyanide ($V_{\text{sample}} = 0.5 \text{ mL}$, $[\text{CN}^-]_{\text{AGJ}} = 40 \mu\text{mol L}^{-1}$) were analysed after different time intervals ($t = 20 - 1470 \text{ min}$) and analysed as described under 2.4. Each experiment was repeated three times to assign mean values and standard deviations. In the same way, experiments were performed for AGJ samples ($V_{\text{sample}} = 0.5 \text{ mL}$, $[\text{CN}^-]_{\text{AGJ}} = 40 \mu\text{mol L}^{-1}$) that were stored for different time intervals ($t = 1 \text{ d} - 55 \text{ d}$) at $-21 \text{ }^\circ\text{C}$.

2.7 Gastric juice cyanide detection in authentic human samples

Cyanide was monitored in diluted human gastric juice samples (HGJ) with (A) and without (B) solid-phase extraction using corrin-based chemosensors. In addition, the samples were analysed by a microdiffusion assay with barbituric acid/ pyridine as reagent (C)⁴¹. Each experiment was either performed three times (A, B) or twice (C) in order to determine the mean value and standard deviations.

1
2
3 A: Ches buffer (472 μL , 0.25 mol L^{-1}) and ACCbs (28 μL , 1.5 mmol L^{-1} , 42 nmol or 42
4 μL , 1 mmol L^{-1} , 42 nmol) were added to a HGJ sample ($V_{\text{sample}} = 0.5 \text{ mL}$). After one
5 minute, the sample was passed through a Chromabond C18ec column. The column
6 was washed with water (3 mL). Immobilized corrinoids were eluted with MeOH (0.4
7 mL). The eluate volume was adjusted to 0.5 mL, transferred to a quartz cuvette and
8 analyzed with UV-vis. The concentration of cyanide in HGJ was determined with the
9 help of the calibration curve shown in Fig. 4.
10
11

12
13
14 B: Ches buffer (200 μL , 0.25 mol L^{-1}) and ACCbs (42 μL , 1 mmol L^{-1} , 42 nmol) were
15 diluted with water (700 μL , $V_{\text{sample}} = 1 \text{ mL}$). Aliquots (10-100 μL) of diluted HGJ
16 (dilution factor: 970) were added. After 5 minutes, the concentration of cyanide in
17 HGJ was determined with the help of the calibration curve shown in Fig. 3 after
18 volume correction and under considering of the dilution factor.
19
20

21
22 C: Sulfuric acid (10%, 0.5 mL) and diluted gastric juice (1 mL, 1:50 and 1:100 dilution
23 with distilled water, respectively) were added to the outer compartment of two
24 Conway microdiffusion cells. To the inner compartment sodium hydroxide (1 M, 0.5
25 mL) was added. The cells were immediately closed, gently agitated and incubated for
26 2 hours. An aliquot (0.1 mL) of the inner compartment was transferred into a tube
27 containing a hydrogen phosphate solution (0.87 mol L^{-1} , 1 mL). A chloramine-T
28 solution (25%, 0.5 mL) was added and incubated for 3 min at room temperature.
29 Finally, a barbituric acid/ pyridine reagent (1.5 mL; Reagent: 3 g of barbituric acid in
30 15 mL of pyridine and hydrochloric acid (32 %, 3 mL) were diluted with distilled water
31 to a final volume of 25 mL) was added. It was incubated for another 10 min and the
32 absorbance of the solution was measured at 580 nm. Concentrations were calculated
33 by comparison with a calibration curve using standard cyanide solutions prepared in
34 the same manner.
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

3. Results and discussion

Figure 1 shows the UV-vis spectrum of aquacyanocobester (ACCbs; $42 \mu\text{mol L}^{-1}$)^{36, 40} in pure water as well as in a diluted sample of artificial gastric juice (AGJ; see Experimental Part).

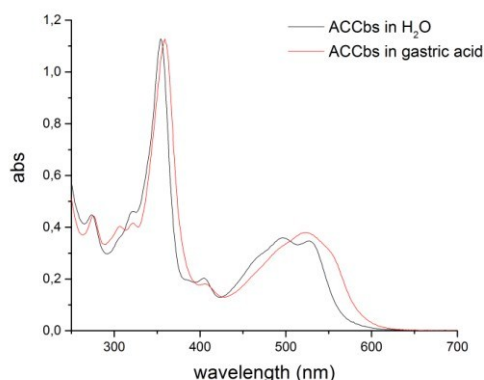


Figure 1. UV-vis spectra of ACCbs (42 nmol) recorded in water and artificial gastric juice (AGJ : H₂O = 1:1; V = 1 mL).

The hypsochromic shift of the γ -band of ACCbs from 355 nm to 359 nm and the broadening of the α -, and β -bands (497 and 527 nm) to one single absorption (525 nm) indicates interactions between the chemosensor and AGJ. Most likely, an amino acid side chain of the pepsin, the main component of AGJ, is coordinated to the vacant coordination site of the chemosensor (Figure 2A).^{42, 43}

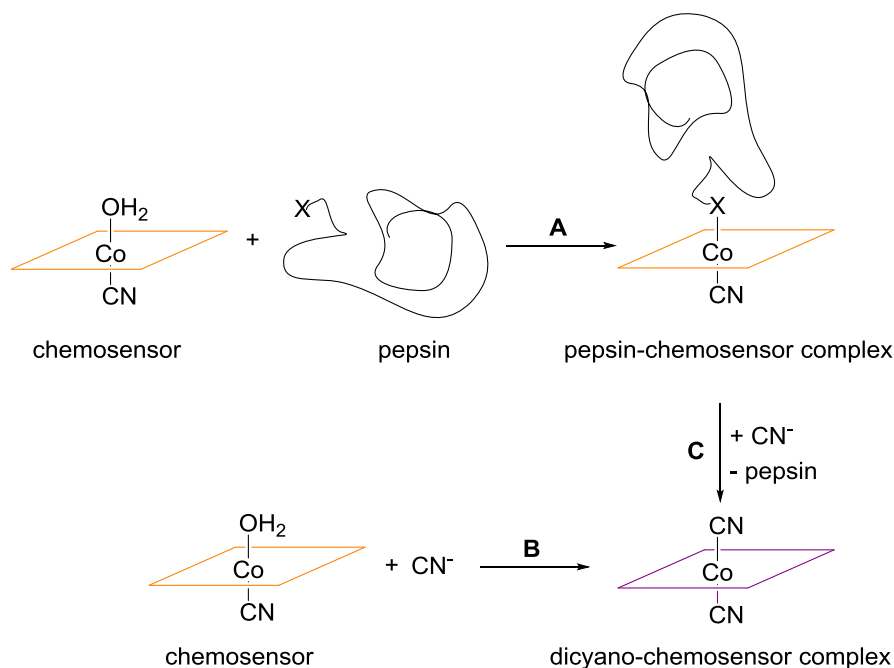


Figure 2. Proposed coordination of pepsin (A) and cyanide (B) to the chemosensor. The displacement of pepsin with cyanide from the pepsin-chemosensor complex

forming the violet coloured dicyano-chemosensor complex is shown in C (X: coordinating group).

Titration of cyanide ($[\text{CN}^-] = 0 - 160 \mu\text{mol L}^{-1}$) to these solutions led to the stepwise formation of the dicyano-form of the indicator (Figures 2, 3). This behaviour is indicated by shifts of the γ -band from 359 nm to 368 nm and of the α/β -band from 526 nm to 583 nm. These characteristic absorptions are identical with those of dicyanocobester in water.^{36, 44}

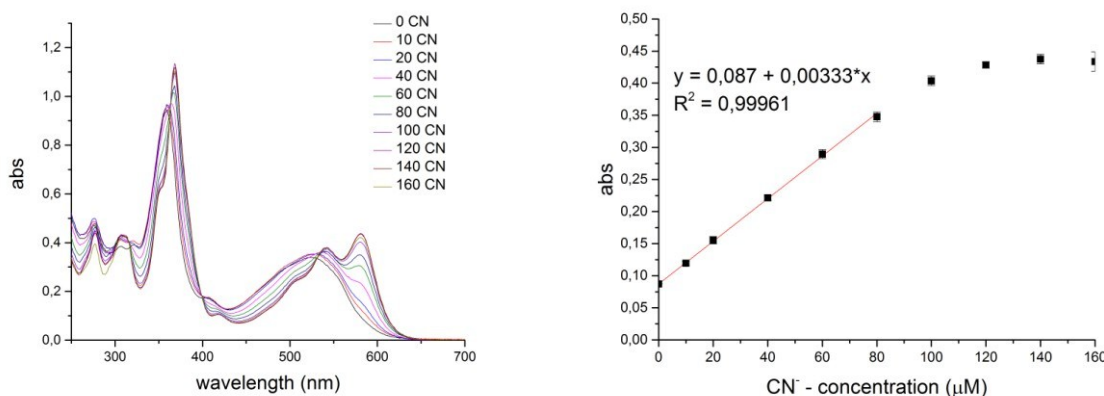


Figure 3. UV-vis spectra of cyanide spiked AGJ (*left*) (AGJ : H₂O = 1:1; V = 1 mL; [CN⁻] = 0 – 160 μmol L⁻¹, ACCbs = 42 nmol; pH 9.5) and the corresponding calibration curve (*right*).

Saturation of the chemosensor (42 μmol L⁻¹) is reached in AGJ containing solutions at ~ 110 μmol L⁻¹. This concentration is approximately twice as high as for the same experiment in pure water (pH 7.5).³⁶ This difference can be rationalized by the competitive binding of pepsin to the chemosensor (Figure 2A) that makes coordination of cyanide more challenging (Figure 2C) compared to the reaction of cyanide with the 'free' chemosensor (Figure 2B).

After having established the detection of cyanide in AGJ under homogenous conditions, we evaluated the possibility to combine the corrin-based chemosensors with solid phase extraction.^{24, 26, 27, 45} For this purpose, the reagent was added to a cyanide spiked AGJ sample and extracted afterward on the top of a commercially available reverse phase extraction column as described in the experimental section. The chemosensor is thereby trapped on the top of the C18ec column and is visible as a coloured ring. Depending on the concentration of cyanide, its colour varies between orange (aquacyano-form) and violet (dicyano-form).^{27, 36} For quantitative determinations, the reagent was subsequently eluted from the column with MeOH and analysed with UV-vis spectroscopy. The spectra unambiguously indicate a shift of the chemosensor ($\lambda_{\gamma\text{-band}} = 359 \text{ nm}$; $\lambda_{\alpha/\beta\text{-band}} = 526 \text{ nm}$) to its dicyano-form ($\lambda_{\gamma\text{-band}} = 368 \text{ nm}$; $\lambda_{\alpha\text{-band}} = 583 \text{ nm}$) with increasing concentrations of cyanide (Figure 4 *right*). Simultaneously, strongly pronounced increases in absorbance are observed. For

example, the intensity of the γ -band increases 2.4 times during titrations (Figure 4 right), whereas it changes solely by $\sim 20\%$ in the same experiment under homogenous conditions (Figure 3 left). This behaviour has been observed earlier and is explained by the more efficient extraction of the neutral dicyano-compound compared to the more polar positively charged aquacyano-form during SPE.²⁴ The corresponding calibration curve for cyanide shows a linear range up to $120 \mu\text{mol L}^{-1}$ (Figure 4).

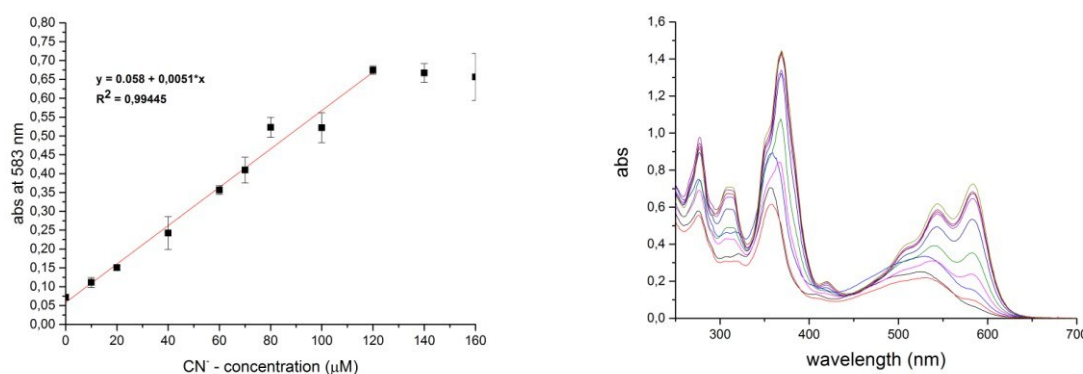


Figure 4. Calibration curve of cyanide in AGJ ($V = 0.5 \text{ mL}$) obtained by plotting the absorbance at 583 nm vs. cyanide ($[\text{CN}^-] = 0 - 160 \mu\text{mol L}^{-1}$, ACCbs = 42 nmol; $n = 3$) (left). The corresponding UV-vis spectra are shown on the right.

Having demonstrated that cyanide detection is possible in AGJ with corrin-based chemosensors, we studied potential influences of incubation times and modes of sample storage.

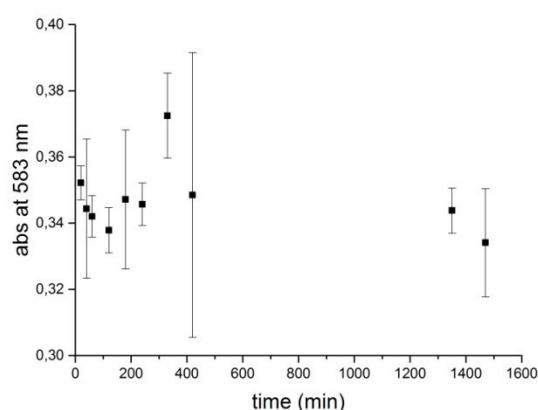


Figure 5. Absorptions at 583 nm versus spiking times ($t = 15 - 1470 \text{ min}$; $V = 0.5 \text{ mL}$, $[\text{CN}^-] = 40 \mu\text{mol L}^{-1}$, ACCbs = 42 nmol; $n = 3$)

Cyanide spiked samples of AGJ were stored at room temperature for up to 24 hours and analysed at different time intervals. No significant deviations were observed indicating that 'free' cyanide is sufficiently stable in AGJ under these conditions

(Figure 5). Storage at $-21\text{ }^{\circ}\text{C}$ was also tested ($t = 24 - 1320\text{ h}$). In this series of experiments, the detectable amount of cyanide dropped by $29 \pm 5\%$ after one week of storage (data not shown). Surprisingly, longer storage times did not show any additional negative effect and cyanide can be still detected in AGJ with corrin-based chemosensors and SPE after 55 days of storage at $-21\text{ }^{\circ}\text{C}$.

After having established the corrin-based SPE method for cyanide detection in AGJ, the system was tested in a proof-of-concept forensic study. An anonymous sample from a suicide case, in which the victim had swallowed a solution of potassium cyanide, was evaluated. In contrast to the colorless AGJ sample, the human gastric juice sample (HGJ) was slightly reddish indicating the presence of additional, unknown components. Samples of HGJ were therefore first tested with SPE to avoid any undesired colour interferences from the HGJ sample.²⁷ Indeed, a clear color change of the chemosensor from orange to violet was observed while testing the HGJ samples (Figure 6 left). This behaviour suggests the presence of free cyanide in the HGJ sample as supported by UV-Vis spectroscopy after eluting the reagent from the column (Figure 6 right). The absorbance spectrum of the eluted compound indicated unambiguously coordination of cyanide to the chemosensor generating its corresponding dicyano-form.³⁶ Quantification of cyanide in HGJ was then performed with the help of the previously established calibration curve (Figure 4).

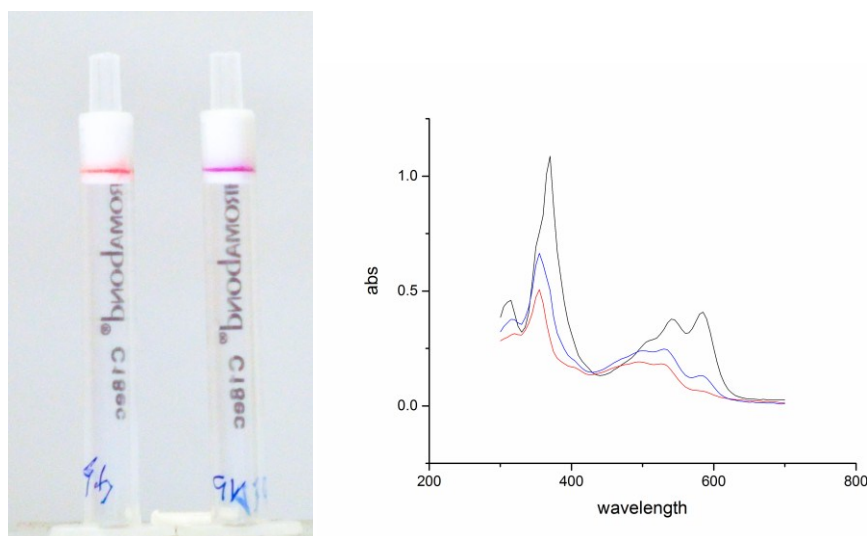


Figure 6. Left: Detection of cyanide in an HGJ sample using corrin-based chemosensors (ACCbs = 42 nmol) and SPE. Negative control (left column) and a diluted HGJ sample (dilution factor: 88; right column) Right: UV-vis spectrum after elution of the chemosensor with MeOH from the solid support (orange: negative control, blue: dilution factor 1052; olive-green: dilution factor 88).

The analysis of a 267 times diluted HGJ sample indicated a cyanide concentration of $11900 \pm 900\text{ }\mu\text{mol L}^{-1}$. This result is in very good agreement with an independent

1
2
3 microdiffusion assay using barbituric acid/ pyridine as reagent.⁴¹ This assay showed
4 a cyanide concentration of $\sim 10800 \pm 100 \mu\text{mol L}^{-1}$ in HGJ of the suicide victim. Apart
5 from this quantitative accordance, it is important to note that cyanide was still
6 detected by `naked-eye` in a ~ 1000 times diluted sample with corrin-based
7 chemosensors and SPE.
8
9

10
11 In another set of experiments, we tested whether the extraction step of the
12 chemosensor from the HGJ sample could be omitted and tried to directly determine
13 the concentration of cyanide in HGJ with the corrin-based reagent. However,
14 although the formation of the corresponding dicyano-form of the chemosensor could
15 be easily detected in the diluted HGJ sample (dilution factor: 969), quantification led
16 to larger deviations compared to the SPE technique. For example, we calculated a
17 cyanide concentration in HGJ of $16100 \pm 800 \mu\text{mol L}^{-1}$ instead of $\sim 11000 \mu\text{mol L}^{-1}$.
18 Apparently, the calibration curve generated from cyanide spiked AGJ (Figure 3)
19 cannot be used for this experimental set-up. Indeed, we demonstrated in this
20 publication that the overestimation can be avoided by separating the reagent from
21 the HGJ sample with SPE. This behaviour suggests the existence of additional
22 (unknown) interferents in HGJ compared to AGJ that are removed during washings
23 (see experimental part) with the SPE technique.
24
25
26
27
28

29
30 To the best of our knowledge, this technical note describes the unprecedented
31 detection of cyanide in HGJ with chromogenic chemosensors. In particular, the
32 results obtained with corrin-based chemosensor and SPE method are in very good
33 agreement with the microdiffusion assay using barbituric acid/ pyridine as reagent.
34 However, the SPE method is advantageous in terms of sample preparation and
35 speed of detection. In particular, only the conditioning of the column and sample
36 dilution is required. Admittedly, only one authentic human sample was studied so far,
37 but the results are encouraging for further studies in order to establish the system for
38 routine forensic investigations. These efforts would greatly benefit from the
39 simultaneous rapid detection of cyanide in authentic human blood samples and
40 corresponding forensic studies are planned for the future.
41
42
43
44
45
46
47

48 **4. Conclusions**

49
50 The detection of cyanide in artificial as well as authentic human gastric juice samples
51 using corrin-based chemosensors and SPE extraction is described. The influence of
52 spiking times and modes of storage were evaluated. It has been demonstrated that
53 rapid, straightforward qualitative yes/ no evaluations by `naked eye` is possible for
54 concentrations of cyanide in HGJ as low as $10 \mu\text{mol L}^{-1}$. Quantitative measurements
55 are in very good agreement with an independent microdiffusion assay using
56 barbituric acid/ pyridine as reagent. The SPE test-kit is therefore expected to
57 complement existing current methods, especially when rapid qualitative and
58 quantitative analyses of cyanide in HGJ are required.
59
60


Acknowledgements

The authors thank the University of Zurich for financial support and DSM Nutritional Products Basel for a generous gift of vitamin B₁₂.

1. E. P. Randviir and C. E. Banks, *Trends Anal. Chem.*, 2015, **64**, 75-85.
2. A. E. Lindsay, A. R. Greenbaum and D. O'Hare, *Anal. Chim. Acta*, 2004, **511**, 185-195.
3. S. I. Baskin and T. G. Brewer, *Medical Aspects of Chemical and Biological Warfare*, TMM Publications, Washington DC, 1997.
4. F. Zelder and R. Alberto, in *The Porphyrin Handbook*, eds. K. M. Kadish, K. M. Smith and R. Guilard, Elsevier Science, San Diego, 2012, vol. 25, pp. 83-130.
5. M. Panda and N. C. Robinson, *Biochemistry-Us*, 1995, **34**, 10009-10018.
6. J. Hamel, *Crit. Care Nurse*, 2011, **31**, 72-82.
7. *Background document for development of WHO Guidelines for Drinking-water Quality*, World Health Organization, Geneva, Switzerland, 2007.
8. H. M. Marques, K. L. Brown and D. W. Jacobsen, *J. Biol. Chem.*, 1988, **263**, 12378-12383.
9. Y. Alarie, *Crit. Rev. Toxicol.*, 2002, **32**, 259-289.
10. J. A. Ma and P. K. Dasgupta, *Anal. Chim. Acta*, 2010, **673**, 117-125.
11. F. H. Zelder and C. Männel-Croisé, *Chimia*, 2009, **63**, 58-62.
12. L. G. Nandi, C. R. Nicoletti, I. C. Bellettini and V. G. Machado, *Anal. Chem.*, 2014, **86**, 4653-4656.
13. J. Lv, Z. J. Zhang, J. D. Li and L. R. Luo, *Forensic Sci. Int.*, 2005, **148**, 15-19.
14. P. Dumas, G. Gingras and A. LeBlanc, *J. Anal. Tox.*, 2005, **29**, 71-75.
15. G. Frison, F. Zancanaro, D. Favretto and S. D. Ferrara, *Rapid Commun. Mass Spectrom.*, 2006, **20**, 2932-2938.
16. P. Boadas-Vaello, E. Jover, J. Llorens and J. M. Bayona, *J. Chromatogr. B*, 2008, **870**, 17-21.
17. R. Jackson, R. P. Oda, R. K. Bhandari, S. B. Mahon, M. Brenner, G. A. Rockwood and B. A. Logue, *Anal. Chem.*, 2014, **86**, 1845-1852.
18. S. Jermak, B. Pranaityte and A. Padaruskas, *Electrophoresis*, 2006, **27**, 4538-4544.
19. L. Meng, X. Liu, B. Wang, G. J. Shen, Z. Q. Wang and M. Guo, *J. Chromatogr. B*, 2009, **877**, 3645-3651.
20. K. Minakata, H. Nozawa, K. Gonmori, M. Suzuki and O. Suzuki, *Anal. Chim. Acta*, 2009, **651**, 81-84.
21. C. Zhang, H. Zheng, J. Ouyang, S. Feng and Y. E. C. Taes, *Anal. Lett.*, 2005, **38**, 247-256.
22. B. Desharnais, G. Huppe, M. Lamarche, P. Mireault and C. D. Skinner, *Forensic Sci. Int.*, 2012, **222**, 346-351.
23. H. A. Schwertner, S. Valtier and V. S. Bebarta, *J. Chromatogr. B*, 2012, **905**, 10-16.
24. C. Männel-Croisé and F. Zelder, *Anal. Methods*, 2012, **4**, 2632-2634.
25. N. Kumari, S. Jha and S. Bhattacharya, *Chem. - Asian J.*, 2014, **9**, 830-837.
26. C. Männel-Croisé, B. Probst and F. Zelder, *Anal. Chem.*, 2009, **81**, 9493-9498.
27. C. Männel-Croisé and F. Zelder, *ACS Appl. Mat. Interf.*, 2012, **4**, 725-729.
28. M. T. Chaudhary, M. Sarwar, A. M. Tahir, M. A. Tahir, G. Mustafa, S. A. Wattoo, M. Imran and A. Subhani, *Aust. J. Forensic Sci.*, 2015, 1-8.
29. F. Zelder, *Chem. Commun.*, 2015, **51**, 14004-14017.
30. F. Zelder and L. Tivana, *Org. Biom. Chem.*, 2015, **13**, 14-17.
31. P. K. Dasgupta, J. Ma, S. I. Ohira, S. K. Mishra, M. Puanggam, S. B. Mahon, M. Brenner, W. Blackledge and G. R. Boss, *Anal. Chem.*, 2011, **83**, 4319-4324.
32. L. A. Greenawald, J. L. Snyder, N. L. Fry, M. J. Sailor, G. R. Boss, H. O. Finklea and S. Bell, *Sens. Actuators, B*, 2015, **221**, 379-385.

- 1
2
3 33. W. C. Blackledge, C. W. Blackledge, A. Griesel, S. B. Mahon, M. Brenner, R. B. Pilz and G. R.
4 Boss, *Anal. Chem.*, 2010, **82**, 4216-4221.
5
6 34. F. H. Zelder, *Inorg. Chem.*, 2008, **47**, 1264-1266.
7 35. C. Männel-Croisé, C. Meister and F. Zelder, *Inorg. Chem.*, 2010, **49**, 10220-10222.
8 36. C. Männel-Croisé and F. Zelder, *Inorg. Chem.*, 2009, **48**, 1272-1274.
9 37. J. Ma, P. K. Dasgupta, F. H. Zelder and G. R. Boss, *Anal. Chim. Acta*, 2012, **736**, 78-84.
10 38. C. Männel-Croisé and F. Zelder, *Chem. Commun.*, 2011, **47**, 11249-11251.
11 39. K. A. Gaither, B. J. Tarasevich and S. C. Goheen, *J. Biomed. Mater. Res. B. Appl. Biomater.* ,
12 2009, **91B**, 135-142.
13 40. L. Werthemann, *PhD thesis*, ETHZ (Switzerland), Zurich, 1968.
14 41. A. C. Moffatt, *Clarke's isolation and identification of drugs*, Pharmaceutical Press, London,
15 1986.
16 42. W. R. Bauriedel, J. C. Picken and L. A. Underkofler, *Proc. Soc. Exp. Biol. Med.*, 1956, **91**, 377-
17 381.
18 43. E. L. Lien and J. M. Wood, *Biochim. Biophys. Acta*, 1972, **264**, 530-537.
19 44. L. Tivana, J. Da Cruz Francisco, F. Zelder, B. Bergenstahl and P. Dejmek, *Food. Chem.*, 2014,
20 **158**, 20-27.
21 45. C. Aebersold and F. Zelder, *Anal. Methods*, 2015, **7**, 5712-5713.
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

Graphical Abstract

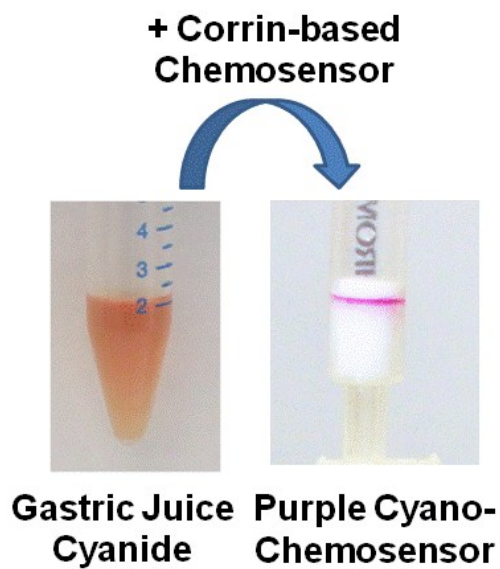

This Technical Note describes the detection of cyanide in artificial gastric juice with corrin-based chemosensors. The application of this method in authentic human samples is demonstrated in a proof-of-principle forensic investigation.