



CrossMark
click for updates

Cite this: *RSC Adv.*, 2015, 5, 62585

DOI: 10.1039/c5ra90070k

www.rsc.org/advances

Correction: Paper-based molecular diagnostic for *Chlamydia trachomatis*

Jacqueline C. Linnes,^a Andy Fan,^a Natalia M. Rodriguez,^a Bertrand Lemieux,^b Huimin Kong^b and Catherine M. Klapperich^{*a}

Correction for 'Paper-based molecular diagnostic for *Chlamydia trachomatis*' by Jacqueline C. Linnes *et al.*, *RSC Adv.*, 2014, 4, 42245–42251.

The authors apologise for the errors in the caption of Fig. 1 in the original manuscript. The correct figure and caption are as follows:

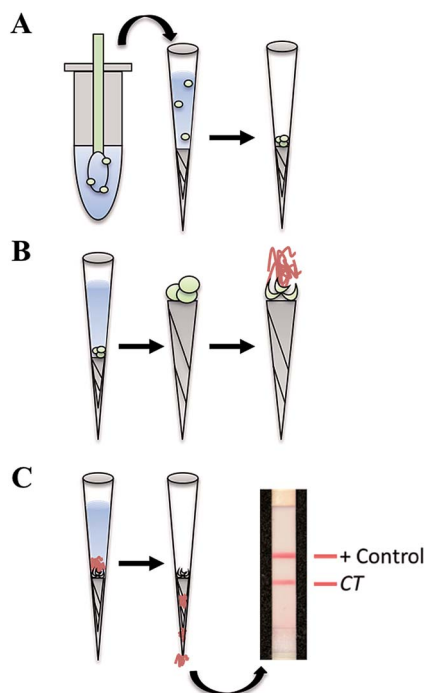


Fig. 1 Schematic of the method to perform the paper-based cell lysis, amplification, and detection. (A) Sample is added to the pipette tip and cells are filtered onto the paper support. (B) tHDA mastermix is added to the pipette tip and the tip is incubated at 65 °C to lyse cells and amplify DNA. (C) Elution buffer is added to the pipette tip and the amplified DNA is eluted onto the lateral flow test.

The Royal Society of Chemistry apologises for these errors and any consequent inconvenience to authors and readers.

^aBiomedical Engineering, Boston University, Boston, MA, 02215, USA. E-mail: catherin@bu.edu; Fax: +1-617-353-6766; Tel: +1-617-358-0253

^bBioHelix Corporation, Beverly, MA, 01915, USA

