



Cite this: *RSC Adv.*, 2018, 8, 14377

Characterization of aluminum, aluminum oxide and titanium dioxide nanomaterials using a combination of methods for particle surface and size analysis†

B. Krause,^a T. Meyer,^b H. Sieg,^c C. Kästner,^d P. Reichardt,^a J. Tentschert,^a H. Jungnickel,^a I. Estrela-Lopis,^b A. Burel,^e S. Chevance,^f F. Gauffre,^f P. Jalili,^g J. Meijer,^h L. Böhmert,^c A. Braeuning,^c A. F. Thünemann,^d F. Emmerling,ⁱ V. Fessard,^g P. Laux,^a A. Lampen^c and A. Luch^a

The application of appropriate analytical techniques is essential for nanomaterial (NM) characterization. In this study, we compared different analytical techniques for NM analysis. Regarding possible adverse health effects, ionic and particulate NM effects have to be taken into account. As NMs behave quite differently in physiological media, special attention was paid to techniques which are able to determine the biosolubility and complexation behavior of NMs. Representative NMs of similar size were selected: aluminum (Al⁰) and aluminum oxide (Al₂O₃), to compare the behavior of metal and metal oxides. In addition, titanium dioxide (TiO₂) was investigated. Characterization techniques such as dynamic light scattering (DLS) and nanoparticle tracking analysis (NTA) were evaluated with respect to their suitability for fast characterization of nanoparticle dispersions regarding a particle's hydrodynamic diameter and size distribution. By application of inductively coupled plasma mass spectrometry in the single particle mode (SP-ICP-MS), individual nanoparticles were quantified and characterized regarding their size. SP-ICP-MS measurements were correlated with the information gained using other characterization techniques, *i.e.* transmission electron microscopy (TEM) and small angle X-ray scattering (SAXS). The particle surface as an important descriptor of NMs was analyzed by X-ray diffraction (XRD). NM impurities and their co-localization with biomolecules were determined by ion beam microscopy (IBM) and confocal Raman microscopy (CRM). We conclude advantages and disadvantages of the different techniques applied and suggest options for their complementation. Thus, this paper may serve as a practical guide to particle characterization techniques.

Received 8th January 2018
 Accepted 22nd March 2018

DOI: 10.1039/c8ra00205c

rsc.li/rsc-advances

Introduction

The specific properties of NMs depend on their physicochemical characteristics. Optical properties build upon the size, the shape and the surface structure,^{1,2} while higher reactivity, for example,

may result from a high surface area,^{3,4} specific surface coatings⁵ or a surface charge.^{6–8} An important factor for increasing their activity is the self-assembly of NMs. Here, NMs associate *via* non-covalent interactions resulting in organized structures of higher-order. Different applications based on advanced functions were

^aGerman Federal Institute for Risk Assessment (BfR), Department of Chemical and Product Safety, Max-Dohrn-Straße 8-10, 10589 Berlin, Germany. E-mail: benjamin-christoph.krause@bfr.bund.de

^bInstitute of Medical Physics and Biophysics, University of Leipzig, Härtelstrasse 16-18, 04275 Leipzig, Germany

^cGerman Federal Institute for Risk Assessment (BfR), Department of Food Safety, Max-Dohrn-Straße 8-10, 10589 Berlin, Germany

^dFederal Institute for Materials Research and Testing (BAM), Unter den Eichen 87, 12205 Berlin, Germany

^eMRIC TEM BIOSIT, Université de Rennes 1, 2 av pro Leon Bernard, France

^fUniv Rennes, CNRS, ISCR UMR6226, F-35000 Rennes, France

^gANSES, French Agency for Food, Environmental and Occupational Health and Safety, Fougères Laboratory, 10B rue Claude Bourgelat, 35306, Fougères Cedex, France

^hFelix Bloch Institute for Solid State Physics, Faculty of Physics and Geosciences, Division of Nuclear Solid State Physics, University of Leipzig, Linnéstraße 5, 04103 Leipzig, Germany

ⁱFederal Institute for Materials Research and Testing (BAM), Richard-Willstätter-Straße 11, 12489 Berlin, Germany

† Electronic supplementary information (ESI) available: NTA size distributions for Al⁰, Al₂O₃, NM103, NM104, DLS number-based distribution for Al⁰, Al₂O₃, NM103, NM104, TEM measurement of TiO₂ NMs in DMEM, SAXS data for Al⁰, Al₂O₃ and AlCl₃ in BSA and DMEM after 24 and 48 h, impurities of used NMs determined by IBM, aluminium aqua complexes at different pH values, CRM surface investigations, colocalization pattern by IBM for Al₂O₃, CRM spectra displaying protein modifications, ToF-SIMS measurements of Al and Al₂O₃ NMs in DMEM, ToF-SIMS measurements of TiO₂ NMs in DMEM. See DOI: 10.1039/c8ra00205c



reported, for example formation of mesoporous TiO₂ mediated by ionic liquids for solar cell conversion, catalysis or electronic devices.^{9–11} Another application is the self-assembly of biomolecules, like lipids and proteins, mediating inner-particle mesoporosity in a macroporous TiO₂ structure.¹²

TiO₂ NMs are classified as granular biodurable particles (GBPs) of low toxicity.¹³ They occur in the form of anatase or rutile as well as in mixtures thereof. While significant accumulation was shown in the liver of rats in the case of orally administered TiO₂ NMs,¹⁴ this was different in studies with Al⁰ NMs in mice, in which predominant accumulation in the brain, thymus and lung was revealed.¹⁵ Characterization is important for both *in vitro* and *in vivo* studies. Currently, the human health risk assessment of NMs is mainly based on *in vivo* experiments in rodents.^{16,17} However, due to the high number of new NMs,¹⁸ it is not ethical or feasible to conduct such studies for each individual NM. On the other hand, *in vitro* systems proved useful, e.g. to generate high throughput data.¹⁹ Extrapolation to the *in vivo* situation remains limited, in particular due to the insufficient comparability of applied dose and particle biotransformation.^{20,21} An accurate characterization of NMs in *in vitro* systems by the application of up-to-date analytical methods may therefore help to establish reliable methods for determination of nanomaterial uptake and translocation as key parameters that affect NM-related toxicity. Such an approach would therefore help to reduce the number of materials that need to be subjected to animal testing. We investigated rather soluble Al⁰ and rather insoluble Al₂O₃ and TiO₂ NMs (Fig. 1).

This classification is important for NMs because even the same chemical composition can exhibit differences in physicochemical properties. Compared to bulk material, variations are much higher for NMs.^{22,23}

For the characterization of test materials, we applied a combination of techniques based on different measuring principles. With DLS as intensity-weighted method, we assessed the hydrodynamic diameter and the polydispersity of the materials in aqueous suspensions and cell culture media (CCM). To validate the results, the more reliable, number-based approach of NTA was applied. The two methods, DLS and NTA, were performed in two different laboratories, allowing for a direct comparison of the results achieved. For particle surface

investigation, XRD was used to test whether the aluminum was already oxidized. The core diameter of Al⁰, Al₂O₃ and both TiO₂ NMs was measured by SP-ICP-MS. These results were compared to TEM measurements. As a further technique for estimation of the core diameter, SAXS was applied. Additionally, IBM and CRM were performed to analyze the interaction of NMs with biomolecules as well as to quantify impurities in the NM composition. ToF-SIMS is capable of visualizing the formation of complexes out of Al⁰ and Al₂O₃ NMs with components of the environmental media. This allows investigation of the behavior of NMs within physiological fluids such as CCM.

With respect to uptake, the dissolution of NMs in different media is of high importance. For example, during an artificial digestion procedure, different pH values, as well as proteins, enzymes and other compounds, mimic the oral uptake route for NMs. For Al⁰ and Al₂O₃ NMs, an increased dissolution within the gastric environment was noticed.²⁴ However, to properly interpret and compare the results, precise knowledge of the properties of the starting materials and of their state in CCM is required. Although there are a lot of studies dealing with silver and copper-containing NMs and their dissolution behavior in biological media,^{25–27} to our knowledge, no study accounts for Al⁰ NMs. Furthermore, the dissolution behavior of aluminum-containing nanomaterials may be very different since aluminum ions already have a different complexation behavior compared to silver or copper ions. By means of the methods described earlier (Fig. 2), we were able to obtain valuable information to hypothesize the behavior of NMs in biological media and to extrapolate to the *in vivo* situation. With these assumptions, it is much easier to understand and explain future data resulting from more complex scenarios.

Experimental

Materials and methods

Al⁰ NMs (mean diameter 18 nm (TEM), 99.9%) and Al₂O₃ NMs (mean diameter 20 nm (TEM), 99+%) were purchased from IoLiTec Ionic Liquids Technologies GmbH, Heilbronn, Germany. TiO₂ NMs (NM103 and NM104, mean diameter 25 nm (TEM)) were purchased from JRC Joint Research Centre, Ispra, Italy. Bovine serum albumin (BSA) was bought from Sigma Aldrich. CCM (DMEM, high glucose (4.5 g l⁻¹), with sodium pyruvate; with L-glutamine; with 1% penicillin/streptomycin (P/S)) and fetal bovine serum were purchased from PAA Laboratories GmbH, Paching, Austria. All other chemicals used in this study were reagent grade.

Sample preparation

NM dispersions were prepared following the NanoGenoTOX dispersion protocol “Final protocol for producing suitable manufactured NMs exposure media” (October 2011).²⁸

For cell culture experiments, stock dispersions of NMs were diluted in DMEM with 10% fetal calf serum (FCS) to either 10 or 100 μg ml⁻¹.

For ion release testing, stock dispersions were diluted in 0.05% BSA to 100 and 10 μg ml⁻¹ to reflect a high and a low

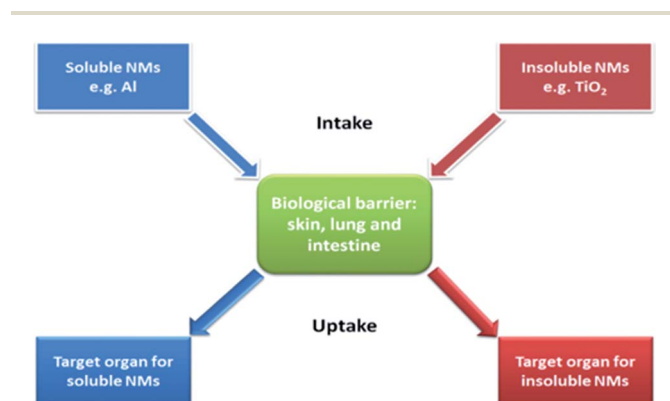


Fig. 1 Hypothesis of different behavior of soluble and insoluble NMs after uptake.



concentration used in cell culture experiments. 1 ml was taken and centrifuged at $16000 \times g$ for 1 h (Hettich Zentrifuge Mikro 220R). 500 μl of the supernatant were taken, 750 μl of HNO_3 (69%) were added and Millipore water was used to fill up to 15 ml.

For IBM and CRM, NMs were centrifuged at $8000 \times g$ for 10 min, supernatant was taken away, mpH_2O was added and the sample was vortexed. The procedure was repeated 3 times. Finally, a small drop of the sample was given on polypropylene foil for IBM and on quartz glass for CRM. The dry samples were measured.

Dynamic light scattering measurements

The distributions of the hydrodynamic diameters of the NMs were determined using a Malvern Nano ZS (Malvern Inc., UK) or a Brookhaven ZetaPALS (Brookhaven Instruments Corporation,

USA). A stock dispersion (2.56 mg ml^{-1} in 0.05% BSA) was diluted to the concentration of $100 \mu\text{g ml}^{-1}$. The NM dispersions in 0.05% BSA as well as in DMEM were analyzed 5–10 min after preparation. Thermal equilibration time was set to 60 s at 25°C . Each intensity-weighted size distribution represents the average of six individual DLS analyses, three replicates and at least three independent experiments using automatic optimization of analytical conditions and data treatment by general purpose size analysis.

Nanoparticle tracking analysis measurements

NTA measurements were performed with a NanoSight LM20 and LM10 (NanoSight, Amesbury, UK), equipped with a 632 nm laser or 532 nm laser. The samples were injected into the sample chamber with sterile syringes. All measurements were performed at room temperature. The samples were diluted to a final concentration of approx. 10^8 particles per ml with mpH_2O , depending on the NMs and media. The software used for recording and analyzing the data was NTA 2.3 and NTA 3.0. All samples were measured for 60 s at five positions. All measurements were performed with at least three independent experiments.

X-ray diffraction measurements

The XRD measurements were achieved on powder samples using a D5000 diffractometer (Siemens AG, Munich, Germany) in Bragg Brentano geometry. A linear detector, a curved $\text{Ge}(111)$ monochromator and $\text{Cu K}\alpha$ radiation ($\lambda = 0.1542 \text{ nm}$) were used. The analysis was performed over the 2θ range of 10 to 90° and at a step size of 0.02° and scanning speed of 2° per step. The experiments were carried out independently three times.

Single particle ICP-MS measurements

For single particle analysis of the NM solutions, a quadrupole ICP-MS (Thermo Scientific XSERIES II, Thermo Fisher Scientific, Waltham, MA, USA) with a PFA ST Nebulizer, a quartz cyclonic spray chamber and a 2.5 mm quartz O-ring-free injector (all from ESI Elemental Service & Instruments GmbH, Mainz, Germany) were used. Using the time-resolved analysis (TRA) mode for data acquisition, intensities as a function of time (counts per dwell-time interval) were collected. The acquisition time for each run was set to 60 s with a dwell time (or data acquisition rate) of 3 ms. The gas flow for the plasma, the nebulizer and the auxiliary (all Ar) was set to 13 l min^{-1} , 0.89 l min^{-1} and 0.7 l min^{-1} respectively. The flow rate of the sample was 0.34 ml min^{-1} . Data were exported to a spreadsheet for further processing. For data processing, an established procedure according to Pace *et al.*²⁹ was followed. Determination of nebulizer efficiency was performed using a described method with reference nanoparticles of known particle size.²⁹ 60 nm gold reference nanoparticles from the U.S. National Institute of Standards and Technology (NIST, RM 8013) were used as reference nanoparticles.

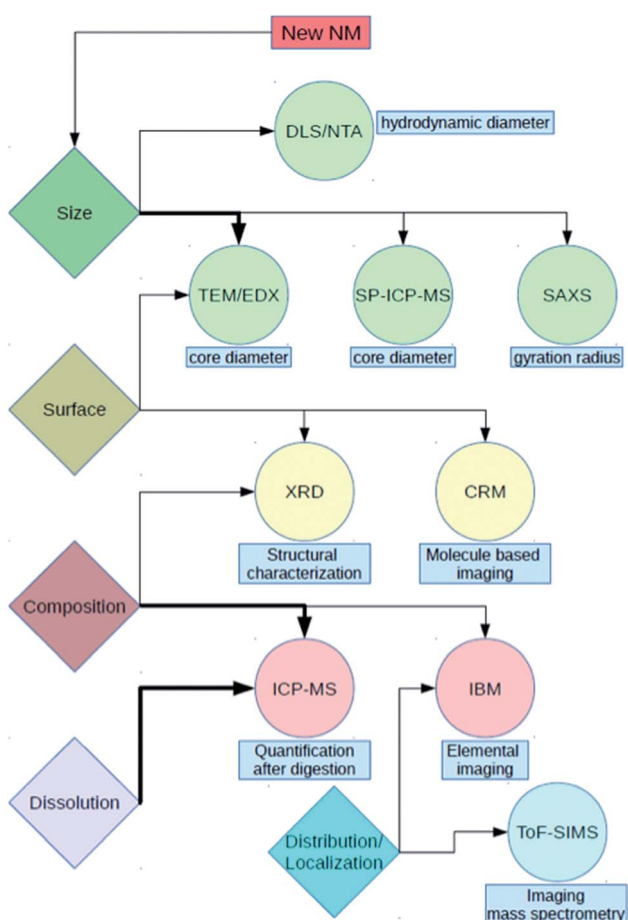


Fig. 2 Overview of key NM characteristics (colored rhombi) and methods (colored circles) used in this study for characterization. Arrows in bold imply the main method for the linked characteristic. Abbreviations: DLS – dynamic light scattering; NTA – nanoparticle tracking analysis; TEM – transmission electron microscopy; EDX – energy dispersive X-ray spectroscopy; SP-ICP-MS – single particle inductively coupled plasma mass spectrometry; SAXS – small angle X-ray scattering; XRD – X-ray diffraction; CRM – confocal Raman microscopy; ICP-MS – inductively coupled plasma mass spectrometry; IBM – ion beam microscopy; ToF-SIMS – time of flight mass spectrometry.



Small angle X-ray scattering measurements

The measurements were conducted in a flow-through capillary with a Kratky-type instrument (SAXSess, Anton Paar, Austria) at 21 ± 1 °C. The SAXSess has a low sample-detector distance of 0.309 m. Deconvolution of the SAXS curves was carried out with the SAXS-Quant software. Curve fitting was performed with the McSAS software (Monte Carlo method, version 1.0.1). The experiments were performed with 120 measurement cycles (each averaged over 10 s). NMs and controls were dispersed according to NanoGenoTOX protocol and diluted into DMEM in a sample concentration of $100 \mu\text{g ml}^{-1}$. Samples were incubated for a time of 24 and 48 h at 37 °C and 5% CO_2 in a cell incubator until sample injection. Stock dispersions were injected directly after ultrasonication.

Ion beam microscopy

Label-free IBM measurements were performed with the LIPSION Nanoprobe. A 2.25 MeV proton beam was applied by a SingletronTM particle accelerator. A vacuum with a pressure of 5×10^{-5} to 10^{-7} torr was applied and the beam was focused to a spot size of around 1 μm . For spatial resolved element analysis, micro proton induced X-ray emission (μPIXE) and micro Rutherford backscattering spectroscopy (μRBS) were recorded simultaneously. The μPIXE detector (Canberra, Meriden, CT, USA) consists of a high-purity Ge crystal covered with a 60 μm polyethylene layer, which covers the detector for backscattered protons. μRBS spectra were detected by a Canberra PIPS detector.

Confocal Raman microscopy

Spectroscopic analysis of NMs was performed by CRM. A Witec alpha300 confocal Raman spectrometer (Witec GmbH, Germany) with a 532 nm laser with 30 mW power was used. Control4.1 (Witec GmbH, Germany) software was used to record and analyze the spectra. The spectra were recorded at an integration time of 0.15 s per point and with a step size of 250 nm.

Transmission electron microscopy

The samples were deposited on a 400-mesh copper grid. The grids were prepared by sample adsorption and left free-standing on top of a 0.8 mg ml^{-1} solution of NMs for 20 s. Excess solution was removed by placing the grid on a filter paper and the sample was dried for 24 h. For samples in DMEM, the grid was washed by dipping the grid in a droplet of water before. Examination was performed with a JEOL 1400 transmission electron microscope, equipped with a tungsten filament and supplied with GATAN Orius 1000 camera. TEM operated at 80 kV (DMEM) or at 120 kV with magnification of $200\,000\times$.

Time-of-flight mass spectrometry

Ion images and spectra were acquired using a ToF-SIMS V instrument (ION-TOF GmbH, Münster, Germany) with a 30 keV nano-bismuth primary ion beam source ($[\text{Bi}]_x^{(q+)}$ -cluster ion source with a BiMn emitter). The ion currents were 0.5 pA at 5 kHz using a Faraday cup. A pulse of 0.7 ns from the bunching

system resulted in a mass resolution that usually exceeded 6000 (full width at half-maximum) at $m/z < 500$ in positive ion mode. The primary ion dose was controlled below 10^{12} ions cm^{-2} to ensure static SIMS conditions. Charge compensation on the sample was obtained by a pulsed electron flood gun with 20 eV electrons.

The primary ion gun scanned a field of view of $500 \mu\text{m} \times 500 \mu\text{m}$ applying a 512×512 pixel measurement raster. Once the primary ion gun was aligned, a ToF-SIMS mass spectrum was generated by summing the detected secondary ion intensities and plotting them against the mass channels. The data were evaluated using the Surface Lab software (ION-TOF GmbH, Münster, Germany).

Results and discussion

We point to the advantages and disadvantages of the methods used and explain whether or not methods can provide complementary results to other techniques. We also analyzed possible dissolution characteristics of different matrix media (BSA and DMEM) for pristine Al^0 and oxide (Al_2O_3 and TiO_2) NMs. Characterization data already published on TiO_2 were retrieved according to JRC report.³⁰ In conclusion, we will present data where the dissolution of NMs in complex media has an impact on particle media interactions. These results were obtained by ToF-SIMS and show the efficiency of that method for obtaining insights into elemental compositions with TEM, IBM, CRM and ToF-SIMS. An overview about the main characterization techniques and their limits is given in Table 3.

A very common and frequently used method for determining the size distribution and polydispersity of NMs in solution is DLS. Fast and easy sample preparation as well as quick measurement give rapid initial indications of the sample. NTA is more appropriate for evaluating polydisperse samples with

Table 1 Z-averages with standard deviation (SD) and polydispersity index (PDI) of Al^0 , Al_2O_3 , NM103 and NM104 NMs in different media determined by dynamic light scattering (DLS). All results represent the average of six repeats. BSA: bovine serum albumin; DMEM: Dulbecco's modified eagle medium; FCS: fetal calf serum

| DLS measurements and comparison | | | | |
|---|-----------------|-----------------|--------------------|-----------------|
| | Lab 1 (Malvern) | | Lab 2 (Brookhaven) | |
| | Z-average [nm] | PDI | Z-average [nm] | PDI |
| Stock solution (0.05% BSA in H₂O) | | | | |
| Al^0 NM | 250 ± 10 | 0.17 ± 0.01 | 270 ± 40 | 0.18 ± 0.02 |
| Al_2O_3 NM | 170 ± 10 | 0.24 ± 0.02 | 210 ± 40 | 0.21 ± 0.06 |
| NM103 | 270 ± 10 | 0.28 ± 0.05 | 610 ± 190 | 0.21 ± 0.30 |
| NM104 | 220 ± 10 | 0.26 ± 0.03 | 370 ± 90 | 0.15 ± 0.03 |
| DMEM (with 10% FCS) | | | | |
| Al^0 NM | 200 ± 10 | 0.18 ± 0.01 | 220 ± 10 | 0.21 ± 0.02 |
| Al_2O_3 NM | 70 ± 10 | 0.52 ± 0.03 | 230 ± 60 | 0.18 ± 0.07 |
| NM103 | 240 ± 20 | 0.24 ± 0.01 | 270 ± 10 | 0.25 ± 0.01 |
| NM104 | 190 ± 10 | 0.28 ± 0.02 | 230 ± 10 | 0.18 ± 0.02 |



various aggregate populations, since it is based on single particle tracking as both techniques determine the hydrodynamic diameter. Due to the fixed working ranges of DLS and NTA, the used concentration of media varies. Since NTA is a counting method, also proteins would be counted and would significantly lower the hydrodynamic diameter of the NM dispersion. Therefore, the particles, as well as the medium were diluted directly before measurement with mPH_2O to avoid agglomeration effects.

For all particles with a primary size of approximately 20 nm, a hydrodynamic diameter between 200 and 270 nm was measured by DLS in DMEM (Table 1). In contrast, different aggregate fractions of NMs in DMEM with a mean value of about 150 nm were found by means of NTA (Fig. S1†). This difference can be explained by the fact that NTA is a particle counting system, sensitive to large as well as small fractions in the sample, and DLS is an intensity-weighted system, highly responsive to the large fractions. In all cases, the NTA size distribution is asymmetrical with a steep slope on the left side (small particles) and a gentle slope on the right side, representing the fraction of agglomerates. Additionally, a calculation of number-based size distribution out of intensity-weighted DLS data was done (Table S1†).

In the case of NM103 and NM104 dispersed in 0.05% BSA water solution, a very high mean value and a large error was measured by the Brookhaven device, while NTA exhibits broad distributions with some fractions and a mean value of around 180 nm. This can be explained by unstable particle agglomerates, which are observed by the DLS.

Comparing the two DLS devices, one can observe that the Malvern DLS detects 15% smaller particles than the Brookhaven machine in 0.05% BSA water solution as well as in DMEM. This systematic deviation could be related to different detection angles of scattered intensity, 90° for Brookhaven and 173° for Malvern, since larger particles mostly scatter light at forward angles. Backscattering at 173° will not overestimate larger particles as much as measurements at 90° .

In the case of NM103 and 104 in BSA and Al_2O_3 in DMEM, the results were not consistent for the two devices. Z-averaged diffusion coefficients were calculated by applying the cumulant method, which is applicable to polydisperse and non-multimodal systems. In contrast, NTA results show the presence of different particle populations. The applied cumulant algorithms are not suitable in certain cases for getting reliable DLS results. Furthermore, it should be kept in mind that the inversion of the DLS autocorrelation function is part of a poorly formulated mathematical problem. It works quite well in the case of monodisperse or low polydisperse particles. Applications of multiangle DLS and sophisticated algorithms are thus necessary to obtain trustworthy results of NM size distributions by means of DLS.^{31,32}

Investigations on primary particle size

With the European commission's definition of a nanomaterial, that is, a nanomaterial should contain 50% or more particles in number size distribution with one or more size dimensions

between 1–100 nm, it is obviously necessary to obtain information about the primary particle size of the investigated particles. TEM as well as SAXS can be used to solve this problem.

Looking at advantages and disadvantages of TEM, the following issues should be considered. Since TEM measurements are performed under high vacuum, only dried samples are observed. For this reason, TEM is not representative of the sample in its solution state. In particular, agglomeration and coffee stain effect³³ may occur during the drying process, resulting in a non-homogeneously covered surface. Size distributions can be determined from TEM pictures by measuring the size of each particle using image analysis software.³⁴ The size of individual nanoparticles may be difficult to extract from agglomerated samples but, recently, some implementations have been proposed.³⁵ In addition, for irregular particles with ill-defined shapes, which dimension should be taken? In practice, size analysis can be time-consuming and TEM generally yields a poor statistical representation of the sample.³⁴ Electron microscopy also enables chemical and crystallographic analysis of the particles. The contrast in TEM is directly linked to the atomic number of electrons, heavier atoms giving higher contrast. This is an advantage when observing metal nanoparticles in a biological environment. However, care should be taken for mineral salts from buffers that may precipitate on the grid when drying. Aqueous washing of the grid after sample deposition might be appropriate in this case.

Fig. 3 shows the dispersion in water with 10% BSA. The shape of Al^0 NMs is globally spherical with rod-like excrescences and the primary particle size varies between 2–50 nm, which matches the manufacturer specification. The Al_2O_3 NMs are not spherical but have rather a needle-like shape. The width is about 10 nm, while the longest dimension varies a bit more between 20–50 nm. The shape of TiO_2 NM104 is rod-like, with a width of approx. 10 nm and length of 20–50 nm (Fig. S2†). Working with a more complex medium, such as CCM, was challenging for TEM analysis. However, we were able to image the particle in DMEM, with very little differences compared to BSA dispersion. Using relatively low voltage, the protein coating can be observed (see Fig. S2†).

SAXS was used for characterization of the primary particle size of NMs. SAXS allows to analyze a broader variety of different sample types than most other techniques. Compared to TEM, the samples can easily be investigated *in situ*. Additionally, SAXS provides statistically more reliable data for particle size distribution quantification since more than 10^6 particles are typically measured, in contrast to TEM, where rarely more than a few

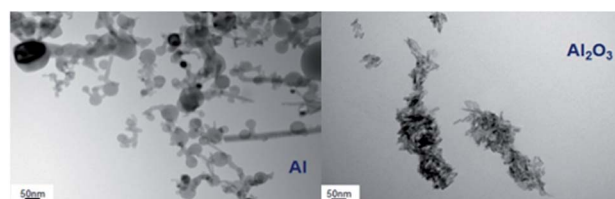


Fig. 3 Comparison of TEM pictures of Al^0 and Al_2O_3 NMs in BSA solution after applying the dispersion protocol.



hundred particles are counted. Size distribution of NMs can be quantified in the range of 1 to 100 nm if the shape is known from a complementary technique like TEM. The classical radius of gyration (Guinier radius) is accessible in any case.

In this study, we observed the size parameters of the particles in BSA as a stock solution and after addition in DMEM at different times of $t = 0$ h, 24 h and 48 h (Fig. 4). Since the particle cores scatter much stronger than the surrounding particle shell, the shell becomes practically invisible. Therefore, SAXS determines the size distribution of the core radii. The resulting distributions of the particles' stock solutions are shown in Fig. 4. Their corresponding SAXS curves are displayed in the ESI (Fig. S3–S5[†]). The accessible size range of the radii is given by the range of the scattering vector q : $R_{\min} = \pi/q_{\max}$ and $R_{\max} = \pi/q_{\min}$. In the present case of the q -range of $0.1 \text{ nm}^{-1} < q < 6 \text{ nm}^{-1}$ corresponds to radii of $30 \text{ nm} > R > 0.5 \text{ nm}$.

The Al^0 NMs showed a broad size distribution including primary particles with radii > 10 nm. Since the detection limit is 30 nm (radius) in this case, bigger aggregates cannot be detected directly. However, from the steep slope of the SAXS curve (Fig. S3[†]) at low q values, it can be assumed that bigger aggregates are present. The defined characterization of these particle aggregates has to be performed using a complementary method like TEM. The inset in Fig. 4a shows that the radii distribution of the Al^0 NMs did not change significantly either after addition in DMEM or 24 h and 48 h thereafter. In contrast to the Al^0 NMs, the Al_2O_3 NM in BSA displays a distribution which consists of small primary particles and aggregates. The sample shows an amount of 75% primary particles with a mean radius of 7.1 ± 0.5 nm. The detected aggregates display radii of > 10 nm. Upon the addition in DMEM, the radii distribution shifts slightly to higher radii of 8.4 ± 0.2 nm. These characteristics did not change significantly over the time of 48 h in DMEM.

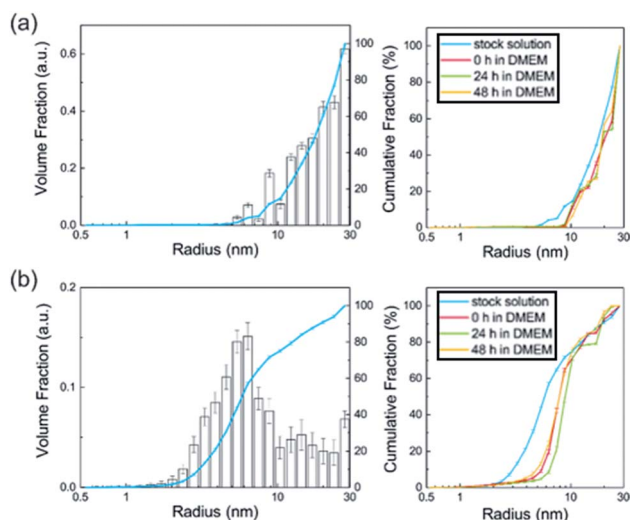


Fig. 4 Volume-weighted radii distributions of Al^0 NMs (a) and Al_2O_3 NMs (b) derived from SAXS measurements. The displayed radii distribution (right panel, black bars) and cumulative fraction presentation (blue line) correspond to the NMs in stock solution (BSA). Left panel shows particle distribution in cumulative fraction presentation at different stages: in stock solution (blue line) and in DMEM after 0 h (red line), 24 h (green line) and 48 h (orange line).

No particles were detected in the ionic control substance AlCl_3 . In contrast, immediately after addition in DMEM, nano-sized particles with sizes of 1–30 nm were observed. Since all curves are background-corrected with the respective solvent control, solvent effects can be excluded and the particles derive directly from the aluminum species. In conclusion, SAXS yields the size distribution of nanoparticles and its changes in DMEM.

SP-ICP-MS is another technique to determine primary particle sizes. The fundamental assumption behind this technique is that, at a sufficiently short dwell time and low particle number concentration, a pulse will represent a single particle event.

There is a direct correlation between the number of pulses and the number concentration of particles (particle number per volume). With the intensity of the pulse (*i.e.* height) and assumptions about the particle geometry, the particle size through particle mass can be determined.

Aside from single pulses, there is always a background, which originates from the ionic part of the analyzed sample. In addition to primary particle size, information about the dissolution rate of a NM sample can be achieved. While quantification is more difficult, a qualitative assessment of ions released can be inferred. For Al^0 , a broad distribution (Fig. 5, left) up to 200 nm is observed compared to Al_2O_3 (Fig. 5, right). This fits very well with the data obtained from TEM analysis. Compared to the Au NIST reference material, which shows almost no dissolution, a higher background for Al^0 NMs was detected, indicating potential ion release.

Particle surface – impact on dissolution in complex media

Al^0 NMs usually become quickly passivated at the surface by the formation of an oxide layer. This event is likely to change the dissolution behavior and the overall physicochemical

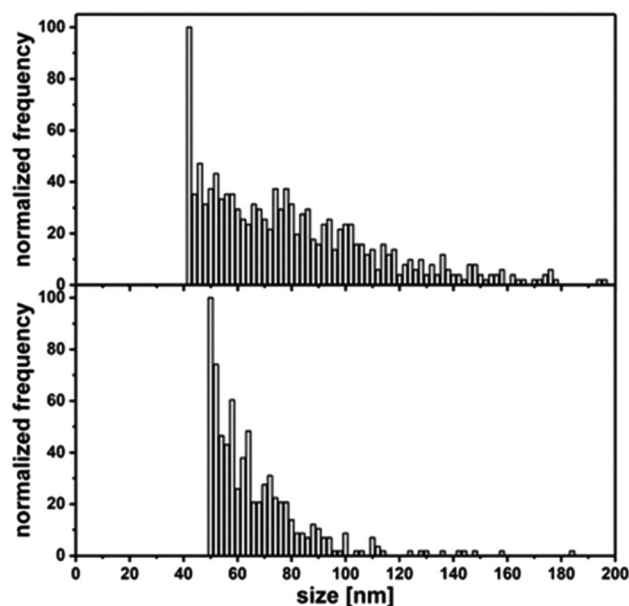


Fig. 5 Top: primary particle size distribution of Al^0 in 0.05% BSA determined by SP-ICP-MS; bottom: Primary particle size distribution of Al_2O_3 in 0.05% BSA determined by SP-ICP-MS.



characteristics of Al⁰ NMs. For comparison, we also investigated Al₂O₃ particles of similar size. To prevent the surface oxidation of Al⁰ NMs, its processing and handling in an inert gas atmosphere was evaluated.

Investigation by XRD revealed a thin aluminum oxide layer at the surface of the Al⁰ NMs (Fig. 6, left). This was confirmed by TEM measurements and has also already been shown in the literature for another Al⁰ NM by TEM measurements (2.5 nm oxide layer).³⁶ The occurrence of an oxide layer can be explained by partial passivation of the material due to manufacturer's processing.

In comparison with Al⁰ NMs, the diffractogram of Al₂O₃ particles showed clear differences (Fig. 6, right). The diffractogram of Al⁰ NMs showed a higher intensity for the aluminum peaks, e.g. at 38°, 45°, 66° and 78° (Fig. 6, left) as compared to Al₂O₃ peaks, e.g. at 37°, 46° and 67° (Fig. 6, right). This demonstrates that even though there is an Al oxide layer at the surface of the Al NMs they are not completely oxidized.

To confirm these results, we used electron energy loss spectroscopy (EELS). Here the sample becomes exposed to an electron beam with defined kinetic energy. Some electrons undergoing inelastic scattering are collected in a detector. The loss of energy reflects the chemical composition of the sample.

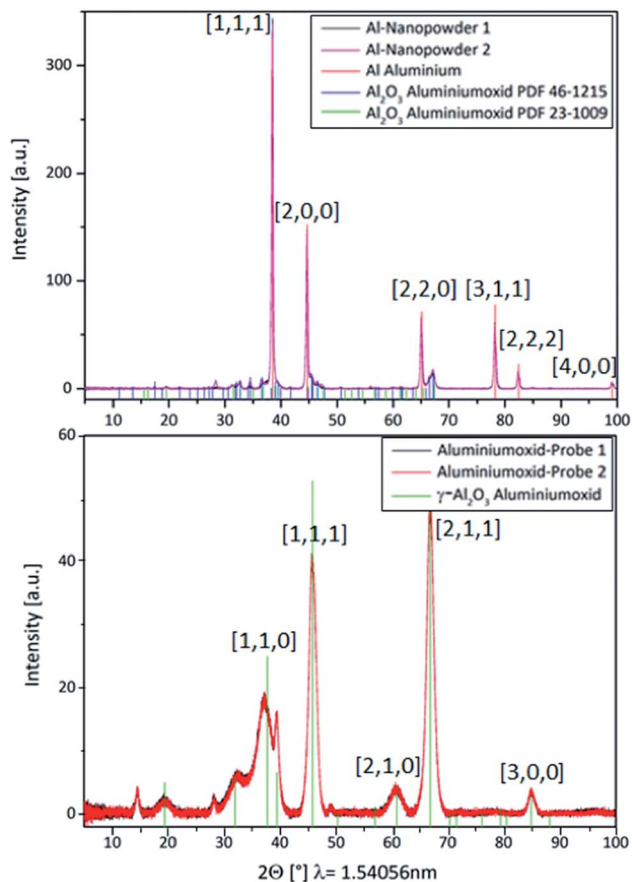


Fig. 6 Top: XR-diffractogram of Al⁰ NMs red: database entry for Al; blue; (green: database entry for Al₂O₃), space group: *Fm3m*, lattice constants: *a* = 4.0494 Å; bottom: diffractogram of Al₂O₃ NMs (red: database entry for Al₂O₃), space group: *Fd3m*, lattice constants: *a* = 7.906 Å.

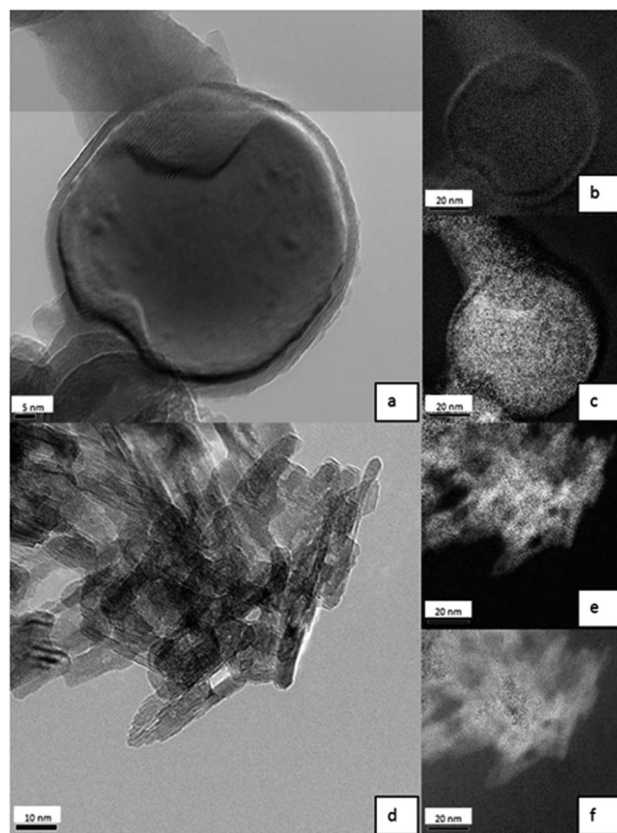


Fig. 7 (a): TEM picture of Al⁰ NMs, 200 k magnification; (b) oxygen mapping of left TEM picture; (c) Aluminum mapping of left TEM picture. (d) TEM picture of Al₂O₃ NMs, 200 k magnification; (e) aluminum mapping of left TEM picture; (f) oxygen mapping of left TEM picture.

Analysis of Al⁰ NMs in 0.05% BSA (Fig. 7a) revealed a core-shell structure. By means of EELS, it was proven that the shell is rich in oxygen (Fig. 7b), while the core consists of elemental aluminum (Fig. 7c). The TEM results indicate an oxide layer of about 2 to 5 nm.

Elemental mapping of Al₂O₃ NMs showed a quite different picture compared to pure Al⁰ NMs (Fig. 7d). The distribution of aluminum and oxygen was homogenous over all NMs (Fig. 7e and f). These results show that Al₂O₃ NMs are fully oxidized while elemental Al⁰ NMs were passivated by an oxide layer. It is

Table 2 Ion release of Al⁰ and Al₂O₃ NMs compared to recovery of AlCl₃ in 0.05% BSA and DMEM

| | | Ion release in BSA [%] | Ion release in DMEM [%] |
|------------------------------------|-------------------------|------------------------|-------------------------|
| Al ⁰ NMs | 10 µg ml ⁻¹ | 0.4 ± 0.1 | 0.5 ± 0.1 |
| | 100 µg ml ⁻¹ | 0.3 ± 0.1 | 0.4 ± 0.1 |
| Al ₂ O ₃ NMs | 10 µg ml ⁻¹ | 0.4 ± 0.1 | 1.4 ± 0.1 |
| | 100 µg ml ⁻¹ | 0.2 ± 0.1 | 0.4 ± 0.1 |
| AlCl ₃ | 10 µg ml ⁻¹ | 140 ± 9 | 112 ± 4 |
| | 100 µg ml ⁻¹ | 94 ± 4 | 66 ± 3 |



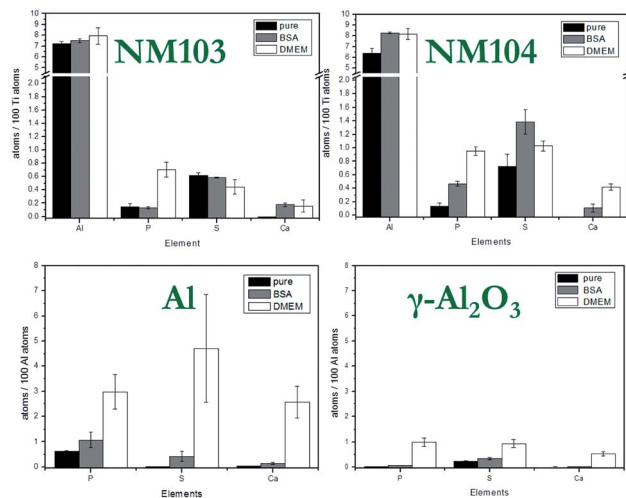


Fig. 8 IBM element analysis of NM103, NM104, Al and Al_2O_3 NMs. NMs as purchased and diluted in water (pure), NMs with albumin corona in H_2O (BSA) and NMs under cell exposure conditions (DMEM). The graph demonstrates the ratio of atoms of several elements compared to 100 atoms of titanium or aluminum.

also visible because Al^0 NMs are dark grey to black, while Al_2O_3 NMs are white.

The results from surface investigations *via* XRD and EELS suggest a different solubility of Al^0 compared to Al_2O_3 . Indeed, the thin oxide layer on Al^0 allows the release of ions while the fully oxidized Al_2O_3 particle should be much more inert. Nevertheless, due to the highly specific surface, a higher solubility compared to Al_2O_3 bulk material could be expected as more potentially ion releasing Al atoms are present on the surface.

Influence of particle composition and impurity patterns

Compared to particle size and surface, the particle composition has a much higher impact on the solubility and dissolution behavior of NMs. One of the most widely used methods due to its high sensitivity, broad range for nearly all elements and detection limits down to the sub-ppb level is the ICP-MS. Unknown samples can be not only detected but also quantified. For more complex samples, microwave-assisted digestion prior to ICP-MS analysis could be performed. In this study, we confirmed the already known composition of the NMs by XRD and EELS measurements as well as ICP-MS analysis. For the assessment of particle toxicity, it is also important to take impurities into account which might alter ion release behavior. Due to element-specific μRBS and μPIXE , IBM became the method of choice for these investigations. The main impurities of aluminum-containing NMs were phosphorus, sulfur and chlorine, which could lead to a different ion release compared to pure materials (see Fig. S6†).

Solubility investigations on Al^0 and Al_2O_3 NMs

To verify our hypothesis that Al^0 NMs are more soluble than Al_2O_3 , we performed ion release experiments in stock

dispersions and DMEM. Adjusting the pH value was not necessary due to almost neutral pH values of 7.3 in stock dispersion compared to 7.2 in DMEM. Keeping in mind that aluminum is an amphoteric material due to the aluminum aqua complexes, one can assume that dissolution of Al^0 NMs in complex media is highly pH-dependent. Compared to an acid, the aluminum aqua complex reacts as a base and *vice versa*. At a neutral pH value, reactivity is very low, thus only low ion release should occur. The possible aluminum aqua complexes at the different pH values are shown in Fig. S7.†

The ion release for both Al^0 and Al_2O_3 NMs after one hour was very low, about 0.2–0.4% in BSA and 0.3–0.5% in DMEM (with 10% FCS) (Table 2). As already described above, this was expected at a neutral pH value. For *in vitro* experiments, this will

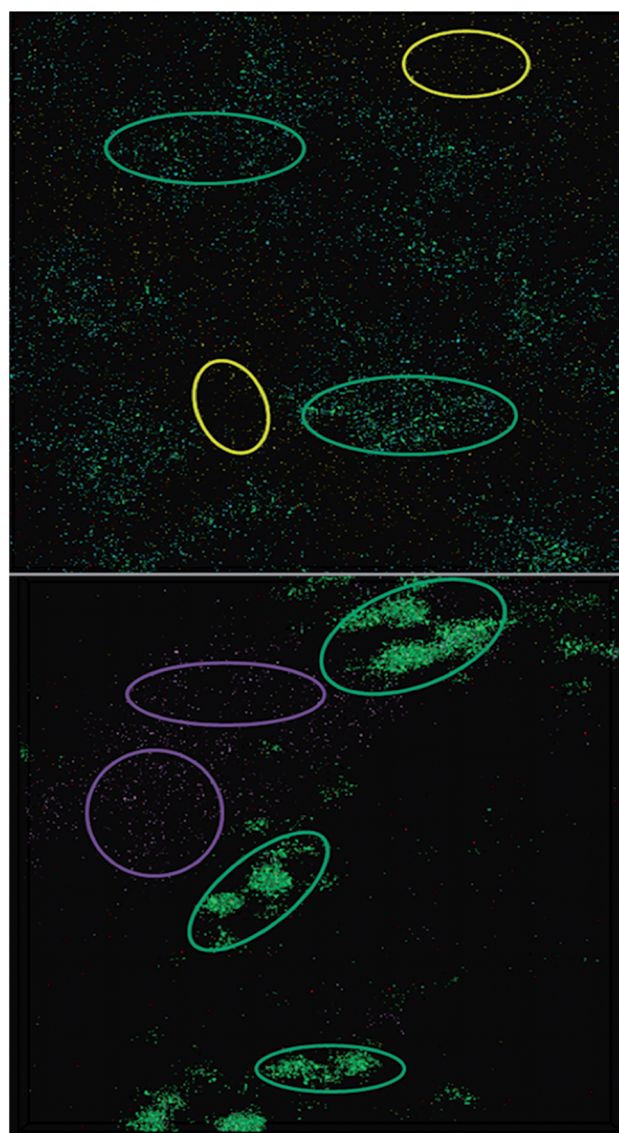


Fig. 9 ToF-SIMS reconstructed ion overlay image ($500\ \mu\text{m} \times 500\ \mu\text{m}$) of Al NM (top) and Al_2O_3 (bottom) agglomerates of different chemical entities from a DMEM solution; yellow: Al NM, purple: Al_2O_3 NM, green: aluminum(III)–serine; orange: phenylalanine aluminate; red: leucine aluminate; blue: polyoxo-aluminum complex.



Table 3 Main characterization techniques and their limits^a

| Methods | TEM | EELS-TEM | XRD | SAXS | SP-ICP-MS | ICP-MS | ToF-SIMS | IBM, atom number % | CRM |
|--------------------------------|--|---|--|---|--|--|--|--|---|
| Aluminum | Primary particle size and shape: 2–50 nm, nearly spherical | Core-shell structure, thin (2–5 nm) oxide layer | Aluminum surface; partially oxidized | Particle radius: > 10 nm | Primary particle size: 54–80 nm | Ion release: 0.2–0.5% | Particle-amino acid agglomerates | Impurities: P (1%); biocorona: S (5%), protein; adsorption from DMEM; Ca ₃ (PO ₄) ₂ coating: P (3%) | No data available |
| Al ₂ O ₃ | Limits No element-specific limits | Light core of Al hinders detailed measurements | No element-specific limits | No element-specific limits | No limits known; results show limit of 54 nm | Detection limit of 10 µg g ⁻¹ in DMEM | No element-specific limits | From Al to higher atomic mass | Raman active molecules |
| Al ₂ O ₃ | Results Primary particle size and shape: 10 × 20–50 nm, grain-like shape | Fully oxidized particle | Fully oxidized surface | Primary particle radius: 7.1 nm aggregates' radius: > 10 nm | Primary particle size: 50–80 nm | Ion release: 0.2–0.4% | Particle-amino acid agglomerates; polyoxo-aluminates | Impurities: S (0.2%); biocorona: S (1%), protein adsorption from DMEM; Ca ₃ (PO ₄) ₂ coating: P (1%) | No data available |
| TiO ₂ NM103 | Limits No element-specific limits | Light core of Al hinders detailed measurements | No element-specific limits | No element-specific limits | No limits known; results show limit of 50 nm | Detection limit of 10 ng g ⁻¹ in DMEM | No element-specific limits | From Al to higher atomic mass | Raman active molecules |
| TiO ₂ NM103 | Results Primary particle size and shape: 20–100 nm, nearly spherical ^b | No data available | Rutile; crystallite size: 20 nm ^b | Gyration diameter: 26 nm ^b | Primary particle size: 60–100 nm | No solubility in BSA, low soluble in DMEM ^b | Particle-amino acid agglomerates | Impurities: Al (7%), S (0.6%); biocorona: S (0.5%), protein; exchange in DMEM; Ca ₃ (PO ₄) ₂ coating: P (0.5%) | Decrease of aliphatic/aromatic compounds on NM surface; higher protein exchange in DMEM |
| TiO ₂ NM104 | Limits No element-specific limits | No element-specific limits | No element-specific limits | No element-specific limits | Limit of ~90 nm ³⁹ | Detection limit of 7.5 ng g ⁻¹ in DMEM | No element-specific limits | From Al to higher atomic mass | Raman active molecules |
| TiO ₂ NM104 | Results Primary particle size and shape: 10–50 nm, nearly spherical | No data available | Rutile; crystallite size: 21 nm ^b | Gyration diameter: 26 nm ^b | Primary particle size: 60–100 nm | No solubility in BSA, low soluble in DMEM ^b | Particle-amino acid agglomerates | Impurities: Al (6%), S (0.7%); biocorona: S (1%); protein; exchange in DMEM; Ca ₃ (PO ₄) ₂ coating: P (0.8%) | Decrease of aliphatic/aromatic compounds on NM surface; higher protein exchange in DMEM |





Table 3 (Contd.)

| Methods | TEM | EELS-TEM | XRD | SAXS | SP-ICP-MS | ICP-MS | ToF-SIMS | IBM, atom number % | CRM |
|----------------|--|------------------------------------|-------------------------------------|---|---|--|--|---|--|
| Limits | No element-specific limits | No element-specific limits | No element-specific limits | No element-specific limits | Limit of ~ 90 nm ³⁹ | Detection limit of 7.5 ng g^{-1} in DMEM | No element-specific limits | From Al to higher atomic mass | Raman active molecules |
| General limits | 1 nm to 2 μm ; only dried samples | Organic matrix contaminates sample | Only powder and crystallite samples | $r = 0.5\text{--}30$ nm (depending on the available q -range) | Only highly diluted samples, limits: Au 10 nm, Ag 20 nm | Sub ng g^{-1} level for most elements | No single particles visible, only agglomerates | Only dry samples under vacuum condition, detection limit: few ppm | Only Raman active molecules observable |

^a Abbreviations: TEM – transmission electron microscopy; EELS – electron energy loss spectroscopy; XRD – X-ray diffraction; SAXS – small angle X-ray scattering; SP-ICP-MS – single particle inductively coupled plasma mass spectrometry; ICP-MS – inductively coupled plasma mass spectrometry; ToF-SIMS – time of flight mass spectrometry; IBM – Ion beam microscopy; CRM – confocal Raman microscopy; BSA – bovine serum albumin; DMEM – Dulbecco's modified eagle medium; ppm – parts per million. ^b Data taken from (ref. 30).

mean that the effects will originate mainly from particles and not from Al ions. The application of an artificial digestion procedure for mimicking *in vivo* situation showed, that the particle dissolution and complexation behavior was quite different in all three studied gastrointestinal compartments.²⁴ After no significant changes in the saliva, the gastric environment leads to a significant increase of the dissolution rate as well as very strong agglomeration of NMs. The addition of intestinal fluid results in a nearly neutral pH value which leads to a decrease in the dissolution rate, a deagglomeration of particles and even *de novo* particle formation in ionic aluminum control.

Particle-CCM interactions

It is of major interest to evaluate the elemental and molecular changes on the particle surface during sample preparation for cell experiments (Fig. S8 and S9[†]). Additionally, two steps were chosen to investigate the surface modification of particles during the sample preparation process. Firstly, the NMs were dispersed. In this step, NMs were covered with albumin corona and are referred to as “BSA” in the text below. The second step was to investigate the NMs under cell culture conditions, diluted in DMEM. After each step, the particles were washed three times in Millipore water. The results of the element analysis, performed by IBM, are shown in Fig. 8.

The variation of the element content represents changes on the surface of NMs, *e.g.* attachment of amino acids, fatty acids, proteins and/or ions to the surface of the NMs. An increase in the Ca and P amount was observed for all studied NMs exposed to DMEM. The highest content of these elements was found in the case of Al NMs. It is suggested that calcium and phosphate ions interact strongly with the albumin corona of NMs and build a calcium phosphate layer on the particle surface. It is known that calcium phosphate has a high affinity to proteins and can increase the efficiency of uptake.^{37,38}

The amount of sulfur on the NMs was analyzed under different conditions. Sulfur was found in association with proteins forming a corona around the NMs. Al and Al₂O₃ NMs acquire more proteins on their surface when exposed to DMEM as compared to dispersion in 0.05% BSA (Fig. S11[†]). In the case of Al and Al₂O₃, the proteins from the culture medium contribute to additional adsorption compared to the existing albumin corona of the particles alone. DMEM shows more physiologic relevant conditions. The salts might induce shielding effects on the protein, so the amount of proteins is likely to be increased. Due to the larger variety of available proteins, a more complex corona will self-assemble on the surface of the particles. In contrast, a decreased amount of proteins was found in the case of NM103 and 104 NMs exposed to DMEM. Substitution of the relatively dense BSA on the particle surface with less dense proteins from the culture media is suggested. This exchange of proteins has a stabilizing effect on TiO₂ NMs in DMEM and results in a strong decrease of aggregate size in DMEM media (Table 1). This finding is also supported by CRM investigations (Fig. S10[†]).

ToF-SIMS was used to image Al NMs and Al₂O₃ NMs as well as nanoparticle agglomerates in cell culture medium and to assess the chemical composition of the nanoparticle agglomerates. The analyses revealed nanoparticle-specific agglomerates, consisting of polyoxo-aluminum complexes, aluminum(III)-serine and amino acid aluminate complexes (leucine and phenylalanine aluminate). These complexes were not observed when ionic AlCl₃ was added to the cell culture medium. ToF-SIMS images revealed a rather homogenous agglomerate distribution with only a slight accumulation of Al NMs in certain areas (see yellow circles in Fig. 9, top) and aluminum(III)-serine and polyoxo-aluminum complexes in others (see green circles in Fig. 9, top). While the aluminates colocalize with both areas, aluminates can be found in regions with predominantly Al NMs and in areas with predominantly aluminum(III)-serine and polyoxo-aluminum. Fig. 9 shows the ToF-SIMS image for Al₂O₃ NMs (bottom). Larger agglomerate areas (green circles in Fig. 9, bottom), where aluminum(III)-serine and polyoxo-aluminum complexes were present in higher amounts, can be distinguished from areas with predominantly smaller nanoparticle agglomerates made of Al₂O₃ NMs (see purple circles in Fig. 9, bottom).

In DMEM with Al NMs, areas where predominantly Al NMs localize, depicted as yellow circles in Fig. 9, top, are distinct from areas where polyoxo-aluminum complexes and aluminum(III)-serine particles localize (green circles). Generally, smaller agglomerates of different chemical entities, Al NMs, aluminum(III)-serine, leucine aluminate, phenylalanine aluminate and polyoxo-aluminum complexes, which do not colocalize in the same area, were observed. In addition to areas where predominantly Al₂O₃ NMs (purple) localize, Al₂O₃ NMs in DMEM show a similar pattern with areas where all chemical entities colocalize but are clearly separated from each other. This indicates a starting mineralization of the larger agglomerates, where different chemical entities colocalize and form mixed agglomerates of Al₂O₃ NMs, amino acids and aluminum salts. Further agglomerate compositions and chemical entities were detected (Fig. S11–14†). For ToF-SIMS measurements for TiO₂ NM103 and 104 in DMEM see Fig. S15–18.†

Conclusions

An extensive characterization of NMs in their different states, from dispersion to *in vitro* conditions, should precede any toxicological testing. In this study, we have characterized two different types of NMs, one metal and one metal oxide. For this purpose, we used a wide range of complementary analytical techniques to characterize particle size, surface and composition in more detail. An in-depth insight into the dissolution, one of the most important determinants of NM toxicity, was achieved by investigation by the examples of Al⁰ and Al₂O₃ NMs. A very low dissolution rate and a small percentage of ion release was observed at a neutral pH value, while higher rates for acidic environment we already reported earlier.²⁴ A significant difference between the surface and the extent of oxidation of Al⁰ and Al₂O₃ NM forms was detected. In contrast to the fully oxidized Al₂O₃ with a rather homogenous distribution of Al and O atoms, Al⁰ NM showed a core-shell structure with an oxide layer only a few nm thick. This was proven

with XRD and the EELS technique, which emphasizes the benefit of using different techniques to get reliable results. It was demonstrated with the help of ToF-SIMS that both aluminum forms are subject to a surprisingly different complexation in biological media: while Al⁰ NMs were shown to form complexes with amino acids, Al₂O₃ NMs mostly formed polyoxo-complexes out of two or more Al₂O₃ molecules. Based on the collected results, all of the investigation methods applied have their own benefits. Thus, with the methods described in this study focusing on size, surface and complex formation, dissolution investigations can perhaps become a bit more predictable. Right now, the recommended limit for aluminum release from food is 5 mg kg⁻¹ food. The various aluminum forms, *e.g.* ions, micro- and nanomaterials, pure Al⁰ or Al₂O₃, are not differentiated here. With this study, it becomes obvious that there should be differentiation for the different forms, as they may be taken up and react differently. For future analytical investigations on aluminum-containing NMs, we propose considering not only Al₂O₃ but also Al⁰ NMs and their interaction with the corresponding ions.

Conflicts of interest

There are no conflicts to declare.

Acknowledgements

This French-German bilateral project SolNanoTOX was funded by the German Research Foundation (DFG, Project ID: DFG (FKZ LA 3411/1-1 and LA 1177/9-1)) and the French National Research Agency (ANR, Project ID: ANR-13-IS10-0005). The authors would like to thank Simone Rolf from the Federal Institute for Materials Research and Testing (BAM) for the XRD measurements, Claudia Kästner from BAM for the SAXS measurements and Dr Uwe Mühle from the Fraunhofer Institute for Ceramic Technologies and Systems (IKTS) for the TEM measurements with elemental information.

Notes and references

- 1 A. Moores and F. Goettmann, *New J. Chem.*, 2006, **30**, 1121–1132.
- 2 K. L. Kelly, E. Coronado, L. L. Zhao and G. C. Schatz, *J. Phys. Chem. B*, 2003, **107**, 668–677.
- 3 D. M. Brown, M. R. Wilson, W. MacNee, V. Stone and K. Donaldson, *Toxicol. Appl. Pharmacol.*, 2001, **175**, 191–199.
- 4 S. Hussain, S. Boland, A. Baeza-Squiban, R. Hamel, L. C. J. Thomassen, J. A. Martens, M. A. Billon-Galland, J. Fleury-Feith, F. Moisan, J. C. Pairon and F. Marano, *Toxicology*, 2009, **260**, 142–149.
- 5 Y. Zhang, N. Kohler and M. Q. Zhang, *Biomaterials*, 2002, **23**, 1553–1561.
- 6 A. Cockburn, R. Bradford, N. Buck, A. Constable, G. Edwards, B. Haber, P. Hepburn, J. Howlett, F. Kampers, C. Klein, M. Radomski, H. Stamm, S. Wijnhoven and T. Wildemann, *Food Chem. Toxicol.*, 2012, **50**, 2224–2242.
- 7 I. A. Rahman, P. Vejayakumaran, C. S. Sipaut, J. Ismail and C. K. Chee, *Mater. Chem. Phys.*, 2009, **114**, 328–332.



- 8 S. E. A. Gratton, P. A. Ropp, P. D. Pohlhaus, J. C. Luft, V. J. Madden, M. E. Napier and J. M. DeSimone, *Proc. Natl. Acad. Sci. U. S. A.*, 2008, **105**, 11613–11618.
- 9 Y. Zhou and M. Antonietti, *J. Am. Chem. Soc.*, 2003, **125**, 14960–14961.
- 10 S. K. Das, M. K. Bhunia and A. Bhaumik, *Dalton Trans.*, 2010, **39**, 4382–4390.
- 11 Z. Q. Sun, T. Liao, L. Y. Sheng, L. Z. Kou, J. H. Kim and S. X. Dou, *Chem.–Eur. J.*, 2016, **22**, 11357–11364.
- 12 X. N. Ren, L. Wu, J. Jin, J. Liu, Z. Y. Hu, Y. Li, T. Hasan, X. Y. Yang, G. Van Tendeloo and B. L. Su, *RSC Adv.*, 2016, **6**, 26856–26862.
- 13 M. Moreno-Horn and T. Gebel, *Crit. Rev. Toxicol.*, 2014, **44**, 849–875.
- 14 J. X. Wang, G. Q. Zhou, C. Y. Chen, H. W. Yu, T. C. Wang, Y. M. Ma, G. Jia, Y. X. Gao, B. Li, J. Sun, Y. F. Li, F. Jiao, Y. L. Zhao and Z. F. Chai, *Toxicol. Lett.*, 2007, **168**, 176–185.
- 15 E. J. Park, H. Kim, Y. Kim and K. Choi, *Toxicol. Environ. Chem.*, 2011, **93**, 120–133.
- 16 Y. R. Kim, S. Y. Lee, E. J. Lee, S. H. Park, N. W. Seong, H. S. Seo, S. S. Shin, S. J. Kim, E. H. Meang, M. K. Park, M. S. Kim, C. S. Kim, S. K. Kim, S. W. Son, Y. R. Seo, B. H. Kang, B. S. Han, S. S. Aan, B. J. Lee and M. K. Kim, *Int. J. Nanomed.*, 2014, **9**, 67–78.
- 17 K. Loeschner, N. Hadrup, K. Qvortrup, A. Larsen, X. Y. Gao, U. Vogel, A. Mortensen, H. R. Lam and E. H. Larsen, *Part. Fibre Toxicol.*, 2011, **8**, 18.
- 18 J. H. E. Arts, M. Hadi, A. M. Keene, R. Kreiling, D. Lyon, M. Maier, K. Michel, T. Petry, U. G. Sauer, D. Warheit, K. Wiench and R. Landsiedel, *Regul. Toxicol. Pharmacol.*, 2014, **70**, 492–506.
- 19 A. R. Collins, B. Annangi, L. Rubio, R. Marcos, M. Dorn, C. Merker, I. Estrela-Lopis, M. R. Cimpan, M. Ibrahim, E. Cimpan, M. Ostermann, A. Sauter, N. E. Yamani, S. Shaposhnikov, S. Chevillard, V. Paget, R. Grall, J. Delic, F. G. de-Cerio, B. Suarez-Merino, V. Fessard, K. N. Hogeveen, L. M. Fjellsbo, E. R. Pran, T. Brzicova, J. Topinka, M. J. Silva, P. E. Leite, A. R. Ribeiro, J. M. Granjeiro, R. Grafstrom, A. Prina-Mello and M. Dusinska, *Wiley Interdiscip. Rev.: Nanomed. Nanobiotechnol.*, 2017, **9**, e1413.
- 20 P. Laux, C. Riebeling, A. M. Booth, J. D. Brain, J. Brunner, C. Cerrillo, O. Creutzenberg, I. Estrela-Lopis, T. Gebel, G. Johanson, H. Jungnickel, H. Kock, J. Tentschert, A. Tlili, A. Schäffer, A. J. A. M. Sips, R. A. Yokel and A. Luch, *NanoImpact*, 2017, **6**, 69–80.
- 21 J. M. Cohen, J. G. Teeguarden and P. Demokritou, *Part. Fibre Toxicol.*, 2014, **11**, 20.
- 22 S. Dekkers, A. G. Oomen, E. A. J. Bleeker, R. J. Vandebriel, C. Micheletti, J. Cabellos, G. Janer, N. Fuentes, S. Vazquez-Campos, T. Borges, M. J. Silva, A. Prina-Mello, D. Movia, F. Nesslany, A. R. Ribeiro, P. E. Leite, M. Groenewold, F. R. Cassee, A. J. A. M. Sips, A. Dijkzeul, T. van Teunenbroek and S. W. P. Wijnhoven, *Regul. Toxicol. Pharmacol.*, 2016, **80**, 46–59.
- 23 A. D. Maynard, R. J. Aitken, T. Butz, V. Colvin, K. Donaldson, G. Oberdorster, M. A. Philbert, J. Ryan, A. Seaton, V. Stone, S. S. Tinkle, L. Tran, N. J. Walker and D. B. Warheit, *Nature*, 2006, **444**, 267–269.
- 24 H. Sieg, C. Kastner, B. Krause, T. Meyer, A. Burel, L. Bohmert, D. Lichtenstein, H. Jungnickel, J. Tentschert, P. Laux, A. Braeuning, I. Estrela-Lopis, F. Gauffre, V. Fessard, J. Meijer, A. Luch, A. F. Thunemann and A. Lampen, *Langmuir*, 2017, **33**, 10726–10735.
- 25 J. M. Zook, S. E. Long, D. Cleveland, C. L. A. Geronimo and R. I. MacCuspie, *Anal. Bioanal. Chem.*, 2011, **401**, 1993–2002.
- 26 K. Loza, J. Diendorf, C. Sengstock, L. Ruiz-Gonzalez, J. M. Gonzalez-Calbet, M. Vallet-Regi, M. Koller and M. Epple, *J. Mater. Chem. B*, 2014, **2**, 1634–1643.
- 27 Z. Y. Wang, A. von dem Bussche, P. K. Kabadi, A. B. Kane and R. H. Hurt, *ACS Nano*, 2013, **7**, 8715–8727.
- 28 A. M. Tavares, H. Louro, S. Antunes, S. Quarre, S. Simar, P. J. De Temmerman, E. Verleysen, J. Mast, K. A. Jensen, H. Norppa, F. Nesslany and M. J. Silva, *Toxicol. in Vitro*, 2014, **28**, 60–69.
- 29 H. E. Pace, N. J. Rogers, C. Jarolimek, V. A. Coleman, C. P. Higgins and J. F. Ranville, *Anal. Chem.*, 2011, **83**, 9361–9369.
- 30 K. Rasmussen, J. Mast, P. J. de Temmerman, E. Verleysen, N. Wegeneers, F. van Steen, J. C. Pizzolon, L. de Temmerman, E. van Doren, K. A. Jensen, R. Birkedal, M. Levin, S. H. Nielsen, I. K. Koponen, P. A. Clausen, V. Kofored-Sørensen, Y. Kembouche, N. Thieriet, O. Spalla, C. Giuot, D. Rousset, O. Witschger, S. Bau, B. Bianchi, C. Motzkus, B. Shivachev, L. Dimowa, R. Nikolova, D. Nihtianova, M. Tarassov, O. Petrov, S. Bakardjieva, D. Gilliland, F. Pianella, G. Ceccone, V. Spampinato, G. Cotogno, P. Gibson, C. Gaillard and A. Mech, *JRC Science and Policy Reports*, 2014, <http://publications.jrc.ec.europa.eu/repository/handle/JRC86291>.
- 31 M. Naiim, A. Boualem, C. Ferre, M. Jabloun, A. Jalocha and P. Ravier, *Soft Matter*, 2015, **11**, 28–32.
- 32 P. A. Hassan and S. K. Kulshreshtha, *J. Colloid Interface Sci.*, 2006, **300**, 744–748.
- 33 R. D. Deegan, O. Bakajin, T. F. Dupont, G. Huber, S. R. Nagel and T. A. Witten, *Nature*, 1997, **389**, 827–829.
- 34 P. J. De Temmerman, E. Van Doren, E. Verleysen, Y. Van der Stede, M. A. D. Francisco and J. Mast, *J. Nanobiotechnol.*, 2012, **10**, 24.
- 35 P. Muneesawang and C. Sirisathitkul, *J. Nanomater.*, 2015, **2015**, 8.
- 36 R. J. Griffitt, A. Feswick, R. Weil, K. Hyndman, P. Carpinone, K. Powers, N. D. Denslow and D. S. Barber, *Environ. Toxicol.*, 2011, **26**, 541–551.
- 37 T. T. Morgan, H. S. Muddana, E. I. Altinoglu, S. M. Rouse, A. Tabakovic, T. Tabouillot, T. J. Russin, S. S. Shanmugavelandy, P. J. Butler, P. C. Eklund, J. K. Yun, M. Kester and J. H. Adair, *Nano Lett.*, 2008, **8**, 4108–4115.
- 38 G. Dordelmann, D. Kozlova, S. Karczewski, R. Lizio, S. Knauer and M. Epple, *J. Mater. Chem. B*, 2014, **2**, 7250–7259.
- 39 S. Lee, X. Y. Bi, R. B. Reed, J. F. Ranville, P. Herckes and P. Westerhoff, *Environ. Sci. Technol.*, 2014, **48**, 10291–10300.

