Lab on a Chip

CORRECTION

View Article Online
View Journal | View Issue

Cite this: *Lab Chip*, 2021, **21**, 447

Correction: Deep-LUMEN assay – human lung epithelial spheroid classification from brightfield images using deep learning

Lyan Abdul,[a] Shravanthi Rajasekar,[b] Dawn S. Y. Lin,[b] Sibi Venkatasubramania Raja,[c] Alexander Sotra,[b] Yuhang Feng,[c] Amy Liu[c] and Boyang Zhang*[ab]

DOI: 10.1039/d0lc90127j

rsc.li/loc

Correction for 'Deep-LUMEN assay – human lung epithelial spheroid classification from brightfield images using deep learning' by Lyan Abdul *et al.*, *Lab Chip*, 2020, DOI: 10.1039/d0lc01010c.

An incorrect version of Fig. 1 was included in the article at proofing stage. The correct version is shown herein.

[a] *School of Biomedical Engineering, McMaster University, 1280 Main Street West, Hamilton, ON, L8S 4L8, Canada*
[b] *Department of Chemical Engineering, McMaster University, 1280 Main Street West, Hamilton, ON, L8S 4L8, Canada. E-mail: zhangb97@mcmaster.ca*
[c] *Faculty of Health Sciences, McMaster University, 1280 Main Street West, Hamilton, ON, L8S 4L8, Canada*

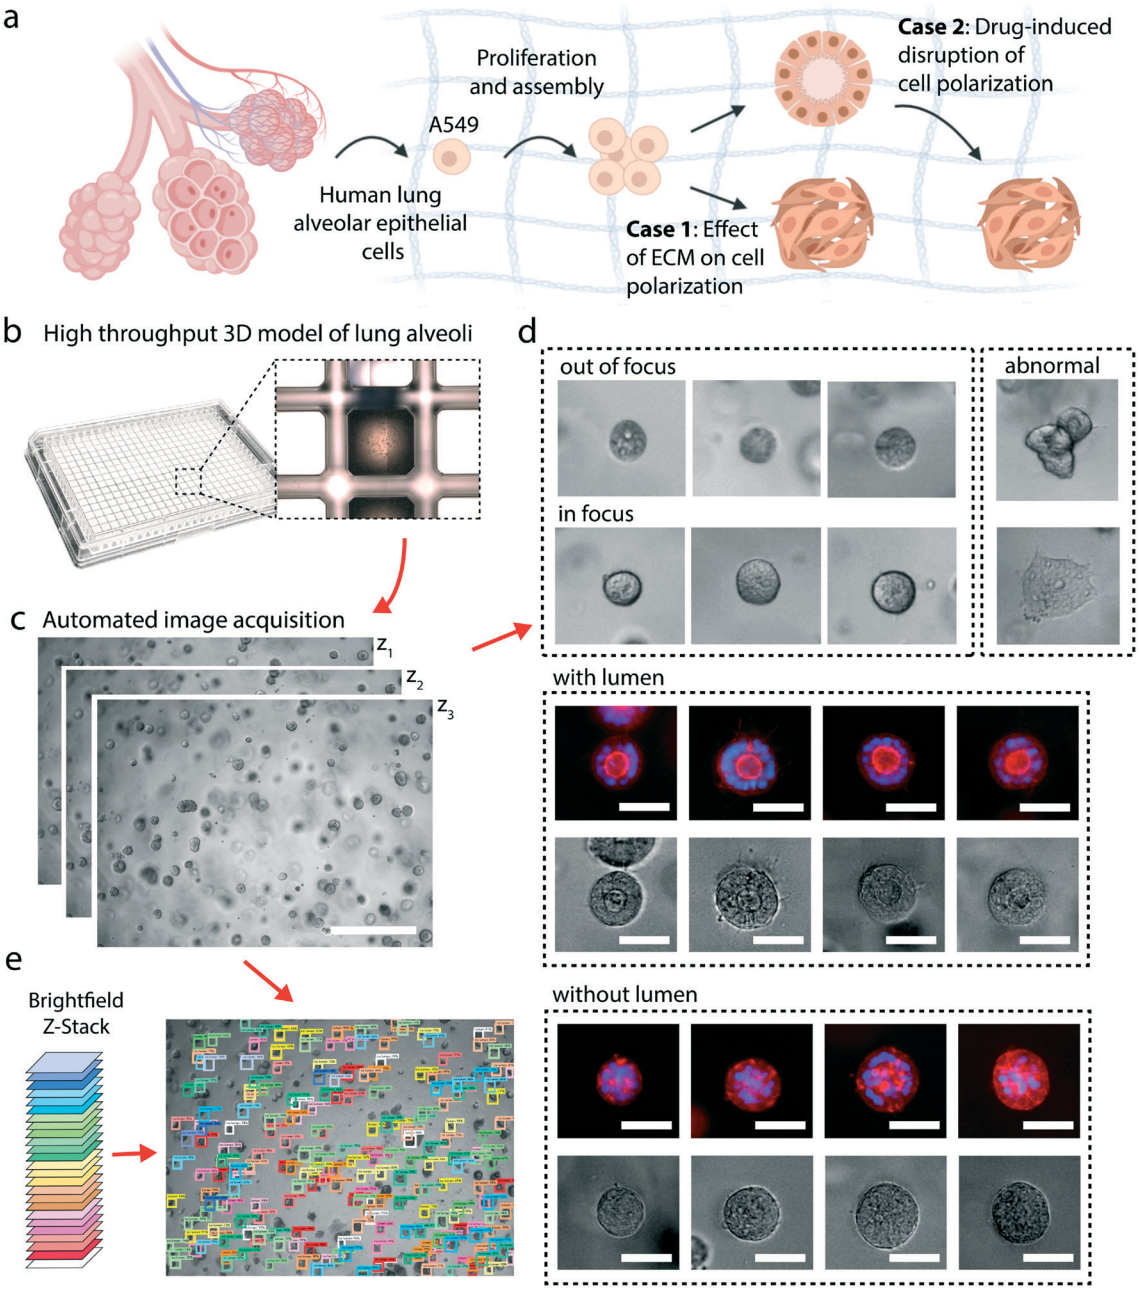

Fig. 1 Differential formation of hollow lung alveolar spheroids. a, Illustration of lung epithelial cells proliferating and assembling into either hollow or solid spheroids in a 3D matrix. b, Tissue culture setup where 25 μL of Matrigel® embedded with cells are cast in standard 384-well plates. c, Acquired *z*-stack transmitted-light images. d, Example scenarios of lung spheroids seen from the collected images. Corresponding fluorescent images stained for F-actin (red) and DAPI (blue) of lung spheroids with or without a lumen (representative images from $n = 6$ samples). Scale bar, 50 μm. e, *z*-Stack acquisition allows for spheroid morphology assessment throughout entire hydrogel. Spheroids on different focal planes were detected with developed deep-LUMEN algorithm from *z*-stack images and then labeled with different colors for visualization.

The Royal Society of Chemistry apologises for these errors and any consequent inconvenience to authors and readers.