

Cite this: *Chem. Sci.*, 2021, 12, 15771

## Correction: Plasticizer and catalyst co-functionalized PEDOT:PSS enables stretchable electrochemical sensing of living cells


Jing Yan,<sup>a</sup> Yu Qin,<sup>a</sup> Wen-Ting Fan,<sup>a</sup> Wen-Tao Wu,<sup>a</sup> Song-Wei Lv,<sup>b</sup> Li-Ping Yan,<sup>a</sup> Yan-Ling Liu<sup>\*a</sup> and Wei-Hua Huang<sup>a</sup>

DOI: 10.1039/d1sc90245h

rsc.li/chemical-science

Correction for 'Plasticizer and catalyst co-functionalized PEDOT:PSS enables stretchable electrochemical sensing of living cells' by Jing Yan *et al.*, *Chem. Sci.*, 2021, 12, 14432–14440, DOI: 10.1039/d1sc04138j.

The authors regret that there was an error in the equation of the calibration curve of PPL/PDMS in Fig. 3. The correct version is shown below.

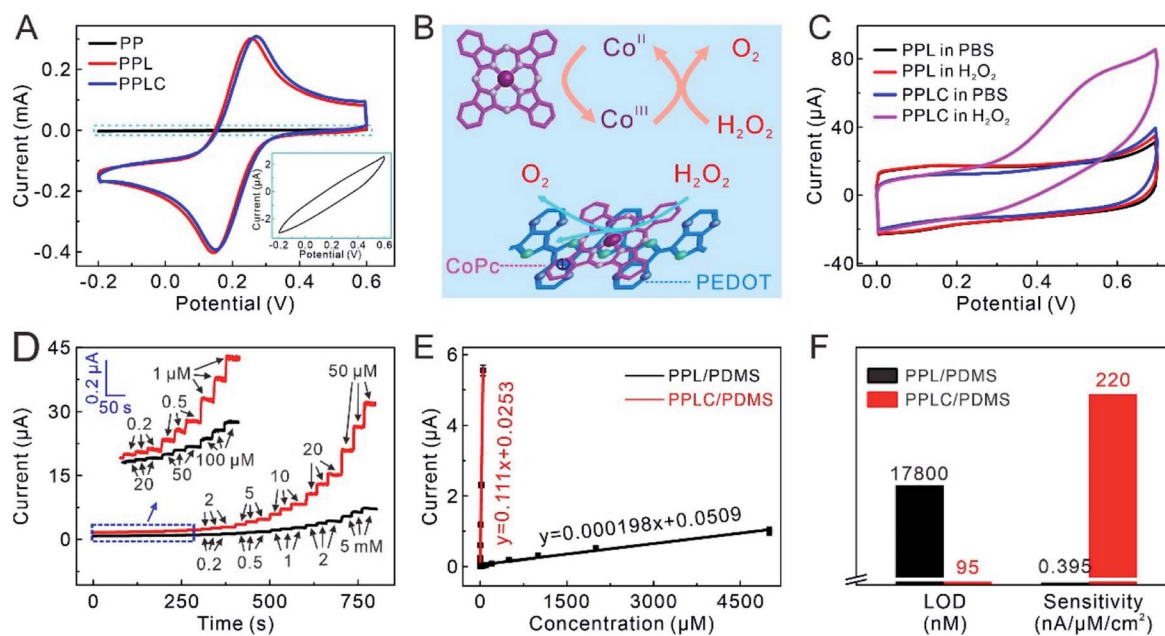

**Fig. 3** (A) CVs of different electrodes obtained in 10 mM K<sub>3</sub>[Fe(CN)<sub>6</sub>]. Inset: the enlarged view for CV of the PP electrode. (B) Schematic illustration of the electrocatalysis mechanism. (C) CVs of different electrodes with and without 1 mM H<sub>2</sub>O<sub>2</sub>. (D) Amperometric responses of PPL/PDMS (black lines) and PPLC/PDMS (red lines) electrodes to H<sub>2</sub>O<sub>2</sub> at a potential of +0.55 V (vs. Ag/AgCl) to increasing H<sub>2</sub>O<sub>2</sub> concentrations. Inset: the enlargements of amperometric responses framed in blue. (E) Calibration curves of PPL/PDMS and PPLC/PDMS electrodes to increasing H<sub>2</sub>O<sub>2</sub> concentrations (data presented as mean ± standard error, *n* = 3). (F) Calculated LOD and sensitivity of PPL/PDMS and PPLC/PDMS electrodes to H<sub>2</sub>O<sub>2</sub>.

The Royal Society of Chemistry apologises for these errors and any consequent inconvenience to authors and readers.

<sup>a</sup>College of Chemistry and Molecular Sciences, Wuhan University, Wuhan 430072, China. E-mail: yanlingliu@whu.edu.cn; whhuang@whu.edu.cn

<sup>b</sup>School of Pharmacy, Changzhou University, Changzhou 213164, China