

## CORRECTION

View Article Online  
View Journal | View Issue



Cite this: *J. Mater. Chem. B*, 2022, 10, 478

DOI: 10.1039/d1tb90187g

rsc.li/materials-b

## Correction: Blood compatibility of a new zwitterionic bare metal stent with hyperbranched polymer brushes

Xiaobo Wang,<sup>a</sup> Xiaoqiang Chen,<sup>b</sup> Lei Xing,<sup>a</sup> Chun Mao,<sup>\*a</sup> Hongxing Yu<sup>a</sup> and Jian Shen<sup>\*a</sup>

Correction for 'Blood compatibility of a new zwitterionic bare metal stent with hyperbranched polymer brushes' by Xiaobo Wang *et al.*, *J. Mater. Chem. B*, 2013, 1, 5036–5044, DOI: 10.1039/C3TB20855A.

The authors of this article have noticed a mistake in Fig. 5 in which the sequence numbers of subfigures B and C were reversed. The corrected Fig. 5 is presented below in this correction notice.

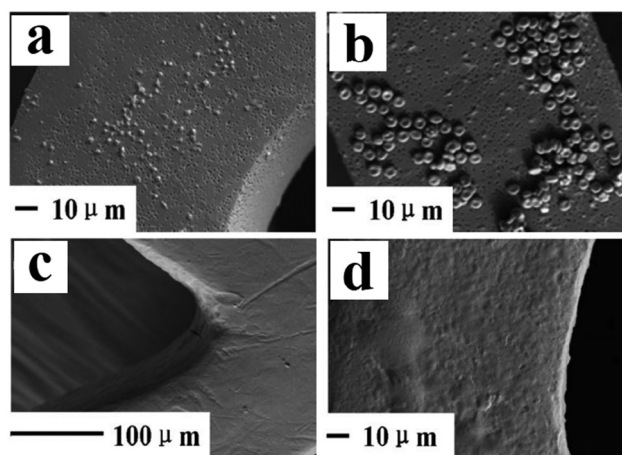


Fig. 5 The platelet and rabbit whole blood adhesion tests of BMS (a and b) and BMS-*g*-HPBBEA-*b*-PDMAPS surfaces (c and d).

The Royal Society of Chemistry apologises for these errors and any consequent inconvenience to authors and readers.

<sup>a</sup> Biofunctional Materials, College of Chemistry and Materials Science, Nanjing Normal University, Nanjing 210023, P. R. China. E-mail: maochun127@yahoo.cn, jshen@njnu.edu.cn; Fax: +86 25 85891653; Tel: +86 25 85891651

<sup>b</sup> State Key Laboratory of Materials-Oriented Chemical Engineering, College of Chemistry and Chemical Engineering, Nanjing University of Technology, Nanjing 210009, China

