


Analytical Methods

Volume 15
Number 14
14 April 2023
Pages 1759–1848

rsc.li/methods

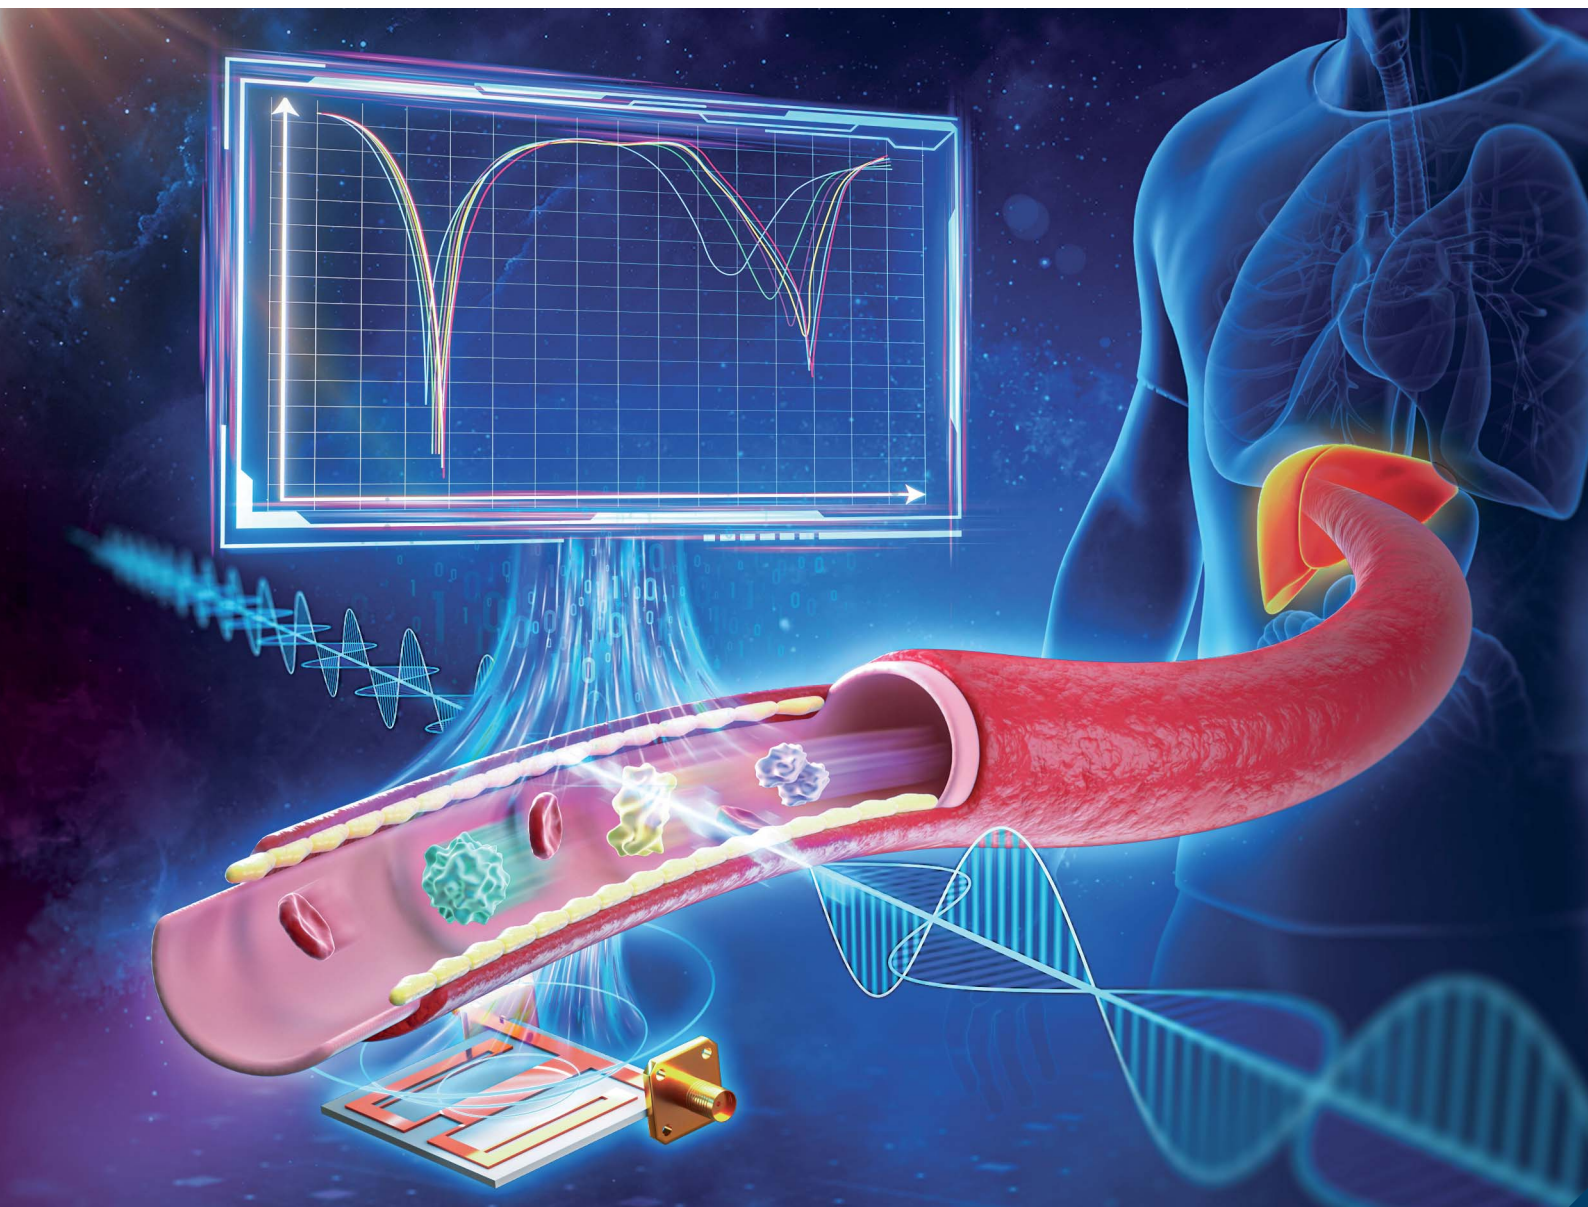

ISSN 1759-9679

PAPER

Yuanyue Li, Zhen Dong, Bin Sun, Zhao Yao *et al.*
Ultrahigh-sensitivity multi-parameter tacrolimus
solution detection based on an anchor planar millifluidic
microwave biosensor

**Indexed in
Medline!**

Royal Society of Chemistry approved training courses

Explore your options.
Develop your skills.
Discover learning
that suits you.

**Courses in the classroom,
the lab, or online**

Find something for every
stage of your professional
development. Search our
database by:

- subject area
- location
- event type
- skill level

Members **get at least 10% off**

Visit rsc.li/cpd-training



**SAVE
10%**