


Sensors & Diagnostics

Volume 2
Number 6
November 2023
Pages 1325-1660

rsc.li/sensors

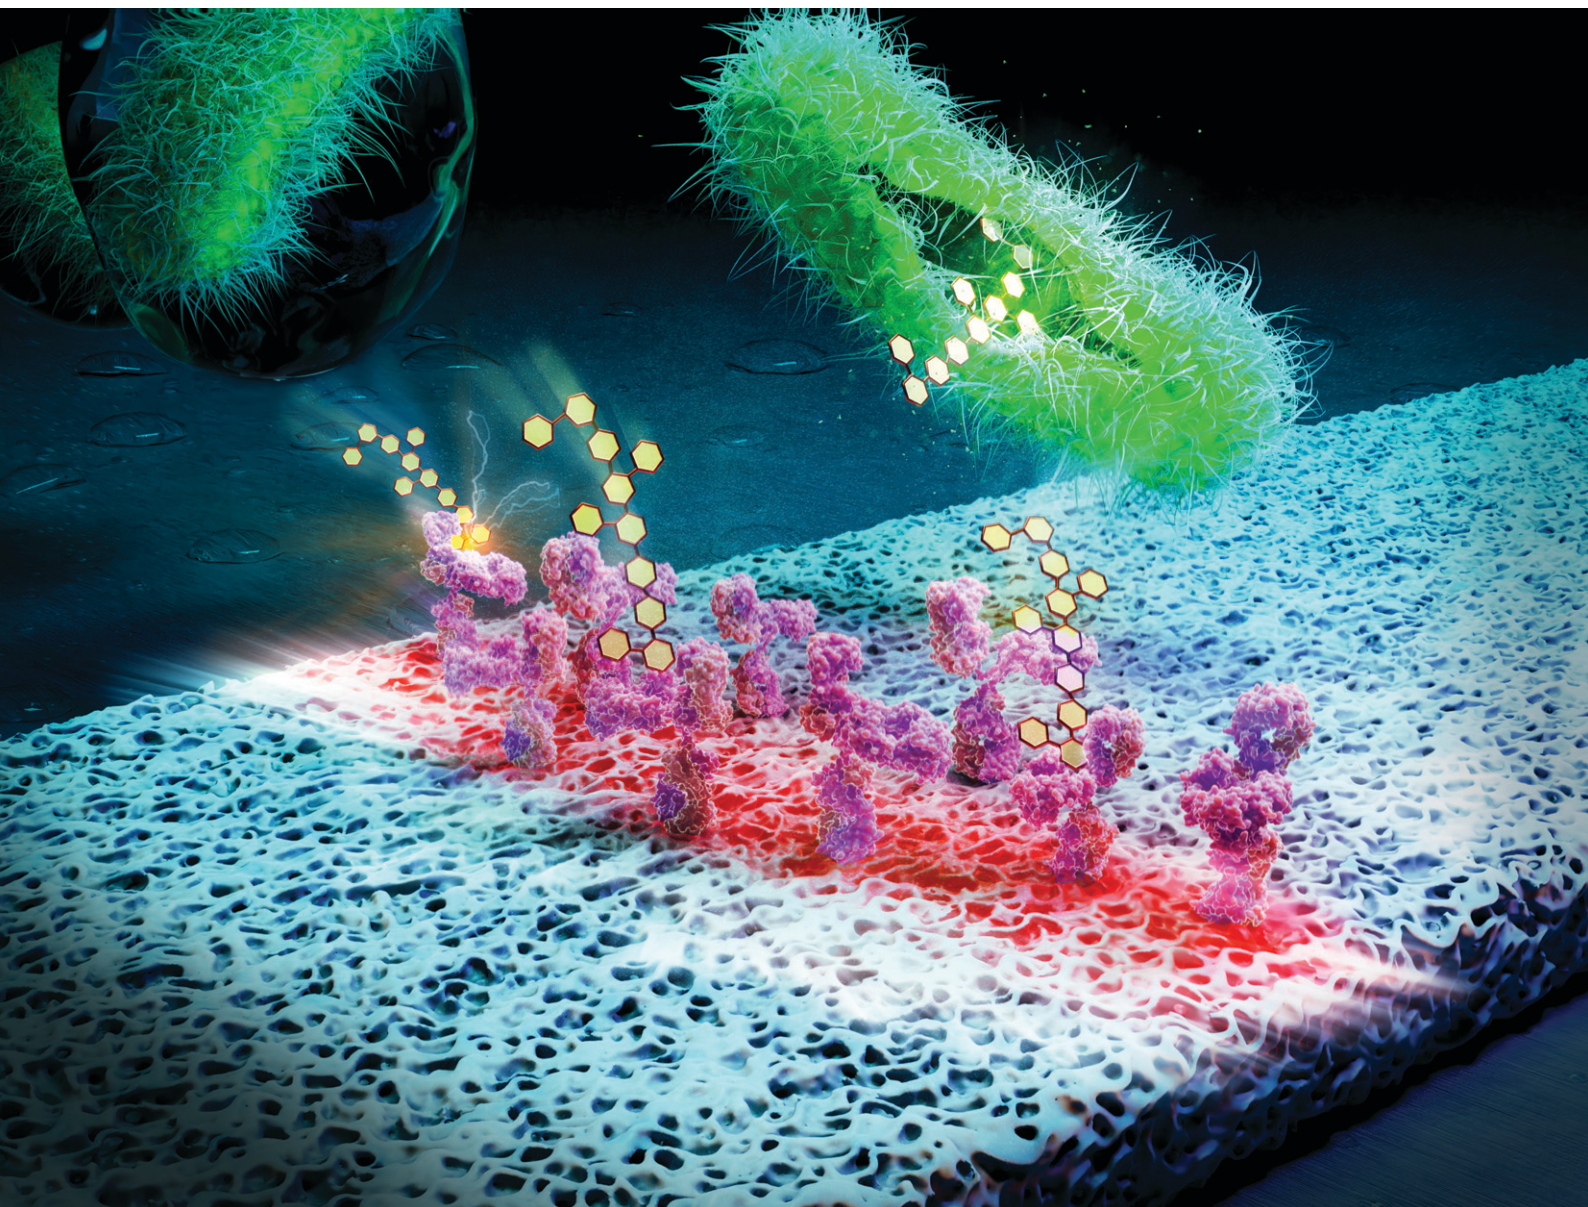

ISSN 2635-0998

PAPER

Andrew J. Steckl *et al.*
Salivary endotoxin detection using combined
mono/polyclonal antibody-based sandwich-type
lateral flow immunoassay device