

Nanoscale

Accepted Manuscript

This article can be cited before page numbers have been issued, to do this please use: R. Memon, J. H. Niazi and A. Qureshi, *Nanoscale*, 2024, DOI: 10.1039/D4NR01175A.



This is an Accepted Manuscript, which has been through the Royal Society of Chemistry peer review process and has been accepted for publication.

Accepted Manuscripts are published online shortly after acceptance, before technical editing, formatting and proof reading. Using this free service, authors can make their results available to the community, in citable form, before we publish the edited article. We will replace this Accepted Manuscript with the edited and formatted Advance Article as soon as it is available.

You can find more information about Accepted Manuscripts in the [Information for Authors](#).

Please note that technical editing may introduce minor changes to the text and/or graphics, which may alter content. The journal's standard [Terms & Conditions](#) and the [Ethical guidelines](#) still apply. In no event shall the Royal Society of Chemistry be held responsible for any errors or omissions in this Accepted Manuscript or any consequences arising from the use of any information it contains.

Biosensors for airborne pathogenic fungal spores detection: a reviewView Article Online
DOI: 10.1039/D4NR01175ARoomia Memon^a, Javed H. Niazi^{a*}, Anjum Qureshi^{a*}

*^aSabanci University, SUNUM Nanotechnology Research and Application Center, Orta Mah.
Tuzla 34956, Istanbul, Turkey*



*Corresponding authors' e-mail: anjum@sabanciuniv.edu; javed@sabanciuniv.edu

Tel: +90 216 483 9879/2441

Abstract

View Article Online
DOI: 10.1039/D4NR01175A

The excessive presence of airborne fungal spores presents major concerns with potential adverse impacts on public health, food safety and contamination. These spores are recognized as pathogens and allergens prevalent in both outdoor and indoor environments, particularly in public spaces such as hospitals, schools, offices and hotels. Indoor environments pose a heightened risk of pulmonary diseases due to continuous exposure to airborne fungal spore particles through constant inhalation, especially in those individuals with weakened immunity who are immunocompromised. Detection methods for airborne fungal spores are often expensive, time-consuming, and lack sensitivity, making them unsuitable for indoor/outdoor monitoring. However, the emergence of micro-nano biosensor systems offers promising solutions with miniaturized designs, nanomaterial integration, and microfluidic systems. This review provides a comprehensive overview of recent advancements in bio-nano sensor system technology for detecting airborne fungal spores, while also discussing future trends in biosensor device development aimed at achieving rapid and selective identification of pathogenic airborne fungi.

Keywords: Biosensors, airborne fungal spores, nanomaterials, microfluidics, automation, Indoor air quality.



1. Introduction

Ever since the advent of the industrial revolution, the global concern over environmental pollution has grown exponentially (1). The deleterious ramifications of air pollution, water pollution, and soil degradation are now recognized as major environmental challenges attributable to a diverse array of emerging contaminants (2). Particularly, concerning is the escalating problem of environmental contamination stemming from newly identified harmful agents, with the discharge of hazardous substances such as toxins, toxic heavy metals, pesticides, pharmaceutical residues and bioaerosol into the ecosystem raising significant worldwide concerns (3, 4). Among these pollutants, bioaerosols are notable for their detrimental impact on both human health and the environment (5). Furthermore, extensive research has consistently revealed that the inhalation of bioaerosol-airborne biological particles can result in a wide spectrum of detrimental health consequences (6). Bio-aerosols are airborne particles that contain varying sizes in nano-to-micron ranges. These particles vary in composition and size, encompassing living organisms such as bacterial (approximately 0.5-10 μm), fungi (around 5- 100 μm), viruses (approximately 50-200 nm), smoke (approximately 50 nm^{-1} μm), and pollen. In recent years, there has been significant attention directed towards the monitoring and sampling analysis of airborne pathogenic microorganisms. This heightened focus is largely attributed to the presence of indoor airborne microbial/mold contamination and bioaerosols, which constitute significant contributors, accounting for approximately 5-34% of indoor air pollution (7, 8). Surveillance and identification of airborne microbial particles represent a significant concern owing to their presence and the resulting health implications, spreading of infectious diseases, acute toxic effects, allergies, cancer and the potential danger of bioterrorism (9, 10). Within these airborne microbial particles, fungi are recognized as a significant contributor to infectious and allergic diseases (11, 12). Public spaces, such as hospitals, schools, offices, and hotels are among the more susceptible places where fungal




particle exospore is at higher risk. Individuals with weak immunity or immunocompromised are most vulnerable to infectious pulmonary diseases caused by the constant inhalation of numerous airborne fungal particles.

Among the airborne microbial fungal particles, *Aspergillus fumigatus* has emerged as a highly prevalent airborne fungal pathogen. It is responsible for dangerous and invasive diseases that are frequently fatal, especially when immunocompromised hosts are present in developed nations (13). Over the past 12 years, there has been a quadruple rise in invasive aspergillosis (IA). IA accounted for around 30% of fungal infections in cancer patients, with an estimated occurrence of 10 to 25% in leukemia patients. Among leukemia patients, the mortality rate remains high at 80 to 90%, even after treatment (13, 14). In leukemia treatment centers, solid-organ transplantation facilities, and bone marrow transplantation (BMT), invasive aspergillosis (IA) has been identified as a major cause of mortality (14). Alveolitis, allergic sinusitis, and asthma are examples of conditions that can result from recurrent exposure to *Aspergillus* sp. conidia or antigens, even in the absence of mycelial colonization. This information is based on a survey by the World Health Organization (WHO) regarding indoor air quality (15). Therefore, it is imperative to develop innovative methods for early monitoring and accurate detection of such pathogenic airborne fungal particles in contaminated air/water/aerosol environments, which may prevent the disease progression. The conventional fungi detection methods include microscopy, histopathology, growth in pure culture and morphologic study of the reproductive structures, which are challenging due to non-specificity and require additional time for the radiological imaging (CT scan) method (16). Currently, there is no tool available to date that can directly allow the detection of fungal pathogens from air/aerosols. Existing detection methods heavily rely on microscopic examination of air/aerosol samples that are qualitative and often inaccurate with false-positive/-negative results. Various assays have been developed for the potential detection of fungal spores in immunocompromised host systems,




specifically from liquid phases (blood/serum) or biopsy tissue samples. These assays encompass polymerase (PCR), DNA-based methods (17), enzyme-linked immunosorbent assay (ELISA) (18), and spectroscopic quantification (19), all utilized for the detection of pathogenic fungal species (20-25). These techniques are rather more complex, expensive, and time-consuming and often face challenges of false positives due to the high probability of cross-reactivity. Therefore, these methods are practically challenging for in situ real-time detection of pathogenic fungal particles from aerosols. Within this context, biosensors have emerged as invaluable tools for detecting minuscule concentrations of bioaerosols. These biosensors, characterized by compact analytical devices, bring forth a host of advantages, including simplicity, portability, ease of use, exceptional sensitivity, and selectivity. They have emerged as powerful solutions for detecting and analyzing a wide spectrum of bioaerosol pollutants across diverse environmental contexts (26, 27). Biosensors can serve as early warning systems and provide active measurements by which precautionary measures can be taken to control the presence and levels of pathogenic fungal spores/particles in air/aerosol contaminants. In recent years, biosensors have particularly excelled as highly effective platforms for analyzing airborne pathogens (28). Simultaneously, the realm of microfluidic bioassays has witnessed significant advancements, facilitating both containment and rapid detection of airborne microbes. Nevertheless, despite these strides, the availability of commercially proven devices for real-world sample analysis remains limited (29). The challenges encompass factors such as low microbes concentrations in the air, the presence of interfering agents, and the intricate task of seamlessly integrating sampling chambers with sensing devices, thereby impeding the success of diagnostic applications (30).

Nevertheless, significant advancements in this domain have been propelled by nanotechnology, leveraging the unique characteristics of nanomaterials, particularly their heightened surface-area-to-volume ratio. This has led to the development of highly efficient



and sensitive detection methodologies (31). The use of nanomaterials has facilitated the miniaturization of sensing devices, leading to the creation of swift, portable, and sensitive diagnostic systems for pathogens (32). These systems can identify airborne pathogens in various settings, ranging from hospitals and ventilation systems to airplanes (33). Furthermore, they hold promise in preempting and identifying bioterrorism threats in public spaces, thereby bolstering overall security and public health.

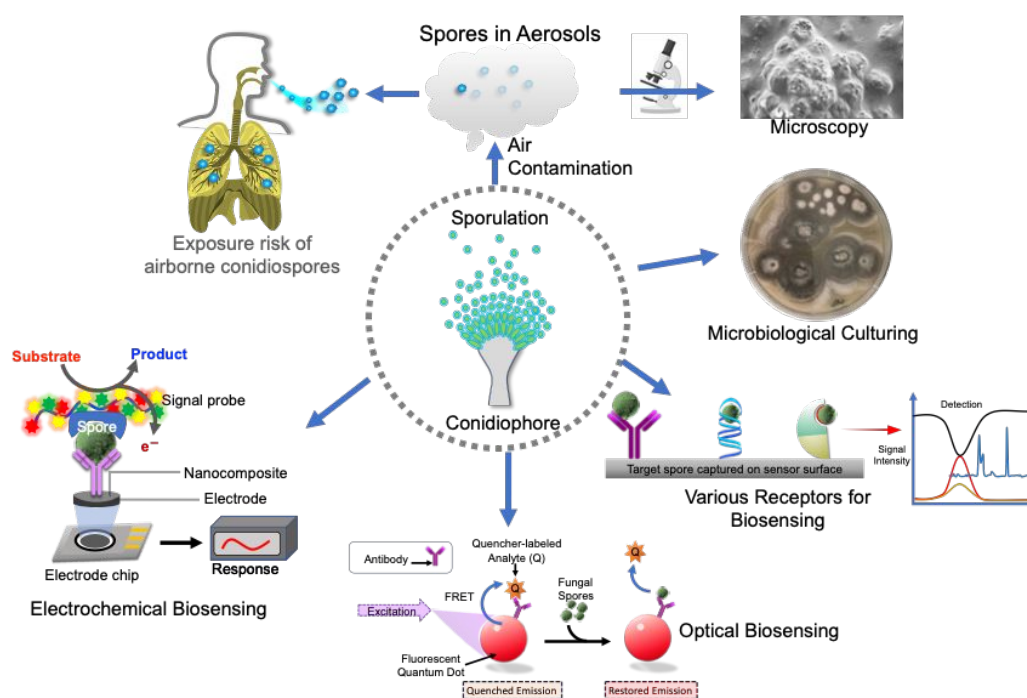

Scheme:1 The schematic diagram showing overview of the main topic of this review related to biosensors for airborne pathogenic fungal spores detection.

In the realm of fungal pathogenicity and environmental health, the detection and characterization of *Aspergillus fumigatus* spores have emerged as a critical focal point. As a ubiquitous airborne fungal species, *Aspergillus fumigatus* presents both a formidable challenge and a compelling opportunity for research and diagnostics. Understanding the intricacies of its ecological role but also mitigating potential health risks. Among the pathogenic aspergilli, *Aspergillus fumigatus* holds the distinction of being the most widespread in the environment



and serves as the primary causative agent of disease. Subsequent in order of importance are *Aspergillus niger*, *Aspergillus flavus*, *Aspergillus terreus*, *Aspergillus nidulans*, and several species belonging to the *fumigati* family. These organisms exhibit comparable morphological characteristics to *Aspergillus fumigatus*. In this review, we delve into the latest advancements in biosensor technologies (Scheme 1), focusing on fabrication processes, materials, and biosensing methodologies in the realm of *Aspergillus fumigates* spore detection, shedding light on the state-of-the-art techniques and their applications in various fields, from clinical diagnostics to environmental monitoring. Through this exploration, we aim to unravel the complexities surrounding *Aspergillus* spores and provide insights into the evolving landscape of detection strategies with sustainable biosensor technologies to revolutionize healthcare diagnostics and contribute to a greener and more environmentally conscious future.

2. Conventional approaches to airborne pathogenic fungal spores detection

Evaluating the presence and quantity of airborne pathogenic fungal spores, notably, those belonging to *Aspergillus fumigatus*, holds paramount importance in gauging the risk of respiratory infections and assessing indoor air quality. Over time, various conventional techniques have been employed to detect these fungal spores, including cell-culturing, molecular techniques involving the amplification of specific genes for identification by PCR reactions, and detection for the presence and quantification of biomarker proteins by Enzyme-Linked ImmunoSorbent Assay (ELISA). These techniques are detailed in the following sections.


2.1 Cell culture-based assay

Traditional culture-based methods are extensively employed for the isolation, cultivation, and quantification of airborne fungal spores, owing to their ease of use, cost-effectiveness, and operational simplicity. This technique involves incubating bioaerosol samples collected on appropriate nutritional agar surfaces or in buffer solutions at an appropriate temperature for 24



h to facilitate the growth and proliferation of fungal spores. The primary sampler widely employed for this approach is the Andersen sampler. This sampler operates as a multi-stage (cascade) impactor, allowing for a separate collection of spores of varying sizes. It has found application in recent studies conducted both indoors and outdoors (34, 35). The resulting colonies (colony-forming units, CFUs) on the agar plates are counted to determine their concentration in bioaerosols followed by identification techniques for cultured microorganisms (36). Microscopic observations are pivotal in identifying fungal pathogens through the examination of morphological features, which are employed for taxonomic classification. These features include sporulation production, spore morphology, and the characteristics of sporulating structures that give rise to both asexual and sexual spore forms (37, 38). Although culture-based methods are regarded as the benchmark for microbial testing, they do come with specific limitations. These include a high labour requirement, long detection times and incompatibility with non-cultural pathogens. Moreover, the culture-based method fails to provide accurate information about the total number of airborne microorganisms, limiting its suitability for on-site applications. In a research investigation by Zengmin Miao et al., the enumeration of airborne *Aspergillus fumigatus* fungal spores in a rabbit house was achieved through both culture-based counting (CCM) and polymerase chain reaction (PCR). In this study, air samples were gathered and subsequently cultured on specific media to facilitate the growth of viable fungal spores. Following incubation, the count of colony-forming units (CFUs) was determined, representing the quantity of viable fungal spores in the air. The results showed the concentrations of *Aspergillus fumigatus* spores, as determined by CCM, were 2.5×10^2 , 2.8×10^2 and 1.1×10^2 CFU/m³ of air in three different houses (A, B and C), respectively (39-42).

2.2 Polymerase chain reaction (PCR)




PCR stands for polymerase chain reaction a highly effective molecular biological approach utilized to amplify and identify DNA sequences. For the detection of fungal spores, including *Aspergillus fumigatus*, it has been extensively employed. PCR is dependent on the synthesis of new DNA strands that are complementary to a target DNA sequence or a gene by DNA polymerase enzymes. The process involves repeated cycles of heating, cooling, and enzymatic reactions to amplify a specific DNA region of interest, a process similar to the popular COVID-19 RT-PCR method, except that it does not use the enzyme reverse transcriptase (RT) and labelled oligonucleotide probes used in RT-PCR for detection. Furthermore, a typical PCR reaction comprises the following constituents. (a) Template DNA: this involves using a sample containing the target DNA, such as fungal spore DNA, as the template for PCR, (b) primers: these are brief DNA sequences crafted to complement the regions bordering the target DNA sequences. They are purposefully designed to bind to the target DNA or a gene, serving as initial points for DNA synthesis. (c) DNA polymerase: utilizing a heat-stable DNA polymerase enzyme, like Taq DNA polymerase, which can synthesize new DNA strands based on the template DNA and the primers. (d) Nucleotides, comprising the essential building blocks (A, T, C, and G), are crucial for DNA synthesis. The PCR procedure involves three main stages, with the first being; (e) denaturation: the reaction mixture undergoes high-temperature heating (typically at 94-98 °C), inducing the separation or denaturation of DNA strands, leading to the formation of single-stranded DNA molecules; (f) annealing: after denaturation, the reaction mixture undergoes cooling to a temperature that enables the primers to selectively bind to their complementary sequences on the single-stranded template DNA. Typically, this step occurs at a temperature around 50-65 °C; (g) extension: following annealing, the reaction mixture is then heated to an optimal temperature, usually around 72 °C. The synthesis of new DNA strands by DNA polymerase enzymes is facilitated at this temperature through the addition of nucleotides to the primers. Thus, complementary copies of the target DNA sequences are generated. These



three steps are repeated through multiple cycles, typically 25-35 cycles, leading to the exponential amplification of the target DNA, if that specific sequence is present in the sample. Significantly, each cycle doubles the amount of DNA, resulting in a substantial increase in the quantity of the target DNA sequence. In another study, the researchers developed and validated a PCR assay targeting the *Aspergillus fumigatus* gene encoding the mitochondrial small subunit rRNA. The PCR assay successfully detected *Aspergillus fumigatus* DNA in various clinical samples including bronchoalveolar lavage fluid, sputum, and lung tissues which confirms its utility for diagnosing *Aspergillosis*, a fungal infection caused by *Aspergillus* species (42, 43). Another study employed real-time PCR (also reverse transcriptase PCR), a molecular technique utilized for the real-time amplification and quantification of specific fungal DNA sequences, has been documented. Here, identification and measurement of the genetic material of *Aspergillus fumigatus* spores in the air were carried out by collecting samples from three rabbit houses. The results indicated that the concentrations of ambient *Aspergillus fumigatus* spores in three distinct residences (A, B, and C) were 3×10^3 - 5×10^3 spores/m³ respectively, as determined by real-time PCR. After comparing both techniques, the real-time PCR method consistently yielded higher spore concentrations compared to the CCM method. The former concentrations were reported to be 12–14 times higher than the latter concentrations in all three rabbit houses.

2.3 Enzyme-linked immunosorbent (ELISA)

The enzyme-linked immunosorbent assay (*ELISA*) is a commonly used immunoassay method utilized for the detection and quantification of proteins, biomarkers or other target molecules. It utilizes the principles of antigen-antibody interactions and an enzymatic detection system to provide a measurable signal. In ELISA, the fungal spores coated on the surface, together with the primary antibody, create an antibody-antigen complex. Subsequently, this complex is identified through a secondary antibody linked to an enzyme, usually horseradish



peroxidase (HRP), which in presence of H₂O₂ and a redox-sensitive chromogenic substrate

View Article Online

DOI: 10.1039/D4NR01175A

Here, the enzyme initiates a reaction with a substrate, resulting in the production of a detectable signal directly proportional to the presence or concentration of *Aspergillus fumigatus* spores in the aerosol samples. The signal is quantified using a spectrophotometer or a plate reader. For example, a study by Sterzenbach *et al.* (2004) demonstrated the application of ELISA in detecting fungal spores from air samples. The researchers coated microplate wells with fungal spores and used specific primary antibodies against the target spores. They then added a secondary antibody conjugated to alkaline phosphatase, which is another enzyme used in ELISA that catalyzes the hydrolysis of a colorless substrate, such as a *p*-nitrophenyl phosphate (pNPP) into yellow colored *p*-nitrophenol (pNP). The resulting colour change is measured spectrophotometrically to quantify the fungal spores present in the aerosol samples collected using an impactor (44, 45).

Conventional techniques for detecting airborne fungi, including culture-based methods, PCR, ELISA, and microscopy, have both merits and demerits. While they offer sensitivity, specificity, and the ability to isolate and identify viable fungal spores, they are also time-consuming, labour-intensive, and may not detect non-viable spores or applicable to all fungal species. Additionally, sampling limitations, laboratory-based analysis, and delayed results (taking days to weeks) can hinder prompt interventions. These limitations highlight the need for alternative, rapid, and on-site detection methods, such as biosensors, to complement conventional techniques and improve airborne fungal detection and monitoring. Despite these drawbacks, traditional techniques are cost-effective and accessible, requiring minimal specialized equipment and expertise. Incorporating modern molecular methods can improve sensitivity and accuracy, offering a more comprehensive assessment of airborne fungal diversity and potential health risks.

3. Biosensors



Biosensors are analytical devices that detect and quantify specific substances by combining a transducer with a biological recognition component. These devices are composed of three fundamental components: the biological recognition element, the transducer, and the signal processing system as shown in (Figure 1). The biological recognition component is typically a biomolecule, such as an enzyme (46), antibody (39, 47) or nucleic acid (48-50). Which interacts specifically with the target analyte. This interaction generates a signal or response that is transduced by the transducer into a measurable output. The transducer converts the biochemical or biophysical signal into an electrical, optical and physical signal which can be quantitatively measured. This transduction process is achieved through various mechanisms such as electrochemical reactions, optical absorption or emission, piezoelectric changes, and thermal effects. Moreover, the signal processing system interprets and analyzes the transduced signal and provides quantitative information about the target analyte's concentration or presence compared to other types of sensors (51). Biosensors offer distinct advantages, such as they exhibit high selectivity and specificity, as the biological recognition element is designed to interact only with the target analyte, including fungal spores. This allows for accurate detection and minimizes interference from other substances. Furthermore, biosensors can offer measurements in real-time, allowing for continuous monitoring and prompt response to fluctuations in analyte concentration. Besides, biosensors also offer excellent sensitivity, often detecting analytes at low concentrations which is crucial in applications such as medical diagnostics and environmental monitoring. Biosensors can be designed for miniaturization, enabling portable and point-of-care testing. This portability and ease of use make biosensors highly suitable for on-site analysis and remote field applications (52). Biosensors possess numerous advantages; but besides this, they also have some limitations. For instance, the stability and shelf-life of biological recognition elements can be a challenge, requiring appropriate storage conditions and periodic replacement. Biosensors may also be susceptible

View Article Online
DOI: 10.1039/C4NR01175A



to interference from complex sample matrices and necessitating sample preparation steps. Additionally, the development and optimization of biosensors for specific analytes may require significant expertise and time, as compared to the other sensors, such as chemical sensors or physical sensors, the biosensors offer superior specificity and sensitivity due to the specific interactions between the biological recognition element and the target analyte. Chemical sensors, for example, often rely on non-selective chemical reactions, leading to potential cross-reactivity with interfering substances. On the other hand, physical sensors may lack the specificity necessary for precise analyte detection. Therefore, the biosensors with their biological recognition elements provide an elegant solution to overcome these limitations (44, 53-55).


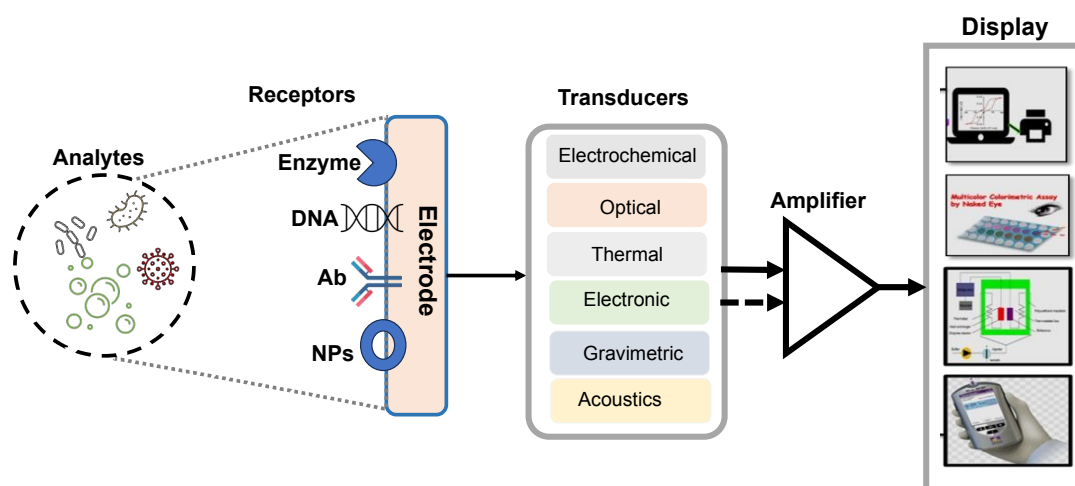


Figure 1: Schematic diagram illustrating the operational principles of a biosensor. This includes (a) bio-recognition elements responsible for detecting specific analytes, such as viruses, bacteria or fungi (b-c) signal generation components like transducers and amplifiers, which convert the recognized signals into measurable data (d) a display unit is shown to visualize the results generated by the biosensor.

Moreover, biosensors provide rapid and on-site detection capabilities, complementing conventional techniques and improving airborne fungal detection and monitoring. These modern methods enhance sensitivity and accuracy, offering a more comprehensive assessment



of airborne fungal diversity and potential health risks. Incorporating biosensors into detection strategies can significantly improve efficiency and effectiveness in identifying and responding to fungal contamination events. In the following section, we explore a range of optical, electrochemical, and microfluidic platforms that utilized nanomaterials with special emphasis on detecting airborne *Aspergillus* spores.

3.1 Optical Biosensors

Optical sensors have a high sensitivity for detecting optical signals produced by analytes binding to probes. Their function is associated with light-matter interactions, which give rise to distinct sensing modes such as colorimetric, plasmonic, and energy transfer sensing methods. Among these, colorimetric sensing is the most employed due to its simplicity and user-friendliness. In a colorimetric biosensor, the signal manifests as a colour change that is easily perceptible and detectable to the naked eye. This eliminates the necessity for intricate equipment and reduces the time-consuming intermediate steps. This approach to detecting infections, pathogens, or endotoxins is extremely effective and trustworthy. Optical biosensors are constructed using fundamental optical principles, including reflection, refraction, absorption, and dispersion (Figure 2a-b). Optical biosensors have been developed and advanced through the utilization of various transducers, including optical fiber, Raman spectroscopy, and surface plasmonic resonance (SPR). In the case of optical fiber, emitted light traverses through the tapered optical fiber on the detection surface and is subsequently detected. Light-spreading optical biosensors that detect airborne particles and endotoxins have been developed as a result of these methods (56). Reflectance spectroscopy, facilitated by SPR, is employed to identify pathogens and endotoxins.

View Article Online
DOI: 10.1039/D4NR01175A

Nanoscale Accepted Manuscript




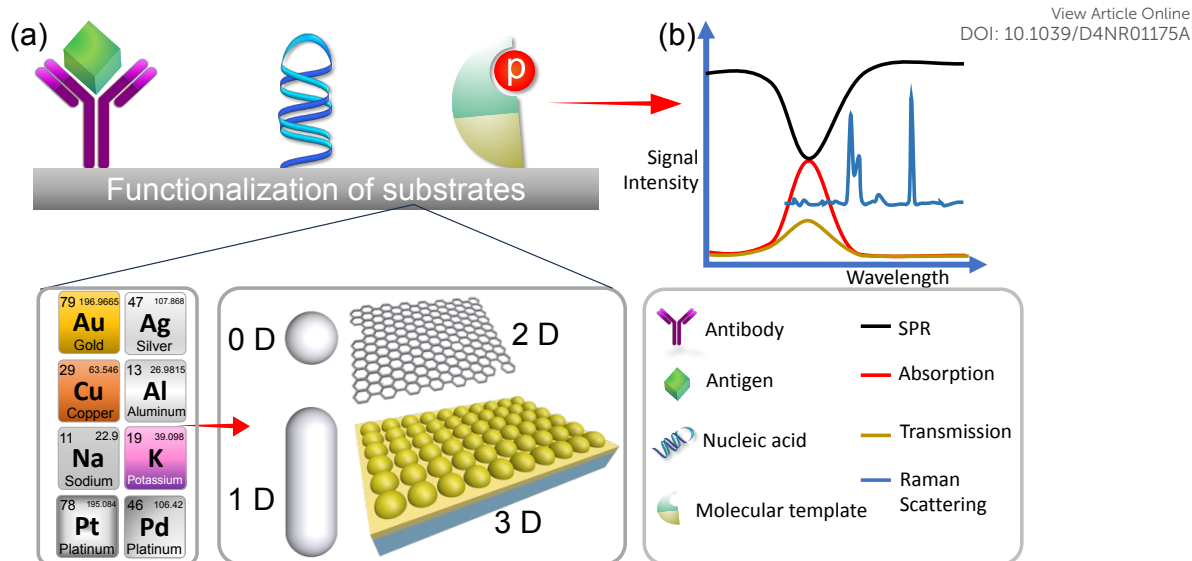


Figure 2: (a) Demonstrates the functionalization process of the substrate with various optical materials and the attachment of specific receptors for enhancement of sensitivity and specificity (b) Depicts the signal detection mechanism, involving the selection of modes such as Surface Plasmon Resonance (SPR), Absorbance, Transmission or Raman Scattering, enabling precise analyte detection and analysis.

Kattke et al., (47) conducted a study to develop a Quantum Dots-based immunoassay for detecting *A. amstelodami* using FRET. The study focuses on developing a quantum dots (QDs)-based immunoassay using Förster Resonance Energy Transfer (FRET) for the rapid and specific detection of *A. amstelodami*. The authors emphasize the importance of optimizing quenching efficiency and addressing challenges like mold autofluorescence to enhance sensitivity and signal consistency. To construct a complex, QDs were attached to antibodies along with the quencher BHQ-3-labeled mold analyte. This mold analyte had a lower affinity for the antibody than *A. amstelodami*. The characterization of QD-antibody conjugates included production and purification assessments concerning concentration and antibody-to-QDs ratio, serving as quality control measures. To mitigate challenges arising from mold autofluorescence, adjustments were made to the excitation wavelength, and a QD with optimal signal-to-noise ratios was strategically selected. Additionally, quenching efficiency required



optimization by choosing a right FRET donor-acceptor pair with maximal spectral overlap. *fumigatus* and *A. amstelodami* were identified as quencher and target analytes, respectively, for the ensuing FRET complex, as depicted in (Figure 3a-b). It took the optimized displacement immunoassay no more than five minutes to find *A. amstelodami* concentrations as low as 10^3 spores/mL for identification. This observation was made while the baseline fluorescence stayed the same even though a negative control of 10^5 CFU/mL of heat-killed *E. coli O157:H7* was present. Scientists did some research and found that they could make detection more sensitive and signal variability less noticeable by creating a more reliable way to attach QDs to antibodies and construct FRET complexes. Optimizing quenching efficiency and regulating the number of antibodies present on QDs were both contemplated as potential strategies to attain reduced detection limits and consistent signal generation.


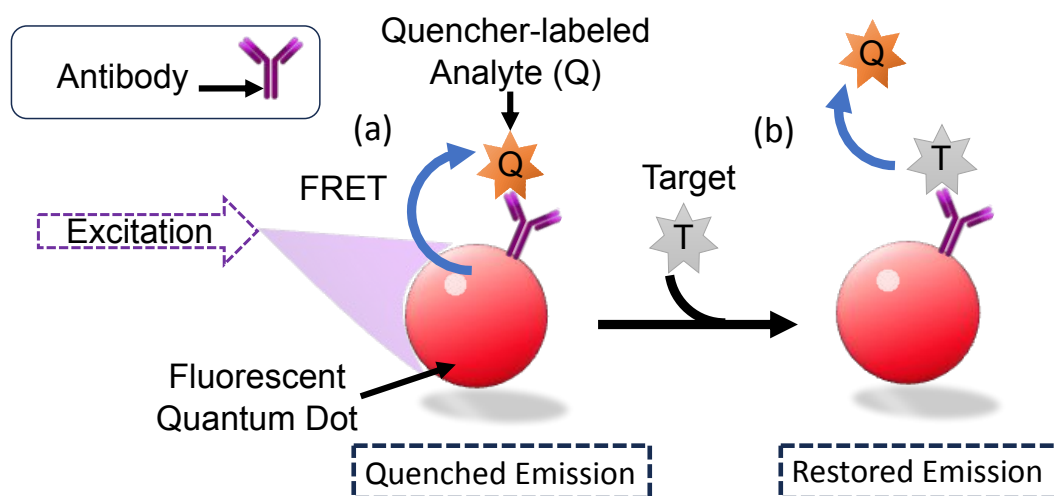


Figure 3: The mechanism of mold detection is illustrated in this figure (a) Antigen-binding of the QDs-conjugated antibody to quencher-labelled analyte results in the formation of the initial biosensor complex. The QD transmits its energy to the adjacent quencher molecules via FRET upon excitation (b) FRET is disrupted and an increased emission signal from the QDs donor results from the displacement of quencher-labeled analytes caused by the introduction of target analytes (47). Reprinted with permission from ref. (47) (copyright open access © 2011 MDPI).



In general, the FRET-based immunoassay has rapidly progressed which provides accuracy and specificity in identifying the fungus species. The FRET mechanism occurs more commonly in fluorescent compounds and, in some nanomaterials, particularly in QDs which have been utilized in the field of pathogen detection coupled with immunoassays offer more sensitivity but face drawbacks including high complexity and cost, stability issues, potential toxicity, and interference from autofluorescence. These challenges can complicate their use in pathogen detection, making alternative approaches like gold nanoparticles (AuNPs) for colorimetric sensing more appealing.

Building on the advancements in fungal spore detection technology, Lee et al., (48) presented a highly selective and sensitive colorimetric sensor based on AuNPs modified with a rodlet-binding peptide from *Aspergillus niger* spores. The authors highlighted the efficiency of receptor-modified AuNPs for real-time detection and their potential for mobile applications. Authors developed colorimetric sensor involving the design of gold nanoparticles (AuNPs) with a rodlet-binding peptide from *Aspergillus niger* spore-binding peptide (ASBP), as illustrated in Figure 4a. To identify the peptide, the scientists used phage display screening and found that a 12-mer peptide known as *Aspergillus niger* spore-binding peptide (ASBP) had a high affinity for binding to *A. niger* spores. They then investigated the use of ASBP-modified AuNPs for the real-time colorimetric detection of fungal spores. The research revealed that a substantial quantity of AuNPs modified with ASBP-based peptides efficiently adhered to particles measuring 3 to 5 μm *Aspergillus niger* spore particles size, causing noticeable color intensity variations in the AuNPs suspension as spores settled. This result demonstrated the strong performance of AuNPs modified with ASBP as efficient colorimetric sensors for *A. niger* spore detection, as shown in Figure 4b. The sensor system could detect as few as 50 spores in just 10 min and demonstrated an outstanding detection range of 50 to 100 spores, facilitated through a mobile device-specific application. These findings suggest that ASBP-



modified AuNPs could be a practical and efficient method for detecting *A. niger* spores with potential applications in mobile technology. The study contributes to broader efforts in developing portable and user-friendly biosensors for environmental and health monitoring, showing the potential of peptide-modified nanoparticles in creating efficient colorimetric sensors for pathogen detection.


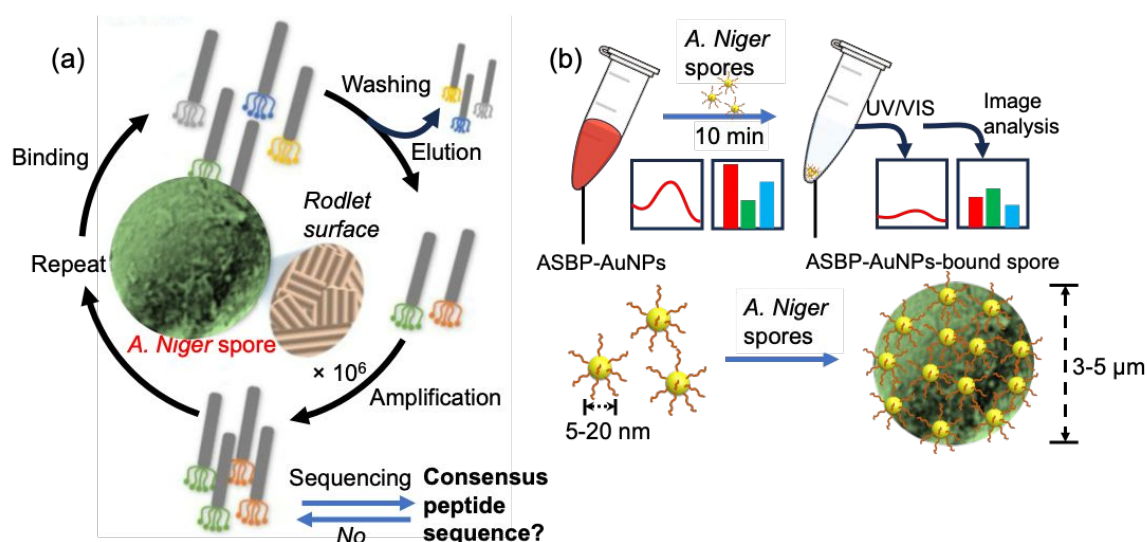


Figure 4: The process of *Aspergillus niger* for identifying spore-binding peptide ligands and their use in detecting fungal spores is illustrated below (a) Firstly, *Aspergillus niger* spore-binding peptide was discovered via screening of a phage display peptide library (b) gold nanoparticles were modified with *Aspergillus niger* spore-binding peptide (ASBP-AuNPs) to enable rapid colorimetric detection of *Aspergillus niger* spores. The change in colour of the *Aspergillus niger* spore-binding peptide-gold nanoparticles (ASBP-AuNPs) dispersion was analyzed by using either UV/Vis spectroscopy (48). Reprinted with permission from ref. (48) (copyright © 2021Published by Elsevier B.V.).

In line with advancement with mobile technology shifting away from bulky equipment for measurement and detection of signals, Ling Shan Yu et al. (57) developed a portable and cost-effective lab-on-a-chip sensor using nucleic acid-based techniques for detecting azole-resistant



Aspergillus fumigatus alleles. They emphasize the platform's compatibility with standard laboratory devices and its potential for early infection detection. The lab-on-a-chip platform utilizes a combination of both loop-mediated isothermal amplification (slightly similar method to PCR implications features discussed above), and ion-sensitive field-effect transistors (FETs) to detect azole-resistant alleles in *Aspergillus fumigatus*. Here, the authors chose two promoter regions with TR34 and TR46 mutations for detection because these mutations are associated with the ubiquitous mechanism of *Aspergillus fumigatus*. The ion-sensitive FETs fabricated using unmodified complementary metal-oxide semiconductor (CMOS) technology enable electrochemical sensing without the need for bulky and complex optical equipment. The loop-mediated isothermal amplification method amplifies specific DNA sequences through isothermal incubation, eliminating the requirement for thermocycling and reducing hardware complexity, power consumption, and diagnostic platform size. This device can accurately detect TR34 and TR46 alleles, responsible for azole resistance, with high sensitivity and specificity within 30 min.

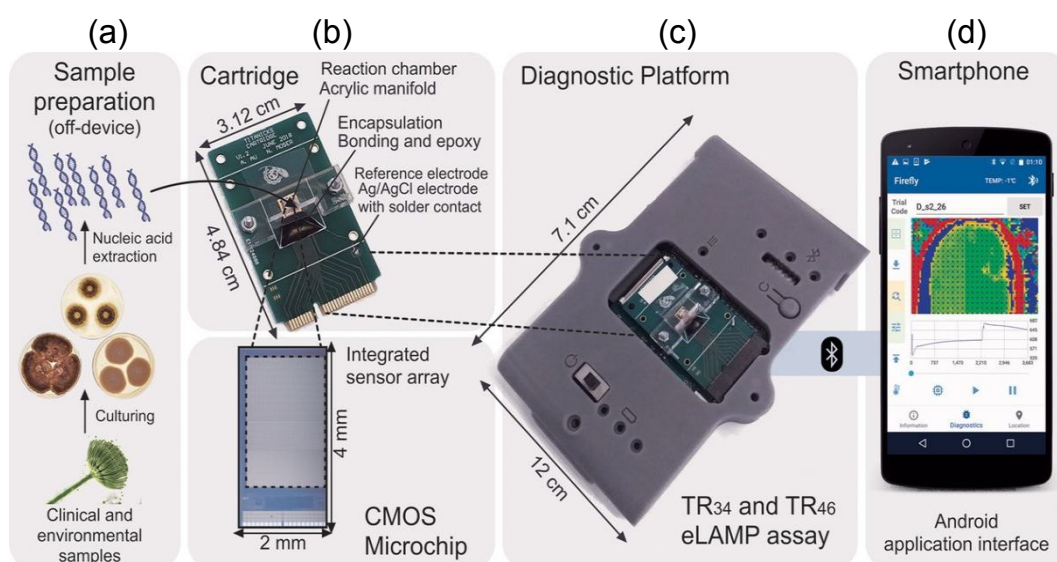


Figure 5: Demonstrates the following: (a) The diagnostic technique for identifying TR34 and TR46 using the lab-on-a-chip platform. After cultivating clinical and environmental



samples, nucleic acids are extracted in an off-device manner. Following this, (b-d) the nucleic acids that were extracted are merged with TR-LAMP reagents and transferred to a disposable cartridge that contains a CMOS microchip featuring 785x ISFET sensors. LoC diagnostic platform establishes a Bluetooth connection with a smartphone upon receiving the inserted cartridge. Reprinted with permission from ref. (57) (copyright open access © 2020 Published by American Society for Microbiology).

Additionally, the AndroidOS mobile application facilitates data acquisition, visualization, and cloud connectivity, making it a powerful tool for point-of-care and environmental surveillance, as illustrated in Figure 5(a-d). The efficacy of the detection method is confirmed by testing samples from various countries, showcasing a notable sensitivity with a detection limit of 10 genomic copies per reaction within 30 min. This work contributed to the field of point-of-care diagnostics and environmental surveillance by integrating nucleic acid amplification and CMOS technology. It aligns with global health initiatives aimed at combating antimicrobial resistance.

Further, other studies (58) introduced a novel nanoengineered plasmonic chip that utilizes colorimetric principle with localized surface plasmonic resonance (LSPR) to modulate bright-field colors for detecting *Aspergillus fumigatus* and develop a portable and smartphone-based detection systems. This approach departs from traditional dark-field imaging. The alternative strategy is well-suited for portable applications and can be integrated into smartphone-based detection systems, as illustrated in Figure 6. For biological specificity of the above sensor system, researchers employed a unique approach by dip-pen nanolithography (DPN) to functionalizing bioreceptors. This method systematically prints biomarkers in microscale, which facilitates high-throughput processes, streamlining the detection process for large-scale screening and simultaneous detection of multiple analytes. The nanofabrication process



combines three technologies, namely dip pen nanolithography, electron beam lithography and molecularly active self-assembly. This combination of techniques enabled the creation of Au-nanodisks (Au-NDs) as solid binding sites, which were subsequently modified with specific probe such as single-stranded DNA (ssDNA) for detecting fungal infections. The surfaces of these modified Au-NDs binding sites were coated with self-assemblies of silver nanoparticle (Ag-NP)-labelled target ssDNA. After the successful hybridization of the ssDNA (sandwiching), a color change occurs at the locations where the self-assembly of Ag-NPs took place. As a result, the electric field localization in the hotspots between the Au-NDs and Ag-NPs enhanced the Raman signals, allowing for Surface-Enhanced Raman Scattering (SERS) mapping.

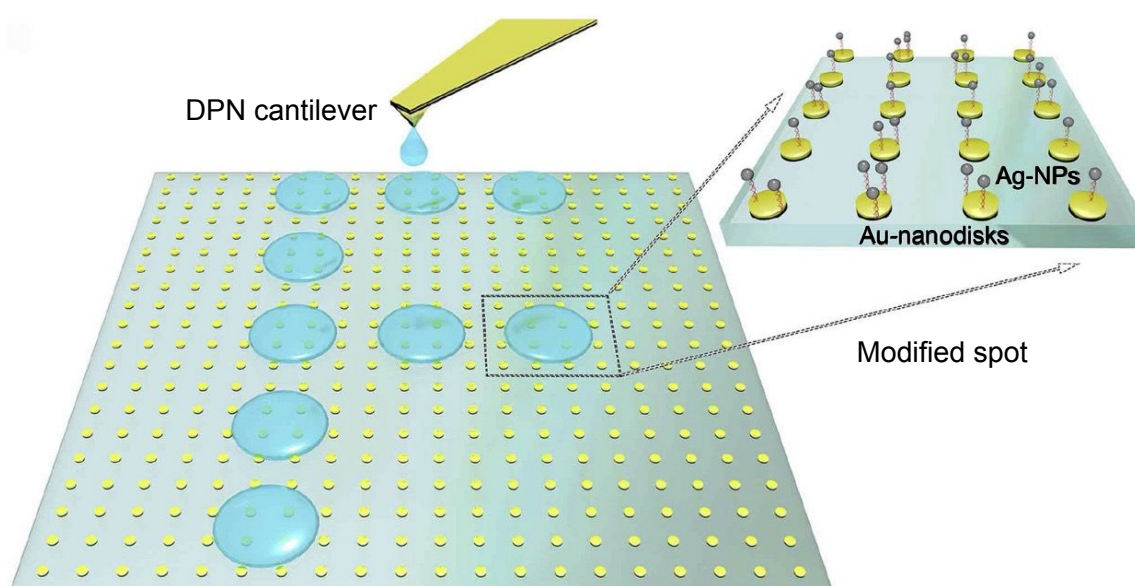


Figure 6: Schematic illustration of the fabrication process of plasmonic nanostructures. The bright-field image of Au-NDs is presented within a square surrounded by gold markers and a green-blue colour scheme. DPN is employed to immobilize and pattern the probe ssDNA onto the binding sites of Au-NDs. The utilization of this method produces the letter F on the left, which indicates an infection with *Aspergillus fumigatus*. A zoomed-in region on the right illustrates the process by which Ag-NPs self-assembles onto the Au-NDs-binding sites to the hybridization of the target ssDNA, which was initially modified by



DPN. Reprinted with permission from ref. (58) (copyright © 2019 Published by Elsevier [View Article Online](#)
DOI: 10.1039/D4NR01175A

B.V.)

The simplest plasmonic sensor system for detecting fungal spores is to mix clinical sample suspected of spores-contamination with receptor-labeled AuNPs. Tobiloba Sojinrin et al. (59) employed this method for detecting fungal hyphae and spores, including human cutaneous fungal infections. The sensitivity and rapid detection capabilities of AuNPs allowed for distinguishing between infected and uninfected samples. Leveraging the localized surface plasmon resonance properties of gold nanoparticles, researchers have devised a swift and sensitive method for detecting fungal hyphae and spores. Gold nanoparticles with a diameter of 40 nm were functionalized with a peptide sequence designed to bind to fungal cell-wall components. These nanoparticles were then exposed to various fungi, including *Candida albicans* and *Aspergillus fumigatus*. The LSPR peak shift observed indicated the binding of the nanoparticles to the fungal cells as illustrated in Figure 7. Researchers have also evaluated the nanoparticles on human skin samples infected with *Trichophyton rubrum*, a common cause of cutaneous fungal infections. These nanoparticles demonstrated the capability to differentiate between infected and uninfected skin samples with the aid LSPR peak shift phenomenon. This pioneering technology marks a significant advancement in the realm of fungal infection detection. This research builds on the application of plasmonic nanoparticles specifically for fungal infection detection, an advancement in biomedical diagnostics. It highlights the potential for clinical use and the importance of early diagnosis in preventing the spread of infections. However, several challenges remain, such as those identifying and harnessing the ability of natural biological receptors (host proteins, cell-wall/membrane structures, or nucleic acid probes that are derived from the analyte of interest, eg., fungal spores) or synthetic molecules



that serve as receptors, and effective ways to labelling them on nanoparticles, while preserving the nanoparticles' colloidal forms.

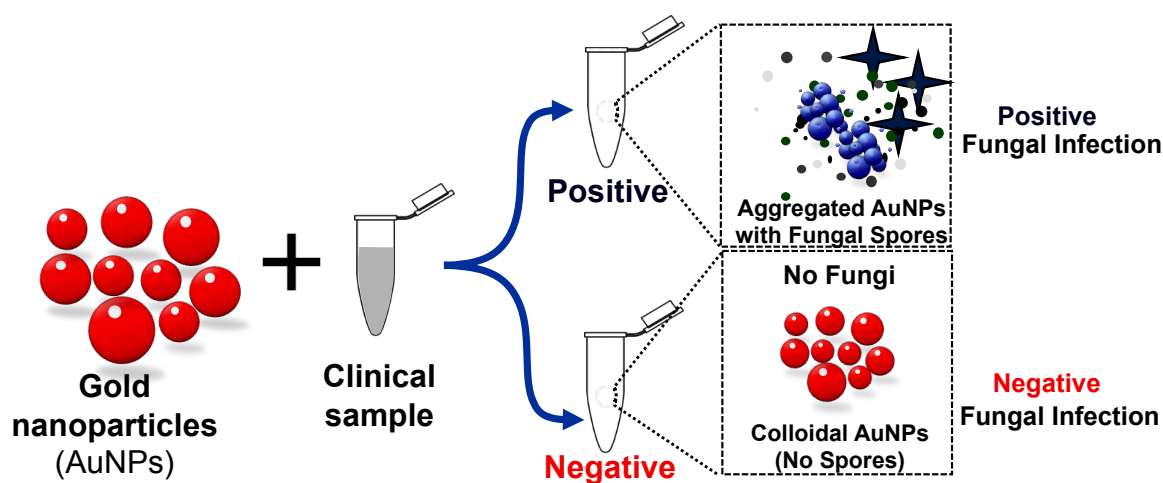


Figure 7: Schematic illustration of the gold nanoparticle system for plasmonic detection of fungi to facilitate self-diagnosis and hygiene control of clinical fungal infections. The progression in hue from red to pink to purple to blue signifies an escalation in the concentration of fungi present in a given clinical sample (59).

Other nanoparticles have non-LSPR features have been utilized for detecting fungal spores. For instance, Gaikwad and colleagues (60) developed an economical method for synthesizing carbon dot (CD) films for detecting *Aspergillus niger* spores. This method relies on the interaction between CDs and spores, leading to fluorescence quenching and potential applications in real-world settings. Here, CD films were synthesized using a flame/combustion technique at the liquid-liquid interface, and these CD films were deposited on quartz plates via the Blodgett process, as shown in Figure 8a-b.



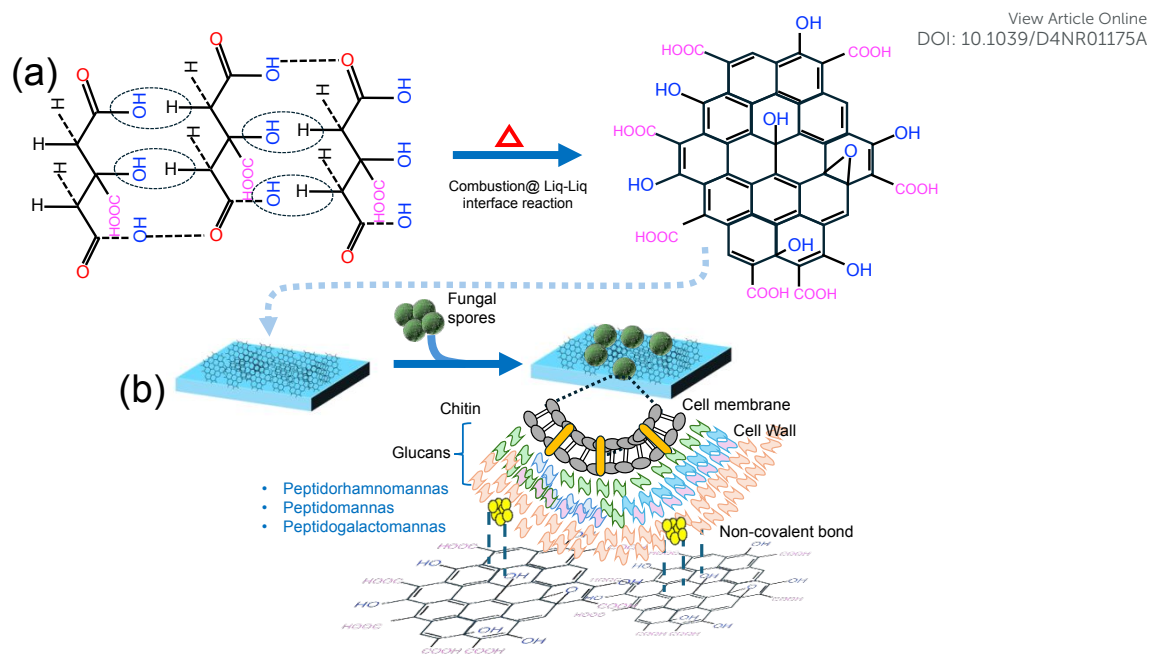


Figure 8: (a) Synthesis of the CDs-based sensor film using flame/combustion at the liquid-liquid interface. (b) Schematic representation of fungal spore detection using the CDs-based sensor film. Reprinted with permission from ref. (60) (copyright © 2019 Published by American Chemical Society).

The sensitivity of the CD film sensor towards *Aspergillus niger* spores was evaluated by measuring the fluorescence intensity against varying spore concentrations while maintaining a constant CD concentration. The resulting gradual decrease in the emission intensity of the CDs corresponded to the increasing concentrations of *A. niger* spores. To further assess the sensor films' ability to detect *Aspergillus* spores, a controlled environment was simulated in a closed wooden box, mimicking typical spore-rich conditions. Twelve sensor films were placed at different locations within the box. It was found that under moist environment conditions, the CD films tend to exhibit significant change in emission properties, while no change observed with the dry sensor films. This system responds efficiently under moist conditions that promote the interaction between the CDs and the fungal spores, conditions ideal for fungal propagation. The sensing mechanism operates by exploiting the increased accessibility of CDs' surface area under moist conditions, facilitating bonding with -OH and -COOH groups on the surface



through van der Waals and hydrogen bonds. This interaction leads to fluorescence quenching of CDs primarily to the inner-filter effect (IFT), where overlapping absorption regions hinder electron relaxation, resulting in quenching. To test the practical application of the sensor films, they were exposed in real-world settings such as near a dustbin, in food and fruit storage areas, and hospitals. The quenching effect observed in these environments mirrored the simulated tests, confirming the sensor films' effectiveness. This study contributes to the advancement of fluorescent sensors for environmental monitoring and food safety, while demonstrating the practicality of carbon-based nanomaterials in detecting fungal spores, aligning with efforts to create cost-effective and efficient biosensors. However, major challenge with this approach is associated with specificity and selectivity, which can be overcome by introducing the bio-/chemical receptors.

Jin Woo Seo et al. (49) employed cell-SELEX and spore-SELEX techniques to isolate aptamers specific to *Aspergillus* spores. The study highlights the high affinity and specificity of the identified aptamer, Asp-3, and its potential integration into sensors for detecting toxic *Aspergillus* species. Here, cell-SELEX and spore-SELEX techniques were employed to isolate aptamers capable of binding to the spores of three *Aspergillus species*, namely *A. fumigatus*, *A. flavus*, and *A. niger* (Figure 9 a-b). These fungal species are known to release airborne spores that can cause allergic reactions and severe invasive fungal infections (IFIs). After 12 successive iterative rounds of SELEX to identify aptamer candidates with high affinity and specificity for *Aspergillus* spores, the most efficient aptamer, Asp-3, emerged as a candidate for application as a bioreceptor (Figure 9c). The dissociation constant (K_d) values for Asp-3 towards *A. fumigatus*, *A. flavus*, and *A. niger* were determined to be 80.12 nM, 35.17 nM, and 101.19 nM, respectively. It has also been found that Asp-3 binds to certain cell surface proteins on the spore surface. Asp-3 demonstrated high specificity towards *Aspergillus* species compared to other fungal species. Furthermore, the aptamer exhibited a quantitative linear



relationship between itself and the concentrations of *Aspergillus* spores. These findings suggest that *Asp-3* is a promising candidate for integration with sensors to detect the spores of three toxic *Aspergillus* species. The robust binding affinity, specificity, and quantitative relationships of *Asp-3* position it as an asset in the advancement of sensor-based systems for the accurate detection of these perilous fungal spores. The research connects to the broader field of aptamer-based biosensors, emphasizing the potential of aptamers as selective recognition elements in diagnostic tools. It also supports ongoing efforts to developing sensitive and specific methods for fungal spore detection.

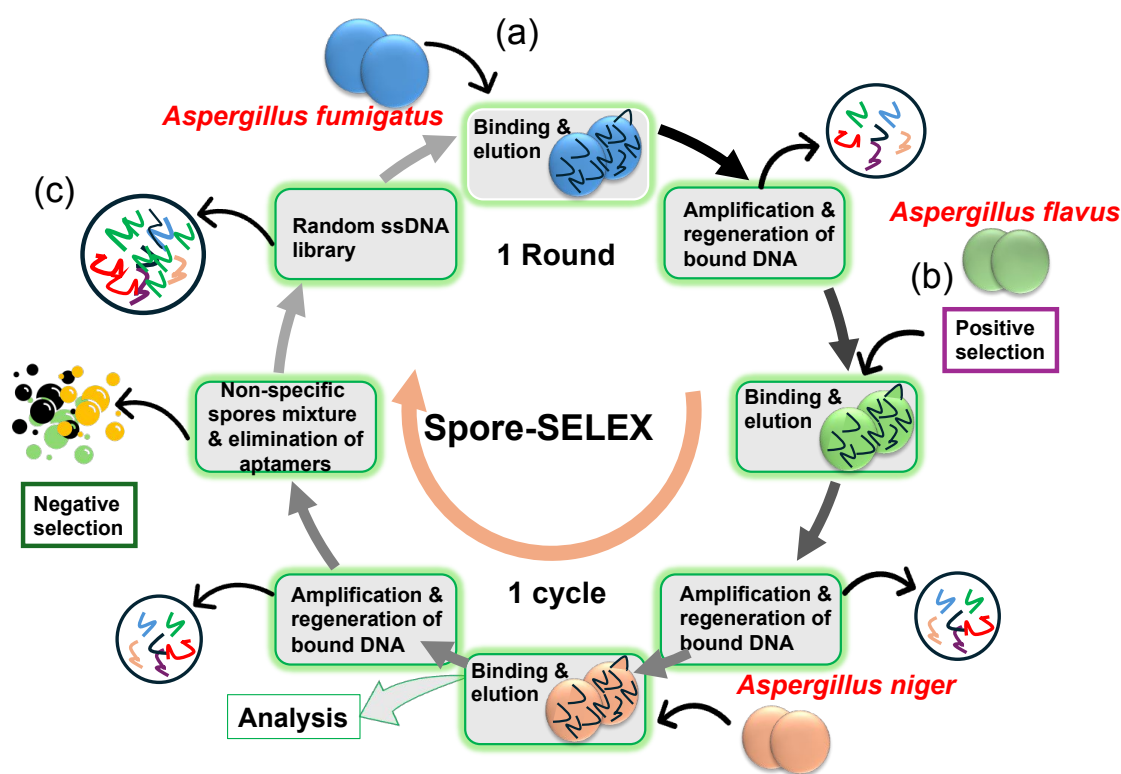


Figure 9: (a) Overview of the methods used to select aptamers that bind to the spores of three toxic *Aspergillus* species, starting with a random ssDNA library and undergoing four cycles of three rounds (a total of twelve rounds). (b) Positive selection was performed for *A. fumigatus*, *A. flavus*, and *A. niger*. (c) To exclude non-specific aptamers, negative selections were conducted at rounds 4 and 7 using non-specific spore mixtures (49) (copyright open access © 2021 Published by RSC).




Table 1 summarizes reported optical sensor performance parameters for the detection of fungal spores.

View Article Online
DOI: 10.1039/C4NR01175A

<i>Species</i>	<i>Dynamic range</i>	<i>LOD</i>	<i>Time</i>	<i>Ref.</i>
<i>Aspergillus niger</i>	50-1500 spores	50 spores	10 min	(48)
<i>TR34 and TR46 mutations associated with Aspergillus fumigatus</i>	5.6×10^3 - 2.9×10^5 copies per reaction	10 genome copies per reaction	20 min	(57)
<i>A. amstelodami</i>	10^2 - 10^5 spores/mL	10^3 spores/mL	Less 5 min	(47)
<i>Aspergillus niger</i>	1-16 CFU/mL	10 CFU/mL	2 min	(59)
<i>Aspergillus niger</i>	1.2×10^7 spores/mL	ND	3 h	(60)
<i>A. fumigatus, A. flavus, & A. niger</i>	5×10^5 , 10^6 , 1.5×10^6 , 2×10^6 , 5×10^6 , 1×10^7 spores/mL	ND	30 min	(49)

3.2 Electrochemical Biosensor

An electrochemical biosensor serves as a tool for detecting and quantifying biological substances (such as biomolecules, cells and pathogens) by transforming their interactions with a biological recognition element into electrical signals. These sensors find extensive applications in diverse fields, including medical diagnostics, environmental monitoring, food safety and biotechnology (56, 61, 62). Figure 10a-d depicts the operational principle of an electrochemical biosensor comprising three key components. (a) Biological Recognition Element: This element is designed to be specific to the target analyte (the biological substance under detection). It could be an enzyme, antibody, DNA/RNA aptamer, or any other biologically active molecule that selectively interacts with the target. The binding of the target



molecule to the recognition element initiates a biological reaction. (b) Transducer: The transducer is responsible for converting the biochemical signal generated by the biological recognition element as a result of interaction with a target analyte, into an electrical, optical, or mechanical signal that can be measured and analyzed. The electric/electrochemical transducer operates based on various electrochemical transduction techniques, such as amperometry, potentiometry, or conductometry (63, 64). Electrochemical measurement involves the interaction of the target analyte with the biological recognition element, leading to a change in the electrical properties of the sensor and the generation of an electrical signal. The magnitude of this signal is directly proportional to the concentration of the target analyte present in the sample. The primary types of electrochemical biosensors include amperometric biosensors, these biosensors quantify the current produced during a redox reaction. The presence of the target analyte triggers an oxidation or reduction reaction at the electrode surface, resulting in a current that is proportional to the analyte concentration. Potentiometric biosensors assess the potential difference between two electrodes. The binding of the target analyte to the recognition element induces a change in the surface charge, resulting in a detectable potential difference (62, 65, 66). Conductometric biosensors quantify alterations in the electrical conductivity of the medium between two electrodes. The recognition or binding of the target analyte to the element modifies the conductivity of the solution (62, 67, 68). The advantages of electrochemical biosensors include their high sensitivity, rapid response times and potential for miniaturization and integration with electronic devices. They have significantly contributed to advancements in healthcare, biotechnology, and environmental monitoring by providing fast and accurate detection of various biological substances.

View Article Online
DOI: 10.1039/D4NR01175A




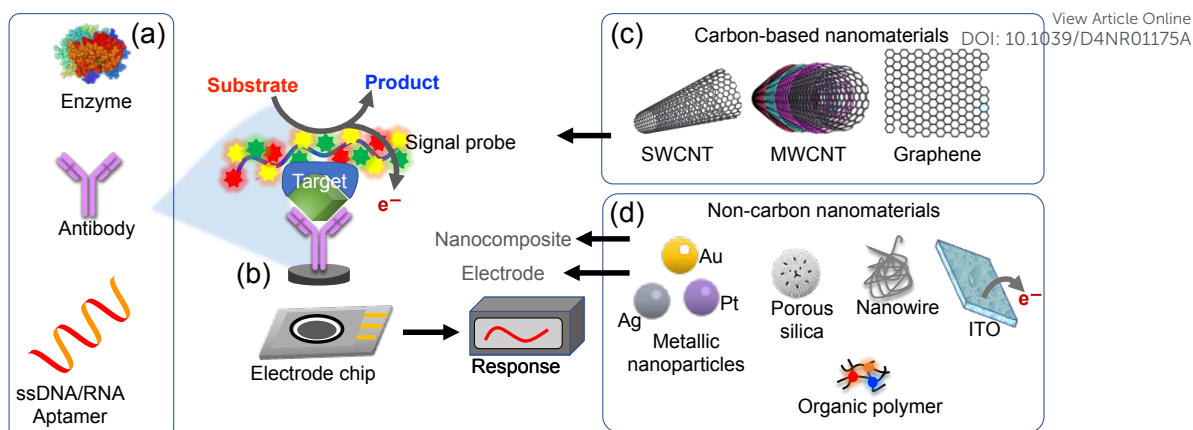


Figure 10: Schematic diagram of an electrochemical sensor: (a) biological recognition elements such as those but not limited to antibodies, enzymes, or DNA are designed for target specificity; (b) these elements are applied onto the working electrode, (c-d) materials that enhance the electrochemical signals that have been used to modify the working electrodes such as carbon and non-carbon materials such as SWCNT, MWCNT, graphene, NPs, polymers, or nanowires. The transducer converts biochemical signals into electrical signals, facilitating accurate measurement and analysis (69).

The following section explores recent advancements in biosensing technologies for fungal detecting fungal contamination or spores, including electrochemical biosensors.

Identifying specific bioreceptors for fungal infections is challenging for two reasons, not all fungal species invasive in nature, and their invasion is largely depends on host's susceptibility, resistance, and immune response, particularly in individuals with compromised immune systems. Therefore, targeting the specific virulent gene as a genetic biomarker for fungus that cause infections, such as Invasive Aspergillosis (IA) proves to be the effective approach to biosensing. For instance, *gliP* gene of a few *Aspergillus* species is linked to the cause of IA disease. Oligonucleotide probe for this *gliP* gene (glip-T) has been utilized as a genetic biomarker for electrochemical biosensing of virulent *Aspergillus* species. The biosensor's sensitivity and specificity, marking the first direct detection of glip-T using a biosensor has been reported (70). This biosensor was constructed by immobilizing glip-P onto



chitosan-stabilized gold nanoparticles (AuNPs) attached to a 1,6-hexanedithiol (HDT) self-assembled monolayer (SAM) prepared on a gold electrode (Au-electrode). Detection of glip-T was accomplished through a hybridization reaction followed by intercalation of toluidine blue, yielding the analytical signal, as illustrated in Figure 11ab. The researchers optimized the analytical parameters for the biosensor, determined the detection limit of glip-T in both standard buffer and real sample matrix, and assessed interference caused by random nucleotides and non-specific biochemicals. One of the advantages of utilizing oligo-probes on sensors is their ability to regeneration by simple chemical or physical denaturation, followed by their renaturing by bringing them back to normal conditions by washing or annealing. Detection limit as determined for glip-T by the above method exhibited $0.32 \pm 0.01 \times 10^{-14}$ (RSD < 5.2%), with a dynamic range between 1×10^{-14} and 1×10^{-2} M concentrations of glip-T (70). It marks the first direct detection of glip-T from the fungal strain using a biosensor for IA diagnosis advancing the field of electrochemical biosensors for fungal infection diagnosis. It aligns with the need for rapid and sensitive diagnostic tools for life-threatening infections, contributing to improved patient outcomes.


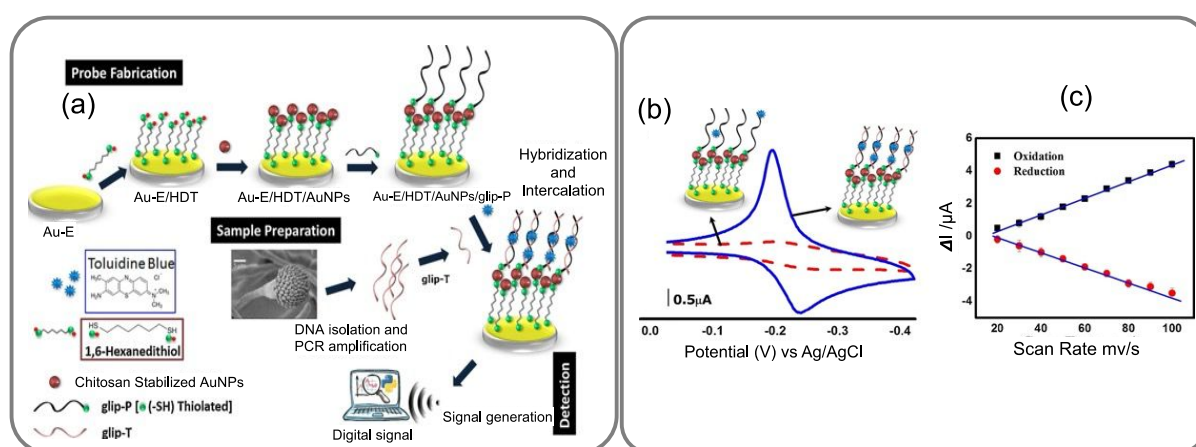


Figure 11: (a) The GLIP biosensor is fabricated by depositing a layer of gold nanoparticles on a gold electrode functionalized with hexane dithiol and immobilizing the GLIP protein on the surface of the AuNPs through covalent bonding. The GLIP biosensor detects target molecules based on the redox properties of the GLIP protein, which has three heme groups enabling it to



participate in redox reactions with various electron acceptors (b) CVs for Au-E/HDT/AuNPs/glip-P (red dotted curve) and Au-E/HDT/AuNPs/glip-P/glip-T (blue curve) after interacting with toluidine blue and (c) Plots of the redox peak currents vs scan rates for Au-E/HDT/AuNPs/glip-P/glip-T interacted with toluidine blue. Reprinted with permission from ref. (70) (copyright © 2018 Published by Elsevier B.V.).

A highly sensitive aptamer-based biosensor was introduced by Xin Ma et al. (71) for detecting gliotoxin using a dual-signal detection mechanism involving AIE and CRISPR Cas12a-mediated cleavage reaction. Gliotoxin (GT) is an epidithiodioxopiperazine metabolite synthesized by several pathogenic fungi, such as *Aspergillus fumigatus*, *Eurotium chevalieri*, *Gliocladium fimbriatum*, and various *Trichoderma* and *Penicillium* species. The biosensor was operated through a dual-signal detection mechanism, by initially activating the AIE effect through target-induced stimulation and subsequently initiating CRISPR Cas12a (LbCpf1)-mediated cleavage (Figure 12a-b). The aptamer-based biosensor involves two key stages: first, the interaction of the target with the aptamers results in the rapid breakdown of DNA building blocks, releasing Ac1 and forming ETTC-dsDNA, which aggregates, creating a fluorescence signal through the AIE effect. Second, the release of Ac2 triggers LbCpf1-crRNA, significantly enhancing ssDNA-Fc cleavage for signal amplification and achieving ultrasensitive target detection (Figure 12c). This approach successfully overcomes the challenge of weak electrochemical signals observed in previous gliotoxin sensors. The breakthrough technique not only reduces detection time by up to 55 minutes but also achieves an impressive low detection limit of 2.4 femtomolar. The biosensor exhibits a highly satisfactory linear range of 50 femtomolar to 1 nanomolar for gliotoxin detection, showcasing a more efficient and effective method for gliotoxin detection. This research contributes to the development of innovative biosensors combining aptamer recognition and CRISPR technology. It supports the trend towards creating highly sensitive and specific diagnostic tools for mycotoxin detection.



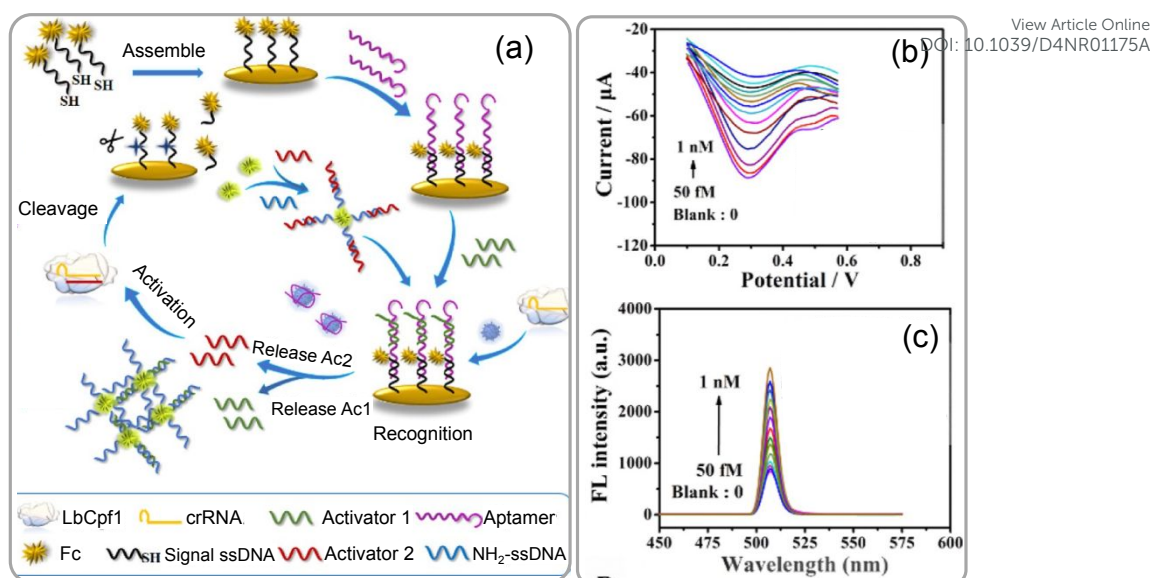


Figure 12: (a) Schematic representation of ultrasensitive electrochemical-fluorescent-biosensing method (b) The response of differential pulse voltage (DPV) was assessed at various concentrations of GT, and (c) variation in the fluorescence intensity of the biosensor at distinct concentrations of GT, as well as the calibration curve of $-\Delta I\%$ against the logarithm. The inset illustrates the calibration curve of $\Delta FL\%$ as a function of the logarithm. Reprinted with permission from ref. (71) (copyright © 2023 Published by American Chemical Society).

Other most efficient, rapid and cost-effective approach for biosensor transducer is field-effect transistor (FET) that detects binding of charged molecules, such as protein receptors on analyte surfaces to the gate of the FET. When these analytes bind, they change the charge distribution of the underlying semiconductor material, resulting in a change in the conductance of the FET channel. The change in current signal FET device can be easily measured. The FET-based biosensors offer advantages such as intrinsic amplification, small size, and compatibility with microfluidic devices for lab-on-chip applications. FET-based biosensors have been employed for fungal allergen detection. For instance, Joon-Hyung Jin et al., (39) presented a sensor designed for the swift detection of *Aspergillus niger*, a well-known allergenic fungal species. The study involves use of single-walled carbon nanotube (SWNT) field-effect transistors (FETs) that were functionalized with pentameric antibodies specifically binding to



Aspergillus species. By utilizing the electrostatic gating effect of the *Aspergillus* fungus this approach facilitated real-time, remarkable sensitivity, and selectivity in detection of *Aspergillus* sp.. The SWNT-FETs were initially functionalized with mouse *anti-Aspergillus* species-specific primary antibodies (WF-AF-1 Abs) by covalently attachment on SWNT channel using EDC/NHS chemistry, as depicted in Figure 13a-b. The sensor exhibited a detection range of 0.5-10 mg/mL with a detection limit of 0.3 pg/mL, representing a threefold improvement in sensitivity and a hundred-fold expansion in the detection range compared to any previously reported sensor (Figure 13 c-h). This research advances the application of carbon nanotube-based FETs in biosensing. It aligns with ongoing efforts to create highly sensitive and selective electrical biosensors for fungal pathogen detection, contributing to improved environmental and health monitoring.


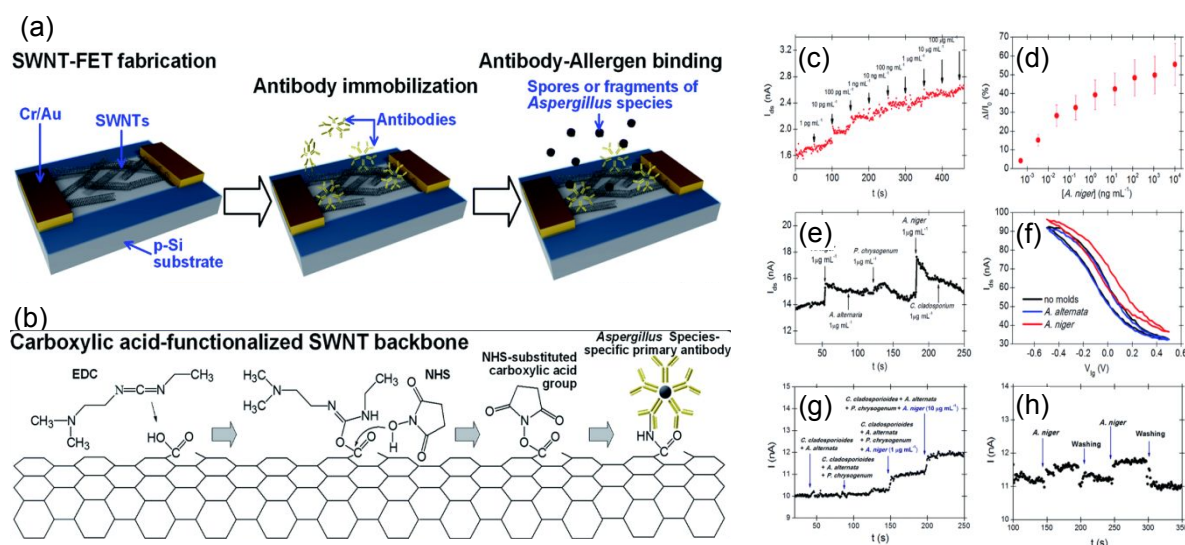


Figure 13: (a) illustration of the antibody-allergen binding and the fabrication of fungi sensors based on SWNT-FETs for binding of allergens (b) EDC/NHS chemistry was utilized to immobilize WF-AF-1 Abs directly onto the carboxylic acid-functionalized SWNT surface (c) The real-time response of an SWNT-FET device immobilized with WF-AF-1 Abs to a series of injections of varying concentrations of *A. niger*-suspended PBS solution (d) corresponding calibration curve (e) response of the functionalized SWNT-FET device in real-time to a random



succession of administrations of various mould-suspended PBS solutions (f) sensor possesses a liquid gating effect that is specific to target and non-target molds (g) Injection of four distinct mixtures of fungal solutions sequentially. The initial two mixtures do not contain *A. niger*, whereas the final two mixtures do contain *A. niger* in ten-fold different concentrations (h) Water and PBS buffer are used to thoroughly rinse the sensor to revive it. Reprinted with permission from ref. (39) (copyright © 2015 Published by RSC advance).

CNTs play a crucial role in FET biosensors because of their high surface-to-volume ratios and excellent electrical properties, biocompatibility and faster response times. Such FET biosensors can be integrated with microfluidic system, which enables extensive washing of the sensor device, sensor regeneration, extend the system operation time, allow for removal of interference from contaminants, especially from bioaerosols that contains micron-sized particles, such as microplastics. Junhyup Kim et al. [74] addressed the above issues and introduced the bioaerosol auto-monitoring instrument (BAMI), integrated with a bioaerosol sampler and two-channel carbon nanotube field-effect transistors (CNT-FETs), enabling real-time monitoring of airborne fungal particles (Figure 14a-b).


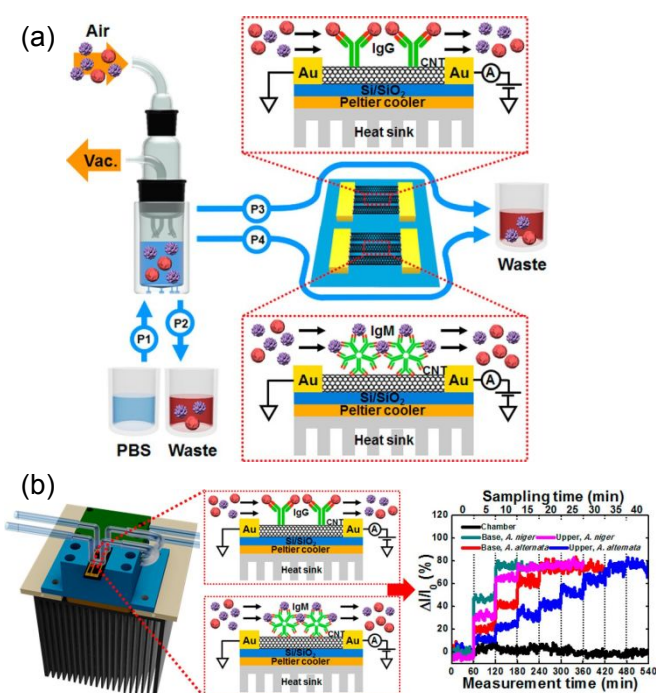


Figure 14: (a) Schematic diagram of the bioaerosol auto-monitoring instrument (BAMI) integrated with a bioaerosol sampler and two-channel carbon nanotube field-effect transistors (CNT-FETs) for real-time monitoring of airborne fungal particles. (b) Illustration of CNT-FET functionalization with specific antibodies for capturing airborne *Aspergillus niger* and *A. alternata* particles, resulting in changes in electrical conductivity for immediate analysis. Reprinted with permission from ref. [74] (copyright © 2016 Published by American Chemical Society).

The CNT-FETs functionalized with specific antibodies, captured airborne *Aspergillus niger* and *A. alternata* fungal particles, resulting in detectable changes in electrical conductivity for immediate analysis. This application in residential settings is crucial for maintaining indoor air quality and preventing health issues associated with fungal exposure. The integration of CNT-FETs with the bioaerosol sampler in a real-world environment demonstrated the system's capability to detect and differentiate between various airborne fungal species, specifically *Aspergillus niger* and *Alternaria alternata*. This enhanced both selectivity and sensitivity for environmental monitoring applications. By effectively identifying harmful fungal particles in homes, the BAMI system helps mitigate potential health risks associated with bioaerosols and ensure a safer living environment.

3.3 Miscellaneous sensor studies

Additionally, the section covers the use of biomarkers like glip-T for the biosensing of invasive Aspergillosis, electromagnetic biosensing techniques that detect changes in magnetoresistance in response to applied oscillating magnetic fields, and the detection of fungal spores or contamination using cantilever-based Atomic Force Microscopy (AFM).

Magnetic biosensors offer rapid and direct signal generation from the ligand-receptor interactions on the sensor surfaces. Giant magnetoresistance type of transducer platforms generate signal based on the dependence of electron scattering on spin orientation, observed in



multilayer structures composed of alternating ferromagnetic and non-magnetic conductive layers. GMR-based biosensors work by detecting changes in the magnetic field caused by the presence of magnetic nanoparticles or magnetic-labels attached to biological receptors. A notable example of such approach is reported recently (72), where a magneto-nanosensor biochip immunoassay method is employed for detecting *Aspergillus fumigatus* allergen *Asp f* using GMR spin-valve sensors. The study highlights the sensitivity and specificity of the detection process. GMR spin-valve sensors quantify the magnetic nanoparticle selectively bound to the sensor surface, as depicted in Figure 15a-d. In the initial steps, antibodies are covalently immobilized on the sensor surfaces. These antibodies are designed to specifically bind to the *Asp* allergens. Upon capturing the *Asp* of allergens, detection antibodies bind, forming a sandwich-like structure. This configuration enhances both the specificity and sensitivity of the detection process. The detection antibodies used are pre-biotinylated and subsequently labelled with nanometer-diameter streptavidin-coated magnetic nanoparticles. During the measurement process, the magnetic nanoparticles generate a stray magnetic field in response to an applied oscillating external magnetic field. This magnetic field induces changes in the resistance of the spin-valve sensor due to the GMR effect. These changes in resistance correspond to the specific biological signal being measured. The study contributes to the development of magneto-nanosensors for allergen, supporting the trend towards integrating advanced sensor technologies in immunoassays and enhancing their application in environmental and clinical diagnostics.

View Article Online
DOI: 10.1039/D4NR01175A



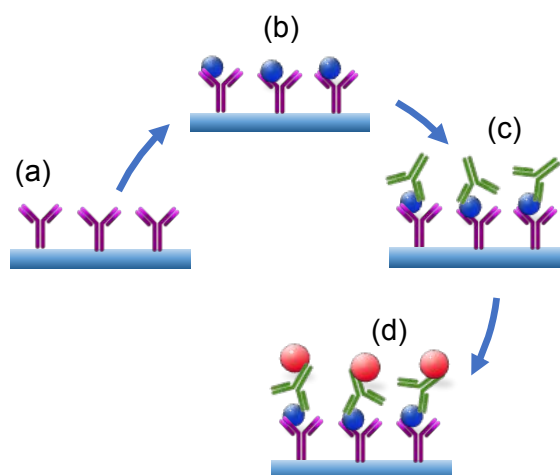


Figure 15: The schematic representation of the magneto-nanosensor biochip immunoassay involves several steps (a-b) immobilization of antibodies on the surface of the working electrode (c) sandwich structures are formed through the addition of biotinylated detection antibodies (d) magnetic nanoparticles bound to the detection antibodies generate a stray magnetic field that results in a change in sensor resistance due to the GMR effect (72).

Other rapid and direct biosensing approaches include cantilever-based atomic force microscopy (AFM) biosensors. This type of biosensor device utilizes the deflection of a microfabricated cantilever to detect and measure biomolecular interactions. Cantilever probes that go into this method can be chemically or biologically modified to tailor them to bind desired target analyte or biomarker on a given surface or medium. Nugaeva's research (73) explored similar technique for detecting individual fungal spores on cantilever surfaces. The authors emphasize the rapid detection capabilities and the potential for assessing spore contamination levels. In this study, two major fungal spores were chosen as a target sample to investigate a novel method for growth and detection using a cantilever array. The cantilever surfaces were functionalized with a variety of proteins. The researchers leveraged the specific biomolecular interactions of grafted proteins with the molecular structure on the fungal cell surface. It was observed that these proteins exhibited different affinities and efficiencies for binding to the spores. This discovery underscored the diverse and selective nature of the



interactions between the proteins and the spore surfaces, as depicted on the immunoglobulin-G functionalized cantilever surface in Figure 16. This rapid detection stood in stark contrast to conventional techniques that typically required several days. The biosensor demonstrated the capability to detect the target fungi in a range of 10^3 – 10^6 CFU/mL. The measured shift's magnitude was directly proportional to the mass of individual fungal spores, facilitating the assessment of spore contamination levels. This study connects to the broader field of AFM-based biosensors, demonstrating their potential for rapid and sensitive pathogen detection. It supports efforts to develop high-resolution and selective biosensors for environmental monitoring.

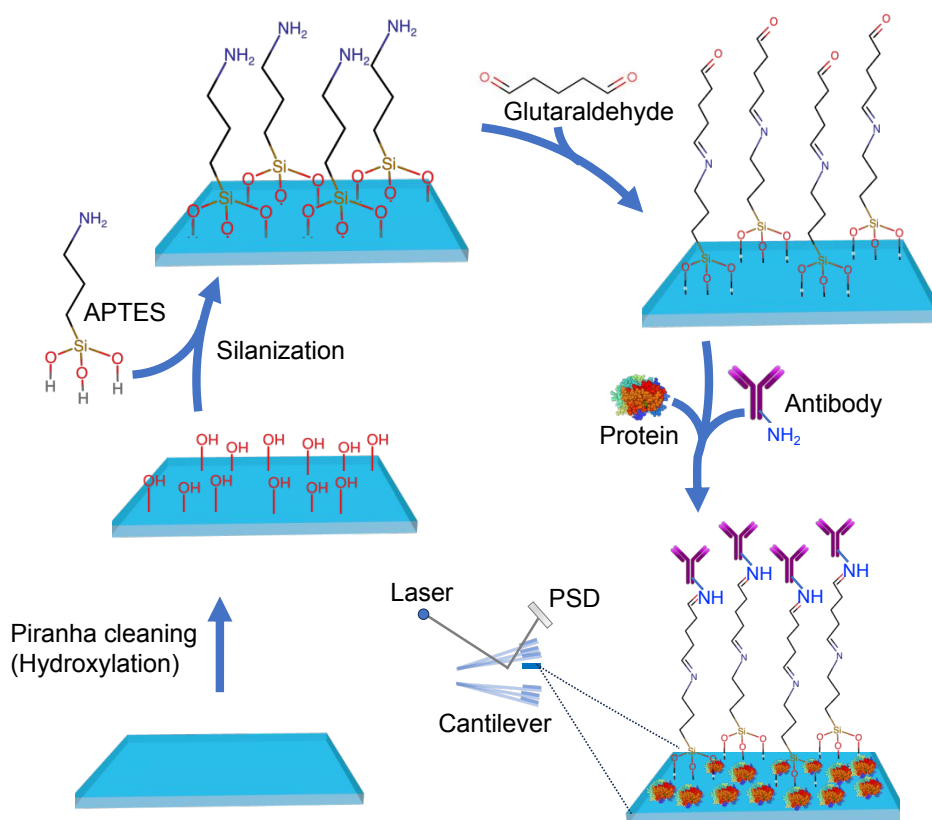


Figure 16: Scheme showing silicon microfabricated cantilever functionalization by treating the surface with APTES, glutaraldehyde followed by covalent attachment of anti-*Aspergillus niger* polyclonal antibodies ~IgG designed to capture fungal spores (73). Binding of spores to



the functionalized cantilever induces its deflection of laser beam falling on it which is sensitively detected by the position sensitive detectors (PSD).

Table 2: The summary of electrochemical sensor performance reported in the literature for detection of fungal spores.

<i>Species</i>	<i>Dynamic range</i>	<i>LOD</i>	<i>Time</i>	<i>Ref.</i>
<i>Glip-T</i>	1×10^{-14} - 10^{-2} M	0.32×10^{-14} M	30 min	(70)
<i>Aspergillus niger</i> <i>mold</i>	0.5 pg/mL-10 μ g/mL weighed amount of spores	0.3 pg/mL	NM	(39)
<i>Glitoxin</i>	50 fM- 1nM	2.4 fM	55 min	(71)
<i>Aspergillus niger</i> <i>and A. alternata</i>	10 pg/mL to 1 ng/mL and 10 pg/mL to 1 μ g/mL weighed amount of spores	10 pg/mL	5 min	(74)
<i>Miscellaneous sensor studies</i>				
<i>Magnetic biosensor- Asp f 1 allergen</i>	~0.1 to ~10 ng/mL	~0.1 ng/mL	NM	(72)
<i>Cantilever deflection biosensor- Aspergillus niger</i>	Used concentration 17 $\times 10^3$ CFU/mL	10^3 CFU/mL	4 h	(73)

3.4 Micro-fluidic Based Biosensors



Microfluidic biosensors are small equipment or systems that incorporate elements for signal transduction directly onto microchips (75, 76). Fluid regulation, target identification, signal transmission, and output are all necessary components of these biosensors. The critical factors that considerably impacts the performance of microfluidic biosensors are fluid control specifically via microchannels, microstructures, and diverse fluid actuation methods (77-79). Design of the microfluidic chips with a focus on appropriate materials and structures, holds paramount importance. The evolution of microfluidic chip concept has led to the development of 2D and 3D materials specifically designed for handling micro-volumes of fluid samples within the microfluidic chip modules. These materials include silicon (80), glass (81), quartz (82), polymethyl methacrylate (PMMA) (83), and polydimethylsiloxane (PDMS) (77, 84, 85). Biosensors integrated microfluidics allow substantial reduction in detection times due to their advantageous characteristics, which include minimal sample requirements and reagent usage, adaptable liquid manipulation, and process integration. These biosensors can then be incorporated with a variety of signal transduction modes including electrical, magnetic, and optical, enabling rapid identification and detection of desired analytes, such as fungal spores within minutes. Microfluidics-based biosensors, with their inherent features, have gained significant attention for detecting pathogenic fungi in various fields, including clinical diagnostics, food safety, and environmental analysis. The term "lab-on-a-chip" coined in 1979, refers to the imparted microfluidic chip's ability of biosensors to scale down fluid flow, heat, and mass transfer to the micrometre or nanometer scales. The microfluidics platform in conjunction with a bio-transducer (biosensor) can be successfully miniaturized to perform complex operations such as specimen preparation (sampling and capture), reagent manipulation, biological recognition, and detection (Figure 17a-c) (86).

View Article Online
DOI: 10.1039/D4NR01175A

Nanoscale Accepted Manuscript



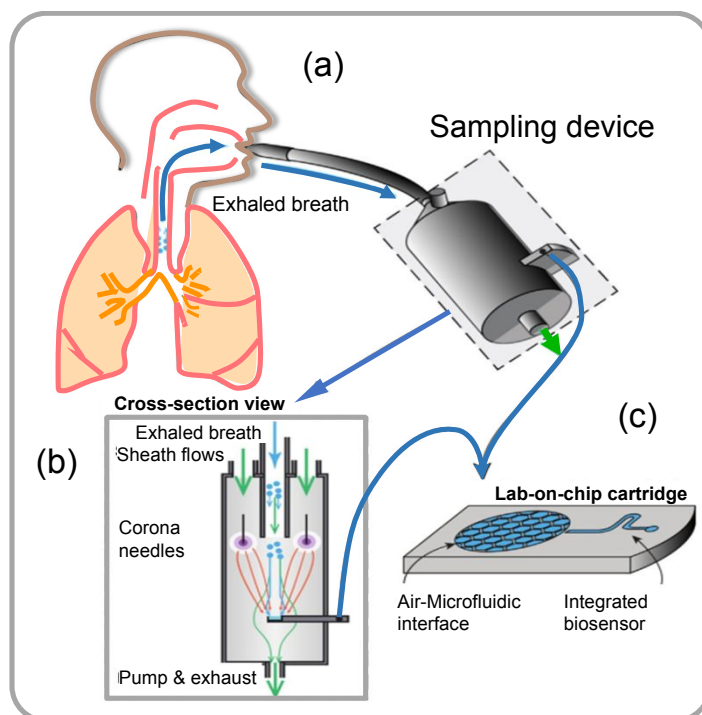



Figure 17: (a) Schematic illustration of a point-of-care (PoC) system designed for sampling aerosol from a high-volume of air directly into a microfluidic device that captures exhaled breath condensate, (b) sampling device cross-sectional view integrated with a microfluidic detector, (c) a lab-on-chip cartridge with a microfluidic interface that allows diagnosis from an exhaled-breath aerosol (86).

These operations, which are otherwise multi-step tedious processes involving higher costs and lengthy procedures, can be streamlined using this microfluidics technology. The continuous advancements in microfluidics-based biosensor technology highlight its potential for revolutionizing analyte detection applications across diverse domains. Microfluidic systems offer high-throughput screening (HTS) capabilities suitable for screening many samples with speed and sensitivity. Researchers have developed a nanoliter-range droplet-based microfluidic system specifically adapted for HTS of large filamentous fungi libraries for secreted enzyme activities.



Portable microfluidic chips are highly useful for conducting multiplexed reactions and detecting airborne fungal spores through sensing fungus-specific nucleic acids. The detection of fungal spores in the environment is challenging using conventional methods, largely due to their dispersion in a large volume area. Researchers have integrated a portable microfluidic chip device that automates the process of nucleic acid detection. This device mechanically lyses fungal cells or spores, treats the samples with reagents, and releases of fungal DNA required to perform Loop-Mediated Isothermal Amplification (LAMP) reactions. LAMP is a rapid and efficient DNA amplification technique that generates visible color change signals, making it a more advanced alternative to traditional PCR [50]. The integrated microfluidic chip device is designed with multiple reaction chambers, each capable of performing independent LAMP reactions. These chambers are connected through microchannels, with a single inlet and three air vents (as shown in Figure 18a-e). For the LAMP reaction to occur, the device requires the target DNA sequence from fungal cells or spores in aerosol, a set of 4-6 specially designed primers (short fragments that stick to ends of the target DNA), a DNA polymerase enzyme that copies the target DNA as a template with the primers and building blocks (deoxynucleotide triphosphates, dNTPs) to finally amplify at a 60-65 °C. Fluorescent dyes in the reaction is added to intercalate the amplified double-stranded DNA to monitor and detect.

The integrated microfluidic device enables quick and efficient detection of various fungal species, such as *Aspergillus fumigatus*, *Aspergillus flavus*, and *Cryptococcus* spores making it a valuable tool for environmental monitoring and diagnosis. To validate the device's performance, a simulated spore-aerosol of *A. fumigatus* was generated and collected using a wet cyclone sampler into 4 mL 1 M sorbitol containing 0.5% Tween 20. After air sample collection, 100 µL of the sample was counted using Petri film and mold count Mold™ to determine the *A. fumigatus* spores quantity in the simulated air samples. The conventional real-time fluorescence LAMP assay carried out in Eppendorf tubes was able to detect spore samples



ranging from 4×10^3 to 4×10^6 spores, while same assay performed using the microfluidic chip device showed consistent signals confirming for 4×10^3 to 4×10^6 spores/sample (as shown in Figure 18f). The above study demonstrated that the integrated microfluidic chip device has the potential to revolutionize the detection of airborne fungi by providing a rapid and efficient method to detect fungal spores [50]. By providing accurate and reliable results, this innovative technology could help protect people's health and safety by identifying potential fungal hazards in the air.


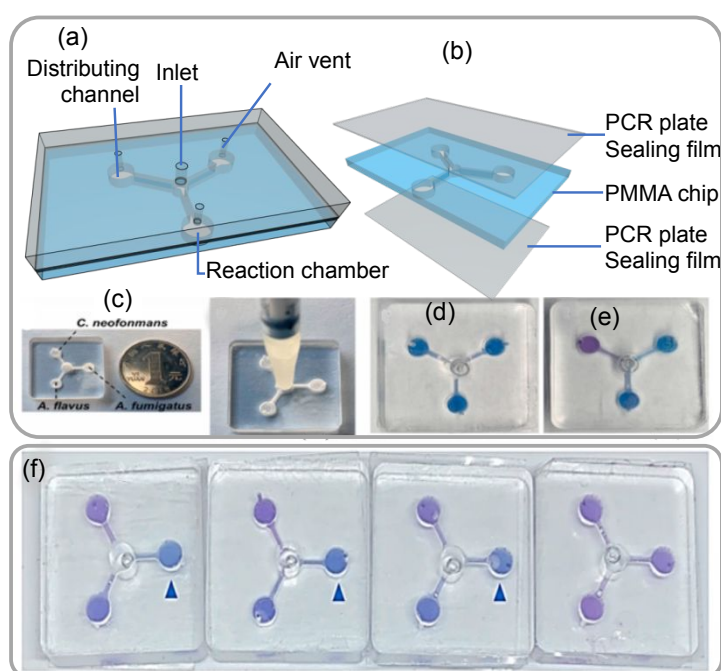


Figure 18: (a) Description of the apparatus (b) assembly of the chip (c) three sets of primers were preloaded with 0.5% low melt agarose in the reaction chamber (d) The chip's adapter (e) Verification of the possibility and cross-contamination of LAMP assays implemented on the microfluidic chips (f) Outcomes of the colorimetric LAMP assays conducted on the chips at 4×10^6 , 4×10^5 , 4×10^4 and 4×10^3 spores per sample. Reprinted with permission from ref. [50] (copyright © 2022 Published by Elsevier B.V.).

Other portable and automated microfluidic devices that are made of different material, design, detection method has been tested for detecting fungus. Zeng et al. (87) developed a microfluidic platform for detecting *Aspergillus niger* spores using immunoassay reactions on



carboxyl-modified microspheres with a size of 20.38 μm that were utilized to capture specific spores (Figure 19a). Microspheres were immobilized with polyclonal rabbit antibodies and introduced into the reaction channels of a microfluidic device for spore detection (Figure 19b). Detection of spores is carried out by sandwiching with a FITC-labeled anti-mouse secondary antibody injected into the reaction channel and the detection of signal from the sandwiched complex can be observed under a microscope, such as Nikon Eclipse Ti fluorescence microscope (Japan) (Figure 19 c-d). This microfluidic chip device comprised 16 identically designed channels (0.04 mm high \times 0.6 mm wide \times 40 mm long), arranged symmetrically from the center with a shared airflow outlet. Each channel had an inlet for air/liquid and a joint hole for liquid flow with a flow rate of 1.3–1.45 $\mu\text{L}/\text{min}$ (80–90 mL/min for each of the 16 channels (Figure 19e-f). The sensor's specific working range was determined to be 300 spores/ m^3 , with a limit of detection (LOD) of as low as approximately 20 spores. This research advances the application of microfluidic platforms in fungal spore detection. It supports ongoing efforts to develop sensitive and specific biosensors for environmental and health monitoring.

View Article Online
DOI: 10.1039/D4NR01175A




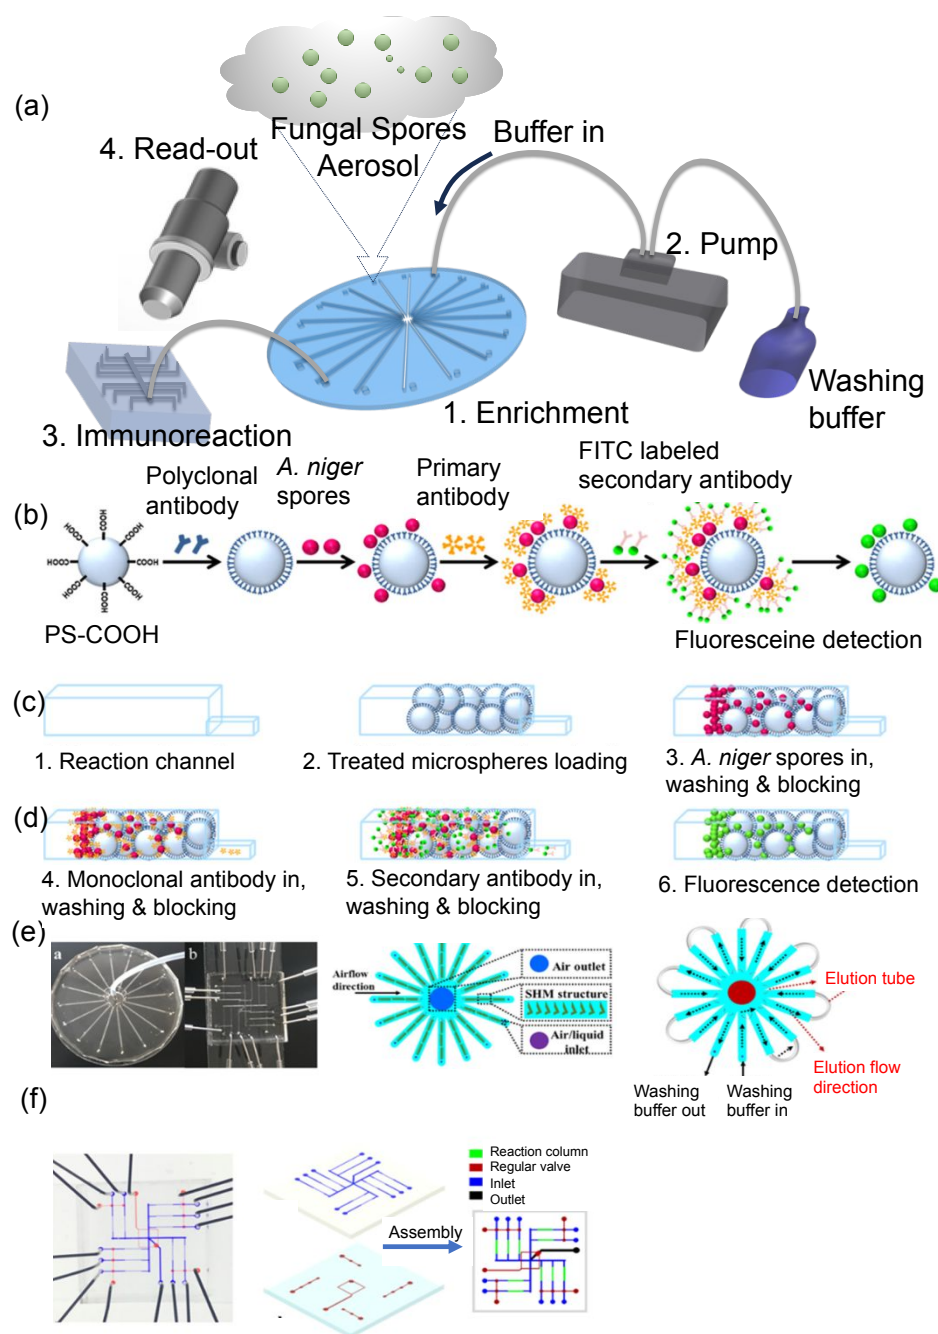


Figure 19: (a) Diagram showing the design of a microfluidic device (b-d) Steps involved in conducting immunoassay reactions for detecting *A. niger* spores on microspheres (e) Illustration of the open and closed inlet and outlets of a microfluidic system used for enriching and detecting airborne spore aerosols during the *A. niger* spore analysis on the detection chip (f) Snapshot of the detection unit, displaying the fluid layer and control layer



Reprinted with permission from ref. (87) (copyright © 2018 Published by American Chemical Society). View Article Online
DOI: 10.1039/D4NR01175A

Other detection schemes can be integrated with microfluidics to generate the signal, such as those reported for fungal enzyme activity measurements (88). For instance, a microfluidic platform is integrated for systematically screening for *Aspergillus niger* strains by probing the enhanced α -amylase activity from fungus. Well-designed microfluidic devices were employed to generate droplets with a volume of 18 nL containing a fluorogenic substrate for enzyme α -amylase activity, which promoted encapsulation of individual spores and enabled measurement of enzyme activity (Figure 20a). The droplets generated by this device-setup composed of a fluorinated oil phase and a fluoro surfactant (KryJeffD900), which facilitate efficient gas delivery to the spores during the incubation period. Spore density within the droplets followed a poisson distribution, maintaining an average number of spores per drop (λ) ranging from 0.1 to 0.3. Over the course of a 24 h incubation at 30 °C, the spores underwent germination, hyphal growth, and α -amylase secretion. The α -amylase activity within the droplets was accurately evaluated using a fluorogenic substrate, and a sorting device with cross-side configuration electrodes enabled the sorting of droplets based on their α -amylase activity (Figure 20b). The sorted fungi were then subsequently retrieved, sporulated, and subjected to further characterization to assess their α -amylase production. This innovative microfluidic platform demonstrated its efficacy in screening large whole-genome mutated libraries of *Aspergillus niger* strains, leading to the identification of strains exhibiting significantly enhanced α -amylase overproduction. Notably, the researchers applied this approach to the strain O58, renowned for its reference production of Soufflet α -amylase, exposing it to a chemical agent during the screening process, thereby proving to be a successful strategy. Furthermore, a robotic microfluidic platform is utilized to screen a sorted fungal population on a solid medium derived from rapeseed meals. After analyzing 1272 sorted fungi with α -amylase activity, 98.9%



of the sorted fungi displayed α -amylase activity, with most displaying activity levels similar to O58. These findings demonstrate the efficiency of the microfluidic platform in identifying strains of *Aspergillus niger* with enhanced α -amylase production potential. This approach connects to the broader field of microfluidic screening platforms, demonstrating their potential not only in industrial biotechnology applications, but also can be applied to detecting fungus in the environmental and clinical settings.


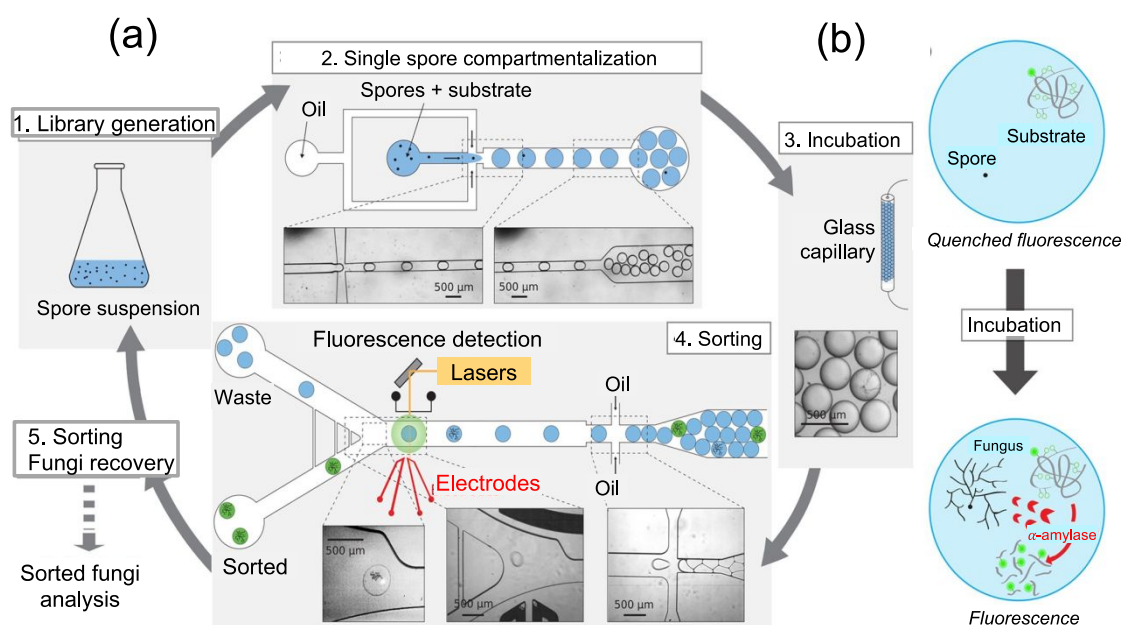


Figure 20: (a) Schematic illustration of sorting fungal spores using microfluidic devices and encapsulation of droplet containing labeled enzyme's substrate; 1. Spore suspension from a whole genome mutated library of fungi; 2. A suitable spore-to-droplet ratio is utilized to compartmentalize the spores into 10 nL droplets containing a fluorogenic enzyme substrate through emulsion; 3. For fungi growth, enzyme secretion, and substrate digestion within the particles, the emulsion was incubated off-chip at 30 °C by passing through a glass capillary tube for 24 h; 4. Enzymatic activity-based sorting of droplets is achieved by reintroducing them into a microfluidic sorting device and assessed their fluorescence intensity; 5. Fungi are extracted from the sorted droplets and subsequently undergo another round of mutagenesis and/or selection, characterization, or α -amylase



fluorogenic assay. (b) Substrate is composed of a backbone composed of starch and numerous neutralized (quenched) BODIPY[®]FL fluorophores. Once the starch backbone is hydrolyzed by α -amylase, the quenched fluorophore unquenches leading to the generation of fluorescence signal (88) (copyright open access © 2016 Published by Springer Nature).

Further developments in microfluidic devices used for detecting fungi can be found in the literature (89) that combines nanoelectrode activation and microwell arrays to achieve highly efficient capture and quantification of the airborne fungal pathogen *Sclerotinia sclerotiorum*. The nanoelectrodes serve to attract and immobilize the fungal spores, enabling their efficient capture within the microwells for subsequent analysis as shown in Figure 21a-b. The microwell array provides a high-throughput platform for capturing multiple fungal spores simultaneously, allowing for efficient quantification of the pathogen in the air sample. By exploiting the unique properties of nanoelectrodes and microwells, this system offers improved sensitivity and specificity in detecting *Sclerotinia sclerotiorum* compared to traditional methods. This innovative approach holds promise for advancing the field of airborne pathogen detection and could have significant implications for disease surveillance and control strategies (89). Table 3 summarizes reported performance parameters for microfluidic sensor for detection of fungal spores.

View Article Online
DOI: 10.1039/D4NR01175A

Nanoscale Accepted Manuscript



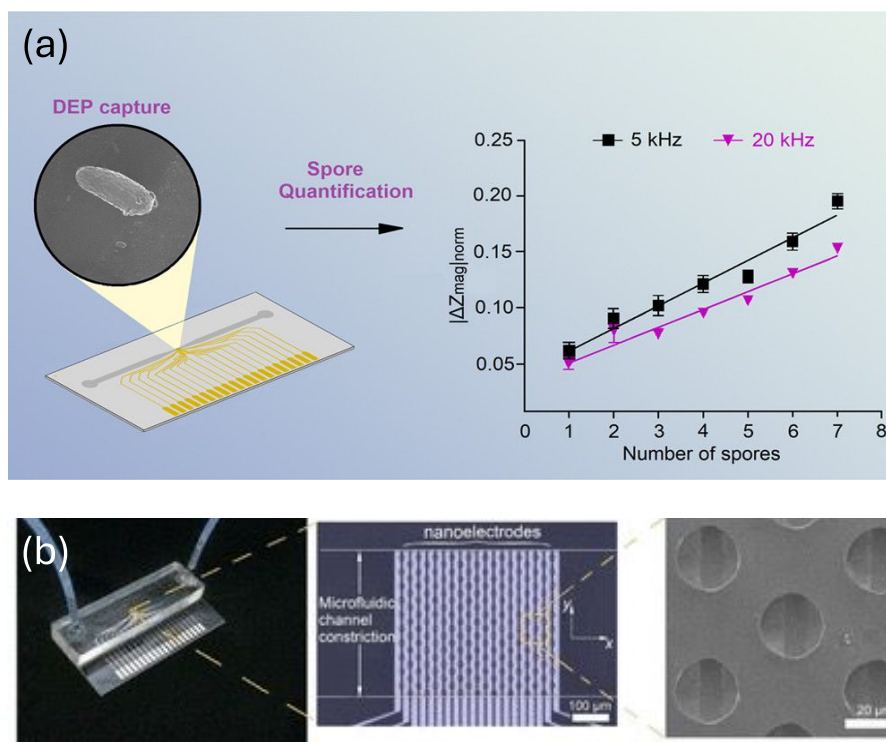


Figure 21: (a-b) A microfluidic device comprising 190 microwells and 20 aluminium nanoelectrodes adapted for performing dielectrophoresis (DEP) to capture spore, and the results of individual electrochemical impedance spectroscopy (EIS) measurements is shown in the line plot on right, enabling precise quantification. Reprinted with permission from ref. (89) (copyright open access © 2021 Published by American Chemical Society).

Table 3: Table showing reported performance parameters for microfluidic sensor for detection of fungal spores.

<i>Species</i>	<i>Dynamic range</i>	<i>LOD</i>	<i>Time</i>	<i>Ref.</i>
<i>Aspergillus fumigatus</i> , <i>Aspergillus flavus</i> , and <i>Cryptococcus</i>	4×10^3 - 10^6 spores/sample	4×10^4 spores	90 min	(50)
<i>Aspergillus niger</i>	1.1×10^6 spores/mL	~20 spores	1 h	(87)



<i>Aspergillus niger</i>	10 ⁴ clone library	Screening of clones ~7,000 h ⁻¹	90 min	(88)
<i>Sclerotinia sclerotiorum</i>	~2 × 10 ⁴ spores/mL	Single spore detection range	~20 s	(89)

The approaches described above for optical, electrochemical and microfluidic based sensors present distinct strengths and weaknesses. Optical sensors, particularly FRET-based assays, demonstrated rapid detection times and high sensitivity for specific fungal species. Colorimetric sensors using AuNPs showed impressive sensitivity and selectivity, with potential for mobile applications suitable for remote settings. Lab-on-a-chip platforms provide portability and a cost-effective solution with high specificity integrating well with standard laboratory devices. Plasmonic chip-based methods offer innovative approaches for portable and smartphone-based detection systems, emphasizing the versatility of optical sensors in various settings.

Electrochemical sensors demonstrate exceptional sensitivity and specificity, often utilizing aptamers or antibodies for targeted detection. Advanced techniques such as magneto-nanosensors and AFM-based methods provided robust and innovative solutions for real-time and high-sensitivity fungal detection. These sensors showed potential for clinical and environmental applications, offering rapid and accurate detection capabilities.

Microfluidic biosensors excel in providing rapid, efficient, and high-throughput detection options suitable for screening large number of samples with speed. These platforms enable the integration of advanced detection techniques such as LAMP and immunoassays in a compact




and portable format. The ability to perform real-time monitoring and high-throughput screening makes microfluidic biosensors highly suitable for both environmental surveillance and industrial applications. The versatility and scalability of these platforms highlighted their potential for widespread adoption in various fields.

Each approach offers distinct advantages in fungal detection.. The choice of method however depends on the specific application requirements, including sensitivity, specificity, detection speed, and practical deployment scenarios, ensuring that the most appropriate technology is used for each unique situation.

4. Commercially Available technology/product for airborne fungal spores

Monitoring airborne fungi and other bio-aerosols in public places and hospitals is crucial for maintaining indoor air quality and mitigating potential health risks. Various bioaerosol sampling instruments have been developed, each exhibiting distinct mechanisms, performance characteristics, and analysis methods. This section provides an in-depth examination of commercially available technologies employed in public places and hospitals, emphasizing their fundamental principles.

Portable and cost-effective lab on-chip platforms have been developed for the detection of infectious diseases using nucleic acid-based techniques. For example, Myconostica Ltd. is designed for the specific detection of genomic DNA from 15 distinct *Aspergillus* species. This assay particularly targets the four most prevalent pathogenic species: *A. fumigatus*, *A. flavus*, *A. terreus*, and *A. niger*. The foundational principle of this diagnostic test relies on molecular beacon real-time polymerase chain reaction (RT-PCR) technology, with the multicopy 18S ribosomal RNA (rRNA) gene as its target. To ensure result accuracy, the assay incorporates an internal amplification control (IAC) sequence from plant sources, crucial for identifying inhibitory factors that may impede the PCR process in the test sample. In the experimental



procedure, PCR reactions are carried out on the Cepheid Smart Cycler, using 10 microliters of DNA template in a final reaction volume of 25 microliters, following manufacturer guidelines. The determination of PCR positivity is based on a predetermined threshold of 36 amplification cycles, corresponding to an analytical sensitivity capable of detecting around 50 copies of the 18S rRNA gene. Notably, this sensitivity is approximately equivalent to the genomic content of a single *A. fumigatus* microorganism (90). The above example method for specific detection of fungus is largely similar to the classical method that has used for popular COVID-19 tests that are not only conducted in centralized laboratories, but also slow, labor intensive, and expensive. However, they provide clues to the current challenges and researchers are continuously attempting to advance detection technologies that are highlighted in the above section. A few other classical tools for detecting fungus that have been commercialized are described in the following sections.

4.1 MycoGenie (*A. fumigatus*; TR34/L98H)

Ademtech in Pessac, France developed MycoGenie assay, which is intricately crafted for the detection of *A. fumigatus*, specifically targeting the 28S rDNA and the TR34/L98H mutation. This versatile assay accommodates a range of clinical specimens, including biopsies, respiratory samples, and serum samples, and is compatible with analytical platforms such as CFX96, ABI 7500, LightCycler 480, SmartCycler, MX3000, and the Rotor-Gene. A comprehensive validation study conducted by Dannaoui et al. in 2017 underscores the robust performance of the MycoGenie R assay. Utilizing 88 respiratory samples (59 culture-positive) and 69 serum samples from individuals with proven or probable aspergillosis, the assay exhibited exceptional sensitivity of 92.9% for respiratory samples and noteworthy specificity of 90.1%. Similarly, serum samples displayed 100% sensitivity and 84.6% specificity. In a broad investigation led by Guegan et al. in 2018, involving 387 subjects across hematological and non-hematological contexts, the MycoGenie assay underwent a rigorous comparative



evaluation against the AspergGenius assay and two distinct in-house assays. Analyzing bronchoalveolar lavage (BAL) samples, the MycoGenie assay demonstrated nuanced sensitivity profiles. Specifically, in patients with hematological conditions, a sensitivity of 53.7% was observed, highlighting its proficiency in detecting *Aspergillus* DNA in this cohort. Conversely, among non-hematological cases, the assay exhibited increased sensitivity at 75%, emphasizing its accuracy in detecting *Aspergillus* DNA. In this context, the AspergGenius R assay showed comparatively diminished sensitivities, highlighting the superior performance of the MycoGenie assay in this specialized diagnostic domain. Notably, sensitivities diminished in patients subjected to antifungal prophylaxis or treatment, suggesting the potential impact of therapeutic interventions on assay outcomes. Furthermore, the MycoGenie assay found meaningful application in the molecular detection of *Aspergillus* in French patients with fungal rhinosinusitis, alongside positive microscopy (N=137). Impressively, the assay yielded positive results in 77.4% of cases, a marked contrast to the 32.1% culture positivity rate. Another investigation by Denis et al. in 2018 positioned the MycoGenie R assay in a comparative context with the *A. fumigatus* Bio-Evolution R assay. Both assays maintained 100% specificity, while sensitivities stood at 71% (MycoGenie) and 81% (*A. fumigatus* Bio-Evolution). Notably, sensitivities remained robust against antifungal treatment, and no resistance markers were identified, demonstrating the assay's reliability [55]. In summary, the MycoGenie assay emerged as a promising diagnostic tool, particularly for its capability to identify a prominent azole-resistant mutation. While its diagnostic prowess is evident, further comprehensive data accumulation remains crucial to ascertain its definitive utility in clinical routine applications. The nuanced sensitivity modulation in the presence of therapeutic interventions underscores the intricate dynamics inherent in accurate assessment and interpretation in the realm of *Aspergillus* detection.

4.2 RenDx Fungiplex Assay



The RenDX, Fungiplex, assay is developed by Renshaw-diagnostic Limited., in Glasgow, UK which is based on a polymerase chain reaction method, targeting specific sequences within the 18S rDNA and 28S rDNA regions. Following PCR amplification, the assay incorporates surface-enhanced raman scattering for the selective and sensitive detection of targeted pathogenic oligonucleotides. Utilizing an *Aspergillus* probe alongside an extensive-range Saccharomycetales probe, the assay enables simultaneous detection of *Aspergillus* and *Candida* spp. In a validation study by White et al. in 2014, plasma samples from 14 predominantly haemato-oncological patients such as chronic leukemia, lymphoma, myeloma, and other disorders with proven/probable invasive aspergillosis (IA) and 80 patients without IA were examined. The assay demonstrated a sensitivity of 82.2% and specificity of 87.5%. Notably, the RenDX Fungiplex R assay transitioned to RT-PCR technology, prompting a reformatting of its operational framework (91). Regarding, the Fungiplex *Aspergillus* PCR assay developed by Bruker Daltonik GmbH in Bremen, researchers conducted a study to develop a Quantum Dots-based immunoassay for detecting *A. amstelodami* using FRET. Analytical performance in detecting DNA from *A. fumigatus*, *Aspergillus flavus*, *Aspergillus niger*, and *Aspergillus terreus*, as reported by Green and Dougan in 2017 (92).

Fundamentally, the RenDX Fungiplex assay demonstrates a sophisticated convergence of PCR and SERS technologies, designed for effective and accurate detection of pathogen-specific oligonucleotides with high sensitivity and specificity. While the assay holds promise in diagnostic capabilities and has embraced the transition to real-time PCR, a comprehensive assessment of its clinical utility, in comparison with the Fungiplex *Aspergillus* PCR assay, is still pending. Early assessments, nonetheless, highlight the assay's robust analytical proficiency in identifying diverse *Aspergillus* species, as evident from preliminary studies involving artificially introduced DNA samples.

4.3 AspergGenius. Assay



PathoNostics (Maastricht, Netherlands) devised the AsperGenius assay which is a multiplex real-time PCR that detect invasive aspergillosis (IA). It is compatible with the LightCycler 480, Rotor-Gene 6000 (Corbett), and Rotor-Gene. Q (Qiagen). This assay provides two respiratory secretions PCR assays; (a) Identification and distinction of *Aspergillus spp.* using the AsperGenius Species multiplex, which targets the 28Sr DNA. A probe for the *A. fumigatus* complex is incorporated, which provides coverage for multiple species, such as *A. fumigatus.*, *A. lentulus*, *A. udagawae* and *A. viridinutans*. Other probe is available to detect a different pool of fungus, such as *Aspergillus spp.*, which includes *A. fumigatus* complex, *A. terreus*, *A. flavus*, and *A. niger*, and (b) Identification of four azole resistance markers (L98H, TR34, T289A, Y121F) within, the Cyp51A gene of *A. fumigatus* using AsperGenius Resistance multiplex R. This assay provides good clinical performance with the added ability to detect azole resistance directly from noninvasive serum samples. While the available fungal burden may limit its application, it represents a significant classical diagnosis and management of aspergillosis.

5. Conclusion and future perspectives

In this comprehensive review, we have explored various technologies and assays specifically developed for the detection of airborne fungal spores present in the air, with a particular emphasis on *Aspergillus species*. The integration of innovative platforms, including optical, electrochemical, microfluidics and molecular diagnostics, has significantly enhanced the precision and efficiency of fungal spore detection. The advancements discussed in this review underscore the importance of continuous innovation in the field of fungal spore detection, crucial for maintaining indoor air quality and preventing associated health risks. These technologies offer valuable insights into the prevalence characteristics of airborne fungal spores, aiding in timely clinical interventions.



Future endeavors in biosensing of airborne pathogenic fungal spores should focus on the development of breath samplers integrated with nanosensors, enabling rapid and in-situ detection. Large-scale production of nanosensors with excellent reproducibility and repeatability, adopting formats like LFIA, FET biosensors, or microfluidic assays, are crucial for broader commercial utilization. Progress is imperative to establish an efficient and proficient biosensing system encompassing automated rapid sampling, heightened sensitivity, affordability, stability, and real-time, on-site analyte detection.

Looking ahead, several avenues present exciting opportunities for further exploration:

Technological Refinement: Ongoing advancements in microfluidics, PCR methodologies, and other detection technologies are anticipated. Continuous refinement and integration of these technologies will likely yield more sophisticated, user-friendly, and cost-effective diagnostic platforms.

Multiplexing and Specificity: Future assays are expected to incorporate enhanced multiplexing capabilities for simultaneous detection of multiple fungal species and specific resistance markers. This will provide a more comprehensive understanding of the fungal landscape.

Point-of-Care Development: The development of point-of-care assays remains a key focus. Portable, rapid, and accessible diagnostic tools are crucial for timely interventions, especially in resource-limited settings.

Big Data and AI Integration: The integration of big data analytics and artificial intelligence will play a pivotal role in data interpretation. These technologies can offer nuanced insights into spore prevalence, geographical variations, and potential outbreaks.

Clinical Validation and Standardization: Rigorous clinical validation studies across diverse patient populations and settings will be imperative. Standardization of methodologies and assays will enhance their reliability and facilitate their integration into routine clinical practices.



Moreover, interdisciplinary collaboration remains key for fostering knowledge exchange and advancing biosensor platforms. Advancements in miniaturization and microfabrication technologies, along with the integration of novel bio-recognition molecules and nanomaterials, contribute to the progress of biosensors. The successful development of biosensor devices involves critical factors such as studying interactions between bio-recognition elements and analytes, immobilization techniques, anti-fouling surface chemistries, device design, fabrication, and integration of biology with devices.

As research continues, the future holds promising prospects for biosensors in revolutionizing pathogen detection, especially in the context of airborne fungal spores, contributing to improved public health outcomes and a better understanding of indoor air quality.

Acknowledgement: The authors acknowledge the support received from TÜBİTAK 1004 NANOSİS, project number 20AG004, which facilitated this work.



References

View Article Online
DOI: 10.1039/D4NR01175A

1. Gong J, Qi J, Beibei E, Yin Y, Gao D. Concentration, viability and size distribution of bacteria in atmospheric bioaerosols under different types of pollution. *Environmental Pollution*. 2020;257:113485.
2. Khan S, Naushad M, Govarthanam M, Iqbal J, Alfadul SM. Emerging contaminants of high concern for the environment: Current trends and future research. *Environmental research*. 2022;207:112609.
3. Harms H, Schlosser D, Wick LY. Untapped potential: exploiting fungi in bioremediation of hazardous chemicals. *Nature Reviews Microbiology*. 2011;9(3):177-92.
4. Brar SK, Verma M, Surampalli R, Misra K, Tyagi R, Meunier N, et al. Bioremediation of hazardous wastes—a review. *Practice Periodical of Hazardous, Toxic, and Radioactive Waste Management*. 2006;10(2):59-72.
5. Grinn-Gofroń A, Bosiacka B. Effects of meteorological factors on the composition of selected fungal spores in the air. *Aerobiologia*. 2015;31:63-72.
6. Xie W, Li Y, Bai W, Hou J, Ma T, Zeng X, et al. The source and transport of bioaerosols in the air: A review. *Frontiers of Environmental Science & Engineering*. 2021;15:1-19.
7. Srikanth P, Sudharsanam S, Steinberg R. Bio-aerosols in indoor environment: composition, health effects and analysis. *Indian J Med Microbiol*. 2008;26(4):302-12.
8. Pollution IA. Indoor air pollution [Available from: <http://www.pollutionissues.com/Ho-Li/Indoor-Air-Pollution.html>].
9. Stetzenbach LD, Buttner MP, Cruz P. Detection and enumeration of airborne biocontaminants. *Curr Opin Biotechnol*. 2004;15(3):170-4.
10. O'Riordan TG, Smaldone GC. Respiratory medical societies and the threat of bioterrorism. *Thorax*. 2004;59(3):265-7.
11. Mendell MJ, Mirer AG, Cheung K, Tong M, Douwes J. Respiratory and Allergic Health Effects of Dampness, Mold, and Dampness-Related Agents: A Review of the Epidemiologic Evidence. *Environ Health Persp*. 2011;119(6):748-56.
12. Breitenbach M. The spectrum of fungal allergy. *Int Arch Allergy Imm*. 2008;145(1):58-86.
13. Latge JP. *Aspergillus fumigatus* and aspergillosis. *Clin Microbiol Rev*. 1999;12(2):310-+.
14. Sipsas NV, Kontoyiannis DP. Invasive fungal infections in patients with cancer in the Intensive Care Unit. *Int J Antimicrob Ag*. 2012;39(6):464-71.
15. Heseltine E, Rosen J. WHO guidelines for indoor air quality: dampness and mould: WHO Regional Office Europe; 2009.
16. Senn L, Robinson JO, Schmidt S, Knaup M, Asahi N, Satomura S, et al. 1,3-beta-D-glucan antigenemia for early diagnosis of invasive fungal infections in neutropenic patients with acute leukemia. *Clin Infect Dis*. 2008;46(6):878-85.
17. Lass-Flörl C, Mutschlechner W, Aigner M, Grif K, Marth C, Girschikofsky M, et al. Utility of PCR in Diagnosis of Invasive Fungal Infections: Real-Life Data from a Multicenter Study. *J Clin Microbiol*. 2013;51(3):863-8.
18. Fisher BT. The Role of Biomarkers for Diagnosis of and Therapeutic Decisions Related to Invasive Aspergillosis in Children. *Curr Fungal Infect Rep*. 2013;7(1):7-14.
19. Chan ECY, Pasikanti KK, Nicholson JK. Global urinary metabolic profiling procedures using gas chromatography-mass spectrometry. *Nat Protoc*. 2011;6(10):1483-99.
20. Snyder AP, Tripathi A, Maswadeh WM, Ho J, Spence M. Field detection and identification of a bioaerosol suite by pyrolysis-gas chromatography-ion mobility spectrometry. *Field Analytical Chemistry & Technology*. 2001;5(4):190-204.
21. Enyoh CE, Verla AW, Qingyue W, Ohiagu FO, Chowdhury AH, Enyoh EC, et al. An overview of emerging pollutants in air: Method of analysis and potential public health concern from human environmental exposure. *Trends in Environmental Analytical Chemistry*. 2020;28:e00107.
22. Tobias HJ, Schafer MP, Pitesky M, Ferguson DP, Horn J, Frank M, et al. Bioaerosol mass spectrometry for rapid detection of individual airborne *Mycobacterium tuberculosis* H37Ra particles. *Applied and Environmental Microbiology*. 2005;71(10):6086-95.



23. Calderon C, Ward E, Freeman J, McCartney A. Detection of airborne fungal spores sampled by rotating-arm and Hirst-type spore traps using polymerase chain reaction assays. *Journal of Aerosol Science*. 2002;33(2):283-96.
24. Miyajima K, Suzuki Y, Miki D, Arai M, Arakawa T, Shimomura H, et al. Direct analysis of airborne mite allergen (Der f1) in the residential atmosphere by chemifluorescent immunoassay using bioaerosol sampler. *Talanta*. 2014;123:241-6.
25. Urbano R, Palenik B, Gaston C, Prather K. Detection and phylogenetic analysis of coastal bioaerosols using culture dependent and independent techniques. *Biogeosciences*. 2011;8(2):301-9.
26. Qiu G, Yue Y, Tang J, Zhao Y-B, Wang J. Total bioaerosol detection by a Succinimidyl-Ester-functionalized Plasmonic biosensor to reveal different characteristics at three locations in Switzerland. *Environmental science & technology*. 2020;54(3):1353-62.
27. Ma J, Jiang G, Ma Q, Wang H, Du M, Wang C, et al. Rapid detection of airborne protein from *Mycobacterium tuberculosis* using a biosensor detection system. *Analyst*. 2022;147(4):614-24.
28. Woo G, Lee DH, Lee BY, Kim T, editors. Real-time bioaerosol detecting via combination of cyclone based collecting system and SiNW biosensor. 2023 IEEE International Symposium on Medical Measurements and Applications (MeMeA); 2023: IEEE.
29. Wang P, Zhang R, Wu Y, Chang Y, Liu M. An Electrochemical Aptasensor Integrating Zeolitic Imidazolate Framework for Highly Selective Detection of Bioaerosols. *Biosensors*. 2022;12(9):725.
30. Su X, Sutarlie L, Loh XJ. Sensors and analytical technologies for air quality: particulate matters and bioaerosols. *Chemistry—An Asian Journal*. 2020;15(24):4241-55.
31. Ibrahim RK, Hayyan M, AlSaadi MA, Hayyan A, Ibrahim S. Environmental application of nanotechnology: air, soil, and water. *Environmental Science and Pollution Research*. 2016;23:13754-88.
32. Kumar N, Kumari M, Arun RK. Development and implementation of portable biosensors in microfluidic point-of-care devices for pathogen detection. *Miniaturized Biosensing Devices: Fabrication and Applications*: Springer; 2022. p. 99-122.
33. Kashyap PL, Rai P, Sharma S, Chakdar H, Kumar S, Pandiyan K, et al. Nanotechnology for the detection and diagnosis of plant pathogens. *Nanoscience in Food and Agriculture 2*. 2016:253-76.
34. Cho S-Y, Myong J-P, Kim W-B, Park C, Lee SJ, Lee SH, et al. Profiles of environmental mold: indoor and outdoor air sampling in a hematology hospital in Seoul, South Korea. *International journal of environmental research and public health*. 2018;15(11):2560.
35. Lv Y, Hu G, Yuan W, Li Y, Liu T, He P, et al., editors. Experimental study of fungal release characteristics in central air. 2018 7th International Conference on Energy, Environment and Sustainable Development (ICEESD 2018); 2018: Atlantis Press.
36. Liu L, Corma A. Metal catalysts for heterogeneous catalysis: from single atoms to nanoclusters and nanoparticles. *Chemical reviews*. 2018;118(10):4981-5079.
37. Ortiz SC, Pennington K, Thomson DD, Bertuzzi M. Novel insights into *Aspergillus fumigatus* pathogenesis and host response from state-of-the-art imaging of host–pathogen interactions during infection. *Journal of Fungi*. 2022;8(3):264.
38. Lee T, Grinshpun SA, Martuzevicius D, Adhikari A, Crawford CM, Reponen T. Culturability and concentration of indoor and outdoor airborne fungi in six single-family homes. *Atmospheric environment*. 2006;40(16):2902-10.
39. Jin J-H, Kim J, Jeon T, Shin S-K, Sohn J-R, Yi H, et al. Real-time selective monitoring of allergenic *Aspergillus* molds using pentameric antibody-immobilized single-walled carbon nanotube-field effect transistors. *RSC Advances*. 2015;5(20):15728-35.
40. Fronczek CF, Yoon J-Y. Biosensors for monitoring airborne pathogens. *Journal of laboratory automation*. 2015;20(4):390-410.
41. Seo G, Lee G, Kim MJ, Baek S-H, Choi M, Ku KB, et al. Rapid detection of COVID-19 causative virus (SARS-CoV-2) in human nasopharyngeal swab specimens using field-effect transistor-based biosensor. *ACS nano*. 2020;14(4):5135-42.
42. Miao Z, Cai Y, Liu J, Li D, Chai T. Quantification of airborne *Aspergillus fumigatus* spores in rabbit houses by real-time polymerase chain reaction. *Aerobiologia*. 2012;28:291-4.



43. Balajee SA, Imhof A, Gribskov JL, Marr KA. Determination of antifungal drug susceptibilities of *Aspergillus* species by a fluorescence-based microplate assay. *Journal of Antimicrobial Chemotherapy*. 2004;55(1):102-5.
44. Stetzenbach LD, Buttner MP, Cruz P. Detection and enumeration of airborne biocontaminants. *Current opinion in biotechnology*. 2004;15(3):170-4.
45. Méheust D, Le Cann P, Reboux G, Millon L, Gangneux J-P. Indoor fungal contamination: health risks and measurement methods in hospitals, homes and workplaces. *Critical Reviews in Microbiology*. 2014;40(3):248-60.
46. West JS, Kimber R. Innovations in air sampling to detect plant pathogens. *Annals of Applied Biology*. 2015;166(1):4-17.
47. Kattke MD, Gao EJ, Sapsford KE, Stephenson LD, Kumar A. FRET-based quantum dot immunoassay for rapid and sensitive detection of *Aspergillus amstelodami*. *Sensors*. 2011;11(6):6396-410.
48. Lee JI, Jang SC, Chung J, Choi W-K, Hong C, Ahn GR, et al. Colorimetric allergenic fungal spore detection using peptide-modified gold nanoparticles. *Sensors and Actuators B: Chemical*. 2021;327:128894.
49. Seo J-W, Kim JY, Oh J-J, Kim YJ, Kim G-H. Selection and characterization of toxic *Aspergillus* spore-specific DNA aptamer using spore-SELEX. *RSC advances*. 2021;11(5):2608-15.
50. Lu H, Zhu J, Zhang T, Zhang X, Chen X, Zhao W, et al. A rapid multiplex nucleic acid detection system of airborne fungi by an integrated DNA release device and microfluidic chip. *Talanta*. 2022;246:123467.
51. Fattahi Z, Hasanzadeh M. Nanotechnology-assisted microfluidic systems for chemical sensing, biosensing, and bioanalysis. *TrAC Trends in Analytical Chemistry*. 2022;152:116637.
52. Kholafazad-Kordasht H, Hasanzadeh M, Seidi F. Smartphone based immunosensors as next generation of healthcare tools: Technical and analytical overview towards improvement of personalized medicine. *TrAC Trends in Analytical Chemistry*. 2021;145:116455.
53. Turner AP, Knechtle SJ. Induction immunosuppression in liver transplantation: a review. *Transplant International*. 2013;26(7):673-83.
54. Sapsford KE, Pons T, Medintz IL, Mattoussi H. Biosensing with luminescent semiconductor quantum dots. *Sensors*. 2006;6(8):925-53.
55. Asal M, Özen Ö, Şahinler M, Baysal HT, Polatoğlu İ. An overview of biomolecules, immobilization methods and support materials of biosensors. *Sensor Review*. 2018;39(3):377-86.
56. Naresh V, Lee N. A review on biosensors and recent development of nanostructured materials-enabled biosensors. *Sensors*. 2021;21(4):1109.
57. Yu L-S, Rodriguez-Manzano J, Moser N, Moniri A, Malpartida-Cardenas K, Miscourides N, et al. Rapid detection of azole-resistant *Aspergillus fumigatus* in clinical and environmental isolates by use of a lab-on-a-chip diagnostic system. *Journal of Clinical Microbiology*. 2020;58(11):10.1128/jcm. 00843-20.
58. Heydari E. Nanoplasmonic biodetection based on bright-field imaging of resonantly coupled gold-silver nanoparticles. *Photonics and Nanostructures-Fundamentals and Applications*. 2019;36:100708.
59. Sojinrin T, Conde J, Liu K, Curtin J, Byrne HJ, Cui D, et al. Plasmonic gold nanoparticles for detection of fungi and human cutaneous fungal infections. *Analytical and bioanalytical chemistry*. 2017;409:4647-58.
60. Gaikwad A, Joshi M, Patil K, Sathaye S, Rode C. Fluorescent carbon-dots thin film for fungal detection and bio-labeling applications. *ACS Applied Bio Materials*. 2019;2(12):5829-40.
61. Heineman WR, Jensen WB. Leland c. clark jr.(1918–2005). *Biosensors and Bioelectronics*. 2006;21(8):1403-4.
62. Chaubey A, Malhotra B. Mediated biosensors. *Biosensors and bioelectronics*. 2002;17(6-7):441-56.
63. Malhotra BD, Ali MA. Nanomaterials in biosensors: Fundamentals and applications. *Nanomaterials for biosensors*. 2018:1.
64. Shanker A, Lee K, Kim J. Synthetic hybrid biosensors. *Encyclopedia of molecular cell biology and molecular medicine*. Wiley-VCH Verlag GmbH & Co. KGaA, Weinheim, Germany; 2014.

View Article Online
DOI: 10.1039/D4NR01175A



65. Shanker A, Lee K, Kim J. Synthetic hybrid biosensors. 2014.
66. Grieshaber D, MacKenzie R, Vörös J, Reimhult E. Electrochemical biosensors-sensor principles and architectures. *Sensors*. 2008;8(3):1400-58.
67. Alaejos MS, Garcia Montelongo FJ. Application of amperometric biosensors to the determination of vitamins and α -amino acids. *Chemical reviews*. 2004;104(7):3239-66.
68. Alkire RC, Kolb DM, Lipkowski J. *Advances in Electrochemical Science and Engineering: Bioelectrochemistry*: Wiley-VCH; 2011.
69. Cho I-H, Kim DH, Park S. Electrochemical biosensors: Perspective on functional nanomaterials for on-site analysis. *Biomaterials research*. 2020;24(1):6.
70. Bhatnagar I, Mahato K, Ealla KKR, Asthana A, Chandra P. Chitosan stabilized gold nanoparticle mediated self-assembled gliP nanobiosensor for diagnosis of Invasive Aspergillosis. *International journal of biological macromolecules*. 2018;110:449-56.
71. Ma X, Zhang Y, Qiao X, Yuan Y, Sheng Q, Yue T. Target-Induced AIE Effect Coupled with CRISPR/Cas12a System Dual-Signal Biosensing for the Ultrasensitive Detection of Gliotoxin. *Analytical Chemistry*. 2023;95(31):11723-31.
72. Kim D, Wang SX. A magneto-nanosensor immunoassay for sensitive detection of *Aspergillus fumigatus* allergen Asp f 1. *IEEE transactions on magnetics*. 2012;48(11):3266-8.
73. Nugaeva N, Gfeller KY, Backmann N, Düggelin M, Lang HP, Güntherodt H-J, et al. An antibody-sensitized microfabricated cantilever for the growth detection of *Aspergillus niger* spores. *Microscopy and Microanalysis*. 2007;13(1):13-7.
74. Kim J, Jin J-H, Kim HS, Song W, Shin S-K, Yi H, et al. Fully automated field-deployable bioaerosol monitoring system using carbon nanotube-based biosensors. *Environmental science & technology*. 2016;50(10):5163-71.
75. Song Y, Lin B, Tian T, Xu X, Wang W, Ruan Q, et al. Recent progress in microfluidics-based biosensing. *Analytical chemistry*. 2018;91(1):388-404.
76. Liu Y, Shen H, Yang X, Kang S, Cai L, Tian T, et al. Recent progress in microfluidic biosensors with different driving forces. *TrAC Trends in Analytical Chemistry*. 2022:116894.
77. Xing G, Zhang W, Li N, Pu Q, Lin J-M. Recent progress on microfluidic biosensors for rapid detection of pathogenic bacteria. *Chinese Chemical Letters*. 2022;33(4):1743-51.
78. Chen K, Dopico P, Varillas J, Zhang J, George TJ, Fan ZH. Integration of Lateral Filter Arrays with Immunoaffinity for Circulating-Tumor-Cell Isolation. *Angewandte Chemie*. 2019;131(23):7688-92.
79. Ruan Q, Ruan W, Lin X, Wang Y, Zou F, Zhou L, et al. Digital-WGS: Automated, highly efficient whole-genome sequencing of single cells by digital microfluidics. *Science advances*. 2020;6(50):eabd6454.
80. Yakovleva J, Davidsson R, Lobanova A, Bengtsson M, Eremin S, Laurell T, et al. Microfluidic enzyme immunoassay using silicon microchip with immobilized antibodies and chemiluminescence detection. *Analytical chemistry*. 2002;74(13):2994-3004.
81. Yalikun Y, Hosokawa Y, Iino T, Tanaka Y. An all-glass 12 μ m ultra-thin and flexible microfluidic chip fabricated by femtosecond laser processing. *Lab on a Chip*. 2016;16(13):2427-33.
82. Dochow S, Beleites C, Henkel T, Mayer G, Albert J, Clement J, et al. Quartz microfluidic chip for tumour cell identification by Raman spectroscopy in combination with optical traps. *Analytical and bioanalytical chemistry*. 2013;405:2743-6.
83. Kim H-J, Choi S-J. Rapid single-cell detection of pathogenic bacteria for in situ determination of food safety. *Analytical Methods*. 2020;12(46):5621-7.
84. Zhou L, Mao S, Huang Q, He X, Lin J-M. Inhibition of anaerobic probiotics on colorectal cancer cells using intestinal microfluidic systems. *Science China Chemistry*. 2018;61:1034-42.
85. Zheng Y, Wu Z, Lin J-M, Lin L. Imitation of drug metabolism in cell co-culture microcapsule model using a microfluidic chip platform coupled to mass spectrometry. *Chinese Chemical Letters*. 2020;31(2):451-4.
86. Pardon G, Ladhani L, Sandström N, Etori M, Lobov G, van der Wijngaart W. Aerosol sampling using an electrostatic precipitator integrated with a microfluidic interface. *Sensors and Actuators B: Chemical*. 2015;212:344-52.
87. Li X, Zhang X, Liu Q, Zhao W, Liu S, Sui G. Microfluidic system for rapid detection of airborne pathogenic fungal spores. *ACS sensors*. 2018;3(10):2095-103.



88. Beneyton T, Wijaya I, Postros P, Najah M, Leblond P, Couvent A, et al. High-throughput screening of filamentous fungi using nanoliter-range droplet-based microfluidics. *Scientific reports*. 2016;6(1):1-10. [View Article Online](#)
DOI:10.1039/D4NR01175A
89. Duarte PA, Menze L, Shoute L, Zeng J, Savchenko O, Lyu J, et al. Highly efficient capture and quantification of the airborne fungal pathogen *Sclerotinia sclerotiorum* employing a nanoelectrode-activated microwell array. *ACS omega*. 2021;7(1):459-68.
90. Rath P-M, Steinmann J. Overview of commercially available PCR assays for the detection of *Aspergillus* spp. DNA in patient samples. *Frontiers in Microbiology*. 2018;9:740.
91. White PL, Hibbitts SJ, Perry MD, Green J, Stirling E, Woodford L, et al. Evaluation of a commercially developed semiautomated PCR–surface-enhanced Raman scattering assay for diagnosis of invasive fungal disease. *Journal of clinical microbiology*. 2014;52(10):3536-43.
92. Green J, Dougan J, editors. The evaluation of a real time PCR assay for aiding the diagnosis of Invasive Candidiasis: Fungiplex Candida. *MYCOSES*; 2017: WILEY 111 RIVER ST, HOBOKEN 07030-5774, NJ USA.



Data Availability Statement

View Article Online
DOI: 10.1039/D4NR01175A

This review article prepared based on findings from previously published studies. All data analyzed during this study are included in the published articles cited within the review. No new data were created or analyzed in this study. For specific data sets or further information, readers are referred to the original publications listed in the references section.

