


# Sensors & Diagnostics

rsc.li/sensors

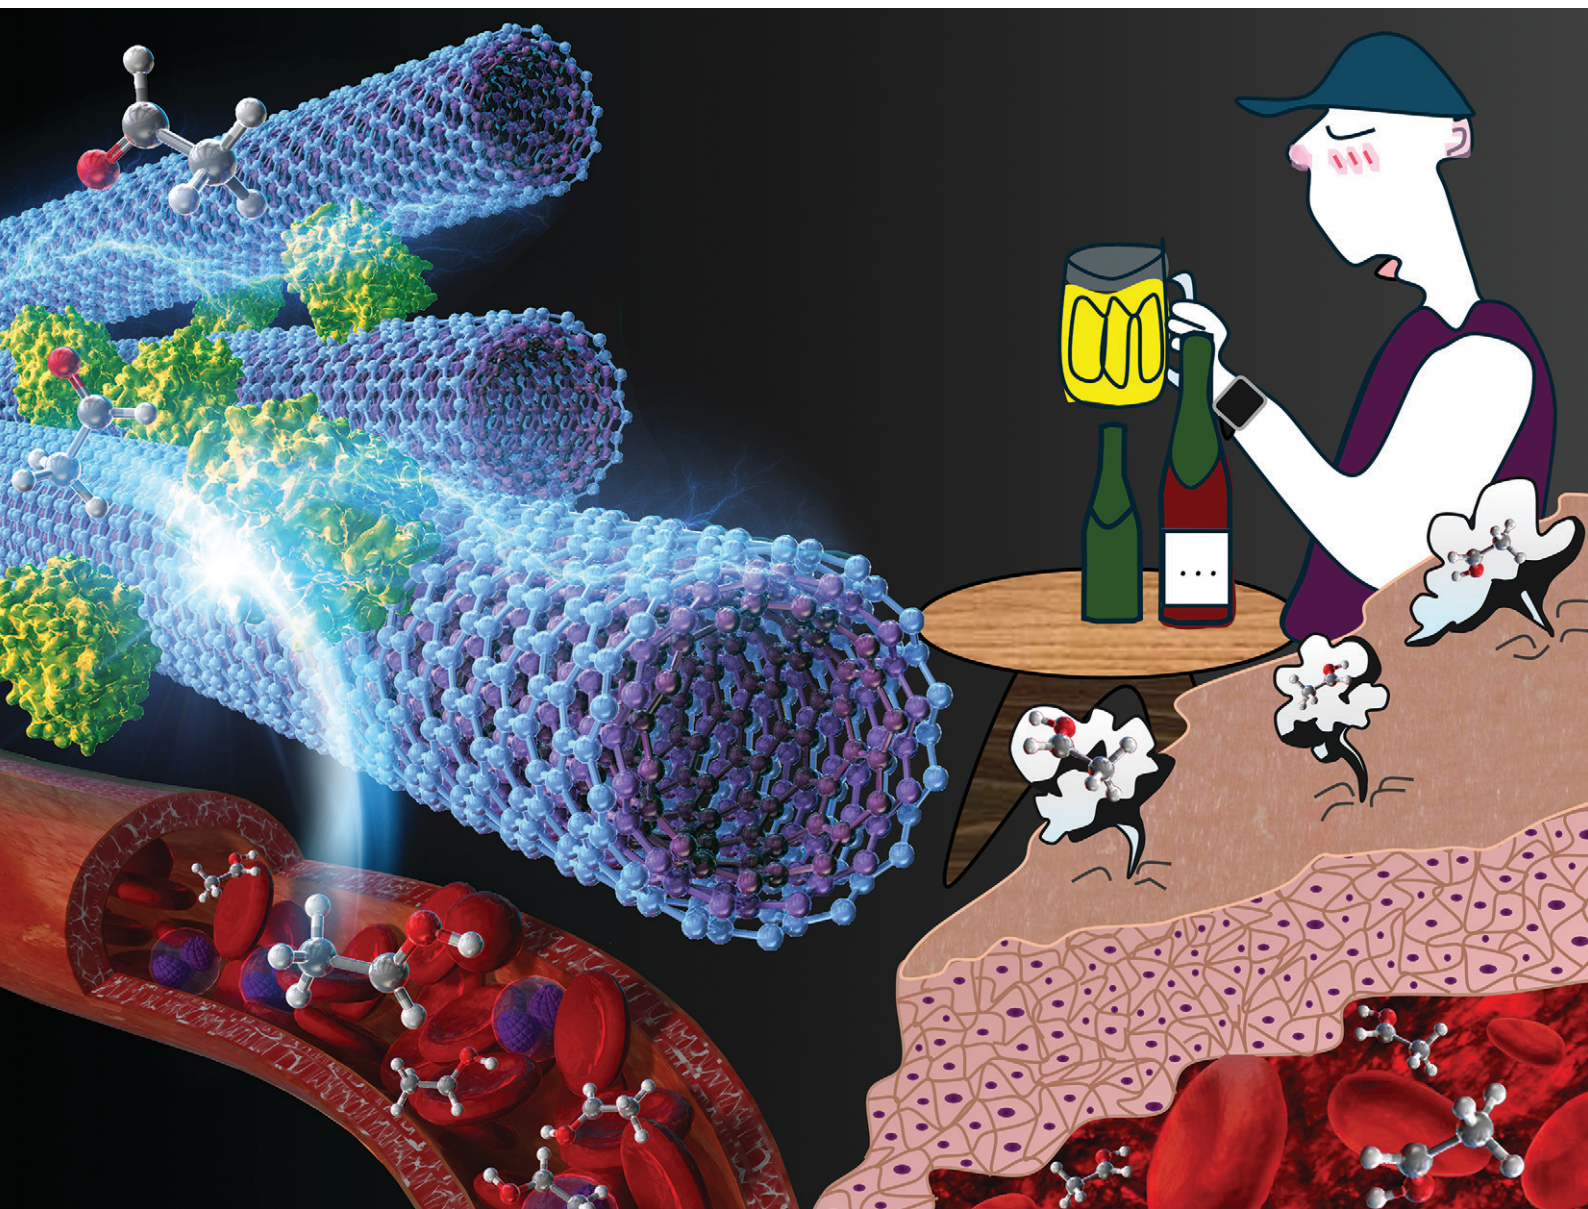

ISSN 2635-0998

## PAPER

Masato Tominaga *et al.*

Highly sensitive flux-type non-invasive alcohol biosensor based on direct electron transfer of PQQ-dependent alcohol dehydrogenases adsorbed on carbon nanotubes