RSC Advances



PAPER

View Article Online
View Journal | View Issue



Cite this: RSC Adv., 2025, 15, 10191

A new method for the rapid determination of sodium percarbonate in aqueous samples using a modified HPLC setup†

Amir Nasreddine, D Sarah Ghazali, Weam Bou Karroum, D Abbas Baalbaki and Antoine Ghauch *

Sodium percarbonate (SPC) is a widely used oxidant with applications in environmental remediation, especially within advanced oxidation processes (AOPs). Despite its prevalence, traditional methods for SPC quantification are often limited by complexity, cost, or lack of adaptability, creating a need for rapid, reliable, and scalable analytical approaches. This study presents a novel method for SPC quantification using a modified high-performance liquid chromatography with visible detection (HPLC-VIS) system. The key innovation lies in replacing the conventional separation column with a narrow-diameter loop reactor made of simple PEEK tubing, allowing SPC to react with acidified potassium iodide directly within the system. This modification eliminates the need for separate sample pretreatment, simplifies the analytical workflow, and enables real-time reaction monitoring while using standard HPLC equipment available in most laboratories. The method demonstrated high repeatability, reproducibility, and strong linearity (R^2) 0.99) across a range of pH values and in complex matrices, including highly saline and organic pollutantcontaining samples. The method effectively monitored residual SPC levels in AOP-treated tramadol samples, where it confirmed continued SPC activity post-degradation of the target compound, indicating potential for comprehensive degradation of byproducts. Additionally, tests on a commercial SPC-based detergent (Vanish) validated the method's applicability for real-world samples. Overall, this HPLC-based technique provides a streamlined, environmentally friendly, and robust solution for SPC quantification, offering significant advantages for both research and industrial applications involving SPC in various water matrices.

Received 17th December 2024 Accepted 27th March 2025

DOI: 10.1039/d4ra08825e

rsc.li/rsc-advances

Introduction

1.1. Sodium percarbonate

Sodium percarbonate (2Na₂CO₃·3H₂O₂) is a crystalline, water-soluble compound often used as a source of hydrogen peroxide.¹ It appears as a granular, white powder and acts as a potent oxidizing agent, releasing sodium carbonate and hydrogen peroxide when dissolved in water. Known for its chemical stability, high solubility, and environmentally benign decomposition products,¹ sodium percarbonate (SPC) has diverse applications. First introduced in the early 20th century as a stable, solid alternative to liquid hydrogen peroxide, it enabled easier handling and storage, meeting the growing demand for efficient and safe oxidizing agents in the chemical industry.²,³ Its utility spans a variety of sectors, including textiles,⁴ pulp and paper bleaching,⁵ and wastewater

American University of Beirut, Faculty of Arts and Sciences, Department of Chemistry, P. O. Box 11-0236, Riad El Solh, Beirut, 1107-2020, Lebanon. E-mail: antoine. ghauch@aub.edu.lb; Fax: +961 1 365217; Tel: +961 1350000

† Electronic supplementary information (ESI) available. See DOI: https://doi.org/10.1039/d4ra08825e

treatment,^{6,7} each of which has been key in driving its industrial relevance.

The market is experiencing rapid global expansion, with a projected compound annual growth rate (CAGR) over the coming years. A recent report from Intellectual Market Insights Research estimates that the global SPC market will grow from USD 1281.2 million in 2021 to USD 1816.76 million by 2028, marking an 8.1% CAGR. This growth is largely driven by the increasing use of SPC in household and personal care applications, such as laundry detergents8 as a bleaching agent, in stain removers,9 and in general household cleaners.10 Moreover, a global shift in consumer preference towards oxygen-based bleaches over traditional chlorine-based bleaches and the rise of eco-friendly cleaning formulations, made SPC-based products appealing to environmentally conscious consumers as it degrades into non-toxic byproducts.11,12 Medically, SPC is incorporated into dental care products, such as toothpaste, where it provides whitening and antibacterial benefits13,14 through the release of hydrogen peroxide, aiding in stain removal and bacterial reduction to enhance oral hygiene.15

Recent developments have sparked greater interest in the application of SPC in advanced oxidation processes (AOPs) for

Table 1 Summary of SPC and H₂O₂ quantification techniques available in the literature, presenting the advantages and drawbacks in comparison to the proposed method

Analytical technique	Description	Application	Advantages	Drawbacks
Titrimetric ²⁴	H ₂ O ₂ is titrated with potassium	ISO number 4321	Accuracy	High reagent requirements, labor-
	permanganate (KMNO ₄)			intensive
Colorimetric and	Perhydrolysis of resorufin pivalate by H_2O_2 ,	Office-scanner-based sodium	Sensitivity (LOD: $0.45 \mu M$),	High reagent requirements, requires
fluorescent reaction-based	produced in situ from percarbonate, to	percarbonate detection	used available apparatus	intensive sample preparation, non-
probe	restore the optical properties of resoruin dye			automated
Attenuated total reflection-	Partial least squares (PLS) treatment of data	Determination of	Accuracy	Non-automated
Fourier transform infrared (ATR-FTIR) ²⁶	obtained by attenuated total reflectance Fourier francform infrared (ATR FT-IR)	percarbonate in commercial		
	spectrometry in wavenumber region of 1435–			
	1342 CIII		1000	
Chemiuminescence	Sensor based on oxalic acid esters (bis(2,4,6-trichloronhenyl) oxalate-TCPO and bis(2,4-	Determination of nerearbonate in commercial	Accuracy, LOD: 54 µg L (for TCPO) and 48 µg L ⁻¹	Keagents used are expensive and
SCHOOL	dinitronhenyl) oxalate-DNPO)	washing nowder detergent	(for DNPO)	tone, requires a special apparatus
Fluorescence-based Fenton	$\frac{1}{2}$ Hydroxylation of henzoic acid by Fe(π) and	Real-time determination of	Sensitivity (LOD: 10 ⁻⁸ M)	Potential interference from SO, at low
reagent method ²⁸	H ₂ O ₂ (Fenton reaction) forms fluorescent	hydrogen peroxide in aqueous	real-time detection	pH and requires calibration
)	hydroxybenzoic acid, which is enhanced by	SPC samples		adjustments for field conditions
	complexation with Al(III)			
Ion chromatography (IC)	Separation of hydrogen peroxide as	Detection and quantification	High specificity	Requires high-pH eluent (>11.6),
with UV detector ²⁹	hydroperoxyl ion (HO_2^-) using an anion	of H_2O_2 in natural waters,		potential interference from strong
	exchange column (AEC) and quantification	wastewater, and		oxidants and organics
	via UV absorption at 210 nm	environmental samples		
High-performance liquid	Uses the vanadium(v)-peroxo complex,	Detection of trace residual	Detection of trace	Requires toxic and hazardous
chromatography with	HPLC-DAD, and the fluorescence of 7-	H ₂ O ₂ in processed fishery	concentrations	reagents (ammonium metavanadate),
diode array detector	hydroxycoumarin formed <i>via</i> Fenton	foods and other food products		high cost, includes derivatization
$(\mathrm{HPLC\text{-}DAD})^{30}$	reaction for indirect H ₂ O ₂ detection			reactions, potential interference from
				matrices and a complex protocol
High-performance liquid	Uses Fenton reaction, where H ₂ O ₂ reacts	Detection of trace H ₂ O ₂ levels	Detection of trace	Requires toxic coumarin, and
chromatography with	with coumarin to form 7-hydroxycoumarin,	in food safety applications	concentrations	potential interference from other
fluorescence detector	a fluorescent product detected at 330 nm			oxidizing agents in food samples
(HPLC-FLD)	(excitation)/460 nm (emission)			
Iodometric (I_3^-)	Based on the oxidation of iodide (I ^{$-$}) by H ₂ O ₂	Detection of H ₂ O ₂ in aqueous	Detection of trace	Requires strict pH control, potential
spectrophotometric	in the presence of ammonium molybdate,	solutions, environmental and	concentrations in small	interference from side reactions in
method^{31}	forming triiodide (I ₃ ⁻), which is measured at	radiation chemistry studies	sample volumes	buffers, ammonium molybdate can
	351 nm			be toxic in large quantities, and lacks automation
High-performance liquid	H_2O_2 is detected via oxidation at a gold	Detection of trace H ₂ O ₂ levels	Highly selective, low	Requires specialized electrochemical
chromatography with	working electrode in a sodium acetate	in forensic samples (post-blast	detection limit (LOD:	detector, electrode fouling can occur
electrochemical detection	mobile phase at pH 10.5	debris), environmental	0.02 mg mL^{-1} , 0.6 mM),	over time
$(HPLC-ED, DC mode)^{32}$		monitoring, and explosive	effective for post-blast	
		residues	forensic analysis	
High-performance liquid	Uses post-column derivatization, where	Forensic analysis of H ₂ O ₂	Highly sensitive, LOD:	Requires toxic hemin reagent,
chromatography with	H_2O_2 reacts with p-hydroxyphenylacetic acid	residues (pre- and post-blast),	$0.19 \text{ mg mL}^{-1} \text{ (6 mM)},$	complex post-column derivatization,
fluorescence detection	(FOPHA) and hemin to form a fluorescent	detection in environmental	fluorescence detection	and precise flow control of multiple
(HPLC-FD)	dimer, detected at 320 nm (excitation)/	and controlled laboratory	provides strong selectivity	reagents
	405 nm (emission)	samples	for H_2O_2	

Paper

wastewater treatment.¹⁶⁻¹⁹ Due to its granular coating, SPC has enhanced stability, longer storage life, and reduced risk of explosion, presenting distinct advantages over liquid hydrogen peroxide.²⁰ In addition, SPC is often added to the Fe(II)/ persulfate(PS) system to address limitations in activation efficiency and effective pH range.²¹ This approach has shown promising results; Fu *et al.* demonstrated benzene removal using Fe²⁺-catalyzed SPC,²² and Epold *et al.* reported effective levofloxacin degradation in aqueous solutions using a combined Fenton and PS system.²³

The broad and varied applications of SPC across multiple industries highlight the importance of developing fast and precise analytical methods for its determination. Despite its widespread use, rapid and accurate determination methods remain limited; such methods are essential for quality control processes, ensuring product purity and meeting desired SPC concentration levels.

1.2. A review of existing SPC determination method

The only established standard method for determining SPC is ISO 4321-1977 (E), titled Washing Powders – Determination of Active Oxygen Content – Titrimetric Method (ISO 4321-1977).²⁴ This method employs titrimetric analysis, a colorimetric technique that, although accurate, is now considered outdated due to its time-intensive preparation and the substantial amounts of reagents required, which drive up costs (see Table 1S†). Moreover, its high limits of detection (LOD) and quantification (LOQ) make it inadequate for measuring low SPC concentrations. The technique is also susceptible to human error, as slight color variations in the titrant across trials can affect accuracy despite rigorous efforts at consistency.

Alternative methods reported in the literature face similar limitations (Table 1). Many are equally labor-intensive, depend on hazardous reagents, or require specialized equipment that is not widely available, restricting their accessibility in typical laboratory settings. Furthermore, these methods often lack automation capabilities, making them impractical for processing large sample volumes efficiently.

1.3. Proposed method theory

The proposed approach uses a repurposed HPLC-VIS setup equipped with autosamplers, facilitating rapid determination of oxidants across numerous samples. By making minor, non-damaging modifications, the setup replaces the traditional reverse or normal phase separation column with a PEEK tube. The mobile phase consists of a concentrated acidified potassium iodide (KI) solution (pH = 3–4, [KI] = 40 mM), which swiftly reduces H_2O_2 in the sample.

In this setup, H_2O_2 reacts with I^- to produce an iodine (I_2) suspension in the PEEK tube (eqn (1)). The generated I_2 then further reacts with excess I^- , forming the triiodide anion (I_3^-) . The PEEK tube functions as a reaction chamber allowing the reaction to reach completion before elution, ensuring accurate measurements. Detection is performed at 352 nm, the maximum absorption wavelength (λ_{max}) of I_3^- , a wavelength where most common emerging organic pollutants do not

absorb. This unique feature, alongside the use of an inorganic yet compatible mobile phase, offers a significant advantage for laboratories focused on advanced oxidation process (AOP) research involving SPC as an oxidant.

This setup allows researchers and industry professionals to process a large number of samples, each requiring minimal volume (<1 mL), and to determine both contaminant and oxidant concentrations using a single instrument. The method is particularly beneficial for laboratories with limited human resources, as it enables high-throughput analysis while reducing the time, labor, and costs associated with traditional techniques.

2. Chemicals

SPC standards were prepared using sodium percarbonate salt $(\geq 99.00\% \text{ assay})$ (Na₂CO₃·1.5H₂O₂) (Sigma-Aldrich, USA). The HPLC mobile phase was prepared using potassium iodide (KI) (puriss, 99.0-100.5%), sodium bicarbonate (NaHCO₃) (Sigma-Aldrich, Germany) in addition to phosphoric acid (H₃PO₄) (Fisher Chemical, UK). Sodium hydroxide (NaOH) (Fisher Chemical, UK), sodium phosphate monobasic (NaH2PO4) (Sigma-Aldrich, Germany) and phosphoric acid (H₃PO₄) (Fisher Chemical, UK) were used for the adjustment of the pH. For spectator ions matrix effect experiments, sodium chloride (NaCl) (Fisher Scientific, UK), technical grade humic acid sodium salt, sodium bicarbonate (NaHCO3) (Sigma-Aldrich, Germany) and fumaric acid (Sigma-Aldrich, Switzerland) were used. Tramadol hydrochloride was obtained by dissolving TRAMAL® 50 mg capsules (STADA, Italy) in deionized water and filtering twice using 0.45 µm S-Pak® membrane filters (Merck, Germany) to remove insoluble excipients (microcrystalline cellulose, sodium starch glycolate, colloidal anhydrous silica, and magnesium stearate). Vanish detergent was purchased from a local store. All water used was of Millipore DI grade.

3. Detection setup

3.1. Modified HPLC setup specifications

The setup for our proposed method utilizes an HPLC-VIS system (Agilent 1100 series) equipped with a quaternary pump, a vacuum degasser, and an autosampler compartment maintained at 4 °C. In place of the conventional separation column, a PEEK tube (Restek, length 44 cm, ID 0.508 mm) is connected in series and kept at room temperature (20–25 °C). Detection is carried out using an integrated diode array detector with an embedded flow cell and a visible lamp (see Fig. 15†).

3.2. Standards and mobile phase preparation

For the HPLC mobile phase, 5 g of sodium bicarbonate (NaHCO₃) was dissolved in 1000 mL of deionized (DI) water to remove all dissolved oxygen.³³ Next, 6.64 g of potassium iodide (KI) and 5 mL of phosphoric acid were added to a 500 mL portion of this solution, which was stirred until fully dissolved before being recombined with the remaining 500 mL. The prepared mobile phase was stored overnight in an airtight

RSC Advances Paper

amber bottle to prevent light-catalyzed oxidation of I to I2 and to ensure complete dissolution. The mobile phase was freshly prepared weekly to maintain solution stability. This preparation protocol was originally developed by our research group for persulfate (PS) and H2O2 determination.33,34

While SPC and H₂O₂ have similar properties, it is essential to account for the carbonate ions released during SPC dissolution, which buffer the acidity of the mobile phase. Therefore, this study was conducted to establish the optimal conditions for accurate measurements in the presence of these buffering ions.

SPC standards were prepared in 2 mL HPLC vials from a stock solution. Standards were discarded after a maximum of 3 hours, as SPC remains stable and active only for 5-6 hours.³⁵

3.3. Mobile phase optimization

Sodium bicarbonate (NaHCO₃) is initially added to the mobile phase to eliminate dissolved oxygen, thereby preventing the oxidation of iodide (I-) to iodine (I2) and enhancing background intensity. Afterward, potassium iodide (KI) is added and fully dissolved, followed by the addition of phosphoric acid. Phosphoric acid is included to promote the Fenton reaction (eqn (2)), which is kinetically favored under acidic conditions, maximizing the generation of I2 as shown in eqn (3). This prepared solution benefits from the use of cost-effective, highly water-soluble, and low-toxicity chemicals, which also avoid any corrosive effects on HPLC components.

$$Na_2CO_3 \cdot 1.5H_2O_2 \rightarrow Na_2CO_3 + 1.5H_2O_2$$
 (1)

$$H_2O_2 \rightarrow 2HO$$
 (2)

$$2HO' + 2I^- \rightarrow I_2 + 2OH^-$$
 (3)

$$I_2 + I^- \rightarrow I_3^- \tag{4}$$

$$OH^- + H^+ \to H_2O \tag{5}$$

3.4. Experimental procedures and conditions

To ensure the reliability of the proposed method, we first evaluated its repeatability, reproducibility, limit of detection (LOD), and limit of quantification (LOQ) using SPC standards prepared in deionized (DI) water. The details of these experiments and their results are provided in Section 4.1.

Following this, we assessed potential sample matrix effects by preparing SPC standards in solutions with specific characteristics. These included varying pH levels (pH 2, 7, and 11, adjusted using a 10 mM phosphate buffer) to investigate pH effects, and the presence of various matrix elements: chloride (Cl⁻ at 20 000 mg L⁻¹), bicarbonate (HCO₃⁻ at 150 mg L⁻¹), ozonated species (O₃⁻ at 150 mg L⁻¹), humic acid (10 mg L⁻¹), and fumaric acid (10 mg L^{-1}). Additionally, samples containing both SPC and tramadol at 10 mg L⁻¹ were tested to simulate a real-life application involving SPC-based AOPs for tramadol

SPC standards were also prepared and tested in natural water matrices, including sea and spring water, each at a concentration of 10 mg L^{-1} . The results of these experiments are discussed in detail in Sections 4.2 and 4.3.

Results and discussion

Quality assurance and method validation

The method validation and quality assurance procedures were based on the guidelines provided in Quantitative Chemical Analysis by Harris (2010, Chapter 4 and 5), which was used to assess the SPC quantification procedure under various testing conditions. To ensure specificity, PEEK tubing configurations were accepted only if they produced high-quality peaks. Linearity was confirmed by an R^2 value of ≥ 0.98 . Accuracy was evaluated by testing freshly prepared standards during repeatability tests. The methods for determining precision (reproducibility), range, limit of detection (LOD), limit of quantitation (LOQ), and robustness are described in the following subsections. The HPLC pump flow rate was set to 0.1 mL min⁻¹, and various injection volumes (5, 20, 50, and 100 µL) were tested to determine optimal conditions. The highest linearity $(R^2 =$ 0.999) was achieved with a flow rate of 0.1 mL min⁻¹ and an injection volume of 100 μL, indicating ideal calibration conditions. The backpressure recorded under these conditions is 4 bars. Furthermore, the PEEK tube had been in use for oxidants determination in our lab for the past 5 years, processing thousands of samples under different methods,34,35 and shows no signs of degradation, and no change in inner diameter as it can be seen in Fig. 5S.†

4.1.1. Repeatability. To confirm the repeatability of the method, three separate PS standards were prepared and tested for each concentration on the same day by a single researcher using a consistent HPLC setup. The average calibration curves obtained are presented in Fig. 1. Error bars were calculated at a 95% confidence interval, using the formula: peak area = mean measurement $\pm ts/\sqrt{n}$, where *t* is the Student's *t*-value (t = 4.303for 2 degrees of freedom at a 95% confidence level), s is the standard deviation from three replicates, and n is the number of calibration standards. The LINEST function in Excel was used to compute the slope, y-intercept, regression coefficient, and other relevant statistical data, including standard deviations for each variable. The method demonstrated strong repeatability, as indicated by the minimal error bar values.

4.1.2. Reproducibility. Reproducibility tests were carried out over a span of three days, encompassing their respective linear dynamic ranges (LDR). Each day, new mobile phase and standards were prepared, followed by the analysis of three replicates of each standard using the same HPLC instrument. Although it is advised to use a different HPLC instrument each day, as suggested by Harris (2010)36 only one HPLC instrument was accessible. Calibration curves, along with their corresponding error bars, are displayed in Fig. 2. Calibration curves exhibited variation from day to day, while maintaining a very good R^2 value greater than 0.99. Therefore, it is strongly recommended to prepare fresh standards and obtain a new calibration curve whenever employing this method to control its low reproducibility.




Fig. 1 SPC calibration curve for repeatability methods. Vertical bars represent the error on the mean of three injections calculated at 95% confidence interval $\left(\frac{ts}{\sqrt{n}}\right)$; absent bars fall within symbols.




Fig. 2 SPC calibration curve for reproducibility methods. Vertical bars represent the error on the mean of three injections calculated at 95% confidence interval $\left(\frac{ts}{\sqrt{n}}\right)$; absent bars fall within symbols.

4.1.3. Limit of detection and quantification. The Harris method (Method Validation, 5-2) was followed to calculate the limit of detection (LOD) and limit of quantification (LOQ) of SPC.³⁶ Seven tests were conducted to determine the LOD and LOQ using eqn (6) and (7), respectively. The LOD and LOQ for SPC were found to be 1.31 \times 10⁻² and 4.39 \times 10⁻² mM, respectively.

$$LOD = \frac{3 \times \text{standard deviation}}{\text{slope}}$$
 (6)

$$LOQ = \frac{10 \times standard\ deviation}{slope}$$
 (7)

4.1.4. Method validation. Method validation was conducted following the procedures outlined in Quantitative Chemical Analysis by Harris³⁶ (2010, Chapter 5, Section 5-2: Method Validation) and (2010, Chapter 4, Section 4-3: Comparison of Means with Student's t). The accuracy of the method was validated by having the reference standards' concentration fall within the precision range of the newly developed method as summarized in Table 2. For the t-test, the validation involved both the iodometric titration method, a widely used technique for SPC quantification, and the calibration method to prepare and test the standards. Each standard was measured twice, and the difference in concentrations between the two methods is summarized in Table 3. After data processing, t-test was used to compare the concentrations obtained via the calibration method with those from the iodometric titration approach in Table 4. Having a Student value at a 95% confidence interval greater than the calculated t shows that the new method is accepted.

4.2. pH effect

To evaluate the impact of sample pH on the proposed method, SPC standards were prepared in a 10 mM phosphate buffer (PB) at pH values of 2, 7, and 11, covering acidic, neutral, and basic conditions with substantial buffer strength (Fig. 3). The calibration curves for each buffered matrix demonstrated strong linearity ($R^2 > 0.99$). The calibration curves for the pH 11 solution and the control (non-buffered) sample were nearly identical,

Table 3 Calibration method results, [SPC] unit: mM

$[SPC]_{theoretical}$	[SPC] _{reference method}	[SPC] _{new method}	D
0.2	0.189	0.155	-0.034
0.3	0.289	0.270	-0.019
0.4	0.415	0.405	-0.009
0.5	0.513	0.522	0.009
0.6	0.594	0.608	0.014
0.7	0.763	0.686	-0.077
0.8	0.803	0.759	-0.044
0.9	0.911	0.893	-0.018
1	1.102	0.982	-0.120

Table 2 Calibration method results, [SPC] unit: mM

[SPC] _{theoretical}	$[SPC]_1$	$[SPC]_2$	$[SPC]_{avg}$	ts/\sqrt{n}	Range ([SPC] _a	$_{ m vg} \pm ts/\sqrt{n}$	Result
0.2	0.151936	0.158515	0.155225	0.059117	0.096108	0.214342	Accepted
0.3	0.272179	0.267991	0.270085	0.03762	0.232465	0.307705	Accepted
0.4	0.412442	0.404309	0.418376	0.073067	0.345308	0.491443	Accepted
0.5	0.513143	0.530987	0.522065	0.160323	0.361742	0.682388	Accepted
0.6	0.608389	0.606708	0.607549	0.015105	0.592444	0.622653	Accepted
0.7	0.680666	0.690507	0.685587	0.088421	0.597166	0.774008	Accepted
0.8	0.764894	0.752842	0.758868	0.108277	0.650591	0.867145	Accepted
0.9	0.884192	0.900834	0.892513	0.149518	0.742995	1.042031	Accepted
1	0.974672	0.988965	0.981818	0.128417	0.853402	1.110235	Accepted

Table 4 Calibration method results

RSC Advances

Mean (d)	-0.033
Std dev. (Sd)	0.048
t calculated	1.822
Degrees of freedom (n)	7
Student value at 95% confidence interval	2.365
Result	Accepted




Fig. 3 The effect of spectator species on the calibration curve. Vertical bars represent the error on the mean of three injections calculated at 95% confidence interval $\left(\frac{ts}{\sqrt{n}}\right)$; absent bars fall within symbols. Experimental conditions: [FA], [HA], [TRA] = 10 mg L⁻¹, [NaCl] = 20 000 mg L⁻¹, [HCO₃⁻] = 150 mg L⁻¹.

suggesting that the method's sensitivity and response remain stable in alkaline environments. This stability may be attributed to the presence of sodium carbonate, a product of SPC dissociation in water. The slight increase in the slope of the calibration curves under acidic conditions (lower pH) likely results from enhanced reactivity, increased sensitivity, improved analyte stability, and reduced buffer interference. Acidic conditions may facilitate more efficient SPC dissolution into hydrogen peroxide and sodium carbonate, contributing to these effects.³⁷

4.3. Matrix effects

It is essential to consider the effects of common ions and organic and inorganic compounds that may be present in sample matrices. To evaluate potential interference, SPC standards were prepared in aqueous matrices containing high concentrations of these substances, ensuring that naturally occurring ions and compounds—typically present in much lower concentrations—do not interfere with the analysis. The tested additives included chlorides (Cl⁻), bicarbonates (HCO₃⁻), humic acids (HA), fumaric acid (FA), and tramadol (TRA). Results indicated minimal impact on the linearity and slopes of their respective calibration curves, with variations from the control calibration curve falling within the experimental error range (see Fig. 4). Further details on the selection of tested species and their concentrations are provided in subsequent sections.

To assess the effect of salinity, which can enhance $\rm H_2O_2$ decomposition, 38,39 standards were prepared in a highly saline matrix with NaCl at 20 000 mg $\rm L^{-1}$, classified as highly saline




Fig. 4 The effect of the SPC sample's pH on the calibration curve. Vertical bars represent the error on the mean of three injections calculated at 95% confidence interval $\left(\frac{ts}{\sqrt{n}}\right)$; absent bars fall within symbols.

water by the Food and Agriculture Organization of the United Nations (FAO).40

Sample hardness was evaluated by preparing standards with 150 mg $\rm L^{-1}$ of $\rm HCO_3^-$. This concentration was chosen because bicarbonate ions ($\rm HCO_3^-$) are commonly present in water due to atmospheric $\rm CO_2$ dissolution and may act as activators of $\rm H_2O_2$.

In addition, natural water matrices often contain organic compounds such as HA and FA, derived from decomposing organic material. Therefore, SPC standards with 10 mg $\rm L^{-1}$ of either HA or FA were prepared to assess their effects. Furthermore, the potential interference of complex organic pollutants, such as micro-contaminants commonly found in AOP-treated water, was examined by preparing standards with tramadol (TRA) at a concentration of 10 mg $\rm L^{-1}$.

Overall, none of these additives had a significant effect on the method's accuracy, as indicated by Fig. 4.

4.4. Application to natural water matrices

To evaluate the effectiveness of the developed analytical method in natural water matrices, SPC standards were prepared in both sea and spring water. The natural water samples' quality parameters are provided in Table 2S.† As shown in Fig. 5, a slight increase in signal intensity (slope) of 17% was observed in sea water, while no significant effect was noted in spring water. The calibration curves for both natural water matrices displayed strong linearity ($R^2 > 0.99$), indicating reliable performance across different water types.

4.5. Application to AOPs research in action

SPC is commonly used as an oxidant in AOPs. However, many studies that focus on optimizing these applications often neglect monitoring the residual oxidant (SPC), a critical step that is labor-intensive and time-consuming with traditional quantification methods. Advanced techniques, meanwhile, are often prohibitively expensive. To address this, we used SPC in a UVC/SPC system for the degradation of tramadol (TRA).

Paper




Fig. 5 The effect of natural water matrices on the calibration curve. Vertical bars represent the error on the mean of three injections calculated at 95% confidence interval $\left(\frac{ts}{\sqrt{n}}\right)$; absent bars fall within symbols.

Samples collected at various degradation intervals were processed using our method to determine the residual [SPC]. Fig. 4S† shows the decreasing absorbance of TRA during the oxidation control experiment from 220 nm to 300 nm over 6 min of reaction time. The calibration method was applied to quantify the remaining [SPC] and to calculate the percentage reaction

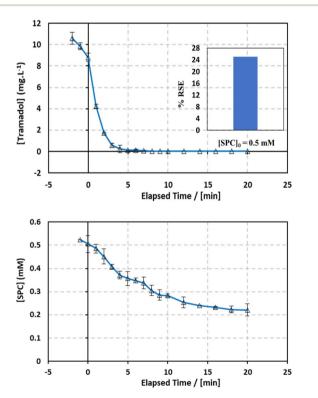


Fig. 6 Application for SPC quantification in AOPs research. Vertical bars represent the error on the mean of three injections calculated at 95% confidence interval $\left(\frac{ts}{\sqrt{n}}\right)$; absent bars fall within symbols. Experimental conditions: [TRA] = 10 mg L⁻¹, [SPC] = 0.5 mM. The inset represents the % RSE determined for the experiment.

stoichiometric efficiency (% RSE) as defined by eqn (8).⁴³ The results (Fig. 6) showed that SPC consumption continued even after the complete degradation of the target compound, indicating that SPC effectively mineralizes the degradation byproducts formed during the process.

$$\% RSE = \frac{[probe degraded]}{[oxidant consumed]}$$
 (8)

Notably, the developed method facilitated a rapid calculation of % RSE, a crucial factor for evaluating UVC's effect on SPC activation. The relatively acceptable % RSE of 25% suggests a high affinity of SPC toward the degradation of byproducts in the reactive medium. However, this value remains much greater than the % RSE obtained in similar AOP systems using persulfate as oxidant with iron species for persulfate activation. These findings highlight the importance of further investigating the role of UVC in this context, as well as monitoring TRA degradation byproducts to optimize the applied AOP.

4.6. Application to washing powder detergents

To evaluate the effectiveness of the developed analytical method, we tested it using the washing powder detergent Vanish (Fig. 2S†), which contains between 10 and 20% SPC,⁴⁷ along with other substances (Table 3S†). Samples with varying detergent concentrations were prepared and analyzed using the proposed method. The resulting "chromatograms" displayed a single peak at the same retention time as SPC (Fig. 3Sa†), confirming the presence of SPC in the samples (Fig. 3Sb†).

The results, shown in Fig. 7, indicate a strong linear relationship between the peak area and the concentration of Vanish. The calibration curve demonstrated high linearity ($R^2 > 0.99$) and consistency, underscoring the method's reliability for quantifying SPC in powder detergents. The small error bars indicate excellent reproducibility and minimal experimental error. Furthermore, the percentage of SPC in Vanish powder was determined using our method to be 10.83%, which is within the range of expected values (10–20%).




Fig. 7 Calibration curve showing the area *versus* the concentration of Vanish. Vertical bars represent the error on the mean of three injections calculated at 95% confidence interval $\left(\frac{ts}{\sqrt{n}}\right)$; absent bars fall within symbols.

5. Conclusions

Sodium percarbonate (SPC), a widely used oxidant with numerous applications, has experienced increased demand in recent years, emphasizing the need for rapid, reliable methods to monitor its concentration in aqueous media. Existing methods for SPC quantification have distinct limitations and specific requirements. Here, we present a novel method using a modified HPLC configuration to quantify SPC across various water matrix conditions. This method offers significant advantages over traditional techniques in terms of simplicity, scalability, automation, and reduced chemical consumption per sample. It has demonstrated excellent repeatability, reproducibility, and adaptability across a wide range of pH and salinity conditions. Furthermore, the method showed minimal interference from organic compounds (OCs) when applied in advanced oxidation process (AOP) research, whether in deionized or natural water matrices. This approach provides an efficient, effective, and environmentally friendly solution for SPC quantification across diverse water matrices.

Data availability

The data supporting this article have been included as part of the ESI. \dagger

Conflicts of interest

There are no conflicts to declare.

Acknowledgements

This research was funded in part by the University Research Board (award number 103603) of the American University of Beirut and USAID-Lebanon through the National Academy of Sciences under PEER project 5-18 (award number 103262) and the MEPI TLP program (award number 103992). A. Nasreddine would like to thank the FAS Dean's office through the undergraduate research experience award. The authors are thankful to Joan Younes, Simon Al-Ghawi and Boutros Sawaya for their technical assistance and graphic designer Dany Khoury for the design of the graphical abstract. They are also very thankful to the personnel of the K. Shair CRSL for their kind help.

References

- 1 M. Khanmohammadi, N. Mashkuri, M. Rostami and A. B. Garmarudi, *J. Anal. Chem.*, 2012, **67**, 330–334.
- 2 H. Xue, J. Li, G. Zhang, B. Liu, M. Li and H. Wang, *Environ. Sci.: Water Res. Technol.*, 2023, **9**, 2171–2187.
- 3 P. Li, X. Cheng, W. Zhou, C. Luo, F. Tan, Z. Ren, L. Zheng, X. Zhu and D. Wu, J. Cleaner Prod., 2020, 269, 122228.
- 4 Q. Li, R. Lu, Y. Liang, K. Gao and H. Jiang, *Materials*, 2022, 15, 5849.
- 5 E. Pesman, S. Imamoglu, E. Ersoy Kalyoncı and H. Kirci, *Bioresources*, 2014, **9**, 523–536.

- 6 Y. Huang, L. Bu, Y. Wu, S. Zhu, S. Zhou, Z. Shi and D. D. Dionysiou, *Chem. Eng. J.*, 2022, 442, 135995.
- 7 X. Ling, J. Deng, C. Ye, A. Cai, S. Ruan, M. Chen and X. Li, *Sci. Total Environ.*, 2021, **799**, 149382.
- 8 G. O. Bianchetti, C. L. Devlin and K. R. Seddon, *RSC Adv.*, 2015, 5, 65365–65384.
- C. Oldfield, R. M. Morgan, H. F. Miles and J. C. French, *Aust. J. Forensic Sci.*, 2018, 50, 345–354.
- 10 E. Igos, R. Moeller, E. Benetto, A. Biwer, M. Guiton and P. Dieumegard, *Chemosphere*, 2014, **100**, 160–166.
- 11 G. L. Liu, Q. L. Cui and C. W. Yu, *Adv. Mater. Res.*, 2011, **183**–**185**, 1423–1427.
- 12 X. Fu, X. Gu, S. Lu, V. K. Sharma, M. L. Brusseau, Y. Xue, M. Danish, G. Y. Fu, Z. Qiu and Q. Sui, *Chem. Eng. J.*, 2017, 309, 22–29
- 13 J. Kaneko, S. Inoue, S. Kawakami and H. Sano, *J. Endod.*, 2000, 26, 25–28.
- 14 R. Date, J. Yue, A. Barlow, P. Bellamy, M. Prendergast and R. Gerlach, *Am. J. Dent.*, 2003, **16**, 3B–8B, https://pubmed.ncbi.nlm.nih.gov/15055980/.
- 15 M. Alam, R. Jagger, R. Vowles and J. Moran, *Int. J. Dent. Hyg.*, 2011, 9, 37–42.
- 16 K. Fedorov, M. P. Rayaroth, N. S. Shah and G. Boczkaj, *Chem. Eng. J.*, 2023, 456, 141027.
- 17 Y. Li, Y. Zhu, D. Wang, G. Yang, L. Pan, Q. Wang, B.-J. Ni, H. Li, X. Yuan, L. Jiang and W. Tang, *Water Res.*, 2020, **174**, 115626.
- 18 B. Pieczykolan, I. Płonka and K. Barbusiński, *Architecture, Civil Engineering, Environment*, 2016, **9**, 135–140.
- 19 J. Gao, R. F. Nunes, K. O'Shea, G. L. Saylor, L. Bu, Y.-G. Kang, X. Duan, D. D. Dionysiou and S. Luo, *Water Res.*, 2022, 219, 118457.
- 20 J. Gao, X. Duan, K. O'Shea and D. D. Dionysiou, Water Res., 2020, 171, 115394.
- 21 J. Mo, T. Lin, X. Zhang, F. Jiang and H. Chen, *Desalination*, 2023, 547, 116258.
- 22 X. Fu, X. Gu, S. Lu, Z. Miao, M. Xu, X. Zhang, Z. Qiu and Q. Sui, *Chem. Eng. J.*, 2015, **267**, 25–33.
- 23 I. Epold, M. Trapido and N. Dulova, *Chem. Eng. J.*, 2015, 279, 452–462.
- 24 ISO 4321:1977 Washing Powders Determination of Active Oxygen Content Titrimetric Method, https://www.iso.org/standard/10192.html.
- 25 K. M. Lee, K. Y. Park, N. Y. Kim, J. H. Yoo, M. G. Choi, S. Ahn and S.-K. Chang, *Dyes Pigm.*, 2021, **184**, 108804.
- 26 K. K. M. Khanmohammadi, Talanta, 2005, 65, 824-827.
- 27 E. Omanovic and K. Kalcher, Int. J. Environ. Anal. Chem., 2005, 85, 853–860.
- 28 J. H. Lee, I. N. Tang, J. B. Weinstein-Lloyd and E. B. Halper, Environ. Sci. Technol., 1994, 28, 1180–1185.
- 29 M. Song, J. Wang, B. Chen and L. Wang, Anal. Chem., 2017, 89, 11537–11544.
- 30 J. Park, H. Noh, H. J. Suh, D. Ryu, H. J. Lee and C. Lee, *Food Sci. Biotechnol.*, 2023, **32**, 27–37.
- 31 N. V. Klassen, D. Marchington and H. C. E. McGowan, *Anal. Chem.*, 1994, **66**, 2921–2925.

Paper

32 M. Tarvin, B. McCord, K. Mount and M. L. Miller, *Forensic Sci. Int.*, 2011, **209**, 166–172.

- 33 O. Tantawi, A. Baalbaki, R. El Asmar and A. Ghauch, *Sci. Total Environ.*, 2019, **654**, 107–117.
- 34 A. Baalbaki, N. Zein Eddine, S. Jaber, M. Amasha and A. Ghauch, *Talanta*, 2018, 178, 237–245.
- 35 Household Uses for Sodium Percarbonate, https://www.chemistrystore.com/sodium_percarbonate2.pdf.
- 36 D. C. Harris, Quantitative Chemical Analysis, 8th edn, 2010.
- 37 A. Rastinfard, B. Dalisson and J. Barralet, *Acta Biomater*., 2022, 145, 390-402.
- 38 C.-H. Liao, S.-F. Kang and F.-A. Wu, *Chemosphere*, 2001, 44, 1193–1200.
- 39 J. De Laat, G. T. Le and B. Legube, *Chemosphere*, 2004, 55, 715–723

- 40 J. D. Rhoades, A. Kandiah and A. M. Mashali, *The use of saline waters for crop production, FAO Irrigation and Drainage paper 48*, FAO, Rome, 1992.
- 41 D. E. Richardson, H. Yao, K. M. Frank and D. A. Bennett, *J. Am. Chem. Soc.*, 2000, **122**, 1729–1739.
- 42 F. J. Stevenson, *Humus Chemistry: Genesis, Composition, Reactions*, John Wiley & Sons, 1994.
- 43 A. Ghauch, A. Baalbaki, M. Amasha, R. El Asmar and O. Tantawi, *Chem. Eng. J.*, 2017, 317, 1012–1025.
- 44 A. Ghauch, G. Ayoub and S. Naim, *Chem. Eng. J.*, 2013, **228**, 1168–1181.
- 45 G. Ayoub and A. Ghauch, Chem. Eng. J., 2014, 256, 280-292.
- 46 S. Naim and A. Ghauch, Chem. Eng. J., 2016, 288, 276-288.
- 47 Reckitt Benckiser Group, Safety Data Sheet for Vanish Oxi Action Powder Fabric Stain Remover, 2019.