

Probing subdiffraction limit separations with plasmon coupling microscopy: concepts and applications

Q1 Q2

Cite this: DOI: 10.1039/c3cs60340g

Linxi Wu and Björn M. Reinhard*

Due to their advantageous material properties, noble metal nanoparticles are versatile tools in biosensing and imaging. A characteristic feature of gold and silver nanoparticles is their ability to sustain localized surface plasmons that provide both large optical cross-sections and extraordinary photophysical stability. Plasmon coupling microscopy takes advantage of the beneficial optical properties and utilizes electromagnetic near-field coupling between individual noble metal nanoparticle labels to resolve subdiffraction limit separations in an all-optical fashion. This Tutorial provides an introduction into the physical concepts underlying distance dependent plasmon coupling, discusses potential experimental implementation of plasmon coupling microscopy, and reviews applications in the area of biosensing and imaging.

Received 26th September 2013

DOI: 10.1039/c3cs60340g

www.rsc.org/csr

Key learning points

- (1) Optical properties of noble metal nanoparticles.
- (2) Distance dependent plasmon coupling.
- (3) Resolving subdiffraction limit separations in the optical microscope through plasmon coupling.
- (4) Experimental implementation of plasmon coupling microscopy (PCM).
- (5) Application of PCM in biosensing and imaging.

1. Introduction – noble metal nanoparticles as labels in optical microscopy

Most cellular processes are complex and require interactions between multiple components well-orchestrated in space and time to generate a desired outcome. It has long been recognized that optical microscopy is – in principle – the method of choice for deciphering the mechanisms of intrinsically dynamic processes in living cells. Monitoring the spatial distribution of selectively labeled components as a function of time represents a powerful approach to determine which components interact, how, and in what sequence. The localization accuracy for an individual emitter in optical microscopy is determined by the uncertainty, σ , with which its point-spread-function (PSF) or “image” can be localized in a selected plane:¹

$$\sigma = \sqrt{\left(\frac{s^2}{N} + \frac{a^2/12}{N} + \frac{8\pi s^4 b^2}{a^2 N^2}\right)} \quad (1)$$

where s is the width of the intensity distribution, N the number of collected photons, a the pixel size of the camera, and b the standard deviation of the background. Bright labels in a low background allow for a high localization accuracy for individual emitters and localization precisions of a few nm have been realized. Light emitted by multiple sources interferes, however, so that the wave nature of light sets strict limitations on the level of detail with which multiple labels with identical emission wavelength can be resolved in a conventional light microscope. The lateral spatial resolution of an optical system is given as $\sim 0.6\lambda/\text{NA}$, where λ is the wavelength of the light and NA is the numerical aperture. In the visible range of the electromagnetic spectrum the diffraction limit is on the order of a few hundreds of nanometers. Unfortunately, this resolution is insufficient to access any molecular details of cellular processes. Dynamic molecular rulers, based on fluorescence resonance energy transfer (FRET), have traditionally been used to circumvent the diffraction limit in fluorescence microscopy and to monitor the separations between fluorescently labeled species on the order of 1–10 nm.² Recently true subdiffraction-limit optical imaging with spatial resolution down to ~ 20 nm has been made possible by fluorescence “nanoscopy” that achieves the separate localization of individual labels at

Department of Chemistry and The Photonics Center, Boston University, Boston, Massachusetts, USA. E-mail: bmr@bu.edu

different points in time by switching the dye labels between on- and off-states.³ Fluorescence nanoscopy – like fluorescence microscopy in general – suffers, however, from the limited photophysical stability of organic dyes. After photoexcitation, dyes show a higher reactivity and can undergo a chemical transformation that results in an irreversible loss of fluorescence.² Photobleaching fundamentally limits the ability to monitor cellular dynamics continuously over extended periods of time with high temporal resolution and, thus, motivates the further improvement of fluorescent labels as well as the development of alternative non-fluorescence based approaches that are not subject to any constraints in observation time.

Due to their large contrast in electron microscopy, Au and Ag nanoparticles (NPs) have long been used as high-contrast labels in electron microscopy.⁴ But noble metal NPs also have exquisite optical properties and can be imaged in optical scattering or photothermal microscopy without any blinking or bleaching and with no physical limitation in observation time. The time varying electric (E -) field component of light incident on a NP induces displacement of the conduction band electrons and results in an oscillating charge pile-up on the NP surface (Fig. 1a). At the localized surface plasmon (LSP) resonance (LSPR) frequency the surface charge density oscillations form a standing wave so that even weak incident E -fields achieve large charge accumulations. For Au and Ag NPs, the LSPRs lie in the visible range of the electromagnetic spectrum. Since the polarizability, α , of a NP is resonantly enhanced at the LSPR,⁵ scattering and absorption cross-sections become maximum at this frequency. The strong charge concentration in a small volume on the surface of the NP creates a strong local E -field enhancement at the LSPR, which is of great interest for many non-linear spectroscopy techniques.

For particles that are much smaller than the wavelength of the incident light it is justified to assume that the phase of the oscillating E -field does not change substantially across the NP diameter, *i.e.* that the quasistatic approximation applies. Under these conditions the scattering and absorption cross-sections of noble metal NPs, C_{sca} and C_{abs} , scale as r^6 and r^3 , respectively, where r is the radius of the NP (Fig. 1a).⁵ We note, however, that the polarizability, α_0 , in Fig. 1a does not account for radiation damping, γ , due to light scattering. To avoid violation of energy conservation, it is therefore necessary to augment the quasistatic approximation with a radiation reaction term, which leads to the corrected polarizability, α_{eff} .⁶ Light absorption dominates in NPs with very small sizes, but the scattering cross-section increases steeply with size. Individual NPs with a radius of $r \geq 15$ nm have sufficiently large scattering cross-sections to facilitate an uncomplicated detection of individual particles in darkfield or total internal reflection microscopy. Both techniques use excitation geometries that eliminate the excitation beam from detection and, thus, make it possible to selectively collect light that is scattered from the NPs in the direction of the objective. A 40 nm Au NP has a scattering cross-section of $\approx 6.0 \times 10^{-12}$ cm² at its resonance wavelength of 535 nm, which compares with $\approx 0.5 \times 10^{-16}$ cm² for a conventional fluorescent dye.⁷ Even if one takes into account the larger size of the NP and corrects for the fact that

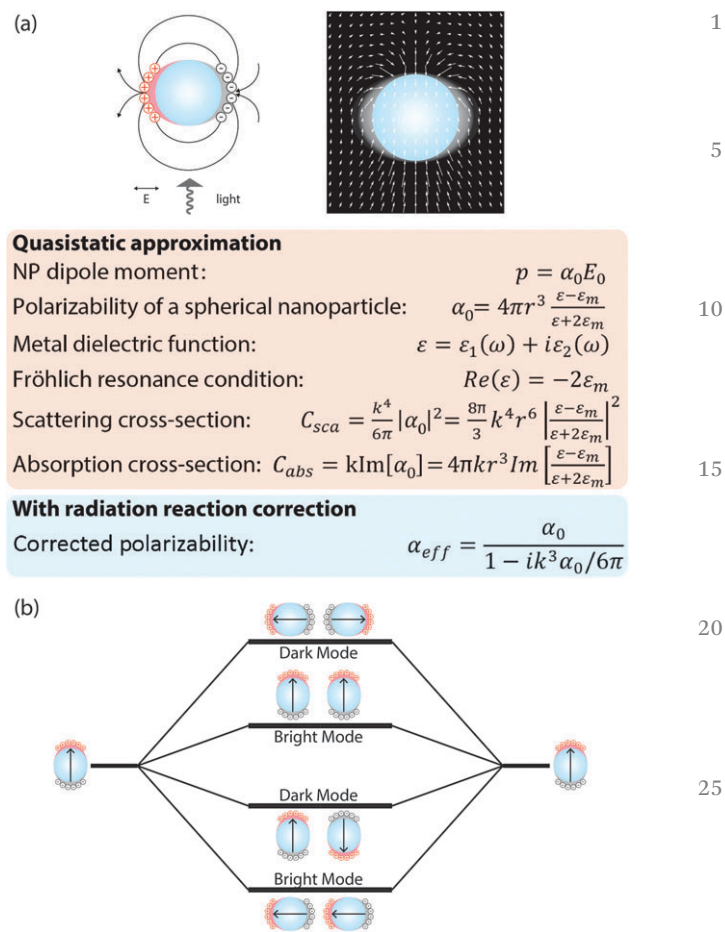


Fig. 1 (a) Left: light incident onto a metal NP creates charge density oscillations on the surface. Right: a plot of the optical powerflow around a noble metal NP at the LSPR frequency shows a rerouting of the incident light towards the NP. Red box: key formulas determining the resonance behavior of the metal NP in the quasistatic approximation (wavenumber $k = 2\pi/\lambda$; ϵ_m : dielectric constant of the ambient medium). Blue box: corrected effective polarizability including radiation reaction. Adapted with permission from Boriskina and Reinhard, *Nanoscale*, 2012, **4**, 76. Copyright 2012 The Royal Society of Chemistry. (b) Plasmon hybridization between strongly coupled NPs leads to the formation of dark and bright modes, depending on the relative orientation of the NP dipoles (indicated by arrows).

one NP corresponds to approximately 1600 dye molecules, the NP still shows a larger cross-section by a factor of ≈ 75 . Considering eqn (1), it is immediately clear that one other advantage of NPs is the possibility to collect a large number of photons per time unit, which is beneficial for an accurate localization of the tracked species even at short acquisition times. While the size of optical NP labels is a disadvantage when compared with smaller organic dyes, their extraordinary signal stability and brightness, as well as their field enhancing properties and their multimodal character, make them versatile probes for processes that either directly involve NPs or occur on length scales of a few tens of nanometers and which can, therefore, tolerate their size. Although the diffraction limit applies to metallic NPs in the same way as for fluorescent labels, oscillating charge distributions in individual NPs create time-dependent electromagnetic fields, which act on the

1 conduction band electrons of other nearby NPs. These fields
can then act back on the conduction band electrons in the
original NP. Due to the sum of all of these electromagnetic
“near-field” interactions, the oscillations in the individual NPs
5 are no longer independent but coupled. This near-field coupling
can be conveniently detected as a shift in the scattering
spectra of the NP labels using conventional far-field light
microscopy.⁸ The fundamental concept of plasmon coupling
and its application for optically resolving subdiffraction limit
10 separations in a cellular context are the focus of this Tutorial.

The manuscript is structured as follows: in Section 2 we will
review the fundamental electromagnetic mechanisms underlying
plasmon coupling in discrete dimers of noble metal NPs, and
in Section 3 we will review the influence of the configuration in
15 larger clusters. In Section 4 we will review the experimental
implementation of plasmon coupling microscopy (PCM), and in
Section 5 we will discuss applications in cellular imaging.

20 2. Distance dependent plasmon coupling: the color of plasmon rulers

We will start our analysis of the collective resonances in NP
clusters with the simplest possible case, the dimer. NP dimers
25 have two natural symmetry axes along which plasmon coupling
can occur (Fig. 1b). Depending on the polarization of the
incident light, the electron density oscillations occur along
the long axis (longitudinal mode) or perpendicular to it (two
degenerate transverse modes). As we will discuss in more detail
30 below, the treatment of the individual NPs as simple dipoles, p ,
with $p = \alpha E_0$, where α is the NP polarizability and E_0 the incident
 E -field, is insufficient to give a correct quantitative description
of plasmon coupling. Nevertheless, the simplified model is still
of great value for conceptualizing the relevant electromagnetic
35 coupling mechanisms. In a dimer the two dipoles representing
the charge distributions of the individual NPs can be oriented
in a parallel or antiparallel fashion. Only the parallel orientations
provide “bright” modes for both longitudinal and transverse
modes, whereas the antiparallel combinations have no net dipole
40 moment and therefore cannot couple to the incident light. These
modes remain “dark”.⁹ This coupling model is adequate for small
NP sizes, but we point out that in dimers of larger particles modes
that are predicted to be dark by this quasistatic model can become
bright.¹⁰ For the relatively small (20–60 nm) NPs of interest in
45 most biological contexts, the quasistatic approximation is acceptable
and we limit our discussion in the following only to the bright
modes, since they will be directly relevant for the optical
studies covered in this Tutorial.

Light-induced displacement of conduction band electrons
50 in metal NPs gives rise to charge accumulations of opposite
sign on opposing surfaces of the particles (Fig. 1a). Assuming a
semi-classical oscillator model for the plasmon, the restoring
force acting on the displacement charge determines the plasmon
eigenfrequency of an individual NP. In a dimer these
55 forces can be modulated by electromagnetic interactions
between the surface charges on two adjacent NPs.¹¹ In the case

of the longitudinal dimer mode the individual NP dipoles are
arranged in a head-to-tail orientation, whereas in the transverse
mode they show a side-by-side orientation (Fig. 1b). The dipole
orientation for the longitudinal mode creates charge accumulations
5 of opposite signs on both sides of the gap, and the accompanying
effective charge screening reduces the net restoring force within
the individual NPs. Consequently, the plasmon eigenfrequency of
the dimer is reduced relative to that of an individual isolated NP.
The reduction in eigenfrequency is equivalent to a spectral red-shift.
10 In contrast, for the bright transverse mode the charge distribution
enhances the restoring force and, therefore, results in a spectral
blue-shift. We note in passing that the longitudinal plasmon mode
has a much higher scattering cross-section than the more weakly
coupled transverse modes and, therefore, dominates the dimer
15 spectrum under unpolarized whitelight excitation.

The exact resonance wavelength of a NP or a NP assembly
depends also on the refractive index, $n_r (= \epsilon_m^{1/2})$, of the ambient
medium (see Fröhlich resonance condition in Fig. 1a).¹² In the
following we will assume that strong electromagnetic coupling
20 between nanoparticles dominates the spectral NP response. This
assumption is justified since the polymer coating assembled on
the NP label surface stabilizes the refractive index in the immediate
vicinity of the NPs and since refractive index fluctuations in
cellular systems – the target application of PCM – are on the order
25 of a few hundredths of refractive index units at most. Changes
of this magnitude lead to variations in the resonance wavelength
that are relatively modest when compared to those associated with
changes of the interparticle separation in the strong electromagnetic
coupling regime.¹³

Direct experimental demonstration of the strong distance
dependence of plasmon coupling was provided by the spectroscopic
characterization of electron beam lithography (EBL) generated
NP dimers^{11,14} and chains of Au NPs.⁸ These and other studies
35 confirmed a monotonic red-shift of the longitudinal plasmon
mode with decreasing interparticle separation for strongly coupled
NPs. The correlation between plasmon resonance wavelength and
interparticle separation obtained with lithographically defined NP
dimers forms the foundation for NP based molecular ruler
40 technologies. The so-called “Plasmon Rulers” utilize the
interparticle separation dependent spectral response of NP dimers
to monitor distances and/or distance changes between biopolymer
linked NPs at a constant refractive index.^{15–19} Experimental
 λ_{plas} vs. interparticle separation (S) calibration curves have been
45 obtained for DNA tethered dimers assembled from $D \approx 40$ nm
diameter Au and Ag NPs and for $D \approx 87$ nm Au NPs under
unpolarized whitelight illumination (Fig. 2a). The calibration
curves confirm a red-shift of the resonance wavelength as a
function of increasing average interparticle separation in the
flexible linked dimers. This spectral red-shift of the Plasmon
50 Rulers is accompanied by an increase in scattering intensity,
as illustrated in the finite-difference time domain (FDTD)
simulation for 40 nm dimers in Fig. 2b.

Fluctuations in the size and shape of the NPs used to
assemble Plasmon Rulers affect the dimer resonance
wavelengths and give rise to some error in the $\lambda_{\text{plas}}(S)$
55 relationship. For a quantitative analysis please refer to ref. 16.

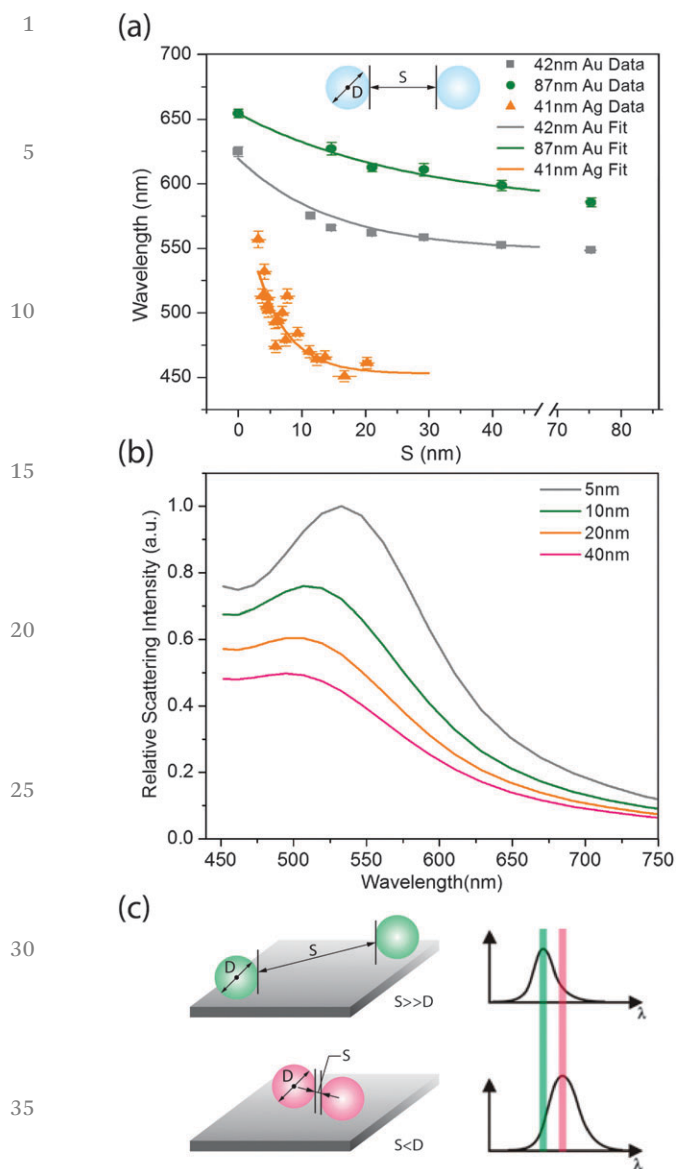


Fig. 2 (a) Experimental calibration curves for 42 nm and 87 nm Au Plasmon Rulers and the 41 nm Ag Plasmon Ruler. Adapted with permission from Reinhard *et al.*, *Nano Lett.*, 2005, **5**, 2246 and Yang *et al.*, *J. Phys. Chem. C*, 2010, **114**, 4901. Copyright 2005 and 2010 American Chemical Society. (b) FDTD-simulated scattering spectra for 40 nm Au dimers as a function of interparticle separation. (c) Principle of plasmon coupling microscopy (PCM): close contacts between NPs are indicated by a spectral red-shift.

This “heterogeneous” broadening of the calibration relationship, however, does not impair the ability to detect even very small changes in the interparticle separation of continuously monitored individual Plasmon Rulers. The ability to monitor interparticle separations with Plasmon Rulers has been utilized in biochemical assays, for instance, for detecting (i) DNA hybridization,^{15,17} (ii) DNA bending upon restriction (EcoRV) enzyme binding,²⁰ (iii) DNA and RNA condensation and cleavage,^{21,22} or (iv) for imaging caspase-3 activation.²³ Other technological applications involved the programmed reversible

switching of interparticle separations.²⁴ Most of these assays utilized the large scattering cross-sections of the noble metal NPs and were performed in a parallel fashion, monitoring many individual Plasmon Rulers at the same time. The thus obtained throughput enables the identification of different sub-populations in one ensemble, which was successfully exploited to reveal different transiently stabilized configurations in RNA Plasmon Rulers.²¹

The experimental Plasmon Ruler calibration curves in Fig. 2a confirm that both Au and Ag Plasmon Rulers allow distance measurements of up to at least 1/2 NP diameter and that the dynamic range of the Plasmon Rulers can be tuned through the choice of the size and chemical composition of the NPs used to assemble the dimers. Due to a steeper slope in their λ_{plas} vs. S calibration curve, Ag Plasmon Rulers provide a higher sensitivity for detecting small distance changes. Interestingly, the experimentally observed $\lambda_{\text{plas}}(S)$ behaviors for all implemented Plasmon Rulers deviate from the expected S^{-3} dependence for purely dipolar interactions and are, instead, well described by single exponentials. Similar observations were made in a series of studies performed with Au or Ag nanodisks nanofabricated on solid supports.^{14,25,26} The deviation from the dipolar coupling mechanism in the experimental studies has been attributed to a highly inhomogeneous field distribution between the two NPs at short separations.²⁷ The inclusion of plasmon modes of higher order angular momenta (quadrupole, *etc.*) is crucial for an accurate description of the distance dependent plasmon coupling between two strongly coupled NPs, even for relatively small NPs that – as individual particles – are accurately described by the dipole approximation. In strongly coupled dimers the dipolar modes of one NP can couple with higher order angular modes of the second NP, resulting in hybrid modes with contributions from many different angular momenta.^{9,28} The sum over all of these interactions leads then to an analytical expression that is well approximated by an exponential function.²⁷ For particles with diameters in the range of 20–70 nm it was shown that the ratio of spectral shift, $\Delta\lambda_{\text{plas}}$, to individual NP resonance wavelength, λ_0 , is to a first approximation independent of the NP diameter and follows a universal scaling relationship.²⁵ For Au NPs, the universal scaling relationship as a function of interparticle separation, S , and particle diameter, D , was determined as

$$\frac{\Delta\lambda_{\text{plas}}}{\lambda_0} = 0.18e^{-\frac{S}{D}} \quad (2)$$

The Au NP calibration curves in Fig. 2a were derived by measuring λ_{plas} for DNA assembled from DNA spacers with a known number of base pairs and converting the number of DNA spacers into an effective length using a statistical polymer model (worm-like-chain model).¹⁶ The Ag Plasmon Ruler calibration curve was obtained by correlating single dimer optical spectroscopy with high resolution transmission electron microscopy (TEM) of surface immobilized Plasmon Rulers.¹⁸ The latter approach made it possible to explore plasmon coupling even at very short separations $S \leq 2$ nm. These studies revealed that – at least in the case of the Ag Plasmon Rulers – the relative magnitude of the spectral red-shift does not continue to increase at these very short separations. This observation was

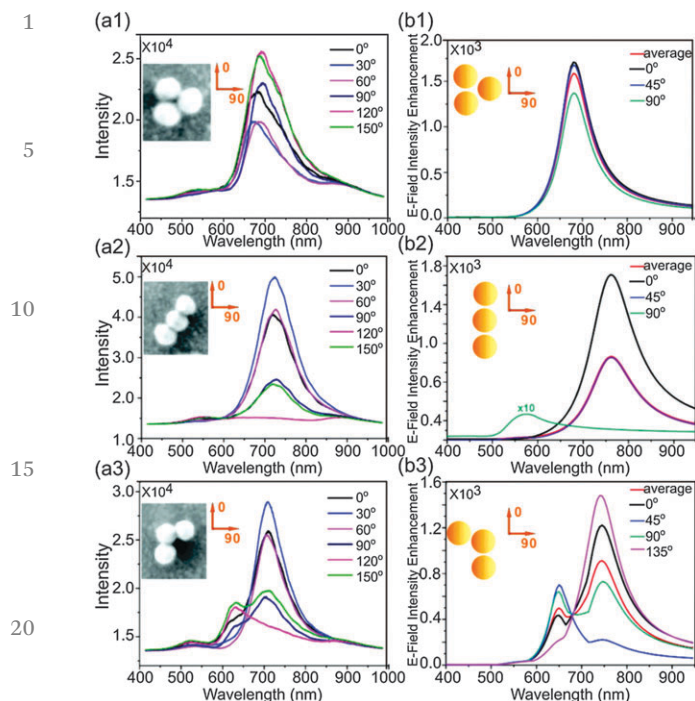


Fig. 3 Experimental scattering spectra from (a1) D_{3h} , (a2) $D_{\infty h}$, and (a3) C_{2v} trimers for different polarization angles. (b1–b3) Simulated E -field intensity enhancement spectra ($|E|^2/|E_0|^2$) of the same structures. Adopted with permission from Yan et al., *J. Phys. Chem. C*, 2011, **115**, 4578. Copyright 2011 American Chemical Society.

discussed in the context of quantum plasmonic²⁹ and/or non-local³⁰ electromagnetic effects.¹⁸ A similar effect was also observed in one-dimensional clusters of Au NPs assembled *via* a template guided self-assembly strategy³¹ and in Ag NP dimers manipulated in a scanning transmission electron microscope.³² Although the ability to access the quantum plasmonic regime through chemical assembly strategies will certainly open new vistas, for applications of noble metal NPs in bioimaging, the assumption of classical electromagnetic coupling behavior is justified. The ligand shells required to stabilize NPs in physiological buffers render the quantum plasmonic regime inaccessible in solution. Consequently, Fig. 2a shows the Ag NP plasmon coupling behavior only for the classic electromagnetic coupling regime with $S > 2$ nm. This classical plasmon coupling behaviour forms the foundation for resolving subdiffraction limit contacts as spectral shift in PCM (Fig. 2c).

3. Plasmon coupling in clusters: the effect of the cluster configuration

Many-body interactions are of great interest in key biological processes such as receptor clustering in two dimensions (*vide infra*), and the ability to resolve these interactions with PCM requires a fundamental understanding of plasmon coupling in clusters. In clusters containing more than two NPs, the measured resonance wavelength is no longer determined by the interparticle separation alone but also depends on the number of NPs in the cluster and their geometric arrangement.^{33,34} In

general, the optical properties of NP clusters are strongly size dependent for small cluster sizes but converge in larger clusters. In one- and two-dimensional clusters of close-packed 40 nm diameter Au NPs, a strong red-shift of the peak plasmon resonance was observed with growing size for cluster sizes $n \leq 4$ (at constant interparticle separation).^{31,33} A further increase in cluster size resulted only in small incremental changes of the resonance wavelength. Electromagnetic simulations and experimental SERS spectra of these systems indicated a similar convergence for the E -field intensity. We emphasize that sharp far-field resonances and strong E -field enhancement can be engineered in cluster sizes $n > 4$ for special configurations that sustain collective cluster resonances, such as Fano resonances.³⁴ These specific structures are, however, of minor relevance in NP labeling experiments due to their stringent symmetry requirements.

The light polarizing properties of anisotropic NP clusters are of high practical value since they provide additional information about the geometry of NP clusters in the optical microscope.³³ This is illustrated for NP trimers with different geometries (D_{3h} , $D_{\infty h}$, C_{2v}) in Fig. 3. The figure contains experimental scattering spectra and simulated near-field spectra for different light polarizations. Both the near- and far-field spectra of the highly symmetric D_{3h} configuration show only a weak polarization dependence, whereas the optical response of the anisotropic $D_{\infty h}$ configuration, the rod-like cluster, is strongly polarization dependent. Scattering and near-field intensities are much stronger for a light polarization pointing along the long trimer axis. The spectra of the C_{2v} configuration contain two clearly distinct spectral features, whose relative intensities can be modulated by rotation of the light polarization. Overall, Fig. 3 illustrates vividly the impact of the geometric cluster configuration on near- and far-field responses and the value of polarization-resolved scattering spectroscopy in retrieving structural information.

4. Implementation of plasmon coupling microscopy (PCM)

After introducing the fundamental concepts of plasmon coupling in noble metal NP dimers and clusters in the previous sections, we will in this section introduce different experimental strategies for its utilization in biosensing and imaging. The spectral and/or light polarization properties collected from a diffraction limited spot in an optical microscope depend on the near-field coupling between the NP labels in this area. The magnitude of the coupling is sensitive to nanoscale interparticle separations and the NP association level. Spatial maps of plasmon coupling, consequently, encode information about the average separation of NP labeled species as a function of location, and the strategy of PCM is to collect this information to provide insight into subdiffraction limit separations and separation changes. As we will outline in more detail below, the spectral and/or polarization properties of NP labels can be monitored in conventional widefield microscopy, which makes it possible, for instance, to track plasmon coupling between

1 laterally diffusing NPs³⁵ or to map the local degree of NP clustering
 2 simultaneously at many locations across the entire cell surface.^{36,37}
 3 Due to the superb photophysical stability of the NP labels, optical
 4 PCM studies can be performed continuously without limitation in
 5 observation time. The latter is a great advantage for the investiga-
 6 tion of stochastic processes that cannot be induced at defined time
 7 points or for slow biological processes. When designing a PCM
 8 experiment, one also has to be aware of the limitations of the
 9 technique. Since PCM is an elastic light scattering based micro-
 10 scopy technique, it is primarily intended for cellular studies with
 11 low background. *In vivo* or tissue imaging is difficult to realize due
 12 to the intrinsically high scattering background of biological tissue.
 13 Before we discuss different experimental strategies that have been
 14 applied to quantify plasmon coupling in optical microscopy, we will
 15 first review appropriate labeling strategies that allow for a selective
 tagging of the moiety of interest with an Au or Ag NP.

4.1 NP immunolabeling

16 Bioconjugation of NPs is an active research area and a review of
 17 all functionalization strategies developed thus far goes beyond
 18 the scope of this Tutorial. We refer the interested reader to the
 19 excellent review in ref. 38 and focus in the following on
 20 functionalizing strategies that we have tested in our laboratory,
 21 instead. Since the analysis of the plasmon resonance wave-
 22 length as an indicator of spatial clustering, for instance, of
 23 receptors in the cell membrane, is only useful when the NP
 24 labels are stable and do not show spontaneous self-association
 25 in salt buffers, one particular challenge in PCM is the develop-
 26 ment of NP labels that combine high colloidal stability with
 27 high selective binding efficacy for their target. We will provide
 28 two examples of labeling strategies that have been demon-
 29 strated to fulfill these requirements.

30 **4.1.1 Secondary antibody assisted NP labeling.** Au NPs with
 31 a diameter of 40 nm are frequently used labels in PCM since they
 32 provide a good compromise between signal intensity and size.
 33 Mammalian cells are coated by a polymeric matrix, which is
 34 referred to as glycocalyx. Overcoming this coating can represent
 35 a significant challenge for achieving an efficient labeling of cell
 36 surface receptors and other functionalities with ~40 nm dia-
 37 meter labels. The NP immunolabeling strategies reviewed in this
 38 and the following sections have been demonstrated to achieve a
 39 successful targeting of cell surface species with NP labels.^{39,40}
 40 The left column in Fig. 4a outlines a secondary antibody assisted
 41 labeling strategy, which was originally developed for the labeling
 42 of the epidermal growth factor receptor (EGFR or ErbB1) in the
 43 plasma membrane of *in vitro* cancer cells.³⁹ The combination of
 44 primary and secondary antibodies on the cell surface in the
 45 secondary antibody assisted labeling procedure creates a spacer
 46 that makes the targets more accessible for the colloidal NP
 47 labels. The binding affinity of the NP label is further increased
 48 by multiple biotins bound per secondary antibody. The NPs
 49 contain a self-assembled brush of 3.4 kDa polyethylene glycol
 50 (PEG) molecules with a thiol terminus to bind to the metal
 51 surface and a terminal azide to conjugate to alkyne functiona-
 52 lized anti-biotin antibody or Neutravidin through a Cu^I catalyzed
 53 1,3-dipolar cycloaddition (Fig. 4b).³⁹ We emphasize in passing

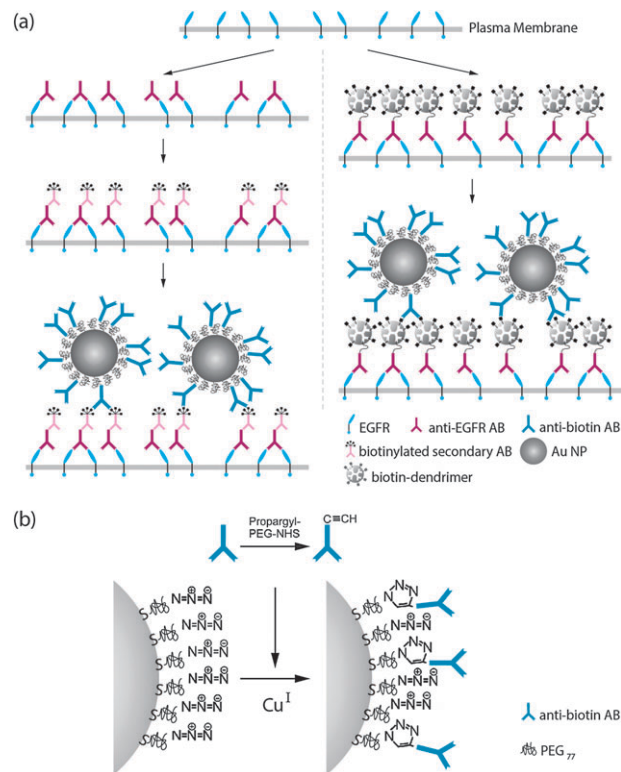


Fig. 4 (a) Secondary antibody assisted NP labeling strategy (left) and dendrimer enhanced binding approach (right). (b) Covalent attachment of antibodies or Neutravidin through 1,3-dipolar cycloaddition. Adopted with permission from Wang *et al.*, *ACS Nano*, 2011, 5, 6619. Copyright 2011 American Chemical Society and Rong and Reinhard, *PLoS One*, 2012, e34175.

that the azide-PEG based NP functionalization strategy is not limited to antibodies, but can be expanded to peptides (growth factors, *etc.*), glycopeptides, and other biomolecules of interest.

The PEG molecules on the NP surface not only allow for a facile functionalization of the particle, but they also achieve an efficient steric stabilization of the NPs. UV-Vis spectroscopy (Fig. 5a) and dynamic light scattering (DLS) (Fig. 5b) have confirmed the stability of the NP immunolabels when incubated with fixed cells in 0.5× phosphate buffered saline (PBS) or living cells in 1× Hank's buffer.^{39,40} The specificity of the labels was validated in a control experiment, in which the cells were incubated without (Fig. 5c) or with (Fig. 5d) free anti-biotin antibody. The efficient competitive inhibition confirms that NP immunolabel binding is target specific.

4.1.2 Dendrimer assisted NP labeling. The dendrimer assisted labeling strategy outlined in the right column of Fig. 4a has been shown to be effective under live cell conditions for which extensive washing or NP co-incubation is not permissible.⁴⁰ Instead of a combination of primary and secondary biotinylated antibody, this scheme uses primary antibodies that are covalently connected to a biotinylated dendrimer through a flexible linker. Small, but highly branched dendrimers introduce multiple biotins per targeted receptor that are easily accessible and, thus, increase the binding affinity of the NP labels. The Au NP labels can be generated through the synthetic strategies outlined in the previous section.

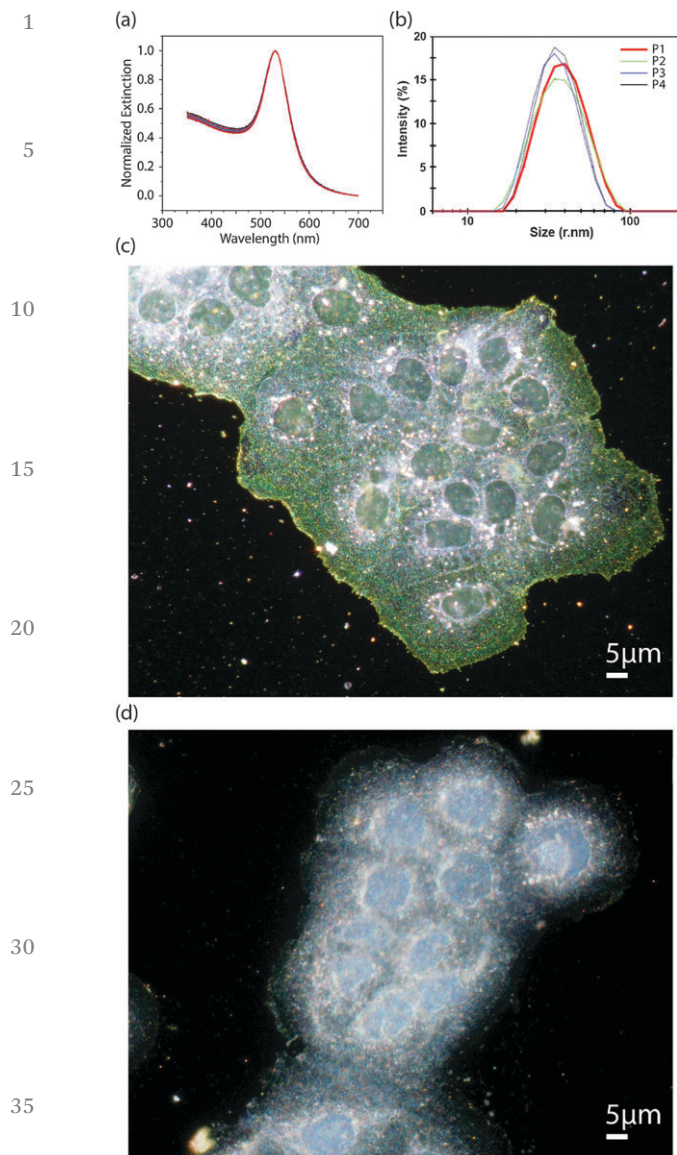


Fig. 5 (a) UV-Vis spectra of antibody functionalized 40 nm Au NPs in 0.5× PBS recorded over a time interval of 225 min (1 spectrum every 15 min) and (b) hydrodynamic radii determined by DLS measured before and after incubation of 40 nm Au NPs with living cells in 1× D-PBS buffer (P1/P2: Neutravidin functionalized NPs before/after incubation with cells; P3/P4: antibody functionalized NPs before/after incubation with cells). (c) Dark-field image of A431 cells labeled with 40 nm Au NPs using a secondary antibody assisted labeling strategy. (d) Dark-field image of A431 cells labeled under identical conditions in the presence of an excess of free anti-biotin antibody (competitive inhibition). The biotin binding sites are blocked by free anti-biotin antibody from solution, preventing Au NP immunolabeling. Adopted with permission from Wang *et al.*, *ACS Nano*, 2011, **5**, 6619 and Yu *et al.*, *Anal. Chem.*, 2013, **85**, 1290. Copyright 2011 and 2013 American Chemical Society.

4.2 Optical approaches for quantifying plasmon coupling

Different optical techniques can be applied to characterize the spectral properties of NPs spatially resolved with two figures of merits determining the details of the instrumental implementation: temporal and spectral resolution. In most practical realizations one has to compromise between these two figures

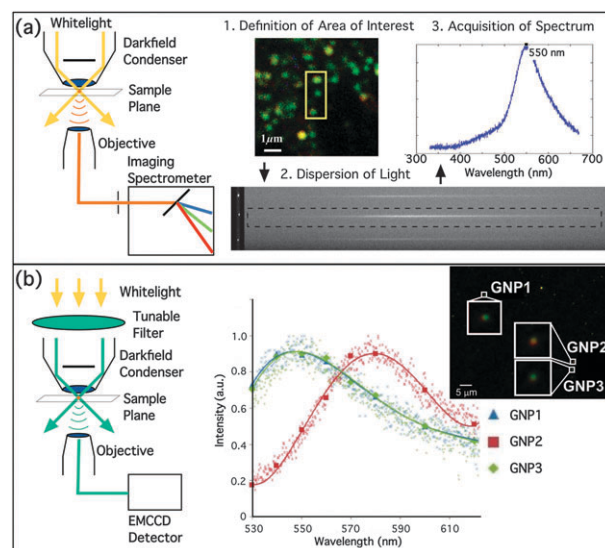


Fig. 6 (a) Spatially resolved spectral analysis of individual NPs and NP clusters using an imaging spectrometer. (b) Multispectral imaging. Left: set-up, right: comparison of scattering spectra for three Au NPs (GNP1–3) using an imaging spectrometer (small symbols) or multispectral imaging (large symbols and continuous lines).

of merits. In Sections 4.2.1–4.2.3 we will review different PCM realizations in the sequence of decreasing spectral but increasing temporal resolution. In Section 4.2.4 we will then show how spectrum-based approaches can be augmented to yield light polarization information, as well.


4.2.1 Full spectral analysis. A typical experimental set-up is shown in Fig. 6a.³⁹ A spectrometer attached to a darkfield microscope is used to analyze the light scattered from a defined area in the sample plane. The opening of the entrance slit of the spectrometer is adjustable along the horizontal axis and the area of interest along the vertical axis can be controlled *via* software control. The collected light is then dispersed and collected on an electron multiplying charge-coupled device (EMCCD). While the method provides detailed spectroscopic information of specific locations, it is not suitable for acquiring simultaneous spectral information from many different locations distributed across large areas with high temporal resolution or throughput. Furthermore, the spectral analysis is also not compatible with monitoring the spectra of moving NP labels.

4.2.2 Multispectral imaging. To overcome some of the limitations of the full spectral analysis, multispectral imaging schemes have been implemented that compromise between spectral and temporal resolution and that allow for a simultaneous monitoring of plasmon coupling at many arbitrary locations in an extended area.^{36,41,42} One implementation is shown in Fig. 6b, which is described in detail in ref. 41. In a conventional darkfield microscope the entire field of view is subsequently illuminated with different wavelengths and at each wavelength a monochromatic image is recorded on a camera. A rapid switching of the excitation wavelength can be achieved, for instance, using an intense light source in combination with a fast filter switching device or a tunable liquid crystal filter, or using a light emitting diode (LED) illumination array. After the individual images have been corrected for the intensity

1 profile of the excitation source, the monochromatic images can be
 2 combined into a composite image, in which each pixel contains the
 3 information about the relative intensities on the monitored wave-
 4 length channels.⁴¹ Multispectral imaging provides spectral informa-
 5 tion of the entire field of view with reasonable acquisition rates; the
 6 collection of multiple complete multispectral images per second is
 7 currently routine and significantly higher acquisition rates are
 8 technically feasible.⁴² Fig. 6b contains the spectra from multiple
 9 Au NPs in one field of view obtained through multispectral imaging
 10 as well as through full spectral analysis using an imaging spectrom-
 11 eter. The direct comparison confirms that multispectral imaging
 12 and full spectral analysis provide equivalent information. The
 13 monitored area in multispectral imaging can be even further
 14 increased if the widefield microscope used for data collection is
 15 replaced with a lensless imaging system.⁴³

16 **4.2.3 Ratiometric imaging.** While multispectral imaging
 17 allows monitoring of plasmon coupling in a large field of view,
 18 the time delays between the individual monochromatic images
 19 used to calculate the composite image is problematic for imaging
 20 dynamic processes or tracking moving objects. The temporal delay
 21 between the individual channels can be avoided through ratio-
 22 metric imaging approaches where wavelength selective (dichroic)
 23 beamsplitters in combination with bandpass filters are used to
 24 image the entire field of view simultaneously on multiple detection
 25 channels. The most common implementation of this technique for
 26 dual color imaging on two wavelength channels λ_1 and λ_2 is
 27 schematically illustrated in Fig. 7a.³⁵ The approach generates two
 28 images of the same field of view at two defined wavelengths (Fig. 7b
 29 and c) simultaneously. Fitting the point-spread-functions (PSFs)
 30 of individual objects on the monitored wavelength channels, after
 31 correction for differences in the transmission properties of the
 32 filters and the excitation profile of the light source, provides the
 33 integrated intensities $I_{\lambda_1}(n)$ and $I_{\lambda_2}(n)$ for a frame n , which can then
 34 be used to calculate the intensity ratio $R(n)$:

$$R(n) = \frac{I_{\lambda_1}(n)}{I_{\lambda_2}(n)} \quad (3)$$

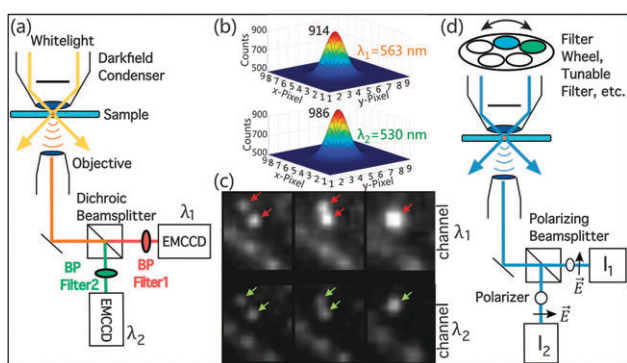

35
 40
 45
 50
 55
 Fig. 7 (a) Experimental set-up for dual color ratiometric imaging. (b) Fitted point-spread-functions (PSFs) for single gold NPs simultaneously recorded on 530 nm and 563 nm channels. (c) Two Au NPs diffusing on a cell surface simultaneously tracked on two wavelength channels. (d) Experimental set-up for polarization resolved PCM. Adapted with permission from Rong *et al.*, *Nano Lett.*, 2008, **8**, 3386. Copyright 2008 American Chemical Society.

1 Although the spectral information encoded in R is limited, it
 2 does allow for a ratiometric detection of NP association.³⁵ If the
 3 monitored wavelength channels are chosen so that $\lambda_1 > \lambda_2$, the
 4 formation of strongly coupled NPs results in an increase in R .

5 **4.2.4 Polarization resolved PCM.** PCM can be augmented
 6 to record both spectral and polarization information. In polar-
 7 ization resolved PCM (PRPCM)²² the light scattered from indi-
 8 vidual NP labels is collected through an adequate objective and
 9 then split into two orthogonal polarization channels using a
 10 polarizing beam splitter (Fig. 7d). The intensities I_s and I_p on
 11 the two polarization channels in each frame n are used to
 12 calculate the degree of polarization, P , defined in this context as

$$P(n) = \frac{I_s(n) - I_p(n)}{I_s(n) + I_p(n)} \quad (4)$$

13 P describes the distribution of the detected light on two ortho-
 14 gonal polarization axes, whose direction is defined in lab coordi-
 15 nates. For anisotropic NP clusters with a strongly enhanced
 16 scattering cross-section along one direction, *e.g.* along the long
 17 axis of a dimer, P encodes direct information about the orienta-
 18 tion of the object in the plane perpendicular to the axis of the
 19 objective. For quasi-one-dimensional plasmonic nanostructures,
 20 the intensity measured on one of the polarization channels is
 21 directly proportional to the square of the cosine of the angle θ ,
 22 formed by the long particle axis and the respective polarization
 23 axis.⁴⁴ For a dimer with a variable interparticle separation, P
 24 depends on both the interparticle separation and the dimer
 25 orientation in space.²² However, for a dimer performing a
 26 rotation in one plane, only fluctuations in the interparticle
 27 separation lead to a change in total scattering intensity, $I_{\text{tot}} =$
 28 $I_s + I_p$, which enables one to decouple separation from orienta-
 29 tion changes. Additional spectral information in PRPCM becomes
 30 available if the sample is illuminated with unpolarized light of
 31 alternating excitation wavelength λ_1 and λ_2 (Fig. 5d).⁴⁵ This can
 32 be accomplished with a rapid filter switching device, LED array,
 33 alternating laser illumination, *etc.* The spectral information can
 34 be quantified by calculating intensity ratios, R , from the total
 35 intensities obtained in two subsequent frames:

$$R(n) = \frac{I_{\text{tot}}(n)}{I_{\text{tot}}(n-1)} \quad (5)$$

40 where $n > 1$. The recorded intensities need to be corrected for the
 41 different transmission properties and the excitation profile of the
 42 light source.

5. PCM in cellular imaging and biosensing

45 In the following, we will review a number of studies in which
 46 PCM was applied to resolve subdiffraction limit contacts in a
 47 cellular context. We emphasize that we focus here primarily on
 48 case studies performed in our own laboratory, but refer the
 49 interested reader also to the related work by Sokolov and
 50 coworkers,⁴⁶ Wax and coworkers,¹³ or El-Sayed and coworkers.⁴⁷
 51 Due to the size of the probes and its dynamic range, plasmon

coupling is particularly useful to probe interactions that occur on length scales of a few tens of nanometers, which is of interest in the large scale association (clustering) of transmembrane proteins, membrane domain formation, *etc.* Applications of PCM have, consequently, focused on probing the dynamic structures of the plasma membrane, the lateral spatio-temporal heterogeneity of specific cell surface proteins, and the uptake and subsequent trafficking of NPs. All of these applications benefitted from at least one of the advantages of the PCM technique, including its ability to monitor subdiffraction limit interactions between NP tagged species at many locations in a large field of view simultaneously, high temporal resolution, or the extraordinary photophysical stability of the probes which are entirely free of blinking or bleaching. Like with any label-based approach, one important point of consideration in PCM studies is the potential impact of the NP label on the biological system of interest. The use of NP labels is generally unproblematic for investigations using fixed cells or living cells when the fate of the NPs itself is of interest. In other live cell studies a potential influence of the NPs needs to be evaluated on a case-by-case basis. Strategies to mitigate potential perturbations involve the development of small but bright monovalent NPs with inert surfaces. We also note that a potential perturbation of a ligand or receptor upon nanoconjugation is not bad *per se*. Instead, it can also provide new opportunities for controlling and manipulating cellular functionalities.⁴⁸ A successful realization of NP-enabled cellular control requires, however, precise understanding of the underlying mechanisms, and PCM techniques are ideally suited to elucidate them.

5.1 Resolving transient interactions between laterally diffusing receptors through ratiometric NP tracking

Many cellular processes involve transient interactions that are difficult to detect due to their short-lived nature and because they occur on deeply subdiffraction limit length scales. Although a multicolor tracking approach makes it possible to discern subdiffraction limit separations through spectral separation, the technique fails for identical labels. Consequently, a systematic investigation of interactions between multiple identical groups, as they occur for instance during self-association of proteins, such as ErbB1, in the cellular plasma membrane,⁴⁹ remains challenging. The ratiometric PCM detection scheme described in Section 4.2.3 provides now a potential alternative to overcome this challenge. Rong *et al.* tested the sensitivity of this approach for detecting the compaction of DNA tethers in Au NP Plasmon Rulers (Au NP diameter ~ 40 nm) as well as for detecting the conversion of NP dimers into monomers by enzymatic cleavage of the DNA tether.³⁵ The DNA tethers were compacted from approx. 15 nm to 6 nm through addition of positively charged dendrimers that bind to the negatively charged DNA. According to the experimental Plasmon Ruler calibration relationship (Fig. 2a), the resonance wavelength of Plasmon Rulers assembled from 40 nm increases from 568 nm to 621 nm if the interparticle separation is decreased from 15 to 6 nm. The resonance wavelength of an individual NP (dimer with infinite separation)

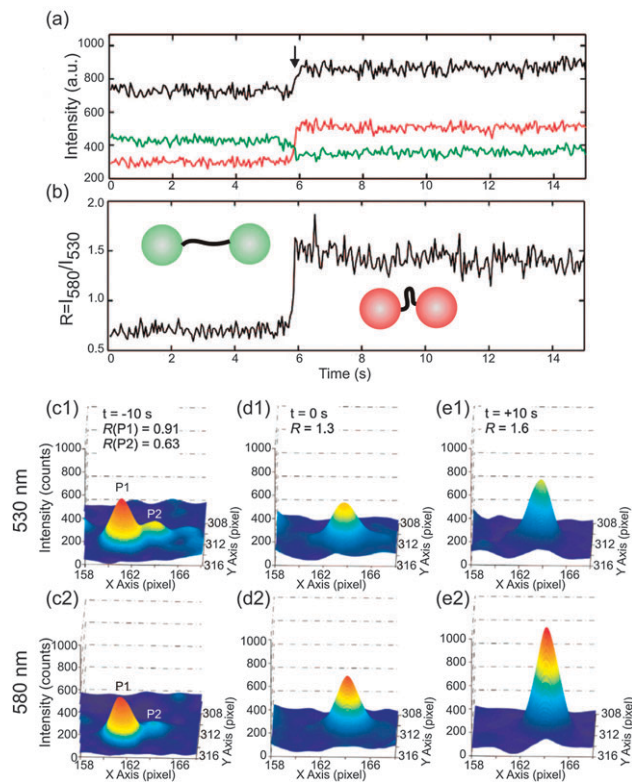


Fig. 8 (a) Scattering intensities $I_{580\text{nm}}$ (red) and $I_{530\text{nm}}$ (green), as well as the total intensity (black) of a single Plasmon Ruler recorded during its compaction. (b) Intensity ratio R plotted as a function of time. A spectral red-shift is indicated by an anti-correlated change of $I_{580\text{nm}}$ and $I_{530\text{nm}}$ and an increase in R . PSFs of two individual Au NPs, P1 and P2, tracked on a 530 nm channel (c1, d1, e1) and a 580 nm channel (c2, d2, e2) at three different time points on the plasma membrane of a HeLa cell. The increase in intensity on the 580 nm channel after optical colocalization indicates a spectral red-shift due to strong electromagnetic coupling between P1 and P2. Reproduced with permission from Rong *et al.*, *Nano Lett.*, 2008, **8**, 3386. Copyright 2008 American Chemical Society.

is approximately 537 nm. Rong *et al.* performed the ratiometric imaging using a dichroic beam splitter with a cutoff wavelength of 560 nm and bandpass filters centered at 530 nm and 580 nm with a spectral width of 10 nm. Fig. 8a shows the intensities on the chosen wavelength channels (I_{580} and I_{530}) and the total intensity for a single Plasmon Ruler as a function of time during a compaction event. Fig. 8b contains the calculated intensity ratio $R = I_{580}/I_{530}$. The induced compaction of the DNA tether is indicated by the sudden increase in total intensity. The intensity on the 580 nm channel increases, whereas the intensity on the 530 nm channel decreases. This anti-correlated intensity change and the resulting increase in R are unique indicators of a spectral red-shift.

After validating the ratiometric detection, Rong *et al.* applied it to resolve nanometer contacts during optical colocalization of NP labeled integrins that performed a lateral diffusion on the dorsal surface of living HeLa cells.³⁵ Some of the tracked Au NP labels approached each other until they were no longer distinguishable, and the duration of these optical colocalization events showed a broad range of variation. While short periods

of colocalization can be coincidental, prolonged colocalization events indicate either a direct association of integrins or a confinement of the labeled integrins to a cell surface compartment with lateral dimensions below the resolution limit of the optical microscope. To differentiate between these two scenarios more information about the separation of the NP labeled integrins is required. This information is available through PCM. Fig. 8c–e shows the point-spread-functions for two integrin tethered NPs on the two monitored wavelength channels at three different time points. In Fig. 8c, the two NPs are still discernible and for both NPs the intensity is higher on the green than on the red channel, $I_{530} > I_{580}$. In Fig. 8d, the PSFs of P1 and P2 overlap and the NPs are no longer optically discernible. Concurrent with the optical colocalization, the relative intensity distribution on the two wavelength channels changes. The peak intensity is now higher on the 580 nm than on the 530 nm channel, resulting in an increase in R . In Fig. 8e, both the total intensity and the R value reach their maximum. The observed strong spectral shifts in this example indicate short interparticle separations of below one NP diameter, which is consistent with the association of the integrins into a larger cluster.

5.2 Mapping lateral membrane compartmentalization through PCM

Diffusion studies of individual lipids and proteins in conventional high speed particle tracking have emerged as an important tool for probing the intrinsically dynamic structure of biological membranes and provided key insights into the structural compartmentalization of the plasma membrane.⁵⁰ PCM augments these approaches now with the ability to simultaneously monitor the separation, S , between individual NP labels once they have approached each other to within approximately one NP diameter and are, thus, no longer optically distinguishable during their lateral diffusion on the plasma membrane. PRPCM provides additional information about the orientation of the long axis in strongly anisotropic clusters, such as NP dimers. This is illustrated in Fig. 9, which contains the diffusion tracks and the corresponding P , R , and S values as a function of time for three different Plasmon Rulers, PR1–3, as described in ref. 45. The Plasmon Rulers were assembled from ~ 30 nm diameter Ag NPs using an ~ 13.7 nm long DNA spacer resulting in an average center-to-center separation of ~ 44 nm. Under the chosen experimental conditions, the Plasmon Rulers attached spontaneously and non-reversibly to plasma membranes isolated from HeLa cells without the need for any specific binding chemistry.

The diffusion trajectory of PR1 was recorded using the PRPCM set-up outlined in Fig. 7d. PR1 was tracked using a combination of bandpass filters centered at 430 nm and 470 nm, and PR2–3 were tracked with filters centered at 450 nm and 490 nm. Approximate S values were obtained by converting the R values into separations using an Ag Plasmon Ruler calibration.⁴⁵ The spatial trajectories in the left column of Fig. 9 show that the spatial confinement of the Plasmon Rulers increases from PR1 over PR2 to PR3. The R , S , and P trajectories in the right column were obtained with a frame rate of 5 images

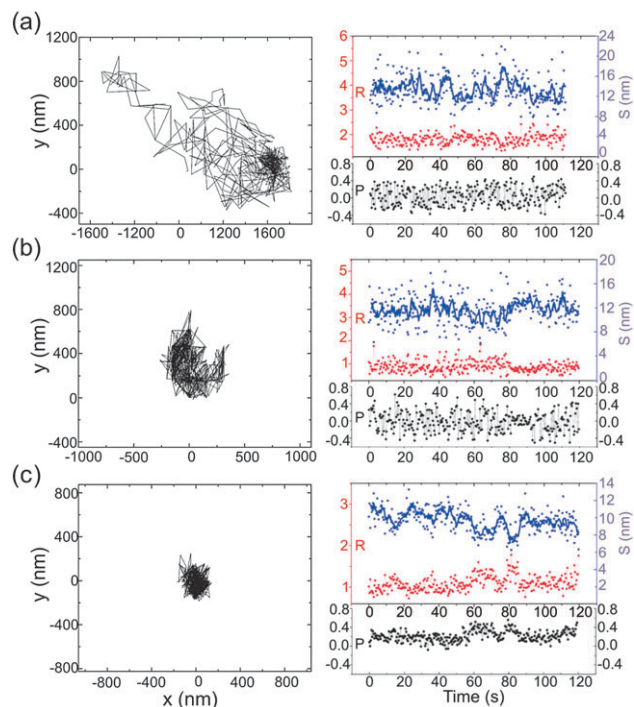


Fig. 9 Tracking of three individual Ag Plasmon Rulers, PR1–3, on isolated plasma membranes through PRPCM. The Ag dimers were assembled through a DNA-programmed self-assembly strategy and were then monitored on plasma membranes of lysed HeLa cells. Left column: Plasmon Ruler trajectory. Right column: intensity ratios, R , degree of light polarization, P , and approximate interparticle separation, S , as a function of time. Reproduced with permission from Rong *et al.*, *Nano Lett.*, 2010, **10**, 230. Copyright 2010 American Chemical Society.

per second. The average interparticle separation S_{av} decreases from 13.4 ± 2.8 nm, over 11.7 ± 2.3 nm to 9.7 ± 1.3 nm for PR1–3.⁴⁵ The decreasing interparticle separation and the accompanying decrease in the dynamic range in the S trajectories indicate an increasing spatial confinement of the Plasmon Ruler in compartments that are of similar dimensions as the total length of the Plasmon Ruler (DNA spacer + NPs). Although the P and R trajectories were recorded with a relatively low frame rate of 5 Hz in this example, the P trajectories, especially for PR1 and PR2, show a large degree of fluctuations due to transient orientation changes. The observation of resolvable fluctuations in P at this frame rate is a clear indication of significantly hindered rotational motion of the spatially confined Plasmon Rulers. In the case of free rotational motion, the polarization information should have been averaged out at this acquisition rate to result in an average $P \approx 0$. For PR3 the frequency and magnitude of the fluctuations in the P trajectory are significantly decreased, but P remains >0 . This observation is consistent with an even stronger spatial confinement and localization of the Plasmon Ruler in a compartment in which rotational motions between different spatial orientations are separated by high energetic barriers. Overall, the polarization resolved tracking studies in Fig. 9 confirm that an increasing spatial confinement is correlated with a decreasing average interparticle separation and decreasing rotational mobility of

the Plasmon Rulers. This correlation makes Plasmon Rulers interesting tools for probing membrane compartmentalization on the length scale of the Plasmon Rulers simultaneously at different locations on a cell surface as a function of time. This advantage was utilized to detect ErbB1 enriched membrane domains and to monitor their structural dynamics during their lateral diffusion on the surface of living cells.⁴⁰

5.3 Quantifying spatial nanoclustering on plasma membranes through plasmon coupling

Plasma membrane proteins are often not homogeneously distributed but locally enriched in specific membrane environments.^{49,50} Especially for proteins that require inter-receptor interactions, spatial clustering represents a potential mechanism for modulating signaling intensity, threshold and response. Quantitative information about the spatial organization of a cell surface protein could, therefore, have similar biomarker relevance as the total expression level.³⁶ As we will discuss in this section, the ability of NP immunolabels to interrogate the relative vicinity on the tens of nanometer length scale and to transduce this information into the far-field provides new opportunities for profiling the spatial clustering of the targeted species in addition to its surface expression through an all-optical approach.

The impact of the NP spatial organization on the collective resonance wavelength, λ_{pl} , as a function of average NP density, ρ , is shown in Fig. 10. The ensemble-averaged resonance wavelengths, $\lambda_{\text{pl}}(\rho)$, were obtained from simulated polarization-averaged dark-field scattering spectra. The simulations were performed at defined ρ values for different degrees of NP clustering in an area of $2 \times 2 \mu\text{m}^2$ using generalized multiple particle Mie theory (GMT).³⁶ Four different clustering configurations were considered in the GMT simulations: random, 50% dimers, 50% trigonal trimers, and 50% random clusters. The latter were generated by randomly placing one-fourth of the total number of NPs near distributed NPs with a minimum separation of 5 nm. In the case of 50% dimers and trimers, the interparticle separation was kept constant at 5 nm. The random NP distribution exhibits a very shallow initial increase in λ_{pl} with increasing ρ since the probability of the formation of electromagnetically strongly coupled NP pairs or clusters is low at low ρ values. With increasing ρ the average interparticle separation gradually decreases and the effect of plasmon coupling increases. In contrast, configurations enriched in dimers and trimers with constant (and very short) interparticle separations show a much steeper increase in resonance wavelength that converges rapidly with increasing ρ . The 50% clustering configuration has larger average interparticle separations than the clustered dimers and trimers and the slope of its $\lambda_{\text{pl}}(\rho)$ curve lies between those of the strongly coupled dimer and trimer configurations and the total random configuration. Overall, Fig. 10 confirms clearly a sensitive dependence of the measured spectral response on NP clustering.

Although PCM cannot directly image individual NP labeled receptors if their separation lies below the resolution limit of the optical microscope, the spectral response of NP immunolabels provides synergistic information about their clustering. Membrane areas that are locally enriched in the receptor

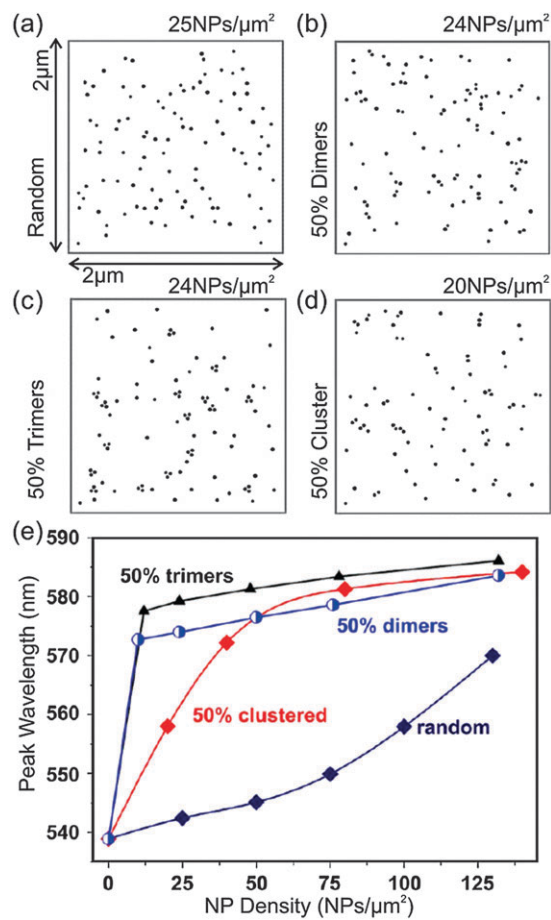


Fig. 10 Evaluating the interplay of average Au NP density, ρ , and local clustering on the ensemble-averaged plasmon resonance wavelength, λ_{plas} , through GMT simulations. Four different 40 nm NP organization levels were considered for different ρ values: (a) random, (b) 50% dimers, (c) 50% trimers, (d) 50% random clusters. (e) Peak resonance wavelength as a function of ρ and NP organization. Adapted with permission from Wang *et al.*, *Nano Lett.*, 2012, **12**, 3231. Copyright 2012 American Chemical Society.

represent high affinity binding sites for NP immunolabels and template the formation of clusters of strongly coupled NPs. These areas are indicated by a spectral red-shift when compared with areas in which the receptors are not clustered and individual NPs dominate the scattering response. Wang *et al.* utilized the clustering dependent spectral NP response to compare the local ErbB1 and ErbB2 densities on the plasma membrane of selected cancer model cells with different expression levels (A431, SKBR3, MCF7).³⁶ For ErbB family type receptors information about their spatial distribution is especially useful since functionality depends on their organization into dimers and potentially higher oligomers, which is anticipated to be influenced by the local receptor density.^{4,36,49} Wang *et al.* utilized the secondary antibody based labeling strategy introduced in Section 4.1.1 to label ErbB1 and ErbB2. The cells were incubated with increasing concentrations of NP immunolabels to systematically vary the average NP density, ρ . Scattering spectra were then recorded from peripheral stretched membrane areas, where the signal to noise was largest, by averaging the spectral content over the entire

1 opening slit of the spectrometer (Section 4.2.1). The cells were
 2 subsequently inspected in the SEM to determine ρ . For the highly
 3 overexpressed ErbB1 receptor on A431 cells, the experimentally
 4 obtained $\lambda_{\text{pl}}(\rho)$ relationship reproduces the simulated curve for the
 5 50% random cluster configuration shown in Fig. 10e.³⁶ This
 6 finding implies an increase in NP clustering throughout the
 7 investigated NP density range. In contrast, for ErbB2 on MCF7
 8 and SKBR3, a much faster convergence of the $\lambda_{\text{pl}}(\rho)$ relationship
 9 against a lower peak resonance wavelength was obtained. The
 10 obtained $\lambda_{\text{pl}}(\rho)$ relationships confirm less NP immunolabel cluster-
 11 ing for MCF7/ErbB2 and SKBR3/ErbB2 than for A431/ErbB1.³⁶ This
 12 finding is consistent with overall lower receptor densities and less
 13 and smaller receptor enriched membrane compartments for
 14 MCF7/ErbB2 and SKBR3/ErbB2.³⁶

15 PCM is not limited to an analysis of area-averaged spectral
 16 information but can, instead, also be used to detect differences in
 17 the spatial organization of the targeted cellular receptors on sub-
 18 cellular length scales. This has been utilized, for instance, to
 19 compare ErbB1 density and spatial organization on filopodia
 20 (quasi-one-dimensional projections from the cell edge) and the
 21 actual cell body.³⁹ Consistent with a higher receptor density, the
 22 average plasmon resonance wavelength measured on filopodia was
 23 significantly red-shifted when compared to that measured on the
 24 actual cell body. The increased NP immunolabel density on the
 25 filopodia was subsequently confirmed *via* SEM. In another study³⁷
 26 both expression and spatial clustering of the cell surface glycopro-
 27 teins CD24 and CD44 on MCF7 and SKBR3 cells were analyzed. The
 28 relative NP labeling intensities were found to be correlated with the
 29 receptor expression levels. An optical inspection of the labeled cell
 30 surface in the microscope revealed discrete spots on the cell surface
 31 with colors ranging from green to orange (Fig. 11a) due to cluster-
 32 ing of the NP immunolabels on the cell surface. According to a
 33 statistical analysis of the scattering spectra of individual spots,
 34 CD24 showed a significantly higher degree of clustering than CD44
 35 (Fig. 11b, top). Lipid raft disruption through cholesterol sequestra-
 36 tion (Fig. 11b, bottom) removed the preferential clustering of CD24,
 37 indicating an enrichment of CD24 in lipid rafts.

5.4 Imaging of NP uptake and subsequent cellular processing in living cells

38 Although the previous sections focused on the applications of
 39 PCM for probing the structure and dynamics of the plasma
 40 membrane, the method is not limited to cell surface processes.
 41 It is also well suited for investigating the intricate cellular
 42 mechanisms orchestrating NP uptake and trafficking. Noble
 43 metal NPs are a unique class of cargo for these studies since
 44 they can be simultaneously tracked and spectrally analyzed in
 45 PCM. It is, therefore, possible to monitor both the spatial
 46 trafficking of the uptaken NPs and their resonance wavelength,
 47 which depends on the local association level of the NPs. This
 48 gain of information is important since receptor mediated
 49 endocytosis involves the incorporation of NPs into membrane
 50 vesicles that can fuse in subsequent trafficking events and,
 51 thus, induce clustering of NPs contained within the vesicles.
 52 Furthermore, PCM can be combined with immunofluorescence
 53 labeling, which makes it possible to investigate the

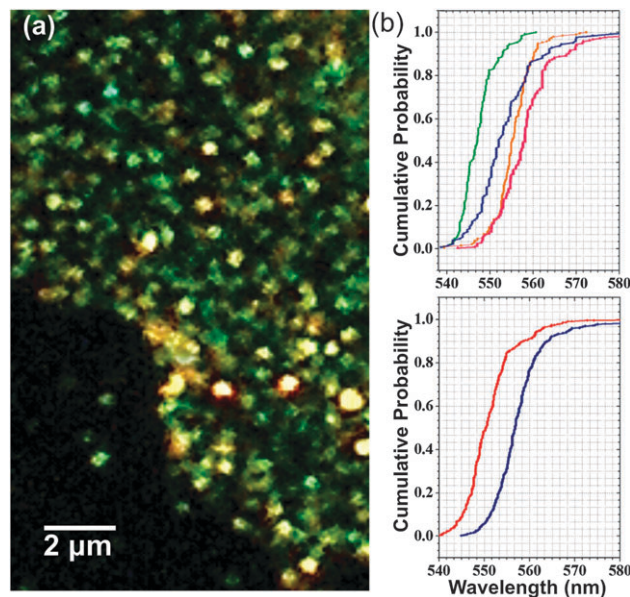


Fig. 11 (a) Magnified view of a section of a MCF7 cell after labeling surface expressed CD24 with 40 nm Au NPs. (b) Top: cumulative distribution plots of λ_{plas} after NP labeling of the following cell/receptors: MCF7/CD44 (blue), SKBR3/CD24 (orange), MCF7/CD24 (pink). The distribution of Au NPs in the ambient medium with a refractive index of $n_r = 1.40$ is indicated by a blue line. Bottom: cumulative distribution plot of λ_{plas} for NPs targeted at MCF7/CD24 before (red) and after (blue) treatment with m- β -CD to sequester cholesterol from the membrane. Adapted with permission from Yu *et al.*, *Anal. Chem.*, 2013, **85**, 1290. Copyright 2013 American Chemical Society.

spatiotemporal distribution of NPs inside cells and to probe their interactions with specific cellular components.

The synergistic gain resulting from a combination of PCM and immunofluorescence microscopy was first utilized in a mechanistic study of the scavenger receptor mediated uptake and trafficking of ~ 60 nm Ag NPs in the mouse macrophage cell line J774A.1.⁴² Multispectral imaging (see Section 4.2.2) was applied to monitor the plasmon resonance wavelength of the uptaken NPs in hundreds of randomly chosen cells. These studies revealed an average red-shift of the plasmon resonance as a function of time and NP concentration (Fig. 12a), indicating that NP internalization is associated with NP clustering within the cells. Optical imaging of the NP association levels on the single cell level showed, however, dramatic cell-to-cell fluctuations in the spatial clustering of the NPs within the cells.⁴² Even after an incubation of the macrophages with increased Ag NP concentrations for 8 h, not all of the cells exhibited a strong intracellular NP association. Instead, a sub-population of cells still contained exclusively individual NPs or small agglomerates that demonstrated vividly blue color. This is illustrated in Fig. 12b, which shows darkfield scattering images of J774A.1 macrophages after exposure to Ag NPs at an effective concentration of $4.5 \mu\text{g mL}^{-1}$ and $8.7 \mu\text{g mL}^{-1}$ for 5 min and subsequent incubation without NPs for 1 h or 8 h, respectively.

To elucidate the mechanisms underlying these striking cellular differences, the impact of a panel of pharmacological inhibitors on the intracellular NP association was investigated by Wang *et al.*⁴² These studies revealed the existence of two

coexisting uptake mechanisms: actin- and clathrin-dependent endocytosis. The clathrin-dependent endocytosis results primarily in an enrichment of non-agglomerated NPs with a strong spectral response in the blue within the cells, while actin-dependent endocytosis is responsible for the formation of compact NP clusters with red-shifted spectral resonances. Wang *et al.* applied immunofluorescence microscopy to correlate the observed NP association levels with macrophage maturation markers F4/80 (higher concentration on mature macrophages) and CD14 (characteristic of monocytes). These studies revealed that F4/80 is preferentially expressed on cells that show NP association while CD14 is associated with cells containing predominantly monomeric NPs (Fig. 12c). Overall, the performed PCM studies – in combination

with SEM cell surface characterization – led to the formulation of the following model.⁴² In one sub-population (monocyte-like macrophages) individual Ag NPs and small NP clusters are directly taken up *via* a clathrin-dependent but actin-independent pathway. A second sub-population (mature macrophages) accumulates NPs first into larger clusters on the cell surface. Similar to conventional phagocytosis the surface-formed NP clusters are finally engulfed in an actin-dependent step.

6. Perspective

The superb photophysical properties of noble metal NPs and the methods reviewed in this Tutorial for monitoring truly nanoscale separations between them *via* optical means make noble metal NPs interesting tools for a broad range of applications in sensing and imaging and also in other materials related fields. The PCM applications demonstrated so far have focused primarily on plasmon ruler tracking and the monitoring of the large-scale association (clustering) of specific cell surface receptors. With the improvement of the NP labels and the development of more homogeneous, smaller, and monovalent NP labels, PCM will be applicable to characterize the spatial distribution of an even broader range of targets beyond the temporal and spatial barriers of FRET. We also envision that PCM based tools will be particularly useful in providing insights into the intricate interactions between nanoscale materials and cellular systems. Many important questions at the nano-bio interface, most importantly, how nanoscale objects can be used to influence cellular processes, remain to be characterized.⁴⁸ Given the wealth of information accessible through PCM tracking of metallic NPs, the technique seems poised to contribute significantly to this important area. Mechanistic information derived from PCM-based imaging approaches will help to mitigate or entirely avoid potential toxic effects associated with nanomaterials and could eventually lead to entire new strategies for controlling cellular activities through nanomaterials.

Acknowledgements

We acknowledge the inspiration from many researchers in the area of bioplasmonics whose work we could not cite due to length limitations. We thank the members of the Reinhard Laboratory who have contributed to this work, in particular Hongyun Wang, Guoxin Rong, Jing Wang, Lynell Skewis, Amin Feizpour, Tianhong Chen, Yan Hong and Xinwei Yu. This work was financially supported by the National Institutes of Health through grant 5R01CA138509 and the National Science Foundation through grants 0953121 and 1159552 to BMR. L.W. acknowledges a National Cancer Institute Cancer Nanotechnology Training Center (NCI-CNTC) Graduate Student Traineeship and financial support through NIH R25 CA153955.

References

- 1 R. E. Thompson, D. R. Larson and W. W. Webb, *Biophys. J.*, 2002, **82**, 2775–2783.

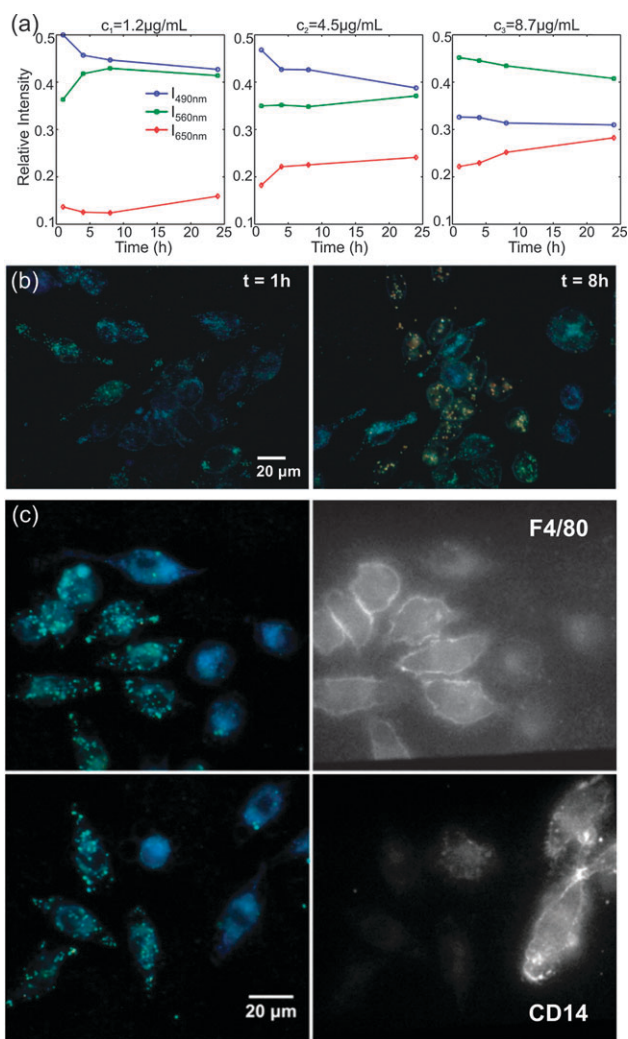


Fig. 12 (a) Scattering intensities of silver NPs after uptake by J774A.1 macrophages as a function of time on three wavelength channels (490 nm (blue), 560 nm (green), and 650 nm (red)) for three different NP concentrations: $1.2 \mu\text{g mL}^{-1}$ (left), $4.5 \mu\text{g mL}^{-1}$ (middle), and $8.7 \mu\text{g mL}^{-1}$ (right). (b) Darkfield images of macrophages exposed to $4.5 \mu\text{g mL}^{-1}$ Ag NPs after 1 h (left) and $8.7 \mu\text{g mL}^{-1}$ Ag NPs after 8 h (right). (c) Correlated darkfield image of NP containing macrophages (left) and fluorescence image (right) after staining with F4/80 (top) or CD14 (bottom) maturity markers. Reproduced with permission from Wang *et al.*, *ACS Nano*, 2012, **6**, 7122. Copyright 2012 American Chemical Society.

- 1 2 in *Molecular Imaging: FRET Microscopy and Spectroscopy*, ed. A. Periasamy and R. N. Day, Oxford University Press, New York, USA, 2005.
- 3 S. W. Hell, *Science*, 2007, **316**, 1153–1158.
- 5 4 S. Yang, M. A. Raymond-Stintz, W. Ying, J. Zhang, D. S. Lidke, S. L. Steinberg, L. Williams, J. M. Oliver and B. S. Wilson, *J. Cell Sci.*, 2007, **120**, 2763–2773.
- 5 S. A. Maier, *Plasmonics: Fundamentals and Applications*, Springer, New York, USA, 2007.
- 10 6 F. Marquier and J.-J. Greffet, in *Optical Antennas*, ed. M. Agio and A. Alu, Cambridge University Press, Cambridge, UK, 2013.
- 7 J. Yguerabide and E. E. Yguerabide, *Anal. Biochem.*, 1998, **262**, 137–156.
- 8 S. A. Maier, M. L. Brongersma, P. G. Kik and H. A. Atwater, *Phys. Rev. B: Condens. Matter Mater. Phys.*, 2002, **65**, 193408.
- 15 9 P. Nordlander, C. Oubre, E. Prodan, K. Li and M. I. Stockman, *Nano Lett.*, 2004, **4**, 899–903.
- 10 B. Rolly, B. Stout and N. Bonod, *Phys. Rev. B: Condens. Matter Mater. Phys.*, 2011, **84**, 125420.
- 20 11 W. Rechberger, A. Hohenau, A. Leitner, J. R. Krenn, B. Lamprecht and F. R. Aussenegg, *Opt. Commun.*, 2002, **220**, 137–141.
- 12 P. K. Jain and M. A. El-Sayed, *Nano Lett.*, 2008, **8**, 4347–4352.
- 13 M. J. Crow, K. Seekell, J. H. Ostrander and A. Wax, *ACS Nano*, 2011, **5**, 8532–8540.
- 25 14 K. H. Su, Q. H. Wei, X. Zhang, J. J. Mock, D. R. Smith and S. Schultz, *Nano Lett.*, 2003, **3**, 1087–1090.
- 15 C. Sönnichsen, B. M. Reinhard, J. Liphardt and A. P. Alivisatos, *Nat. Biotechnol.*, 2005, **23**, 741–745.
- 30 16 B. M. Reinhard, M. Siu, H. Agarwal, A. P. Alivisatos and J. Liphardt, *Nano Lett.*, 2005, **5**, 2246–2252.
- 17 J. I. L. Chen, Y. Chen and D. S. Ginger, *J. Am. Chem. Soc.*, 2010, **132**, 9600–9601.
- 18 L. Yang, H. Wang, B. Yan and B. M. Reinhard, *J. Phys. Chem. C*, 2010, **114**, 4901–4908.
- 35 19 E. R. Encina and E. A. Coronado, *J. Phys. Chem. C*, 2010, **114**, 3918–3923.
- 20 B. M. Reinhard, S. Sheikholeslami, A. Mastroianni, A. P. Alivisatos and J. Liphardt, *Proc. Natl. Acad. Sci. U. S. A.*, 2007, **104**, 2667–2672.
- 40 21 L. R. Skewis and B. M. Reinhard, *Nano Lett.*, 2008, **8**, 214–220.
- 22 H. Wang and B. M. Reinhard, *J. Phys. Chem. C*, 2009, **113**, 11215–11222.
- 45 23 Y. Jun, S. Sheikholeslami, D. R. Hostetter, C. Tajon, C. S. Craik and A. P. Alivisatos, *Proc. Natl. Acad. Sci. U. S. A.*, 2010, **106**, 17735–17740.
- 24 L. Lermusiaux, A. Sereda, B. Portier, E. Larquet and S. Bidault, *ACS Nano*, 2012, **6**, 10992–10998.
- 50 25 P. K. Jain, W. Huang and M. A. El-Sayed, *Nano Lett.*, 2007, **7**, 2080–2088.
- 26 L. Gunnarsson, T. Rindzevicius, J. Prikulis, B. Kasemo, M. Käll, S. Zou and G. C. Schatz, *J. Phys. Chem. B*, 2005, **109**, 1079–1087.
- 27 B. N. Khlebtsov, A. G. Melnikov, V. P. Zharov and N. G. Khlebtsov, *Nanotechnology*, 2006, **17**, 1437–1445.
- 28 G. Sun and J. B. Khurgin, *Appl. Phys. Lett.*, 2010, **97**, 263110.
- 29 J. Zuloaga, E. Prodan and P. Nordlander, *Nano Lett.*, 2009, **9**, 887–891.
- 30 F. J. G. de Abajo, *J. Phys. Chem. C*, 2008, **112**, 17983–17987.
- 31 T. Chen, M. Pourmand, A. Feizpour, B. Cushman and B. M. Reinhard, *J. Phys. Chem. Lett.*, 2013, **4**, 2147–2152.
- 32 J. A. Scholl, A. García-Etxarri, A. Leen Koh and J. A. Dionne, *Nano Lett.*, 2013, **13**, 564–569.
- 33 B. Yan, S. V. Boriskina and B. M. Reinhard, *J. Phys. Chem. C*, 2011, **115**, 24437–24453.
- 15 34 N. J. Halas, S. Lal, W. Chang, S. Link and P. Nordlander, *Chem. Rev.*, 2011, **111**, 3913–3961.
- 35 G. Rong, H. Wang, L. R. Skewis and B. M. Reinhard, *Nano Lett.*, 2008, **8**, 3386–3393.
- 20 36 J. Wang, X. Yu, S. V. Boriskina and B. M. Reinhard, *Nano Lett.*, 2012, **12**, 3231–3237.
- 37 X. Yu, J. Wang, A. Feizpour and B. M. Reinhard, *Anal. Chem.*, 2013, **85**, 1290–1294.
- 38 K. E. Sapsford, W. R. Algar, K. B. Gemmill, B. J. Casey, E. Oh, M. H. Stewart and I. L. Medintz, *Chem. Rev.*, 2013, **113**, 1904–2074.
- 25 39 J. Wang, S. V. Boriskina, H. Wang and B. M. Reinhard, *ACS Nano*, 2011, **5**, 6619–6628.
- 40 G. Rong and B. M. Reinhard, *PLoS One*, 2012, **7**, e34175.
- 30 41 H. Wang, G. Rong, B. Yan, L. Yang and B. M. Reinhard, *Nano Lett.*, 2011, **11**, 498–504.
- 42 H. Wang, L. Wu and B. M. Reinhard, *ACS Nano*, 2012, **6**, 7122–7132.
- 43 Q. Wei, E. McLeod, H. Qi, Z. Wan, R. Sun and A. Ozcan, *Sci. Rep.*, 2013, **3**, 1699.
- 35 44 C. Sönnichsen and A. P. Alivisatos, *Nano Lett.*, 2005, **5**, 301–304.
- 45 G. Rong, H. Wang and B. M. Reinhard, *Nano Lett.*, 2010, **10**, 230–238.
- 46 J. Aaron, K. Travis, N. Harrison and K. Sokolov, *Nano Lett.*, 2009, **9**, 3612–3618.
- 47 W. Qian, X. Huang, B. Kang and M. A. El-Sayed, *J. Biomed. Opt.*, 2010, **15**, 046025.
- 48 L. Wu, X. Yu, A. Feizpour and B. M. Reinhard, *Biomater. Sci.*, 2013, DOI: 10.1039/C3BM60142K, in press.
- 45 49 N. Ariotti, H. Liang, Y. Xu, Y. Zhang, Y. Yonekubo, K. Inder, G. Du, R. G. Parton, J. F. Hancock and S. J. Plowman, *Mol. Cell. Biol.*, 2010, **30**, 3795–3804.
- 50 50 A. Kusumi, C. Nakada, K. Ritchie, K. Murase, K. Suzuki, H. Murakoshi, R. S. Kasai, J. Kondo and T. Fujiwara, *Annu. Rev. Biophys. Biomol. Struct.*, 2005, **34**, 351–378.