

# Analyst

Accepted Manuscript



This is an *Accepted Manuscript*, which has been through the Royal Society of Chemistry peer review process and has been accepted for publication.

*Accepted Manuscripts* are published online shortly after acceptance, before technical editing, formatting and proof reading. Using this free service, authors can make their results available to the community, in citable form, before we publish the edited article. We will replace this *Accepted Manuscript* with the edited and formatted *Advance Article* as soon as it is available.

You can find more information about *Accepted Manuscripts* in the [Information for Authors](#).

Please note that technical editing may introduce minor changes to the text and/or graphics, which may alter content. The journal's standard [Terms & Conditions](#) and the [Ethical guidelines](#) still apply. In no event shall the Royal Society of Chemistry be held responsible for any errors or omissions in this *Accepted Manuscript* or any consequences arising from the use of any information it contains.

## COMMUNICATION

# Diagnosing malaria infected cells at the single cell level using focal plane array Fourier transform infrared imaging spectroscopy

Cite this: DOI: 10.1039/x0xx00000x

Received 00th January 2014,  
Accepted 00th January 2012

DOI: 10.1039/x0xx00000x

www.rsc.org/

Bayden R. Wood<sup>1\*</sup>, Keith. R. Bambery<sup>1,2</sup>, Matthew W. A. Dixon<sup>3</sup>, Leann Tilley<sup>3</sup>,  
Michael J. Nasse<sup>4</sup>, Eric Mattson<sup>5</sup> and Carol J. Hirschmugl<sup>5\*</sup>

**New methods are needed to rapidly identify malaria parasites in blood smears. The coupling of a Focal Plane Array (FPA) infrared microscope system to a synchrotron light source at IRENI enables rapid molecular imaging at high spatial resolution. The technique, in combination with hyper-spectral processing, enables imaging and diagnosis of early stage malaria parasites at the single cell level in a blood smear. The method relies on the detection of distinct lipid signatures associated with the different stages of the malaria parasite and utilises resonant Mie extended multiplicative scatter correction to pre-process the spectra followed by full bandwidth image deconvolution to resolve the single cells. This work demonstrates the potential of focal plane technology to diagnose single cells in a blood smear. Brighter laboratory based infrared sources, optical refinements and higher sensitive detectors will soon see the emergence of focal plane array imaging in the clinical environment.**

The malaria parasite *Plasmodium falciparum* causes one of the most deadly diseases of humans, with a mortality rate approaching 1.2 million per annum.<sup>1</sup> To reduce mortality and prevent overuse of antimalarial drugs early diagnosis followed by the immediate treatment of infections is critical.<sup>2</sup> Technologies to diagnose malaria must have high sensitivity and be cost effective for the developing world. Moreover, they need to be able to detect the immature asexual stage of the parasite (ring stage), which are the only stages that are present in the peripheral circulation in new infections and the mature sexual stage (gametocytes), which appear later are the only stage capable of transmission to mosquitoes. Optical diagnosis is still the method of choice for thick blood films because it is inexpensive and has good sensitivity (5-10 parasites/ $\mu$ l blood).<sup>3-5,6</sup> Unfortunately it is labour-intensive and is increasingly burdensome as malaria rates decline due to treatment, with most smears examined being negative. Rapid Diagnostic Tests (RDTs), which are based on capture of parasite antigens by monoclonal antibodies incorporated into a test strip, are easy to apply but are unable to quantify parasitemia.<sup>6</sup> Other techniques include gene amplification

techniques such as polymerase chain reaction (PCR).<sup>7, 8</sup> PCR is arguably the most sensitive and specific method, but is expensive, sophisticated and time consuming. Serological detection tests using antibodies such as immunofluorescence (IFA)<sup>9</sup> and enzyme-linked immunosorbent assay (ELISA) are also highly sensitive but are difficult to implement.<sup>9, 10</sup> Given the distinct morphological stages of the parasite and dramatic chemical changes between uninfected and infected cells, a spectroscopic method in combination with a morphological approach would seem a logical alternative.

Fourier Transform Infrared (FTIR) spectroscopy detects molecular vibrations from the absorption of light in the 4000-400  $\text{cm}^{-1}$  (2.5-25  $\mu\text{m}$ ) range. The FTIR spectrum of *P. falciparum*-infected red blood cell shows bands mainly associated with protein, lipid, nucleic acids and haemozoin (malaria pigment).<sup>11</sup> Other optical spectroscopic techniques including Raman microscopy<sup>12-16</sup> and magneto-based technologies<sup>5, 17, 18</sup> have also been applied to diagnose malaria. Unlike FTIR spectroscopy, these techniques rely on detecting the presence of haemozoin, which only appears in significant amounts in late stage ring forms, gametocytes, trophozoites and schizonts and not the early stage rings especially those less than 10 hours old, which are often found in peripheral blood. Recently we demonstrated the potential of Attenuated Total Reflection (ATR) spectroscopy to diagnose malaria.<sup>19</sup> While the ATR technique can detect very low parasitemia levels it does have the capability to make the diagnosis at the single cell level. Here we show that FPA technology coupled with sophisticated data pre-treatment can be applied to spatially resolve images of malaria infected red blood cells in a blood smear. Moreover, we demonstrate that the averaged spectrum from each single cell can be used to unequivocally to diagnose the stage of the parasite in a highly reproducible manner from independent trials.

## Materials and Methods

### 1. Cell culture

*Plasmodium falciparum* was cultured as previously described<sup>21</sup>. Briefly, parasite infected RBCs were cultured in O+ RBCs (Australian Red Cross blood service), in RPMI-GlutaMAX<sup>(TM)</sup>-HEPES (Invitrogen) supplemented with 5%v/v human serum (Australian Red Cross blood service), 0.25%w/v AlbuMAX II

(Invitrogen), 0.58 mg/L Gentamycin (Invitrogen) and 10 mM Glucose. Parasite infected RBCs were maintained at 37°C in a low oxygen environment (5% CO<sub>2</sub>, 1% O<sub>2</sub> in Nitrogen). Ring stage parasites (0-12 hrs. post invasion) were prepared from culture by sorbitol synchronisations<sup>22</sup>. Purified and harvested parasite infected RBC's were allowed to recover under standard culture conditions prior to sample preparation. Infected red blood cells (RBCs) and uninfected RBCs (controls) were fixed in solution using 2% paraformaldehyde, 0.0075% glutaraldehyde, and 0.1 M cacodylate buffer for 1 h before being washed twice with Milli-Q water and placed on individual 12 mm diameter × 0.5 mm thick CaF<sub>2</sub> IR grade polished windows. Excess water was removed, and the windows were allowed to dry. The experiment was repeated two times from two separate visits to IRENI. In all cases the cells were fixed in glutaraldehyde and transported from Australia to the USA. The data was analysed using Principal Component Analysis (PCA) in the spectral range 3100-2800 cm<sup>-1</sup> using normalised second derivatives. Classification of the cell types was based on morphological assessment from highly enriched ring, trophozoite and schizont samples compared to the uninfected cells. The gametocyte data was excluded from this model as we only had data from one trial for this stage.

## 2. FTIR data collection

Synchrotron FTIR (sFTIR) image data were recorded in transmission mode at the IRENI beamline (SRC, University of Wisconsin-Madison). sFTIR images were acquired using a 74 × objective (Ealing Inc., Rocklin, CA, USA), with a pixel size of 0.54 × 0.54 mm<sup>2</sup> at 4000 cm<sup>-1</sup> on the Focal Plane Array (FPA). Spectra were recorded at 6 cm<sup>-1</sup> with a zero-filling factor of 2. Second derivatives were calculated using a Savitsky-Golay algorithm convolved to a 9 smoothing point smoothing function. 128 scans were co-added in order to obtain good signal to noise. Each tile was selected to be 64 × 64 pixels; mosaic images are comprised of 2 × 2, to 3 × 2 tiles.

## 3. Data pre-processing

### 3.1 Mie scatter correction

Image data were resonance Mie scatter corrected using the RMie-EMSC algorithm.<sup>20, 21</sup> The FTIR image data was passed as input to the RMie-EMSC algorithm by a MATLAB® script written by us. This routine preserved the *x,y* spatial coordinates for each spectrum for later image reconstruction and passed suitable job lots of spectra to the MASSIVE high performance computing facility (www.massive.org.au). The RMie-EMSC algorithm options were set such that the spectral resolution was left unchanged and correction was applied for a modelled range of scattering particles radii from 3 to 8 μm. Lower and upper ranges for average refractive indices were 1.1 and 1.5 respectively and from the above scattering parameters equidistant values were used to construct 1000 element Mie scattering curve matrices which were compressed to 6 orthogonal principal components. A Mie scatter corrected uninfected cells average spectrum was used as the starting reference spectrum for correction of the image spectra. All RMie-EMSC corrected images and spectra presented in this manuscript were obtained by iterating the algorithm 5 times.


### 3.2 Deconvolution

Hyperspectral deconvolution was performed using a custom-written two-dimensional IR deconvolution algorithm applied to each wavelength in the recorded spectra.<sup>22</sup> The process involves deconvolution of experimentally-determined, wavelength-dependent

point spread functions (PSFs) from each image in three-dimensional IR data sets. The PSFs, determined from IR transmission measurements, are converted to absorbance by taking the natural logarithm of the transmission. Next, the PSFs are deconvoluted from IR absorbance images by using a Fourier Filtering approach and then truncated at the high spatial frequencies using a Hanning apodisation kernel. Finally, an inverse FT is applied to recover deconvoluted images. Deconvoluted images from each mid-IR wavelength so obtained are reassembled in a hyperspectral cube to reconstruct IR images and spectra.

## Results and Discussion

Figure 1 shows averaged second derivative FTIR spectra (20 spectra for each stage and 3 central pixels per cell) extracted from FPA images recorded from fixed *P. falciparum*-infected cells at different stages of the parasite's asexual (ring and trophozoite stages) and sexual (gametocyte) intraerythrocytic development acquired at IRENI in the 1800-950 cm<sup>-1</sup> (Figure 1A) and the 3050-2750 cm<sup>-1</sup> (Figure 1B) ranges.

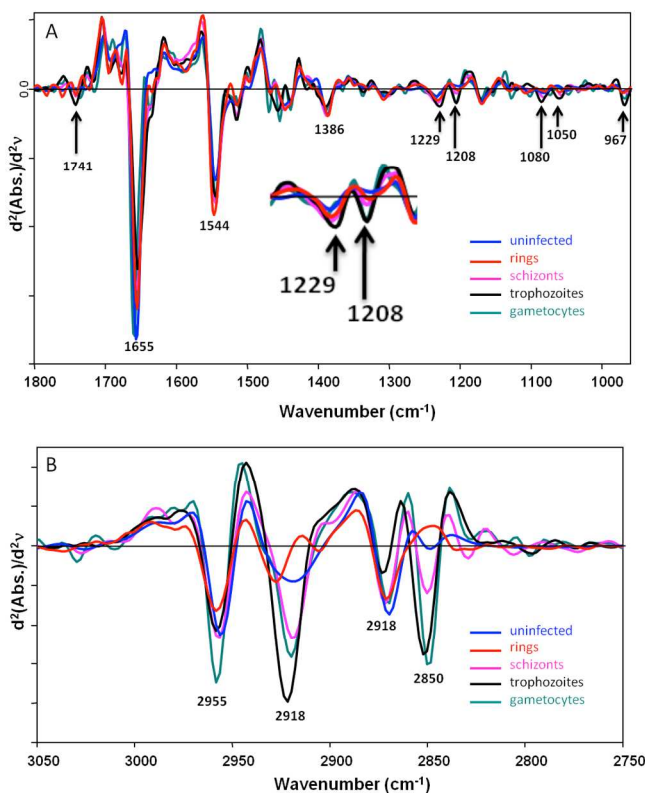

**Fig. 1.** A. Averaged spectra extracted from single uninfected red blood cells (blue) and single *P. falciparum*-infected red blood cells at different stages in the parasite's development, rings (red), schizonts (pink), trophozoites (black) and gametocytes (aqua green). The spectra were extracted from the IRENI FPA images cut to 1800-950 cm<sup>-1</sup> and processed using a second derivative with 9 smoothing points. B. An expanded view of the CH stretching region 3050-2750 cm<sup>-1</sup>.

The spectra are rich in detail and show clear differences between each of the parasitic stages. Ring forms and, in some patients, transmissible gametocytes, are found in peripheral blood. The gametocytes, like the later stage trophozoites, show high levels of

1 haemozoin as evidenced by a small but pronounced band at 1208  
 2  $\text{cm}^{-1}$  from the C-O stretching vibration of the propionate functional  
 3 group.<sup>23</sup> The gametocyte haemozoin band at 1208  $\text{cm}^{-1}$  is totally  
 4 overlapped by the trophozoite band indicating the gametocytes have  
 5 significant amounts of haemozoin. This band is not observed in the  
 6 uninfected cells and is barely discernable in the ring stage consistent  
 7 with the extremely low levels of haemozoin found in rings. The  
 8 trophozoite spectra also show evidence of high concentrations of  
 9 nucleic acids compared to the other stages including a sharp band at  
 10 1080  $\text{cm}^{-1}$  assigned to the symmetric phosphodiester vibration and  
 11 another band at 1229  $\text{cm}^{-1}$  assigned to the asymmetric  
 12 phosphodiester vibration. The band at 967  $\text{cm}^{-1}$  is assigned to a C-C  
 13 stretching vibration from the DNA backbone and supports the other  
 14 DNA assignments. Both the gametocytes and trophozoites also show  
 15 a strong ester carbonyl band at 1741  $\text{cm}^{-1}$  indicating a higher  
 16 concentration of lipids compared to the other stages. The amide I  
 17 mode at 1655  $\text{cm}^{-1}$  appears most intense in the uninfected cells,  
 18 which is consistent with the higher haemoglobin content in these  
 19 cells especially when compared to the trophozoites where the  
 20 majority of haemoglobin has been catabolised and converted to  
 21 haemozoin. The gametocytes also have a strong amide I mode  
 22 indicating a high protein content in these cells. However, the amide  
 23 II mode at 1544  $\text{cm}^{-1}$  is weaker for the uninfected cells compared to  
 24 the rings and other infected cells. This is likely the result of light  
 25 dispersion and scattering, which results in a reduced amide I/amide  
 26 II ratio and is often seen in FTIR spectra recorded at the edges of  
 27 cells and tissues. The band at 1386  $\text{cm}^{-1}$  is tentatively assigned to the  
 28 amide III mode, which follows a similar pattern to the amide I mode  
 29 where the trophozoites show a low protein concentration compared  
 30 to uninfected cells and the other stages. The discrimination in the CH  
 31 stretching region (Figure 1B) is even more dramatic due to strong  
 32 and distinctive lipid contributions from the parasite. While single  
 33 point measurements with a synchrotron source can be used to  
 34 determine differences between functional red blood cells at early  
 35 stages of infection the technique is not conducive for rapid  
 36 diagnosis.

37 FPA infrared detectors were originally developed by defence as  
 38 infrared seekers in antitank guided missiles.<sup>24</sup> These detectors were  
 39 declassified approximately 15 years ago but FPAs with fast  
 40 electronics and robust epitaxial fabrication are quite recent (~5  
 41 years).<sup>25-27</sup> A  $64 \times 64$  pixel FPA detector is capable of recording  
 42 4096 spectra in 20 seconds at 8  $\text{cm}^{-1}$  and 32 scans. However, the  
 43 image processing can take a further 5 minutes using a standard CPU  
 44 and Unsupervised Hierarchical Cluster Analysis in Cytospec<sup>TM</sup>. Still  
 45 this is rapid compared to RDTs, which take 10-15 minutes to achieve  
 46 a result. Moreover, with a motorised microscope stage, mosaic  
 47 images can be collected for analyzing large fields of cells. At the  
 48 new IRENI (IR ENvironmental Imaging) facility, Synchrotron  
 49 Radiation Center (SRC) Madison, WI (USA), 12 synchrotron beams  
 50 illuminate an FPA detector, thereby multiplexing the advantages of  
 51 the parallel pixel detection of a multi-element FPA detector with the  
 52 large-area illumination from the high brightness, stable, broadband  
 53 synchrotron source.<sup>27</sup> IRENI with  $74 \times$  magnification provides an  
 54 effective geometric pixel size of  $0.54 \times 0.54 \mu\text{m}^2$  exceeding  
 55 conventional FTIR-FPA configurations by an order of magnitude.<sup>25</sup>  
 56 Details of the instrumental parameters and sample preparation are in  
 57 the Supplementary Information (SI), while a schematic of the  
 58 instrumental configuration is shown in an earlier publication.<sup>27</sup>


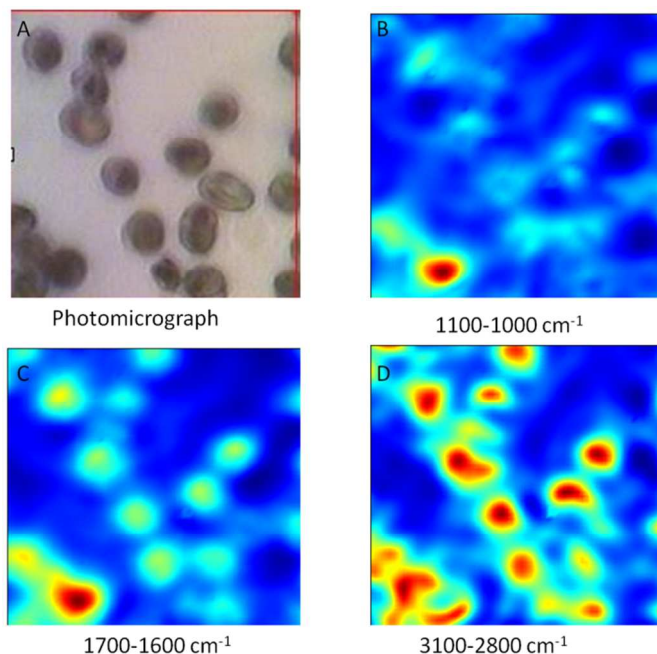


Fig. 2A Photomicrograph of a mixture of uninfected red blood cells and mainly ring stage *P. falciparum*-infected red blood cells. 2B FPA image produced by integrating the area underneath the bands in the 1100-1000  $\text{cm}^{-1}$  region for the same cells shown in 2A. 2C Same as 2B except the integration was performed in the 1700-1600  $\text{cm}^{-1}$  region. 2D Same as 2B except the integration was performed in the 3100-2800  $\text{cm}^{-1}$  region.


Figure 2A shows a photomicrograph of fixed red blood cells infected with mainly ring stage parasites on a  $\text{CaF}_2$  window while Figure 2B-2D shows FTIR mosaic images of the same cells generated by integrating the bands between 1100-1000  $\text{cm}^{-1}$  (2B), 1700-1600  $\text{cm}^{-1}$  (2C) and 3100-2800  $\text{cm}^{-1}$  (2D). There is an improvement in image quality as the wavenumber value increases because of the wavelength dependence on spatial resolution. Consequently the best images are achieved when using the 3100-2800  $\text{cm}^{-1}$  characteristic of the CH stretching region of lipids and proteins. The FTIR images of the cells appear similar in resolution to those in the visible photomicrograph even though the visible wavelengths are an order of magnitude smaller than the infrared wavelengths. The red areas in the images show areas of high lipid concentration mainly associated with mature ring stage parasites. The light blue areas are mainly associated with uninfected and immature ring stage parasites, while the dark blue is the background. A similar image showing early stage gametocytes exhibiting their distinct crescent shapes is presented in Figure 3.

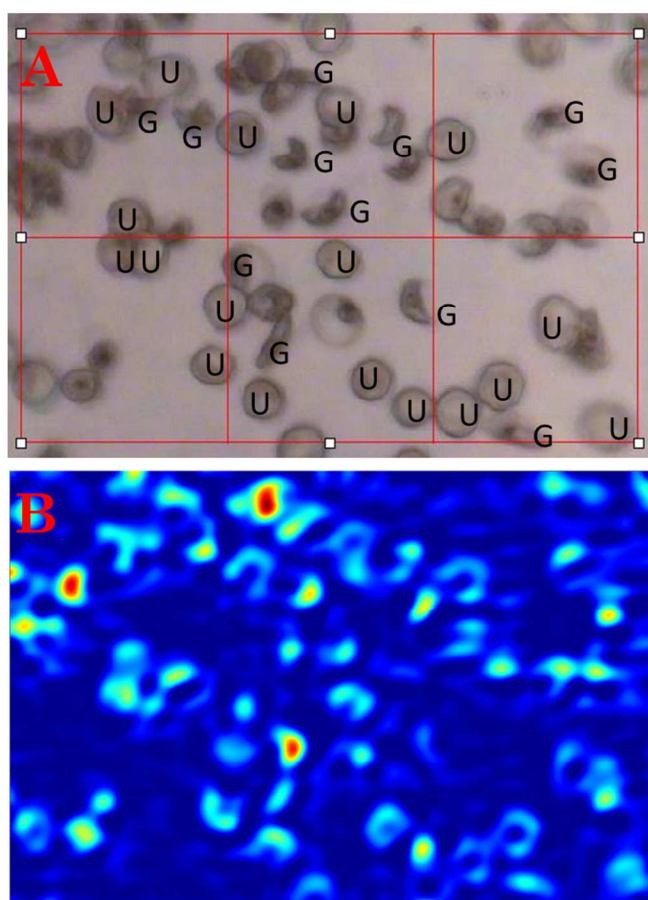

**Fig. 3.** Photomicrograph showing gametocytes (G) and uninfected cells (U). **B.** Corresponding FTIR FPA images generated by integrating the area under the CH stretching region ( $3100\text{--}2800\text{ cm}^{-1}$ ) following R-MieEMSC and full bandwidth image deconvolution.


Because of the higher spatial resolution along with the excellent discrimination of the different parasitic stages we chose the  $3100\text{--}2800\text{ cm}^{-1}$  range for the ensuing Unsupervised Hierarchical Cluster Analysis (UHCA). The spectra for the UHCA were processed using Resonance Mie Extended Multiplicative Scatter Correction (RMie-EMSC)<sup>20, 21, 28, 29</sup> followed by full bandwidth image deconvolution for each resolved wavelength (every  $4\text{ cm}^{-1}$ ) based on measured point spread functions. RMie-EMSC corrects spectra for baseline distortions resulting from Mie scattering effects of single cells due to their wavelength-comparable size<sup>21</sup> while deconvolution removes blur mainly from diffraction effects, and is scaled appropriately for each image to recover realistic spectra.<sup>22</sup> Background pixels with low absorbance were removed prior to UHCA using a routine in Cytospec<sup>TM</sup>. Figure 4A shows a photomicrograph of a monolayer blood film of mainly ring stage infected red blood cells. Figure 4B shows the corresponding chemical image after deconvolution generated by integrating CH stretching region ( $3100\text{--}2800\text{ cm}^{-1}$ ). The deconvolution improves the discrimination of the single cells in the image. This is further improved when the low absorbance pixels are removed and UHCA is performed (Figure 4C). The pink cluster is associated with high lipid content from parasite lipid inclusions and membranes. The light blue areas result mainly from CH stretching vibrations from a mixture of haemoglobin and lipid, while the dark blue cluster correlates with uninfected stacked cells. The corresponding mean second derivative spectra extracted as averages for each cluster show the pronounced lipid bands indicative of the ring form. The infected cells have very intense and shifted

asymmetric methyl and methylene stretching modes at  $2955\text{ cm}^{-1}$  and  $2917\text{ cm}^{-1}$  (pink spectrum) compared to the normal haemoglobin spectrum (blue).

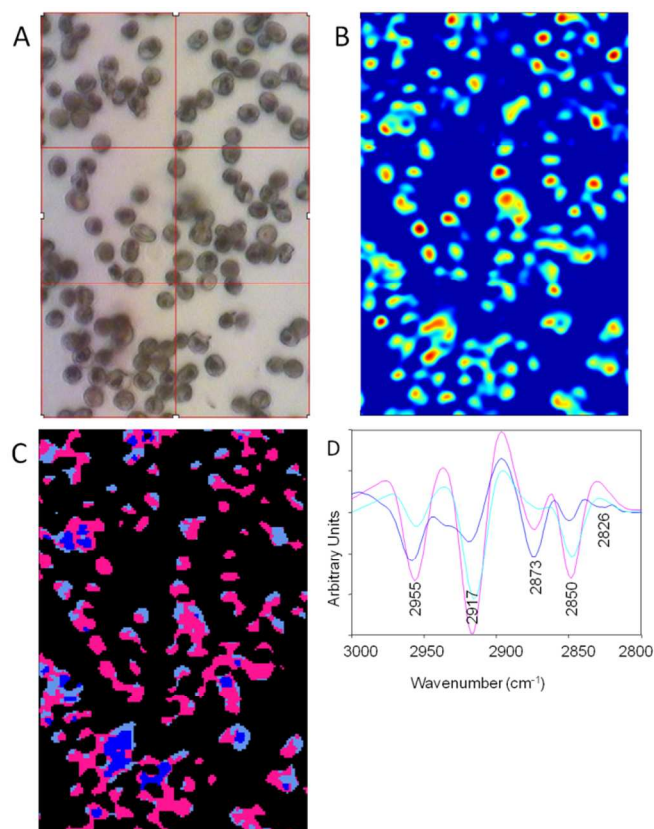

**Fig. 4A** Photomicrograph of a blood film with mainly ring stage parasites. **4B** Chemical image generated by integrating the area under the CH stretching region ( $3100\text{--}2800\text{ cm}^{-1}$ ) following deconvolution. **4C.** UHCA performed on the CH stretching region ( $3100\text{--}2800\text{ cm}^{-1}$ ) showing three clusters. The spectra were pre-processed using the broad band deconvolution followed by RMie-EMSC and then the second derivative was calculated with 9 smoothing points prior to the UHCA. The pink cluster is associated with mainly lipid inclusions from the infected cells while the light blue cluster shows mainly normal haemoglobin. The mid blue cluster is associated with stacked non-infected cells and is dominated by haemoglobin. **4D** The averaged second derivative spectra extracted from each cluster showing the dramatic variation within the cells caused by parasite lipids and normal haemoglobin. The colours match those in the UHCA image in **4C**.

To further investigate the reproducibility of the FPA diagnostic approach we combined data sets from two independent trials over a two-year period. The results of the PCA for spectra processed with and without RMie-EMSC are shown in Figure 5.

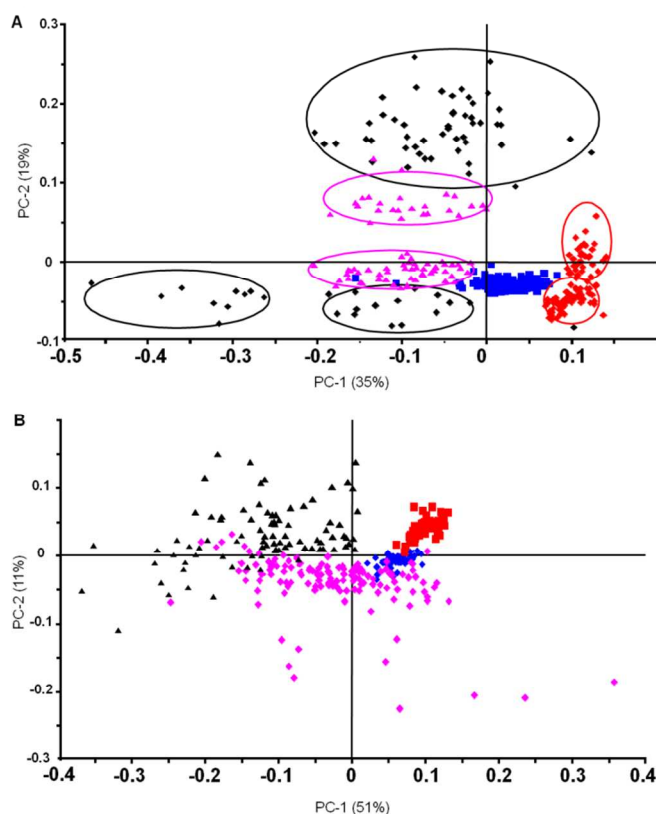

**Figure 5A** Principal Component Analysis (PCA) PC1 versus PC2 Scores plot of second derivative min/max normalised spectra (3100-2800  $\text{cm}^{-1}$ ) of uninfected (blue), rings (red), schizonts (pink) and trophozoites (black) generated from two independent visits to IRENI. The circles highlight the clusters from each visit. In the case of uninfected cells there was no separation between the spectra recorded from the two visits. The clusters of trophozoites with PC2 score values below 0 are early stage trophozoites while those with large positive PC2 scores are late stage trophozoites. **5B** PC1 versus PC2 Scores Plot of second derivative min/max normalised spectra (3100-2800  $\text{cm}^{-1}$ ) after performing RMie-EMSC of uninfected (blue), rings (red), schizonts (pink) and trophozoites (black) showing much tighter and reproducible spectra compared to **5A**.

Figure 5A shows a PC1 versus PC2 scores plot for uncorrected second derivatives after min/max normalisation, while Figure 5B shows the same data but after RMie-EMSC. The uninfected, schizont and ring stage parasites group extremely well for the two independent trials on the uncorrected spectra. The trophozoite spectra, on the other hand, were more heterogeneous and formed three distinct clusters, two of which were oppositely correlated with a third along PC2. The two clusters of trophozoite spectra with PC2 scores below 0 were early stage trophozoites from two trials, while the group with positive PC2 scores were late stage trophozoites. The opposite correlation comes from scattering effects from haemozoin crystals, which manifests in the spectra as sinusoidal modulations. Because haemozoin crystal aggregates are in the range of infrared wavelengths ( $\sim 2\text{-}3\ \mu\text{m}$ ) significant light scattering can result especially from parasites in the trophozoite and schizont stages. To address the scattering we performed RMie-EMSC on the spectra prior to taking the second derivative and min/max normalisation. The PC1 versus PC2 Scores plot (Figure 5B) show that following RMie-EMSC the spectra from both trials are grouped much more tightly yet still show excellent discrimination between all stages investigated. The combination of FPA imaging coupled with rigorous pre-processing using full bandwidth image deconvolution

and RMie-EMSC enables malaria diagnosis to be performed at the single cell level in a blood smear.

At present a synchrotron source is required to achieve the high contrast in the images presented. Recently the Bhargava group demonstrated the feasibility of recording FPA images using a  $74 \times$  objective of tissue without a synchrotron source.<sup>30</sup> With the development of tuneable quantum cascade lasers for cell and tissue analysis<sup>31</sup> and amplified frequency difference lasers generated broadband mid-infrared laser sources,<sup>32</sup> along with refinements to the optic and detector electronics, a new laboratory-based gold standard for malaria diagnosis utilising FTIR focal plane array imaging is on the horizon.

The combination of FPA technology with  $74 \times$  magnification and sophisticated algorithms to correct for Mie scattering prior to full bandwidth image deconvolution can produce high contrast chemical images of single cells in a blood smear. The application of a simple classification algorithm following pre-processing such as UHCA or PCA can then be used to diagnose and identify the early ring stages, which are diagnostic of new infections, as well as gametocytes, which are diagnostic of carriage of forms that can be transmitted to mosquitoes. Other optical/magneto-based technologies are often based on detecting haemozoin from the later stage trophozoites and schizonts, which are scarce in peripheral blood and tend to accumulate in small capillaries in organs, such as the brain. The key to this approach is using the CH stretching region first, enhancing the image quality through the spatial wavelength dependence advantage gained at  $3100\text{-}2800\ \text{cm}^{-1}$  and secondly, using the unique profile to not only diagnose the parasite but also classify its stage of development.

## Acknowledgements

We acknowledge travel funding provided by the International Synchrotron Access Program (ISAP) managed by the Australian Synchrotron and funded by the Australian Government. BRW is supported by an Australian Research Council Future Fellowship (FT120100926). We acknowledge funding from the Australian Research Council and the National Health & Medical Research Council. We also acknowledge the Multi-modal Australian Science Imaging and Visualisation Environment (MASSIVE) ([www.massive.org.au](http://www.massive.org.au)). This work has been done with support from a National Science Foundation (NSF) Major Research Instrumentation grant (DMR-0619759) and also NSF Chemistry: CHE-1112234. This research is based upon work performed at the Synchrotron Radiation Center. The SRC is funded by the University of Wisconsin-Madison and University of Wisconsin-Milwaukee and through user fees.

## Notes and references

<sup>1</sup>Centre for Biospectroscopy, School of Chemistry, Monash University, VIC 3800, Australia

<sup>2</sup>Australian Synchrotron, 800 Blackburn Rd., Clayton, VIC 3168, Australia

<sup>3</sup>Department of Biochemistry and Molecular Biology, Bio21 Institute, and ARC Centre of Excellence for Coherent X-ray Science, University of Melbourne, Melbourne, VIC 3010, Australia


<sup>4</sup>Laboratory for Applications of Synchrotron Radiation, Karlsruhe Institute of Technology, Karlsruhe, 76049, Germany

<sup>5</sup>Department of Physics, University of Wisconsin-Milwaukee, Milwaukee, 53211, Wisconsin, USA

\*To whom correspondence is addressed

## References

1. C. J. Murray, L. C. Rosenfeld, S. S. Lim, K. G. Andrews, K. J. Foreman, D. Haring, N. Fullman, M. Naghavi, R. Lozano and A. D. Lopez, *Lancet*, 2012, 379, 413-431.
2. A. M. Dondorp, F. Nosten, P. Yi, D. Das, A. P. Phyto, J. Tarning, K. M. Lwin, F. Ariey, W. Hanpithakpong, S. J. Lee, P. Ringwald, K. Silamut, M. Imwong, K. Chotivanich, P. Lim, T. Herdman, S. S. An, S. Yeung, P. Singhasivanon, N. P. Day, N. Lindegardh, D. Socheat and N. J. White, *N Engl J Med*, 2009, 361, 455-467.
3. N. Tangpukdee, C. Duangdee, P. Wilairatana and S. Krudsood, *Korean J Parasitol*, 2009, 47, 93-102.
4. S. J. Rogerson, P. Mkundika and M. K. Kanjala, *J Clin Microbiol*, 2003, 41, 1370-1374.
5. A. Butykai, A. Orban, V. Kocsis, D. Szaller, S. Bordacs, E. Tatrai-Szekeres, L. F. Kiss, A. Bota, B. G. Vertessy, T. Zelles and I. Kezsmarki, *Sci Rep*, 2013, 3, 1431.
6. B. E. Barber, T. William, M. J. Grigg, K. Piera, T. W. Yeo and N. M. Anstey, *J Clin Microbiol*, 2013, 51, 1118-1123.
7. H. A. Dawoud, H. M. Ageely and A. A. Heiba, *J Egypt Soc Parasitol*, 2008, 38, 329-338.
8. G. F. Lima, J. E. Levi, M. P. Geraldi, M. C. Sanchez, A. A. Segurado, A. D. Hristov, J. Inoue, J. Costa-Nascimento Mde and S. M. Di Santi, *Mem Inst Oswaldo Cruz*, 2011, 106, 691-700.
9. R. C. She, M. L. Rawlins, R. Mohl, S. L. Perkins, H. R. Hill and C. M. Litwin, *J Travel Med*, 2007, 14, 105-111.
10. H. Noedl, K. Yingyuen, A. Laoboonchai, M. Fukuda, J. Sirichaisinthop and R. S. Miller, *Am J Trop Med Hyg*, 2006, 75, 1205-1208.
11. G. T. Webster, K. A. de Villiers, T. J. Egan, S. Deed, L. Tilley, M. J. Tobin, K. R. Bambery, D. McNaughton and B. R. Wood, *Anal Chem*, 2009, 81, 2516-2524.
12. B. R. Wood and D. McNaughton, *Expert Review of Proteomics*, 2006, 3, 525-544.
13. B. R. Wood, S. J. Langford, B. M. Cooke, J. Lim, F. K. Glenister and D. McNaughton, *FEBS Lett.*, 2003, 554, 247-252.
14. B. R. Wood, A. Hermelink, P. Lasch, K. R. Bambery, G. T. Webster, M. A. Khiavi, B. M. Cooke, S. Deed, D. Naumann and D. McNaughton, *Analyst*, 2009, 134, 1119-1125.
15. L. Puskar, R. Tuckermann, T. Frosch, J. Popp, V. Ly, D. McNaughton and B. R. Wood, *Lab on a chip*, 2007, 7, 1125-1131.
16. A. J. Hobro, A. Konishi, C. Coban and N. I. Smith, *Analyst*, 2013, 138, 3927-3933.
17. P. F. Mens, R. J. Matelon, B. Y. Nour, D. M. Newman and H. D. Schallig, *Malar J*, 2010, 9, 207.
18. D. M. Newman, J. Heptinstall, R. J. Matelon, L. Savage, M. L. Wears, J. Beddow, M. Cox, H. D. Schallig and P. F. Mens, *Biophys J*, 2008, 95, 994-1000.
19. A. Khoshmanesh, M. W. Dixon, S. Kenny, L. Tilley, D. McNaughton and B. R. Wood, *Anal Chem*, 2014, DOI: 10.1021/ac500199x.
20. P. Bassan, A. Kohler, H. Martens, J. Lee, H. J. Byrne, P. Dumas, E. Gazi, M. Brown, N. Clarke and P. Gardner, *Analyst*, 2010, 135, 268-277.
21. P. Bassan, A. Kohler, H. Martens, J. Lee, E. Jackson, N. Lockyer, P. Dumas, M. Brown, N. Clarke and P. Gardner, *J Biophotonics*, 2010, 3, 609-620.
22. E. C. Mattson, M. J. Nasse, M. Rak, K. M. Gough and C. J. Hirschmugl, *Anal Chem*, 2012, 84, 6173-6180.
23. A. F. G. Slater, W. J. Swiggard, B. R. Orton, W. D. Flitter, D. Goldberg, A. Cerami and G. B. Henderson, *Proc. Natl. Acad. Sci. USA*, 1991, 88, 325-329.
24. A. V. R. Warriar, P. K. Basu and P. K. Chaudhry, *Defense Science Journal*, 1995, 45, 229-232.
25. C. J. Hirschmugl and K. M. Gough, *App. Spectrosc.*, 2012, 66, 475-491.
26. M. J. Nasse, B. Bellehumeur, S. Ratti, C. Olivieri, D. Buschke, S. J., K. Eliceiri, B. Ogle, C. Schmidt Patterson, M. Giordano and C. J. Hirschmugl, *Vibrational Spectroscopy*, 2012, 60, 10-15.
27. M. J. Nasse, M. J. Walsh, E. C. Mattson, R. Reininger, A. Kajdacsy-Balla, V. Macias, R. Bhargava and C. J. Hirschmugl, *Nat Methods*, 2011, 8, 413-416.
28. P. Bassan, H. J. Byrne, F. Bonnier, J. Lee, P. Dumas and P. Gardner, *Analyst*, 2009, 134, 1586-1593.
29. P. Bassan, H. J. Byrne, J. Lee, F. Bonnier, C. Clarke, P. Dumas, E. Gazi, M. D. Brown, N. W. Clarke and P. Gardner, *Analyst*, 2009, 134, 1171-1175.
30. R. K. Reddy, M. J. Walsh, M. V. Schulmerich, P. S. Carney and R. Bhargava, *Applied spectroscopy*, 2013, 67, 93-105.
31. P. Bassan, M. J. Weida, J. Rowlette and P. Gardner, *Analyst*, 2014, DOI: 10.1039/c4an00638k.
32. E. B. Brauns, *Applied spectroscopy*, 2014, 68, 1-4.

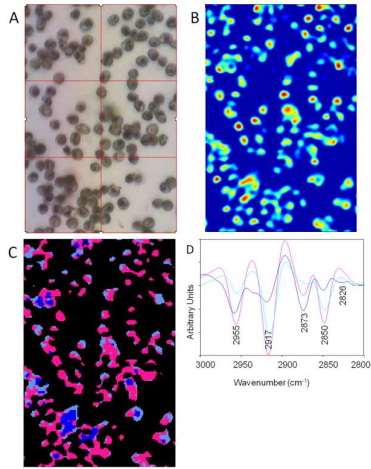

FTIR focal plane array imaging can be applied to diagnose single malaria infected cells in a thick film blood smear.

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60