

Analyst

Accepted Manuscript



This is an *Accepted Manuscript*, which has been through the Royal Society of Chemistry peer review process and has been accepted for publication.

Accepted Manuscripts are published online shortly after acceptance, before technical editing, formatting and proof reading. Using this free service, authors can make their results available to the community, in citable form, before we publish the edited article. We will replace this *Accepted Manuscript* with the edited and formatted *Advance Article* as soon as it is available.

You can find more information about *Accepted Manuscripts* in the [Information for Authors](#).

Please note that technical editing may introduce minor changes to the text and/or graphics, which may alter content. The journal's standard [Terms & Conditions](#) and the [Ethical guidelines](#) still apply. In no event shall the Royal Society of Chemistry be held responsible for any errors or omissions in this *Accepted Manuscript* or any consequences arising from the use of any information it contains.

ARTICLE

Self-cleaning properties in engineered sensors for dopamine electroanalytical detection

Cite this: DOI: 10.1039/x0xx00000x

Guido Soliveri^{†,a,b}, Valentina Pifferi^{†,a,b}, Guido Panzarasa^c, Silvia Ardizzone^{a,b}, Giuseppe Cappelletti^{a,b}, Daniela Meroni^{a,b}, Katia Sparnacci^c, and Luigi Falciola^{a,b*}

Received 00th January 2012,
Accepted 00th January 2012

DOI: 10.1039/x0xx00000x

www.rsc.org/

Fouling and passivation are the major drawbacks for a wide applicability of electroanalytical sensors based on nanomaterials, especially in biomedical and environmental fields. The production of highly engineered devices, designed ad hoc for specific applications, is the key factor in the direction of overcoming the problem and accessing to effective sensors. Here, the fine tuning of the system, composed by a highly ordered distribution of silver nanoparticles between a bottom silica and a top titania layer, confers multifunctional properties to the device for a biomedical complex challenge: the dopamine detection. The crucial importance of each component towards a robust and efficient electroanalytical system is studied. The total recovery of the electrode performance after a simple UV-A cleaning step (self-cleaning), due to the photoactive interface and the aging resistance are deeply investigated

Introduction

New types of sensing devices have been recently attracting tremendous attention because of environmental concerns and biomedical demands.¹⁻⁷ The fast development of nanotechnology has paved the way for the design of tailored systems exhibiting superior properties.⁸⁻¹²

Composite oxide/metal systems employing silver nanoparticles (Ag NPs) have gained increasing attention^{8,9,13} especially in the case of electroanalysis for traces detection, due to Ag NPs unique properties.^{8,9} Silver possesses the highest electrical conductivity and a good stability at different potentials and pH, and, more relevantly, it shows large electrocatalytic properties compared to other metals. For these reasons, it is a widely used electrode material and the advent of nanotechnology has further improved its possibilities. As a matter of fact, compared to the traditional bare noble metal electrodes, nanostructured surface morphologies can enhance the response of the sensing system. The high surface to volume ratio, proper of nano-dimensions, enormously increases the availability of interaction sites for the analyte, improving sensitivity and lowering detection limits, fundamental characteristics for trace analysis. Moreover, the small dimensions may allow to control locally the sensing process, in terms of analyte diffusion mechanism and site-

analyte recognition. The effects described above are particularly maximized in the case of well ordered structures.

A problem often encountered during the use of these nanosized, complex devices, is represented by passivation and fouling phenomena leading to a poor reusability.^{1,8}

Passivation and fouling are mainly due to electrochemically produced byproducts or interfering compounds present in the analyzed complex real matrix, chemisorbed at the electrode surface. The conventional cleaning procedures applied to bulk metal electrodes (mechanical or electrochemical etching) are inapplicable in the case of metal nanoparticles, since these systems can be irreversibly modified or the nanoparticles even removed from the electrode surface. This is a critical limitation for a commercial sensor which, apart from high sensitivity, low detection limits and high selectivity, should be also characterized by portability, online and onsite usability and especially re-usability.^{1,4} In this context, self-cleaning electrodes could represent a step beyond the current state of the art.

Self-cleaning materials mediated by UV and visible light have had a main role in both fundamental and applicative studies in the last 30 years.^{14,15} Self-cleaning coatings¹⁶, windows and cements, and also self-sterilizing medical devices and surgical rooms are, nowadays, appealing products for the market.¹⁴ Titanium dioxide (TiO₂) is the main protagonist for present and

under development products. TiO₂ was firstly investigated plentifully for its highly attractive photo-oxidative and photo-reductive power, and for its appealing band-gap (3.2 eV for anatase and 3.0 eV for rutile). Besides its semiconductor properties, the oxide shows high bio-compatibility, high refractive index and, above all, high availability and low costs.

A very recent work by Kamat *et al.*¹⁷ has reported a “*detect and destroy*” approach for SERS analyses, in which the combination of SERS experiments supported by Ag NPs, with the photocatalytic degradation of the molecule by TiO₂ is described.

On the other hand, to the authors best knowledge, the study of self-cleaning layers potentially applicable on whatever electrode surface to prevent passivation, caused either by silver oxidation or by interferences presence, has not been explored yet. Literature reports only few examples of self-cleaning electrodes for hydrogen detection,¹⁸ and for methanol electro-oxidation or glucose determination.^{19,20} These systems are based on anodized titania nanotubes supports decorated with noble metals (Pt and Pd), where the titania photoeffect is exploited to restore the activity of the device. In the Literature, neither a proper electrode design for re-usability, nor a deep study of fouling/cleaning effects on the electroanalytical parameters are investigated.

In this very promising context, we propose an innovative self-cleaning engineered device to be used as an electroanalytical sensor. The device is composed by a transparent metal-oxide composite multilayer in which Ag NPs are deposited to give a controlled and organized structure between a bottom silica and a top titania layer. Each component of the device was chosen for its relevant properties: the silica layer was essential to govern the distribution of silver nanoparticles, which were the actual sensing tool, imparting electrocatalytic properties and conductivity between the two semiconducting oxides; the top titania film was used to confer the self-cleaning properties, but also to protect Ag NPs from oxidation and deterioration.

In order to check the applicability of the designed device in a real, challenging and complex system, the electroanalytical detection of dopamine was studied.^{21,22} Dopamine is a neurotransmitter with great biomedical and analytical interest, since the molecule anomalous levels are diagnostic for the Parkinson's disease and for many neurological pathologies. In the literature, its determination has been faced by different electrodes and strategies,^{23–25} but, in almost all cases, fouling and passivation of the electrode surface affected the measurements. In particular, the chemisorption of dopamine or of its byproducts at metal and oxide interfaces makes the reusability of the electrode generally impossible.²¹ The present self-cleaning sensor is *ad hoc* designed for the detection of such critical molecules, affording a total sensitivity recovery after fouling and cleaning by a simple UV irradiation step. Moreover, aging, over-usage and environmental conditions did not introduce appreciable modifications of the initial characteristics of the electrode.

Results and discussion

Device assembly and structure

The device, described in the present work, was engineered with the aim of tuning its photocatalytic and electrochemical properties in order to obtain an electroanalytical sensor for the detection of molecules with biomedical interest. We controlled the synthesis in order to promote the self-cleaning properties and tune the electrocatalytic features by modulating the sandwich composition and Ag NPs organization, preserving the film transparency. Figure 1a shows the material architecture.

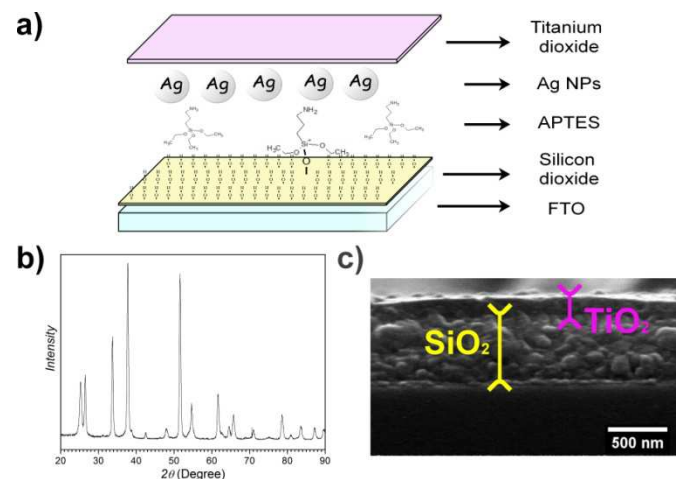


Figure 1: Device structure: a) schematic description of the architecture, b) X-ray diffraction pattern of the titania top layer and c) SEM cross section of the film.

Each layer/component was finely designed in order to control the final performance: **support**, **silica layer**, **bifunctional siloxane** ((3-Aminopropyl)triethoxysilane, APTES), **Ag NPs**, **titania**. As the **support**, a conductive glass, withstanding calcination, FTO, was selected. The subsequent presence of a **silica layer** was chosen in order to promote the dispersion of the Ag NPs. The layer of silica was obtained by dip coating the FTO surface in a non-aqueous sol, synthesized by the procedure reported by Wang *et al.*²⁶ The subsequent calcination conditions were chosen in order to decompose the organic components of the sol while maintaining the film transparency and increasing its mechanical stability and adhesion onto the support. The role played by time, temperature and atmosphere were preliminarily studied to tune the reactivity of the surface. A calcination step of one hour at 400 °C in N₂ flow was finally adopted. The calcined silica layer was further grafted by a **bifunctional siloxane** in order to promote stable attachment of Ag NPs. APTES was chosen as a coulombic binder between the SiO₂ surface and the Ag NPs. APTES ethoxy groups generally react with –OH groups at the oxide surface, exposing –NH₃⁺ groups at the interface.²⁷ The negative charged Ag NPs (Z-potential measurement, supporting information, Figure S1) strongly interact with –NH₃⁺ groups, so that the number and the arrangement of APTES molecules highly influence the concentration and disposition of Ag NPs at the surface.

The Ag NPs, synthesized by the procedure of Panzarasa,²⁸ were stabilized by PVP10 to avoid the presence of agglomerates and multilayers at the functionalized surface. The HR TEM picture (Figure 2a) shows particles of around 11 nm in diameter (10.8 ± 1.3 nm) with high crystallinity (the lattice spacing of ~ 230 pm corresponds to (111) planes of silver fcc cell) and quite sharp distribution. The aqueous particle suspension presented the typical plasmonic resonance associated with Ag NPs of dimensions lower than 30 nm (Figure 2b inset).²⁹ After dipping 15 minutes in such a suspension, the material showed the orange colour correlated with the spectrum reported in Figure 2b. The red-shift of the band derived from a change of environment, as reported by Evanoff *et al.*³⁰

Finally, the engineered sensor is covered by a TiO₂ layer with the aim to impart photoactivity and self-cleaning properties.

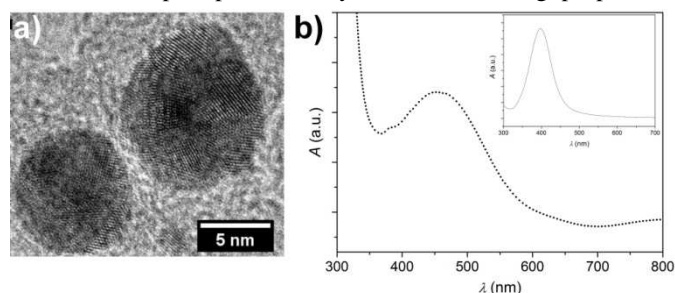


Figure 2: a) HR TEM picture of Ag NPs, showing high crystallinity and lattice spacing of about 230 pm; b) UV-Vis spectrum of Ag NPs grafted on the silica surface; inset: UV-Vis spectrum of the Ag NPs suspension.

The oxide external layer was demonstrated to confer further crucial properties to the material, such as protection for the Ag NPs from unavoidable oxidation/deactivation ensuing from the contact with the environment. The TiO₂ film was obtained by dip-coating the multilayer device in a non-aqueous sol, synthesized following a procedure previously developed by our group.³¹ Temperature and, particularly, the atmosphere of calcination were chosen in order to prevent Ag oxidation. In the absence of the protective TiO₂ layer, Ag degradation is generally observed after few days of environmental condition exposure, dramatically changing both the chemical nature and the morphology of such particles. We tested different times and conditions for the TiO₂ crystallization and growth. A fast calcination of 1 hour at 400 °C under N₂ flow allowed the organic compounds mineralization and the growth of the oxide crystallinity, without altering the film transparency (supporting information, Figure S2).

The XRD lines (Figure 1b) of the sandwich show the predominance of the anatase polymorph, with traces of brookite. The peaks of cassiterite (SnO₂), proper of the FTO support are also appreciable. The size of anatase crystallites was evaluated to be 17 nm. The cross-section SEM picture, reported in Figure 1c, reveals two distinct and homogenous layers, 550 nm and 150 nm in thickness, for SiO₂ and TiO₂, respectively. Thickness data were confirmed by FILMETRICS® analysis, comparing the experimental

reflectance spectrum with a calculated one (supporting information, Figure S3), showing reproducible values in different areas of the film. The SEM top picture (supplementary information, Figure S4) shows good homogeneity of the surface.

The role of silver in electrocatalysis both as massive electrodes and as nanoparticles has been amply discussed in the literature^{32–34} also for sensing applications,^{8,9,35} where Ag can change favourably the potential of redox reactions, also allowing interferences management.

The actual presence of Ag in the device was shown by cyclic voltammetry performed in the absence of an electroactive probe. Electrodes without Ag behaved similarly to bare FTO, showing completely capacitive voltammograms without peak formation (Figure 3a, curve 1), typical of oxide materials. In the presence of Ag (Figure 3a, curve 2 and 3), oxidation and

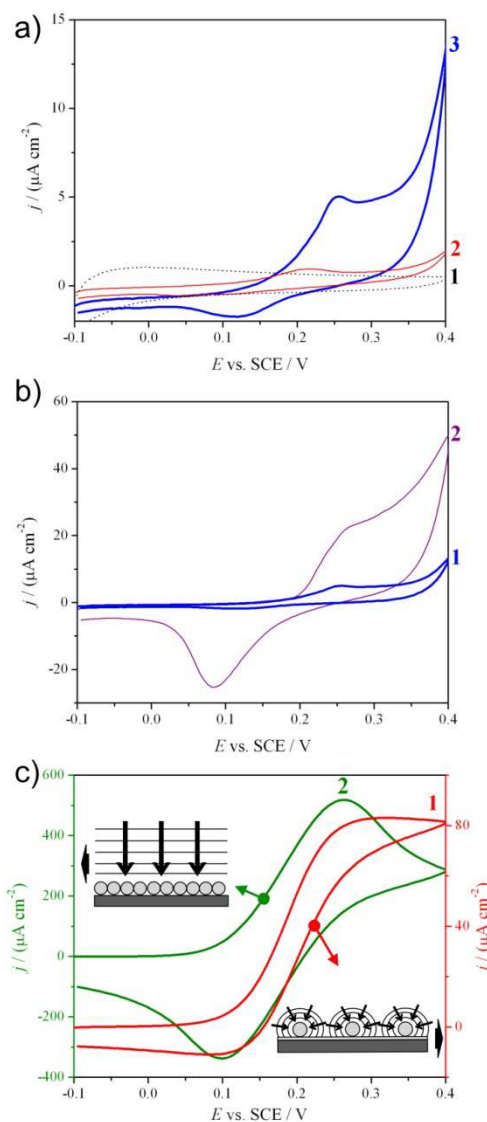


Figure 3: Cyclic voltammograms in the a,b) absence or c) presence of K₄[Fe(CN)₆] probe molecule. Study of a) the effect of titania layer (curve 1: FTO+SiO₂+TiO₂; curve 2: FTO+SiO₂+Ag; curve 3: FTO+SiO₂+Ag+TiO₂), b) the effect of silica layer (curve 1: FTO+SiO₂+Ag+TiO₂, curve 2: FTO+Ag+TiO₂), c) the distribution of Ag NPs (curve 1: FTO+SiO₂+Ag; curve 2: FTO+Ag).

1 reduction peaks around +0.25 V (SCE) and +0.1 V (SCE)
2 appeared, as generally reported^{36,37}.

3 Moreover, silver, due to its reactive nature, can be oxidized by
4 oxygen present in the air, with passivation effects. To avoid this
5 phenomenon, protective oxides are often used on metal
6 surfaces.³⁸ In our case, the titania layer provided a protective
7 action for Ag NPs. This effect can be proved by comparing the
8 final electrode (Figure 3a, curve 3) with a device prepared in
9 the same manner, but without the final TiO₂ layer (Figure 3a,
10 curve 2). In the case of titania covered silver nanoparticles,
11 higher Ag peak currents were observed, reflecting the presence
12 of more active and non-oxidized silver nanoparticles.

13 A key point to take into consideration in the use of modified
14 electrodes supporting silver for sensor applications is the
15 density, distribution and organization of nanoparticles on the
16 electrode surface.⁸ In electroanalysis, the analyte reacts on the
17 surface of the electrode, generating an increase of the measured
18 current. The resulting signal is the sum of the capacitive
19 background current and of the reaction current, which is the
20 sole related to the analyte concentration. The voltammograms
21 shape is related to the NPs size and density:^{39,40} a steady-state
22 sigmoidal step can be registered for convergent independent
23 diffusion at NPs low coverage (Figure 3c, Scheme 1), while a
24 peak is obtained in the case of planar diffusion regime at high
25 NPs coverage (Figure 3c, Scheme 2).

26 In order to obtain high sensitivity and low detection limits, high
27 faradaic and low capacitive currents have to be preferred. An
28 optimal disposition for this purpose is an ordered array of well
29 isolated nanoparticles, where the convergent mass transport
30 must be predominant.⁴⁰⁻⁴² In this case, the current response is
31 greater with respect to that of a macroelectrode. In fact, while
32 the current at a macroelectrode follows the Randles-Sevčik
33 equation (Equation 1):⁴³

$$I_{peak} = 2.69 \times 10^5 n^3/2 D^{1/2} C_{bulk} v^{1/2} A \quad (1)$$

34 (where I_{peak} is the current in amperes, n is the number of
35 electrons involved in the reaction, D is the diffusion coefficient
36 in (cm² s⁻¹), C_{bulk} is the bulk concentration of active species in
37 (mol cm⁻³), v is the potential scan rate in (V s⁻¹) and A is the
38 surface area in cm²), in the case of a nanoparticle array of the
39 same macrodimensions of the previous macroelectrode in
40 which the nanoparticles are at a distance of $10r$ (where r is the
41 radius of the nanoparticle), the limiting current at each
42 nanoparticle and the total array current are given by:^{8,9,41,44}

$$I_{lim} = 8.71 n F D C_{bulk} r \quad (2)$$

$$I_{tot} = I_{lim} [A / (10r)^2] = (8.71 n F D C_{bulk} A) / (100r) \quad (3)$$

43 In Equation 3, it is evident the current dependence from the
44 particle radius (the smaller, the better) and the independence
45 from the potential scan rate, since a convergent mechanism is
46 attained.

47 Using typical values for the parameters and a value of $r = 10$
48 nm, a current increase of seven hundred times can be obtained⁸
49 with respect to the macroelectrode.

50 It is worthwhile noticing that the above considerations are valid
51 assuming that the nanoparticles are sufficiently far apart as to
52 be diffusively independent. Too closely packed electrodes

result in the overlapping of the diffusion layers, characterized
by the loss of convergent diffusion. The nearest-neighbours
NPs minimum distance of $10r$ required for diffusional
independency, although debated,^{40,45} is assumed to be a good
indicative value.⁸

Moreover, the NPs array is characterized by a larger surface
area-to-volume ratio of the electrocatalytic material. This fact
lowers the costs of the electrodes and, increasing the active
sites, enhances the signal-to-noise ratio, particularly abating the
capacitive background currents, which are dependent to the real
active surface area.⁸

Devices based on ordered arrays are normally produced
lithographically by long, difficult and costly procedures and
only few papers rely on simple and effective techniques,⁴¹ since
simpler methodologies usually produce random or
uncontrollable distributions. The preparation method presented
in this work allows the obtainment of organized and regularly
distributed arrays of Ag NPs by a simple and low cost
procedure. The key factor is represented by the interaction sites
for silver, produced by -NH₃⁺ APTES groups, in terms of
quantity and distribution. We carefully tuned the conditions of
APTES deposition and silica calcination in order to produce
well-organized and separated sites. With the method reported
by Moon *et al.*,⁴⁶ we collected evidence that the concentration
of amino groups at the surface was almost double for bare FTO
(10 (NH₂ nm⁻²)) compared to FTO covered by silica (5 (NH₂
nm⁻²)) in the same conditions. In the latter case, a lower
quantity of silver nanoparticles was expected on the silica layer.
Figure 3b shows voltammograms registered for the two Ag NPs
electrodes, differing only for the presence or absence of the
silica layer. When Ag nanoparticles are deposited on silica
(Figure 3b, curve 1), a lower quantity of metal is present, as
demonstrated by the above considerations, and a lower peak
current is registered in comparison with Ag NPs directly
deposited on bare FTO (Figure 3b, curve 2). It is important to
say that the current registered in the presence of the non-
conductive silica layer is, anyway, really high and of the same
order of magnitude of the electrode without silica. The
contribution brought by the distribution (array) of isolated NPs
(convergent diffusion) is evident and will be of paramount
importance in the detection of analyte at trace levels, as already
explained.

The distribution of silver nanoparticles on silica was studied by
registering cyclic voltammograms, this time in the presence of a
redox probe (K₄[Fe(CN)₆]), before TiO₂ deposition (Figure 3c).
Only in the presence of a redox reaction the diffusion
mechanism and, as a consequence, the distribution of
nanoparticles can be studied. Figure 3c curve 1 shows a step-
shaped voltammogram typical of a convergent diffusion
mechanism on isolated ordered nanoparticles (scheme 1) in the
case of Ag NPs anchored on silica. On the other hand, a peak-
shaped voltammogram (Figure 3c, curve 2), reflecting semi-
infinite diffusion on non isolated particles (scheme 2), was
observed in the case of silver directly deposited on FTO.

Figure 4 shows electrochemical impedance spectroscopy (EIS) measurements in the presence of the redox probe $K_4[Fe(CN)_6]$. The analyses were performed on different electrodes at different steps of preparation and at different compositions of the sandwich. Impedance analysis measures the current response of the device to an external potential variation and allows modelling the systems by an electrical circuit. In the complex plane plots (Figure 4, Bode plots shown in supporting information, Figure S5), the semicircle shape common to all the combinations can be represented by the same equivalent circuit (Figure 4, inset), composed by the solution resistance (R_{Ω}) in series with a parallel formed by the charge transfer resistance (R_{CT}) and the double layer capacitance (CPE_{DL}). This trend of experimental data and circuits derived from modelling are typical for a redox reaction of a model probe at the electrode. From the diameter of the semicircle, we obtained the values of the charge transfer resistance (Figure 4, Table), critical to describe the electron transfer between the model probe and the electrode. As expected, these values increase enhancing the number of layers, while the introduction of Ag NPs produces a drastic decrease of resistance in otherwise identical conditions. We demonstrated the crucial presence of Ag nanoparticles in order to enhance the electrode conductivity in the architecture of our final device, since electrons of the probe reaction can more easily pass throughout the two semiconductor layers.

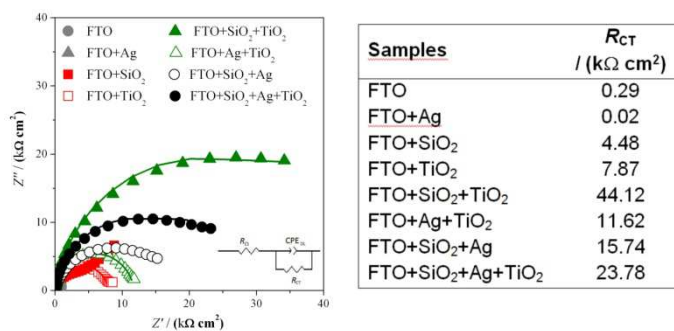


Figure 4: Complex plane plot spectra for all the electrode architectures, registered at +0.1 V (SCE) in the presence of the model probe molecule $K_4[Fe(CN)_6]$; inset: equivalent circuit used to fit data. Table: charge transfer resistance (R_{CT}) values calculated from the fitting.

Top layer photoactivity

The role played by TiO_2 more external layer in protecting Ag NPs from oxidation has already been discussed.

The self-cleaning properties of the final device can be achieved by the presence of TiO_2 on the top of the sandwich. The accurate engineering of the final layer had the aim to impart photoactivity at the interface without altering transparency, mechanical properties and the state of Ag NPs. As a matter of fact, the crystallinity growth (and the degradation of the organic components) promoted by the calcination step are crucial in order to impart photoactivity.¹⁴ Here, the careful modulation of the sol composition associated with a rapid calcination at

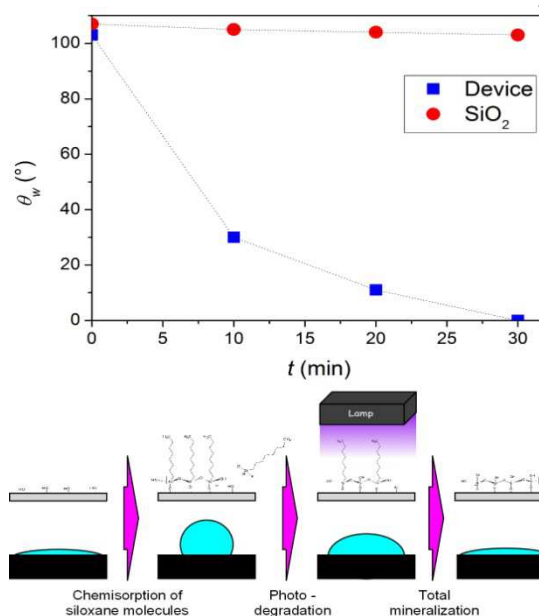


Figure 5. Kinetic of θ_w decrease of the device covered by a chemisorbed siloxane layer under UV irradiation; scheme of the siloxane chemisorption and degradation.

400 °C in an inert atmosphere not only assured high photoactivity under UV-A irradiation, but also preserved the transparency of the film. The photoactivity was proved by degradation of chemisorbed hydrophobic organic chains (SILRES 1701) monitoring the water contact angle decrease by a procedure previously reported in literature for the simulation of finger print / oily stain self-cleaning.^{47,48} The presence of silane molecules chemisorbed at the electrode surface (Figure 5, scheme), shifted the θ_w value from hydrophilic (30 - 0°) to ~ 110°. Under irradiation in the UV region, electron-hole pairs were created at the TiO_2 interface. That makes the surface reactive. Peroxide and superoxide radicals were generated,¹⁴ reacting and oxidizing the organic chains of the chemisorbed siloxane, bringing back the θ_w to the hydrophilic value.

Figure 5 shows the degradation kinetic of the siloxane chains on the device, monitored by θ_w decrease, compared to the bare silica. Whilst the water contact angle of the bare silica was almost constant upon irradiation, the device, covered by the titania layer, showed fast kinetics of contact angle decrease. That proves that the organic chains mineralization was carried out by the radicals produced by the active titania and not by simple photolytic degradation of the molecule. Eventually, we proved the high activity of the interface as a self-cleaning electrode.

Determination of dopamine

Dopamine, an important molecule of biomedical interest,^{21,22} was chosen for testing the electroanalytical performances of the optimized multilayer electrodes. After an extensive literature research and experimental investigation, differential pulse voltammetry (DPV) was chosen as the best technique for the detection of dopamine. Figure 6a shows the calibration plot, obtained in the case of the final device (FTO+SiO₂+AgNP+TiO₂, empty circles) in the 5 – 35 ppm

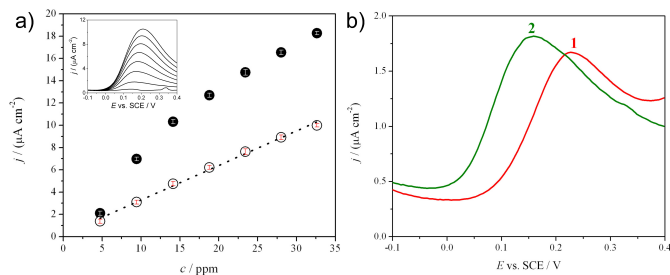


Figure 6. a) DPV calibration plots obtained for dopamine detection on two different electrode architectures (FTO+Ag+TiO₂ (●); FTO+SiO₂+Ag+TiO₂(○)); inset: differential pulse voltammograms referred to (○) data; **b)** differential pulse voltammograms, showing electrocatalytic peak displacement caused by Ag NPs (curve 1: FTO+SiO₂+TiO₂; curve 2: FTO+SiO₂+Ag+TiO₂).

dopamine concentration range, and, as inset, the corresponding differential pulse voltammograms.

Dopamine can be detected with a good sensitivity also on the device without the silica layer (FTO+Ag+TiO₂, Figure 6a, full circles; corresponding voltammograms in supporting information Figure S6), although the calibration plot obtained is not linear and a strong saturation effect is observed. This problem was overcome when the silica layer was present, obtaining a linear range. Moreover, it is worthwhile saying that, in the case of the presence of silica, the convergent diffusion on silver NPs can be reached (see paragraph 2.1), with important advantages at trace level of analyte concentration, particularly in terms of lower limits of detection. Preliminary results in this sense are validating this conclusions.

In dopamine detection, silver has the double function of both facilitating the electron transfer through the semiconductor layers, in order to provide the required conductivity (see previously reported impedance discussion, Figure 4), and of allowing metal electrocatalytic effect on the analyte. The latter is demonstrated in Figure 6b, showing a decrease of dopamine peak potential from +0.26 V (curve 1) to +0.15 V (SCE) (curve 2) in the case of presence of Ag in the sandwich. As

discussed in the introduction, chemisorption and consequent fouling of the electrode surface is a general concern in electroanalysis, particularly in the detection of organic analytes at trace levels.^{1,21} This affects the analytical sensitivity and requires strong surface polishing treatments or even the complete replacement of the electrode. In the present case, the fouling phenomenon was significant, causing an analytical sensitivity decrease (evaluated by the decrease in the calibration plot slope in Figure 7a, triangles, compared to the fresh one, circles) for consecutive analysis performed using the same electrode.

In order to “clean” the surface, removing all the byproducts and the residues of dopamine detection, after the recording of a complete calibration curve, the electrode was simply irradiated with UV-A light for one hour, exploiting the photoactivity of the external titania layer. The sensitivity was completely recovered as revealed in Figure 7 (squares), where the recovered electrode calibration plot completely overlaps the pristine electrode ones (circles).

For a better understanding of the phenomenon, in a fresh solution of electrolyte (in the absence of dopamine), we recorded cyclic voltammograms of the same electrode in different moments of the fouling-cleaning process (Figure 7b). Line 1 corresponds to the clean electrode before sensing and shows the presence of Ag NPs peak around +0.2 V, as expected; line 2 represents the voltammogram registered at the electrode, washed with water, after one dopamine calibration experiment (ten additions 10⁻² M dopamine). Line 3 was acquired on the washed electrode after two dopamine calibration analyses. The voltammograms 2 and 3 are significantly different compared to curve 1, showing a clear evidence of progressive fouling at the sandwich surface. Both voltammograms show peak shoulders (around +0.35 V), and a narrowing of the accessible potential window, probably due to the presence of adsorbed dopamine or other fouling byproducts derived by the reaction. Line 4 shows the voltammogram after one hour of UV-A irradiation and 24 h of storage in the dark. In this case, the electrode completely recovers the initial shape

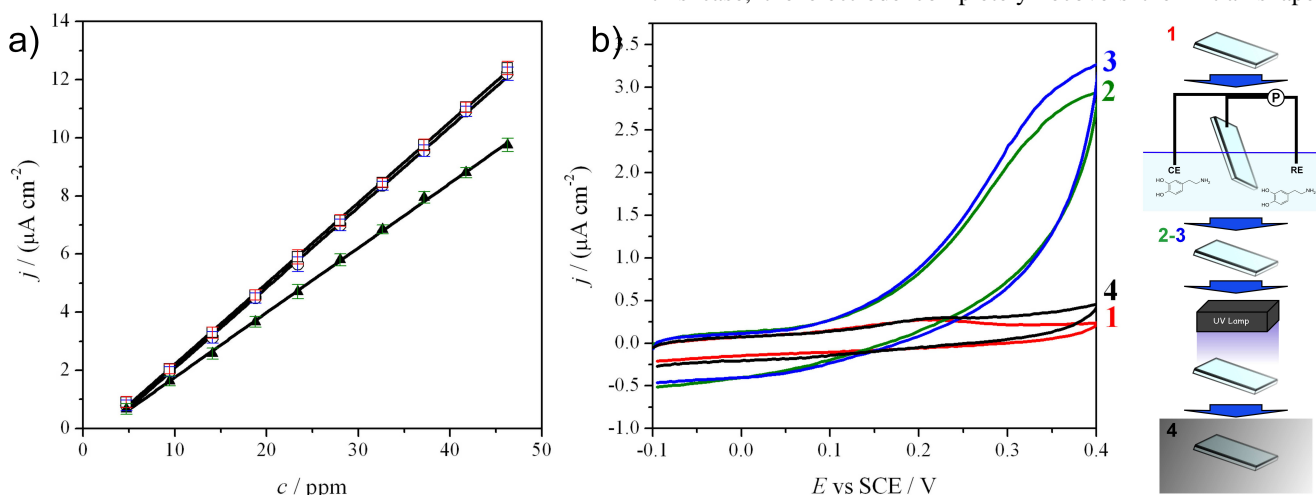


Figure 7. a) Dopamine calibration plots obtained at different analytical steps [squares (□): first calibration plot; triangles (▲): calibration plot after fouling; circles (○): calibration plot after UV cleaning]; **b)** Cyclic voltammograms registered at 0.1 V s⁻¹ at different analytical steps during the fouling/cleaning procedure and relevant scheme.

(line 1), demonstrating the high efficiency of the cleaning process; the removal of adsorbed species was achieved and the possibility of electrode reuse was proved.

Finally, the robustness of the optimized device in aging and wear was considered. The sensor has maintained the same sensitivity and behaviour after many months, detections and irradiations without adopting any specific care in storage.

Experimental

All chemicals were of reagent grade purity and used as received. Distilled water purified with a Millipore Milli-Q apparatus (resistivity $\geq 18.2 \text{ M}\Omega \text{ cm}^{-1}$) was used to prepare solutions and sols. An UV iron halogenide lamp Jelosil HG500 with an effective power density, measured using a Thorlabs S314C radiometer, of $23 \text{ (mW cm}^{-2}\text{)}$ emitting between 280 and 400 nm (emission spectrum in supporting information, Figure S7) was used for the photocatalytic tests and for the irradiation steps included in the device synthesis.

Device synthesis: the fluorine doped tin oxide coated glass slides (FTO, Sigma-Aldrich®, $\sim 7 \text{ (}\Omega \text{ sq)}$, $2 \times 3 \text{ cm}$) adopted as conductive supports were previously sonicated in a cleaning solution ($\text{H}_2\text{O} : \text{acetone} : \text{propanol} = 1:1:1$) and irradiated for 1 hour under UV light.

The silica sol was prepared by the procedure reported by Wang *et al.*²⁶ Briefly, 10 g of TEOS was added into the solution containing 25 g of ethanol and 4.5 g of hydrochloric acid solution (0.1 M). The mixture was stirred at lab temperature for 2 hours and then refluxed at $60 \text{ }^\circ\text{C}$ for 60 min. Eventually, 25 g of an ethanol solution of CTAB cationic surfactant (2 g in 25 mL) was dissolved in the as-obtained solution by slowly stirring at lab temperature for 1 hour. The FTO was dipped in such a sol and quickly calcinated at $500 \text{ }^\circ\text{C}$ for 1 hour under N_2 flow. The functionalization by (3-aminopropyl)triethoxysilane (APTES) was performed by irradiating for 1 hour the adsorbent (either the silica layer or the bare FTO layer), then dipping in anhydrous toluene under N_2 at $70 \text{ }^\circ\text{C}$. After 1 hour, a solution of APTES in anhydrous toluene was added to obtain a final concentration of $5 \text{ }\mu\text{M}$. After 3 hours at $70 \text{ }^\circ\text{C}$ the sample was cleaned by sonication for few minutes in toluene, ethanol and water in order to eliminate the un-grafted silane and eventually dried under a nitrogen stream.

The sample was then immersed in a solution of Ag NPs for 15 minutes and dried under N_2 flux. The final titania layer was obtained by dipping the sample in a titania sol and calcinating it under N_2 flow for 1 hour at $400 \text{ }^\circ\text{C}$. The titania sol has been developed in our group and was previously reported³¹. Briefly, 0.9 mL of HCl 37 % was added to a solution of $\text{Ti(OC}_3\text{H}_7)_4$ in ethanol (0.1 mol in 100 mL) under stirring. Then, 0.47 g of Lutensol ON70 (BASF) was added to the sol after being dissolved in 100 mL of ethanol.

Silver nanoparticles (Ag NPs) were synthesized by adapting the procedure reported by Panzarasa.²⁸ Briefly, 0.15 g of silver nitrate were dissolved in 25 mL of water and this solution was added under stirring to a solution of 0.5 g of trisodium citrate

and 0.25 g of poly(vinylpyrrolidone) (PVP10, $M_w \sim 10000 \text{ (g mol}^{-1}\text{)}$) in 125 mL of water. The resulting solution was poured in a three-necked, round-bottomed 250 mL flask equipped with a mechanical stirrer and a dropping funnel. The solution was cooled in an ice bath and an ice-cooled solution of sodium borohydride, obtained by dissolving 12 mg of solid in 30 mL of water, was added dropwise under stirring. The resulting dark brown suspension was left under stirring for 5 minutes after the addition, aged at $+4 \text{ }^\circ\text{C}$ for 24 hours before use and stored at this temperature.

Film characterization: room-temperature X-ray diffraction (XRD) patterns were collected between 5° and 90° with a powders diffractometer Philips X'Pert $\theta/2\theta$ in grazing angle geometry, $\omega = 1.0^\circ$, utilizing X Cu K_α radiation ($\lambda = 1.5416 \text{ \AA}$ and power 1.6 kW). The results were obtained on the basis of Hanawalt method on the data set of PDF-2 (Powder Diffraction File, ICDD). Scanning electron microscopy (SEM) images were obtained by a Zeiss LEO 1430 working at 30 keV. HR TEM images were acquired using a JAM 2010 equipped with a LAB6 electron gun (beam energy 200 keV) and a Gatan CCD camera allowing high resolution imaging. Film transparency and plasmonic resonance were evaluated by UV-Visible spectroscopy (Beckman DU640). Z-potential was determined by a Malvern Zetasizer Nano-ZS equipped with a universal dip cell (Malvern) and standard polystyrene cuvettes. Water contact angles were measured by a Krüss Easydrop. Film thicknesses were evaluated using a Filmetrics® F20 reflectometer (Filmetrics).

CV and EIS experiments were carried out with an Autolab PGStat30 (Ecochemie, The Netherlands) potentiostat/galvanostat equipped with FRA module and controlled by GPES and FRA softwares. Impedance data were processed with Z-View 3.1 software.

Cyclic voltammetric characterization was performed in 0.1 M NaClO_4 aqueous solution at room temperature, in a three-electrode conventional cell, with a saturated calomel and a platinum wire as reference and counter electrodes, respectively. No N_2 degassing of the solution was necessary, since dissolved O_2 did not affect the measurements. The potential was varied between -0.1 V and $+0.4 \text{ V}$ (SCE) at $0.1 \text{ (V s}^{-1}\text{)}$ scan rate. The potential window was chosen considering the Pourbaix diagrams¹⁴ for TiO_2 and metallic Ag. Electrochemical impedance spectra were registered at -0.1 , $+0.1$ and $+0.25 \text{ V}$ (SCE), with a range of frequencies between 65000 and 0.1 Hz and an amplitude of 10 mV in the same experimental conditions of cyclic voltammetry. The behaviour of the electrodes was studied both in the presence or in the absence of a redox reaction, using $\text{K}_4[\text{Fe(CN)}_6]$ as model probe molecule.

Photoactivity test: the photocatalytic activity of the device was tested by following in time the degradation of an hydrophobizing organic molecule deposited onto the titania layer. The adopted hydrophobizing/staining molecule (SILRES BS 1701) is produced and commercialized by Wacker Chemie

AG. It is a mixture of isomeric octyltriethoxysilanes with iso-octyltriethoxysilane as the main component. The molecules were chemisorbed at the tested surface by the chemical vapor deposition protocol previously reported by us⁴⁹. The device was placed in a glass container together with a Teflon[®] cup filled with the siloxane. The container was placed in an oven at 100 °C for 3 hours to vaporize the siloxane. Eventually, the substrate was sonicated in toluene and dried.

The degradation of the organic moieties was monitored by measuring the water contact angle as a function of the time of UV irradiation.

Dopamine detection: the dopamine hydrochloride was of analytical purity and purchased by Sigma-Aldrich. It was detected using Differential Pulse Voltammetry, scanning the potential between -0.1 V and +0.4 V (SCE), with the following parameters: modulation time 0.05 s, interval time 0.5 s, step potential 0.005 V, modulation amplitude 0.05 V, in a three electrodes cell. Three voltammograms at each dopamine concentration were recorded. The calibration curve was repeated three times, with comparable results. Saturated calomel, Pt wire and the modified FTO were used as reference, counter and working electrodes, respectively. Phosphate buffer (pH 7.4, 0.1 M) was used as the supporting electrolyte.

Conclusions

Fouling and fragility of complex engineered electrochemical devices for the detection of biomolecules are solved by the development of sandwich structured electrodes endowed with a photoactive top layer. The lack of investigation in this field caused the scarce applicability of many specific sensors for the detection of highly relevant molecules in biomedical and environmental protection fields. Here, we engineered a simple system with the purpose to detect an organic biomolecule with absolute relevance in the medical context, dopamine. We solved the problem of chemisorption and fouling of such molecules by covering the sandwich with a photoactive external top layer. We proved the total recovery of sensitivity after irradiating the device by UV-A lamp for a short time (1 hour). No change in the electrode signal was observed after numerous usages and irradiations. Silver nanoparticles, deposited in a controlled manner inside the sandwich, not only are critical for the detection of dopamine, but were demonstrated to maintain their structure and metallic nature. We proved, for the first time in the sensing field, the protective effect of the titania top layer on nanoparticles modified electrodes, making their behavior unchanged in time. Hence, the proof of concept of sensors with highly applicative and commercial appealing, reusable and potentially not affected by aging, was demonstrated. The described know-how, deriving from the ability to create such transparent, photoactive, multilayer structures, can be potentially employed on other electrode supports and tailored on different target molecules, solving, one for all, the problem of the “cleaning” process.

Acknowledgements

The authors wish to thank Dr. Gianluigi Marra from the Research Center for Non-Conventional Energies, ENI Donegani Institute, Novara, for kindly providing XRD and HR TEM analyses.

This work was financially supported by INSTM and Regione Lombardia (agreement signed on 13/11/2012).

Notes and references

^a Dipartimento di Chimica, Università degli Studi di Milano, Via Golgi 19, 20133 Milano, Italy.

^b Consorzio Interuniversitario Nazionale per la Scienza e Tecnologia dei Materiali (INSTM), Via Giusti 9, 50121 Firenze, Italy.

^c Dipartimento di Scienze e Innovazione Tecnologica, Università del Piemonte Orientale “Amedeo Avogadro”, Viale T. Michel 11, 15100 Alessandria, Italy.


† These authors contributed equally.

Electronic Supplementary Information (ESI) available: Z-potential spectrum for Ag NPs suspension; transparency, reflectance spectrum and SEM top picture of the device; Bode plots corresponding to complex plane plot spectra; voltammograms for FTO+Ag+TiO₂; emission spectrum of the UV lamp. See DOI: 10.1039/b000000x/

1. C. M. a. Brett, *Pure Appl. Chem.*, 2001, **73**, 1969–1977.
2. L. Rassaei, M. Amiri, C. M. Cirtiu, M. Sillanpaa and F. Marken, *Trac-Trends Anal. Chem.*, 2011, **30**, 1704–1715.
3. M. Pumera, S. Sánchez, I. Ichinose and J. Tang, *Sensors Actuators B Chem.*, 2007, **123**, 1195–1205.
4. G. Hanrahan, D. G. Patil and J. Wang, *J. Environ. Monit.*, 2004, **6**, 657–64.
5. S.-J. Bao, C. M. Li, J.-F. Zang, X.-Q. Cui, Y. Qiao and J. Guo, *Adv. Funct. Mater.*, 2008, **18**, 591–599.
6. X. Ma, W. Hu, C. Guo, L. Yu, L. Gao, J. Xie and C. M. Li, *Adv. Funct. Mater.*, 2014, n/a–n/a.
7. M. Zhang, C. Liao, Y. Yao, Z. Liu, F. Gong and F. Yan, *Adv. Funct. Mater.*, 2014, **24**, 978–985.
8. C. M. Welch and R. G. Compton, *Anal. Bioanal. Chem.*, 2006, **384**, 601–19.
9. F. W. Campbell and R. G. Compton, *Anal. Bioanal. Chem.*, 2010, **396**, 241–59.
10. I. Streeter, R. Baron and R. G. Compton, *J. Phys. Chem. C*, 2007, **111**, 17008–17014.
11. Q. Wang and Y. Yun, *Microchim. Acta*, 2012, **180**, 261–268.
12. X. L. Luo, A. Morrin, A. J. Killard and M. R. Smyth, *Electroanalysis*, 2006, **18**, 319–326.
13. D. Meroni, S. Ardizzone, U. S. Schubert and S. Hoeppeper, *Adv. Funct. Mater.*, 2012, **22**, 4376–4382.
14. A. Fujishima, X. Zhang and D. A. Tryk, *Surf. Sci. Rep.*, 2008, **63**, 515–582.
15. X. Chen and S. S. Mao, *Chem. Rev.*, 2007, **107**, 2891–959.
16. G. Soliveri, R. Annunziata, S. Ardizzone, G. Cappelletti and D. Meroni, *J. Phys. Chem. C*, 2012, **116**, 26405–26413.
17. R. Alam, I. V Lightcap, C. J. Karwacki and P. V Kamat, *ACS Nano*, 2014, **8**, 7272–8.

18. G. K. Mor, M. A. Carvalho, O. K. Varghese, M. V. Pishko and C. A. Grimes, *J. Mater. Res.*, 2011, **19**, 628–634.
19. Y.-Y. Song, Z. Gao, K. Lee and P. Schmuki, *Electrochem. commun.*, 2011, **13**, 1217–1220.
20. Y.-Y. Song, Z.-D. Gao and P. Schmuki, *Electrochem. commun.*, 2011, **13**, 290–293.
21. K. Jackowska and P. Krysinski, *Anal. Bioanal. Chem.*, 2013, **405**, 3753–71.
22. M. Perry, Q. Li and R. T. Kennedy, *Anal. Chim. Acta*, 2009, **653**, 1–22.
23. N. G. Shang, P. Papakonstantinou, M. McMullan, M. Chu, A. Stamboulis, A. Potenza, S. S. Dhesi and H. Marchetto, *Adv. Funct. Mater.*, 2008, **18**, 3506–3514.
24. X. Wang, X. Liu, L. Lai, S. Li, J. Weng, Z. Zhou, Q. Cui, X. Chen, M. Cao and Q. Zhang, *Adv. Funct. Mater.*, 2008, **18**, 1809–1823.
25. M. Wei, L.-G. Sun, Z.-Y. Xie, J.-F. Zhii, A. Fujishima, Y. Einaga, D.-G. Fu, X.-M. Wang and Z.-Z. Gu, *Adv. Funct. Mater.*, 2008, **18**, 1414–1421.
26. X. Wang, R. Xiong and G. Wei, *Surf. Coatings Technol.*, 2010, **204**, 2187–2192.
27. R. G. Acres, A. V. Ellis, J. Alvino, C. E. Lenahan, D. A. Khodakov, G. F. Metha and G. G. Andersson, *J. Phys. Chem. C*, 2012, **116**, 6289–6297.
28. G. Panzarasa, *J. Chem. Educ.*, 2014, **91**, 696–700.
29. D. D. Evanoff and G. Chumanov, *Chemphyschem*, 2005, **6**, 1221–31.
30. D. D. Evanoff, R. L. White and G. Chumanov, *J. Phys. Chem. B*, 2004, **108**, 1522–1524.
31. G. Maino, D. Meroni, V. Pifferi, L. Falciola, G. Soliveri, G. Cappelletti and S. Ardizzone, *J. Nanoparticle Res.*, 2013, **15**, 2087.
32. V. Pifferi, G. Facchinetti, A. Villa, L. Prati and L. Falciola, *Catal. Today*, 2014.
33. L. Falciola, A. Gennaro, A. A. Isse, P. R. Mussini and M. Rossi, *J. Electroanal. Chem.*, 2006, **593**, 47–56.
34. C. Bellomunno, D. Bonanomi, L. Falciola, M. Longhi, P. R. Mussini, L. M. Doubova and G. Di Silvestro, *Electrochim. Acta*, 2005, **50**, 2331–2341.
35. V. Pifferi, V. Marona, M. Longhi and L. Falciola, *Electrochim. Acta*, 2013, **109**, 447–453.
36. M. Giovanni and M. Pumera, *Electroanalysis*, 2012, **24**, 615–617.
37. I. Boskovic, S. V. Mentus and M. Pjescic, *Electrochim. Acta*, 2006, **51**, 2793–2799.
38. S. D. Standridge, G. C. Schatz and J. T. Hupp, *Langmuir*, 2009, **25**, 2596–2600.
39. Y.-G. Zhou, F. W. Campbell, S. R. Belding and R. G. Compton, *Chem. Phys. Lett.*, 2010, **497**, 200–204.
40. G. Herzog and V. Beni, *Anal. Chim. Acta*, 2013, **769**, 10–21.
41. A. O. Simm, S. Ward-Jones, C. E. Banks and R. G. Compton, *Anal. Sci.*, 2005, **21**, 667–671.
42. S. Daniele, M. Baldo and C. Bragato, *Curr. Anal. Chem.*, 2008, **4**, 215–228.
43. A. J. Bard and L. R. Faulkner, *Electrochemical Methods: Fundamentals and Applications*, 2001.
44. I. Streeter and R. G. Compton, *J. Phys. Chem. C*, 2007, **111**, 18049–18054.
45. T. J. Davies and R. G. Compton, *J. Electroanal. Chem.*, 2005, **585**, 63–82.
46. J. H. Moon, J. W. Shin, S. Y. Kim and J. W. Park, *Langmuir*, 1996, **12**, 4621–4624.
47. A. Antonello, G. Soliveri, D. Meroni, G. Cappelletti and S. Ardizzone, *Catal. Today*, 2014, **230**, 35–40.
48. Y. Paz, *Beilstein J. Nanotechnol.*, 2011, **2**, 845–61.
49. G. Soliveri, D. Meroni, G. Cappelletti, R. Annunziata, V. Aina, G. Cerrato and S. Ardizzone, *J. Mater. Sci.*, 2014, **49**, 2734–2744.

Table of Content

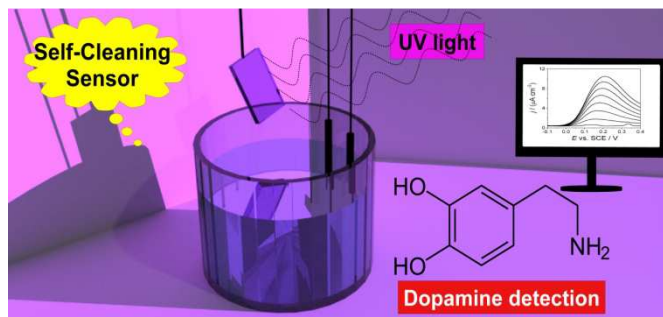

Self-cleaning reusable composite electrode is ad hoc designed to bypass the fouling problem connected with biomedical molecule detection (e.g. dopamine).