

Analytical Methods

Accepted Manuscript



This is an *Accepted Manuscript*, which has been through the Royal Society of Chemistry peer review process and has been accepted for publication.

Accepted Manuscripts are published online shortly after acceptance, before technical editing, formatting and proof reading. Using this free service, authors can make their results available to the community, in citable form, before we publish the edited article. We will replace this *Accepted Manuscript* with the edited and formatted *Advance Article* as soon as it is available.

You can find more information about *Accepted Manuscripts* in the [Information for Authors](#).

Please note that technical editing may introduce minor changes to the text and/or graphics, which may alter content. The journal's standard [Terms & Conditions](#) and the [Ethical guidelines](#) still apply. In no event shall the Royal Society of Chemistry be held responsible for any errors or omissions in this *Accepted Manuscript* or any consequences arising from the use of any information it contains.

1
2
3 **Development of sensitive and rapid liquid-phase microextraction**
4 **method followed by liquid chromatography mass spectrometry for**
5 **the determination of zearalenone residues in beer samples**
6
7
8
9

10
11
12
13
14
15
16 Ioanna. E. Rempelaki, Vasilios A. Sakkas*, Triantafyllos. A. Albanis
17
18
19
20

21
22 *Laboratory of Analytical Chemistry, Department of Chemistry, University of*
23 *Ioannina, Ioannina 45110, Greece*
24
25
26
27
28
29
30
31
32

33 *Assistant Professor Dr. Sakkas, Tel: +3026510-08303, email: vsakkas@cc.uoi.gr*
34
35
36
37

38 * Corresponding Author
39

40 Dr. V.A. Sakkas
41

42 Laboratory of Analytical Chemistry, Department of Chemistry,
43

44 University of Ioannina, Ioannina 45110, Greece
45

46
47 Tel: +3026510-08303
48

49 Fax: +3026510-08796
50

51
52 *E-mail address: vsakkas@cc.uoi.gr*
53
54
55
56
57
58
59
60

Abstract

In this work, a new, rapid and sensitive, dispersive suspended microextraction procedure, followed by liquid chromatography mass spectrometry, was employed for the determination of zearalenone in beer samples. The liquid-phase microextraction method is based on solvent dispersion and magnetic stirring. Validation was carried out according to the Commission Decision 2006/406/EC guidelines. Under the optimum conditions, limit of detection (LOD) was determined at $0.44 \mu\text{g kg}^{-1}$ and the limit of quantification was calculated at $1.45 \mu\text{g kg}^{-1}$. The relative standard deviation (RSD, $n = 5$) for inter-day precision was found to be 5.4 % and for intra-day precision 3.6 %. The linearity was obtained by five points in the concentration range of 1.5-45 $\mu\text{g kg}^{-1}$ and the recovery was $> 91\%$. The occurrence of the selected mycotoxin was studied in several beer samples collected from local market from the region of Epirus.

Keywords: Dispersive suspended microextraction; Mycotoxins; Zearalenone; Beers; LC-MS.

1. Introduction

Mycotoxins are toxic natural secondary metabolites produced under particular environmental conditions by molds on agricultural commodities such as maize, wheat, oats and barley, in the field or during storage.¹⁻⁶ The occurrence, amount and type of mycotoxin may depend on the environment, fungi species, infection severity and of the kind of crop.^{7, 8} Food contaminated by mycotoxins could be potential hazards to consumers⁹ and could produce acute and chronic effects.¹⁰

Zearalenone (ZON) belongs to type B of trichothecenes.¹¹ It is an estrogenic resorcylic acid lactone compound mainly produced by *Fusarium graminearum* and is classified as group 3 carcinogen in 1993 and 1999 by IARC.^{12, 13} The main concern is that ZON is a naturally occurring estrogen that is well recognized to cause hormonal and endocrine disrupting effects in animals.¹⁴⁻¹⁸

Since cereals are raw materials of beer and beer-based drinks, it is necessary to consider that the risk of ZON and other mycotoxins contamination exists in such products. Beer is the oldest alcoholic beverage that contains water, alcohol, protein substances, mineral salts, carbohydrates¹⁹ and according to the World Health Organization, the European countries are consuming the largest quantity of beer. European Union has established a maximum permitted limit for ZON at 100 $\mu\text{g kg}^{-1}$ for cereals and suggested 20 $\mu\text{g kg}^{-1}$ for their sub products.

To deal with the increasing number of sample matrices and mycotoxins of interest, fast and accurate analytical methods are needed for their determination in different commodities. Numerous analytical methods have been developed for the determination of mycotoxins in beer samples.²⁰⁻³⁰ In recent years, there is a shift to the development of new liquid-phase microextraction protocols that make analysis faster and cheaper by using smaller volumes of solvents. These methods include

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60


dispersive liquid-liquid microextraction based on solidification of floating organic droplet (DLLME-SFO),³¹⁻³³ temperature-controlled ionic liquid dispersive liquid-liquid microextraction (TC-IL-DLLME),³⁴ manual shaking-enhanced ultrasound-assisted emulsification microextraction (MS-USAEME),^{35,36} dispersive liquid-liquid microextraction (DLLME),³⁷ hollow fiber-based liquid phase microextraction (HF-LPME),³⁸ array capillary in-tube solid-phase microextraction (ACIT-SPME),³⁹ single drop microextraction (SDME)⁴⁰ and dispersive suspended microextraction (DSME)⁴¹. With the above in mind, the aim of the present study was to develop a liquid-phase microextraction method based on DSME followed by liquid chromatography for the determination of ZON in beer samples. The novelty of the method relies not only in the introduction of a new extraction method that is employed for the first time in such matrix, but also to its efficiency to eliminate the bottleneck of LC/MS analysis in food samples, co-eluting matrix interferences, by the combination of a dilution factor of 1 to 5 and external matrix-matched calibration.

2. Experimental

2.1. Chemicals and reagents

Zearalenone $\geq 98\%$ (ZON, Scheme 1) analytical standard was purchased from Sigma-Aldrich Chemie (Steinheim, Germany). The individual stock solution of ZON at concentration of 100 mg kg^{-1} was prepared in acetonitrile, purchased from Panreac (Barcelona, Spain), and kept at $-20 \text{ }^\circ\text{C}$, in the dark. Before use, the solution was brought to room temperature. Working standard solutions were prepared using adequate aliquots of standard stock solution and diluting in acetonitrile. Analytical LC grade solvents, acetonitrile and water, were obtained from Fischer Chemicals (Leics,

1
2
3 UK). Toluene, hexane, isooctane, and p-xylene were supplied by Labscan (Dublin,
4
5 Ireland). Potassium dihydrogen phosphate (KH_2PO_4), which was used for the
6
7 preparation of buffer solution, was purchased from Merck (Darmstadt, Germany).
8
9

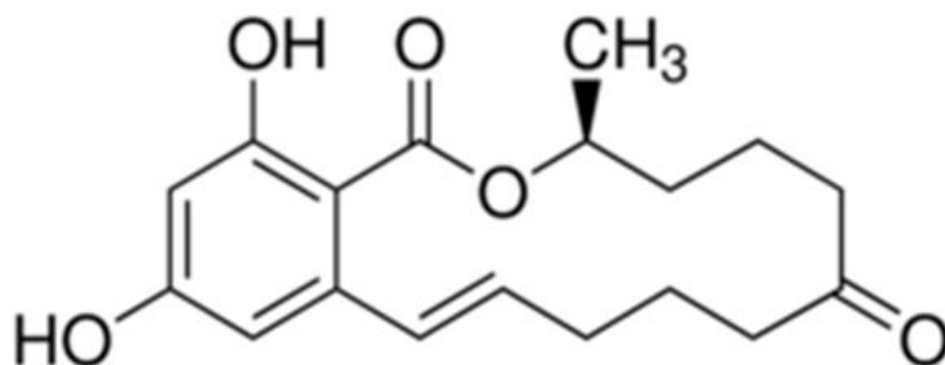

40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

Scheme 1. ZON chemical structure

2.2. Apparatus

The analysis was carried out using liquid chromatography (LC-MS Shimadzu, Japan), equipped with an auto sampler (SIL-20A, Shimadzu, Japan) and a mass spectrometry detector (LC-MS 2010- EV, Shimadzu, Japan). The analytical column was a Pinnacle II C18 (150 x 4.6 mm, 5 μm Restek, Bellefonte, PA). Positive and negative ionization mode using an isocratic gradient consisted of methanol:acetonitrile (60:40% v/v) - based on earlier investigations with ZON⁴² - was evaluated for the detection of the target analyte in beer samples. During LC-MS ESI (-) mode the resulting spectra are simpler with fewer background ions compared to LC-MS ESI (+), since negative ionization essentially produces only the deprotonated $[\text{M}-\text{H}]^-$ ion ($m/z=317.1$), while at the same time the signal-to-noise ratio is

1
2
3 significantly improved. Concerning the ionization mechanism, it has been stated that
4
5 in some circumstances neutral analytes can be converted to negatively charged
6
7 species simply by loss of a proton as they pass through the sprayer capillary²⁹. Mass
8
9 spectrometry was used in selected ion monitoring (SIM) mode, with the following
10
11 selected ions m/z: 317.1 and 318.1. The nebulizer pressure was 75 bar (1125 psi), the
12
13 detector voltage (V) 1500 and flow rate 0.5 mL min⁻¹. Under these chromatographic
14
15 conditions the retention time of ZON was 3.7 min.
16
17
18
19
20
21
22
23

24 **2.3. Sample Collection and preparation**

25
26
27 Commercial available domestic and imported bottled beers were collected from
28
29 different stores, from the region of Epirus, and kept at 4 °C, in a dark and dry place.
30
31 Each bottled beer sample was gently shaken and approximately 1 mL was degassed
32
33 by ultra-sonication (Elma-S 30 H, Made in Germany) and diluted 1 to 5 (total volume
34
35 6.0 mL) with buffer solution adjusted to pH 5. The samples with undetectable levels
36
37 of ZON (blank samples) were used for optimization and validation studies.
38
39
40
41
42
43
44

45 **2.4. Dispersive suspended microextraction (DSME) procedure**

46
47
48 When needed, the degassed and diluted (1:5) beer sample was fortified with a solution
49
50 of the target compound to obtain the desired final concentration. A 550 µL aliquot of
51
52 toluene was delivered, as extraction solvent, to the surface of the sample. A magnetic
53
54 micro stirring bar (10 mm × 3 mm o.d., VWR, Arlington Heights, Illinois, USA) was
55
56 placed at the bottom of the vial and the latter was placed on the magnetic stirrer
57
58 (Hotplate Stirrer, LMS-100, Daihan Labtech, Made in Korea).
59
60

1
2
3 The DSME procedure first involved an extraction step, followed by a restoration step.
4
5 In the extraction step (from opening the magnetic stirrer at a higher rate, to reducing
6
7 its speed to the final restoration speed), the mixture was agitated for 30s (extraction
8
9 time) at 800 rpm (extraction speed) and formed a cloudy solution (aqueous sample
10
11 and toluene). ZON was extracted into the fine toluene droplets.
12
13
14

15
16 When the stirring speed was adjusted to 400 rpm, the restoration step began. At this
17
18 stirring speed, a gentle vortex was formed and the toluene droplets began to coalesce.
19
20 After 14 min (restoration time), the organic phase had absolutely separated from
21
22 aqueous phase and had formed the final suspended phase in the bottom center of the
23
24 vortex (500 μ L). Then, the suspended phase was withdrawn and 20.0 μ L of the
25
26 organic phase was injected into the LC-MS for further analysis.
27
28
29
30
31
32
33

34 **3. Results and discussion**

35 **3.1. Preliminary studies**

36
37
38 Concerning the DSME extraction method, several factors may affect its efficiency,
39
40 such as, extraction solvent, extraction solvent volume, and extraction time. During
41
42 method development, the first consideration was to select an appropriate extraction
43
44 solvent to recover efficiently the study compound. The solvent should fulfill the
45
46 following criteria: i) to be insoluble in water in order to form two different phases in
47
48 solution and facilitate the phase separation, ii) to exhibit a lower density than water to
49
50 rise above the aqueous phase, iii) to have a high extraction capability toward ZON
51
52 and iv) to display good liquid chromatographic behavior considering the matrix
53
54 complexity. The solvents studied were toluene, hexane, isooctane, *p* xylene and
55
56
57
58
59
60

1
2
3 benzene. The results revealed that toluene had the highest extraction efficiency (75%)
4
5 compared to the other tested solvents (hexane 60%, isooctane 64%, p-xylene 69%,
6
7 benzene 72%).
8
9

10
11 Matrix effects are common problems that occur when using LC/MS and have adverse
12
13 impacts on the analytical results²⁸. More specifically, electrospray ionization is
14
15 susceptible to matrix-related signal suppression/enhancement that is attributed to the
16
17 competition between the analyte ions and matrix components²⁰. To evaluate the
18
19 presence and extension of this effect, ZON standards of different concentrations were
20
21 analyzed in pure solvent and beer matrix. The combination of a dilution factor of 1 to
22
23 5 (beer to water), as well as, the use of matrix-matched standards (according to
24
25 Council Decision 2002/657/EC (European Community 2002) and document
26
27 SANCO/10684 (2009)) compensated the suppression signal effects, achieving an
28
29 accurate quantification (matrix effect less than 18% was calculated and was
30
31 considered as no matrix effect, because this variation would be close to the
32
33 repeatability values) (Figure S1). Our observation was in agreement with Rubert et
34
35 al.²⁵ who showed that the addition of established internal standards did not significant
36
37 compensate the matrix effect compared to external matrix-matched calibration. In
38
39 light of these results, the choice of toluene as extraction solvent, as well as, of the
40
41 selection of dilution factor 1:5, were done with respect to resolve and diminish effects
42
43 from the matrix constituents and make it applicable in real samples with a minimum
44
45 of sample preparation (Fig. 1).
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

<Fig. 1>

1
2
3 Moreover, some “technical” details of the DSME procedure were preliminary
4 evaluated before optimization. The extraction speed was adjusted to 800 rpm due to
5
6 the adequate dispersion of toluene to diluted beer sample and to the easiness of
7
8 retrieving the droplets. The adjusted restoration speed of 400 rpm forced the droplets
9
10 to gather up at the top center position of the vortex. When a restoration speed higher
11
12 than 400 rpm was selected, the suspended phase was not stable and it was hard for the
13
14 dispersive droplets to gather up. On the contract, when the restoration speed was
15
16 below 400 rpm, a vortex was not created at the center of the vial, so it was hard to
17
18 withdraw the droplets with the micro-syringe. Finally, the restoration time of toluene
19
20 droplet was calculated to be 14 min, until all the dispersive droplets were gathering
21
22 up.
23
24
25
26
27
28
29
30
31
32

33 **3.2. Optimization of extraction time**

34
35
36 In the DSME, extraction time is defined as the time from opening the magnetic stirrer
37
38 to turning down to the restoration speed. The extraction of ZON from the diluted beer
39
40 samples into the organic solvent is an equilibrium process. The effect of extraction
41
42 time was evaluated over the time range between 10s and 60s. Time shorter than 30s
43
44 does not permit adequate dispersion of toluene to the entire mass of the sample, so the
45
46 extraction yield of ZON was low (Fig. 2). Increasing from 40s to 60s, the
47
48 reunification of the droplets became very difficult and it was impossible to carry out
49
50 further analysis. This phenomenon revealed that the contact surface between organic
51
52 phase and aqueous phase was infinitely large and the equilibrium state was obtained
53
54 in a few seconds. Based on the above considerations, 30s was selected as the
55
56 extraction time.
57
58
59
60

1
2
3
4
5
6
7 <Fig. 2>
8
9
10
11
12
13
14
15

16 **3.3. Optimization of extraction solvent volume**

17
18
19 In order to achieve the best extraction efficiency, different volumes of toluene (100 -
20 600 μL) were examined. As well, the diluted beer sample was settled to 6.0 mL.
21
22 Results have shown that addition of toluene at the range of 100 – 200 μL , is not
23
24 efficient for ZON extraction, due to toluene solubility to ethanol, that resulted at a
25
26 small recovered/restored solvent phase, which was difficult to withdraw. At higher
27
28 toluene volumes (250 to 500 μL , Fig. 3) the extraction of the target analyte to the
29
30 organic solvent was increased and 550 μL was selected as the most adequate, since
31
32 under these conditions, toluene was more efficiently dispersed in the diluted beer
33
34 sample and restored to form the organic droplet. At higher toluene amounts there was
35
36 not any notable improvement or recrudescence of the extraction yield.
37
38
39
40
41
42
43
44
45
46
47

48 <Fig. 3>
49
50
51
52
53

54 **3.4. Optimization of pH addition**

55
56 Different pH values, ranging from 3 to 10 (including the pH of diluted beer sample),
57
58 were studied in order to evaluate its influence in the DSME process. Results revealed
59
60 that the best response for ZON was accomplished at pH 5 (Fig. 4), which was selected

1
2
3 for further experiments. The environmentally relevant pK_a value of ZON is defined to
4
5 7.6. While at $pH > 9.6$ the anion is dominant in the solution, at $pH < 5.6$ is mainly in the
6
7 neutral form, and therefore ZON was efficiently extracted from toluene.
8
9

10
11
12
13
14 <Fig. 4>
15
16
17
18
19
20

21 3.5. Optimization of ionic strength

22
23
24 Addition of salt to the sample may have several effects on the DSME. Ionic presence
25
26 on the extraction procedure, was investigated with sodium chloride concentration in
27
28 the range of 0-6% (w/v). The effect of salt concentration on the extraction efficiency
29
30 of ZON is illustrated in Fig. 5. As can be seen, the addition of salt 3% w/v has a
31
32 positive effect on the extraction efficiency of the target analyte. Salt attracts water
33
34 molecules in an effort to "solvate" the ions therefore decreasing the solubility of ZON
35
36 and increasing the extraction yield. However, extraction efficiency for ZON decreases
37
38 with the increase of NaCl concentration at higher values (6% w/v). This observation
39
40 could be attributed to the formation of a physical barrier across aqueous phase and
41
42 organic phase interface, which prevents the mass transfer of the target analyte into the
43
44 extraction solvent⁴². Based on the above experimental results, ionic strength of 3%
45
46 w/v (NaCl) was selected.
47
48
49
50
51

52
53
54
55
56 <Fig. 5>
57
58
59
60

3.6. Analytical performance of DSME

Performance characteristics of the optimized method were established by a validation procedure, studying trueness, precision, linear range, sensitivity and specificity.

3.6.1. Method trueness

Method trueness was assessed through relative recovery studies, spiking blank samples at two fortification levels (1.5 and 10.0 $\mu\text{g kg}^{-1}$) processing five samples in each experiment. The relative recovery was defined as the ratios of the peak areas of the analyses in the spiked blank samples and the peak area of the analyses in distilled water sample, spiked with the same amount of the analyte. Mean relative recovery calculated was 91% and were within the criteria approved by the European Committee for Standardization, for the acceptability of analytical methods (Commission Directive 2006/401/EC).

3.6.2. Precision

The intra-day repeatability ($\text{RSD}_r\%$, $n=5$) and inter-day reproducibility ($\text{RSD}_R\%$, $n=5 \times 3$ days) were expressed by calculating the relative standard deviation (RSD %). Experiments were carried out by extracting a beer sample spiked at 1.5 and 10 $\mu\text{g kg}^{-1}$.

¹. Intra-day repeatability and inter-day reproducibility were lower than 10%.

3.6.3. Linear range

Method linearity was evaluated by performing matrix-matched calibration curves at a concentration range of 1.5 to 45 $\mu\text{g kg}^{-1}$. The obtained peak area versus concentration was linear (least-squares linear regression) in the assayed range achieving coefficient of determination equal to 0.9974.

3.6.4. Limit of detection (LOD) and quantification (LOQ) and specificity

LODs and LOQs were calculated, analyzing blank samples spiked at 0.025, 0.050, 0.10, 0.50, and 1.0 $\mu\text{g kg}^{-1}$, and they were determined as the lowest concentrations of analyte for which signal-to-noise ratios were 3 and 10, respectively. The detection and quantification limits of ZON with the proposed method were 0.44 and 1.45 $\mu\text{g kg}^{-1}$, respectively. These values were below the guidance levels established by European Commission regulation (EU) for cereal sub-products (20 $\mu\text{g kg}^{-1}$).

The specificity of the method was tested by the analysis of blank samples. The absence of any chromatographic peak in every matrix, at the same retention time as ZON, indicated that there were no matrix compounds that might give a false positive signal in these blank samples (Fig. 1).

The developed DSME method could be equally compared in relation to the pretreatment time, sensitivity and LODs with other liquid-phase microextraction methods such as DLLME [28]. Recovery of ZON after DLLME and high performance thin layer chromatography (HPTLC) equipped with a densitometer was 83% while the proposed method provides up to 91%. The limits of detection were

quite comparable at $0.12 \mu\text{g kg}^{-1}$ (for DLLME) and $0.44 \mu\text{g kg}^{-1}$ (for DSME).

However, limitation of both methods could be the use of toxic extraction solvents.

3.7. Application to real samples

The optimized method was applied to analyze seven blond beer samples collected from local stores from the region of Epirus. The results are depicted at Table 1. No ZON residues were found in analyzed beer samples. To validate the results, real samples spiked with known amount of ZON were analyzed. Good recoveries were obtained in the range of 86 to 95%.

[Table 1]

4. Conclusions

The present study reports a new, rapid, sensitive and low cost analytical method for the determination and quantification of a well-known endocrine disruptor, ZON, in the oldest and most worldwide consumed beverage. The extraction procedure allows the preconcentration of ZON by a factor of 2, while at the same time overcomes the problem of possible interfering compounds allowing a LOQ below the guidance levels established by European Commission regulation. The validated DSME was found to be suitable for the routine monitoring of ZON in beer samples by regulatory laboratories. Moreover, implementing the negative ion mode seems to be of general

1
2
3 applicability also to other mycotoxins and their metabolites. In such case, further
4
5 studies should be carried out improving the chromatographic conditions and the
6
7 efficiency of separation between the target analytes.
8
9

10 11 12 13 14 **Acknowledgements**

15
16
17 This research project has been co-financed by the European Union (European
18
19 Regional Development Fund- ERDF) and Greek national funds through the
20
21 Operational Program “THESSALY- MAINLAND GREECE AND EPIRUS-2007
22
23 2013” of the National Strategic Reference Framework (NSRF 2007-2013).
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

References:

1. S. Doll, J. A. Schrickx, H. Valenta, S. Danicke., J. Fink-Gremmels, Interactions of deoxynivalenol and lipopolysaccharides on cytotoxicity protein synthesis and metabolism of DON in porcine hepatocytes and Kupffer cell enriched hepatocyte cultures, *Toxicol Lett.*, 2009, **189**, 121-129
2. A. L. Capriotti, P. Foglia, R. Gubbiotti, C. Rocchia, R. Samperi, A. Lagana, Development and validation of a liquid chromatography/atmospheric pressure photo-ionization-tandem mass spectrometric method for the analysis of mycotoxins subjected to commission regulation (EC) No. 1881/2006 in cereals, *J. Chromatog. A*, 2010, **1217**, 6044–6051
3. Fakhrunnisa, M. H. Hasmhi, A. Ghaffar, Seed-borne mycoflora of wheat, sorghum and barley, *Pakistan J. Bot.*, 2006, **38**, 185–192
4. P. M. Oliveira, A. Mauch, F. Jacob, D. M. Waters, E. K. Arendt, Fundamental study on the influence of Fusarium infection on quality and ultrastructure of barley malt *Int. J Food Microbiol.*, 2012, **156**, 32–43
5. A. Vaughan, T. O. Sullivan, D. V. Sinderen, Enhancing the microbiological stability of malt and beer, *J. I. Brewing*, Rev. 2005, **111**, 355–371
6. J. W. Bennett, M. Klich, Mycotoxins, *Clin. Microbiol. Rev.* 2003, **16**, 497–516
7. P. Havlová, K. Lancová, M. Vánová, J. Havel, J. Hajslová, The effect of fungicidal treatment on selected quality parameters of barley and malt, *J Agric Food Chem.*, 2006, **4**, 1353-60
8. B. Skrbic, A. Malachová, J. Zivancev, Z. Vepríková, J. Hajslová, Fusarium mycotoxins in wheat samples harvested in Serbia: A preliminary survey. *Food Control*, 2011, **22**, 1261-1267

- 1
2
3
4 9. H. P. Van Egmond, R. C. Schothorst, M. A. Jonker, Regulations relating to
5
6 mycotoxins in food: perspectives in a global and European context, *Anal.*
7
8 *Bioanal. Chem.* 2007, **389**, 147–157
- 9
10 10. F. Fung, R. F. Clark, Health effects of mycotoxins: A toxicological overview,
11
12 *J. Toxicol. Clin. Toxicol.* 2004, **42**, 217–234
- 13
14 11. Y. Ueno, Trichothecenes: Chemical, Biological and Toxicological Aspects,
15
16 *Elsevier, New York, USA*, 1983, **59**, 1-5
- 17
18 12. R. W. Coppock, B. J. Jacobsen, Mycotoxins in animal and human patients,
19
20 *Toxicol Ind Health.*, 2009, **10**, 637-655
- 21
22 13. C. P. Wild and Y. Y. Gong, Mycotoxins and human disease: a largely ignored
23
24 global health issue, *Carcinogenesis*, 2010, **31**, 71-82
- 25
26 14. P. Zollner, D. Berner, J. Jodlbauer, W. Lindner, Determination of zearalenone
27
28 and its metabolites a- and b-zearalenol in beer samples by high-performance
29
30 liquid chromatography-tandem mass spectrometry, *J. Chromatog. B* 2000,
31
32 **738**, 233-241
- 33
34 15. . *European Mycotoxins Awareness Network* <http://www.mycotoxins.org>
- 35
36 16. M. Plotan, C. T. Elliott, C. Frizzell, L. Connolly, Estrogenic endocrine
37
38 disruptors present in sports supplements. A risk assessment for human health,
39
40 *Food Chem.*, 2014, **159**, 157-165
- 41
42 17. A. Bergman, J. Heindel, S. Jobling, K. A. Kidd, and T. Zoeller, (Eds.). State
43
44 of the science of endocrine disrupting chemicals. *An assessment of the state of*
45
46 *the science of endocrine disruptors prepared by a group of experts for the*
47
48 *United Nations Environment Program and World Health Organization*, 2012
49
50
51
52
53
54
55
56
57
58
59
60

- 1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60
18. R. Hampl, J. Kubátová, L. Starka, Steroids and endocrine disruptors—
History, recent state of art and open questions *J Steroid Biochem Mol
Biol*, 2014, **14**, 960-760
 19. J. Rubert, C. Soler, R. Marin, K. J. James, J. Manes, Mass spectrometry
strategies for mycotoxins analysis in European beers, *Food Control*, 2013, **30**,
122-128
 20. R. Romero-Gonzalez, J. L. Martinez-Vidal, M. M. Aguilera-Luiz and A.
Garrido Frenich, Application of conventional solid-phase extraction for
multimycotoxin analysis in beers by ultrahigh-performance liquid
chromatography-tandem mass spectrometry, *J. Agric. Food Chem.*, 2009, **57**,
9385-9392
 21. A. Desmarchelier, S. Tessiot, T. Bessaire, L. Racault, E. Fiorese, A. Urbani,
C WC, P. Cheng, P. Mottier, Combining the quick, easy, cheap, effective,
rugged and safe approach and clean-up by immune-affinity column for the
analysis of 15 mycotoxins by isotope dilution liquid chromatography tandem
mass spectrometry, *J. Chromatogr. A*, 2014, **1337**, 75-84
 22. M. Vaclavikova, S. MacMahon, K. Zhang, T. H. Begley, Application of
single immunoaffinity clean-up for simultaneous determination of regulated
mycotoxins in cereals and nuts, *Talanta*, 2013, **117**, 345-351
 23. E. Beltran, M. Ibanez, T. Portolisa, C. Ripollis, J. V. Sancho, V. Yusu, S.
Marvn, F. Hernandez, Development of sensitive and rapid analytical
methodology for food analysis of 18 mycotoxins included in a total diet study,
Anal. Chim. Acta, 2013, **783**, 39– 48

- 1
2
3
4 24. J. Rubert, J. Manes, K. J. James, C. Soler Application of hybrid ion trap-high
5 resolution mass spectrometry to the analysis of mycotoxins in beers, *Food*
6 *Addit. Contam.*, 2011, **28**, 1438-1446
7
8
9
10 25. F. Al-TaHER, K. Banaszewski, L. Jackson, J. Zweigenbaum, D. Ryu, and J.
11 Cappozzo, Rapid Method for the Determination of Multiple Mycotoxins in
12 Wines and Beers by LC-MS/MS Using a Stable Isotope Dilution Assay, *J.*
13 *Agric. Food Chem.*, 2012, **10**, 2378-2384
14
15
16
17 26. M. Tamura, A. Uyama, and N. Mochizuki, Development of a multi-mycotoxin
18 analysis in beer-based drinks by a modified QuEChERS method and ultra-
19 high-performance liquid chromatography coupled with tandem mass
20 spectrometry, *Anal. Sci.*, 2011, **27**, 629-635
21
22
23
24 27. O. Vendl, F. Berthiller, C. Crews, R. Krska, Simultaneous determination of
25 deoxynivalenol, zearalenone, and their major masked metabolites in cereal-
26 based food by LC-MS-MS, *Anal Bioanal Chem*, 2009, **395**, 1347-1354,
27
28
29
30 28. H. Mine and M. Merdivan, Development of new dispersive liquid-liquid
31 microextraction technique for the identification of zearalenone in beer, *Anal*
32 *Methods*. 2012, **4**, 4129-4134
33
34
35
36 29. N. C. Maragou, E. Rosenberg, N. S. Thomaidis, M. A. Koupparis, Direct
37 determination of the estrogenic compounds 8-prenylnaringenin, zearalenone, a-
38 and b-zearalenol in beer by liquid chromatography-mass spectrometry, *J.*
39 *Chromatog. A*, 2008, **1202**, 47-57
40
41
42
43 30. T. Bertuzzi, S. Rastelli, A. Mulazzi, G. Donadini, A. Pietri, Mycotoxin
44 occurrence in beer produced in several European countries, *Food Control*,
45 2011, **22**, 2059-2064
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

- 1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60
31. Q. Wu, C. Wu, C. Wang, X. Lu, X. Li and Z. Wang, Sensitive determination of cadmium in water, beverage and cereal samples by a novel liquid-phase microextraction coupled with flame atomic absorption spectrometry, *Anal. Methods*, 2011, **3**, 210-216
32. M. Tajbakhsh and M. Helalizadeh, H Faraji Validation and optimization of a liquid-phase microextraction method for trace analysis of BTEX in water samples, *Anal. Methods*, 2012, **4**, 3372-3380
33. R. E. Rivas, I. Lopez Garcia and M. Hernandez-Córdoba, Microextraction based on solidification of a floating organic drop followed by electrothermal atomic absorption spectrometry for the determination of ultratracés of lead and cadmium in waters, *Anal. Methods*, 2009, **2**, 225-230
34. Q. Zhou and Y. Gao, Determination of polycyclic aromatic hydrocarbons in water samples by temperature-controlled ionic liquid dispersive liquid-liquid microextraction combined with high performance liquid chromatography, *Anal. Methods*, 2014, **6**, 2553-2559
35. M-W. Shu, M-I Leong, M-R Fuh and S-D Huang, Determination of endocrine-disrupting phenols in water samples by a new manual shaking-enhanced, ultrasound-assisted emulsification microextraction method, *Analyst.*, 2012, **9**, 2143-2150
36. Y. Abdollahzadeh, Y. Yamini, A. Jabbari, A. Esrafilí and M. Rezaee, Application of ultrasound-assisted emulsification microextraction followed by gas chromatography for determination of organophosphorus pesticides in water and soil samples, *Anal. Methods*, 2012, **4**, 830-837

- 1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60
37. P. Zhang, Lu Hu, R. Lu, W. Zhou and H. Gao, Application of ionic liquids for liquid–liquid microextraction, Mini Review, *Anal. Methods*, 2013, **5**, 5376-5385
38. X. Yan, D. Wu, H. Meng, L. Hao, K. Ding and, Y Guan, Further investigation of array capillary in-tube solid-phase microextraction of trace organic pollutants in water samples, *Anal. Methods*, 2013, **6**, 750-757
39. Z. H. Yang, Y. Liu, Y. L. Lu, T. Wu, Z. Q. Zhou, D. H. Liu, Dispersive suspended microextraction, *Anal. Chim. Acta*, 2011, **706**, 268-274
40. M. Kaykhai and M. H. Ghalehno, Rapid and sensitive determination of fluoride in toothpaste and water samples using headspace single drop microextraction-gas chromatography, *Anal. Methods*, 2013,**5**, 5622-5626
41. N. P. Petridis, V. A. Sakkas, T. A. Albanis, Chemometric optimization of dispersive suspended microextraction followed by gas chromatography–mass spectrometry for the determination of polycyclic aromatic hydrocarbons in natural waters, *J. Chromatog. A*, 2014, **1355**, 46-52
42. E. Perrez-Torrado, J. Blesa, J. C. Molto, G. Font, Pressurized liquid extraction followed by liquid chromatography-mass spectrometry for determination of zearalenone in cereal flours, *Food Control*, 2010, **21**, 399-402
43. L. K. Sorensen and T. H. Elbaek, Determination of mycotoxins in bovine milk by liquid chromatography tandem mass spectrometry, *J. Chromatogr. B*, 2005, **820**, 183-196
44. S. Endo, A. Pfennigsdorf and K. U. Goss, Salting-out effect in aqueous NaCl solutions: trends with size and polarity of solute molecules, *Environ. Sci. Technol.*, 2012, **46**, 1496-1503

Table 1 Analysis of different type commercial beers by the DSME method using LC-MS (n=3)

Sample	Added ($\mu\text{g kg}^{-1}$)	Found ($\mu\text{g kg}^{-1}$)	Recovery (%)
Pilsner 1	–	N.D	N.D
	20.0	17.4 ± 0.2	87%
Pilsner 2	–	N.D	N.D
	20.0	18.4 ± 0.2	92%
Pilsner 3	–	N.D	N.D
	20.0	17.8 ± 0.3	89%
Lager 1	–	N.D	N.D
	20.0	18.2 ± 0.3	91.2%
Lager 2	–	N.D	N.D
	20.0	17.2 ± 0.1	86%
Ale 1	–	N.D	N.D
	20.0	18.8 ± 0.2	94%
Ale 2	–	N.D	N.D
	20.0	17.6 ± 0.2	88%

Legends of figures

Fig. 1 LC–MS chromatograms of a) direct analysis of degassed beer sample, b) analysis of degassed beer sample after dilution (1:5), c) analysis of degassed blank beer sample after dilution (1:5) and subjected to DSME, d) analysis of degassed beer sample after dilution (1:5), and subjected to DSME (spiked with $10 \mu\text{g kg}^{-1}$ ZON)

Fig. 2 Effect of extraction time on the efficiency of DSME

Fig. 3 Comparison of the extraction recoveries attained with different toluene volume

Fig. 4 Effect of pH on the extraction of ZON

Fig. 5 Extraction yields (%) of three different concentrations of salinity

Fig. 1

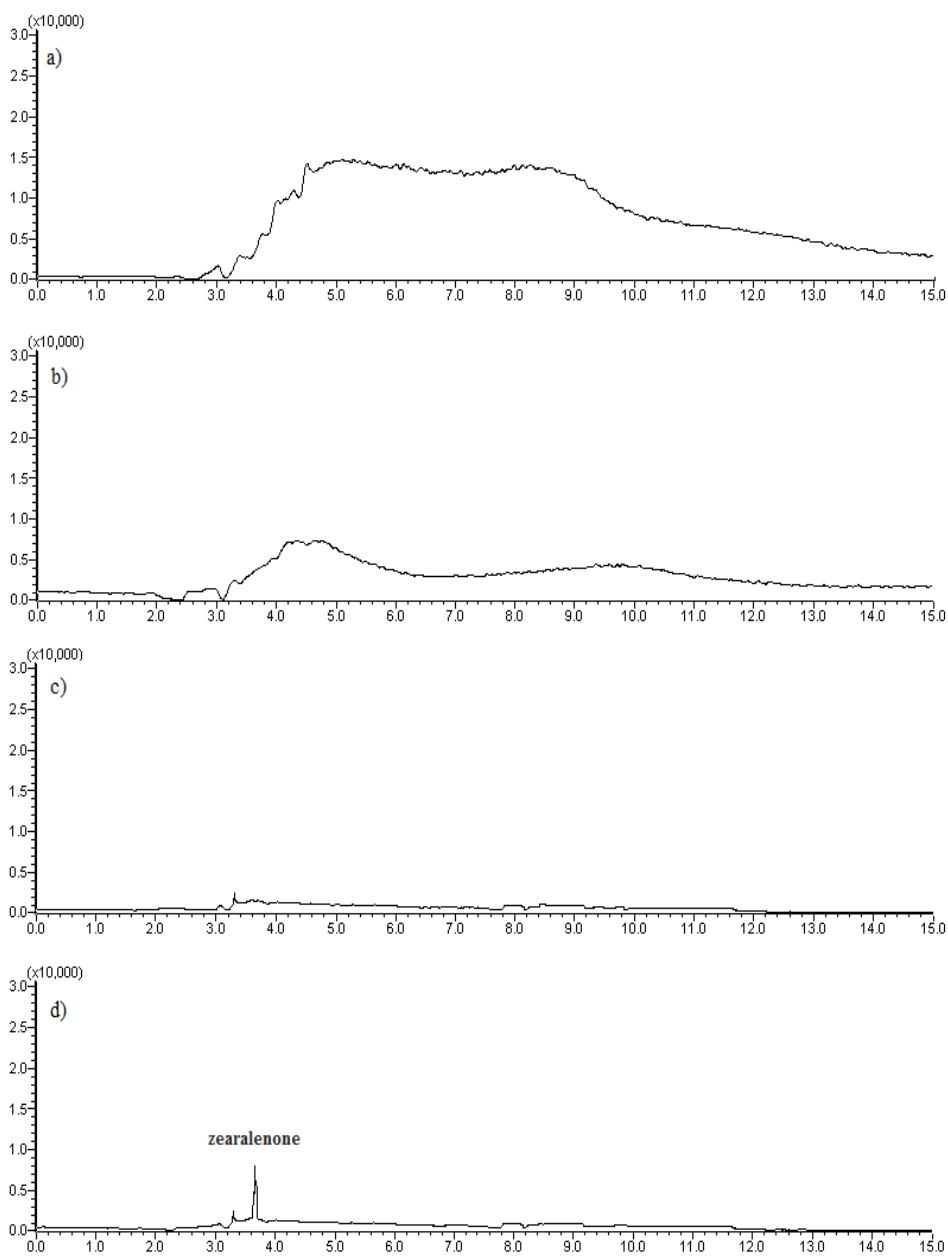


Fig. 2

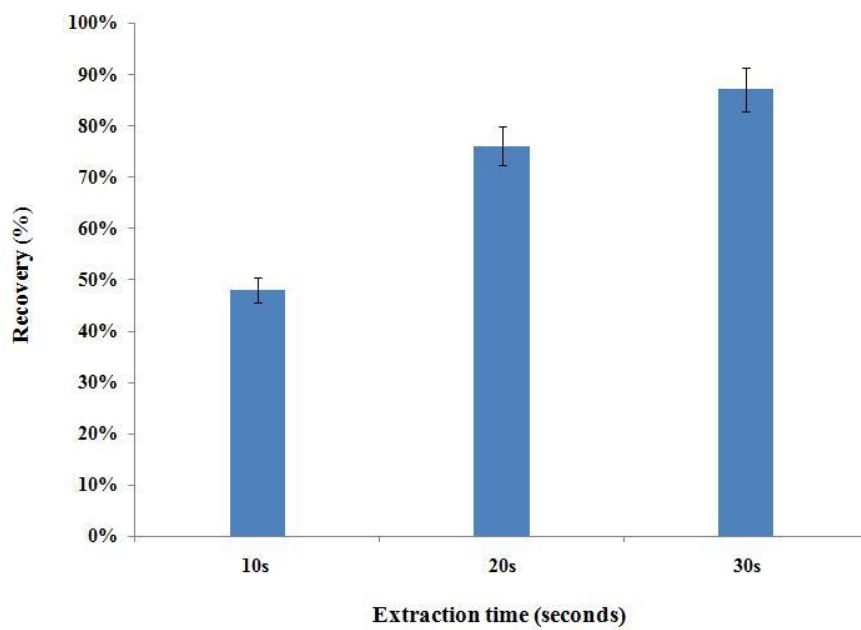


Fig. 3

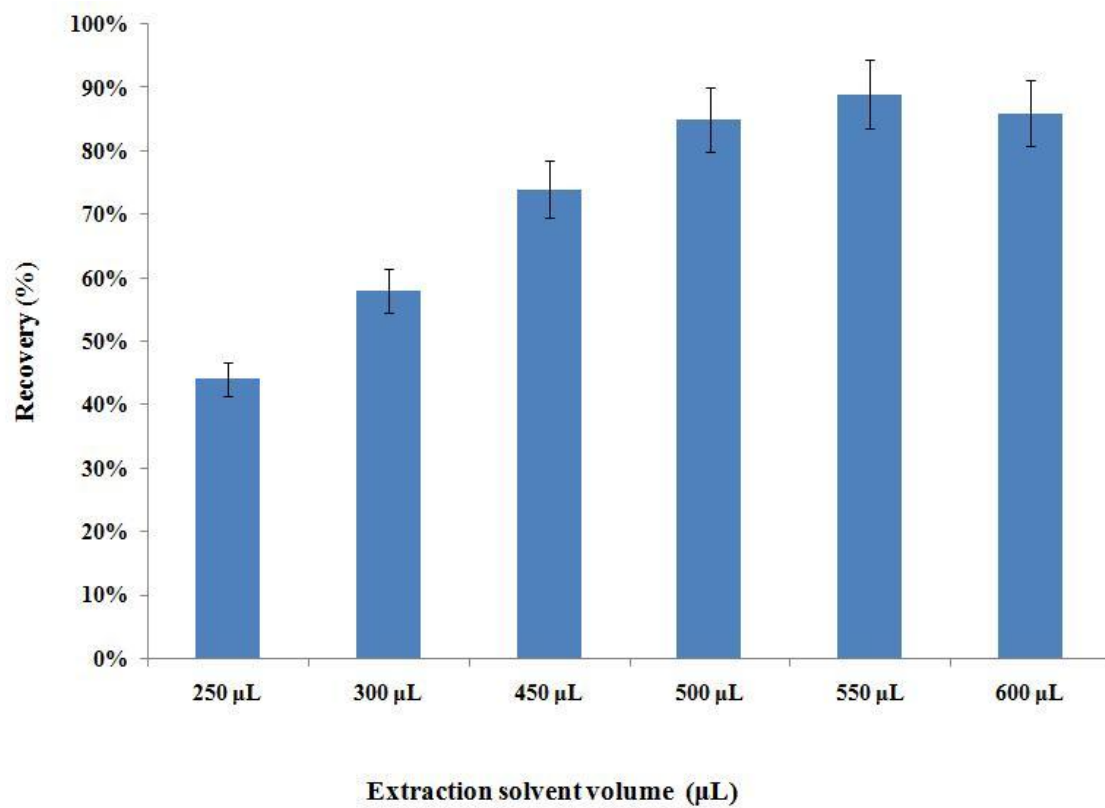


Fig. 4

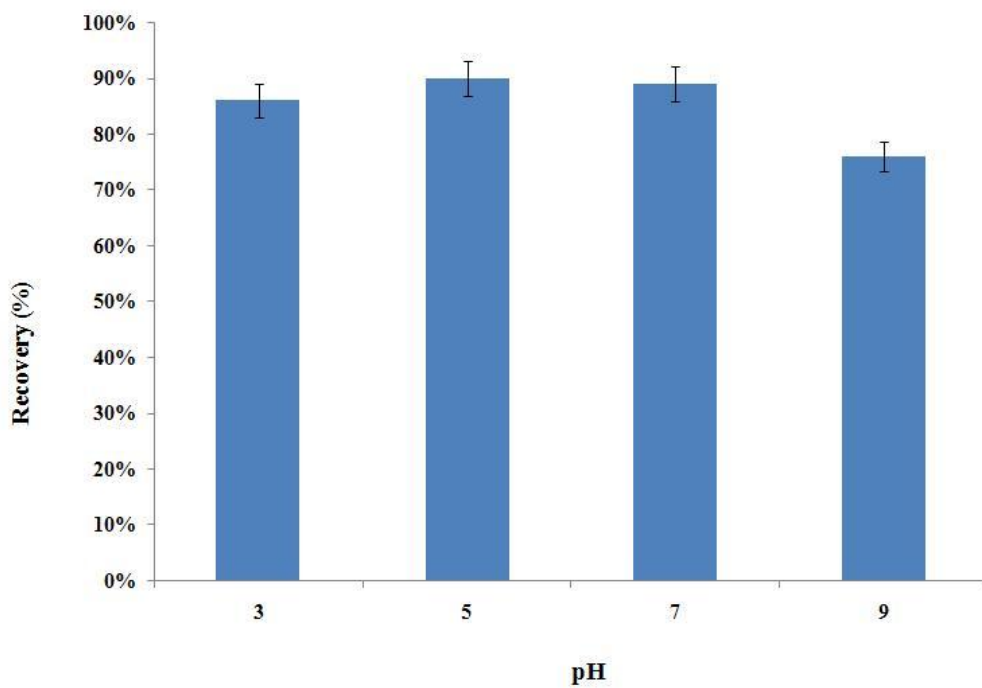


Fig. 5

