



**Optical Methods for Sensing and Imaging of Oxygen:
Materials, Spectroscopies and Applications**

Journal:	<i>Chemical Society Reviews</i>
Manuscript ID:	CS-REV-01-2014-000039.R1
Article Type:	Review Article
Date Submitted by the Author:	04-Feb-2014
Complete List of Authors:	Wang, James; University of Regensburg, Analytical Chemistry Wolfbeis, Otto; University of Regensburg,

Review:**Optical Methods for Sensing and Imaging of Oxygen:
Materials, Spectroscopies and Applications****Xu-dong Wang and Otto S. Wolfbeis***

Abstract. We review the current state of optical methods for sensing oxygen. These have become a powerful alternative to electrochemical detection and in the process of replacing the Clark electrode in many fields. The article (with 688 refs.) is divided into main sections on direct spectroscopic sensing of oxygen, on absorptiometric and luminescent probes, on polymeric matrices and supports, on additives and related materials, on spectroscopic schemes for read-out and imaging, and on sensing formats (such as waveguide sensing, sensor arrays, multiple sensors and nanosensors). We finally discuss future trends and applications and summarize the properties of the most often used indicator probes and polymers. A Supporting Information (with 381 refs.) gives a selection of specific applications of such sensors in medicine, biology, marine and geosciences, in intracellular sensing, aerodynamics, industry and biotechnology, among others.

Institute of Analytical Chemistry, Chemo- and Biosensors,
University of Regensburg, D-93040 Regensburg, Germany.
E-mail: otto.wolfbeis@ur.de; Fax: +49(0)941 943 4064;
Tel: +49(0)941 943 4065



Xu-dong Wang, born in 1985, received his Ph.D. degree in Chemistry from Xiamen University (Xiamen, China) in 2011. He was an Alexander von Humboldt fellow in the group of Prof. Wolfbeis and is currently working at the Karlsruhe Institute of Technology. His research interests include the design of optical chemical and biosensors, nanosensors and molecular probes, developing novel (bio)sensing schemes, in novel (nano)-materials and methods, and their applications to biological and chemical analysis. He has authored or coauthored more than 20 articles in the past five years, and his current *h*-index is 13 (as per Jan. 2014).

Otto S. Wolfbeis was a Full Professor of Analytical and Interface Chemistry at the University of Regensburg from 1995 to 2012. He has authored numerous papers on optical (fiber) chemical sensors, fluorescent probes, labels and assays, on nanomaterials for use in sensing schemes, and in spectroscopic methods including fluorescence (lifetime) imaging. He has acted as the (co)organizer of several conferences related to fluorescence spectroscopy (MAF) and to chemical sensors and biosensors (Eurotrode). His current *h*-index is 73. He is one of the 10 curators of *Angewandte Chemie* and the editor of two other journals. Also see: www.wolfbeis.de.

Contents

1. Introduction	4
2. A Look Back	7
3. Methods for Direct Spectroscopic Sensing of Oxygen	9
4. Sensing Oxygen Using Absorptiometric Probes	11
4.1. Hemoglobin and Myoglobin as Optical Probes for Oxygen	11
4.2. Molecular Absorptiometric Probes for Oxygen	12
4.3. Methods Based on the Oxidative Power of Oxygen	13
4.4. Inorganic Chromogenic Materials	17
5. Oxygen as a Quencher of Luminescent Probes	18
6. Luminescent Probes for Oxygen	21
6.1. Organic Probes	21
6.1.1. Polycyclic Aromatic Hydrocarbons (PAHs)	21
6.1.2. Fullerenes	25
6.1.3. Room Temperature Phosphorescent Organic Probes	26
6.2. Metal-Ligand Complexes	31
6.2.1. Ruthenium(II) Complexes	31
6.2.2. Iridium(III) Complexes	40
6.2.3. Osmium and Rhenium Complexes	46
6.2.4. Lanthanide Complexes	49
6.2.5. Porphyrins and Metalloporphyrins	51
6.2.5.1 Conventional Metalloporphyrins	51
6.2.5.2 Metalloporphyrins with large Q-band absorption and NIR emission	53
6.2.5.3 Water-soluble Metalloporphyrins	56
6.2.5.4 Functionalized Metalloporphyrins	57
6.2.5.5 Metalloporphyrins that Undergo Two-Photon Excitation	57
6.2.5.6. Metalloporphyrins for Sensors with Visual (Bare-Eye) Read-out	58
6.2.6. Other Metal Complex-Based Probes for Oxygen	65
6.3. Intrinsically Luminescent Nanomaterials as Probes for Oxygen	69
6.4. Multiple Emitter Probes	69
6.5. Various Other Probes for Oxygen	71
7. Polymeric Matrices (Hosts) and Supports	74
7.1. General Considerations	74
7.2. Permeability, Solubility, and Diffusion of Gases in Polymer	76
7.3. Organic Host Polymers	79
7.3.1. Organic Homopolymers	80
7.3.1.1. Silicone Rubber	80
7.3.1.2. Ethyl Cellulose	81
7.3.1.3. Poly(vinyl chloride)	81
7.3.1.4. Polymethacrylates	82
7.3.1.5. Polystyrene	82
7.3.1.6. Other Homopolymers	83
7.3.1.7. Hydrophilic Polymers	84
7.3.2. Organic Copolymers (including fluoropolymers and mesoporous materials)	86
7.3.3. Organic Nanofilms	90
7.4. Inorganic Supports and Matrix Materials	91
7.4.1. Silicates (including Sol-Gels)	91
7.4.2. Organically Modified Silicates (Ormosils)	94
7.4.3. Organic Polymers with Inorganic Fillers	97
7.4.4. Metals and Metal Oxides as Solid Supports	98

7.5. Nanoparticles	98
7.5.1. Organic Materials for Nanosensors	99
7.5.2. Silica-Based Materials for Nanosensors	101
8. Additives, Coatings, and Other Components	102
8.1. Plasticizers	103
8.2. Scattering particles	103
8.3. Photostabilizers	104
8.4. Optical Isolations.....	105
8.5. Materials Acting as Inert Solid Supports.....	106
9. Spectroscopies and Readout Schemes in Luminescent Sensors.....	106
9.1. Sensing Based on the Measurement of Luminescence Intensity	106
9.2. Sensing Based on the Measurement of Luminescence Decay Time.....	107
9.2.1. Frequency Domain Fluorometry	108
9.2.2. Time domain fluorometry and RLD	110
9.2.3. Dual Lifetime Determination (DLD).....	111
9.3. Sensing Based on Measurement of Luminescence Resonance Energy Transfer.....	112
9.4. Sensing Based on Measurement of Fluorescence Anisotropy.....	113
9.5. Sensing Based on Two-Photon Excitation	114
9.6. Sensing Based on Chemi- and Bioluminescence.....	115
9.7. Other Luminescent Sensing Schemes for Oxygen.....	117
9.8. Multiple Sensing	118
9.8.1. Multiple Sensing Using Single Probes	118
9.8.2. Multiple Sensing Using Two or More Luminescent Probes.....	119
9.9. Referenced Sensing and Imaging.....	124
9.10. Specific Aspects of Luminescent Imaging of Oxygen	129
9.10.1. Intensity based Imaging	130
9.10.2. Lifetime based Imaging	133
10. Selectivity, Sensitivity, and Effects of Temperature	134
10.1. Selectivity and Interferences	134
10.2. Sensitivity, Precision, and Limits of Detection.....	135
10.3. Effects of Temperature and Other Parameters.....	137
10.4. Low-Level Oxygen Sensors.....	139
11. Sensing Formats	141
11.1. Planar Sensors	141
11.2. Fiber Optic and Other Waveguide Sensors.....	141
11.3. Evanescent Wave and Plasmonic Sensing.....	145
11.4. Distributed Sensing of Oxygen	150
11.5. Microparticle-Based Sensing	151
11.6. Microsensors (not Fiber Optic, not Microparticle-Based).....	153
11.7. Dendrites and Nanosensors.....	155
11.7.1. Dendrites	155
11.7.2. Fluorescent Probes Incorporated into Nanoparticles.....	158
12. Applications	160
13. Conclusions and Outlook	161
14. List of Acronyms	165
15. References	166

1. Introduction

Almost all living organisms utilize oxygenⁱ for energy generation and respiration. Discovered by Joseph Priestley in the 1770s, this event was elected as one of the top 100 greatest science achievements because of the significance of oxygen in science and technology.¹ Oxygen is involved in practically all forms of living organism and played a major role in evolution.² Adult humans metabolize ~200 g of oxygen per day. Human beings can live up to 1 month without food, up to 2 weeks without water, but not longer than maximally 10 min without supply of oxygen. It therefore does not come as a surprise that the (analytical) chemistry of oxygen plays a major role in biology and medicine. Sensing (i.e., continuous monitoring) of oxygen has attracted particular attention as can be seen from the numbers of respective references. A search for "oxygen sensor" in SciFinder yields ~8670 references, and ~27500 references are found that contain the concept "oxygen sensor" (search performed on August 1st, 2013).

There are four major methods known for determination of oxygen. These are (a) the classical Winkler titration,³ (b) electroanalytical,⁴ (c) pressure-based, and (d) optical methods. The latter can be subdivided in numerous single methods that range from direct spectroscopy to indicator based methods. Each method has its specific merits and applications.⁵⁻⁷ The Winkler method is precise but does not enable continuous sensing. The Clark electrode⁸ is state of the art for the determination of oxygen at room temperature and in small volume. It works both in gaseous and fluid samples (whole blood included). Clark electrodes can be applied at temperatures up to ~200 °C. They perform excellently but consume the analyte and are interfered by gases such as chlorine, ozone or nitrogen oxides. The quantitation of oxygen in (car) exhaust gases (which is challenging in view of the high temperatures of such samples) is performed with solid-state electrically conducting sensor materials to provide a feedback signal in catalytic converters. This so-called lambda probe (for a review, see ref.⁹) was developed by the Bosch company during the late 1960s and is based on a zirconia ceramic coated on both the exhaust and reference sides with a thin layer of platinum to form a solid-state electrochemical fuel cell, where CO (if present) is oxidized by oxygen to form CO₂. Both heated (>300 °C) and (less often) nonheated forms are known. The sensor does not actually measure oxygen concentration, but rather the difference between the amount of oxygen in the exhaust gas and the amount of oxygen in supply air.

Optical oxygen sensors have become attractive in the past four decades because of features such as (a) the lack of oxygen consumption during measurements; (b) full reversibility; (c) good precision and accuracy; (d) the possibility of remote sensing using optical fibers; (e) the ease of miniaturization (down to the size of nanosensors); (f) the option of performing non-invasive measurements; and (g) the highly attractive feature of enabling imaging of oxygen both over large

ⁱ Note: we use the common term "oxygen" for the more correct but less usual term "dioxygen".

areas and on a micrometer scale. The success of optical sensors for oxygen is corroborated by the number of companies that are manufacturing respective instrumentation, examples being Presens (probably the largest; www.presens.de); Centec (www.centec.de); Ocean Optics, Inc. (www.oceanoptics.com); Oxysens, Inc. (www.oxysense.com); Finesse, Inc. (www.finesse.com); PyroScience (www.pyro-science.com); and Hach-Lange (www.hach-lange.de), to mention the larger ones. In the medical field, OptiMedical Systems, Inc. (www.optimedical.com) and Terumo (www.terumo-cvs.com/products/) probably are the largest.

There is some confusion in terms of definitions and terminology. We refer to a sensing element as a material composed of both an oxygen-sensitive probe (OSP) and a proper (polymer) matrix that acts as a host or support (see **Table 1**). A complete sensor device will also incorporate a readout unit to give an electrical (or digital) signal. Ideally, the following ("Cambridge") sensor definition applies: A sensor is a (small) instrumental system capable of (optically) detecting and quantifying a physical or chemical parameter over time and with high specificity (under the given circumstances). The vast majority of sensors for oxygen consists an oxygen sensitive probe, a polymer or matrix for hosting the oxygen sensitive probe, a read-out (electronic) system, and a device to process data. A discussion on the definitions for sensors, probes and labels was presented.¹⁰


Table 1. Terms used in this review, and respective definitions. Several definitions are ambiguous.

Term	Definition
(Optical) probe; indicator; molecular probe	A molecule that displays an optical effect with a specific analyte such as oxygen (or pH, or a metal ion). Whatever their name: they are not sensors. OSP is used here as an acronym for oxygen-sensitive probe.
Polymer, host, binder, matrix, paint	These terms relate to a polymer that hosts a probe (an indicator), for example an OSP. The choice of the polymer (and any additives) is a very critical step in sensor development.
Sensor chemistry, "stimulus-responsive polymer"	A combination of materials (typically a polymer containing a probe and, possibly, additives) that enables continuous chemical sensing of oxygen; can be manufactured in various formats such as in the form of a sensor film, of sensor nanoparticles, or as a coating on (or at the distal end of) an optical waveguide.
Sensor cocktail; ink; paint	A <i>solution</i> of a sensor "chemistry" in an appropriate solvent.
Sensor	The definition of a sensor as a "miniaturized device that can deliver real-time and on-line information on specific parameters" was used for decades until organic chemists spoiled it by referring to molecules, probes, indicators and the like as "sensors". Sensors are devices according to this definition, and they are produced by the millions. One may differentiate between physical sensors (such as those for temperature, pressure, acceleration) and chemical sensors (such as for pH, oxygen, methane, NO _x , glucose). Sensors incorporate a readout system and are expected to provide a digital signal.

In addition to direct spectroscopic methods (see **Section 3**), oxygen can be sensed via absorptiometric probes, i.e. those that undergo a color change on exposure to oxygen (see **Section 4**), but the vast majority of optical sensors for oxygen is based on luminescent probes (**Section 6**) that are contained in an oxygen-permeable polymer (**Section 7.1**). **Figure 1** shows a cross-section of a typical planar luminescent sensor for oxygen. It consists of a solid but optically transparent

support and a polymer matrix (referred to as the "sensing layer") permeable to oxygen that contains a quenchable probe. Optionally, a black cover (the so-called "optical isolation", see **Section 8.4**) is placed on top to prevent sample luminescence originating from blood or (plant) tissue, for example, to interfere. The sensor layer is illuminated on one side and luminescence is collected at the same side. The sample to be analyzed is in contact with the sensing element on the other side, in **Figure 1** placed on top.

Figure 1. Schematic cross-section of a typical planar luminescent sensor layer (not to scale)

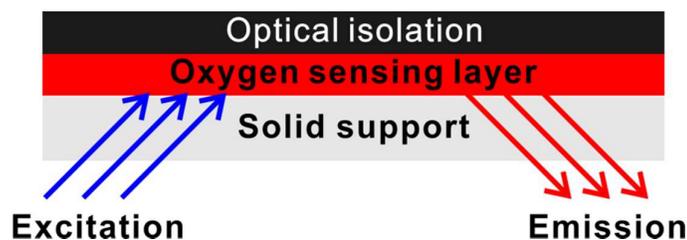

Most oxygen-sensitive probes (OSPs) are used either in surface-absorbed or in polymer-dissolved form. In their pioneering work back in 1931, Kautsky and Hirsch¹¹ used probes such as tryptaflavin adsorbed on a silica gel solid support. The use of solid (polymeric) supports not only separates the OSP from the sample, but also can increase the QY of an OSP (due to rigidization) and may also result in the formation of long-lived phosphorescent emissions resulting from long-lived triplet states.¹²⁻¹⁵ This is quite beneficial because long decay times increase quenching efficiency.^{16,17} The immobilization of OSPs in matrices offers additional advantages such as improved diffusion and permeability¹⁷ so that sensitivity and detection range can be adjusted. In addition, the sensing element can be used for a long time, and the polymer matrix can shield the OSPs from interferences by other quenchers. In fact, some polymers have excellent permeation selectivity. On the other hand, organic polymers and (metal) organic probes tend to decompose at temperatures < 200 °C. There is a vast variety of luminescent and other methods to readout the effects caused by oxygen (see **Sections 4, 5 and 9**)

Once an appropriate material has been identified for use in a sensing element, it can be applied in various formats as outlined in **Section 11**. The materials are often applied in the form of a (viscous) solution in a (usually organic) solvent, the so-called "sensor cocktail", which then may be deposited on a mechanical support such as a thin film of an inert and transparent polymer to form a sensor film (or sensor layer, or "paint"). Following solvent evaporation, the resulting (solid) sensor element then can be interrogated by various kinds of optical spectroscopies. The cocktail may also be deposited at the tip of an optical fiber, on another kind of waveguide, or even be incorporated into its core or cladding. This will result in so-called fiber optic or waveguide sensors. If placed on the clad of an optical fiber in intervals over certain distance, so-called distributed sensors are obtained that can be interrogated by time-resolved methods of spectroscopy. They allow for

continuous and spatially resolved sensing of oxygen along an optical fiber. Sensor chemistries also may be shaped in the form of (nano)particles as will be outlined in **Section 11.6**. If the sensor material is deposited on the whole object or area of interest, 2-dimensional imaging of oxygen becomes feasible, for example in so-called pressure-sensitive paints that are used to measure the air pressure on cars and aircrafts, to sense oxygen in (cancerous) skin, to monitor photolytic or photosynthetic processes, or the consumption of oxygen in fuel cells.


In this review, we summarize the state of the art in optical sensing and imaging of oxygen. More specifically, we review sensors based on the measurement of absorbance, reflectance and luminescence (including fluorescence, phosphorescence, bioluminescence and chemiluminescence.) The spectral range spans the ultraviolet, visible, and near infrared. On the other hand, X-ray fluorescence, X-ray photoelectron spectroscopy, and electron paramagnetic resonance are not covered. Several reviews^{5-7, 18-25} and book chapters²⁶⁻²⁸ related to aspects of optical oxygen sensing have appeared, but they usually cover a narrow field or a limited time frame. Some earlier but useful work has resided hidden for a long time but is cited here.

Papkovsky et al.²⁹ have summarized applications of optical oxygen sensors in biosciences, with a focus on enzymatic assays, respiration, food and microbial safety, bioreactors and fluidic chips. We summarize the subject as a whole and are presenting a comprehensive and hopefully clear blueprint for optical sensing of oxygen. It covers the state of the art from the first reported optical sensing scheme for oxygen¹¹ to the present. Quaranta et al.³⁰ have summarized the wealth of metal ligand complexes that is available for use in optical sensing of oxygen.

2. A Look Back

Quenching of luminescence by oxygen and other quenchers was long known but not understood until Stern & Volmer derived their famous equation.³¹ Optical continuous sensing of oxygen probably started back in the 1930's when Kautsky and Hirsch reported^{11, 32} that the room-temperature phosphorescence (RTP) of certain dyes adsorbed on silica particles is quenched by even trace quantities of oxygen. Sensing beads were prepared by soaking silica gel particles with a solution of dyes such as tryptaflavine or fluorescein. They were then dried and placed in a flow-through cell schematically shown in **Figure 2**. RTP was monitored using a fluorometer and it was found that even ppm quantities of oxygen gas (equivalent to a pO_2 of as little as 0.5×10^{-3} Torr) were detectable. The effect was found to be fully reversible within 1 – 2 s. The device led to the discovery of the Kautsky effect, i.e. the delay in the production of oxygen following the illumination of a leaf. This is a good example on how chemical sensor technology can impact other kinds of science.

Figure 2. Schematic of the first continuous sensor for oxygen. A sample gas containing oxygen (S) is passed via valve H_1 over silica beads dyed with a quenchable probe for oxygen and placed in a small flow-through cell. The room temperature phosphorescence of the beads on the bottom is quenched by even traces of oxygen and was monitored with a simple fluorometer.

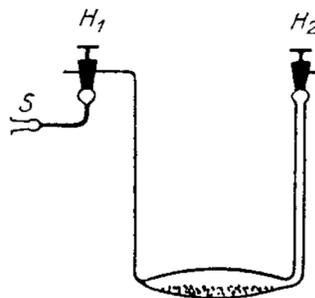

This RTP method was later applied by others^{33,34} to monitor oxygen in seawater. The first fluorescent sensor system was described by Bergman³⁵ in 1968 and comprised a UV light source, an oxygen-sensitive fluorescent layer composed of porous glass (or a thin film of polyethylene) soaked with the oxygen-sensitive probe fluoranthene, and a photodetector. Thus, it contained all the elements of a modern optical sensor. Oxygen quenches the fluorescence of fluoranthene, and intensity served as the analytical information. The system responds to oxygen at levels above 1 Torr.

The milestone paper by Lakowicz and Weber³⁶ in 1973 on the potential of probing structural fluctuations in proteins with oxygen-quenchable probes also revealed, for many, the potential of such probes for sensing oxygen in unknown (gaseous or fluid) samples. A device similar to the one of Bergman was described, a few years later, in a patent.³⁷ It also mentions the possibility of using a radioactive source (rather than a UV light source) to excite fluorescence. In 1974, Hesse³⁸ described a device that appears to have been the first fiber optic chemical sensor. An oxygen-sensitive chemistry was placed in front of a fiber optic light guide through which exciting light was guided. The fluorescence emitted was guided back through either the same fiber, or through other bundle of fibers. The system is based on the measurement of either fluorescence intensity or fluorescence decay time, both of which are affected by oxygen. In 1975 and 1976, Lübbers and Opitz^{39,40} described instruments capable of monitoring oxygen or carbon dioxide. They first referred to it as an "optrode" (by lingual analogy to the electrode), and later as an "optode" (οπτιχος οδος ; Greek for "optical way"). They also were the first to apply an oxygen sensor as a transducer in an enzyme-based biosensor.⁴¹

The fiber optic oxygen sensor described by Peterson et al.⁴² in 1984 was a milestone in optical fiber sensor technology for use in medicine. The sensor was used to monitor oxygen in the blood of a ewe *in vivo*. A planar sensor for oxygen based on the covalent immobilization of the probe pyrene on a porous glass support and with milliseconds response time was reported in the same year.⁴³ A chemiluminescence (CL) based sensor for oxygen was reported by the Seitz group⁴⁴ that exploits the CL produced in the reaction of oxygen with an electron-rich ethylene. The AVL company has filed a patent⁴⁵ that describes oxygen sensitive materials based on polycyclic aromatic hydrocarbons

dissolved in a film of poly(vinyl chloride) containing a plasticizer. Deposited on an acrylate glass, and covered with microparticles of ferric oxide act as optical isolations to prevent interferences by the intrinsic fluorescence of a biological matter, they can be used to monitor oxygen in bioreactors, in blood samples and in breath gas.

The first dual sensor (for simultaneous determination of oxygen and the inhalation narcotic halothane) was reported⁴⁶ in 1985. It is based on dynamic quenching of the fluorescence of the probe decacyclene in silicone rubber by both oxygen and halothane. Interferences by oxygen are taken into account by a second sensor layer covered with polytetrafluoroethylene (which is impermeable to halothane) and responds to oxygen only. Halothane concentrations can be calculated with the help of an extended Stern-Volmer relation (**Section 9.8.1**). The probe is practically specific for the two analytes, since other gases present in inhalation gases or blood do not interfere.

Quenchable ruthenium ligand complexes for use in optical oxygen sensing were reported⁴⁷ in 1986. Ruthenium tris(bipyridyl) was adsorbed onto silica gel and placed in a silicone membrane. Ruthenium probes with better QY and known from the work of Alford et al.⁴⁸ were applied as OSPs by Demas and coworkers⁴⁹ in 1987. Such complexes have decay times in the order of a few microseconds. The first article⁵⁰ on luminescence decay time-based sensing of oxygen appeared in 1988. The Wilson group⁵¹ introduced a quenchometric scheme for oxygen based on the phosphorescence of metalloporphyrins in aqueous solution and bound to albumin, later to dendritic molecules. Both intensity and decay time were measured as a function of oxygen partial pressure. (Metallo)porphyrin-based sensor membranes were developed in the 1980s by the Gouterman group⁵² that are suitable for phosphorescent sensing of oxygen, and a strong patent was published⁵³ that covers pressure-sensitive paints based on the same effect. A 2-volume book that appeared in 1991 gives an account of the work on fiber optic chemical sensors and biosensors.²⁷ The first reliable fiber optic oxygen microsensors were introduced⁵⁴ in 1995. A look back on the history of optical chemical sensor technology up to the year 2000 has been published.⁵⁵

3. Methods for Direct Spectroscopic Sensing of Oxygen

Molecular oxygen has two main absorption bands in its UV-vis spectrum, one deep in the UV, the other at 760 nm which is very weak. It also has an intrinsic emission peaking at 1270 nm. Geddes et al.⁵⁶ in 1992 monitored breath gas oxygen via its UV absorption at 145 nm. Not unexpectedly, water vapor and carbon dioxide (and probably many other species) interfere. The weak absorption lines at ~760 nm can be exploited to sense oxygen in high concentration or if large penetration lengths can be accomplished such as in astronomy.^{57, 58} This direct spectroscopic method also enables monitoring of ¹⁶O¹⁸O and ¹⁶O¹⁷O isotopes, which provides valuable data with

respect to the composition of the protoatmosphere via the trapped gas in the polar ice. The oxygen line absorption also was used to monitor oxygen in harsh environment at high temperature, such as exhaust gas in combustion engines or burners.⁵⁹ Respective instrumentation requires high-power lasers, long optical pathways (~ 100 m), and highly sensitive detectors.

Oxygen also was sensed directly by employing gas correlation absorption spectroscopy using multimode diode lasers.⁶⁰ A diode laser was applied that has an emission spectrum that overlaps the oxygen absorption lines of the absorption band at 760 nm. A detection limit of 700 ppm was achieved with good accuracy (2%) and linearity ($R^2 = 0.999$). For comparison, measurements of ambient oxygen were also performed by tunable diode laser absorption spectroscopy (TDLAS) employing a vertical cavity surface emitting laser. The sensor is based on correlation spectroscopy and displays good stability, is easy to use, and instrumentation is more simple than in the TDLAS-based instrument. On the other hand, it can only be applied to gaseous samples.

In rather related work, wavelength modulation absorption spectroscopy of oxygen at 760.241 nm was applied⁶¹ to determine its concentration in the 0 – 100% range at ambient pressure. TDLAS was applied, and the oxygen absorption was scanned with a tunable laser, while wavelength modulation spectroscopy was used to obtain the harmonics (1f, 2f, 3f and 4f) of the oxygen absorption signal. The modulation parameters such as the modulation voltage, modulation frequency, reference phase, time constant of lock-in amplifier, the tuning voltage, and the tuning frequency were optimized to obtain the harmonics of high amplitude and narrow half width. Oxygen concentrations were measured by the following three methods: (i) Using only the 2nd harmonic; (ii) using the 2nd and 4th harmonics; and, (iii), using the 1st and 2nd harmonics.

Direct sensing of oxygen via the intrinsic luminescence of singlet oxygen ($^1\Delta$) with its peak at 1270 nm also has been reported,^{62, 63} but emission is weak (QY in water is 9.3×10^{-7}).⁶⁴ Sensing of *liquid* oxygen at high pressure and at high flow rates is challenging. Dynamic quenching of the luminescence of OSPs is very strong at high oxygen concentrations as they occur in fluids, and therefore is not the method of choice to sense *liquid* oxygen. Here, Raman spectroscopy is superior, as shown by Tiwari et al.⁶⁵ who designed an integrated fiber optic Raman sensor that employs a frequency-doubled 532-nm cw Nd:YAG laser as the light source. A standard spectrometer can be used to collect the Raman spectrum of *liquid* oxygen or its mixtures with liquid nitrogen (such as cryogenic fluids used in the supercritical environment of rocket engines). The method is safe, but background luminescence can interfere.

While direct spectroscopic sensing of oxygen appears to be much easier in terms of handling and effort, one has to face the fact that bulky and expensive instrumentation is needed to obtain a practical sensor because the UV absorbance and the emission of singlet oxygen are weak. This makes such approaches less economical and much less convenient. In addition, omnipresent substances such as water and carbon dioxide may interfere. Thus, these approaches cannot be

recommended for practical uses except for very special situations.

4. Sensing Oxygen Using Absorptiometric Probes

Such sensors are based on the use of optical probes that undergo a chromogenic reaction with oxygen (mostly certain leuco dyes) or where oxygen causes a color shift (such as in the hemoglobin-oxyhemoglobin system). Many of these sensors respond irreversibly. Readout usually is performed by reflectometry, not by absorptiometry. The law of Kubelka & Munk relates the intensity of reflectance at a specific wavelength to the concentration of the absorber dye formed with oxygen in a chromogenic reaction:

$$c = \frac{S \cdot (1 - R_{diff})^2}{2 \epsilon_R \cdot R_{diff}} \quad (\text{eq.4.1})$$

Here, c is the concentration of the dye, R_{diff} is the intensity of reflected light (maximally 1), ϵ_R is the molar decadic coefficient of reflectivity (almost identical with the molar absorbance ϵ in the Lambert-Beer law), and S is a parameter that is specific for the surface of the sensor film and depends on its microstructure, material, and scattering properties.

Chromogenic (irreversible) test stripes are widely used in semiquantitative analysis, for example to determine pH values, blood glucose, or nitrate in water samples. The reflectivity of a sensing area typically is read out via small (mostly hand-held) reflectometers comprising (i) a first LED light source operated at the analytical wavelength, (ii) a second LED operated at a wavelength where reflectivity does not change with analyte concentration; (iii) a photodiode detector that alternatively (in ms intervals) reads the reflectivity of the colored and non-colored area; (iv) a power source (usually a battery); (v) an electronic circuit that amplifies the signal of the photodiode; and (vi) a microprocessor that converts the amplified signal into comprehensive information such as a concentration unit.

Absorbance/reflectance-based oxygen sensors can be divided into three sub-groups, viz. (a) those using biological OSPs (such as hemoglobin), (b) those using synthetic oxygen binders (such as certain cobalt complexes), and (c) those using redox chemistry (using the oxidative power of oxygen). The probes can undergo a change in absorbance (intensity) or peak wavelength, or both. All suffer from the fact that they can readily detect the presence of oxygen, sometimes even quantify it, but that they are hardly capable of detecting an *increase* in the concentration of oxygen over time, and – even less easily – a *decrease*. The various absorptiometric (reflectometric) methods will be discussed in the following.

4.1. Hemoglobin and Myoglobin as Optical Probes for Oxygen

Hemoglobin and myoglobin, when binding oxygen, undergo a large spectral change. Seitz et al.⁶⁶ constructed an optical oxygen sensor by immobilizing deoxyhemoglobin on a cation exchange resin. The *Soret* absorption band of deoxyhemoglobin shifts to longer wavelengths when exposed to oxygen to form oxyhemoglobin. The ratio of reflectances at 405 and 435 nm serves as the analytical information. This ratiometric method is suitable to measure oxygen partial pressure from 20 to 100 Torr. However, the response time is long (around 3 min). This kind of oxygen sensor has several limitations: (1) The useful lifetime is short because of irreversible degradation of hemoglobin; (2) response to oxygen partial pressure is nonlinear and not readily described mathematically; (3) the sensor is interfered by gases that can also bind to hemoglobin (such as carbon monoxide), and by pH, because the affinity of hemoglobin for oxygen is a function of pH and ionic strength.

Myoglobin was used in another absorbance based oxygen sensor. It reversibly binds dissolved oxygen to form oxy-myoglobin whose absorption spectrum is quite different. Valentine et al.⁶⁷ used the effect by encapsulating myoglobin in a sol-gel glass matrix to prepare a reversible sensor for dissolved oxygen (DO). The absorbances at 418, 432 and 436 nm change linearly on exposure to dissolved oxygen, but the signal change is small. McCurley et al.⁶⁸ also encapsulated myoglobin in a sol-gel, reduced it to deoxy-myoglobin by bathing the gel in a dithionite solution, and exposed the sensor gel to DO upon which deoxy-myoglobin is oxidized to oxy-myoglobin. A fluorescent dye, brilliant sulfaflavine, was added to the system. It absorbs light at 430 nm and emits radiation at 520 nm. The excitation light for the dye is passed through the myoglobin-containing gel. The emission of the fluorescent dye changes as the absorbance of the myoglobin at 430 nm changes in response to DO. Carbon monoxide, HCN and SO₂ are likely to interfere in both methods.

4.2. Molecular Absorptiometric Probes for Oxygen

Several cobalt-organic compounds are capable of reversibly binding molecular oxygen. The respective absorption spectra change with oxygenation. Baldini et al.⁶⁹ screened a large number of oxygen carriers and found some of them to be viable optical probes, while others do not give large signal changes or have slow response. The bis(histidinato)cobalt(II) complex [Co(His)₂] is well suited. Its absorbance at 408 nm increases strongly with oxygen concentration. An optical fiber sensor was designed that consisted of a polymeric hollow-fiber membrane filled with a solution of Co(His)₂. However, its response time is quite long (up to 30 min) and the color of Co(His)₂ depends on pH. In order to improve performance, the probe was absorbed on thin layer chromatography plates and then coated with silicone rubber.⁷⁰ If exposed to an oxygen free environment, the color of the plate changes markedly and can be detected with bare eyes. The effect is reversible and the response time is shorter.

The oxygen carrier cobalt(II)-tetrakis(o-pivalamidophenyl)porphinato (CoP) has a unique structure in that it possesses a cavity for reversibly binding oxygen and a coordination site with a

nitrogenous ligand to further increase the affinity for oxygen. It was used⁷¹ along with two methacrylate-co-vinylimidazole copolymers (one partially fluorinated) to reversibly bind oxygen. The oxygenated complex exhibits a maximum absorbance at 547 nm and an isosbestic point at 536 nm. The sensor was used to determine oxygen in the 1–1000 hPa range, has a short response time (5 – 15 s) and good long-term stability, but is interfered by humidity. Tsuchida et al.⁷² synthesized polymers with nitrogenous ligands capable of coordinating CoP. They found that the binding of oxygen by CoP is strongly affected by the kind of polymer depending on their nitrogen ligands. The CoP coordinated to fluorinated polymers is well suited to sense oxygen in water.

The iridium complex $\text{Ir}(\text{CO})\text{Cl}(\text{PPh}_3)_2$ undergoes a reversible(!) reaction with oxygen to form $\text{Ir}(\text{CO})\text{Cl}(\text{O}_2)(\text{PPh}_3)_2$ (which however is photosensitive), and this accompanied by substantial changes in the spectral properties of the complex.⁷³ Various other oxygen-carriers (mainly complexes of cobalt, iron, manganese, platinum and iridium for potential use in oxygen transport) have been described.^{74, 75} The *Vaska* iridium complex also has been studied⁷⁶ but was found to react too slowly and not to be sensitive enough.

An optical fiber sensor^{77, 78} utilizes the change in the contact charge-transfer absorption (CCTA) of *N,N*-dimethyl-*p*-toluidine in the presence of oxygen. The probe has a broad CCTA band in the UV/Vis region whose absorbance increases with increasing oxygen concentration. The band disappears if oxygen is removed. There is a linear relationship between absorbance and oxygen concentration in accordance with the Beer-Lambert law. Response is reversible, and the sensitivity is higher at shorter wavelength. However, the slope decreases at high oxygen levels, and elemental chlorine and SO_2 interfere like in many other sensors for oxygen.

Absorption is not limited to transitions from the ground state to an excited state. The group of Amao⁷⁹⁻⁸¹ used the transient triplet-triplet absorption of the excited states of the fullerenes C_{60} and C_{70} to sense oxygen. The efficiency of this absorption depends on $p\text{O}_2$. The method of triplet-triplet (excited state) absorption was also applied to platinum(II) complexes such as PtOEP,⁸² PtTFPP,⁸² and certain zinc porphyrins.⁸³ The photoacoustic response⁸⁴ also may be utilized to measure transient absorptions and thus to optically sense oxygen.

4.3. Methods Based on the Oxidative Power of Oxygen

Oxygen is a powerful oxidant that can convert certain colorless species into colored products, or can cause a color change of a dye due to oxidation.⁸⁵ The reduced ("leuco") form of Methylene Blue (MB) is colorless and quickly converted back to blue MB by oxygen, a reaction that occurs at room temperature.²⁰ In some cases it has been reported that the chromogenic reaction can be reversed by applying reducing agents or by electroreduction. Early work⁸⁶ involved the use of leuco MB to determine low levels ($<100 \mu\text{g L}^{-1}$) of oxygen in power station water. Iron(II) and copper(II) ions

interfere and must be removed before analysis by passing the water sample through a cation-exchange column. Others⁸⁷ have determined dissolved oxygen using photoreduced leuco phenothiazine dyes. Perlman & Linschitz⁸⁸ have tested numerous oxygen indicators (by placing it in or on irreversibly responding test stripes) for use in packaging, examples including the leuco forms of MB. The leuco forms were generated by reaction with (strongly smelling) mercaptoethanol and deposited on filter paper, silica particles, nitrocellulose and other solid supports. Other leuco forms include those of thionine and methyl violet. Blue MB can be chemically reduced back to the leuco form with reducing agents such as dithionite, ferrous compounds, sulfite, ascorbic acid, or glucose in alkaline medium.

The Mitsubishi Gas Company has patented^{89,90} and commercialized respective chromogenic oxygen indicators for use in food packaging (called the "Ageless Eye", **Figure 3**). It is also based leuco MB which was chemically reduced using glucose in alkaline medium. The exposure of the Ageless Eye to oxygen can oxidize the leuco form into the blue form.

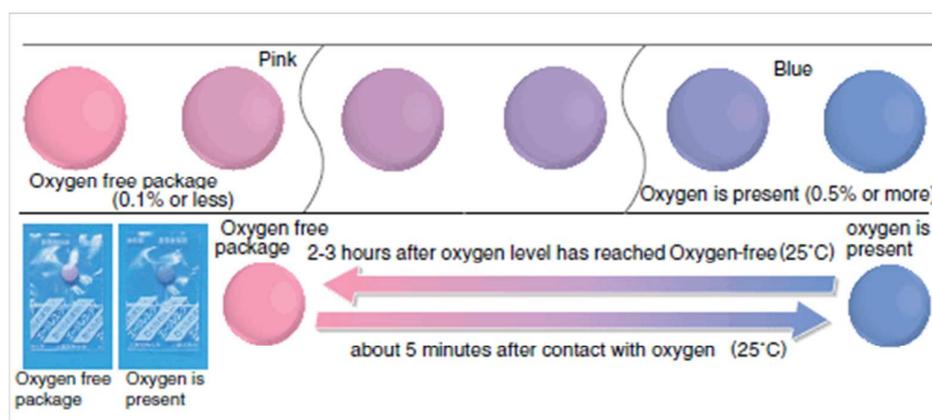



Figure 3. The color of Ageless Eye oxygen indicator changes from pink to blue in the presence of oxygen.

MB can also be reduced by irradiation with UV light.^{91,92} Re-usable oxygen-sensitive inks were obtained by immobilizing TiO_2 , the sacrificial electron donor triethanolamine (TEOA), and MB in a hydroxyethyl cellulose (HEC) matrix. The resulting blue TiO_2 -TEOA-MB-HEC film bleaches under UV irradiation, but not under ambient room light or visible light. If exposed to oxygen, the colorless film is irreversibly oxidized to give a blue film which again can be converted into its colorless form by UV irradiation for about 2.5 min. This cycle can be repeated at least 5 times. The working principle of this scheme is based on the formation of electron-hole pairs in the TiO_2 semiconductor particles by UV light. The holes oxidize the TEOA, and the photogenerated electrons reduce the MB dye into its leuco form. Its irreversibility and reusability make this intelligent ink useful for applications in packed food technology. The feature of generating the leuco form by UV irradiation after packing simplifies the process, because handling of leuco dyes is complicated as it requires the complete absence of oxygen. Semiconductors such as ZnO or SnO_2 can also be applied for preparing the UV activated oxygen indicator film, but TiO_2 works best. The

response time can be adjusted by varying the thickness of the sensor film or by using polymers with different oxygen permeability.⁹³

The same group⁹⁴ later modified the hydrophilic, water-soluble and cationic indicator MB into a hydrophobic MB by exchanging the anion. The hydrophobic indicator is soluble in organic solvents and the blue ink can be printed direct on food package. A film made of TiO₂, ion-paired MB, glycerol and a polymer named zein (a prolamine-type of protein found in maize) loses its color rapidly (<30 s) upon exposure to UVA light and remains colourless in an oxygen-free atmosphere, returning to its original blue color upon exposure to air. In the latter step the rate of color recovery is proportional to the level of ambient oxygen and the same film can be UV-activated repeatedly (see **Figure 4**). This makes the ink useful for direct printing on food package.

Figure 4. Sensor film printed with an ink made of titanium dioxide, Methylene Blue, glycerol and a polymer. The film loses its color upon exposure to UV light but becomes blue again on exposure to air. (Reprinted with permission from ref.⁹⁴ Copyright Royal Society of Chemistry, 2008)

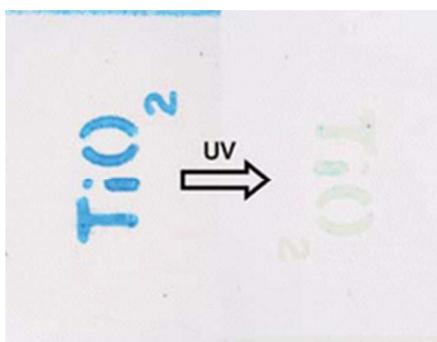

A photoinitiator was employed^{95,96} to photoreduce MB via UV irradiation in an acrylate matrix. Irradiation generates radicals that reduce blue MB to its leuco form. Simultaneously, the acrylate monomer is polymerized to form a solid film that contains the indicator. This kind of photoreduction is reversible due to the cyclic processes of (1) oxidation on air, and (2) reduction in an oxygen-free environment under UV light. However, the cycles come to an end once the photoinitiator is consumed. The absorption of MB decreases with the number of cycles on air because of partial photo-decomposition of the indicator.

The polyviologens form a class of less sensitive irreversible oxygen indicators.⁹⁷ They also can be reduced to colorless forms by exposure to UV light via mediated reduction in the presence of EDTA and TiO₂ as described above for MB. However, the rate for reduction is much faster than in case of MB. The reduced (leuco) forms of thionine and 2,2'-dicyano-1,1'-dimethylviologen were seen to persist until the oxygen concentration exceeded 2.3% and 4.0%, respectively. It was also reported⁹⁸ that beige-colored anthraquinone β -sulfonate can be reduced to its red phenolate dianion by sodium thiosulfate in alkaline solution. When contacted with oxygen, the red color turns back to beige. This was suggested to serve as a time label to monitor the freshness of food. The rate of the color change can be adjusted by varying the chemical composition of the polyacrylate matrix.

In a fiber optic oxygen sensor for medical use, a viologen indicator is employed that becomes a

strong absorber after brief stimulation with UV light. Its color thereafter disappears over time, and the rate of indicator return to transparency is proportional to the local concentration of oxygen.⁷⁹ Absorbance is monitored with a red LED and a photodiode, and data are processed by a dedicated processor. The solid-state sensor system has a performance that compares to existing oxygen techniques and may be applied to both in vitro and in vivo oxygen assays.

Colorimetric oxygen-sensitive films also can be based on the redox chemistry of 2,6-dichlorophenolindophenol (2,6-DCPIP) in the presence of fructose and an organic base in a thin film of ethyl cellulose.⁹⁹ The respective sensor film is colorless in the absence of oxygen, but turns to blue in its presence at levels of 30 Torr and above. This represents a simple means for colorimetric detection of oxygen. The oxidized form of 2,6-DCPIP can be reduced by fructose in presence of a base contained in the polymer film. This "sensor" reversibly responds to oxygen over 10 nitrogen-oxygen switching cycles within a period of ~ 5h. At oxygen pressures between 0 and 50 Torr, there is a linear relationship between the absorbance of the film and oxygen partial pressure, and response occurs within 20 s.

The leuco forms of indigo and thioindigo were immobilized¹⁰⁰ in poly(ethylene glycol), polyurethane hydrogel and poly(styrene-co-acrylonitrile) respectively, in order to adjust the permeability for oxygen and, thus, the response time. The reduced (leuco) forms are better soluble and almost colorless. On interaction with oxygen, a vivid blue or red color develops as can be seen in **Figure 5**. The color change can be used to irreversibly detect oxygen. The sensor can be reversed (converted into the faintly colored form) by treatment with dithionite. In one further approach,¹⁰¹ an indicator system was described that gives a color changes that result from the fact that the interaction of oxygen with the indicator layer causes a change in the local pH value. Numerous indicators were presented.

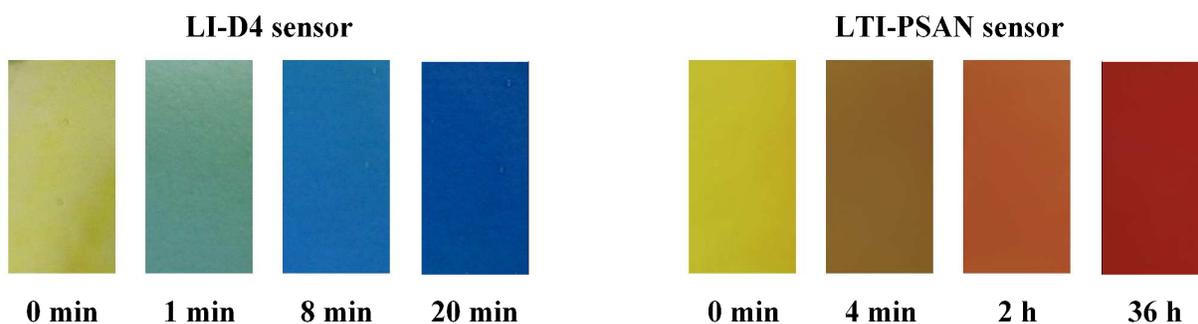


Figure 5. *Left:* Real color images of an irreversibly responding test stripe (consisting of a solution of leuco indigo in a polyurethane hydrogel; LI-D4) for oxygen over a time interval of 20 min. *Right:* Real color images of an irreversibly responding test stripe (consisting of a solution of leuco thioindigo in poly(styrene-co-acrylonitrile); LTI-PSAN) for oxygen over a time interval of 36 h. (Reprinted from ref.¹⁰⁰ with permission from Elsevier)

The same sensor material also was filled into thin capillaries that can serve as opto-chemical

timers. The "clock" is started by opening one end of the capillary filled with leuco (thio)indigo.¹⁰² The length of the colored section increases over time as oxygen diffuses in. By using different molecular weight poly(ethylene glycols), one can control the permeability for oxygen and, thus, the time frame of the clock. Significant properties of several absorption-based irreversible probes for oxygen are summarized in **Table 2**. The above technologies also are covered by various patents.

Table 2. Selected irreversibly acting chromogenic probes for oxygen along with respective polymeric supports and color transitions

Dye/Matrix	Color transition	Comments	Ref.
Phenothiazine	Colorless → Blue	Photoreduced at pH above 9.5; Methylene Blue is best because of its stability; the Methylene blue-EDTA solution undergoes more than 150 cycles of photoreduction-air oxidation without apparent degradation of the dye.	87
Malachite Green (leuco form) on silica gel	Colorless → Greenish blue	Oxidized by reactive oxygen species only.	32
2,6-Dichloroindophenol (leuco form) in ethyl cellulose	Colorless → Blue	Indicator is co-immobilized with fructose and base; reversible response with short response time (~20 s); applicable to oxygen partial pressure between 0 – 50 Torr, linear relationship between absorbance and oxygen partial pressure.	99
Methylene blue (leuco form), TiO ₂ and triethanolamine in hydroxyethyl cellulose	Colorless → Blue	UV-activated reusable ink; irreversible oxygen response but regenerable via UV irradiation; regeneration time 2.5 min; stable in oxygen-free environment; colorimetric determination; response time adjusted via the thickness of the matrix or using polymers with different permeabilities.	91, 93, 103
Anthraquinone β-sulfonate in pHEMA	Red → Beige	Reduced form (dianion) is red; color fades into beige with oxygen; useful for fadable printed signs for food packaging	98
Indigo (leuco form) and PEG	Colorless → Blue	Reduced in basic solution with Na ₂ S ₂ O ₄ ; time frame adjusted by using different molecular weight PEG; fairly stable but undergoes some photobleaching under exposure to visible light; also used as a timer material; periods can be adjusted to up to 40 years.	100, 102
Thioindigo (leuco form) and PEG	Colorless → Red	Reduced in basic solution with Na ₂ S ₂ O ₄ ; the timer covered time frame could be adjusted by using different molecular weight PEG; fairly stable but undergoes some photobleaching on exposure to visible light.	100, 102
Polyviologens (leuco form), TiO ₂ , EDTA	Pale yellow → Purple	More quickly reduced than Methylene Blue under UV exposure; high anodic redox potential; suitable for oxygen at above 0.5%, even above 4% (the upper LOD for MB is 0.1% only).	97

4.4. Inorganic Chromogenic Materials

Butler and Ricco¹⁰⁴ coated optical fibers with nm-thin films of metals (such as nickel) and found that their reflectivity at 860 nm changes on exposure to oxygen as a result of the formation of a thin layer of an oxide. The film thickness also changes and so affects reflectivity. Instrumentation and techniques are simple and applicable to monitor the corrosion rates of metals. An oxygen sensor for

car exhaust gases¹⁰⁵ comprises a supported film of a heat-responsive inorganic sensing material having a light reflective surface which reversibly reacts with oxygen to form an oxide which causes a change in the reflectivity of the surface. The sensor also includes a temperature sensing means and a 3-way optical system.

5. Oxygen as a Quencher of Luminescent Probes

Most sensors for oxygen are based on the effect of the quenching of the luminescence (fluorescence or phosphorescence) of oxygen-sensitive probes (OSPs). The process involves dynamic collision between molecular (triplet) oxygen and the excited electronic state of the OSP and leads to a reduction of its intensity and decay time. Quenching often is accompanied by the formation of singlet oxygen. It is noted in this context that not a single sensor is known for singlet oxygen. However, several irreversibly responding molecular probes have been reported that can be used to quantify singlet oxygen.¹⁰⁶

The kinds of methods used in luminescence spectrometry vary to a large extent as will be briefly discussed in this section. The analytically responsive ("dynamic") range of a sensor material can be easily adjusted by (a) proper choice of the OSP (discussed in **Section 6**), (b) the matrix materials (discussed in **Section 7**), and (c) by various additives (**Section 8**). A discussion of the various read-out schemes and geometries of sensors will then be presented in **Section 9**.


Dynamic (collisional) quenching by oxygen is a photophysical (rather than a photochemical) process. It is fully reversible, does not alter the optical probe, and thus has no effect on its absorption spectrum. Rather, it leads to a drop in luminescence intensity and decay time.^{107, 108} The relationship between intensity (or decay time) and the concentration of oxygen ($[O_2]$) is reflected by the Stern-Volmer equation which, in its most simple form, reads as

$$F_0/F = \tau/\tau_0 = 1 + K_{SV}[O_2] \quad (\text{eq. 1})$$

where F_0 and F , respectively, are the fluorescence (luminescence) intensities of a probe in the absence and presence of oxygen, K_{SV} is the Stern-Volmer constant which is a function of the lifetime of the probe and the (polymeric) solvent, and $[O_2]$ is the concentration of oxygen in the sample. The term $[O_2]$ (a concentration) may be replaced by pO_2 , the partial pressure of oxygen, and the numerical value of K_{SV} and its unit obviously has to be different then.

In an ideal quencher system, there is a linear relationship between F_0/F (or τ_0/τ) and oxygen concentration as shown in **Figure 6**. Unfortunately, data for K_{SV} are given by authors in various units including inverse (partial) pressure, $(\text{ppm})^{-1}$, $\%^{-1}$, inverse molarity, and others. If data are given in $\%^{-1}$ or $(\text{ppm})^{-1}$ unit, the barometric pressure must be indicated.

Figure 6. Intensity plot of the quenching of luminescence intensity by oxygen, and respective Stern-Volmer plot.

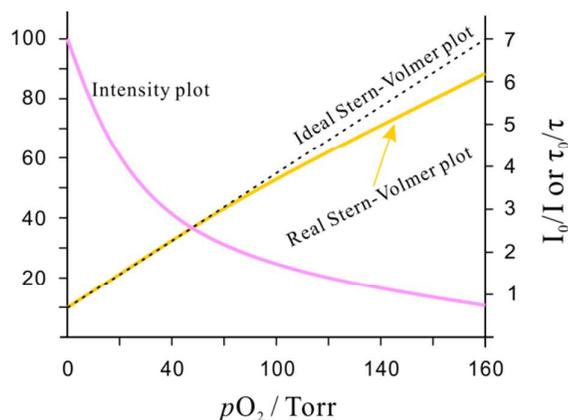

Stern-Volmer plots (SVPs) can be established by measurement of either luminescence intensity or decay time. However, luminescence intensity data can be adversely affected by a poor stability of the light source, variations in the efficiency of the transmission optics, drifts in detector sensitivity, leaching and photodecomposition of probes, inhomogeneous probe distribution, background luminescence and stray light. In order to correct for these effects, an inert reference fluorophore emitting at a different wavelength is often used. See **Section 9.9** on referenced sensing.

The Stern-Volmer constant determines the limits of detection (LODs) of a sensor. The LOD is governed by both the initial slope (K_{SV}) of the quenching plot and by the resolution of the instrument. Assuming a $\pm 0.1\%$ uncertainty in light intensity measurement (which is the lower limit and requires a well-thermostatted device), the detection limit is $0.003/K_{SV}$ (K_{SV} expressed in Torr^{-1} units and at a signal-to-noise ratio of 3). Phosphorescence based sensors, in contrast to fluorescent sensors, often have much larger K_{SV} values and therefore have much lower LODs.

Many SVPs of sensor films exhibit downward curvature as shown in **Figure 6**. This usually is indicating contributions by less efficient mechanisms of quenching. A general discussion of situations where both static and dynamic quenching occur can be found in respective textbooks.^{107, 108} Specifically for the situation of sensing oxygen, Demas et al.^{109, 110} have investigated the photophysics and photochemistry of the quenching by oxygen of several Ru(II) polypyridyl complexes in various polymers. Their results showed that downward curved SVPs originate from the heterogeneity of the microenvironment of the OSPs. They assumed that the Ru(II) polypyridyl complex exists in (at least) two distinctly different environments, one being quenchable, the other either not being quenched at all, or being quenched at a very different rate. A two-site model^{110, 111} was introduced to fit the curved SVPs, which has been widely used ever since. In the conventional form, it reads as follows (**eq. 2**),

$$\frac{F}{F_0} = \frac{f_1}{1 + K_{SV}^1 \cdot [O_2]} + \frac{f_2}{1 + K_{SV}^2 \cdot [O_2]} \quad (\text{eq. 2})$$

where F and F_0 , respectively, are the fluorescence (or phosphorescence) intensities of the probe in

the presence and absence of oxygen, respectively, f_1 and f_2 the fractions of the total emission for each component, respectively (with $f_1 + f_2$ being 1), and K_{SV}^1 and K_{SV}^2 are the Stern–Volmer constants for each component. The equation may also be written in the lifetime form by replacing (F/F_0) for (τ/τ_0) .

It shall be reminded here that this model is sensitive to signals that contain contributions by stray light, ambient light and background luminescence. There are several reports on the literature where rather low values for K_{SV}^2 have been calculated, and where contributions from these two sources of error to the overall second quenching constant cannot be excluded. Stray light and background luminescence, but not ambient light, can be reduced – if not eliminated – if gating (time-resolved detection) is applied. Gating must not be confused with lifetime detection and is possible only if long-lived ($> 1 \mu\text{s}$) OSPs are used.

Another model was presented¹¹² that relies on the analysis of the multi-exponential luminescence decay of a luminophore, specifically of Ru(dpp), in various polymers. A fit with a sum of exponentials gives physically unreasonable dependences of the pre-exponential factors of the decay components on the oxygen pressure. This is clear evidence that the decay profile is the total of many single but different relaxation rates. A spatial disorder model can relate the distribution of relaxation rates to a distribution of different distances between the OSP and the sites of interaction in the polymer. The two models for multiple-site quenching have been applied to different situations. Generally, the two-site model is well-suited to describe quenching in heterogeneous systems, while the spatial disorder model better fits homogeneous systems. On the other side, the two-site model can also describe nonlinear quenching in homogeneous systems.^{113, 114}

Phosphorescence lifetime analysis also was accomplished with a quadratic programming algorithm that can provide information on the distributions of quenchers in heterogeneous systems.¹¹⁵ The method is based on decomposition of the data vector to a linearly independent set of exponentials and uses quadratic programming principles. Solution of the resulting algorithm requires a finite number of calculations (it is not iterative) and is computationally fast and robust. The algorithm has been tested on various simulated decays and for analysis of phosphorescence data of palladium(II) porphyrins with discrete distributions of lifetimes. The technique is recommended for resolution of the distributions of quencher concentration in heterogeneous samples, of which oxygen distributions in tissue is an important example. Improved calibration of phase-fluorometric oxygen sensors has been demonstrated on the basis of physical models,¹¹⁶ and the response of phase-fluorometric oxygen sensors can be modeled with respect to effects of temperature and operational requirements.¹¹⁷

6. Luminescent Probes for Oxygen

These form by far the largest group of oxygen-sensitive probes (OSPs). Kautsky and coworkers^{11, 16, 32} in the 1930s observed that both the phosphorescence and fluorescence of surface-adsorbed OSPs such as acriflavin, tryptaflavin, benzoflavin, safranin, chlorophyll, porphyrins and others are quenched by molecular oxygen. This effect was used to detect the formation of oxygen as a result of photosynthesis, and in turn led to the discovery of the Kautsky effect. After more than 80 years of development, numerous OSPs are available now,³⁰ with excitation and emission maxima ranging from the UV to the NIR, and with excited-state lifetimes ranging from a few nanoseconds to milliseconds if not seconds in case of phosphorescent probes.

Luminescent OSPs can be classified into four subtypes: (1) organic OSPs (mainly polycyclic aromatic hydrocarbons and fullerenes); (2) metal-ligand complexes (mainly transition metal-ligand complexes and metalloporphyrins); (3) luminescent nanomaterials; and (4) multiple emitters and related species. Absorption-based (non-luminescent) OSPs are not included in this part but were discussed in **Section 4**. Luminescence-based oxygen sensor technologies are covered by numerous patents which cannot be included here.

6.1. Organic Probes

6.1.1. Polycyclic Aromatic Hydrocarbons (PAHs)

Luminescent polycyclic aromatic hydrocarbons can be regarded as the first generation OSPs. As summarized in **Table 3**, almost all PAHs (except those carrying nitro groups or carbonyl groups and some fullerenes) are strongly luminescent and have natural lifetimes of up to 200 ns. This makes them very amenable to quenching by oxygen. Some display fairly good photostability. In 1939, Bowen and Norton¹¹⁸ reported on the quenching of the fluorescence of anthracene by oxygen in various solvents. However, the effect is small. Weil-Malherbe and Weiss¹¹⁹ in 1942 studied the response of several PAHs to oxygen and found that the fluorescence of 3,4-benzopyrene is completely quenched by oxygen and this effect is fully reversible. Bergman³⁵ in 1968 described an apparatus for the determination of atmospheric oxygen by measuring the intensity of the fluorescence of fluoranthene absorbed on porous glass or polyethylene. Oxygen acts as a quencher and can be detected in the 0 – 40 kPa range.

Decacyclene and benzo(g,h,i)perylene¹²⁰ have much better photostability. Decacyclene was converted into a silicone-soluble derivative by alkylation with *t*-butyl groups.¹²⁰ The resulting sensor film was used in a steam-sterilizable fiber waveguide sensor to monitor oxygen concentration in a bioreactor. The sensor layer was covered with a black layer that acts as an optical isolation to avoid interferences by the fluorescence of cellular matter. When immersed into a bioreactor, response times were 9 – 65 s, and the drift was -0.01 to -0.09% (signal loss per hour).

No effects of stirring were observed. Okazaki et al.¹²¹ have frequency-doubled the 780-nm emission of a semiconductor laser to obtain a 390 nm line with 50 nW intensity which is suitable to excite benzo(g,h,i)perylene. The beam was launched into a fiber which guided light to the sensing material (the indicator dissolved in silicone grease) placed at its end. A second fiber was used to collect fluorescence at 430 nm which depends on pO_2 in the 0 – 30% range at atmospheric pressure.

Perylenedibutyrate⁴² on polystyrene beads was used in the first fiber optic sensor for monitoring oxygen in blood. It is quite photostable and has excitation and emission maxima of 468 and 514 nm, respectively. Its fluorescence is strongly quenched by oxygen, thereby allowing a resolution of ± 1 Torr up to 150 Torr (20 kPa) of oxygen. A sensor was constructed that consisted of two thin fibers, one guiding blue excitation light to the dyed particles in a tubing at the common end of the two fibers, the other guiding scattered blue light and green fluorescence to a photodetector. The dyed polystyrene beads are contained in a 25- μm polypropylene tubing whose end was sealed with epoxy. The sensor measures the ratio of scattered blue light (F_0) and green fluorescence (F). An electronic circuit processes the blue and green signal intensities according to the following relationship:

$$pO_2 = (\text{gain})(F_0/F - 1)^m \quad (\text{eq. 3})$$

Note that this is the Stern-Volmer equation re-arranged with an exponent m added for curvature because plots are not linear. This relationship is an alternative to the mathematical models for non-linear SVPs as described in **Section 5**. This ratiometric method also can eliminate temperature effects and drifts resulting from photobleaching. Coronene on polystyrene,⁴² and coronene and diphenylanthracene in polydimethylsiloxane also were used¹²² but require more shortwave excitation wavelengths.

Pyrene and its derivatives, in contrast, have fairly good photostabilities, quantum yields of > 0.3 , and surprisingly long excited state lifetimes of up to 200 ns. They also display good sensitivity to oxygen and a low temperature coefficient at ambient temperatures. However, pyrene – like other PAHs – lacks good solubility in polymers and tends to aggregate.¹²³ Thus, pyrene derivatives bearing lipophilic side chains have been prepared to overcome these drawbacks.¹²⁴ The better water-soluble derivative pyrenebutyric acid has an absorption maximum at 355 nm, a monomer emission maximum at 396 nm, and another band peaking at $\sim 450 - 470$ nm which is attributed to the excimer. Its fluorescence lifetime is reported⁶ to be ~ 200 ns. The probe was used, in DMF solution,³⁹ in a device called "optode" or "optrode", and later was immobilized on glass.³⁸ In closely related work,¹²⁵ pyrenebutyric acid was chemically bound to controlled pore glasses, and the quenching by oxygen of its regular emission and its excimer emission was studied, also at -196 °C. Pyrenes later have been immobilized on various kinds of other supports.^{43, 126-133} Pyrene also was covalently immobilized, along with the enzyme glucose oxidase (GOx), on poly(vinyl alcohol)

enhanced (rather than quenched) by oxygen in exceptional cases. The fluorescence of dibenzanthracene in a poly(vinyl acetate) matrix is reported to undergo a 10% fluorescence enhancement on exposure to air compared to evacuated samples.¹³⁶ Similar results were obtained for other PAHs in PVA and other polymers.¹³⁷ Arguable explanations for the effect were given.¹³⁸ Another unusual finding is the observation that the fluorescence of the Förster resonance energy transfer (FRET) system formed between pyrene and perylene is much more strongly quenched than the fluorescence of each single component.¹³⁹ The ratio of the Stern-Volmer quenching constants between pyrene, perylene, and the FRET system is 165:12:520.

Photostable heterocyclic OSPs have been reported¹⁴⁰ with longwave excitation wavelengths between 465 and 566 nm, and emissions in the 511 – 652 nm range. Such probes can be excited with light emitting diodes (LEDs), and yield intense fluorescence, but they are suitable for higher pressures of oxygen only. Decacyclene (**Figure 7**) is an attractive visible-light excitable organic probe for oxygen sensing because it works well for ambient levels for oxygen. It can be photoexcited with (purple) LEDs, has a large Stokes' shift, and displays good photostability. Its absorption maximum is at 380 nm, but extends far into the visible and ends at around 480 nm. It was also used as a probe for simultaneous sensing of oxygen and halothane,⁴⁶ and in an oxygen transducer to sense glucose.¹⁴¹ Its poor solubility in apolar polymers (such as silicone) was overcome by alkylating it with tertiary butyl groups which renders decacyclene well soluble even in silicone rubber.¹⁴² This sensor was used for many years in clinical oxygen analyzers until it was replaced by certain ruthenium-type probes.

Strongly fluorescent derivatives of coumarin also were used as OSPs in oxygen sensors,^{143, 144} but they are not strongly quenched by oxygen. Thin-films of a substituted terfluorene¹⁴⁵ have a fluorescence that was found to be quickly quenched by oxygen due to its specific morphology. Fast response ($\ll 100$ ms), full reversibility and high efficiency are typical features. Sensitivity can be further enhanced up to 10-fold and 20-fold in amplified spontaneous emission and lasing action, respectively. A variety of other dyes was tested for use as OSPs. Excellent quenching by oxygen was observed²⁷ with the following fluorophores (the excitation/emission maxima given in brackets) when adsorbed on silica-based chromatographic plates: Acridine yellow (458/530 nm), perylene-tetracarboxylic acid N-alkylimide (PTAI) (495/555 nm) and Greengold (another perylene dye; 460/520 nm), and anthranilic acid (330/410 nm). In a typical experiment for quenching studies, PTAI is immobilized via established silyl reagent chemistry to give a sensing material that can be excited at 480-500 nm with blue LEDs. Response times are in the order of 1 s. The probe PTAI displays two emissions (with peaks at 540 and 575 nm, respectively) whose respective quenching constants are different (0.022 and 0.028 %⁻¹ O₂ at 760 Torr). Similar effects were found with the other dyes. However, a marked influence of humidity was observed in all cases which makes the material better suitable for sensing oxygen in aqueous samples. Possibly, the use of hydrophobic

supports may eliminate the cross-sensitivity to moisture.

6.1.2. Fullerenes

Similar to PAHs, fullerenes have a large conjugate structure and possess useful electronic and photochemical properties. The luminescence of C_{70} is atypical in several ways. Its fluorescence occurs from two excited singlet states. The weak prompt fluorescence (with a QY of 0.05%, and a decay time of 650 ps) occurs between 650 and 725 nm. Strong energy overlap and many low-lying excited states cause the QY for triplet formation to be close to 1. Multiple weak phosphorescence bands can be observed in the region 750 – 950 nm, with lifetimes of 20 – 25 ms at room temperature. C_{70} displays a remarkably strong thermally activated E-type delayed fluorescence. An increase in temperature leads to a stronger coupling between excited singlet and triplet states. The E-type delayed fluorescence of C_{70} was applied to detect oxygen.^{146, 147} The lifetimes of the delayed fluorescence are as long as >20 ms at room temperature, so that the respective oxygen sensor (C_{70} in polystyrene) displays extremely high sensitivity. Molecular oxygen in concentrations as low as 200–800 ng/L can be determined by this method either at single sensor spots or spatially resolved (by imaging using sensor films with a thickness of a few μm) over a temperature range of more than 100 °C. The sensor works at temperatures of up to 240 °C. The response is instantaneous (< 0.1 s) and fully reversible over hundreds of cycles. There was no detectable degradation after three months of storage at room temperature in the dark. It shall be kept in mind that the above work is based on the measurement of E-type delayed fluorescence of C_{70} whose lifetime can be as long as >20 ms. The sensing scheme described in ref.⁸⁰, in contrast, relies on the measurement of the triplet-triplet absorption. The lifetime of the triplet state of C_{70} is 410 μs only.

Sensors with even lower limit of detections (LODs) were obtained¹⁴⁸ by employing the quenching of the thermally activated delayed fluorescence of isotopically enriched carbon-13 fullerene C_{70} ($^{13}C_{70}$). This fullerene was dissolved in either polystyrene (PS), ethyl cellulose (EC) and an organically modified silica gel ("ormosil"). The respective sensor films (5 – 10 μm thick), on photoexcitation at 470 nm, display a strong delayed photoluminescence with peaks between 670 and 700 nm. Its quenching by molecular oxygen was studied at 25 °C and 60 °C, and in concentrations from zero up to 150 ppmv of oxygen in nitrogen. The rapid lifetime determination method was applied to determine oxygen-dependent lifetimes (which are in the order of 15 – 45 ms) and for lifetime imaging of oxygen. The lower limits of detection (at 1% quenching) vary with the polymer used (ethyl cellulose ~250 ppbv, ormosil ~320 ppbv, polystyrene ~530 ppbv at 25 °C) and with temperature. These oxygen sensors are the most sensitive ones (in terms of limits of detection) described so far.

Fullerenes such as C_{60} and C_{70} , also display triplet-triplet absorption in the IR region that is sensitive to oxygen. The QY of intercrossing system from the photoexcited singlet state to the

triplet state of fullerene is estimated to be 1.0, and the triplet state is efficiently quenched by oxygen. Thus, fullerene is an attractive probe for optical oxygen sensing using the T_1 - T_n absorption based on laser flash photolysis. Amao and Okura et al.⁷⁹ studied the decay of T_1 - T_n absorption of C_{60} in films of polystyrene and found the photoexcited triplet state of C_{60} to be strongly quenched by oxygen. This resulted in an oxygen sensor with very low limits of detection. The lifetime of the excited triplet state of C_{60} is $\sim 100 \mu\text{s}$, and the oxygen sensitivity (expressed as τ_0/τ_{100}) is ~ 51 . In the same year, this group⁸⁰ also studied the use of fullerene C_{70} for oxygen sensing and found that the lifetime of the photoexcited triplet state of C_{70} ($\sim 410 \mu\text{s}$) is about four times longer than that of C_{60} , which results in much higher sensitivity than with C_{60} in view of a τ_0/τ_{100} ratio of > 400 .

6.1.3. Room Temperature Phosphorescent Organic Probes

Phosphorescent probes were, in fact, the first OSPs. The Kautsky effect¹⁴⁹ (viz., the delayed production of minute quantities of oxygen by leaflets following illumination) obviously could only be discovered with a method possessing an extremely low limit of detection. Phosphorescence has a rather long decay time, and the probability of collisional quenching in the excited state of phosphors therefore is very high. Useful phosphorescent probes for oxygen include tryptaflavine, benzoflavine, euchrysin, rheonine 3A, rhoduline yellow, safranin, chlorophyll, hematoporphyrin isoquinoline red, uranine (fluorescein sodium salt), eosin, erythrosin, and rhodamines B and G.¹¹ Notably, all these OSPs have rather longwave excitation and emission wavelengths (which makes them LED-excitabile), and phosphorescence generally has a large Stokes' shift which facilitates spectral separation. Silica gel, aluminium oxide were found to be suitable adsorbents, while the use of cellulose, silk, or synthetic fibers resulted in very low sensitivity if completely dry, but moderate sensitivity after exposure to humid air. However, the absorption of water on sensor beads (of silica or aluminum oxide) also compromises the intensity of phosphorescence which can be completely extinguished in aqueous surrounding.³² On the other hand, the preparation of such adsorbates is experimentally simple in that the particles are placed in aqueous or methanol solutions of the dyes and left there for a defined period of time. After filtering, washing with water and heat-drying, they are ready for use. Phosphorescence is totally quenched by oxygen at levels of around 0.001 to 0.01 Torr. The effects were used to detect oxygen in the range between 0.004 and 0.0005 Torr. It was also observed that the dyes photobleach in presence of oxygen (which implies that oxygen is consumed), unless singlet oxygen is quenched by another species. Such an acceptor was found in isoamylamine which obviously acts as a stabilizer.

An even more sensitive oxygen sensor is based on the finding¹⁴⁹ that the slow-decaying phosphorescence observed at temperatures below $-70 \text{ }^\circ\text{C}$ is converted into a rapidly decaying fluorescence when oxygen is admitted. In a typical experiment, tryptaflavine was adsorbed on silica and placed in an evacuated flask in liquid air or solid CO_2 . When excited with visible light, the


material has orange phosphorescence with a decay time as long as 40 – 50 s(!). If, after switching off the excitation light source, traces of oxygen are allowed to enter the flask, phosphorescence is instantaneously quenched, but a flash of green fluorescence is observed. The effect is observed with traces of oxygen and has been exploited to detect it at pressures around 5 μ Torr (i.e., 10 pmol of oxygen in a volume of 50 mL). The effect is the same under vacuum, hydrogen, or nitrogen, and the working range is 10^{-6} to 10^{-4} Torr under visual absorption. Rhodamines B and 6G, uranine, phosphine, benzoflavine, 1-hydroxypyrene-3,6,8-trisulfonate (HPTS) and 7-hydroxycoumarins also showed this effect at -180 °C. Pollack et al.³³ have modified the Kautsky method and were able to detect the production of 4×10^{12} oxygen molecules when a green leaf was exposed to a flash of light. Another field of application was found in the detection of the onset of oxygen production in water electrolysis when the voltage is raised from 0 to 2.6 Volt.

Zakharov and Grishaeva³⁴ have utilized the phosphorescence quenching effect of oxygen to devise an optosensor for low levels of oxygen in water. It was found that with their material, the phosphorescence was retained even if immersed in water or various organic solvents, with decay times ranging from 50 to 100 ms. Dye-loaded silica gels of various structures and celluloses of varying viscosity phosphoresce in water, ethanol, isoamyl alcohol, heptane and chloroform. Deoxygenation led, in most cases, to a significant increase in intensity. In addition, the emission intensity depends on the structure of silica gels in that those having fine pores display the strongest intensity. The findings were applied to sense oxygen in water. The afterglow of acridine orange adsorbed on Silochrome S-120 was most sensitive to quenching by water-dissolved oxygen and used for its continuous determination in the 0.06 to 1.0 $\mu\text{g L}^{-1}$ concentration range.³⁴ With acriflavine, the detection limit is 0.35 $\mu\text{g L}^{-1}$ when adsorbed on silica gel, and from 10 to 100 $\mu\text{g L}^{-1}$ when adsorbed on cellulose. Other kinds of supports have also been studied and dynamic ranges from 0.4 to 400 $\mu\text{g L}^{-1}$ were reported.¹⁵⁰ Sensitivity can considerably be improved by using hydrophobic supports such as silanized silica gel.¹⁵ Detection limits then are 5×10^{-4} $\mu\text{g L}^{-1}$, but it was observed¹⁵¹ that the dye undergoes "photoabsorption of oxygen" which resulted in a distortion of the SVPs at high illumination intensity. This effect is negligible if the exciting light is sufficiently attenuated.

Camphorquinone (CQ) (see **Figure 8**) displays intense room temperature phosphorescence (RTP) when immobilized in a polymer matrix. The excitation and emission bands lie in the visible and the RTP is quenched by oxygen. This effect was exploited¹⁵² to sense oxygen via the RTP of CQ immobilized in several polymer matrices. The sensors can be operated in both the intensity and the lifetime mode, and oxygen can be determined in the gas phase in the 0.1 – 25 % concentration range. However, CQ suffers from photodecomposition, which causes signal loss over time and, thus, compromises the accuracy in intensity-based measurements. Erythrosine B is another commonly used phosphorescent OSP. It has a decay time of almost a microsecond in the dry state. If

immobilized¹⁵³ on a silica-based ion exchanger, a material is obtained which under excitation at 547 nm displays an intense red phosphorescence (peaking at 695 nm) that is strongly quenched by oxygen. The response time is < 2 s on both the forward and reverse direction which is unusual because the response time of most sensors on going from oxygen-free environment to air or pure oxygen is longer than in the reverse direction.¹⁵⁴ This sensor has good photochemical stability and does not photodegrade if continuously irradiated with a xenon discharge lamp for more than 24 h. The detection limit is 0.6 ppm of oxygen in dry argon. Humidity may interfere. The related dye pyronine in various polymers may also be used.¹⁵⁵

Figure 8. The chemical structures of the RTP oxygen-sensitive probes.

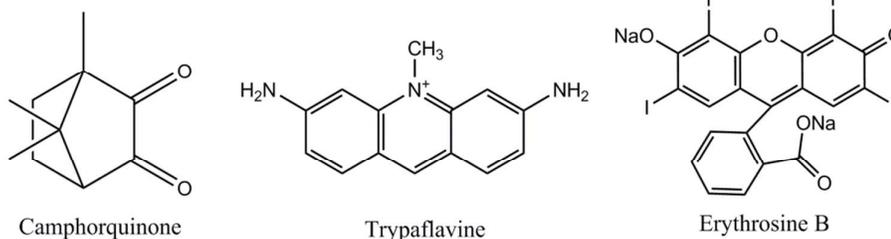

Erythrosine B was doped into a sol-gel film where its RTP is strongly quenched ($I_0/I_{100} \sim 123$) by oxygen.¹⁵⁶ It has two emission peaks, a weak one at 570 nm (attributed to delayed fluorescence), and a phosphorescent peak at 691 nm. The delayed fluorescence and the phosphorescence are oppositely dependent on temperature in that the phosphorescence intensity decreases as temperature increases. By contrast, the intensity of the delayed fluorescence is enhanced with an increase of temperature. This unique behavior may be applied for temperature self-compensation, and is observed within the temperature range from -50 to 200 °C. Porphyrins also may be used as OSPs but will be treated in **Section 6.2.5**.

Table 3. Organic fluorescent probes for oxygen, their excitation/emission wavelengths (in nm), quenchability ("sensitivity"), along with the polymer solvent or support used, and the method for read-out (RO). Quenchability is expressed as either I_0/I_{100} (the ratio of fluorescence intensity at zero % oxygen in the carrier gas and the intensity at 100% oxygen (at atmospheric pressure), or in a fluid equilibrated with such gases. Correspondingly, I_{21} is the intensity under air at atmospheric pressure. *Codes:* I: intensity-based readout; I-RTP: intensity of room temperature phosphorescence; L-RTP: lifetime of RTP-based readout; TA: triplet absorption-based readout; LIM: lifetime imaging; IR: ratiometric intensity-based readout. QY: quantum yield; SVP: Stern-Volmer plot. For other acronyms see the list in Section 14.

Dye/Matrix	$\lambda_{exc}/\lambda_{em}$	Sensitivity [†]	Comments	RO	Ref.
Fluoranthene in polyethylene	330/390	$I_0/I_{100} \sim 1.11$	First PAH-based optical sensors for oxygen.	I	35
Pyrene-1-butyric acid in gel	345/460		Short wave excitation; Pyrene-1-butyric acid dissolved in organic solvent and then encapsulated into an oxygen-permeable gel to form nanoparticles	I	39, 157
Pyrene in silicone rubber (PDMS)	335/372,384	$I_0/I_{100} \sim 6$	Acrylate-PDMS composite; non-linear SVPs; downward curvature is explained by domain model; other PDMSs also investigated.	I	158
Pyrene-1-butyric acid on oxidized alumina	355/474	$I_0/I_{100} = 6.14$	Anodic oxidized alumina plate; photostable; non-linear SVPs; quenching of excimer.	I	128
Pyrenedecanoic acid on alumina plate	340/376	$I_0/I_{100} = 18.6$	Anodic oxidized alumina plate; perfluorohydrocarbon added to improve sensitivity and response time; suffers from UV absorption and emission.	I	133
Pyrenedecanoic acid & perfluorodecanoic acid on alumina plate	340/396	$I_0/I_{100} = 20.2$			
Perylenedibutyrate on silica	468/514	$I_0/I_{100} = 1.67$ $I_0/I_{21} = 1.19$	Good stability, low toxicity, loss in sensitivity of about 3 % per day during dry storage; loss is 0.1 % per day when stored in water.	I	42
(a) Pyrene in silicone rubber (b) Perylene in silicone rubber (c) Pyrene/peryene in silicone rubber	320/400 400/474 320/474	$I_0/I_{21} = 1.90$ $I_0/I_{21} = 1.14$ $I_0/I_{21} = 4.36$	Fluorescence of the energy transfer system (pyrene/peryene) is more efficiently quenched by oxygen than the fluorescence of pyrene itself.	I	139
Decacyclene in PDMS	385/510	$I_0/I_{100} = 7.8$	Photostable; excitable in blue range, large Stokes' shift; lifetime is ~ 21 ns; QY 0.29 in toluene; decacyclene used in the form of its silicone-soluble <i>tert</i> -butyl derivative; black Teflon used as an optical isolation; also used to sense halothane.	I	6, 46, 141
Camphorquinone in PS	470/560	$I_0/I_{6\%} = \tau_0/\tau_{6\%} \sim 19$	Monoexponential decay; time and intensity plots coincide for all the polymer matrixes; not photostable. Photostable, but intensity drifts.	I-RTP; L-RTP	152
Camphorquinone in PVC	470/560	$I_0/I_{21} \sim 2.5$			
Camphorquinone in PMMA	470/560	$I_0/I_{21} \sim 7.7$			
Erythrosine B on amino-modified silica	547/695	$I_0/I_{0.05\%} \sim 4.2$	Works well in dry state only; good photostability, fast response (< 2 s); suitable for sensing extremely low oxygen concentration; non-linear SVP; decay time > 0.2 ms.	I-RTP	153
Erythrosine B immobilized in/on ormosil	520/660	$I_0/I_{0.015\%} = 2.77$	Probe covalently immobilized; oxygen sensitivity influenced by pH, TMOS/MTMOS ratio, and alcohol media; good photostability.	I-RTP	159
Erythrosine B in sol-gel	532/570, 691	$I_0/I_{100} \sim 123$	Unusual (and non-linear) SVPs; intensity of delayed fluorescence (at 570 nm) increases with temperature, but phosphorescence (at	I-RTP	156, 160

[†] The "equal to" symbol (=) indicates a value given by the authors. The " \approx " symbol indicates a value that was estimated by the authors of this review from data presented in the respective article. A blank indicates that sensitivity could not be easily calculated for various reasons.

			691 nm) decreases with increasing temperature, response time ~100 ms; works from -50 to 200 °C; τ_{phos} 280 μs , QY_{phos} 2 %.		
Fluorescent Yellow on silica gel	466/519	$I_0/I_{21} \sim 3$	Used to visualize surface gas flows.	I	161
C ₆₀ fullerene in PS	532/750	$\tau_0/\tau_{100} \sim 51$	Quenching of the excited triplet state ; $\tau_0 \sim 100 \mu\text{s}$; high sensitivity; linear SVPs.	L, TA	79 81
C ₇₀ fullerene in PS	532/860	$\tau_0/\tau_{100} > 400$	Quenching of the excited triplet state; $\tau_0 = 414 \mu\text{s}$; very high sensitivity; linear SVPs.	L, TA	80
C ₇₀ fullerene in ormosil C ₇₀ fullerene in ethyl cellulose	470/650-710	$\tau_0/\tau_{300 \text{ ppm}} \sim 8.5$ $\tau_0/\tau_{300 \text{ ppm}} \sim 12.5$	E-type delayed fluorescence; lifetime >25 ms; response (<0.1 s); fully reversible, also used at elevated temperatures.	I; LIM	146
¹³ C ₇₀ fullerene in polystyrene ¹³ C ₇₀ fullerene in ormosil ¹³ C ₇₀ fullerene in ethyl cellulose	470/600-750	$\tau_0/\tau_{150 \text{ ppm}} \sim 3.0$ $\tau_0/\tau_{150 \text{ ppm}} \sim 4.5$ $\tau_0/\tau_{150 \text{ ppm}} \sim 5.5$	Suitable for trace oxygen sensing; fully reversible; fluorescence lifetime imaging; temperature influences.	I; LIM	148

6.2. Metal-Ligand Complexes


Probes with long decay times are well suited for oxygen sensing because the long-lived excited state makes collisional quenching by oxygen more likely. It can be stated that the detection limits of an OSP mainly depend on the lifetime of its emitting state in that longer lifetimes favor quenchability. However, there is no linear relationship between quenchability and decay time. Luminescent transition-metal complexes, unlike PAHs, have relatively long lifetimes, absorption in the visible, large Stokes' shifts, and often are photostable. Their spectroscopic and chemical properties can be tuned to some extent via modification of the structure of the complexes. Molar absorption coefficients (ϵ ; these are important with respect to brightness which is defined as the product of $QY \cdot \epsilon$) are moderate except for the Soret bands of porphyrins.

On photoexcitation, transition metal complexes usually undergo metal-ligand charge transfer to form an excited triplet (or higher multiplicity) state. Triplet-singlet back transitions are spin-forbidden, and the triplet-state lifetimes therefore are much longer than those of a singlet state. This provides enough time for oxygen to collide with the excited-state molecule and results in high sensitivity to oxygen. The triplet states have lower energy than singlet states so that the wavelength of phosphorescence is longer than that of fluorescence. The resulting large Stokes' shifts facilitate spectral separation. Early quenching studies in fluid solution¹⁶² revealed that the luminescence of complexes of ruthenium(II), osmium(II) and iridium(III) is strongly quenched by oxygen. Numerous other OSPs based on transition-metal complexes have been synthesized meanwhile. Depending on the central metal ion, we have categorized them into six groups, viz. the complexes of ruthenium(II), iridium(III), osmium(II), rhenium(II), the trivalent lanthanides, and the large group of metallophorphyrins.

6.2.1. Ruthenium(II) Complexes

Ruthenium(II) complexes (see **Figure 9**) have broad absorption bands located most often in the blue region (400 – 480 nm) of the visible spectrum. They have large Stokes' shifts and emit at > 600 nm. Their long excited-state lifetimes (in the order of microseconds) make them viable probes for sensing and imaging of oxygen. Both intensity and lifetime are affected by oxygen. Their luminescence can be tuned by changing ligands. Often used ruthenium(II) based OSPs include Ru(bipyridine)₃ [denoted as Ru(bpy) in the following], Ru(1,10-phenanthroline)₃ [denoted as Ru(phen)], and Ru(4,7'-diphenyl-1,10'-phenanthroline)₃ [denoted as Ru(dpp)]. All are commercially available. Others are less common. The ruthenium complexes and the metal porphyrin complexes form the largest group of OSPs.

Figure 9. Chemical structures of representative Ru(II) complexes for use in oxygen sensing

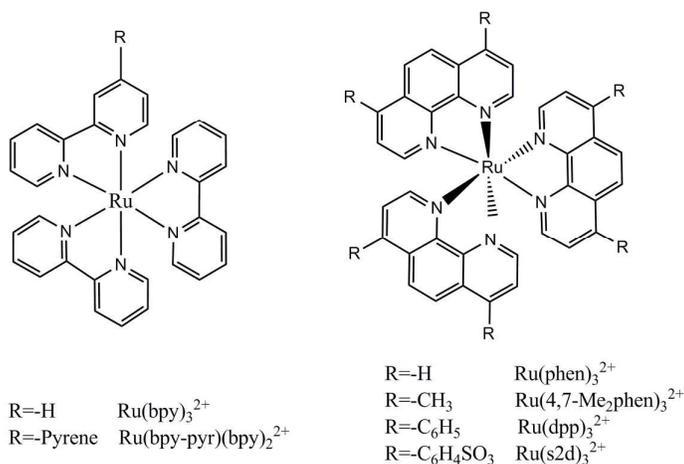

The water-soluble probe Ru(bpy) in the form of its dichloride is the earliest ruthenium-based OSP ever used in a sensor for oxygen.⁴⁷ It was immobilized by adsorbing it on silica microparticles which then were incorporated into silicone rubber. Silicone was chosen as a matrix because of its excellent permeability to oxygen and its flexibility in terms of designing sensor geometries and formats (fiber optics included). The results obtained with this sensor already revealed typical issues such as downward curved Stern-Volmer plots (SVPs), differences in the forward and back response times, and sensitivity to relative humidity in case of gaseous samples (which of course play no role in case of aqueous or blood samples). The probe has an absorption maximum at 460 nm and can be excited with blue LEDs. Its molar absorption coefficient is moderate ($< 20,000 \text{ M}^{-1} \text{ cm}^{-1}$), and its emission maximum peaks at 610 – 630 nm depending on the (polymer) solvent. The large Stokes' shift of ~160 nm facilitates the separation of the analytical signal (the luminescence) from scattered excitation light and reduces self-absorption of luminescence. However, this probe has a fairly low QY (~ 0.02), and quenching by oxygen is moderately efficient.

Enhanced stability and oxygen sensitivity of the Ru(bpy) complex is found if the probe is placed in an ionic liquid doped into electrospun fibers made from poly(methyl methacrylate) and ethyl cellulose.¹⁶³ The use of electrospun polymer microfibers results in increased surface area and sensitivity. However, ionic liquids tend to leach if the sensor is immersed into aqueous solutions or organic solvent. Steady state and lifetime data were used to sense oxygen in the gas phase. The luminescence intensity of the sensor is said not to drift over 44 months.

Similar to Ru(bpy), the ionic probe Ru(phen)₃Cl₂ is fairly water-soluble and has an unquenched lifetime of 1 μs. Its spectra are quite similar to those of Ru(bpy), but the molar absorption coefficient and QY (~0.05) are somewhat better.¹⁶⁴⁻¹⁶⁹ It has the highest temperature sensitivity¹⁷⁰ among the Ru(II) polypyridyl complexes. In fact, it was incorporated in the gas-blocking polymer polyacrylonitrile and used to sense temperature.¹⁷⁰⁻¹⁷²

The probe Ru(dpp) has a fairly strong absorption in the visible region ($\lambda_{\text{max}} = 463 \text{ nm}$, $\epsilon = 28,400$

$\text{M}^{-1}\cdot\text{cm}^{-1}$) which makes it compatible with blue LEDs and with the argon ion laser (488 nm). Its luminescence QY is much higher (up to 0.5), and the unquenched excited-state lifetime is $\sim 6 \mu\text{s}$ (under nitrogen). This results in high brightness ($\epsilon \cdot \text{QY}$; here $10,200 \text{ M}^{-1}\cdot\text{cm}^{-1}$). It also exhibits good photostability.^{173, 174} These features make Ru(dpp) the most commonly used ruthenium-based OSP. The better soluble perchlorate of Ru(dpp) was incorporated into silicone rubber to yield a widely used sensor material.⁴⁹

The probe later has been intensely studied in various matrices including organic polymers, inorganic sol-gel films, and organically modified silicate (ormosil) matrix. Typical data are given in **Table 4**. Oxygen sensing can, in fact, be well adjusted via the choice of the polymer matrix. Ru(dpp) with counter anions such as chloride, perchlorate, or sulfate has poor solubility in hydrophobic polymers such as silicone rubbers. If the inorganic anion is replaced by lipophilic organic counter anions such as dodecyl sulfate or trimethylsilylpropansulfonate,¹⁷⁵ distinctly improved solubility in silicones and other apolar polymers is warranted. The introduction of the new counterion does not cause measurable changes in the absorption and emission spectra, but the luminescence intensity of sensing films is increased. The ligand dpp may also be modified with a lipophilic chain (such as 5-octadecanoylamido)¹⁷⁶ or 4-octylphenyl groups¹⁷⁷ to obtain hydrophobic luminescent probes that are fairly well soluble in silicone.

Most Ru(II) polypyridyl complexes can be excited with blue light to emit in the red region, but more long-wavelength absorbing and emitting OSPs are desired for biological applications. Klimant et al.¹⁷⁸ synthesized several long-wavelength Ru(II) complexes by replacing one or two ligands of Ru(bpy) and Ru(dpp) with 6,7-dihydro-5, 8-dimethyl-dibenzo[*i,j*][1,10]phenanthroline. These long-wavelength Ru(II) complexes can be photoexcited between 450 and 580 nm and have large Stokes' shifts. The emission bands sometimes even extend into the NIR region. These OSPs are photostable and compatible with green LEDs but have not been investigated ever since, possibly because their QYs are at <0.01 .

In order to ultimately overcome leaching from the polymer matrices, a Ru(II) complex bearing a polymerizable acrylate group can be covalently linked to a matrix.¹⁷⁹ The introduction of acrylate group into the phenanthroline ring does not affect the MLCT and the spectral properties. In fact, the probe fully maintains its oxygen sensing capability. The co-polymerized sensing films are stable in aqueous solutions and even in hydrophobic organic solvents. Moreno-Bondi et al.¹⁸⁰ prepared three sulfonated Ru(II) complexes and linked them to amino-functionalized matrices such as amino-modified porous glass. The material displayed strong emission with a peak at 610 nm if excited at 475 nm. Again, the material was completely resistant to leakage even on long-term usage. It is suitable for sensing oxygen in aqueous solution and in organic solvents. Similarly, a Ru(II) polypyridyl complex was functionalized¹⁸¹ with a triethoxysilane group via reaction with (3-

aminopropyl)trimethoxysilane in acidic solution. The probe was condensed into sol-gel glass films and the resulting sensing films revealed enhanced stability in water and organic solvents compared to similar films where probes were incorporated physically. Ru(bpy) modified with a triethoxysilane group also was condensed¹⁸² into ormosil films. The Winnik group¹⁸³ have synthesized alkylamino functionalized Ru(phen) and linked it to a sulfur-nitrogen-phosphorus polymer. The respective sensing film exhibited almost linear Stern-Volmer behavior and good quenchability.

In a study¹⁸⁴ on the performance of the probe Ru(dpp) in polystyrene films and of Ru(bpy) in fumed silica gel it was found that the response of the Ru(dpp)/polystyrene system to oxygen can be well fit with the model of a spatially disordered environment. In contrast, the SVPs of the Ru(bpy)/silica-gel system are nonlinear, and this was explained by microheterogeneity. Additionally, in fumed silica gels, oxygen reaches the probe via surface diffusion and absorption isotherms are expected to provide an additional effect on the curvature of such plots. It was attempted¹⁸⁵ to eliminate effects of microheterogeneity by synthesizing a Ru(bpy)-centered polystyrene-derived star polymer and expecting that the resulting probes may be evenly surrounded inside the star polymer so that effects of microcrystallization and leaching may be avoided. However, microheterogeneity could not be completely eliminated in that the decays profiles were still multi-exponential. Heterogeneity possibly is caused by the wide range of molecular weights of the polymer prepared during the polymerization.

Solid-state OSPs usually cannot be used directly for sensing oxygen because of strong inner filter effects, self-quenching, and poor accessibility for oxygen. It was shown,¹⁸⁶⁻¹⁸⁸ however, that crystals of Ru(II) polypyridyl complexes of the type $[\text{Ru}(\text{phen})_3]\text{tfpb}_2$, $[\text{Ru}(5,6\text{-Me}_2\text{Phen})_3]\text{tfpb}_2$ and $[\text{Ru}(\text{phen})_3](\text{PF}_6)_2$ can be used directly as solid-state probes for oxygen. Obviously, the crystal lattices contain enough void space to allow oxygen to diffuse in and to quench luminescence. The crystals give strictly linear SVPs, and sensitivity does not change if crystals are stored for more than a year. A single crystal can be used directly as an oxygen sensor rather than using hosting materials to immobilize any OSPs.

The polystyrene-soluble probe $[\text{Ru}(\text{dpp})](\text{TMS})_2$ (where TMS stands for the trimethylsilylpropylsulfonate anion) was shown¹⁸⁹ to enable sensing of oxygen via two-photon excitation (2-PE). Amino-modified polystyrene nanoparticles (85 ± 19 nm i.d.) were soaked with a solution of the probe in a water-THF mixture to obtain monodisperse nanoparticles with an average diameter of 121 ± 3 nm and a polydispersity index of 0.04. The particles can be conventionally photoexcited with the 488-nm line of an argon laser. If, however, a mode-locked Ti:sapphire laser with an output wavelength of 830 nm and an average pulse duration of 75 fs is applied, strong 2-PE luminescence is observed. As expected, luminescence intensity increases nonlinearly with the

power of the laser. Double-logarithmic plots of laser power (between 25 and 125 mW) versus the emission intensity of the oxygen show the slope for 1-PE to be ~ 1 and that for 2-PE to be ~ 2 . The emission spectra at 2-PE are the same as obtained by 1-PE. The SVPs obtained after excitation in the visible and the NIR (i.e., 2-PE) are identical and both are strictly linear ($R^2 = 1.000$).

Ruthenium probes such as Ru(dpp) are well compatible with present-day low-cost electronics (such as LEDs and silicon photodiodes). These can be well packed into small-sized instrumentation as shown¹⁹⁰ for a hand-held optical sensor for dissolved oxygen. A blue LED served as a light source to photoexcite the luminescence of Ru(dpp) absorbed on silica gel in a silicone rubber membrane. The respective instrument has a size of 48×148×20 mm and weighs only 96 g. It is powered by batteries and gives luminescence intensity data on dissolved oxygen. A miniaturized sensor with a size smaller than a fingernail was obtained¹⁹¹ by integrating an oxygen-sensitive ormosil film with a low-power complementary metal oxide semiconductor (CMOS) chip.

Table 4. Luminescent ruthenium(II) complex-derived probes for oxygen, along with their excitation/emission wavelengths (in nm), quenchability ("sensitivity"), the polymer solvent or support used, and the method for read-out (RO). Quenchability is expressed as either I_0/I_{100} (the ratio of fluorescence intensity at zero % oxygen in the carrier gas and the intensity at 100% oxygen (at atmospheric pressure), or in a fluid equilibrated with such gases. Correspondingly, I_{21} is the intensity under air at atmospheric pressure. Codes: I: intensity-based readout; L: lifetime-based readout; SVP: Stern-Volmer plot; QY: quantum yield. For other acronyms see the list in Section 14..

Dye/Matrix	$\lambda_{exc}/\lambda_{em}$	Sensitivity	Comments	RO	Ref.
Ru(dpp) ⁱ ₃ (ClO ₄) ₂ in plasticized PVC Ru(dpp) ₃ (laurylsulfate) ₂ in silicone Ru(dpp) ₃ (ClO ₄) ₂ in ethyl cellulose (46%) Ru(dpp) ₃ (ClO ₄) ₂ in PS	465/610	$I_0/I_{100} \sim 3.5$ $I_0/I_{100} \sim 5.3$ $I_0/I_{100} \sim 3.2$ $I_0/I_{100} \sim 2.0$	Decay is not single exponential; double-exponential fit possible for PVC membranes.	I	112
Ru(dpp) ₃ (ClO ₄) ₂ in PS	470/610	$I_0/I_{100} \sim 2.3$	Dye aggregates at higher concentrations, and QY decreases; QY _{phos} = 0.6 for low concentrations.	I	113
Ru(dpp) ₃ (ClO ₄) ₂ in PS, TiO ₂ particles added	455/610	$I_0/I_{100} \sim 1.25$	TiO ₂ is used as a scatterer to increase the brightness of the microsensor; excellent long-term stability and storage stability.	I	54
Ru(dpp) ₃ (ClO ₄) ₂ in PVC + plasticizer (2-nitrophenyl octyl ether)	480/610	$I_0/I_{21} = 2.0$	Fast response times, but severe leaching of the plasticizer in water containing detergent; used for determination of biochemical oxygen demand.	I	192
Ru(dpp) ₃ Cl ₂ in polyacrylamide	488/610	$I_0/I_{100} = 3.2$	Dye encapsulated in polyacrylamide during polymerization process on optical fiber; used to sense oxygen in solution.	I	193
Ru(dpp) ₃ (TMS) ⁱⁱ ₂ in silicone, TiO ₂ added Ru(dpp) ₃ (DS) ₂ in silicone, TiO ₂ added	465/610	$I_0/I_{21} = 2.5$	Self-quenching not observed at high dye concentration; other silicones also investigated; TiO ₂ added as light scatterers and as optical isolation.	I	175
Ru(5-odap) ⁱⁱⁱ ₃ on controlled pore glass Ru(5-odap) ₃ on silica gel Ru(5-odap) ₃ on XAD4 Ru(5-odap) ₃ on C ₁₈ -silica Ru(5-odap) ₃ in silicone	449/600 449/600 449/600 449/600 449/600	$I_0/I_{140 \text{ torr}} \sim 3.5$ $I_0/I_{140 \text{ torr}} \sim 2.8$ $I_0/I_{140 \text{ torr}} \sim 1.5$ $I_0/I_{140 \text{ torr}} \sim 1.3$ $I_0/I_{140 \text{ torr}} \sim 1.1$	QY 0.027, τ_0 0.5 μ s; highly soluble in silicone; linear SVPs in pure silicone.	I	176
Ru(dpp) ₃ on controlled pore glass Ru(dpp) ₃ on silica gel Ru(dpp) ₃ on C ₁₈ silica Ru(dpp) ₃ in silicone	462/618 462/618 462/618 462/618	$I_0/I_{140 \text{ torr}} \sim 6.0$ $I_0/I_{140 \text{ torr}} \sim 6.0$ $I_0/I_{140 \text{ torr}} \sim 2.7$ $I_0/I_{140 \text{ torr}} \sim 1.2$	More sensitive than Ru(5-odap) ₃ in all matrices downward curved SVPs; QY 0.366; τ_0 5.9 μ s.	I	176
Ru(dpp) ₃ (Ph ₄ B) ₂ in CAB+TBP ^{iv} Ru(dpp) ₃ (Ph ₄ B) ₂ in PVA+TBP Ru(dpp) ₃ (Ph ₄ B) ₂ in PS+TBP Ru(dpp) ₃ (Ph ₄ B) ₂ in PMMA+TBP Ru(dpp) ₃ (Ph ₄ B) ₂ in PVC+TBP	430/596 430/596 430/596 430/596 430/596	$I_0/I_{100} \sim 6.8$ $I_0/I_{100} \sim 3.8$ $I_0/I_{100} \sim 3.3$ $I_0/I_{100} \sim 3.1$ $I_0/I_{100} \sim 3.0$	Effect of plasticizer also investigated; the fraction of plasticizer increases sensitivity and decreases response and recovery times; films are very photostable; tributylphosphate is the most effective plasticizer.	I	194
Ru(dpp) ₃ in polyacrylic acid on alumina plate Ru(dpp) ₃ on poly(sodium 4-styrene) sulfonate	443,470/610 447,475/610	$I_0/I_{100} = 2.3$ $I_0/I_{100} = 3.73$	Electrostatically attached to anionic polymers, then chemisorbed on alumina plate; non-linear SVPs; Ru(phen) and Ru(bpy) also studied,	I	167

ⁱ dpp = 4,7-diphenyl-1,10-phenanthroline

ⁱⁱ TMS = trimethylsilylpropane sulfonate; DS = dodecyl sulfate

ⁱⁱⁱ 5-odap = 5-octadecanamide-1,10-phenanthroline

^{iv} Ph₄B = tetraphenyl borate, TBP = tri-*n*-butylphosphate

			but display low sensitivity; long-term stability not tested.		
Ru(dpp) ₃ in poly(acrylic acid) on alumina plate Ru(dpp) ₃ in silicone rubber	470/610	$I_0/I_{100} = 3.7$ $I_0/I_{100} = 2.7$	Ru(dpp) ₃ immobilized in poly(acrylic acid) by electrostatic effect and chemisorbed on aluminum plate via carboxy group; non-linear SVPs; response time ~4.6 s; good photostability.	I	195
Ru(dpp) ₃ Cl ₂ in PDMS-co-7FBMA ^v	450/610	$I_0/I_{100} \sim 17$	PDMS copolymerized with methacrylate based monomers (including fluorinated and nonfluorinated); close to linear SVPs; good mechanical properties; effect of hydrocarbon chain and fluorination also studied.	I	196
Ru(dpp) ₃ Cl ₂ on SiO ₂ in PDMS (silanol-silanol condensed)	470/>550	$I_0/I_{21} = 1.4$	PDMS is silanol-silanol condensed; dye was adsorbed on SiO ₂ and dispersed in PDMS; quenching is sensitive to humidity and temperature.	I	197
Ru(dpp) ₃ Cl ₂ on SiO ₂ in PDMS (cross-linked)	470/>550	$I_0/I_{21} = 1.68$	PDMS is vinyl-hydride cross-linked; more stable but quenching properties change with time.	I	197
Ru(dpp) ₃ (ClO ₄) in RTV silicone	450/610	$I_0/I_{100} = \tau_0/\tau_{100} = 7.5$	SVPs close to linear, lifetime and intensity plots coincide; sensitivity is higher in RTV-118 silicone than in any other silicone.	I, L	49
Ru(dpp) ₃ (ClO ₄) ₂ on SiO ₂ in silicone	467/598	$I_0/I_{100} = 14.6$	Dye first adsorbed on SiO ₂ , then mixed into silicone; more oxygen sensitive and more linear SVPs than for Ru(dpp) ₃ (ClO ₄) ₂ in silicone due to better solubility; recovery time longer; SiO ₂ also acts as a light scatterer.	I	198
Ru(dpp) ₃ (ClO ₄) ₂ on SiO ₂ in gelatine	469/612	$I_0/I_{DO, 10mM} \sim 7.5$	Dye first adsorbed on SiO ₂ , then mixed into gelatine. Used for determination of oxygen in organic solvents.	I	199
Ru(dpp) ₃ in ormosil	450/620	$I_0/I_{100} \sim 8.8$	Sensitivity to dissolved oxygen increased due to increased hydrophobicity.	I	200
Ru(dpp) ₃ in sol-gel Ru(bpy) ₃ in sol-gel		$I_0/I_{100} = 3.7$ $I_0/I_{100} = 2.0$	Sensitivity adjusted by changing the pH of sol-gel precursor solution; good stability; sol-gel films are not stable in aqueous solution on long-term storage.	I	201
Ru(dpp) ₃ in ormosil	470/610	$\tau_0/\tau_{air} = 1.4$	Phase modulation; sensor properties slowly change over time.	L	202
Ru(dpp) ₃ Cl ₂ in TEOS and octyl-triEOS ormosil ^{vi}	475/>570	$I_0/I_{100} \sim 15$	Sensitivity and long-time stability are higher than for pure TEOS-based films; single exponential decay; uniform and crack-free sensing films.	I, L	203
Ru(dpp) ₃ in ormosil	505/red PD ^{vii}	$\tau_0/\tau_{air} = 1.53$	Ormosil dissolves in organic solvents, but is insoluble in water, methanol, ethanol; no aging; high photostability; linear SVPs; response time 250 ms; τ_0 5.1 μ s.	I, L	204
Ru(dpp) ₃ in DMOS ormosil	467/592	$I_0/I_{100} \sim 14$	Good photostability; fast response (10 s); linear SVPs if cured at high temperature.	I	205
Ru(dpp) ₃ Cl ₂ + Oregon Green in sol-gel nanoparticles	488/610	$I_0/I_{air} \sim 6$	Particles size 50 – 300 nm; PEG added as a sterical stabilizer; also good for sensing in solution; stable to leaching and decomposition; reference dye Oregon Green is pH sensitive.	I	173
Ru(dpp) ₃ (TMS) ₂ in ethyl cellulose (46%) Ru(dpp) ₃ (TMS) ₂ in ethyl cellulose (49%) Ru(dpp) ₃ (TMS) ₂ in PTBS ^{viii}	470/>570 470/>570	$\tau_0/\tau_{air} \sim 1.95$ $\tau_0/\tau_{air} \sim 1.67$	Phase modulation techniques used to measure lifetime; combinatorial approach for rapid screening of probes and polymers.	I, L	206

^v GP-163: an acrylate containing polydimethylsiloxane rubber (PDMS); 7FBMA = 1H, 1H-heptafluorobutyl methacrylate

^{vi} Octyl-triEOS = *n*-octyltriethoxysilane, TEOS = tetraethoxysilane

^{vii} PD = photodiode

Ru(dpp) ₃ (TMS) ₂ in cellulose acetate	470/>570	$\tau_0/\tau_{\text{air}} \sim 1.8$			
Ru(dpp) ₃ (TMS) ₂ in PTFE-co-VP	470/>570	$\tau_0/\tau_{\text{air}} \sim 1.65$			
Ru(dpp) ₃ (TMS) ₂ in PSAN	470/>570	$\tau_0/\tau_{\text{air}} \sim 1.2$			
Ru(dpp) ₃ (TMS) ₂ in PVMK	470/>570	$\tau_0/\tau_{\text{air}} \sim 1.15$			
	470/>570	$\tau_0/\tau_{\text{air}} \sim 1.07$			
Ru(8-dpp ^{ix}) ₃ (ClO ₄) ₃ in PS	460/620	$I_0/I_{100} = 3.5$	Good solubility in polar polymers; QY 0.19; green emitting Ir(III) complexes also reported.	I	177
Ru(bpy)(DMCH ^x) ₂ (PF ₆) ₂ on SiO ₂ silicone	528/736	$I_0/I_{\text{air}} = 1.45$	Low QY (0.005); longer wavelength than other Ru probes; almost linear SVP; QY _{phos} ~ 0.01; Silicone soluble ion pairs; QY _{phos} ~ 0.01.	I	178
Ru(dpp)(DMCH) ₂ (PF ₆) ₂ in PVC	563/738	$I_0/I_{\text{air}} = 1.39$			
Ru(dpp) ₂ (DMCH)(DS) ₂ in silicone	532/732	$I_0/I_{\text{air}} = 1.37$			
Ru(5-acrylamido-phen) ₃ Cl ₂ in polyacrylamide	488/600	$I_0/I_{100} \sim 6$	Compound co-polymerized with acrylamide; no leaching; high stability in aqueous and organic solutions.	I	179
Ru(phen) ₃ in poly(n-butylaminothionylphosphazene)	450/610	$I_0/I_{\text{air}} \sim 1.75$ $\tau_0/\tau_{\text{air}} \sim 1.75$	Indicator covalently attached to the polymer; intensity-based and lifetime-based SVPs are linear and coincide; sensitivity independent of dye concentration; τ_0 1.23 μs (multi-exponential).	I, L	183
Ru(4,7-Me ₂ phen) ₃ (ClO ₄) ₂ in RTV silicone	450/-	$I_0/I_{\text{air}} = 5.6$	SVPs are non-linear; lifetime plots deviate from intensity-based plots.	I, L	110
Ru(4,7-Me ₂ phen) ₃ (Ph ₄ B) ₂ in RTV silicone	450/-	$I_0/I_{\text{air}} = 4.3$			
Ru(phen) ₂ (CN) ₂ in RTV silicone	450/-	$I_0/I_{\text{air}} = 4.0$			
Ru(dpp) ₃ (ClO ₄) ₂ in RTV silicone	450/620	$I_0/I_{\text{air}} = 7.4$			
Ru(bpy) ₃ in RTV silicone	450/620	$I_0/I_{100} = 2.6$			
[Ru(s2d) ₃] ⁴⁺ on controlled pore glass	475/620	$I_0/I_{100} \sim 5$	For determination of oxygen in organic solvents; QY 0.17 for aqueous solution; $\tau \sim 0.3 \mu\text{s}$ in aerated methanol; long response time.	I, L	180
[Ru(s2d) ₂ (acap)] ²⁻ on controlled pore glass ^{xi}	475/615				
Ru dye ^{xii} in silicone and C ₁₀ F ₂₁ CH ₂ COOH	340/597	$I_0/I_{100} = 12.6$	Silicone not specified; pH sensitive; sensitivity increases with addition of perfluorochemicals; poor article.	I	207
Ru(bpy) ₃ in silicone rubber	460/610	$I_0/I_{100} = 1.49$	Weak signal and quenching effect in silicone only matrix; OSP tends to aggregate.	I	47
Ru(bpy) ₃ on SiO ₂ in silicone		$I_0/I_{100} = 3.57$	Intense signal and good quenching effect in silica gels, in silicone matrix; QY ~10 %; non-linear SVPs.	I	47
Ru(bpy) ₃ Cl ₂ in silicone + TiO ₂	460/610	$I_0/I_{100} \sim 4.5$ $\tau_0/\tau_{100} \sim 3.6$	First lifetime sensor; LED excitation; phase modulation; TiO ₂ acts as light scatterer and optical isolation.	I, L	50
Ru(bpy) ₃ in poly(hydroxyethyl methacrylate)	450/593	$\tau_0/\tau_{100} = 1.01$	Virtually no quenching. Contains monomer; sensitivity increases with monomer concentration; τ vs. O ₂ concentration plots are close to linearity up to 100% O ₂ (non-monoexponential behavior probably the reason); sensitivity decreases with aging.	I	208
Ru(bpy) ₃ in poly(hydroxyethyl methacrylate) and hydroxyethyl methacrylate	450/593	$\tau_0/\tau_{100} = 1.98$			
Ru(bpy) ₃ inside zeolite Y in silicone rubber	480/610	$I_0/I_{100} = 3.44$	Sensitivity dramatically increased compared to non-zeolitic matrix; no	I	209

^{viii} PTBS = poly(4-tert-butylstyrene); PTFE-co-VP = poly(tetrafluoroethylene-co-vinylidene fluoride-co-propylene); PSAN = poly(styrene-co-acrylonitrile); PVMK = poly(vinyl methyl ketone)

^{ix} 8-dpp = 4,7-bis(4-octylphenyl)-1,10-phenanthroline

^x DMCH = 6,7-dihydro-5,8-dimethyl-dibenzo(*i,j*)(1,10-phenanthroline)

^{xi} s2d = 1,10-phenanthroline-4,7-bis(phenylsulfonate); acap = 5-acetamide-1,10-phenanthroline

^{xii} Ru dye = Ru(II)dichloro-(2,6-bis[1-(4-dimethylaminophenylimino)ethyl]pyridine)

Ru(bpy) ₃ on SiO ₂ in silicone	480/610	$I_0/I_{100} = 1.69$	self-quenching and leaching; excellent storage stability. Change in sensitivity on storage.		
Ru(bpy) ₃ on SiO ₂ spheres	360/600	$I_0/I_{100} \sim 2.1$	Sphere diameter 0.1 – 0.2 mm; properties only for the spheres without matrix; non-linear SVPs; long response time (2 – 4 min); sensitive to humidity.	I	210
Ru(bpy) ₃ in sol-gel	500/600	$I_0/I_{100} \sim 1.28$	Poor sensitivity and reproducibility.	I	211
Ru(bpy) ₃ on Nafion	444/595	$I_0/I_{DO}^{xiii}, 8 \text{ mM} \sim 1.5$	Many parameters change properties. τ_0 has 3 components; spectral properties depend on the solvent; quenching increases dramatically in swelling solvents (methanol, water).	I	212
Ru(phen) ₃ on Nafion	442/583	$I_0/I_{DO, 8 \text{ mM}} \sim 1.4$			
Ru(dpp) ₃ on Nafion	460/598	$I_0/I_{DO, 8 \text{ mM}} \sim 6.0$			
Ru(odap) ₃ on Nafion	440/583	$I_0/I_{DO, 8 \text{ mM}} \sim 5.1$			
Ru(bpy) ₃ in MTEOS ormosil	450/610	$I_0/I_{100} = 1.5$	Probe functionalized with triethoxysilane group, and covalently incorporated in sol-gel film; short response times; linear SVP.	I	181
Ru(bpy) ₃ in AOT ^{xiv} in a water-gelatine matrix	416/580	$I_0/I_{DO, 15 \text{ ppm}} \sim 1.4$	For use in organic solvents; reversed micelle structure; properties depend on the concentration of all components.	I	213
Ru(bpy-pyr)(bpy) ₂ in aqueous solution	456/632	$I_0/I_{Ox \text{ satu}}^{xv} = 13$	Water soluble probe, used for intracellular oxygen sensing; same photostability as Ru(phen) ₃ , τ_0 1.3 μ s, QY 0.5.	I, L	214
Ru(bpy-pyr)(bpy) ₂ in lipobeads	456/632	$I_0/I_{Ox \text{ satu}} = 2.5$	2.1 μ m lipobeads; for intracellular oxygen; high photo- and chemical stability; QY 0.1.	I	215
[Ru(phen) ₃](tfpb) ₂ as a crystal ^{xvi}	400/518	$\tau_0/\tau_{100} = 3.43$	Crystal based solid state oxygen sensors; good sensitivity; fast response; strictly linear SVPs except for [Ru(phen) ₃](PF ₆) ₂ crystal; intense luminescence with high QYs and long lifetimes; sensitivity and photostability do not change after more than a year of storage.	I, L	186-188
[Ru(5,6-Me ₂ Phen) ₃](tfpb) ₂ as a crystal	-/572	$\tau_0/\tau_{100} = 1.83$			
[Ru(phen) ₃](PF ₆) ₂ as a crystal	465/600	$\tau_0/\tau_{100} \sim 2.9$			

^{xiii} DO = Dissolved Oxygen

^{xiv} AOT = bis(2-ethylhexyl)sulfosuccinate


^{xv} O_x satu = oxygen saturated solution

^{xvi} tfpb = tetrakis(bis-3,5-trifluoromethylphenyl)borate

6.2.2. Iridium(III) Complexes

Ruthenium(II) polypyridyl complexes possess low-lying, non-emitting metal-centered excited states. This leads to an early deactivation of the luminescent MLCT excited states by thermal depopulation.²¹⁶ Cyclometalated Ir(III) complexes, in contrast, are excellent triplet emitters and widely used in organic LEDs. They are soluble in organic polymer films, display remarkably strong luminescence (with QYs between 0.2 and 1.0), and have molar absorption coefficients of $\sim 5,000 \text{ M}^{-1} \text{ cm}^{-1}$ and long lifetimes. Thus, Ir(III) complexes are attractive candidates for use as OSPs. **Figure 10** gives representative chemical structures of a typical complex and various ligands. Their physicochemical and oxygen sensing properties are summarized in **Table 5**. The use of luminescent Ir(III) polypyridine complexes as chemical and biological probes (but not so much for oxygen) has been reviewed.²¹⁷ More recently, crystalline iridium(III)-containing coordination polymers were shown to be viable materials for fiber-optic sensing of oxygen.²¹⁸ The crystallites in the polymer were doped into a sol-gel matrix and also used as a transducer in a glucose biosensor.

Figure 10. Basic chemical structures of cyclometalated Ir(III) complexes and of commonly used ligands.

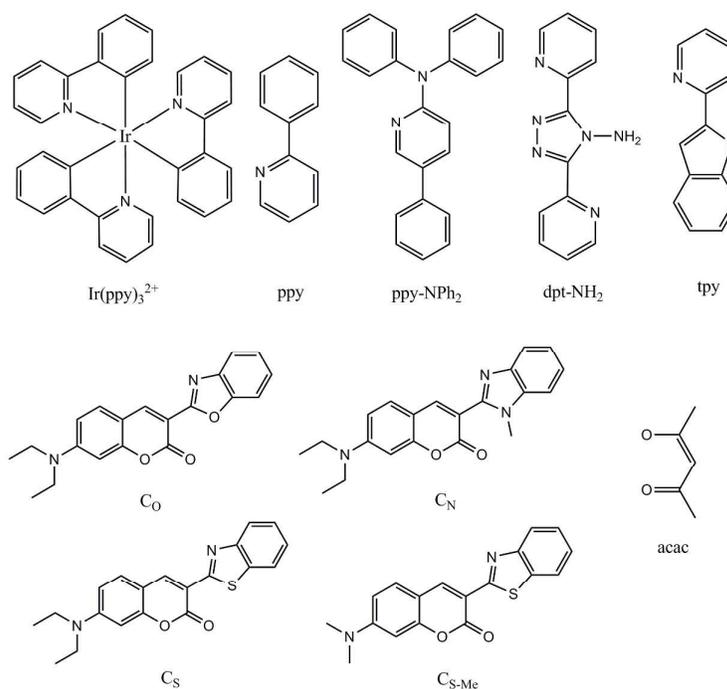

The probe [Ir(ppy)₂(dpt-NH₂)](PF₆) (see Figure 10) has a QY of ~ 0.25 in deoxygenated acetonitrile solutions, exhibits two emission peaks (at 490 and 530 nm), and displays good photostability, fully reversible response, and strictly linear Stern-Volmer plots (SVPs).²¹⁶ Mononuclear and dinuclear Ir(III) cyclometalated complexes were synthesized and immobilized in polymer matrices.²¹⁹ The resulting sensor materials emit intense luminescence with maxima in the 500 – 650 nm range and linear SVPs. The authors came to the conclusion that quenching by oxygen

is affected by (a) the lifetime of the chromophore, (b) the permeability of the polymer, (c) the size, and (d) the charge of the chromophore. With increased molecular sizes and lower charges of the chromophores, sensitivity is enhanced.

The easily accessible probe Ir(ppy)₃ was immobilized²²⁰ in the fluoropolymer poly(styrene-*co*-TFEM) where it displays a strong green luminescence, with a QY as high as 0.90 and a relatively long lifetime (1.5 μs). The sensor is photostable, and its fluorescence is strongly quenched by oxygen ($I_0/I_{100} = 15.3$). The sensitivity of the probe depends on the matrix. If the fluoropolymer is replaced by polystyrene, its sensitivity (I_0/I_{100}) drops to 1.1 and serious photodecomposition does occur. A very high sensitivity is also found if the probe is incorporated into poly(*n*-butylamino) thionylphosphazene.²²¹ The same Ir(III) OSP was functionalized with amino acids to enable phosphorescence-based imaging of oxygen in living cells,²²² but this modification cause the QYs to drop to 0.2. If the ppy ligands of the Ir(III) complexes are substituted by ppy-NPh₂, an OSP is obtained²²³ that has better solubility in organic solvents and polymers, and a QY of 0.70. The broad excitation range makes it compatible with 405-nm lasers or LEDs, and the large dynamic range makes the probe well suitable for sensing oxygen. The decay time in the absence of oxygen is almost independent of temperature in the 1 – 24 °C range.

Borisov et al.²²⁴ have synthesized other cyclometalated Ir(III) coumarin complexes. They possess large molar absorption coefficients (in the order of 30,000 to 60,000 M⁻¹ cm⁻¹ which are even higher than those of Ru(dpp) and of the longwave bands of porphyrins), lifetimes on the order of 8 – 13 μs in the unquenched state, QYs between 0.3 and 1.0, and absorption bands that are compatible with purple and blue LEDs. Their brightness ($\epsilon \times \text{QY}$) is nearly 5 times of that of Ru(dpp) or PtTFPP so that the signal-to-noise ratio is much better. Spectral properties and oxygen sensitivity can be fine-tuned by varying the coumarin ligand, or by using respective monomeric or dimeric complexes. In addition, these OSPs show lower sensitivity to temperature than the widely used probe Ru(dpp). On the other side, they are less photostable, and this restricts their application to short-term sensing. The photophysical properties of cyclometalated Ir(III) complexes were described,²²⁵ and the utility of these [Ir(ppy)₂(N-N)]Cl complexes (where ppy stands for 2-phenylpyridine and N-N is a substituted bipyridine, biquinoline, or phenanthroline) were assessed, but the probes have not been converted into sensor materials by incorporating them into an appropriate solid support. A cyclometalated Ir(III) complex with red luminescence also was reported.²²⁶

Dimeric Ir(III) coumarin complexes were also investigated. Both their absorption and emission peaks are red-shifted, but their QYs are lower than the respective monomeric complexes. The same group²²⁷ also have synthesized Ir(C_{S-Jul})₂(acac), which can be even excited by the 488-nm argon laser. It has a high QY (0.52), and intense absorption peaks are found at 481 nm and 452 nm. Emission peaks at 572 nm. The photophysical properties of this probe are quite similar to those of

the Ir(III) coumarin complexes except for the long luminescence lifetime (20.8 μs). Hence, the probe is highly sensitive to oxygen, but its photostability is moderate.

A luminescent Ir(III) complex was reported²²⁸ that has an unusually longwave emission maximum at 650 nm. The phosphorescence of the probe (referred to as Ir-N-948) also has a useful QY (0.58), a long decay time (102 μs), strong absorption bands between 400 and 500 nm, and a good sensitivity to oxygen. It is soluble in apolar polymers such as polystyrene, and the respective sensor films are quite stable on storage. Its outstanding photophysical properties make the material most suitable for sensing oxygen. Various other Ir(III) complexes were presented in the Supporting Information of the article. In the same year, this group¹⁷⁷ also reported on three green-emitting Ir(III) OSPs with similarly high QYs. Organometallic osmium and iridium complexes were reported for use in barometric coatings (pressure-sensitive paints).²²⁹ These charge-neutral phosphorescent dyes dissolve well into the host polymer FIB, a highly oxygen-permeable fluoropolymer (see **Section 7**). The photo-degradation, temperature sensitivity, and SVPs of pressure sensitive paints based on these complexes were studied in detail.

The luminescence intensity of an OSP exponentially decreases with linearly increasing concentration (or partial pressure) of oxygen (see **Figure 6**). Thus, the sensitivity of OSPs is best at low levels of oxygen but decreases as the oxygen tension increases. This is disadvantageous when it comes to sense oxygen at levels such as at air saturation. A smart approach was made²³⁰ by synthesizing an Ir(III) complex with a caged ligand structure. Quenching of the caged Ir(III) complex by oxygen was remarkably retarded initially due to caged ligand structure, and this makes the probe better suitable for high-level oxygen sensing. This OSP has a fairly good QY (~ 0.5 in dimethylformamide) and a longwave emission (peaking at 570 nm), while the quenching efficiency – compared to Ir(ppy)₃ – is decreased by 80%.

Similar to the situation with Ru(II) polypyridyl complexes, Ir(III) complexes have been synthesized that can be covalently linked to a polymer matrix to overcome leaching. For example, Ir(III) complex carrying vinyl groups have been reported²³¹ that are non-ionic, have long luminescence lifetimes, and good QY. They can be covalently attached to hydride-containing silicones via transition-metal-catalyzed hydrosilylation, or chemically bound into polymer backbones during polymerization of vinylic monomers. The same group²³² has synthesized amino-reactive cyclometalated Ir(III) complexes which then were covalently bound to a water-soluble amino-functionalized polymeric silamine. The resulting materials were blended with different ratios of colloidal microcrystalline cellulose to prepare a water-soluble PSP. Both probes have long lifetimes (17.3 and 35.6 μs) and QYs of typically 0.3. Their sensitivities ($I_0/I_{\text{air}} \sim 3$) make them fairly well suitable for sensing purposes. However, luminescence intensities are strongly affected by temperature. Similar Ir(III) complexes were functionalized with silane groups through which they

can be covalently bound to sol-gel or ormosil matrices.²³³ Such materials can be used to generate singlet ($^1\Delta$) oxygen during photodynamic therapy but also are likely to act as sensor materials. The non-ionic cyclometalated iridium(III) complex $\text{Ir}(\text{ppy})_2(\text{vpy})\text{Cl}$ contains a vinyl group and therefore can be covalently linked to a silicone backbone during polymerization.²³⁴ This results in a sensor material that displays high sensitivity to oxygen, physical stability, and a QY of 0.32. However, it has to be excited in the UV.

Four oxygen-sensitive iridium(III)-containing coordination crystals were synthesized²³⁵ using $\text{Ir}(\text{ppy})_2(\text{H}_2\text{dcbpy})\text{PF}_6$ as the bridging ligand (H_2dcbpy = 4,4'-dicarboxy-2,2'-bipyridine). The bridging ligand was crystallized with $\text{M}(\text{ClO}_4)_2$ (M = Zn, Cd, Co and Ni, respectively) to form Ir(III)-containing single crystals. These have emission QYs in air of 0.27, 0.19, 0.001 and 0.002, respectively, and give linear SVPs. The corresponding K_{SV} values were found to be 0.83, 2.82, 1.33, 1.11, and 2.48 $\%^{-1}$, respectively. The lowest detection limit was 0.5% for oxygen in nitrogen gas. However, the response time of these crystals is rather long (> 70 s), and – like in other Ir(III) complexes – the photostability of the crystals is moderate.

Nanocomposites containing cyclometalated Ir(III) emitters also have been used to sense oxygen.²³⁶ They consist of an aluminum oxide-hydroxide nanostructured solid support and a cyclometalated Ir(III) complex as a cover layer. The results were compared to data on the same dyes immobilized in polystyrene films. Since the photoluminescence of the complexes is totally quenched for oxygen concentrations just over 10%, these systems are promising for oxygen detection at low concentration. In particular, dyes on the aluminum support provide sensitivity to oxygen down to 1% of oxygen in a sample gas.

Water-based oxygen sensor films were reported,²³² where a luminescent cyclometalated Ir(III) complex was bound to the water-soluble amino-functionalized polymer silamine. Oxygen-sensor films were prepared using aqueous blends of the conjugate with silamine and colloidal microcrystalline cellulose. Like in other cases, the diffusion of oxygen decreases with increasing fraction of filler and thereby decreases sensitivity. These novel materials offer an environmentally friendly alternative to the preparation of oxygen-sensor films.

Table 5. Luminescent iridium(II) complex-derived probes for oxygen, along with their excitation/emission wavelengths (in nm), quenchability ("sensitivity"), the polymer solvent or support used, and the method for read-out (RO). Quenchability is expressed as either I_0/I_{100} (the ratio of fluorescence intensity at zero % oxygen in the carrier gas and the intensity at 100% oxygen (at atmospheric pressure), or in a fluid equilibrated with such gases. Correspondingly, I_{21} is the intensity under air at atmospheric pressure. *Codes:* I: intensity-based readout; L: lifetime-based readout. SVP: Stern-Volmer plot.

Dye/Matrix	$\lambda_{exc}/\lambda_{em}$	Sensitivity	Comments	RO	Ref.
Ir(ppy) ₃ in poly(styrene-co-TFEM) ⁱ	376/512	$I_0/I_{100} = 15.3$	SVPs; almost linear; short response times ($t_{95} = 7$ s); highly photostable.	I	220
Ir(ppy) ₃ in PS	376/512	$I_0/I_{100} = 1.1$	QY ~ 90%.		
Ir(ppy) ₃ in <i>n</i> BuPTP ⁱⁱ polymer	370/510	$I_0/I_{159\text{ Torr}} = 3.36$	High sensitivity; $\tau_0 = 1.4$ μ s.	I	221
Bu ₄ N[Ir(ppy) ₂ (CN) ₂] in <i>n</i> BuPTP polymer	340/470	$I_0/I_{159\text{ Torr}} = 6.04$	High sensitivity; $\tau_0 = 4.78$ μ s.		
Ir(ppy) ₂ (dpt-NH ₂)PF ₆ in pPEGMA ⁱⁱⁱ	380/490(530)	$I_0/I_{100} = 2.5$	QY _{phos} = 0.25 in acetonitrile; $\tau_0 = 1.3$ μ s	I	216
Ir(L)(L1)(PF ₆) ₂ ^{iv} in pPEGMA	- / ~ 605	$\tau_0/\tau_{100} = 2.76$	$\tau_0 = 2.1$ μ s.		
Ir(L1) ₂ PF ₆ in pPEGMA	- / ~ 615	$\tau_0/\tau_{100} = 1.61$	$\tau_0 = 1.4$ μ s.		
[(ppy)Ir(dpt-cy-dpt)Ir(ppy)](PF ₆) ₂ in pPEGMA	- / ~ 520	$\tau_0/\tau_{100} = 2.90$	$\tau_0 = 1.13$ μ s. Size and charge of the chromophore affect sensitivity (slope).	I, L	219
Ir(ppy) ₂ (vpy ^v)Cl in PDMS silicone	265,396/509	$I_0/I_{100} \sim 1.65$	Covalently attached to H-terminated PDMS; QY _{phos} = 0.32, $\tau_0 = 190$ ns; polymerizable probe; blending with PS improves sensitivity.	I	234
Ir(C _S) ₂ (acac) ^{vi} in PS	448,477/566	$\tau_0/\tau_{175\text{hPa}} \sim 1.51$			
Ir(C _N) ₂ (acac) in PS	421,455/544	$\tau_0/\tau_{175\text{hPa}} \sim 1.5$	Brightness is 5 times that of Ru(dpp) ₃ or PtTFPP; strong visible absorption; less temperature-sensitive than Ru(dpp) ₃ ;		
Ir(C _O) ₂ (acac) in PS	444,472/554	$\tau_0/\tau_{175\text{hPa}} \sim 1.59$	spectral properties fine-tuned by varying the ligand; non-linear SVPs; poor photostabilities. QYs and lifetimes also reported in detail.	L	224
Ir(C _{S-Me}) ₂ (acac) in PS	446,475/566	$\tau_0/\tau_{175\text{hPa}} \sim 1.7$			
(C _S) ₂ Ir(μ -Cl) ₂ Ir(C _S) ₂ in PS	457,484/588	$\tau_0/\tau_{175\text{hPa}} \sim 1.96$			
(C _N) ₂ Ir(μ -Cl) ₂ Ir(C _N) ₂ in PS	432,463/567	$\tau_0/\tau_{175\text{hPa}} \sim 1.85$			
Ir(C _{S-Jul}) ₂ (acac) in PS-PVP nanoparticles ^{vii}	452,481/572	$\tau_0/\tau_{20\text{KPa}} \sim 3.5$	QY = 0.52; $\tau_0 = 20.8$ μ s, (longer than other Ir(III) coumarin complexes); high brightness; poor photostability.	L	227
Ir(ppy-NPh ₂) ₃ in 2-methyl-tetrahydrofuran	405/525,565	$\tau_0/\tau_{\text{air sat}} \sim 170$	QY = 0.70; $\tau_0 = 4.3$ μ s; good solubility in organic solvents and polymers; compatible with 405 nm LEDs; low temperature dependence.	L	223
Ir(ppy-NPh ₂) ₃ in ethyl cellulose		$\tau_0/\tau_{\text{air}} \sim 4.5$			
[Ir(fppy) ₂ (<i>t</i> -Bu-iCN) ₂]CF ₃ SO ₃ on silamine ^{viii}	258,367/496	$\tau_0/\tau_{\text{air}} \sim 3$	QY = 0.35; $\tau_0 = 17.3$ μ s.	I, L	232
[Ir(tpy) ₂ (<i>t</i> -Bu-iCN) ₂]CF ₃ SO ₃ on silamine					

ⁱ ppy = 2-phenylpyridine anion; TFEM = 2,2,2-trifluoroethyl methacrylate

ⁱⁱ *n*BuPTP = poly[(*n*-butylamino)thionylphosphazene]

ⁱⁱⁱ dpt-NH₂ = 4-amino-3,5-di-2-pyridyl-4 *H* 1,2,3,4-triazole; pPEGMA = poly (polyethylene glycol ethyl ether methacrylate)

^{iv} L = 2,6-bis(7'-methyl-4'-phenyl-2'-quinolyl)pyridine; L1 = monoanion of L

^v vpy = vinylpyridine

^{vi} C_S = 3-(benzothiazol-2-yl)-7-(diethylamino)-coumarin; C_N = 3-(1-methylbenzimidazol-2-yl)-7-(diethylamino)-coumarin; C_O = 3-(5-chlorobenzoxazol-2-yl)-7-(diethylamino)-coumarin; C_{N-Me} = 3-(benzothiazol-2-yl)-7-dimethylaminocoumarin, acac = acetylacetonate

^{vii} C_{S-Jul} = 10-(2-benzothiazolyl)-2,3,6,7-tetrahydro-1,1,7,7-tetramethyl-1*H*, 5*H*, 11*H*-(1)benzopyrano(6,7-8*i,j*)quinolizin-11-one; PS-PVP = Poly(styrene-block-vinylpyrrolidone)

^{viii} fppy = 4-(2-pyridyl)benzaldehyde, *t*-Bu-NC = *tert*-butyl isocyanide, tpy = 2-*p*-tolylpyridine

	260,348/458	$\tau_0/\tau_{\text{air}} \sim 3$	QY = 0.28; $\tau_0 = 35.6 \mu\text{s}$. Can be covalently bound to amino-modified polymer; non-linear SVPs; temperature dependent.		
Ir(btpy) ^{ix} in Cellulose acetate butyrate	366,408/596,645	$\tau_0/\tau_{\text{air}} \sim 1.9$	$\tau_0 \sim 8.6 \mu\text{s}$; temperature dependent; excitable with purple LED.	L	237
Ir(C6) ₂ (vacac) ^x Ir(ppy) ₂ (vacac) fac-Ir(ppy) ₂ (vppy) mer-Ir(ppy) ₂ (vppy)	445,474/568 257,400/520 287,384/542 274,390/535		$\tau_0 = 6.0 \mu\text{s}$; QY = 0.22. $\tau_0 = 0.1 \mu\text{s}$; QY = 0.02. $\tau_0 = 0.4 \mu\text{s}$; QY = 0.2. $\tau_0 = 0.2 \mu\text{s}$; QY = 0.03. All these probes carry vinyl groups and can be polymerized into hydride-containing silicones.	I, L	231
Ir-N-948 ^{xi} in PS	494/665	$\tau_0/\tau_{\text{air}} \sim 8.0$	First Ir(III) complex emitting at > 650 nm; high QY and long lifetime (QY = 0.58, $\tau_0 = 102 \mu\text{s}$); good long-term storage stability; non-linear SVPs.	I, L	228
Caged Iridium (III) complex in DMF Hemi-caged Iridium (III) complex in DMF Ir(ppy) ₃ in DMF	462/570 462/580 462/523	$\tau_0/\tau_{\text{air}} = 7.7$ $\tau_0/\tau_{\text{air}} = 9.6$ $\tau_0/\tau_{\text{air}} = 23.7$	$\tau_0 = 1.27 \mu\text{s}$. Suitable for high levels of oxygen. $\tau_0 = 1.20 \mu\text{s}$. Suitable for high levels of oxygen. $\tau_0 = 1.87 \mu\text{s}$.	I, L	230

^{ix} btpy = 2-(benzo[*b*]thiophene-2-yl)pyridinato-C³,*N*

^x C6 = coumarin 6; vacac = vinylacetoacetate, ppy = 2-phenylpyridine, and vppy = 2-(4-vinyl)-phenylpyridine.

^{xi} Ir-N-948 = Ir(2-phenylpyridine)2(4,4'-bis(2-(4-*N,N*-methylhexylaminophenyl)ethyl)-2,2'-bipyridine)Cl

6.2.3. Osmium and Rhenium Complexes

Os(II) polypyridyl complexes represent another kind of commonly used OSPs. Compared to the Ru(II) polypyridyl complexes, they possess high-lying *dd* states which pave the way for an additional decay channel and cause excellent photostability.²³⁸ Complexes of Os(II) are highly toxic! Meyer et al.²³⁸ reported on a series of Os(II) polypyridyl complexes with luminescence lifetimes from 101 to 3462 ns in degassed acetonitrile solution. The excited-state properties can be predictably and precisely designed via variation of ligands, so that sensitivity to oxygen can be adjusted. Some Os(II) polypyridyl complexes can be excited even in the NIR. This makes them very suitable for in vivo biological applications because biological matter is poorly penetrated by shortwave visible and UV light.²³⁹ Quenching of the luminescence by oxygen of a series of Os(II) complexes with α -diimine ligands in polydimethylsiloxane and related polymers was also described.²⁴⁰ Such Os(II) complexes have wide absorption spectra and can be efficiently excited in the green and yellow region by either LEDs or diode lasers. The NIR emissions have a fairly long excited-state lifetime (~ 400 ns; unquenched). However, the response of these Os(II) OSPs to oxygen is weaker than those for analogous Ru(II) complexes, mainly because of their shorter excited-state lifetimes.

Metal-ligand complexes of Re(I) typically have excited-state lifetimes between 0.5 and 5 μ s, large Stokes' shifts, and good photostability. Quenching of the luminescence by oxygen shows a high degree of heterogeneity in silicone polymers.^{241, 242} Such a microheterogeneity induces nonlinear Stern-Volmer plots that can be described by the two-site model (see **Section 5**). The Re(I) complexes display exceptionally strong luminescence (with QYs of up to 0.7) and strong quenching by oxygen. However, they easily photodegrade on exposure to oxygen. The same group²⁴³ also synthesized and tested the complexes $\text{ReL}(\text{CO})_3\text{Cl}$ and $\text{ReL}(\text{CO})_3\text{CN}$ (where L represents the ligand, these including *bpy*, *terpy*, *dpp*, $\text{Me}_2\text{Ph}_2\text{phen}$, and Me_4phen). The cyano complexes are poorly photostable in polymers,²²¹ but the chloro complexes are fairly photostable and have both long excited-state lifetimes and good QYs.

The excited-state properties of such Re(I) complexes are strongly influenced by ligand variation. The introduction of a phenanthroline ligand increases sensitivity to oxygen and lengthens the decay time. The introduction of *t*-butyl groups into the *bpy* ligand also results in greater sensitivity and a longer decay. However, the addition of two methyl groups to the *Ph}_2\text{phen} group has an adverse effect. The Re(I) complexes with *terpy* as the ligand have the shortest lifetimes and lowest sensitivities to oxygen. The ligand *terpy* is also a poor ligand for luminescent Ru(II) complexes, and the $\text{Ru}(\text{terpy})_2^{2+}$ complex even is non-luminescent at room temperature.*

All these OSPs display nonlinear SVPs and relatively low sensitivity to oxygen. This makes

them suitable, however, for sensing high-level barometric (in fact oxygen) pressure such as in wind tunnels. The Lakowicz group has described²⁴⁴ hydrophobic probes such as cis-Re(CO)₂(c-dppene)(dpp) and the water-soluble equivalent cis-Re(CO)₂(c-dppene)(SO₃-dpp), where *c-dppene* stands for cis-[bis(diphenylphosphino)ethylene]. Both OSPs are highly emissive, have excited-state lifetimes of around 10 μs, and are strongly quenched by oxygen, but photostability is moderate. A recent article²⁴⁵ describes the first Re(I)-dipyrinato complexes for sensing dissolved oxygen. They have fairly large molar absorption coefficients ($2.5 - 4.2 \times 10^4 \text{ M}^{-1} \text{ cm}^{-1}$) and Stokes' shifts, but their QYs are low (< 0.01) so that brightness is inadequate. An oxygen-quenchable luminescent Re(I) complex containing a carbazole “shield” in its diamine ligand was applied²⁴⁶ in a poly(vinylpyrrolidone) host to sense oxygen with high sensitivity ($I_0/I_{100} = 20.5$) and short response/recovery times (6 s and 28 s), and a Re(I) complex was used to dope nanofibers so to obtain optical nanosensors for oxygen.²⁴⁷

All Re(I) complexes show high emission anisotropies which makes them attractive probes for polarization. On the other hand, they lack significant absorption beyond 400 nm and their molar absorptions often are 3 times smaller (at 370 - 380 nm) than those of Ru(II) complexes at 450 nm. Figures of merit for oxygen sensors based on osmium and rhenium complexes are summarized in **Table 6**.

Table 6. Luminescent osmium(II) and rhenium(II) derived probes for oxygen, along with their excitation/emission wavelengths (in nm), quenchability ("sensitivity"), the polymer solvent or support used, and the method for read-out (RO). Quenchability is expressed as either I_0/I_{100} (the ratio of fluorescence intensity at zero % oxygen in the carrier gas and the intensity at 100% oxygen (at atmospheric pressure), or in a fluid equilibrated with such gases. Correspondingly, I_{21} is the intensity under air at atmospheric pressure. Codes: I: intensity-based readout; L: lifetime-based readout. SVP: Stern-Volmer plot.

Dye/Matrix	$\lambda_{exc}/\lambda_{em}$	Sensitivity	Comments	RO	Ref.
Os(dpp) ₃ (PF ₆) ₂ in PDMS rubber	480(502)/729	$I_0/I_{air} = 1.1$	PDMS contains (methacroyloxy)propyl side chains; $\tau_0 = 340$ ns.	I, L	240
Os(dpp) ₃ (PF ₆) ₂ in PDMS rubber	480(502)/729	$I_0/I_{air} = 1.7$	Methyl diacetoxo terminated PDMS; $\tau_0 = 200$ ns.		
Os(trpy) ¹ ₂ ²⁺	698/729	$\tau_0/\tau_{air} > 6.73$	---		
(trpy)(dppene)OsCl ⁺	624/718	$\tau_0/\tau_{air} > 2.53$	---		
Os(phen) ₃	650/720	$\tau_0/\tau_{air} = 1.39$	QY = 0.013		
(phen) ₂ Os(MeCN) ₂ ²⁺	600/688	$\tau_0/\tau_{air} = 4.28$	QY = 0.035		
(phen) ₂ Os(Me ₂ PPh) ₂ ²⁺	590/672	$\tau_0/\tau_{air} = 1.84$	QY = 0.072		
(bpy) ₂ Os(dppm) ²⁺	480/652	$\tau_0/\tau_{air} = 1.64$	QY = 0.046		
(phen) ₂ Os(dppm) ²⁺	500/624	$\tau_0/\tau_{air} = 4.85$	QY = 0.12	I, L	238
(phen) ₂ Os(dppene) ²⁺	455/609	$\tau_0/\tau_{air} = 5.00$	QY = 0.20		
(bpy) ₂ Os(das) ²⁺	450/592	$\tau_0/\tau_{air} = 2.95$	QY = 0.22		
(bpy) ₂ Os(Me ₂ SO) ₂ ²⁺	443/575	$\tau_0/\tau_{air} = 2.23$	QY = 0.31		
(bpy)Os(dppene) ₂ ²⁺	400/537	$\tau_0/\tau_{air} = 1.22$	QY = 0.47		
(3,4,7,8-Me ₄ phen) ₂ Os(dppene) ²⁺	450/594	$\tau_0/\tau_{air} = 5.59$	QY = 0.17		
			All data for acetonitrile solutions. Excellent photostability; some emitting in the NIR region.		
Re(phen)(CO) ₃ CN in silicone RTV rubber	385/520	$I_0/I_{air} = 2.5$	Other polypyridyl ligands also tested; photolabile; multi-exponential decay; non-linear SV plots	I, L	241
Re(bpy)(CO) ₃ Cl in GP-163-co-T3642 ⁱ	388/540	$I_0/I_{100} = 1.5$			
Re(dpp)(CO) ₃ Cl in GP-163-co-T3642	388/540	$I_0/I_{100} = 3.9$			
Re(Me ₄ phen)(CO) ₃ Cl in GP-163-co-T3642	388/540	$I_0/I_{100} = 3.7$			
Re(<i>t</i> -Bu) ₂ bpy(CO) ₃ Cl in GP-163-co-T3642	388/540	$I_0/I_{100} = 1.7$			
Re(terpy)(CO) ₂ Cl in GP-163-co-T3642	388/540	$I_0/I_{100} = 1.2$			
Re(Me ₂ Ph ₂ phen)(CO) ₃ Cl in GP-163-co-T3642	388/540	$I_0/I_{100} = 3.4$			
[Re(CO) ₃ (bpy)(CN- <i>t</i> -Bu)]Cl in <i>n</i> BuPTP ⁱⁱⁱ polymer	340/507	-	Poor sensitivity and serious photodecomposition.	I	221

ⁱ trpy = 2,2',2''-terpyridine, dppene = *cis*-bis(1,2-diphenylphosphino)-ethylene, Me₂PPh = dimethylphenylphosphine, dppm = bis(diphenyl phosphino)methane, das = *o*-phenylenebis(dimethylarsine), Me₂SO = dimethyl sulfoxide,

ⁱⁱ GP-163 = acrylate containing PDMS; T3642 = trimethylsilylmethyl methacrylate

ⁱⁱⁱ *n*BuPTP = poly(*n*-butylamino)thionylphosphazene)

6.2.4. Lanthanide Complexes

Lanthanide ions coordinated with sensitizers exhibit intense and narrow emission bands under photoexcitation at 300 – 330 nm (in most cases, see **Table 7**). The luminescence of lanthanide complexes often strongly depends on temperature, and they therefore also may be used to probe temperature. Amao et al.^{248, 249} have systematically studied the oxygen sensing properties of several europium complexes in a poly(styrene-*co*-TFEM) fluoropolymer (also see **Section 7.1.2**). These OSPs display pink luminescence (peaking at 612 nm) with a good QY and long lifetime. The sensitivity to oxygen strongly depends on the ligands, the highest sensitivity (I_0/I_{100}) being 2.4 which makes these OSPs useful for moderately high levels of oxygen only, but not for trace level. SVPs are linear, and responses are fully reversibly. Europium complexes with much lower sensitivity (and for use at higher partial pressures of oxygen)^{250, 251} and those with much higher oxygen sensitivity^{252, 253} also have been described by the Amao group.

Terbium(III) complexes emit green luminescence peaking at 546 nm. The Tb(acac)₃(phen) complex was synthesized and adsorbed on silica (an alumina plate as used for TLC) to test it for the quenching of its luminescence by oxygen.^{254, 255} Its QY is 0.5, and lifetimes can be as long as several ms. Its luminescence is more efficiently quenched by oxygen than that of the europium complex. Terbium(III) complexes with an azaxanthone sensitizer and a naphthyl group also are sensitive to oxygen, while the corresponding europium complexes are not.²⁵⁶ This finding may be used for ratiometric (2-wavelength) sensing of oxygen. However, most lanthanide OSPs have to be excited in the UV region. OSPs that can be excited with blue light were first reported by Borisov et al.²⁵⁷ The complexes of Eu(III) and Gd(III) were incorporated into a film of poly(styrene-*co*-4-N-acridonomethylstyrene) film, where the acridone group act as light-harvesting antenna and the absorbed energy is transferred to the Eu(tta)₃ and Gd(tta)₃ complexes. These Eu(III) complexes possess bright red room temperature luminescence in polymers (with a QY of ~20% and a lifetime ~100 μs), while the Gd(III) complexes emit orange light (QY ~50%, lifetime ~2 ms). Both emissions are efficiently quenched by molecular oxygen.

Table 7. Luminescent lanthanide(II) complex-derived sensor materials for oxygen, along with excitation/emission wavelengths (in nm), quenchability ("sensitivity"), the polymer solvent or support used, and the method for read-out (RO). Quenchability is expressed as either I_0/I_{100} (the ratio of fluorescence intensity at zero % oxygen in the carrier gas and the intensity at 100% oxygen (at atmospheric pressure), or in a fluid equilibrated with such gases. Correspondingly, I_{21} is the intensity under air at atmospheric pressure. Codes: I: intensity-based readout; L: lifetime-based readout. QY: quantum yield; SVP: Stern-Volmer plot.

Dye/Matrix	$\lambda_{exc}/\lambda_{em}$	Sensitivity	Comments	RO	Ref.
Eu(tta ⁱ) ₃ phen in poly(styrene-co-TFEM)	342/612	$I_0/I_{100} = 2.4$	Moderate sensitivity to oxygen; potentially useful at high air pressures such as in wind tunnels; linear SVPs; response time 6 - 7 s.	I	248
Eu(tta) ₃ in poly(styrene-co-TFEM)	342/612	$I_0/I_{100} = 1.5$			
Eu(fod) ₃ in poly(styrene-co-TFEM)	293/612	$I_0/I_{100} = 1.27$			
Eu(pta) ₃ in poly(styrene-co-TFEM)	295/612	$I_0/I_{100} = 1.19$			
Eu(tta) ₃ (phencarz) ⁱⁱ in polystyrene nanofiber	326/612	$I_0/I_{100} = 3.38$	Nanofiber was prepared via electrospinning; response time 5.0 s, recovery time 8.0 s; downward curved SVPs.	I	258
Tb(acac ⁱⁱⁱ) ₃ (phen) on silica alumina plate (for TLC)	268/546	$I_0/I_{100} = 2.68$	Static quenching dynamic competes with quenching; non-linear SVP; highly photostable; UV excitation; QY _{phos} = 0.11.	I	254 255
Tb(III) azaxanthone complex	355/480,540	$I_0/I_{100} \sim 1.5$	Corresponding Eu(III) complex is insensitive to oxygen; mixture of Eu(III) and Tb(III) complex used for ratiometric oxygen measurement; efficient generation of singlet oxygen; cell permeable.	I	256
Ga(TTA) ₃ in poly(styrene-co-4-N-acridonomethylstyrene)	400/514	$\tau_0/\tau_{100 \text{ kPa}} \sim 1.13$	Both the Ga(TTA) ₃ and Eu(TTA) ₃ were encapsulated into the poly(styrene-co-4-N-acridonomethylstyrene) film, the acridone group in the polymer acts as antenna to absorb blue light and the energy transferred to both probes; high brightness, compatible with a 405-nm LED.	IL	257
Eu(TTA) ₃ in poly(styrene-co-4-N-acridonomethylstyrene)	400/617	$I_0/I_{8.5 \text{ kPa}} \sim 8.0$			

ⁱ tta = thenoyltrifluoroacetate; fod = 1,1,1,2,2,3,3-heptafluoro-7,7-dimethyl-4,6-octadionate; pta = 1,1,1-trifluoro-5,5-dimethyl-2,4-hexandionate

ⁱⁱ phencarz=2-(N-ethylcarbazolyl-4)imidazo[4,5-f]1,10-phenanthroline)

ⁱⁱⁱ acac = acetylacetone

6.2.5. Porphyrins and Metalloporphyrins

Optical oxygen sensor devices using porphyrins and, in particular, metalloporphyrins are among the most common.²⁴ The phosphorescence and the fluorescence (less so) of porphyrins complexed with platinum(II), palladium(II), zinc(II), and of the metal-free forms is strongly quenched by oxygen. This is valid for both either surface-adsorbed species and for (metallo)porphyrins in solid matrices, and the effect has been often exploited to measure oxygen concentration. (Metallo)porphyrins have strong absorptions (with molar absorbances of up to $150,000 \text{ M}^{-1} \text{ cm}^{-1}$) between 390 and 420 nm (the so-called *Soret* bands), and weaker ($>10,000 \text{ M}^{-1} \text{ cm}^{-1}$; the so-called Q-bands) at $>500 \text{ nm}$. Obviously, the brightness of the indicators is much higher if they are photoexcited via the *Soret* band.

Tetraphenylporphyrin (TPP) without a central metal ion can be photoexcited at wavelengths between 520 and 550 nm, for example with LEDs. Adsorbed on porous polystyrene,²⁵⁹ two fluorescence bands with peaks at 650 and 720 nm can be seen that and probably originate from the monomer and dimer species. Fluorescence is quenched by ca. -60% and -55% at 650 and 720 nm, respectively, in going from an oxygen-free environment to pure oxygen. TPP on polystyrene is moisture-insensitive, but the emission strongly depends on temperature. TPPs are not often used for purposes of sensing oxygen because of their poor photostability and for other reasons.

6.2.5.1 Conventional Metalloporphyrins

Metalloporphyrins (for chemical structure see **Figure 11**), while completely insoluble in water unless chemically modified, display fairly good solubility in many organic polymers but tend to aggregate at higher concentrations. Other features include (1) intense and sharp red luminescence with *Stokes'* shifts of up to 250 nm; (2) luminescence lifetimes in the order of hundreds of microseconds in the absence of oxygen; (3) good chemical stability, in particular if fluorinated; and (4) tunable excitation and emission spectra by peripheral substitution.²⁶⁰ Eastwood and Gouterman²⁶¹ screened a large number of cobalt(II), nickel(II), platinum(II) and palladium(II) porphyrin complexes. The Pt(II) and Pd(II) metalloporphyrins display strong phosphorescence and long lifetimes, both of which are strongly reduced in the presence of oxygen. They suggested the use of PtTPP and PdTPP as OSPs. Ever since, such kinds of metalloporphyrins have been widely used.

In general, the Pd(II) metalloporphyrins have much longer lifetimes and higher sensitivity to oxygen than their Pt(II) analogs. This can be attributed to increased spin-orbit coupling of the heavier metal ion.²⁶¹ On the other side, the Pt(II) complexes have 2 – 3 times higher emission QYs than those of the respective Pd(II) metalloporphyrins. Initially, the Pt(II) and Pd(II) complexes of


coproporphyrin (CP), octaethylporphyrin (OEP), and TPP have been used. Wilson et al.^{51,262} studied the quenching of the phosphorescence of PdCP to image oxygen in cells and tissue, and PdTPP was deposited in organized monolayer assemblies using the Langmuir-Blodgett technique.²⁶³ The monolayers were coated onto an optical fiber to give a respective sensor. PtOEP, dissolved in silicone rubber, also was used in the first paint for sensing air pressure in wind tunnel tests.²⁶⁴ PtOEP has a QY of 0.42, and its red luminescence (peaking at 650 nm) is strongly quenched by oxygen.²⁶⁵ However, PtOEP easily photodegrades on exposure to shortwave light due to photooxidation of the porphyrin ring.²⁶⁴

In order to improve photostability, several halogen-substituted platinum porphyrins (PtTDCPP, PtTFMPP, PtBr₈TMP; see **Table 8**) were synthesized and studied, in silicone rubber films,²⁶⁶ with respect to photostability and suitability to sense oxygen. The incorporation of halogenated substituents into the porphyrin ligand can substantially increase photostability, but lifetimes and QYs are decreased. Not unexpectedly, the introduction of heavy halogen atom such as bromine causes a further decrease in QY and lifetime. Fluorine, in contrast, is an excellent choice as a substituent to improve photostability. It generally renders porphyrins and other dyes more photostable. The fluorine-substituted porphyrin PtTFPP has become the most often used OSP among the metalloporphyrins.⁵³ It has three main absorption bands, viz. an intense Soret band peaking at 395 nm, and two Q absorption bands at 508 and 540 nm, respectively, which are much weaker. The four electron-withdrawing pentafluorophenyl substituents raise the redox potentials and the electron density of the probe. This renders PtTFPP even more photostable than Ru(dpp). In addition, PtTFPP is less sensitive to temperature than Ru(dpp).

PtTFPP also is highly photostable in polymers such as polystyrene and therefore well suited for long-term continuous monitoring of oxygen.²⁶⁷ If continuously photoexcited at the Q bands at 508 or 540 nm for 50 h, the decreases in emission intensity (at 650 nm) are only 9% and 15%, respectively. PtTFPP also was immobilized in the fluoropolymer PTFEM (see section 7) where it was found²⁶⁸ to be quite photostable. On continuous irradiation for 24 h, only minimal deterioration (~0.5 %) was observed. The resulting oxygen sensor material has better sensitivity (the I_0/I_{100} ratio is 15.4) compared to that of the same probe in polystyrene ($I_0/I_{100} = 3.0$), and the response time was reduced to 5.6 s.

The brightness of PtTFPP can be further enhanced using light-harvesting antennas. This approach is particularly beneficial because luminescent sensor films as thin as < 0.5 μm can be produced that still possess an adequate signal-to-noise ratio.²⁶⁹ The palladium analogue (PdTFPP) has an exceptionally long lifetime (~1 ms at room temperature), and has such a high sensitivity that it can only be used to sense oxygen at trace levels (from 0.02 to 100 Pa).²⁷⁰ Also see the section on low-level oxygen sensors.

Figure 11. Chemical structures of major OSPs based on metalloporphyrins. M stands for a metal ion such as Pt(II) or Pd(II). Complexes with trivalent ions such as Ir(III) also have been reported but require an additional (axial) ligand.

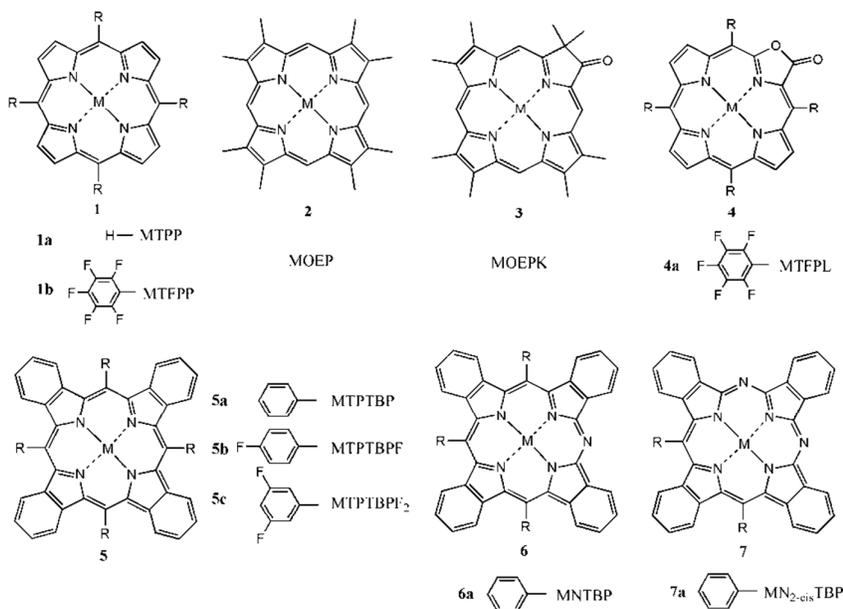

6.2.5.2 Metalloporphyrins with large Q-band absorption and NIR emission


As was stated before, the probe PtTFPP has outstanding photophysical properties in terms of oxygen sensing, the weak Q bands being the only shortcoming. This situation was (partially) improved by synthesizing metalloporphyrins possessing much stronger Q-band absorptions, for examples the various porphyrin lactones, porphyrin ketones, benzoporphyrins, and azatetrabenzoporphyrins.²⁷¹⁻²⁷³ Simultaneously, the emission bands were shifted to the NIR. For example, the probe PtTFPL has a fairly strong absorption of its Q-band centered at 550 nm, while the emission peak is red-shifted to 730 nm (compared to that of PtTFPP at 650 nm). The probe is more sensitive to oxygen than PtTFPP. Its unquenched lifetime is 72 μ s, and luminescence is less sensitive to temperature than PtTFPP. The Pd(II) analog (PdTFPL) has an even longer lifetime of \sim 1 ms. Both probes are quite resistant to photo-oxidation because of the presence of a lactone functionality.²⁷⁴

Fluorinated complexes of Pt(II) and Pd(II) with *meso*-substituted benzoporphyrins represent another group of longwave absorbing and NIR-emitting probes.²⁷⁵⁻²⁷⁷ Such fluorinated probes are more photostable, and their emission bands extend to above 800 nm. This is an analytical wavelength that is hardly interfered by background luminescence. They possess intense Soret bands and fairly strong Q-band absorptions, and thus can be effectively excited with blue or red LEDs or lasers. The *meso*-substituted benzoporphyrins do not tend to aggregate in nonpolar polymers. Compared to classical metalloporphyrins such as PtTFPP and PtOEP, the benzoporphyrins display a more intense second Q-band absorption and higher QYs, some having QYs exceeding those of PtOEP (0.415).

As was to be expected in view of their longer lifetimes, the respective Pd(II) complexes are more sensitive to oxygen than the Pt(II) probes. Dissolved in polystyrene, the latter are ideally suited for sensing oxygen partial pressures up to air pressure, and both of gaseous and fluid samples. The Pd(II) complexes, on the other hand, are more adequate for sensing low levels of oxygen because their luminescence is almost completely quenched at air saturation. The Pd(II)benzoporphyrins are more prone to thermal quenching than the Pt(II) complexes. All these OSPs have good photostability, the Pt(II) complexes in particular. Fluorination of the benzo ring resulted in a further red shift of the Q-band and the emission band, and also improves photostability, however at the expense of phosphorescence QY. Among the fluorinated metal benzoporphyrin complexes, Pt(II) *meso*-tetra(4-fluorophenyl) tetrabenzoporphyrin (PtTPTBPF) has the highest brightness and photostability. Its synthesis is difficult, however.

Papkovsky^{278, 279} et al. have synthesized the blue Pt(II) and Pd(II) complexes of certain ketoporphyrins (PtOEPK). Their absorptions peak at around 590 nm, and this makes them compatible with yellow LEDs. In addition, they display large Stokes' shifts, almost linear Stern-Volmer plots in polystyrene, and excellent sensitivity to oxygen. All Pt(II) and Pd(II) complexes of porphyrin lactones and ketoporphyrins have relatively intense absorptions at 570 – 600 nm, but QYs are moderate. Borisov et al.²⁸⁰ reported on Pt(II) and Pd(II) complexes of azatetrabenzoporphyrins. The strong Q-band absorptions were found to be excellently compatible with the 635-nm laser diode (**Figure 12**), and the strong NIR phosphorescence is efficiently quenched by oxygen. The luminescence decay times are shorter than those of the respective TPTBP complexes, and this enabled the design of less sensitive probes with wider analytical range. The QYs are lower (~ 0.1) than those of the TPTBP complexes, especially for the case of Pd(II) azatetrabenzoporphyrins, their synthesis is more complicated, and the solubility in organic polymers is limited.

Figure 12. Absorption spectra of the Pt(II) and Pd(II) complexes with azatetrabenzoporphyrins NTBP and N_2 -cisTBP. The Q-band absorption is very intensive and compatible with laser diodes. (Reprinted from ref.²⁸⁰ with permission from the American Chemical Society)

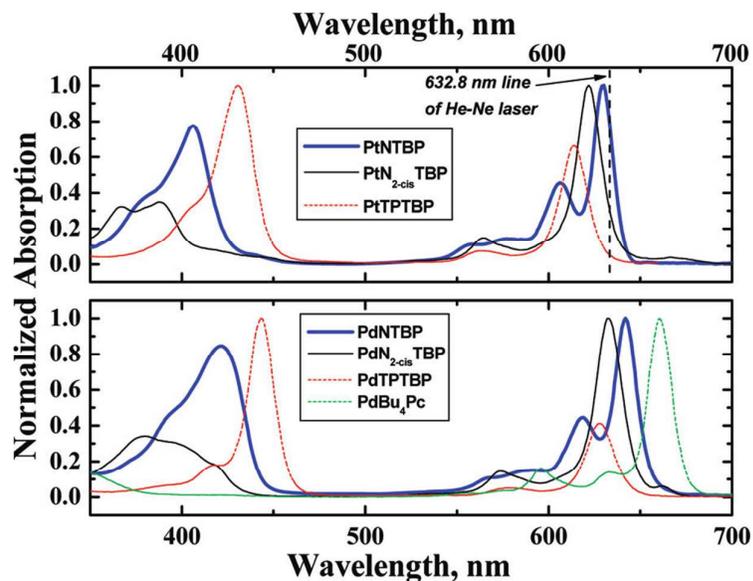


The absorption and emission peaks of porphyrins were further longwave shifted by extending the π -system. The Vinogradov group²⁸¹ described metal complexes of tetranaphthoporphyrin (TNP) which, compared to the respective tetrabenzoporphyrins, have red-shifted Q-band absorptions and longwave emissions, but their QYs are smaller (0.22 for PtTPTNP; 0.08 for PdTPTNP), as are their photostabilities. Other π -extended hybrid benzo- and naphthoporphyrin complexes of Pt(II) and Pd(II) were reported²⁸² with tuned spectral properties, intense absorption in the NIR region (628 – 691 nm), and emissions peaking between 815 and 882 nm. It was observed that both the QY and luminescence decay time decrease with increasing number of naphtho groups in the system.

Many tetraarylporphyrins and their Pt(II) complexes were investigated with respect to uses in sensors for oxygen.²⁸³ The Pt(II) complexes of tetraphenylporphyrin, tetranaphthoporphyrin, and tetrapyrrenyl-porphyrins possess rather similar photophysical properties. Placed in polymer films, both the emission intensity and lifetime are quenched by oxygen. The naphthyl derivatives display better sensing capability, with a quenching constant (K_{SV}) of 0.068 Torr^{-1} (versus 0.040 Torr^{-1} for the parent tetraphenyl derivative).

The Ir(III) porphyrin complexes form a rather recent class of OSPs.²⁸⁴ The photophysical properties of these hexa-coordinated complexes can be tuned by changing the axial ligands. The neutral Ir-OEP-CO-Cl complex has a good QY (0.21) and its emission is quite sensitive to oxygen, and the lifetime is 97 μs . By proper choice of the axial ligand, the solubility of the complexes in polymers can be improved. Respective structures are shown in **Figure 13**. The axial ligand may also be modified with functional groups for covalent coupling, for example to a peptide.²⁸⁵

Figure 13. Chemical structures of the four Ir-octaethylporphyrin complexes. The change of axial ligand with functional group is beneficial for post-modification and coupling. (Reprinted from ref.²⁸⁴ with permission from Wiley-VCH).

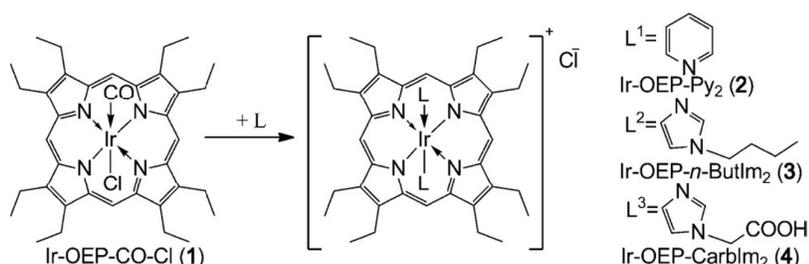

6.2.5.3 Water-soluble Metalloporphyrins

Water-soluble porphyrins, in contrast to the former ones, are useful for sensing dissolved oxygen in aqueous solutions. Vasil'ev and Borisov²⁸⁶ synthesized water-soluble cationic complexes of Pt(II), Pd(II) and Rh(III) with the water-soluble porphyrins *meso*-tetrakis (4-*N*-methylpyridyl)porphyrin and *meso*-tetrakis (4-*N,N,N*-trimethylaminophenyl)porphyrin. The resulting cationic metalloporphyrins have been immobilized on (anionic) ion-exchange films of the Nafion type to result in sensitive, stable and fast-responding sensor films. Linear Stern-Volmer plots were obtained over the entire range of oxygen partial pressure.

The Pt(II) and Pd(II) complexes of coproporphyrins represent another kind of water-soluble OSPs.^{287, 288} They are non-toxic, have high phosphorescence QY and relatively long decay times at room temperature, but photostabilities are not excitingly good. Papkovsky et al.²⁸⁹ synthesized the hydrophilic coproporphyrin ketones PtCPK and PdCPK. They are water-soluble, display acceptable photostability and red-shifted emission in the NIR (PtCPK: λ_{em} 767 nm; PdCPK: λ_{em} 796 nm). Moreover, they can be photo-excited at 370 – 410 nm (Soret bands) or, less efficiently, at 580 – 600 nm (Q bands). Compared to the Pt(II) and Pd(II) coproporphyrins, the PtCPK and PdCPK probes have enhanced Q-band absorbance, and the emissions are red-shifted by ~60 nm. The relatively strong Q-band absorbance and intense NIR emission make these probes viable intracellular OSPs.²⁹⁰ Unlike PtOEPK or PdOEPK (which have very high quenchability), the two probes exhibit moderate sensitivities to oxygen (τ_0/τ_{100} is 1.7 and 4.44 for PtCPK and PdCPK, respectively), which is kind of unexpected.

The water-soluble Pt(II) and Pd(II) *meso*-tetra[4-carboxyphenyl]porphine (TCPP) were also shown to be useful OSPs. Both the dissolved form (for intracellular studies²⁹¹⁻²⁹³) and the adsorbed form (on silica²⁹⁴⁻²⁹⁶) for sensing gaseous oxygen were studied. They do not exhibit high QYs or long lifetimes. However, the carboxy groups enable further modifications in that they can be functionalized with positively charged groups for promoting the loading efficiency into cells.²⁹⁷ Alternatively, they may be covalently linked to peptides and loaded into cells without any transfer

reagent.²⁹⁸

6.2.5.4 Functionalized Metalloporphyrins


In order to render metalloporphyrins conjugatable to solid matrices they have to be functionalized. For example, a PtTPP derivative with a polymerizable methacrylate group was prepared and copolymerized with the host polymer IBM-*co*-TFEM (see **Section 7**).²⁹⁹ The introduction of the methacrylate group and copolymerization did not influence its oxygen sensing properties. The resulting copolymer has good oxygen sensitivity, and the SVPs are linear, which indicates that chemical binding to the polymer backbone does not result in large microheterogeneity. In contrast, a sensing film prepared by dissolving PtTPP in poly-IBM-*co*-TFEM has a downward curved Stern-Volmer plot (SVP). Similar findings were reported by Tian et al.³⁰⁰ who modified PtTPP with a polymerizable group to obtain an oxygen sensitive monomer. The monomer was copolymerized with hydroxyethyl methacrylate and acrylamide to give a hydrophilic sensor film. A polymerizable pH probe was also incorporated so that a dually (pH- and oxygen-)responsive material was obtained that has green and red emission spectra. No toxicity to HeLa cells was detectable after 40 h of incubation. The groups of Tian³⁰¹ and Lu et al.³⁰² have chemically modified PtTFPP with hydroxyethyl methacrylate (HEMA) moieties in order to cross-link it with acrylamide and styrene. The poly-HEMA matrix is more suitable than polystyrene (PS) for sensing dissolved oxygen, because sensitivity in poly-HEMA is higher than that in PS, and response is faster. Compared to sensing films prepared by physical entrapment of PtTFPP in polymers, chemical cross-linking alleviated the leaching problem and improved photostability. PtTFPP also was modified³⁰³ with a silane group and covalently attached to the network of a sol-gel and an organically modified sol-gel. The modification of PtTFPP or PdTFPP with thiol group enables them to be covalently attached to polymer or a silica matrix.³⁰⁴ No leakage of the OSPs does occur as a result.

6.2.5.5 Metalloporphyrins that Undergo Two-Photon Excitation

The Soret band of Pt(II) and Pd(II) porphyrin-based phosphorescent OSPs is in the near UV region, and this causes substantial autofluorescence in case of biological samples. The Q band may also be used for excitation, but at the expense of brightness because the molar absorption coefficients of the Q bands are much weaker. Two-photon excitation (2-PE; typically performed at > 700 nm) provides an alternative, but commonly used metalloporphyrins exhibit extremely low two-photon absorption cross-sections. Vinogradov et al.³⁰⁵ designed several water-soluble Pt(II) porphyrin-coumarin based dendrimers, in which 2-photon absorbing antennas (the coumarin moieties) were coupled to the metalloporphyrin core (see **Section 9.5**). The introduction of an antenna largely improves 2-PE via intermolecular energy transfer. The resulting metalloporphyrin-antenna construct was further

incorporated in a protecting dendritic jacket to isolate the core from interactions with biological macromolecules, to control diffusion of oxygen, and to make the entire sensor water-soluble. Combined with multi-photon laser scanning microscopy, 3D imaging of oxygen with submicron spatial resolution was accomplished. The same group³⁰⁶ synthesized the highly phosphorescent Pt(II) porphyrin poly(arylglycine) dendrimer and used it for mapping oxygen in brains of mice and rats. Again, several coumarin units were attached at the periphery of the dendrimer to efficiently capture 2-photons and to transfer their energy nonradiatively to the Pt(II) porphyrin. Upon excitation with light of wavelength 780 nm, Pt(II) porphyrin undergoes fast intersystem crossing to its triplet state and emits phosphorescence which is quenched by molecular oxygen. Another phosphorescent probe, referred to as PtP-C343 (**Figure 14**), is based on the photonic energy transfer from a coumarin antenna unit to a Pt(II)tetrabenzoporphyrin, and this also enables 2-PE in the NIR region.^{307, 308} Lecoq et al.³⁰⁹ employed this in combination phosphorescence lifetime microscopy to image oxygen partial pressure in the brain at depths up to 300 μm with μm - resolution. In addition, the method allowed simultaneous measurements of blood flow and of oxygen in capillaries. Sensory stimulation evokes functional hyperemia, accompanied by an increase in $p\text{O}_2$ in capillaries. Two-photon laser scanning microscopic imaging of $p\text{O}_2$ opens new avenues for studies of brain metabolism and blood flow regulation.

Figure 14. Two-photon-enhanced oxygen probe PtP-C343 consisting of phosphorescent Pt meso-tetraarylporphyrin (PtP, red), several coumarin-343 units (C343, blue), polyarylglycine dendrimer (black) and peripheral oligoethyleneglycol residues (green). Arrows in the cartoon depict excitation of the C343 antenna via 2PA (brown), FRET (yellow) and phosphorescence of PtP-core (red). (Reprinted from ref.³⁰⁷ with permission from Wiley-VCH)

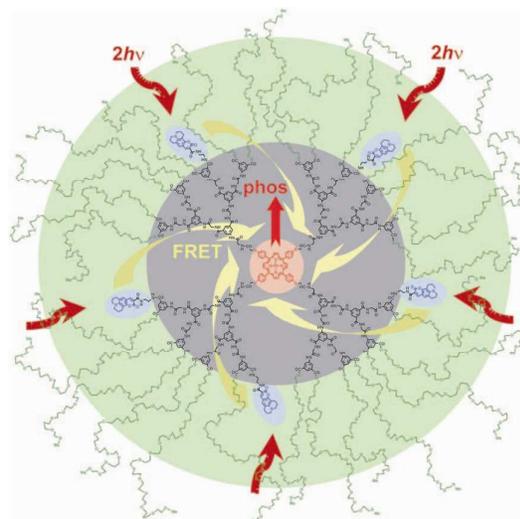

6.2.5.6. Metalloporphyrins for Sensors with Visual (Bare-Eye) Read-out

Sensing oxygen with bare eyes via luminescent probes becomes possible if luminescence occurs in the visible and has strong intensity which is the case when using porphyrin-based OSPs. The human eye can identify ~ 10 million color types. This was exploited³¹⁰ in a two-color sensor where the green (and constant) luminescence of an inert dye serves as the color background, while the red

emission of a porphyrin OSP varies in color according to the actual oxygen pressure. This sensing scheme has a kind of "traffic light response". The contrast can be further improved³¹¹ by using the emission of a green LED as the background and the red emission of PtOEP as the signal. The green LED also photoexcites the luminescence of the OSP. In yet another kind of visual-readout oxygen sensor,³¹² quantum dots with green background luminescence were placed in a sol-gel film, while the red emission of the oxygen probe PtTFPP yields the analytical information. The colors of the sensors at various oxygen concentrations are shown in **Figure 15**. A resolution of up to 1.0 % is accomplished even with visual inspection. All these approaches are making the quantitation of oxygen simple and convenient.

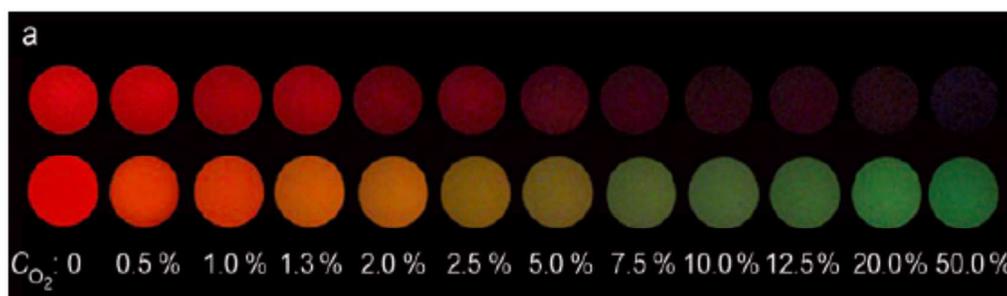


Figure 15. The apparent colors of luminescence colorimetric oxygen sensor without (upper) and with (lower) green-color background at different oxygen concentrations. (Reprinted from ref.³¹² with permission from Wiley-VCH)

Quantitative oxygen sensing and imaging also was accomplished with a photographic technique³¹³ in which a colorimetric oxygen sensor is used to quantitatively image ("photographing") oxygen. The technique is convenient in that it can be performed by unskilled persons, and simple in that a commercial camera (along with software that processes the data stored in the memory of the camera) can be applied (see **Section 9.10.1**). A similar system is commercially available (www.presens.de).

Table 8. Luminescent metalloporphyrin-based probes for oxygen, along with their excitation/emission wavelengths (in nm), quenchability ("sensitivity"), the polymer solvent or support used, and the method for read-out (RO). Quenchability is expressed as either I_0/I_{100} (the ratio of fluorescence intensity at zero % oxygen in the carrier gas and the intensity at 100% oxygen (at atmospheric pressure), or in a fluid equilibrated with such gases. Correspondingly, I_{21} is the intensity under air at atmospheric pressure. *Codes:* I: intensity-based readout; L: lifetime-based readout. I-RTP: intensity-based room temperature phosphorescence; QY: quantum yield; SVP: Stern-Volmer plot. For other acronyms see the list in Section 14.

Dye/Matrix	$\lambda_{exc}/\lambda_{em}$	Sensitivity	Comments	RO	Ref.
H ₂ TPP ⁱ in plastic-clad silica particles	590/650	$I_0/I_{100} \sim 1.54$	Dye adsorbed on particles from solution; some photobleaching; intensity decreases on storage due to diffusion of the dye in the polymer.	I	314
PtOEP in TEOS sol-gel	586/645	$I_0/I_{100} = 41$	Preparation time ~1 month; response time up to 9 min.	I	315
PtOEP in TEOS sol-gel	535/646	$I_0/I_{100} \sim 8.5$	Addition of surfactant improves film homogeneity and results in crack-free monoliths.	I	316
PtOEP in polystyrene (PS) PtOEP in PMMA PtOEPK in PS PdOEP in PS Ru(dpp) ₃ in PS	535/640 535/640 592/760 545/670 450/600	$\tau_0/\tau_{air} = 5$ $\tau_0/\tau_{air} = 1.54$ $\tau_0/\tau_{air} = 4$ $\tau_0/\tau_{air} = 50$ $\tau_0/\tau_{air} = 1.28$	Phase modulation technique employed for lifetime determination. Poor photostability. Excellent photostability.	L	317
PtOEP in poly-IBM PtOEP in poly(IBM-co-TFPM) ⁱⁱ	535/644 535/644	$I_0/I_{100} = 69.3$ $I_0/I_{100} = 86.4$	Linear SVPs. Linear SVPs.	I	318
PtOEP in poly-IBM PtOEP in poly(IBM-co-TFEM) PtOEP in PS PtOEP in poly(styrene-co-TFEM)	535/646 535/646 535/646 535/646	$I_0/I_{100} = 69$ $I_0/I_{100} = 288$ $I_0/I_{100} = 4.5$ $I_0/I_{100} = 296$	Extremely high sensitivities and linear SVPs in fluoropolymers; good photostability.	I	319
PtOEP in PS PtOEP in poly(styrene-co-PFS) ⁱⁱⁱ PdOEP in PS PdOEP in poly(Styrene-co-PFS)	535/645 535/645 546/664 546/664	$I_0/I_{100} = 4.5$ $I_0/I_{100} = 25$ $I_0/I_{100} = 46.0$ $I_0/I_{100} = 93.6$	Sensitivity in poly(styrene-co-PFS) is much higher than in PS; linear SVPs for PdOEP in the 0 – 20% oxygen range.	I	320
PtOEP in poly(1-trimethylsilyl-1-propyne) PtOEP in PS PtOEP in PDMS rubber	535/646	$I_0/I_{100} = 225, I_0/I_{air} \sim 80$ $I_0/I_{100} = 4.5$ $I_0/I_{100} = 5.5$	High photostability; suitable for trace oxygen determination; extremely gas permeable polymer; non-linear SVPs.	I	321
PtOEP in PFE-VFP ^{iv}	510/630	$I_0/I_{O_2 \text{ satur}} = 1.8$	For dissolved oxygen; poor sensitivity; dye aggregates during film preparation; non-linear SVPs.	I	322
PtOEP in pPEGMA PdOEP in pPEGMA RuOEP in pPEGMA	535/644 545/663 532/656	$I_0/I_{100} \sim 56$ $I_0/I_{100} \sim 300$ $I_0/I_{100} \sim 4.5$	τ_0 100 μ s; more photostable than other complexes; linear SVP. τ_0 770 μ s; linear SVPs. τ_0 140 μ s; low phosphorescence QY; poor photostability	I, L	323

ⁱ TPP = *meso*-tetraphenylporphyrin, OEP = octaethylporphyrin

ⁱⁱ IBM = isobutyl methacrylate, TFPM = tetrafluoropropyl methacrylate

ⁱⁱⁱ PFS = pentafluorostyrene

^{iv} PFE-VFP = poly(tetrafluoroethylene)-*co*-(vinylidene fluoride)-*co*-(propylene)

PdOEP in ethyl cellulose/CAB ^v /PVC PtOEP in ethyl cellulose/CAB/PVC	546/670 535/644	$I_0/I_{\text{air}} \sim 42/18/2.4$ $I_0/I_{\text{air}} \sim 20/12/2$	τ_0 1.41/1.45/1.34 ms. τ_0 81/100/90 μs .	I, L	324
PtOEP in PDMS; SiO ₂ added as scatterer PtOEP in C ₄ PATP ^{vi} ; SiO ₂ added	534/641 535/645	$I_0/I_{100} = 175-8$ $I_0/I_{100} = 60-50$	Larger fractions of SiO ₂ result in less sensitivity and larger τ_0 (65-91 μs); dye adsorbed on SiO ₂ and aggregated. Small dependence on SiO ₂ content; τ_0 104 μs ; the dye is located in the matrix polymer.	I, L	325
PtOEP + DiO in PTMOS MTMOS ormosil nanoparticles ^{vii} PtOEPK + OEP in PTMOS MTMOS ormosil nanoparticles	570/640 568/750	$I_0/I_{\text{O}_2 \text{ satur}} \sim 33.3$ $I_0/I_{\text{O}_2 \text{ satur}} \sim 33.3$	Ratiometric nanosensors (120 nm in diameter); DiO and OEP are reference dyes; linear SVPs; good storage stability, no leakage; reference dyes are less photostable.	I _r	326
PtOEP/PTMOS+MTMOS ormosil	505/red PD	$\tau_0/\tau_{\text{air}} = 10.6$	τ_0 88 μs ; linear SVPs; short response times (t_{90} 250 ms) .	I, L	204
PdOEP in 8F-PEKEK(6FBA/HF) ^{viii}	546/664	$I_0/I_{100} = 240/227$ $I_0/I_{\text{air}} \sim 80/75$	SVPs close to linear up to air saturation; suitable for trace oxygen.	I	327
PtOEP in 8F-PEKEK(6FBA/HF)	535/646	$I_0/I_{100} = 32.4/23.6$	SVPs close to linear up to 100% of O ₂ .	I	327
Poly-PtOEP	540/644	$\tau_0/\tau_{\text{air satur}} = 41$	τ_0 110 μs ; response times < 100 ms; film thickness 0.2 μm ; highly photostable.	L	328
Poly-PtTPP	514/648	$\tau_0/\tau_{\text{air satur}} = 57$	τ_0 69 μs ; linear SVPs; response times < 20 ms; film thickness 0.2 μm ; highly photostable.	L	328
Poly(PtTPP-co-IBM-co-TFEM)	402,510/665	$I_0/I_{100 \text{ KPa}} > 10$	Polymerizable PtTPP probe; highly sensitive to oxygen; linear SVPs.	I	299
PtOEP in CAB (+TPB) ^{ix} PdOEP in CAB (+TPB) PtOEP in PMMA (+TPB) PdOEP in PMMA (+TPB)		$I_0/I_{\text{air}} = 13.4$ (170.2) $I_0/I_{\text{air}} = 106.5$ (631) $I_0/I_{\text{air}} = 1.78$ (57.5) $I_0/I_{\text{air}} = 21$ (671)	Addition of the plasticizer increases sensitivity and accelerates response and recovery.	I	329
PtOEP in PTP ^x Ru(dpp) ₃ in PTP	380/645 450/610	$I_{0.01\text{atm}}/I_{1.00\text{atm}} = 58$ $I_{0.01\text{atm}}/I_{1.00\text{atm}} = 2.55$	τ_0 79 μs ; linear SVPs. τ_0 6.9 μs ; slight downward curvature of SVPs.	I, L	330
PtOEP Schiff base in PVC PdCP Schiff base in PVC	398,443/650 398,443/650	$I_0/I_{21\text{KPa}} \sim 3.0$ $I_0/I_{21\text{KPa}} \sim 8.5$	Oxygen and pH dual sensor based on a single probe; absorption changes with pH; luminescence and lifetime change with oxygen; non-linear SVPs; PdCP Schiff-base suitable for low oxygen.	L	331
PtOEPK ^{xi} in PS	592/759	$\tau_0/\tau_{\text{air}} = 3.6$	QY_{phos} 0.12; τ_0 61 μs ; photostability 9 times better than for PtOEP.	L	278
PdOEPK in PS	602/790		QY_{phos} 0.04; τ_0 480 μs .	L	279
PtOEPK in PS	591/760	$\tau_0/\tau_{\text{air}} = 3.76$	$QY_{\text{phos}} \sim 0.1$; τ_0 64 μs ; linear SVP; sterilizable in ethanol or by	L	279

^v CAB = cellulose acetate butyrate^{vi} C₄PATP = poly[(*n*-butylamino)thionylphosphazene]^{vii} DiO = 3,3'-dioctadecyloxycarbocyanine perchlorate, PTMS = phenyl trimethoxysilane, MTMS = methyl trimethoxysilane^{viii} 8F-PEKEK(Ar) = poly(aryl ether ketone) where Ar is 2-2-bis(4-hydroxyphenyl)-1,1,1,3,3,3-hexafluoropropane (6FBA), or 9,9'-bis(4-hydroxyphenyl)propane (HF)^{ix} TBP = tributyl phosphate^x PTP = poly(aminothionylphosphazene)^{xi} OEPK = octaethylporphyrin ketone

PdOEP in PS	546/670	$\tau_0/\tau_{\text{air}} \sim 198$	heat. $QY_{\text{phos}} 0.2$; $\tau_0 990 \mu\text{s}$; linear SVP.		
PtOEPK in PVC	592/758	$\tau_0/\tau_{728 \text{ torr}} \sim 2.05$	$\tau_0 \sim 60 \mu\text{s}$; linear SVP in PVC, slight downward curvature in PS. $\tau_0 \sim 450 \mu\text{s}$; linear SVP in PVC, slight downward curvature in PS.	I, L	332
PtOEPK in PS	592/758	$\tau_0/\tau_{728 \text{ torr}} \sim 20$			
PdOEPK in PS	602/790	$\tau_0/\tau_{728 \text{ torr}} \sim 9.5$			
PdOEPK in PVC	602/790	$\tau_0/\tau_{728 \text{ torr}} \sim 29$			
PtOEPK in PVC + plasticizer	592/758	$I_0/I_{100} \sim 13.6$	Response time < 100 ms; addition of plasticizer reduces response time to 66 ms.	I	333
PdOEPK in Teflon AF	590/760	$I_0/I_{0.01\%} \sim 1.17$	Phase modulation technique; linear SVP; for trace oxygen; polymer is 130-times more permeable for oxygen than PS; highly oxygen permeable (130 times better than PS); highly photostable.	L	334
PtTFPP ^{xii} in PS	541/650	$I_0/I_{100} = 3.0$ $I_0/I_{\text{air}} = 1.9$	SVPs linear up to 20% oxygen; response time 18 s; much more photostable than PtOEP.	I	267
PtTFPP in poly(tBS-co-TFEM) ^{xiii}	465/650	$I_0/I_{14.7 \text{ PSI}} = 11$	Polymer has good oxygen permeability (even better than poly(styrene-co-TFEM)); excellent mechanical properties, adheres to glass and metal substrates.	I	335
PtTFPP in PTFEM	544/648	$I_0/I_{100} = 15.4$	Excellent photostability; linear SVPs; response time 5.6 s. Good photostability; non-linear SVP; moderate sensitivity.	I	268
PtTFPP in PS	544/648	$I_0/I_{100} = 3.0$			
PtTFPP in octyl-triEOS TEOS ormosil	380/650	$I_0/I_{100} = 22$	Response time 0.6 s; good stability for long-term usage.	I	336
PtOEP in octyl-triEOS TEOS ormosil	380/645	$I_0/I_{100} = 47$			
PtTFPP in octyl-triEOS TEOS ormosil and silica nanoparticles	405/650	$I_0/I_{100} = 106$	Addition of silica nanoparticles improves oxygen quenching; response time 1.3 s; non-linear SVPs.	I	337
PtTFPP in <i>n</i> -propyl-TriMOS and TFP-TriMOS ormosil	400/650	$I_0/I_{100} = 68.7$	Fluorinated ormosil; response time ~3 s; linear SVPs.	I	338
PtOEP in <i>n</i> -propyl-TriMOS and TFP-TriMOS ormosil	400/646	$I_0/I_{100} = 82.5$			
PtTFPP in ormosil made from 3 precursors	405/650	I_0/I_{100} from 101 to 155	Three precursors used to make ormosil films; extremely high sensitivities; response time ~3 s; good oxygen mechanical flexibility; linear SVPs.	I	339
Poly(PtTFPP-co-HEMA)	405/650	$I_0/I_{100} = 1.1$	PtTFPP modified with polymerizable group or silane group; covalently bound to polymer or sol-gel; excellent stability; no leaching; photostable; fast response.	I	303
Poly(PtTFPP-co-styrene)	405/650	$I_0/I_{100} = 5.8$			
PtTFPP in sol-gel film	405/650	$I_0/I_{100} = 70$			
PtTFPP in silica gel beads in silicone	405/650	$I_0/I_{100 \text{ Pa}} \sim 1.4$	Covalently immobilization; highly photostable; low temperature dependence. PdTFPP has an exceptionally long lifetime (~1 ms).	I, L	270
PdTFPP in silica gel beads in silicone	405/680	$I_0/I_{1000 \text{ Pa}} \sim 5$			
PtOEP in poly(styrene-co-TFEM)	535/654	$I_0/I_{100} = 87.6$	Sensitivity decreases with increasing PS/TFEM ratio; for trace O ₂	I	340
PdOEP in poly(styrene-co-TFEM)	546/664	$I_0/I_{100} = 661.7$			
PtTFPL in FIB ^{xiv}	400(574)/738	$I_0/I_{\text{air}} \sim 5$	Sensitivity comparable to PtTFPP; lower dependence on temperature than PtTFPP; $\tau_0 72 \mu\text{s}$, QY_{phos} is ~60% of PtTFPP (τ_0)	I, L	271

^{xii} TFPP = 5,10,15,20-tetrakis-(2,3,4,5,6-pentafluorophenyl)porphyrin

^{xiii} tBS = 4-tert-butylstyrene, TFEM = trifluoroethyl methacrylate

^{xiv} PtTFPL = platinum tetra(pentafluorophenyl)porpholactone; FIB = copolymer of heptafluoro-*n*-butyl methacrylate and hexafluoroisopropyl methacrylate

			120 μ s).		
PdPC10COOH ^{xv} on Al ₂ O ₃	418/708	$I_0/I_{\text{air}} \sim 15$	Probe has long alkyl chain and self-assembles on aluminum plate; non-linear SVPs; seems to be photostable; strong quenching	I	341 342
PtTCPP ^{xvi} on a alumina plate	538/665	$I_0/I_{\text{air}} \sim 10$	Non-linear SVPs for both sensors	I	294-296
PdTCPP on a alumina plate	523/701	$I_0/I_{\text{air}} \sim 14$			
PdTMPyP ⁴⁺ in Nafion ^{xvii}	442/668	$I_0/I_{100} = 70$	Other metalloporphyrins are also tested; linear SVPs; single exponential phosphorescence decays for all metalloporphyrins; phosphorescence lifetimes increased in Nafion; low QYs.	I- RTP, L	286
PtTMPyP ⁴⁺ in Nafion	442/645	$I_0/I_{100} = 6$			
ZnTPP on silica gel	551/697	–	In silica gel, phosphorescence quenching is temperature dependent. In NaCl crystal, quenching obeys Stern-Volmer kinetics; low temperature dependence.	I- RTP	343
ZnTPP in NaCl crystal					
PtCPTTE ^{xviii} in PS	382(535)/647	$\tau_0/\tau_{\text{air satur}} = 3.69$	Hydrophobic probes; QYs between 0.6 and 0.9); high concentration of probes used in polymers.	I- RTP, L	344
PtCPTTE in silicone rubber	376(535)/647	$\tau_0/\tau_{\text{air satur}} = 13.0$			
PtTPP in PS	404(508)/662	$\tau_0/\tau_{\text{air satur}} = 4.56$			
PtOEP in PS	383(535)/647	$\tau_0/\tau_{\text{air satur}} = 3.60$			
PtEP	380(535)/647				
Pt coproporphyrin in PMMA	378(512,544)/66 7	$\tau_0/\tau_{\text{air}} \sim 6$	Low toxicity; soluble in basic aqueous solution, DMF, pyridine; response not only depends on polymer, but also on the solvent used for dissolving the polymer.	L	287
Pt coproporphyrin in PVC		$\tau_0/\tau_{\text{air}} \sim 4.3$			
Pt coproporphyrin in PS		$\tau_0/\tau_{\text{air}} \sim 11.7$			
Pt coproporphyrin in silicone rubber		$\tau_0/\tau_{\text{air}} \sim 46$			
PtTDCPP ^{xix} in silicone rubber	394/650	$I_0/I_{100} = 51$	Good photostability; downward curved SVP; response time < 10 s; self-quenching may occur at high concentration.	I	266
PtTFMPP in silicone rubber	395/646	$I_0/I_{100} = 42$			
PtBr ₈ TMP in silicone rubber	425/721	$I_0/I_{100} = 45$			
PtTPTBP in PS ^{xx}	432,615/772	$\tau_0/\tau_{\text{air}} = 3.08$	Strong red Q band enables the probes to be excited using red LEDs or lasers; high QYs and photostability (especially Pt complexes), low tendency to aggregation in nonpolar polymers; non-linear SVPs; palladium complexes are more prone to thermal quenching; all probes also can be incorporated in PS-co-PVP or polysulfone nanoparticles.	L	275, 276
PtTPTBPF in PS	431,617/777	$\tau_0/\tau_{\text{air}} = 3.31$			
PtTPTBPF ₂ in PS	425,619/785	$\tau_0/\tau_{\text{air}} = 2.96$			
PdTPPTBP in PS	445,630/800	$\tau_0/\tau_{\text{air}} = 5.78$			
PdTPPTBPF in PS	444,631/801	$\tau_0/\tau_{\text{air}} = 5.34$			
PdTPPTBPF ₂ in PS	439,630/812	$\tau_0/\tau_{\text{air}} = 6.48$			
PtNTBP ^{xxi} in PS	406,630/844	$\tau_0/\tau_{\text{air}} = 2.34$	Intense Q-band absorption; compatible with red laser diode; less bright and less sensitive than the TPTBP complex; good photostabilities; negligible thermal quenching at RT; QYs of palladium complexes < 10 %.	I	280
PtN _{2-cis} TBP in PS	388,621/841	$\tau_0/\tau_{\text{air}} = 1.72$			
PdNTBP in PS	421,642/875	$\tau_0/\tau_{\text{air}} = 7.31$			
PdN _{2-cis} TBP in PS	380,631/873	$\tau_0/\tau_{\text{air}} = 3.92$			

^{xv} PdPC10COOH = [5-(1-carboxydecyl-4-pyridyl)-10,15,20-tritolylporphyrinato]palladium

^{xvi} TCPP = tetrakis(4-carboxyphenyl)porphyrin

^{xvii} TMPyP = *meso*-tetrakis (4-*N*-methylpyridyl) porphyrin

^{xviii} CPTTE = coproporphyrin tetraethyl ester, EP = etioporphyrin

^{xix} TDCPP = *meso*-tetra(2,6-dichlorophenyl)porphyrin, TFMPP = *meso*-tetra(3,5-bis(trifluoromethyl)phenyl)porphyrin, Br₈TMP = *meso*-tetramesityl- β -octabromoporphyrin

^{xx} TPTBP = *meso*-tetraphenyltetrabenzoporphyrin; TPTBPF = *meso*-tetra(4-fluorophenyl)tetrabenzoporphyrin; TPTBPF₂ = *meso*-tetra(3,5-difluorophenyl)tetrabenzoporphyrin

^{xxi} NTBP = 6-aza-13,20,27-triphenyltetrabenzoporphyrin, N_{2-cis}TBP = 6,13-diaza-20,27-diphenyltetrabenzoporphyrin

Pt1NF in PS ^{xxii} Pt2NF in PS Pt3NF in PS Pd1NF in PS Pd2NF in PS Pd3NF in PS	434, 628/815 438, 652/835 441, 667/870 450, 641/849 452, 666/868 456, 681/882	$\tau_0/\tau_{20\text{kPa}} = 3.6$ $\tau_0/\tau_{20\text{kPa}} = 3.2$ $\tau_0/\tau_{20\text{kPa}} = 2.6$ $\tau_0/\tau_{20\text{kPa}} = 13$ $\tau_0/\tau_{20\text{kPa}} = 11$ $\tau_0/\tau_{20\text{kPa}} = 10.4$	τ_0 44 μs ; QY 0.53. τ_0 28 μs ; QY 0.27. τ_0 21 μs ; QY 0.25. τ_0 203 μs ; QY 0.18. τ_0 138 μs ; QY 0.12. τ_0 106 μs ; QY 0.07.	L	282
Ir-OEP-CO-Cl in PS Ir-OEP-Py ₂ Ir-OEP- <i>n</i> -butIm ₂ in buffer ^{xxiii} Ir-OEP- <i>n</i> -barbIm ₂ in silica gel	404, 550/672 389, 539/655 390, 541/655 388, 538/652	$\tau_0/\tau_{20\text{kPa}} \sim 9$ - $\tau_0/\tau_{0.5\text{kPa}} \sim 8$ $\tau_0/\tau_{0.4\text{kPa}} \sim 1.7$	τ_0 97 μs ; QY 0.14. τ_0 40 μs ; QY 0.195 τ_0 27 μs ; QY 0.20 τ_0 37 μs ; QY 0.21.	L	284, 285
Poly(DDA-co-PtTPP) in LB film ^{xxiv} Poly(DDA-co-PtTPP) in LB film and silver nanoparticles	400/660	$I_0/I_{100} = 74$ $I_0/I_{100} = 25$	PtTPP covalently bound to polymer to form LB films; addition of silver nanoparticles enhances luminescence, but decreases sensitivity; nearly linear SVPs.	I	345
AlPc(OH) ^{xxv} in PS	606/706	$I_0/I_{10} = 1.04$	Poorly sensitivity; non-linear SVP; τ_0 11.7 ns.	I	346

^{xxii} 1NF = *meso*-tetra-(4-fluorophenyl)mononaphthotribenzoporphyrin, 2NF = *meso*-tetra-(4-fluorophenyl)dibenzodiazeporphyrin,

3NF = *meso*-tetra-(4-fluorophenyl) monobenzotrinaphthoporphyrin

^{xxiii} *n*-ButIm = *N*-(*n*-butyl)imidazole, CarbIm = 1-imidazoleacetic acid

^{xxiv} DDA = *N*-dodecyl acrylamide; LB = Langmuir-Blodgett

^{xxv} Pc(OH) = 2,9,16,23-tetraphenoxy-29*H*, 31*H*-phthalocyanine hydroxide

6.2.6. Other Metal Complex-Based Probes for Oxygen

The group of Sanz-Medel³⁴⁷⁻³⁵¹ has systematically investigated the room-temperature phosphorescence (RTP) of 8-hydroxy-7-iodo-5-quinolinesulfonate ("ferron") chelated with metals such as Al(III), Zr(IV), Ga(III), and Nb(V). They found these complexes to undergo efficient quenching by oxygen with good linear Stern-Volmer plots (SVPs) and to be fairly photostable when immobilized on anion-exchange resins³⁴⁷ or in an ormosil matrix.³⁴⁹⁻³⁵¹ The immobilized complexes do not leach out into water or common organic solvents, and thus can be applied to sense oxygen both in aqueous solution and in organic solvents. The Al(III)-ferron complex has a long phosphorescence lifetime (460 μ s), which was measured as a function of pO_2 with a low-cost lifetime based portable oxygen meter³⁵⁰ and also enabled fiber optic-based multi-position sensing.³⁵¹ Certain gold complexes (see **Table 9**) display oxygen-quenchable RTP emission in solid-state, and it was suggested to exploit the effect to sense oxygen in the gas phase and in non-aqueous media.^{352, 353} These OSPs have relatively large Stokes' shift and good sensitivity to oxygen, but photostability is poor even if exposed to sunlight where complete photodegradation occurs within several hours.

The copper(I) complex of a pyridinyl-5-tolyl-1,3,4-oxadiazole has a yellow luminescence with a lifetime of 64 μ s under pure nitrogen atmosphere.³⁵⁴ The complex was doped into a silica supporting matrix (MCM-41) to construct an oxygen-sensitive material that has a sensitivity (I_0/I_{100}) of 6.0, a response time of 10 s, and good photostability. Several crystalline highly emissive copper(I) complexes with high QY (0.66), long lifetime (~ 30 μ s), fast response (51 ms) and strictly linear SVPs also can act as OSPs.^{355, 356} The crystals can be excited in the near-UV at ~ 375 nm to emit yellow-green luminescence with a maximum at 540 nm. Another phosphorescent copper(I) complex³⁵⁷ with an RTP phosphorescence peaking at 545 nm and a long excited state lifetime (4.7 μ s) was incorporated into electrospun composite nanofibers of polystyrene to obtain an oxygen sensing material with a sensitivity (I_0/I_{100}) of 7.2 and a response time of 7 s. No photobleaching was detectable. The exceptionally long-lived luminescence of certain $Cu(I)(isocyanido)_2(phen)]^+$ complexes in the form of nanoporous crystals may also be exploited for sensing oxygen.³⁵⁸ They display strong emissions with peaks at ~ 530 nm if excited at 375 nm, and lifetimes between 100 - 120 μ s. Both intensity and decay times are quenched by oxygen. The respective SVPs are strictly linear, and sensitivity is almost 38 times better than that of Ru(phen) complexes.

A phosphorescent Cu(I) complex with pyridine and triphenylphosphine ligands was reported³⁵⁹ that displays a yellow phosphorescence peaking at 552 nm and a long excited state lifetime (83.5 μ s) under nitrogen. It was doped into a mesoporous silica matrix to obtain an oxygen-sensing material with a sensitivity ($I_0/I_{100} = 4.48$) for oxygen, a short response time (due to a large surface-

to-volume ratio), and no photobleaching. While Cu(I) complexes are affordable, they suffer from the drawbacks of UV excitation and – sometimes – low brightness.

While Pt(II)porphyrins are widely used as OSPs, other complexes of Pt(II) have been rarely used. Wong et al.³⁶⁰ demonstrated that the Pt(dtbp)(CN)₂ and Pt(dpp)(CN)₂ complexes dissolved in a silicone rubber matrix are viable materials for optical sensing of oxygen. The probes do not carry a charge, can be mixed with silicone matrix more easily than Ru(bpy), and do not leach into aqueous solutions. The resulting sensors have fast response (< 3 s), and alkyl halides do not interfere. Triphenylamine-based cyclometalated Pt(II) complexes also were shown to be efficient OSPs.³⁶¹ They contain a pyridyl moiety and a cyano group and were dissolved in a polymer film. The luminescence of these new OSPs is quenched by oxygen with highest efficiency and an apparent Stern-Volmer constant of 0.102 Torr⁻¹.

Numerous other luminescent metal complexes are known³⁶² but haven't been studied so far. Many of them are likely to be viable probes for oxygen that may cover various ranges of oxygen levels. However, it needs to be seen whether they are better than some of the existing probes that perform quite well.

Table 9. Luminescent probes for oxygen based on complexes of other metal ions, along with their excitation/emission wavelengths (in nm), quenchability ("sensitivity"), the polymer solvent or support used, and the method for read-out (RO). Quenchability is expressed as either I_0/I_{100} (the ratio of fluorescence intensity at zero % oxygen in the carrier gas and the intensity at 100% oxygen (at atmospheric pressure), or in a fluid equilibrated with such gases. Correspondingly, I_{21} is the intensity under air at atmospheric pressure. Codes: I: intensity-based readout; L: lifetime-based readout; QY: quantum yield; SVP: Stern-Volmer plot.

Dye/Matrix	$\lambda_{exc}/\lambda_{em}$	Sensitivity	Comments	RO	Ref.
[Cu(dbp)(dmp)]PF ₆ in PS ⁱ	450/610	$I_0/I_{100} = 1.60$	Low QY and lifetime (QY _{phos} 0.01); τ_0 0.73 μ s.	I	363
[Cu(dipp) ₂]BF ₄ as a crystal ⁱⁱ	400/670	$I_0/I_{100} = 1.30$	Solid-state oxygen sensors, other Cu(I) crystals also tested; strictly linear SVPs; high solid-state QYs and lifetime (10 times larger than those in solution); response time 280 ms.	I	355
[Cu(dipp) ₂]tfpb as a crystal	400/679	$I_0/I_{100} = 1.15$			
[Cu(dmp)(dbp)]tfpb as a crystal	400/608	$I_0/I_{100} = 1.10$			
[Cu(POP)(dmp)]tfpb as a crystal ⁱⁱⁱ	400/517	$I_0/I_{100} = 4.60$	Solid state oxygen sensors, other Cu(I) crystals also tested; strictly linear SVPs; QYs >0.66; lifetimes ~30 μ s; fast response (51 ms).	I, L	356
[Cu(xantphos)(dmp)]tfpb as a crystal	375/540	$I_0/I_{100} = 6.65$			
[Cu(xantphos)(dipp)]tfpb as a crystal	400/513	$I_0/I_{100} = 4.41$			
([Cu(CNxylyl) ₂ (dmp)]tfpb as a crystal ^{iv}	375/520	$I_0/I_{100} = 91.9$	Solid state oxygen sensors, other Cu(I) crystals also tested (lifetime of other crystal is from 100 μ s to 1.2 ms); strictly linear SVPs; QYs around 0.23; fast response (67 ms).	I, L	358
[Cu(PTO)(PPh ₃) ₂]BF ₄ crystal in MCM-41 silica ^v	355/515	$I_0/I_{100} = 5.95$	Crystals doped into MCM-41 silica to obtain a oxygen sensor; downward curved SVPs; good photostability; lifetime ~ 64.4 μ s; sensitivity depends on the doped concentration of Cu(I) crystal in silica.	I	354
Pt(dpp)(CN) ₂ in silicone RTV rubber	290/520	$I_0/I_{100} \sim 14$	Highly photostable; absorption in UV; forms excimer at high concentration; response time < 3 s.	I	360
Pt(dtpy)(CN) ₂ in silicone RTV rubber	302/486	$I_0/I_{100} \sim 5$			
Pt(thpy) ₂ ^{vi} in PDMS rubber	470/>530	$I_0/I_{100} \sim 10$	QY _{phos} 0.36, τ_0 4.8 μ s; low absorption (2000 M ⁻¹ cm ⁻¹ at 470 nm); PDMS not specified, used with curing agent; dye crystallizes at high concentrations; non-linear SVPs. Intensity is 25 times higher than in PDMS; SVP almost linear.	I, L	364
Pt(thpy) ₂ in PS	470/>530	$I_0/I_{100} \sim 3$			
[Pt ₂ (pop) ₄](Bu ₄ N) ₄ in silicone RTV rubber ^{vii}	368/509	$I_0/I_{100} \sim 2.2$	Water-soluble probe; intense luminescence; high QY, excellent photostability in silicone rubber film.	I	365
[Pt ₂ (pop) ₄](Bu ₄ N) ₄ in PVA		$I_0/I_{100} \sim 1.1$			
Au complex ^{viii} in PS (high molecular weight)	418/530	$I_0/I_{air} = 1.85$	Linear SVPs for all the polymers; sensitivity depends on polymer molecular weight; dye photodegrades in sunlight within several hours.	I	352, 353
Au complex in PS (low molecular weight)		$I_0/I_{air} = 1.30$			
Au complex in silicone RTV rubber		$I_0/I_{air} = 1.38$			
Au complex in CAB		$I_0/I_{air} = 1.46$			
Au complex in PMMA		$I_0/I_{air} = 1.17$			
Pb(7-SO ₃ -Ox) ^{ix} in Dowex 1-X2-200 basic	385/625	$I_0/I_{3\%} = 1.28$,	RTP emission; good photostability; no leaching; no quenching if dry	I	348

ⁱ dbp = 2,9-di-tert-butyl-1,10-phenanthroline; dmp = 2,9-dimethyl-1,10-phenanthroline

ⁱⁱ dipp = 2,9-diisopropyl-1,10-phenanthroline

ⁱⁱⁱ POP = bis[2-(diphenylphosphino)phenyl]ether; xantphos = 4,5-bis(diphenylphosphino)-9,9-dimethylxanthene

^{iv} CN-xylyl = 2,6-dimethylphenylisocyanide

^v PTO = 2-(pyridin-2-yl)-5-p-tolyl-1,3,4-oxadiazole

^{vi} Pt(thpy)₂ = *cis*-bis(2-(2'-thienyl)pyridine)platinum (II)

^{vii} pop = P₂O₅H₂²⁻

^{viii} Au complex = bis(μ -(bis(diphenylphosphino)octadecylamine-P,P'))diiodo gold (I)

anion-exchange resin beads		$I_0/I_{\text{air sat}} \sim 2.85$	gases are used; τ_0 154 μs under moist argon.		
Nb-Ferron on Dowex resin	365/570	$I_0/I_{\text{air}} = 6.3$	RTP emission only in anion-exchange resin; high photostability; do not easily leach; for aqueous and organic solutions; linear SVPs.	I, L	347
Zr-Ferron on Dowex resin	380/585	$I_0/I_{\text{air}} = 5.8$			
Al-Ferron on Dowex resin	390/600	$I_0/I_{\text{air}} = 5.5$			
Ga-Ferron on Dowex resin	390/600	$I_0/I_{\text{air}} = 5.2$			
Al-Ferron complex ^x in TMOS MTMOS ormosil	380/580	$I_0/I_{\text{air}} \sim 6$ $\tau_0/\tau_{\text{air}} \sim 3.7$	Sensitivity depends on the concentration of indicator; lifetime SVPs are downward curved; τ_0 460 μs .	I	349 350

^{ix} $\text{Pb}(7\text{-SO}_3\text{-Ox})$ = the 8-hydroxy-7-quinolinesulfonate chelate complex of lead(II)

^x ferron = 8-hydroxy-7-iodo-5-quinolinesulfonate

6.3. Intrinsically Luminescent Nanomaterials as Probes for Oxygen

Numerous kinds of intrinsically (non-doped) luminescent nanomaterials including nanocrystals have been discovered in the past three decades, including quantum dots (QDs), carbon dots, silicon dots, luminescent (conjugated) polymer dots, luminescent noble-metal nanoparticles, luminescent graphenes and photon upconversion nanoparticles. However, quenching by oxygen has hardly been studied. Zhu et al.³⁶⁶ reported that the luminescence cadmium telluride QDs capped with cysteine is reversible but weakly quenched by oxygen. The particle size, capping molecules and pH value govern the quenching process and thereby strongly affect the sensing capability. In addition, effects such as surface oxidation, oxidation of capping molecules, blinking (up to seconds), and cytotoxicity are not well under control. The use of these materials for oxygen sensing is still challenging. Nanoparticles doped with OSPs, on the other hand, play an important role and will be treated in **Section 7.3**.

6.4. Multiple Emitter Probes


The need for OSPs that enable ratiometric sensing has resulted in the design of luminescent dyes that have at least two distinct emission bands, one being sensitive to oxygen, the other not. Such dyes are useful for referenced sensing of oxygen. See the respective section. Franck and Pringsheim¹⁷ studied the effect of oxygen on the fluorescence and room-temperature phosphorescence (RTP) of tryptaflavine absorbed on (dry) silica gel. Tryptaflavine exhibits fluorescence in aqueous solution but becomes phosphorescent if absorbed on silica gel, paper, or gelatine. The RTP is very sensitive to oxygen, while fluorescence is not. Albeit weak, it may serve as a reference signal. Similarly, certain bromonaphthyl ketones immobilized on cellulose display oxygen-dependent RTP along with oxygen-independent fluorescence in the dry state.³⁶⁷ This finding resulted in a ratiometric sensing system with a large change in intensity ratios. However, the sensor can only be used in dry state. Air of 100 % relative humidity completely quenches RTP.

A probe referred to as dppe-Pt2P has two distinct emission peaks of differing sensitivity to oxygen.^{355,356} The long-lived triplet emission (15 μ s) with a peak at 680 nm is sensitive to oxygen while the short-lived singlet excited state (with an emission maximum at 570 nm and a decay time of 0.5 ns) is not quenched. It was suggested that this dual-emission probe can be used for ratiometric intensity based sensing, for frequency-modulation lifetime discrimination,^{368, 369} and for fluorescence polarization based³⁷⁰ sensing. Similar dual emitters were reported by Zhao et al.^{371, 372} who synthesized several cyclometalated Pt(II) complexes of general formula $C^N Pt(acac)$. These exhibit both fluorescence (500 – 650 nm; QY ~0.95; lifetimes ~60 ps) and phosphorescence (650 –

850 nm; QY \sim 0.22; decay time \sim 1.53 μ s), and can be applied to ratiometric sensing of oxygen. In addition, several Cu(I) complexes with indole derivatives were also reported to possess dual-emission and to be useful for ratiometric oxygen sensing.³⁷³

Following the observation Parker and Barnes³⁷⁴ that the UV-excitable fluorescence of the borate-benzoin complex is quenched by oxygen, a dually emissive iodine-substituted difluoroboron dibenzoylmethane was conjugated to poly(lactic acid) to form a solid-state oxygen sensing material (**Figure 16**).^{362,363} It displays intense blue fluorescence and an unusual, long-lived green RTP. While its fluorescence is insensitive to oxygen, its RTP is quenched by oxygen. The ratio of fluorescence to RTP can be adjusted by systematic variation of the chain length of the poly(lactic acid). Films made from low-molecular weight poly(lactic acid) have weak fluorescence and strong RTP and therefore are single-wavelength probes, while higher molecular-weight polymers give balanced fluorescence and phosphorescence intensities so to enable dual-wavelength ratiometric sensing. The RTP has a decay time of around 4 ms which is easy to determine. This material also was applied to fabricate nanoparticles for intracellular imaging of hypoxia. The only limitation of these attractive OSPs is their excitation wavelength in the UV where biomatter has poor optical transparency and background luminescence can be strong. A related dual emissive probe was used in polylactide nanoparticles of <100 nm in size. The material displays intense blue fluorescence, two-photon absorption, and long-lived room temperature phosphorescence (RTP) which strongly quenched by oxygen.³⁷⁵ The nanoparticles are internalized by cells and can be visualized by fluorescence microscopy. Multiple emitter probes can also be synthesized by combination of oxygen-insensitive fluorescent moieties and functionalized OSPs. A copolymer was synthesized by polymerization of functionalized PtTFPP monomer and fluorine monomer.³⁷⁶ The luminescence intensity from polyfluorine is not oxygen dependent but that of the PtTFPP moiety is sensitive to oxygen concentration. The ratio of the two emissions (can be adjusted by changing the initial feed ratio of two monomers) serves as a ratiometric dual emissive oxygen sensing system.

Figure 16. Synthetic route and chemical structure of a luminescent polymer (a), its spectra (showing dual-emission), and its quenching by oxygen. The emission spectra of polymers in air (b) and in nitrogen (c). (Reprinted from ref.³⁷⁷ with permission from Nature Publication group)

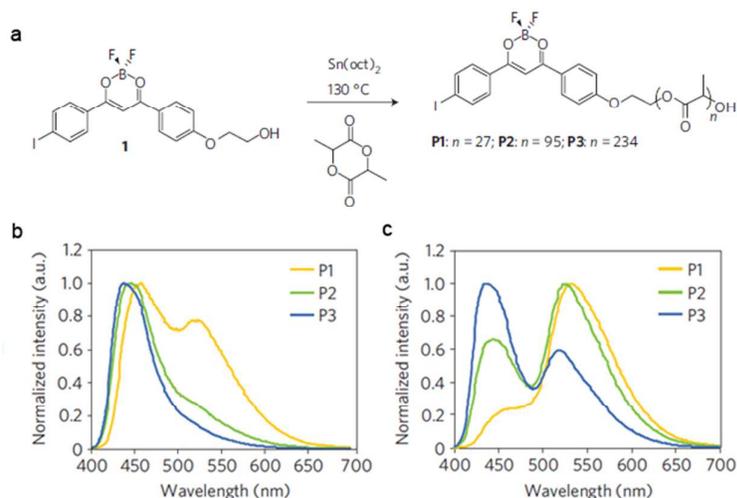

6.5. Various Other Probes for Oxygen

Hendricks³⁷⁸ observed the thermally stimulated luminescence of poly(ethylene 2,6-naphthalenedicarboxylate) (PEN). If irradiated with 330 or 390 nm UV light and exposed to oxygen (or air), the luminescence of the polymer is activated. After switching off the light source and heating to above 71 °C, PEN begins to emit luminescence that increases with temperature up to a maximum output at 130 °C. Its intensity depends on pO_2 , but even more on temperature. The samples would not luminesce if kept in darkness or in a vacuum. The mechanism of this thermally stimulated luminescence is still unknown. It was tentatively attributed to a photochemical reaction involving UV light, oxygen, and PEN. From a present day view it cannot be excluded that the actual species that causes luminescence to occur is ozone rather than oxygen, since ozone is known to react with various polymers. Subsequent thermal decomposition of the endoperoxides formed may result in chemiluminescence. Ozone may be present in ambient air but also may be produced in-situ by the UV light of the lamp.

The fluorescence of a thin film of photo-oxidized poly(9,9-dioctylfluorene) reversibly responds to oxygen if excited with a 325-nm He-Cd laser.³⁷⁹ However, sensitivity is moderate, and the sensor degrades irreversibly after 12 h of continuous illumination. Monolithic silica aerogel absorb light in the UV region (300 – 360 nm) and emit visible light at 400 – 600 nm if treated with ammonia and 2.45 GHz microwave radiation in a reducing atmosphere.³⁸⁰ The aerogel has a high surface area and porosity that allows rapid diffusion of oxygen, which quenches its luminescence. The material has a high sensitivity (with an I_0/I_{100} of > 12) and can be used to sense gaseous and dissolved oxygen. An aqueous solution containing 1-bromonaphthalene and a cyclodextrin was found³⁸¹ to display intense RTP while adding various alcohols. Phosphorescence decreases with increasing concentrations of oxygen. The sensitivities and analytical ranges strongly depend on the sort of alcohol. Under optimized conditions, the system responded to dissolved oxygen in the 0 to 40.2 mM concentration range.

Conventional organic OSPs and metal-ligand OSPs cannot be used for high temperature sensing due to their thermal lability. Ghosh et al.³⁸²⁻³⁸⁴ found on the Mo_6Cl_{12} cluster to possess a wide absorption band that extends from 300 to 400 nm, an emission extending from 600 to 900 nm, a lifetime of $>100 \mu s$, and a large Stokes' shift (> 300 nm), The red luminescence is reversible quenched by oxygen. The cluster can withstand repeated cycling between air and nitrogen and showed no signs of decomposition at temperatures even higher than 600 °C. This makes it suitable for monitoring oxygen in power plants and exhaust gas in cars. It can sense oxygen with high resolution (0.1% absolute oxygen concentration change) both in the gas phase and in aqueous solution. Remillard et al.³⁸⁵ noticed that the fluorescence of Cu-ZSM-5 zeolites reversibly changes

on cycling between oxidative and reduced atmospheres, and this was exploited to sense oxygen at temperatures as high as 500 °C. However, the material has to be regenerated by exposing it to reducing gases, and this limits practical usage. Table 10 summarizes the kinds and properties of the various other luminescent OSPs.

Table 10. Miscellaneous other luminescent probes for oxygen, along with their excitation/emission wavelengths (in nm), quenchability ("sensitivity"), the polymer solvent or support used, and the method for read-out (RO). Quenchability is expressed as either I_0/I_{100} (the ratio of fluorescence intensity at zero % oxygen in the carrier gas and the intensity at 100% oxygen (at atmospheric pressure), or in a fluid equilibrated with such gases. Correspondingly, I_{2l} is the intensity under air at atmospheric pressure. *Codes:* I: intensity-based readout; L: lifetime-based readout; QY: quantum yield; SVP: Stern-Volmer plot.

<i>Dye/Matrix</i>	$\lambda_{exc}/\lambda_{em}$	<i>Sensitivity</i>	<i>Comments</i>	<i>RO</i>	<i>Ref.</i>
dppe-Pt2P ⁱ in cellulose acetate and plasticizer	470/570, 680	$I_0/I_{100} \sim 3.5$	RTP at 680 nm with lifetime of 15 μ s is sensitive to oxygen; singlet emission with lifetime of 0.5 ns is insensitive to oxygen; both ratiometric and lifetime discrimination are used; QY _{fl} 0.002, QY _{phos} 0.01; τ_0 28.8 μ s.	I	368, 369
L1-Pt(acac) ⁱⁱ L2-Pt(acac)	459/502, 683 474/521, 692	$I_0/I_{0.2 \text{ bar}} \sim 2$ $I_0/I_{0.2 \text{ bar}} \sim 6$	Dual emitter; fluorescence (500 – 650 nm, QY \sim 0.95, lifetime \sim 0.06 ns) is not sensitive to oxygen, but phosphorescence (650 – 850 nm, QY \sim 0.22, lifetime \sim 1.53 μ s) is quenched by oxygen. Data for probes in organic solvent.	I	371, 372
BF ₂ dbm(I) in PLA polymer	405/460,525	$I_0/I_{100} \sim 1.8$	Fluorescence peaks at 460 nm, RTP at 525 nm; luminescent polymer; fluorescence and RTP emission ratio can be varied by variation of polymer molecular weight; RTP lifetime \sim 4 ms, suitable for lifetime based imaging; also fabricated in the form of nanoparticles.	I, L	377
Mo ₆ Cl ₁₂ in poly(1-trimethylsilyl-1-propyne)	325/>590	$I_0/I_{air} = 5.5$	τ_0 50 – 180 μ s; slow photodegradation even at high temperature (up to 600 °C); also be used for dissolved oxygen sensing.	I, L	382, 384
Photoluminescent silica aerogel	330/>450	$I_0/I_{air} \sim 4.1$	Prepared by irradiation of aerogel with 2.45 GHz in the presence of ammonia.	I	380
Cu-ZSM-5 (zeolite)	UV/470, 550	$I_0/I_{2.0\%} \sim 1.22$	Copper-containing zeolite; operated at 300 – 575 °C; response depends on the redox nature of the gases.	I	385

ⁱ dppe-Pt2P = [1,2-bis(diphenyl phosphino)ethane-Pt[S₂C₂(CH₂-CH₂-N-2-pyrimidine)](BPh₄), TEC = triethyl citrate

ⁱⁱ For the detailed chemical structure see the corresponding reference.

7. Polymeric Matrices (Hosts) and Supports

7.1. General Considerations

Polymer chemistry forms an integral part of chemical sensor technology. The function of polymers most often is that of (i), a solid support in which, or onto which, OSPs can be immobilized, and (ii), to warrant some permeation selectivity for oxygen, while rejecting other species. The use of polymers in various sensor applications has been reviewed.³⁸⁶ Korotcenkov³⁸⁷ has summarized the wealth of composite materials that is available to manufacture oxygen sensitive materials.

Online monitoring of oxygen in air or (flowing) liquid samples requires an OSP to be firmly immobilized in a host matrix while its luminescence is measured over time. This is important in case of medical sensing where OSPs must not leach out to enter blood or skin. The incorporation of OSPs into an oxygen-permeable host polymer has several additional beneficial effects: (a) the host provides a constant microenvironment and protects the OSPs from potential interferents. (b) Quenching constants can be adjusted by proper choice of materials. (c) The interaction of the OSP with sample materials (such as protein) is prevented. Combinatorial methods²⁰⁶ were applied to speed up optical sensor material (OSM) development by studying numerous combinations of polymers, solvents, indicators, and additive plasticizers in different ratios. The combinatorial approach creates a large database that facilitates the selection of proper OSMs. It offers an alternative to the cumbersome search for new materials on the basis of theoretical predictions which so often is hampered by practical limitations such as poor compatibility of solvents, polymers, indicator dyes, and plasticizers, but also by poor solubility.

There are several requirements for the matrix to be a viable host for the OSPs: (1) The OSPs and the matrices are to be compatible in terms of solubility so that the OSPs will enter and remain inside the matrix without leaching or aggregation. (2) The matrix has to be optically transparent, possess good adhesion to a conceivable mechanical support, and should be easy to handle. (3) Its permeability and diffusion rate for oxygen should match the specific needs of the sensor with respect to quenchability and response time. (4) The polymer is expected to possess good long-term stability and not to degrade. Certain sol-gels, for example, change their microstructure over even months. (5) The host should not significantly alter the photophysical properties (such as spectra or decay times) of the OSPs. (6) If used in-vivo, biocompatibility should be warranted.

Methods for immobilization of OSPs in an oxygen-permeable polymer can be divided into three main subgroups. In method A, the OSP is homogeneously dissolved in a polymer. In method B, the OPS is first adsorbed on the surface of a (particle) support and then incorporated into a polymer. In method (C), the OSP is first homogeneously incorporated into micro/nanoparticles which then are

incorporated into a – usually other kind of – host polymer. This is schematically shown in **Figure 17**.

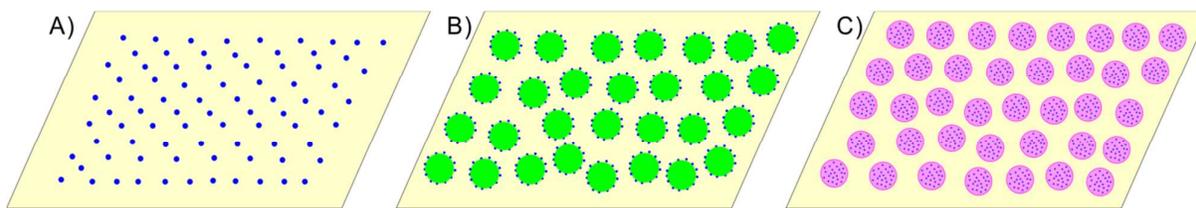


Figure 17. Schematic of the three most common methods for immobilizing oxygen-sensitive probes (OSPs) in a polymer host. In (A), the OSP molecules (symbolized by blue dots) are homogeneously distributed in the (yellow) host polymer. It can be present in dissolved form or covalently bound to the polymer. In (B), the OSP molecules are adsorbed on the surface of the (green) micro- or nanoparticles (silica or polystyrene, for example) which, in turn, are incorporated into the host polymer. In (C), the OSP molecules are first homogeneously distributed in micro- or nanoparticles (pink) which then are incorporated into the host polymer.

Method A, in its most simple form, involves the dissolution of an OSP in a polymer which obviously has to be a solvent for the OSP. This is easily performed and therefore the preferred method. Alternatively, the OSP may be covalently linked to the host polymer as described farther below. In a typical process, the OSP is dissolved in a suitable solvent, mixed with a solution of a host polymer to form a sensor cocktail, spread on a support or waveguide, and dried so to form an optical oxygen sensor layer. The leakage of dyes from such sensor layers only depends on the strength of the interaction of the OSPs with the hosting matrix material. Most often, this interaction is of hydrophobic nature. This method is convenient and time- and labor-saving. It works well if both the probe and the host polymer have similar polarity. It does not work if, for example, the polymer is highly hydrophobic (such as most silicones) and the OSP is rather polar if not ionic.

OSPs also have been covalently linked to the host polymer to yield homogeneous sensing layers or micro/nano-particles with firmly bound (and thus non-leaching) probes. OSPs bearing alkene groups^{185, 234, 299-301} or amino, carboxy, or siloxane functional groups^{43, 180, 183, 233} have been covalently immobilized in this way. Respective OSMs display excellent stability in terms of leakage, and the OSPs are evenly distributed in the hosting matrix. If properly executed, the OSP do not aggregate so that there is no self-quenching.

In method B, viz. the adsorption of a (charged) OSP on the surface of a (particle) support, the probe is deposited on particles with polar surface, examples being alumina, silica, or porous glass beads (all possessing a negative charge at pH 7), or amino-modified polystyrene particles (possessing a positive charge at pH 7). The OSP is firmly bound, usually due to electrostatic interaction. Examples include the immobilization of phosphorescent dyes on silica as described by Kautsky and others (see **Table 3**), or of ionic ruthenium probes on silica particles (see **Table 4**). The particles can be used as such (mainly for gaseous samples), or incorporated into a host matrix

such as silicone rubber or polystyrene. Unlike in method A, the bulk polymers need not be a solvent for the OSP. In fact, they should not at all. In a typical process, the OSP is dissolved in water or ethanol, and the silica particles are suspended in this solution for up to one hour. The particles are filtered off, washed, dried, and dispersed into an organic solution of the host polymer of choice. The resulting cocktail can then be used to form an optical oxygen sensor layer of almost any desired shape. Leakage of ionic dyes from such composite sensor layers is negligible. On the other hand, surface-adsorbed dyes without a host polymer easily leach if exposed to liquid solutions but are adequate for sensing oxygen in the gas phase. Surface-adsorbed OSPs also tend to be sensitive to the relative humidity of gaseous samples.

In method C, the OSPs are first dissolved in micro/nanoparticles (rather than adsorbed on a particle's surface) which acts as a "solvent" for the OSP. The particles then are incorporated in a (different) host polymer that needs not be a solvent for the OSP. It has become quite common in recent years. This is due to several advantages in that (a) fluorescence resonance energy transfer between OSPs and any other dyes (such as reference dyes or other probes) is prevented; (b) the quantities of particles (sometimes more than one kind) can be precisely controlled; (c) the polymers can be optimized in that a highly oxygen permeable polymer is used for the beads, while a biocompatible host polymer or well-adhering polymer may be chosen as the host; (d) the host can be chosen such that leaching of the probes out of the beads is prevented; and (e), the method also is applicable to simultaneously immobilize enzyme-loaded beads inside a sensor layer. This bead-based approach also is quite suitable in case of multiple-analyte sensing.

Methods for preparing dyed sensor microparticles³⁸⁸ include silane reagent-based techniques (including the Stöber process for making sol-gel particles), swelling of polymer nanoparticles in the presence of OPSs, nanoprecipitations of polymers in the presence of OPSs, and direct (emulsion) polymerization. The resulting oxygen-sensitive micro/nano-particles also may be used as such, i.e. without incorporating them into sensor layers.

It is obvious from these considerations that the selection of favorable matrix is a key to successful sensor design as will be further outlined in the following subsections 7.3. to 7.5. According to the chemical properties of host matrices, the polymers were subdivided into three main classes, viz. organic polymers, inorganic materials (including organic modified silicates and organic polymers with inorganic fillers), and nanomaterials.

7.2. Permeability, Solubility, and Diffusion of Gases in Polymer

There are three important parameters that characterize a polymer and govern the response of sensors for oxygen: Permeability (P), solubility (S), and diffusion (D). These are related by the equation $P = S \cdot D$ and shall be briefly discussed here. When oxygen permeates through a polymer membrane,

the rate of permeation is given by the *permeability coefficient* P . Typical data for P and S for oxygen in various polymers are compiled in **Table 11**. The unique properties of silicone are obvious.

Table 11. Permeability coefficients (expressed as $10^{-15} \text{ mol s}^{-1} \text{ N}^{-1}$), and solubility coefficients (expressed as $10^{-6} \text{ mol m}^{-1} \text{ N}^{-1}$), and diffusion coefficients (expressed as $10^{-12} \text{ m}^2 \text{ s}^{-1}$) of oxygen in various organic polymers at 25 °C. Data are taken from various sources, and the relation $P = S \cdot D$ obviously not always is not given.

Polymer	P	S	D
Polydimethylsiloxane ^{a)}	200 – 400	138	1500 - 2500
Polyethylene (low density)	0.7 – 0.9	21	46 – 60
Polyethylene (high density)	0.13 – 2.3	8.0	17
Polypropylene	0.77	-	-
Polyisoprene	7.7	-	-
Polystyrene	0.88	25	11
Polycarbonate	0.5	2.3	2.1
Poly(vinyl acetate)	0.4	6.2	5.5 ^{b)}
Poly(vinyl alcohol)	0.007 ^{b)}	-	-
Poly(vinyl chloride); not plasticized	0.015 – 0.03	13	1.2
Poly(vinylidene dichloride)	0.0018	-	-
Teflon	1.65	1.3 – 2.5	15
Polyacrylonitrile	0.00007	-	-
Natural rubber	7.8	50	173
Nylon 6	0.013 – 0.03	-	-
Cellulose acetate (not plasticized)	0.2 – 0.6	-	-
Poly(ethyl methacrylate)	0.4 – 0.8	38	10
Poly(hydroxyethyl methacrylate)	-	-	0.03 – 0.06 ^{c)}
Water	-	-	0.025

^{a)} With 10% filler; ^{b)} at 30 °C; ^{c)} at 20 °C

The concentration c of oxygen in a polymer can be described by the equation $c = S \cdot p$, where p is its partial pressure and S is the *solubility coefficient* of oxygen in a polymer. It decreases with increasing temperature above the glass temperature. The temperature dependence of both P and S again can be described by an Arrhenius type of equation. The concentration of oxygen in air-saturated water is 8 ppm (8 mg/L; equal to 0.25 mM at 22 °C, and 1.24 mM if saturated with 100% oxygen at atmospheric pressure.

The oxygen partial pressure of the arterial blood of healthy and normally breathing persons is around 90 Torr, this corresponding to a 143 μM oxygen concentration only. Blood solubility may also be expressed in terms of gas volumes: 100 mL blood dissolve 3.1 μL of oxygen at 37 °C per Torr of oxygen pressure applied. The largest fraction of oxygen in blood, however, is bound to hemoglobin. A typical value for *bound* oxygen is 20 – 21 mL of oxygen per 100 mL blood.

The *solubility coefficient* (S) of oxygen in all polymers decreases with increasing temperature above the glass temperature and obeys an Arrhenius relationship

$$S_{(T)} = S_0 e^{(-\delta H/RT)} \quad (\text{eq. 4})$$

where δH is the enthalpy of the solution process and S_0 is the pre-exponential term. The enthalpy can be calculated from the temperature dependence of the relative solubility. It is -3 kcal/mol in both fluid and fully polymerized silicone.

The *diffusion coefficient* (or diffusion constant) of oxygen in silicone also obeys an Arrhenius relationship with

$$D = D_0 \exp(-E_D/RT) \quad (\text{eq. 5})$$

where D_0 is the normalized diffusion constant, and E_D is the activation energy. Experimentally³⁸⁹ it was found for a series of poly(dimethyl siloxanes) of various viscosity that oxygen has a large diffusion coefficient (D_0) of $0.115 \text{ cm}^2 \text{ s}^{-1}$, and a low activation energy (E_D) of 4.77 kcal/mol which is not temperature-dependent between 5 and 45 °C. For comparison, the diffusion coefficient for oxygen in water is very much smaller ($2.5 \times 10^{-5} \text{ cm}^2 \text{ s}^{-1}$ at 25 °C). The diffusion coefficient is independent of oxygen concentration and fluorophore concentration in silicone over the usual pressure and temperature range. In the presence of small weight fractions of fumed silica, the diffusion of oxygen is reduced, but the activation energy is not affected.³⁹⁰

Experiments on the diffusion of oxygen in poly(methyl methacrylate) (PMMA) have been performed³⁹¹ using the room temperature phosphorescence technique. The diffusion of oxygen through PMMA as studied by phosphorimetry is very slow, with coefficients varying from 2.7 to $5.5 \times 10^{-9} \text{ cm}^2 \text{ s}^{-1}$ at 20 °C. It is constant within the used dye concentration and independent of the nature of the OSP. The activation energy (D_0 in the equ. above) is 250 cal mol^{-1} .

Oxygen diffusion in the much more hydrophilic polymer poly(hydroxyethyl methacrylate) (PHEMA) has been studied by fluorescence quenching techniques.³⁹² The diffusion constant is $1.36 \times 10^{-7} \text{ cm}^2 \text{ s}^{-1}$ at 20 °C. It was calculated that the maximum possible oxygen concentration in an aqueous polyHEMA matrix is 0.4 mM under pure oxygen at atmospheric pressure. The value of this study lies in the fact that a material was studied that closely resembles the composition of a sensing membrane composed mainly of hydrogel and water. This type of material was used to incorporate hydrophilic sensor micro- and nanoparticles, and in biosensors using immobilized enzymes. Quenching of fluorescence obeys Stern-Volmer kinetics with a K_{sv} of 0.016 Torr^{-1} . Diffusion data for other hydrogels also have been determined.³⁹³ Draxler et al.¹¹² have studied numerous polymers with respect to their permeability for oxygen via its effect on the quenching of polymer-dissolved ruthenium-based OSPs.

Badocco et al.³⁹⁴ have studied the experimental parameters that characterize the sensitivity and precision of sensor materials composed of polysulfone and Ru(dpp). The asymmetric shape of the emission band was used to define two parameters (the asymmetry factor and the percent variation of emission intensity) to characterize the sensitivity (= slope) of the sensor. Correlations between asymmetry factor and variation in intensity were established, and a double working curve was


introduced to to optimize precision. Mathematical modeling enabled the calculation of oxygen diffusion coefficients inside the sensor layer ($2 \times 10^{-8} \text{ cm}^2 \text{ s}^{-1}$), and of oxygen solubility ($2.2 \times 10^{-3} \text{ mol atm}^{-1} \text{ cm}^{-3}$) in the polymer matrix by using experimental data for membrane thickness, response time (t_{90}), and luminescence lifetime. In subsequent work,³⁹⁵ the group has determined the activation energies of the non-radiative decay and the gas solubility enthalpy inside a PtTFFP/polysulfone-based oxygen sensor layer using experimental data such as K_{sv} , decay time, diffusion coefficients and solubility. The dependence of the three parameters on temperature ranging between 40 and 90 °C was taken into account.





7.3. Organic Host Polymers

The permeabilities of many organic polymers for various gases vary to a very wide extent. Respective data are compiled in the *Polymer Handbook*, for example.³⁹⁶ Data (as far as available) on polymers often used for sensing oxygen are summarized in **Table 11**. Organic polymers usually are preferred because they often are commercially available or can be fabricated fairly easily and at affordable costs, come in a large variety, and can be easily further modified. **Figure 18** gives chemical structures (on monomeric building blocks) of commonly used polymers.

Many organic polymers are good solvents for OSPs but also act as barriers against notorious quenchers such as heavy metal ions or anions such as iodide or salicylate. Most polymers for use in oxygen sensors are hydrophobic in nature because oxygen dissolves and diffuses quite well through such polymers. If hydrophilic matrices are used, they usually act as a host matrix for oxygen-sensitive particles made from hydrophilic materials.

Figure 18. Chemical structures (of building blocks) and respective acronyms^{a)} of polymers frequently used as hosts in optical sensors. Many polymers contain fluorine or silica and are hydrophobic (except for Nafion™)

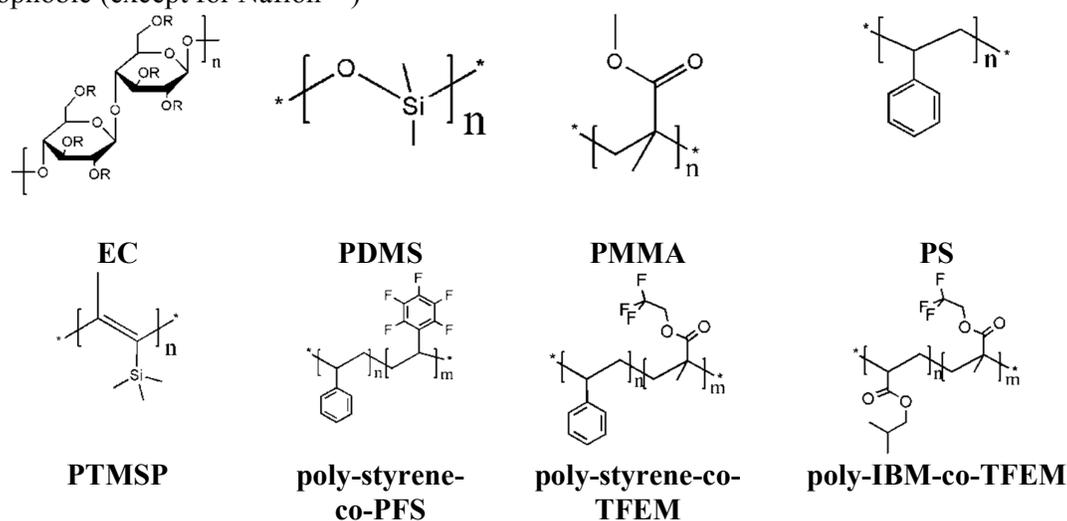

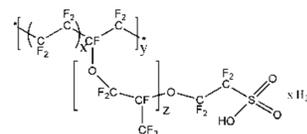**poly-tBS-co-TFEM****FIB****PSAN****Nafion™**

^{a)} EC: ethyl cellulose; PDMS: poly(dimethylsiloxane); PMMA: poly(methyl methacrylate); PS: polystyrene; PTMSP: poly(1-trimethylsilyl-1-propyne); poly(styrene-co-PFS): poly(styrene)-co-(pentafluorostyrene); polystyrene-co-TFEM: poly(styrene)-co-(trifluoroethyl methacrylate); poly-IBM-co-TFEM: poly(isobutyl methacrylate)-co-(trifluoroethyl methacrylate); poly-tBS-co-TFEM: poly(4-tert.-butylstyrene)-co-(trifluoroethyl methacrylate); FIB: poly(hexafluoroisopropyl methacrylate)-co-(heptafluoro-n-butyl methacrylate); PSAN: poly(styrene-co-acrylonitrile).

7.3.1. Organic Homopolymers

7.3.1.1. Silicone Rubber

Silicones are very hydrophobic and have unique properties in possessing a higher permeability for oxygen than most other polymers, but being impermeable to ions including the proton. Silicones also have excellent optical and mechanical properties, and a unique solubility for oxygen. This is particularly true for fluorosilicones. This needs to be considered in case of very small sample volumes because such polymers can deplete the aqueous sample of oxygen, and this may result in substantial analytical bias.

Silicone rubbers were among the earliest used homopolymers for constructing optical oxygen sensors. Silicone rubbers (polysiloxanes) such as poly(dimethyl siloxane) (PDMS) are cross-linked polymers with excellent gas permeability, high thermal stability, excellent chemical and mechanical stability, ease of handling, good adhesion to glass, inertness to biological samples, and good optical transparency. Many silicones are of the room-temperature vulcanizing (RTV) type that cures on exposure to moist air to release products such as acetic acid or amines. Other silicones cure as a result of addition reactions, for example by hydride addition under the catalytic effect of certain metal organic compounds. These silicones are of the two-component type. No acid or base is released in this case. The respective (commercial) prepolymers can be dissolved in aprotic solvents such as toluene or chloroform which facilitates handling.

Silicones cannot be easily plasticized by conventional plasticizers, but form copolymers which may be used instead. Their hydrophobic nature makes silicone rubbers rather poor solvents for ionic or highly polar OSPs.^{101, 102} Methods for solubilizing *ionic* species in silicone matrices have been developed that rely on the exchange of the inorganic counter ion (anionic or cationic) by an organic counter ion.^{175, 397} Another way to overcome poor solubility of probes in general is to adsorb the (charged) OSP on (silica) beads, which then are dispersed into the silicon prepolymer before curing.⁴⁷ As can also be seen in **Tables 3 to 8**, silicones have been used for immobilizing

OSPs quite often.^{49, 122, 127, 398, 399} Respective sensors may be sterilized by standard methods, for example by steam sterilization at 127 °C, or with hydrogen peroxide.

Silicone rubbers are elastomers and many of them have rather low glass transition temperatures (e.g., PDMS; -127 °C). Silicone films often are mixed with hardening additives (“binder”, “filler”) such as silica or alumina. Curing time, temperature, and humidity affect the properties of the final polymer and therefore the oxygen sensing capability. Commercially available prepolymers may contain solvents, fillers, low molecular weight cross-linkers, catalysts and other additives. These 'unknown' components may cause unexpected results.^{175, 176} In some cases, silicones were blended with other polymers. An Ir(ppy)-labeled PDMS was blended with polystyrene to form a sensing film for oxygen.⁴⁰⁰ The morphology and oxygen sensing properties of blend film were studied and results revealed that the oxygen permeability in the blend film is spatially heterogeneous. There are circular, 2-5 μm diameter regions of high oxygen permeability surrounded by a majority phase that is luminescent, but relatively less sensitive to oxygen quenching. This morphology is due to micro scale phase segregation between the Ir-labeled PDMS and the polystyrene.

7.3.1.2. Ethyl Cellulose

Ethyl cellulose (EC) is a derivative of cellulose in which most of the hydroxy groups on the repeating glucose units are ethylated. EC is very hydrophobic and has been widely used as matrix to host OSPs.^{147, 367, 369, 401, 402} EC is also used because of its oxygen permeability, optical transparency, mechanical strength, and photo- and thermal stability. It is a better solvent for OSPs than silicone rubber, but its permeation selectivity is less expressed. There is one report that the sensing performance of these matrixes was influenced by humidity.⁴⁰¹ This effect can be reduced by plasticizing the EC matrix. Oxygen-quenching often does not follow a linear Stern-Volmer equation, but rather is downward curved. In order to improve the sensing performance, a plasticizer is often added.⁴⁰³ Like poly(vinyl chloride), polyethylene, polystyrene and poly(tetrafluoroethylene), EC efficiently reject ionic species. Except for polystyrene, they all are difficult to chemically modify so that their function is confined to that of a "solvent" for oxygen and a permeation-selective matrix, while electrostatic or covalent immobilization is tedious.

7.3.1.3. Poly(vinyl chloride)

Plasticized PVC has been used to incorporate OSPs, mainly by physical entrapment, rarely by covalent immobilization. Sensor films are readily produced by casting solutions of PVC in tetrahydrofuran and possess good optical and mechanical properties. Pure (non-plasticized) PVC suffers from oxygen permeabilities that are 200 to 10,000-fold lower than those of polysiloxanes.⁴⁰⁴

In addition, hydrolysis of plasticizers of the ester type can occur in basic solution when applying common sterilization techniques. Useful plasticizers include dioctyl sebacate, tributyl- and trioctyl phosphate, dioctyl- and dinonyl phthalate, 2-cyano- and 2-nitrophenyloctyl ether, and related long-chain (and often branched) esters and ethers. Nitrophenyloctyl ether unfortunately can act as a quencher of luminescence, and 2-cyanophenyloctyl ether was recommended instead.⁴⁰⁵ Plasticizers are added to PVC in fractions up to 66% and can be used to govern quenching constants. Plasticized PVC has been used as a host in oxygen sensors in few cases, not the least because the plasticizers tend to leach into the water phase and, in particular, into blood. This is unacceptable and also causes the quenching constants to shift over time.

7.3.1.4. Polymethacrylates

Thermoplastic polymers such as poly(methyl methacrylate) (PMMA; plexiglass)¹⁹⁴ need not be cured, their composition can be easily varied, and oxygen sensitivity can be adjusted by addition of a plasticizer, however with the same compromises as in case of PVC. The glass transition temperature of PMMA is rather high (110 °C), but despite its excellent optical properties, it has not often been used as a sensor matrix, mainly because of low oxygen permeabilities which are 200 – 10⁴ fold lower than those of polysiloxanes.⁴⁰⁴ Permeability increases with the length of the alkyl ester, and in particular in case of silyl esters. The quenching of the RTP of the aromatic hydrocarbons triphenylene and phenanthrene in PMMA has been studied³⁹¹ in order to determine the diffusion coefficients of oxygen. It was found that reduction of the phosphorescence lifetime of the probes in the presence of oxygen is much smaller (by -10% only) than the reduction of phosphorescence intensity (-80%). This was explained in terms of both static and dynamic quenching.

The quenching of the luminescence of a bis(phenylethynyl)anthracene by oxygen at pressures of up to 25 atm in thin films of PMMA was reported⁴⁰⁶ to be due to the structural inhomogeneity of the polymer and the migration of electronic excitation. The local and volume-averaged diffusion coefficients for oxygen were determined. Demas et al.^{243, 407} report that the addition of small amounts of trimethylsilylmethyl methacrylate to a methacryloxy containing PDMS polymer can dramatically improve the quenching of the luminescence of Re(I) complexes by oxygen. In contrast to polymeric esters of (meth)acrylic acid, the respective nitriles, polyacrylonitrile included, are virtually impermeable to oxygen. In fact, they are well suited to shield any kind of probe (for temperature, for example) from oxygen.

7.3.1.5. Polystyrene

Polystyrene (PS) has good optical properties and acceptable permeability and solubility coefficients for oxygen. Sensor films typically are cast from solutions of PS and an OSP in toluene, ethyl acetate,

or acetone. The resulting sensing films show excellent shelf-life and operational stability also in aqueous solutions. Given its moderate solubility for oxygen, it requires probes that are efficiently quenched. PS is not a good solvent for ionic OSPs such as the ruthenium diimine complexes unless the anion is made hydrophilic as discussed in the section on silicones. PS-based sensors may be sterilized by standard methods. Quenching constants are smaller in PS than in silicone by a factor of typically 10 – 100. Its glass transition temperature is ~ 90 °C.

The dynamic range and sensitivity of optical oxygen-sensors based on the probe PtTFFP can be fine-tuned by employing differently substituted PSs.⁴⁰⁸ Poly(2,6-dichlorostyrene) gives linear SVPs, while poly(4-tert-butylstyrene) and poly(2,6-fluorostyrene) yield sensors with increased sensitivity (quenchability) but non-linear SVPs. It was noticed⁴⁰⁹ that PS can be emulsified with silicone to yield films with improved mechanical properties and good adhesion to an optical isolation layer (black silicone).

7.3.1.6. Other Homopolymers

Winnik et al.^{183, 330} reported on a new class of sulfur-nitrogen-phosphorus polymers called poly(thionylphosphazenes) (PTPs) for use in sensor films for oxygen that were referred to as pressure-sensitive paints. The PTPs possess a large free volume, and the polymer structure and the sensitivity can be adjusted over a wide range. High quality films can be obtained without the need of cross-linking. The probe PtOEP was encapsulated in this polymer where it displays extremely high sensitivity to oxygen, with an $I_{0.01\text{atm}}/I_{1\text{atm}}$ value of 58. The material also was used to synthesize gas permeable block copolymers.⁴¹⁰ One of the first articles ever on fluorescent sensing of oxygen describes a sensor film made from polyethylene and oped with various polycyclic aromatic hydrocarbons.³⁵ Polypropylene in the form of non-woven membranes and doped with various porphyrin type OPSs was recently used to sense oxygen.⁴¹¹ The resulting sensors exhibited high brightness, optimal lifetime signals (22 - 30 μs at 21 kPa and 50-60 μs at 0 kPa O_2), linear Stern-Volmer plots, temperature dependence and low cross-sensitivity to humidity.

Polyacetylene and its derivatives (often containing trimethylsilyl groups) form another class of highly gas-permeable polymers).⁴¹² Poly(1-trimethylsilyl-1-propyne) probably has the highest oxygen permeability of all known polymers. The probe PtOEP in this polymer has a quenching factor (I_0/I_{100}) of 225, which makes this combination most useful for trace oxygen sensing.³²¹ However, the long-term stability of this polymer is rather poor and the sensor degrades fast. This is accompanied by pronounced changes in response function. The polysulfones form a group of thermoplastic polymers known for their toughness and stability at high temperatures. They have been used to encapsulate Ru(dpp) with octylsulfonate counterion for oxygen sensing.⁴¹³ The effects of probe concentration and thickness of film on the sensitivity and response time of the obtained

sensors have been systematically studied. Highest sensitivity was obtained with a film thickness of 1.6 μm , and the sensor exhibited linear SVP in the whole range of oxygen concentration. The spectral asymmetry of Ru(dpp) in polysulfone was studied in some detail and used to improve the precision of respective sensors.³⁹⁴ Polysulfone also was found to be a good host for the probe PtTFPP.³⁹⁵

7.3.1.7. Hydrophilic Polymers

Hydrophilic polymers are less permeable to oxygen than most hydrophobic polymers. They are less often used but offer advantages in case of biosensing, in particular in combination with enzymes. They often serve as a host for hydrophobic sensor microparticles.^{313, 414-416} Many polymers of that kind (polyurethanes, for example) are soluble in ethanol or dimethylsulfoxide. The solvent can be easily evaporated at room temperature, so that the preparation of sensing film is convenient and environmentally friendly. Díaz-García et al.²¹³ used gelatin organogels originating from reverse micelle solution to immobilize Ru(bpy). Such organogels are optically transparent and stable in contact with various organic solvents, and have good long-term stability without swelling and/or solubility problems in contact with organic solutions. Grafted hydrophilic polymers also were studied with respect to applications in optical sensor membranes.⁴¹⁷ Specifically, poly(hydroxyethyl methacrylate) (poly-HEMA) containing 9,10-diphenylanthracene as the oxygen-sensitive material was covalently grafted via silane coupling techniques onto fused silica optical fibers. Fluorescence was stimulated by the evanescent wave of a UV laser or a xenon lamp and quenched by -20% when the sensor went from an oxygen-free to an oxygen-saturated (40 ppm) aqueous environment. In additional experiments, glucose oxidase was co-polymerized with HEMA, and a hydrophilic material was obtained that eventually was used as a sensing material for glucose by coupling it to an oxygen probe.

Chitosan is a highly biocompatible composed of aminoglucose monomers that was widely used as a hydrophilic matrix because it is easily accessible. In a typical example, dendrimeric and free forms of the OSP Pd(II) meso-tetra(4-carboxyphenyl)porphyrin were incorporated into a matrix of chitosan-based colloidal particles.⁴¹⁸ UV-cured inorganic-organic polymer composite was used as a host for chitosan-coated magnetic microparticles or on commercial microbeads modified with a ferrofluid and for a ruthenium-based probes.⁴¹⁹ Chitosan also is an excellent host for enzymes. In the given case, the enzyme diamine oxidase was immobilized in the matrix where it catalyzes the oxidation of the amines putrescine and cadaverine under consumption of oxygen. See the Supporting Information for uses of oxygen sensors in enzyme-based biosensors.

Polyurethanes (PUs) form another large class of hydrogels. Hydrophilic supports such as PU are characterized by a large number of hydrogen-bridging functions such as hydroxy, amino, or

carboxamide groups, or by anionic groups (mainly carboxy and sulfo) linked to the polymer backbone. Typical other examples include polyacrylamides and polyglycols. Depending on the degree of polymerization and cross-linking, they are water-soluble or water-insoluble. All swell in water. Throughout, they are easily penetrated by aqueous solutions but have been rarely used in sensors for oxygen due to the lack of permeation selectivity and slow diffusion of oxygen. These materials also are well biocompatible, and various enzymatic biosensors have been reported (see the Supporting Information) with oxygen transduction, where both the enzyme and the OSP are immobilized in the polyurethane. A sensor for uric acid is a typical example.⁴²⁰ Polyurethanes also were used as a paint into which hydrophilic oxygen sensor particles were incorporated,^{416, 421, 422} and in irreversibly responding sensors for oxygen using leuco dyes.¹⁰²

Poly(ethylene glycol) (PEG) hydrogel films were applied⁴²³ as a matrix to incorporate oxygen-responsive ruthenium OSPs which then was grafted and patterned by photopolymerization. An optofluidic sensing platform was obtained that contained embedded oxygen sensing elements that exhibited excellent performance when sensing dissolved oxygen. In another kind of oxygen sensor,⁴²⁴ the probe dichloro(tris-1,10-phenanthroline) ruthenium(II) was immobilized in a photopolymerized hydrogel made from PEG diacrylate, a polymer known to minimize protein and cell adhesion. A low-average molecular weight polymer was employed to prevent fluorophore leaching. The PEG sensors stored were in water for several months and retained their physical shape and sensitivity to oxygen (0 - 9 ppm). Porphyrins can be used as efficient cross-linkers to generate a new class of hydrogels for use in sensing and imaging of oxygen.⁴²⁵ A porphyrins carrying four carboxy groups was reacted with a poly(ethylene glycol) possessing terminal amino groups to form a polyamide in a range of appropriate conditions. The network structure of the hydrogel maintained a porphyrin spacing that prevented excessive fluorescence self-quenching despite high (5 mM) porphyrin density. The near-infrared properties readily enabled low background, noninvasive fluorescence monitoring of the implanted hydrogel in vivo. An oxygen-insensitive copper(II)porphyrin hydrogel was used as a reference dye.

Poly(vinyl alcohol) (PVA) also is easily available and tunable in terms of hydrophilicity but was rarely used in unmodified form because it does not well retain probes and other dyes. Rather, composites were employed, for example⁴²⁶ in a glucose sensor based on oxygen transduction where an organically modified silicate film was doped with Ru(dpp) and covered with a poly(vinyl alcohol) composite with a silica sol-gel containing immobilized glucose oxidase. PVA also served as a support in an optical fiber sensor for biochemical oxygen demand (BOD) because the bacteria needed in such a sensor can be physically immobilized in a PVA matrix.¹⁹² Covalent immobilization of dyes is more promising, and the OSP pyrene was covalently immobilized on PVA via "click" chemistry, a copper(I)-catalyzed azide/alkyne cycloaddition reaction proceeding at

room temperature and in water solution at neutral pH values.¹³⁴

Silamines, a group of water-soluble (di)alkylpolysiloxanes with terminal amino groups (described earlier in the section 6 on iridium-based OSPs) were used in hydrophilic oxygen sensor films along with microcrystalline cellulose.²³² These materials are environmentally friendly and particularly well suited if combined with biomolecules to form biosensors. In subsequent work,⁴²⁷ charged and uncharged iridium luminophores were covalently bound to the silamine by either reductive amination or coupling reactions. Paints sensitive to barometric pressure were obtained by blending the materials with microcrystalline cellulose, and luminophore charge effects were studied by (lifetime) fluorometry. Rather than covalently immobilizing the OSP (and more often in recent years), the oxygen transducer may be first incorporated into hydrophobic micro- or nano-particles which then can be placed in the (silamine) hydrogel matrix (see above; method C).

7.3.2. Organic Copolymers (including fluoropolymers and mesoporous materials)

The use of copolymers is an alternative way to govern sensor properties. Compared to homopolymers, the oxygen permeability of copolymers can be tuned over a wide range by varying the ratio of monomers. Demas et al.¹⁹⁶ have systematically investigated the effects of kind of comonomer (fluorinated and non-fluorinated alkyl methacrylates) and their chain length on the oxygen sensing properties. They observed that with increasing length of hydrophobic chain or the degree of fluorination, the copolymers exhibit enhanced sensitivity to oxygen, but with an optimal chain length. Sensor nanoparticles were obtained by mini-emulsion solvent evaporation of solutions of poly(styrene-co-maleic anhydride) containing a Pt(II)porphyrin complex that acts as a luminescent probe for oxygen, and black magnetite (Fe₃O₄). The size and the polydispersity of magnetic oxygen-sensitive nanoparticles with a typical size of 200 nm was mathematically modeled (by experimental design and response surface methodology).⁴²⁸

Fluorinated copolymers are useful for the construction of optical oxygen sensors of extremely high oxygen permeability. The solubility of oxygen in fluorocarbons is 3 – 10 times better than in the parent hydrocarbons. The C-F chemical bond is short and strong (with a binding energy of 116 kcal mol⁻¹), and the fluoropolymers therefore are quite resistant toward photooxidation. The group of Amao⁴²⁹ have developed several fluoropolymers for oxygen sensing with extremely high sensitivity, these including poly(styrene-co-pentafluorostyrene),³²⁰ poly(styrene)-*co*-(trifluoroethyl methacrylate) ("poly-styrene-co-TFEM"),^{319, 340} poly(isobutyl methacrylate)-*co*-(trifluoroethyl methacrylate) ("poly-IBM-co-TFEM"),⁴³⁰ and fluorinated poly(aryl ether ketone).³²⁷ They observed that the sensitivity of the polymer increased with the degree of fluorination, and all fluoropolymers are highly sensitive.⁴³⁰ The probe PtOEP displays extremely high sensitivities to oxygen, with an I_0/I_{100} of 288 and 296 for poly-IBM-co-TFEM and poly-styrene-co-TFEM, respectively.^{319, 340} The

sensing films are fairly photostable and have response times of ~ 5 s. Schanze et al.¹⁷¹ replaced the styrene monomer by 4-*tert*-butylstyrene (*t*BS) and copolymerized it with TFEM to obtain the copolymer poly-*t*BS-co-TFEM with even higher gas permeability than poly-styrene-co-TFEM, and the immobilized probe PtTFPP also displays very high sensitivity.

Poly[(hexafluoroisopropyl methacrylate)-co-(heptafluoro-*n*-butyl methacrylate)] ("FIB") is a unique fluoropolymer for producing sensors and pressure-sensitive paints.^{229, 271, 272, 431} It has excellent permeability for oxygen and a temperature dependence that is much smaller than that of other polymers. Ertekin et al.²⁰⁷ have doped silicone host matrices with four kinds of perfluorinated hydrocarbons having different degrees of fluorination. It was found that the sensitivity of the ruthenium probe was greatly enhanced when increasing the "fluorine number". Even the medically used oxygen carrier F₁₉-decanoic acid can serve as a sensor matrix,⁴³² and the luminescence of ruthenium-based oxygen probes was found to be strongly quenched therein. In subsequent work, the sensitivity and stability of TPP-based optical oxygen sensing films made from polystyrene, ethyl cellulose, poly(1-trimethylsilyl-1-propyne) and poly(isobutylmethacrylate) also was improved by adding perfluorochemicals.⁴³³

Nafion is a fluorinated copolymer based on sulfonated tetrafluoroethylene. It is not soluble in, but highly permeable to water. Nafion is a chemically inert, gas-permeable ionomer material that can be easily cast (from commercially available solutions) in the form of thin films or other coatings. Ionic and polar probes can be easily immobilized on the surface of cast films of commercially available membranes in order to construct oxygen sensors, for example via adsorption^{434, 435} or cation exchange.²¹² However, the spectral properties of the obtained sensing films are sensitive to the degree of Nafion swelling by organic solvent, and the leakage of ionic probes from the film cannot be excluded. Cationic metalloporphyrins were irreversibly immobilized on Nafion by a simple method.²⁸⁶

While fluoropolymers increase quenchability, the addition of gas-blocking polymers can reduce it. This enables quenching to be adjusted to a desired efficiency. The copolymer poly(styrene-co-acrylonitrile) (PSAN), for example, enables the sensitivity of oxygen sensors to be tuned by varying the fraction of poly(acrylonitrile).⁴¹⁴⁻⁴¹⁶ Compared to PS, the oxygen sensitivity in PSAN is significantly decreased. Tian et al.^{301, 303} co-polymerized 2-hydroxyethyl methacrylate and styrene with PtTFPP bearing four methacrylate groups. The dye is covalently attached and sensitivity can be adjusted via the fraction of the methacrylate.

Stubenrauch et al.⁴³⁶ have immobilized PtTFPP in various poly(norbornenes) that were obtained by ring opening metathesis copolymerization. These materials have high glass transition temperatures and high optical clarity. The oxygen permeability was increased by introducing bulky side groups. Sensing layers based on polymers with bulky groups exhibited high sensitivity to

oxygen ($I_0/I_{35\text{hPa}} \sim 2.75$) and were used for trace oxygen sensing. Di Marco et al.²¹⁶ co-polymerized the macromonomer poly(ethylene glycol) with an ethyl ether methacrylate to obtain the co-polymer pPEGMA. This polymer is affordable, chemically stable, fully amorphous, and has a low glass transition temperature. This results in a good permeability and adhesion. The quenching of the luminescence of the probe $[\text{Ir}(\text{ppy})_2(\text{dpt-NH}_2)](\text{PF}_6)$ incorporated into this polymer follows a strictly linear Stern-Volmer plot. The same group³²³ also studied the effect of molecular weight of pPEGMA on the oxygen sensing performance. The Winnik group⁴³⁷ have prepared nonaqueous dispersions of poly(vinyl acetate) particles that were sterically stabilized with poly(ethylhexyl methacrylate). Trace quantities of phenanthrene were covalently bound to either polymer. Their fluorescence is very similar in degassed samples, but strong differences were noted in the presence of oxygen. The effect was used to study effects of morphology and swelling. In a very different and new approach, very small amounts of Ru(II) were doped into a flexible, ultramicroporous, fluorescent Zn(II) azolate coordination polymer to produce phosphorescent materials with very high and tunable oxygen quenching efficiency. This approach resulted in a simple color-changing ratiometric oxygen sensor.⁴³⁸ However, this sensor is more complex (both in terms of materials synthesis and sensor fabrication) than known sensors with either instrumental or visual read-out.

Table 12. Significant properties of representative polymers for use in oxygen sensing. Representative chemical structures are given in Figure 18. Permeability (P) data are given in $10^{-13} \text{ cm}^3 \cdot \text{cm}(\text{cm}^2 \cdot \text{s} \cdot \text{Pa})^{-1}$ units.

<i>Polymer [acronym]</i>	<i>P</i>	<i>Comments</i>	<i>Refs.</i>
Ethyl cellulose [EC]	11.0	Biocompatible; good optical transparency; good mechanical strength.	439
Poly(dimethyl siloxane) [PDMS]	695	Excellent gas permeability, high thermal stability, excellent chemical and mechanical stability, ease of handling, good adhesion to glass fibers, inertness to biological samples, optically transparent; hydrophobic; low glass transition temperature; many commercially available prepolymers contain solvents, fillers, low molecular weight cross-linkers, catalysts and other additives; need for curing.	49, 122, 127, 398, 399
Poly(methyl methacrylate) [PMMA]	0.116	Thermoplastic; easy to manufacture and reproducible; low cost; poor oxygen permeability; only useful for sensing oxygen at high partial pressure; photostable; good optical transparency; no need for curing.	194, 287, 329, 335
Polystyrene [PS]	1.9	Easy to manufacture; low cost; moderate oxygen permeability; allows oxygen sensing at high concentration; may be sterilized; excellent shelf time and stability in aqueous solutions; good optical transparency; no need for curing; much lower sensitivity than PDMS.	267, 440, 441
Poly(1-trimethylsilyl-1-propyne) [PTMSP]	11251 ⁱ	High gas permeability; no need for cross-linking; good photostability; useful for trace oxygen sensing.	321
Poly(styrene)- <i>co</i> -(pentafluorostyrene) [poly-styrene- <i>co</i> -PFS]	n.d.	Extremely high gas permeability; excellent photostability; short response time; useful for trace oxygen sensing.	320, 429
Poly(styrene)- <i>co</i> -(trifluoroethyl methacrylate) [poly-styrene- <i>co</i> -TFEM]	n.d.	Extremely high gas permeability; excellent photostability; short response time; useful for trace oxygen sensing.	220, 340
Poly(isobutyl methacrylate)- <i>co</i> -(trifluoroethyl methacrylate) [poly-IBM- <i>co</i> -TFEM]	n.d.	Extremely high gas permeability; excellent photostability; short response time; useful for trace oxygen sensing.	319, 430
Poly(4- <i>tert</i> -butylstyrene)- <i>co</i> -(trifluoroethyl methacrylate) [poly- <i>t</i> BS- <i>co</i> -TFEM]	n.d.	Extremely high gas permeability (even higher than poly-styrene- <i>co</i> -TFEM); excellent photostability; short response time; useful for trace oxygen sensing.	171
Poly(hexafluoroisopropyl methacrylate)- <i>co</i> -(heptafluoro- <i>n</i> -butyl methacrylate) [FIB]	n.d.	Extremely high gas permeability; excellent photostability; short response time; small temperature dependence; suitable for application in wind tunnels with temperature compensation.	271, 272, 431
Poly(styrene- <i>co</i> -acrylonitrile) [PSAN]	0.0032	Moderate gas permeability that can be tuned by changing the ratio of monomers; good stability; easy to handle.	271, 272, 431
Nafion	0.81 ⁱⁱ	Ionic polymer; chemically inert; good gas permeability; probes can be absorbed on the polymer; sensitivity depends on the swelling in different solvent.	212, 286, 434, 435

ⁱ Calculated from S. Asakawa, Y. Saitoh, K. Waragai, T. Nakagawa, *Gas Sep. Purif.*, **1989**, 3, 117–122.

ⁱⁱ Oxygen permeability of dry Nafion 117 at 35 °C and 1 atm. Data from Chiou, J. S.; Paul, D. R. *Industr. Eng. Chem. Res.* **1988**, 27, 2161.

7.3.3. Organic Nanofilms

The most common nanofilms are those prepared by the Langmuir-Blodgett (LB) technique. LB layer-based sensors can be produced fairly reproducibly and in a well-defined thickness, and they display short response times. On the other hand, conventional LB layers are prone to mechanical disruption, quickly destroyed by (blood) serum, and yield poor signal-to-noise ratios (SNRs). Polymeric lipid membranes may be a more stable alternative as shown by Mitsuishi et al.,³⁴⁵ and evanescent wave (multiple) excitation may improve the SNR. Beswick and Pitt²⁶³ assembled PdTPP in LB films made from arachidic acid or pentacosanoic, 12-diyonic acid. The films give fast response due to the ordered structure within the monolayer assemblies. The results showed that the LB technique enables the production of nanofilms of fairly good optical quality. LB films can be used as claddings on optical waveguides since the thickness and refractive index of LB films can be well controlled. Schaffar & Wolfbeis⁴⁴² described sensors for oxygen, halides and pH by incorporating lipophilic fluorescent probes (ter.-butyldecacyclene in case of oxygen) into LB films. The sensors, while only a few nm thin, were found to be prone to disruption by detergents and blood samples.

Multilayer fluorescent thin film chemical sensors also were obtained by electrostatic layer-by-layer self-assembly.⁴⁴³ Ruthenium-based oxygen indicators were used as model fluorophores. Three techniques for building fluorescent sensing films were considered, viz. direct electrostatic assembly of charged fluorescent indicators, fluorophore/polyion premixing, and conjugation of indicator to the polyelectrolyte. In all cases, the films retained oxygen sensitivity and did not exhibit significant self quenching. Another polyion with entrapped OSP was applied to manufacture spin-assembled oxygen sensitive nanofilms.⁴⁴⁴ The sensor demonstrated good correlation to the Stern–Volmer relationship, with linear decay in sensitivity of approximately 1.6% per week. Response to gaseous oxygen was linear over a 0 – 100% concentration range, with a resolution of $\pm 0.2\%$.

Self-assembled ionic nanofilms on top of fluorescent nanoparticles represent another type of nanoscale oxygen sensors.⁴⁴⁵ The probe Ru(dpp) was immobilized within polyelectrolyte multilayers deposited on the surface of nanoparticle templates by the layer-by-layer (LbL) technique. The ionically bound nanofilms create a porous scaffold into which controlled precipitation of the OSP is achieved using a combination of electrostatic attraction and dye insolubility in water. The fluorescent nanoparticles act as physical scaffolds and also provide a complementary spectral signature for use as an internal reference. Oxygen sensors created on 100-nm yellow-green fluorescent particles exhibit a linear Stern–Volmer response. The nanosensors were chemically delivered into human dermal fibroblasts with no apparent loss in cell viability.

Papkovsky et al.⁴⁴⁶ described oxygen sensitive materials based on nanostructured films of high-density polyethylene and polypropylene. The polymer substrates were subjected to solvent crazing to produce well-defined 3D networks of nanopores (size < 15 nm) and with a volume porosity of up to 60 %. OSPs such as PtTFPP and PtOEPK were added during or after the solvent crazing process, and found to be firmly trapped in the nanopores. Such sensing materials are chemically and mechanically stable, and their preparation is simple.

7.4. Inorganic Supports and Matrix Materials

Inorganic materials are attractive materials for fabricating optical oxygen sensors because they have good mechanical strength, high thermal and oxidative stability, and often can be produced at room temperature. The following sections cover the most important groups of solid materials, viz. (porous) glass, silica, sol-gels, organically modified silicates, but also metals and metal oxides.

7.4.1. Silicates (including Sol-Gels)

The use of such materials in optical chemical sensors and biosensors has been reviewed.⁴⁴⁷ The surfaces of silica materials (glass included) can be varied to a very wide extent by applying either hydrophilic or hydrophobic surface-modifying reagents, often of the silane type. Reagents such as aminopropyl triethoxysilane have been widely used to introduce amino groups on glassy surfaces and to immobilize various probes and biomolecules thereon. Glass does not measurably swell but is difficult to handle in view of its brittleness. Sol-gels (see below) and hybrid materials form a more attractive alternative to conventional glass. Moreover, OSPs may be easily incorporated into such glasses at room temperature conditions. Materials are preferred that have high specific surface and strong absorption. Kautsky³² and Terwoord et al.³³ have absorbed OSPs on silica gel which is useful because of its excellent thermal stability, but practically all such sensors are cross-sensitive to humidity. Numerous other OSPs have been deposited on silica gel later and applied for solid-state oxygen sensing.^{14-17, 32, 33, 161, 343, 448} Silica also has been used as a filler^{47, 190, 198, 325, 390, 398, 449, 450} to improve the oxygen sensing performance of inorganic-organic hybrid materials. This will be discussed in **Section 7.2.3**.

Porous glass has good optical transparency and excellent mechanical strength. Because of the inner porous structure, it has a high specific surface. Bergman³⁵ absorbed the OSP fluoranthene in porous glass to sense the atmospheric oxygen. Pyrenebutyric acid was covalently coupled to amino-functionalized controlled pore glass (CPG),⁴³ and a sulfonated Ru(II) complex was covalently linked onto CPG particles which allowed direct monitoring of oxygen in many solvents and without leaching.¹⁸⁰

Zeolites and mesoporous silica can be used for absorbing OSPs into their inner pores so to

develop another kind of oxygen sensor. Wolfbeis et al.²⁰⁹ encapsulated Ru(bpy) in zeolite Y cages and mixed the particles with silicone rubber prepolymers to form oxygen sensing films after vulcanization. The sensing films display high quenching efficiency (with an I_0/I_{100} value of ~ 4 which, surprisingly, is higher than without the zeolite cage) and excellent stability. Even if stored in water at ambient temperature for several months, there is no obvious change in the sensing properties. Such sensors can be operated at temperatures up to 200 °C. The positively charged probe Ru(bpy) also was absorbed in mesoporous silica materials such as C₁₈-FSM,⁴⁵¹ MCM-41,⁴⁵² MCM-48⁴⁵³ and silica spheres.²¹⁰ However, the results of Pang et al.²¹⁰ who absorbed Ru(bpy) in 100-200 μm mesoporous silica spheres revealed that it displays rather poor sensitivity and slow response. Very efficient quenching of luminescence by oxygen was observed⁴⁵⁴ with functionalized mesoporous silica of types SBA-15 and MCM-41 and doped with a novel Pt(II)–porphyrin complex. The ratios of luminescence intensities under 0% and 100% oxygen are $> 8,700$ for the doped SBA-15 material, and $> 3,800$ for MCM-41 (at a doping of 20 mg/g).

On the other hand, Wang et al.⁴⁵⁵ report on a multifunctional mesoporous nanocomposite with magnetic, optical, and excellent oxygen-sensing performance. This multifunctional nanomaterial was prepared by covalently grafting Ru(II) polypyridyl complexes into the channels of magnetic mesoporous silica nanocomposites. The super-paramagnetic nanocomposites allow oxygen to be sensed with good sensitivity ($I_0/I_{100} = 5.2$) and short response and recovery times. Similar findings on flexible ultramicroporous frameworks were reported by others.⁴³⁸ A synthetic layered porous clay mineral (Sumecton) was doped with Pt(II) and Pd(II) porphyrins.⁴⁵⁶ These are known to be very efficient agents for sensing applications because of a “heavy atom effect”. The combination of metalloporphyrin and layered materials results in good sensitivity at aerobic conditions, but the sensors are very slow.

Sol–gel glasses have favorable mechanical properties, chemical stability, and superior optical clarity. They are prepared by room-temperature reaction of organic precursors, and their chemical properties can be flexibly tuned by using different precursors. The properties of sol-gels made from tetraalkoxy silanes resemble those of controlled porous glass (CPG). The bulk phases (unlike the pores) of conventional sol-gels and CPGs are impermeable to oxygen, and OSPs therefore have to be deposited on their surface which, however, can be quite large in view of the micro/nano-porous structure of sol-gels and CPGs. Moreover, with alkyl(aryl)triethoxy silanes or dialkyl (or aryl alkyl)diethoxy silanes can be applied to yield organically modified silicates (“ormosils”, see **Section 7.2.2**). These are permeable to oxygen (higher fractions of alkyl and – in particular – aryl siloxanes favoring oxygen permeability and probe solubility), so that the OSPs can be directly incorporated into the matrix. Drying and heat treatment have been applied to progressively densify the gel by elimination of solvents and water. By adding the OSPs to the sol and by appropriate

choice of initial pH value and reaction temperature, the OSPs can be trapped in the nanocages formed during the gelation. At the sol stage, films can be coated onto a variety of substrates including optical fibers, capillaries and (waveguide) planar glass.

MacCraith et al.²⁰¹ used the sol-gel technique to prepare microporous glass films with immobilized ruthenium probes for use in oxygen sensing. The sensor preparation (hydrolysis of tetraethyl orthosilicate in acidic solution at room temperature) is simple and reliable. The films are tough, inert, and often chemically bound to the supporting substrate which further improves physical stability. Sensitivity can be adjusted by varying the pH of the precursor solution to increase the overall pore volume. Lee and Okura^{315,316} doped PtOEP into sol-gel glasses prepared by hydrolysis of tetraethoxysilane. The addition of the surfactant Triton X-100 improved the homogeneity of the silica sol and results in crack-free sensing films. The probe PtOEP was immobilized in this material where it is efficiently quenched (with an I_0/I_{100} of > 40). Again, the preparation of the sensing films takes > 2 weeks. Fluorinated xerogels doped with quenchable Pt(II) complexes were reported³³⁸ to have fast response (4 – 7 s), good sensitivity, and linear SVPs. Rather similar materials resulted in even faster responses as reported in a second paper by this group.³³⁶ However, most other oxygen sensors based on mixed polymer materials display nonlinear Stern-Volmer relationship, and this can be described by the so-called two-site model (see above).

It was also noticed²⁰⁰ that the structure and oxygen quenching capability of sol-gel sensor films is strongly related to parameters such as the speed of dip-coating, the water-to-precursor ratio, pH value, and aging time. The porosity and average pore size of the films strongly depend on the water-to-precursor ratio, and this affects the diffusion of oxygen. On the positive side, this enables the quenching efficiency of sol-gel films to be fine-tuned and optimized. On the less positive side, this implies compromised reproducibility. Kuncová and coworkers¹⁶⁵ immobilized Ru(phen) in xerogels. The preparation of the film is simple, but takes 1 – 2 weeks. However, the xerogel – like many sol-gels and ormosils – is not stable over time in aqueous solution, probably the result of ongoing condensations in the network.

The response to oxygen of Ru(dipy) in two room-temperature ionic liquids (RTILs) has been evaluated in terms of sensitivity, stability, regeneration ability and response time of a sensor.⁴⁵⁷ The response times range from 2 to 5 s. The RTILs warrant good oxygen solubility, enhanced brightness and photostability. The stability the Ru(II) complex in RTILs was tested over 12 months when stored on laboratory air. The sensing performance of a sensor composed of Ru(bpy) in a sol-gel matrix modified with an RTIL is reported to be much better than that of a plain sol-gel.⁴⁵⁸ An ionic liquid was added during acid-catalyzed formation of the sol-gel from TEOS to give sol-gel sensor films that exhibit larger quenching constants, linear Stern-Volmer plots, and crack-free surfaces. The addition of the ionic liquid also caused a 23-nm red-shift in the emission peak wavelength, but

the composite is only applicable to gas phase measurements.

7.4.2. Organically Modified Silicates (Ormosils)

The use of hydrophobic organically modified precursors (for example of octyl- or phenyl-triethoxysilane) leads to the so-called ormosils that are hardly permeated by ionic species, but quite well by oxygen and other small-molecule gases. Such materials have properties that are intermediate between glass and organic polymers, and are attractive host matrices for OSPs. The hydrophobicity (and permeation selectivity) of the materials may be adjusted either via the nature of the organic groups introduced into the glass, or by adjusting the ratio of precursors of the type $\text{Si}(\text{OR})_4$, $\text{R}_1\text{-Si}(\text{OR})_3$, and $\text{R}_1\text{-Si}(\text{OR})_3\text{-R}_2$, where R_1 and R_2 stand for alkyl or aryl groups. Ormosils contain fewer free silanol groups and consequently will be less densified over time. As a result, they possess improved long-term and storage stability. Their micro-polarity can be easily probed by using a solvatochromic dye.⁴⁵⁹

MacCraith et al.⁴⁶⁰ systematically modified the water-to-precursor ratio in order to tailor the microstructure and sensitivity of ormosil sensing films for gaseous and dissolved oxygen. Hydrophobicity was increased by using organically modified precursors such as methyltrimethoxysilane (MeTriMOS) or ethyltrimethoxysilane. The addition of MeTriMOS was found to strongly increase the sensitivity for dissolved oxygen. Murtagh et al.⁴⁶¹ made similar observations in a study on the oxygen sensing properties of Ru(dpp) immobilized in MeTriMOS-based ormosil gels. The incorporation of platinum porphyrins into the ormosil coating also has been reported⁴⁶² to give luminescent sensor materials for oxygen.

Sensors for oxygen based on an ormosil matrix were presented⁴⁶³ along with a large set of luminescence decay time based chemical sensors for clinical analytes including oxygen, pH, CO_2 , K^+ and glucose. Sanz-Medel et al.³⁴⁹ prepared sol-gel films from TMOS and MeTriMOS to immobilize the Al(III)-ferron complex. The resulting RTP-based oxygen sensor was used for monitoring oxygen in gas phase, in water and in organic solvents. The sensing films are quite rigid (which favors RTP and prolongs the triplet lifetime of the probe). The sensors have fast response, good reproducibility and detection limits as low as 5 ppm (v/v) in the gas phase. The use of MeTriMOS increases film stability in both aqueous and organic solutions. García and coworker¹⁵⁹ applied the same ormosil to entrap erythrosine B (via its isothiocyanate) to obtain another kind of RTP oxygen sensor. The physical properties and oxygen sensing performance were governed by parameters such as the ratio of TMOS-to-MTMOS and even the fraction of alcohol when dissolving the precursors. If prepared at high pH, highly porous silica glass is obtained, while low pH values lead to rather dense sol-gel films.

Phenyl-substituted ormosils have particularly attractive properties with respect to sensing oxygen.

An ormosil that is soluble in organic solvents such as chloroform was prepared²⁰⁴ from phenyltrimethoxysilane (Ph-TriMOS) and the end-capping agent trimethylmethoxysilane (TMMOS). The mechanical and photophysical properties of the sensing films were tuned by adjusting the ratio of Ph-TriMOS and TMMOS. Sensing films with a low content of TMMOS display high oxygen sensitivity and fast response time (250 ms), most likely because the presence of phenyl groups improves oxygen permeability. The solubility in polar organic solvents is a unique feature that facilitates the preparation of various kinds of sensor formats including fiber optic, planar, or evanescent wave sensors. The material is used in a commercial sensor for oxygen. On the other side, it is insoluble in water, ethanol and methanol, and thus well suitable for sensing bioliquids. Similar ormosil films were prepared later²⁰⁵ from dimethoxydimethylsilane as the organic modifier. This kind of sensor also is highly sensitive and has a fast response and long-term stability.

The polycondensation of *n*-octyltriethoxysilane (octyl-TriEOS) and TEOS in the presence of the probe Ru(dpp) leads to ormosils that display purely single-exponential luminescence decay times and linear Stern-Volmer plots (SVPs).²⁰³ Unlike in sensing films derived from TEOS, where sensitivity decreases by a factor of almost 5 after 11 months, response remained virtually constant. The authors also studied⁴⁶⁴ the effect of alkyl chain length of the organically modified precursors on the sensors' performance. The same ormosils served as a host matrix for the probes PtTFPP and PtOEP, and the resulting sensors were found³³⁶ to possess high sensitivity ($I_0/I_{100} = 22.3$ for PtTFPP, and $I_0/I_{100} = 47.8$ for PtOEP) and short response time (0.6 s). It was also observed³³⁷ that the addition of silica nanoparticles (prepared by the Stöber method) to the ormosil material enhances quenching by oxygen. Sensing films based on PtTFPP, silica nanoparticles and ormosil display, in fact, extremely high sensitivities ($I_0/I_{100} = 166$), and very short response time (1.3 s). The probe PdTFPP was doped⁴⁶⁵ late into an ormosil prepared from *n*-propyltrimethoxysilane (*n*-propyl-TriMOS), tetraethylorthosilane, and *n*-octyltriethoxysilane ormosil, and the material show very high sensitivity ($I_0/I_{100} = 263$).

Sensitivity (in terms of detection limits) can be substantially improved by employing fluorinated precursors.⁴⁶⁶ The precursors *n*-propyl-TriMOS and 3,3,3-trifluoropropyltrimethoxysilane were co-condensed under acidic conditions and doped with Ru(dpp) to give a sensor material of high sensitivity ($I_0/I_{100} = 35$) and very small signal drift (<2 % over 6 months). The same material was doped with probes PtTFPP and PtOEP,³³⁸ this again leading to improved sensitivities ($I_0/I_{100} = 68.7$ for PtTFPP and $I_0/I_{100} = 82.5$ for PtOEP) and response times ~ 3 s. The same group³³⁹ used three other precursors (partially fluorinated). The introduction of both fluoro substituents and octyl groups made the sensing film even more sensitive (I_0/I_{100} up to 155). An overview on fluorinated ormosil xerogels as optical chemical sensors have been provided⁴⁶⁷ and showed how, together with

the dye quenching rate, the subtle structural features of an organofluorosilica matrix is of fundamental importance in determining the overall sensor performance.

Fluorinated xerogel films containing Ru(bpy) were employed⁴⁶⁸ in fiber optic sensors for dissolved oxygen. The response time is 4 s, and 0.04 ppm of oxygen can be detected in water. The SVP is linear so that two-point calibration is possible. Another fiber optic (and evanescent wave) sensor is making use of a fluorinated ormosil doped with a ruthenium probe, and a fluorinated ormosil was obtained⁴⁶⁹ by co-condensation of *n*-propyltrimethoxysilane and 3,3,3-trifluoropropyltrimethoxysilane. The OSP in the fluoro-ormosil was photoexcited by the evanescent wave produced on the surface of the fiber core using a blue LED as the light source, and luminescence detected with a miniaturized photomultiplier tube. The LOD of this sensor material is 0.01% of oxygen, and the response time is about 1 s. The same xerogel was used in an integrated micro-volume fiber optic sensor based on Ir(III) complexes.⁴⁷⁰

Xerogel ormosils doped with platinum(II) porphyrin dyes represent other sensing materials with a widely adjustable sensitivity, reversible and fast response (1 s), linear calibration plots, and long-term stability.⁴⁷¹ They have been prepared from pentafluorophenylpropyl-trimethoxysilane, *n*-octyltrimethoxysilane, tetramethoxysilane and 3,3,3-trifluoropropyl-trimethoxysilane. The sensitivity of the materials to oxygen was tuned by adjusting the xerogel composition and the luminophore.

In one further kind of highly sensitive fluorinated sol-gel sensor film,⁴⁷² the matrix was prepared from 3,3,3-trifluoropropyltrimethoxysilane and TMOS, and the well-known OSP Ru(dpp) was entrapped in a wide range of ormosils in different precursor ratios. The influence of matrix composition on sensitivity, interference by humidity, and on long-term stability was investigated, and performance was compared to that of similar but non-fluorinated films. The lowest limit of detection is 0.002% of oxygen. It is obvious from the compilation in this section that the number of ormosils for use in sensors for oxygen (and other gases) is virtually unlimited. In fact, the number seems to exceed the current need.

Ormosils with covalently linked (rather than physically embedded) OSPs were obtained by co-condensation of OSPs carrying trimethoxysilane groups with various siloxanes. A triethoxysilyl-functionalized Ru(bpy) was chemically linked to a conventional ormosil matrix,¹⁸² and the probe PtTFPP was modified in the same way.³⁰³ The sensing films obtained have excellent stability and high sensitivity ($I_0/I_{100} = 70$). Mesostructured silica covalently grafted with Ru(II)(bpy)₂(phen) was reported⁴⁷³ to represent an excellent sensor material. The network was prepared via a sol-gel approach with the help of cetyltrimethylammoniumbromide (CTAB) surfactant. 1,10-Phenanthroline was covalently grafted to 3-(triethoxysilyl)propyl isocyanate which not only is the sol-gel precursor but also acts as the second ligand of the Ru(II) complex. The bulk xerogels were

spin-coated to form thin films that show good homogeneity and sensitivity to oxygen. The covalently grafted OSPs are said to be superior to the physically incorporated ones.

7.4.3. Organic Polymers with Inorganic Fillers

The rheological properties of polymers can be modified by the addition of "fillers". This can improve the strength of the polymer without altering the chemistry of the network. There are several requirements for a filler to be suitable: (1) It must not substantially alter the properties of the polymer; (2) it must not act as a quencher of luminescence; (3) it should be substantially alter the properties of the luminescent probe. White particles (such as fumed silica, or TiO₂ or Ba₂SO₄ micro/nanoparticles) can be added as fillers but also can improve the intensity of the optical signal because of improved scattering of both the exciting light and luminescence. Black particles also can act as fillers and simultaneously can act as optical isolation (see below).

The effects of mineral fillers of nanometer dimensions on the performances of optical oxygen sensor based on organic polymers were studied by the groups of Cox^{389, 390} and Winnik.⁴⁷⁴ It was found³⁸⁹ for a series of poly(dimethyl siloxanes) of various viscosity that oxygen has a large diffusion constant D ($0.115 \text{ cm}^2 \text{ s}^{-1}$) and a low activation energy E_D ($4.8 \text{ kcal mol}^{-1}$) which is not temperature-dependent between 5 and 45 °C. For comparison, the diffusion coefficient for oxygen in water is $2.5 \times 10^{-5} \text{ cm}^2 \text{ s}^{-1}$ at 25 °C. The diffusion coefficient is independent of oxygen concentration and fluorophore concentration in silicone over the usual pressure and temperature range. In the presence of small weight fractions of fumed silica fillers, the diffusion of oxygen is reduced, but the activation energy is not affected at all.³⁹⁰

If OSPs are poorly soluble in polymers, inorganic particles can serve as carriers to transfer the OSP molecules into polymer matrix. It is thought that the probes are bound to the particle surface or trapped inside the pores of silica or porous glass. In its most simple form,⁴⁷ a probe such as Ru(bpy) is placed in and on silica gel, and the dye-doped particles are then dispersed into a silicone rubber matrix to obtain an oxygen-responsive material. In this particular case, silica acts as (a) a filler, (b) a mechanical support of the probe, and (c) as a scattering material. It is mandatory, however, to warrant an even distribution of the probe on the particle, but even if so, the SVPs are mostly nonlinear. This method has been widely used in subsequent years and has experienced many modifications.²⁰⁹ Wong et al.¹⁹⁸ have compared the oxygen sensing properties of silica-containing silicone rubber sensing films with silicone films without silica fillers. The probe Ru(dpp) was first absorbed onto fumed silica and then dispersed in silicone rubber to form sensing films. Compared to films without silica, the response time of the silica-containing silicone rubber films both in the backward direction is much longer than in films without silica. This was interpreted in terms of strong adsorption of oxygen so that the desorption kinetics is slow.

Similarly,¹⁹⁹ Ru(dpp) was absorbed on silica gel and dispersed in a film of gelatin to obtain an oxygen sensor that works in organic solvents. The sensing material is photochemically inert and can be easily molded into different shape with good mechanical and chemical stability. It also has good sensitivity and low detection limits. The same probe also was encapsulated^{172, 475} in ormosil microbeads, which then were immobilized in a hydrogel to construct planar oxygen sensors.

Winnik et al.³²⁵ have systematically examined the influence on oxygen diffusion and permeation in the linear hybrid polymers obtained from PDMS and poly(*n*-butylaminothionylphosphazene) (C₄PATP) in the presence of 10-nm silica particles. The results revealed improved mechanical properties of both polymers, but perturbed oxygen diffusion and permeability. The quenching constants depended on the fraction of silica filler. The luminescence both in silica-free and in silica-filled C₄PATP films decays mono-exponentially in the absence of oxygen, which proves that the PtOEP remain dispersed molecularly in the polymer rather than being absorbed on silica nanoparticles.

7.4.4. Metals and Metal Oxides as Solid Supports

The group of Amao have studied sensor films based on chemically binding of a mercapto group to metal surface (Au, Ag, or Pt) or of a carboxy group to an oxidic surface (such as Al₂O₃, Fe₂O₃, TiO₂). OSPs bearing carboxy groups, such as 1-pyrenedecanoic acid,^{129, 130} pyrene-1-butyric acid,^{128, 131-133} PtTCPP,^{295, 296} PdTCPP,²⁹⁴ PdP-C₁₀-COOH with long alkyl chains,^{341, 342} and Tb(acac)₃(phen)^{254, 255} have been successfully assembled. Positively charged probes such as Ru(dpp), Ru(phen) and Ru(bpy) were first electrostatically attached to (negatively charged) poly(acrylic acid) and poly(sodium 4-styrene sulfonate), and then were chemisorbed onto an alumina plate to obtain planar optical oxygen sensors.^{167, 195} However, the resulting sensor layers only exhibit moderate sensitivity. The group of Mills⁴⁷⁶ have introduced titania sol-gels as a novel kind of sol-gel derived film for luminescence-based oxygen sensing using the OSP Ru(bpy). A titania sol-gel paste film was cast onto microscope slides, and the cationic OSP electrostatically to the negatively charged hydroxy groups on the film's surface from an aqueous solution at pH 11. The resulting sensor film is extremely oxygen sensitive in that a *p*O₂ of 0.011 atm reduced luminescence by 50%.

7.5. Nanoparticles

Oxygen sensitive nanoparticles (NPs) have experienced a large success because they enable micro- and nanostructured systems such as cells, tissue, or nanoscale devices to be studied. In terms of sensing oxygen, there is no alternative to such NPs at present. Due to their small size, there is virtually no diffusion barrier for oxygen, and response therefore is fast. Nanobead sensors also are

widely used now for imaging oxygen. Other nanostructured materials (including nanofilms) have been discussed in **Section 6.3**. Applications are summarized in the **Supporting Information**.

7.5.1. Organic Materials for Nanosensors

The most direct approach to obtain nanosensors for oxygen is to entrap the probe inside an appropriate NP. In one early method,¹⁵⁷ pyrenebutyric acid was dissolved in a benzene/poly(dimethylsiloxane) cocktail and entrapped in polyacrylate capsules with an average diameter of 150 to 250 nm. In another method,⁴⁷⁷ the dye was dissolved in dioctyl phthalate, encapsulated in polyurethane, and suspended or embedded in silicone rubber or water. The quenching efficiency was found to be slightly smaller than in homogeneous solution, an effect that was attributed to boundary layer phenomena at the interface between the different phases.

Many conventional bulk polymers can be converted into nanosized particles using the so-called precipitation method.⁴⁷⁸ This method is simple in that it only requires the OSPs and polymers to be dissolved in a – usually water-miscible – solvent and to precipitate the nanoparticles by slow addition of water. Polyacrylonitrile (PAN) NPs dyed with Ru(phen) were obtained⁴⁷⁹ by precipitating them from a solution in dimethylformamide. Such particles are impermeable to oxygen so that the indicator in the particles is not quenched. Rather, such particles may serve as labels, as reference fluorophores, or as oxygen-insensitive probes for temperature. Borisov et al.²⁷⁵ incorporated Pt(II) and Pd(II) benzoporphyrins into polysulfone nanobeads prepared by the precipitation method. The group also applied used this method⁴⁷⁸ to transform the following bulk polymers into the respective NPs for use in nanosensors: Poly(styrene-*co*-maleic anhydride), polysulfone, cellulose acetate, poly(vinylidene chloride)-*co*-(acrylonitrile), poly(methyl methacrylate)-*co*-(methacrylic acid), poly(hydroxyethyl methacrylate), polyurethane, hydrothane, ethyl cellulose, Nafion and Eudragit. The resulting uncharged beads (with an average diameter of ~ 380 nm) are stable in water and do not aggregate. The biocompatible cationic Eudragit was converted⁴⁸⁰ into nanoparticles by the precipitation method in the presence of the probe PtTFPP to give sensor NPs with an average particle size of ~ 30 nm. Such particles are easily internalized by cells.

Commercially available polymer NPs are another source for fabricating oxygen nanosensors. They can be swollen in an organic solvent, and the OSPs also contained in the solvent are taken up by the NPs to give oxygen-sensitive nanobeads. Schmäzlin et al.^{440, 481} have encapsulated PtTFPP in carboxylated microbeads of polystyrene (PS) and used them to determine dissolved oxygen in plant cells. The hydrophobic and inert nature of PS prevents dye leakage, and the beads are well compatible with living cells. Wang et al.⁴⁸² stained amino-functionalized polystyrene (PS) nanoparticles with PtTFPP along with a reference dye via the swelling method to obtain a NPs for

imaging intracellular oxygen. Both dyes are retained by the nanoparticles, and PtTFPP has a good sensitivity to oxygen. Commercially available poly(styrene-*co*-vinylpyrrolidone) NPs are excellent matrices for simple preparation of optical nanosensors.²⁷⁵ They are uncharged, have an average diameter of ~ 245 nm, are stable even in complex media such as those used in biotechnology, and do not aggregate at high ionic strength. These NPs possess two sites for probe immobilization, viz. a hydrophobic polystyrene core and a hydrophilic shell consisting of poly(vinyl pyrrolidone).⁴⁸³ Hydrophobic probes prefer the hydrophobic polystyrene core, while hydrophilic probes prefer the shell. Borisov et al.²²⁷ incorporated the OSPs PtTFPP, PdTFPP, Ru(dpp) and Ir(III) coumarin complexes in this host. The resulting nanosensors displayed high sensitivity to oxygen and very fast response, especially for nanosensors based on PtTFPP and the Ir(III) complex which is particularly bright.

Polymer NPs also can be prepared via polymerization of monomers. The technique for polymerizing styrene is quite established, and the size of resulting PS NPs can be adjusted via the experimental conditions during polymerization. In addition, the charge of the surface can be governed and chemical functions can easily be introduced. Cywinski et al.⁴⁸⁴ synthesized 20-nm sized NPs for encapsulating PtTFPP (possessing red luminescence) and a perylene reference dye (with green fluorescence) via microemulsion polymerization of styrene. The resulting NPs respond quickly and sensitively and can be used for ratiometric sensing of oxygen in cell culture media. Monodisperse PS beads loaded with the probe PtOEP and a reference dye were synthesized using dispersion polymerization.^{485, 486} The PS beads were monodisperse with very uniform size, and the size was controlled by adjusting the concentration of initiator or steric stabilizer. Loaded with PtOEP, the particles exhibit high sensitivity to oxygen, while the fluorescence of the reference dye is not quenched by oxygen. Because of the hydrophobic nature of dyes and polymer, both dyes are firmly encapsulated in the beads, which enable both ratiometric and colorimetric readout. However, such beads cannot be directly used in aqueous media.

Kopelman et al.⁴⁸⁷ introduced on spherical optical nanosensors (called PEBBLEs) of 20 – 200 nm in diameter. Polyacrylamide NPs were stained with hydrophilic fluorescent probes. Such PEBBLEs are biocompatible, and the probes are well protected from potential interferents as present in the cytosol of cells. However, some probe leakage in aqueous samples was observed. The hydrophobic probe PtOEPK and the reference dye OEP also were doped into emulsion polymerized poly(decyl methacrylate) NPs with a diameter of about 150 – 250 nm.⁴⁸⁸ The nanosensors thus obtained are more hydrophobic, have good stability and probes do not leach. The same group⁴⁸⁹ later prepared polyacrylamide hydrogel NPs by a microemulsion polymerization to encapsulate the NIR-probe PdTPTBP (a dendrimer) along with reference dye. Hydrophilicity, surface charge and oxygen permeability were controlled by using monomers with different functional groups to form

copolymers. The dyes were covalently bound to the polymer so that enhanced loading was possible, whilst leaching was eliminated. The NPs have a size of 30 nm and functional groups on their surface. This may be used for conjugation to peptides for targeted oxygen level monitoring in live cancer cells. Polyacrylamide NPs also were loaded with Ru(dpp) with a hydrodynamic diameter of 45 nm. The nanoparticles were prepared by radical polymerization of an inverse microemulsion, and the OSP was encapsulated during polymerization.⁴⁹⁰ The NPs were used to image intracellular oxygen. In a related approach, a PtTFPP-bearing a styrene group was copolymerized with 2,2'-*N*-isopropylacrylamide (NIPAM) and acrylic acid to form core-shell nanoparticles with an average size of 45 nm.⁴⁹¹ These nanosensors have biocompatible shells which improve storage stability and make them suitable for intracellular application. In addition, the oxygen probe PtTFPP is chemically attached inside the nanoparticle and evenly distributed. Its response to dissolved oxygen was investigated and showed that dynamic range of phosphorescence lifetime to be improved (up to 44 μ s). The extended dynamic range also warrants better sensitivity.

OSPs also have been linked to biological macromolecules to obtain oxygen nanosensors. Johnson et al.²⁹¹ and Papkovsky et al.^{288, 289} physically attached several water-soluble metalloporphyrins (referred to as PtCP, PdCP, PtCPK and PdCPK) to albumin so to form a probe-albumin complex for monitoring oxygen in microvascular vessels in a rat muscle. The results proved that such "sensor probes" enable rapid collection of oxygen concentration data in the microcirculatory system and can assist in the understanding of relationships between oxygen tension, metabolism and blood flow regulation. However, the probe-albumin complex is not very stable in that the probe can dissociate from the albumin. To overcome this limitation, the probes PtCP and PdCP were modified with isothiocyanate (NCS) groups and then covalently linked to the amino groups of albumin proteins.^{492, 493} The Rosenzweig group introduced^{215, 494} nanosized lipobeads with encapsulated ruthenium probes as another kind of nanosensors for oxygen. The lipobeads consisted of a polymer particle coated with a phospholipid membrane. Lipophilic OSPs were then immobilized in the hydrophobic regions of the membrane. Such lipobead nanosensors are capable of real-time monitoring of oxygen in tissue and single cells with an excellent signal-to-noise ratio and high sensitivity. Polymeric lipid vesicles (150 nm in diameter) may also serve as a host particle for the probe Ru(phen).⁴⁹⁵

7.5.2. Silica-Based Materials for Nanosensors

Silica-based PEBBLES (100 – 600 nm in diameter) can be prepared¹⁷³ by the Stöber method which is a polycondensation method. Poly(ethylene glycol) monomethyl ether was added to the tetraethoxysilane (TEOS) precursor as a steric stabilizer to reduce cracking and aggregation between particles. The probe Ru(dpp) and a reference dye were immobilized in the nanosensors,

which then were delivered into rat glioma cells via microinjection. The same group³²⁶ also developed sensors based on an organically modified silica (ormosil) matrix made from phenyl-trimethoxysilane and methyl-trimethoxysilane precursors, and with diameters of ~120 nm. Such nanosensors exhibit good sensitivity to oxygen ($I_0/I_{ox\ satur} > 30$) and linear Stern-Volmer plots. Klimant et al.⁴⁹⁶ encapsulated Ru(dpp) and magnetic nanoparticles in phenyl-substituted ormosil microbeads. The use of magnetic nanoparticles enables the sensing positions to be precisely and remotely controlled using a magnet. This is beneficial with respect to sensing oxygen in bioreactors where homogeneous oxygen distribution is to be warranted.

Present-day methods of surface chemistry enable the net charge, particle size (from a few nm to several μm), pore size and hydrophobicity of silica NPs to be adjusted. OSPs may be covalently immobilized inside pores⁴⁹⁷ or on the outer surface of particles.⁴⁹⁸ The OSP pyrenebutyric acid was covalently immobilized in the pores of porous glass beads⁴³ to obtain a sensor with fast response. The probe PtTCPP was covalently conjugated⁴⁹⁷ into the nanopores of mesoporous silica NPs with diameters of 70 – 100 nm. McShane et al.⁴⁹⁸ chemically linked the probe PtTCPP and NIR quantum dots on the surface of ~ 10 μm silica microparticles and used these for ratiometric oxygen sensing.

Micro-sized silica gels have a porous structure comparable to that of controlled porous glass. They have been exploited in nanomaterials to immobilize OSPs. Acosta et al.⁴⁹⁹ absorbed Ru(dpp) and the reference dye Nile red in ~10-nm silica gel NPs, and then coated them with PDMS to prevent dye leaching. The resulting micro-sized oxygen sensors can be suspended in optically transparent biomaterial and enabled ratiometric determination of oxygen in culture media. However, microscope images revealed that the OSP and reference dye were not uniformly distributed inside the microparticles. Thus, the spatial resolution of the sensor is moderate. It shall be remembered here that most sensors based on silica-type of materials are cross-sensitive to humidity. In fact, this was exploited to design a sensor for humidity.⁵⁰⁰

8. Additives, Coatings, and Other Components

In order to improve and enhance the performance of oxygen sensitive materials (OSMs), various kinds of additives have been developed and applied. These include (a) plasticizers, (b) photostabilizers that reduce the rate of photodegradation of the OSPs, (c) optical isolations that reduce or eliminate interference by ambient light, (d) scattering particles that give rise to more homogeneous excitation and emission light fields, and (e) various other additives to enhance signals, sensing performance, or mechanical integrity. Antifouling polymers containing phosphorylcholine (PC)-substituted methacrylate units have been reported⁵⁰¹ were obtained by

copolymerization of the PC-methacrylates with dodecyl methacrylate and used to coat luminescent oxygen sensors. Nanometer-sized coatings of such materials can reduce the adhesion of marine bacteria by more than 70%, and of thrombocytes by more than 90% to the surface silicone sensor layers doped with Ru(dpp). The PC-coated and the uncoated sensor films perform very well in aqueous media and are mechanically stable for more than one year of continuous immersion. If blood clotting is to be prevented, sensors typically are coated with a thin layer containing covalently bound heparin.

8.1. Plasticizers

Plasticizers are added to polymers in order to improve the efficiency of quenching by oxygen and to facilitate the handling of brittle polymers. Polystyrene, ethyl cellulose, polysiloxanes, poly(meth)acrylamides and polyurethanes are rarely softened by addition of plasticizers. Rather, they are intrinsically plasticized by using monomers that possess long-chain alkyl and (ideally) bulky substituents that prevent pseudo-crystalline or liquid crystal kind of domains to be formed. that would retard diffusion of oxygen. Poly(vinyl chloride) and several other brittle polymers are almost always plasticized by addition of viscous and hydrophobic materials such as long-chain alkyl phthalates, phosphates, sebacates, or phosphine oxides. Nitrophenyloctyl ether (which can act as a quencher unfortunately) and *o*-cyanophenyloctyl ether also have been used. If plasticizers can be avoided, this is recommended because they tend to leach which has two major consequences: The first relates to the response function which will change as a result of leaching. The second is related to the approval of oxygen sensor instrumentation for *in-vivo* use which is unlikely to be granted if (potentially toxic) plasticizers cannot be prevented from leaching into a sample matrix such as blood. Mills⁴⁰³ has performed a study on the effect of the viscosity of plasticizers (mainly triethyl phosphate) on the sensitivity of Ru(bpy)-dyed oxygen sensor films made from either cellulose acetate butyrate or poly(methyl methacrylate). The Stern–Volmer constant is found to be inversely dependent upon the viscosity of the quenching medium, although the natural lifetime of the electronically excited state of the OSP is largely independent of medium.

8.2. Scattering particles

The addition of scattering particles to sensing films can much improve the uniformity of excitation and emission light fields. The addition of SiO₂, TiO₂ or BaSO₄ particles, for example, enables a more efficient excitation of the OSP due to multiple scattering of the excitation light in the sensor material layer and can improve the mechanical stability of the respective sensor films. Klimant et al.⁴⁹⁶ reported on the use of TiO₂ nanoparticles as scattering centers in planar sensors based on magnetic oxygen-sensitive microbeads. The addition of the black magnetic particles causes an inner

filter effect and absorption of luminescence. The addition of scattering TiO_2 particles results, however, in better excitation of the OSP and in enhanced signals. The use of white cellulose powder may also improve light scattering and signal collection.⁵⁰² Ricketts and Douglas³¹¹ constructed a colorimetric oxygen sensor using a green LED that gives a background signal. The LED was covered with an ethyl cellulose sensor film whose red emission (originating from PtOEP) serves as the oxygen-sensitive signal. Scattering agents such as TiO_2 or ZnO were added to the sensing matrix to produce spatially uniform luminescence. Microporous light-scattering supports also have been used.⁵⁰³ Noble-metal nanoparticles have strong surface plasmon resonance absorption, and silver nanoparticles have been suggested³⁴⁵ as additives to luminescent Langmuir-Blodgett films containing the probe PtTPP where they enhanced luminescence intensity by a factor of 10, however at the expense of quenchability by oxygen. Practically all sensors containing fillers display non-linear SVPs because the probes located near the particles are less amenable to quenching than probes located in the bulk polymer.

8.3. Photostabilizers

The photo-degradation of OSPs in most cases is due to the formation of singlet oxygen ($^1\Delta$) that is produced from ground state (triplet; $^3\Sigma$) oxygen in the quenching process.¹⁷⁴ The production of singlet oxygen ($^1\Delta_g$) by ruthenium(II) complexes in microheterogeneous systems was studied in some detail.⁵⁰⁴ Similarly, the formation of singlet oxygen by three kinds of poly(ethylene glycol)-coated palladium(II) tetrabenzoporphyrins ("Oxyphors"; a widely used group of dendritic oxygen nanosensors) was investigated.⁵⁰⁵ It was found that an increasing size of the dendrimer has practically no effect on singlet oxygen sensitization efficiency in spite of the strong attenuation of the triplet quenching rate with an increase in size. While generating singlet oxygen, the dendritic probes are non-phototoxic which is in contrast to the commonly used photodynamic drug PhotofrinTM. The lack of phototoxicity is presumably due to the inability of PEGylated probes to associate with cell surfaces and/or penetrate cellular membranes. In contrast, conventional photosensitizers bind to cell components and act by generating singlet oxygen inside, or in the immediate vicinity of cellular organelles.

Singlet oxygen can react with OSPs to give non-luminescent products. It can also attack polymer backbones. Photodecomposition is particularly efficient under strong UV radiation and when powerful lasers are used as light sources. It can be reduced by applying pulsed light excitation or low radiant powers. Davidson et al.⁵⁰⁶ found that olefinic systems having tertiary amino-substituent groups are very stable towards oxidation by $^1\text{O}_2$. They have reported that the tertiary amino group effectively quenches $^1\text{O}_2$ and protects olefinic systems from oxidation. The addition of compounds bearing tertiary amino-group to the hosting materials was suggested to prevent OSPs from being

oxidized by $^1\text{O}_2$. Other donors that can quench $^1\text{O}_2$ include 1,4-diazabicyclo-[2.2.2]octane (DABCO),^{311,507} other tertiary amines,^{506,508} certain sulfur compounds,⁵⁰⁹ carotene,⁵¹⁰ allylurea and azides.^{511,512} In a systematic study on the stability of OSP towards oxidation by singlet oxygen,⁵¹³ singlet oxygen was produced in situ via a red light-excitable metalloporphyrin sensitizer, and the degradation of the OPSs was studied via UV-Vis spectroscopy. Electron paramagnetic resonance also was applied to monitor singlet oxygen. Practically all dyes faded away in the presence of singlet oxygen.

8.4. Optical Isolations

In order to eliminate interferences caused by (a) ambient light, (b) straylight from light sources, (c) sample fluorescence, and (d) changing sample refractive index (which affects the numerical aperture of an optical waveguide), a non-transparent optical isolation layer can be applied when aiming for high-performance optical sensors (see **Figure 1**). Such an optical isolation is expected to be impermeable to exciting light, but permeable to the analyte and to possess good adhesion to the sensing layer (unless the sensor layer is directly blackened). Optical isolations can cause an increase in response time by increasing the diffusion path length of oxygen from the sample into the sensing layer. Most commercial optical sensors for oxygen contain optical isolations.

Kroneis and Marsoner¹²⁰ used silicone rubber pigmented with (black) Fe_3O_4 for optical isolation and constructed a long-term stable optical oxygen sensor for monitoring oxygen in bioreactors. A thin cover layer (ca. 20 μm thick) composed of red (ferric oxide-pigmented) silicone may also be used.^{50,514} Klimant and Wolfbeis¹⁷⁵ tested various types of other potentially useful optical isolations. The first was a layer of silicone rubber blackened with carbon black and deposited in 10- μm thickness on the sensor. It has the advantages of excellent adhesion and oxygen permeability, does not affect the sensitivity, but the signal intensity dropped by some 15%. The second was a black 12- μm teflon membrane, uniformly spread over the sensing layer. Compared to pure silicone matrix, it shows distinctly lower oxygen permeability. The third was white titanium dioxide (TiO_2) powder dispersed into the silicone matrix. It turned out that the white particles not only act as an optical isolation but also as scattering centers, thereby improving the excitation efficiency and the strength of the signal (fluorescence). The TiO_2 particle may be replaced by barium sulfate.

Klimant et al.⁵⁴ coated the tip of a fiber optic sensor for oxygen with a layer of black silicone to avoid interferences from ambient light, and to make the signal independent of background fluorescence from marine sediments and biofilms (e.g. from chlorophyll). Especially in natural systems with a high density of biomass, the optical signal can decrease a lot if an uncoated sensor tip enters a marine mat. The black silicone coating also acts as a barrier to potential quenchers such as heavy metal ions. There are also reports on the use of black layers of commercial charcoal¹⁹² or

carbon black⁵¹⁵ as an optical isolation. The features of various (including white) materials have been discussed.¹⁷⁵

Contributions by straylight to the overall signal can be eliminated mathematically. The apparent (total) signal I' can be considered as being composed of I (the true fluorescence at a given pO_2) and straylight (I_x). A fairly simple method has been worked out to precisely determine K_{sv} and I from three sets of intensity data.¹⁴¹

8.5. Materials Acting as Inert Solid Supports

Solid supports (see **Figure 1**) are used to facilitate the handling of the rather thin (0.5 to 10 μm) sensing by depositing them on their surface. Supports are expected to be impermeable to oxygen, and also to be optically transparent at the wavelength of interrogation unless the sensor material is illuminated from top. In case of imaging the oxygenation of skin, the oxygen-impermeable support forms the upper layer that also prevents air to enter the sensor layer placed on skin.

Most initial optical sensors for oxygen were of the planar sensor type and prepared by depositing the sensor chemistry on quartz, on other high-quality glass, or on poly(methyl methacrylate) (known as "plexiglass"). Films of poly(ethylene terephthalate) (Mylar™), typically in a thickness of 100 – 200 μm , were later found to be better suited⁵¹⁴ in view of the ease of mass fabrication of sensor spots by simply punching them out. This material also is optically well transparent, flexible, cheap, inert, and oxygen-blocking, and thus has been widely used thereafter.^{100, 175, 192, 209, 515, 516} Care has to be taken not to use materials that exhibit intrinsic and usually shortwave fluorescence that may interfere with the luminescence of the sensor chemistry. Care also has to be taken not to use solvents (for sensor cocktails) that dissolve the solid support. Other, and less common supports, include anodized alumina and the various materials used in objects and models investigated in wind tunnels to measure oxygen partial pressure. This is described in more detail in the Supporting Information.

9. Spectroscopies and Readout Schemes in Luminescent Sensors

Luminescence spectroscopy knows numerous methods that can be exploited for purposes of sensing. All have found applications, and this has resulted in quite a number of read-out schemes that shall be discussed in the following.

9.1. Sensing Based on the Measurement of Luminescence Intensity


The ratio between luminescence intensity (F) and the concentration of a fluorophore is well described by Parker's law. In its most simple version – that is valid for absorbances of $>0.05 \text{ M}^{-1} \text{ cm}^{-1}$ only – it is stating that F is directly related to the intensity of the light source (I), the molar absorbance of the probe (ϵ), its concentration (c), the penetration length (l), and the quantum yield (QY) of the probe (Φ) in the following way:

$$F = I \cdot \epsilon \cdot c \cdot l \cdot QY \cdot k$$

The geometrical factor k accounts for effects caused by the instrumental arrangement. The product of ϵ and QY is sometimes termed brightness (B_s) and represents an important and practical parameter as it indicates how much of the incident light is absorbed and then converted into luminescence. The relationship between quencher concentration and fluorescence intensity is given by the Stern-Volmer law and its various modifications as outlined in **Section 5**.

Measurement of luminescence intensity may be combined with time-resolution if the OSPs possesses a comparably long decay times, typically $> 1 \mu\text{s}$. Time-resolved ("gated") fluorometry enables background fluorescence (with decay times less than $1/10$ of the decay time of the OSP) to be suppressed. In this scheme, luminescence is excited with a short pulse of light, but rather than detecting luminescence immediately after the light source has been turned off, it is detected only after certain time interval during which the short-lived intrinsic fluorescence has decayed. **Figure 19** shows a schematic of sensing based on time resolved fluorometry.

Figure 19. Time resolved fluorometry. Following an excitation pulse (during which luminescence rises to a maximum), the photodetector is opened only after a certain delay time during which background luminescence (yellow) is allowed to decay. The luminescence of the oxygen probe, in contrast, decays much slower (red) and can be detected after the delay time at virtually zero background. The method does not compensate, however, for constant levels of ambient light or long-lived background luminescence.

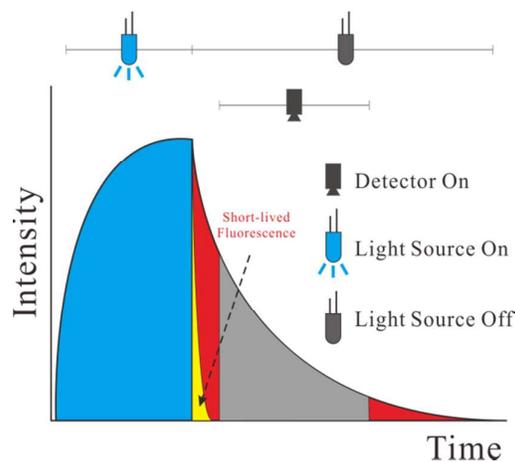

9.2. Sensing Based on the Measurement of Luminescence Decay Time

Luminescence lifetime is an intrinsically referenced parameter of a luminophore. It is independent of probe concentration, photobleaching (to a wide extent), drifts in source intensity, detector sensitivity, and inner filter effects, all of which are major limitations of intensity-based sensors. Finally, the effects of fiber bending remain small. It is obvious that this kind of sensor has considerable stability advantages over sensors based on measurement of intensity.

Fluorescence lifetime can be measured in either the time-domain or the frequency-domain mode (**Figure 20**). In frequency-domain fluorometry, the lifetime is determined via the phase shift between the phase angle of the luminescence and that of the sinusoidally modulated excitation light. If long-lived (metal-organic) excited-state luminophores are used, modulation frequencies are comfortably low (1 – 10 kHz) and instrumentation is small. Time-domain fluorometry often uses time-correlated single-photon counting techniques to record the luminescence decay profile, and the decay curve is analyzed in terms of one or more decay times.

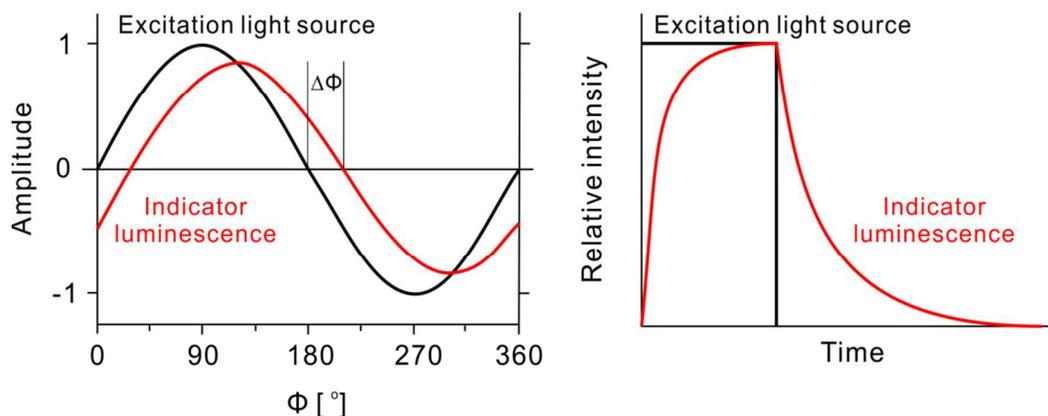


Figure 20. *Left:* The principle of phase fluorometry. Luminescence is photoexcited with sinusoidally modulated light (black trace), and the luminescence of the indicator probe (red trace) is phase shifted as a function of oxygen by an angle of $\Delta\Phi$. The phase shift can be related to pO_2 . *Right:* Photoluminescence is excited with a short pulse of light (black trace) upon which it rises to a constant (steady-state) value (red trace). Once the light source is turned off, the indicator luminescence decays as a function of oxygen particle pressure.

9.2.1. Frequency Domain Fluorometry

In frequency-domain fluorometry, the probe is excited by sinusoidally modulated light (see **Figure 20** left), and luminescence intensity therefore also is sinusoidally modulated, but phase shifted. The phase shift (ϕ), in case of a single-exponential decay, is related to the modulation frequency (f) and to the lifetime (τ) as follows:

$$\tan \phi = 2 \pi f \tau \quad (\text{eq 9.1})$$

The modulation frequency (f) is kept constant so that the tangent of the phase shift is directly related to the decay time, which in turn is related to the oxygen concentration via the Stern-Volmer equation. The selection of the proper modulation frequency is critical with respect to precision and sensitivity. The optimal modulation frequency in some cases is different from the theoretically calculated frequencies.^{517, 518}

Long lifetime OSPs require less complicated instruments for the determination lifetime. The first lifetime-based oxygen sensor⁵⁰ was based on phase fluorometry. The probe Ru(bpy) was absorbed on a silica gel and then immobilized in silicone rubber to construct a sensor film. A frequency-

modulated blue LED served as the excitation light source. The system was later miniaturized and eventually led to a portable device. Quite similar systems were reported recently.⁵¹⁹ The group of MacCraith^{517, 520} developed similar systems using sol-gel based sensor chemistries. Two lifetime-based sensor arrays for multi-site fiber optic measurements were reported by the groups of Holst⁵²¹ and Klimant³¹⁷ and used to determine oxygen in biofilms and aquatic sediments. A solid state electroluminescent lamp (ELL) with a peak emission at 454 nm represents an inexpensive intensity-modulated excitation light sources for phase fluorometric sensing of oxygen.⁵²² Planar surface ELLs can be produced in various shapes and in large sizes. Accordingly, the overall optical output power emitted by ELLs is much higher than that of blue LEDs. For a sinusoidal driving voltage at a frequency f , the ELL output light is modulated at $2f$ and at harmonics of $2f$. Because of this nonlinear modulation characteristics, a square wave driving signal can be applied and results in a pulsed light output at a repetition rate twice the square wave frequency. The shortest light pulses have a typical half width of 1 μ s and this cover practically all OSP except for the PAHs. However, the high driving voltage requires effective shielding to avoid electromagnetic crosstalk between the light source and the photodetector. Also, the optical output power of the ELLs decreases rapidly during the first 100 h of operation.

In addition to sinusoidally modulated excitation, light sources may also be modulated in the shape of a square-wave function. Trettnak et al.⁴⁰⁹ constructed a small sized (120 \times 60 \times 30 mm) sensor module based on the use of LEDs and photodiodes. The oxygen-dependent lifetime was calculated from the phase shift between the square-wave excitation and the quasi-square-wave of the emission of a metalloporphyrin probe.

Phase modulation fluorometry is more prone to interference by autofluorescence than pulse fluorometry. Schmäzlin et al.⁴⁴⁰ noted, for example, that the green and red autofluorescence of green plant cells strongly interferes with the luminescence of the platinum(II) porphyrin OSP. This was overcome by using a multi-frequency phase-modulation technique which enabled the separation of the analytical signal from autofluorescence. The method was applied in later work⁴⁸¹ to sense oxygen in individual gland tubules during hormone-induced secretory activity of a blowfly. Multi-frequency phase modulation also was shown to work in ratiometric oxygen sensing^{368, 369} and imaging.⁵²³

A frequency domain instrument was described⁵²⁴ for real-time measurements of phosphorescence lifetime distributions in microheterogeneous samples. An array of harmonics (typically 100 – 200 frequencies) was used to modulate the excitation source, a light emitting diode. The dependence of the phase/amplitude factor on the modulation frequency was determined by linear least-squares analysis of the multiple decay profiles of emission. The instrument may also be applied to measure phosphorescence in a single-frequency mode. This is useful for rapid evaluation

of apparent luminescence lifetimes. The instruments were tested in Stern–Volmer calibrations of Pd-porphyrin based phosphorescent OSPs and can determine lifetimes in the range of 10 – 3000 μ s. In the single-frequency mode, the measurement time was reduced to about 0.2 – 0.5 s. The instruments provide complete correction for the in-phase signal of up to 40 % of the total emission intensity. Time resolved fluorometry is the preferred method in high-precision oxygen sensor.

Figure 21 shows a commercial lifetime spectrometer that is used as a detector in fiber optic oxygen microsensors.

Figure 21. A commercial lifetime spectrometer as used in a fiber optic oxygen microsensor (Fibox 4). Each fiber sensor linked to this reader has a unique ID and can measure oxygen at levels between 1 ppb and 100 % (in gas or in gas-saturated water). Calibration is performed via a barcode scan, and effects of temperature, pressure and salinity are electronically compensated for. From Presens GmbH (www.presens.de) with permission.




9.2.2. Time domain fluorometry and RLD

A short and narrow light pulse is applied in this method to excite the luminophore (see **Figure 20** right panel). The decay profile of its emission is recorded by time-correlated single-photon counting. In an ideal system, the emission intensity decays mono-exponentially and can be fit by a single-exponential function to obtain the lifetime τ . This is the time during which luminescence intensity drops to 1/e of its initial value. In practice, multi-exponential decays are often obtained and data processing is more complex.¹⁰⁸ The rapid lifetime determination (RLD) method is particularly useful in context with sensing and imaging because usually one does not wish to determine the multiplicity of decays, but rather the effect of oxygen on the apparent decay time. RLD was introduced by Ashworth & Love et al.⁵²⁵ to measure lifetimes in the range of 0.1 – 10 ms. Luminescence decay is integrated over two equal time intervals (A_1 and A_2 in **Figure 22**), and lifetime can be calculated via **equation 9.2**.

$$\tau = \frac{t_2 - t_1}{\ln \frac{A_1}{A_2}} \quad (\text{eq. 6})$$

Figure 22. Schematic presentation of the RLD method. The integrated areas A_1 and A_2 are used to calculate decay time rapidly. Note that short-lived background luminescence (until time t_1) is suppressed.

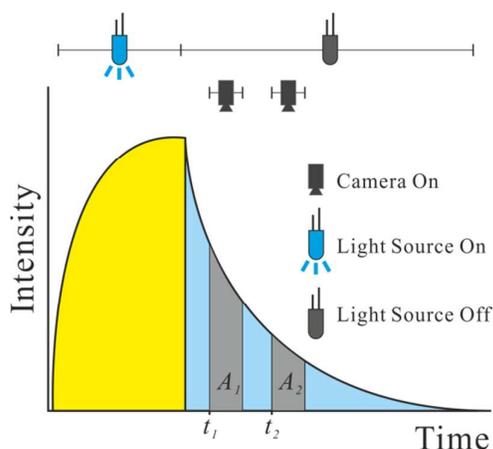


Demas et al.⁵²⁶ evaluated the precision of the RLD method for a single exponential decay as a function of integration time relative to the lifetime and the total photon counts. Their results showed the RLD method to exhibit good precision and accuracy. Its speedy and its simple instrumentation make RLD an excellent tool for data acquisition even under conditions of real-time analysis. On the other hand, it can produce large errors under the certain conditions.⁵²⁷ Unexpected and uncharacteristic Stern-Volmer quenching plots may be obtained for two-component systems. Artifacts include bimodal quenching curves as well as "anti-quenching" curves. These phenomena are further exacerbated in the presence of fractions of unquenched long-lived components. As the RLD method is always combined with gated (time-resolved) detection, it enables short-lived intrinsic fluorescence of samples to be suppressed. This method is particularly useful for purposes of imaging.

9.2.3. Dual Lifetime Determination (DLT)

Optical sensing enables simultaneous sensing of two or more parameters. One important example is the simultaneous determination of oxygen and temperature. Temperature is major source of error in sensors for oxygen because luminescence intensity and its decay time are temperature-dependent. In order to account for this and other effects, the dual lifetime determination (DLT) method³⁸⁸ was developed that is a two-fold rapid lifetime determination (RLD) method (see **Section 9.2.2**). It is capable of rapidly detecting the change in the lifetimes of two luminophores (probes) at the same time. **Figure 23** shows its principle. In this method, the optical signals are not separated via optical filters but rather via the difference in the luminescence decay times of the two indicators. The method is applicable if the decay times of the two probes are different by a factor of at least 10. The resulting lifetimes can be calculated from the respective pair of gates (A_1 and A_2 , A_3 and A_4 , respectively) according to **eq. 6**.

Figure 23. The principle of DLD determination. Following an excitation phase (yellow), the detection gate is opened 4 times to give 4 integrated areas (A_1 to A_4) that can be used to calculate two lifetimes.

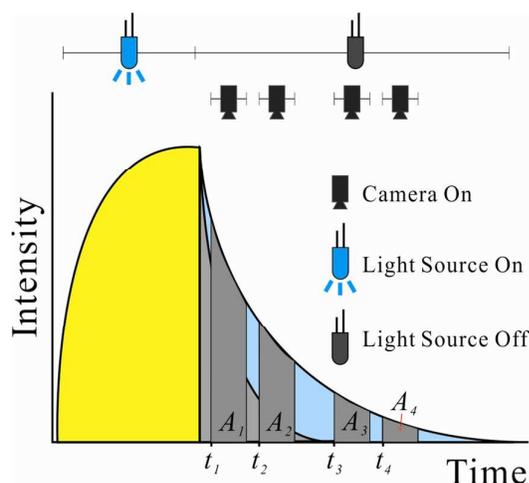

9.3. Sensing Based on Measurement of Luminescence Resonance Energy Transfer

Fluorescence (luminescence) energy transfer (FRET) occurs if two fluorophores with spectral match between the emission of the first (the donor) and the absorption of the second (the acceptor) come in close proximity, typically <10 nm. In this case, photonic energy pumped into the donor is transferred to the acceptor whose luminescence is then observed. FRET systems are widely used in biophysical studies and can serve as molecular bars on a nanoscale. FRET also is one way to enlarge the Stokes' shift and amenable to ratiometric (mostly 2-wavelength) sensing.

Wolfbeis & Sharma^{139, 528} reported on a FRET system where the oxygen quenchable fluorophore pyrene acts as the donor, and the oxygen insensitive fluorophore perylene as the acceptor. If photoexcited at 320 nm, the FRET system gives a strong luminescence at 476 nm. Unlike in many FRET sensors (for pH etc.), in which the acceptor is analyte-sensitive, the donor is analyte-sensitive here. The system strongly responds to oxygen, and the quenching efficiency even exceeds the quenching efficiency of pyrene alone. In fact, a 4-fold increase in the Stern-Volmer quenching constant was observed in the FRET system compared to the quenching of pyrene alone. This led to a strong increase in signal resolution and sensitivity.¹³⁹

Like in other sensors, FRET sensors are preferred that emit longwave light. Bawendi and Nocera et al.⁵²⁹ conjugated oxygen probes of the Os(II) polypyridyl type to quantum dots. The Os(II) complexes have broad absorptions that extend up to 600 nm, and this feature makes them viable acceptors of resonance energy from QDs donors. The QDs display strong two-photon absorption, so that the conjugates can be excited with NIR light. The emission of the QDs is insensitive to oxygen, but that of the Os(II) polypyridyl complexes is quenched. The QDs emission can be used as internal reference to correct for any fluctuations in the photoluminescence intensity. These features make

the two-photon excitable oxygen sensors quite suitable for application in colored or turbid media. However, the quenching efficiency of this conjugate is rather low ($\tau_0/\tau_{100} = 1.45$), and both the Os(II) complexes and the QDs are highly toxic.

Photon upconversion nanoparticles (UCNPs) were used⁵³⁰ to photoexcite the probe Ir(C_S)₂(acac) (see **Section 6.2.2**) to obtain an NIR-excitable oxygen sensor. The use of UCNPs has outstanding features such as (a) excitation at 980 nm which results in zero luminescence background in the visible, (b) deep penetration of excitation light into biomaterials, and (c) no photodamage. The UCNPs are nontoxic and do not suffer from size-dependent emission and blinking. Their emission is not at all quenched by oxygen. Rather, they act as nanolamps for exciting the iridium OSP because its absorption band perfectly matches the blue emission of the NaYF₄:Yb,Tm UCNPs. The green emission of the Ir(II) probe is quenched by oxygen. Thus, an oxygen sensing system is obtained that can be excited using an NIR laser, even though the OSP is not directly excitable in the NIR. This scheme represents one further approach to overcome the lack of NIR-excitable oxygen probes. However, the oxygen quenching sensitivity of the sensor film is moderate. It was also reported that the Stern-Volmer quenching constants are different depending on whether the luminescence of the probe Ir(C_S)₂(acac) was directly excited with blue light or via the up-converting particles. In a related approach,¹⁶⁸ UCNPs of the type NaYF₄:Yb,Tm were coated with Ru(phen)-doped silica. The resulting particles have an average size of around 72 nm, and sharp blue emission peaks at 450 and 474 nm. They were used to photoexcite the Ru(phen) probe in the shell. These nanoparticles have high sensitivity ($I_0/I_{100} = 3.9$) and their hydrophilic surface can be functionalized with reactive groups for further conjugations.

9.4. Sensing Based on Measurement of Fluorescence Anisotropy

Fluorescence anisotropy r is defined as

$$r = \frac{r_0}{1 + \tau / \phi} \quad (\text{eq. 7})$$

where r is the observed anisotropy, r_0 is the intrinsic anisotropy of the probe, τ is the luminescence decay time and ϕ is the so-called rotational time constant. Anisotropy is defined as

$$r = \frac{I_{VV} - I_{VH}}{I_{VV} + 2I_{VH}} \quad (\text{eq. 8})$$

and represents a self-referenced ratiometric parameter resulting in an absolute value for each r value. It offers robust analytical information that is insensitive to photobleaching, migration or varying concentration of fluorophores, and variations in illumination intensity, at least in a first approximation.

Sensing of oxygen via anisotropy is based on the fact that polarization depends on the decay time of the OSP^{107, 108} as can be seen from **eq. 7**. The decay time of the OSPs is reduced by oxygen so that anisotropy can be related to the concentration (or partial pressure) of oxygen. Rao and Lakowicz⁵³¹ showed that the anisotropy of immobilized Ru(dpp) and an inert reference dye, both contained in a stretched film of poly(vinyl alcohol), depend on the local concentration of oxygen. The reference dye has a linear structure, and its emission is highly polarized. The global anisotropy is the weighed sum of the anisotropy contributions of the two emissions. An increase of the fraction resulting from the oxygen sensing luminophore results in decreased anisotropy, and vice versa. As expected, the polarization values displayed large changes, from -0.33 to +0.45 on changing from 0 to 100% oxygen. Since polarization values can be routinely determined to better than ± 0.01 , the accuracy of sensing oxygen is around 1 % or better. The group later reported³⁷⁰ on a sensor based on the changes in the emission polarization of a dual-emitter dye (dppe-Pt2P, see **Table 10**) that exhibits both a short and a long lifetime emission.

Fluorescence polarization also was used to separate the analytical luminescence signal from scattered excitation light.⁵³² Optical signals were separated by cross-polarization, which is simple and wavelength-independent. A stable and sensitive optical oxygen sensor was constructed based on a consumer CMOS image sensor array and polarization signal isolation. The image sensor is inherently color discriminating, while the polarization is a wavelength-independent scheme for filtering excitation light. The combination of the two components generates a compact, multi-color detection system that was applied to point-of-use oxygen sensing based on the quenching of the PtOEP luminophore by oxygen. The method has a high extinction ratio and can separate even weak luminescence from a strong background signal.


9.5. Sensing Based on Two-Photon Excitation

Two-photon excitation (2-PE)^{305, 306, 529} enables OSPs to be excited with long-wavelength (even NIR) light. This is beneficial in terms of biological research because most biomatter has strong absorption and fluorescence at < 500 nm. However, if cross-sections for 2-PE are low, intense lasers are needed that may burn samples. A major benefit of 2-PE in case of phosphorescent probes is the confinement of the triplet state to the immediate vicinity of the laser focus, thereby eliminating oxygen consumption and formation of reactive oxygen species along the excitation path.

The two-photon absorption (2-PA) cross-sections of porphyrins are low, typically in the order of a few Goepfert-Meyer (GM) units (where 1 GM equals 10^{-50} cm⁴ s/photon). In order to increase cross-sections, light-harvesting antennas were used to capture two-photon energy, and the captured energy was transferred to the OSPs via resonance energy transfer. Commonly used

metalloporphyrins exhibit extremely low 2-PA cross-sections. Vinogradov et al.³⁰⁵ designed several water-soluble Pt(II) porphyrin-coumarin based dendrimers, in which the antenna (a coumarin) was coupled to the metalloporphyrin core (**Figure 24**). The resulting metalloporphyrin-antenna construct was further incorporated in a protecting dendritic jacket to isolate the core from interactions with biological macromolecules, to control diffusion of oxygen, and to make the entire sensor water-soluble. The same group⁵³³ also studied photophysical processes of rhodamine antennas in combination with various metalloporphyrins. The probe PtP-C343 was found to possess a high 2-PA coefficient because of the use of C343 coumarin as the antenna. It enabled 2-PE-based imaging of oxygen and blood flow in deep cerebral vessels.³⁰⁹

Figure 24. Mechanisms of the antenna-based two-photon excitation of metalloporphyrins for intracellular sensing of oxygen. (Reprinted from ref.³⁰⁵ with permission from American Chemical Society)

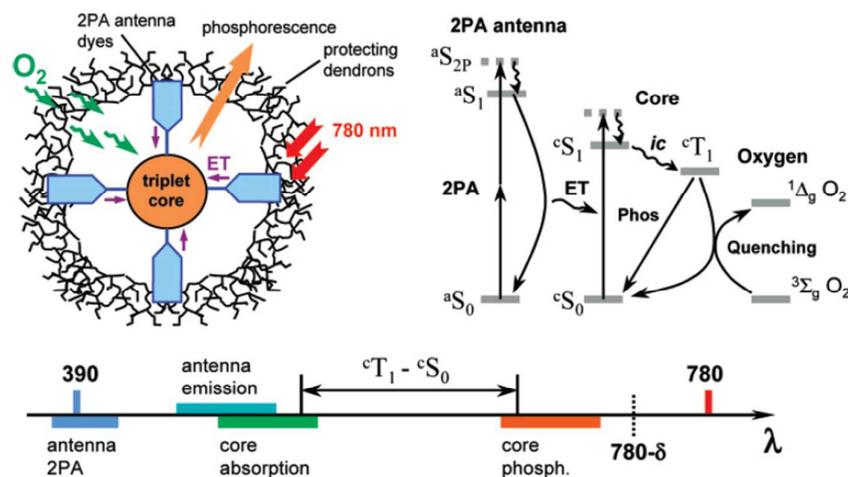

In yet another kind of 2-PE system, Kondrashina et al.⁵³⁴ have used a highly photostable platinum(II)porphyrin along with poly(9,9-dioctylfluorene). The latter acts as a two-photon antenna and as a FRET donor. The Ru(dpp) complex has a 2-PA cross-section (210 GM units) that is much higher than that of porphyrins. Incorporated into polystyrene microparticles, Ru(dpp) was shown¹⁸⁹ to enable 2-PE-based sensing of oxygen (also see **Section 6.2.1**). Quantum dots also possess high brightness and large 2-PA cross-section. They were coupled to Os(II) polypyridyl type oxygen probe to give nanosensors for oxygen.³⁵⁶ The QDs can capture two-photon energy from excitation laser and transfer it to the Os(II) complex. The method enables oxygen being ratiometrically detected via NIR excitation. However, the quenching effect is not satisfied, and both QDs and Os(II) complex are highly toxic.

9.6. Sensing Based on Chemi- and Bioluminescence

Sensors based on measurement of chemiluminescence (CL) or bioluminescence do not require external light sources and optical filters, but chemical reagents that are consumed over time. In addition, oxygen is consumed which is in contrast to quenchemetric sensors. CL methods in sensor

technology (oxygen included) have been reviewed.⁵³⁵ Seitz et al.⁴⁴ reported that the cyclic aminoethylene EIA (which can be easily prepared) reacts with oxygen under emission of chemiluminescence (CL). Tetraaminoethylenes without aromatic functions also react with oxygen to produce CL. Its intensity is directly proportional to the concentration of oxygen. Low levels of CL can be easily measured, and a device has been presented in which the oxygen diffuses through a teflon membrane before reacting with the CL reagent (a 10% hexane solution of 1,1',3,3'-tetraethyl bisimidazoline). Steady state CL intensity is proportional to pO_2 , but response to oxygen decays gradually over a 12-h period because of reagent consumption. The detection limit of oxygen in the gas phase is estimated to be as low as 1 ppm (v/v). An increase in the reaction temperature causes an increase in signal. Response times are in the order of 10 – 20 s.

Another CL-based detection scheme is based on the luminol reaction⁵³⁶ but is not practical. All CL-based method suffers from the disadvantages of (a) storing the reagent under exclusion of oxygen; (b) being interfered by ambient light; (c) poor reversibility, and (d) consumption of oxygen. This makes them applicable to a limited number of applications only.

For bioluminescence (BL) to occur in luminous biospecies, the presence of oxygen is mandatory.⁵³⁷⁻⁵⁴⁰ The intensity of the BL therefore can be unambiguously related to the oxygen concentration. Beijerinck⁵⁴¹ back in 1902 utilized bacterial BL to detect oxygen during photosynthesis with low detection limits. Other studies⁵³⁷ revealed the relationship between the BL intensity of luminous bacteria and fungi and the concentration of oxygen, and between the BL of *P. phosphoreum* and oxygen.⁵³⁸ They resulted in convenient and sensitive methods for quantifying dissolved oxygen with high accuracy at 10^{-6} to 10^{-8} mol/L levels. Williams et al.⁵⁴⁰ used *Photobacterium fischeri* to quantify dissolved oxygen. A suspension of the bacterium was covered with oxygen-permeable membranes (polypropylene or silicone rubber), and BL was detected as a function of pO_2 . The sensor responds quite rapidly (< 8 s), and there is a linear relationship between BL intensity and dissolved oxygen concentration in the range from 35 nmol/L to 8.4 μ mol/L. Response is fully reversible both in the gas and the liquid phase. On the less favorable side, luminous bacteria often require the presence of high salinity, and their own respiration may compromise accuracy. The BL of cells also is sensitive to metabolic inhibitors, and depends on the age of bacteria.

A solid phase reagent (composed of a fluorinated polyalcohol, luminol and ferric sulfate) was reported⁵⁴² to display CL if exposed to a stream of oxygen. It can sense oxygen in moderately low concentration (2.4 ppm in water). In an electrochemiluminescence (ECL) based sensor for oxygen,⁵⁴³ ECL was generated at a disposable CdS-modified screen printed carbon electrodes during cathodic pulse polarization. Two emissions, with peaks located at 520 nm and 580 nm, are found. The intensity of ECL is linearly related to the concentration of dissolved oxygen in the range of 1.7 – 33 mg/L, with a detection limit of 0.02 mg/L. The method was applied to detect the

dissolved oxygen concentration and biochemical oxygen demand.

9.7. Other Luminescent Sensing Schemes for Oxygen

Borisov et al.⁵⁴⁴ have introduced a sensing scheme for oxygen that exploits the oxygen-sensitive anti-Stokes' emission of OSPs. This emission is generated via triplet–triplet annihilation-based upconversion using the probe pair of PtTPTBP and diisobutyl 3,9-perylenedicarboxylate. Porous glass beads carry the “sensing chemistry” that includes a sensitizer, an annihilator, both dissolved in a high boiling solvent. The beads are dispersed in silicone rubber or Teflon and deposited in the form of sensor films. LED light sources are used for excitation, and the upconverted emission is very sensitive to oxygen both in terms of decay time and intensity. The latter follows a quadratic Stern-Volmer relationship which is quite a novel finding. The NIR luminescence of the sensitizer also is quenched but to a much lesser extent. Oxygen can be sensed over a wide dynamic range and at very low levels.

A fluorescence turn-on sensing scheme for dissolved oxygen was introduced⁵⁴⁵ that is based on the use of a perylene diimide dye (PDD) which is electro-chemically reduced to its non-fluorescent dianion form (PDD^{2-}). In the presence of oxygen, the dianion is oxidized to its initial form via an electron transfer reaction with oxygen upon which fluorescence is recovered. As a result, the fluorescence intensity of the dianion in solution increases upon the addition of oxygen gas. High sensitivity is obtained when the emission intensity reaches its maximum by the addition of 2.4% (v/v) oxygen gas. Electrochemical reduction can regenerate this "sensor". The limit of detection is 0.14% of oxygen in argon gas at atmospheric pressure.

A surface plasmon-coupled emission (SPCE) based oxygen sensor was presented.⁵⁴⁶ It is making use of a ruthenium OSP electrostatically attached to a protective layer of SiO_2 above a silver film deposited on a glass slide. SPCE is a highly localized phenomenon occurring when excited fluorophores are within 200 nm of thin, continuous metallic films. The observed SPCE of the probe is highly directional (at an angle of 45.5°) and results in a 27-fold enhancement in intensity over the free space fluorescence. Like in certain evanescent types of arrangements, this so-called Kretschmann configuration allows for an optical filter-free detection of emission. Quenching efficiency is somewhat reduced due to the metallic effects on fluorescence lifetimes but response is very fast. Balushev et al.⁵⁴⁷ have presented first results of ultralow excitation intensity continuous-wave excited up-conversion fluorescence in a Kretschmann SPR geometry. The active system is a blue-emitting polymer matrix of polyfluorene blended with metalated porphyrins such as PtOEP. The up-conversion fluorescence is a consequence of a two-particle triplet–triplet annihilation process near a silver surface and at very low (a few Watt cm^{-2}) laser intensity. The cw luminescence

spectra reveal the fluorescence of the polyfluorene, the fluorescence of PtOEP, and the phosphorescence of PtOEP. A working prototype fiber-optic intensity-based oxygen sensor was also briefly described.

9.8. Multiple Sensing

Optical sensing has the unique feature of enabling multiple (= multi-analyte) sensing and imaging, examples being the simultaneous sensing (or imaging) of temperature and oxygen, or even of three parameters (pH, temperature and oxygen). Multiple sensors have the advantage of gathering substantially more information at a single sensing site. Space is limited in case of fiber optic microsensors, inside cells, and in case of nanoparticle-based sensors. The state of the art in luminescence based multiple chemical sensing and imaging has been reviewed.³⁸⁸ Two main methods have to be differentiated, viz. (a) multiple sensing using single probes, and (b), multiple sensing using more than one probe. They shall be discussed in the following.

9.8.1. Multiple Sensing Using Single Probes

Many probes are affected by two (or more) parameters. Examples for single-probe dual sensing include probes whose color or luminescence intensity is affected by a first parameter (such as pH value), and whose decay time is affected by another (such as oxygen). Dual sensing of pH and oxygen may serve as a typical example.⁵⁴⁸ The green fluorescent pH indicator 1-hydroxypyrene-3,6,8-trisulfonate (HPTS) suffers both pH induced spectral changes and dynamic quenching of fluorescence by oxygen. The ratio of absorbances at a first wavelength and at the isosbestic (reference) wavelength, whose absorbance does not vary with pH, can serve as a signal for pH. The quenching of the intensity or decay time of HPTS, on the other hand, serves as a parameter for calculating pO_2 .

Sodium fluorescein (uranine) is an example for a probe that is affected by both pH and very low levels of oxygen. When adsorbed on silica gel, it has a pH-dependent absorption and displays a phosphorescence intensity and decay time that are strongly quenched by even traces of oxygen. Typical couples of other parameters that may be simultaneously determined by measurement of intensity (I) and lifetime (τ) of a single(!) indicator are the following: NH_3 /oxygen, CO_2 /oxygen, or oxygen/temperature.⁵⁴⁸ Single-probe dual sensing also includes methods where probes are used that have dual emission bands that are differently modulated by two analytes.³⁶⁷

In yet another version, a single probe is placed in a polymer host that has varying permeability for quencher analytes. The simultaneous determination of oxygen and the inhalation narcotic halothane, both of which act as dynamic quenchers of the fluorescence of the OSP decacyclene is a typical example.⁴⁶ In this case, the Stern-Volmer equation (eq. 1) has to be extended⁵⁴⁹ to give eq. 9

which accounts for the contribution of an additional quencher (Q)

$$F_0/F = 1 + {}^oK_{SV}[Q] + {}^oK_{SV}[O_2] \quad (\text{eq. 9})$$

Here, [Q] and [O₂], respectively, are the concentrations of the second quencher and of oxygen, respectively. ${}^oK_{SV}$ and ${}^oK_{SV}$ are the respective Stern-Volmer constants. The equation can be solved if use is made of two sensors (referred to as A and B here) with different sensitivity and different quenching constants (i.e. made from different materials) for the two quenchers. Let sensor A display a total response function ($F_0/F - 1$) termed α , and sensor B display a response function ($F_0/F - 1$) termed β . The Stern-Volmer quenching constants of sensors A and B for oxygen (oK_A and oK_B) and the second quencher (oK_A and oK_B), respectively, have to be obtained first by calibration. The concentration of the oxygen can be calculated then according to

$$[O_2] = (\alpha {}^oK_B - \beta {}^oK_A) / ({}^oK_A \cdot {}^oK_B - {}^oK_A \cdot {}^oK_B) \quad (\text{eq. 10})$$

To obtain [Q], a similar expression can be given (eq. 11):

$$[Q] = (\alpha {}^oK_B - \beta {}^oK_A) / ({}^oK_A \cdot {}^oK_B - {}^oK_A \cdot {}^oK_B) \quad (\text{eq. 11})$$

As a consequence, measurement of fluorescence quenching with two different sensors allows the determination of oxygen and/or the other quencher simply by measuring α and β .

Sometimes, one of the two sensors can be made specific for oxygen (for example by covering it with a thin membrane consisting of polytetrafluoroethylene (PTFE). As a result, the quenching constant for the second quencher (oK_B) becomes zero, and eq. 10 is considerably simplified

$$[Q] = (\alpha {}^oK_B - \beta {}^oK_A) / ({}^oK_A \cdot {}^oK_B) \quad (\text{eq. 12})$$

Simultaneously, eq. 11 can be transformed to give

$$[O_2] = \beta / {}^oK_B \quad (\text{eq. 13})$$

which, of course, is the Stern-Volmer equation again.

The most accurate sensor type consists of two identical sensing membranes, one of which is covered with a membrane that is impermeable to the second quencher (PTFE in case of halothane). In this case the two quenching constants for oxygen (oK_A , and oK_B in eq. 12) become identical, which leads to the final and very simple equation that describes the relation between the two sensor signals and the concentration of the second quencher:

$$[Q] = (\alpha - \beta) / {}^oK_A \quad (\text{eq. 14})$$

9.8.2. Multiple Sensing Using Two or More Luminescent Probes

This kind of multiple sensing is based on the use of two or more optical probes whose signals can be differentiated by either spectral, temporal or means such as polarization. These are widely used and often applied in the form of mixtures of (nano)particles, each kind containing a specific indicator probe. **Figure 25** shows a typical cross section of a planar sensor film on a solid support for sensing two parameters via two kinds of analyte-sensitive microbeads in a binder matrix.

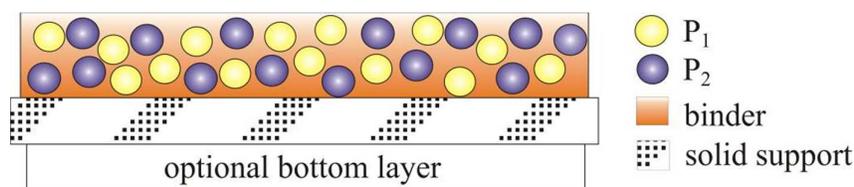


Figure 25. Cross section of a dual optical chemical sensor. The particles (P1, P2) are responsive to the respective analytes and yield the optical information provided their optical emissions can be discriminated (by color, decay time, or the like). The particles are incorporated into a matrix polymer (the binder) whose choice is critical. (Reprinted from ref.³⁸⁸ with permission from The Royal Society of Chemistry)

Numerous kinds of methods for dual sensing of oxygen and a second species have been reported. Examples include oxygen/temperature,^{147, 172, 237, 415, 550-552} oxygen/pH,^{172, 422} oxygen/CO₂ in blood,⁵¹⁴ in fluidic circuits,⁵⁵³ and in aquatic systems,⁵⁵⁴ and oxygen/glucose¹⁶⁴. A triple sensor has been reported⁴⁵ for pH, oxygen and temperature, and a quadruple sensor for simultaneous determination of oxygen, CO₂, pH, and temperature.^{388, 555} Temperature always exerts an effect (see section 10.3.) and often has to be measured in parallel in order to correct the oxygen signal for the effect of temperature. **Table 13** summarizes the state of the art in multiple sensing.

Dual fiber optic microsensors for oxygen and pH, and for oxygen and temperature based on optical fibers were reported¹⁷² that have sensor tips with a diameter of ~140 μm. The sensor chemistries consist of luminescent microbeads that respond to the respective parameters by a change in the decay time, or the intensity of luminescence, or both. The use of microbeads enables the ratio of the signals to be easily varied, reduces the risk of fluorescence resonance energy transfer between indicator dyes, and reduces the adverse (oxidative) effect of singlet oxygen that is generated in the oxygen-sensitive beads. Tian et al.³⁰⁰ have used a PtTPP probe (for oxygen) and a green emitting polymerizable pH probe to obtain a (hydroxyethyl methacrylate)-co-acrylamide copolymer with a dual response. Simultaneous monitoring of oxygen and pH also was accomplished⁵⁵⁶ using a multicolor microcavity organic LEDs as a light source along with small-molecule- or polymer-based detectors with selective spectral response, and a sensor film composed of a structured high molecular weight polystyrene/poly(ethylene glycol) blend.

A dual sensor for oxygen and T is based on a referenced oxygen-sensitive and temperature sensitive paint with color camera read-out and full compensation for effects of T , in one version based on a lipophilic polymer,⁴²¹ in another on a water-based and sprayable paint.⁵⁵¹ Two iridium(III) complexes were shown to enable dual sensing in that the red emission of the first and the green emission of the second can be directly related to pO₂ and T , respectively.²³⁷ Another method for simultaneous luminescent lifetime-based sensing of T and pO₂ was applied to monitor an enzymatic reaction at varying T .⁵⁵² In this sensing scheme – which was referred to as dual

lifetime determination (DLD; see **Section 9.2.3**) – two lifetimes can be extracted from a complex decay profile. DLD was applied to sense oxygen and temperature independently and to monitor the consumption of oxygen in the glucose oxidase–catalyzed oxidation of glucose at varying temperatures. Other sensor materials for simultaneous imaging of oxygen and T on surfaces are known,^{415, 550} and a T -sensitive europium(III) probe along with PdTFPP was used for simultaneous sensing of T and oxygen.⁴¹⁴

Dual luminescent arrays sensor were also fabricated by inkjet-printing of pressure-sensitive and temperature-sensitive paints.⁵⁵⁷ This dual sensor consists of discrete dot arrays of a PSP and a TSP and has been developed for a precise measurement of barometric pressure on the solid surface of aircraft models. The PSP and TSP luminophores are spatially isolated from each other so that there is no interaction between the two luminophores. This technology enables an optimal solvent and binder to be found for each luminophore. In this study, a solution of PtTFPP in 2-propanol and a solution of ZnS–AgInS₂ (ZAIS) nano-particles in toluene were employed as PSP and TSP solutions, respectively.

In yet another version of a dual sensor for oxygen and T , the probes Eu(tta)₃ and Gd(tta)₃ were placed in an acridone-polystyrene matrix to form ultra-thin (250 nm) sensing layers.²⁵⁷ The acridone in the polymer acts as antenna to capture excitation energy which is then transferred to the luminescent lanthanide complex. The luminescence of an Eu(tta)₃-doped sensing layer is only slightly affected by oxygen but highly sensitive to T in physiological range (293 – 313 K). The Gd(tta)₃ has long phosphorescence lifetimes (up to 1 ms) that are very sensitive to oxygen.

The rates of enzymatic reactions strongly depend on temperature and pH value, and a triple sensor therefore was reported³⁸⁸ that can sense glucose (via O₂) but also any (undesired) deviations in temperature and local pH value. A cross section of such a sensor is shown in **Figure 26**.

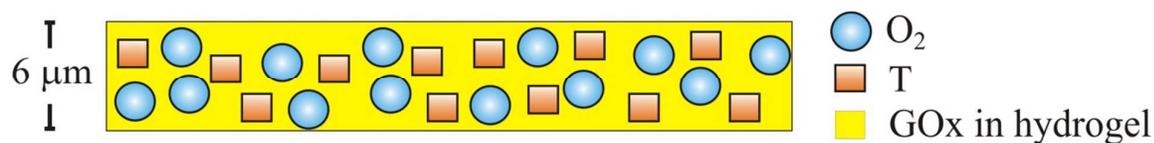


Figure 26. Cross-section of a triple sensor for glucose (via oxygen), temperature and pH. The sensor layer consists of polyurethane hydrogel into which luminescent sensor beads (typically 3 μm in diameter) for temperature (T) and oxygen (O₂) were incorporated along with cross-linked glucose oxidase (GOx). The size of the beads is 3 ± 1 μm. The yellow coloration of the hydrogel matrix symbolizes the presence of GOx that converts glucose into gluconolactone and simultaneously consumes oxygen which is measured. (Reprinted from ref.³⁸⁸ with permission from The Royal Society of Chemistry)

Table 13. Optical sensors that enable oxygen to be sensed along with one or more other parameters

<i>Analytes</i>	<i>Sensor Materials</i>	<i>Sensor Format</i>	<i>Spectroscopy</i>	<i>Remarks</i>	<i>Ref.</i>
O ₂ halothane	Decacyclene in silicone rubber/ polytetrafluoroethylene Decacyclene in silicone rubber	Fiber optics	Intensity	Two sensing films. Film A: decacyclene in silicone rubber for sensing oxygen and halothane; Film B: decacyclene in silicone rubber covered with Teflon; senses oxygen only. Both parameters calculated via equ. 9.8 and 9.9.	46
O ₂ glucose	Ru(dpp) in siloxane coated with polyHEMA hydrogel Ru(dpp) in siloxane coated with polyHEMA hydrogel containing glucose oxidase	Fiber optics	Intensity	Distal end of an imaging fiber (350 μm) deposited with individual sensor materials for oxygen and glucose; sensor maintains the sensitivity for 2 days; detection limit for glucose: 0.6 mM.	164
O ₂ T	PtTFPP in tBS/p-tBS-co-TFEM Ru(phen) in PAN particles	Film	Ratiometric intensity	Spectrally well separated; used in a temperature-compensated pressure sensitive paints.	171
O ₂ T	PdTFPP in PSAN particles Ru(phen) in PAN particles	Film	Lifetime	particles immobilized in hydrogel; signal separated via different lifetimes	415
O ₂ T	Ru(dpp) in sol-gel Magnesium fluoro-germanate in sol-gel	Film	Lifetime	PSP application, temperature compensation; excited with a single LED at 460 nm; time gated technique to temporally separate signals.	558
O ₂ T	PtTFPP in FIB La ₂ O ₃ :Eu ³⁺ phosphor in FIB	Film	Lifetime	PSP application, sprayable sensor; temperature compensation.	559
O ₂ T	PtTFPL in FIB EuD2 in FIB	Film	Lifetime	Sprayable sensor for PSP applications; signals separated via their colors or via time-gating; both probes excited at 400 nm.	271
O ₂ T	PdTFPP in PSAN microbeads Eu complex in poly(4-tert-butyl styrene) microbeads	Film	Lifetime	Sensor particles immobilized in hydrogel; excited at 405 nm; signal separated using optical filters or decay time with certain delay; not influenced by humidity, suitable for PSP, biological and medical applications.	414
O ₂ T	C ₇₀ in ethyl cellulose or ormosils Ru(phen) in PAN	Film	Lifetime	Excited using a single LED at 470 nm; extremely sensitive to oxygen (ppbv range); signal separated either by optical filters or lifetime.	147
O ₂ T	PtTFPP in PSAN microparticles Eu(tta) ₃ (dpbt) in PVC particles	Film	Lifetime	Both particles immobilized in hydrogel to form composite material; excited using a single LED at 405 nm; dual lifetime determination (DLD) used for signal separation and analysis; high spatial resolution	550
O ₂ T	Ir(btpy) ₃ in cellulose acetobutyrate Ir(ppy) ₂ (carbac) in PAN microparticles	Film	Lifetime	Signal separated using optical filters; both probes were excited using a 405-nm LED.	237
O ₂ T	PtTFPP in polystyrene Eu(tta) ₃ (dpbt) in poly(vinyl methylketone)	Film	Lifetime	Two layer approach; oxygen sensitive layer on top of the temperature sensitive layer; excited with a single 405-nm LED; DLD used for signal separation and analysis; used as a transducer for monitoring glucose.	552
O ₂ T	PtTFPP in PS/PVP core/shell nanoparticles Ir(ppy) ₂ (carbac) in PAN microparticles	Particles	Lifetime	Particles dispersed in water, and use as water-sprayable paint; can be washed away easily; both probes excited at 405 nm; signals separated using optical filters.	551
O ₂ T	PtTFPP in PS/PVP core/shell nanoparticles Pt(Br-thq)(acac) in poly(VDC-co-AN) particles	Film	Ratiometric intensity	Particles immobilized in hydrogel; signal separated and recorded using a color CCD digital camera; image data processed using photographing technique.	421
O ₂ T	PtTFPP in silica nanoparticles CdSe QDs in silica nanoparticles	Film	Intensity	Both dyes encapsulated in core/shell silica nanoparticles and excited at 409 nm; the nanoparticles immobilized in ormosil film; signals spectrally separated.	560
O ₂	Ru(dpp) in sensing film (commercial product)	Film	Lifetime	Two layer structure; frequency domain technique used to measure oxygen, time	561

T	Tris(dibenzoylmethane) mono(5-amino-1,10-phenanthroline)europium(III) in PMMA			domain RLD used for temperature; single photodetector; requires fast electronics	
O ₂ pH	Ru(dpp) in ormosil microparticles Carboxyfluorescein covalently attached to polyHEMA microbeads	Film	Lifetime Intensity	Both microparticles immobilized in hydrogel; signal spectrally separated using optical filters; selectivity and sensitivity can be adjusted; few cross-sensitivities	475
O ₂ pH	PtTFPP in hydrogel 2'-Chloro-7'-hexylfluorescein octadecyl ester in hydrogel	Film	Lifetime	pH measured via DLR; signals separated using optical filters; cross-sensitivity to ionic strength is small; used for image pH and oxygen distribution in a marine sediment	554
O ₂ pH	Pt-octaethylporphyrin (PtOEP)-Schiff-base group (SB) and Pd-coproporphyrin-I tetraester (PdCP)-SB in PVC	Film	Emission intensity Absorption	Dual sensing of oxygen and pH based on one probe; absorption intensity for pH sensing; emission intensity or lifetime used for ratiometric oxygen sensing.	331
O ₂ pH	PtTFPP copolymerized with HEMA 4-amino-1,8-naphthalimide based monomer polymerized with HEMA	Film	Ratiometric intensity	Probes copolymerized into planar sensing film to prevent dye leakage; pH-sensitive emission and oxygen-sensitive emission spectrally separated; not cytotoxic	300, 302
O ₂ pH	PtTFPP in polystyrene particles FITC on amino-cellulose particles	Film	Ratiometric intensity	Particles immobilized in hydrogel; signal separated and recorded using a color CCD digital camera; image data processed using photographing technique.	562
O ₂ pH	PtTPTBP in Pluronic-silica nanoparticles FITC in Pluronic-silica nanoparticles	Nano- particles	Ratiometric	ultra-small size (12 nm) nanosensors; PtTPTBP in hydrophobic core, and FITC covalently attached on the surface of the nanoparticles; signals spectrally separated; used for sensing oxygen and pH in cytosol	563
O ₂ pH	PtOEP in a polystyrene/poly(ethylene glycol) blend	Film	Ratiometric	Uses multicolor microcavity OLEDs as a light source, sensor film composed of a polystyrene/poly(ethylene glycol) blend.	556
O ₂ CO ₂	PtTFPP in polystyrene HPTS(TOA) ₃ in Ethyl cellulose particle	Film	Lifetime (frequency domain)	Two-layer structure; CO ₂ -sensitive layer spread on the oxygen sensitive layer; signal separated using optical filters; excited at two wavelengths; CO ₂ measured using dual lifetime referencing method.	553
O ₂ CO ₂	Ru(dpp) in Ethyl Cellulose HPTS(TOA) ₃ in Ethyl Cellulose	Film	Lifetime Intensity	Signal separated using optical filters or gated lifetime; sensor used for intrinsically referenced mapping of CO ₂ and O ₂ in aquatic biofilms	564
O ₂ T pH	PtTFPP or PtTFPL in PSAN microparticles Eu(tta) ₃ (dpbt) in PVC particles HPTS covalently attached to amino-modified polyHEMA microparticles	Film	Lifetime DLD Intensity	First triple sensor; particles immobilized in hydrogel; excited with a 405-nm LED; signal separated using optical filters or lifetime with certain delay.	416
O ₂ CO ₂ T pH	Ir(C ₈) ₂ (acac) in PSAN particles HPTS(TOA) ₃ in EC49 particles Cr-YAB particles SNARF-derivative in hydrogel	Film	Lifetime Intensity Lifetime Intensity	First quadruple sensor; three layer structure, oxygen-sensitive particles and CO ₂ -sensitive particles immobilized at the bottom, temperature-sensitive particle and pH indicator were immobilized on top; the two layers separated by a layer of silicon contain SiO ₂ beads as a scatterer; signals separated via optical filters.	555

9.9. Referenced Sensing and Imaging

Single-wavelength intensity-based luminometry suffer from a number of drawbacks such as drifts of the opto-electronic system (source and detectors), variation in the optical properties of the sample (including probe concentration, leaching, photobleaching, turbidity, coloration and varying refractive index), inner filter effects, interfering ambient light, and background luminescence. In order to (partially) overcome these, referenced analytical techniques have been developed. The following referenced sensing schemes are most common: Two-wavelength ratiometry, luminescence resonance energy transfer, measurement of oxygen-dependent decay time ("lifetime"), dual lifetime referencing, and anisotropy. Some will be discussed in the following, some have been treated in earlier sections.

Two-wavelength referencing is quite common. One method is based on the use of a single OSP possessing two emission bands that are differently quenched by oxygen. In another scheme, the oxygen-dependent luminescence is referenced to a Raman signal that obviously is independent of oxygen. In a third, an OSP is used along with an inert fluorophore. An inert reference fluorophore is not needed in methods based on the measurement of decay time, Raman scattering, or anisotropy. Their merits have been discussed in the respective **Sections 9.2 and 9.4** earlier in this review.

Schaeferling and Duerkop⁵⁶⁵ have surveyed aspects of referenced fluorometric detection schemes. Among those, two-wavelength referencing is about as old as luminescent sensing of oxygen. The signal of the OSP is divided by that of a reference dye, and this simple method can suppress the adverse effects of fluctuations of opto-electronic components (source, detector), effects of varying distance, of bleaching and leaching (provided both dyes do so and at the same rate), and – in case of fiber sensors – effects of fiber bending. However, working at two wavelengths also makes the optical configurations more complicated, and at least two optical filters are required. If the OSP and the reference dye photobleach (or even leach) at a different rate, the method is hardly applicable.

Two-wavelength ratiometric oxygen sensing⁵⁶⁶ is rather simple. Ideally, the two luminophores have the same excitation wavelength but different emission bands. Lübbers et al.⁵⁶⁷ used pyrenebutyric acid as the OSP and an inert fluorescent that gives a constant reference signal. Another way⁴² is to relate more longwave fluorescence to the intensity of blue scattered light originating from the excitation light source. This can compensate for lamp fluctuations and detector sensitivity drifts. Zhang and Seitz⁶⁶ determined the ratio of reflected light (at 405 and 435 nm) of an oxygen-sensitive layer composed of immobilized hemoglobin plus deoxyhemoglobin. One may also use indicators with two luminescence bands, one of which is quenched by oxygen while the other remains unaffected.³⁶⁷ The probe 4-bromo-1-naphthoic acid in a γ -cyclodextrin cavity was linked

to cellulose where it shows oxygen-dependent phosphorescence and oxygen-independent fluorescence. The ratio of luminescence intensities can be measured at two wavelengths and yields a parameter for oxygen pressure. It was also suggested to use the ratio of the intensities of monomer or excimer bands of pyrenes (which are differently affected by oxygen).

Referencing is almost mandatory in case of intensity-based oxygen nanosensors. Kopelman et al.¹⁷³ immobilized Ru(dpp) and the reference dye Oregon Green 488 in PEG-stabilized silica nanoparticles. The fluorescence of Oregon Green is not affected by oxygen. This makes it an ideal reference dye with good spectral match. The resulting ratiometric nanosensors have excellent reversibility and enable real-time monitoring of intracellular oxygen at pH values above 6. The group also reported⁴⁸⁸ on the use of the oxygen-insensitive dye octaethylporphyrin (OEP) and the probe PtOEPK in poly(decyl methacrylate) nanoparticles to obtain plastic oxygen nanosensors. Because of the hydrophobic nature of both dyes, they do not leach and are well protected from non-specific binding to proteins inside the nanoparticles.

OEP is not a good reference dye because it suffers from photobleaching. A combination of PtOEPK and a bodipy dye is better and was used in a ratiometric sub- μm fiber optic oxygen sensor.⁵⁶⁸ Ormosil-based nanoparticles also have been reported³²⁶ containing dye pairs (PtOEP and 3,3'-dioctadecyloxycarbocyanine, or PtOEPK and OEP). Both exhibit high sensitivity to oxygen ($I_0/I_{\text{O}_2 \text{ satur}} > 30$) and linear SVPs over the entire range of water-dissolved oxygen (0 - 43 ppm). However, the reference dyes suffer from photobleaching. The same group later⁴⁸⁹ encapsulated the NIR emitting probe PtTCPTBP and the reference dyes Alexa 647 or Hilyte 680 in hydrophilic nontoxic polyacrylamide nanoparticles. The nanoparticles were further functionalized with peptides for targeted monitoring of oxygen in cancer cells. The use of a NIR probe has the advantage of deeper penetration of light into tissue and generating less autofluorescence. McNeill et al.⁵⁶⁹ doped PtOEP into a luminescent conjugated polymer and prepared luminescent polymer nanoparticles with a diameter of around 25 nm. The blue emission of the conjugated polymers is not quenched by oxygen and serves as a reference, whilst the red phosphorescence of PtOEP is strongly quenched by oxygen.

Gouterman and Khalil et al.^{272, 273} reported on a referenced pressure-sensitive paint which, in fact, is an oxygen-sensitive paint. It is making use of the longwave emitting oxygen probe PtTFPL and a reference dye that has a short lifetime and a fluorescence peaking at 650 nm. The paint was used for ratiometric measurement of oxygen partial pressure in wind tunnels. Tian et al.³⁰² copolymerized the probe PtTFPP containing a polymerizable group with a luminescent monomer to obtain oxygen sensing polymer films possessing two emission bands. The blue luminescence of the conjugated polymer is insensitive to oxygen and can be used as reference signal. Jorge et al.⁵⁷⁰ employed luminescent core/shell quantum dots (QDs) as reference luminophores and Ru(bpy) as

the OSP. The QDs have a wider excitation range and narrower emission spectra. This enables the reference dye and the OSP to be excited with a single excitation source. The narrow emission favors spectral separation, and the color of the emission of the QDs can be tuned via their size.

Other reference dyes include the silica complex of OEP which was used in PS beads,⁴⁸⁵ certain stilbenes,⁴⁸⁶ and a yellow perylene dye in 20-nm PS nanoparticles.⁴⁸⁴ The perylene dyes are probably the most stable reference dyes. Even smaller particles (only ~8 nm in diameter) were obtained⁵⁷¹ by partially exchanging the capping ligand of QDs by a pyrenylimidazole. The resulting nanosensors display emissions from both the QDs and the pyrene derivative. The red emission of the former is insensitive to oxygen and can act as a reference signal, while the blue emission of the pyrene derivative is sensitive to oxygen. However, the hydrophobic nature of capping agents renders these NPs poorly soluble in water, and this may compromise applications in biosystems. McShane et al.⁴⁹⁸ covalently linked PtTCPP and carboxy-modified QDs onto amino-modified silica particles with a diameter of around 10 μm . Again, the NIR emission of the QDs is not quenched by oxygen, but the luminescence of PtTCPP is, and this was used for ratiometric sensing. Unfortunately, almost all authors working with QD-based sensors for oxygen do report on conceivable interferences by other species also known to quench the fluorescence of QDs.

A ratiometric fiber optic oxygen sensor⁵⁷² reported on that is based on a sol-gel matrix doped with two fluorophores. The Pt(II) or Pd(II) complexes of a pentafluorophenylporphyrine acted as the red-emitting OSPs, while the blue-emitting laser dye 7-amino-4-trifluoromethylcoumarin acted as the reference dye. This ratiometric sensor has good sensitivity, a response time of ~3 s, and is fully reversible. Effects of spurious fluctuations in the intensity of the excitation source and optical transmission properties of the optic fiber are eliminated. **Table 14** summarizes and assesses the common spectroscopic methods for readout in sensors for oxygen based on the use of optical probes.

Multiple emitters (see **Section 6.4**) also can be used to construct self-referenced ratiometric oxygen sensors.^{368, 573} These intrinsic ratiometric OSPs normally possess multiple emission bands, and each band has different oxygen response. Sensors based on such OSPs not only compensate for effects of common interferences in two-wavelength referencing, but also for photobleaching. Another ratiometric probe was reported⁵⁷⁴ that may also be used in a sensor, but this has not been demonstrated so far. Schemes for the design of fluorescent ratiometric nanosensors for oxygen (and other species) have been reviewed.⁵⁷⁵

A phosphoroscope with no moving parts was described that enables detection of both fluorescence and phosphorescence which is useful in ratiometric sensing.⁵⁷⁶ The total luminescence, the long-lived phosphorescence, and the short-lived fluorescence can be determined in a single scan. A 50% duty cycle excitation from a diode laser was used to excite the sample. Phosphorescence is extracted from the off period of the digitized waveform, the total emission from

the full cycle, and fluorescence from the on-period corrected for the phosphorescence contribution. The performance of the system was demonstrated by acquiring the RTP spectra of (a) organic dyes in boric acid glasses, (b) a multi-emissive and oxygen-quenchable boron-polymer dye, and (c) a europium chelate.

A patent⁵⁷⁷ describes a smart referenced sensor element that is schematically shown in **Figure 27**. In essence it consists of an LED light source (14) whose emission is reflected (in elements 29 and 31) into two minute prism-shaped waveguides (22 and 27), one being covered with analyte-sensitive chemistry (30), the other not. Attenuated light and fluorescence are guided to another pair of reflectors (28 and 32) and directed to photodiode detectors (16 and 18). This system is simple, widely self-referenced, and can be mass manufactured at low costs from semiconductor and plastic (plexiglass) components. Several other versions also are described.

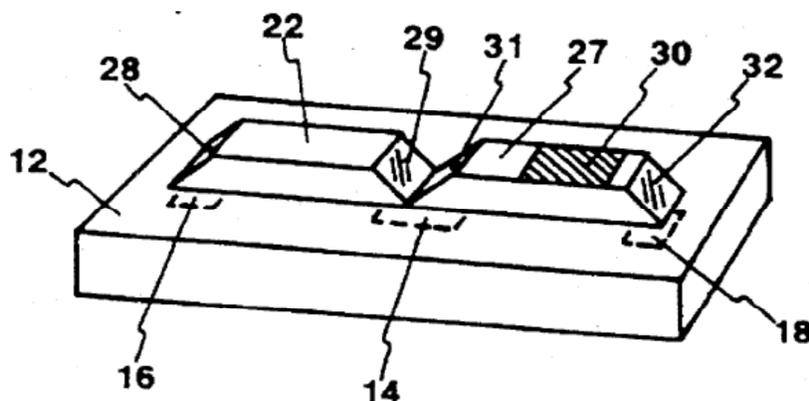


Figure 27. A smart waveguide sensor element for referenced indicator-based chemical sensing. Reprinted from ref.⁵⁷⁷ Light from an LED (14) is directed by reflective end faces 29 and 31 into the two arms (22, 27; one acting as the sensor arm, the other as a reference) and then is reflected again (28, 32) to hit the detector (18) and reference detector (16), respectively. The sensing arm also contains a sensor layer (30) that affects the intensity of light passing it (27).

Table 14. Comparison of spectroscopic methods for readout in sensors based on the use of optical probes

<i>Method</i>	<i>Advantages</i>	<i>Disadvantages</i>	<i>Compensation of interferences by¹</i>								
			Optical Components (e.g. filters, optical gratings)	Instrumental drift (e.g. light source, detector)	Optical misalignment	Background fluorescence from samples	Light scattered by sensor materials	Intrinsic color of samples	Dye leaching and bleaching	Inhomogeneous dye loading	Temperature
Absorption; reflectance	Simple instrumentation; low-cost; portable	Moderate sensitivity; many interferents (such as ambient and background light)	-	-	-	-	-	-	-	-	-
Luminescence intensity	Sensitive; low-cost; portable devices; enables imaging	Interfered by many parameters	-	-	-	-	-	-	-	-	-
Luminescence decay time	Sensitive; precise; self-referenced; enables imaging; 1-point calibration	Relatively expensive; works best in case of OSPs with long lifetime	++	++	++	++	++	++	++	++	-
Anisotropy	Applicable to solution with high viscosity; 1-point calibration	Relatively poor sensitivity and precision; requires OSPs with high anisotropy	+	++	+	-	-	++	++	++	-
Two-wavelength referencing	good precision	Two dyes needed; photodecomposition and leaching of the dyes may be different	-	+	++	-	+	-	-	-	+
Dual lifetime referencing (DLR)	sensitive; precise; enables imaging; simple calibration	Two dyes needed with different excited-state lifetimes; more complex	++	++	++	++	++	++	++	++	+
Fluorescence resonance energy transfer	low-cost instrumentation	Two dyes (donor and acceptor dye) needed that have to be in close proximity; and to spectrally overlap	-	+	-	-	+	-	-	0	-
Luminescent colorimetry	Low cost; visual inspection also possible; good sensitivity and selectivity;	Two dyes needed; semiquantitative in case of visual read-out; influenced by ambient light	0	0	0	-	-	-	-	-	-
Photographing (RGB)	Simple; low-cost; easy of imaging; works best of two dyes are employed	probes emissions have to match the RGB channels of digital cameras	0	+	++	-	+	-	-	-	-

¹ (++) : Efficient compensation; (+) Partial compensation; (-) No compensation; (0) No effect

9.10. Specific Aspects of Luminescent Imaging of Oxygen

This section covers methods for imaging oxygen using either planar sensor films or nanoparticles. The art of fluorescence imaging using chemical sensors (including oxygen sensors) has been reviewed.⁵⁷⁸ The use of molecular probes, though often used, has limitations, the most serious one being the complex interaction of such probes with membranes, cell compartments and proteins. This results in complex quenching constants and uneven distribution if not aggregation of molecular probes. Nanosized sensor particles do not suffer from such limitations in a first approximation.

Peterson and Fitzgerald¹⁶¹ probably were the first to show that quenching by oxygen can be used to visualize the flow of gas blown onto a surface. The OSP Fluorescent Yellow was absorbed on silica gel to form a planar oxygen sensor layer. Streams of oxygen and nitrogen were directed onto the surface of the sensor to result in patterns of different brightness. This approach paved the way to quantitatively imaging oxygen and – indirectly – air pressure, but is sensitive to humidity.

Considerably improved results were obtained when porous polystyrene particles were applied as a support.²⁵⁹ Water vapor and N₂O do not interfere. The response time is <5 ms for 90% of the total signal change, which is distinctly quicker than many other oxygen sensors. Following this initial work, numerous other methods and materials have been reported thereafter. This will be discussed in the following.

Imaging of phosphorescence was introduced²⁶² in 1988 as a novel method for imaging its distribution in perfused tissue. Isolated rat liver was perfused through the portal vein with media containing palladium coproporphyrin whose phosphorescence was used to image the oxygenation of liver at various perfusion rates. Because oxygen is a powerful quenching agent for phosphors, the transition from well-perfused liver to anoxia (no flow of oxygen) resulted in a large increase of phosphorescence intensity. During stepwise restoration of the flow of oxygen, the images showed marked heterogeneous patterns of tissue reoxygenation, which indicated that there were regional inequalities in oxygen delivery. While not using sensors along with lifetime imaging (that would have warranted more precise data that are not affected by probe binding by proteins and by uneven spatial distribution), this method paved the way for sensing oxygen in medicine. Hartmann & Ziegler⁵⁷⁹ reported on an all solid-state method (LED light sources; photodiode detectors) for imaging of oxygen using a sensor foil containing silica particles dyed with the Ru(phen) complex and dispersed in a layer of silicone. The spatial resolution was 1 mm, and the oxygen resolution was between 0.4 and 2.5 Torr depending on the actual pO_2 .

Several instrumental approaches are common at present. The first is based on the use of CCD cameras and works in the intensity mode. The second is in the lifetime mode if the CCD device has an adequately fast response. Both methods also work in combination with microscopy. Advanced

instrumentation is commercially available. A substantial collection of protocols on the use of hand-held optical imagers is available on the internet.⁵⁸⁰


9.10.1. Intensity based Imaging

In principle, all the spectroscopic methods described before may be applied to imaging of oxygen. Intensity based imaging does not require complex devices, and one of its first application was to sense barometric pressure. The probe PtOEP and polydimethylsiloxane were dissolved in toluene, and this cocktail was sprayed onto a model of an aircraft to form a uniform film.²⁶⁴ After drying, the barometric pressure distribution was measured in a wind tunnel by recording the distribution of luminescence intensity using a CCD. However, intensity is strongly affected by inhomogeneous illumination because the intensity of light decays with the square of distance, and this holds, of course, both for the exciting light and emitted light. In fact, this effect is detrimental in case of 3-dimensional objects such as aircrafts or cars. Other, less harmful limitations of intensity-based imaging result from inhomogeneous probe distribution, non-uniform thickness of the sensing film and background light.

A pixel-by-pixel calibration method was developed to overcome these problems and achieve quantitative imaging.⁵⁸¹ Each pixel on the CCD or CMOS chip was treated as an individual oxygen sensor and calibrated *in-situ*. The method enables oxygen imaging with a spatial resolution of 3.0 μm and eliminates the effects of uneven probe distribution and light source distribution. It is mandatory, though, that the sensing film is firmly fixed to prevent major errors caused by pixel movement. The influence of excitation light distribution can be prevented by using cross-aligned polarizers, which led to the design of a compact oxygen sensor without using any optical filters.⁵³² A more simple approach consists in the use of a reference dye to correct for such interferences.²⁷³


Color CCD and CMOS cameras even better serve the purpose of sensing and imaging oxygen via luminescent sensor layers⁵⁸² A read-out scheme by means of digital color camera and the application of a Bayer filter (pixels or layers that are sensitive to different ranges of wavelengths, typically red, green and blue (RGB) is schematically shown in **Figure 28**. Such detectors may be considered as very simple (3-color) spectrophotometers that can be used to separate multi-color sensor signals or referenced signals, the only stipulation being the availability of indicators that emit at different wavelengths.

Figure 28. Scheme of color CCD equipped with red-green-blue optical filters.

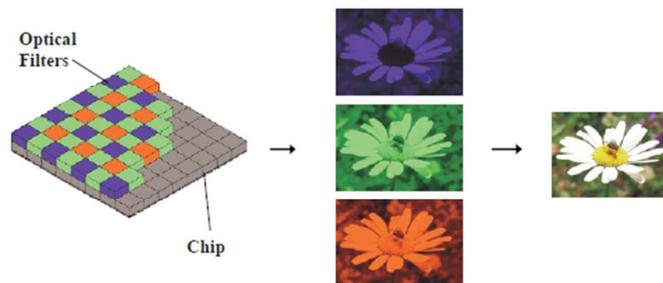

RGB-based detectors have been often explored for imaging of oxygen.^{313, 486, 583-585} If the chosen OSP and the reference dye match the spectral characteristics of RGB filters, the luminescence intensities of the OSP and the reference dye can be recorded in the RGB channels of color pictures and easily referenced using routine software. In a typical example, a ratiometric intensity-based imaging scheme was reported³¹³ where a red-emitting probe and a green fluorescent reference dye (whose luminescences match the red and green optical filters on the color CCD in a digital camera, respectively) were incorporated into a hydrogel matrix. The method enables photographing of the oxygen distribution by taking a picture using a digital camera (**Figure 29**). It was also used to image oxygen-deficiency by taking pictures of a sensory cloth.⁴⁸⁶ By introducing a blue-emitting reference dye, adverse effects of inhomogeneous illumination and non-uniform film thickness can be referenced out, but it is mandatory that the concentrations of probe and reference dye are the same at each data point/pixel.

Figure 29. Imaging of oxygen distribution using planar sensing films and photographic (RGB) readout. The sensing film was first put in nitrogen environment. Exposure to a stream of oxygen causes the luminescence intensity change of the red dye and imaged using the photographic technique. A) Regular photo (14-bit color depth per channel) obtained for colorimetric readout; B) Pseudo color image of the G/R ratio calculated with data of the green channel and the red channel. (Reprinted from ref.³¹³ with permission from Wiley-VCH).

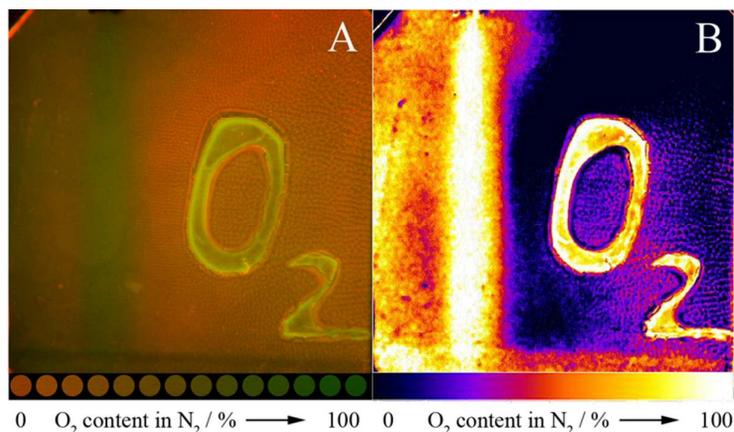

A similar approach has been reported by Park et al. In the first,⁵⁸⁵ a light panel screen with light-emitting diode backlight was used as a light source to excite a sensor film containing PtOEP as the OSP in an ethyl cellulose host polymer. A green LED light uniformly displayed from the light panel

excited the sensor film to exhibit two-dimensional luminescence distribution corresponding to the pressure of gaseous oxygen. A color camera was used as a photodetector for registering oxygen images and analyzing the oxygen contents quantitatively. In the second,⁵⁸⁶ commercial RedEye oxygen sensor patches were applied. Two methods of color intensity analysis are investigated and compared. The first is to analyze the total Red-Green-Blue (RGB) color intensity of the original color image. The second involves extracting the red color element to enhance the sensitivity of oxygen measurement. Results showed the linearity and sensitivity of the red intensity analysis to be improved over those of spectrometric measurement and total color intensity analysis. However, the method do not use a reference dye for ratiometric readout, and the distribution of excitation light and dye, ambient light and background luminescence may compromise the precision of imaging.

Intensity-based imaging of oxygen with a display screen and a color camera was demonstrated⁵⁸⁴ and can give both quantitative and qualitative results. A liquid crystal display (LCD) screen was employed as a light source for photoexcitation, and a color CCD camera as a photodetector for measurement of emission. Small fluidic channels and oxygen sensor films were integrated. A ruthenium-based OSP was used in the sensor films that can be photoexcited with blue light emitted by the LCD screen. The color camera can map the distribution of red fluorescence emission. This combination of ubiquitous LCD and color camera enables a potential capability of uniform illumination and distribution recording over a large area with variable wavelength ranges. Possible niche application areas include multiple-analyte and high throughput analysis over a large-area fluidic network.

The photographic approach was coupled to microscopy to image oxygen distribution in microfluidic devices with integrated optical sensors.⁵⁸³ The same principle led to the development of hand-held compact imaging devices, which are beneficial to fast oxygen imaging *in vivo* (**Figure 30**).⁵⁸⁷⁻⁵⁸⁹ Imaging was shown to possess the same precision and accuracy as the ratiometric intensity-based measurement using a fluorometer.⁵⁹⁰ It was later applied to ratiometric imaging of the oxygenation of mouse skin.⁵⁹¹


Figure 30. A commercial hand-held and portable oxygen imager based on the RGB technique. The imager is linked to a computer (via a USB interface) where calibration functions are used to convert the data into a pseudo-color picture. From Presens GmbH (www.presens.de). It is particularly useful for ratiometric (2-dye) imaging.



9.10.2. Lifetime based Imaging

Fluorescence lifetime-based imaging (FLIM) has many advantages over single-dye intensity-based methods. Background luminescence can be suppressed by making use of long-lived OSPs along with time gating and/or RLD-based methods. Lifetime imaging is not affected by inhomogeneous illumination, leaching, photobleaching, variable probe concentrations, and uneven film thickness. The use of long lifetime OSPs and the utilization of the RLD method (see **Section 9.2.2**) make FILM quite rapid.^{439, 554, 592,359,360,383} **Figure 31** shows the beneficial effect of lifetime-based imaging over intensity-based imaging. The effects of inhomogeneous light illumination, uneven probe distribution, and distance between object and camera can be almost completely suppressed.


Figure 31. In rapid lifetime-based imaging, effects caused by inhomogeneous distribution of excitation light and of probe concentration are suppressed. (A) Luminescence intensity of an oxygen sensor foil which more or less records the inhomogeneity of the light field on illumination with a point source. (B) Uncorrected intensity response of an oxygen sensor in the presence (bottom) and absence (top) of oxygen. (C) Intensity response of the oxygen sensor corrected for the light field using the data of graph A. (D) Time-resolved ("gated") images of the same sensor film showing even signal distribution both under nitrogen and oxygen. (Reprinted from ref.⁴³⁹ with permission from the Society for Applied Spectroscopy)

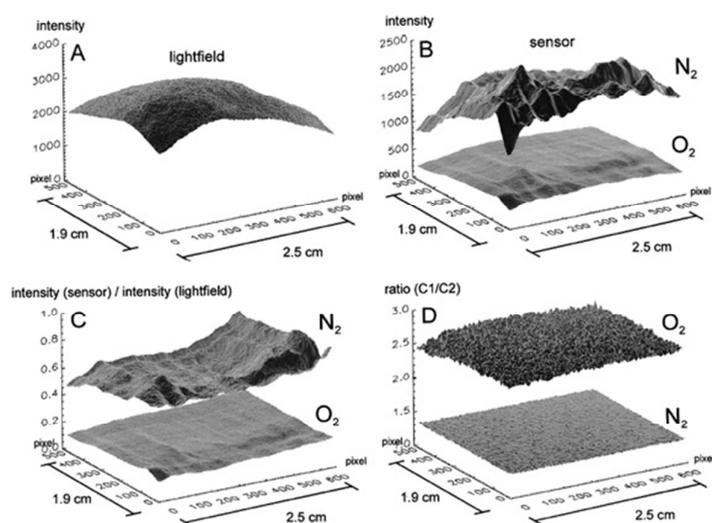

Oxygen imaging based on the RLD method also can be performed with time-gated CCD devices. A simple fluorescence lifetime imaging system using a gated microchannel plate image intensifier coupled to a CCD camera has been developed as early as 1991.⁵⁹³ Nanosecond-level time-resolved fluorescence images of a sample under pulsed light excitation can be detected directly. Coupled to the RLD method for multi-gate detection, fluorescence lifetime imaging can be easily performed. Holst et al.⁵⁹² applied the RLD method to luminescence lifetime imaging using a fast gateable CCD camera. Probes with lifetimes from 1 μ s to 1 s in may be applied in this method. Other features include good contrast enhancement and suppression of background. A hand-held time-gated imaging device for oxygen imaging based on the RLD method (**Figure 32**) was reported later.⁴³⁹ The method takes less than 1 min to acquire oxygen images. A modular luminescence lifetime imager (MOLLI) was presented⁵⁹⁴ that enables both luminescence intensity images and luminescence lifetime images to be acquired. By making use of transparent sensor layers (i.e., films not containing scattering particles or binders), the method was applied to study (a) coral sand

sediment samples (a macrolens application with an resolution of approximately 50 μm per pixel); (b) lichen with cyanobacteria as symbionts (an endoscope application with a resolution of approximately 15 – 62 μm per pixel); and (c) foraminifer with diatoms as symbionts (a microscope application with a resolution of approximately 4 μm per pixel).

Figure 32. Schematic of a CCD array for imaging sensor films ("paints") deposited on the subject of interest.

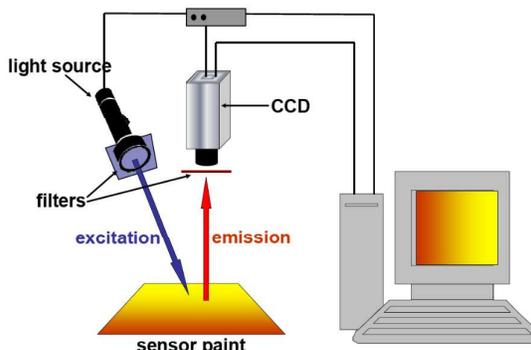

Frequency domain based lifetime imaging can be performed using phase-sensitive CCD cameras. Lakowicz et al.⁵⁹⁵ reported the creation of two-dimensional fluorescence lifetime images based on a sinusoidally modulated image intensifier that is operated as a radio-frequency phase-sensitive CCD camera. By combining the image intensifier with a CCD camera and applying digital image processing, lifetime-selective signal suppression was realized even for fluorophores with comparable lifetimes, such as rhodamine 6G (4 ns) and rhodamine B (1.5 ns). Because the lifetimes of many dyes are sensitive to the chemical environments of the fluorophore, FLIM can reveal the local chemical composition and properties of the molecular environment that surrounds the fluorophore. Thus, the system has the potential use for oxygen imaging. Lo and coworkers⁵⁹⁶ later built a modulation system for the phase-resolved two-dimensional fluorescence phase imaging of oxygen using a sensing film composed of PtTFPP-doped sol-gel. Two-dimensional oxygen distribution imaging was obtained using the modulation system which is suitable to sense gaseous oxygen at levels between 0 and 20 %.

10. Selectivity, Sensitivity, and Effects of Temperature

10.1. Selectivity and Interferences

Molecular triplet oxygen ($^3\Sigma$) is not the only powerful quencher of the luminescence of luminophores. Depending on the kind of emitter, numerous other species can also act as quenchers, albeit to a largely different extent. Examples include elemental chlorine, bromine and iodine, SO_2 and – less so – SO_3 , all NO_x species, brominated and iodinated organic species (including the inhalation narcotic halothane), all nitro compounds, and many olefines and quinones. These species

are electrically neutral and can hardly be excluded from exerting a quenching effect because they (slowly) penetrate polymeric matrices hosting OSPs.

On the other hand, heavy metal ions, bromide and iodide are notorious ionic quenchers, whilst sulfite and thiocyanate have not been well studied but are likely, though weak, interferents. Sulfide can "quench" by undergoing a chemical addition reaction with the fluorophore.⁵⁹⁷ The effect of ionic species can, however, be eliminated by incorporating the OSPs in an ion-impermeable matrix material (such as silicone, polystyrene or ethyl cellulose) as will be described in **Section 7.1**. If hydrophilic matrix materials have to be employed for any reason, ionic quenchers will interfere. Many of the above quenchers do not occur in biological matrices, however.

No (or negligible) interferences are to be expected from gases such noble gases, hydrogen, nitrogen, CO₂ (with limitations as it is a weakly acidic gas), alkanes (gaseous and fluidic), vapors of alcohols (with limitations), ethers, and of chlorinated solvents. Some organic solvents can destroy sensor films, however. All alkali and earth alkaline ions remain inert as do the anions sulfate, nitrate, nitrite, bicarbonate, carbonate, chlorate, acetate and the like. All these species do not enter hydrophobic polymer membranes anyway. Similarly, solutions of main group element ions and all ionic surfactants remain fairly inert. Bioorganic species such as saccharides, lipids and proteins do not act as efficient quenchers. Their quenching constants (K_{sv}) are below 1 M⁻¹. However, tryptophan in proteins can act as an energy acceptor in FRET system if very shortwave absorbing probes are used which is not recommended anyway in optical sensor technology.

Humidity, often referred to as "relative humidity" (RH), interferes in sensors based on surface-adsorbed probes, in particular conventional silica which strongly absorbs water, and with some sol-gels as outlined in **Section 7.3**. Practically all suffer from the presence of water vapor in gaseous samples because RH is a notorious quencher of luminescence. This is, of course, not the case if (water-)dissolved oxygen is to be sensed, but in such cases the luminescence intensity of the sensors can be weak as a result of quenching by adsorbed water. The effect of RH on the response characteristics of luminescent PtOEP-based oxygen sensors has been studied in some detail.⁴⁰¹ If hydrophilic host polymers are replaced by more hydrophobic hosts such as ethyl cellulose, the effects is strongly reduced but not eliminated. Sensors based on host materials such as silicones, polystyrene, or poly(vinyl chloride) are not severely affected. Plasticizers also exert a beneficial effect in reducing the effects of RH. Lifetime data suggested that the effect of RH is due to its effect on oxygen permeability. The use of a silver-octadecanethiol coating along with a reference gas correction algorithm can minimize the effect of RH in fluorescent sensors for oxygen.⁵⁹⁸

10.2. Sensitivity, Precision, and Limits of Detection

Sensitivity is defined as the slope of a calibration plot, in the simplest form as the signal change

(ΔS) divided by the change in concentration (ΔC) of oxygen. However, many authors refer to sensitivity as the lowest detectable concentration of oxygen (or any other analyte). This parameter is defined by IUPAC, however, by the limits of detection (LOD) and of quantification (LOQ). The LOD usually is expressed as the concentration where the analytical signal is 3 times that of the noise, in other words at a signal-to-noise ratio (SNR) of 3.

The analytical range of a luminescence based sensor for oxygen is governed by the shape of the respective quenching plot and the Stern-Volmer constant (which, of course, is the slope of the plot). Most sensors have been adjusted (by proper choice of OSP and polymer) to perform best in the range between 0 to 300 Torr. Phosphorescence-based sensors are much more sensitive than fluorescent sensors by principle (not the least due to much longer decay times), with typical limits of detection as low as 0.004 Torr. Higher quenching constants result in (a) high accuracy at low levels (because of a larger relative signal change per Torr oxygen), and (b) in dynamic ranges not exceeding ~ 200 Torr after which signal changes become vanishingly small. The proper adjustment of a quenching constant always is a compromise between analytical range and accuracy. A bi-label oxygen sensor was reported⁵⁹⁹ where two luminophores were incorporated into a polymeric matrix with the aim to enlarge the analytical range of sensors. The luminophores Pt(II)-TPP, Pd(II)-TFPP and Ru(dpp) octylsulfate in plasticized poly(vinyl chloride) or polysulfone behave as if they were independent. This lifetime-based approach also resulted in improved precision.

The sensitivity ("slope") of all such sensors is highest at the initial part of the curve, i.e., at low oxygen tensions where $\Delta S/\Delta[O_2]$ is maximal and almost linear. At high pO_2 , on the other hand, the slope is small and sensitivity poor. One might therefore assume that luminescent based sensors are most precise in this range. This is largely true. However, even minute experimental errors in the pO_2 at low pO_2 result in large errors in the calibration step.

The *precision and accuracy* of any optical sensor for oxygen are governed by the uncertainties in the determination of F_0 (or τ_0) at zero oxygen, of K_{sv} , and of F or τ at a given pO_2 . As a rule of thumb, the first two govern the precision, and F (τ) values govern accuracy. Precise determination of F or τ obviously is essential for obtaining precise calibration plots and K_{sv} values as needed to establish the Stern-Volmer relationship. F_0 (τ_0) are typically obtained with oxygen-free gases, or with solutions bubbled ("tonometered") with nitrogen or argon, or containing sodium dithionite which completely removes oxygen by reduction. If Stern-Volmer plots are linear, the quenching plot may be established with data obtained with two solutions (or gases) containing lower and higher concentration of oxygen. A final source of error results from contributions of straylight to the fluorescence signal which gives an apparent signal F' composed of F (the true intensity at given pO_2) and the contribution by straylight (I_x). A fairly simple method has been worked out to precisely determine K_{sv} and F_0 from three sets of intensity data.¹⁴¹ Frequency-domain lifetime

fluorometry also is affected by straylight, but time-domain lifetime fluorometry is not.

The *detection limits* of a sensor are governed by both the initial slope of the quenching curve and instrumental resolution. Assuming a $\pm 0.1\%$ uncertainty in light intensity measurement (which is the optimum in a well-thermostatted device), the detection limit is $0.003/K_{sv}$, where K_{sv} is expressed as Torr^{-1} and the signal-to-noise ratio is 3. K_{sv} values ranging from 0.001 to 0.1 Torr^{-1} have been reported for fluorosensors, which results in detection limits from 3 to 0.03 Torr . Phosphorescence based sensors, in contrast, are much more sensitive for the reasons outlined before.

The imprecision of sensors resulting from the signal drift in intensity-based detection was studied more recently⁶⁰⁰ for the case of a polysulfone-based sensor membrane incorporating PtTFPP as the luminescent probe. Photochemical, thermal and oxidative degradation of luminophore and host polymer were examined. The respective contributions were quantified. Oxidative degradation played no role, but thermal and photochemical degradation of the luminophore cause a drift that affects precision independent of whether intensity is measured, or lifetime in the frequency domain or time domain. The design of an intensity-based sensor with high accuracy and precision is suggested. In an extension of this work,⁶⁰¹ an iterative algorithm for drift correction and its experimental verification in intensity-based detection was presented. The signal of a reference oxygen mixture (on air) is needed. The “classical” Stern–Volmer approach is not useful here because it produced a large positive systematic error that increases over time and with increasing fractions of oxygen. The algorithm resulted in accuracy as good as that of phase shift-based commercial sensors.

10.3. Effects of Temperature and Other Parameters

It may be stated that any sensor in this world measures temperature (T) and – ideally – another species too. Unless T itself is to be sensed, its effects are not truly welcome. Remarkably, there are relatively few reports on the T dependence of sensors for oxygen. This may be due to the fact that T exerts rather complex effects on solubility, diffusion and permeability of gases in polymers, on fluorescence QYs and decay times and quenching constants. As a result, mathematical modeling of its effects is complicated. Temperature is probably the single biggest source of error in optical sensors for oxygen. It was stated in one case⁵⁷⁰ that ratiometric (2-wavelength) sensing can widely reduce effects of T , but this probably was an exception. A review on optical probes and sensors for T is available.⁶⁰²

The determination of T coefficients (“tempcos”) of sensors is a complex task. T is known to affect the luminescence QY of the dye (usually with a negative tempco), (b) the quenching constant(s) (with a positive tempco), (c) the solubility of oxygen in the membrane (negative tempco), (d) the diffusion of oxygen into the membrane (positive tempco), and (e), in case of blood

measurement, the oxygen/hemoglobin binding curve (negative tempco). Furthermore, increasing temperatures usually shorten fluorescence lifetimes (τ) and facilitates $S_1 \rightarrow T_1$ and $T_1 \rightarrow S_1$ transitions. All these factors contribute to the "apparent tempco" of a sensor. Most of the reports on the tempco of sensors refer to one of these effects only. Throughout, increased temperature shortens the response time of sensors. Typically, the 37 °C response time is around 2/3 of that of the 22 °C value.

In a study⁶⁰³ on the tempco of the quenching constant of the OSP benzo(g,h,i)perylene in silicone rubber over the 25 to 60 °C range, it was found that K_{sv} increases from 0.0112 to 0.0140 Torr⁻¹, and the slope of a plot of temperature vs. K_{sv} is almost the same as the slope of a plot of oxygen permeability vs. temperature. Peterson et al.⁴² on the other hand, observed a 0.6% decrease in pO_2 indication per 1 °C increase with a dye adsorbed on resin beads. Under nitrogen, the signal was found to be temperature-independent. Bacon & Demas⁴⁹ reported the lifetime of a ruthenium probe to decrease from 5.8 μ s at 0 °C to 3.3 μ s at 60 °C. The fluorescence of surface-adsorbed Ru(bpy) drops by almost -30% on going from 25 to 37 °C, but the quenching constant remains practically unchanged.

For 9,10-diphenylanthracene in poly(dimethyl siloxane), a decrease of ca. -37% in the quenching constant was reported^{122,390} on increasing temperature from 2 to 48 °C. This is a very large effect that can severely compromise the precision of such optical sensors. At constant oxygen level, a temperature change of 1 °C, therefore introduces an error of 4% in oxygen determination when assuming a T -independent fluorescence QY. A study on the effects of viscosity on the quenching of the fluorescence of diphenylanthracene by oxygen in poly(dimethylsiloxane) solvent revealed¹²² a distinct viscosity dependence of fluorescence intensity, but the slope of the SVP is not a function of viscosity, as it was constant for fluids and fully polymerized silicone. It shall also be kept in mind that bimolecular quenching is a complex process that also is affected by parameters such as solvent cage effects in addition to viscosity and temperature.⁶⁰⁴

The fluorescence of silicone membranes doped with pyrenebutyric acid displays an unexpectedly small effect of T (a 20% signal loss only on changing from 20 to 200 °C in air).¹²⁶ The overall quenching constant, in contrast, varies strongly with T . The fiber optic oxygen probe described by Miller et al.⁶⁰⁵ using decacyclene as an OSP displays an error of ± 7 Torr at 100 Torr oxygen, when the temperature used in calculations is 36 rather than 37 °C.

Erythrosine B contained in a sol-gel matrix displays both delayed fluorescence and strong phosphorescence.¹⁵⁶ The two emissions are oppositely dependent on temperature, and this unique behavior was applied for temperature self-compensation within the temperature range from -50 to 200 °C. The effect of T on the luminescence of the oxygen probe tetraphenylporphyrin (without a central metal ion) also is rather high.²⁵⁹

Most metal-ligand and metal organic complexes have a luminescence that strongly depends on T . The sensitivity of a cyclometalated iridium complex to T is -1.1 and -1.4% per $^{\circ}\text{C}$ at vacuum and 1 bar atmospheric pressure, respectively.²³² Such metal complexes are well suited for use in T -sensitive paints (TSPs). For other data see the comments in the Tables on oxygen-sensitive probes (**Section 6.2.4**) and the review by Wang et al.⁶⁰² Given its adverse effect, attempts have been made to measure T simultaneously with oxygen, in particular in context with imaging of oxygen over large areas where T can vary locally. Multiple sensing was discussed in **Section 9.8**.

Optical probes stable enough to enable sensing of oxygen at high-temperatures are rare. Ghosh et al.^{279,280} report on a $\text{Mo}_6\text{Cl}_{12}$ cluster that has a broad absorption at 300–400 nm, an emission between 600 and 900 nm, a long cluster lifetime (>100 μs), and a large Stokes' shift (>300 nm). Its red luminescence is reversibly quenched by oxygen. The cluster can withstand repeated cycling and showed no signs of decomposition to temperatures higher than 600 $^{\circ}\text{C}$. This makes it suitable for monitoring oxygen in power plants and exhaust gases. It can sense oxygen with high resolution (0.1% absolute oxygen concentration change) both in the gas phase and in aqueous solution. Remillard et al.³⁸⁵ noticed that the fluorescence of Cu-ZSM-5 zeolites reversibly changes on cycling between oxidative and reduced atmospheres, and this was exploited to sense oxygen at temperatures as high as 500 $^{\circ}\text{C}$. However, the material has to be regenerated by exposing it to reducing gases, and this limits practical usage. For the effects of T on the diffusion, permeability and solubility of oxygen in polymers, see **Section 7.1** on "Organic Polymers".

The feasibility of sensing oxygen between 25 and 220 $^{\circ}\text{C}$ has been investigated¹²⁶ using a silicone membrane doped with pyrenebutyric acid and attached to the end of a quartz light guide that was exposed to gases of varying temperatures. The fluorescent signal decreases almost linearly on going from 20 to 200 $^{\circ}\text{C}$ under either nitrogen, 10% oxygen, or 100% oxygen, with a total signal change of -18%). However, after being corrected for straylight (which contributes to more than 50% of the signal), the behavior is more complex. Chu et al.⁶⁰⁶ have introduced a method for temperature compensation in the range of 25 and 70 $^{\circ}\text{C}$ by making use of two PtTFPP-based oxygen sensors, and an algorithm was developed that provides an effective means for improving the accuracy of (fiber optic) sensor without an additional temperature sensor.

10.4. Low-Level Oxygen Sensors

The interest in sensors for detecting extremely low levels of oxygen is so high that it deserves an extra section. Low-oxygen situations are encountered in the chemical industry, in the production of gases, in space research, and numerous other and often unexpected fields. Extremely low levels of oxygen in a nitrogen carrier gas were determined by Kautsky back in 1931 by exploiting the quenching of the phosphorescence of surface-adsorbed tryptaflavin by traces of oxygen.^{11, 32}

Eventually, this led to the discovery of the Kautsky effect, i. e. the delay in the production of oxygen by plants following illumination with light. Low levels of oxygen in water (0.06 to $1 \mu\text{g L}^{-1}$) typically are determined via quenching of phosphorescence of organic dyes adsorbed on silica type of supports. Analytical ranges between 0.4 and $400 \mu\text{g L}^{-1}$ can be accomplished with other kinds of supports as shown by the Zakharov group.⁶⁰⁷ The lowest detection limits reported by this group for oxygen in water is 0.5 ng L^{-1} of dissolved oxygen.

The use of long lifetime metalloporphyrins (such as palladium porphyrin with a lifetime of ~ 1 ms) and high gas-permeable matrices (such as fluorinated polymers) will substantially improve the detection limits for gaseous and dissolved oxygen. Many sensors also work in harsh organic solvents where the survival of sensor material becomes critical because polymers may become dissolved or deteriorated by strong acids or bases. Again, the selection of a proper sensing material is critical for sensor design and still represents a challenge. **Table 15** summarizes the current state.

Table 15. Representative optical sensors for trace oxygen. The limits of detection (LODs) are given in ppm (v/v) units; calculated for 1% quenching (I/I_0 or $\tau/\tau_0 = 0.99$), unless otherwise specified.

<i>Probe</i>	<i>Host polymer</i> ^{a)}	<i>LOD</i>	<i>ref.</i>
Acridine orange	Adsorbed on Silochrome S-120, afterglow	0.04	607
Acriflavine	Adsorbed on silica gel	0.25	150
Acriflavine	Silanized silica gel	0.35 ppbv	15
Erythrosine B	Sol-gel silica	14	160
Organic dyes	Trypaflavin, chlorophyll, porphyrins etc adsorbed on silica gel or aluminium oxide gel; oxygen detected in ppm concentrations in a flow of nitrogen	-	11, 32
Organic dyes	Various organic phosphorescent dyes adsorbed on silica gel; can detect the formation of 50 pL (!) of oxygen per minute	-	33
¹² C ₇₀	Polystyrene	23	146
¹³ C ₇₀	Polystyrene	0.53	148
¹³ C ₇₀	Ethyl cellulose	0.25	148
PtOEP	Poly(styrene-co-TFEM)	33	319
PtOEP	Cellulose acetate butyrate + poly(tetraphenyl butadiene)	12	329
PdOEP	Poly(methyl methacrylate) + poly(tetraphenyl butadiene)	3	329
PdOEP	Polystyrene	40	279
PtTFPP	Octyl-triEOS/TEOS, doped with dye entrapped core-shell silica particle	28	337
PtTFPP	n-propyl-triMOS/TEOS/octyl-triEOS	67	339
PtTFPP	Polydimethylsiloxane (PDMS)	27	608
PtOEP	Poly(1-trimethylsilyl-1-propyne)	18	321
PdOEP	8F-PEKEK(6FBA/HF)	26	327
PdOEP	Poly(styrene-co-TFEM)	14	340
PdOEPK	Teflon	6	334
PtTFPP	Covalently labeled on the surface of silica gel	1.5	270
Al(III)-feron	Sol-gel silica from TMOS and MeTriMOS	5	349

^{a)} TFEM: poly(trifluoroethyl methacrylate); PFS: polypentafluorostyrene; 8F-PEKEK: poly(aryl ether ketone); 6FBA: 2,2-bis(4-hydroxyphenyl)-1,1,1,3,3,3-hexafluoropropane; HF: 9,9'-bis(4-hydroxyphenyl)fluorine; Octyl-triEOS: n-octyltriethoxysilane-based sol-gel; TEOS: tetraethoxysilane-based sol-gel; TFP-triMOS: 3,3,3-trifluoropropyltrimethoxysilane-based sol-gel.

11. Sensing Formats

Once an appropriate sensor material and a method for read-out have been identified, they may be applied in numerous formats. These are divided here into the following four main categories: (a) Planar films for sensing and imaging (also over large areas); (b) fiber optic sensors (including point sensors and distributed sensors); (c) microparticle based sensors, and (d) nanosensors, mainly for biological (intracellular) research and in microscopy.

11.1. Planar Sensors

The planar film sensing format is most widely used. Sensing films are prepared by dissolving the hosting material and the OSPs in certain solvents, spreading the resulting “cocktail” on a mechanical support, and allowing it to dry (or polymerize or cure) to form a thin film (See **Figure 1**) that may be applied as a coating or from which sensor spots may be punched. They can be prepared at low cost using standard film technology. The sensor spots often are used in disposables. **Figure 33** shows the portable blood gas analyzer and a disposable kit with integrated sensor spots for several species (O_2 included) in a microfluidic channel.



Figure 33. Portable blood gas analyzer and a disposable kit with integrated sensor spots for several species. *Left:* Portable analyzer for blood gases (incl. oxygen), blood electrolytes, and glucose. Blood is inserted via the syringe on the right. The disposable kit is placed under the lid. *Right:* The disposable contains an integrated microfluidic system and 6 (dark) sensor spots for sensing oxygen (along with pH, CO_2 , Na^+ , K^+ , glucose and chloride in whole blood. The pH sensor is of yellow orange color, the others are black because they are covered with optical isolations (see **Section 8.4**) to prevent blood fluorescence to interfere. The instrument is widely used in ambulance cars and peripheral stations. © OptiMedical Inc.


11.2. Fiber Optic and Other Waveguide Sensors

Optical fiber sensors (OFSs) enable oxygen to be determined remotely, at poorly accessible sites, and in harsh or hazardous environment. There is a substantial literature on fiber optic chemical

sensors and biosensors.^{24,609-614} Waveguide sensors for oxygen are obtained by depositing the sensor materials (or "cocktails") at the tip (the "distal" end) of an optical fiber, and integrated optical system, or a capillary waveguide, for example. Again, the choice of the sensor materials governs selectivity, sensitivity and analytical ranges. **Figure 34** shows a typical tip of a fiber optic sensor.

Plastic, glass, and quartz fibers may be used, depending on the analytical wavelength applied. Plastic fibers have a larger aperture, are flexible and easy to work with, but have poor transmission below 420 nm and do not tolerate multiple heat sterilization. Glass fibers are available in small size and have low attenuation, but have a small aperture. They are suitable only down to ~380 nm. Quartz fibers transmit in the UV, but their aperture is not better than that of glass. Both glass and quartz fibers are fragile and present a risk when breaking *in-vivo*.

Figure 34. Typical terminal end of a fiber optic sensor for oxygen. The tip is coated with sensor chemistry and covered with black silicone which acts as an optical isolation (see **Section 8.4.**) that prevents ambient light and sample fluorescence to interfere.




Needle-type OFSs for oxygen are used to measure oxygen partial pressure in the vascular system, tissue, bacterial mats, in plants and in numerous other situations. Typical examples are summarized in the Supporting Information on this review. If inserted into blood vessels or tissue, such sensors must not cause local disturbance, be safe and non-toxic. Peterson et al.⁴² were the first to demonstrate the feasibility of fiber optic sensing of oxygen *in-vivo*. The probe perylene dibutyrate was incorporated into porous polypropylene that was placed at the tip of an optical fiber, which then was inserted into the bloodstream of a ewe. The results obtained with the OFS agreed well with those of a blood oxygen analyzer. Miller et al.⁶⁰⁵ developed a disposable triple sensor for simultaneous monitoring of pH, $p\text{CO}_2$ and $p\text{O}_2$ directly in the artery of the forearm. The sensor was biocompatible and nontoxic, sterilizable and usable for 72 h of operation. The triple sensor consists of a bundle of three 140- μm optical fibers with respective sensor chemistries. Its performance was carefully investigated,⁶¹⁵ and precision, stability, consistency and accuracy were found to be excellent and more than adequate. However, and unlike the extracorporeal (non-invasive) triple sensor (GasStatTM) from the same company (later to become part of 3M Inc., and even later of Terumo), this fiber optic triple sensor has not been commercialized. This was due to difficulties in the proper placement of the sensor tip in the artery where an oxygen gradient exists in that oxygen levels are higher in blood flowing in the center of the artery but lower near its wall. The performance of continuous systems of ex-vivo and in-vivo monitoring of blood gases was made by Fogt.⁶¹⁶ Lübberts⁶¹⁷ has highlighted the specific features of optical sensors for clinical monitoring,

and Leiner has reviewed the performance of optical sensors for blood gas analysis.⁶¹⁸ A recent review covers fluorescent optical fiber sensors for oxygen and carbon dioxide.⁶⁰⁶

An OFS for oxygen in respiration gases of guinea pigs also was reported⁶¹⁹. The fiber optic sensor has a response time of less than 20 ms, which is short enough to continuously monitor oxygen in breath air. A fiber optic oxygen microsensor using Ru(dpp) in polystyrene was applied⁵⁴ to measure oxygen gradients in marine sediments and microbial mats. Kopelman and Rosenzweig¹⁹³ reported on a similar OFS, but using polyacrylamide as the host material which has poor permeation selectivity. The microsensor has a diameter of 0.8 μm , requires 100 fL only of a sample for analysis, and is fairly sensitive to oxygen ($I_0/I_{\text{air}} = 3.2$). It enables a spatial resolution of 1 μm . Subsequent work¹⁷⁹ describes the immobilization of the oxygen probe, and a referenced readout scheme was applied⁵⁶⁸ in a ratiometric sub- μm fiber optic sensor. A cylindrical-core FOS was developed⁶²⁰ where the probe PtOEP was immobilized in a poly(ethyl methacrylate) film that was deposited on the cylindrical core of a silica optical fiber. The response time of this sensor is <50 ms, but the choice of materials is not perfect in that PtOEP is photolabile and polymers with better permeability are known.

In an FOS for oxygen based on measurement of decay time,^{45, 450, 621} a ruthenium probe was employed having an unquenched decay time in the order of 2 μs . Phase fluorometry was performed in the MHz domain. Numerous other versions for lifetime based OFS for oxygen have been described thereafter.⁶²² Commercial systems also are using this approach. Needle-type fiber optic sensors using metal-ligand probes have had the largest success. **Figure 35** shows the tip of a decay time-based OFS for oxygen. The red luminescence of the ruthenium-based sensor material is generated by photoexcitation with a blue LED, and decay time is measured as a function of the local $p\text{O}_2$ at the tip of the fiber.

Figure 35. Tip of an optical fiber sensor viewed through a 600 nm longpass filter. Blue light from the light source (not seen here) photoexcites the luminescence of the sensor chemistry (a ruthenium OSP in a sol-gel) at the tip. Both intensity and decay time are a function of the concentration (partial pressure) of oxygen in the sol-gel.

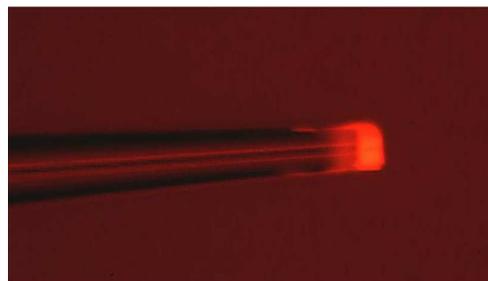

A configuration with crossed optical fibers was reported⁶²³ that comprises silver nanoparticles covalently attached to the core of a fiber and labeled with luminescent ruthenium molecules. A second optical fiber (containing the ruthenium probe incorporated into nanoparticle) was placed at right angle of the first fiber to form a fiber-fiber junction. The system was used to detect the

luminescence from the ruthenium molecules bound to the first fiber. To employ the effect of metal-enhanced luminescence, the ruthenium complex was kept at an appropriate distance from the silver nanoparticles by polyelectrolyte spacer layers. Luminescence enhancement factors were determined for silver nanospheres, nanotriangles and nanorods and for spacer-layer thicknesses from 2 – 14 nm. A 27-fold enhancement was found when the ruthenium complex was placed 4 nm away from silver nanotriangles. The same group⁶²⁴ used the crossed optical fiber with a covalently immobilized ruthenium complex to sense dissolved oxygen via either luminescence intensity ratios or lifetime, the latter performing much better. The sensing properties of an Pt(II) complex were much improved by using metal-coated silica nanoparticles.⁶²⁵ An optical fiber was coated at one end with the probe PtTFPP and silver metal-coated nanoparticles embedded in an n-octyltriethoxysilane-triethoxysilane xerogel. Its sensitivity (I_0/I_{100}) is as high as 167 which is much better than that of a sensor without silver coating.

Unlike most of the OFSs treated so far, one may also prepare sensors where the core (rather than the clad/coating or the tip) is the sensing material.⁶²⁶ When placed on a suitable substrate, light can propagate directly through the reagent film which is effectively serving as the new "core" of a waveguide. This requires the index of refraction of the sample to be lower than that of the "old" core. The advantage of such a system is the high efficiency with which exciting light is used, the large sampling areas that can be achieved, and the possibility of working with sensing materials containing very low amounts of indicators (some of which are poorly soluble). Side-illuminated polymer optical fiber sensors were described⁶²⁷ that consist of a tapered optical fiber with a ruthenium complex directly embedded in the fiber. The complete setup is based on a side-illumination scheme, and both intensity- and lifetime-based measurements were demonstrated. Sub- μm silica gel fiber made from an organic sol-gel were reported by Yang et al.⁶²⁸ **Table 16** summarizes the various kinds of OFS for oxygen reported in the literature.

In addition to the nanofiber sensor reported in earlier sections, there is a recent report on such a sensor consisting of a polydimethylsiloxane core and a polycaprolactone shell.⁶²⁹ The nanofibers containing oxygen-sensitive probes were prepared by electrospinning and can be applied as optical oxygen sensors for both gaseous and dissolved oxygen. The protective shell layer maintains the fiber's morphology during the slow curing process of the silicone and renders the surface more biocompatible. The response time is very short (0.5 s). The core-shell fibers were integrated into standard cell culture plates of glioma cell lines and glioma-derived primary cells and did not display strong cytotoxic effects.

Table 16. Representative examples of optical fiber sensors for oxygen.

<i>Waveguide type</i>	<i>Sensor material</i>	<i>Core Diameter</i>	<i>Sensing scheme</i>	<i>ref.</i>
-----------------------	------------------------	----------------------	-----------------------	-------------

		(μm)		
Multi-mode	perylene dibutyrate in polypropylene	250	Intensity	42
Single-mode fiber optic	oxygen sensitive ruthenium dye in silicone	140	Intensity	605
Multi-mode	TPP or pyrene absorbed on 0.1 mm Porapak Q and fixed on a film	3000	Intensity	619
Multi-mode	Ru(dpp) in polystyrene	100	Intensity	54
Single-mode	Ru(phen) in polyacrylamide	100, 3-5, 0.8	Intensity	193
Multi-mode	PtOEPK and OEP in PVC	0.1-0.5	Ratiometric Intensity	179
Cylindrical core silica	PtOEP in poly(ethyl methacrylate)	200	Intensity	620
Bifurcated fiber	Ru(phen) absorbed in silica gel and immobilized in silicone	50	Lifetime (Frequency domain)	450
Multi-mode	Ru(phen) in poly(ethylene glycol)-diacrylate	200	Lifetime	623
Multi-mode	Ru(phen) and rhodamine 110 in poly(ethylene glycol)-diacrylate	200	Ratiometric Intensity	624
Multimode fiber optic dual sensor	Ru(dpp) in ormosil microbeads (oxygen and pH), or Pt-TFPP in polystyrene (oxygen and temperature)	80	Lifetime and DLR	172
Multimode sensor for biochemical oxygen demand	Ru(dpp) in organic polymer; bacteria in hydrogel layer	1 mm	Intensity	192
Bifurcated fiber biosensor for glutamate using oxygen transducer	Decacyclene in silicone	3 mm	Intensity	630
Multimode fiber glucose biosensor using oxygen transducer	Ru(phen) on silica particles in silicone matrix at the tip of the fiber	3 mm	Intensity	515
Bifurcated fiber optic cholesterol biosensor using an oxygen transducer	Decacyclene in silicone matrix, enzyme immobilized on Nylon	1 mm	Intensity	631
Dual sensor (oxygen and halothane)	Decacyclene in silicone ; covered with black Teflon	2 mm	Intensity	46
Multimode	Ru(bpy) in silicone	1 mm	Lifetime	50


Fiber optics represent but one kind of optical waveguides. Other formats include planar waveguides such as the versatile chip level waveguide sensor described in a patent⁵⁷⁷ and consisting of on a chip package which contains an LED light source and a photodiode detector. Simple waveguide elements are mounted on the chip. The waveguide can be coated with various sensor chemistries to form a chemically sensitive element. See **Figure 27**. Only very recently, a capillary oxygen sensor was described that is based on luminescence lifetime measurements and utilizing monolithically integrated organic photodiodes.⁶³² Such sensors also may be considered as a kind of evanescent sensor as described in the following section.

11.3. Evanescent Wave and Plasmonic Sensing

In an optical waveguide (such as an optical fiber, a planar waveguide, or inside capillaries), light is totally reflected at the interface between the optically more dense medium and the optically rare medium if the angle of refraction is larger than a critical angle α . However, light is not instantaneously reflected at the interface. Rather, it penetrates to some extent into the optically rare

phase (**Figure 36**). The amplitude of the electric field in the rare phase does not drop abruptly to zero somewhere near the boundary, but rather has a tail that decreases exponentially in the direction of an outward normal to the boundary. This penetration phenomenon is referred to as an evanescent wave.⁶³³ In absorptiometry, the attenuation of the propagating beam is measured. In emission spectroscopy, the evanescent wave can be used to generate luminescence (of an OSP, for example) or Raman scatter. The wavelength range extends from the UV to the far infrared depending on the quality of the waveguide. Evanescent wave spectroscopy and evanescent wave sensing (EWS) is closely related to plasmonic resonance spectroscopy and cavity ring-down spectroscopy which is outside the scope of this article, however.

Figure 36. Schematic presentation of an evanescent wave in a waveguide in contact with the sample (such as an oxygen sensor coating). Redrawn from www.tau.ac.il/~applphys/research_fews.htm (with permission from the Tel Aviv University School of Physics and Astronomy).

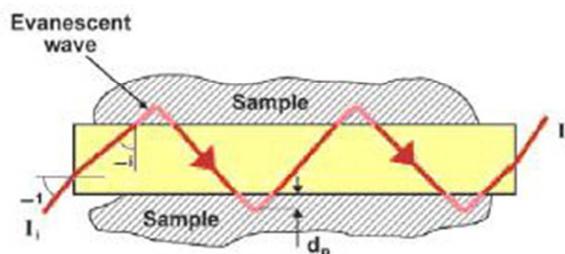


The depth of penetration (d_p) of an evanescent wave is defined as the distance within which the electric field of the wave drops to $1/e$. In a first approximation, d_p depends on the wavelength of the light and the refraction indices of the two media. Typically, d_p ranges from 300 to 1200 nm for visible light, which often is in the same order as the thickness of a sensor layer immobilized on the surface of the waveguide. Light protruding into the reagent phase will be absorbed and – hence – induce the fluorescence of the fluorophore. EWS is particularly attractive when sensing colored species such as blood because the evanescent wave is penetrating the sensor layer on top of the waveguide only, but not the (blood) sample.

EWS along with time resolution techniques^{634, 635} can considerably improve the selectivity of the method (via gated measurements) and has specific features in lifetime-based sensing of oxygen. On the other hand, EWS is adversely affected by changes in the refractive index of the outer medium (usually the sensor layer). Such changes may be caused if organic solvents (alcohol included) enter the sensor layer. The potential of EWS is based on the fact that all the methods described so far for sensing oxygen can be used also in combination with the evanescent wave mode.

Given such features, it does not come as a surprise that EWS has been applied rather early in a fiber optic sensor for oxygen.⁶³⁶ Fiber optic EWS is best demonstrated⁶³⁷ by work on sensing dissolved oxygen (DO) where the clad portion of an optical fiber was coated with a microporous

sensor cocktail prepared from trifluoropropyl trimethoxysilane, n-propyl trimethoxysilane, and a ruthenium complex. Excitation by the evanescent wave that is generated at the surface of the core (see **Figure 37**) induces luminescence whose intensity depends on the level of DO. The sensor has a detection limit as small as 0.05 ppm of DO and a short response time (15 s).

Figure 37. Schematic of evanescent wave excitation using a fiber optic waveguide that carries both the exciting light and back-reflected luminescence. (Reprinted from ref.⁶³⁷ with permission from Springer)

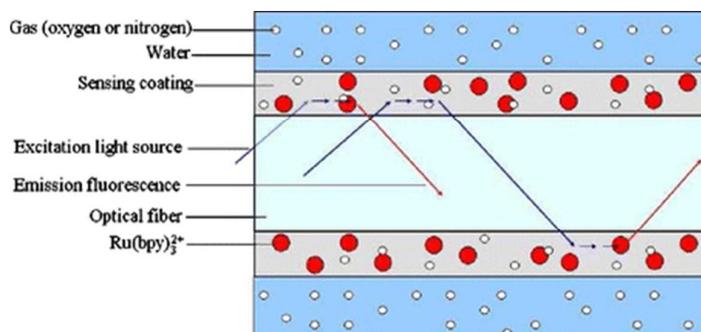


Earlier examples include oxygen sensors for breath gas analysis (**Section 12.1 in the Supporting Information**),⁶⁰³ and a fiber optic sensor⁴¹⁷ that uses the probe 9,10-diphenylanthracene in a poly(hydroxyethyl methacrylate) host. This coating was covalently grafted via silane coupling techniques onto fused silica fibers. Fluorescence was stimulated by the evanescent wave of a UV dye laser or a xenon lamp and quenched by -20% on going from an oxygen-free to an oxygen-saturated (40 ppm; 100% oxygen saturation) aqueous environment. The group of MacCraith²⁰¹ reported on a fiber optic oxygen sensor based on the quenching of the luminescence of evanescent-wave excited ruthenium complexes in a sol-gel coating. The coating was placed on a declad portion of an optical fiber via a microporous sol-gel film. The OSP was photoexcited by the evanescent field of the 488-nm radiation guided by the optical waveguide. The method later was extended to phase fluorometric sensing of oxygen using an LED-compatible sensor material and evanescent wave excitation.⁵¹⁷ Singer et al.⁶³⁸ have deposited a ruthenium complex on an optical fiber by adsorption and then coated with a membrane. It was photoexcited both by the evanescent field associated with light guided in the optical fiber and by direct irradiation, dependent on the refractive index profile of the fiber-membrane-medium system. The emitted light is collected by the same fiber. The thermostatted sensor was exposed to a liquid containing defined concentrations of oxygen which was detectable in the range from 0 to 800 Torr, with a resolution of 2 Torr in the 0 – 100 Torr range, and of 2% for oxygen partial pressures above 100 Torr. Response times are of the order of 30 s.

In an optical fiber evanescent wave absorptiometric sensor for (irreversible) detection of oxygen deficiency detection,⁶³⁹ the leuco form of the dye Methylene blue (MB) was immobilized in the cladding of the fiber using a sol-gel process. On exposure to oxygen, the dye is oxidized to form MB. The sensor is said to (irreversibly) respond to oxygen at levels between 0.6 and 20.9 % in

nitrogen. The same sensor chemistry was later applied in an integrated planar Bragg grating probe for (irreversible) detection of oxygen (**Figure 38**).⁶⁴⁰ An optical waveguide containing a Bragg grating is an effective method of detecting minute changes in refractive index (RI). Removal of a part of the waveguide's clad allows the evanescent field of the optical mode to interact with a sensor layer. The device works by detecting the change in the RI when the sensor coating is exposed to an analyte. This change across the Bragg grating causes a shift in the Bragg wavelength of the grating. The sensory coating of this particular sensor was obtained by modifying the surface of the waveguide with a silica sol-gel containing immobilized leuco MB. On exposure to molecular oxygen, the leuco dye turns blue, and this is "seen" via the absorption of the evanescent wave by the coating. Such Bragg grating based sensors can be small and yet are very sensitive. **Figure 38** shows a photograph of the sensor and how the interaction of the sensitive coating with the analyte leads to a change in the RI and, thus, the Bragg wavelength.

Figure 38. Schematic of an oxygen-sensitive integrated planar Bragg grating waveguide. (a) Photograph of a pigtailed etched Bragg grating device. (b) Schematic representation of the structure and function of a chemically sensitive waveguide integrated Bragg grating with an analyte-sensitive coating. (Reprinted from ref.⁶⁴⁰ with permission)

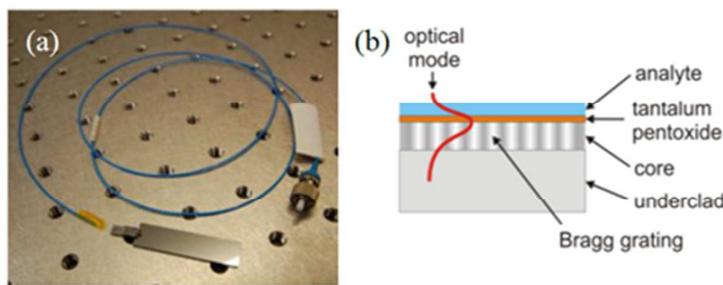

The scope of EWS fiber optic sensors can be enlarged by nanoparticle scattering deposited in the evanescent field of the sensing fiber.⁶⁴¹ The extent of scattering is dominated by the dimensions of the particles. Increasing the radius enhances the scope of the evanescent field and causes a red shift of scattered light. The scattering efficiency accounts for about 74% of the extinction efficiency when the radius is 50 nm at an excitation wavelength of 420 nm. Moreover, the scope of the evanescent field can be extended to approximately 3 μm by silver nanoparticle scattering, which – in fact – enhances the evanescent field to a relatively far-field scope.

So far, mainly (multimode) optical fibers have been discussed, but these represent only one kind of optical waveguides. Other formats include planar waveguides,⁶⁴² capillary waveguides,⁶⁴³ or integrated optics.⁶⁴⁴ All these can be operated in the evanescent wave mode, in principle, and used for purposes of sensing. Application of optical waveguide sensors in analytical chemistry, with aspects on instrumentation and applications, has been reviewed.⁶⁴⁵ A versatile chip level waveguide sensor was described in a patent of Texas Instruments⁶⁴⁶ as shown in **Figure 27**. It can be applied to both absorptiometry and fluorescence.

The number of EWS sensors for oxygen other than fiber optic sensors is small. Kroneis reports


on a breath gas analyzer consisting of a planar waveguide coated with a silicone/decaacyclene-based sensor chemistry.⁶⁰³ Another article⁶⁴⁷ reports on the use of lipophilic palladium porphyrins (in the form of self-assembled monolayers) in such sensors. The films were deposited on gold-coated glass slides and photoexcited via the evanescent field of the laser beam passing the glass slab. An integrated optic oxygen sensor was presented⁶⁴⁸ that serves as an example for a novel and generic evanescent wave sensing platform based on fluorometry. The sensor element comprises a multimode ridge waveguide patterned with an analyte-sensitive fluorescent spot (a ruthenium OSP in a sol-gel) which is photoexcited by an LED. Intensity-based calibration data were generated from the oxygen-dependent waveguide output. This sensor has a limit of detection (LOD) of 0.62% and a resolution of less than 1% of gaseous oxygen. A further kind of integrated optical oxygen sensor⁶⁴⁹ exploits the evanescent wave interaction of light confined in the waveguide that forms part of a microfluidic system. A ruthenium OSP was immobilized on the waveguide by a combined spin-coating and electrostatic LbL technique. Exposure of the OSP to a fluid containing dissolved oxygen in the microfluidic system enables pO_2 to be sensed across a wide range of interest and with an LOD of 0.6 ppm.

The filtering effect of a gold film was exploited in a method for enhancing the luminescence of probes and of sensor materials in general.⁶⁵⁰ The oxygen probe Ru(dpp) was incorporated into a trimethoxysilane xerogel and spin-coated in a thickness of ~ 100 nm. Off-axis illumination of the sensor film results in a luminescence that can be detected with a photodiode placed below the plane of the gold film and the doped sensor film. The use of a gold nanofilm improves the performance of the sensor via two mechanisms: Firstly, the transmission of the gold film is high at 520 nm but weak at 450 nm (the wavelength of excitation light), thereby reducing straylight. Secondly, even relatively insensitive luminophores within a distance of ~ 10 nm of the gold film are well quenched, and this results in noise reduction by removal of unquenched luminescence of the metal ion–ligand complex. It was questioned whether an element of radiative-decay-engineering of luminescence is occurring with luminophore emission coupling to the gold film and initiating plasmonic emission from the underside of the film, but no evidence either in terms of solely p-polarization or increased intensity of luminescence was evidenced. This confirmed that the sensor enhancement mechanism is primarily the function of metal quenching as revealed by reduced blank intensity and improved response time. A related plasmon-enhanced sensor was reported³⁴⁵ where ultrathin hybrid polymers doped with a Pt(II) porphyrin were used to image oxygen. Langmuir–Blodgett films containing a Pt(II) porphyrin probe were assembled plane-to-plane with a silver nanoparticle array. The use of nanoassemblies resulted in a >10 -fold luminescence enhancement. Luminescence intensity and lifetime were studied as a function of the number of layers, and the strong enhancement enables imaging of oxygen on the micrometer scale and with little noise.

11.4. Distributed Sensing of Oxygen

The possibility of performing spatially resolved measurements is a specific feature of fiber optic based sensing.⁶⁵¹ In this scheme, the sensor chemistry is placed as a clad on an optical waveguide, and this will enable distributed sensing of oxygen over large distances, for example via time-domain reflectometry^{169, 651} This method (commonly used to characterize the loss and length of optical fibers) enables (a) the localization of zones along the fiber where attenuation or fluorescence occur, and (b) the quantification of the local concentration of chemical species (such as oxygen) by measuring the magnitude of the variation of the signal.⁶⁵² The luminescence emitted by the probe for oxygen usually returns through the same (or another) waveguide and is received as a signal very much like an acoustical echo. The time after which the echo is registered is a measure for the distance between light source and sensor spot, while its intensity depends on (a) the distance where the echo is generated (due to the usual and linear attenuation along an optical waveguide), and (b) on the extent to which the signal is affected by the local concentration of oxygen. OTDR instrumentation is fairly small and affordable. **Figure 39** gives a typical signal as obtained by OTDR.

Figure 39. A typical signal trace as obtained by optical time domain reflectometry which is widely used in distributed sensing of gases. From ref.⁶⁵³ (open access)

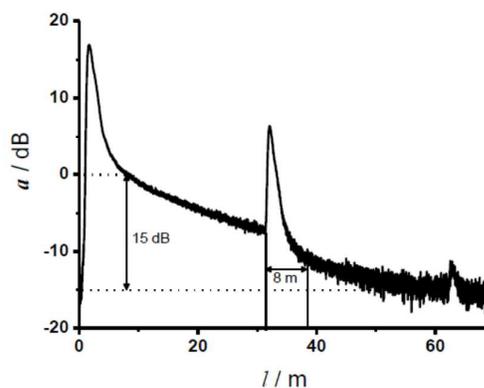

The decay time of a probe is a critical parameter in that it compromises the spatial resolution of distributed sensors. Spatial resolution obviously is limited by lifetime since a minimum separation of the fluorophores is required to resolve returning light pulses. Long lifetime probes will not allow for good spatial resolution. Since the decay time of the most OSPs based on polycyclic aromatic hydrocarbons is only 20 ns or lower, they are preferred when aiming for high spatial resolution.³¹⁴ Extended-length fibers have been prepared, for example, where spatially resolved sensing was accomplished by time-of-flight fluorescence detection.⁶⁵⁴ Sensing also was performed with a fluorescent triangular phenylene dye (whose fluorescence decay times is around 80 ns in absence of oxygen and around 20 ns in the presence of air in a polymer film), and good spatial resolution was reported using time-correlated single photon counting.⁶⁵⁵ Distributed sensing of oxygen by OTDR also was accomplished⁶⁵³ by using a fluorescent triangular phenylene dye as the

OSP. Immobilized in a polymer matrix, it has a decay time of 86 ns only. This makes it a viable probe to achieve a spatial resolution of a few meters.

If probes with long decay times are used, spatial resolution is more difficult. However, a closer spacing of sensor regions is desirable for many applications. This can be accomplished⁶⁵⁶ by using a second fiber as an optical delay line, and the minimum spacing between adjacent sensor regions then can be well below the fluorescence lifetime limit. Since the coupling between the two fibers is evanescent, the attenuation of the excitation pulse is low, making long arrays of sensor regions feasible.^{169, 651} Following pulsed, evanescent excitation of the sensor dyes through the first fiber, the second fiber captures their fluorescence and delivers it to the detector. Crossed optical fibers were also shown to enable high-spatial-resolution sensing of dissolved oxygen.⁶²⁴ The luminescent probe (a ruthenium dye) was located in certain spots along the optical fiber in the cladding, and a short laser pulse propagating through the fiber core allows for the determination of the location of the luminophores. The spatial resolution in such quasi-distributed fiber optic sensor arrays is increased beyond the fluorescence-lifetime limit by such a sensing platform. Both luminescence-intensity and luminescence-lifetime changes of the OSP (in response to changes in the concentration of dissolved oxygen) can be used as the analytical information. In case of intensity measurements, a second adjacent sensor region can be employed as a reference to account for laser pulse energy fluctuations.

Distributed sensing also was performed in another kind of referenced mode⁶⁵⁴ where an analyte-insensitive fluorophore was added to the sensor material, and intensity was related (referenced) to that of the oxygen probe. In yet another scheme,⁶⁵⁷ time-correlated single photon counting and stroboscopic detection were combined with an evanescent-wave fiber optic sensing. While demonstrated in this case for sensing pH values, the scheme awaits its extension to distributed lifetime-based sensing of oxygen. Methods also have been developed for optical time-of-flight discrimination of multiple signals along a fiber waveguide.⁶⁵⁸

11.5. Microparticle-Based Sensing

Microparticle (μP)-based sensors are mainly used as a bulk material or incorporated into an oxygen-permeable host matrix. μP -sensors are not often used for intracellular sensing because of their size, which is often larger than that of a cell (see **Table 17**). Sensors beads made from silica μP s were reported¹⁶ as early as in 1935. In this case, the dyes were adsorbed on the surface. Other kinds of μP sensors were prepared by polymerization, precipitation, or by doping polymer microparticles with OSPs as outlined in more detail in **Section 7.3**. Such microsensors also were dispersed in hybrid sensing films, in hydrogels and in silicone matrices. Many of them can be sterilized. Klimant et al.⁴⁹⁶ prepared magnetically separable sensor μP s from phenyltriethoxysilane, Ru(dpp), Fe_3O_4 , and

TiO₂ nanoparticles. Because of their magnetic nature, handling is simple and flexible. If placed inside a glass or plastic bioreactor, the sensor film can be magnetically drawn to almost any desired position inside the vessel and the optical signal can be read from outside (**Figure 40**, left).

Specifically, contactless monitoring of oxygen in cultures of *Escherichia coli* was demonstrated. These features also make such sensor beads attractive for use in flow-through systems, shaking flasks, and microtiter plates. The same group⁶⁵⁹ reported on spray-coated magnetic stainless steel microspheres with polymeric sensor matrices containing the iridium-coumarin complex Ir(C_S)₂(acac) or PtTPTBP to obtain spheres that serve the same purposes (see **Figure 40**, right).

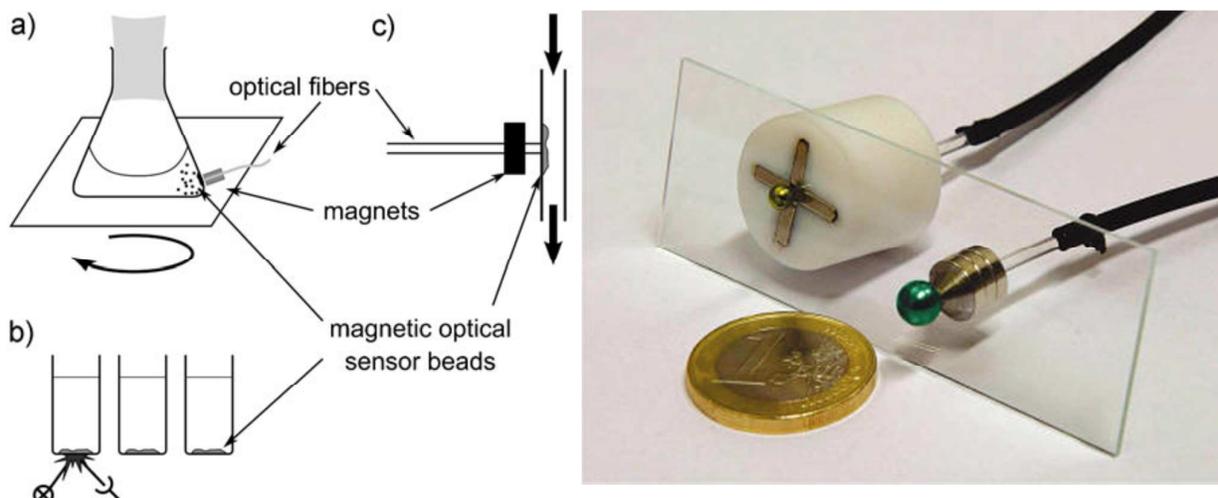


Figure 40. Magnetic oxygen sensitive macrospheres. *Left:* Schematic representation of the potential range of application of magnetic sensor beads in: a) a shaking flask, b) microtiter plate measurements, and c) flow-through systems. *Right:* Magnetic sensor macrospheres (brown and green spheres) captured in front of an optical fiber with a radial or axial separator. (Reprinted from refs.⁴⁹⁶ (*left*) and ⁶⁵⁹ (*right*) with permission from Wiley-VCH and American Chemical Society, respectively)

“Smart tattoo” μ P sensors (comprising fluorescent microspheres that can be implanted intradermally and interrogated noninvasively using light) were developed⁶⁶⁰ as potential tools for *in vivo* biochemical monitoring. Particles were prepared by immobilizing PtOEP in hybrid silicate microspheres along with glucose oxidase. Rhodamine B-doped multilayer nanofilms were subsequently assembled on the surfaces of the particles to provide a reference signal and provide critical control of glucose transport into the particle. The enzymatic oxidation of glucose within the sensor results in the glucose concentration-dependent depletion of local oxygen levels, enabling indirect monitoring of glucose by measuring relative changes in the emission of PtOEP. The sensors respond fairly rapidly ($t_{95} \sim 1.5$ min) and fully reversibly to changes in bulk glucose levels, while demonstrating high baseline stability.⁶⁶¹ The role of the porosity in tuning the response range of the microsphere sensors was investigated.⁶⁶²

Mesoporous alginate-silica μ Ps represent another kind of hybrid matrix.⁶⁶³ The probe PtOEP was

loaded into microspheres using a solvent-mediated precipitation method. The beads were then loaded with the enzyme cholesterol oxidase by covalent conjugation. The surface was then "closed" by layer-by-layer self-assembly of alternatively charged polyelectrolytes. Similarly, glucose oxidase was entrapped into calcium alginate along with a ruthenium probe to create a sensor for glucose.⁶⁶⁴ The μ Ps were again coated with polyelectrolyte multilayers and used as implantable biosensors — so-called "smart tattoos." The multilayer nanofilms on the surface of the microspheres can stabilize enzyme entrapment and control substrate diffusion.

Oxygen-responsive fluorescent microbeads embedded into a biocompatible polyacrylamide gel sheet have been attached to target cells for fluorescent imaging of metabolic activity.⁶⁶⁵ This resulted in a patch-type oxygen imaging sheet useful for in vitro cellular metabolic assays. The sensor beads were deposited in a microfluidic device using electrical manipulation techniques, this followed by coverage with a hydrogel. Fluorescent imaging of oxygen-consuming activity was demonstrated for glucose oxidase-modified μ Ps as cellular models to show the applicability of the imaging sheet to bioassays.

Table 17. Overview on typical kinds of microparticles for use in optical sensing of oxygen.

Matrix	Probe	Size(μ m)	Remarks	Ref.
Silica gel	tryptaflavin	10	Room temperature phosphorescence	16, 17
Silica gel	Ru(bpy)	2 – 5	Room temperature phosphorescence	47
Silica gel	Ru(dpp)	9.5-11	Luminescence quenched by oxygen	499
Fumed silica	Ru(dpp)	0.2 – 0.3	Dye absorbed on the surface of hydrophilic fumed silica	198
Silica	PtTCPP	10.3	Amino-modified silica microsphere, co-encapsulated with QDs for ratiometric oxygen sensing.	498
Phospholipid coated polystyrene	Ru(bpy-pyr)(bpy) ₂	2.1	Dye dissolved lipid and coated on polystyrene microparticle	215
Porous glass beads	fluoranthene	~ 10	Fluorescence quenched by oxygen	35
Ormosil	Ru(dpp)	~ 10	Magnetic microparticles, luminescence quenched by oxygen,	496
Ormosil	Ru(dpp)	1-2	Luminescence quenched by oxygen	475
Polystyrene	PtOEP	1.0	PtOEP encapsulated during polymerization, reference dye was co-encapsulated for ratiometric readout.	485 435
Polystyrene	PtTFPP	0.3-1.0	Fluorescence lifetime (frequency domain) based measurement	440, 481
Poly(styrene-co-acrylonitrile)	Metalloporphyrin	~1.0	Prepared using precipitation method, sensitivity can be tuned by changing the ratio of acrylonitrile in the polymer.	414-416 551
Polystyrene or polysulfone	Ir(C ₈) ₂ (acac) PtTPTBP	3.2 mm	Magnetic stainless steel macrospheres, luminescence quenched by oxygen	659
FIB	PtTFPL	5 cm	Glass spheres	388


11.6. Microsensors (not Fiber Optic, not Microparticle-Based)

This section covers microsensors that are *not* of the fiber optic and *not* of the microparticle type. Such sensors typically consist of a micro-sized semiconductor covered with an oxygen-sensitive coating. In a typical example, such a microsensors was obtained⁶⁶⁶ by covalently functionalizing a

GaN semiconductor with a ruthenium(II) OSP. This resulted in an innovative sensing scheme in which the semiconductor plays the role of both the support and the light source for photoexcitation. Luminescence decay time studies and time-resolved emission spectra confirmed the presence of the dye on the semiconductor surfaces. The sensitivity of the device to oxygen is comparable to that of other ruthenium-based sensor systems. Such microsensors are very compact and intriguing because of the full integration of semiconductor components. In subsequent work, the indicator dyes were grafted onto a blue LED⁶⁶⁷ following plasma activation of its surface. Confocal fluorescence microscopy with single-photon-timing detection revealed emission lifetimes of $\sim 2 \mu\text{s}$ under nitrogen, which however dropped, in case of n-GaN-functionalized surfaces to $0.6 \mu\text{s}$. This was interpreted in terms of photoinduced electron injection from the dye to the semiconductor conduction band, followed by a fast back electron transfer. Hence, the n-GaN/dye system is less suitable. The decay time of the p-GaN/dye material, in contrast, decreases in the presence of oxygen.

A completely embedded microsensor array was introduced⁶⁶⁸ that can be read out with an imaging system to sense oxygen (with a ruthenium OSP) and pH values (with a carboxyfluorescein pH probe; both in a hydrogel) in parallel. The system consists of an ultra-bright blue LED source, coupling optics, interference filters and a compact moisture-resistant CCD camera. The microarray was created by photoreaction injection molding and contains two separate hydrogel based sensing elements (see **Figure 41**). The standard error when sensing both dissolved oxygen and pH values during a bioprocess was 0.75% and 0.092, respectively. This microsensor approach also may be considered as a lab-on-a-chip type sensor. High-throughput micropatterning of optical oxygen sensors was also reported and applied to single cell analysis.⁶⁶⁹ Other work related to microsensors and arrays relates to photolithographic patterning of polymer-encapsulated optical oxygen sensors,⁶⁷⁰ to micro-patterned sensors and cell self-assembly for measuring the oxygen consumption rate of single cells,⁶⁷¹ and to photo-patternable polymeric membranes for optical oxygen sensors.⁶⁷²

Figure 41. Image of the sensor as captured by the camera. The top row contains a fluorescent pH microsensor, and the bottom row an oxygen sensor layer. It can be seen that signal loss on the edges of the oxygen sensors is evident due to swelling and leaching and therefore box A is used as the average fluorescent signal. (Reprinted from ref.⁶⁶⁸ with permission from Elsevier)

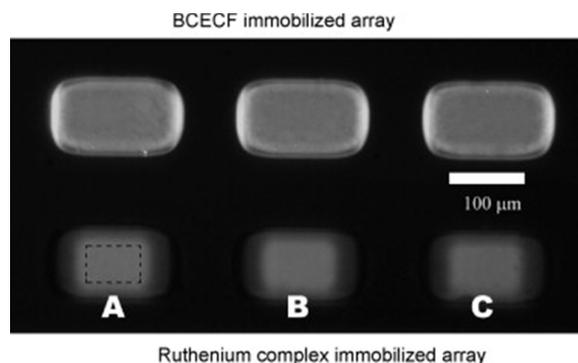

Oxygen sensors also have been designed in the format of a screen-printed flexible radiofrequency identification tag.⁶⁷³ It consists of an oxygen-sensitive membrane containing the OPS PtOEP (which is not the best choice) along with an electronic system for RFID communication, all printed on a flexible plastic substrate. Luminescence is excited by an LED operated at 385 nm wavelength, and its intensity is registered by means of a digital color detector. The output data corresponding to red coordinate of the RGB colour space is directly related to the concentration of gaseous oxygen, and it is sent to a microcontroller. The RFID tag is designed for the wireless transmission of the data to a remote reader.

Optical sensing films adaptable to microdevices were also obtained by electrophoretic deposition (EPhD).⁶⁷⁴ Nanoparticles made from poly(styrene-co-maleic anhydride) and containing the OSP Pt(II) meso-tetra(pentafluorophenyl)porphine were deposited by EPhD which is possible because they carry a charge at near-neutral pH values. Compared to other deposition methods, EPhD is simple and allows control over the rate of deposition. This is crucial for the implementation of optical sensing films in microdevices.

11.7. Dendrites and Nanosensors


Optical oxygen sensors can be miniaturized to the nanodimension which is in striking contrast to the size of even the smallest electrochemical oxygen sensors. Such nanosensors can have radii as small as 10 nm and therefore occupy only ~1 ppb of the volume of an average mammalian cell, thereby causing rather negligible mechanical and functional perturbation.

11.7.1. Dendrites

Dendritic nanoprobess have been reported mainly by the Vinogradov group. They have developed four generations of these oxygen-sensitive dendrimers. The water-soluble metalloporphyrins of the type PtTCPP and PdTCPP (see **Section 6.2.5**) can be regarded as the first generation but were steadily improved. The *Oxyphors* of generation 2 are polyglutamic dendrimers containing Pd-meso-tetra-(4-carboxyphenyl) porphyrin and Pd-meso-tetra-(4-carboxyphenyl) tetrabenzoporphyrin, designated as *Oxyphor R2* and *Oxyphor G2* (**Figure 42**), respectively.^{675, 676} Both phosphors are water soluble and bear 16 (negatively charged) carboxy groups on the outer layer, so their ability to penetrate biological membranes is very low, and this increases the circulation time in blood and renders them quite suitable for sensing oxygen over time. The maxima in the absorption spectra are at 415 and 524 nm for *Oxyphor R2*, and 440 and 632 nm for *Oxyphor G2*, while emissions are very longwave (near 700 and 800 nm, respectively). The calibration plots of the phosphors are essentially independent of pH in the 6.4 to 7.8 range. The following figure shows the *Oxyphore 2* based on a palladium probe which is quite often used in *Oxyphor* systems. These polyglutamic dendrimers are loaded with Pd(II) benzoporphyrins and show excellent sensing characteristics and a

12% QY, but they form complexes with albumin. Modification of the dendrimer periphery with poly(ethylene glycol) reduces quenching but does not prevent binding of the phosphors to albumin. The dendrimer was further endowed with 2-photon absorption capability³⁰⁵ to image oxygen in three dimensions using 2-photon laser scanning microscopy. The dendrimer also was functionalized with poly(arylglycine) to further improve its solubility and stability in biological fluids and to prevent the interaction with biomolecules.⁶⁷⁷⁻⁶⁷⁹ The outer layer carboxy groups of such dendrimers were used by Kopelman et al.⁴⁸⁹ to covalently link them to polymer nanoparticles.


Figure 42. Chemical structure of Oxyphor G2. (Reprinted from ref. ⁶⁷⁶ with permission from Elsevier)

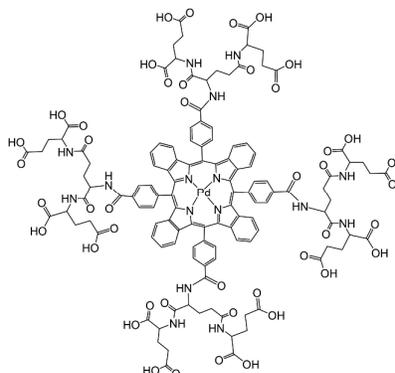

In a phosphorescence imaging system for monitoring oxygen distribution in rat liver under ischemia and oxygen reperfusion⁶⁸⁰ using the probes *Oxyphor* R2 and *Oxyphor* G2, the changes of hepatic oxygen pressure under ischemia and subsequent reperfusion were monitored in real-time. The images indicated a transient recovery of hepatic oxygen level during the reperfusion. The lack of complete restoration of oxygen level resembles a similar pattern of hepatic blood flow observed during reperfusion in previous studies.

The third generation of *Oxyphor* (referred to as *Oxyphor* G3)⁶⁷⁸ is based on Pd-tetrabenzoporphyrin dendrimers having *both* a polyarylglycine scaffold and a poly(ethylene glycol) surface coating as shown in **Figure 43**. *Oxyphor* G3 has a molecular mass of 16.1 kDa and is designed not to interact with albumin and other biomolecules. It folds tightly around the porphyrin core in aqueous media and controls accessibility of oxygen to the phosphor. Its QY is around 10%, and the lifetime is 270 μ s in deoxygenated aqueous solution.

Figure 43. The chemical structure of *Oxyphor* G3. (Reprinted from ref.⁶⁷⁸ with permission from the American Chemical Society)

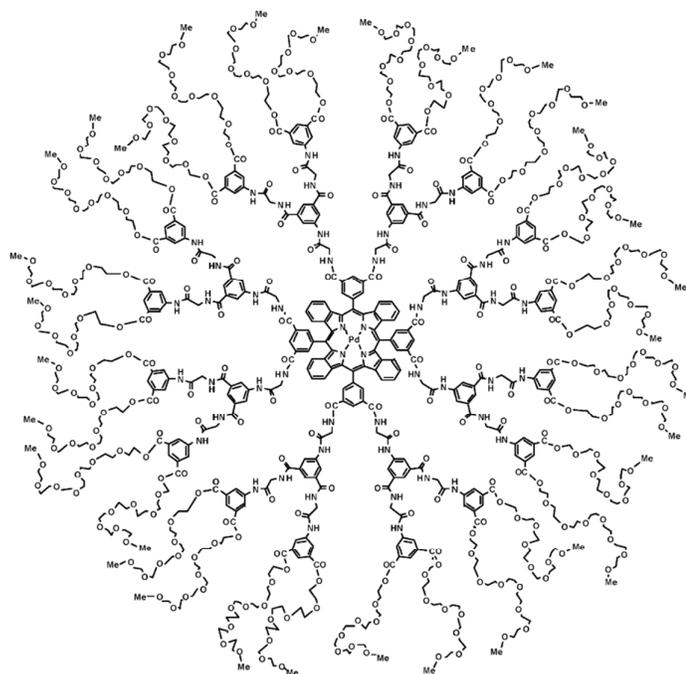

The *Oxyphor* generation four (referred as *Oxyphor* R4 and *Oxyphor* G4)⁶⁸¹ is the latest and was applied to tumor imaging. Like the *Oxyphors* of generation 3, they are derived from phosphorescent palladium(II) complexes of tetraphenylporphyrin or tetraphenyl-tetrabenzoporphyrins, respectively, but their phenyl groups have been replaced by 3,5-dicarboxyphenyl groups. These are negatively charged at pH values around 7, and this renders the probes better soluble and, at the same time, cell-impermeable. They possess all the other features that are common for protected dendritic probes, i.e., hydrophobic encapsulation of the luminescent probe and a hydrophilic PEGylated periphery.

Metalloporphyrin-containing dendrimers were also designed for imaging oxygen *in vivo* based on two-photon excitation.⁶⁸² Antenna dyes which capturing the two-photon energy were covalently attached to the dendrimers to form nanosized architectures. In these constructs, the generation of porphyrin triplet states following two-photon excitation is induced by an intramolecular Förster-type resonance energy transfer from a covalently attached antenna dye (a coumarin) to a phosphorescent Pt(II) porphyrin. The dendrimer forms an insulating layer between the porphyrin and the antenna dye and simultaneously controls the rate of quenching by oxygen. Modification of the dendrimer periphery with oligo(ethylene glycol) made the signal insensitive to the presence of albumin and other macromolecular solutes. Combined with multi-photon laser scanning microscopy, 3D imaging of oxygen with submicron spatial resolution was accomplished.

The same group³⁰⁶ later synthesized the highly phosphorescent Pt(II) porphyrin poly(arylglycine) dendrimer with several coumarin units attached to the periphery to capture two-photon excitation energy. The dendrimers were used to measure pO_2 in the cortical microvasculature and tissue in depths of up to 250 μm and with sub-second temporal resolution. High-resolution images of oxygen

distribution also were obtained³⁰⁷ by two-photon laser scanning microscopy using such dendritic nanoprobe in various kinds of cells. Other applications include diffuse tomographic imaging⁶⁸³ and monitoring of oxygen in cortical microvessels by confocal microscopy⁶⁸⁴ and are summarized in the Supporting Information in section S1.

11.7.2. Fluorescent Probes Incorporated into Nanoparticles

The encapsulation of fluorescent OSPs into nanoparticles results in another kind of nanosensors. These have special features because their properties can be tuned by using materials possessing highly different gas permeabilities. In addition, their surface may be modified to enable special applications such as site-specific placement (via appropriate antibodies), or attachment to enzymes including DNAzymes. Lübbers et al.¹⁵⁷ probably were the first to incorporate an oxygen probe (pyrenebutyric acid) into nanosized spheres to which they referred as "nanocapsules". Imaging of pO_2 with submicroscopic resolution was envisioned. Several other methods have been reported ever since, examples being the swelling-stain technique,⁴⁸² precipitation,⁴⁷⁸ and chemical modifications.⁴⁹⁸ Such nanoparticles (NPs) also can be prepared by bottom-up techniques such as the Stöber method^{173, 326} and monomer polymerization.^{484, 486, 489} OSPs have been chemically attached or physically entrapped inside the NPs during formation. NP sensors are mainly used in combination with microscopy for intracellular sensing because cell viability is usually maintained. Cellular metabolism, respiration, and response to external stimulations including potential drugs have been studied this way. Such applications are discussed in more detail in the **Supporting Information**. Kopelman et al.⁶⁸⁵ have reviewed the use of their so-called PEBBLE (*photonic explorer for bioanalysis with biologically localized embedding*) sensors in live cells and *in vivo*. Selected nanosensors for oxygen already have been described in **Section 7.3** from a materials point of view.

In addition to more conventional host materials of the silica gel or hydrogel type, conjugated fluorescent polymers also were doped⁵⁶⁹ with a Pt(II) porphyrin probe, and the resulting NPs exhibited bright phosphorescence that is highly sensitive to oxygen. The small size, extraordinary brightness, excellent sensitivity, and ratiometric emission, together with the demonstration of single-particle sensing and cellular uptake, indicate the potential of the NP sensors for quantitative mapping of local molecular oxygen concentration. In another (and cell-permeable) phosphorescent nanosensor, called MM2 and being commercially available, the highly photostable probe PtTFPP and the conjugated polymer poly(9,9-dioctylfluorene) act as a Förster resonance energy transfer donor and as a two-photon antenna, respectively.⁵³⁴ Both fluorophores were placed in NPs with an average size of 70 nm and madFe from a cationic hydrogel. These nanosensors can be internalized into cells, and this paves the way for high-resolution imaging of cellular oxygen. Both ratiometric

(2-wavelength) intensity sensing and phosphorescence lifetime-based imaging under single-photon and two-photon excitation were demonstrated. The nanosensors were placed inside adherent cells and neurospheres to image the oxygen distribution and fluctuation during treatment with drugs.

Ultra-small nanosensors were described for dual sensing of oxygen and pH directly in the cytosol.⁵⁶³ These dually-responsive nanosensors have a unique nanostructure in that a soft core structure is rigidized with a silane reagent to form a mesoporous silica shell, while poly(ethylene glycol) chains form an hydrophilic outer surface (**Figure 44**). Lipophilic oxygen-sensitive probes and reference dyes were placed inside the hydrophobic core, while a pH-sensitive probe is covalently attached to the terminal of the poly(ethylene glycol) chains on the surface. The core/shell structure renders the nanosensors well dispersed and highly stable in various kinds of aqueous media. Their average size is 12 nm, and they respond to both pH and oxygen in the physiological range. They do not pass cell membranes, but can be internalized into the cellular cytosol by electroporation, upon which they enable sensing and imaging of pH values and oxygen directly in the cytosol with high spatial resolution. **Table 18** gives selected examples of nanosized optical sensors for oxygen.

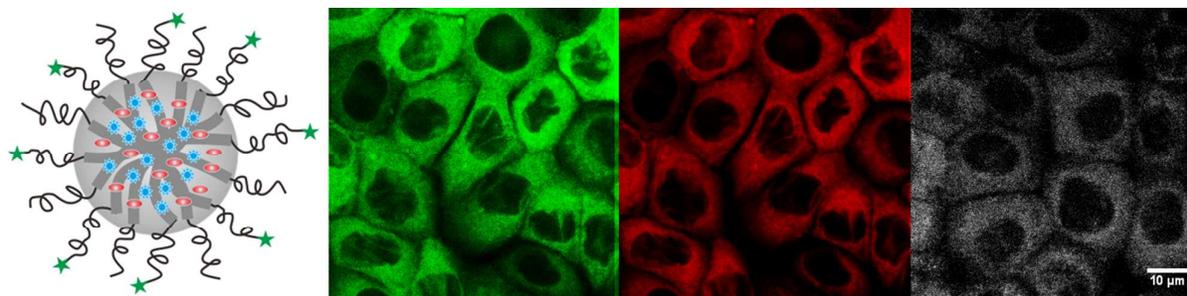


Figure 44. Ultra-small dual nanosensors for sensing pH and oxygen values in cytosol. From left to right: the structure of dual nanosensors, oxygen indicator and reference dye in the hydrophobic core, and the pH-sensitive FITC covalently attached at the PEG end; nanosensors delivery in cytosol using electroporation, the green luminescence from FITC, red luminescence from reference dye, and the NIR luminescence (in grey) resulting from the OSP. (Reprinted from ref.⁵⁶³ with permission of the American Chemical Society)

Other nanoparticles (NPs) of the core-shell type were described⁴⁹¹ that consist of a biocompatible shell and a hydrophobic core (containing the covalently immobilized oxygen probe PtTFPP) that was obtained via radical-initiated microemulsion co-polymerization. The NPs can be readily loaded into cells and then are capable of recording intracellular oxygen levels. The NPs have a diameter of <50 nm and luminescence decay times of up to 44 μ s. Most importantly, the dye is not leached and the outer shell is biocompatible so that cytotoxicity is strongly reduced.

Table 18. Overview on nanosensors for oxygen. *Codes:* I: intensity-based readout; RI: ratiometric intensity-based readout; L: lifetime-based readout; n.m.: not mentioned.

<i>Probe</i>	<i>Matrix</i>	<i>Size(nm)</i>	<i>Readout</i>	<i>Sensitivity</i>	<i>Measurement range</i>	<i>Ref.</i>
Ru(phen)	Liposome	36	I	$I_0/I_{100} = 7$	0-100 %	494
Ru(phen)	NaYF ₄ :Yb ³⁺ , Tm ³⁺ /SiO ₂ core/shell nanoparticle	40-100	I	$I_0/I_{100} = 3.9$	0-100 %	168
Ru(dpp)	Silica	50-300	RI	$I_0/I_{100} = 6$	0-100 %	173
Ru(phen)	Phospholipid vesicles	150	RI	$I_0/I_{40 \text{ mg/L}} \sim 3.8$	0-40 mg/L	495
Ru(dpp)	Polystyrene (amine-functioned)	100	I	n.m.	n.m.	686
Ru(dpp(SO ₃ Na) ₂) ₃	Polyacrylamide	45	L	$\tau_0/\tau_{100} = 2.14$	0-100 %	490
PtOEP	Ormosil	120	RI	$I_0/I_{42.5 \text{ ppm}} = 33.3$	0-42.5 ppm	326
PtTFPP	Ormosil	170	I	$I_0/I_{100} = 166$	0-100 %	337
PtTFPP	Poly(styrene-block-vinylpyrrolidone)	245	L	$I_0/I_{20 \text{ kPa}} \sim 4.0$	0-20 kPa	227 483
PtTFPP	Eudragit RL-100	35	L	$\tau_0/\tau_{209 \mu\text{M}} = 2.33$	0-209 μM	480, 534
PtTFPP	Polystyrene (amine-functioned)	100 or 500	RI	$I_0/I_{100} \sim 4.5$	0-100 %	482
PtTFPP with styrene group	2,2'-N-isopropylacrylamide and Acrylic acid based copolymer	45	L	$\tau_0/\tau_{20} \sim 2.5$	0-20 %	491
PdTCPP	Mesoporous silica	70-100	n.m.	n.m.	n.m.	497
PtOEP	Conjugated fluorescent polymer PFO and PDHF	50	RI	$I_0/I_{100} = 20$	0-100 %	569
PtOEP	Poly(methyl methacrylate)	150-170	RI	$I_0/I_{100} = 4.35$	0-100 %	687
PtOEP	Polystyrene/poly-L-lysine core/shell nanoparticle	130	RI	$I_0/I_{42.5 \text{ ppm}} = 16.67$	0-42.5 ppm	688
PtOEPK	Poly(decyl methacrylate)	150-250	RI	$I_0/I_{42.5 \text{ ppm}} = 40$	0-42.5 ppm	488
PtTPTBP	Pluronic F127/silica core/shell nanoparticle	12	RI	$I_0/I_{42.5 \text{ ppm}} = 10.05$	0-42.5 ppm	563
Oxphor G2	Polyacrylamide	30	RI	$I_0/I_{100} = 28$	0-100 %	489
No need	Boron polylactide polymer nanoparticle, BF ₂ dbmPLA	96	RI	$I_0/I_{1\%} \sim 1.41$	0-1%	377 375
Ir(C ₅) ₂ (acac)	Eudragit RL-100 polymer Eudragit RS-100 polymer	~ 360	L	$\tau_0/\tau_{\text{air}} = 2.36$ $\tau_0/\tau_{\text{air}} = 2.03$	0-21 %	478

12. Applications

Numerous applications of optical sensors for oxygen have been described, and some are presented in the Supporting Information which contains the following sections:

- S1. Sensing of Oxygen in Blood and in the Vascular System
- S2. Sensing Oxygen in Breath Gas: Respiratory Diagnosis
- S3. Sensing and Imaging of Oxygen in Skin (Tumor) Research, Diagnosis and Therapy
- S4. Sensing Oxygen in Medicine and Lab (and Test) Animals (except skin)
- S5. Intracellular Sensing of Oxygen
- S6. Oxygen Sensors in Tissue Engineering and Stem Cell Research
- S7. Oxygen Sensors in Animal Biology

- S8. Oxygen Sensors in Plant Biology
- S9. Oxygen Sensors in Drug Screening, Toxicity Testing, Mitochondrial Activity Studies, and Related Areas
- S10. Oxygen Sensors in Biotechnology, Fermentation and Microbiology
- S11. Oxygen Sensors in Marine and Freshwater Research
- S12. Oxygen Sensors in Environmental and Geosciences
- S13. Oxygen Sensors in Food Technology and Packaging
- S14. Oxygen Sensors in Gas Pressure-Sensitive Paints
- S15. Oxygen Sensors as Transducers in Biosensors
- S16. Oxygen Sensors Integrated into Microfluidic Devices and Lab-on-a-Chip Systems
- S17. Oxygen Sensors in Industry, Material Research, Production and Surveillance

13. Conclusions and Outlook

Optical sensing of oxygen is at a rather advanced state. At present, technology is driven by new materials, new nanotechnologies and spectroscopies. Exciting current research activities cover probe design, nanosensors and nanofiber sensors, new sensing schemes such as (localized) surface plasmon resonance, or effects that occur on surfaces of noble metals. These activities will not only further enlarge the range of sensors and the fields of applications, but also improve the performance of current sensors. It can also be stated that the design of sensor materials still is a kind of trial-and-error game because their performance cannot be modeled mathematically so far.

By now, optical sensors for oxygen have been applied to numerous impressive applications, but one may state that existing sensors not so much are competing with the classical electrochemical sensor (the Clark electrode). Rather, they have been applied (and are being applied) to fields and research challenges for which appropriate electrochemical or other methods did not exist so far. Typical examples include (a) fiber optic sensors for sensing over large distances, under harsh conditions or in strong electromagnetic fields, (b) imaging of oxygen over large areas, mainly in (skin) medicine, aerodynamics, marine sciences, and biotechnology; (c) nanosensors for use inside cells, in interstitial or vascular fluids, or directly in the flow of a microfluidic system; and (d) contactless sensing of oxygen inside a bioreactor by placing the sensor spot on the inner side of a transparent window and monitoring its optical properties through this window. It is another matter of fact that optical sensors for oxygen ("optodes" as they sometimes are referred to) are in the process of replacing the classical Clark electrode which is the gold standard at present. We predict the oxygen optode to displace the Clark electrode within 10 years from around 50% of its current market.

Any question for the "best" sensor for oxygen cannot be answered unless the problem is specified. Unlike the Clark electrode which comes in a few variations only, hundreds of kinds of optical sensors for oxygen are known or may be envisioned. While sensing of oxygen in engine exhaust gases at temperatures of $>400\text{ }^{\circ}\text{C}$ is best performed with a sensor material such as $\text{Mo}_6\text{Cl}_{12}$ clusters, the detection of oxygen at ppb levels at temperatures between $-100\text{ }^{\circ}\text{C}$ and $+100\text{ }^{\circ}\text{C}$ is better performed by exploiting the strongly quenched delayed fluorescence of certain fullerenes. It is a fortunate situation that most sensors for oxygen based on the use of luminescent probes contained in a polymer host do survive chemical and/or thermal sterilization. Other situations (such as barometric sensing) require sensors with very fast response times so to acquire images at a kHz

rate. This requires sensor materials that are very different from those where response time plays no role. As for *in vivo* studies, oxygen sensors whose excitation and emission bands located in the NIR are preferred to prevent interferences from biological luminescence background. NIR oxygen sensors are developing very rapidly in recent years and such this trend will continue to enlarge the database in this field. Sensors with long decay times offer an alternative because they are amenable to time-resolved fluorometry which can suppress background luminescence, but this has limitations if data or images are to be required a fast rates or with high spatial resolution such as in distributed sensing of oxygen along a large distance fiber. We have summarized the most frequently used molecular probes (or indicators; OSPs) and the most frequently used polymer hosts in Tables 19 and 20, respectively. These are widely used but it shall be kept in mind that special situations may require other combinations of materials and, of course, spectroscopies.

Tables 19 and 20 near here

Despite these attractive features, one cannot ignore the fact that practically all reversible sensors for oxygen are based on the quenching of luminescence by oxygen. This can be considered as being a disadvantage because the human eye can much better differentiate the color and intensity of reflected light than the color and intensity of luminescent light. Practically all commercially available optical tests (like the stripes used for measurement of pH values, or the widely used pregnancy tests) are color-, i.e. reflectometry-based for this reason. Unfortunately, reflectometric test stripes for reversible(!) sensing of oxygen do not exist. This would be great to have but has not been realized so far. There are, however, sensor known that change color (such as from colorless to blue) on exposure to oxygen (see section 4), but the respective color changes are irreversible. Such "sensors" (better "probes") cannot monitor the decrease of oxygen concentration over time, for example. Some can be chemically regenerated, though. Single-shot colorimetric probes for oxygen predictably will find more applications in the future, typically in areas where millions of products need to be quickly monitored, for example in the food and pharmaceutical industry. Another drawback of oxygen sensors based on luminescence quenching is their inadequate performance when measuring high concentrations of oxygen. This "market" is still dominated by electrochemical sensors, but there is an urgent demand for such sensors, not the least for safety reasons.

It is noted that optical imaging of oxygen has experienced particularly exciting applications. Field of applications include (a) the use of nanosensors for microscopic imaging of the distribution of oxygen inside cells, (b) the use of sensor paints to image the distribution of barometric pressure on vehicles including aircrafts, (c) the detection of hypoxia in skin tumors, (c) the distribution of oxygen in benthic systems, (d) the read-out of microtiterplates or arrays of micro-vials with oxygen sensors placed on their bottom, to give a few representative examples only.

Fluorescent sensors usually are read out by instrumental means, and it is a fortunate situation that respective readers, due to advances in optoelectronics, are truly small, typically of the size smaller than a cigarette pack. This also holds for imagers. Predictably, sensors will become much smaller (< 1 cubic mm) in the future, and this will pave the way to mass production. Such sensors will find large scale applications such as in fuel cells, in mobile phones and computers, or as microbarometers in aircrafts to measure cabin pressure. All this is indication that research in this field will continue to go on strongly and in many directions.

Table 19. List of the most often used kinds of luminescent probes for optical sensing and imaging of oxygen (in the form of polymer-based coatings, films, or nanoparticles), along with excitation and emission maxima (in nm) and specific comments.

<i>Probe</i>	<i>Exc./Em. maxima</i>	<i>Comments</i>
Ru(dpp) ₃ 2X ⁻	460/597	Fairly photostable; well established; cationic; counter anions (X ⁻) include those of long chain fatty acids, trimethylsilyl propanesulfonate, or tetrafluoroborates; moderate brightness; well soluble in hydrophilic polymers but a lipophilic counterion is needed if to be used in non-polar polymer hosts such as silicones; fairly long decay time (0.5 – 6 μs)
PtTFPP PdTFPP	392 (540)/650 407 (552)/670	Very photostable; well established; uncharged; well soluble in apolar polymers except silicones; lifetimes in the upper μs to ms range; excellent brightness under UV excitation, moderate brightness under excitation with visible light; these probes have widely replaced the formerly used probes PtOEP and PdOEP which suffer from poor photostability.
PtTPTBP PdTPTBP	430 (614)/770 444 (629)/797	Very photostable; uncharged; well soluble in apolar polymers except silicones; long lifetime (the Pd complex in particular); emission in NIR, excellent brightness; the Q absorption band of the Pd(II) porphyrin is compatible with red He-Ne laser and laser diode
PtOEPK PdOEPK	398 (598)/760 408 (601)/791	Fairly photostable; uncharged; well soluble in apolar polymers except silicones; long lifetime (the Pd complex in particular); emission in the NIR, moderate brightness
PtTFPL	400 (574)/738	more photostable than the PtOEPK complex, but otherwise rather similar
Dendrimeric (benzo)porphyrins	415 (524, 632, 678)/ 700 - 800	Can be well dispersed in watery systems; very fast response; known as <i>Oxyphors</i> ; widely used in physiological studies (see section 12); dendritic structure with hydrophilic outer shell and a core consisting of a Pd(II) (benzo)porphyrin; molecular mass of nanoparticles typically is 15 – 20 MDa; can be negatively charged to prevent cell permeation, but charge can be varied to prevent interaction with albumins.
Ir(III)-coumarin complexes	421-484/544-588	High brightness (high quantum yield and absorption coefficient); uncharged; moderately long lifetime; moderate photostability.
Polycyclic hydrocarbons: (a) pyrene; (b) decacylene	(a) 335/384 and 450 (b) 385/510	(a) Fair stability; requires UV excitation; used in fast-responding pressure sensitive paints; less suitable for biological application due to UV excitation; moderate sensitivity and brightness (b) Good photostability; compatible with blue LEDs; good oxygen quenching efficiency; large Stokes shift.
Fullerenes	C ₆₀ : 532/750 C ₇₀ : 470 and 532/860	Very good stability; extremely high sensitivity; very long lifetime (ms); E-type delayed fluorescence; works at temperatures up to 240 °C, moderate brightness.

Table 20. List of the most often used kinds of polymeric host materials for use in luminescent sensing and imaging of oxygen (in the form of coatings, films, or nanoparticles), and specific comments.

<i>Polymer</i>	<i>Comments</i>
Ethyl cellulose	Biocompatible; good optical transparency; good mechanical strength; ease of handling.
Silicone rubbers (incl. fluorosilicones)	Excellent gas permeability, high thermal stability, excellent chemical and mechanical stability, ease of handling, good adhesion to glass fibers, inertness to biological samples, optically transparent; hydrophobic; many commercially available prepolymers contain solvents, fillers, low molecular weight cross-linkers, catalysts and other additives; need for curing. Poor compatibility with many indicators due to string tendency for aggregation; fluorosilicones have very high chemical resistances and even better oxygen permeability.
Fluorinated copolymers: (a) Poly-styrene- <i>co</i> -PFS and poly-styrene- <i>co</i> -TFEM; (b) Poly-IBM- <i>co</i> -TFEM and poly- <i>t</i> BS- <i>co</i> -TFEM; (c) FIB	(a) – (c): High gas permeability; excellent photostability; useful for trace oxygen sensing; (a) – (b): gas permeability can be tuned by varying different monomers and the ratio of monomers; (c) poly(hexafluoroisopropyl methacrylate)- <i>co</i> -(heptafluoro- <i>n</i> -butyl methacrylate); high gas permeability; excellent photostability; small temperature dependence; suitable for application in wind tunnels (barometry) with temperature compensation
Polyurethane hydrogels	highly biocompatible; ease of handling; good optical transparency; more often used as a matrix to host other kinds of sensor particles; swellable.
Polystyrene	Easy to manufacture; low cost; moderate oxygen permeability; can be sterilized; excellent shelf time and stability in aqueous solutions; good optical transparency; no need for curing. Copolymers can be used to prepare water-dispersible oxygen-sensitive nanoparticles.
PMMA (plexiglass)	Ease of manufacture; low cost material; moderate oxygen permeability; suitable for sensing oxygen above air saturation; copolymers known for preparing water-dispersible sensor nanoparticles; moderate hydrolytic stability under harsh conditions; background fluorescence under UV excitation.
Poly(1-trimethylsilyl-1-propyne) (PTMSP)	Extremely high gas permeability; no need for cross-linking; useful for trace oxygen sensing; prone to aging affects (decrease of oxygen permeability with time)
Polystyrene- <i>co</i> -acrylonitrile (PSAN)	Gas permeability can be tuned by changing the ratio of monomers; good stability; easy to handle; the monomer acrylonitrile is toxic.
Silica gels	Commercially available in different size and porosity; can physically absorb oxygen sensitive probes; easy handling; good optical transparency and low fluorescence background; biomolecules can be incorporated.
Ormosils (organically-modified silica gels)	Easily prepared at room temperature; hydrophobicity is tunable by changing precursors; fluorinated ormosils have very high gas permeability that may change over time; good mechanical and chemical stability.

14. List of Acronyms

Acronym	Stands for
2-D	2-dimensional
APTES	(3-aminopropyl)trimethoxysilane
CAB	cellulose acetate butyrate
CCD	charge coupled device
CCTA	contact charge-transfer absorption
CL	chemiluminescence
CMOS	complementary metal oxide semiconductor
CPG	controlled porous glass
DiMe-DMOS	dimethoxydimethylsilane
DLD	dual lifetime determination
EC	ethyl cellulose
Et-TriMOS	ethyltrimethoxysilane
OFS	fiber optic sensor
FRET	fluorescence resonance energy transfer
LB	Langmuir-Blodgett
LED	light-emitting diode
MAP	modified atmosphere packaging
MLCT	metal-ligand charge transfer
μ P	microparticle
Me-TriMOS	methyltrimethoxysilane
NIR	near infrared
NP	nanoparticle
n-propyl-TriMOS	n-propyl-trimethoxysilane
Octyl-triEOS	n-octyltriethoxysilane
ormosil	organically modified silicate
OSM	optical sensor material
OSP	oxygen sensitive probe
PAHs	polycyclic aromatic hydrocarbons
PDMS	poly(dimethyl siloxane)
PFCs	perfluorochemicals
pHEMA	poly(2-hydroxyethyl methacrylate)
PMMA	poly(methyl methacrylate)
pPEGMA	poly(ethylene glycol) ethyl ether methacrylate
PS	polystyrene
PSAN	poly(styrene-co-acrylonitrile)
PSP	pressure sensitive paints
Ph-TriMOS	phenyltrimethoxysilane
pTMSP	poly(1-trimethylsilyl-1-propyne)
PTPs	poly(thionylphosphazenes)
PVA	polyvinyl alcohol

PVC	polyvinyl chloride
QDs	quantum dots
RLD	rapid lifetime determination
ROMPs	ring opening metathesis polymers
RSD	relative standard deviation
RTP	room-temperature phosphorescence
RTV	room-temperature vulcanizing
SVP	Stern-Volmer plot
TEOS	tetraethyl orthosilicate
TFP-TriMOS	3,3,3-trifluoropropyltrimethoxysilane
TLC	thin layer chromatography
Tri-MOS	Trimethylmethoxysilane
UCNPs	(photon)up-conversion nanoparticles
UV	ultraviolet

Acknowledgements

This work was financially supported by the Alexander von Humboldt foundation (Bonn) through a fellowship for Dr. Xu-dong Wang which is gratefully acknowledged.

15. References

- G. L. Semenza, *Science*, 2007, **318**, 62-64.
- H. Decker and K. E. Van Holde, *Oxygen and the Evolution of Life*, Springer Verlag, Berlin Heidelberg, 2011.
- L. W. Winkler, *Ber. Dtsch. Chem. Ges.*, 1888, **21**, 2843-2854.
- K. Kinoshita, *Electrochemical Oxygen Technology*, Wiley-Interscience, 1992.
- R. Ramamoorthy, P. K. Dutta and S. A. Akbar, *J. Mater. Sci.*, 2003, **38**, 4271-4282.
- Y. Amao, *Mikrochim. Acta*, 2003, **143**, 1-12.
- X. D. Wang, H. X. Chen, Y. Zhao, X. Chen and X. R. Wang, *TrAC, Trends Anal. Chem.*, 2010, **29**, 319-338.
- J. R. Stetter and J. Li, *Chem. Rev.*, 2008, **108**, 352-366.
- R. Moos, in *Springer Series on Chemical Sensors and Biosensors*, 2012, vol. 11, pp. 173-188.
- O. S. Wolfbeis, *Angew. Chem. Int. Ed.*, 2013, **52**, DOI: 10.1002/anie.201305915.
- H. Kautsky and A. Hirsch, *Ber. Dtsch. Chem. Ges.*, 1931, **64**, 2677-2686.
- G. N. Lewis and M. Calvin, *Chem. Rev.*, 1939, **25**, 273-328.
- G. N. Lewis, D. Lipkin and T. T. Magel, *J. Am. Chem. Soc.*, 1941, **63**, 3005-3018.
- I. A. Zakharov and T. I. Grishaeva, *J. Appl. Spectrosc.*, 1979, **31**, 1295-1298.
- I. A. Zakharov and T. I. Grishaeva, *Zh. Prikl. Spektrosk.*, 1982, **36**, 697-701.
- H. Kautsky and A. Hirsch, *Z. Anorg. Allg. Chem.*, 1935, **222**, 126-134.
- J. Franck and P. Pringsheim, *J. Chem. Phys.*, 1943, **11**, 21-27.
- A. Mills, *Platinum Met. Rev.*, 1997, **41**, 115-126.
- J. N. Demas, B. A. DeGraff and P. B. Coleman, *Anal. Chem.*, 1999, **71**, 793A-800A.
- A. Mills, *Chem. Soc. Rev.*, 2005, **34**, 1003-1011.
- O. S. Wolfbeis, *J. Mater. Chem.*, 2005, **15**, 2657-2669.
- C. O'Donovan, J. Hynes, D. Yashunski and D. B. Papkovsky, *J. Mater. Chem.*, 2005, **15**, 2946-2951.
- O. S. Wolfbeis, *Adv. Mater.*, 2008, **20**, 3759-3763.
- Y. Amao and I. Okura, *J. Porphy. Phthalocya.*, 2009, **13**, 1111-1122.
- A. P. Demchenko, *Meth. Appl. Fluoresc.*, 2013, **1**, 022001.
- N. Optiz and D. W. Lübbers, *Int. Anesthesiol. Clin.*, 1987, **25**, 177-197.
- O. S. Wolfbeis, *Fiber optic chemical sensors and biosensors*, CRC Press, Boca Raton, Florida, 1991.
- X. Lu and M. A. Winnik, in *Mol. Supramol. Photochem.*, eds. V. Ramamurthy and K. S. Schanze, CRC, 2000, vol. 6, pp. 311-352.

29. D. B. Papkovsky and R. I. Dmitriev, *Chem. Soc. Rev.*, 2013, DOI: 10.1039/C1033CS60131E.
30. M. Quaranta, S. Borisov and I. Klimant, *Bioanal Rev.*, 2012, **4**, 115-157.
31. O. Stern and M. Volmer, *Physikalische Zeitschrift*, 1919, **20**, 183-188.
32. H. Kautsky, *Trans. Faraday Soc.*, 1939, **35**, 216-219.
33. M. Pollack, P. Pringsheim and D. Terwoord, *J. Chem. Phys.*, 1944, **12**, 295-299.
34. I. Zakharov and T. Grishaeva, *Zh. Anal. Khim.*, 1980, **35**, 481.
35. I. Bergman, *Nature*, 1968, **218**, 396-396.
36. J. R. Lakowicz and G. Weber, *Biochemistry*, 1973, **12**, 4161-4170.
37. P. R. Stevens, US Patent 3.612.866 1982.
38. H. H. Hesse, East Ger. Pat. 106086 1974.
39. D. W. Lübbers and N. Opitz, *Z. Naturforsch C, Biosci.*, 1975, **30C**, 532.
40. D. W. Lübbers and N. Opitz, *Adv Exp Med Biol*, 1976, **75**, 65-68.
41. K. P. Völkl, N. Opitz and D. W. Lübbers, *Fresenius' Journal of Analytical Chemistry*, 1980, **301**, 162-163.
42. J. I. Peterson, R. V. Fitzgerald and D. K. Buckhold, *Anal. Chem.*, 1984, **56**, 62-67.
43. O. S. Wolfbeis, H. Offenbacher, H. Kroneis and H. Marsoner, *Mikrochim. Acta*, 1984, **82**, 153-158.
44. T. M. Freeman and W. R. Seitz, *Anal. Chem.*, 1981, **53**, 98-102.
45. H. Marsoner and H. Kroneis, Eur. Pat. Appl. 109958 & 109959; US Pat. 4.587.101, 1984.
46. O. S. Wolfbeis, H. E. Posch and H. W. Kroneis, *Anal. Chem.*, 1985, **57**, 2556-2561.
47. O. S. Wolfbeis, M. J. P. Leiner and H. E. Posch, *Mikrochim. Acta*, 1986, **90**, 359-366.
48. P. C. Alford, M. J. Cook, A. P. Lewis, G. S. G. McAuliffe, V. Skarda, A. J. Thomson, J. L. Glasper and D. J. Robbins, *J. Chem. Soc. Perk. Trans. 2*, 1985, 705-709.
49. J. R. Bacon and J. N. Demas, *Anal. Chem.*, 1987, **59**, 2780-2785.
50. M. E. Lippitsch, J. Pusterhofer, M. J. P. Leiner and O. S. Wolfbeis, *Anal. Chim. Acta*, 1988, **205**, 1-6.
51. J. M. Vanderkooi, G. Maniara, T. J. Green and D. F. Wilson, *J. Biol. Chem.*, 1987, **262**, 5476-5482.
52. H. E. Kahil, M. P. Gouterman and E. Green, *PCT Appl. WO 87.00023*, 1987.
53. G. E. Khalil, M. P. Gouterman and E. Green, US Patents 4,810,655, 1989.
54. I. Klimant, V. Meyer and M. Kuhl, *Limnol. Oceanogr.*, 1995, 1159-1165.
55. R. Narayanaswamy and O. Wolfbeis, in *Optical Sensors for Industrial, Environmental and Clinical Applications*, Springer, 2003, pp. 1-34; ISBN 33-540-40888-X.
56. P. B. Arnouldse, H. L. Pardue, J. D. Bourland, R. Miller and L. A. Geddes, *Anal. Chem.*, 1992, **64**, 200-204.
57. L. Gianfrani, A. Sasso and G. M. Tino, *Sens. Actuators, B*, 1997, **39**, 283-285.
58. V. Weldon, J. O'Gorman, J. J. Pérez-Camacho, J. Hegarty, J. C. Connolly and N. A. Morris, *Sens. Actuators, B*, 1997, **42**, 163-168.
59. C. Jia, H. Andreas, S. Rainer, F. Maximilian and A. Markus-Christian, Conference on Lasers and Electro-Optics/International Quantum Electronics Conference, 2009.
60. X. Lou, G. Somesfalean, B. Chen and Z. Zhang, *Appl. Opt.*, 2009, **48**, 990-997.
61. S. Neethu, R. Verma, S. S. Kamble, J. K. Radhakrishnan, P. P. Krishnapur and V. C. Padaki, *Sens. Actuators, B*, 2014, **192**, 70-76.
62. G. E. Khalil, A. Chang, M. Gouterman, J. B. Callis, L. R. Dalton, N. J. Turro and S. Jockusch, *Rev. Sci. Instrum.*, 2005, **76**, -.
63. S. Jockusch, N. J. Turro, E. K. Thompson, M. Gouterman, J. B. Callis and G. E. Khalil, *Photoch. Photobio. Sci.*, 2008, **7**, 235-239.
64. A. P. Losev, I. M. Byteva and G. P. Gurinovich, *Chem. Phys. Lett.*, 1988, **143**, 127-129.
65. V. S. Tiwari, A. T. Luanje, R. R. Kalluru, F. Y. Yueh and J. P. Singh, *Rev. Sci. Instrum.*, 2011, **82**, 043108-043108-043109.
66. Z. Zhang and R. W. Seitz, *Anal. Chem.*, 1986, **58**, 220-222.
67. K. E. Chung, E. H. Lan, M. S. Davidson, B. S. Dunn, J. S. Valentine and J. I. Zink, *Anal. Chem.*, 1995, **67**, 1505-1509.
68. M. F. McCurley, G. J. Bayer and S. A. Glazier, *Sens. Actuators, B*, 1996, **36**, 491-496.
69. F. Baldini, M. Bacci, F. Cosi and A. Del Bianco, *Sens. Actuators, B*, 1992, **7**, 752-757.
70. A. Del Bianco, F. Baldini, M. Bacci, I. Klimant and O. S. Wolfbeis, *Sens. Actuators, B*, 1993, **11**, 347-350.
71. S. Rööslä, E. Pretsch, W. E. Morf, E. Tsuchida and H. Nishide, *Anal. Chim. Acta*, 1997, **338**, 119-125.
72. Y. Suzuki, H. Nishide and E. Tsuchida, *Macromolecules*, 2000, **33**, 2530-2534.
73. L. Vaska, *Science*, 1963, **140**, 809-810.
74. L. Vaska, *Acc. Chem. Res.*, 1976, **9**, 175-183.
75. R. D. Jones, D. A. Summerville and F. Basolo, *Chem. Rev.*, 1979, **79**, 139-179.
76. F. Baldini and A. D. Bianco, *Fiber Integr. Opt.*, 1992, **11**, 123-133.
77. M. F. Choi and P. Hawkins, *Sens. Actuators, B*, 1996, **30**, 167-171.
78. M. F. Choi and P. Hawkins, *Talanta*, 1995, **42**, 987-997.
79. Y. Amao, K. Asai and I. G. Okura, *Chem. Lett.*, 1999, **1**, 95-96.
80. Y. Amao, K. Asai and I. Okura, *Bull. Chem. Soc. Jpn.*, 1999, **72**, 2223-2227.
81. Y. Amao, K. Asai and I. Okura, *Analyst*, 2000, **125**, 523-526.
82. Y. Amao, K. Asai and I. Okura, *J. Porphyr. Phthalocya.*, 2000, **4**, 292-299.

83. T. Furuto, S.-K. Lee, Y. Amao, K. Asai and I. Okura, *J. Photochem. Photobiol., A*, 2000, **132**, 81-86.
84. S. Ashkenazi, S. W. Huang, T. Horvath, Y. E. L. Koo and R. Kopelman, *J. Biomed. Opt.*, 2008, **13**, -.
85. H. Zollinger, *Color chemistry: syntheses, properties, and applications of organic dyes and pigments*, Wiley-VCH, 2004.
86. G. I. Goodfellow and H. M. Webber, *Analyst*, 1979, **104**, 1105-1118.
87. P. A. Hamlin and J. L. Lambert, *Anal. Chem.*, 1971, **43**, 618-620.
88. D. Perlman and H. Linschitz, US Patent 4,526,752, 1985.
89. Y. Yoshikawa, T. Nawata, M. Goto and Y. Fujii, US Patent 4,169,811, 1979.
90. Y. Yoshikawa, T. Nawata, M. Goto and Y. Kondo, US Patent 4,349,509, 1982.
91. S.-K. Lee, A. Mills and A. Lepre, *Chem. Commun.*, 2004, 1912-1913.
92. D. Gutiérrez-Tauste, X. Domènech, N. Casañ-Pastor and J. A. Ayllón, *J. Photochem. Photobiol., A*, 2007, **187**, 45-52.
93. S.-K. Lee, M. Sheridan and A. Mills, *Chem. Mater.*, 2005, **17**, 2744-2751.
94. A. Mills and D. Hazafy, *Analyst*, 2008, **133**, 213-218.
95. Y. Galagan and W. F. Su, *J. Photochem. Photobiol., A*, 2008, **195**, 378-383.
96. Y. Galagan, S.-H. Hsu and W.-F. Su, *Sens. Actuators, B*, 2010, **144**, 49-55.
97. L. Roberts, R. Lines, S. Reddy and J. Hay, *Sens. Actuators, B*, 2011, **152**, 63-67.
98. Y. Galagan and W. F. Su, *Food Res. Int.*, 2008, **41**, 653-657.
99. K. Eaton, *Sens. Actuators, B*, 2002, **85**, 42-51.
100. S. Wilhelm and O. S. Wolfbeis, *Sens. Actuators, B*, 2011, **153**, 199-204.
101. K. C. Krumhar and M. Karel, US Patent 5,096,813, 1992.
102. S. Wilhelm and O. Wolfbeis, *Mikrochim. Acta*, 2010, **171**, 211-216.
103. A. Mills, K. Lawrie, J. Bardin, A. Apedaile, G. A. Skinner and C. O'Rourke, *Analyst*, 2012, **137**, 106-112.
104. M. A. Butler and A. J. Ricco, *Sens. Actuators*, 1989, **19**, 249-257.
105. G. A. Nyberg, US Patent 4,764,343, 1988.
106. H. Lin, Y. Shen, D. Chen, L. Lin, B. Wilson, B. Li and S. Xie, *J. Fluoresc.*, 2013, **23**, 41-47.
107. J. Lakowicz, *Principles of fluorescence spectroscopy*, 3 edn., Springer, New York, 2006.
108. B. Valeur, *Molecular fluorescence: principles and applications*, Wiley-VCH, Weinheim, 2002.
109. E. R. Carraway, J. N. Demas and B. A. DeGraff, *Anal. Chem.*, 1991, **63**, 332-336.
110. E. R. Carraway, J. N. Demas, B. A. DeGraff and J. R. Bacon, *Anal. Chem.*, 1991, **63**, 337-342.
111. J. N. Demas, B. A. DeGraff and W. Xu, *Anal. Chem.*, 1995, **67**, 1377-1380.
112. S. Draxler, M. E. Lippitsch, I. Klimant, H. Kraus and O. S. Wolfbeis, *J. Phys. Chem.*, 1995, **99**, 3162-3167.
113. P. Hartmann, M. J. P. Leiner and M. E. Lippitsch, *Anal. Chem.*, 1995, **67**, 88-93.
114. W. Xu, R. C. McDonough, B. Langsdorf, J. N. Demas and B. A. DeGraff, *Anal. Chem.*, 1994, **66**, 4133-4141.
115. S. A. Vinogradov and D. F. Wilson, *Biophys. J.*, 1994, **67**, 2048-2059.
116. V. I. Ogurtsov, D. B. Papkovsky and N. Y. Papkovskaia, *Sens. Actuators, B*, 2001, **81**, 17-24.
117. V. I. Ogurtsov and D. B. Papkovsky, *Sens. Actuators, B*, 2006, **113**, 917-929.
118. E. J. Bowen and A. Norton, *Trans. Faraday Soc.*, 1939, **35**, 44-48.
119. H. Weil-Malherbe and J. Weiss, *Nature*, 1942, **149**, 471-472.
120. H. W. Kroneis and H. J. Marsoner, *Sens. Actuators*, 1983, **4**, 587-592.
121. T. Okazaki, T. Imasaka and N. Ishibashi, *Anal. Chim. Acta*, 1988, **209**, 327-331.
122. M. E. Cox and B. Dunn, *Appl. Opt.*, 1985, **24**, 2114-2120.
123. B. J. Basu, C. Anandan and K. S. Rajam, *Sens. Actuators, B*, 2003, **94**, 257-266.
124. B. J. Basu, A. Thirumurugan, A. R. Dinesh, C. Anandan and K. S. Rajam, *Sens. Actuators, B*, 2005, **104**, 15-22.
125. J. Zilberstein, A. Bromberg and G. Berkovic, *J. Photochem. Photobiol., A*, 1994, **77**, 69-81.
126. N. Opitz, H. J. Graf and D. W. Lübbers, *Sens. Actuators*, 1988, **13**, 159-163.
127. T. Ishiji and M. Kaneko, *Analyst*, 1995, **120**, 1633-1638.
128. Y. Amao, I. Okura and T. Miyashita, *Bull. Chem. Soc. Jpn.*, 2001, **74**, 1159-1160.
129. Y. Fujiwara and Y. Amao, *Sens. Actuators, B*, 2002, **85**, 175-178.
130. Y. Fujiwara, I. Okura, T. Miyashita and Y. Amao, *Anal. Chim. Acta*, 2002, **471**, 25-32.
131. Y. Fujiwara and Y. Amao, *Sens. Actuators, B*, 2003, **89**, 58-61.
132. Y. Fujiwara and Y. Amao, *Sens. Actuators, B*, 2003, **89**, 187-191.
133. Y. Fujiwara and Y. Amao, *Sens. Actuators, B*, 2004, **99**, 130-133.
134. D. Odaci, B. N. Gacal, B. Gacal, S. Timur and Y. Yagci, *Biomacromolecules*, 2009, **10**, 2928-2934.
135. T. Abe, M. Matsuguchi and Y. Sakai, *Chem. Sens. (Japanese)*, 2000, **16(Suppl. B)**, 109-111.
136. N. Geacintov, G. Oster and T. Cassen, *J. Opt. Soc. Am.*, 1968, **58**, 1217-1228, and refs. cited therein.
137. P. H. Bolton, R. D. Kenner and A. U. Khan, *The Journal of Chemical Physics*, 1972, **57**, 5604-5605.
138. P. F. Jones and R. S. Nesbitt, *The Journal of Chemical Physics*, 1973, **59**, 6185-6186.
139. A. Sharma and O. S. Wolfbeis, *Anal. Chim. Acta*, 1988, **212**, 261-265.
140. O. S. Wolfbeis and F. M. Carlini, *Anal. Chim. Acta*, 1984, **160**, 301-304.
141. W. Trettnak, M. J. P. Leiner and O. S. Wolfbeis, *Analyst*, 1988, **113**, 1519-1523.
142. H. Marsoner, H. Kroneis and O. S. Wolfbeis, US Patent 4,657,736, 1987.

143. P. Y. F. Li and R. Narayanaswamy, *Analyst*, 1989, **114**, 663-666.
144. P. Y. F. Li and R. Narayanaswamy, *Analyst*, 1989, **114**, 1191-1195.
145. H.-W. Lin, M.-H. Huang, Y.-H. Chen, W.-C. Lin, H.-C. Cheng, C.-C. Wu, T.-C. Chao, T.-C. Wang, K.-T. Wong, K.-C. Tang and P.-T. Chou, *J. Mater. Chem.*, 2012, **22**, 13446-13450.
146. S. Nagl, C. Baleizao, S. M. Borisov, M. Schaferling, M. N. Berberan-Santos and O. S. Wolfbeis, *Angew. Chem. Int. Ed.*, 2007, **46**, 2317-2319.
147. C. Baleizao, S. Nagl, M. Schaferling, M. N. Berberan-Santos and O. S. Wolfbeis, *Anal. Chem.*, 2008, **80**, 6449-6457.
148. S. Kochmann, C. Baleizão, M. N. Berberan-Santos and O. S. Wolfbeis, *Anal. Chem.*, 2013, **85**, 1300-1304.
149. H. Kautsky and G. O. Müller, *Z. Naturforsch* 1947, **2A**, 167-172.
150. I. A. Zakharov and T. I. Grishaeva, *Zh. Prikl. Spektrosk.*, 1984, **57**, 1240.
151. I. A. Zakharov and T. I. Grishaeva, *Zh. Anal. Khim.*, 1982, **37**, 1753.
152. J. M. Charlesworth, *Sens. Actuators, B*, 1994, **22**, 1-5.
153. R. Badía, M. E. Díaz-García and A. Sanz-Medel, *Mikrochim. Acta*, 1995, **121**, 51-61.
154. A. Yekta, Z. Masoumi and M. A. Winnik, *Can. J. Chem.*, 1995, **73**, 2021-2029.
155. N. Kraus, G. Israel, F. W. Müller, K. Schiller and M. Rätzsch, *Die Angewandte Makromolekulare Chemie*, 1991, **192**, 93-101.
156. S. K. Lam, M. A. Chan and D. Lo, *Sens. Actuators, B*, 2001, **73**, 135-141.
157. D. W. Lübbers, N. Opitz, P. P. Speiser and H. J. Bisson, *Zeitschrift für Naturforschung. Section C: Biosciences*, 1977, **32**, 133-134.
158. W. Xu, R. Schmidt, M. Whaley, J. N. Demas, B. A. DeGraff, E. K. Karikari and B. A. Famer, *Anal. Chem.*, 1995, **67**, 3172-3180.
159. R. Badia and M. E. D. Garcia, *Anal. Lett.*, 2000, **33**, 307-322.
160. M. A. Chan, J. L. Lawless, S. K. Lam and D. Lo, *Anal. Chim. Acta*, 2000, **408**, 33-37.
161. J. I. Peterson and R. V. Fitzgerald, *Rev. Sci. Instrum.*, 1980, **51**, 670-671.
162. J. N. Demas, E. W. Harris and R. P. McBride, *J. Am. Chem. Soc.*, 1977, **99**, 3547-3551.
163. M. Z. Ongun, O. Oter, G. Sabancı, K. Ertekin and E. Celik, *Sens. Actuators, B*, 2013, **183**, 11-19.
164. L. Li and D. R. Walt, *Anal. Chem.*, 1995, **67**, 3746-3752.
165. G. Kuncová and M. Fialová, *Biotechnol. Tech.*, 1995, **9**, 175-178.
166. J. F. Gouin, F. Baros, D. Birot and J. C. André, *Sens. Actuators, B*, 1997, **39**, 401-406.
167. Y. Amao and I. Okura, *Sens. Actuators, B*, 2003, **88**, 162-167.
168. L. Liu, B. Li, R. F. Qin, H. F. Zhao, X. G. Ren and Z. M. Su, *Nanotechnology*, 2010, **21**, 285701.
169. M. V. Rigo, R. Olsson and P. Geissinger, *Sensors & Transducers Journal*, 2010, **113**, 18-32.
170. G. Liebsch, I. Klimant and O. S. Wolfbeis, *Adv. Mater.*, 1999, **11**, 1296-1299.
171. M. E. Köse, B. F. Carroll and K. S. Schanze, *Langmuir*, 2005, **21**, 9121-9129.
172. A. S. Kocincova, S. M. Borisov, C. Krause and O. S. Wolfbeis, *Anal. Chem.*, 2007, **79**, 8486-8493.
173. H. Xu, J. W. Aylott, R. Kopelman, T. J. Miller and M. A. Philbert, *Anal. Chem.*, 2001, **73**, 4124-4133.
174. Z. J. Fuller, W. D. Bare, K. A. Kneas, W. Y. Xu, J. N. Demas and B. A. DeGraff, *Anal. Chem.*, 2003, **75**, 2670-2677.
175. I. Klimant and O. S. Wolfbeis, *Anal. Chem.*, 1995, **67**, 3160-3166.
176. F. J. Mingoarranz, M. C. Moreno-Bondi, D. García-Fresnadillo, C. de Dios and G. Orellana, *Mikrochim. Acta*, 1995, **121**, 107-118.
177. J. F. Fernández-Sánchez, T. Roth, R. Cannas, M. K. Nazeeruddin, S. Spichiger, M. Graetzel and U. E. Spichiger-Keller, *Talanta*, 2007, **71**, 242-250.
178. I. Klimant, P. Belser and O. S. Wolfbeis, *Talanta*, 1994, **41**, 985-991.
179. K. P. McNamara, X. Li, A. D. Stull and Z. Rosenzweig, *Anal. Chim. Acta*, 1998, **361**, 73-83.
180. M. P. Xavier, D. García-Fresnadillo, M. C. Moreno-Bondi and G. Orellana, *Anal. Chem.*, 1998, **70**, 5184-5189.
181. C. Malins, H. G. Glever, B. D. MacCraith, S. Fanni and J. G. Vos, *Anal. Commun.*, 1999, **36**, 3-4.
182. E. Holder, D. Oelkrug, H.-J. Egelhaaf, H. A. Mayer and E. Lindner, *J. Fluoresc.*, 2002, **12**, 383-395.
183. Z. Wang, A. R. McWilliams, C. E. B. Evans, X. Lu, S. Chung, M. A. Winnik and I. Manners, *Adv. Funct. Mater.*, 2002, **12**, 415-419.
184. P. Hartmann, M. J. P. Leiner and M. E. Lippitsch, *Sens. Actuators, B*, 1995, **29**, 251-257.
185. S. J. Payne, G. L. Fiore, C. L. Fraser and J. N. Demas, *Anal. Chem.*, 2010, **82**, 917-921.
186. K. A. McGee, D. J. Veltkamp, B. J. Marquardt and K. R. Mann, *J. Am. Chem. Soc.*, 2007, **129**, 15092-15093.
187. K. A. McGee, B. J. Marquardt and K. R. Mann, *Inorg. Chem.*, 2008, **47**, 9143-9145.
188. K. A. McGee and K. R. Mann, *J. Am. Chem. Soc.*, 2009, **131**, 1896-1902.
189. X.-d. Wang, D. E. Achatz, C. Hupf, M. Sperber, J. Wegener, S. Bange, J. M. Lupton and O. S. Wolfbeis, *Sens. Actuators, B*, 2013, **188**, 257-262.
190. D. Xiao, Y. Mo and M. M. F. Choi, *Meas. Sci. Technol.*, 2003, **14**, 862.
191. D. S. Daivasagaya, L. Yao, K. Y. Yung, M. Hajj-Hassan, M. C. Cheung, V. P. Chodavarapu and F. V. Bright, *Sens. Actuators, B*, 2011, **157**, 408-416.
192. C. Preininger, I. Klimant and O. S. Wolfbeis, *Anal. Chem.*, 1994, **66**, 1841-1846.
193. Z. Rosenzweig and R. Kopelman, *Anal. Chem.*, 1995, **67**, 2650-2654.

194. A. Mills and M. Thomas, *Analyst*, 1997, **122**, 63-68.
195. Y. Amao and I. Okura, *Polym. J.*, 2000, **32**, 452-455.
196. A. M. Morin, W. Xu, J. N. Demas and B. A. DeGraff, *J. Fluoresc.*, 2000, **10**, 7-12.
197. H. He, R. J. Fraatz, M. J. P. Leiner, M. M. Rehn and J. K. Tusa, *Sens. Actuators, B*, 1995, **29**, 246-250.
198. C.-M. Chan, M.-Y. Chan, M. Zhang, W. Lo and K.-Y. Wong, *Analyst*, 1999, **124**, 691-694.
199. M. M. F. Choi and D. Xiao, *Anal. Chim. Acta*, 1999, **387**, 197-205.
200. A. K. McEvoy, C. McDonagh and B. D. MacCraith, *J. Sol-Gel Sci. Technol.*, 1997, **8**, 1121-1125.
201. B. D. MacCraith, C. M. McDonagh, G. O'Keefe, E. T. Keyes, J. G. Vos, B. O'Kelly and J. F. McGilp, *Analyst*, 1993, **118**, 385-388.
202. C. McDonagh, C. Kolle, A. K. McEvoy, D. L. Dowling, A. A. Cafolla, S. J. Cullen and B. D. MacCraith, *Sens. Actuators, B*, 2001, **74**, 124-130.
203. Y. Tang, E. C. Tehan, Z. Tao and F. V. Bright, *Anal. Chem.*, 2003, **75**, 2407-2413.
204. I. Klimant, F. Ruckruh, G. Liebsch, C. Stangelmayer and O. S. Wolfbeis, *Mikrochim. Acta*, 1999, **131**, 35-46.
205. X. Chen, Z. Zhong, Z. Li, Y. Jiang, X. Wang and K. Wong, *Sens. Actuators, B*, 2002, **87**, 233-238.
206. A. Apostolidis, I. Klimant, D. Andrzejewski and O. S. Wolfbeis, *J. Comb. Chem.*, 2004, **6**, 325-331.
207. K. Ertekin, S. Kocak, M. Sabih Ozer, S. Aycan and B. Cetinkaya, *Talanta*, 2003, **61**, 573-579.
208. G. Di Marco, M. Lanza and S. Campagna, *Adv. Mater.*, 1995, **7**, 468-471.
209. B. Meier, T. Werner, I. Klimant and O. S. Wolfbeis, *Sens. Actuators, B*, 1995, **29**, 240-245.
210. P. Zhang, J. Guo, Y. Wang and W. Pang, *Mater. Lett.*, 2002, **53**, 400-405.
211. M. Ahmad, N. Mohammad and J. Abdullah, *J. Non-Cryst. Solids*, 2001, **290**, 86-91.
212. D. Garcia-Fresnadillo, M. D. Marazuela, M. C. Moreno-Bondi and G. Orellana, *Langmuir*, 1999, **15**, 6451-6459.
213. N. Velasco-Garcia, M. J. Valencia-Gonzalez and M. E. Diaz-Garcia, *Analyst*, 1997, **122**, 1405-1410.
214. J. Ji, N. Rosenzweig, I. Jones and Z. Rosenzweig, *J. Biomed. Opt.*, 2002, **7**, 404-409.
215. J. Ji, N. Rosenzweig, I. Jones and Z. Rosenzweig, *Anal. Chem.*, 2001, **73**, 3521-3527.
216. G. Di Marco, M. Lanza, M. Pieruccini and S. Campagna, *Adv. Mater.*, 1996, **8**, 576-580.
217. K. K.-W. Lo, S. P.-Y. Li and K. Y. Zhang, *New J. Chem.*, 2011, **35**, 265-287.
218. M.-L. Ho, J.-C. Wang, T.-Y. Wang, C.-Y. Lin, J. F. Zhu, Y.-A. Chen and T.-C. Chen, *Sens. Actuators, B*, 2014, **190**, 479-485.
219. G. Di Marco, M. Lanza, A. Mamo, I. Stefio, C. Di Pietro, G. Romeo and S. Campagna, *Anal. Chem.*, 1998, **70**, 5019-5023.
220. Y. Amao, Y. Ishikawa and I. Okura, *Anal. Chim. Acta*, 2001, **445**, 177-182.
221. L. Huynh, Z. Wang, J. Yang, V. Stoeva, A. Lough, I. Manners and M. A. Winnik, *Chem. Mater.*, 2005, **17**, 4765-4773.
222. P. Steunenbergh, A. Ruggi, N. S. van den Berg, T. Buckle, J. Kuil, F. W. B. van Leeuwen and A. H. Velders, *Inorg. Chem.*, 2012, **51**, 2105-2114.
223. C. S. K. Mak, D. Pentlehner, M. Stich, O. S. Wolfbeis, W. K. Chan and H. Yersin, *Chem. Mater.*, 2009, **21**, 2173-2175.
224. S. M. Borisov and I. Klimant, *Anal. Chem.*, 2007, **79**, 7501-7509.
225. B. H. Leavens, C. Trindle, M. Sabat, Z. Altun, J. Demas and B. A. DeGraff, *J. Fluoresc.*, 2012, **22**, 163-174.
226. P. Jin, Z. Guo, J. Chu, J. Tan, S. Zhang and W. Zhu, *Industrial & Engineering Chemistry Research*, 2013, **52**, 3980-3987.
227. S. M. Borisov and I. Klimant, *Mikrochim. Acta*, 2009, **164**, 7-15.
228. A. L. Medina-Castillo, J. F. Fernandez-Sanchez, C. Klein, M. K. Nazeeruddin, A. Segura-Carretero, A. Fernandez-Gutierrez, M. Graetzel and U. E. Spichiger-Keller, *Analyst*, 2007, **132**, 929-936.
229. B. Carlson, B. E. Eichinger, W. Kaminsky and G. D. Phelan, *Sens. Actuators, B*, 2010, **145**, 278-284.
230. A. Ruggi, M. Berenguel Alonso, D. N. Reinhoudt and A. H. Velders, *Chem. Commun.*, 2010, **46**, 6726-6728.
231. M. C. DeRosa, D. J. Hodgson, G. D. Enright, B. Dawson, C. E. B. Evans and R. J. Crutchley, *J. Am. Chem. Soc.*, 2004, **126**, 7619-7626.
232. A. Habibagahi, Y. Mébarki, Y. Sultan, G. P. A. Yap and R. J. Crutchley, *ACS Appl. Mater. Interfaces*, 2009, **1**, 1785-1792.
233. Y.-K. Peng, C.-W. Lai, C.-L. Liu, H.-C. Chen, Y.-H. Hsiao, W.-L. Liu, K.-C. Tang, Y. Chi, J.-K. Hsiao, K.-E. Lim, H.-E. Liao, J.-J. Shyue and P.-T. Chou, *ACS Nano*, 2011, **5**, 4177-4187.
234. M. C. DeRosa, P. J. Mosher, G. P. A. Yap, K. S. Focsaneanu, R. J. Crutchley and C. E. B. Evans, *Inorg. Chem.*, 2003, **42**, 4864-4872.
235. M.-L. Ho, Y.-A. Chen, T.-C. Chen, P.-J. Chang, Y.-P. Yu, K.-Y. Cheng, C.-H. Shih, G.-H. Lee and H.-S. Sheu, *Dalton Transactions*, 2012, **41**, 2592-2600.
236. M. Marin-Suárez, B. F. E. Curchod, I. Tavernelli, U. Rothlisberger, R. Scopelliti, I. Jung, D. Di Censo, M. Grätzel, J. F. Fernández-Sánchez, A. Fernández-Gutiérrez, M. K. Nazeeruddin and E. Baranoff, *Chem. Mater.*, 2012, **24**, 2330-2338.
237. L. H. Fischer, M. I. J. Stich, O. S. Wolfbeis, N. Tian, E. Holder and M. Schaferling, *Chem. Eur. J.*, 2009, **15**, 10857-10863.

238. E. M. Kober, J. L. Marshall, W. J. Dressick, B. P. Sullivan, J. V. Caspar and T. J. Meyer, *Inorg. Chem.*, 1985, **24**, 2755-2763.
239. S. B. Bambot, G. Rao, M. Romauld, G. M. Carter, J. Sipior, E. Terpetchnig and J. R. Lakowicz, *Biosens. Bioelectron.*, 1995, **10**, 643-652.
240. W. Xu, K. A. Kneas, J. N. Demas and B. A. DeGraff, *Anal. Chem.*, 1996, **68**, 2605-2609.
241. L. Sacksteder, J. N. Demas and B. A. DeGraff, *Anal. Chem.*, 1993, **65**, 3480-3483.
242. L. Sacksteder, M. Lee, J. N. Demas and B. A. DeGraff, *J. Am. Chem. Soc.*, 1993, **115**, 8230-8238.
243. K. A. Kneas, W. Xu, J. N. Demas, B. A. DeGraff and A. P. Zipp, *J. Fluoresc.*, 1998, **8**, 295-300.
244. Y. Shen, B. P. Maliwal and J. R. Lakowicz, *J. Fluoresc.*, 2001, **11**, 315-318.
245. T. M. McLean, J. L. Moody, M. R. Waterland and S. G. Telfer, *Inorg. Chem.*, 2012, **51**, 446-455.
246. C.-e. Wang, *J. Lumin.*, 2014, **145**, 531-538.
247. H. Hong, L. Zhu, A. Wang and H. Lu, *Spectrochim. Acta, Part A*, 2012, **98**, 466-473.
248. Y. Amao, I. Okura and T. Miyashita, *Bull. Chem. Soc. Jpn.*, 2000, **73**, 2663-2668.
249. Y. Amao, I. Okura and T. Miyashita, *Chem. Lett.*, 2000, **29**, 934-935.
250. Y. Li, *Spectrochim. Acta, Part A*, 2011, **79**, 356-360.
251. Q. Zuo, B. Li, L. Zhang, Y. Wang, Y. Liu, J. Zhang, Y. Chen and L. Guo, *J. Solid State Chem.*, 2010, **183**, 1715-1720.
252. S. Li and X. Zhao, *Synth. Met.*, 2011, **161**, 737-742.
253. N. Feng, J. Xie and D. Zhang, *Spectrochim. Acta, Part A*, 2010, **77**, 292-296.
254. Y. Amao, I. Okura and T. Miyashita, *Chem. Lett.*, 2000, **29**, 1286-1287.
255. Y. Amao, Y. Ishikawa, I. Okura and T. Miyashita, *Bull. Chem. Soc. Jpn.*, 2001, **74**, 2445-2449.
256. G. L. Law, R. Pal, L. O. Palsson, D. Parker and K. L. Wong, *Chem. Commun.*, 2009, 7321-7323.
257. S. Borisov and I. Klimant, *Anal. Bioanal. Chem.*, 2012, **404**, 2797-2806.
258. Y. Wang, B. Li, L. Zhang, Q. Zuo, P. Li, J. Zhang and Z. Su, *ChemPhysChem*, 2011, **12**, 349-355.
259. O. Burkhard and W. K. R. Barnikol, *Z. Naturforsch.*, 1985, **40B**, 1719.
260. B. W. Atwater, *J. Fluoresc.*, 1992, **2**, 237-246.
261. D. Eastwood and M. Gouterman, *J. Mol. Spectrosc.*, 1970, **35**, 359-375.
262. W. Rumsey, J. Vanderkooi and D. Wilson, *Science*, 1988, **241**, 1649-1651.
263. R. B. Beswick and C. W. Pitt, *Chem. Phys. Lett.*, 1988, **143**, 589-592.
264. J. Kavandi, J. Callis, M. Gouterman, G. Khalil, D. Wright, E. Green, D. Burns and B. McLachlan, *Rev. Sci. Instrum.*, 1990, **61**, 3340-3347.
265. A. K. Bansal, W. Holzer, A. Penzkofer and T. Tsuboi, *Chem. Phys.*, 2006, **330**, 118-129.
266. W. W.-S. Lee, K.-Y. Wong, X.-M. Li, Y.-B. Leung, C.-S. Chan and K. S. Chan, *J. Mater. Chem.*, 1993, **3**, 1031-1035.
267. S.-K. Lee and I. Okura, *Anal. Commun.*, 1997, **34**, 185-188.
268. Y. Amao, T. Miyashita and I. Okura, *J. Fluorine Chem.*, 2001, **107**, 101-106.
269. T. Mayr, S. M. Borisov, T. Abel, B. Enko, K. Waich, G. Mistlberger and I. Klimant, *Anal. Chem.*, 2009, **81**, 6541-6545.
270. S. M. Borisov, P. Lehner and I. Klimant, *Anal. Chim. Acta*, 2011, **690**, 108-115.
271. B. Zelelow, G. E. Khalil, G. Phelan, B. Carlson, M. Gouterman, J. B. Callis and L. R. Dalton, *Sens. Actuators, B*, 2003, **96**, 304-314.
272. G. E. Khalil, C. Costin, J. Crafton, G. Jones, S. Grenoble, M. Gouterman, J. B. Callis and L. R. Dalton, *Sens. Actuators, B*, 2004, **97**, 13-21.
273. G. Martin, C. James, D. Larry, K. Gamal, M. Youssef, R. C. Kevin and G. Michel, *Meas. Sci. Technol.*, 2004, **15**, 1986.
274. G. Khalil, M. Gouterman, S. Ching, C. Costin, L. Coyle, S. Gouin, E. Green, M. Sadilek, R. Wan and J. Yearyeen, *J. Porphyr. Phthalocya.*, 2002, **6**, 135-145.
275. S. M. Borisov, G. Nuss and I. Klimant, *Anal. Chem.*, 2008, **80**, 9435-9442.
276. S. M. Borisov, G. Nuss, W. Haas, R. Saf, M. Schmuck and I. Klimant, *J. Photochem. Photobiol., A*, 2009, **201**, 128-135.
277. S. M. Borisov, D. B. Papkovsky, G. V. Ponomarev, A. S. DeToma, R. Saf and I. Klimant, *J. Photochem. Photobiol., A*, 2009, **206**, 87-92.
278. D. B. Papkovsky, G. V. Ponomarev, W. Trettnak and P. O'Leary, *Anal. Chem.*, 1995, **67**, 4112-4117.
279. D. B. Papkovsky, *Sens. Actuators, B*, 1995, **29**, 213-218.
280. S. M. Borisov, G. Zenkl and I. Klimant, *ACS Appl. Mater. Interfaces*, 2010, **2**, 366-374.
281. O. S. Finikova, A. V. Cheprakov and S. A. Vinogradov, *J. Org. Chem.*, 2005, **70**, 9562-9572.
282. F. Niedermair, S. M. Borisov, G. Zenkl, O. T. Hofmann, H. r. Weber, R. Saf and I. Klimant, *Inorg. Chem.*, 2010, **49**, 9333-9342.
283. W. Wu, W. Wu, S. Ji, H. Guo, X. Wang and J. Zhao, *Dyes and Pigments*, 2011, **89**, 199-211.
284. K. Koren, S. M. Borisov, R. Saf and I. Klimant, *Eur. J. Inorg. Chem.*, 2011, **2011**, 1531-1534.
285. K. Koren, R. I. Dmitriev, S. M. Borisov, D. B. Papkovsky and I. Klimant, *ChemBioChem*, 2012, **13**, 1184-1190.
286. V. V. Vasil'ev and S. M. Borisov, *Sens. Actuators, B*, 2002, **82**, 272-276.

287. P. Gewehr and D. Delpy, *Med. Biol. Eng. Comput.*, 1993, **31**, 11-21.
288. T. C. O'Riordan, A. V. Zhdanov, G. V. Ponomarev and D. B. Papkovsky, *Anal. Chem.*, 2007, **79**, 9414-9419.
289. T. C. O'Riordan, K. Fitzgerald, G. V. Ponomarev, J. Mackrill, J. Hynes, C. Taylor and D. B. Papkovsky, *Am. J. Physiol. Reg. I.*, 2007, **292**, R1613-R1620.
290. Y. Will, J. Hynes, V. I. Ogurtsov and D. B. Papkovsky, *Nat. Protoc.*, 2006, **1**, 2563-2572.
291. R. D. Shonat, K. N. Richmond and P. C. Johnson, *Rev. Sci. Instrum.*, 1995, **66**, 5075-5084.
292. L.-W. Lo, C. J. Koch and D. F. Wilson, *Anal. Biochem.*, 1996, **236**, 153-160.
293. T. Saito, N. Asakura, T. Kamachi and I. Okura, *J. Porphyr. Phthalocya.*, 2007, **11**, 160-164.
294. Y. Amao, K. Asai and I. Okura, *Anal. Commun.*, 1999, **36**, 179-180.
295. Y. Amao and I. Okura, *Analyst*, 2000, **125**, 1601-1604.
296. Y. Amao, K. Asai and I. Okura, *J. Porphyr. Phthalocya.*, 2000, **4**, 179-184.
297. A. Fercher, G. V. Ponomarev, D. Yashunski and D. B. Papkovsky, *Anal. Bioanal. Chem.*, 2010, **396**, 1793-1803.
298. R. I. Dmitriev, A. V. Zhdanov, G. V. Ponomarev, D. V. Yashunski and D. B. Papkovsky, *Anal. Biochem.*, 2010, **398**, 24-33.
299. M. Obata, Y. Tanaka, N. Araki, S. Hirohara, S. Yano, K. Mitsuo, K. Asai, M. Harada, T. Kakuchi and C. Ohtsuki, *J. Polym. Sci., Part A: Polym. Chem.*, 2005, **43**, 2997-3006.
300. Y. Q. Tian, B. R. Shumway, A. C. Youngbull, Y. Z. Li, A. K. Y. Jen, R. H. Johnson and D. R. Meldrum, *Sens. Actuators, B*, 2010, **147**, 714-722.
301. Y. Tian, B. R. Shumway and D. R. Meldrum, *Chem. Mater.*, 2010, **22**, 2069-2078.
302. H. Lu, Y. Jin, Y. Tian, W. Zhang, M. R. Holl and D. R. Meldrum, *J. Mater. Chem.*, 2011.
303. Y. Tian, B. R. Shumway, W. Gao, C. Youngbull, M. R. Holl, R. H. Johnson and D. R. Meldrum, *Sens. Actuators, B*, 2010, **150**, 579-587.
304. K. Koren, S. M. Borisov and I. Klimant, *Sens. Actuators, B*, 2012, **169**, 173-181.
305. R. P. Briñas, T. Troxler, R. M. Hochstrasser and S. A. Vinogradov, *J. Am. Chem. Soc.*, 2005, **127**, 11851-11862.
306. S. Sakadzic, E. Roussakis, M. A. Yaseen, E. T. Mandeville, V. J. Srinivasan, K. Arai, S. Ruvinskaya, A. Devor, E. H. Lo, S. A. Vinogradov and D. A. Boas, *Nat. Methods*, 2010, **7**, 755-759.
307. O. S. Finikova, A. Y. Lebedev, A. Aprelev, T. Troxler, F. Gao, C. Garnacho, S. Muro, R. M. Hochstrasser and S. A. Vinogradov, *ChemPhysChem*, 2008, **9**, 1673-1679.
308. O. S. Finikova, T. Troxler, A. Senes, W. F. DeGrado, R. M. Hochstrasser and S. A. Vinogradov, *J. Phys. Chem. A*, 2007, **111**, 6977-6990.
309. J. Lecoq, A. Parpaleix, E. Roussakis, M. Ducros, Y. G. Houssen, S. A. Vinogradov and S. Charpak, *Nat Med*, 2011, **17**, 893-898.
310. R. C. Evans, P. Douglas, J. A. G. Williams and D. L. Rochester, *J. Fluoresc.*, 2006, **16**, 201-206.
311. S. R. Ricketts and P. Douglas, *Sens. Actuators, B*, 2008, **135**, 46-51.
312. X. D. Wang, X. Chen, Z. X. Xie and X. R. Wang, *Angew. Chem. Int. Ed.*, 2008, **47**, 7450-7453.
313. X. D. Wang, R. J. Meier, M. Link and O. S. Wolfbeis, *Angew. Chem. Int. Ed.*, 2010, **49**, 4907-4909.
314. R. A. Potyrailo and G. M. Hieftje, *Anal. Chim. Acta*, 1998, **370**, 1-8.
315. S.-K. Lee and I. Okura, *Anal. Chim. Acta*, 1997, **342**, 181-188.
316. S. K. Lee and I. Okura, *Analyst*, 1997, **122**, 81-84.
317. I. Klimant, M. Kühn, R. N. Glud and G. Holst, *Sens. Actuators, B*, 1997, **38**, 29-37.
318. Y. Amao, T. Miyashita and I. Okura, *React. Funct. Polym.*, 2001, **47**, 49-54.
319. Y. Amao, K. Asai, T. Miyashita and I. Okura, *Polym. Adv. Technol.*, 2000, **11**, 705-709.
320. Y. Amao, T. Miyashita and I. Okura, *Analyst*, 2000, **125**, 871-875.
321. Y. Amao, K. Asai, I. Okura, H. Shinohara and H. Nishide, *Analyst*, 2000, **125**, 1911-1914.
322. R. N. Gillanders, M. C. Tedford, P. J. Crilly and R. T. Bailey, *Anal. Chim. Acta*, 2004, **502**, 1-6.
323. G. DiMarco and M. Lanza, *Sens. Actuators, B*, 2000, **63**, 42-48.
324. P. Douglas and K. Eaton, *Sens. Actuators, B*, 2002, **82**, 200-208.
325. X. Lu, I. Manners and M. A. Winnik, *Macromolecules*, 2001, **34**, 1917-1927.
326. Y. E. L. Koo, Y. F. Cao, R. Kopelman, S. M. Koo, M. Brasuel and M. A. Philbert, *Anal. Chem.*, 2004, **76**, 2498-2505.
327. Y. Amao, Y. Tabuchi, Y. Yamashita and K. Kimura, *Eur. Polym. J.*, 2002, **38**, 675-681.
328. A. Sheila Holmes-Smith, A. Hamill, M. Campbell and M. Uttamlal, *Analyst*, 1999, **124**, 1463-1466.
329. A. Mills and A. Lepre, *Anal. Chem.*, 1997, **69**, 4653-4659.
330. Z. Pang, X. Gu, A. Yekta, Z. Masoumi, J. B. Coll, M. A. Winnik and I. Manners, *Adv. Mater.*, 1996, **8**, 768-771.
331. N. B. Borchert, G. V. Ponomarev, J. P. Kerry and D. B. Papkovsky, *Anal. Chem.*, 2010, **83**, 18-22.
332. P. Hartmann and W. Trettnak, *Anal. Chem.*, 1996, **68**, 2615-2620.
333. C. Kolle, W. Gruber, W. Trettnak, K. Biebernik, C. Dolezal, F. Reiningger and P. O'Leary, *Sens. Actuators, B*, 1997, **38**, 141-149.
334. M. Trinkel, W. Trettnak and C. Kolle, *Quim. Anal.*, 2000, **19**, 112-117.
335. K. Öge, T. Avarmaa, A. Suisalu and R. Jaaniso, *Sens. Actuators, B*, 2005, **106**, 424-430.
336. T.-S. Yeh, C.-S. Chu and Y.-L. Lo, *Sens. Actuators, B*, 2006, **119**, 701-707.

337. C.-S. Chu, Y.-L. Lo and T.-W. Sung, *Talanta*, 2010, **82**, 1044-1051.
338. C.-S. Chu and Y.-L. Lo, *Sens. Actuators, B*, 2007, **124**, 376-382.
339. C. S. Chu and Y. L. Lo, *Sens. Actuators, B*, 2011, **155**, 53-57.
340. Y. Amao, T. Miyashita and I. Okura, *J. Porphy. Phthalocya.*, 2001, **5**, 433-438.
341. Y. Amao, K. Asai, K. Miyakawa and I. Okura, *J. Porphy. Phthalocya.*, 2000, **4**, 19-22.
342. Y. Amao, K. Miyakawa and I. Okura, *J. Mater. Chem.*, 2000, **10**, 305-308.
343. A. J. Twarowski and L. Good, *J. Phys. Chem.*, 1987, **91**, 5252-5257.
344. D. B. Papkovsky, J. Olah, I. V. Troyanovsky, N. A. Sadovsky, V. D. Romyantseva, A. F. Mironov, A. I. Yaropolov and A. P. Savitsky, *Biosens. Bioelectron.*, 1992, **7**, 199-206.
345. M. Mitsuishi, H. Tanaka, M. Obata and T. Miyashita, *Langmuir*, 2010, **26**, 15117-15120.
346. Y. Amao, K. Asai and I. Okura, *Anal. Chim. Acta*, 2000, **407**, 41-44.
347. Y. M. Liu, R. Pereiro-Garcia, M. J. Valencia-Gonzalez, M. E. Diaz-Garcia and A. Sanz-Medel, *Anal. Chem.*, 1994, **66**, 836-840.
348. F. Alava-Moreno, M. J. Valencia-González, A. Sanz-Medel and M. E. Díaz-García, *Analyst*, 1997, **122**, 807-810.
349. J. M. Costa-Fernández, M. E. Diaz-García and A. Sanz-Medel, *Anal. Chim. Acta*, 1998, **360**, 17-26.
350. J. M. Costa-Fernández, N. Bordel, J. C. Campo, F. J. Ferrero, M. A. Pérez and A. Sanz-Medel, *Mikrochim. Acta*, 2000, **134**, 145-152.
351. J. Díaz-García, J. M. Costa-Fernández, N. Bordel-García and A. Sanz-Medel, *Anal. Chim. Acta*, 2001, **429**, 55-64.
352. A. Mills, A. Lepre, B. R. C. Theobald, E. Slade and B. A. Murrer, *Anal. Chem.*, 1997, **69**, 2842-2847.
353. A. Mills, C. Tommons, R. T. Bailey, P. Crilly and M. C. Tedford, *Anal. Chim. Acta*, 2011, **702**, 269-273.
354. H. Jiang, H. Yang, F. Liu and Y. Li, *J. Lumin.*, 2012, **132**, 198-204.
355. C. S. Smith and K. R. Mann, *Chem. Mater.*, 2009, **21**, 5042-5049.
356. C. S. Smith, C. W. Branham, B. J. Marquardt and K. R. Mann, *J. Am. Chem. Soc.*, 2010, **132**, 14079-14085.
357. C. Wen, G. Tao, X. Xu, X. Feng and R. Luo, *Spectrochim. Acta, Part A*, 2011, **79**, 1345-1351.
358. C. S. Smith and K. R. Mann, *J. Am. Chem. Soc.*, 2012, **134**, 8786-8789.
359. J. Jia, Y. Tian and Z. Li, *Synth. Met.*, 2011, **161**, 1377-1382.
360. W. W. S. Lee, K. Y. Wong and X. M. Li, *Anal. Chem.*, 1993, **65**, 255-258.
361. C. Liu, X. Song, X. Rao, Y. Xing, Z. Wang, J. Zhao and J. Qiu, *Dyes and Pigments*, 2014, **101**, 85-92.
362. A. Vogler and H. Kunkely, in *Top. Curr. Chem.*, ed. H. Yersin, Springer Berlin / Heidelberg, 2001, vol. 213, pp. 143-182.
363. M. T. Miller and T. B. Karpishin, *Sens. Actuators, B*, 1999, **61**, 222-224.
364. E. Vander Donckt, B. Camerman, R. Herne and R. Vandeloise, *Sens. Actuators, B*, 1996, **32**, 121-127.
365. X.-M. Li and K.-Y. Wong, *Anal. Chim. Acta*, 1992, **262**, 27-32.
366. Y. S. Xia, T. L. Zhang, X. L. Diao and C. Q. Zhu, *Chem. Lett.*, 2007, **36**, 242-243.
367. E. D. Lee, T. C. Werner and W. R. Seitz, *Anal. Chem.*, 1987, **59**, 279-283.
368. Y. Kostov, P. Harms, R. S. Pilato and G. Rao, *Analyst*, 2000, **125**, 1175-1178.
369. Y. Kostov and G. Rao, *Sens. Actuators, B*, 2003, **90**, 139-142.
370. Y. Kostov, Z. Gryczynski and G. Rao, *Anal. Chem.*, 2002, **74**, 2167-2171.
371. Y. Liu, H. Guo and J. Zhao, *Chem. Commun.*, 2011, **47**, 11471-11473.
372. W. Wu, W. Wu, S. Ji, H. Guo, P. Song, K. Han, L. Chi, J. Shao and J. Zhao, *J. Mater. Chem.*, 2010, **20**, 9775-9786.
373. X. Liu, W. Sun, L. Zou, Z. Xie, X. Li, C. Lu, L. Wang and Y. Cheng, *Dalton Transactions*, 2012, **41**, 1312-1319.
374. C. A. Parker and W. J. Barnes, *Analyst*, 1957, **82**, 606-618.
375. A. Pfister, G. Zhang, J. Zareno, A. F. Horwitz and C. L. Fraser, *ACS Nano*, 2008, **2**, 1252-1258.
376. H. Xiang, L. Zhou, Y. Feng, J. Cheng, D. Wu and X. Zhou, *Inorg. Chem.*, 2012, **51**, 5208-5212.
377. G. Zhang, G. M. Palmer, M. W. Dewhirst and C. L. Fraser, *Nat. Mater.*, 2009, **8**, 747-751.
378. H. D. Hendricks, *Mol. Phys.*, 1971, **20**, 189-191.
379. M. Anni and R. Rella, *J. Phys. Chem. B*, 2009, **114**, 1559-1561.
380. M. R. Ayers and A. J. Hunt, *J. Non-Cryst. Solids*, 1998, **225**, 343-347.
381. Y. Zhang and D. T. Johnson, *Anal. Chim. Acta*, 2004, **511**, 333-337.
382. R. Ghosh, *Appl. Phys. Lett.*, 1999, **75**, 2885.
383. R. N. Ghosh, D. Osborn and G. L. Baker, *Proceedings of IEEE Sensors*, 2003, **2**, 807-808.
384. R. N. Ghosh, P. A. Askeland, S. Kramer and R. Loloee, *Appl. Phys. Lett.*, 2011, **98**, 221103-221103-221103.
385. J. T. Remillard, B. D. Poindexter and W. H. Weber, *Appl. Opt.*, 1997, **36**, 3699-3707.
386. B. Adhikari and S. Majumdar, *Prog. Polym. Sci.*, 2004, **29**, 699-766.
387. G. Korotcenkov, in *Handbook of Gas Sensor Materials*, Springer New York, 2014, pp. 209-222.
388. M. I. J. Stich, L. H. Fischer and O. S. Wolfbeis, *Chem. Soc. Rev.*, 2010, **39**, 3102-3114.
389. M. Cox and B. Dunn, *J. Polym. Sci., Part A: Polym. Chem.*, 1986, **24**, 621-636.
390. M. E. Cox and B. Dunn, *J. Polym. Sci., Part A: Polym. Chem.*, 1986, **24**, 2395-2400.
391. G. Shaw, *Trans. Faraday Soc.*, 1967, **63**, 2181-2189.

392. J. W. Parker and M. E. Cox, *J. Polym. Sci., Part A: Polym. Chem.*, 1988, **26**, 1179-1188.
393. M. Kubin and P. Spacek, *Coll. Czechoslov. Chem. Commun.*, 1965, **30**, 3294.
394. D. Badocco and P. Pastore, *Anal. Chem.*, 2008, **80**, 2091-2096.
395. D. Badocco, A. Mondin and P. Pastore, *Sens. Actuators, B*, 2012, **163**, 165-170.
396. J. Brandrup, E. H. Immergut and E. A. Grulke, *Polymer handbook*, Wiley, New York, 1999, vols. 1 and 2.
397. G. J. Mohr, T. Werner, I. Oehme, C. Preininger, I. Klimant, B. Kovacs and O. S. Wolfbeis, *Adv. Mater.*, 1997, **9**, 1108-1113.
398. E. R. Carraway, J. N. Demas and B. A. DeGraff, *Langmuir*, 1991, **7**, 2991-2998.
399. S. B. Bambot, R. Holavanahali, J. R. Lakowicz, G. M. Carter and G. Rao, *Biotechnol. Bioeng.*, 1994, **43**, 1139-1145.
400. M. E. Köse, R. J. Crutchley, M. C. DeRosa, N. Ananthkrishnan, J. R. Reynolds and K. S. Schanze, *Langmuir*, 2005, **21**, 8255-8262.
401. K. Eaton and P. Douglas, *Sens. Actuators, B*, 2002, **82**, 94-104.
402. X. Yang, L. Peng, L. Yuan, P. Teng, F. Tian, L. Li and S. Luo, *Opt. Commun.*, 2011, **284**, 3462-3466.
403. A. Mills and M. D. Thomas, *Analyst*, 1998, **123**, 1135-1140.
404. J. Brandrup, E. Immergut and E. Grulke, in *Polymer handbook*, John Wiley & Sons, New York, 1989, pp. 435-449.
405. D. B. Papkovsky, G. J. Mohr and O. S. Wolfbeis, *Anal. Chim. Acta*, 1997, **337**, 201-205.
406. G. Lashkov and A. Kavtrev, *Polymer Science U.S.S.R.*, 1986, **28**, 1885-1891.
407. K. A. Kneas, W. Xu, J. N. Demas and B. A. Degraff, *Appl. Spectrosc.*, 1997, **51**, 1346-1351.
408. K. Koren, L. Hutter, B. Enko, A. Pein, S. M. Borisov and I. Klimant, *Sens. Actuators, B*, 2013, **176**, 344-350.
409. W. Trettnak, C. Kolle, F. Reininger, C. Dolezal and P. O'Leary, *Sens. Actuators, B*, 1996, **36**, 506-512.
410. R. Ruffolo, C. E. B. Evans, X.-H. Liu, Y. Ni, Z. Pang, P. Park, A. R. McWilliams, X. Gu, X. Lu, A. Yekta, M. A. Winnik and I. Manners, *Anal. Chem.*, 2000, **72**, 1894-1904.
411. C. Kelly, C. Toncelli, J. Kerry and D. B. Papkovsky, *Journal of Materials Chemistry C*, 2014, DOI: 10.1039/C1033TC32529F.
412. H. N. Kim, Z. Guo, W. Zhu, J. Yoon and H. Tian, *Chem. Soc. Rev.*, 2011, **40**, 79-93.
413. D. Badocco, A. Mondin, P. Pastore, S. Voltolina and S. Gross, *Anal. Chim. Acta*, 2008, **627**, 239-246.
414. S. M. Borisov and O. S. Wolfbeis, *Anal. Chem.*, 2006, **78**, 5094-5101.
415. S. M. Borisov, A. S. Vasylevska, C. Krause and O. S. Wolfbeis, *Adv. Funct. Mater.*, 2006, **16**, 1536-1542.
416. M. I. J. Stich, M. Schaeferling and O. S. Wolfbeis, *Adv. Mater.*, 2009, **21**, 2216-2220.
417. R. Shah, S. Margerum and M. Gold, *Proc. SPIE*, 1988, **906**, 65-73.
418. P. Nowak-Sliwinska, P. uper, H. van den Bergh, Wagni and G. res, *CHIMIA International Journal for Chemistry*, 2011, **65**, 691-695.
419. K. Pospiskova, I. Safarik, M. Sebela and G. Kuncova, *Mikrochim. Acta*, 2013, **180**, 311-318.
420. P. Schrenkhammer and O. S. Wolfbeis, *Biosens. Bioelectron.*, 2008, **24**, 994-999.
421. L. H. Fischer, C. Karakus, R. J. Meier, N. Risch, O. S. Wolfbeis, E. Holder and M. Schäferling, *Chem. Eur. J.*, 2012, **18**, 15706-15713.
422. A. S. Kocincová, S. Nagl, S. Arain, C. Krause, S. M. Borisov, M. Arnold and O. S. Wolfbeis, *Biotechnol. Bioeng.*, 2008, **100**, 430-438.
423. G. Zhan, D. B. Henthorn and K. Chang-Soo, *IEEE Sensors*, 2010, 79-82, DOI: 10.1109/ICSENS.2010.5690839.
424. D. P. O'Neal, M. A. Meledeo, J. R. Davis, B. L. Ibey, V. A. Gant, M. V. Pishko and G. L. Cote, *Sensors Journal, IEEE*, 2004, **4**, 728-734.
425. J. F. Lovell, A. Roxin, K. K. Ng, Q. Qi, J. D. McMullen, R. S. DaCosta and G. Zheng, *Biomacromolecules*, 2011, **12**, 3115-3118.
426. X.-D. Wang, T.-Y. Zhou, X. Chen, K.-Y. Wong and X.-R. Wang, *Sens. Actuators, B*, 2008, **129**, 866-873.
427. A. Habibagahi, Y. Mébarki, Y. Sultan and R. J. Crutchley, *J. Photochem. Photobiol., A*, 2011, **225**, 88-94.
428. M. Marín-Suárez, M. Arias-Martos, T. Galeano-Díaz, J. Fernández-Sánchez and A. Fernández-Gutiérrez, *Mikrochim. Acta*, 2013, DOI: 10.1007/s00604-00013-01054-z.
429. Y. Amao, K. Asai, T. Miyashita and I. Okura, *Anal. Commun.*, 1999, **36**, 367-369.
430. Y. Amao, T. Miyashita and I. Okura, *Anal. Chim. Acta*, 2000, **421**, 167-174.
431. E. Puklin, B. Carlson, S. Gouin, C. Costin, E. Green, S. Ponomarev, H. Tanji and M. Gouterman, *J. Appl. Polym. Sci.*, 2000, **77**, 2795-2804.
432. O. Oter, K. Ertekin, O. Dayan and B. Cetinkaya, *J. Fluoresc.*, 2008, **18**, 269-276.
433. C. Hirel, O. Oter, A. G. Gürek, K. Ertekin, E. Önal and S. Z. Topal, *J. Porphyr. Phthalocya.*, 2013, **17**, 431-439.
434. M. Kaneko and S. Hayakawa, *J. Macromol. Sci., Chem*, 1988, **25**, 1255-1261.
435. T. Ishiji, K. Kudo and Kaneko, *Sens. Actuators, B*, 1994, **22**, 205-210.
436. K. Stubenrauch, M. Sandholzer, F. Niedermair, K. Waich, T. Mayr, I. Klimant, G. Trimmel and C. Slugove, *Eur. Polym. J.*, 2008, **44**, 2558-2566.
437. L. S. Egan, M. A. Winnik and M. D. Croucher, *Langmuir*, 1988, **4**, 438-445.

438. X.-L. Qi, S.-Y. Liu, R.-B. Lin, P.-Q. Liao, J.-W. Ye, Z. Lai, Y. Guan, X.-N. Cheng, J.-P. Zhang and X.-M. Chen, *Chem. Commun.*, 2013, **49**, 6864-6866.
439. G. Liebsch, I. Klimant, B. Frank, G. Holst and O. S. Wolfbeis, *Appl. Spectrosc.*, 2000, **54**, 548-559.
440. E. Schmälzlin, J. T. van Dongen, I. Klimant, B. Marmodee, M. Steup, J. Fisahn, P. Geigenberger and H. G. Lohmannsröben, *Biophys. J.*, 2005, **89**, 1339-1345.
441. A. Bizzarri, H. Koehler, M. Cajlakovic, A. Pasic, L. Schaupp, I. Klimant and V. Ribitsch, *Anal. Chim. Acta*, 2006, **573**, 48-56.
442. B. P. H. Schaffar and O. S. Wolfbeis, *Proc. SPIE*, 1989, **990**, 122-129.
443. P. S. Grant and M. J. McShane, *Sensors Journal, IEEE*, 2003, **3**, 139-146.
444. D. A. Chang-Yen, A. Badardeen and B. K. Gale, *Sens. Actuators, B*, 2007, **120**, 426-433.
445. K. B. Guice, M. E. Caldorera and M. J. McShane, *J. Biomed. Opt.*, 2005, **10**, 064031-064031.
446. R. N. Gillanders, O. V. Arzhakova, A. Hempel, A. Dolgova, J. P. Kerry, L. M. Yarysheva, N. F. Bakeev, A. L. Volynskii and D. B. Papkovsky, *Anal. Chem.*, 2010, **82**, 466-468.
447. P. C. A. Jerónimo, A. N. Araújo and M. Conceição B.S.M. Montenegro, *Talanta*, 2007, **72**, 13-27.
448. G. T. John, I. Klimant, C. Wittmann and E. Heinzle, *Biotechnol. Bioeng.*, 2003, **81**, 829-836.
449. P. Hartmann, M. J. P. Leiner and M. E. Lippitsch, *J. Fluoresc.*, 1994, **4**, 327-330.
450. G. A. Holst, T. Köster, E. Voges and D. W. Lübbers, *Sens. Actuators, B*, 1995, **29**, 231-239.
451. M. Ogawa, T. Nakamura, J.-i. Mori and K. Kuroda, *J. Phys. Chem. B*, 2000, **104**, 8554-8556.
452. H. Zhang, Y. Sun, K. Ye, P. Zhang and Y. Wang, *J. Mater. Chem.*, 2005, **15**, 3181-3186.
453. M. Fang, Y. Wang, P. Zhang, S. Li and R. Xu, *J. Lumin.*, 2000, **91**, 67-70.
454. B. Wang, L. Zhang, B. Li, Y. Li, Y. Shi and T. Shi, *Sens. Actuators, B*, 2014, **190**, 93-100.
455. Y. Wang, B. Li, L. Zhang and H. Song, *Langmuir*, 2013, **29**, 1273-1279.
456. A. Čeklovský and S. Takagi, *Cent. Eur. J. Chem.*, 2013, **11**, 1132-1136.
457. S. Z. Topal, K. Ertekin, D. Topkaya, S. Alp and B. Yenigul, *Mikrochim. Acta*, 2008, **161**, 209-216.
458. O. Oter, K. Ertekin and S. Derinkuyu, *Mater. Chem. Phys.*, 2009, **113**, 322-328.
459. A. Lobnik and O. S. Wolfbeis, *Analyst*, 1998, **123**, 2247-2250.
460. C. McDonagh, B. D. MacCraith and A. K. McEvoy, *Anal. Chem.*, 1998, **70**, 45-50.
461. M. T. Murtagh, M. R. Shahriari and M. Krihak, *Chem. Mater.*, 1998, **10**, 3862-3869.
462. B. J. Basu, *Sens. Actuators, B*, 2007, **123**, 568-577.
463. O. S. Wolfbeis, I. Klimant, T. Werner, C. Huber, U. Kosch, C. Krause, G. Neuraüter and A. Dürkop, *Sens. Actuators, B*, 1998, **51**, 17-24.
464. Z. Tao, E. C. Tehan, Y. Tang and F. V. Bright, *Anal. Chem.*, 2006, **78**, 1939-1945.
465. C.-S. Chu, *J. Lumin.*, 2013, **135**, 5-9.
466. R. M. Bukowski, R. Ciriminna, M. Pagliaro and F. V. Bright, *Anal. Chem.*, 2005, **77**, 2670-2672.
467. R. Ciriminna and M. Pagliaro, *Analyst*, 2009, **134**, 1531-1535.
468. Y. Xiong, J. Xu, D.-q. Zhu, C.-f. Duan and Y.-f. Guan, *J. Sol-Gel Sci. Technol.*, 2010, **53**, 441-447.
469. Y. Xiong, D. Zhu, S. Chen, H. Peng and Y. Guan, *J. Fluoresc.*, 2010, **20**, 269-274.
470. Y. Xiong, Z. Ye, J. Xu, Y. Zhu, C. Chen and Y. Guan, *Analyst*, 2013, **138**, 1819-1827.
471. V. S. Tripathi, G. Lakshminarayana and M. Nogami, *Sens. Actuators, B*, 2010, **147**, 741-747.
472. J. Estella, D. Wencel, J. P. Moore, M. Sourdain and C. McDonagh, *Anal. Chim. Acta*, 2010, **666**, 83-90.
473. B. Lei, B. Li, H. Zhang, S. Lu, Z. Zheng, W. Li and Y. Wang, *Adv. Funct. Mater.*, 2006, **16**, 1883-1891.
474. X. Lu and M. A. Winnik, *Chem. Mater.*, 2001, **13**, 3449-3463.
475. G. S. Vasylevska, S. M. Borisov, C. Krause and O. S. Wolfbeis, *Chem. Mater.*, 2006, **18**, 4609-4616.
476. A. Mills, A. Graham and C. O'Rourke, *Sens. Actuators, B*, 2014, **190**, 907-912.
477. N. Opitz and D. W. Lübbers, *Adv Exp Med Biol*, 1984, **169**, 899-905.
478. S. M. Borisov, T. Mayr, G. Mistlberger, K. Waich, K. Koren, P. Chojnacki and I. Klimant, *Talanta*, 2009, **79**, 1322-1330.
479. J. M. Kürner, I. Klimant, C. Krause, H. Preu, W. Kunz and O. S. Wolfbeis, *Bioconjugate Chem.*, 2001, **12**, 883-889.
480. A. Fercher, S. M. Borisov, A. V. Zhdanov, I. Klimant and D. B. Papkovsky, *ACS Nano*, 2011, **5**, 5499-5508.
481. E. Schmälzlin, B. Walz, I. Klimant, B. Schewe and H. G. Lohmannsröben, *Sens. Actuators, B*, 2006, **119**, 251-254.
482. X. D. Wang, H. H. Gorris, J. A. Stolwijk, R. J. Meier, D. B. M. Groegel, J. Wegener and O. S. Wolfbeis, *Chem. Sci.*, 2011, **2**, 901-906.
483. S. M. Borisov, T. Mayr and I. Klimant, *Anal. Chem.*, 2008, **80**, 573-582.
484. P. J. Cywinski, A. J. Moro, S. E. Stanca, C. Biskup and G. J. Mohr, *Sens. Actuators, B*, 2009, **135**, 472-477.
485. S. H. Im, G. E. Khalil, J. Callis, B. H. Ahn, M. Gouterman and Y. Xia, *Talanta*, 2005, **67**, 492-497.
486. X. D. Wang, T. Y. Zhou, X. H. Song, Y. Jiang, C. J. Yang and X. Chen, *J. Mater. Chem.*, 2011, **21**, 17651-17653.
487. H. A. Clark, M. Hoyer, M. A. Philbert and R. Kopelman, *Anal. Chem.*, 1999, **71**, 4831-4836.
488. Y. F. Cao, Y. E. L. Koo and R. Kopelman, *Analyst*, 2004, **129**, 745-750.
489. Y. E. Koo Lee, E. E. Ulbrich, G. Kim, H. Hah, C. Strollo, W. Fan, R. Gurjar, S. Koo and R. Kopelman, *Anal. Chem.*, 2010, **82**, 8446-8455.

490. M. P. Coogan, J. B. Court, V. L. Gray, A. J. Hayes, S. H. Lloyd, C. O. Millet, S. J. A. Pope and D. Lloyd, *Photoch. Photobio. Sci.*, 2010, **9**, 103-109.
491. H. Liu, H. Yang, X. Hao, H. Xu, Y. Lv, D. Xiao, H. Wang and Z. Tian, *Small*, 2013, **9**, 2639-2648.
492. T. C. O'Riordan, A. E. Soini and D. B. Papkovsky, *Anal. Chem.*, 2002, **74**, 5845-5850.
493. M. Burke, P. J. O'Sullivan, A. E. Soini, H. Berney and D. B. Papkovsky, *Anal. Biochem.*, 2003, **320**, 273-280.
494. K. P. McNamara and Z. Rosenzweig, *Anal. Chem.*, 1998, **70**, 4853-4859.
495. Z. Cheng and C. A. Aspinwall, *Analyst*, 2006, **131**, 236-243.
496. P. Chojnacki, G. Mistlberger and I. Klimant, *Angew. Chem. Int. Ed.*, 2007, **46**, 8850-8853.
497. S. H. Cheng, C. H. Lee, C. S. Yang, F. G. Tseng, C. Y. Mou and L. W. Lo, *J. Mater. Chem.*, 2009, **19**, 1252-1257.
498. B. B. Collier, S. Singh and M. McShane, *Analyst*, 2011, **136**, 962-967.
499. M. A. Acosta, P. Ymele-Leki, Y. V. Kostov and J. B. Leach, *Biomaterials*, 2009, **30**, 3068-3074.
500. H. E. Posch and O. S. Wolfbeis, *Sens. Actuators*, 1988, **15**, 77-83.
501. F. Navarro-Villoslada, G. Orellana, M. C. Moreno-Bondi, T. Vick, M. Driver, G. Hildebrand and K. Liefeyth, *Anal. Chem.*, 2001, **73**, 5150-5156.
502. O. S. Wolfbeis, B. Kovács, K. Goswami and S. M. Klainer, *Mikrochim. Acta*, 1998, **129**, 181-188.
503. D. B. Papkovsky, A. N. Ovchinnikov, V. I. Ogurtsov, G. V. Ponomarev and T. Korpela, *Sens. Actuators, B*, 1998, **51**, 137-145.
504. M. I. Gutiérrez, C. G. Martínez, D. García-Fresnadillo, A. M. Castro, G. Orellana, A. M. Braun and E. Oliveros, *J. Phys. Chem. A*, 2003, **107**, 3397-3403.
505. P. Ceroni, A. Y. Lebedev, E. Marchi, M. Yuan, T. V. Esipova, G. Bergamini, D. F. Wilson, T. M. Busch and S. A. Vinogradov, *Photoch. Photobio. Sci.*, 2011, **10**, 1056-1065.
506. R. S. Atkinson, D. R. G. Brimage, R. S. Davidson and E. Gray, *J. Chem. Soc., Perkin Trans. 1*, 1973, 960-964.
507. C. Ouannes and T. Wilson, *J. Am. Chem. Soc.*, 1968, **90**, 6527-6528.
508. I. B. C. Matheson and J. Lee, *J. Am. Chem. Soc.*, 1972, **94**, 3310-3313.
509. R. A. Ackerman, I. Rosenthal and J. N. Pitts, *J. Chem. Phys.*, 1971, **54**, 4960-4961.
510. J. P. Guillory and C. F. Cook, *Journal of Polymer Science: Polymer Chemistry Edition*, 1973, **11**, 1927-1937.
511. C. S. Foote, T. T. Fujimoto and Y. C. Chang, *Tetrahedron Lett.*, 1972, **13**, 45-48.
512. N. Hasty, P. B. Merkel, P. Radlick and D. R. Kearns, *Tetrahedron Lett.*, 1972, **13**, 49-52.
513. B. Enko, S. M. Borisov, J. Regensburger, W. Bäumlner, G. Gescheidt and I. Klimant, *J. Phys. Chem. A*, 2013, **117**, 8873-8882.
514. O. S. Wolfbeis, L. J. Weis, M. J. P. Leiner and W. E. Ziegler, *Anal. Chem.*, 1988, **60**, 2028-2030.
515. M. C. Moreno-Bondi, O. S. Wolfbeis, M. J. P. Leiner and B. P. H. Schaffar, *Anal. Chem.*, 1990, **62**, 2377-2380.
516. T. Mayr, I. Klimant, O. S. Wolfbeis and T. Werner, *Anal. Chim. Acta*, 2002, **462**, 1-10.
517. G. O'Keefe, B. D. MacCraith, A. K. McEvoy, C. M. McDonagh and J. F. McGilp, *Sens. Actuators, B*, 1995, **29**, 226-230.
518. V. I. Ogurtsov and D. B. Papkovsky, *Sens. Actuators, B*, 1998, **51**, 377-381.
519. W. Feng, N. Zhou, L. Chen and B. Li, *Journal of Optics*, 2013, **15**, 055502.
520. B. D. MacCraith, G. O'keeffe, C. McDonagh and A. McEvoy, *Electron. Lett.*, 1994, **30**, 888-889.
521. G. Holst, R. N. Glud, M. Kühl and I. Klimant, *Sens. Actuators, B*, 1997, **38**, 122-129.
522. K. W. Berndt and J. R. Lakowicz, *Anal. Biochem.*, 1992, **201**, 319-325.
523. H. Malak, J. W. Dobrucki, M. M. Malak and H. M. Swartz, *Biophys. J.*, 1998, **74**, A189-A189.
524. S. A. Vinogradov, M. A. Fernandez-Searra, B. W. Dugan and D. F. Wilson, *Rev. Sci. Instrum.*, 2001, **72**, 3396-3406.
525. R. J. Woods, S. Scypinski, L. J. C. Love and H. A. Ashworth, *Anal. Chem.*, 1984, **56**, 1395-1400.
526. R. M. Ballew and J. N. Demas, *Anal. Chem.*, 1989, **61**, 30-33.
527. S. J. Payne, J. N. Demas and B. A. DeGraff, *Appl. Spectrosc.*, 2009, **63**, 437-441.
528. A. Sharma and O. S. Wolfbeis, *Appl. Spectrosc.*, 1988, **42**, 1009-1011.
529. E. J. McLaurin, A. B. Greytak, M. G. Bawendi and D. G. Nocera, *J. Am. Chem. Soc.*, 2009, **131**, 12994-13001.
530. D. E. Achatz, R. J. Meier, L. H. Fischer and O. S. Wolfbeis, *Angew. Chem. Int. Ed.*, 2011, **50**, 260-263.
531. I. Gryczynski, Z. Gryczynski, J. R. Lakowicz and G. Rao, *Analyst*, 1999, **124**, 1041-1044.
532. L. Shen, M. Ratterman, D. Klotzkin and I. Papautsky, *Sens. Actuators, B*, 2011, **155**, 430-435.
533. O. S. Finikova, P. Chen, Z. Ou, K. M. Kadish and S. A. Vinogradov, *J. Photochem. Photobiol., A*, 2008, **198**, 75-84.
534. A. V. Kondrashina, R. I. Dmitriev, S. M. Borisov, I. Klimant, I. O'Brien, Y. M. Nolan, A. V. Zhdanov and D. B. Papkovsky, *Adv. Funct. Mater.*, 2012, **22**, 4931-4939.
535. H. Y. Aboul-Enein, R.-I. Stefan, J. F. van Staden, X. R. Zhang, A. M. Garcia-Campana and W. R. G. Baeyens, *Crit. Rev. Anal. Chem.*, 2000, **30**, 271-289.
536. A. Burr and D. Mauzerall, *Biochim. Biophys. Acta, Bioenerg.*, 1968, **153**, 614-624.
537. J. W. Hastings, *J. Cell. Comp. Physiol.*, 1952, **39**, 1-30.
538. R. Oshino, N. Oshino, M. Tamura, L. Kobilinsky and B. Chance, *Biochim. Biophys. Acta, Gen. Subj.*, 1972, **273**, 5-17.

539. B. Chance and R. Oshino, *Methods Enzymol.*, 1978, **Volume 57**, 223-226.
540. D. Lloyd, K. James, J. Williams and N. Williams, *Anal. Biochem.*, 1981, **116**, 17-21.
541. M. Beijerinck, *Koninklijke Nederlandse Akademie van Wetenschappen Proceedings Series B Physical Sciences*, 1902, **4**, 45-49.
542. G. E. Collins and S. L. Rose-Pehrsson, *Anal. Chem.*, 1995, **67**, 2224-2230.
543. R.-J. Zheng, Y.-M. Fang, S.-F. Qin, J. Song, A.-H. Wu and J.-J. Sun, *Sens. Actuators, B*, 2011, **157**, 488-493.
544. S. M. Borisov, C. Lardorfer and I. Klimant, *Adv. Funct. Mater.*, 2012, **22**, 4360-4368.
545. I.-S. Shin, T. Hirsch, B. Ehl, D.-H. Jang, O. S. Wolfbeis and J.-I. Hong, *Anal. Chem.*, 2012, **84**, 9163-9168.
546. D. S. Smith, Y. Kostov and G. Rao, *Sens. Actuators, B*, 2007, **127**, 432-440.
547. S. Balushev, F. Yu, T. Miteva, S. Ahl, A. Yasuda, G. Nelles, W. Knoll and G. Wegner, *Nano Lett.*, 2005, **5**, 2482-2484.
548. O. S. Wolfbeis, *Proc. SPIE*, 1990, **1368**, 218-222.
549. O. S. Wolfbeis and E. Urbano, *Anal. Chem.*, 1983, **55**, 1904-1906.
550. M. I. J. Stich, S. Nagl, O. S. Wolfbeis, U. Henne and M. Schaeferling, *Adv. Funct. Mater.*, 2008, **18**, 1399-1406.
551. L. H. Fischer, S. M. Borisov, M. Schaeferling, I. Klimant and O. S. Wolfbeis, *Analyst*, 2010, **135**, 1224-1229.
552. S. Nagl, M. I. J. Stich, M. Schaeferling and O. S. Wolfbeis, *Anal. Bioanal. Chem.*, 2009, **393**, 1199-1207.
553. S. M. Borisov, C. Krause, S. Arain and O. S. Wolfbeis, *Adv. Mater.*, 2006, **18**, 1511-1516.
554. C. R. Schroder, L. Polerecky and I. Klimant, *Anal. Chem.*, 2007, **79**, 60-70.
555. S. Borisov, R. Seifner and I. Klimant, *Anal. Bioanal. Chem.*, 2011, **400**, 2463-2474.
556. R. Liu, T. Xiao, W. Cui, J. Shinar and R. Shinar, *Anal. Chim. Acta*, 2013, **778**, 70-78.
557. T. Kameya, Y. Matsuda, Y. Egami, H. Yamaguchi and T. Niimi, *Sens. Actuators, B*, 2014, **190**, 70-77.
558. J. Hradil, C. Davis, K. Mongey, C. McDonagh and B. D. MacCraith, *Meas. Sci. Technol.*, 2002, **13**, 1552.
559. L. M. Coyle and M. Gouterman, *Sens. Actuators, B*, 1999, **61**, 92-99.
560. T.-W. Sung and Y.-L. Lo, *Sens. Actuators, B*, 2012, **173**, 406-413.
561. H. Lam, G. Rao, J. Loureiro and L. Tolosa, *Talanta*, 2011, **84**, 65-70.
562. R. J. Meier, S. Schreml, X.-d. Wang, M. Landthaler, P. Babilas and O. S. Wolfbeis, *Angew. Chem. Int. Ed.*, 2011, **50**, 10893-10896.
563. X.-d. Wang, J. A. Stolwijk, T. Lang, M. Sperber, R. J. Meier, J. Wegener and O. S. Wolfbeis, *J. Am. Chem. Soc.*, 2012, **134**, 17011-17014.
564. C. R. Schroeder, G. Neurauder and I. Klimant, *Mikrochim. Acta*, 2007, **158**, 205-218.
565. M. Schaeferling, A. Duerkop and U. Resch-Genger, in *Springer series on fluorescence*, ed. U. Resch-Genger, Springer, Berlin, 2008, vol. 5, pp. 373-414.
566. Y. Feng, J. Cheng, L. Zhou, X. Zhou and H. Xiang, *Analyst*, 2012, **137**, 4885-4901.
567. D. W. Lübbers, US Patent 4,306,877, 1981.
568. E. J. Park, K. R. Reid, W. Tang, R. T. Kennedy and R. Kopelman, *J. Mater. Chem.*, 2005, **15**, 2913-2919.
569. C. F. Wu, B. Bull, K. Christensen and J. McNeill, *Angew. Chem. Int. Ed.*, 2009, **48**, 2741-2745.
570. P. A. S. Jorge, M. Mayeh, R. Benrashid, P. Caldas, J. L. Santos and F. Farahi, *Appl. Opt.*, 2006, **45**, 3760-3767.
571. M. Amelia, A. Lavie-Cambot, N. D. McClenaghan and A. Credi, *Chem. Commun.*, 2011, **47**, 325-327.
572. C.-S. Chu and Y.-L. Lo, *Sens. Actuators, B*, 2008, **134**, 711-717.
573. Y. Kostov, K. A. Van Houten, P. Harms, R. S. Pilato and G. Rao, *Appl. Spectrosc.*, 2000, **54**, 864-868.
574. T. Yoshihara, Y. Yamaguchi, M. Hosaka, T. Takeuchi and S. Tobita, *Angew. Chem.*, 2012, **124**, 4224-4227.
575. T. Doussineau, A. Schulz, A. Lapresta-Fernandez, A. Moro, S. Körsten, S. Trupp and G. J. Mohr, *Chem. Eur. J.*, 2010, **16**, 10290-10299.
576. S. J. Payne, G. Zhang, J. N. Demas, C. L. Fraser and B. A. Degraff, *Appl. Spectrosc.*, 2011, **65**, 1321-1324.
577. D. P. Saini, S. M. Klainer and S. L. Coulter, US Patent 5,737,457, 1998.
578. M. Schäferling, *Angew. Chem. Int. Ed.*, 2012, **51**, 3532-3554.
579. P. Hartmann and W. Ziegler, *Anal. Chem.*, 1996, **68**, 4512-4514.
580. [www.presens.de/references/application-notes.html?tx_presensapplicationnotes_pi1\[product_group\]=16](http://www.presens.de/references/application-notes.html?tx_presensapplicationnotes_pi1[product_group]=16): accessed in January 2014.
581. D. H. Song, H. D. Kim and K. C. Kim, *Optics and Lasers in Engineering*, 2012, **50**, 74-81.
582. M. I. J. Stich, S. M. Borisov, U. Henne and M. Schäferling, *Sens. Actuators, B*, 2009, **139**, 204-207.
583. B. Ungerböck, V. Charwat, P. Ertl and T. Mayr, *Lab Chip*, 2013, **13**, 1593-1601.
584. S. Park, S. G. Achanta, J. Yang and C.-S. Kim, *Sens. Actuators, B*, 2012, **164**, 101-108.
585. S. Achanta, P. Sanghan and K. Chang-Soo, *Sensors, 2012 IEEE*, 2012, 1-4.
586. J. Park, W. Hong and C.-S. Kim, *Sensors Journal, IEEE*, 2010, **10**, 1855-1862.
587. K. Kellner, G. Liebsch, I. Klimant, O. S. Wolfbeis, T. Blunk, M. B. Schulz and A. Gopferich, *Biotechnol. Bioeng.*, 2002, **80**, 73-83.
588. P. Babilas, G. Liebsch, V. Schacht, I. Klimant, O. S. Wolfbeis, R. M. Szeimies and C. Abels, *Microcirculation*, 2005, **12**, 477-487.
589. P. Babilas, P. Lamby, L. Prantl, S. Schreml, E. M. Jung, G. Liebsch, O. S. Wolfbeis, M. Landthaler, R. M. Szeimies and C. Abels, *Skin Res. Technol.*, 2008, **14**, 304-311.

590. R. J. Meier, L. H. Fischer, O. S. Wolfbeis and M. Schäferling, *Sens. Actuators, B*, 2013, **177**, 500-506.
591. J. Hofmann, R. J. Meier, A. Mahnke, V. Schatz, F. Brackmann, R. Trollmann, C. Bogdan, G. Liebsch, X. Wang, O. S. Wolfbeis and J. Jantsch, *Meth. Appl. Fluoresc.*, 2013, **1**, 045002.
592. G. Holst, O. Kohls, I. Klimant, B. Konig, M. Kuhl and T. Richter, *Sens. Actuators, B*, 1998, **51**, 163-170.
593. X. F. Wang, T. Uchida, D. M. Coleman and S. Minami, *Appl. Spectrosc.*, 1991, **45**, 360-366.
594. G. Holst and B. Grunwald, *Sens. Actuators, B*, 2001, **74**, 78-90.
595. J. R. Lakowicz and K. W. Berndt, *Rev. Sci. Instrum.*, 1991, **62**, 1727-1734.
596. C.-S. Chu and Y.-L. Lo, *Sens. Actuators, B*, 2010, **147**, 310-315.
597. O. S. Wolfbeis and W. Trettnak, *Spectrochimica acta. Part A: Molecular spectroscopy*, 1987, **43**, 405-408.
598. A. Mondin, D. Badocco and P. Pastore, *Sens. Actuators, B*, 2014, **190**, 775-781.
599. D. Badocco, A. Mondin and P. Pastore, *Sens. Actuators, B*, 2011, **158**, 54-61.
600. D. Badocco, A. Mondin and P. Pastore, *Sens. Actuators, B*, 2013, **181**, 943-948.
601. D. Badocco, A. Mondin and P. Pastore, *Sens. Actuators, B*, 2013, **181**, 949-954.
602. X.-d. Wang, O. S. Wolfbeis and R. J. Meier, *Chem. Soc. Rev.*, 2013, DOI: **10.1039/C3CS60102A**
603. H. Kroneis, PhD thesis, TU Graz, 1983.
604. E. Reynolds, J. N. Demas and B. A. DeGraff, *J. Fluoresc.*, 2013, **23**, 237-241.
605. W. Miller, M. Yafuso, C. Yan, H. Hui and S. Arick, *Clin. Chem.*, 1987, **33**, 1538-1542.
606. C.-S. Chu, Y.-L. Lo and T.-W. Sung, *Photonic Sens*, 2011, **1**, 234-250.
607. I. A. Zakharov and T. I. Grishaeva, *Zh. Anal. Khim.*, 1981, **36**, 112.
608. B.-H. Han, M. A. Winnik, A. B. Bourlinos and E. P. Giannelis, *Chem. Mater.*, 2005, **17**, 4001-4009.
609. O. S. Wolfbeis, *Anal. Chem.*, 2000, **72**, 81-90.
610. O. S. Wolfbeis, *Anal. Chem.*, 2002, **74**, 2663-2678.
611. O. S. Wolfbeis, *Anal. Chem.*, 2004, **76**, 3269-3284.
612. O. S. Wolfbeis, *Anal. Chem.*, 2006, **78**, 3859-3874.
613. O. S. Wolfbeis, *Anal. Chem.*, 2008, **80**, 4269-4283.
614. X.-D. Wang and O. S. Wolfbeis, *Anal. Chem.*, 2012, **85**, 487-508.
615. B. A. Shapiro, C. K. Mahutte, R. D. Cane and I. J. Gilmour, *Critical Care Medicine*, 1993, **21**, 487-494.
616. E. J. Fogt, *Clin. Chem.*, 1990, **36**, 1573-1580.
617. D. W. Lübbers, *Acta Anaesthesiologica Scandinavica*, 1995, **39**, 37-54.
618. M. J. P. Leiner, *Sens. Actuators, B*, 1995, **29**, 169-173.
619. W. Barnikol, T. Gaertner, N. Weiler and O. Burkhard, *Rev. Sci. Instrum.*, 1988, **59**, 1204-1208.
620. R. Chen, A. D. Farmery, A. Obeid and C. E. W. Hahn, *Sensors Journal, IEEE*, 2012, **12**, 71-75.
621. P. A. S. Jorge, P. Caldas, C. C. Rosa, A. G. Oliva and J. L. Santos, *Sens. Actuators, B*, 2004, **103**, 290-299.
622. C. A. Browne, D. H. Tarrant, M. S. Olteanu, J. W. Mullens and E. L. Chronister, *Anal. Chem.*, 1996, **68**, 2289-2295.
623. M. V. Rigo and P. Geissinger, *J. Nanomaterials*, 2010, **2010**, 1-11.
624. M. V. Rigo and P. Geissinger, *Journal of Sensors*, 2012, **2012**, 1-10.
625. C.-S. Chu, T.-W. Sung and Y.-L. Lo, *Sens. Actuators, B*, 2013, **185**, 287-292.
626. E. E. Hardy, D. J. David, N. S. Kapany and F. C. Unterleitner, *Nature*, 1975, **257**, 666-667.
627. Ó. Esteban and C. Pulido, *Proc. SPIE*, 2013, **8794**, 879410.
628. X. Yang, Y. Liu, F. Tian, L. Yuan, Z. Liu, S. Luo and E. Zhao, *Opt. Lett.*, 2012, **37**, 2115-2117.
629. R. Xue, P. Behera, J. Xu, M. S. Viapiano and J. J. Lannutti, *Sens. Actuators, B*, 2014, **192**, 697-707.
630. B. A. A. Dremel, R. D. Schmid and O. S. Wolfbeis, *Anal. Chim. Acta*, 1991, **248**, 351-359.
631. W. Trettnak and O. S. Wolfbeis, *Anal. Lett.*, 1989, **22**, 2191-2197.
632. B. Lamprecht, A. Tschepp, M. Cajlakovic, M. Sagmeister, V. Ribitsch and S. Kostler, *Analyst*, 2013, DOI: **10.1039/C3AN00208J**.
633. V. G. Bordo and H.-G. Rubahn, *Optics and spectroscopy at surfaces and interfaces*, Wiley-VCH, Weinheim, 2008.
634. Z.-M. Qi, S. Xia and N. Matsuda, *Anal. Biochem.*, 2008, **374**, 196-202.
635. B. W. Dodson, *Proc. SPIE*, 1984, **497**, 91.
636. R. C. Murray and S. M. Lefkowitz, *Eur. Pat. 190,830*, 1986.
637. Y. Xiong, J. Xu, J.-W. Wang and Y.-F. Guan, *Anal. Bioanal. Chem.*, 2009, **394**, 919-923.
638. E. Singer, G. L. Duveneck, M. Ehrat and H. M. Widmer, *Sens. Actuators, A*, 1994, **42**, 542-546.
639. W. Cao and Y. Duan, *Sens. Actuators, B*, 2006, **119**, 363-369.
640. D. Wales, R. Parker, J. Gates, M. Grossel and P. Smith, *Integrated planar Bragg grating oxygen sensor*, 2010, <http://eprints.soton.ac.uk/340796/340791/344630.pdf>. Visited in Jan. 2014.
641. J. Luo, X. Zhuang and J. Yao, *Journal of Nanoengineering and Nanosystems*, 2012, **226**, 39-43.
642. C. R. Lavers, K. Itoh, S. C. Wu, M. Murabayashi, I. Mauchline, G. Stewart and T. Stout, *Sens. Actuators, B*, 2000, **69**, 85-95.
643. O. S. Wolfbeis, *TrAC, Trends Anal. Chem.*, 1996, **15**, 225-232.
644. C. Monat, P. Domachuk and B. J. Eggleton, *Nat Photon*, 2007, **1**, 106-114.
645. R. A. Potyrailo, S. E. Hobbs and G. M. Hieftje, *Fresenius' Journal of Analytical Chemistry*, 1998, **362**, 349-373.

646. D. P. Saini, US Patent 5,439,647, 1995.
647. Z. Wang, S. Y. Al-Raqa, I. Chambrier, D. A. Russell and M. J. Cook, *J. Porphyr. Phthalocya.*, 2012, **16**, 1186-1195.
648. C. S. Burke, O. McGaughey, J.-M. Sabattie, H. Barry, A. K. McEvoy, C. McDonagh and B. D. MacCraith, *Analyst*, 2005, **130**, 41-45.
649. D. A. Chang-Yen and B. K. Gale, *Lab Chip*, 2003, **3**, 297-301.
650. P. J. R. Roche, M. C. K. Cheung, K. Y. Yung, A. G. Kirk, V. P. Chodavarpu and F. V. Bright, *Sens. Actuators, B*, 2010, **147**, 581-586.
651. B. J. Prince, A. W. Schwabacher and P. Geissinger, *Anal. Chem.*, 2001, **73**, 1007-1015.
652. S. Personick, *Bell Syst. Tech. J.*, 1977, **56**, 355-366.
653. S. Eich, E. Schmälzlin and H.-G. Löhmansröben, *Sensors*, 2013, **13**, 7170-7183.
654. R. A. Potyrailo and G. M. Hieftje, *Anal. Chem.*, 1998, **70**, 3407-3412.
655. S. Eich, E. Schmälzlin and H.-G. Löhmansröben, *Proc. SPIE*, 2010, 77260A-77260A.
656. B. J. Prince, N. T. Kaltcheva, A. W. Schwabacher and P. Geissinger, *Appl. Spectrosc.*, 2001, **55**, 1018-1024.
657. P. E. Henning and P. Geissinger, *Meas. Sci. Technol.*, 2012, **23**, 045104.
658. P. E. Henning, A. Benko, A. W. Schwabacher, P. Geissinger and R. J. Olsson, *Rev. Sci. Instrum.*, 2005, **76**, 062220-062220-062228.
659. G. Mistlberger, K. Koren, S. M. Borisov and I. Klimant, *Anal. Chem.*, 2010, **82**, 2124-2128.
660. E. W. Stein, P. S. Grant, H. Zhu and M. J. McShane, *Anal. Chem.*, 2007, **79**, 1339-1348.
661. E. W. Stein, S. Singh and M. J. McShane, *Anal. Chem.*, 2008, **80**, 1408-1417.
662. S. Singh and M. McShane, *Biosens. Bioelectron.*, 2011, **26**, 2478-2483.
663. J. Prasad, A. Joshi, R. D. Jayant and R. Srivastava, *Biotechnol. Bioeng.*, 2011, **108**, 2011-2021.
664. J. Q. Brown, R. Srivastava and M. J. McShane, *Biosens. Bioelectron.*, 2005, **21**, 212-216.
665. K. Nagamine, S. Ito, M. Takeda, S. Otani and M. Nishizawa, *Electrochemistry*, 2012, **80**, 318-320.
666. J. López-Gejo, A. Arranz, Á. Navarro, C. Palacio, E. Muñoz and G. Orellana, *J. Am. Chem. Soc.*, 2010, **132**, 1746-1747.
667. J. López-Gejo, Á. Navarro-Tobar, A. Arranz, C. Palacio, E. Muñoz and G. Orellana, *ACS Appl. Mater. Interfaces*, 2011, **3**, 3846-3854.
668. S. Lee, B. L. Ibey, G. L. Coté and M. V. Pishko, *Sens. Actuators, B*, 2008, **128**, 388-398.
669. H. Zhu, X. Zhou, F. Su, Y. Tian, S. Ashili, M. R. Holl and D. R. Meldrum, *Sens. Actuators, B*, 2012, **173**, 817-823.
670. V. Nock, M. Alkaisi and R. J. Blaikie, *Microelectron. Eng.*, 2010, **87**, 814-816.
671. J. R. Eitzkorn, W.-C. Wu, Z. Tian, P. Kim, S.-H. Jang, D. R. Meldrum, A. K. Y. Jen and B. A. Parviz, *Journal of Micromechanics and Microengineering*, 2010, **20**, 095017.
672. R. Ambekar, P. Jongwon, D. B. Henthorn and K. Chang-Soo, *Sensors Journal, IEEE*, 2009, **9**, 169-175.
673. A. Martínez-Olmos, J. Fernández-Salmerón, N. Lopez-Ruiz, A. Rivadeneyra Torres, L. F. Capitan-Vallvey and A. J. Palma, *Anal. Chem.*, 2013, **85**, 11098-11105.
674. M. Marín-Suárez, S. Medina-Rodríguez, O. Ergeneman, S. Pané, J. F. Fernández-Sánchez, B. J. Nelson and A. Fernández-Gutiérrez, *Nanoscale*, 2014, **6**, 263-271.
675. I. Dunphy, S. A. Vinogradov and D. F. Wilson, *Anal. Biochem.*, 2002, **310**, 191-198.
676. I. B. Rietveld, E. Kim and S. A. Vinogradov, *Tetrahedron*, 2003, **59**, 3821-3831.
677. D. F. Wilson, W. M. F. Lee, S. Makonnen, O. Finikova, S. Apreleva and S. A. Vinogradov, *J. Appl. Physiol.*, 2006, **101**, 1648-1656.
678. A. Y. Lebedev, A. V. Cheprakov, S. Sakadzović, D. A. Boas, D. F. Wilson and S. A. Vinogradov, *ACS Appl. Mater. Interfaces*, 2009, **1**, 1292-1304.
679. L. S. Ziemer, W. M. F. Lee, S. A. Vinogradov, C. Sehgal and D. F. Wilson, *J. Appl. Physiol.*, 2005, **98**, 1503-1510.
680. L.-W. Lo, S. H.-Y. Huang, C.-H. Chang, W.-Y. Chen, P.-J. Tsai and C.-S. Yang, *Journal of Medical and Biological Engineering*, 2003, **23**, 19-28.
681. T. V. Esipova, A. Karagodov, J. Miller, D. F. Wilson, T. M. Busch and S. A. Vinogradov, *Anal. Chem.*, 2011, **83**, 8756-8765.
682. A. Y. Lebedev, T. Troxler and S. A. Vinogradov, *J. Porphyr. Phthalocya.*, 2008, **12**, 1261-1269.
683. S. V. Apreleva, D. F. Wilson and S. A. Vinogradov, *Appl. Opt.*, 2006, **45**, 8547-8559.
684. M. A. Yaseen, V. J. Srinivasan, S. Sakadi, W. Wu, S. Ruvinskaya, S. A. Vinogradov and D. A. Boas, *Opt. Express*, 2009, **17**, 22341-22350.
685. Y.-E. K. Lee, R. Smith and R. Kopelman, *Annu. Rev. Anal. Chem.*, 2009, **2**, 57-76.
686. Y. Kuang and D. R. Walt, *Biotechnol. Bioeng.*, 2007, **96**, 318-325.
687. X.-H. Wang, H.-S. Peng, Z. Chang, L.-L. Hou, F.-T. You, F. Teng, H.-W. Song and B. Dong, *Mikrochim. Acta*, 2012, **178**, 147-152.
688. X.-H. Wang, H.-S. Peng, H. Ding, F.-T. You, S.-H. Huang, F. Teng, B. Dong and H.-W. Song, *J. Mater. Chem.*, 2012, **22**, 16066-16071.

... end

Entry for the Table of Contents

