


Faraday Discussions

Accepted Manuscript



This manuscript will be presented and discussed at a forthcoming Faraday Discussion meeting. All delegates can contribute to the discussion which will be included in the final volume.

Register now to attend! Full details of all upcoming meetings: <http://rsc.li/fd-upcoming-meetings>

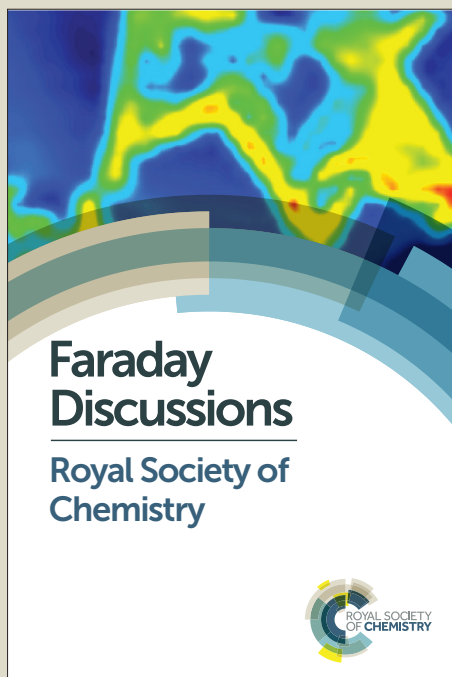

This is an *Accepted Manuscript*, which has been through the Royal Society of Chemistry peer review process and has been accepted for publication.

Accepted Manuscripts are published online shortly after acceptance, before technical editing, formatting and proof reading. Using this free service, authors can make their results available to the community, in citable form, before we publish the edited article. We will replace this *Accepted Manuscript* with the edited and formatted *Advance Article* as soon as it is available.

You can find more information about *Accepted Manuscripts* in the [Information for Authors](#).

Please note that technical editing may introduce minor changes to the text and/or graphics, which may alter content. The journal's standard [Terms & Conditions](#) and the [Ethical guidelines](#) still apply. In no event shall the Royal Society of Chemistry be held responsible for any errors or omissions in this *Accepted Manuscript* or any consequences arising from the use of any information it contains.

Protein A conjugated iron oxide nanoparticles for separation of *Vibrio cholerae* from water samples

Tran Quang Huy^a, Pham Van Chung^a, Nguyen Thanh Thuy^a, Cristina Blanco-Andujar^b, Nguyễn Thị Kim Thanh^{*b}

Abstract

Pathogen separation is of great significance for precise detection and prevention of outbreaks. For the first time, protein A conjugated with chitosan-coated iron oxide nanoparticles was prepared for pathogen separation at low concentrations from liquid samples. *Vibrio cholerae* O1 (VO1) bacteria were used for testing the effectiveness of this conjugate. Transmission electron microscopy (TEM) was used to confirm the presence of captured VO1. The results showed that after binding with a specific antibody, the conjugate allows separating VO1 bacteria from water samples at a concentration as low as 10 cfu/mL. Moreover, the conjugate can be used in parallel with conventional or modern diagnostic tests for quick and accurate detection of pathogens.

Introduction

Recently, the world has witnessed an increased number of emerging and re-emerging infectious outbreaks caused by viruses and bacteria such as severe acute respiratory syndrome-associated coronavirus (SARS-CoV), avian influenza (A/H₅N₁, A/H₇N₉), foot-hand-mouth diseases, measles, diarrhea or cholera, among others. The outbreaks not only have public health consequences, but also socio-economic tolls¹. Rapid and accurate detection of pathogens is paramount important for the control and prevention of these infectious diseases spreading to the community.

Particularly, cholera outbreak caused by *Vibrio cholerae* (*V. cholerae*) is one of the continuous risks threatening public health and socio-economy in many developing countries². *V. cholerae* is a Gram-

negative, comma-shaped bacterium, which causes abrupt onset of watery diarrhoea, occasional vomiting, renal failure, coma and even death. There are more than 200 known *V. cholerae* serogroups, but only the O1 and O139 strains are pathogenic and cause epidemics. *V. cholerae* bacteria can be alive up to one year in an aquatic environment due to a protective bio-film². It is not easy to detect *V. cholerae* using conventional diagnostic methods, because it is non-culturable and generally found in low levels in water³. Several techniques have been developed for detection of *V. cholerae* in environmental water including immunomagnetic beads, nucleic acid-based methods (such as PCR and DNA probe hybridization) or fluorescent labeling techniques⁴. Immunomagnetic bead detection offers good sensitivity, but has the possibility of false positives. Nucleic acid-based methods require biological agents such as primers, standardised bio-safe laboratories, and can only detect nucleic acids rather than live bacterial cells. The fluorescent labeling technique is preferred for the detection of *V. cholerae* in environmental water samples, but filtering is necessary for the concentration of bacteria from a large volume of water.

In recent years, many studies have shown the potential applications of magnetic nanoparticles in biomedicine such as imaging, targeted drug delivery and therapy⁵, but only a few studies used magnetic nanoparticles for detection of pathogens from infectious diseases so far⁶. The main challenges in the preparation of magnetic nanoparticles for pathogen detection are surface modification and biofunctionalisation, particularly the immobilisation of biomolecules onto the surface of nanoparticles as probes⁷.

In this study, a conjugate of protein A and chitosan-coated magnetic nanoparticles was prepared for separation of *V. cholerae* bacteria at low concentrations from water samples. Chitosan, a polysaccharide obtained from the N-deacetylation of chitin, is one of the most abundant polysaccharides in nature. It has been used for a wide range of biological applications thanks to its biocompatibility and biodegradability⁸. Its use for the functionalisation of nanoparticles offers not only the incorporation of amine groups to the surface of the nanoparticles, but also, positive charge to the

system, which has been shown to be preferred by some cell lines.⁹ On the other hand, protein A is well known as a molecule which binds with high affinity to the Fc region of IgG antibodies and orientate binding sites of the antibody molecule outwards from the surface of nanoparticles for capturing antigens¹⁰.

Herein, chitosan-coated iron oxide nanoparticles (IONPs) were firstly conjugated with protein A and then the conjugate was incubated with its specific IgG antibody against *V. cholerae* strain just before testing. The *V. cholerae* bacteria could be easily magnetically separated and collected by binding to iron oxide nanoparticles.

Experimental Procedures

Materials

Protein A (PrA, extracellular from *Staphylococcus aureus*, lyophilized, $\geq 90\%$ protein basis), glutaraldehyde solution (GA, grade I, 25%), paraformaldehyde (reagent grade), sodium cacodylate trihydrate ($(\text{CH}_3)_2\text{AsO}_2\text{Na}\cdot 3\text{H}_2\text{O}$, $\geq 98\%$), and chitosan ($\text{C}_6\text{H}_{11}\text{NO}_4$)_n, $M_w \sim 60000$ g/mol were obtained from Sigma Aldrich, UK. *Vibrio cholerae* (*V. cholerae*) O1 bacteria, anti-*V. cholerae* O1 polyclonal antibody, and *Escherichia coli* (*E.coli*) were provided by Professor Nguyen Binh Minh and Dr. Tran Huy Hoang at Department of Bacteriology, National Institute of Hygiene and Epidemiology (NIHE), Hanoi. Bacterial strains were inoculated at the laboratory of enteric bacteria, certified by ISO 15189: 2012, and all proper and standard biosafety procedure were followed when handling them. All chemical used were of analytical grade.

Synthesis and characterization of chitosan coated IONPs

Chitosan coated IOPNs were synthesized by a chemical method¹¹, and then characterized by transmission electron microscopy (TEM), dynamic light scattering (DLS), zeta-potential (ζ -potential), and attenuated total reflectance-Fourier transformed infrared spectroscopy (ATR-FTIR).

Bio-conjugation of protein A to IONPs

Protein A was conjugated to the surface of chitosan-coated IONPs via a cross-linkage with glutaraldehyde (GA) (Fig. 1). Thanks to two functional aldehyde groups of GA, they can easily co-bind with amine groups of chitosan layer on the surface of IONPs and those of PrA. Firstly, the solution of chitosan-coated IONP (IONP@CHI) was diluted in distilled water to a concentration of 10 $\mu\text{g/mL}$, and the solution pH adjusted to pH 6.5. Next, 5% GA was added, incubated for 45 min at room temperature (RT), and washed with phosphate-buffered saline, PBS (0.01 M, pH 7.4) three times to remove residual GA (Fig. 1, step 1). Then, 2 $\mu\text{g/mL}$ of protein A was added to the solution of IONPs, and incubated overnight at 4 $^{\circ}\text{C}$ (Fig. 1, step 2). After washing two times with PBS, the non-specific binding sites on the surface of nanoparticles were blocked with 0.5% bovine serum albumin (BSA) in PBS for 20 min at RT. Finally, the conjugate was washed with PBS twice, and then re-suspended in 0.5 mL PBS, and kept at 4 $^{\circ}\text{C}$ for testing. Due to two carbonyl functional groups of GA as well as multiple amine groups of protein A, cross-linking could occur between IONP@CHI leading to aggregation or precipitation; however, these agglomerates can easily be discarded. This phenomenon can easily be checked by naked eye or using dynamic light scattering technique to observe the increase in size of particle aggregates in the solution. Also, round shape IONPs may help to minimize the effect of aggregation, because that there might be some free spaces remaining on the surface of each IONP@CHI for binding to target molecules, even several particles stuck together. In our study, the preparation of the conjugate was done in triplicate and no flocculation was detected. The conjugate can

then be incubated with specific IgG antibodies against pathogens in advance before separation (Fig. 1, step 3).

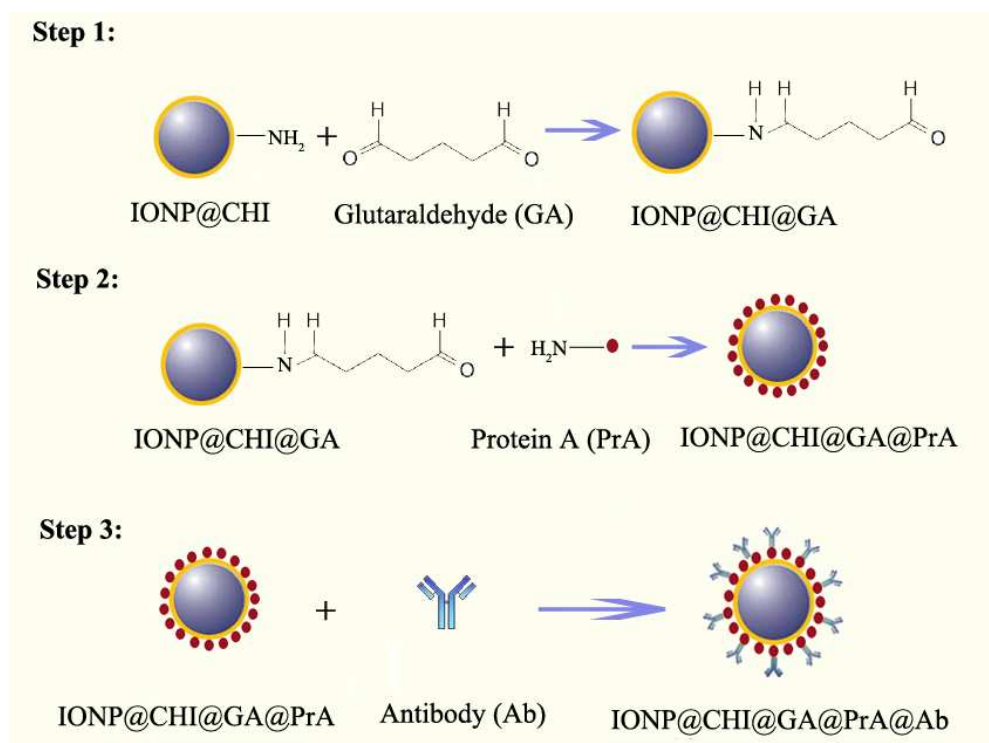


Fig. 1. *Step 1:* Glutaraldehyde (GA) chitosan was conjugated to chitosan coated IONP (IONP@CHI) and. *Step 2:* Reaction of IONP@CHI@GA and protein A (PrA) to form the conjugate of IONP@CHI@GA@PrA. *Step 3:* Preparation of IONP@CHI@GA@PrA linked with specific antibodies against pathogens via their bio-affinity.

To separate *V. cholerae* bacteria from a water sample, 0.5 mL of IONP@CHI@GA@PrA was incubated in advance with polyclonal antibody against *V. cholerae* O1 at a concentration of 2 $\mu\text{g}/\text{mL}$, for 45 min at RT. In this step, IgG antibody molecules would bind with high affinity to protein A-IONPs (IONP@CHI@GA@PrA). A magnet was used to collect the product of IgG antibody conjugated IONPs (IONP@CHI@GA@PrA@Ab) on the wall of the tube, washed two times with PBS to remove unbound antibodies, and then re-suspended in 0.5 mL of PBS (Fig. 1C). This procedure can

be carried out just before separation and detection at RT in the laboratory or prepared in advance and then kept at 4 °C for further detection on-site.

Investigation of bacterial cells before testing

Scanning electron microscopy (SEM) (S-4800, Hitachi) was used to check the presence and morphology of bacterial cells in the samples before testing with the conjugate of IONPs and protein A. At a concentration of 10^6 cfu/mL, the samples of *V.cholerae* and *E.coli* were fixed in 2% paraformaldehyde / 2.5% glutaraldehyde for 1 h, then washed with 0.1 M cacodylate buffer before post-fixing with 2% aqueous OsO_4 in 0.2 M cacodylate buffer for 2 h. After washing with 0.1 M cacodylate buffer again, samples were dehydrated with increasing ethanol solutions (from 30% to 100% with 10% increments), dried using a critical point dryer (Emitech, K850, Quorum Technologies), and coated with Pt-Pd using ion sputter before SEM imaging.

Separation of *Vibrio cholerae* O1 from water samples

V. cholerae O1 bacteria were dispersed in 0.01 M PBS (pH 7.4) with an initial concentration of 10^3 cfu/ mL. Ten-fold serial dilutions in water were then prepared in test tubes to a final volume of 5 mL from the original concentration of bacteria. A 50 μL aliquot of the complex of IONP@CHI@GA@PrA@Ab was added to the test tube (with the ratio of 1:100 v/v), and mixed at RT for about 15 min (Fig. 2a). The IONPs-bound VO1 bacteria were collected on the wall of the tube using a bar magnet, and most of the supernatant was removed with a pipette. The conjugate was then re-suspended with the remaining water in the tube (Fig. 2b). A drop of this solution was transferred to a carbon coated copper grid to determine the presence of VO1 bacteria under a TEM (JEM1010, JEOL), operating at 80 kV.

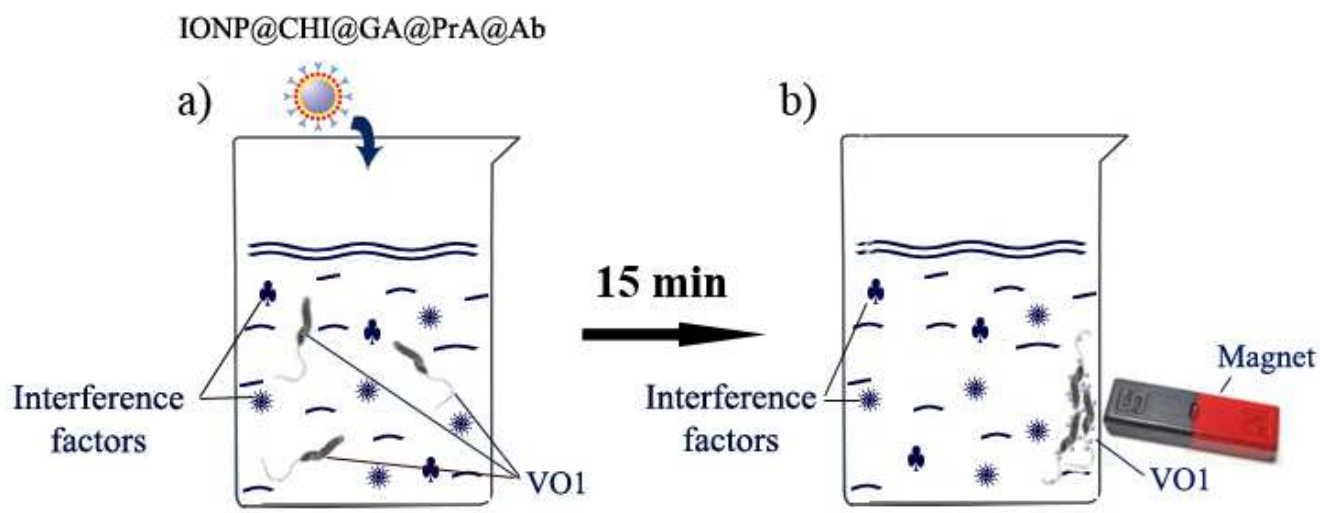


Fig. 2. Separation of VO1 bacterial cells from water samples with interference factors: (a) adding the complex of IONP@CHI@GA@PrA@Ab to the sample, and (b) attracting bacterial cells with a bar magnet

Results and Discussion

The synthesised nanoparticles are spheroidal as observed by TEM (Fig. 3A and 3B) with an average particle size of 13.4 ± 2.5 nm, as calculated from the measurement of 400 particles (Fig. 3C). The hydrodynamic size of the chitosan-IONPs, as observed by DLS, is 82.9 ± 13 nm. The measured ζ -potential of 45 mV indicated the presence of chitosan around the IONPs (Fig. 3D). From ATR-FTIR spectra (Fig. 3E), we could observe the NH_2 bending bands appearing at 1658 and 1588 cm^{-1} for free chitosan, merging to the 1616 cm^{-1} band after coating. The peak at 1378 cm^{-1} for the ν_{CO} vibration of the hydroxyl group, the C-N stretching at 1153 cm^{-1} and the stretching of the aliphatic CH_2 group around 2900 cm^{-1} were found in the coated samples. The coordination of chitosan to the surface of the nanoparticles occurs via charge affinity as the reaction occurs at acidic pH where chitosan presents a high positive charge density and thus high affinity for the negatively charged nanoparticle surface. Nonetheless, not all the amine groups are bound to the nanoparticles as surface charge was 46.5 mV,

due to the presence of positively charged groups. As a result, the obtained system is highly stable due to steric repulsion of the nanoparticles provided by the polymer backbone and the surface charge obtained from the amine groups.

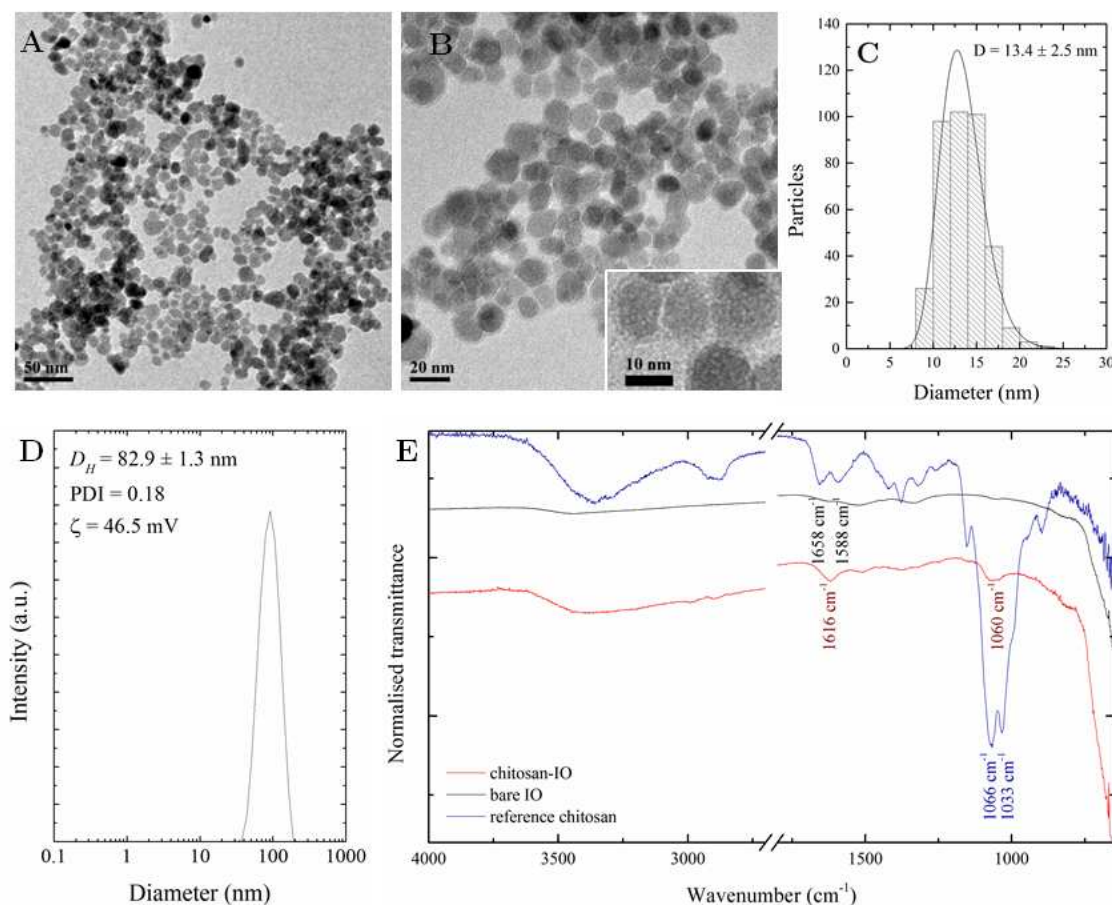


Fig. 3. A-B) TEM images of chitosan coated iron oxide nanoparticles and C) particle size distribution from image analysis obtained from the measurement of 400 particles. Size distribution was fitted with a log normal function. D) DLS and ζ -potential of chitosan-iron oxide nanoparticles and E) ATR-FTIR spectra of iron oxide nanoparticles before and after chitosan coating. Reference spectrum for chitosan is included for reference. All spectra have been normalized and offset for better comparison. The 1800 - 2700 cm^{-1} range has been excluded as no significant information was found.

Before testing with the complex of IONP@CHI@GA@PrA@Ab, the solution containing bacterial strains were checked by scanning electron microscopy. SEM images revealed the presence of *V.*

cholerae and *E. coli* bacterial cells in the samples. *V. cholerae* bacteria were found to have comma-shape, measuring 0.3 μm in diameter and 1.3 μm in length and a flagellum at one cell pole (Fig. 4A). *E. coli* bacterial cells have rod-shape, measuring 0.5 μm in diameter and 1.2 μm in length (Fig. 4B)

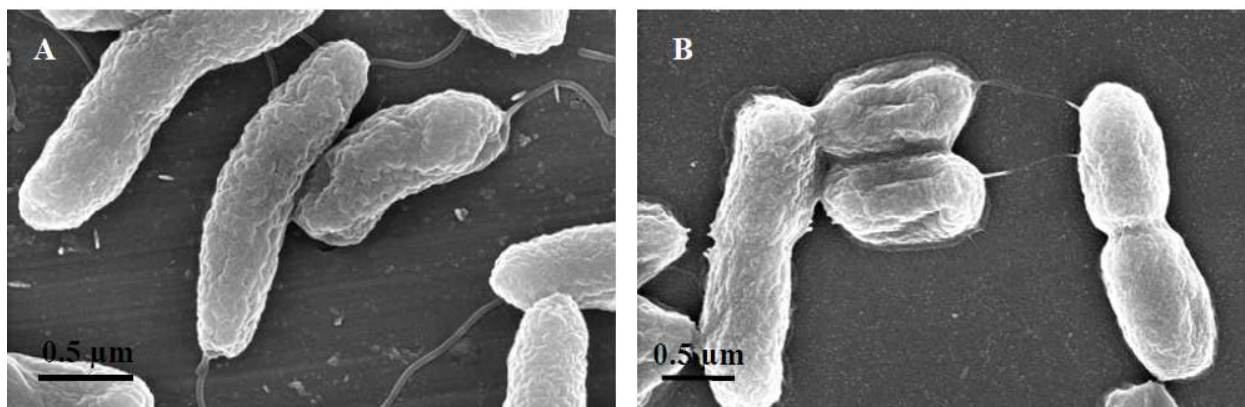


Fig. 4. Scanning electron microscopic images of A) *V. cholerae* and B) *E. coli* (B)

To test the effectiveness of the conjugate, IONP@CHI@GA@PrA was incubated with anti-*V. cholerae* O1 polyclonal antibody before dropping into the tubes containing *V. cholerae* bacteria.

The TEM images show that before the test with the complex of IONP@CHI@GA@PrA@Ab, *V. cholerae* bacterial cell could be clearly seen without the presence of IONPs (Fig. 5a). After using IONP@CHI@GA@PrA@Ab to separate the bacterial cells from water, *V. cholerae* cells were found to aggregate on the grid and were bound by IONPs (Fig. 5b). In this study, we used polyclonal IgG antibodies specific to *V. cholerae* O1 bacteria, so IONPs would specifically bind around the bacterial cell wall (Fig. 5c) as well as the bacterial flagellum (Fig. 5d). All *V. cholerae* O1 bacterial cells found on the grids were covered with IONPs, which demonstrates the capture efficiency of IONP@CHI@GA@PrA@Ab to *V. cholerae* O1 bacterial cells is up to 100%. This may be the result of the diffusion capacity of IONPs in solution as well as the specificity of the IONP@CHI@GA@PrA@Ab complex to pathogens. By series dilutions of bacterial cultures, the results also showed VO1 bacteria could be detected at a level as low as 10 cfu/mL as indicated by the IONPs presence (repeated three times). Interestingly, most of IONPs were found sticking around

bacterial cells, with only a few small clusters of IONPs found on the TEM grids. After separation, the supernatant was also checked by TEM for the presence of bacterial cells remaining there, but none were found on the grids. This confirmed that most of the bacterial cells adhered to IONPs and were attracted by a magnet towards the wall of the tube.

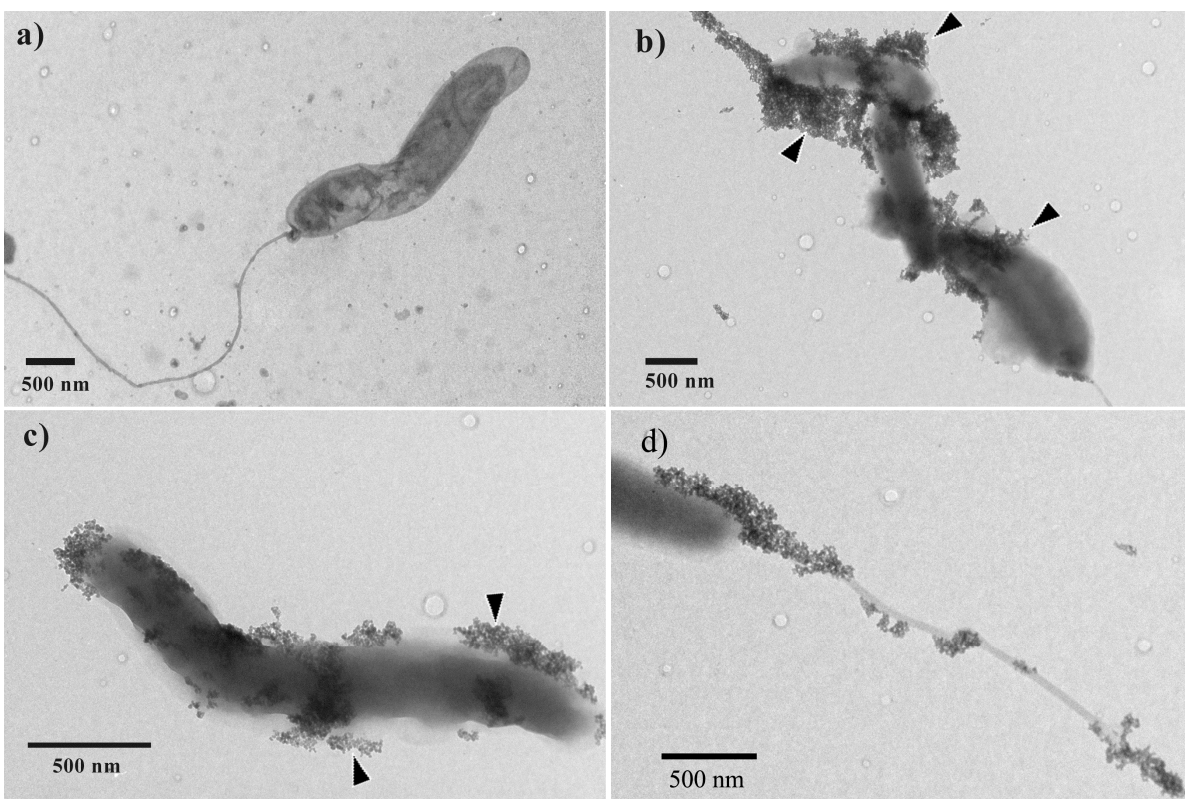


Fig. 5. TEM images of *V. cholerae* bacteria (a) before interaction with the complex of IONP@CHI@GA@PrA@Ab, (b) aggregated and bound by IONPs, (c) IONPs bound to the cell wall, and (d) IONPs bound to the bacterial flagellum.

For positive controls, the solutions containing IONP@CHI, and IONP@CHI@GA@PrA were incubated with *V. cholerae* bacteria diluted in water from an initial concentration of 10^3 cfu/mL. The same procedures used for testing the IONP@CHI@GA@PrA@Ab complex was followed. A significant amount of nanoparticles were found clustered on the grid, but no *V. cholerae* bacterial cells were found (data not shown).

To demonstrate the specificity of the complex to the pathogens, as negative controls, *Escherichia coli* (*E. coli*) bacteria were also prepared in 5 mL of PBS with an initial concentration of 10^3 cfu/mL. Ten-fold serial dilutions in water were also prepared in 5 mL for testing. The complex of IONP@CHI@GA@PrA@Ab (using anti-*V. cholerae* O1 polyclonal IgG antibody) was then added to the tubes and mixed for 15 min at RT. The same procedure used for VO1 was followed; however, TEM images did not show the presence of *E. coli* bacterial cells on the grids.

After incubation of the protein A - conjugated IONPs with anti-*V. cholerae* O1 polyclonal IgG antibody, the separation ability of VO1 bacteria from water samples could be found at concentrations as low as 10 cfu/mL, as confirmed by TEM. More importantly, the detection level was found to be better than with conventional diagnostic techniques, where bacterial pathogens at concentrations lower than 10^2 cfu/mL cannot be detected without inoculation, especially non-culturable bacteria that present their own bio-films such as *V. cholerae*¹². Following isolation and culture, direct fluorescent antibody (DFA) test is known to be an effective method for direct detection of *V. cholerae*. Hasan *et al.*¹³ applied DFA to detect *V. cholerae* O139 in water samples, and the sensitivity of *V. cholerae* O139 detection reached 150 cfu/mL, which was 15-fold higher than the detection levels reported here. In this work, the complex serves as a convenient and versatile agent for separation of different pathogens on-site or in the laboratory. It can be used for selective enrichment of pathogens for early diagnostic tests and preliminary pathogenic screening for a large number of patients who got infected in a short period of time during outbreaks. Noticeably, before testing, the samples and the complex should be adjusted to pH 7.0 - 7.4 to ensure their bioactivity, but all procedures of separation and detection can be performed at RT.

There are several reports on the preparation of magnetic nanoparticles for pathogen detection. Gu *et al.*¹⁴ showed that biofunctionalised magnetic nanoparticles could capture Vancomycin-resistant enterococci and other Gram-positive bacteria at concentrations of ~ 10 cfu/mL within 1 h. In this study,

the authors proposed the use of either optical microscopy or SEM to confirm the presence of “magnetized” bacterial cells. However, to the best of our knowledge, it is very difficult to use optical microscopy to identify the differences between bacterial strains due to the limitation of optical resolution. On the other hand, SEM is time-consuming as it requires complex sample preparation by dehydration and critical point drying steps before imaging. Gao *et al.*¹⁵ also prepared Vancomycin-functionalised FePt nanoparticles, but in combination with a Vancomycin-conjugated fluorescent probe to detect bacteria in human blood with a response time of 2 h. Cheng *et al.*¹⁶ combined the biofunctional magnetic nanoparticles and adenosine triphosphate (ATP) bioluminescence to detect *E. coli* inoculated into pasteurized milk with a detection limit of 20 cfu/mL and a detection time of about 1 h. Recently, the development of a magneto-DNA platform based on magnetic nanoparticles that could detect a panel of 13 bacterial species within 2 h was reported¹⁷. The reported literature demonstrates the use of biofunctionalised magnetic nanoparticles for detection of different pathogens with high sensitivity; however, they all present some intrinsic limitations. Firstly, biofunctionalised nanoparticles need to be prepared in advance against specific pathogens. Moreover, modern complex facilities and equipment are needed, and response time still requires more than 1 h. It is important to consider that for magnetic nanoparticles conjugated directly to antibodies, the bio-activity may be reduced due manipulation or with time.

In this work, the conjugate of protein A and IONPs overcomes some of the aforementioned limitations. Firstly, it serves as a convenient platform for enrichment and separation of various pathogens in different liquid samples, just after a prior incubation with their specific IgG antibodies. Moreover, this conjugate can be used as a smart material to selectively concentrate pathogens from a large volume of water, which indirectly may improve the sensitivity of other diagnostic techniques. Finally, it can also be applied for purifying water infected by pathogens.

Concluding remarks

Our preliminary study showed that the conjugate of protein A and IONPs was successfully prepared, and tested for separation of *V. cholerae* bacteria at low concentrations from water samples in the laboratory. The results showed that the conjugate could easily separate *V. cholerae* bacteria from water samples at concentrations as low as 10 cfu/mL by TEM observation. The selective separation of specific pathogens from liquid samples is achieved by incubation of the conjugate with a specific monoclonal or polyclonal antibody. The pathogens separated from a large volume of liquid samples, can then be detected simply by conventional diagnostic methods or immunochromatographic strip tests on-site. More importantly, it has the potential to be used for the separation and detection of even unknown pathogens in clinical samples collected from emerging outbreaks. This conjugate would be incubated in advance with serum collected from the patients presenting typical symptoms of the outbreak, and perform the immunolabelling reaction to recognise the preliminary morphology of pathogens using SEM or TEM. This approach may help other advanced techniques to confirm the causing agent of the outbreak. Further investigation is planned to optimize the bio-activity and stability of the conjugate over time.

Acknowledgements

Nguyễn T. K. Thanh thanks the Royal Society for her Royal Society University Research Fellowship and Foreign Common Wealth Office for a travel grant.

Notes

^a *National Institute of Hygiene and Epidemiology, 1 Yersin Street, Hai Ba Trung District, Hanoi, Vietnam.*

^b *Department of Physics and Astronomy, University College London, London, WC1E 6BT and UCL Healthcare Biomagnetic and Nanomaterials Laboratories, 21 Albemarle Street, London W1S 4BS. Tel: 44 (0) 207 4916509; E-mail: ntk.thanh@ucl.ac.uk*

References

1. E. K. Jones, G. N. Patel, A. M. Levy, A. Storeygard, D. Balk, L.J. Gittleman and P. Daszak, *Nature* 2008, **451**, 990; J. R. Koker, M. B. Hunter, W.J. Rudge, M. Liverani and P. Hanvoravongchai, *Lancet*, 2011, **377**, 599; A. S. Fauci and D. M. Morens. *N. Engl. J. Med.*, 2012, **366**, 454
2. S. Chaiyanan, A. Huq, T. Maugel, and R. R. Colwell, *Syst. Appl. Microbiol.*, 2001, **24**, 331; P. R. Mason, *J. Infect. Developing Countries* 2009, **3**, 148; N. Sithivong, T. Morita-Ishihara, A. Vongdouangchanh, T. Phouthavane, K. Chomlasak *et al. Emerg. Infect. Dis.* 2011, **17**, 2060; D. D. Anh, A. L. Lopez, V. D. Thiem, S.L Grahek, T. N. Duong *et al. PloS. Aegl. Trip. Dis*, 2011, **5**, e1006; A. M. Devault, G. B. Golding, N. Waglechner, J.M. Enk and M. Kuch, *N. Engl. J. Med.* 2014, **370**, 334
3. S. Banoo, D. Bell, P. Bossuyt, A. Herring, D. Mabey *et al. Nat. Rev. Microbiol.* 2010, **8** (12 Suppl), S17; F.S. Nolte, *Clin. Infect. Dis*, 2008, **47** (Supplement 3), S123; P. Yager, G. J. Domingo and J. Gerdes, *Annu. Rev. Biomed. Eng.* 2008, **10**, 107; A. van Belkum, N. H. Renders, S. Smith, S. E. Overbeek and H. A. Verbrugh, *FEMS Immunol. Med. Microbiol.*, 2000, **27**, 51
4. K.H. Seo, R. E. Brackett, and J. F. Frank, *Int. J. Food Microbiol.* 1998, **44**,115; S. Chakraborty, J. Khanam, Y. Takeda, and G. B. Nair, *Trans. R. Soc. Trop. Med. Hyg.* 1999, **93**, 527; E. K. Lipp, I. N. Rivera, A. I. Gil, E. M. Espeland, N. Choopun, V. R. Louis, E. Russek-Cohen, A. Huq, and R. R. Colwell, *Appl. Environ. Microbiol.* 2003, **69**, 3676; D. Wang, X. Xu. X, Deng, C. Cheng, B. Li *et al. Appl. Environ. Microbiol.* 2010, **76**, 5520
5. Q. A. Pankhurst, N. T. K. Thanh, S. K. Jones and J. Dobson, *J. Phys. D: Appl. Phys.* 2009, **42**, 224001; I. Robinson, L. D. Tung, S. Maenosono, C. Walti and N.T.K. Thanh, *Nanoscale*, 2010, **2**, 2624; O. Veiseh, J. W. Gunn, M. Zhang., *Adv. Drug Delivery Rev.*, 2010, **62**, 284; X. Meng, H. Seton, L.T. Lu, I. Prior, N.T.K. Thanh and B. Song, *Nanoscale*, 2011, **3**, 977; Y. Wang, C. Blanco-Andujar, Z. Zhi, P. W. So , N. T. K. Thanh and J. C. Pickup, *Chem. Comm.* 2013, **49**, 7255; R Hachani, M. Lowdell, M. Birchall and N. T. K. Thanh, *Nanoscale*, 2013, **5**, 11362; A. Hervault and N. T. K. Thanh, *Nanoscale*, 2014, In Press.
6. N. Tran and T. J. Webster. *Mater. Chem.*, 2010, **20**, 8760; P. Tallury, A. Malhotra, L. M. Byrne and S. Santra, *Adv. Drug Delivery Rev.*, 2010, **62**, 424; T. S. Hauck, S. Giri, Y. Gao and W. C. W. Chan, *Adv. Drug. Delivery Rev.*, 2010, **62**, 438
7. N. T. K. Thanh, L. A. W. Green, *Nano Today*, 2010, **5**, 213; T. D. Schladt, K. Schneider, H. Schild and W. Tremel, *Dalton Trans.*, 2011, **40**, 6315; R. A. Sperling and W. J. Parak. *Phil.*

- Trans. R. Soc. A*, 2010, **368**, 1333; H. Xu, Z. P. Aguilar, L. Yang, M. Kuang, H. Duan, Y. Xiong, H. Wei and A. Wang, *Biomaterials*, 2011, **32**, 9758; A. K. Gupta and M. Gupta, *Biomaterials*, 2005, **26**, 3995
8. M. N. V. Ravi Kumar, R. A. A. Muzzarelli, C. Muzzarelli, H. Sashiwa and A. J. Domb, *Chem Rev* 2004, **104**, 6017; Y. Yi, L. Q. Wu, W. E. Bentley, R. Ghodssi, G. W. Rubloff, J. N. Culver and G. F. Payne, *Biomacromolecules* 2005, **6**, 2881
 9. E. Frohlich, *Int J Nanomed* 2012, **7**, 5577; Y. Ge, Y. Zhang, J. Xia, M. Ma, S. He, F. Nie and N. Gu, *Colloids Surf B: Biointerfaces* 2009, **73**, 294; Z. G. Yue, W. Wei, P. P. Lv, H. Yue, L. Y. Wang, Z. G. Su and G. H. Ma, *Biomacromolecules* 2011, **12**, 2440
 10. I. Takeshi, H. Yumehiro, N. Ken-ichi, I. Yoshiaki, T. Keigo, A. Satoka, H. Ryuichi and K. Akio, *Anal. Biochem.*, 2009, **385**, 132; A.K. Minkstimiene, A. Ramanaviciene, J. Kirlyte and A. Ramanavicius, *Anal. Chem.* 2010, **82**, 6401; G. Shen, C. Cai, K. Wang and J. Lu, *Anal. Biochem.* 2011, **409**, 22; T. Q. Huy, N. T. H. Hanh, P. V. Chung, D. D. Anh, P. T. Nga and M. A. Tuan, *Appl. Surf. Sci.* 2011, **257**, 7090.
 11. C. Blanco-Andujar. Sodium carbonate mediated synthesis of iron oxide nanoparticles to improve magnetic hyperthermia efficiency and induce apoptosis. *PhD thesis, University College London, London, UK.* 2014.
 12. M. Alam, M. Sultana, G. B. Nair, A. K. Siddique, N. A. Hasan, R. B. Sack, D.A. Sack, K.U. Ahmed, A. Sadique, H. Watanabe, C.J. Grim, A. Huq and R. R. Colwell, *Proc. Natl. Acad. Sci. USA*, 2007, **104**, 17801; A. Safa, G. B. Nair and R. Y. C. Kong, *Trends Microbiol.*, 2010, **18**, 46; K Bahrain and S. K. Bhattacharya. *Curr. Top. Microbiol. Immunol.* 2014. DOI:10.1007/82_2014_362
 13. J.A. Hasan, A Huq, G.B Nair, S. Garg, A.K. Mukhopadhyay, L. Loomis, D. Bernstei and R. R. Colwell, *J Clin Microbiol.* 1995, **33**, 2935
 14. H. W. Gu, P. L. Ho, K. W. T. Tsang, L. Wang and B. Xu, *J. Am. Chem. Soc.* 2003, **125**, 15702
 15. J. Gao, L. Li, P.-L. Ho, G. C. Mak, H. Gu and B. Xu, *Adv. Mater.* 2006, **18**, 3145
 16. Y. Cheng, Y. Liu, J. Huang, K. Li, W. Zhang, Y. Xian and L. Jin. *Talanta*, 2009, **77**, 1332
 17. H. J. Chung, C. M. Castro, H. Im, H. Lee and R. Weissleder, *Nat. Nanotech.*, 2013, **8**, 369