

# Lab on a Chip

Accepted Manuscript



This is an *Accepted Manuscript*, which has been through the Royal Society of Chemistry peer review process and has been accepted for publication.

*Accepted Manuscripts* are published online shortly after acceptance, before technical editing, formatting and proof reading. Using this free service, authors can make their results available to the community, in citable form, before we publish the edited article. We will replace this *Accepted Manuscript* with the edited and formatted *Advance Article* as soon as it is available.

You can find more information about *Accepted Manuscripts* in the [Information for Authors](#).

Please note that technical editing may introduce minor changes to the text and/or graphics, which may alter content. The journal's standard [Terms & Conditions](#) and the [Ethical guidelines](#) still apply. In no event shall the Royal Society of Chemistry be held responsible for any errors or omissions in this *Accepted Manuscript* or any consequences arising from the use of any information it contains.

**An integrated microspectrometer for localised multiplexing measurements**

Zhixiong Hu<sup>a,b</sup>, Andrew Glidle<sup>a</sup>, Charles Ironside<sup>a</sup>, Jon Cooper<sup>a</sup>, Huabing Yin<sup>a\*</sup>

<sup>a</sup> Division of Biomedical Engineering, School of Engineering, University of Glasgow, Glasgow, UK.

<sup>b</sup> Division of Medical and Biological Measurements, National Institute of Metrology, Beijing, P.R.China.

\*Corresponding authors: [huzhixiong@nim.ac.cn](mailto:huzhixiong@nim.ac.cn) and [huabing.yin@glasgow.ac.uk](mailto:huabing.yin@glasgow.ac.uk)

**ABSTRACT**

We describe the development of an integrated, lensed Arrayed Waveguide Grating (AWG) microspectrometer for localized multiplexing fluorescence measurements. The device, which has a footprint of only 1mm wide and 1cm long, is capable of spectroscopic measurements on chip. Multiple fluorescence signals were measured simultaneously based upon simple intensity readouts from a CCD camera. We also demonstrate the integration of the AWG spectrometer with a microfluidics platform using a lensing function to confine the beam shape for focused illumination. This capability enhances signal collection, gives better spatial resolution, and provides a route for the analysis of small volume samples (e.g. cells) in flow. To show these capabilities we developed a novel “bead-AWG” platform with which we demonstrate localized multiplexed fluorescence detection either simultaneously or successively. Such an integrated system provides the basis for a portable system capable of optical detection of multi-wavelength fluorescence from a single, defined location.

**Keywords:**

Microspectrometer, fluorescence, optical sensors, focusing effect, microfluidics.

## INTRODUCTION

Portable diagnostic systems, such as lab-on-a-chip devices, are widely perceived as being promising platforms to address health care challenges worldwide as well to offer possibilities for emerging applications in remote settings.<sup>1-6</sup> Although most of these systems have demonstrated the ability to accommodate several steps involved in an assay (e.g. separation, purification and concentration) on chip, many of them still rely on conventional instrumentation for detection. This is especially the case for those relying on optical detection - the method most widely employed in biological and chemical analysis<sup>7-9</sup>. The needs for low cost, sensitive and portable optical microengineered spectroscopic detection systems are still to be met.

Fluorescence detection is perhaps the most commonly used optical method in biological analysis, due to its high sensitivity and specificity. It remains the method of choice in many optical microsystems<sup>3,10,11</sup>. Fluorescence detection requires efficient separation of fluorescence from excitation light, which is commonly achieved by filtering technology<sup>12</sup>. Although many examples have demonstrated the integration of optical elements for on-chip fluorescence measurement<sup>13-19</sup>, (using optical fibers<sup>15,16</sup>, planar waveguides<sup>1,17</sup> and on-chip filters<sup>18,19</sup>) these systems are often fabricated for a specific range of wavelengths of a particular fluorophore. For applications that require simultaneous detection of multiple fluorophores (e.g microflow cytometry), detection is still conducted off-chip using conventional filters and detectors<sup>20</sup>.

At the microengineering level, spectroscopic analysis (e.g. fluorescence, Raman, IR spectroscopy) has been well established for a vast range of applications. Previously, we have demonstrated a proof-of-concept that a monolithic integrated Arrayed Waveguide Grating (AWG) microspectrometer can be used to discriminate different wavelengths in the visible wavelength range<sup>21</sup>, thereby enabling multiplexed fluorescence analysis. In this work, we now build upon our initial demonstrator and show the development of a focusing AWG device for localized microspectroscopic measurements of a single point enabling new methods for the control the light pathway and for implementing sample spatial location within the microsystem.

Lenses are key optical elements for focusing light to a sample, collecting the specific signals of interest. Although this can be easily achieved using commercially available objective lenses in the case of conventional bulky instrumentation, incorporation of on-chip microlenses (e.g. fluid-filled polymer lenses<sup>22</sup>, ball lenses<sup>23</sup>, and microlens arrays<sup>17</sup>) requires demanding fabrication processes. Similarly, microfabricated structures provide effective means for controlling the sample on chip<sup>24-26</sup>. However,

when combined with an optical microsystem, precise control of samples is restricted by the limitations of the microsystem (e.g. fabrication, detection and physical dimensions).

In this work we purpose designed lens-aided waveguides, introducing a focusing effect onto the AWG microspectrometer. To enable precise control of samples for localized detection, integration of the device with other instruments was explored in two formats, namely in a flow format with an integrated microfluidic device and in a microwell format with immobilized functional beads. The former allows continuous, multiplex analysis of samples with high sensitivity and spatial resolution (with the potential for many applications, for example, as a miniaturized microflow cytometer with the unique capability of spectroscopic analysis). The latter formed a novel “bead-AWG” device, allowing multiplexed detection of a series of associated events with minimal sample handling – all of these strengths make it an appealing platform for use in a remote setting.

## MATERIALS AND METHODS

### Device fabrication and integration

The dense arrayed waveguide grating section was fabricated as described previously<sup>21</sup>. To fabricate the designed lens radius and sample cuvette, e-beam lithography was used to define the curvature of the lens in a UVIII (Shipley) resist layer that was spun on top of the waveguide. This was followed by reactive ion etching (CHF<sub>3</sub>/Ar in a Oxford Instruments RIE80+ machine) to transfer the lens shape from the resist to the waveguide. These combined e-beam lithography – dry etching pattern transfer processes developed in-house have a success rate of >90% for features of these dimensions. An integrated AWG-microfluidic device was made by bonding a PDMS microfluidic chip to the AWG device via oxygen plasma treatment (100mW for 20s).

To create the “bead-AWG” device, functional beads were immobilized within the sample cuvette as detailed in Protocols & Scheme 1 & Figure S1 (supplementary information). Briefly, a gold disk with diameter of 40μm was patterned in the centre of the sample cuvette. The device was then immersed in a 5mM aqueous solution of cysteamine hydrochloride overnight to generate a NH<sub>2</sub>-terminated functionalised gold surface. Water-soluble “long arm” biotin was covalently linked to the gold disk using the ethyl(dimethylaminopropyl) carbodiimide /N-Hydroxysuccinimide (EDC/NHS) conjugation method. The resultant biotinylated surface serves as a binding site for immobilization of streptavidin coated microbeads and subsequent biotinylated quantum dot (QDs) binding events. The streptavidin coated microspheres with internal fluorophores (Flash Red, Excitation 660nm, Emission 690nm, diameter

0.97 $\mu$ m) were from Bangs Laboratories. The quantum dots were purchased from Invitrogen (Life Technologies Corporation).

### Device characterization and on chip fluorescence measurements

The spectral range and throughput of each output channel was characterized using a white light source (Anritsu MG922A) and a conventional spectrometer (TRIAX320 from JOBIN YVON). Optical images of the device were obtained using a fluorescence microscope. The fluorescence signal from the output channels of the integrated AWG device was recorded using a CCD camera (Figure S2, supplementary information). As a means of verification of the AWG outputs, measurements were simultaneously made using an objective lens placed above the cuvette and coupled to a spectrophotometer (Triax 320 spectrometer, Jobin Yvon) (Figure S2, supplementary information).

## RESULTS AND DISCUSSION

### Design and characterization of an AWG device with focusing waveguides

The design of the integrated AWG device with lensed waveguides is shown in Figure 1a. The AWG chip consists of five essential parts, including input waveguides (C-WG and E-WG), a 1st slab of arrayed waveguides, a 2nd slab region and output waveguides. These were designed around a center wavelength of 680 nm and channel–channel wavelength spacing of 10 nm for the output channels, as detailed previously<sup>21</sup>. The sample cuvette was located in front of the AWG input waveguide. The straight waveguide (C-WG) on the left is used for characterization while the curved waveguide (E-WG) is to introduce excitation light for fluorescence measurements.

To introduce the focusing effects, lens curvatures were incorporated into the ends of the input and collect waveguides (I-AWG), as shown in Figure 1b. The design of the curvature and spacing of the end facets take into account the refractive indexes of the waveguides and the aqueous sample solution according to equation 1<sup>27,28</sup>,

$$\frac{1}{f} = (n_{WG} - n_{H_2O}) \frac{1}{R}, \quad \text{Equation 1}$$

where  $f$  is the focal length,  $R$  is the radius of the lens curvature,  $n_{WG}$  and  $n_{H_2O}$  are the refractive indexes of the waveguide material and water respectively ( $n_{WG}=1.478$ ,  $n_{H_2O}=1.33$ ).

Simulation using Beam Propagation Method (BPM) was used to understand the beam shape from both lensed and flat end waveguides (Figure 1b & 1c). A focusing and strong coupling effect was observed for the lensed waveguide (Figure 1b). In contrast, diverging light paths were seen for the flat end waveguide (Figure 1c). Based on the simulation, a two-dimensional lens with radius of 4  $\mu\text{m}$  was incorporated at the end of each of the three waveguides, which are intercepted by the sampling cuvette (Figure 1b). The three identical lenses share the same focal area, which is located in the center of the cuvette. With lens curvature at the end of integrated waveguide focused excitation and highly localized collection could be realized.

The transmission spectrum of each channel in the lensed AWG device is shown in Figure 2. The full width half maximum (FWHM) of each output peak was  $\sim 10$  nm, consistent with the design. Similar to a conventional diffraction grating, an AWG device generally has more than one order, which can be used for light dispersion. As an illustration, the transmission spectrum for two diffraction orders ( $m=7$  and  $m=8$ ) are shown in Figure 2, where the free spectral range (i.e. the largest wavelength range for a given order that does not overlap with the spectrum of adjacent order) is 80 nm. This periodicity allows selection of an effective wavelength range with order-sorting filter. For example, by inserting specific order-sorting filters (i.e. a bandpass filter) in front of the detector, the light to be investigated can be restricted to the wavelength range between 560 nm and 640 nm. In addition, using a cascade design for the AWG, a larger free spectral range can be achieved.

### **Evaluation of focusing effects in flow**

A simple integrated AWG-microfluidic platform was fabricated to evaluate the focusing capabilities of the lensed waveguides (Figure 3a). To investigate the spatial regions of the cuvette sampled by each of the waveguides, a fluorescent dye solution (10  $\mu\text{M}$  Cy5) was delivered into the microfluidic channel at a flow rate of 6.7 mm/s. Laser light (632.8 nm) was then introduced into the cuvette area through C-WG, E-WG and the appropriate output channel (i.e. Ch 8) waveguides in turn (Figure 3b). (Note, Ch 8 is the specific channel that will allow 632.8 nm light to traverse the slab regions of the AWG device and exit from the AWG input waveguide). Cy5 molecules in the light path were excited and fluorescence emitted at longer wavelengths (670 nm). This emission was imaged using an upright fluorescence microscope with a Cy5 filter cube, allowing easy visualization of the light path from each of the three waveguides (Figure 3b (i, ii, and iii)).

With the lensed waveguides, the focusing effect can be seen clearly in Figure 3b. Figure 3b (iv) is a composite image of the light paths corresponding to the three waveguides, using different colors to label

each path. A tight intersection of the three light paths was clearly seen in the middle of the sample cuvette, illustrating the capability of lens-aided focusing for localised collection. In contrast, for the AWG system without lensing, each of the light paths associated with the waveguides field of view are inherently divergent, as shown in Figure 3c.

This lens-aided focusing capability for confining beam shape offers obvious advantages by enhancing signal collection: Focusing light to a small spot can increase fluorescence emission, and likewise collecting light from a highly localized area and can greatly reduce unwanted signals from light scattered by other features/objects nearby. In addition, the AWG device can be integrated with hydrodynamic focusing microfluidics to deliver the objects of interest into the focused region<sup>29</sup>. This, in conjunction with its capability for fluorescence multiplexing measurements, makes it an appealing platform for a broad range of applications such as microflow cytometry and fast diagnostics.

#### **Localized spectroscopic measurements with a “bead-AWG” format**

Assays that offer easy operation and fast “yes” or “no” answers are often highly desirable. In this context, bead based assays can be a promising choice. Beads have a large surface area, and therefore can serve as a solid phase for capturing targets and simplifying purification processes. Incorporated bead assays within microfluidics have showed promise for applications in diagnostic tests<sup>30, 31</sup> to multiplexing bioassays<sup>32</sup>, although signal detection still relies on external, bulky instrumentation. The combination of bead assays with the “AWG” platform could therefore provide a miniaturized platform offering both easy operation and multiplexed measurements.

As a proof of concept, streptavidin coated beads were immobilized within the biotin functionalized sample cuvette via specific streptavidin-biotin binding (Protocols detailed in supplementary information). This allowed the whole process (i.e. capturing of targets, purification and detection) to occur at a defined location. Since streptavidin-biotin binding is reversible, the immobilised beads from one assay can be easily removed and replaced with fresh ones in performing a second assay.

A patterned gold disk was used to immobilize microbeads at a defined location within the sample cuvette (Figure 4a). An optimized incubation time of 30 minutes was employed to reduce non-specific absorption of beads. As shown in Figure 4b, the beads closest to the E-WG excitation waveguide were illuminated most strongly and partially occluded those on more distant parts of the gold disk. This indicates that in an optimized device it might be beneficial to reduce the size of the central sampling



area. Nevertheless, the configuration used here still allowed for effective collection of the fluorescence signal from the immobilized beads by the AWG input waveguide as detailed in the following section.

### **Localized spectroscopic measurements allowing successive fluorescence detection**

Fluorescence detection via filter technologies requires efficient removal of the other wavelengths except for the fluorescence of interest. This can be a problem for samples containing natural fluorescent substances (e.g. GFP cells or bacteria cells containing carotenoid) or high levels of autofluorescence. As an optical (de)multiplexer, the AWG device is capable of detecting multiple narrow emissions simultaneously by imaging the channel outputs directly onto a CCD. If a broad band of fluorescence measurements is required, the intensities in each of these images can be simply aggregated, with no loss in light collection efficiency. Thus, with the “bead - AWG” format, it is feasible to detect fluorescence signals from a series of successive events/targets through collection of a series of CCD images for each channel.

As a model system, streptavidin coated microbeads with flash red fluorescence labels (central emission peak at 690 nm), 605 nm biotin conjugated quantum dots (605-QDs) and 655 nm streptavidin conjugated quantum dots (655-QDs) were employed. Successive assembly of the 690 nm microbeads to the gold disk, followed by 605- QDs and then 655-QDs was evaluated on chip, step-by-step.

Figure 5 shows the fluorescence spectra (on the left) collected using the spectrophotometer and the CCD images of selected output channels (on the right). The intensity of each channel in the CCD images are also displayed as histograms for easy comparison and quantification. Note, only the AWG output channels, Ch4, Ch5 and Ch1 are shown since these correspond to the central wavelengths of the three fluorophores employed (i.e. 682 nm is detected in Ch4, 605 nm in Ch5 and 655 nm in Ch1).

It is clear that after adsorption of the flash red fluorescent microbeads, the peak of the fluorescence spectrum was at 690 nm (Figure 5a, left graph) and as expected, Ch4 was found to have the brightest spot (Figure 5a, right graph) with weaker spots being found in the other two channels due to the broad spectrum of the flash red fluorescence emission. After the addition of the 605-QDs, a peak around 605 nm was observed in the fluorescence spectrum (Figure 5b), and the highest level of light intensity was found in Ch5 of the CCD image. The high wavelength spectral tail in Figure 5b (i.e. left graph) reveals that the CCD image was a combination of fluorescence emission from both the quantum dots and the flash red fluorescence. In the same way, addition of 655-QDs caused the brightest spot to move to Ch1

(Figure 5c). The relative fluorescence intensity for each binding step is presented in Table 1. The channel with the highest intensity corresponds well to the emission peak of the latest targets.

Finally, to verify the reversibility of the immobilization process, the sampling cuvette was washed with a biotin solution three times. Having done this, it was found that the fluorescence signal was too weak to be detected by either the TRIAX spectrophotometer or CCD camera, indicating the absence of microbeads and quantum dots. This enables the device to be reused for further measurements.

Taken together, these results conceptually prove the great potential of “additive” fluorescence assays with the “bead-AWG” device. It has no demanding requirements for eliminating non-targeted fluorescence, and is capable of detecting a series of associated events in a simple readout (e.g. an optical image).

## CONCLUSIONS

We have developed a portable AWG microspectrometer for localized multiplex measurements. Using an integrated AWG-microfluidics platform, we demonstrated that the lensing function of the device confined the beam shape for focused illumination and signal collection. This capability can enhance signal collection and give better spatial resolution, and would benefit analysis of small volume samples (e.g. cells) in flow. Future integration of the focusing AWG device with advanced microfluidics and lab-on-a-chip platform will have great potential for applications that require both sophisticated handling of samples and versatile detection capability, for example, those requiring simultaneous multiplexing measures.

In addition, we have developed a “bead-AWG” method capable of localized fluorescence detection for a series of events. This new detection method can detect fluorescence of interest without the need of isolation from the background (which would normally be required if using current technologies). Furthermore, it is capable of measuring several events simultaneously or successively, and reporting these results in a simple image readout. Considering the small footprint of the device, simple assay procedure and visually direct readout, it can serve as a promising portable platform for fast analysis in remote settings where resource and specialized skills are limited.

## ACKNOWLEDGMENTS

Z.H thanks the support from the Chinese Council Scholarship and the University of Glasgow for his scholarship. We also thank partial support from EPSRC (EP/H04986X/1 and EP/J009121/1). We

gratefully acknowledge the technical team of the James Watt Nanofabrication Centre (JWNC) at University of Glasgow for the support in fabricating the devices. JMC acknowledges the support of ERC Bio-Phononics, 340117 and EPSRC Advanced Fellowship award, EP/K027611/1.

## SUPPORTING INFORMATION

The protocol for the bead immobilization procedure, and schematic set-up of microbeads based multiplexing fluorescence assay are provided in detail.

## REFERENCES

1. C. H. Ahn, J. W. Choi, G. Beaucage, J. H. Nevin, J. B. Lee, A. Puntambekar and J. Y. Lee, *Proc. IEEE*, 2004, **92**, 154-173.
2. S. Balslev, A. M. Jorgensen, B. Bilenberg, K. B. Mogensen, D. Snakenborg, O. Geschke, J. P. Kutter and A. Kristensen, *Lab Chip*, 2006, **6**, 213-217.
3. S. M. Borisov and O. S. Wolfbeis, *Chem. Rev.*, 2008, **108**, 423-461.
4. M. Bally, M. Halter, J. Voros and H. M. Grandin, *Surf. Interface Anal.*, 2006, **38**, 1442-1458.
5. P. Yager, T. Edwards, E. Fu, K. Helton, K. Nelson, M. R. Tam and B. H. Weigl, *Nature*, 2006, **442**, 412-418.
6. L. Bissonnette and M. G. Bergeron, *Clin. Microbiol. Infect.*, 2010, **16**, 1044-1053.
7. J. P. Golden, J. S. Kim, J. S. Erickson, L. R. Hilliard, P. B. Howell, G. P. Anderson, M. Nasir and F. S. Ligler, *Lab Chip*, 2009, **9**, 1942-1950.
8. K. Goda, A. Ayazi, D. R. Gossett, J. Sadasivam, C. K. Lonappan, E. Sollier, A. M. Fard, S. C. Hur, J. Adam, C. Murray, C. Wang, N. Brackbill, D. Di Carlo and B. Jalali, *Proc. Natl. Acad. Sci. U. S. A.*, 2012, **109**, 11630-11635.
9. J. Skommer, J. Akagi, K. Takeda, Y. Fujimura, K. Khoshmanesh and D. Wlodkowic, *Biosens. Bioelectron.*, 2013, **42**, 586-591.
10. A. Pais, A. Banerjee, D. Klotzkin and I. Papautsky, *Lab Chip*, 2008, **8**, 794-800.
11. E. Thrush, O. Levi, W. Ha, G. Carey, L. J. Cook, J. Deich, S. J. Smith, W. E. Moerner and J. S. Harris, *IEEE J. Quantum Electron.*, 2004, **40**, 491-498.
12. O. Hofmann, X. H. Wang, A. Cornwell, S. Beecher, A. Raja, D. D. C. Bradley, A. J. deMello and J. C. deMello, *Lab Chip*, 2006, **6**, 981-987.
13. F. B. Myers and L. P. Lee, *Lab Chip*, 2008, **8**, 2015-2031.
14. K. Misiakos, P. S. Petrou, S. E. Kakabakos, D. Yannoukakos, H. Contopanagos, T. Knoll, T. Velten, M. DeFazio, L. Schiavo, M. Passamano, D. Stamou and G. Nounesis, *Biosens. Bioelectron.*, 2010, **26**, 1528-1535.
15. Y. C. Tung, M. Zhang, C. T. Lin, K. Kurabayashi and S. J. Skerlos, *Sens. Actuator B-Chem.*, 2004, **98**, 356-367.
16. M. L. Chabinye, D. T. Chiu, J. C. McDonald, A. D. Stroock, J. F. Christian, A. M. Karger and G. M. Whitesides, *Anal. Chem.*, 2001, **73**, 4491-4498.
17. P. Kozma, A. Lehmann, K. Wunderlich, D. Michel, S. Schumacher, E. Ehrentreich-Forster and F. F. Bier, *Biosens. Bioelectron.*, 2013, **47**, 415-420.
18. M. Dandin, P. Abshire and E. Smela, *Lab Chip*, 2007, **7**, 955-977.
19. Y. Fainman, M. P. Nezhad, D. T. H. Tan, K. Ikeda, O. Bondarenko and A. Grieco, *Appl. Optics*, 2013, **52**, 613-624.
20. N. Hashemi, J. S. Erickson, J. P. Golden, K. M. Jackson and F. S. Ligler, *Biosens. Bioelectron.*, 2011, **26**, 4263-4269.

21. Z. X. Hu, A. Glidle, C. N. Ironside, M. Sorel, M. J. Strain, J. Cooper and H. B. Yin, *Lab Chip*, 2012, **12**, 2850-2857.
22. J. Godin, V. Lien and Y. H. Lo, *Appl. Phys. Lett.*, 2006, **89**.
23. Y. J. Fan, Y. C. Wu, Y. Chen, Y. C. Kung, T. H. Wu, K. W. Huang, H. J. Sheen and P. Y. Chiou, *Biomicrofluidics*, 2013, **7**.
24. H. B. Yin and D. Marshall, *Curr. Opin. Biotechnol.*, 2012, **23**, 110-119.
25. J. C. Jokerst, J. M. Emory and C. S. Henry, *Analyst*, 2012, **137**, 24-34.
26. D. Mark, S. Haeberle, G. Roth, F. von Stetten and R. Zengerle, *Chem. Soc. Rev.*, 2010, **39**, 1153-1182.
27. K. W. Ro, K. Lim, B. C. Shim and J. H. Hahn, *Anal. Chem.*, 2005, **77**, 5160-5166.
28. P. Nussbaum, R. Volke, H. P. Herzig, M. Eisner and S. Haselbeck, *Pure Appl. Opt.*, 1997, **6**, 617-636.
29. S. H. Cho, J. M. Godin, C. H. Chen, W. Qiao, H. Lee and Y. H. Lo, *Biomicrofluidics*, 2010, **4**.
30. P. B. Monaghan, K. M. McCarney, A. Ricketts, R. E. Littleford, F. Docherty, W. E. Smith, D. Graham and J. M. Cooper, *Anal. Chem.*, 2007, **79**, 2844-2849.
31. T. Aytur, J. Foley, M. Anwar, B. Boser, E. Harris and P. R. Beatty, *J. Immunol. Methods*, 2006, **314**, 21-29.
32. S. Rauf, A. Glidle and J. M. Cooper, *Chem. Commun.*, 2010, **46**, 2814-2816.

**Figure captions:**

Figure 1. Figure showing (a) the configuration of a typical AWG device. C-WG: white light characterisation waveguide. E-WG: excitation waveguide. I-AWG: AWG input waveguide. (b) the design and simulation of (i) focusing waveguides and (ii) flat end waveguides.

Figure 2. Figure showing normalized transmission spectral response of the AWG device for two different diffraction orders:  $m=7$  and  $m=8$ . The 8 output channels were numbered in order from shorter to longer wavelength.

Figure 3. Figure showing (a) a schematic of the integrated AWG-microfluidic platform. (b) fluorescence microscopic images of the optical system with the lens waveguides. (c) fluorescence microscopic images of the optical system with the flat-end waveguides. For both the systems, a Cy5 fluorescent dye solution was delivered into the microfluidic channel and a laser excitation light (632.8 nm laser) was introduced into different integrated waveguides: (i) C-WG; (ii) E-WG; (iii) AWG input waveguide. By filtering the excitation light, the fluorescence microscopic images of the cuvette area were acquired respectively and (iv) is their composite image by using different colors for each light path. The arrows in (i) to (iii) indicate the direction of laser excitation. In (iv), the intersection area of the three light paths is highlighted with a pink dashed circle.

Figure 4. Figure showing (a) the gold disk pattern in the centre of the sampling cuvette and (b) fluorescence image of the cuvette with adsorbed flash Red fluorescence microbeads. The beads were excited with 633nm laser through the E-WG waveguide. The borders of the sampling cuvette and the three integrated waveguides were marked with grey dashed lines.

Figure 5. Showing fluorescence spectra and corresponding AWG and CCD detection results of the flow (successive) assay. The figure comprises (a) micrograph of flash red fluorescence micro beads. A 650 nm long pass filter in the light path to totally eliminate the 633 nm excitation signal (n.b. the detected light corresponds to the AWG diffraction order  $m=7$ ); (b) as above, after addition of 605 nm biotin conjugated quantum dots and 532 nm laser excitation with a 550 nm long pass filter (selecting diffraction orders  $m=7$  and  $m=8$ ); (c) as for (b) after addition of 655nm streptavidin conjugated quantum dots. On the left are the pre-acquired fluorescence spectra while the right provides the CCD images of specific output channels and their histograms of light intensity maximum. Error bars are standard deviations from at least three independent, repeated experiments.

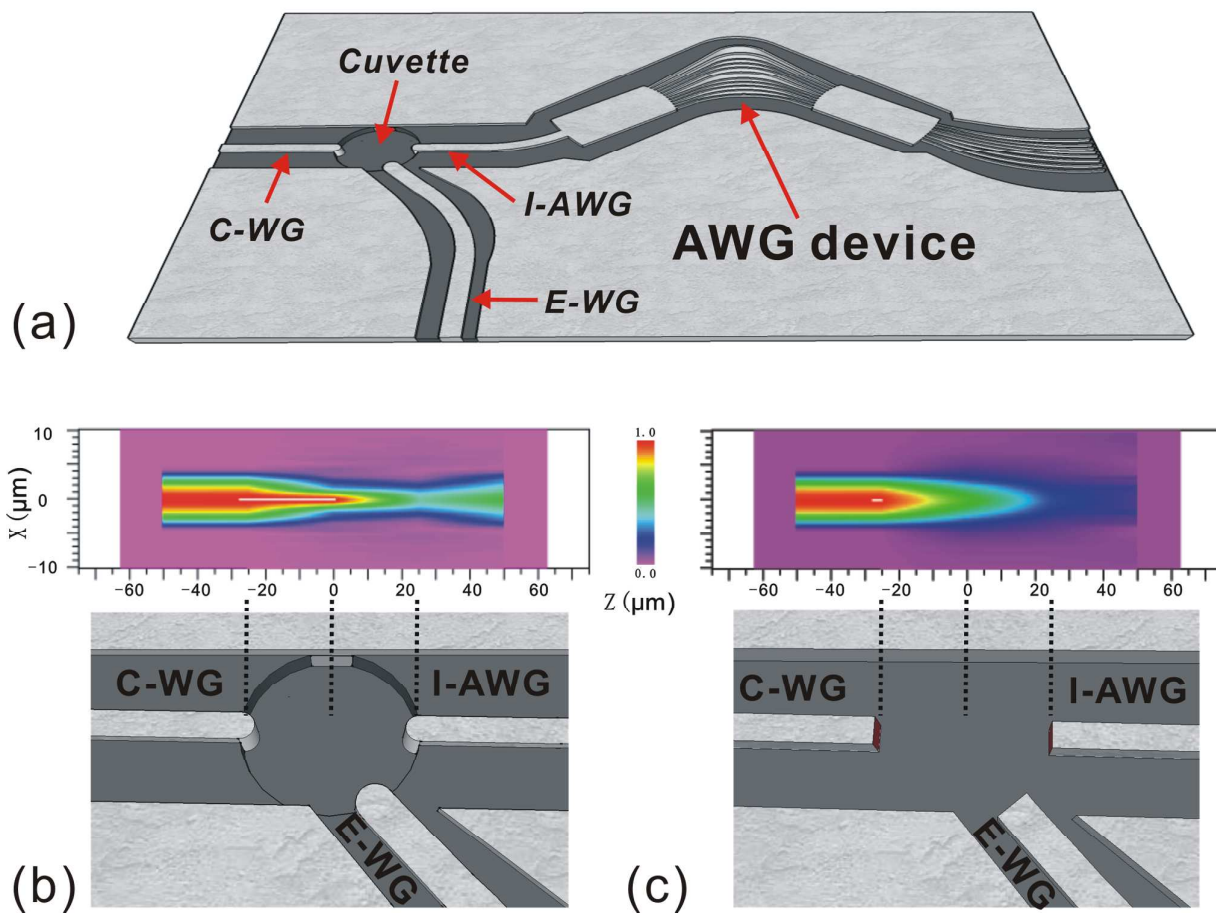


Figure 1.

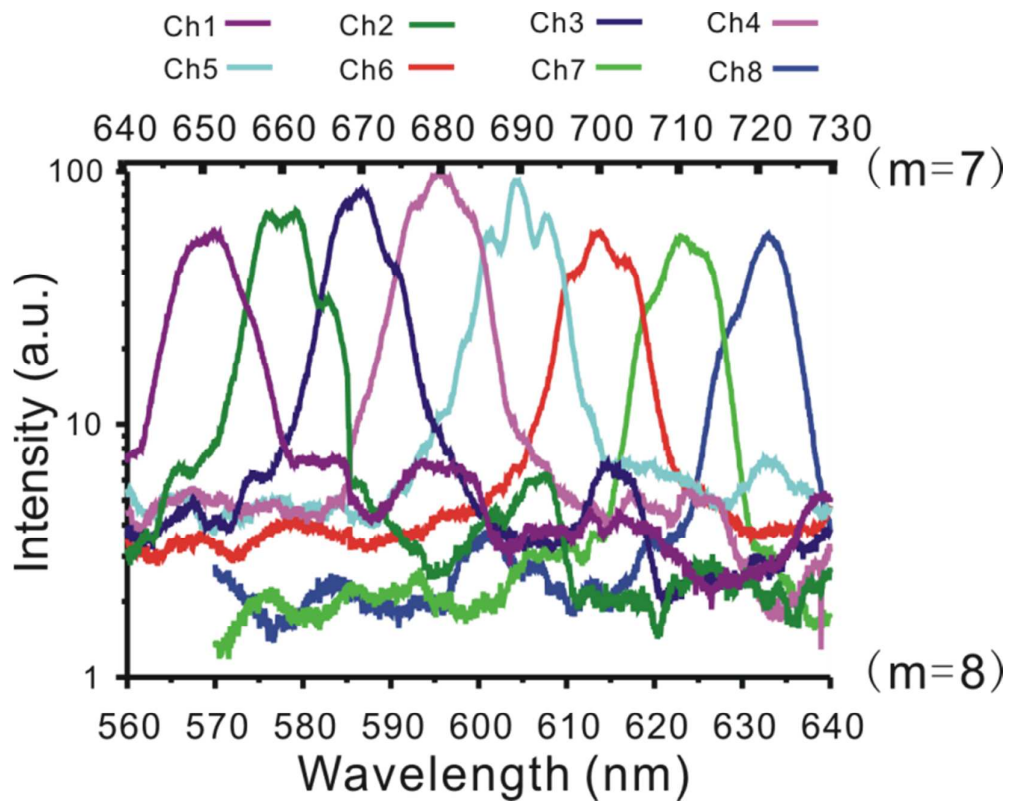


Figure 2.

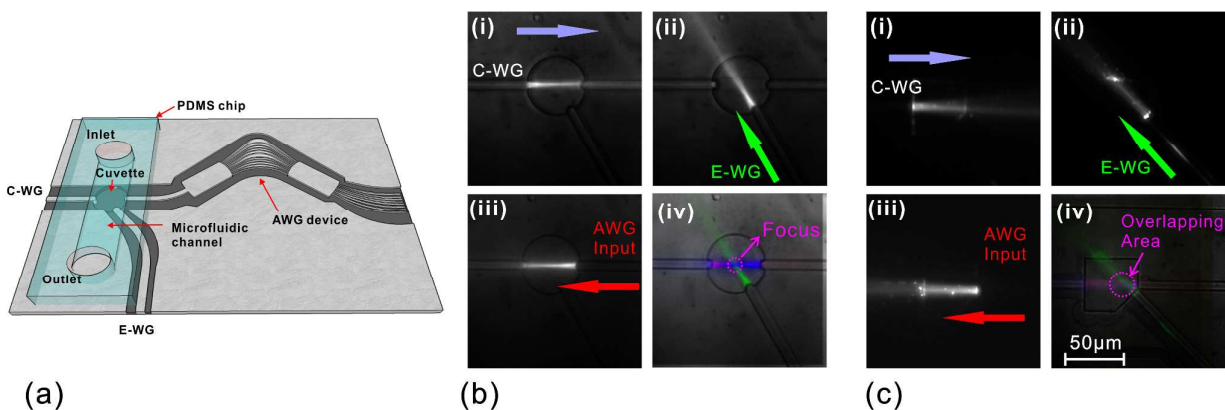


Figure 3.

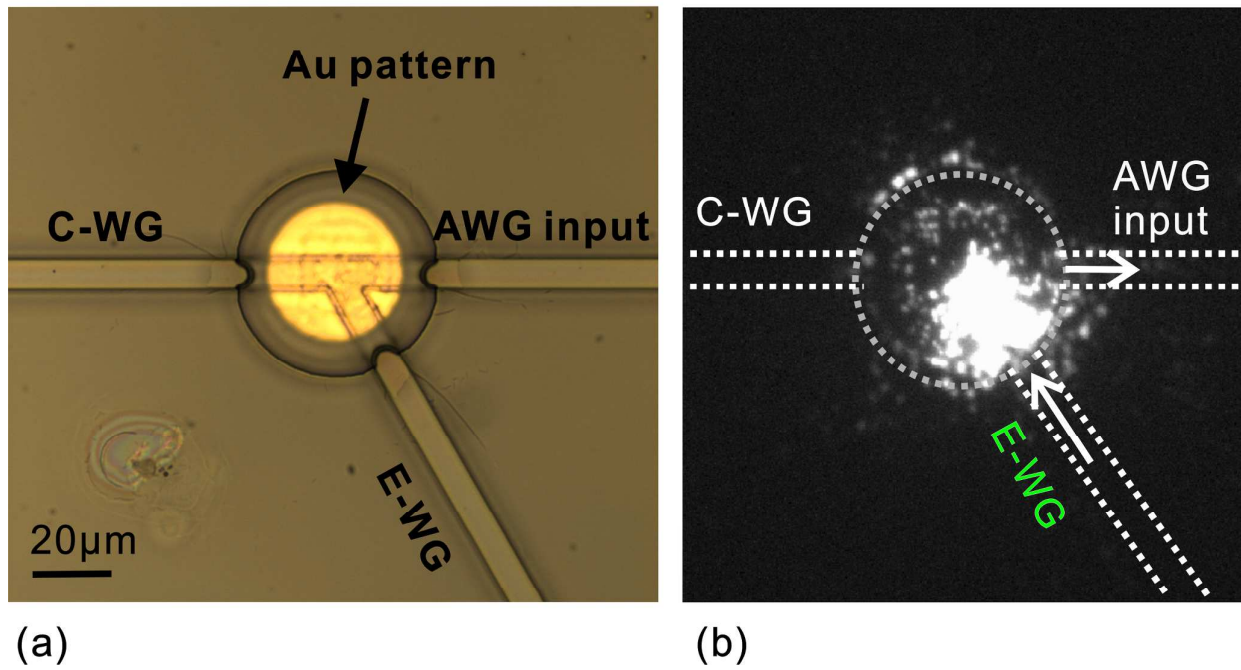


Figure 4.



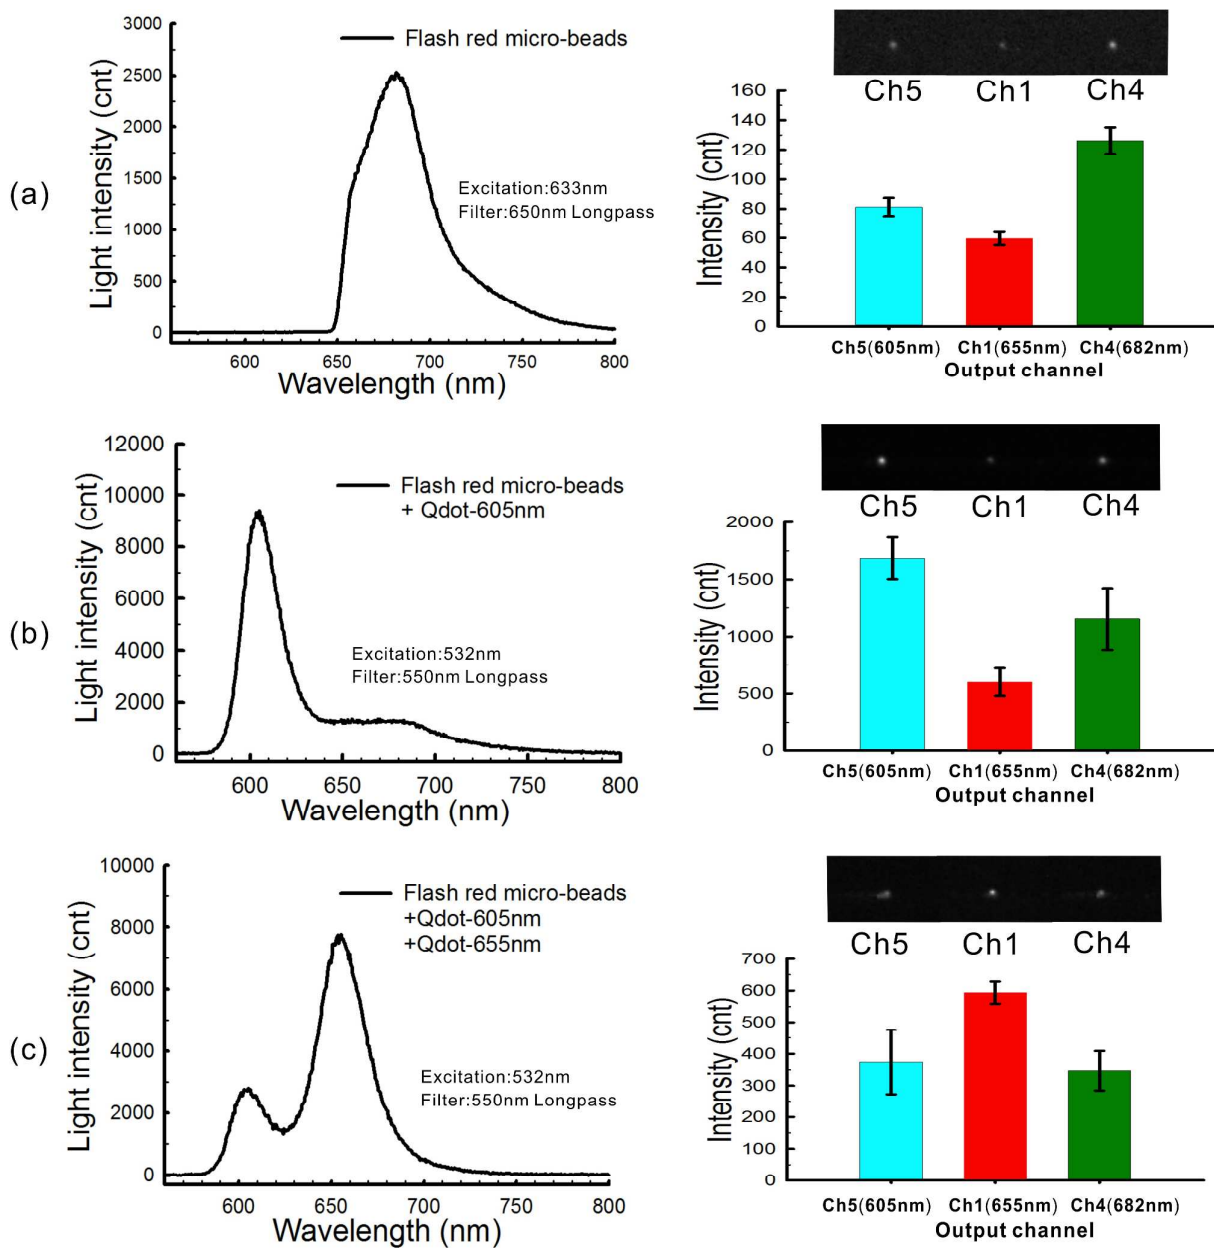


Figure 5.

Table 1. Relative fluorescence intensity for each binding step\*

Relative Intensity	Ch4	Ch5	Ch1
A (/Ch4)	1	0.64	0.47
B (/Ch5)	0.68	1	0.36
C (/Ch1)	0.58	0.63	1

\* A-flash red fluorescence microbeads. B- after adding biotin conjugated quantum dots (605 nm). C - after adding streptavidin conjugated quantum dots (655 nm).