

RSC Advances




This is an *Accepted Manuscript*, which has been through the Royal Society of Chemistry peer review process and has been accepted for publication.

Accepted Manuscripts are published online shortly after acceptance, before technical editing, formatting and proof reading. Using this free service, authors can make their results available to the community, in citable form, before we publish the edited article. This *Accepted Manuscript* will be replaced by the edited, formatted and paginated article as soon as this is available.

You can find more information about *Accepted Manuscripts* in the [Information for Authors](#).

Please note that technical editing may introduce minor changes to the text and/or graphics, which may alter content. The journal's standard [Terms & Conditions](#) and the [Ethical guidelines](#) still apply. In no event shall the Royal Society of Chemistry be held responsible for any errors or omissions in this *Accepted Manuscript* or any consequences arising from the use of any information it contains.

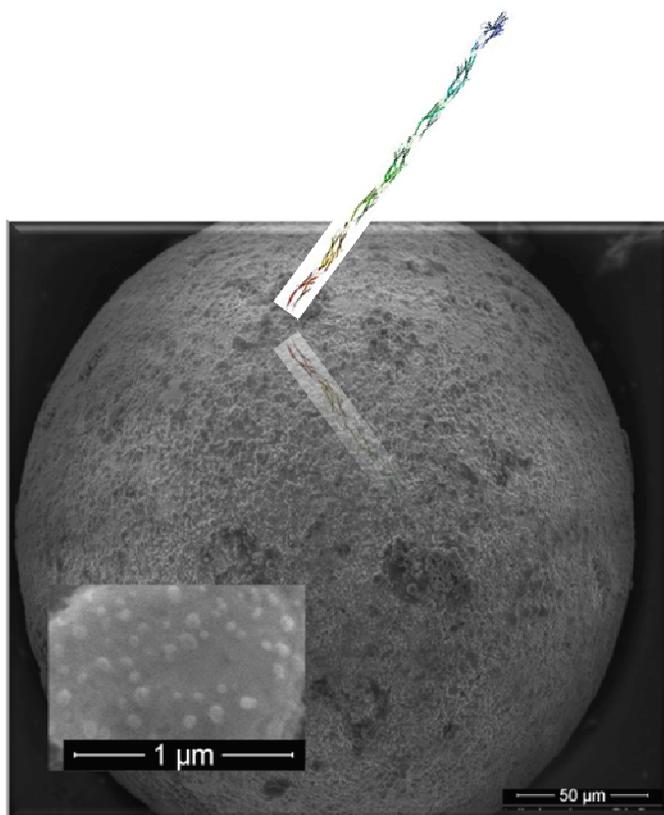

Engineered nanoporous gold microspheres based stochastic sensors detect carcynoembrionic antigen in a concentration as low as 16ng/mL in whole blood.

Engineered Nanoporous Gold Microspheres for Stochastic Sensing

Raluca-Ioana Stefan-van Staden^{1,2,*}, Iuliana Moldoveanu^{1,2}, Cristina Carmen Surdu-Bob³,
Camelia Stanciu-Gavan⁴

¹Laboratory of Electrochemistry and PATLAB Bucharest, National Institute of Research for Electrochemistry and Condensed Matter, Splaiul Independentei No.202, Bucharest, Romania.

²Faculty of Applied Chemistry and Material Science, Politehnica University of Bucharest, Bucharest, Romania.

³Low Temperature Plasma Laboratory, National Institute for Lasers, Plasma and Radiation Physics (NILPRP), Str. Atomistilor 409, Magurele, Romania

⁴Department of Surgery 4, University of Medicine and Pharmacy “Carol Davila”, Bucharest, Romania

Abstract

Engineered nanoporous gold microspheres were designed and used as new materials for stochastic microsensors. Carcinoembryonic antigen was used as model analyte to prove the stochastic sensing capabilities of the new material. New sensor based on gold particles was used for assay of carcinoembryonic antigen in biological fluids. Stochastic sensing was used to determine the antigen in samples. The working concentration range of the stochastic microsensor (1.6×10^{-8} - 1.6×10^{-5} mg/mL) as well as its sensitivity (3.0×10^3 s mg/mL) and limit of quantification (16ng/mL) made possible its reliable utilization for screening tests of whole blood for carcinoembryonic antigen.


Keywords: nanoporous gold microsphere, stochastic sensing, carcinoembryonic antigen

* Corresponding author: Tel. +40751507779; Fax +4021 3163113; e-mail: iustinavanstaden@yahoo.com

Introduction

Bayley and Cremer demonstrated in 2001¹ the basic principles of stochastic sensing through a protein pore; they were also stating the importance of the stochastic sensing for qualitative and quantitative analysis and the principles associated ($1/t_{\text{on}} = A + B \times \text{Conc}_{\text{analyte}}$; t_{off} – used for qualitative analysis). Stochastic sensing (introduced for the first time in bioanalysis and biomedical analysis by Stefan-van Staden) is a powerful technique in biomedical analysis²⁻⁵. Pattern recognition of different antigens and neurotransmitters was possible by determining the signatures of each of them in the diagrams obtained using stochastic sensors and microsensors²⁻⁵.

Of high importance were both qualitative and quantitative analysis of the analytes, obtained in the two stage process of the stochastic sensing when a potential of a certain value was applied. The mechanism of current development consists on two stages: stage 1 on which the analyte extracted from the solution into the membrane-solution interface blocks the channel, the intensity of the current recorded being zero for a certain period of time, named signature of the analyte which is measured using t_{off} (the channel is losing the conductivity, and the intensity of current became 0); and stage 2 when the analyte (A) is interacting with the wall, the following equilibrium equation is taking place:



where Ch is the channel, and i is the interface.

Due to the fact that t_{off} value depends on: the size of the analyte, of its capacity of unfolding, geometry of the analyte, and velocity to pass through the channel, it is difficult to find two or

more analytes that will give the same value for t_{off} ; all these should correlate with size and geometry of the channel/pore. At this stage is difficult to predict which geometry or size will be the best for a certain analyte, especially for proteins like CEA, because the proteins are unfolding before going through the pores.¹ Accordingly, this method is selective, and it is not necessary to add antibodies, or other analytes in order to improve the selectivity. The principle of the recognition (based on blocking of a channel for a certain time) made from this method the only reliable electrochemical method for recognition (qualitative analysis) of a biomolecule in biological samples. Furthermore, the analytes are getting into the channel in a certain order, accordingly with their size and geometry, from the smallest to the biggest; these processes are giving the form of the signal.

In this paper, stochastic sensors based on engineered nanoporous gold microspheres were designed and used for chemical analysis. Carcinoembryonic antigen (CEA) was chosen as model analyte to prove the stochastic sensing capabilities of the new designed microsensor. Carcinoembryonic antigen is a glycoprotein discovered by Gold and Freedman^{6,7}, often associated with certain cancers. It is hardly present in the serum of healthy adults; but it appeared in the serum of patients with cancer⁸⁻¹⁵. To date, CEA (a protein biomarker used in cancer diagnosis and assessment of treatment) was detected using different techniques, including chemiluminescence¹⁶, radioimmunoassay¹⁷, ELISA (applied as standard method in clinical laboratories)¹⁸, and electrochemical techniques¹⁹⁻²². Circulating tumor cells are also analysed reliably using electrochemical and fluorescence based methods²³⁻²⁷.

Experimental

Materials and Reagents

CEA (carcinoembryonic antigen), monosodium phosphate, disodium phosphate were purchased from Aldrich (Milwaukee, USA); paraffin oil and NaN_3 were purchased from Fluka (Buchs, Switzerland). Monosodium phosphate and disodium phosphate were used for preparation of phosphate buffer 0.1 mol/L, pH = 7.4. Deionized water obtained from a Millipore Direct-Q 3 System (Molsheim, France) was used for the preparation of all solutions. All standard solutions were prepared in buffer solution pH=7.4, with NaN_3 0.1%.

Instrumentation

All voltammograms were recorded using a PGSTAT 12 potentiostat/galvanostat connected to a three-electrode cell, and connected to a computer via an Eco Chemie (Utrecht, The Netherlands) software version 4.9. A Pt electrode and an Ag/AgCl electrode served as the counter and reference electrodes for the cell. The working electrode was the microsensor based on engineered nanoporous gold microspheres. The pH measurements were performed using a CyberScan PCD 6500 Multiparameter.

Design of the stochastic microsensor

Engineered nanoporous 14 K gold microspheres were obtained using NILPRP. In order to obtain the nanopores on its surface, the particle was chemically corroded in an acid solution consisting of $\text{HCl}:\text{HNO}_3$ in a 3:1 ratio, for 15 minutes and then rinsed with deionized water. As different sizes of gold microsphere were obtained, micrometers were used to select the microspheres with a certain diameter – of 300 μm . A typical SEM image of the microsphere surface is presented in Figure 1a. A zoom in an area with a pore (able to show better the surface morphology) is shown

in Figure 1B. The stochastic micro-sensor was prepared as following: a 300 μm diameter gold nanoporous microparticle was tightly fixed inside a plastic tube together; a silver wire (diameter 150 μm) served as electrical connection to the external circuit (Figure 2). The active surface of the sensor was rinse in between measurements with distilled water, and gently dried with absorbent paper.

Stochastic sensing

For the stochastic sensing, a chronoamperometric technique was selected for the measurements of t_{on} and t_{off} at a constant potential of 125mV. The applied potential is the one driving the analyte through the channel/pore; accordingly, one should chose a value for which the signature value (t_{off}) can be read reliable – usually it is preferred to do not be lower than 1ms. The electrodes were dipped into a cell containing solutions of antigen of different concentrations. Values of t_{on} were read on the diagram, and the equation of calibration $1/t_{\text{on}} = f(\text{Conc.})$ for CEA was determined using statistics. The unknown concentrations of the CEA in whole blood samples were determined from the calibration equations.

Results and discussions

Response characteristics of the sensor based on gold particles used for screening of CEA.

The t_{off} of 2.9s serving as signature of CEA in biological fluids was determined while t_{on} values were used for assessing the equation of calibration ($1/t_{\text{on}} = A+B \times \text{Concentration}$). Statistic calculations used for the equation of calibrations were extended to determine the working concentration range, sensitivity, and the limit of quantification of the stochastic microsensor. The

stochastic microsensor proposed for the assay of CEA covered a linear concentration range between 16 and 1.6×10^4 ng/mL with a sensitivity of 3.00×10^3 s mg/mL. The lowest concentration of CEA that could be reliably determined was 16ng/mL. The microsensor was stable over a period of six months, when used daily for measurements, its sensitivity varying with a RSD less than 0.1%.

Analytical applications

Whole blood samples were obtained from eight confirmed breast cancer patients from the University Hospital in Bucharest (ethics committee approval nr. 11/2013). These samples were used for screening tests using the proposed stochastic microsensor without any pretreatment. Pattern recognition of CEA based on its signature was performed using typical diagrams recorded using the stochastic microsensor (Figure 3). The signature (t_{off} value) of CEA was identified in the patterns recorded (Figure 3) for whole blood samples – these results being in agreement with the standard method (ELISA) performed in the clinical laboratories of the hospital; after identifying the signature of the analyte, the t_{on} was measured and inserted in the calibration graph for determining the concentration of CEA (arrows were used in Figure 3 to show on the pattern selected where t_{on} and t_{off} values were measured). Table 1 shows the quantities of CEA found in the eight whole blood samples using both: the stochastic sensing as well as ELISA (the standard method). Blood samples were collected from ten healthy people (negative control) and analysed with the proposed method as well with ELISA; the signature of CEA (value of t_{off}) was not found in any diagram recorded for these patients, this result being confirmed by ELISA method.

Statistical analysis based on pair t-test was performed for a confidence level of 99.00%. The results have shown that there is no significant difference between the values obtained using the

stochastic microsensor and ELISA (standard method) at 99.00% confidence level ($t_{\text{theoretical}}=4.032$). The comparison refers to paired data.

Conclusions

The new material based on engineered nanoporous gold microsphere is an excellent material for the design of stochastic microsensors with features for biomedical analysis. For carcinoembryonic antigen – selected as model analyte, high sensitivity and low limit of determination was recorded. The microsensor was validated using whole blood samples obtained from confirmed patients. The stochastic microsensor was stable for a 6 month period when was used daily.

Acknowledgements This work was supported by PNII Program Capacity, 2012-2014, Contract nr. 3ERC-like/2012, PNII Ideas project number PN-II-ID-PCE-2011-3-0953 and by the Sectorial Operational Programme Human Resources Development (SOP HRD), financed from the European Social Fund and the Romanian Government under the contract number POSDRU/159/1.5/S/137390/.

References

1. Bayley, H.; Cremer, P.S., *Nature*, 2001, 413, 226-230.
2. Stefan-van Staden, R.I.; Moldoveanu, I.; Sava, D.F.; Kapnissi-Christodoulou, C.; van Staden, J.F., *Chirality*, 2013, 25, 114-118.
3. Stefan-van Staden, R.I.; van Staden, J.F. *J Mod Med Chem.*, 2013, 1, 86-91.
4. Stefan-van Staden, R.I., Moldoveanu, I., *J Electrochem Soc*, 2014, 161, B45-B48.
5. Stefan-van Staden, R.I.; Moldoveanu, I.; van Staden J.F. *J Neurosci Meth*, 2014, 229, 1-7.
6. Oikawa, S.; Inuzuka, C.; Kuroki, M.; Matsuoka, Y.; Kosaki, G.; Nakazato H.; *Biochem. Biophys. Res. Comm.*, **1989**, 164, 39–45.
7. Gold, P.; Freedman, S. O.; *J. Exp. Med.*, **1965**, 121, 439-462.
8. Jiang, J.; Zhao, S.; Huang, Y.; Qin, G.; Ye, F.; *J. Chromatogr. A*, **2013**, 1282, 161–166.
9. Benchimol, S.; Fuks, A.; Jothy, S.; Beauchemin, N.; Shirota, K.; Stanners, C. P.; *Cell*, **1989**, 57, 327–334.
10. Goldenberg, D. M.; Sharkey, R. M.; Primus, F. J.; *J Natl Cancer Instit.*, **1976**, 57, 11–22.
11. Shi, Y. T.; Yuan, R.; Chai, Y. Q.; He, X. L.; *Electrochim Acta*, **2007**, 52, 3518–3524.
12. Kong, F. Y.; Zhu, X.; Xu, M. T.; Xu, J. J.; Chen, H. Y.; *Electrochim. Acta*, **2011**, 56, 9386–9390.

13. Hernández, L.; Espasa, A.; Fernández, C.; Candela, A.; Martín, C.; Romero, S.; *Lung Cancer*, **2002**, *36*, 83–89.
14. Duffy, M. J. ; van Dalen A.; Haglund, C.; Hansson, L.; Klapdor, R.; Lamerz, R.; Nilsson, O.; Sturgeon, C.; Topolcan, O.; *European J. Cancer*, **2003**, *39*, 718–727.
15. Engelen, M. J. A.; de Bruijn, H. W. A.; Hollema, H.; ten Hoor, K. A; Willemse, P. H. B.; Aalders, J. G.; van der Zee, A. G. J.; *Gynecol. Oncol.*, **2000**, *78*, 16–20.
16. Dungchai, W.; Siangproh, W.; Lin, J. M.; Chailapakul, O.; Lin, S.; Ying, X.; *Anal. Bioanal. Chem.*, **2007**, *387*, 1965–1971.
17. Herlyn, M.; Blaszczyk, M.; Sears, H. F.; Verrill, H.; Lindgren, J; Colcher, D.; Steplewski, Z.; Schlom, J.; Koprowski, H.; *Hybridoma*, **1983**, *2*, 329–339.
18. Kumada, Y.; Ohigashi, Y.; Emori, Y.; Imamura, K.; Omura, Y.; Kishimoto, M.; *J. Immunol. Meth.*, **2012**, *385*, 15–22.
19. Cao, X.; Wang, N.; Jia, S.; Guo, L.; Li, K.; *Biosens. Bioelectron.*, **2013**, *39*, 226–230.
20. Shi, T. Yuan, R. Chai, Y. Q. He, X. L. *Electrochim. Acta*, **2007**, *52*, 3518–3524.
21. Kong, Y F. Y.; Zhu, X.; Xu, M. T.; Xu, J. J.; Chen, H. Y.; *Electrochim. Acta*, **2011**, *56*, 9386–9390.
22. Sun, X.; Ma, Z.; *Anal. Chim. Acta*, **2013**, *780*, 95– 100.
23. Maltez-da Costa, M.; de la Escosura-Muñiz, A.; Nogués, C.; Barrios, L.; Ibáñez, E.; Merkoçi, A.; *Nano Lett.*, **2012**, *12*, 4164-4171.

24. Maltez-da Costa, M.; de la Escosura-Muñiz, A.; Nogués, C.; Barrios, L.; Ibáñez E.; Merkoçi, A.; Small, **2012**, *8*, 3605–3612.
25. Ivanov, I.; Stojcic, J.; Stanimirovic, A.; Sargent, E.; Nam, R.K.; Kelley, S.O.; Anal. Chem., **2013**, *85*, 398–403
26. Liu, J.; Qin, Y.; Li, D.; Wang, T.; Liu, Y.; Wang, J.; Wang, E.; Biosens. Bioelectron., **2013**, *41*, 436–441.
27. Moscovici, M.; Bhimji, A.; Kelley, S.O.; Lab Chip, **2013**, *13*, 940-946.

Table 1. Analysis of CEA from whole blood samples using the stochastic microsensor based on nanoporous gold microsphere and ELISA.

Sample no	CEA, ng/mL		t-test
	Sensor based on gold particles	ELISA	
1	2.06±0.12	1.98±0.32	1.89
2	2.10±0.10	2.00±0.40	1.90
3	1.40±0.13	1.20±0.38	1.95
4	1.09±0.09	0.89±0.29	2.10
5	1.64±0.12	1.32±0.30	2.25
6	1.32±0.15	1.15±0.29	1.76
7	1.37±0.11	1.28±0.42	1.70
8	0.93±0.09	0.74±0.28	2.90

All values are the average of ten determinations.

Caption to Figures

Figure 1 SEM image of (a) 24K gold microparticle; (b) engineered pore in the 24K gold microparticle.

Figure 2 Schematic diagram of the stochastic sensor.

Figure 3 Specific diagram obtained for the pattern recognition of CEA in whole blood sample using the stochastic microsensors.

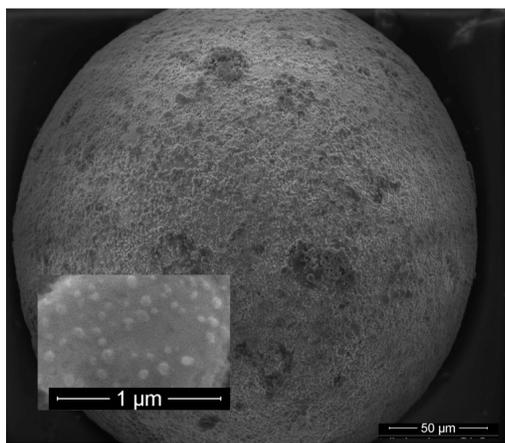


Figure 1 a

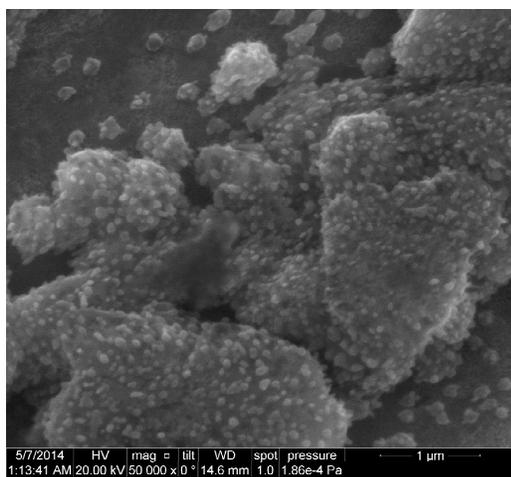


Figure 1 b

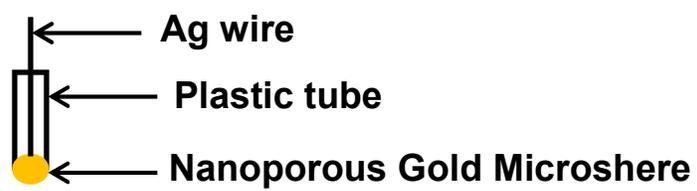
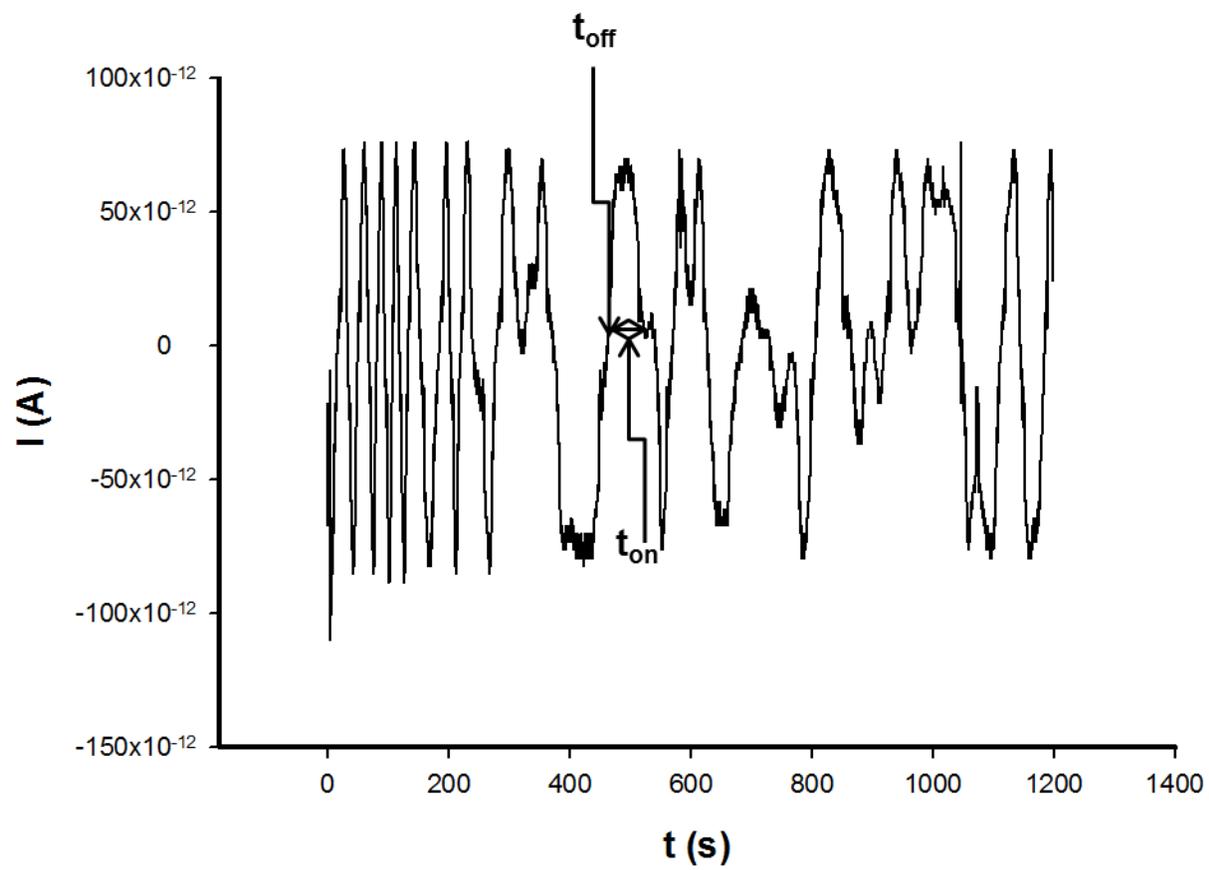


Figure 2

**Figure 3**