

# Analytical Methods

Accepted Manuscript



This is an *Accepted Manuscript*, which has been through the Royal Society of Chemistry peer review process and has been accepted for publication.

*Accepted Manuscripts* are published online shortly after acceptance, before technical editing, formatting and proof reading. Using this free service, authors can make their results available to the community, in citable form, before we publish the edited article. We will replace this *Accepted Manuscript* with the edited and formatted *Advance Article* as soon as it is available.

You can find more information about *Accepted Manuscripts* in the [Information for Authors](#).

Please note that technical editing may introduce minor changes to the text and/or graphics, which may alter content. The journal's standard [Terms & Conditions](#) and the [Ethical guidelines](#) still apply. In no event shall the Royal Society of Chemistry be held responsible for any errors or omissions in this *Accepted Manuscript* or any consequences arising from the use of any information it contains.


1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

## Sensitive and stable pre-calibrated solid-phase extraction columns for environmental and forensic quantification using isotope dilution mass spectrometry

Rebecca L. Wagner,<sup>1,2</sup> Andrew J. Boggess,<sup>1</sup> Stephanie J. Wetzel,<sup>1</sup> H.M. Skip Kingston<sup>1</sup>

<sup>1</sup>Department of Chemistry and Biochemistry, Duquesne University, Pittsburgh, PA, USA

<sup>2</sup>Present affiliation: Virginia Department of Forensic Science, Richmond, VA, USA

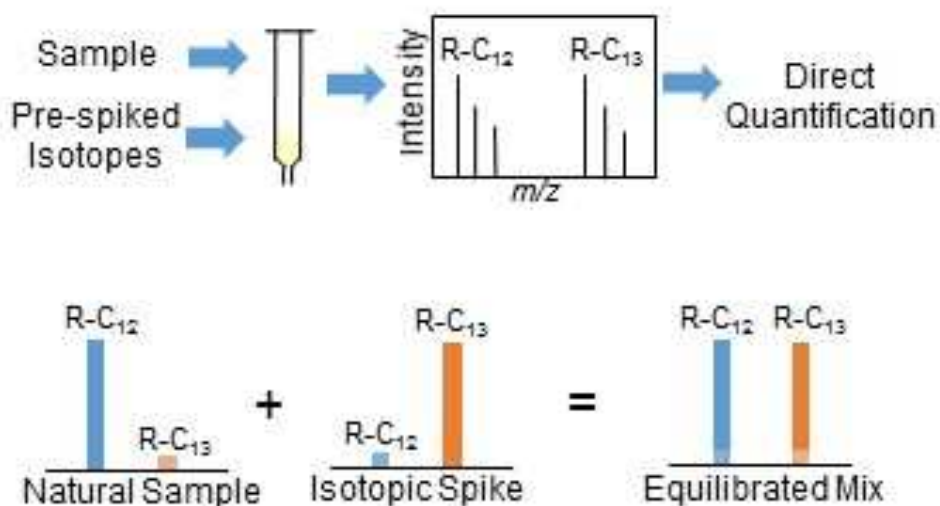

**Abstract**

A method was developed to pre-load solid-phase extraction columns (SPE) with isotopic calibrant for use with isotope dilution mass spectrometry (IDMS). The pre-calibration method was developed, optimized, and validated for the quantification of the pesticide glyphosate in drinking water using anion-exchange SPE, electrospray-ionization, and time-of-flight mass spectrometry (ESI-TOF-MS). The instrumental method obtained a mass-accuracy of 3 ppm and a limit of quantification (LOQ) of 0.3 ng/mL. Quantification of glyphosate by IDMS significantly improved quantitative error and LOQ compared with calibration curve. The pre-loading methodology was optimized for stability over time and validated in drinking water, exhibiting an accuracy of  $1.25\% \pm 0.87\%$  error with no significant difference from certified concentrations or traditional SPE. Method LOQ was 0.4 ng/mL. Quantifying glyphosate in spiked drinking water sample produced high accuracy up to two-weeks after pre-loading columns, with an accuracy of  $6.41\% \pm 7.10\%$  error. A potential forensic application was investigated by adapting the pre-loading method to the quantification of seven drugs in synthetic urine using a mixed-mode SPE column. The ESI-TOF-MS method using traditional SPE produced accurate quantification of all seven drugs in synthetic urine with a mean error of  $4.16\% \pm 3.07\%$  and LOQ of 0.780 ng/mL. The pre-loading method produced accurate quantification with  $5.36\% \pm 4.73\%$  error, with no significant difference from traditional SPE or certified standards. Five of seven drugs were quantified at high accuracy one week after pre-loading, with  $5.40\% \pm 4.57\%$  error from certified values. This method may be applicable to analysts seeking to develop methods to improve the transfer of high-accuracy and precision methods between laboratories.

## Introduction

Implementation of high-quality mass spectrometry-based analytical methods has improved overall analytical accuracy, precision, and sensitivity attained in routine analyses.<sup>1</sup> Clinical and commercial laboratories have sought validated techniques to improve sensitivity, reproducibility, and accuracy through improved sample preparation, instrumental methodology, and quantitative procedures.<sup>2, 3</sup> To achieve higher analytical quality, many laboratories have adjusted analytical emphasis from common techniques, like assays, to higher-accuracy methods, like mass spectrometric identification and quantification.<sup>4</sup> However, without significant training, many novel methods requiring complex sample preparation steps may not be replicated with the same quality by analysts or technicians in independent laboratories.<sup>5</sup> The methodological shift toward higher sensitivity and higher accuracy analytical methods<sup>6, 7</sup> has elevated the necessity for simplified sample preparation techniques reduce the influence of sample preparation steps on final analytical quality.

Often, quantitative accuracy is negatively impacted by errors introduced by the large number of highly precise sample preparation steps required in many methods and by inherent instrumental uncertainty.<sup>8, 9</sup> One technique used for reducing the influence of sample preparation and instrumental uncertainty on final quantitative quality is called isotope dilution mass spectrometry (IDMS).<sup>10</sup> IDMS is a quantification technique involving the spiking of accurate amounts of isotopically labeled analogs into an unknown sample. Using known isotopic abundances, concentration and mass of isotopically labeled spike, and mass of the unknown sample, the concentration of each analyte can be calculated mathematically without the use of calibration curves. IDMS can correct for many sources of error often associated with extraction, mass spectrometry, and quantification. These common sources include imprecise sample

1  
2  
3 preparation, poor extraction reproducibility, sample loss, low analyte recovery, instrumental  
4 drift, matrix effects, and physical or chemical interferences. Much of the error introduced in  
5 sample preparation to change the concentration of natural analyte in a sample will affect the  
6 isotopic analog identically and be corrected in the final IDMS equation.<sup>10, 11</sup> By reducing the  
7 influence of common error-introducing analytical steps on final quantitative quality, IDMS is  
8 capable of transferring high accuracy methods between laboratories and analysts with minimal  
9 additional training.<sup>12</sup> However, in-laboratory spiking of the isotopically labeled analogs into the  
10 unknown samples remains a potential source of analytical error when transferring developed  
11 methods using IDMS.  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23

24  
25 Commonly, laboratories analyzing environmental and forensic samples utilize gas  
26 chromatography / mass spectrometry (GC/MS), liquid chromatography / mass spectrometry  
27 (LC/MS), or the enzyme-linked immunosorbent assay (ELISA).<sup>13-15</sup> However, with increased  
28 availability, many laboratories have begun adopting sensitive and high-resolution  
29 instrumentation like time-of-flight mass spectrometers (TOF-MS) to eliminate the requirements  
30 of derivatization and chromatography.<sup>16, 17</sup> With the advent of highly sensitive analytical  
31 methods, sample cleanup has become an important part of sample preparation to reduce harmful  
32 biological material and to pre-concentrate the analytes of interest.  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42

43  
44 Solid-phase extraction (SPE) is a sample cleanup and pre-concentration procedure to  
45 isolate analytes of interest from potentially interfering or harmful biological compounds using  
46 primarily hydrophobic interactions and cationic or anionic exchange.<sup>18</sup> SPE is often used on  
47 aqueous and biological samples to selectively extract and pre-concentrate analytes prior to  
48 analysis by LC/MS or electrospray ionization (ESI) TOF-MS. It was hypothesized in the  
49 research presented here that modified SPE columns could be pre-calibrated by, prior to analysis  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

1  
2  
3 of an unknown sample, the loading of accurately known concentration of isotopically labeled  
4  
5 analogs by highly skilled analysts. Pre-calibrated columns may be useful in transferring  
6  
7 analytical quality between and among laboratories by removing the spiking of isotopically  
8  
9 labeled analogs from the in-laboratory sample preparation, potentially further reducing the  
10  
11 influence of sample preparation on final quantitative quality.  
12  
13

14  
15 This research focused on developing a SPE pre-loading method for future  
16  
17 implementation in improving the transfer of high accuracy and precision analytical methods  
18  
19 between and among laboratories. For optimization experiments, the environmentally relevant  
20  
21 pesticide glyphosate was chosen for its high usage rates, analytical difficulty, and inclusion in  
22  
23 national drinking water regulations. Glyphosate is a polar organophosphate pesticide extensively  
24  
25 used in the U.S. for vegetation control. The hydrophilicity and ionic character of this molecule  
26  
27 make quantification in aqueous solution difficult. The U.S. Environmental Protection Agency  
28  
29 (USEPA) has regulated a maximum contaminant limit of glyphosate in drinking water of 0.7  
30  
31  $\mu\text{g}/\text{mL}$ .<sup>19</sup> Following development, optimization, and validation for the pesticide glyphosate, the  
32  
33 potential forensic applications were explored by analysis of seven drugs of abuse in synthetic  
34  
35 urine. For both glyphosate and the drugs of abuse, experiments were performed to assess  
36  
37 quantitative stability over time to simulate future experiments in which pre-loaded SPE columns  
38  
39 will be shipped to off-site laboratories for analysis.  
40  
41  
42  
43  
44  
45  
46  
47

## 48 **Results**

49  
50 A method for the quantification of glyphosate using ESI-TOF-MS, traditional SPE, and  
51  
52 IDMS quantification were validated by adapting and optimizing existing methods.<sup>10, 20</sup>  
53  
54 Validation results using IDMS quantification were compared with calibration data. Various  
55  
56  
57  
58  
59  
60

1  
2  
3 techniques were assessed for increasing the quantitative stability over time of columns pre-  
4 loaded with glyphosate-2-<sup>13</sup>C. The optimal pre-loading technique was then validated in drinking  
5 water samples spiked with unlabeled glyphosate analyzed with the pre-loaded SPE columns.  
6  
7 Robustness of the pre-loading method was then assessed for potential forensic application by  
8  
9 adapting and optimizing the instrumental method for seven drugs of abuse in synthetic urine.  
10  
11 Quantitative stability over time for the SPE pre-loading method was assessed for both  
12  
13 environmental and forensic applications.  
14  
15  
16  
17  
18  
19  
20  
21

### 22 *Optimization of SPE and ESI-TOF-MS*

23  
24 Strata-SAX (Phenomenex) columns were used in the experimental optimization of SPE  
25 elution volume and pH. It was found that the optimum efficiency of glyphosate elution occurred  
26 at pH 6.0. Therefore, an eluting solvent consisting of 1:1 acetonitrile/methanol acidified to 6%  
27 formic acid was used. Analysis of eluent fractions determined 16 mL was required to elute the 4  
28 mL of 6 µg/mL solution loaded onto the SPE column.  
29  
30  
31  
32  
33  
34  
35

36 Instrumental parameters were optimized for signal intensity using negative ionization  
37 ESI-TOF-MS. Experimentally optimized instrumental parameters for drinking water samples  
38 spiked with glyphosate can be found in table 1.  
39  
40  
41  
42

43 Accurate quantification was attained using isotopic distribution patterns, expected  $m/z$   
44 shift between glyphosate and glyphosate-2-<sup>13</sup>C, and mass accurate resolution of glyphosate and  
45 glyphosate-2-<sup>13</sup>C.<sup>21</sup> For unlabeled glyphosate, a mean mass accuracy of 3.2 ppm was obtained  
46 with mean deviation of 4.3 ppm. For glyphosate-2-<sup>13</sup>C, a mean mass accuracy was obtained of  
47 1.7 ppm with a mean deviation of 4.1 ppm. At 168  $m/z$ , a resolving power of 18,000  $m/\Delta m$  was  
48 obtained. Mass bias was calculated to determine the differential instrument response between the  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

1  
2  
3 natural and isotopically labeled forms of glyphosate. A mass bias factor of 1.0006 was  
4  
5 determined for the IDMS quantification procedure for glyphosate.<sup>22</sup> Optimized instrumental  
6  
7 parameters produced the resolved spectra seen in figure 1. While high-resolution mass  
8  
9 spectrometry (HR-MS) was used for mass accurate compound identification in this research on  
10  
11 simple samples containing known compounds, it has been reported elsewhere that mass  
12  
13 accuracy, even below 1 ppm experimental mass error, is not sufficient to accurately identify  
14  
15 unknown analytes in samples.<sup>23</sup> This research optimized an instrumental method for the  
16  
17 quantification of glyphosate in known samples only as a means of assessing the developed pre-  
18  
19 loading technique and the mass accuracy of 3 ppm was therefore deemed adequate. This  
20  
21 optimized instrumental method would not be suitable for absolute identification of samples  
22  
23 containing unknown compounds.  
24  
25  
26  
27  
28  
29  
30  
31

### 32 *Validation of SPE and ESI-TOF-MS*

33  
34 Instrument limit of quantification (LOQ) of ESI-TOF-MS for glyphosate in drinking  
35  
36 water was found to be 0.312 µg/mL. Method LOQ for ESI-TOF-MS using traditional SPE and  
37  
38 IDMS quantification for glyphosate in drinking water was found to be 0.401±0.01 µg/mL. Using  
39  
40 IDMS, quantitative accuracy and precision was maintained as concentration values were  
41  
42 decreased approaching method LOQ, confirming previous studies on molecular IDMS  
43  
44 quantification.<sup>12</sup> This LOQ sufficiently exceeded the National Primary Drinking Water  
45  
46 Regulations from the USEPA, which specified a maximum glyphosate contaminant level of  
47  
48 0.700 µg/mL.  
49  
50  
51  
52

53 Drinking water spiked with glyphosate standard at a certified concentration of 6.00  
54  
55 µg/mL was analyzed using the optimized ESI-TOF-MS parameters and the traditional SPE,  
56  
57  
58  
59  
60



1  
2  
3 quantified using IDMS (n=20). The optimized method produced an experimental concentration  
4  
5 of  $5.95 \pm 0.08$   $\mu\text{g/mL}$ , representing an overall accuracy with 0.83% error and a precision of 1.3%  
6  
7 RSD. These results indicate that a valid, optimized instrumental method was adapted from  
8  
9 previously published sources to provide precise and mass-accurate quantification to be applied to  
10  
11 the assessment of SPE pre-loading techniques.  
12  
13  
14

### 17 *Comparison of Quantitative Methodologies*

20 Samples spiked with both labeled and unlabeled analytes at concentrations approaching  
21  
22 the LOQ were used to create a calibration curve. Figure 2 shows calibration data approaching the  
23  
24 determined LOQ as well as the same data treated with IDMS quantification from the same  
25  
26 samples, showing percent error from certified concentration, with 95% confidence intervals, at  
27  
28 various concentrations points (n=5 at each point). Quantitative methodologies were compared  
29  
30 using the validated ESI-TOF-MS method with traditional SPE. Drinking water samples spiked  
31  
32 with certified concentrations of glyphosate were quantified using IDMS with a mean accuracy of  
33  
34  $4.22\% \pm 5.81\%$  error over the concentration range 0.600 – 6.25  $\mu\text{g/mL}$ , losing quantitative  
35  
36 accuracy below 0.401  $\mu\text{g/mL}$ . For quantification, glyphosate-2- $^{13}\text{C}$  was spiked into all samples at  
37  
38 5.00  $\mu\text{g/mL}$ . Calibration curve quantification lost quantitative accuracy at the 95% confidence  
39  
40 level at 3.25  $\mu\text{g/mL}$ , exhibited  $59.4\% \pm 43.0\%$  error the studied concentration range, but remained  
41  
42 detectable to a concentration of 0.401  $\mu\text{g/mL}$ . IDMS and calibration curve quantification  
43  
44 demonstrated identical limits of detection, but IDMS produced a significantly lower LOQ.  
45  
46  
47  
48  
49  
50

### 53 *Optimization of Pre-loading Method*

56 Samples containing glyphosate-2- $^{13}\text{C}$  in drinking water were loaded onto the SPE  
57  
58  
59  
60

1  
2  
3 columns using the manufacturer recommended procedure. These pre-loaded columns lost  
4 adequate accuracy when used for quantification of spiked drinking water samples after 1 day of  
5 storage. Several optimization procedures were then undertaken to increase on-column stability.  
6  
7  
8  
9  
10 The techniques that meaningfully impacted percent error are summarized in figure 3, showing  
11 absolute value of percent error using each specified method with 95% confidence intervals.  
12  
13  
14

15 Three techniques of storing SPE columns loaded with glyphosate-2-<sup>13</sup>C: air-drying  
16 columns (AD), storing with 2 mL water-rinse (WR), and storing with 2 mL methanol-rinse (MR)  
17 were assessed for quantitative stability over time. Two modifications of applying the pre-loading  
18 spikes were assessed: decreasing volume from 4 mL to 200 µL of spiking solution (DV), and  
19 spiking the solution onto an individual frit (IF) above the column packing. Combinations of  
20 storage conditions and pre-loading techniques were assessed in the optimization experiments.  
21  
22 The optimization experiments were performed using 5 µg/mL of pre-loaded glyphosate-2-<sup>13</sup>C  
23 and 5 µg/mL of glyphosate (n=5 for each technique).  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33

34 At one week of storage, AD and WR showed no statistical difference in percent error, but  
35 MR exhibited statistically decreased percent error from both AD and WR (p<0.05). However,  
36 both WR and MR produced disruption of the SPE column packing material, which lead to  
37 irreversible binding of glyphosate-2-<sup>13</sup>C. Irreversible binding of the pre-loaded isotope was  
38 suspected in WR and MR by the production of large positive bias after storage for two weeks.  
39 Irreversible binding was confirmed by the observation of large negative bias by pre-loading  
40 unlabeled analytes and quantifying a solution of isotopically labeled analytes after two weeks of  
41 storage. Therefore, WR and MR were eliminated from the optimization experiments. The  
42 modified pre-loading procedure of DV+AD significantly reduced percent error compared with  
43 AD, WR, and MR (all p<0.05). The modified pre-loading procedure of IF+DV+AD produced  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

1  
2  
3 significantly decreased percent error compared with AD and WR (all  $p < 0.05$ ).  
4

5 After two weeks of storage, all optimization techniques increased in percent error  
6 compared with the same technique after one week. DV+AD exhibited significantly lower percent  
7 error compared with AD after two weeks of storage ( $p < 0.05$ ), but did not demonstrate adequate  
8 quantitative accuracy ( $26.6\% \pm 1.12\%$  error). IF+DV+AD exhibited further significant decrease in  
9 percent error compared with DV+AD ( $p < 0.05$ ) and maintained adequate quantitative accuracy  
10 ( $6.41\% \pm 7.14\%$  error).  
11  
12  
13  
14  
15  
16  
17  
18  
19

20 When extended to four weeks of storage, no technique or combination of techniques  
21 yielded adequate quantitative accuracy, with IF+DV+AD exhibiting  $47.2\% \pm 1.35\%$  error. Results  
22 for IF+DV+AD over four weeks can be found in figure 4. Significant loss of stability was  
23 observed between two and four weeks for pre-loaded columns. It was determined that the  
24 combination IF+DV+AD would be used in the pre-loading method to maintain high-quality  
25 quantification up to two weeks after pre-loading. Future research will work to improve the  
26 stability of on-column analyte stability during storage.  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36

### 37 *Validation of Pre-loading Technique*

38  
39 Using the validated instrumental parameters from the optimized ESI-TOF-MS method  
40 and the IF+DV+AD technique optimized for SPE pre-loading, a validation experiment was  
41 performed on drinking water spiked with  $6 \mu\text{g/mL}$  of glyphosate ( $n=20$ ). Columns were pre-  
42 loaded with isotopically labeled glyphosate at a concentration of  $6 \mu\text{g/mL}$  30 minutes prior to  
43 analysis of the spiked drinking water to allow the columns time to air-dry. Drinking water  
44 samples analyzed 30-minutes after pre-loading columns with isotopes produced a final  
45 concentration of  $5.93 \pm 0.052 \mu\text{g/mL}$ , representing a 1.25% error and a 0.87% RSD. A method  
46 LOQ of  $0.401 \mu\text{g/mL}$  was obtained for the pre-loaded columns, identical to the LOQ obtained for  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

1  
2  
3 ESI-TOF-MS using traditional SPE. These results indicate that the IF+DV+AD pre-loading  
4  
5 technique produced valid quantitative results that did not differ significantly from either the  
6  
7 certified value or quantitative results from the ESI-TOF-MS method using traditional SPE at the  
8  
9 95% confidence level.  
10  
11

#### 12 13 14 15 *Potential Application to Drugs of Abuse in Synthetic Urine* 16

17  
18 The optimized and validated ESI-TOF-MS analytical method was optimized for the  
19  
20 quantification in synthetic urine of seven common opioids and alkaloids used as adulterants.  
21  
22 Experimentally optimized instrumental parameters can be found in table 2. Analysis of these  
23  
24 opioid and alkaloid compounds required changing the SPE column from the anion-exchange  
25  
26 column used for glyphosate to a Clean Screen DAU (UCT) mixed-mode hydrophobic and  
27  
28 cation-exchange column.  
29  
30

31  
32 The optimized instrumental parameters produced valid quantification for all seven drugs  
33  
34 spiked in synthetic urine at 40 ng/mL following traditional SPE extraction. Validation results for  
35  
36 ESI-TOF-MS using traditional SPE and IDMS can be found in table 3 comparing certified  
37  
38 concentrations with experimentally determined concentrations with 95% confidence intervals.  
39  
40 All drugs of abuse were quantified with <10% quantitative error and <20% RSD. Accuracy  
41  
42 ranged from 0.689% to 9.33% error for methadone and cocaine, respectively. Precision ranged  
43  
44 from 0.973% to 11.6% RSD for fentanyl and morphine, respectively. Mean quantitative accuracy  
45  
46 for samples analyzed using ESI-TOF-MS with traditional SPE exhibited mean accuracy of  
47  
48 4.16%±3.07% error and mean precisions of 5.93%±3.03% RSD. Experimentally determined  
49  
50 concentrations did not differ significantly from certified concentrations at the 95% confidence  
51  
52 level.  
53  
54  
55  
56  
57  
58  
59  
60

1  
2  
3 The method LOQ determined for the drugs of abuse using the optimized ESI-TOF-MS  
4 with traditional SPE and IDMS of 0.780 ng/mL for all analytes. As with the work with  
5 glyphosate, quantification with IDMS produced significantly higher accuracy and precision  
6 approaching the LOQ. In figure 5, IDMS and typical calibration curve quantitation are compared  
7 in the same samples using the validated ESI-TOF-MS method and traditional SPE, showing  
8 mean percent difference from certified concentrations of all analytes included in this study at  
9 various concentration points, with 95% confidence ranges (n=5). IDMS exhibited a mean percent  
10 error across all concentration points for all analytes of 5.66%±10.9%. Calibration curve lost  
11 quantitative accuracy below 3.13 ng/mL, exhibiting a mean percent error for the concentrations  
12 range 25.0 ng/mL through 3.13 ng/mL of 11.5%±27.8%.

13  
14  
15 The IF+DV+AD pre-loading technique was validated for the drugs of abuse using the  
16 mixed-mode SPE column, analyzed by the optimized and validated ESI-TOF-MS instrumental  
17 method. Analysis of synthetic urine spiked with 40 ng/mL of all seven drugs of abuse using pre-  
18 loaded SPE columns 30-minutes after pre-loading produced highly accurate quantitative results.  
19 All opioids and alkaloids with the exception of cocaine were quantified with ≤10% quantitative  
20 error and <20% RSD. Accuracy ranged from 0.766% to 13.0% error for codeine and cocaine,  
21 respectively. A mean accuracy of 5.36%±4.73% error and mean precision of 6.58%±2.92% RSD  
22 were produced by the pre-loading method. The mean experimental values obtained did not differ  
23 from the mean certified values or from the concentrations obtained using the validated ESI-TOF-  
24 MS and traditional SPE method at the 95% confidence level. Validation results for the  
25 quantification of all seven opioids and alkaloids spiked in synthetic urine and extracted using  
26 pre-loaded SPE columns 30 minutes after pre-loading can be found in table 4.

1  
2  
3 Using the ESI-TOF-MS instrumental method and the IF+DV+AD pre-loading method,  
4 stability over time was assessed for the analysis of synthetic urine samples spiked with the drugs  
5 of interest. Morphine, codeine, methadone, 6-acetylmorphine, and fentanyl were quantified with  
6 adequate accuracy when analyzed one week after column pre-loading. Methadone, fentanyl, and  
7 codeine maintained adequate quantitative accuracy when quantified two weeks after column  
8 loading. At the two-week time interval, codeine maintained accuracy at the 95% confidence  
9 interval, but produced poor precision ( $\pm 12\%$ ). Cocaine and heroin were not quantified accurately  
10 after one week (15%, 17% error, respectively) or after two weeks (15%, 25% error, respectively)  
11 of storage. The stability over time results are summarized in figure 6.  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23

24 The work presented here demonstrates the viability of isotopically pre-loaded SPE  
25 columns for the quantification of environmentally and forensically relevant analytes by IDMS.  
26 This viability was demonstrated with different SPE column packing types and a wide range of  
27 investigated analytes. While the pre-loading technique produced stable quantitative accuracy  
28 over time for 70% of the chosen drugs of abuse, the concept of pre-loading and storing SPE  
29 columns for future analysis has been proven viable by this research. Future work will increase  
30 the breadth and robustness of this developed method. In subsequent research, the transfer of  
31 analytical quality using this pre-loading method will be tested in by shipment of pre-loaded SPE  
32 columns to independent laboratories for quantification of determined analytes. Providing  
33 analysts with pre-calibrated, pre-loaded SPE columns to be used for IDMS quantification may  
34 help to improve overall analytical quality.  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49

50 A limitation of this research is the potential for introduction of matrix-effect errors into  
51 quantitative analysis. Traditional IDMS eliminates errors introduced by matrix-effects by  
52 equilibrating isotopic and natural molecules in a native solution prior to all other sample  
53  
54  
55  
56  
57  
58  
59  
60

1  
2  
3 preparation. Any matrix effects altering the concentration of a free molecule of interest will  
4  
5 equally affect the isotopic analog, without altering the isotope-to-natural ratio within the sample.  
6  
7 Using the process described in this work, equilibration between the isotopic and naturally  
8  
9 occurring molecules of interest will not occur until after elution from the SPE column.  
10  
11 Equilibration at this post-elution step allows IDMS to correct for analytical errors typically  
12  
13 introduced in instrumentation, but will not correct for matrix effects that have already altered the  
14  
15 concentration of naturally occurring molecule in the sample. This research used only drinking  
16  
17 water samples and synthetic urine samples, both relatively simple matrices. As high accuracy  
18  
19 and precision were obtained in method validation, the post-elution equilibration was determined  
20  
21 to have little effect on analytical quality. However, as the isotopes were pre-loaded in a relatively  
22  
23 simple sample matrix (drinking water), future research will focus on the analysis of unknown  
24  
25 water and urine samples containing complex matrixes to investigate potential effects on  
26  
27 quantitative accuracy.  
28  
29  
30  
31  
32  
33  
34  
35

## 36 **Experimental**

### 37 *Chemicals and Standards*

38  
39  
40  
41 Glyphosate (99% pure) and glyphosate-2-<sup>13</sup>C (99% pure, 99% enriched) were acquired  
42  
43 from Sigma-Aldrich (St. Louis, MO, USA). Drinking water samples were supplied by Pittsburgh  
44  
45 Municipal Water (Pittsburgh, PA, USA). Heroin, 6-AM, morphine, cocaine, methadone, and  
46  
47 fentanyl analytical standards at certified concentrations of 1.0 mg/mL and codeine analytical  
48  
49 standard at a certified concentration of 100 µg/mL were purchased from Cerilliant (Round Rock,  
50  
51 TX, USA). The deuterium-enriched analogs: heroin-D<sub>9</sub>, morphine-D<sub>3</sub>, cocaine-D<sub>3</sub>, codeine-D<sub>3</sub>,  
52  
53 methadone-D<sub>3</sub>, and fentanyl-D<sub>5</sub> at certified concentrations of 100 µg/mL and 6-AM-D<sub>3</sub> at a  
54  
55  
56  
57  
58  
59  
60

certified concentration of 1.0 mg/mL were purchased from Cerilliant. Synthetic urine, HPLC grade methanol, HPLC grade water, Hyclone phosphate buffered saline (PBS), HPLC grade 2-propanol, and ammonium hydroxide were purchased from Fisher Scientific (Pittsburgh, PA, USA). Acetate buffer was prepared using sodium acetate and acetic acid purchased from Fisher Scientific. Each naturally occurring analyte was prepared in separate stock solutions at 10 µg/mL for the drugs of abuse and 60 µg/mL for glyphosate in HPLC grade water. For glyphosate, two solutions were prepared by mass in drinking water: one spiked with 6 µg/mL of glyphosate and one spiked with 6 µg/mL of glyphosate-2-<sup>13</sup>C. Two solutions were prepared by mass in synthetic urine for the drugs: one containing all unlabeled drugs at 40 ng/mL and one containing all isotopically labeled analogs at 40 ng/mL.

#### *Solid-Phase Extraction*

For glyphosate experiments, Strata-SAX SPE columns (500 mg bed mass, 6 mL volume) were purchased from Phenomenex (Torrance, CA, USA) for the analysis of glyphosate in drinking water. Columns were conditioned per manufacture recommendations with 4.0 mL HPLC grade methanol and 4.0 mL HPLC grade water. Then, 4.0 mL of drinking water sample was loaded onto the column and washed with 4.0 mL of HPLC grade methanol. Elution was performed with 16 mL of a 1:1 solution of acetonitrile and methanol acidified at 6% with formic acid. All SPE analyses were performed with a negative pressure vacuum chamber at 1 mL/min. For IDMS quantification, a solution of glyphosate-2-<sup>13</sup>C in HPLC grade water was loaded onto the column after conditioning but before the spiked drinking water sample was loaded.

For the drugs of abuse, CSDAU303 (UCT, Bristol, PA) SPE were used for extraction of drugs from synthetic urine. Columns were conditioned with 2.0 mL of HPLC methanol, 2.0 mL HPLC water, and 2.0 mL PBS. Extraction was performed on 4.0 mL synthetic urine spiked with



1  
2  
3 unlabeled analytes, followed by a wash of 4.0 mL water, 3.0 mL acetate buffer, and 3.0 mL of  
4  
5 methanol. For IDMS experiments, a 4.0 mL aliquot of the isotopically enriched working solution  
6  
7 (phosphate-buffered to pH 6) in synthetic urine was loaded onto the column next. After a two  
8  
9 minute on-column drying period, all extracted compounds were eluted from the column using  
10  
11 11.0 mL ethyl acetate:2-propanol:ammonium hydroxide (84:12:1) solution.  
12  
13  
14  
15  
16

### 17 *ESI-TOF-MS*

18  
19  
20 A Bruker Daltonics microTOF (Billerica, MA, USA) mass spectrometer with an  
21  
22 orthogonal ESI source was experimentally optimized for the analysis of all analytes of interest  
23  
24 and their deuterium-enriched analogues. Samples were infused using the ESI source at a flow  
25  
26 rate of 240  $\mu\text{L}/\text{hour}$  with a Cole Palmer 74900-00 syringe pump (Vernon Hills, IL). The  
27  
28 experimentally optimized method parameters can be found in the Results section. Quantitative  
29  
30  $m/z$  ions were experimentally found for each labeled and unlabeled analyte. Quantitative ions for  
31  
32 each natural and isotopic compound can be found in table 5.  
33  
34  
35  
36  
37  
38

### 39 *SPE Pre-loading*

40  
41 SPE column pre-loading followed the same conditioning and washing procedures for the  
42  
43 separate columns listed in the Solid-Phase Extraction section. For pre-loading, matrix-matched  
44  
45 solutions containing isotopic analogs were extracted and allowed to air-dry for a determined  
46  
47 period prior to extraction of solutions spiked with certified concentrations of unlabeled analytes.  
48  
49

50  
51 Optimization of pre-loading procedure assessed three methods of storing columns:  
52  
53 allowing columns to air-dry (AD) in an upright position, rinsing the columns with 2 mL of  
54  
55 HPLC grade water (WR) and storing wet with Parafilm sealing both ends of the column, and  
56  
57  
58  
59  
60

1  
2  
3 rinsing the columns with 2 mL of HPLC grade methanol (MR) and sealing with Parafilm. Two  
4  
5 sample extraction modifications were assessed: decreasing the volume (DV) of the isotopically  
6  
7 labeled solution from 4 mL to 200  $\mu$ L, and placing an individual frit (IF) approximately 2 cm  
8  
9 above the column packing. Assessment of these techniques followed a reasonable order. The  
10  
11 storage methods were testing first and comparisons were generated between all three. The  
12  
13 optimal method that provided the greatest long-term quantitative stability was used for all future  
14  
15 analyses. Pre-loaded columns were cold-stored at 15  $^{\circ}$ C for one week, two weeks, and four  
16  
17 weeks prior to analysis of a solution of drinking water spiked with certified concentrations of  
18  
19 glyphosate. Five replicates were performed for each technique at each time interval. Prior to ESI-  
20  
21 TOF analysis, all eluted mixtures of naturally occurring and isotopically labeled molecules were  
22  
23 vortexed for 5 minutes to allow time for equilibration.  
24  
25  
26  
27  
28  
29  
30  
31

### 32 *Method Validations*

33  
34 For validation experiments, solutions were prepared by spiking certified standards for  
35  
36 each analyte being studied into either drinking water or synthetic urine matrix by mass. The  
37  
38 appropriate sample preparation was applied (either SPE using the above method or SPE pre-  
39  
40 loading using the above method) and the eluate was analyzed using the above method for ESI-  
41  
42 TOF-MS. Quantification was performed by IDMS. Replicates were performed for all validation  
43  
44 experiments (n=20 for glyphosate by SPE and SPE pre-loading, n=5 for drugs by SPE and SPE  
45  
46 pre-loading). Experimentally obtained values were compared with calculated values at the 95%  
47  
48 confidence level. For assessment of accuracy, an adequate percent error to be achieved by the  
49  
50 method being validated was set at  $\pm 10\%$ .  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

### Quantification Methods

Quantification was accomplished using IDMS, as defined in EPA Method 6800.<sup>10</sup> The concentration of the unknown natural molecule was calculated as:

$$\text{Concentration } (\mu\text{mol/g}) = \frac{[(C_s W_s / W_x) \times {}^i P_s - (R_{i/n} \times {}^n P_s)]}{[(R_{i/n} \times {}^n P_x) - {}^i P_x]} \quad (\text{eq. 1})$$

$$R_{i/n} = \text{Signal intensity of enriched molecule} / \text{Signal intensity natural molecule}$$

In the IDMS quantitation procedure,  $C_s$  and  $C_x$  are the concentrations, in  $\mu\text{mol/g}$ , of the selected analyte in the isotope-enriched spike and the spiked sample, respectively.  ${}^i P_s$  and  ${}^i P_x$  are the percent purity of the isotopically enriched molecule in the spike and the pre-spiked sample, respectively. Likewise,  ${}^n P_s$  and  ${}^n P_x$  are the percent purity of the naturally occurring analyte in the spike and the pre-spiked sample, respectively.  $R_{i/n}$  is the ratio of peak areas of the quantitative ion for the natural and isotopically enriched form of the compound being analyzed obtained in the same analysis. Finally,  $W_s$  and  $W_x$  are the masses of the spike and sample, respectively. Peak areas corresponding to the pair of natural and isotopically enriched analytes were exported to an in-house spreadsheet for IDMS quantitation.

For comparison of quantification methodologies, solutions were prepared in the appropriate matrix, drinking water or synthetic urine, at various concentrations. For glyphosate, drinking water samples were prepared containing unlabeled glyphosate at the concentrations 6.25, 3.25, 1.50, 1.00, and 0.600  $\mu\text{g/mL}$ . At each concentration point, an equal concentration of isotopically labeled glyphosate was used for IDMS. For the drugs, synthetic urine samples were prepared containing unlabeled versions of each analyte six concentration points: 25.0, 12.5, 6.25, 3.13, 1.56, and 0.780  $\text{ng/mL}$ .

For all IDMS quantification during method development, method validation, and application, isotopically labeled analogs of all analytes of interest were spiked into samples by volume to a precisely known concentration. Glyphosate-2-<sup>13</sup>C was spiked into all samples at 5.00 μg/mL and all illicit drugs at 40.0 ng/mL.

### *Mass Bias Factor*

A mass bias factor was determined experimentally to mathematically correct for the differences in signal intensity between the natural and isotopic forms of an analyte in samples at identical concentrations. Samples of 4.0 mL of the mixture of working solutions containing both natural and isotopically enriched analytes at 20.0 ng/mL were analyzed (n=28) to determine mean signal intensities for each natural and each isotopic analyte. A ratio was computed representing the signal intensity of a natural compound as a function of the signal intensity of the isotopic analog at identical concentrations.<sup>22</sup> This mass bias factor was applied as a correction factor to the isotope signals in the IDMS equation, as given by the following equation:<sup>10</sup>

Concentration (μmol/g) =

$$\text{Mass Bias} \times [(C_s W_s / W_x) \times {}^i P_s - (R_{i/n} \times {}^n P_s)] / [(R_{i/n} \times {}^n P_x) - {}^i P_x] \quad (\text{eq. 2})$$

$$\text{Mass bias} = A_N C_i / A_i C_N$$

Where  $A_N$  and  $A_i$  are the signal obtained from the TOF-MS for the natural analyte and the isotopic analog, respectively.  $C_N$  and  $C_i$  are the concentrations of the natural analyte and isotopic analog, respectively. Mass bias factors were computed for each compound and used as an internal correction factor in the quantitative method.

### *Statistics*

1  
2  
3  
4 For measurements of accuracy and precision, the percent error from calculated  
5 concentration (%error), percent relative standard deviation (%RSD), and 95% confidence  
6 intervals were used. For validation comparisons, the 95% confidence interval of the  
7  
8 experimentally determined mean was compared with the accompanying  $\pm 5\%$  standard deviation  
9  
10 of the certified standard. For comparison of means, p-values were computed to compare the  
11  
12 statistical similarity of two means with unequal variance, with  $p < 0.05$  indicating statistically  
13  
14 significant difference. All analyses in synthetic urine were blank-subtracted using synthetic urine  
15  
16 samples that were not spiked with either the natural or isotopically enriched analytes. Analyte-  
17  
18 specific limit of detection (LOD) was calculated using replicate measurements ( $n=10$ ) of a  
19  
20 method blank multiplied by three-times the standard deviation of the blank measured at expected  
21  
22 measured mass of the compounds determined in method development.<sup>24</sup> Limit of quantification  
23  
24 (LOQ) was determined as the concentration at which the experimentally determined  
25  
26 concentration ( $n=10$ ) of a compound differs to a statistically significant degree from the  
27  
28 calculated concentration of the compound at the 95% confidence level. Essentially, LOQ was  
29  
30 established to be the concentration at which quantitative accuracy was lost at the 95% confidence  
31  
32 level.  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42

### 43 **Conclusions**

44  
45  
46 This research has demonstrated viability of modifying SPE columns to produce pre-  
47  
48 calibration by loading columns with accurately known concentrations of isotopically labeled  
49  
50 analogs to remain quantitatively stable over a necessary amount of time. The method for column  
51  
52 pre-loading was developed, optimized, and validated for quantification of the organophosphate  
53  
54 pesticide glyphosate in drinking water. This pre-loading method was then adapted and applied to  
55  
56  
57  
58  
59  
60

1  
2  
3 a different column packing material for the quantification of seven drugs of abuse in synthetic  
4 urine. The pre-loading method was shown to be highly quantitatively stable over a period of two  
5 weeks for glyphosate and one week for all drugs of abuse, excluding cocaine and heroin. This  
6 work is useful to researchers seeking to develop methods to improve the transfer of high  
7 accuracy and precision analytical methods between and among laboratories. It was the objective  
8 of this research to reduce the complexity of sample analysis by producing a method without  
9 derivatization, chromatography, or calibration curves. As such, this work did not explore the  
10 application of pre-loaded SPE columns to the many forms of instrumental analysis for which  
11 IDMS has been previously successfully performed, including gas and liquid chromatography –  
12 mass spectrometry. Future work will expand the method validation to include a range of  
13 analytical instrumentation. However, as IDMS requires mass analysis, the method validated by  
14 this work is incompatible with instrumentation utilizing measurement techniques that do not  
15 measure ion mass, such as electromagnetic spectroscopy (e.g. fluorometry, atomic  
16 absorption/emission spectroscopy, infrared spectroscopy) and electroanalytical methods (e.g.  
17 amperometry, coulometry, potentiometry). Future work will be conducted on further increasing  
18 the on-column stability of analytes, increasing the breadth of applicable analytes and columns,  
19 and evaluation of field-deployment into off-site laboratories.  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44

#### 45 **Acknowledgements**

46  
47 The authors would like to thank Mizanur Rahman, Mesay Mulugetta Wolle, and Applied Isotope  
48 Technologies for intellectual contributions to this work.  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

## References

1. G. A. Theodoridis, H. G. Gika, E. J. Want and I. D. Wilson, *Anal. Chim. Acta*, 2012, 711, 7-16.
2. A. H. Wu and D. French, *Clin. Chem. Acta*, 2013, 420, 4-10.
3. A. C. Heijboer, M. A. Blankenstein, I. P. Kema and M. M. Buijs, *Clin. Chem.*, 2012, 58, 543-548.
4. S. Ranque, A. C. Normand, C. Cassagne, J. B. Murat, N. Bourgeois, F. Dalle, M. Gari - Toussaint, P. Fourquet, M. Hendrickx and R. Piarroux, *Mycoses*, 2014, 57, 135-140.
5. M. A. Jensen, L. Mortier, E. Koh, B. Keevil, S. Hyttinen and Å. M. Hansen, *Scand. J. Clin. Lab. Inv.*, 2014, 74, 454-461.
6. R. P. Grant and A. N. Hoofnagle, *Clin. Chem.*, 2014, 60, 941-944.
7. C. Lacroix, A. Gicquel, B. Sendid, J. Meyer, I. Accoceberry, N. François, F. Morio, G. Desoubieux, J. Chandenier and C. Kauffmann - Lacroix, *Clin. Microbiol. Infec.*, 2014, 20, 153-158.
8. P. Konieczka and J. Namieśnik, *J. Chromatogr. A*, 2010, 1217, 882-891.
9. K. Ridgway, S. P. Lalljie and R. M. Smith, *J. Chromatogr. A*, 2007, 1153, 36-53.
10. USEPA, ed. SW846, Washington, DC, 2008.
11. J. H. Pérez, M. Dabrio, B. Sejerøe-Olsen, A. F. Alba and H. Schimmel, *Talanta*, 2015.
12. A. J. Boggess, G. M. Rahman, M. Pamukcu, S. Faber and H. S. Kingston, *Analyst*, 2014, 139, 6223-6231.
13. I. Marginean, W. F. Rowe and I. S. Lurie, *Forensic Sci. Int.*, 2015.
14. L. Gao, J. Liu, C. Wang, G. Liu, X. Niu, C. Shu and J. Zhu, *J. Chromatogr. B*, 2014, 944, 136-140.
15. M. J. Swortwood, W. L. Hearn and A. P. DeCaprio, *Drug Test. Anal.*, 2014, 6, 716-727.
16. I. González-Mariño, J. B. Quintana, I. Rodríguez, M. González-Díez and R. Cela, *J. Anal. Chem.*, 2012, 84, 1708-1717.
17. M. R. Meyer, A. G. Helfer and H. H. Maurer, *Bioanalysis*, 2014, 6, 2275-2284.
18. H.-R. Lin, K.-I. Choi, T.-C. Lin and A. Hu, *J. Chromatogr. B*, 2013, 929, 133-141.

- 1
- 2
- 3
- 4 19. USEPA, Basic Information about Glyphosate in Drinking Water,  
5 <http://water.epa.gov/drink/contaminants/basicinformation/glyphosate.cfm>,  
6 Accessed February 12, 2015, 2015.
- 7
- 8 20. E. L. Delmonico, J. Bertozzi, N. E. de Souza and C. C. Oliveira, *Acta Scientiarum.*  
9 *Technology*, 2014, 36, 513-519.
- 10
- 11 21. E. L. Schymanski, H. P. Singer, P. Longrée, M. Loos, M. Ruff, M. A. Stravs, C. Ripollés  
12 Vidal and J. Hollender, *Environ. Sci. Technol.*, 2014, 48, 1811-1818.
- 13
- 14 22. R. Wagner, S. J. Wetzel, J. Kern and H. Kingston, *J. Mass Spectrom.*, 2012, 47, 147-154.
- 15
- 16 23. T. Kind and O. Fiehn, *BMC Bioinform.*, 2006, 7, 234.
- 17
- 18 24. D. Skoog, F. J. Holler and S. R. Crouch, *Instrumental Analysis*, Brooks/Cole, Andover,  
19 MA, 2007.
- 20
- 21
- 22
- 23
- 24
- 25
- 26
- 27
- 28
- 29
- 30
- 31
- 32
- 33
- 34
- 35
- 36
- 37
- 38
- 39
- 40
- 41
- 42
- 43
- 44
- 45
- 46
- 47
- 48
- 49
- 50
- 51
- 52
- 53
- 54
- 55
- 56
- 57
- 58
- 59
- 60



## Tables

Table 1: Experimentally optimized mass spectrometry parameters for the quantification of glyphosate.

Parameter	Value	Parameter	Value
<i>Ionization Mode</i>	Negative	<i>Dry Temperature</i>	200 °C
<i>Scan Range</i>	50 - 1000 <i>m/z</i>	<i>Capillary Exit</i>	-100 V
<i>Endplate Offset</i>	-500 V	<i>Skimmer 1</i>	-40.0 V
<i>Capillary Voltage</i>	+3750 V	<i>Hexapole 1</i>	-23.0 V
<i>Nebulizer</i>	0.5 Bar	<i>Hexapole RF</i>	65 Vpp
<i>Dry Gas</i>	4.0 L/min	<i>Skimmer 2</i>	-22.0 V

Table 2: Experimentally optimized mass spectrometry parameters for the quantification of opioid and alkaloid drugs of abuse.

Parameter	Value	Parameter	Value
<i>Ionization Mode</i>	Positive	<i>Dry Temperature</i>	200 °C
<i>Scan Range</i>	240-400 <i>m/z</i>	<i>Capillary Exit</i>	135 V
<i>Endplate Offset</i>	-500 V	<i>Skimmer 1</i>	40.0 V
<i>Capillary Voltage</i>	-4500 V	<i>Hexapole 1</i>	23.0 V
<i>Nebulizer</i>	0.4 Bar	<i>Hexapole RF</i>	250 Vpp
<i>Dry Gas</i>	4.0 L/min	<i>Skimmer 2</i>	24.0 V

Table 3: Validation values for opioids and alkaloids using ESI-TOF-MS, traditional SPE, and IDMS quantification for drugs of abuse in synthetic urine, showing 95% confidence

SPE-ESI-TOF-MS (n=5)	Calculated Value (ng/mL)	Experimental Value (ng/mL)	%Error	%RSD	LOD (ng/mL)	LOQ (ng/mL)
Morphine	40±2.00	42.2±6.65	5.57	11.6	0.446	0.800
Codeine	40±2.00	42.3±4.44	5.86	7.73	0.202	0.800
Cocaine	40±2.00	43.7±2.18	9.33	3.69	0.773	0.800
Methadone	40±2.00	39.7±2.32	0.689	4.32	0.128	0.800
6-AM	40±2.00	40.3±0.531	0.797	6.12	0.0502	0.800
Fentanyl	40±2.00	42.4±4.10	0.710	0.973	0.234	0.800
Heroin	40±2.00	42.2±6.65	6.18	7.13	0.238	0.800

Table 4: Validation values for opioids and alkaloids using ESI-TOF-MS, SPE pre-loading method, and IDMS quantification in synthetic urine, showing 95% confidence

Pre-loading (n=5)	Calculated Value (ng/mL)	Experimental Value (ng/mL)	%Error	%RSD	LOD (ng/mL)	LOQ (ng/mL)
Morphine	40±2.00	40.6±1.61	1.59	2.93	0.429	0.8
Codeine	40±2.00	39.7±3.40	0.766	6.32	0.214	0.8
Cocaine	40±2.00	34.8±5.07	13.0	10.1	0.737	0.8
Methadone	40±2.00	44.0±6.23	10.0	10.4	0.156	0.8
6-AM	40±2.00	39.4±1.87	1.56	3.43	0.0552	0.8
Fentanyl	40±2.00	40.3±4.49	0.873	8.21	0.222	0.8
Heroin	40±2.00	36.2±1.94	9.52	3.95	0.223	0.8

Table 5: Quantitative ions for each studied analyte and the corresponding exact and measured masses

Analyte	Quantitative Ion	Exact Mass ( $m/z$ )	Measured Mass ( $m/z$ )
Glyphosate	$C_3H_7NO_5P^+$	168.00618	168.00673
Morphine	$C_{17}H_{20}NO_3^+$	286.14432	286.15051
Codeine	$C_{18}H_{22}NO_3^+$	300.15997	300.16225
Cocaine	$C_{17}H_{22}NO_4^+$	304.15488	304.15816
Methadone	$C_{21}H_{28}NO^+$	310.21709	310.22002
6-AM	$C_{19}H_{22}NO_4^+$	328.15488	328.15521
Fentanyl	$C_{22}H_{29}N_2O^+$	337.22799	337.2277
Heroin	$C_{21}H_{24}NO_5^+$	370.16545	370.16887
Glyphosate-2-13C	$C_2^{13}C_1H_7NO_5P^-$	169.01485	169.01455
Morphine-D3	$C_{17}H_{17}D_3NO_3^+$	289.17031	289.1708
Codein-D3	$C_{18}H_{19}D_3NO_3^+$	303.18596	303.18769
Cocaine-D3	$C_{17}H_{19}D_3NO_4^+$	307.18088	307.18249
Methadone-D3	$C_{21}H_{25}D_3NO^+$	313.24308	313.24389
6-AM-D3	$C_{19}H_{19}D_3NO_4^+$	331.18088	331.1833
Fentanyl-D5	$C_{22}H_{24}D_5N_2O^+$	342.27131	342.27417
Heroin-D9	$C_{21}H_{15}D_9NO_5^+$	379.24343	379.24523

## Figure Captions

Figure 1: Averaged mass spectra (n=7) obtained from the analysis of drinking water spiked with 50 µg/mL of glyphosate and 50 µg/mL of glyphosate-2-<sup>13</sup>C showing baseline resolution and mass accuracy

Figure 2: A comparison of percent error of glyphosate quantification obtained in drinking water at various concentrations using IDMS and calibration curve quantifications. Dashed black line indicates certified value and shaded area represents ±5% certified error.


Figure 3: The effects on absolute value of percent error of multiple optimization techniques after (top) one week of storage and (bottom) two weeks of storage, with 95% confidence intervals shown

Figure 4: Quantitative stability over time of SPE columns pre-loaded with isotopically labeled glyphosate. Percent error and 95% confidence errors are shown.

Figure 5: A comparison of mean accuracy and precision (95% confidence range) of experimental values obtained in synthetic urine with calibration curve and IDMS across all listed analytes. Dashed black line indicates certified value and shaded area representing ±5% certified error.

\*Confidence interval falls outside of viewable range

Figure 6: Mean %error of pre-loaded columns after storage for indicated amounts of time, showing 95% confidence intervals. Dashed line represents the 10% error from certified value defined as adequate accuracy in this study.

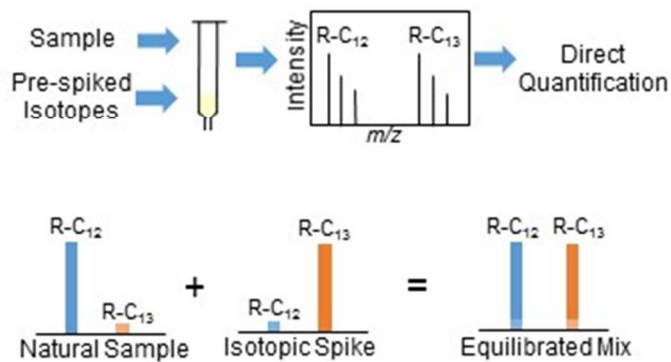

A technique has been developed to pre-calibrate solid-phase extraction columns for quantification using isotope dilution mass spectrometry.

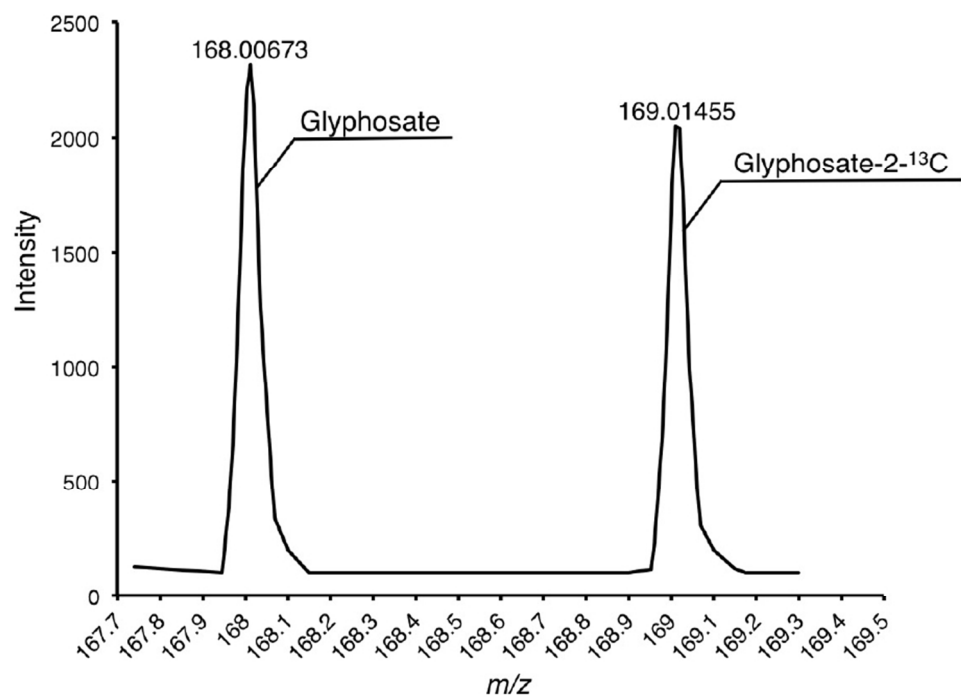


Figure 1: Averaged mass spectra (n=7) obtained from the analysis of drinking water spiked with 50  $\mu\text{g}/\text{mL}$  of glyphosate and 50  $\mu\text{g}/\text{mL}$  of glyphosate-2- $^{13}\text{C}$  showing baseline resolution and mass accuracy 81x60mm (300 x 300 DPI)

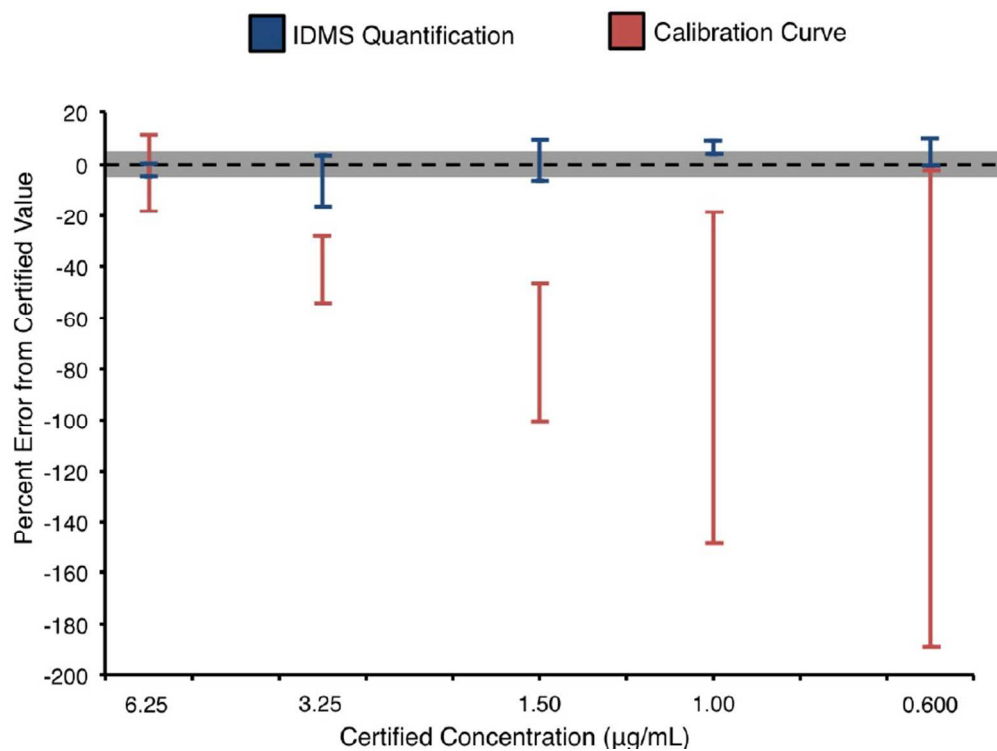


Figure 2: A comparison of percent error of glyphosate quantification obtained in drinking water at various concentrations using IDMS and calibration curve quantifications. Dashed black line indicates certified value and shaded area represents  $\pm 5\%$  certified error.  
81x60mm (300 x 300 DPI)

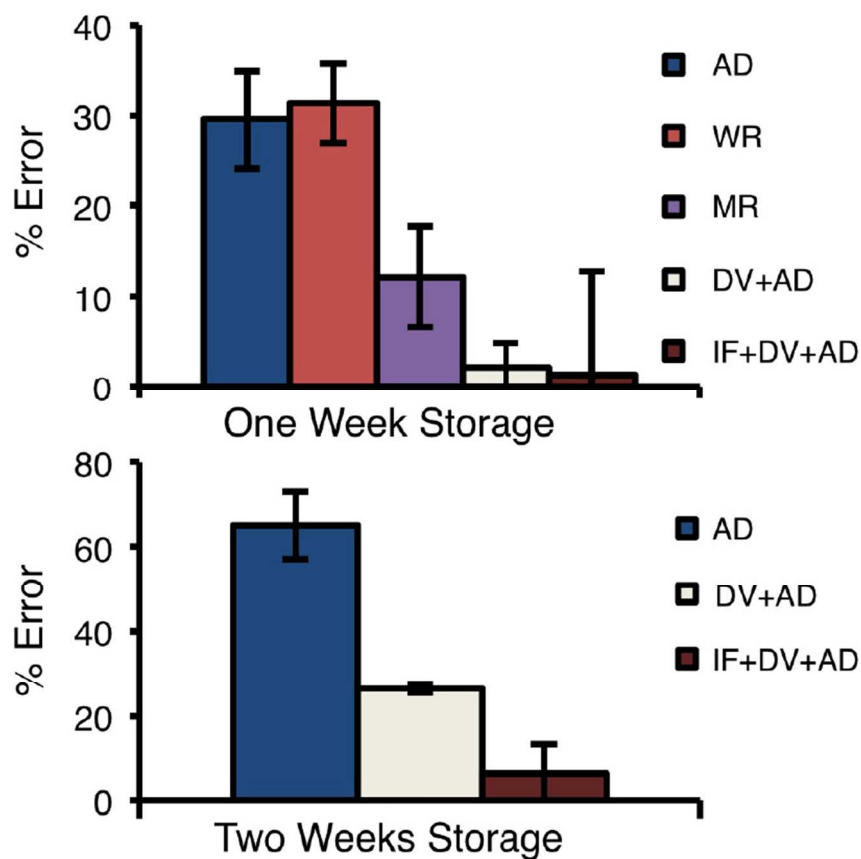


Figure 3: The effects on absolute value of percent error of multiple optimization techniques after (top) one week of storage and (bottom) two weeks of storage, with 95% confidence intervals shown  
81x71mm (300 x 300 DPI)

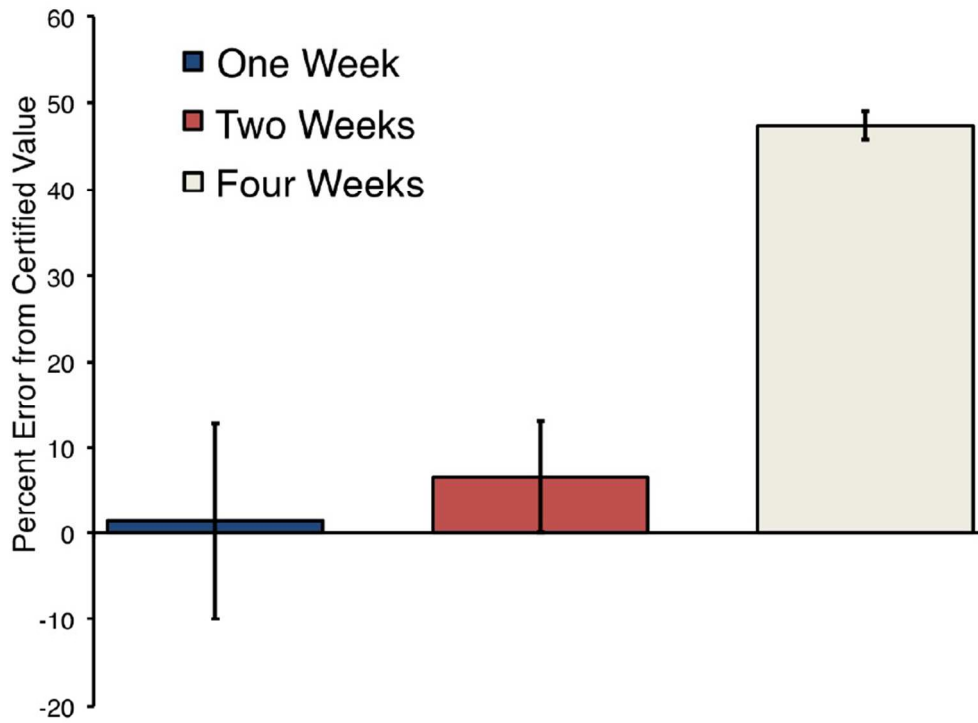


Figure 4: Quantitative stability over time of SPE columns pre-loaded with isotopically labeled glyphosate. Percent error and 95% confidence errors are shown.  
81x60mm (300 x 300 DPI)



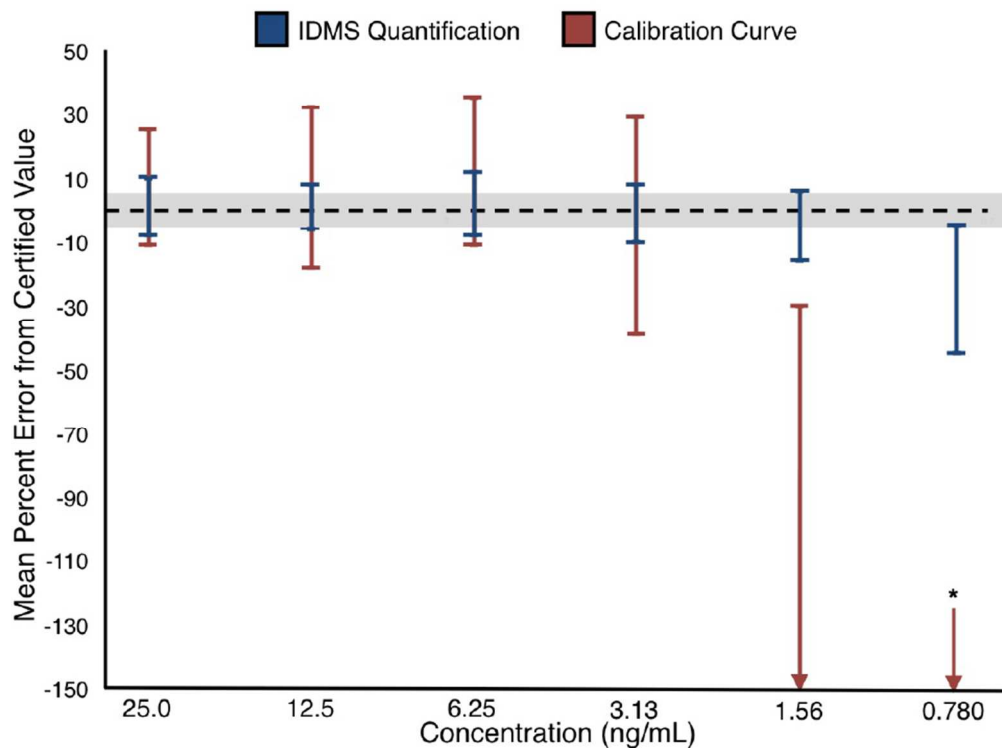


Figure 5: A comparison of mean accuracy and precision (95% confidence range) of experimental values obtained in synthetic urine with calibration curve and IDMS across all listed analytes. Dashed black line indicates certified value and shaded area representing  $\pm 5\%$  certified error.

\*Confidence interval falls outside of viewable range

81x60mm (300 x 300 DPI)

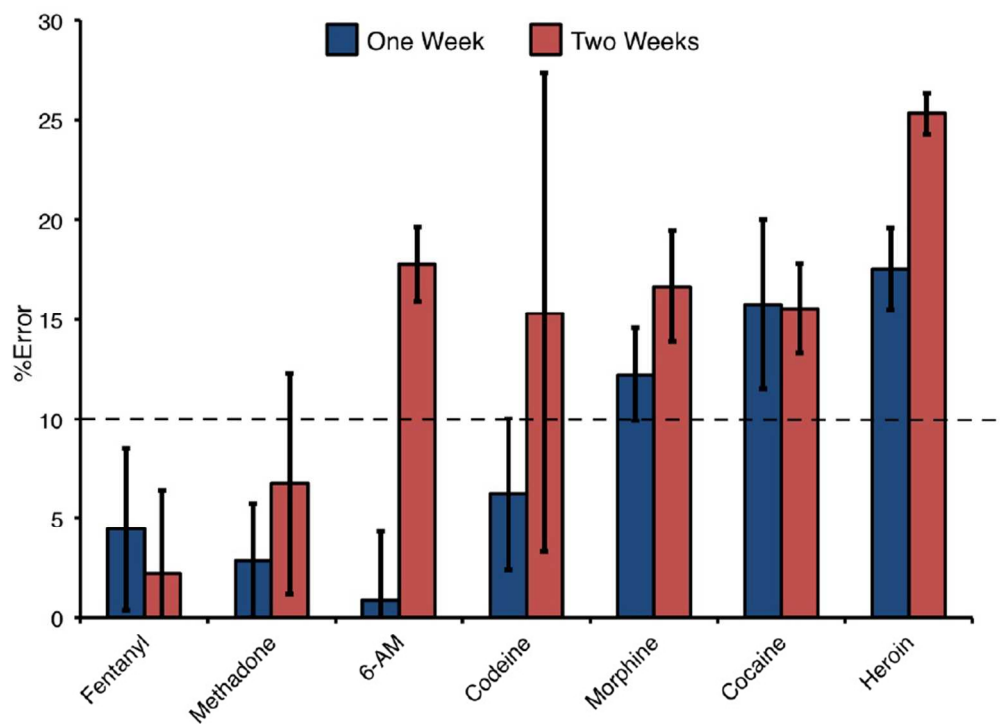


Figure 6: Mean %error of pre-loaded columns after storage for indicated amounts of time, showing 95% confidence intervals. Dashed line represents the 10% error from certified value defined as adequate accuracy in this study.  
81x60mm (300 x 300 DPI)