

# JAAS

Accepted Manuscript



This is an *Accepted Manuscript*, which has been through the Royal Society of Chemistry peer review process and has been accepted for publication.


*Accepted Manuscripts* are published online shortly after acceptance, before technical editing, formatting and proof reading. Using this free service, authors can make their results available to the community, in citable form, before we publish the edited article. We will replace this *Accepted Manuscript* with the edited and formatted *Advance Article* as soon as it is available.

You can find more information about *Accepted Manuscripts* in the [Information for Authors](#).

Please note that technical editing may introduce minor changes to the text and/or graphics, which may alter content. The journal's standard [Terms & Conditions](#) and the [Ethical guidelines](#) still apply. In no event shall the Royal Society of Chemistry be held responsible for any errors or omissions in this *Accepted Manuscript* or any consequences arising from the use of any information it contains.

Demonstration of a commercially-available, fully-automated, offline chromatography method capable of simultaneously purifying both Ca and Sr for stable and radiogenic isotope analysis.

Fully-Automated Purification of Sr and Ca from Complex Matrices

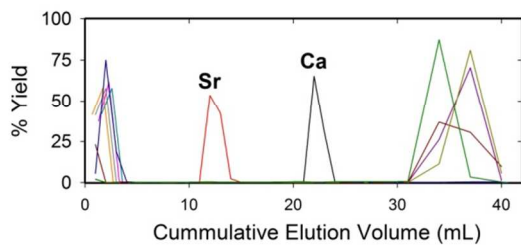

## Fully Automated Chromatographic Purification of Sr and Ca for Isotopic Analysis

S. J. Romaniello<sup>a</sup>, M. P. Field<sup>b</sup>, H. B. Smith<sup>a</sup>, G. W. Gordon<sup>a</sup>, M. H. Kim<sup>b</sup> and A. D. Anbar<sup>a,c</sup>

<sup>a</sup> School of Earth & Space Exploration, Arizona State University, Tempe, AZ, USA

<sup>b</sup> Elemental Scientific, Inc., Omaha, NE, USA

<sup>c</sup> Department of Chemistry & Biochemistry, Arizona State University, Tempe, AZ, USA

### Abstract

We present a commercially-available, fully-automated, offline chromatography method capable of simultaneously purifying both Ca and Sr for stable and radiogenic isotope analysis. The method features effective purification and mutual separation of Ca and Sr from multiple complex matrixes using a single, highly-reusable chromatographic column. Low carryover combined with high yield for multiple extractions indicate the column can be reused for at least 200 samples. Accurate and precise stable and radiogenic data are presented for the USGS standard BCR-2 basalt, NIST-1400 bone ash, IAPSO seawater, and an in-house llama bone standard (CUE-0001). The Sr-Ca method was designed to accommodate a wide variety of sample types, including carbonates, bones, and teeth; silicate rocks and sediments; fresh and marine waters; and biological samples such as blood and urine. The system is highly adaptable and capable of unattended processing up to 60 samples per run at a rate of 32 samples per day on a single chromatographic column.

### Introduction

High throughput methods for sample purification are required to effectively exploit new opportunities in the study of radiogenic and non-traditional stable isotopes. Many isotope studies in geochemistry, anthropology, biomedicine and forensics would benefit from larger data sets, but these are often impractical with manual drip chromatography techniques, which can be time-consuming and demand the attention of skilled laboratory staff. Automated methods have been successfully adopted in

1  
2  
3 other fields of isotope studies, including continuous-flow gas-source isotope ratio mass  
4 spectrometry and noble gas mass spectrometry.<sup>1,2</sup> Development and adoption of similar approaches for  
5 radiogenic and non-traditional stable isotopes has been slower, hindered by the requirement for very  
6 low sample carryover and the materials challenge of working with concentrated strong acids.  
7  
8  
9

10 Applications for Ca and Sr isotopic analysis, including paleoceanography, isotope stratigraphy  
11 and sedimentology, isotope forensics, and anthropology are driving a demand for large Ca and Sr  
12 isotope datasets.<sup>3-13</sup> Moreover, emerging applications for stable isotope fractionation of metals, such as  
13 Ca, are poised to dramatically alter the field.<sup>14-19</sup> Large-scale clinic trials for medical applications of Ca  
14 isotopes will require increased sample throughput, rapid turnaround time, and reduced analytical  
15 costs—all of which point toward the need for automation. There have been multiple efforts to automate  
16 the chromatographic purification of Ca and Sr, including both online and offline methods.<sup>20-25</sup> Although  
17 individually successful, these methods have not enjoyed widespread adoption. We believe this is  
18 because the proposed approaches often required substantial modification of commercially available  
19 hardware, only functioned for a subset of potential sample types, and/or were perceived as analytically  
20 inferior to established manual techniques.  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36

37 The main barriers to automation of Ca and Sr chromatography are the requirements for low  
38 blanks and negligible sample carryover, particularly due to the large natural isotope range for radiogenic  
39 Sr isotopes. Furthermore, Ca and Sr should be mutually separated both from each other as well as  
40 sample matrix for analysis on higher throughput MC-ICP-MS instruments. Eichrom SrSpec<sup>TM</sup> resin is  
41 commonly used both to purify Sr and to remove traces of Sr from Ca samples before isotopic analysis.<sup>26-</sup>  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

<sup>31</sup> However, SrSpec<sup>TM</sup> is difficult to repeatedly reuse without extensive cleaning due to a tendency to  
retain ~0.01-1% of Sr as sample carryover.<sup>27, 32</sup>

Here we present a novel fully-automated, offline Ca and Sr separation method which attempts  
to circumvent the aforementioned difficulties. The method exploits a commercially-available hardware

1  
2  
3 platform and a novel, highly-reusable Sr-Ca column. The analytical performance of this method is  
4  
5 evaluated for a range of representative sample matrixes.  
6  
7

## 8 **Experimental**

### 9 **Reagents and Materials**

10 All reagents used in the sample digestion and separation chemistry are prepared from high  
11  
12 purity hydrochloric acid, nitric acid, hydrogen peroxide, and hydrofluoric acid. HCl and HNO<sub>3</sub> were  
13  
14 prepared by sub-boiling distillation at ASU. H<sub>2</sub>O<sub>2</sub> and HF were Fluka TraceSelect Ultra grade (Sigma-  
15  
16 Aldrich, St. Louis, Missouri, USA). Solutions were prepared by dilution with 18.2 MΩ-cm deionized water  
17  
18 (Table 1).  
19  
20  
21  
22  
23

24 All materials used for sample handling are made of fluoropolymer, polypropylene or polyethylene, and  
25  
26 were acid washed for >24 hours each in 20 vol. % HNO<sub>3</sub> and 20 vol. % HCl prior to use.  
27  
28

### 29 **Samples**

30  
31 Chemical purification of Ca and Sr was tested on a variety of sample types including seawater  
32  
33 (IAPSO), basalt (BCR-2), bone ash (NIST-1400), and an in-house llama bone standard (CUE-0001).  
34  
35 Samples were chosen to span a range of matrix types, Ca/Sr ratios (110, 320, 3350, and 560 mol:mol,  
36  
37 respectively) and to provide an intentionally wide range of stable Ca, stable Sr, and radiogenic <sup>87</sup>Sr/<sup>86</sup>Sr  
38  
39 ratios for the purposes of testing sample carryover.  
40  
41

### 42 **Digestion and Sample Dissolution**

43  
44 15 mL of seawater and 100 mg each of bone ash and bone standards were digested on a hot  
45  
46 plate using 5mL of concentrated HNO<sub>3</sub> in Savillex™ PFA vials. Vials were sealed and heated overnight on  
47  
48 a hot plate at 110°C, then evaporated to dryness. Any residual organic residue was digested by heating  
49  
50 for several hours at 110°C in 0.5mL concentrated HNO<sub>3</sub> + 0.2 mL 30% H<sub>2</sub>O<sub>2</sub>. The BCR-2 basalt standard  
51  
52 (100mg) was dissolved using 5 mL of HNO<sub>3</sub> and 1 mL of concentrated HF in a sealed Savillex™ PFA vial.  
53  
54  
55  
56 The sample was ultrasonicated for 30 minutes and then heated at 110°C overnight on a hotplate.  
57  
58  
59  
60

1  
2  
3 Following this, 90% of the solution was evaporated and 5 mL of concentrated HCl was added. This  
4  
5 solution was heated for several hours to dissolve any residual fluorides. All samples were dried down  
6  
7 and dissolved in 2 M HNO<sub>3</sub> in preparation for column chemistry.  
8  
9

### 10 **Ca and Sr Separation**

11  
12 The automated purification of Ca and Sr for isotopic analysis is performed using the  
13  
14 prepFAST MC (ESI, Omaha, NE, USA) and the supplied 1 mL Sr-Ca column (Part Number CF-MC-SrCa-  
15  
16 1000). The prepFAST MC is a fully-automated, low pressure (<100 psi), fluoropolymer chromatography  
17  
18 system that performs several basic functions to isolate elements of interest. It consists of an  
19  
20 autosampler, two 6-port 2-position valves, one 10-port multi position valve, a S400V syringe pump with  
21  
22 a fill-dispense valve, and a 13 mL sample loop.  
23  
24

25  
26 The system's integrated software is programmed to perform various functions required for  
27  
28 matrix removal and sample purification including column pre-cleaning, column conditioning, sample  
29  
30 loading, and matrix and analyte elution and collection. The software allows the user to define the  
31  
32 location, volume, flow rate, and destination for each sample and reagent. The software also includes an  
33  
34 option to automatically generate sample elution curves by dispensing small reagent increments into  
35  
36 user-pre-defined tubes (column calibration mode) or collect cuts in their entirety for normal sample  
37  
38 processing.  
39  
40

41  
42 A description of the column elution protocol used in this study is provided in Table 1. Elution  
43  
44 with 2M HNO<sub>3</sub> + 1 wt. % H<sub>2</sub>O<sub>2</sub> removes most major and trace matrix elements. Sr is eluted in 6 M HNO<sub>3</sub>  
45  
46 and Ca with 12 M HNO<sub>3</sub>. In the final step, 10 mL of 1 M HF is used to remove all remaining elements on  
47  
48 the resin (REEs, HF, Cd, and U) leaving the resin clean for the next sample. The entire automated  
49  
50 protocol requires 45 minutes per sample, allowing 32 samples to be processed per 24 hours.  
51  
52

### 53 **Elemental Concentrations**

Blanks and yields were measured on a ICAP-Q quadrupole inductively-coupled plasma mass spectrometer (Thermo Scientific, Bremen, Germany) at Arizona State University. Samples were analyzed in 0.32 M HNO<sub>3</sub> and quantified using a multielement internal standard in combination with external calibration curves. Doubly-charged Sr (<sup>84</sup>Sr<sup>++</sup>, <sup>86</sup>Sr<sup>++</sup>, <sup>88</sup>Sr<sup>++</sup>) represents a significant interference on <sup>42</sup>Ca<sup>+</sup>, <sup>43</sup>Ca<sup>+</sup>, and <sup>44</sup>Ca<sup>+</sup>, which was corrected by measuring <sup>87</sup>Sr<sup>++</sup> at mass 43.5 AMU in high-resolution mode and assuming an <sup>87</sup>Sr/<sup>86</sup>Sr ratio of 0.71.

### Ca and Sr Isotopic Measurements.

Ca and Sr isotopic compositions were measured at Arizona State University using a Neptune multi-collector inductively-coupled plasma mass spectrometer (MC-ICP-MS, Thermo Scientific, Bremen, Germany) equipped with a Jet sample cone, an H-skimmer cone, and an Apex-Q desolvating nebulizer (ESI, Omaha, NE, USA).

Ca isotope measurements were performed using sample-standard bracketing in medium resolution following previous published methods.<sup>16, 30, 33</sup> Optimized instrument operating parameters were sample gas = 0.9 L min<sup>-1</sup>, auxiliary gas = 0.9 L min<sup>-1</sup>, cool gas = 14.50 L min<sup>-1</sup>, N<sub>2</sub> = 2-5 mL min<sup>-1</sup>. Ca samples were introduced at a concentration of 3 ppm and flow rate of 200 μL min<sup>-1</sup>, yielding a sensitivity of ~3.3V <sup>44</sup>Ca<sup>+</sup> / ppm Ca. Samples were introduced in a matrix of 0.16 M HNO<sub>3</sub> which eliminates nebulizer clogging associated with the formation of CaNO<sub>3</sub> precipitates when using a higher concentration HNO<sub>3</sub> matrix. Faraday cups were positioned to collect <sup>42</sup>Ca<sup>+</sup>, <sup>43</sup>Ca<sup>+</sup>, <sup>44</sup>Ca<sup>+</sup>, <sup>45</sup>Sc<sup>+</sup>, <sup>47</sup>Ti<sup>+</sup>, and <sup>48</sup>Ca<sup>+</sup>. The Ca and Ti positions were offset relative to <sup>45</sup>Sc<sup>+</sup>, aligning the peak center of <sup>45</sup>Sc<sup>+</sup> on the center cup with the uninterfered low-mass shoulder of the Ca and Ti isotopes.<sup>33</sup> In medium resolution, the typical width of the uninterfered low-mass shoulder was 0.004 AMU and the optimal peak position was determined by systematically measuring the standard deviation of the Ca isotopic ratios at 0.001 AMU intervals across the peak shoulder. Each measurement consisted of 25 8.4s cycles. Samples were measured relative to an in-house ICP Ca solution (ICP1; NIST 10,000 ppm ICP Ca standard, lot #X-10-39A)

1  
2  
3 and converted to the SRM915a scale by subtracting  $\delta^{44/42}\text{Ca} = -0.25 \pm 0.01\text{‰}$  (2se, N = 188).<sup>30</sup> Data  
4  
5 quality and precision was assessed by measuring each sample 3 times as well as intercomparison of the  
6  
7  $\delta^{44/42}\text{Ca}$ ,  $\delta^{44/43}\text{Ca}$ ,  $\delta^{48/42}\text{Ca}$  on a per AMU basis. Final data are reported on as  $\delta^{44/42}\text{Ca}_{\text{SRM915a}}$  with a typical  
8  
9  $2\sigma$  precision of 0.06‰.

10  
11 Radiogenic ( $^{87}\text{Sr}/^{86}\text{Sr}$ ) and stable ( $\delta^{88/86}\text{Sr}$ ) Sr data were obtained simultaneously in low-  
12  
13 resolution using sample-standard bracketing with Zr-element doping.<sup>28, 29, 34</sup> Zr was added to all samples  
14  
15 and standards at a concentration of 15 ppb. Sr samples were introduced at 25 ppb and a flow rate of  
16  
17 200  $\mu\text{L min}^{-1}$  in a matrix of 0.32M  $\text{HNO}_3$  yielding a sensitivity of  $\sim 0.7 \text{ V } ^{88}\text{Sr}^+ / \text{ppb Sr}$ . Faraday cups were  
18  
19 positioned to collect  $^{82}\text{Kr}^+$ ,  $^{83}\text{Kr}^+$ ,  $^{84}\text{Sr}^+$ ,  $^{85}\text{Rb}^+$ ,  $^{86}\text{Sr}^+$ ,  $^{87}\text{Sr}^+$ ,  $^{88}\text{Sr}^+$ ,  $^{90}\text{Zr}^+$ , and  $^{91}\text{Zr}^+$ . Each measurement  
20  
21 consisted of 20 8.4s cycles, and samples were run in blank-standard-sample-standard-blank blocks, with  
22  
23 SRM 987 Sr as the bracketing standard. Kr, a trace impurity in high-purity Ar gas, was measured at  $^{83}\text{Kr}^+$   
24  
25 with a typical intensity of  $\sim 280 \text{ uV}$ . A first-order correction was performed by subtracting on-peak blank  
26  
27 intensities measured every fourth analysis in “blank-std-smpl-std-blank” brackets. This reduced the  
28  
29 magnitude of the blank-subtracted  $^{83}\text{Kr}$  to  $\pm 30 \text{ uV}$ . Correction for the residual Kr was made assuming an  
30  
31  $^{83}\text{Kr}/^{84}\text{Kr}$  ratio of 0.201750, an  $^{83}\text{Kr}/^{86}\text{Kr}$  ratio of 0.664533, and an exponential mass bias correction based  
32  
33 on an  $^{86}\text{Sr}/^{88}\text{Sr}$  ratio of 0.1194. A Rb correction was applied similarly, assuming an  $^{85}\text{Rb}/^{87}\text{Rb}$  ratio of  
34  
35 2.58896. The typical magnitude of the Kr and Rb correction following subtraction of the on-peak blanks  
36  
37 was  $\sim 15 \text{ ppm}$  on the  $^{87}\text{Sr}/^{86}\text{Sr}$  ratio. Following interference correction, radiogenic Sr was corrected for  
38  
39 instrument mass bias by normalizing to  $^{86}\text{Sr}/^{88}\text{Sr} = 0.1194$ . Stable Sr values were corrected in two stages  
40  
41 by first normalizing all samples and standards to a constant  $^{91}\text{Zr}/^{90}\text{Zr}$  ratio followed by sample-standard  
42  
43 bracketing. Each sample was measured 3 times, with a typical  $2\sigma$  precision of 0.00001 for  $^{87}\text{Sr}/^{86}\text{Sr}$  and  
44  
45 0.04‰ for  $\delta^{88/86}\text{Sr}$ .  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55

## 56 Results and Discussion



### Ca and Sr Elution

High precision isotopic analyses of Ca and Sr by MC-ICP-MS can be affected by a number of isobaric and matrix interferences summarized in Table 2. The most important direct isobaric interferences for Ca include  $^{48}\text{Ti}^+$  on  $^{48}\text{Ca}^+$ , doubly-charged  $^{84,86,88}\text{Sr}^{++}$  on  $^{42,43,44}\text{Ca}^+$ , respectively, and gas-derived interferences such as  $^{14}\text{N}_3^+$ ,  $^{12}\text{C}^{16}\text{O}_2^+$ , and  $^{14}\text{N}_2^{16}\text{O}^+$ .<sup>30, 31, 33</sup> The most important isobaric interferences for Sr include  $^{87}\text{Rb}^+$  on  $^{87}\text{Sr}^+$ , gas-derived  $^{84,86}\text{Kr}^+$  on  $^{84,86}\text{Sr}^+$ , and sample-derived Zr which interferes with the Zr-doping procedure commonly used to correct instrument mass bias for stable Sr isotope measurements.<sup>35</sup> Both Ca and Sr stable isotope measurements are also subject to matrix interferences resulting from variations in instrument mass bias due to variable sample ionic strength.<sup>30</sup> As a result, major matrix elements such as Na, Mg, K, and Fe must be separated from Ca and Sr prior to analysis.

The Sr-Ca column allows direct separation of Ca and Sr from complex sample matrices using a single column. Figure 1 shows elutions curves for each standard used in this study. These curves were generated automatically, using the column calibration feature of the prepFAST-MC. The first step efficiently removes most matrix elements including Na, Mg, Al, K, Ti, Fe, Rb, Zr, and Ba in 2M  $\text{HNO}_3$ . This is followed by elution of Sr and Ca in 6M and 12M  $\text{HNO}_3$ , respectively. Previous studies have shown that doubly-charged Sr is a potentially significant interference on MC-ICP-MS measurements of Ca isotopes and requires a Ca/Sr ratio >10,000 to avoid significant analytical artifacts.<sup>30</sup> This method allows for consistent separation of Sr from Ca with a Ca/Sr ratio greater than 100,000 (Table 3). The remaining retained elements, including rare earths, Cd, Zr, and U are discarded from the column in the final wash column step using 1 M HF. The purity of the BCR-2 Sr and Ca elution cuts are tabulated as Ca and Sr/elemental ratios before and after separation (Table 3).

### Column Yield and Lifespan

1  
2  
3 The capability to reuse the column for multiple samples is crucial in determining the length of  
4 automated runs. Percent yields for Ca and Sr are plotted for 60 consecutive samples processed over 48  
5 hrs (Figure 2). High constant yields of greater than  $93 \pm 2\%$  for both Ca and Sr indicate no degradation in  
6 binding efficiency for up to 60 extractions. Continued sample processing beyond this experiment did not  
7 exhaust the column and our experience suggests that up to 200 samples can be extracted on a single  
8 column.  
9

### 17 **Column Capacity**

18  
19 Previous work has shown low chromatographic yields can result in isotopic fractionation of Ca  
20 and Sr during purification.<sup>30, 36-39</sup> Although the method described here results in nearly quantitative  
21 recovery of Ca and Sr, Ca and Sr yields can be negatively impacted if the sample size exceeds the  
22 capacity of the resin to bind analyte ions. To determine the column capacity, yields and stable Ca and Sr  
23 isotopes were measured as function of sample mass (Figure 3). The samples consisted of 0.026-2.6 mg  
24 of NIST 1400 Bone Ash (10-1000 $\mu$ g Ca).  
25  
26  
27  
28  
29  
30  
31  
32

33 Because Ca is the only major element which binds to the Sr-Ca column during separation, Ca and  
34 Sr yields are primarily controlled by the mass of Ca loaded onto the column. Samples up to 300  $\mu$ g Ca  
35 show greater than 95% yield for Sr and Ca. Loading more than 300  $\mu$ g of Ca on the 1 mL column results  
36 in breakthrough and parallel decreases in Ca and Sr yields to approximately 75% at 1000  $\mu$ g of Ca. Based  
37 on these results, a typical sample size of 100  $\mu$ g Ca is suggested (Figure 3a).  
38  
39  
40  
41  
42  
43  
44

45 An interesting feature of the Sr-Ca column is that isotopic fractionation on the column appears  
46 to be minimal for both Ca and Sr (Fig. 3b). Even with yields as low as 75%, the measured stable isotopic  
47 composition of Ca and Sr in NIST 1400 was indistinguishable from samples with nearly 100% yield at  
48 current measurement precision (Fig 3b).  
49  
50  
51  
52

### 54 **Blanks and Sample Carryover**

1  
2  
3 Overall method blanks were determined by processing 2 M HNO<sub>3</sub> blank samples randomly  
4 interspersed with samples during a typical run sequence. Measured blanks were similar to conventional  
5 Ca and Sr manual drip methods, 100 ng Ca and 30-150 pg Sr, respectively.<sup>27, 31, 32</sup> Correlation of  
6 measured Sr blanks with the total Sr in the previous sample suggests that carryover was limited to a  
7 factor of  $< 4 \times 10^{-5}$ . This level of carryover is similar to reagent blanks and results in negligible isotopic  
8 shift even for relatively large variations in radiogenic <sup>87</sup>Sr/<sup>86</sup>Sr ratios. For example, for similarly-sized  
9 samples, the calculated carryover of a radiogenic sample with <sup>87</sup>Sr/<sup>86</sup>Sr = 0.74 on a sample with <sup>87</sup>Sr/<sup>86</sup>Sr  
10 = 0.70, would represent only a 2.4ppm error.  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21

### 22 Method Validation Samples

23  
24 In order to test overall method performance, four samples were chosen to represent a range of  
25 sample matrix types with variable Sr/Ca ratios. The samples include three CRMs (USGS BCR-2 basalt,  
26 NIST 1400 bone ash, OSIL IAPSO seawater) and one in-house llama bone standard (CUE-0001). These  
27 samples were intentionally chosen to span a range of isotopic compositions, particularly for <sup>87</sup>Sr/<sup>86</sup>Sr,  
28 demanding low sample carryover for accurate and precise results. Each sample was analyzed 4-5 times  
29 in a randomly ordered sequence, such that any carryover effects of one sample on the next should be  
30 evident as increased scatter in the sample precision.  
31  
32  
33  
34  
35  
36  
37  
38  
39

40 The results of this test suggest that a variety of matrix types can be processed sequentially with  
41 high yields and low carryover, allowing accurate and precise Ca and Sr isotopic measurements (Table 4,  
42 Figure 4). Calcium and strontium yields were greater than 95% for all samples, demonstrating near-  
43 quantitative recovery for all matrix types (Figure 4). Radiogenic <sup>87</sup>Sr/<sup>86</sup>Sr for replicate sample aliquots are  
44 consistent within the long-term reproducibility of the bracketing SRM 987 standard (2sd = 0.000017)  
45 demonstrating negligible sample carryover. The accuracy and precision of both Ca and Sr isotopes are  
46 similar to published literature values indicating that the automated method produces high-quality data  
47 comparable to existing manual methods.  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

## Conclusion

We present a commercially-available, fully-automated, offline chromatography method capable of purifying both Ca and Sr for stable and radiogenic isotope analysis. This method allows >200 samples to be processed sequentially on the same separation column at a rate of ~32 samples/day.

In addition to increasing sample throughput and reducing personnel costs, automating sample preparation of Ca and Sr for MC-ICP-MS analyses will facilitate acquisition of large, high-resolution data sets and help to expand the use of these isotopic systems in new fields such as biomedical applications of non-traditional stable isotopes.

This method is part of a family of new fully-automated chromatographic methods being developed to address many different isotopic systems including B, Ca, Fe, Cu, Zn, Sr, Cd, Pb, and U using the prepFAST MC. These methods are designed to be rugged and transferrable, and to allow the preparation of large, diverse sample sets via a highly repeatable process with minimal effort.

## Acknowledgements

The authors appreciate Professor Kelly Knudson's permission to use the CUE-0001 standard. Funding support was provided by the NASA Human Research Program (NNX14AB78G), NASA Exobiology Program (NNX13AJ71G), and Elemental Scientific, Inc.

## Notes and references

<sup>a</sup> School of Earth & Space Exploration, Arizona State University, Tempe, AZ, USA

<sup>b</sup> Elemental Scientific, Inc., Omaha, NE, USA

<sup>c</sup> Department of Chemistry & Biochemistry, Arizona State University, Tempe, AZ, USA

1. J. T. Brenna, T. N. Corso, H. J. Tobias and R. J. Caimi, *Mass Spectrometry Reviews*, 1997, 16, 227-258.
2. R. H. R. Stanley, B. Baschek, D. E. Lott and W. J. Jenkins, *Geochemistry, Geophysics, Geosystems*, 2009, 10, Q05008.
3. R. Alexander Bentley, *J Archaeol Method Theory*, 2006, 13, 135-187.
4. J. B. West, G. J. Bowen, T. E. Dawson and K. P. Tu, eds., *Isoscapes: Understanding Movement, Pattern and Process on Earth Through Isotope Mapping*, Springer, 2010.
5. C. L. Blättler, G. M. Henderson and H. C. Jenkyns, *Geology*, 2012, 40, 843-846.

6. J. L. Payne, A. V. Turchyn, A. Paytan, D. J. DePaolo, D. J. Lehrmann, M. Yu and J. Wei, *Proceedings of the National Academy of Sciences*, 2010, 107, 8543-8548.
7. C. L. Blättler and J. A. Higgins, *Geology*, 2014.
8. S. R. Brennan, D. P. Fernandez, G. Mackey, T. E. Cerling, C. P. Bataille, G. J. Bowen and M. J. Wooller, *Chemical Geology*, 2014, 389, 167-181.
9. L. A. Chesson, B. J. Tipple, G. N. Mackey, S. A. Hynek, D. P. Fernandez and J. R. Ehleringer, *Ecosphere*, 2012, 3.
10. M. S. Fantle and E. T. Tipper, *Earth-Science Reviews*, 2014, 129, 148-177.
11. E. M. Griffith, M. S. Fantle, A. Eisenhauer, A. Paytan and T. D. Bullen, *Earth and Planetary Science Letters*, 2015, 419, 81-92.
12. E. M. Griffith, A. Paytan, A. Eisenhauer, T. D. Bullen and E. Thomas, *Geology*, 2011, 39, 683-686.
13. H. Vollstaedt, A. Eisenhauer, K. Wallmann, F. Boehm, J. Fietzke, V. Liebetrau, A. Krabbenhoeft, J. Farkas, A. Tomasovych, J. Raddatz and J. Veizer, *Geochimica Et Cosmochimica Acta*, 2014, 128, 249-265.
14. G. W. Gordon, J. Monge, M. B. Channon, Q. Wu, J. L. Skulan, A. D. Anbar and R. Fonseca, *Leukemia*, 2014, 28, 2112-2115.
15. A. Heuser and A. Eisenhauer, *Bone*, 46, 889-896.
16. J. L. L. Morgan, J. L. Skulan, G. W. Gordon, S. J. Romaniello, S. M. Smith and A. D. Anbar, *Proceedings of the National Academy of Sciences of the United States of America*, 2012, 109, 9989-9994.
17. J. Skulan, T. Bullen, A. D. Anbar, J. E. Puzas, L. Shackelford, A. LeBlanc and S. M. Smith, *Clinical Chemistry*, 2007, 53, 1155-1158.
18. J. Skulan and D. J. DePaolo, *Proceedings of the National Academy of Sciences*, 1999, 96, 13709-13713.
19. M. B. Channon, G. W. Gordon, J. L. L. Morgan, J. L. Skulan, S. M. Smith and A. D. Anbar, *Bone*, 2015, 77, 69-74.
20. P. Galler, A. Limbeck, S. F. Boulyga, G. Stinger, T. Hirata and T. Prohaska, *Anal. Chem.*, 2007, 79, 5023-5029.
21. S. Garcia-Ruiz, M. Moldovan and J. I. Garcia Alonso, *Journal of Analytical Atomic Spectrometry*, 2008, 23, 84-93.
22. C. Latkoczy, T. Prohaska, M. Watkins, M. Teschler-Nicola and G. Stinger, *Journal of Analytical Atomic Spectrometry*, 2001, 16, 806-811.
23. P. Galler, A. Limbeck, M. Uveges and T. Prohaska, *Journal of Analytical Atomic Spectrometry*, 2008, 23, 1388-1391.
24. C. L. Blättler, N. R. Miller and J. A. Higgins, *Earth and Planetary Science Letters*, 2015, 419, 32-42.
25. A.-D. Schmitt, S. Gangloff, F. Cobert, D. Lemarchand, P. Stille and F. Chabaux, *Journal of Analytical Atomic Spectrometry*, 2009, 24, 1089-1097.
26. E. P. Horwitz, M. L. Dietz and D. E. Fisher, *Anal. Chem.*, 1991, 63, 522-525.
27. C. Pin, D. Briot, C. Bassin and F. Poitrasson, *Analytica Chimica Acta*, 1994, 298, 209-217.
28. L. Yang, C. Peter, U. Panne and R. E. Sturgeon, *Journal of Analytical Atomic Spectrometry*, 2008, 23, 1269-1274.
29. J. Ma, G. Wei, Y. Liu, Z. Ren, Y. Xu and Y. Yang, *Chin. Sci. Bull.*, 2013, 58, 3111-3118.
30. J. L. L. Morgan, G. W. Gordon, R. C. Arrua, J. L. Skulan, A. D. Anbar and T. D. Bullen, *Anal. Chem.*, 2011, 83, 6956-6962.
31. T. Tacail, E. Albalat, P. Telouk and V. Balter, *Journal of Analytical Atomic Spectrometry*, 2014, 29, 529-535.
32. C. Pin, A. Gannoun and A. Dupont, *Journal of Analytical Atomic Spectrometry*, 2014, 29, 1858-1870.
33. M. E. Wieser, D. Buhl, C. Bouman and J. Schwieters, *Journal of Analytical Atomic Spectrometry*, 2004, 19, 844-851.

- 1  
2  
3 34. K. J. Knudson, H. M. Williams, J. E. Buikstra, P. D. Tomczak, G. W. Gordon and A. D. Anbar,  
4 *Journal of Archaeological Science*, 2010, 37, 2352-2364.  
5 35. P. Z. Vroon, B. van der Wagt, J. M. Koornneef and G. R. Davies, *Anal Bioanal Chem*, 2008,  
6 390, 465-476.  
7 36. Y. Fukuda, Y.-H. Zhang, M. Nomura, T. Suzuki, Y. Fujii and T. Oi, *Journal of Nuclear Science*  
8 *and Technology*, 2010, 47, 176-183.  
9 37. T. Oi, H. Ogino, M. Hosoe and H. Kakahana, *Separation Science and Technology*, 1992, 27,  
10 631-643.  
11 38. W. A. Russell and D. A. Papanastassiou, *Anal. Chem.*, 1978, 50, 1151-1154.  
12 39. Y. Fujii, M. Nomura, T. Kaneshiki, Y. Sakuma, T. Suzuki, S. Umehara and T. Kishimoto,  
13 *Isotopes in Environmental and Health Studies*, 2010, 46, 233-241.  
14 40. D. Hippler, A.-D. Schmitt, N. Gussone, A. Heuser, P. Stille, A. Eisenhauer and T. F. Nägler,  
15 *Geostand. Newsl.*, 2003, 27, 13-19.  
16 41. M. Amini, A. Eisenhauer, F. Böhm, C. Holmden, K. Kreissig, F. Hauff and K. P. Jochum,  
17 *Geostand. Geoanal. Res.*, 2009, 33, 231-247.  
18 42. M. Schiller, C. Paton and M. Bizzarro, *Journal of Analytical Atomic Spectrometry*, 2012, 27,  
19 38-49.  
20 43. F. Wombacher, A. Eisenhauer, A. Heuser and S. Weyer, *Journal of Analytical Atomic*  
21 *Spectrometry*, 2009, 24, 627-636.  
22 44. J. Fietzke and A. Eisenhauer, *Geochemistry, Geophysics, Geosystems*, 2006, 7, Q08009.  
23 45. M. S. Fantle, *Geochimica et Cosmochimica Acta*, 2015, 148, 378-401.  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

**Table 1.** Chromatographic steps for the automated separation of Ca and Sr (1mL ESI Sr-Ca Column).

Step	Purpose	Volume	Reagent
1	Condition Column	10 mL	2M HNO <sub>3</sub> + 1% wt. H <sub>2</sub> O <sub>2</sub>
2	Load Sample	1 mL	2M HNO <sub>3</sub>
3	Elute Sample Matrix	10 mL	2M HNO <sub>3</sub> + 1% wt. H <sub>2</sub> O <sub>2</sub>
4	Elute Sr	10 mL	6M HNO <sub>3</sub>
5	Elute Ca	10 mL	12M HNO <sub>3</sub>
6	Elute REEs, Hf, Cd, U	10 mL	1M HF

**Table 2.** Major isobaric and matrix interferences for Ca and Sr isotopes measurements by MC-ICP-MS.

	$^{42}\text{Ca}^+$	$^{43}\text{Ca}^+$	$^{44}\text{Ca}^+$	$^{48}\text{Ca}^+$
C			$^{12}\text{C}^{16}\text{O}_2^+$	
N	$^{14}\text{N}_3^+$		$^{14}\text{N}_2^{16}\text{O}^+$	
K	$^{41}\text{K}^1\text{H}^+$			
Ti				$^{48}\text{Ti}^+$
Sr	$^{84}\text{Sr}^{++}$	$^{86}\text{Sr}^{++}$	$^{88}\text{Sr}^{++}$	
	$^{84}\text{Sr}^+$	$^{86}\text{Sr}^+$	$^{87}\text{Sr}^+$	$^{88}\text{Sr}^+$
Ca	$^{40}\text{Ar}^{44}\text{Ca}^+$	$^{40}\text{Ar}^{46}\text{Ca}^+$	$^{43}\text{Ca}^{44}\text{Ca}^+$	$^{40}\text{Ar}^{48}\text{Ca}^+$
Rb			$^{87}\text{Rb}^+$	
Kr	$^{84}\text{Kr}^+$	$^{86}\text{Kr}^+$		
	BCR-2	CUE-0001	IAPSO	NIST 1400
Matrix	Al, Fe, Mg	Ca, P	Na, Mg, K	Ca, P



**Table 3.** Efficiency of chromatographic separation for BCR-2 (1.9 mg BCR-2, 100 µg Ca).


Sr Ratios	Before Separation	After Separation	Improvement Factor
Sr/Ca	0.007	0.121	16.4
Sr/Rb	7.17	>2237*	>312
Sr/Zr	1.97	1051	535
Ca Ratios			
Ca/K	3.26	1735	533
Ca/Ti	3.63	>18742*	>5170
Ca/Sr	136	129612	955

\*Interference below limit of detection following purification.


**Table 4.** Comparison of measured Ca and Sr isotope data with previously published results.

	Measured	Reported	Ref.
$\delta^{44/42}\text{Ca}_{915a}$ (‰ $\pm 2\sigma$ )			
IAPSO	$0.92 \pm 0.06$	$0.93 \pm 0.07$	30, 33, 40-42
BCR-2	$0.41 \pm 0.07$	$0.47 \pm 0.07$	41-43
NIST 1400	$-0.54 \pm 0.05$		
CUE-0001	$0.83 \pm 0.05$		
$\delta^{88/86}\text{Sr}_{987}$ (‰ $\pm 2\sigma$ )			
IAPSO	$0.36 \pm 0.03$	$0.36 \pm 0.04$	34, 44
BCR-2	$0.22 \pm 0.07$	$0.22 \pm 0.02$	29
NIST 1400	$-0.32 \pm 0.03$		
CUE-0001	$-0.39 \pm 0.04$	$-0.41 \pm 0.05$	34
$^{87}\text{Sr}/^{86}\text{Sr}$ (‰ $\pm 2\sigma$ in the last digits)			
IAPSO	$0.709187 \pm 9$	$0.709182 \pm 4$	29
BCR-2	$0.705038 \pm 9$	$0.705015 \pm 5$	29, 45
NIST-1400	$0.713129 \pm 19$	$0.713150 \pm 160$	20
CUE-0001	$0.704455 \pm 9$		


## Figures:

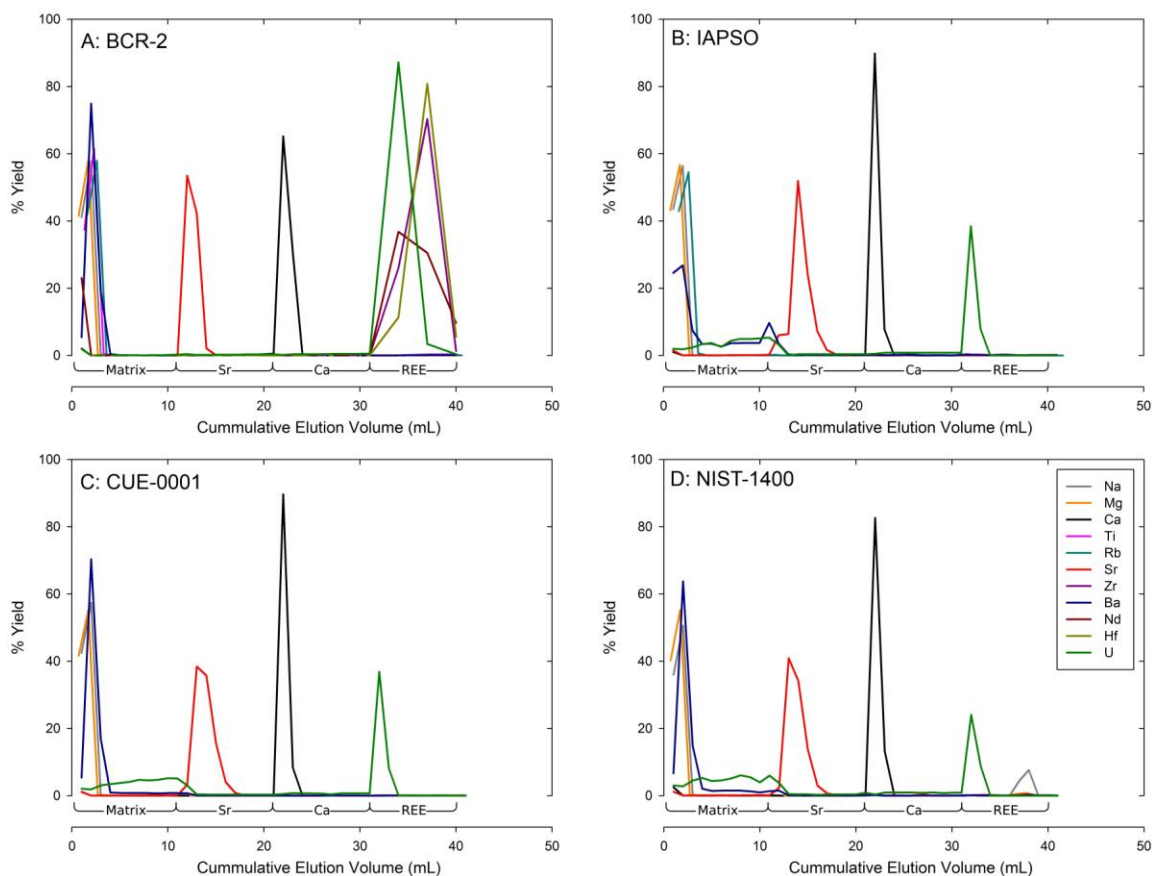


**Figure 1.** Elution profiles for BCR-2 basalt (A), IAPSO seawater (B), CUE-0001 llama bone (C), and NIST-1400 bone ash (D). Elution curves were generated automatically using the prepFAST-MC column calibration mode. Sample sizes for each standard were  $\sim 100 \mu\text{g}$  Ca, corresponding to 1.9 mg BCR-2, 240  $\mu\text{L}$  IAPSO, 0.26 mg NIST-1400, and 0.50 mg of CUE-0001. Sr and Ca are separated from all major matrix components and potential interferences.

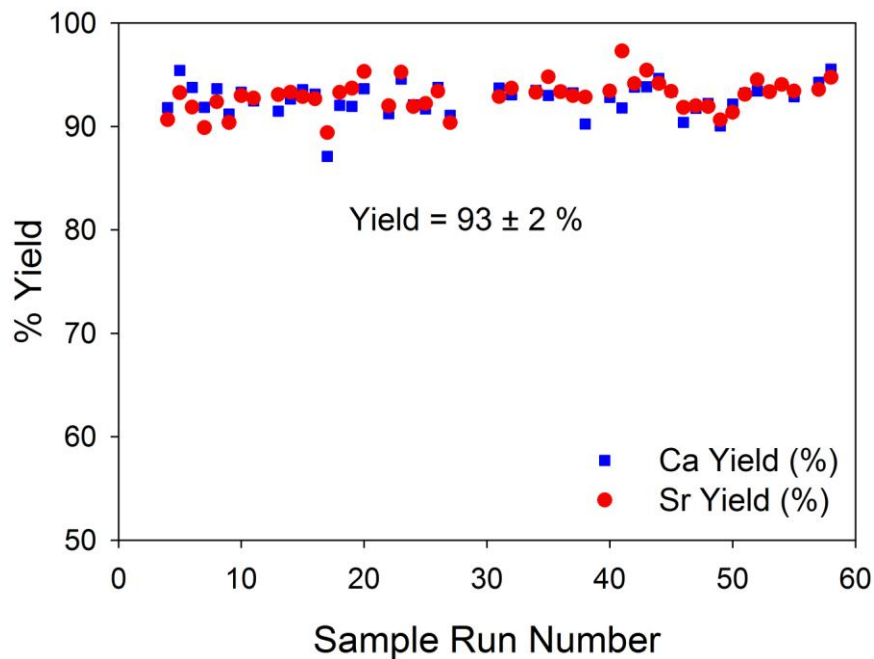

**Figure 2.** Recovery of Ca and Sr collected during a typical sample run consisting of 60 limestone, dolostone, coral, and seawater samples.

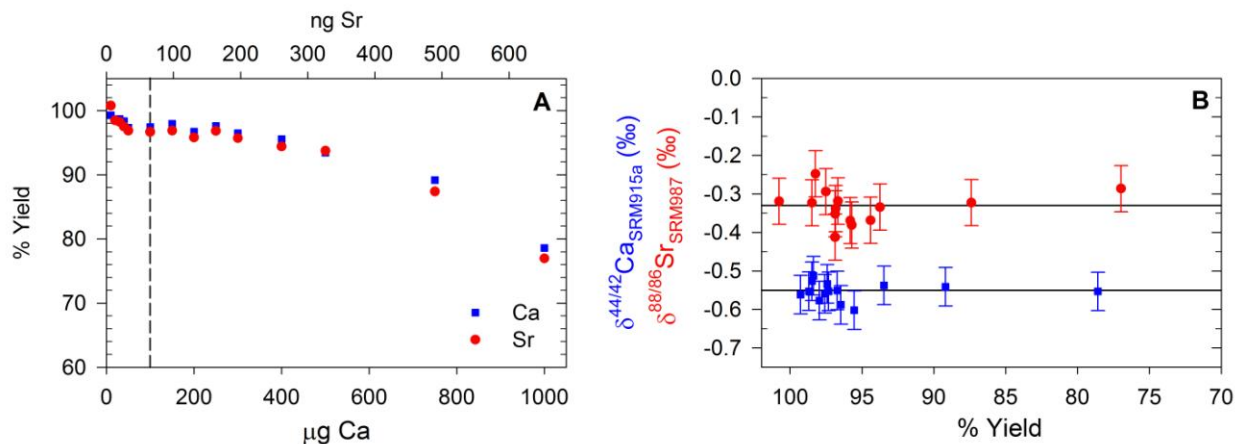

**Figure 3.** (A) Recovery of Ca and Sr from NIST 1400 Bone Ash (Ca/Sr ratio of 1550) plotted as a function of sample mass ( $\mu\text{g Ca}$ ). The recommend sample size ( $\sim 100 \mu\text{g Ca}$ ) is represented by the vertical dashed line. (B) Stable Ca ( $\delta^{44/42}\text{Ca}$ ) and Sr ( $\delta^{88/86}\text{Sr}$ ) isotope composition of NIST 1400 bone ash versus recovery of Ca and Sr, respectively. The data demonstrate no measurable stable isotopic fractionation of Ca and Sr on the column even when the column is intentionally saturated with Ca producing yields as low as 75%.

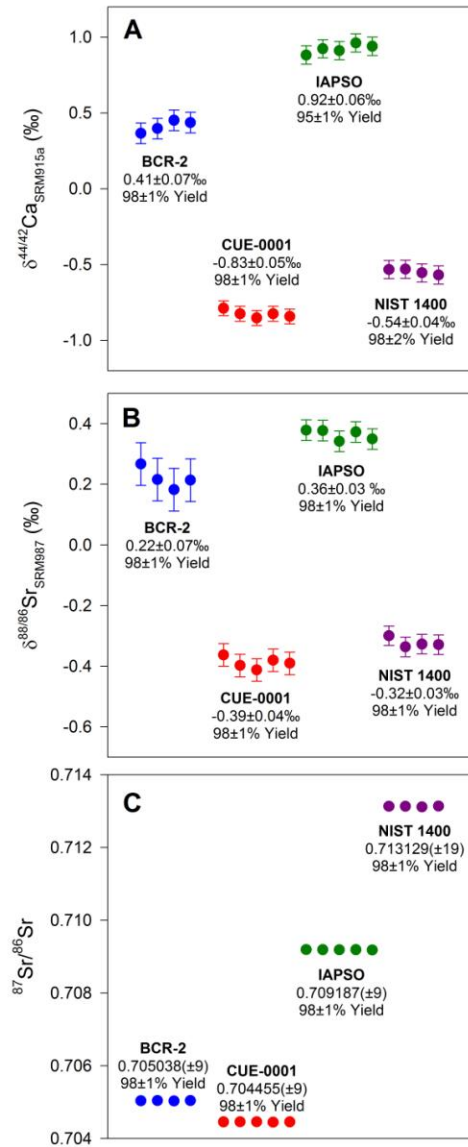

**Figure 4.** Reproducibility of Ca and Sr isotope data for a sequence of randomly ordered analyses containing samples of widely varying isotopic compositions. Agreement between replicates demonstrates low system carryover and a high degree of reproducibility.