

Lab on a Chip

Accepted Manuscript




This is an *Accepted Manuscript*, which has been through the Royal Society of Chemistry peer review process and has been accepted for publication.

Accepted Manuscripts are published online shortly after acceptance, before technical editing, formatting and proof reading. Using this free service, authors can make their results available to the community, in citable form, before we publish the edited article. We will replace this *Accepted Manuscript* with the edited and formatted *Advance Article* as soon as it is available.

You can find more information about *Accepted Manuscripts* in the [Information for Authors](#).

Please note that technical editing may introduce minor changes to the text and/or graphics, which may alter content. The journal's standard [Terms & Conditions](#) and the [Ethical guidelines](#) still apply. In no event shall the Royal Society of Chemistry be held responsible for any errors or omissions in this *Accepted Manuscript* or any consequences arising from the use of any information it contains.

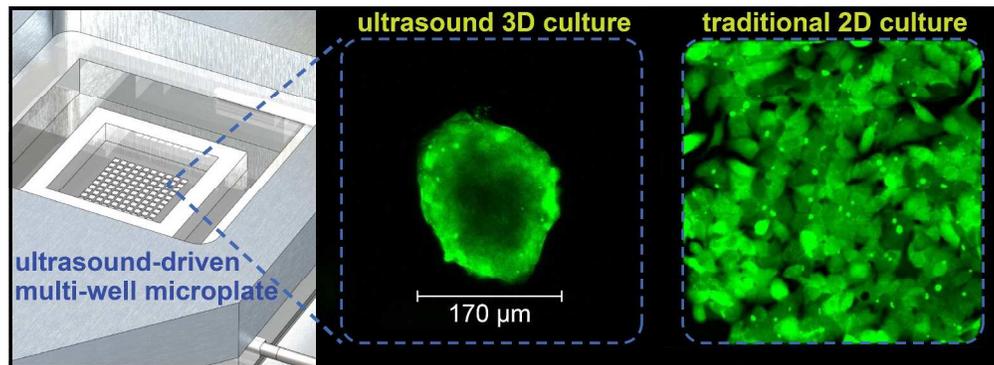

We demonstrate 3D ultrasound cell culture for the formation of solid liver tumors in a multi-well microplate, and we use the method for simulating early stages of tumor development under immune natural killer cell attack.

397x145mm (300 x 300 DPI)

Ultrasonic three-dimensional cell culture on chip for dynamic studies of tumor immune surveillance by natural killer cells

Athanasia E. Christakou^{1*}, Mathias Ohlin^{1*}, Björn Önfelt^{1,2} and Martin Wiklund¹

¹ Dept. of Applied Physics, KTH - Royal Institute of Technology, Stockholm, Sweden.

² Dept. of Microbiology, Tumor and Cell Biology, Karolinska Institute, Stockholm, Sweden

ABSTRACT

We demonstrate a simple method for three-dimensional (3D) cell culture controlled by ultrasonic standing waves in a multi-well microplate. The method gently arranges cells in suspension into a single aggregate in each well of the microplate and by this nucleates 3D tissue-like cell growth for culture times between two and seven days. The microplate device is compatible with both high-resolution optical microscopy, and maintenance in a standard cell incubator. The result is a scaffold- and coating-free method for 3D cell culture that can be used for controlling the cellular architecture, as well as the cellular and molecular composition of the microenvironment in and around the formed cell structures. We demonstrate the parallel production of one hundred synthetic 3D solid tumors comprising up to thousands of human hepatocellular carcinoma (HCC) HepG2 cells, we characterize the tumor structure by high-resolution optical microscopy, and we monitor the functional behavior of natural killer (NK) cells migrating, docking and interacting with the tumor model during culture. Our results show that the method can be used for determining the collective ability of a given number of NK cells to defeat a solid tumor having a certain size, shape and composition. The ultrasound-based method itself is generic and can meet any demand from applications where it is advantageous to follow the cell culture from production to analysis of 3D tissue or tumor models by the use of microscopy in one single microplate device.

* Contributed equally.

Contact:

Martin Wiklund (martin.wiklund@biox.kth.se)

Björn Önfelt (bjorn.onfelt@scilifelab.se)

INTRODUCTION

In cellular research, there is a need for improved *in vitro* model systems mimicking the complex *in vivo* microenvironment of living tissue. Cells within tissue interact with other cells, the extracellular matrix (ECM) and other soluble factors in a 3D communication network that is crucial for the tissue development, function and survival^{1, 2}. For this reason, the traditional 2D culture that has been used for long is insufficient and its experimental outcome can sometimes be of limited relevance. This is of great importance for pharmaceutical companies who need appropriate cell-based assays to evaluate drugs in early stages of development³. In tumor biology it is increasingly recognized that the heterogeneous composition of tumors with mixtures of cell types spatially arranged in 3D creates microenvironment that affect tumor aggressiveness, gene expression and resistance to drug treatments⁴⁻⁷.

The tumor microenvironment can also shape the immune response, which is exemplified by the commonly observed phenomena that NK cells, a type of cytotoxic lymphocyte important for the body's defense against cancer and virus infections, isolated from explanted tumors often display an exhausted, inactive phenotype⁸. This is in stark contrast to the cytotoxic activity often observed by NK cells when interacting with tumor cells *in vitro*, even if the target cells originate from solid tumors^{9, 10}. Recent studies have shown that both human cervical carcinoma cells and Ewing's sarcoma family tumor cells were more resistant to NK-mediated lysis when grown in 3D spheroids compared to monolayer^{11, 12}. NK cell infiltration in tumors have been associated with better prognosis in lung, gastric and colorectal carcinoma, suggesting a potential future role for NK cells in cell therapy against solid tumors^{13, 14}. However, more relevant model systems where the tumor microenvironment and architecture can be controlled are needed to better understand how NK cells interact with solid tumors.

Several techniques for 3D cultures have been developed and optimized over the last decades. Today there are several commercially available tools for multicellular 3D cultures for applications in biology and medicine¹⁵. Most of these methods are based on assembling the cells in a 3D structure by a supporting physical scaffold around the cells using, for example, proteins and hydrogels¹⁶. Limitations of such scaffold-based systems include the difficulty for the cell culture to interact with its environment due to the inert and/or non-transparent scaffold. It is also possible to obtain 3D cell cultures by the use of different cell adhesion resistant surface coatings such as agarose and poly-HEMA¹⁷. For example, coatings may be applied in microstructure patterns or combined with conical-bottom plates¹⁸. An alternative to scaffold- and coating-based methods for 3D cell culture is to use self-assembly of cells assisted by an external force field. The most commonly used method here is the "hanging drop" where cells assemble into spheroids by gravity in drops within an upside-down oriented microplate¹⁹. This method is limited by the difficulty to keep the drops stable over extended culture times, in particular to prevent evaporation which adds some complexity to the otherwise simple principle. Another reported method uses magnetic levitation of a hydrogel composed of cells, magnetic iron oxide, gold nanoparticles, and bacteriophage²⁰.

In this paper, we demonstrate a novel 3D cell culture method based on ultrasonic standing waves (USWs). USWs have long been used for the purpose of trapping, concentrating or separation of particles and cells, in particular in microfluidic systems²¹. We have previously developed a device based on this method for the controlled manipulation of individual cells in a multi-well microplate²², and we have used the method for studying the interaction between individual NK cells and individual leukemia cells^{23, 24}. We have also in several studies demonstrated that continuous ultrasound exposure at MHz-frequencies and a few hundred kPa acoustic pressure amplitudes is not compromising viability or function of cells over time periods up to at least one week^{22, 25-27}. In the present paper, we have combined these findings in order to develop a new and simple method for producing synthetic 3D solid tumors of human hepatocellular carcinoma (HCC) HepG2 cells. HCC is the most common malignancy of the liver and the one of the most common and aggressive human cancers worldwide. HCC is an inflammation related cancer as the initiation and development of liver tumors appears to be caused by chronic inflammations deriving from infections with hepatitis viruses, alcohol and drug abuse, toxins and metabolic or hereditary disorders^{28, 29}. HepG2 was selected in this study since it is a widely used and well-characterized liver tumor cell model which is also susceptible to NK cell-mediated lysis³⁰. In addition, recent studies suggest that immunotherapy with cytokine-activated NK cells increased recurrence-free and overall survival of HCC patients³¹. We characterize the dimension (from 2D to 3D) and compactness of the tumor models, and we use the method for monitoring the docking and infiltration of NK cells towards, onto and into the tumors. Furthermore, we monitor the rate of NK cell-mediated lysis of tumor cells, relative the rate of tumor growth and could thereby determine the number of NK cells needed for defeating tumors of different sizes and morphologies. The method is integrated with live-cell confocal microscopy for time-lapse high-resolution imaging of the 3D structure of the solid tumor, as well as for tracking the interaction behavior between individual NK cells and the tumors. The methodology presented is a novel, simple and generic assay for 3D cell culture, seamlessly combining tumor/tissue production with tumor/tissue analysis. It allows constructing more complex tumor models consisting of different cell types, architectures, and with more accurately modelled microenvironment including extracellular matrix and soluble factors.

MATERIAL AND METHODS

Preparation and culture of peripheral blood NK cells. Polyclonal primary human NK cells were isolated by negative selection from lymphocyte-enriched buffy coat residues derived from anonymous healthy donors as previously described²³. Briefly, peripheral blood mononuclear cells (PBMCs) were isolated from buffy coat by centrifugation on Ficoll-Paque Plus according to the manufacturer's instructions (GE Healthcare). NK cells isolation was performed by negative immuno-magnetic bead isolation (EasySep® Human NK Cell Enrichment Kit, Stem Cell Technologies) according to the manufacturer's instructions. Primary human NK cells were cultured for 7 – 14 days before used in experiments in Iscove's modified Dulbecco's medium (IMDM, I3390, Sigma-Aldrich, St. Louis, MO, USA), supplemented with 10%

autologous human serum, 2 mM L-glutamine(G7513 Sigma-Aldrich, St. Louis, MO, USA), 100 U/ml Penicillin-100 µg/ml Streptomycin (P4333; Sigma Aldrich, St. Louis MO, USA), 1× non-essential amino acids (M7145, Sigma-Aldrich, St. Louis, MO, USA), 1 mM sodium pyruvate (S8636, Sigma-Aldrich, St. Louis, MO, USA) and 200 U/ml human interleukin (IL)-2 (PeproTech, Rocky Hill, NJ, USA).

Cell lines. HepG2 cells were cultured in RPMI-1640 (SH30027 Thermo Scientific, MA, USA) supplemented with 10% fetal bovine serum, and 100 U/ml penicillin-100 µg/ml streptomycin, 1× non-essential amino acids, 1 mM sodium pyruvate, 2mM L-glutamine and maintained, at 37° C, 5% CO₂.

Cell seeding and labeling. Cell suspension of HepG2 cells was added by pipetting to the microplate primed with cell medium, and the cells were settled to the bottom of the wells by gravity resulting in a stochastic distribution with an average number of cells per well controlled by the total number of added cells. The number of seeded HepG2 cells into the microplate was either 7000 or 20000 (the lower number was used for the NK cell experiments), and the number of seeded NK cells ranged from 5000 to 10000. Typically, 70% of the seeded cells settled into the wells of the microplate. HepG2 tumors were labeled in the chip with the viability probe calcein green AM and with far-red DDAO-SE, while NK cells were stained with calcein red-orange AM (all from Invitrogen, Carlsbad, CA, USA) as described previously²³. After seeding and on-chip culturing, the growth medium was removed gently and cells were washed four times (with RPMI-1640), and a pre-heated (37 °C) solution of calcein green AM (0.25 µM) and far-red DDAO-SE (1 µM) was added to the microplate under gentle mixing. The chip was placed in the incubator for 30 minutes and the dye solution was removed by washing twice with RPMI-1640 after which cell culture medium was added.

Multi-well microplate and ultrasound transducer. The device for ultrasonic cell manipulation, illustrated in Fig. 1, consists of a multi-well microplate and a ring-shaped ultrasonic transducer which is described in detail in Refs.^{22, 32}. In brief, the microplate consists of an array of 10×10 wells etched in the center of a silicon layer bonded to a coverslip-thickness glass layer forming a sandwiched-type of a microplate measuring 22×22×0.475 mm³. The wells, with either straight or slightly rounded walls, are 350×350 µm² in cross-section and 300 µm deep. A polydimethylsiloxane (PDMS) frame is bonded to the top layer, i.e. the silicon surface, around the wells to increase the sample volume capacity (thus providing a pool of approx. 50 µl cell medium above the wells). Furthermore, to minimize evaporation a cover glass is placed on top of the PDMS frame. This cover glass can easily be removed for adding or removing liquid from the microplate. The transducer consisted of a ring-shaped piezoceramic plate (Pz-26, Ferroperm, Denmark) with dimensions 38 mm (outer diam.) and 0.86 mm (thickness) and with an 8 mm center hole for visual access from the microscope. When assembling the piezoceramic plate into the microdevice shown in Fig. 1, the transducer became broadbanded with suitable driving frequencies in the range 1.9-2.5 MHz.

Temperature control system and cell incubator. The microplate device was integrated into a small tabletop cell incubator, allowing control of the environmental

conditions (temperature, CO₂ and humidity), while being operated by ultrasound continuously for up to 7 days. To maintain a physiological temperature independent of the ultrasound actuation voltage, the temperature in the microplate was regulated using an in-house built temperature control system consisting of a PID (KT4, Panasonic, Japan) controlled liquid heat exchanger capable of both cooling and heating. This was achieved by varying the temperature of a water block clamped to the microdevice and integrated into the table-top cell incubator, with feedback from the temperature measured by two type-T thermocouple micro probes attached to the microplate (Fig. S1).

Ultrasound cell culture. The ultrasound transducer was actuated by a signal generator and RF amplifier. We used a frequency modulation method as described previously³³, for achieving a robust and uniform two-dimensional (2D) acoustic force field in each well in the microplate. This actuation method resulted in driving seeded cells by acoustic radiation forces into the pressure nodes of standing waves located in the center of each well, where they were trapped and aggregated. Thus, each well acts as a 2D half-wave resonator producing a single trapping position. With the frequency-modulation method we were able to decouple any mutual resonance interferences (causing spurious or unsymmetrical modes) between different wells in the 100-well microplate. For the microplates used in this work, the selected center frequencies were 1.96 MHz for the straight-wall wells, and 2.46 MHz for the wells with slightly rounded walls (depending on the resonance frequency of each plate design), and the frequency was cycled linearly in 50 and 100 kHz wide bands around the center frequency, respectively, at the rate of 1 kHz. Actuation voltages ranged from 60-110 V_{pp} measured with a 10× attenuator probe. HepG2 cells were seeded into the microplate according to the method described in Ref.²⁴. Cell aggregation and positioning in each well was monitored by microscopy during the initial (approx. 5 min) phase of transducer actuation. The device was then moved to the cell incubator and clamped to the water block for temperature control. During the relocation of the device, ultrasound was temporarily turned off. When the device was reactivated, the ultrasound cell culture was operated continuously for time periods varying from 15 min up to as long as 7 days. For long culture times (more than 3 days), short breaks were performed for medium exchange. Passive cell incubation (ultrasound OFF) was implemented in some experiments for investigating the continuing growth of the formed tumors without the effect of ultrasound.

Microscopy. Images were acquired with two different microscope systems: an inverted laser scanning confocal microscope (LCSM, Zeiss LSM 5 Pascal) equipped with a motorized stage, and an inverted bright-field microscope (Axiovert 40 CFL, Zeiss, Germany) equipped with a DSLR camera (Sony α77, Sony, Japan) and objective (Epiplan 5×/0.13, Zeiss, Germany). High resolution 3D confocal imaging of individual tumors was performed using a 40×/1.3 oil objective and pinhole adjusted according to the fluorescence signal in order to acquire the optimal image. Fluorescence imaging of the entire chip was performed with a 10×/0.3 objective using the moving stage to form a 4×4 tile scan. When time-lapse imaging was performed, the 4×4 tile scan was repeated every 20-30 minutes.

Image analysis. ImageJ and MATLAB were used for image analysis and 3D reconstruction. The normalized tumor volume was estimated by multiplying the measured area in the images with the average of the inverted grey scale value within that area (the latter being a rough measure of the height of the tumor based on the bright-field images). As a comparison, the average tumor volume corresponded to a tumor having a bottom area of $43000 \mu\text{m}^2$ and a height of approx. $150 \mu\text{m}$. Such an aggregate contains about 2200 HepG2 cells (estimated by counting the cells in the small 3D structure in Fig. 2E-F, assuming the same shape (category I), and scaled with the tumor volume in Fig. 6). The number of NK cells in each tumor was estimated by the initial fluorescence intensity within the marked boundary of the tumor with the mean intensity of individual NK cells (determined from individual measurements of $n=30$ NK cells). The calcein-AM penetration depth was calculated by implementing a method based on offsetting the boundary of the aggregate, hence dividing each aggregate into several surface segments, from the outer boundary towards the center. Target cell death was scored by visual inspection of the calcein-AM fluorescence (decreases upon cell death) and far-red DDAO-SE fluorescence (increases upon cell death) from target cells in conjunction with morphological features (e.g. cell blebbing) in the bright-field image.

Statistical analysis. Kruskal-Wallis test was used to evaluate overall statistical differences between groups in experiments. To indicate pairwise differences between groups the Mann Whitney U test was used. Stars were used to indicate statistical significance according to: ns ($p>0.05$); * ($0.01<p\leq 0.05$); ** ($0.001<p\leq 0.01$); *** ($0.001<p\leq 0.0001$); **** ($p> 0.0001$).

RESULTS

Temperature control of the ultrasound cell culture device. The multi-well microplate device^{22, 32} used for ultrasonic cell culture is illustrated in Fig. 1. The device was operated with frequency-modulated actuation, which eliminates the need for frequency calibration and resonance tracking. This actuation method requires broadband (low quality factor) ultrasound technology, which is known to generate more heat than single-frequency (high quality factor) technology, and therefore we incorporated a custom-built regulator controlling the temperature of the microplate independently of the surrounding temperature (cf. Fig. S1). To investigate whether our device was compatible with long-term cell culture, the device was placed in a tabletop cell incubator, and the temperature in the microplate was monitored with and without the external temperature control system during continuous ultrasound exposure for up to 63 hours. The external control system can regulate the temperature within less than $\pm 0.3 \text{ }^\circ\text{C}$, independently on both the ultrasound power delivered to the device, as well as the preferred setpoint temperature (cf. Fig. S2), which is better than needed for most cell culture applications²⁷. Thus, frequency modulated ultrasonic cell manipulation combined with temperature control is robust allowing long-term cell studies.

Ultrasound 3D culture of HepG2-based tumor models. A demonstration of ultrasound 3D cell culture is shown in Fig. 2, where the result of a seven days active culture (ultrasound ON, Fig. 2A) is compared with a seven days passive culture (ultrasound OFF, Fig. 2B). The cells formed compact 3D “tumors” in the active culture (Fig. 2C) while they spread out in 2D monolayers on the glass surface in the passive culture (Fig. 2D). Here, a “tumor” means a compact tissue-like 3D cluster of HepG2 cells with tight intercellular junctions, in contrast to the initially trapped cell aggregate of loosely bound cells. In these tumors, we note that the green viability probe (calcein-AM) could not penetrate far into the tumor core (Fig. 2C), due to the tight junctions between cells formed in the active culture (clearly seen in Fig. 2E). The width (Fig. 2E, top view) and height (Fig. 2F, side view) of the tumors were assessed by 3D confocal microscopy. In addition to fluorescence imaging the tumor models display a characteristic morphology in both bright field and dark field imaging due to the distinctive cell boundary surrounding the tumors (cf. Fig. S3). This typical morphology is in agreement with HepG2 spheroid structures reported in other 3D cell culture studies^{34, 35}. Another typical feature of the active culture is the flat bottom facing the glass layer, forming “hemi-spheroid” 3D structures adhered to the bottom in contrast to the spheroid structures formed by 3D cell culture methods based on preventing the cells to adhere to any substrate⁵. This feature of our method is advantageous since the tumors are not accidentally removed when exchanging the medium.

Characterization of compactness, shape and size of ultrasound-cultured tumor models. As an indicator of hemi-spheroid formation and compactness of 3D tumor models with tight intercellular junctions, we compared manual classification of the formed tumors from Fig. 2A with a quantification of the fluorescence intensity from calcein-AM at different horizontal depths relative the outer boundary of the tumors (cf. Fig. 3). Here, 99 tumors from one experiment were manually sorted into two different categories, I (89%) and II (10%), according to their appearance in bright field microscopy imaging (cf. Fig. 4): Category I = dominating 3D structure (i.e., the majority of the apparent area of the tumor in the image is a compact 3D hemi-spheroid) and category II = dominating 2D structure (i.e., the majority of the apparent area of the tumor in the image is a 2D monolayer). The average cross-section area of the category I hemi-spheroids was $2.9 \pm 0.5 \times 10^4 \mu\text{m}^2$, corresponding to circles with diameters $200 \pm 20 \mu\text{m}$. Based on manual counting of the cells in Fig. 2E-F, this corresponds to (category-I) 3D solid tumors containing on average 1400 HepG2 cells. We also measured the change in size of the tumors during growth in the active ultrasound culture. For this purpose, we compared the average size of the tumors shown in Fig. 2A after two days of active culture (data not shown) with the size after seven days of active culture (cf. Fig. 2A). For category-I and category-II tumors the average tumor area in the images increased by $49 \pm 17\%$ and $53 \pm 12\%$, respectively, during five days of culture (i.e. from day 2 to 7 in the active culture).

Tumor classification after different time periods of active and passive culture. For the tumors shown in Fig. 2, we operated the active ultrasound culture for 7 days. However, we examined the outcome for a range of ultrasound exposure times, from short exposure (15 min) up to 7 days (see Fig. 4). Here, tumors from nine different

experiments are sorted into three different categories (I-III) based on the same manual classification as in previous section. In addition to categories I-II (dominating 3D and 2D tumors), category III represents fragmented cell cultures in the well, i.e., insufficient ultrasonic cell trapping. For category I (tumors with dominating 3D structures), we get on average $85\pm 5\%$ for any active culture time between 2 and 7 days (the group “only active culture” in Fig. 4B). We also studied if the successfully formed 3D structures were retained when switching from active (ultrasound ON) to passive (ultrasound OFF) culture after 2-3 days of initial active culture (the group “active+passive culture” in Fig. 4B). Here, the corresponding percentage of category-I tumors was $78\pm 16\%$. The slightly lower success rate can be explained by a small transformation from category I (more 3D-type) into II (more 2D-type) when cells spread on the bottom glass substrate of the microplate without the supporting acoustic forces. However, most 3D structures were retained and continued growing during several days without losing their shape. Finally, we also examined shorter culture times (15 min and 4 hours), resulting in 16% and 31% of category-I tumors (last group in Fig. 4B). Thus, our data indicates that an active culture time of 2 days or more is suitable in order to produce a great majority of useful 3D tumors of HepG2 cells, and a great majority of these 3D tumors are retained even after switching to passive culture.

NK cell migration, docking to tumors and lysis of tumor cells. After establishing a protocol for forming HepG2 tumors we exposed them to NK cells to follow the different stages of immune surveillance. In all the following NK cell experiments, we did not use an active ultrasound culture. Instead, human IL-2 activated NK cells were seeded into wells in microplates and allowed to spontaneously migrate and interact with the ultrasound-formed tumors. In the early stages when NK cells docked onto the tumors, they often stretched out and migrated across the tumor surface (cf. Fig. 5A). Immediately after seeding only a few NK cells had docked onto the tumors while at $t = 28$ h almost all NK cells were on, or inside the tumor (cf. Fig. 5B). Z-scans from the initial phases of the interaction revealed that NK cells were mainly situated at the tumor periphery, although we also observed some NK cells that infiltrated the tumor mass (cf. Movie S1). Time-lapse movies confirmed this observation as NK cells moved across the tumor surface, at the tumor-glass interface under the tumor and also inside the tumors (Movie S2). To monitor target cell death we used the fluorescence signals from calcein-AM (leaks out) and far-red DDAO-SE (increases), as well as visual signs in the bright-field images. Consistent with previous results³⁰ NK-mediated lysis started immediately after addition of the NK cells and within a few hours signs of tumor cells death were evident mainly at the periphery of the tumor (Figs. S4 and S5).

Time-lapse studies of NK-cell mediated tumor defeat. In the next set of experiment we acquired time-lapse sequences of all wells of the microplate in parallel allowing us to quantify the battle between tumor growth and NK-mediated lysis. We examined both the initial phase (first day) of either decrease or increase of apparent tumor size, as well as the final outcome of either defeated or living tumor (after up to five days).

From bright-field microscopy images, each initial tumor area was manually marked (see white boundary in Fig. 6A), and we then assessed if the tumor shrunk by tumor

cells being lysed inside the boundary (Fig. 6A, upper panel), if they remained constant (Fig. 6A, middle panel), or if they grew outside this boundary (Fig. 6A, lower panel) during the initial 16 hours of NK cell – tumor interactions. Based on fluorescence and bright-field images we estimated the tumor volumes, giving a rough estimate of the number of HepG2 cells per tumor (approx. 2200), and the number of NK cells interacting with each tumor. Plotting the estimated number of NK cells per average category-I tumor volume for the three outcomes (decreased, constant or increased tumor size) suggested that the number of NK cells per tumor volume had an immediate impact on the development of the tumor (Fig 6B). The cutoff value between causing a decrease or an increase in tumor size (i.e. for suppressing tumor growth) was on average around 50 NK cells per ~0.2-mm-diameter sized HepG2 tumor (mean value of the middle bar in Fig. 6B). This corresponds to a ratio between NK cells and HepG2 cell of roughly 1:40.

In a second experiment, the monitoring time was increased to track the full process from initial tumor decrease or increase until final tumor outcome. After 124 hours some tumors were completely defeated (Figs. 7A-B, Movie S3) while others were viable and continued to grow (Fig. 7C-D). In this experiment, the average cutoff value for suppressing initial tumor growth (after 22 hours) was around 40 NK cells per average tumor volume (middle bar in Fig. 7E). Here, note that new calcein green AM was added to the microplate at times 51 hours (cf. Fig. S6) and 124 hours, resulting in that both NK cells and viable HepG2 cells appear in the same color at these time points in the presented sequence. The full process, including both the initial first day (22 hours) and the final fifth day (124 hours) is quantified in Fig. 7E-F. Here, we used the same quantification method for estimating the tumor volume as in the first experiment (cf. Fig. 6), however NK cell estimation was performed manually without taking into account NK cell fluorescence intensity. As the average tumor volume was smaller, corresponding to approx. 700 HepG2 cells, in these experiments, this corresponds to a ratio between NK cells and HepG2 cells of about 1:20.

After additional four days of continued NK cell – tumor culture, we were able to score whether the tumor had been completely defeated or if parts of the tumor was still viable, see Fig. 7F. Here, we note that on average 20 NK cells per tumor were present in the wells where the tumor had survived.

DISCUSSION AND CONCLUSION

We have demonstrated a novel method for 3D cell culture based on ultrasonic standing waves in a multi-well microplate. The method is designed for producing small (~0.2 mm-sized) 3D solid tumors or tissue structures in parallel without the need for any supporting scaffold or surface coating. Our results can be compared with a previous study where HepG2 spheroids were formed after initial aggregation of cells by ultrasound for 5 min, followed by inserting the aggregate in a gel-based passive culture^{36, 37}. Our method is gel-free, and thus requires longer active culture times than 4 hours for producing stable 3D structures. On the other hand, the active culture time can

also be used as a steering parameter for choosing different solid tumor shapes (short time for more 2D shapes and long time for more 3D shapes).

The ultrasound is coupled into the microplate by a broadband transducer operating in a frequency-modulated mode, without the need for any calibration or resonance control during long-term operation. This is accomplished by a temperature-controlled water block connected to the microplate and placed inside a table-top cell incubator. In this way, both the temperature of the microplate device, as well as of the surrounding air is carefully controlled, and can be kept constant at any preferred relevant temperature independently on the ultrasound power delivered to the device, something that is more difficult to realize with single frequency ultrasound technology. The microplate device is compatible with high-resolution optical microscopy, offering a method for combined 3D cell culture and cell characterization.

Here the method was used for culturing 3D solid HepG2 tumor models, followed by studying the interaction between small populations (approx. 10-100) of primary human NK cells and the HepG2 tumors. We found that a large majority (85%) of the produced solid tumors were 3D hemi-spheroids and we outlined a routine for classification based on their shape and compactness. NK cells were observed to interact with the tumors, primarily by adhering and migrating across their surface but also by infiltrating into the tumor mass. In consistence, target cell death was primarily observed at the tumor periphery suggesting that NK cells attack the tumors from the outside-and-in rather than the opposite. Furthermore, we demonstrate how the method could be used for determining the average number of NK cells needed for initial suppression of tumor growth or completely defeating a tumor the following days of culture. For the experimental conditions used in this work, we observed that a ratio between NK cells and HepG2 cells in the range 1:20 - 1:40 was needed to prevent tumor growth in the first day, while a ratio of approx. 1:10 was needed to destroy the tumor in five days. These results are average values, when studying individual tumors the standard deviations were large. Still, statistical analysis confirms that the observed trends of increasing number of NK cells observed for shrinking or defeating tumors, relative the numbers observed for growing tumors are significant (cf. Fig. 6B and 7B), with the only exception of the threshold between constant and growing size in Fig. 6B.

Although a simple cell model was used in this initial work, the method allows production of more complex tumor models, including several cell types, extracellular matrix and different relevant soluble factors. One important advantage with the ultrasound cell culture method is the possibility to vary between ordered and chaotic structure of the building blocks in the tumor model and its microenvironment. This can be achieved by, e.g., changing between adding the components into the microplate one by one, or in a mixture. In future, we believe that the method will be useful for applications where it is of interest to create sophisticated in vitro models of tissue or solid tumors, with the additional functionality of real-time and detailed optical monitoring of individual multi-cellular structures.

ACKNOWLEDGEMENTS

We thank the Swedish Research Council, the Swedish Foundation for Strategic Research and Stockholms Läns Landsting for financial support.

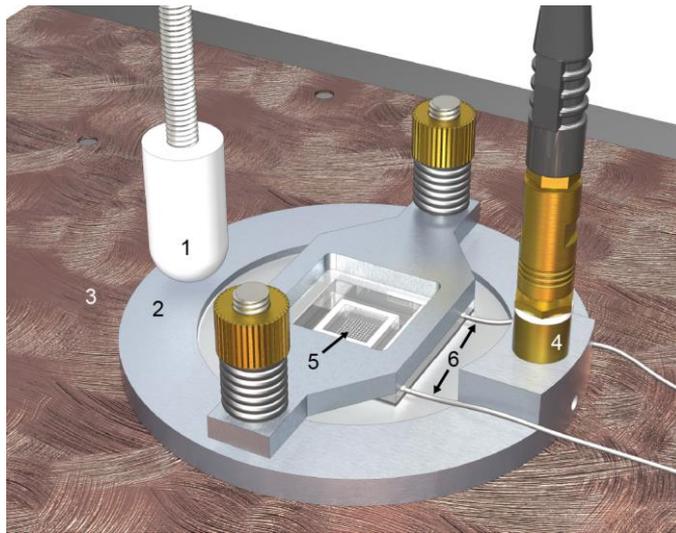


Figure 1: The micro-device for 3D ultrasound cell culture: Clamp (1) to ensure good contact between the multi-well micro-device (2) and the water block (3), which is connected to the temperature control system via a liquid-loop. The ultrasound is delivered using a SMB connector (4). The temperature on the multi-well microplate (5) is monitored using two thermocouple probes (6) placed next to the wells. One probe is connected to the temperature control system's PID unit for feedback and the other probe is connected to a data logger for monitoring. The diameter of the micro-device (2) is 58 mm.

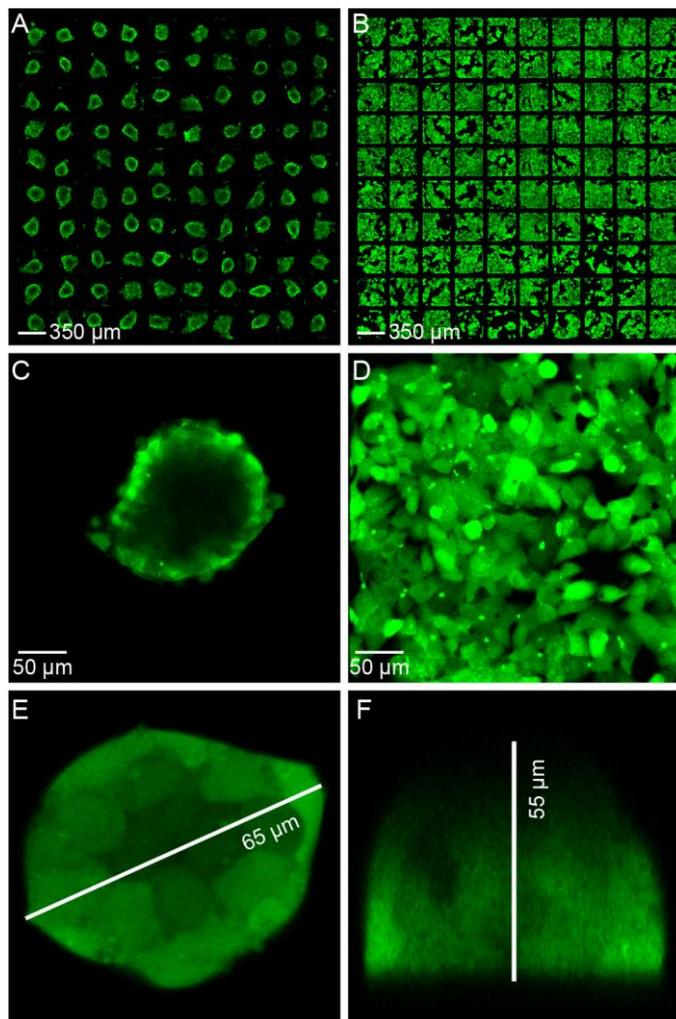


Figure 2: Calcein green AM-stained HepG2 cells in active and passive culture. (A) Result after 7 days of continuous ultrasound exposure (active culture). (B) Control experiment, 7 days incubation without ultrasound exposure (passive culture). (C) A magnified image showing one of the wells from the active culture. (D) Equivalent magnified image from the passive culture. (E) Horizontal cross-section image from a 3D confocal microscopy scan of a small 3D tumor. (F) Vertical cross-section image from the same 3D confocal microscopy scan.

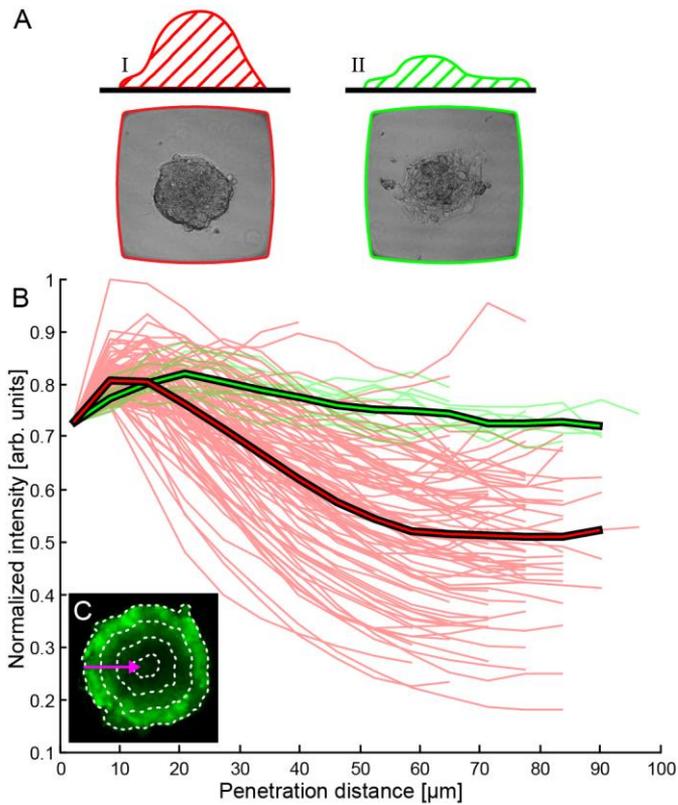


Figure 3: Characterization of compactness and shape of the HepG2 tumors in Fig. 2A. (A): Manual classification of the formed tumors into two different categories with sketch and photo examples (width of each photo is $350\ \mu\text{m}$ = width of the wells): Category I (dominating 3D structure, red curves in (B)) and II (dominating 2D structure, green curves in (B)). (B): Fluorescence intensity versus penetration depth of the viability probe calcein-AM. The penetration depth is measured from the surface towards the center of the tumor in the horizontal cross section. The bold colored curves in the diagram show the respective average values for the two categories. (C) Example of the step-wise layer-by-layer segmentation algorithm, here a segment is the area between two dotted lines. For each segment the average intensity is calculated and plotted as a function of penetration depth.

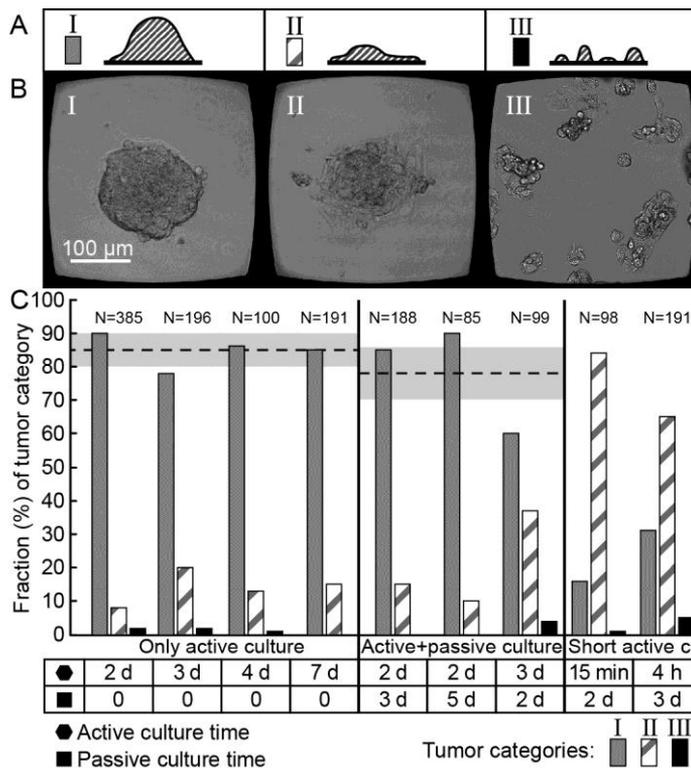


Figure 4: Tumor classification after different times of active (ultrasound ON) and passive (ultrasound OFF) culture. Side-view sketches (A) and bright field images (B) of the three different tumor categories I-III. Here, categories I-II (dominating 3D and 2D structure, respectively) are the same as in Fig. 3, while category III represents a non-aggregated structure, associated with failed ultrasound trapping. (C): Tumors from nine different experiments with various times of active and passive culture were classified into the three different categories, I-III. Here, ‘d’ stand for days, ‘h’ for hours, and ‘N’ for number of assessed wells. The dotted lines and light gray zones are the mean and standard deviation of the fractions of category-I tumors (dominating 3D) for each actuation group (only active, and active+passive culture, respectively) where we used at least two days of active culturing time.

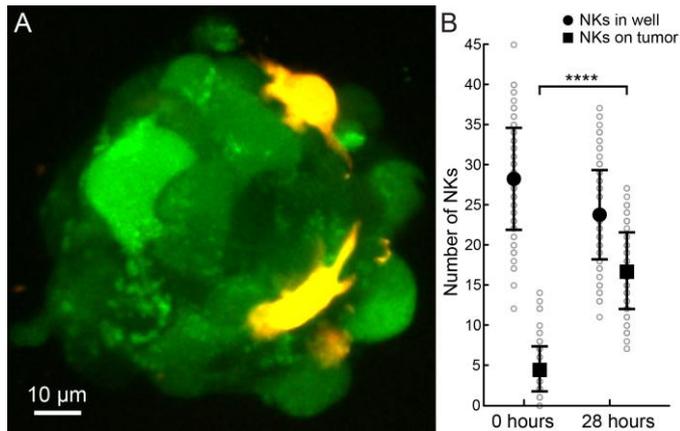


Figure 5: NK cell docking to HepG2 tumors. (A) High-resolution confocal 3D image of a solid tumor (stained with calcein green AM) and two NK cells (stained with calcein red-orange AM). (B) Quantification of the total number of NK cells per well in 90 wells versus the number of NK cells docked to the tumor in each well at 0 hours and 28 hours after NK cells were settled in the chip. Statistical significance was calculated by the Mann-Whitney U test based on the fractions of NKs on tumor/NKs in well and indicated by stars ($P < 0.0001$).

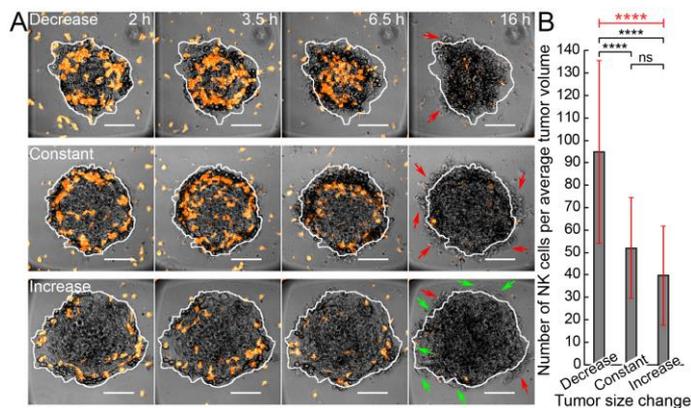


Figure 6: Development of HepG2 tumors under NK cell aggression. (A) Time-lapse sequences of NK cells (stained with calcein red-orange AM) interacting with three different tumors (bright field). In the first panel (“Decrease”), the apparent tumor area decreases due to NK induced lysis from 99 NK cells interacting with the tumor. In the second panel (“Constant”), the apparent area of the tumor remains unchanged due to 72 NK cells interacting with the tumor, indicating NK induced lysis is balanced with cancer cell division. Red arrows point at dead cancer cells detached from the tumor and drop outside the marked area. In the last panel (“Increase”), 28 of NK cells interact with the tumor; here cancer cells grow in monolayers outside the marked area (green arrows). Note that the lack of orange NK cells in the last column is due to calcein being incompatible with long incubation times. (B) Quantification of the number of NK cells interacting with each category-I (3D) tumor divided by the average tumor volume, as a function of the tumor size change (decreased, constant of increased tumor size) over 16 hours assay. All scale bars correspond to 70 μm . Red horizontal bar and stars indicate the overall significance of all three sets of data tested by the Kruskal-Wallis test and black horizontal bars and stars indicate the statistical significance of the data when analysed pairwise by the Mann-Whitney U test. ‘ns’ indicates ‘not significant’.

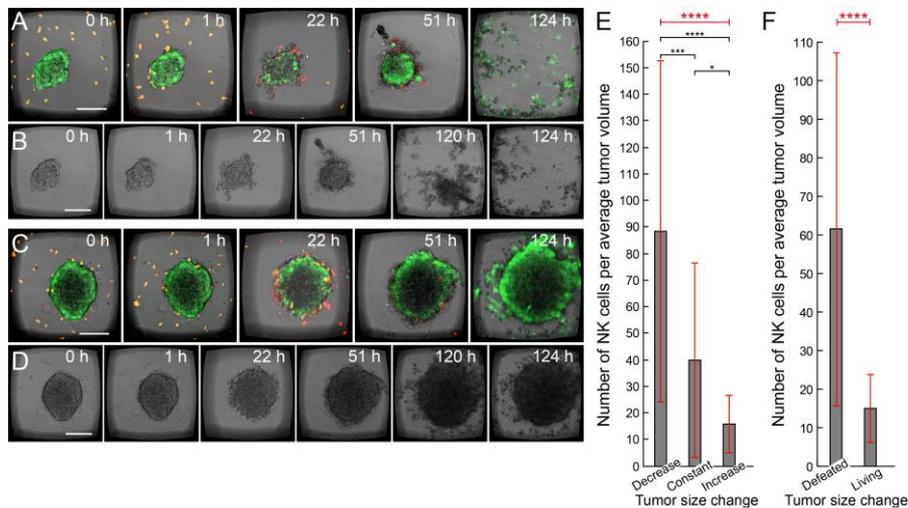


Figure 7: Image sequence of NK cells interacting with solid HepG2 tumors over a 124 hour time period. Fluorescence (A) and bright field (B) images of NK cells shown in orange (calcein red-orange AM) and tumor shown in green (calcein green AM for live cancer cells) and red (far-red DDAO-SE for dead cancer cells). At $t = 0$ h very few NK cells are in contact with the tumor. At $t = 1$ h more NK cells are interacting with the tumor. At $t = 22$ h the perimeter of the tumor has altered by dead cancer cells (red) detached from the tumor (green intensity has decreased due to NK mediated death and bleaching). At $t = 51$ h and 124 h, calcein green AM labeling was repeated, staining the cells that are alive (i.e., both NK cells and cancer cells appear green after 51 h). At $t = 120$ h before the second re-labelling (only present in panel B), the tumor has already started to disintegrate. (C-D): Corresponding sequence as in (A-B), but for a tumor that continues to grow over the full time period of 124 h. (E): Quantification of the number of NK cells interacting with each category-I (3D) tumor divided by the average tumor volume, as a function of the tumor size change (decreased, constant or increased tumor size) over a 22 hours assay. (F): Quantification of the number of NK cells interacting with each category-I (3D) tumor divided by the average tumor volume, as a function of the final tumor outcome (either defeated or living tumor) after a 124 hours assay. All scale bars correspond to $100 \mu\text{m}$. Red horizontal bars and stars indicate the overall significance of all three sets of data tested by the Kruskal-Wallis test, and black horizontal bars and stars indicate the statistical significance of the data when analysed pairwise by the Mann-Whitney U test.

REFERENCES

1. C. J. Lovitt, T. B. Shelper and V. M. Avery, *Biology*, 2014, **3**, 345-367.
2. C. L. Li, T. Tian, K. J. Nan, N. Zhao, Y. H. Guo, J. Cui, J. Wang and W. G. Zhang, *Oncol Rep*, 2008, **20**, 1465-1471.
3. E. C. Butcher, E. L. Berg and E. J. Kunkel, *Nat Biotechnol*, 2004, **22**, 1253-1259.
4. D. Hanahan and R. A. Weinberg, *Cell*, 2000, **100**, 57-70.
5. F. Pampaloni, E. G. Reynaud and E. H. K. Stelzer, *Nat Rev Mol Cell Biol*, 2007, **8**, 839-845.
6. S. Ghosh, G. C. Spagnoli, I. Martin, S. Ploegert, P. Demougin, M. Heberer and A. Reschner, *Journal of Cellular Physiology*, 2005, **204**, 522-531.
7. K. E. Sung and D. J. Beebe, *Advanced Drug Delivery Reviews*, 2014, **79-80**, 68-78.
8. A. Stojanovic, M. P. Correia and A. Cerwenka, *Cancer Microenviron*, 2013, **6**, 135-146.
9. M. R. Parkhurst, J. P. Riley, M. E. Dudley and S. A. Rosenberg, *Clin Cancer Res*, 2011, **17**, 6287-6297.
10. T. Igarashi, J. Wynberg, R. Srinivasan, B. Becknell, J. P. McCoy, Jr., Y. Takahashi, D. A. Suffredini, W. M. Linehan, M. A. Caligiuri and R. W. Childs, *Blood*, 2004, **104**, 170-177.
11. A. Giannattasio, S. Weil, S. Kloess, N. Ansari, E. H. K. Stelzer, A. Cerwenka, A. Steinle, U. Koehl and J. Koch, *BMC Cancer*, 2015, **15**, 351.
12. T. D. Holmes, Y. M. El-Sherbiny, A. Davison, S. L. Clough, G. E. Blair and G. P. Cook, *The Journal of Immunology*, 2011, **186**, 1538-1545.
13. P. A. Albertsson, P. H. Basse, M. Hokland, R. H. Goldfarb, J. F. Nagelkerke, U. Nannmark and P. J. Kuppen, *Trends Immunol*, 2003, **24**, 603-609.
14. K. Iwasaki, H. Kikuchi, S. Miyatake, T. Aoki, T. Yamasaki and Y. Oda, *Cancer Res*, 1990, **50**, 2429-2436.
15. M. Rimann and U. Graf-Hausner, *Curr Opin Biotechnol*, 2012, **23**, 803-809.
16. D. Gao, H. Liu, Y. Jiang and J.-M. Lin, *TrAC Trends in Analytical Chemistry*, 2012, **35**, 150-164.
17. F. Hirschhaeuser, H. Menne, C. Dittfeld, J. West, W. Mueller-Klieser and L. A. Kunz-Schughart, *Journal of Biotechnology*, 2010, **148**, 3-15.
18. A. Ivascu and M. Kubbies, *Journal of Biomolecular Screening*, 2006, **11**, 922-932.
19. Y. C. Tung, A. Y. Hsiao, S. G. Allen, Y. S. Torisawa, M. Ho and S. Takayama, *Analyst*, 2011, **136**, 473-478.
20. G. R. Souza, J. R. Molina, R. M. Raphael, M. G. Ozawa, D. J. Stark, C. S. Levin, L. F. Bronk, J. S. Ananta, J. Mandelin, M.-M. Georgescu, J. A. Bankson, J. G. Gelovani, T. C. Killian, W. Arap and R. Pasqualini, *Nat Nano*, 2010, **5**, 291-296.
21. H. Bruus, J. Dual, J. Hawkes, M. Hill, T. Laurell, J. Nilsson, S. Radel, S. Sadhal and M. Wiklund, *Lab on a Chip*, 2011, **11**, 3579-3580.
22. B. Vanherberghen, O. Manneberg, A. Christakou, T. Frisk, M. Ohlin, H. M. Hertz, B. Onfelt and M. Wiklund, *Lab on a Chip*, 2010, **10**, 2727-2732.

23. A. E. Christakou, M. Ohlin, B. Vanherberghen, M. A. Khorshidi, N. Kadri, T. Frisk, M. Wiklund and B. Önfelt, *Integrative Biology*, 2013, **5**, 712-719.
24. M. Wiklund, A. Christakou, M. Ohlin, I. Iranmanesh, T. Frisk, B. Vanherberghen and B. Önfelt, *Micromachines*, 2014, **5**, 27-49.
25. J. Hultström, O. Manneberg, K. Dopf, H. M. Hertz, H. Brismar and M. Wiklund, *Ultrasound in Medicine and Biology*, **33**, 145-151.
26. J. Svennebring, O. Manneberg and M. Wiklund, *Journal of Micromechanics and Microengineering*, 2007, **17**, 2469.
27. M. Wiklund, *Lab on a Chip*, 2012, **12**, 2018-2028.
28. C. Berasain, J. Castillo, M. J. Perugorria, M. U. Latasa, J. Prieto and M. A. Avila, *Annals of the New York Academy of Sciences*, 2009, **1155**, 206-221.
29. D. Capece, M. Fischietti, D. Verzella, A. Gaggiano, G. Ciccirelli, A. Tessitore, F. Zazzeroni and E. Alesse, *BioMed Research International*, 2013, **2013**, 15.
30. H.-R. Kim, H.-J. Park, J. Park, S. Kim, K. Kim and J. Kim, *Cancer Immunol Immunother*, 2004, **53**, 461-470.
31. J. H. Lee, J.-H. Lee, Y.-S. Lim, J. E. Yeon, T.-J. Song, S. J. Yu, G.-Y. Gwak, K. M. Kim, Y. J. Kim, J. W. Lee and J.-H. Yoon, *Gastroenterology*.
32. M. Ohlin, A. E. Christakou, T. Frisk, B. Önfelt and M. Wiklund, *Journal of Micromechanics and Microengineering*, 2013, **23**, 035008.
33. O. Manneberg, B. Vanherberghen, B. Önfelt and M. Wiklund, *Lab on a Chip*, 2009, **9**, 833-837.
34. J. M. Kelm, N. E. Timmins, C. J. Brown, M. Fussenegger and L. K. Nielsen, *Biotechnology and Bioengineering*, 2003, **83**, 173-180.
35. R.-Z. Lin, L.-F. Chou, C.-C. Chien and H.-Y. Chang, *Cell Tissue Res*, 2006, **324**, 411-422.
36. D. Bazou, W. T. Coakley, A. J. Hayes and S. K. Jackson, *Toxicology in Vitro*, 2008, **22**, 1321-1331.
37. D. Bazou, *Cell Biol Toxicol*, 2010, **26**, 127-141.