

# RSC Advances



This is an *Accepted Manuscript*, which has been through the Royal Society of Chemistry peer review process and has been accepted for publication.

*Accepted Manuscripts* are published online shortly after acceptance, before technical editing, formatting and proof reading. Using this free service, authors can make their results available to the community, in citable form, before we publish the edited article. This *Accepted Manuscript* will be replaced by the edited, formatted and paginated article as soon as this is available.

You can find more information about *Accepted Manuscripts* in the [Information for Authors](#).

Please note that technical editing may introduce minor changes to the text and/or graphics, which may alter content. The journal's standard [Terms & Conditions](#) and the [Ethical guidelines](#) still apply. In no event shall the Royal Society of Chemistry be held responsible for any errors or omissions in this *Accepted Manuscript* or any consequences arising from the use of any information it contains.

## One-pot synthesis of polyaniline-gold nanocomposite and its enhanced electrochemical properties for biosensing application

Amrita Soni, Chandra Mouli Pandey, Shipra Solanki, Gajjala Sumana\*

Biomedical Instrumentation Section, CSIR-National Physical Laboratory, New Delhi-110012, India.

### Abstract

One pot synthesis of polyaniline-gold (PANI-Au) nanocomposite has been conducted using chemical route in the presence of dodecyl benzene sulfonic acid. This PANI-Au nanocomposite was further electrophoretically deposited onto indium tin oxide (ITO) coated glass substrates and the electrochemical kinetics were compared with chronopotentiometrically deposited PANI-Au (in presence of HCl) composite. The electrochemical results indicate that the composite prepared by chemical route exhibits enhanced electron transfer coefficient ( $\alpha$ ) of 0.92 and charge transfer rate constant ( $k_s$ ) of  $0.0848 \text{ s}^{-1}$  as compared to the film deposited using chronopotentiometric technique ( $\alpha = 0.85$  and  $k_s = 0.0368 \text{ s}^{-1}$ ). These fabricated matrices have been further utilized as biosensing platforms for the detection of sexually transmitted disease. The PANI-Au based genosensor has demonstrated enhanced sensitivity ( $10^{-16} \text{ M}$ ; linear range from  $10^{-6}$  to  $10^{-16} \text{ M}$ ) with a response time of 60 s and shows excellent specificity over other bacterial pathogens. The results of these studies help in understanding the method of synthesis on the electrochemical as well as catalytic properties of the composite and its potential for wide range of biomedical applications.

---

\*Corresponding author: [sumanagajjala@gmail.com](mailto:sumanagajjala@gmail.com), Tel: +91-11-42342439

## 1. Introduction

Conducting polymers and their nanocomposites have aroused much interest in recent years due to their good electrical conductivity, redox properties, ease of synthesis, and enhanced stability.<sup>1,2</sup> Among various conducting polymers, polyaniline (PANI) is widely investigated because of its unique redox tunability, sensitivity, excellent process ability together with the presence of a number of intrinsic redox states has substantially enhanced the potential applications of PANI in biomedical devices.<sup>2-6</sup> Composites of PANI containing amino groups and gold nanoparticles (AuNPs) possessing high affinity for thiols helps in the interaction of the PANI-Au nanocomposite with biomolecules.<sup>7,8</sup> Moreover, the large surface area to volume ratio of the nanoparticles provides suitable transducer surface for attaching the biomolecules.<sup>9</sup> Afzal *et al.* examined that the electrical conductivity as well as thermal stability of composite can be increased with respect to the concentration of AuNPs in the PANI-Au nanocomposite.<sup>10, 11</sup> Liu *et al.* have fabricated polystyrene/polyaniline/Au composite based biosensor and investigated that fabricated sensor shows excellent redox ability in a wide pH range from 1.0 to 9.0 with high catalytic activity.<sup>12</sup> Tian *et al.* have prepared polyaniline/gold nanoparticles multilayer films by layer by layer method and showed that sensor can be used with very good electroactivity in a neutral pH environment.<sup>13</sup> Feng *et al.* also have described the Au/PANI matrix to construct sensor and has showed the sensor is having high catalytic activity and enhanced detection sensitivity.<sup>14</sup>

Gonorrhoea has been reported as second most common bacterial sexually transmitted disease (STD).<sup>15</sup> An etiologic pathogen named *N. gonorrhoeae* causes gonorrhoea and its related clinical syndromes such as urethritis, cervicitis, salpingitis, bacteremia, arthritis etc.<sup>16</sup> Globally, an estimated 12 million people are infected every year, and the majority of infections are believed to occur in developing countries.<sup>17</sup> The incidence of gonorrhoea varies with age i.e seventy-five percent of cases occur in persons aged less than 30 years. Gonorrhoea infection spreads in healthy person by physical contact with the mucosal surfaces of an infected sexual partner.<sup>18</sup> During birth, ophthalmic gonococci infection may be develop in new born baby due to passage of infected mother's genital tract. The main seriousness of this infection is caused by its asymptomatic behavior i.e upto 80% of women and 10% of men, are asymptomatic and gonorrhoea is co-factor for other STD like HIV. Various techniques are available for the

detection of gonorrhoea which includes culture, gram stain test and nucleic acid amplification test (NAAT). Culture has been used most widely, but it can be used for the detection of living cells only and needs multiple steps for processing specimens with addressing of quality assurance at each step.<sup>19, 20</sup> Gram stain test which is having specificity (>99%) and sensitivity (>95%) for symptomatic men or women but, for asymptomatic men or women test is less useful, because of lower sensitivity.<sup>21</sup> NAATs test is applicable for variety of specimen types including endocervical swabs, vaginal swabs and urethral swabs in men but sensitivity of NAATs varies with NAAT type and is very expensive.<sup>22</sup> These various conventional techniques are having limitations in terms of time consumption which also need skilled laboratory personnel.<sup>18</sup> Therefore, there is an immediate demand for the development of low cost, reliable, rapid biosensor for diagnosis of *Neisseria gonorrhoeae*.

In the present work, efforts have been made to synthesize PANI-Au nanocomposite using chemical route and chronopotentiometric techniques. Further, the bioelectrodes have been fabricated by immobilizing probe sequence specific to *Neisseria gonorrhoeae* on to the deposited films.

## 2. Materials and methods

### 2.1 Chemical and reagents

Aniline, aurochloric acid ( $\text{AuCl}_3$ ), sodium citrate, methylene blue, tris base, ethylene diamine tetra acetic acid (EDTA), potassium monohydrogen phosphate, potassium dihydrogen phosphate, oligonucleotide probes (20 bases), ammonium peroxydisulfate, copper sulphate, dodecyl benzene sulfonic acid (DBSA) and all other reagents and solvents have been procured from Sigma-Aldrich (India). Indium-tin oxide (ITO) coated glass plates with resistivity  $30\Omega$  have been purchased from Balzers, UK. All other chemicals were of analytical grade and used without purification. Deionized water (resistance  $18.2\text{ M}\Omega$ ) from the Millipore water purification system was used for the preparation of desired aqueous solutions. DNA probes used for hybridization are as follows.

**Probe:** thiol-5'-CCGGTGCTTCATCACCTTAG-3';

**Complementary target:** 5'-CTAAGGTGATGAAGCACCGG-3';

**Non-complementary target:** 5'-GTATGGTGATCAAGCTCCCG-3';

**One-base mismatch DNA:** 5'-CTAAGTTGATGAAGCACCGG-3';

**Two-base mismatch DNA:** 5'-CTAAGTTTGATGAAACCACCGG-3';

**Three-Base mismatch DNA:** 5'-CTAAGTTTTGATGAAAGGACCGG-3';

## 2.2 DNA extraction and processing of microbial samples

DNA has been isolated from a panel of strains comprising of control strains of *N. gonorrhoeae*, *Escherichia coli*, *Neisseria sicca*, *Staphylococcus aureus* and *Klebsiella pneumoniae* for specificity studies. For this, 200 $\mu$ L sterile MilliQ water is taken in a 2mL eppendorf and a suspension of colonies is made and then vortexed. The suspension is further boiled for about 15 min and is centrifuged at 10,000rpm for about 10min. To this, equal volume (200 $\mu$ L) of 24:1 (v/v) chloroform: iso-amyl alcohol is added followed by centrifuging at 12,000rpm for about 10 min. The aqueous layer containing DNA is carefully pipetted out and is kept at  $-20^{\circ}\text{C}$  prior to being used.<sup>32</sup>

## 2.3 Preparation of gold nanoparticles

Gold nanoparticles (AuNPs) were synthesized using previous reported method with slight modification. In brief 1 ml of sodium citrate (1%w/v) has been added drop wise in 10 ml of AuCl<sub>3</sub> (2 mM) with continuous stirring for 30 min at 80 $^{\circ}\text{C}$  till the color of solution changes from pale yellow to ruby red, indicating the formation of colloidal AuNPs.<sup>23</sup>

## 2.4 Fabrication of electrochemically deposited PANI-Au/ITO electrodes

Figure 1(a) illustrates the electrochemical (EC) polymerization of aniline (0.1 M) which has been carried out using 1M HCl in the presence of AuNPs (5mM) onto ITO electrode (0.5 cm<sup>2</sup>). Polymerization was done chronopotentiometrically using Ag/AgCl as the reference electrode, platinum (Pt) as the counter electrode, and ITO as the working electrode at 150  $\mu$ A for 300 s (EC-PANI-Au/ITO).<sup>24</sup>

## 2.5 Fabrication of electrophoretically deposited PANI-Au/ITO electrodes

PANI-Au nanocomposite has been synthesized by mixing 100 ml of diluted AuNPs (5 mM) in aniline (0.1 M) and polymerization has been carried out in presence of DBSA with continuous stirring till the color of solution changes from red to turbid white.<sup>25</sup> Solution was cooled down to 0 $^{\circ}\text{C}$  after which 1ml of CuSO<sub>4</sub> and 5 ml ammonium peroxydisulfate (1 M) was added. After six hours, dark green mixture was formed, which was further centrifuged, collected and dispersed in 10 ml of ethanol. The electrophoretic deposition (EPD) was carried out at 50 V for 30 s using a

two electrode system (shown in figure 1(b)) in which ITO electrode was used as cathode and thin platinum foil as anode, which results in the formation of PANI-Au nanocomposite films (EPD-PANI-Au/ITO).

## 2.6 Characterization

The structural and morphological characterization of PANI-Au nanocomposite have been carried out using transmission electron microscope (TEM, Hitachi Model, H-800) and scanning electron microscope (SEM, JEOLJSM-6700F, 10kV). Dynamic light scattering (DLS) measurements were performed with a Zetasizer Nano-ZS90 (Malvern Instruments) at a scattering angle of 90° and at constant temperature of 25°C to determine the zeta potential and particle size of GNPs and PANI-Au nanocomposite. Fourier transform infrared (FT-IR) spectroscopic measurements have been carried out using Perkin-Elmer spectrometer (model Spectrum BX) at 25°C. Contact angle (CA) has been recorded using contact angle meter (Data Physics OCA15EC). Electrochemical characterizations have been conducted on an Autolab potentiostat/galvanostat (Eco Chemie, Utrecht, The Netherlands) using a three-electrode cell with PANI-Au/ITO as working electrode, platinum as an auxiliary electrode and Ag/AgCl as a reference electrode in phosphate buffer (PBS, 50 mM, pH 7.0, 0.9% NaCl) containing 5 mM  $[\text{Fe}(\text{CN})_6]^{3-/4-}$ . Subsequently, the DPV measurements of pDNA/EPD-PANI-Au/ITO electrodes have been carried out in 50  $\mu\text{M}$  MB, pre-treatment at +0.5 V for 10 s, at step potential of 5 mV and modulation amplitude of 250mV.

## 2.7 Fabrication of bioelectrodes for *N. gonorrhoeae* detection

Composites prepared by both the techniques (EC-PANI-Au/ITO, EPD-PANI-Au/ITO) have been utilized for the biosensor fabrication by immobilizing thiolated oligonucleotide (thiol-DNA, 20  $\mu\text{l}$ , 1.0  $\mu\text{M}$ ) specific to *N. gonorrhoeae* having 20 base pairs in a humid chamber at 25°C and incubated for about 12 h. These modified electrodes were washed with tris buffer several times to remove any unbound pDNA. The hybridization studies of pDNA/EPD-PANI-Au bioelectrode with target DNA sequences (complementary DNA concentration range ( $1 \times 10^{-16}$  M to  $1 \times 10^{-6}$  M), non-complementary, one-base mismatch, two base mismatch and three base mismatch) have been carried out in a humid chamber for 60 s at 25°C.

## 3. Results and discussions

### 3.1 Surface characterization

TEM studies were conducted to confirm the particle size and the core structure of the PANI-Au nanocomposite. Figure 2(a) represents TEM image of AuNPs having spherical structure with a diameter in the range of 30-40 nm. The TEM images of EC-PANI-Au (Fig. 2 (b)) and EPD-PANI-Au (Fig. 2(c)) indicate AuNPs as dark spots encapsulated by gray PANI shells. However, it has been observed that AuNPs are well dispersed in PANI synthesized by using chemical route (Fig.2 (d)) in comparison to that synthesized by direct electrochemical polymerization of PANI, where accumulation of AuNPs is observed.

The particle size distribution and zeta potential of the AuNPs and PANI-Au have been determined via dynamic light scattering and is shown in figure S1. The average size of formed AuNPs is about 38 nm with a polydispersity index of  $\sim 0.5$  (Fig. S1 (a)), while the surface charge determined using the Smoluchowski method, is found to be  $-25.6$  mV (Fig. S1 (b))<sup>26</sup>. However, the zeta potential value of PANI-Au nanocomposite has been found to be  $43.2$  mV (Fig. S1(c)) which indicates that the formed nanocomposites are quite stable, which is the requisite property for the electrophoretic deposition.

Brunauer–Emmett–Teller (BET) measurement was performed for evaluating the specific surface area of the EC-PANI-Au nanocomposite and PANI-Au nanocomposite synthesized by chemical route. For BET analysis both the nanocomposites were degassed in a vacuum at  $150^{\circ}\text{C}$  for 5h. The surface area was calculated on the basis of BET theory and shown in figure S2.<sup>27</sup> It can be seen the value of BET surface area for PANI-Au nanocomposite synthesized by chemical route was found to be  $43.17\text{ m}^2\text{g}^{-1}$  (Fig.S2; curve (ii)), which is higher than the value for EC-PANI-Au nanocomposite ( $32.23\text{ m}^2\text{g}^{-1}$ ; Fig.S2, curve (i)).<sup>28</sup> The average pore size of the chemically synthesized PANI-Au nanocomposite is  $19.4\text{ \AA}$  and that of EC-PANI-Au is  $34.5\text{ \AA}$ . The value indicates that the nanocomposite synthesized by chemical route is having large surface area in comparison to nanocomposite synthesized by electrochemical route.

SEM images of EC-PANI-Au/ITO electrode (Fig. 3(a)) and EPD-PANI-Au/ITO electrode (Fig. 3(c)) show a uniformly distributed three-dimensional structure which suggests homogeneity in the matrix. However, it has been observed that more intensified porous structures were formed in case of EPD-PANI-Au/ITO where AuNPs are well distributed in the porous PANI. After immobilization of pDNA on EC-PANI-Au/ITO electrode (Fig. 3(b)) and EPD-PANI-Au/ITO electrode (Fig. 3(d)) globular structure has been noticed. Interestingly, it has

been perceived that the immobilization of pDNA on the EC-PANI-Au/ITO electrode is not uniform (inset fig. 3(b)). However, the even distribution of the pDNA can be easily observed for the EPD-PANI-Au/ITO electrode (inset fig. 3(d)) which is due to enhanced porosity and increased surface roughness of EPD-PANI-Au/ITO electrode. Furthermore, a magnified view of the pDNA/EPD-PANI-Au/ITO electrode surface (inset fig. 3(d)) reveals the presence of globules in isolation that exclude the probability of steric hindrance to target oligonucleotide and hence plays an important role in determining the performance of the sensor.<sup>29</sup>

Contact angle (CA) measurements have been carried out using the sessile drop method to investigate immobilization of pDNA on the surface of PANI-Au matrix. Change in contact angle of immobilized probe in respect of matrix shows the hydrophilicity/hydrophobicity of the prepared bioelectrode which in turn can be related to immobilization of pDNA. CA of ITO electrode (Fig. 4 (a)) was found to be 78.3°, which decreases to 65.4° for EC-PANI-Au/ITO electrode (Fig. 4 (b)) and to 42.2° for EPD-PANI-Au/ITO electrode (Fig. 4 (c)). The decrease in CA of electrode can be related to the presence of hydrophilic functional groups (–NH and –COOH). The decrease in CA to 16.4° (Fig. 4 (d)) for EC-PANI-Au/ITO electrode and to 10.2° for EPD-PANI-Au/ITO electrode (Fig. 4 (e)) after the immobilization of pDNA, may be due to the enhancement of hydrophilicity caused by the presence of negatively charged phosphodiester backbone of pDNA.<sup>26</sup> With variation in time the value of CA decreases and becomes constant after 8h of immobilization indicating the complete immobilization of DNA in this duration.

To determine the interactions between AuNPs, PANI and pDNA, FT-IR spectrum of EPD-PANI-Au/ITO and pDNA/EPD-PANI-Au/ITO electrodes have been performed. Peaks at 1576 and 1495 cm<sup>-1</sup> in figure S3 (a) for PANI/ITO films have been attributed to C=C stretching deformation of quinoid and benzenoid rings respectively showing oxidation state of PANI as reported in literature.<sup>30</sup> Whereas, for EPD-PANI-Au/ITO electrode, there is a shift in the peaks to 1590 and 1511 cm<sup>-1</sup> (Fig. S3(b)). Peaks at 1300 and 1140 cm<sup>-1</sup> in fig S3 (a) corresponding to C–N stretching of secondary aromatic amine and aromatic C–H in-plane bending respectively where as in figure S3 (b) there is shift in the peaks at 1315 and 1149 cm<sup>-1</sup>. The shifting in the peaks shows that the C-N bonds within the composite are influenced by the AuNPs (Fig. S3 (b)). Further, the shift in energy to higher energy levels indicates that the Au directly influences the electron density of the C-N bond.<sup>31</sup> The peak seen at 794 cm<sup>-1</sup> in figure S3 (a) related to out-of-

plane deformation vibration of C–H. The shifting in the peaks to high energy in figure S3 (b) at  $833\text{ cm}^{-1}$  for PANI-Au in comparison to the PANI films directly related to differences in chemistry and electron density.<sup>31</sup> FT-IR spectrum of pDNA/EPD-PANI-Au/ITO electrode (Fig. S3 (c)) shows absorption bands at  $1036\text{ cm}^{-1}$  and  $1398\text{ cm}^{-1}$  which are associated with anti-symmetric stretching vibration of P–O–C and symmetric stretching vibration of P=O of the phosphoric acid group, respectively. Whereas, the bands at  $1512\text{ cm}^{-1}$  and  $1603\text{ cm}^{-1}$  are attributed to carbonyl stretching vibration and C=C bonds in the purine and pyrimidine.

### 3.2 Electrochemical characterization

Electrochemical characterization has been conducted using cyclic voltammetry (CV) in phosphate buffer saline (100 mM, pH 7.0, 0.9% NaCl) containing  $5\text{ mM } [\text{Fe}(\text{CN})_6]^{3-/4-}$  to examine the electro-active behavior of the electrodes (Fig. S4). There was a decrease in the peak current for both EC-PANI-Au/ITO (0.46 mA) and EPD-PANI-Au/ITO (0.60 mA), as compared to ITO (1.7 mA) electrode at a scan rate of  $50\text{ mVs}^{-1}$  (Fig. S4 (a)). Interestingly for EPD-PANI-Au/ITO electrode the peak current was higher than EC-PANI-Au/ITO which may be due to strong physio-chemical interaction between AuNPs and PANI which is due to charge transfer process from the positively charged imine nitrogen of PANI to the negatively charged AuNPs. This results in uniform distribution of AuNPs in the conducting polymeric chains of PANI without any aggregation resulting in a favorable pathway for the transfer of electrons.<sup>32</sup> Moreover, the large surface area of the PANI/Au nanocomposite is due to presence of AuNPs provides more active sites for the electron transfer and effective charge migration through the polymer. In case of EC-PANI-Au there is possibility that insufficient time is available for the binding of AuNPs on the surface of PANI which may result in phase separation.<sup>25, 33, 34</sup> After the immobilization of probe DNA there was a large increase in the peak current for EPD-PANI-Au/ITO electrode (1.14 mA) in comparison to EC-PANI-Au/ITO electrode (0.83 mA), which suggest that there is immobilization of more probe DNA onto EC-PANI-Au/ITO electrode that creates a negative charge on the surface thus repels the negatively charged redox marker,  $[\text{Fe}(\text{CN})_6]^{3-/4-}$ .

The CV investigations at various potential scan rates ( $v$ ; 10 to 300 mV/s) have been performed onto EPD-PANI-Au/ITO electrode (Fig. S4 (b)) and EC-PANI-Au/ITO electrode (Fig. S4 (c)). As the scan rate increases, the anodic peak potential shifts to more positive value and the cathodic peak to more negative value, suggesting a quasi-reversible process. The positive and

negative peaks correspond to the oxidation and reduction of the  $[\text{Fe}(\text{CN})_6]^{3-/4-}$  respectively. The peak current values of these electrodes have linear relationship with respect to the square root of scan rate indicating the existence of diffusion-controlled electrochemical reaction (Fig.S4 inset). Both anodic and cathodic peak potentials are found to change linearly with respect to log of  $v$ , which agrees with Laviron's theory:<sup>35</sup>

$$E_{pa} = E^o + X \ln[(1 - \alpha)Fv/RTk_s] \quad 1$$

$$E_{pc} = E^o + Y \ln[\alpha Fv/RTk_s] \quad 2$$

$$\ln k_s = \alpha \ln(1 - \alpha) + (1 - \alpha) \ln \alpha - \ln(RT/nFv) - \alpha(1 - \alpha)nF\Delta E_p/RT. \quad 3$$

where  $\alpha$  and  $k_s$  denotes electron transfer coefficient and charge transfer rate constant respectively and  $X = RT/(1 - \alpha)nf$  and  $Y = RT/\alpha nf$  are the slopes of straight line plotted by  $\ln v$  versus the anodic peak potential ( $E_{pa}$ ) and cathodic peak potential ( $E_{pc}$ ) respectively. The values of  $\alpha$  and  $k_s$  for EPD-PANI-Au/ITO electrode is found to be 0.92 and  $0.0848 \text{ s}^{-1}$  respectively. Similarly, for EC-PANI-Au/ITO electrode the values for  $\alpha$  is found to be 0.85 and  $k_s$  is  $0.0368 \text{ s}^{-1}$  respectively. By using Randles–Sevcik equation:<sup>30</sup>

$$I_p = (2.99 \times 10^5) \alpha^{1/2} n^{3/2} AC D^{1/2} v^{1/2} \quad 4$$

diffusion coefficient (D) has been calculated as  $6.9 \times 10^{-15} \text{ cm}^2 \text{ s}^{-1}$  for EPD-PANI-Au/ITO electrode and  $2.6 \times 10^{-15} \text{ cm}^2 \text{ s}^{-1}$  for EC-PANI-Au/ITO electrode. Here C is the molar concentration of  $[\text{Fe}(\text{CN})_6]^{3-/4-}$ , n is the number of transferred electrons for the redox reaction and  $v$  is the scan rate ( $50 \text{ mVs}^{-1}$ ). The effective surface areas (A) of the EPD-PANI-Au/ITO electrode and EC-PANI-Au/ITO electrode have been calculated using the Eqn.5. and found to be  $0.53 \text{ mm}^2$  and  $0.48 \text{ mm}^2$  respectively.

$$A = S/(2.99 \times 10^5) \alpha^{1/2} n^{3/2} C D^{1/2} \quad 5$$

These enhanced kinetic parameters for EPD-PANI-Au/ITO electrode in comparison to the EC-PANI-Au/ITO electrode are due to better charge transfer and electrostatic interaction between PANI and AuNPs.

### 3.3 Genosensor response studies

Differential pulse voltammetry (DPV) has been used to study the electrochemical response of the fabricated pDNA/EPD-PANI-Au/ITO by immobilizing target DNA using methylene blue (MB,  $20 \mu\text{M}$ ) as redox hybridization indicator. MB is known to have affinity with the nitrogenous guanine bases of pDNA and undergo reduction by oxidizing them.<sup>36-38</sup> In figure 5 (a) bar

diagram showing the MB peak current is highest ( $1.07 \times 10^{-5}$  A) for pDNA/EPD-PANI-Au/ITO which is due to the presence of nitrogenous bases, but after incubation with complementary target sequence, peak current reduces to  $5.8 \times 10^{-6}$  A. This may be due to the nonaccessibility of nitrogenous bases on the electrode surface due to the formation of duplex. After incubation of the bioelectrode with non-complementary DNA, no significant change in MB peak current ( $1.09 \times 10^{-5}$  A) was observed in comparison to the pDNA/EPD-PANI-Au/ITO which indicates non-hybridization at the electrode surface. However after incubating the bioelectrode with one base, two base and three base mismatch DNA sequences the peak current substantial decreases in comparison with the noncomplementary DNA sequence showing that the biosensor can even distinguish a single nucleotide variation in target DNA sequence. The response characteristics of the electrode as a function of complementary DNA concentration ranging from  $1 \times 10^{-16}$  to  $1 \times 10^{-6}$  M shown in figure 5 (b).<sup>39</sup> The results reveals that with decrease in concentration of complementary target DNA, there is an increase in the MB reduction current which can be correlated to extent of hybridization<sup>40</sup> Figure 5(c) shows the peak current values of the sensor which attributes a linear correlation to the log [target concentration] from  $1 \times 10^{-6}$  M to  $1 \times 10^{-16}$  M and follows Eq. (6).

$$\text{MB oxidation current } I_{\mu\text{A}} = -0.47 \times \log(\text{target DNA concentration}) - 2.8; R = 0.9963 \quad 6$$

The detection limit calculated using the standard equation  $3\sigma/\text{sensitivity}$  was found to be  $1 \times 10^{-16}$  M, where  $\sigma$  is standard deviation of the electrode without hybridization.<sup>41</sup> The comparison of response characteristics of EPD-PANI-Au nanocomposite with other PANI based nanocomposites reported in literature for nucleic acid detection shows that this sensor exhibits higher linear range, sensitivity and stability (as shown in Table T2).<sup>37, 42-45</sup>

### 3.4 Genosensor response studies with culture, positive patient and spiked samples

DPV response of the fabricated pDNA/EPD-PANI-Au/ITO bioelectrode with clinical samples has been studied by identifying change in MB oxidation peak current and is shown in bar diagram (Fig 5(d)). Specificity of the biosensor has been studied by incubating the bioelectrode with DNA extracted from different real samples containing *N. gonorrhoeae* (culture, positive patient, pus sample spiked) and cultures of *Escherichia coli*, *Neisseria sicca*, *Staphylococcus aureus*, *Klebsiella pneumoniae*. The bar diagram shows decrease in the value of peak current after

treating with *N. gonorrhoeae* (patient, spiked and culture) samples indicating specific hybridization, however no significant change in the peak current was observed when pDNA/EPD-PANI-Au/ITO bioelectrode was treated with DNA samples of other non *gonorrhoeae* species and other gram-negative bacterial samples (*E. coli*). These results indicate that the fabricated pDNA/EPD-PANI-Au/ITO bioelectrode is highly specific for *N. gonorrhoeae* detection.

### 3.5 Stability and reproducibility

The regeneration of the pDNA/EPD-PANI-Au/ITO bioelectrode has been carried out by dipping it in the buffer solution (pH 8.0) containing Tris-HCl (10 mM) and EDTA (1 mM) at 100°C for 5 min, followed by cooling in ice bath for about 30 min, which completely removes complementary DNA via thermal denaturation.<sup>46, 47</sup> The MB peak current decreases after each consecutive use of pDNA bioelectrode, as initially it was  $1.07 \times 10^{-5}$  A and after twelfth use it reached to  $0.90 \times 10^{-5}$  A (Fig. S5 (a)). It has been found that biosensor can be re-used for 12 times after which the bioelectrodes has lost around 15.3% of its sensitivity (Fig. S5(a)). The decrease in MB current after each use can be related to loss of pDNA from the surface of bioelectrode. To investigate the storage stability of the fabricated sensor, three measurements have been recorded each week for over 14 weeks of continuous analysis. The decrease in signal response of the bioelectrode is less than 20% when stored at 4 °C (Fig.S5 (b)).

### 4. Conclusions

We have successfully prepared the PANI-Au nanocomposite based electrodes by using chronopotentiometric and electrophoretic technique. The CV and morphological studies clearly reveal that the electrodes prepared by EPD technique have enhanced conductivity and conducive morphology. EPD-PANI-Au/ITO electrodes were further used for the fabrication of genosensor specific for *N. gonorrhoeae* which provides an increased surface area due to its porous structure. The wide detection range ( $10^{-6}$  to  $10^{-16}$  M), reduced response time (60 s) with high stability (4 weeks) and reusability (12 times) of the genosensor have been successfully demonstrated. The fabricated genosensor has been found to be highly specific to distinguish clinical and real samples of *N. gonorrhoeae* from other non *gonorrhoeae* and gram negative bacteria species. Attempts should be made to use this PANI-Au nanocomposite platform for detection of other biomolecules and may have significance in point-of-care diagnostics.

## Acknowledgments

We thank Director, National Physical Laboratory, India for providing facilities. A.S and G.S are thankful to CSIR for financial support received under the project ESC- 0103. C.M.P. is thankful to CSIR, India, for the award of Senior Research Fellow. S.S. is grateful to UGC, India for the award of Junior Research Fellowship. We thank Prof. B.D Malhotra, Dr. A.M Biradar and Ms Monali Singh for their valuable suggestions. We extend our sincere thanks to Dr Seema Singh (AIIMS, New Delhi) for providing the bacterial culture samples.

## References

1. J. Janata and M. Josowicz, *Nat. Mater.*, 2003, **2**, 19-24.
2. S. Virji, J. Huang, R. B. Kaner and B. H. Weiller, *Nano Lett.*, 2004, **4**, 491-496.
3. Y. Zhou, H. Itoh, T. Uemura, K. Naka and Y. Chujo, *Langmuir*, 2002, **18**, 277-283.
4. Y. Ma, N. Li, C. Yang and X. Yang, *Colloids Surf. A: Physicochem. Eng Asp.*, 2005, **269**, 1-6.
5. T. K. Sarma and A. Chattopadhyay, *J. Phy. Chem. A.*, 2004, **108**, 7837-7842.
6. J. Han, L. Li and R. Guo, *Macromolecules*, 2010, **43**, 10636-10644.
7. W. Yang, J. Liu, R. Zheng, Z. Liu, Y. Dai, G. Chen, S. Ringer and F. Braet, *Nanoscale Res. Lett.*, 2008, **3**, 468-472.
8. S. K. Pillalamarri, F. D. Blum, A. T. Tokuhiko and M. F. Bertino, *Chem. Mater.*, 2005, **17**, 5941-5944.
9. S. K. Arya, A. Dey and S. Bhansali, *Biosens. Bioelectron.*, 2011, **28**, 166-173.
10. A. B. Afzal, M. J. Akhtar, M. Nadeem and M. M. Hassan, *J. Phy. Chem. C*, 2009, **113**, 17560-17565.
11. Z. Peng, L. Guo, Z. Zhang, B. Tesche, T. Wilke, D. Ogermann, S. Hu and K. Kleinermanns, *Langmuir*, 2006, **22**, 10915-10918.
12. Y. Liu, X. Feng, J. Shen, J.-J. Zhu and W. Hou, *J. Phys. Chem. B*, 2008, **112**, 9237-9242.
13. S. Tian, J. Liu, T. Zhu and W. Knoll, *Chem. Mater.*, 2004, **16**, 4103-4108.
14. X. Feng, C. Mao, G. Yang, W. Hou and J.-J. Zhu, *Langmuir*, 2006, **22**, 4384-4389.
15. Z. A. Memish and A. O. Osoba, *Int. J. Antimicrob. Agents*, 2006, **4**, 86-93.

16. D. S. Kellogg, W. L. Peacock, W. E. Deacon, L. Brown and C. I. Pirkle, *J. Bacteriol.*, 1963, **85**, 1274-1279.
17. D. Mabey, *Medicine*, 2010, **38**, 216-219.
18. B. S. Shim, *Korean J. Urol.*, 2011, **52**, 589-597.
19. R. Singh, G. Sumana, R. Verma, S. Sood, M. K. Pandey, R. K. Gupta and B. D. Malhotra, *J. Biotechnol.*, 2010, **150**, 357-365.
20. M. Alam, F. Khayat, A. Al-Kayali and Y. Al-Suhaibani, *Indian J. Med. Microbiol.*, 2002, **20**, 37-39.
21. R. L. Cook, S. L. Hutchison, L. Åstergaard, R. S. Braithwaite and R. B. Ness, *Ann. Intern. Med.*, 2005, **142**, 914-925.
22. E. H. Koumans, R. E. Johnson, J. S. Knapp and M. E. St. Louis, *Clin. Infect. Dis.*, 1998, **27**, 1171-1180.
23. M.-C. Daniel and D. Astruc, *Chem. rev.*, 2004, **104**, 293-346.
24. N. Prabhakar, K. Arora, H. Singh and B. D. Malhotra, *J. Phy. Chem. B*, 2008, **112**, 4808-4816.
25. T. Berzina, A. Pucci, G. Ruggeri, V. Erokhin and M. P. Fontana, *Synth. Met.*, 2011, **161**, 1408-1413.
26. C. M. Pandey, A. Sharma, G. Sumana, I. Tiwari and B. D. Malhotra, *Nanoscale*, 2013, **5**, 3800-3807.
27. V. Divya and M. V. Sangaranarayanan, *Euro. Polym. J.*, 2012, **48**, 560-568.
28. M. A. Ali, K. Mondal, C. Singh, B. D. Malhotra and A. Sharma, *Nanoscale*, **7**, 7234-7245.
29. A. A. Ansari, R. Singh, G. Sumana and B. D. Malhotra, *Analyst*, 2009, **134**, 997-1002.
30. C. Dhand, G. Sumana, M. Datta and B. D. Malhotra, *Thin Solid Films*, 2010, **519**, 1145-1150.
31. J. M. Kinyanjui, D. W. Hatchett, J. A. Smith and M. Josowicz, *Chem. Mater.*, 2004, **16**, 3390-3398.
32. R. J. Tseng, C. O. Baker, B. Shedd, J. Huang, R. B. Kaner, J. Ouyang and Y. Yang, *Appl. Phy. Lett.*, 2007, **90**, 053101.

33. I. Šedeňkova, M. Trchová, J. Stejskal and J. Prokes, *ACS Appl. Mater. Inter.*, 2009, **1**, 1906-1912.
34. Q. Xu, J. Leng, H.-b. Li, G.-j. Lu, Y. Wang and X.-Y. Hu, *React. Funct. Polym.*, 2010, **70**, 663-668.
35. J. C. Vidal, E. García a and J. R. Castillo, *Anal. Chim. Acta.*, 1999, **385**, 213-222.
36. J. Wang, *Anal. Chim. Acta.*, 2002, **469**, 63-71.
37. R. Singh, R. Prasad, G. Sumana, K. Arora, S. Sood, R. K. Gupta and B. D. Malhotra, *Biosens. Bioelectron.*, 2009, **24**, 2232-2238.
38. O. A. Loaiza, S. Campuzano, M. Lopez-Berlanga, M. a. Pedrero and J. M. Pingarron, *Sensors*, 2005, **5**, 344-363.
39. C. M. Pandey, I. Tiwari and G. Sumana, *RSC Adv.*, 2014, **4**, 31047-31055.
40. S. Radhakrishnan, C. Sumathi, A. Umar, S. J. Kim, J. Wilson and V. Dharuman, *Biosens. Bioelectron.*, 2013, **47**, 133-140.
41. J.-C. Vidal, E. García-Ruiz and J.-R. Castillo, *Electroanalysis*, 2001, **13**, 229-235.
42. N. Zhu, Z. Chang, P. He and Y. Fang, *Electrochimica Acta*, 2006, **51**, 3758-3762.
43. T. Yang, N. Zhou, Y. Zhang, W. Zhang, K. Jiao and G. Li, *Biosens. Bioelectron.*, 2009, **24**, 2165-2170.
44. J. Wilson, S. Radhakrishnan, C. Sumathi and V. Dharuman, *Sens. Actuators B: Chemical*, **171-172**, 216-222.
45. Y. Bo, H. Yang, Y. Hu, T. Yao and S. Huang, *Electrochimica Acta*, 2010, **56**, 2676-2681.
46. C. M. Pandey, R. Singh, G. Sumana, M. K. Pandey and B. D. Malhotra, *Sens. Actuators B: Chemical*, 2010, **151**, 333-340.
47. A. Sharma, C. M. Pandey, Z. Matharu, U. Soni, S. Sapra, G. Sumana, M. K. Pandey, T. Chatterjee and B. D. Malhotra, *Anal. Chem.*, 2012, **84**, 3082-3089.

## Figure Captions

**Figure 1.** Schematic illustration for the preparation of (i) electrochemical deposition of PANI-Au nanocomposite on ITO electrode (ii) electrophoretical deposition of PANI-Au nanocomposite synthesized via chemical route on ITO electrode and fabrication of pDNA/PANI-Au/ITO bioelectrode.

**Figure 2.** TEM images of (a) AuNPs (b) electrochemical synthesized PANI-Au nanocomposite. PANI-Au nanocomposite synthesized by chemical route (c) at lower magnification (d) at higher magnification.

**Figure 3.** SEM images of (a) EC-PANI-Au/ITO (b) pDNA/EC-PANI-Au/ITO (c) EPD-PANI-Au/ITO and (d) pDNA/EPD-PANI-Au/ITO.

**Figure 4.** Contact angle measurements of (a) bare ITO (b) EC-PANI-Au/ITO (c) EPD-PANI-Au/ITO (d) pDNA/EC-PANI-Au/ITO and (e) pDNA/EPD-PANI-Au/ITO.

**Figure 5.** Bar diagram showing the (a) DPV response of (i) pDNA/EPD-PANI-Au/ITO after the incubation with (ii) complementary DNA (iii) three base mis-match (iv) two base mis-match (v) one base mis-match (vi) non complementary DNA (b) pDNA/EPD-PANI-Au/ITO electrode as the function of complementary DNA concentration ( $1 \times 10^{-6}$  to  $1 \times 10^{-16}$  M) (c) linearity plot showing the relationship between the MB peak current values with log [target DNA concentration]. Inset figure shows MB peak current values as a function of target DNA concentration. (d) Bar diagram showing the incubation of pDNA/EPD-PANI-Au/ITO with real samples of (i) *N. gonorrhoeae* patient (ii) *N. gonorrhoeae* cultured (iii) spiked *N. gonorrhoeae* (iv) *E. coli* (v) *N. sicca* (vi) *S. aureus* (vii) *K. pneumonia*.

**Table T1.** Kinetic parameters calculated for the EPD-PANI-Au/ITO electrode and EC-PANI-Au/ITO electrode.

**Table T2.** Comparison of the response characteristics of EPD-PANI-Au nanocomposite with other Polyaniline based nanocomposites.

Figure 1.

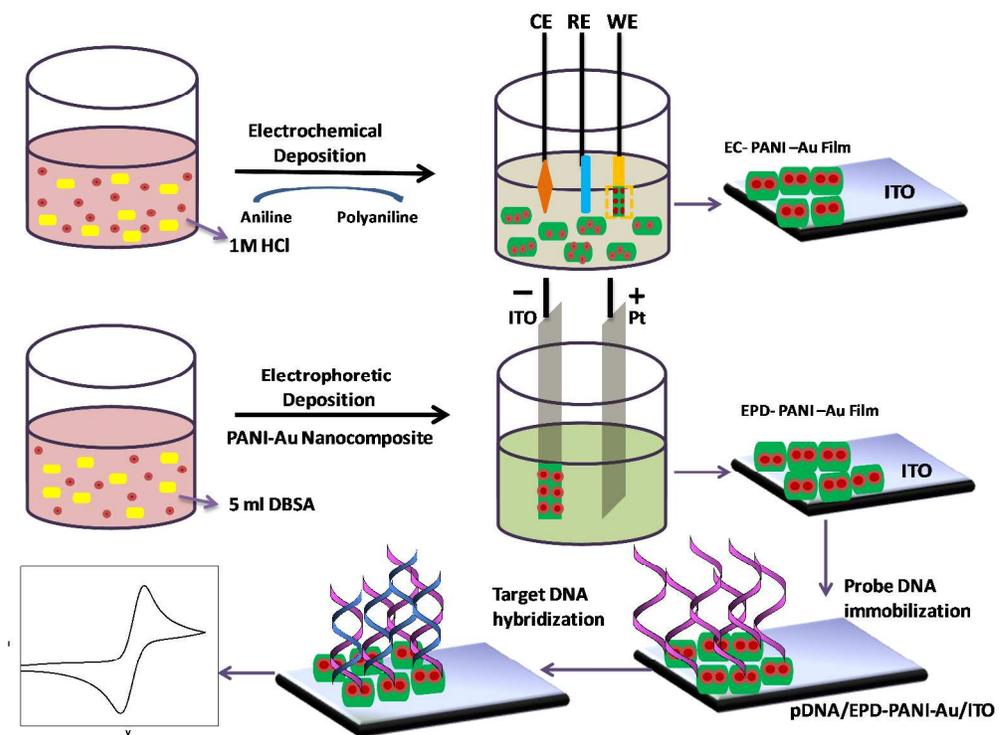


Figure 2.

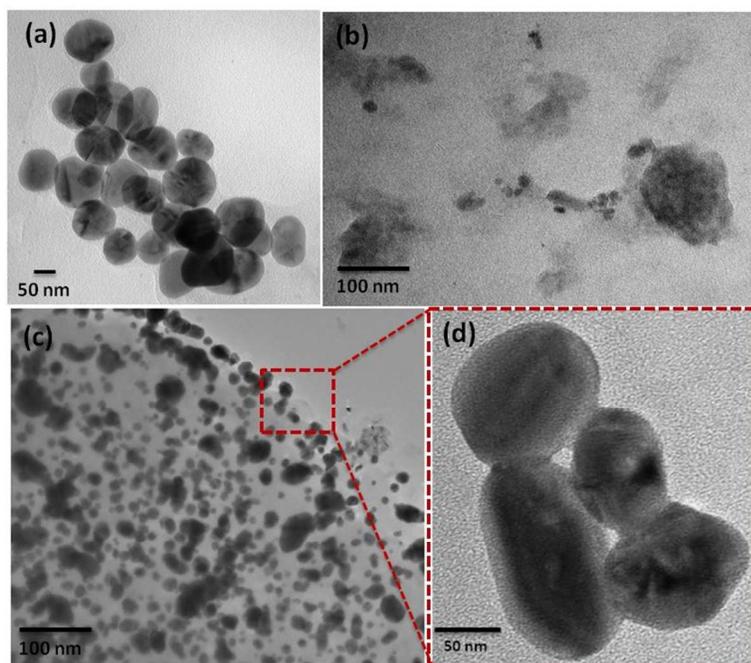


Figure 3.

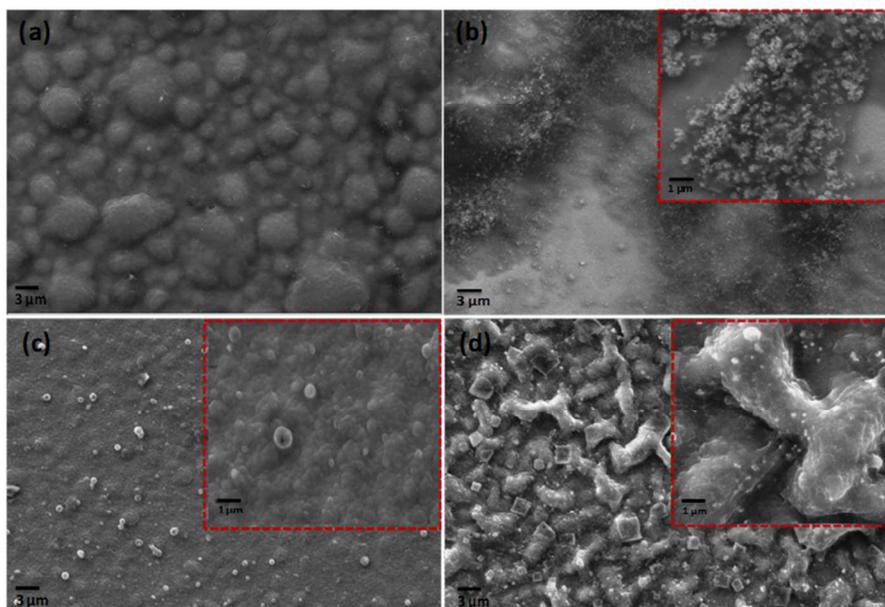


Figure 4.

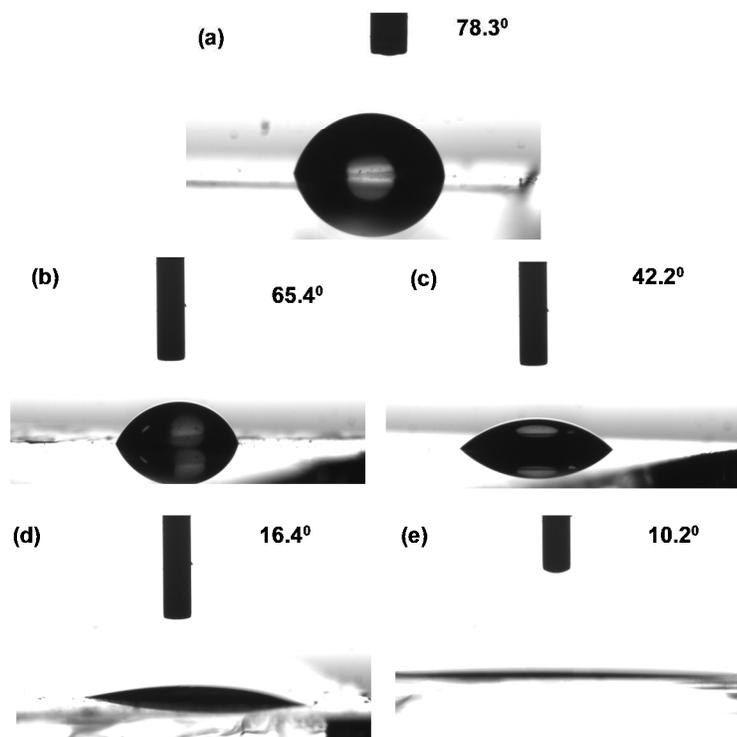


Figure 5.


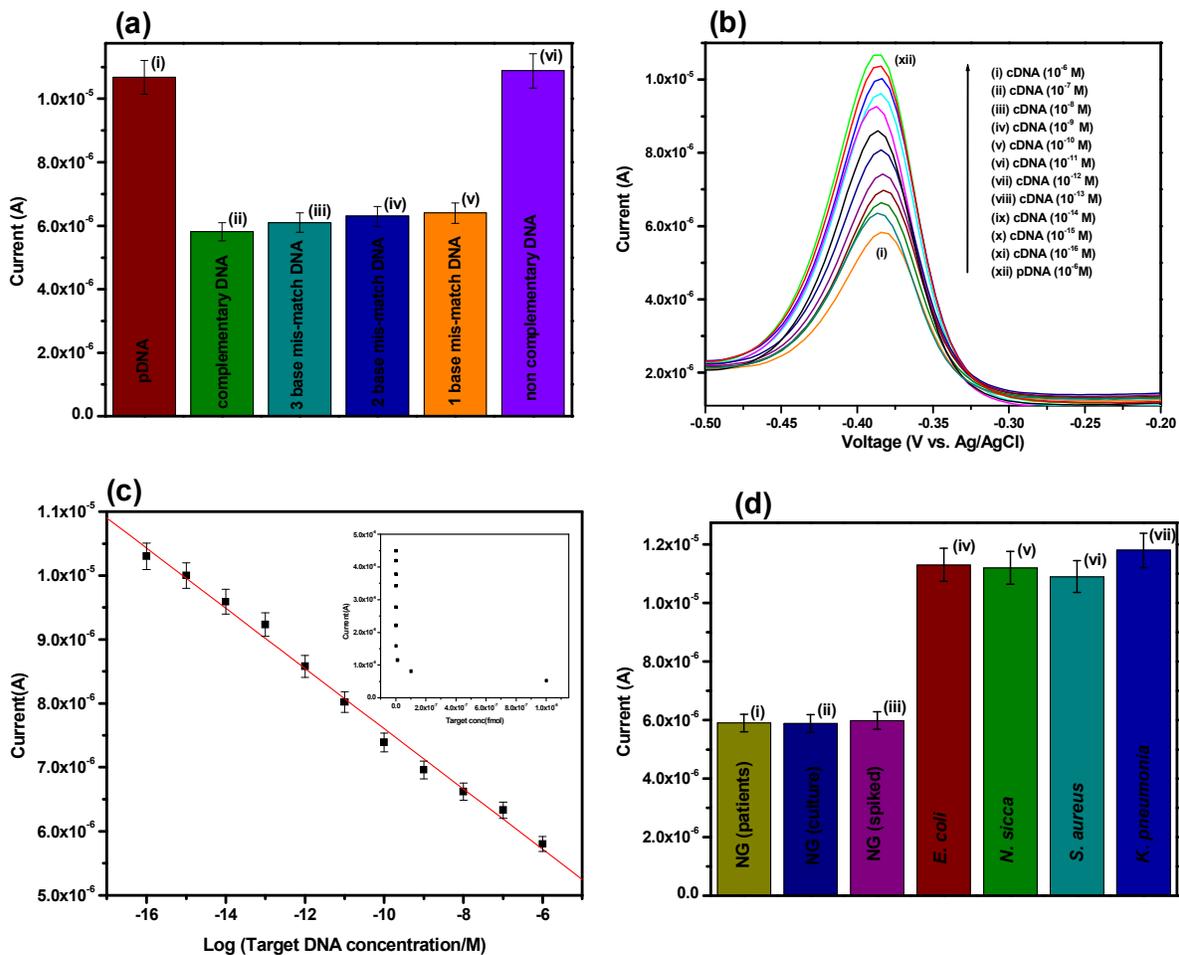


Table T1.

Name of electrode	Electron transfer coefficient, $\alpha$	Charge transfer rate constant, ( $k_s/s^{-1}$ )	Effective surface area, ( $A_{\text{eff}}/\text{mm}^2$ )	Diffusion coefficient, $D(\text{cm}^2\text{s}^{-1})$
EPD-PANI-Au/ITO	0.92	0.0848	0.53	$6.9 \times 10^{-15}$
EC-PANI-Au/ITO	0.85	0.0368	0.48	$2.6 \times 10^{-15}$

Table T2.

S. No.	Electrode	Method of immobilization	Electrochemical technique	Detection limit (M)	Detection range (M)	Hybridization time	References
1.	BdNG-avidin-nsPANI/ITO	Biotin-avidin coupling	DPV, CV	$0.5 \times 10^{-15}$	$1 \times 10^{-16} - 1 \times 10^{-6}$	60 s	37
2.	GCE coating polyaniline nanowire	EDC/NHS	DPV, CV	$1 \times 10^{-12}$	$2.25 \times 10^{-12} - 2.25 \times 10^{-10}$	30 min	42
3.	PANIMWNT/CHIT/CPE	Covalent bonding	EIS, CV	$2.7 \times 10^{-14}$	$1.0 \times 10^{-13} - 1.0 \times 10^{-7}$	40 min	43
4.	PPy-PANi-Au nano composite	Covalent bonding	EIS, CV	$1.0 \times 10^{-13}$	$1 \times 10^{-13} - 1 \times 10^{-6}$	90 min	44
5.	PANIw/graphene/GCE	EDC/NHS	DPV, CV	$3.25 \times 10^{-13}$	$2.12 \times 10^{-12} - 2.12 \times 10^{-6}$	30 min	45
6.	EPD-PANI-Au/ITO	Covalent bonding	DPV, CV	$1 \times 10^{-16}$	$1 \times 10^{-16} - 1 \times 10^{-6}$	60 s	Present work

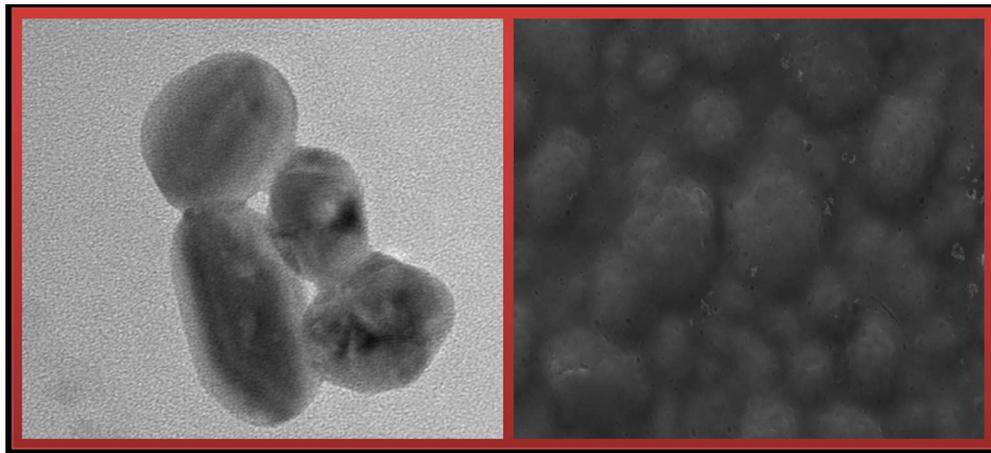

One pot synthesis of polyaniline-gold nanocomposite using chemical route in the presence of dodecyl benzene sulfonic acid.  
210x96mm (150 x 150 DPI)