

RSC Advances



This is an *Accepted Manuscript*, which has been through the Royal Society of Chemistry peer review process and has been accepted for publication.

Accepted Manuscripts are published online shortly after acceptance, before technical editing, formatting and proof reading. Using this free service, authors can make their results available to the community, in citable form, before we publish the edited article. This *Accepted Manuscript* will be replaced by the edited, formatted and paginated article as soon as this is available.

You can find more information about *Accepted Manuscripts* in the [Information for Authors](#).

Please note that technical editing may introduce minor changes to the text and/or graphics, which may alter content. The journal's standard [Terms & Conditions](#) and the [Ethical guidelines](#) still apply. In no event shall the Royal Society of Chemistry be held responsible for any errors or omissions in this *Accepted Manuscript* or any consequences arising from the use of any information it contains.



Advances

ARTICLE

Maximizing Fibroblast Adhesion on Protein-Coated Surfaces Using Microfluidic Cell Printing

S.N. Davidoff^{a,*}, D. Au^{a,*}, B.K. Gale^b, B.D. Brooks^{a,†}, A.E. Brooks^{c,d,†,§}

Received 00th January 20xx,
Accepted 00th January 20xx

DOI: 10.1039/x0xx00000x

www.rsc.org/

Abstract: translation of *in vitro* cell based assays to *in vivo* cellular response is imprecise at best. The advent of three-dimensional cell culture in addition to bioreactor type microfluidics has improved the situation. However, these technical advances cannot be easily combined due to practical limitations. Development of a vertical microfluidic cell printer overcomes this obstacle, providing the ability to more closely recapitulate complex cellular environments and responses. As a proof of concept, we investigated the adhesion of fibroblasts under flow on protein-coated surfaces using a novel vertical microfluidic print head to isolate and manipulate both mechanical and biological factors as a model of fibroblast behavior during the foreign body response following implant insertion. A low flow rate with larger microfluidic channels onto a serum-coated surface has been determined to allow the highest density of viable fibroblasts to attach to the surface. While these insights into fibroblast surface attachment may lead to better material designs, the methods developed herein will certainly be useful as a biomaterials testing platform.

Introduction

Over the last decade the appeal of “lab-on-a-chip” microfluidic devices has increased in relation to their miniaturization, high-throughput capability, and low sample consumption¹. Unfortunately, microfluidic designs have not fulfilled their promise for *in vivo* relevant cellular assays due to their limiting two-dimensional nature, which prevents important three-dimensional cellular contacts, particularly critical in the case of the chronic foreign body response (FBR). Nevertheless, microfluidics offer a valuable *in vitro* tool to study biologically applicable, cellular responses under flow since cells, particularly those attached to implants, are often subjected to flowing biological milieu, such as blood and lymph^{2,3}. Founded on fundamental biological fluid dynamics, the microfluidic printing of cells can determine the attachment strength of cells to different material surfaces^{1,4,5}.

Cellular adhesion is not only altered by the mechanical microenvironment, but also by the composition of the cellular substrate. In the case of an implanted biomedical device, host proteins coat the device surface almost immediately and mediate all cellular interactions, promoting cellular recruitment and adhesion, ultimately masking the underlying

implant surface^{2,6}. The potentially pathological wound healing response that occurs in the presence of an implanted material (i.e., FBR represents a coordinated inflammation cascade directed by responding macrophages that act to recruit host cells, such as fibroblasts, in an organized effort to sequester the implant^{3,7} (Figure 1). Although cellular and surface factors that arbitrate the interactions of macrophages with a foreign material have been well characterized^{6,8–12}, the precise interaction of fibroblasts and a host protein encapsulated foreign material is less understood. Nevertheless, fibroblasts are the primary cell type responsible for matrix deposition; essentially walling off the material from the rest of the body and preventing the full integration of the material or device into the native tissue^{3,13}. An understanding of the integration of fibroblasts in the foreign body response, particularly their attachment to the host proteins that coat the implanted foreign material, is key to the biocompatibility, longevity, and functionality of the medical device³. By manipulating the host protein adlayer and promoting healthy cellular adhesion with native extracellular matrix proteins such as albumin, the device/host tissue interaction can be improved, thereby improving the device functionality, reducing infection⁷, and increasing life-span^{14–17}. Using a vertical flow microfluidics platform, the cell/material interface can be modelled and manipulated to tease apart the cellular attachment to an implant surface while maintaining a more physiologically relevant cellular microenvironment.

As a proof of concept, this article describes the development and utility of a vertical Continuous Flow Microspotter (CFM) to deposit fibroblasts onto various protein-coated (i.e. collagen, fibrinogen, albumin, and serum) surfaces (i.e. tissue culture polystyrene) as a first step in

^a Wasatch Microfluidics, Salt Lake City, UT 84103

^b Department of Mechanical Engineering, University of Utah, Salt Lake, UT 84112

^c Department of Pharmaceutics, University of Utah, Salt Lake City, UT 84112

^d Department of Pharmaceutical Sciences, North Dakota State University, Fargo, ND 58105

* These authors contributed equally to the work.

† These authors are co-senior authors on the work.

§ Corresponding author: amanda.e.brooks@ndsu.edu

developing a simplified, yet FBR relevant, *in vitro* cell culture model. Controlled flow conditions, designed to impose differing shear stress intensity on the fibroblasts were also explored. The vertical flow CFM can better replicate events that take place during the FBR because of the CFM's ability to regulate flow conditions and substrates and provide depth to the cellular model when compared to two-dimensional microfluidic platforms (See Figure 2). Additionally, a vertical print head can alter the printing environment to accommodate different cell lines, such as macrophages and neutrophils, and to recapitulate the complexity of the cellular response in an iterative way. Added complexity can also provide a platform for more relevant morphological studies.

A thorough discussion of the advantages of using vertical printing in a submerged environment has been previously reported¹⁸. Briefly, the CFM allows for the sealing and printing of cellular microarrays onto submerged surfaces in an automated and multiplexed manner. The CFM creates a microfluidic flow cell array (MFCA) when the vertical printhead tip is lowered into a liquid-filled well and subsequently forms a watertight seal on the bottom of the well. Other cell printing technologies, such as pin or ink-jet printers, are not capable of printing in submerged applications. A traditional, two-dimensional flow cell also has limited throughput and only allows for longer cell "spots". Conversely, a vertical, submerged print allows cells to maintain desired phenotypes without disturbing the material surface characteristics. Applications of vertical, submerged-printed, cell microarrays include "drug screening and cytotoxicity assessment in a multitude of areas including cancer, diabetes, inflammation, infections, and cardiovascular disease"¹⁸.

In this work, the versatility of the CFM is used to not only alter the surface, but also the flow rates, tubing size, print head dimensions, and surface contact time (pause time). These parameters are grouped into either mechanical parameters (i.e., tubing size, print head dimensions, print pauses) or biological parameters (i.e., flow rate and surface biology). These five general parameters can also be classified by those that affect shear stress (i.e., tubing size, print head, flow rate) and those that affect cellular adhesion (surface biology, pause times). Using a comprehensive matrix of these mechanical and biological factors, printing conditions that led to the greatest cell density, cellular viability, and adhesion strength were identified as the standard print conditions. Testing various vertical printing conditions with the aforementioned mechanical and biological factors allowed us to determine printing parameters that can (1) produce a high or low cell surface density and (2) build increasingly complex *in vitro* cell culture models with increased throughput and decreased sample consumption.

Results and discussion

Although parameters for planar flow microfluidic cell printing are relatively well established^{19,20}, vertical printing parameters and conditions were explored in an effort to define standard vertical printing parameters to produce a single layer

of fibroblasts with maximal surface area coverage, as well as to tease apart fibroblast adhesion on various proteins. A variety of mechanical (i.e., tubing diameters, print head dimensions, and flow rates) and biological factors (i.e., surface protein coatings, pause times) were considered (Figure 2). Shear stress, average velocity, Reynolds number, and Péclet number were calculated based on the fluid viscosity of DMEM with 10% serum, the diffusion coefficient for fibroblasts in media, the flow rates used, the radius of a fibroblast, and the dimensions of the flow cells in the print head (Table I). Calculation of the Reynolds number indicated that all conditions tested would produce laminar flow ($Re < 2000$). The highest Reynolds number, which fell well below the threshold for turbulent flow, occurred at the highest flow rate used for the 12 channel print head, while the highest shear stress was found for the lowest flow rate considered for the 48 channel print head. Not surprisingly, the Péclet number followed the trend in average velocity, with the highest velocity being achieved in the 48 channel printhead despite the use of the lowest flow rate.

The standard printing condition was determined experimentally to optimize cell density by printing cells on a serum-coated surface at 15 $\mu\text{L}/\text{min}$ flow rate using 250 μm tubing in a 12 channel print head with a 5 minute pause half way through the print to allow adhesion and gravitational settling; therefore, all data were statistically compared to this condition. Importantly, in the absence of the pause time, 43% less cells attached to the serum-coated surface. Tubing diameter and print head dimensions, both mechanical factors, were significantly different than the standard print ($p=0.00016$, $p=0.00038$, respectively), with the standard print providing a significantly higher cell density than prints produced from varying any of the mechanical factors tested in this study (Figure 3). A higher flow rate than the standard print had a significantly lower cell density than the standard print (20 $\mu\text{L}/\text{min}$: $p=0.0016$, 25 $\mu\text{L}/\text{min}$: $p=0.026$, 30 $\mu\text{L}/\text{min}$: $p=0.0025$) as shown in Figure 5. Concurrently, the velocity, and shear stress increased with increasing flow as did the Péclet number. Despite increasing shear rates and velocity, the flow rate, tubing diameter, and print head configuration did not appear to have an effect on the cell morphology as the cells appeared rounded in all cases (Figure 4). Importantly, in the identified "standard print condition" cells appeared to be evenly distributed along the length of the channel while cells were only sparsely distributed in the other conditions.

Collagen was the only surface protein that generated cell densities not significantly different than the standard print ($p=0.0698$). A non-coated surface or coating the surface with fibrinogen or albumin significantly decreased the cell density on the surface.

Experimental

Cell culture

The adherent fibroblast cell line ATCC CRL-1658 NIH/3T3 (3T3) was cultured in Dulbecco's Modified Eagle Medium

(DMEM, Life Technologies) supplemented with 10% fetal bovine serum (FBS, Life Technologies), 1% penicillin-streptomycin (Life Technologies), 1% HEPES buffer (Life Technologies), and 1% sodium pyruvate (Life Technologies). 3T3 cells with a maximum passage number of 25 were cultured to 70-80% confluence before experimental use. The cells were cultured at 37°C with 5% CO₂.

Microfluidic cell printing

3T3 cells were printed at 50,000 cells/mL in complete DMEM (described above) using a modified version of the vertical Continuous Flow Microspotter (CFM, Wasatch Microfluidics)²¹ that allows for submerged printing¹. The printer was modified to minimize the amount of tubing the cells contact before reaching the surface. The CFM uses a 24 channel peristaltic pump (Ismatec, Switzerland) to pull the cells through the system, from a well plate, to the surface and then to waste (Figure 2). Conditions were changed one at a time to isolate the factors that change shear stress, cellular adhesion, cellular density, and cellular viability. A 1x12 (12) channel print head, with flow cell surface area 5.8 mm² and a 6x8 (48) channel print head, with flow cell surface area 0.43 mm² were tested. Exchanging the Tygon® tubing diameter between 250 µm and 500 µm modified the shear stress. Printing cells on serum, albumin, collagen, and fibrinogen provided an evaluation of the effect of surface coating on cellular adhesion.

Reynolds Number

The Reynolds number, which is an indicator of the type of flow, laminar or turbulent, and the relative effects of inertia, was calculated for a rectangular flow according to the following equation:

$$\frac{Q\rho}{(W+H)\mu} \quad [Equation 1]$$

where Q , in m³/s, is the flow rate, ρ is the density of the media, μ is the viscosity of the media (0.007 g/cm/s), W (m) is the width (1 mm for the 12 channel print head and 0.51 mm for the 48 channel print head) and H (m) is the height of the rectangular channel (300 µm for the 12 channel print head and 250 µm for the 48 channel print head). The density and viscosity were taken from reported literature values, for DMEM with 10% FBS: ρ is 1.007 g/mL and η is 1.011 Pa*s²².

Péclet Number

The Péclet number, which is the ratio of advective over diffusional mass transport in a flow displacement system, was calculated according to the following equation:

$$\frac{3vR^3}{2(H/2)^2D} \quad [Equation 2]$$

where the radius (R) of a fibroblast was 9×10^{-6} meters, the diffusion coefficient (D) of a fibroblast in media was 10^{-10}

m²/sec¹⁹, and average velocity (v) was calculated as shown in Table I.

Shear Stress and Average Velocity

Shear stress was calculated using:

$$\mu \left(\frac{6Q}{H^2W} \right) \quad [Equation 3]$$

where μ is the viscosity of the media (0.0007 g/cm/s), and Q is the volume flow rate ($WH^2 = 0.00009$ cm³ for the 12 channel print head and 0.000032 cm³ for the 48 channel print head)²³.

Protein surface coating

Albumin, collagen, fibrinogen, and serum were all pipetted onto the surfaces of tissue culture treated polystyrene 12 well dishes. Each spot contained 100 µL of the protein solution. Serum was used undiluted. Albumin, collagen, and fibrinogen were all pipetted onto the surface at a concentration of 0.5 mg/mL. Protein coated plates were allowed to dry in a biosafety hood overnight. Collagen coated dishes were rinsed before use to remove any residual acid. The collagen dishes were rinsed for 10 minutes with phosphate buffered saline followed by two rinses with distilled water. Protein coated dishes were stored at 4°C for no more than one week before use.

Cell imaging and analysis

Cells were imaged using a Leica DM IL LED microscope (Leica Microsystems) with Leica Application Suite imaging software (Leica Microsystems). Trypan blue was used at 0.1% concentration to stain the cells (Life Technologies). Images were taken at 10X magnification for cell density calculations and morphology assessment using a Leica DMIL LED Fluor (Leica, USA). ImageJ 64 software (NIH) was used to analyse the images using the cell counter plug-in.

Statistical Analysis

A one-way ANOVA was performed using Microsoft Excel to compare each condition back to the standard print (12 channel print head with 250 µm tubing over a serum coated surface, flowing at 15 µL/min with a 5 minute pause time half way through the print and at the end of the print). Experiments were performed in triplicate.

Conclusions

The foreign body response continues to plague the ever-increasing market of biomedical devices. Thus, efforts to mitigate the foreign body response have been primarily materials focused, using biocompatible coatings fabricated from man-made and natural-derived polymers, including collagen and albumin^{2,14,24-27}. Unfortunately, material improvements are often frustrated by incongruent responses between *in vitro* and *in vivo* assays. The biocompatibility of a

material cannot be fully evaluated by a single test or method, and endpoint assays for determining the potential compatibility are time intensive and costly^{28–31}.

Although many events of FBR related fibroblast adhesion are known from previous surface micro-patterning, lateral 2-D printing, and parallel plate flow chamber techniques^{1,4,23,32–35}, the submerged microfluidic printing technology described herein provides a more accurate model of cellular material interactions that occur at the surface under shear flow conditions. The vertical, submerged microfluidic cell printing technology described here is ideal for creating a viable printing condition that allows cells direct access to the designated surface and can iteratively build complexity into the model; whereas, other technologies utilize lateral two dimensional print conditions and orient cell flow parallel to the designated surface, inadvertently increasing cell contact with the tubing and detracting from the desired surface interactions. Microfluidic lateral flow devices also impose shear stress more focused on the adhesive edges, potentially skewing the interpretation of the results. The orientation of the vertical flow channels with respect to the printing substrate allows additional cell-surface contact due to inlets and outlets that are oriented perpendicular to the print surface. The vertical, submerged CFM utilizes this design to allow additional cell-surface exposure from the vertical columns of liquid in the inlets and outlets on top of cells that make contact within the actual flow channel (Figure 7). This allows a greater depth of cell diffusion through the medium and onto the designated substrate, providing a printing advantage that other devices do not have. The vertical design can also be used to create complex layered structures in future studies. While various applications of surface micro-patterning are limited by the real-time analysis of the printing process^{33–35}, the microfluidic printing technology described herein utilizes a microscope objective aligned with the print surface, allowing real-time analysis of the process. A parallel plate flow chamber is an often used and validated model for determining cell adhesion³²; however, cellular interactions constrained by two material surfaces may not be an appropriate model for many FBR cell adhesion measurements in which cells directly experience unrestrained differential flow based on their relative location to the device surface. The ability to interrogate cellular interactions under continuous flow over time represents a distinct advantage of the described vertical microfluidic printing device, which is able to create a reversible seal on a wet or dry surface¹⁹. While there are other assays designed to assess cellular adhesion in relation to FBR, utilizing a microfluidics approach, in which the model surface could be patterned with multiple coatings, offers a tool for biomaterials testing that (1) increases throughput through isolated channels, (2) decreases reagent consumption and the associated costs, and (3) offers a more relevant platform for in vitro biomaterials testing when compared to other techniques (e.g., 2D printing, parallel plate flow chambers for bacteria, surface micro-patterning, etc.)^{1,4,5,32,36}. Increased throughput leads not only to condition scouting experiments to determine cellular adhesion as an indication of the FBR, but also allows

replicate assays to be performed at a reduced cost and monitored in real time on a feasible time scale. As opposed to various 2D microfluidic approaches, cells are provided direct access to protein-coated surfaces due to the surface perpendicular flow direction (Figure 7).

Since microfluidic devices provide flowing conditions, factors that affect cell adhesion, such as shear stress, flow rate, and surface topography, can be explored³⁴. Notably, shear stress in the blood vessel ranges from 1 dyn/cm² to 15 dyn/cm²^{37,38}; however the flow rate at the interface of a device is considerably less; thus, the shear stress rates utilized here were about 1/10 of the lowest physiological vascular shear rate to provide the greatest cell density (Table 1). Adhesive force represents the integration of shear stress from flow as well as the force of cellular adhesion to the surface. Several recent studies have emphasized the importance of the surface, particularly the protein composition of the surface, as a primary mediator of cellular adhesion, retention, proliferation, and differentiation^{34,39–43}. In fact, in certain systems using jet impingement to determine cellular adhesion strength, collagen, a major component of the extracellular matrix, provides the most adherent surface¹. This corresponds well with our observed results with a collagen-coated surface. The specific complement of cellular adhesion molecules cannot be underestimated in these assays. Cell-cell interactions during the printing process cannot be completely eliminated as contributing to the observed cellular density and certain substrate protein coatings led to more clumped cells (data not shown); however, single cell thickness prints were obtained through optimizing the cell confluency and seeding density. Future efforts to adapt and validate the jet impingement technique to the CFM system described will provide additional insight into cell-material interactions.

Because of the novelty and advantages of a submerged and vertical microfluidic print head, relevant flow and stress calculations have not previously been reported. Although many of the altered parameters had an effect on the calculated values for flow and other numerical values that describe cellular adhesion, altering the print head had the most interesting effect, likely due to the different channel dimensions (12 channel: width = 1 mm, length = 6 mm, height = 0.3 mm; 48 channel: width = 0.51 mm, length = 0.85 mm, height = 0.25 mm), which increased shear stress and velocity (Table 1). Using cell density, shear stress, and velocity, a standard print condition (12 channel print head with 250 μ m tubing and a flow rate of 15 μ L/min) was defined in this study. Minimizing the shear stress and velocity under laminar flow, such as under the standard print condition, was hypothesized to increase the time that the cells were in contact with the surface. The 12 channel print head has a surface area of 5.843 mm², providing maximum surface area for cell attachment to occur when compared to the 48 channel print head with flow cells having an area of 0.43 mm². Increasing cell-surface contact time is mirrored in the use of the lowest flow rate, 15 μ L/min, increasing the number of cells on the surface. Trypsinization of the fibroblast cells creates a suspension medium for the microfluidic device, and is likely the reason for

the rounding of the cells in the initial printing period. The initial adhesion of fibroblast cells from a suspension has been observed to be approximately 5 minutes, while full adhesion onto a surface is dependent on the culture environment, but is commonly observed to be over 30 minutes⁴⁴. This is believed to be the reason why printed fibroblast cells, when imaged, appear rounded, but still attach to the surface. Cell distention cannot be excluded as an additional factor to increase adhesion¹; however, based on the roundness of the imaged cells, this effect was thought to be negligible. This was likely due to more uniform shear stresses imposed on the cell during vertical printing.

Future work may better integrate immunohistochemistry for cell surface receptors in conjunction with jet impingement methods modified for vertical microfluidic systems to calculate the adhesive strength of the cells attributed to the presence of certain integrin receptors. Additionally, future work will include looking into other biologically relevant proteins, such as fibronectin, that have been shown to change the adhesion and cytoskeletal organization of fibroblasts⁵². It will also be important to expand the cell printing system discussed in this paper to a co-culture system of macrophages and fibroblasts (as they are both key to the foreign body response^{53–55}) and image prints over time. The microfluidics platform described may significantly impact our study of the FBR, particularly in relation to the “race for the surface”⁵⁵.

Acknowledgements

The authors would like to thank the NIH funding support received from grant number 1R43CA177146-01A1. The authors would also like to acknowledge Dr. David Grainger (Pharmaceutics and Pharmaceutical Chemistry, University of Utah) for the use of his lab space.

Conflict of Interest Statement

Sherry Davidoff, David Au, and Benjamin Brooks are employees of Wasatch Microfluidics. Bruce Gale has a financial interest in Wasatch Microfluidics.

Notes and references

- X. Zhang, P. Jones and S. J. Haswell, *Chem. Eng. J.*, 2008, 135, Supplement 1, S82–S88.
- J. M. Morais, F. Papadimitrakopoulos and D. J. Burgess, *AAPS J.*, 2010, 12, 188–196.
- J. M. Anderson, A. Rodriguez and D. T. Chang, *Semin. Immunol.*, 2008, 20, 86–100.
- C. Visser, M. Gielen, Z. Hao, S. Le Gac, D. Lohse and C. Sun, *Biophys. J.*, 108, 23–31.
- H. Busscher and H. Van Der Mei, *Clin. Microbiol. Rev.*, 2006, 19, 127–141.
- J. M. Anderson, in *Biological Interactions on Materials Surfaces*, eds. D. A. Puleo and R. Bizios, Springer US, 2009, pp. 225–244.
- B. D. Brooks, A. E. Brooks and D. W. Grainger, in *Biomaterials Associated Infection*, eds. T. F. Moriarty, S. A. J. Zaat and H. J. Busscher, Springer New York, 2013, pp. 307–354.
- D. T. Luttkhuizen, M. C. Harmsen and M. J. V. Luyn, *Tissue Eng.*, 2006, 12, 1955–1970.
- S. MacLauchlan, E. A. Skokos, N. Meznarich, D. H. Zhu, S. Raoof, J. M. Shipley, R. M. Senior, P. Bornstein and T. R. Kyriakides, *J. Leukoc. Biol.*, 2009, 85, 617–626.
- R. J. Schutte, A. Parisi-Amon and W. M. Reichert, *J. Biomed. Mater. Res. A*, 2009, 88, 128–139.
- S. M. van Putten, D. T. A. Ploeger, E. R. Popa and R. A. Bank, *Acta Biomater.*, 2013, 9, 6502–6510.
- D. Diekjiirgen, A. Astashkina, D. W. Grainger, D. Holt and A. E. Brooks, *J. Biomater. Sci. Polym. Ed.*, 2012, 23, 1231–1254.
- J. R. Anderson, D. T. Chiu, R. J. Jackman, O. Cherniavskaya, J. C. McDonald, H. Wu, S. H. Whitesides and G. M. Whitesides, *Anal. Chem.*, 2000, 72, 3158–3164.
- B. Ratner, A. Hoffman, F. Schoen and J. Lemons, in *Biomaterials science: an introduction to materials in medicine*, Elsevier, San Diego, 2nd edn., pp. 67–127.
- N. Wisniewski and M. Reichert, *Colloids Surf. B Biointerfaces*, 2000, 18, 197–219.
- V. P. Shastri, *Curr. Pharm. Biotechnol.*, 2003, 4, 331–337.
- M. Shen and T. A. Horbett, *J. Biomed. Mater. Res.*, 2001, 57, 336–345.
- S. N. Davidoff, A. R. Miles, V. Romanov, B. K. Gale, J. W. Eckman and B. D. Brooks, *J. Vis. Exp. JoVE*, 2014.
- S. N. Davidoff, D. Au, S. Smith, A. E. Brooks and B. D. Brooks, *Biomed. Sci. Instrum.*, 2015, 51, 24–30.
- S. N. Davidoff, K. L. Stallings, A. E. Brooks, B. K. Gale and B. D. Brooks, *Biomed. Sci. Instrum.*, 2015, 51, 17–23.
- S. Natarajan, P. S. Katsamba, A. Miles, J. Eckman, G. A. Papalia, R. L. Rich, B. K. Gale and D. G. Myszk, *Anal. Biochem.*, 2008, 373, 141–146.

- 22 P. M. Hinderliter, K. R. Minard, G. Orr, W. B. Chrisler, B. D. Thrall, J. G. Pounds and J. G. Teeguarden, *Part. Fibre Toxicol.*, 2010, 7, 36.
- 23 J. Hu, C. Hardy, C.-M. Chen, S. Yang, A. S. Voloshin and Y. Liu, *PLoS ONE*, 2014, 9, e104502.
- 24 A. L. Nelson and J. M. Reichert, *Nat. Biotechnol.*, 2009, 27, 331–337.
- 25 K. Fujioka, M. Maeda, T. Hojo and A. Sano, *Adv. Drug Deliv. Rev.*, 1998, 31, 247–266.
- 26 M. Geiger, R. H. Li and W. Friess, *Adv. Drug Deliv. Rev.*, 2003, 55, 1613–1629.
- 27 H.-Y. Cheung, K.-T. Lau, T.-P. Lu and D. Hui, *Compos. Part B Eng.*, 2007, 38, 291–300.
- 28 A. Pizzoferrato, G. Ciapetti, S. Stea, E. Cenni, C. R. Arciola, D. Granchi and Lucia, *Clin. Mater.*, 1994, 15, 173–190.
- 29 B. D. R. S. H. J. S. E. Lemons, Ed., in *Biomaterials Science (Third Edition)*, Academic Press, 2013, pp. 587–588.
- 30 C. J. Kirkpatrick, F. Bittinger, M. Wagner, H. Köhler, T. G. van Kooten, C. L. Klein and M. Otto, *Proc. Inst. Mech. Eng. [H]*, 1998, 212, 75–84.
- 31 C. J. Kirkpatrick, K. Peters, M. I. Hermanns, F. Bittinger, V. Krump-Konvalinkova, S. Fuchs and R. E. Unger, *ITBM-RBM*, 2005, 26, 192–199.
- 32 W. O. Lane, A. E. Jantzen, T. A. Carlon, R. M. Jamiolkowski, J. E. Grenet, M. M. Ley, J. M. Haseltine, L. J. Galinat, F.-H. Lin, J. D. Allen, G. A. Truskey and H. E. Achnack, *J. Vis. Exp.*, 2012.
- 33 Y. Ito, *Biomaterials*, 1999, 20, 2333–2342.
- 34 T. F. Didar and M. Tabrizian, *Lab. Chip*, 2010, 10, 3043–3053.
- 35 M. E. Moustafa, V. S. Gadepalli, A. A. Elmak, W. Lee, R. R. Rao and V. K. Yadavalli, *J. Biol. Eng.*, 2014, 8, 24.
- 36 S. Mittal, I. Y. Wong, W. M. Deen and M. Toner, *Biophys. J.*, 2012, 102, 721–730.
- 37 P. Nigro, J. Abe and B. C. Berk, *Antioxid. Redox Signal.*, 2011, 15, 1405–1414.
- 38 J. M. Barnes, J. T. Nauseef and M. D. Henry, 2012.
- 39 R. Gristina, E. D'Aloia, G. S. Senesi, A. Milella, M. Nardulli, E. Sardella, P. Favia and R. d'Agostino, *J. Biomed. Mater. Res. B Appl. Biomater.*, 2009, 88B, 139–149.
- 40 J. Shaikh-Mohammed, M. Li, D. Terala and M. J. McShane, 2004, vol. 5345, pp. 43–50.
- 41 K. W. Kwon, S. S. Choi, S. H. Lee, B. Kim, S. N. Lee, M. C. Park, P. Kim, S. Y. Hwang and K. Y. Suh, *Lab. Chip*, 2007, 7, 1461–1468.
- 42 E. W. K. Young, A. R. Wheeler and C. A. Simmons, *Lab. Chip*, 2007, 7, 1759–1766.
- 43 C. Yan, J. Sun and J. Ding, *Biomaterials*, 2011, 32, 3931–3938.
- 44 J. Albuschies and V. Vogel, *Sci. Rep.*, 2013, 3.
- 45 C. A. Buck and A. F. Horwitz, *Annu. Rev. Cell Biol.*, 1987, 3, 179–205.
- 46 L. Koivisto, J. Heino, L. Häkkinen and H. Larjava, *Adv. Wound Care*, 2014, 3, 762–783.
- 47 E. Tamariz and F. Grinnell, *Mol. Biol. Cell*, 2002, 13, 3915–3929.
- 48 E. Bell, B. Ivarsson and C. Merrill, *Proc. Natl. Acad. Sci.*, 1979, 76, 1274–1278.
- 49 A. K. Harris, D. Stopak and P. Wild, *Nature*, 1981, 290, 249–251.
- 50 F. Grinnell, *J. Cell Biol.*, 1994, 124, 401–404.
- 51 J. J. Tomasek, G. Gabbiani, B. Hinz, C. Chaponnier and R. A. Brown, *Nat. Rev. Mol. Cell Biol.*, 2002, 3, 349–363.
- 52 A. Woods, J. R. Couchman, S. Johansson and M. Höök, *EMBO J.*, 1986, 5, 665–670.
- 53 D. J. Holt, L. M. Chamberlain and D. W. Grainger, *Biomaterials*, 2010, 31, 9382–9394.
- 54 G. Voskerician and J. M. Anderson, in *Wiley Encyclopedia of Biomedical Engineering*, John Wiley & Sons, Inc., 2006.
- 55 A. Gristina, *Science*, 1987, 237, 1588–1595.

Figure Legends

Figure 1. Steps of the host foreign body response following the implantation of a device/foreign material from both the tissue perspective (yellow) and the biomaterial (blue). Notice that the exudate tissue and the biomaterial interface are intimately connected.

Figure 2. Schematic of the cell printing set-up including the various parameters tested to determine the effects of mechanical and biological factors on fibroblast attachment.

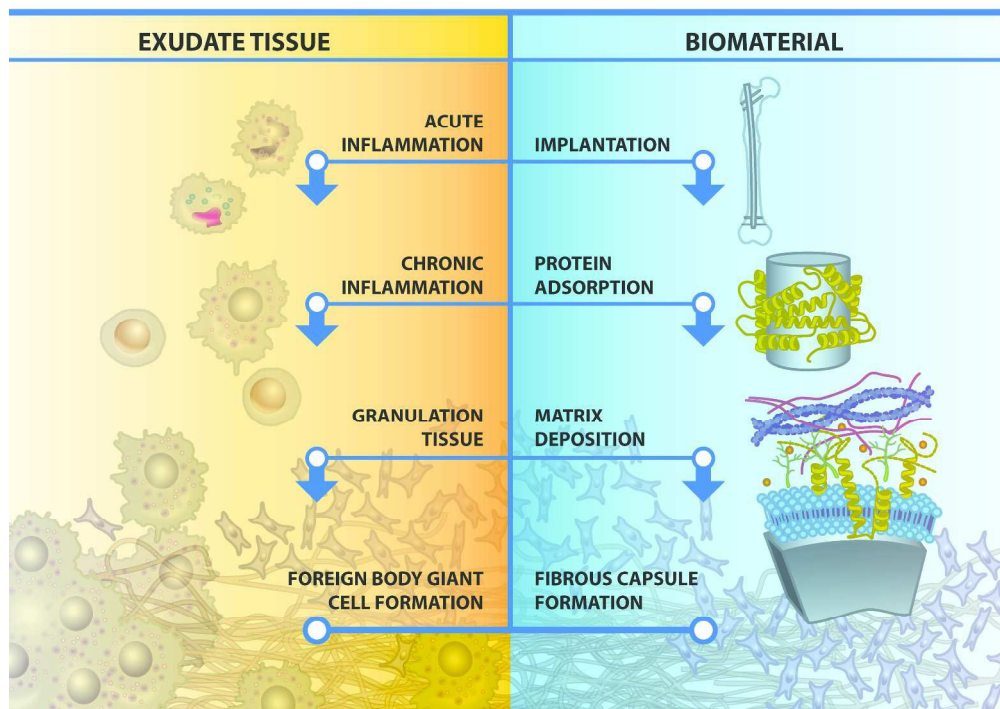
Figure 3. Comparison of cell density for printed fibroblasts varying mechanical factors (tubing diameter, print head dimensions, and flow rate) that affect cell attachment. An asterisk indicates statistical significance using a one-way ANOVA ($p < 0.05$).

Figure 4. 10X magnification microscope images with 200 μm scale bars to compare the cell density and morphology of mechanical factors that affect cell attachment: A) standard print, B) 500 μm tubing, C) 20 $\mu\text{L}/\text{min}$, D) 25 $\mu\text{L}/\text{min}$, and E) 30 $\mu\text{L}/\text{min}$ flow rates.


Figure 5. Comparison of cell density for printed fibroblasts varying biological factors (pause time and surface coating) that affect cell attachment. An asterisk indicates statistical significance using a one-way ANOVA ($p < 0.05$).

Figure 6. 10X magnification microscope images with 200 μm scale bars to compare the cell density and morphology of biological factors that affect cell attachment: A) standard print, B) pause time, C) bare tissue culture surface, D) collagen, E) fibrinogen, and F) albumin coated surfaces.

Figure 7. Cells are provided direct access to protein-coated surfaces due to the flow direction being perpendicular to the surface.

INJURY IMPLANTATION

278x218mm (300 x 300 DPI)

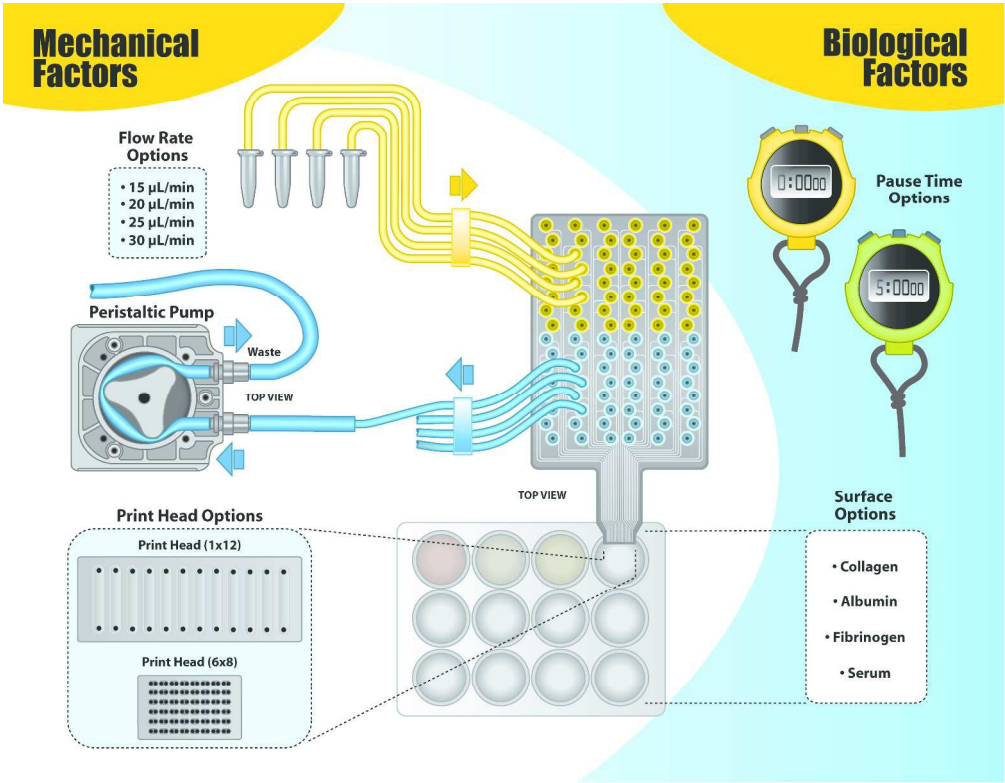

285x222mm (300 x 300 DPI)

Comparison of Mechanical Factors Affecting Cell Attachment

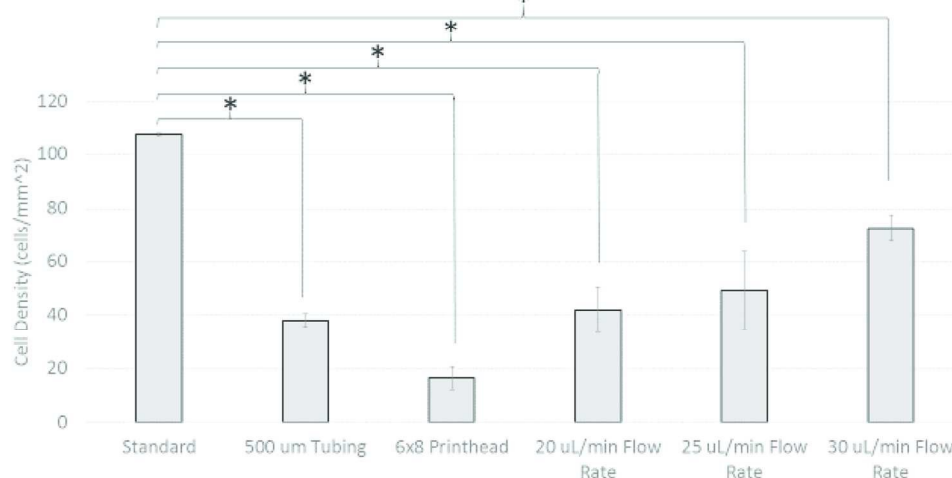


Figure 3. Comparison of cell density for printed fibroblasts varying mechanical factors (tubing diameter, print head dimensions, and flow rate) that affect cell attachment. An asterisk indicates statistical significance using a one-way ANOVA ($p < 0.05$).

152x107mm (300 x 300 DPI)

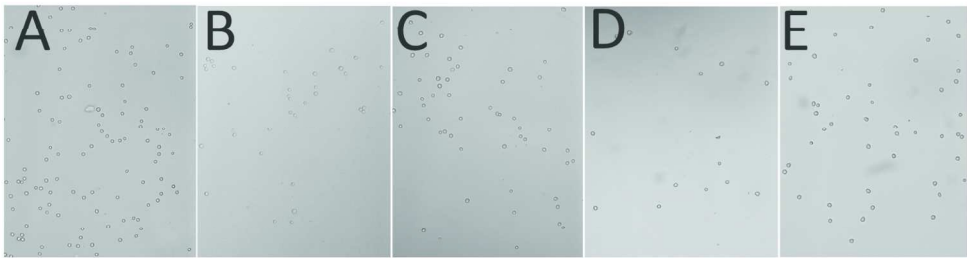


Figure 4. 10X magnification microscope images with 200 μm scale bars to compare the cell density and morphology of mechanical factors that affect cell attachment: A) standard print, B) 500 μm tubing, C) 20 $\mu\text{L}/\text{min}$, D) 25 $\mu\text{L}/\text{min}$, and E) 30 $\mu\text{L}/\text{min}$ flow rates.

171x85mm (300 x 300 DPI)


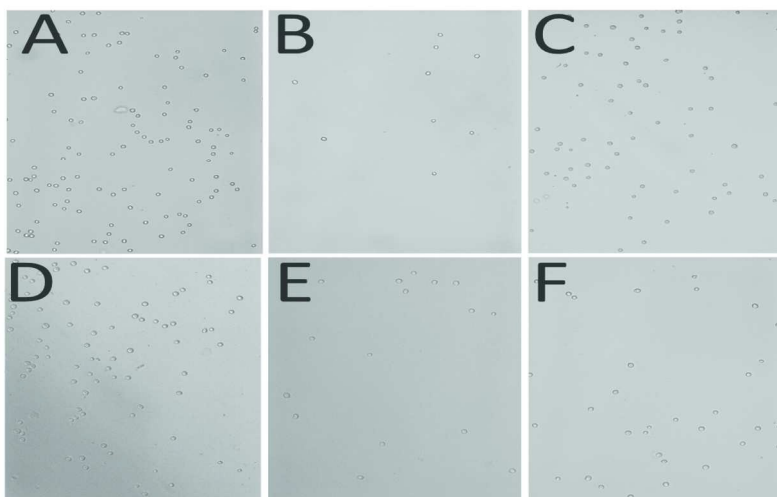


Figure 6. 10X magnification microscope images with 200 μm scale bars to compare the cell density and morphology of biological factors that affect cell attachment: A) standard print, B) pause time, C) bare tissue culture surface, D) collagen, E) fibrinogen, and F) albumin coated surfaces.

171x120mm (300 x 300 DPI)

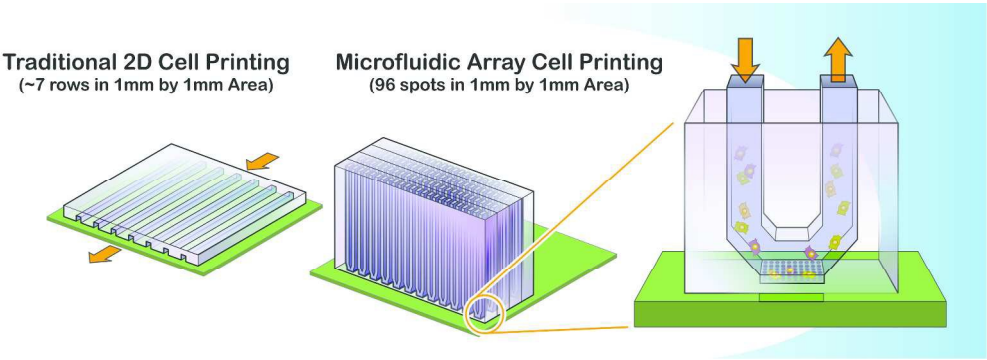

287x101mm (300 x 300 DPI)

Flow Rate (Q)	Print head	Surface coating	Velocity (m/sec) $Q/(w \cdot h)$	Shear Stress (dyn/cm ²) $\mu \cdot ((6Q)/(w \cdot h))$	Reynolds Number $Q\rho/(w+h)\eta$	Péclet Number $(3 \cdot v \cdot R_b^3)/2(h_0/2)^2 D$
15µl/min	12 channel	Serum	0.00083	0.12	$1.92 \cdot 10^{-7}$	$4.05 \cdot 10^{-11}$
20µl/min	12 channel	Serum	0.00111	0.16	$2.55 \cdot 10^{-7}$	$5.40 \cdot 10^{-11}$
25µl/min	12 channel	Serum	0.00139	0.19	$3.19 \cdot 10^{-7}$	$6.75 \cdot 10^{-11}$
30µl/min	12 channel	Serum	0.00167	0.23	$3.83 \cdot 10^{-7}$	$8.10 \cdot 10^{-11}$
15µl/min	48 channel	Serum	0.00196	0.33	$3.28 \cdot 10^{-7}$	$1.37 \cdot 10^{-10}$

Table I. Calculated parameters for the different flow rates utilized.

$\mu = 0.007$ g/cm/sec; $\rho = 1.007$ g/ml; $\eta = 1.011$ Pa*s; $R_b = 9 \cdot 10^{-6}$; $D = 1 \cdot 10^{-9}$