



Accuracy of methods for reporting inorganic element concentrations and radioactivity in oil and gas wastewaters from the Appalachian Basin, U.S. based on an inter-laboratory comparison

Journal:	<i>Environmental Science: Processes & Impacts</i>
Manuscript ID	EM-ART-08-2018-000359.R2
Article Type:	Paper
Date Submitted by the Author:	09-Oct-2018
Complete List of Authors:	<p>Tasker, Travis; The Pennsylvania State University, Civil and Environmental Engineering Burgos, Bill; Pennsylvania State University, Ajemigbitse, Moses; Penn State, Lauer, Nancy; Duke University, Nicholas School of the Environment Gusa, Alen; University of Pittsburgh, Department of Civil and Environmental Engineering Kuatbek, Maksat; The Pennsylvania State University, Department of Mechanical and Nuclear Engineering May, Dustin; University of Iowa Landis, Joshua; Dartmouth College Alessi, Daniel; University of Alberta, Earth and Atmospheric Sciences Johnsen, Amanda; The Pennsylvania State University, Radiation Science and Engineering Center Kaste, James; The College of William & Mary, Department of Geology Headrick, Kurt; Maxxam Analytics Wilke, Franziska D. H.; Helmholtz Ctr Potsdam McNeal, Mark; ACZ Laboratories Engle, Mark; USGS Jubb, Aaron; USGS Vidic, Radisav; University of Pittsburgh, Radisav Vidic; Radisav Vidic, Radisav Vidic Vengosh, Avner; Duke University, Nicholas School of the Environment Warner, Nathaniel; Penn State, CEE; Penn State CEE</p>

1
2
3 **Accuracy of methods for reporting inorganic element concentrations and radioactivity in**
4 **oil and gas wastewaters from the Appalachian Basin, U.S. based on an inter-laboratory**
5 **comparison**
6
7

8
9 **Significance Statement**

10 Accurate analyses are important for regulating oil and gas (O&G) development and tracing
11 potential contamination events. In this work, an inter-laboratory comparison among commercial and
12 academic labs revealed that reported radioactivity and trace metal concentrations (i.e., Ra, Cr, Ni, Cu, Zn,
13 As, Cd, and Pb) in O&G wastewaters can be over $\pm 40\%$ different from the most probable value (MPV).
14
15 Out of all the analytes measured in this study, reported ^{226}Ra activities—a known carcinogen—were the
16 most inconsistent and ranged by approximately 200% for a single sample. This variability in reported Ra
17 activities could influence how the wastewaters are managed or identified in the environment, warranting
18 further attention and research. We propose that the variable Ra activities could be due to calibration
19 inconsistencies among labs, radon leakage, or failure to account for self-attenuation. Future work is
20 necessary to develop standard methods and reference materials for Ra analyses of O&G wastewaters.
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

1
2
3 **Accuracy of methods for reporting inorganic element concentrations and radioactivity in**
4 **oil and gas wastewaters from the Appalachian Basin, U.S. based on an inter-laboratory**
5 **comparison**
6

7
8 Tasker, T.L.^{a*}, Burgos, W.D.^a, Ajemigbitse, M.A.^a, Lauer, N.E.^b, Gusa, A.V.^c, Kquatbek, M.^{d,e},
9 May, D.^f, Landis, J.D.^g, Alessi, D.S.^h, Johnsen, A.M.^d, Kaste, J.M.ⁱ, Headrick, K.^j, Wilke,
10 F.D.H.^k, McNeal, M.^l, Engle, M.^m, Jubb, A.M.^m, Vidic, R.^c, Vengosh, A.^b, Warner, N.R.^a
11

12 ^aDepartment of Civil and Environmental Engineering, The Pennsylvania State University, 212 Sackett
13 Building, University Park, Pennsylvania 16802, United States
14

15 ^bDivision of Earth and Ocean Sciences, Nicholas School of the Environment, Duke University, Durham,
16 North Carolina 27708, United States
17

18 ^cDepartment of Civil and Environmental Engineering, University of Pittsburgh, Pittsburgh, Pennsylvania
19 15213, United States
20

21 ^dRadiation Science and Engineering Center, The Pennsylvania State University, 101 Breazeale Nuclear
22 Reactor, University Park, Pennsylvania 16802, United States
23

24 ^eDepartment of Mechanical and Nuclear Engineering, The Pennsylvania State University, 137 Reber
25 Building, University Park, Pennsylvania, 16802, United States
26

27 ^fState Hygienic Laboratory, University of Iowa, 2490 Crosspark Road, Coralville, Iowa 52241, United
28 States
29

30 ^gDepartment of Earth Sciences, Dartmouth College, 6105 Fairchild Hall, Hanover, New Hampshire
31 03755, United States
32

33 ^hDepartment of Earth and Atmospheric Sciences, University of Alberta, 1-26 Earth Sciences Building,
34 Edmonton, Alberta T6G 2E3, Canada
35

36 ⁱDepartment of Geology, The College of William & Mary, Williamsburg, Virginia 23185, United States
37

38 ^jMaxxam Analytics, 6790 Kitimat Road, Unit 4, Mississauga, Ontario L5N 5L9, Canada
39

40 ^kHelmholtz Centre Potsdam – German Centre for Geosciences (GFZ), Telegrafenberg, Potsdam 14473,
41 Germany
42

43 ^lACZ Laboratories, Inc., 2773 Downhill Drive, Steamboat Springs, Colorado 80487, United States
44

45 ^mU.S. Geological Survey, 12201 Sunrise Valley Drive, Reston, Virginia 20192, United States
46

47
48
49
50
51
52 *Corresponding author
53
54
55
56
57
58
59
60

Abstract

Accurate and precise analyses of oil and gas (O&G) wastewaters and solids (e.g., sediments and sludge) are important for the regulatory monitoring of O&G development and tracing potential O&G contamination in the environment. In this study, 15 laboratories participated in an inter-laboratory comparison on the chemical characterization of three O&G wastewaters from the Appalachian Basin and four solids impacted by O&G development, with the goal of evaluating the quality of data and the accuracy of measurements for various analytes of concern. Using a variety of different methods, analytes in the wastewaters with high concentrations (i.e., > 5 mg/L) were easily detectable with relatively high accuracy, often within $\pm 10\%$ of the most probable value (MPV). In contrast, often less than 7 of the 15 labs were able to report detectable trace metal(oids) concentrations (i.e., Cr, Ni, Cu, Zn, As, and Pb) with accuracies of approximately $\pm 40\%$. Despite most labs using inductively coupled plasma mass spectrometry (ICP-MS) with low instrument detection capabilities for trace metal analyses, large dilution factors during sample preparation and low trace metal concentrations in the wastewaters limited the number of quantifiable determinations and likely influenced analytical accuracy. In contrast, all the labs measuring Ra in the wastewaters were able to report detectable concentrations using a variety of methods including gamma spectroscopy and wet chemical approaches following Environmental Protection Agency (EPA) standard methods. However, the reported radium activities were often greater than $\pm 30\%$ different than the MPV possibly due to calibration inconsistencies among labs, radon leakage, or failing to correct for self-attenuation. Reported radium activities in solid materials had less variability ($\pm 20\%$ from MPV) but accuracy could likely be improved by using certified radium standards and accounting for self-attenuation that results from matrix interferences or a density difference between the calibration standard and the

1
2
3 unknown sample. This inter-laboratory comparison illustrates that numerous methods can be
4 used to measure major cation, minor cation, and anion concentrations in O&G wastewaters with
5 relatively high accuracy while trace metal(loid) and radioactivity analyses in liquids may often
6 be over $\pm 20\%$ different from the MPV.
7
8
9
10
11

12
13 **Keywords:** brine; analysis; trace metals; radium; solids (TENORM)
14

15 **Introduction:**

16
17 Horizontal drilling and hydraulic fracturing has increased oil and gas (O&G) production
18 from low permeability shale formations throughout the United States (U.S.). In 2017, the U.S.
19 Energy Information Administration (EIA) estimated that nearly 60% (0.48 trillion cubic meters)
20 of the U.S. natural gas production was produced from shale resources throughout the U.S.,
21 including the Marcellus, Utica, Permian, Haynesville, Eagle Ford, Barnett, Woodford, and
22 Bakken Shales¹. This shale development has lowered national carbon dioxide (CO₂), nitrogen
23 oxide (NO_x), and sulfur dioxide (SO₂) emissions by shifting energy production from coal to
24 natural gas². However, the increased production has also resulted in concerns with respect to
25 seismic activity³, methane emissions⁴, ground water and surface water contamination^{5, 6}, and the
26 disposal of solid and liquid wastes that can lead to substantial increases in seismic activity and
27 concentrations of some contaminants in surface waters^{7, 8}.
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42

43 O&G production creates large quantities of high salinity (>100,000 mg/L total dissolved
44 solids [TDS]) liquid wastes that cause challenges for wastewater management and disposal.
45 Wastewater production volumes from U.S. shale plays have been estimated at 27 - 130 liters of
46 produced water per billion cubic meter of gas (L/Bm³) in the Eagle Ford and Haynesville shales,
47 more than 130 L/Bm³ from the Barnett Shale, and approximately 3.3 - 94 L/Bm³ from the
48 Marcellus Shale, which generated approximately 0.67 billion cubic meters of natural gas per day
49
50
51
52
53
54
55
56
57
58
59
60

1
2
3 (Bm³/day) in 2017^{9, 10}. Depending on the shale play, these fluids typically contain high
4
5 concentrations of salts, metals, naturally occurring radioactive materials (NORMs), and organic
6
7 compounds that make proper management via treatment and/or disposal particularly important in
8
9 limiting potential human and environmental health concerns^{11, 12}. O&G wastewater disposal
10
11 options include injection into subsurface formations, reuse to develop other wells, treatment at
12
13 wastewater treatment facilities with surface water discharge permits, storage in evaporation
14
15 ponds, or beneficial reuse for other practices such as irrigation, dust suppression and de-icing of
16
17 roads, or livestock watering¹³⁻¹⁶. Particular concerns with these practices are related to the
18
19 salinization of freshwater resources¹⁷, accumulation of radium or trace metals in roads treated
20
21 with O&G wastewaters^{15, 18} or in sediments downstream of O&G wastewater treatment
22
23 facilities¹⁹, and human health impacts (e.g., mutagenesis, endocrine disruption, neurotoxicity, or
24
25 cytotoxicity) by exposure to organic compounds in the wastewaters^{20, 21}. One way that state and
26
27 federal regulators monitor O&G wastewater disposal is by requiring chemical analyses of surface
28
29 water discharges from facilities treating O&G wastewaters (40 CFR Part 122) or analyses of
30
31 O&G wastewaters being permitted for other beneficial uses (e.g., irrigation, dust suppression, de-
32
33 icing, or livestock)^{13, 15}. States such as Pennsylvania also require O&G operators who generate
34
35 more than 1,000 kilograms of waste per well in a calendar year to report the chemistry of their
36
37 wastewater to the Pennsylvania Department of Environmental Protection (PADEP) along with a
38
39 description of disposal facilities that have received the waste²². The accuracy of these chemical
40
41 analyses are important for regulatory purposes, proper treatment, as well as fingerprinting
42
43 applications for identifying O&G wastewaters after potential contamination events²³⁻²⁵.

44
45
46
47
48
49
50
51 Accurate analyses of metal and radioactivity concentrations in O&G wastewaters are
52
53 challenging due to the complex fluid matrix²⁶. Common analytical methods for detecting metals
54
55
56
57
58
59
60

1
2
3 in O&G wastewaters, such as inductively coupled plasma optical emission spectrometry (ICP-
4 OES) or mass spectrometry (ICP-MS), can be hampered by non-spectral and spectral
5
6
7 interferences in high salinity fluids. Non-spectral interferences include signal suppression from
8
9
10 easily ionized elements (e.g., Na and K) as well as the accumulation of salts or oxide minerals on
11
12 cones in ICP-MS systems²⁶. Other spectral interferences such as superimposing element
13
14 emission lines in ICP-OES or the presence of polyatomic species (e.g., as $^{40}\text{Ar}^{23}\text{Na}^+$ on $^{63}\text{Cu}^+$) in
15
16 ICP-MS can also influence analytical results^{27, 28}. A number of techniques exist to correct for
17
18 these differences, including sample dilution, wet chemical separation, alternative sample
19
20 introduction, mathematical calculations, and calibration and internal standard modifications.^{29, 30}
21
22 Sample dilution is the most common way of reducing potential matrix effects, but often results in
23
24 decreased sensitivity and elevated method detection limits for trace metal(oids) of concern (e.g.,
25
26 As, Pb) in O&G wastewaters²⁶.

27
28
29
30
31 Numerous techniques exist for measuring radium in O&G wastewaters including
32
33 methods by alpha particle spectrometry (EPA Method 903.0)³¹, ^{222}Rn emanation counting in a
34
35 scintillation cell (EPA Method 903.1)³², gamma ray spectrometry (EPA Method 901.1)³³, beta
36
37 particle spectroscopy (EPA Method 904.0)³⁴, or ICP-MS³⁵. Some of these methods measure Ra
38
39 activities directly by ICP-MS or alpha, beta, and gamma emissions while other methods measure
40
41 Ra indirectly based on emissions by daughter products. Among these, the ^{222}Rn emanation
42
43 technique involves the collection and indirect counting of alpha particles emitted by ^{222}Rn , a
44
45 daughter product of ^{226}Ra ³². In some cases, this method may also require the pre-concentration
46
47 of ^{226}Ra from samples using co-precipitation techniques with barium sulfate (EPA Method
48
49 903.1)^{32, 36, 37}. There are some undesirable aspects of this method including long waiting periods
50
51
52
53
54 required for radon ingrowth (>21 days ingrowth) and potential loss of Ra during sample pre-
55
56
57
58
59
60

1
2
3 concentration^{32, 36, 37}. Co-precipitation techniques are also required to remove ²²⁸Ra from
4
5 solutions prior to indirect measurements of its ²²⁸Ac daughter using beta particle spectroscopy³⁴.
6
7 Methods by alpha particle spectrometry can measure ²²⁶Ra directly based on α emissions at 4.78
8
9 MeV but also often require pre-concentration, chemical separation, and purification techniques
10
11 to remove other alpha emitters³⁸. High salinity O&G samples can reduce Ra yields during
12
13 chemical separation and purification but can likely be accounted for using tracers^{37, 38}. Because
14
15 of the high salinity of O&G wastewaters and potential difficulty in recovering Ra from these
16
17 solutions, standard EPA methods that require Ra separation prior to analyses have been
18
19 discouraged for analyses of O&G wastewaters³⁷.
20
21
22
23

24 One method that has been encouraged for radioactivity analyses of O&G waste is gamma
25
26 ray spectrometry³⁷. This method requires no sample preparation or pre-concentration techniques
27
28 potentially reducing the risk of low Ra yields from co-precipitation or chemical separation
29
30 methods; yet, it is still common to concentrate Ra in co-precipitates or evaporites and analyze the
31
32 solids using gamma ray spectrometry³⁹. ²²⁶Ra can be measured directly using the gamma
33
34 emission energy at 186.2 keV. However, gamma emissions from ²³⁵U at 185.7 keV can also
35
36 interfere with direct ²²⁶Ra measurements. This interference is more likely an issue in O&G drill
37
38 cuttings or sediment materials than O&G wastewaters due to their relative activities of ²³⁵U³⁷.
39
40

41
42 An alternative method for ²²⁶Ra is to measure the indirect gamma emission of ²¹⁴Pb at 295.2 keV
43
44 and 351.9 keV and ²¹⁴Bi at 609.3 keV following equilibrium between ²²⁶Ra and ²²²Rn. Similarly,
45
46 the indirect method for determining ²²⁸Ra is based on the gamma emission of its ²²⁸Ac daughter
47
48 at 911.2 keV. There are several factors that could lead to inaccurate Ra measurements of O&G
49
50 wastes using gamma spectrometry. Rn leakage in sample containers can influence indirect
51
52 measurements of ²²²Rn progeny (i.e., ²¹⁴Pb and ²¹⁴Bi). Leakage could occur by improperly sealed
53
54
55
56
57
58
59
60

1
2
3 containers or by diffusion through polyethylene plastics which commonly make up Marinelli
4
5 beakers and other containers used for gamma ray spectroscopy measurements⁴⁰. O&G solid and
6
7 liquid wastes may also have different chemical compositions (e.g., high salinity; radio-barite co-
8
9 precipitates) and densities (e.g., often greater than 1.2 g/mL densities in O&G wastewaters) in
10
11 comparison to standards. This can result in differences in attenuation of gamma photons between
12
13 samples and standards, leading to analytical inaccuracies⁴¹. Attenuation may be accounted for
14
15 using a variety of techniques although standard EPA methods do not require these corrections³³,
16
17
18
19 41, 42.

20
21 An inter-laboratory comparison was organized among commercial, academic, and
22
23 government labs throughout the U.S., Canada, and Germany to determine how these potential
24
25 sources of error effect the accuracy of O&G waste characterizations. Several of the commercial
26
27 labs had previously analyzed O&G wastes for certificate of analyses in regulatory applications.
28
29 The main goals of the comparison were to 1) evaluate the overall quality of data from
30
31 laboratories analyzing O&G wastes, 2) identify methods that produce acceptable quality data for
32
33 the analytes of concern in O&G wastes, and 3) evaluate the analytical accuracy for various
34
35 analytes of concern in O&G wastes, including Na, K, Mg, Ca, Sr, Ba, Li, B, Al, Fe, Mn, Cr, Ni,
36
37 Cu, Zn, As, Pb, Cl, Br, SO₄, ²²⁶Ra, and ²²⁸Ra.
38
39
40
41

42 **Methods**

43
44 **Sample preparation and shipment.** Three O&G wastewaters chosen for the study were
45
46 collected from oil and gas wells throughout the Appalachian Basin, located in the northeastern
47
48 United States and stored in 20 liter high density polyethylene (HDPE) containers. One liter of
49
50 each of the wastewaters were filtered with a 0.45 μm cellulose acetate filter and then stored at
51
52 4°C for anion analyses (i.e., Cl, Br, SO₄). The remaining wastewaters were acidified with 5%
53
54
55
56
57
58
59
60

1
2
3 nitric acid and filtered for elemental and radioactivity analyses (i.e., Na, K, Mg, Ca, Sr, Ba, Li,
4 B, Al, Fe, Mn, Cr, Ni, Cu, Zn, As, Pb, ^{226}Ra , ^{228}Ra). Thereafter, sub aliquots of each of the
5
6 samples were stored in HDPE bottles for sample shipment.
7
8
9

10 In addition to the three oil and gas wastewaters, four solid samples were pulverized and
11 sieved (<1.18 mm) for interlab comparisons. Each solid sample was selected to have a matrix
12 similar to solids commonly analyzed in environmental studies accessing O&G impacts (i.e., river
13 sediments impacted by O&G wastewater, barite sludge from treatment facilities, and shale core
14 or cuttings). These solid samples were as follows: solid sample 1 (SS1) was a stream sediment
15 collected from the Blacklick Creek, Pennsylvania, solid sample 2 (SS2) was a Marcellus Shale
16 outcrop, and solid sample 3 (SS3) and 4 (SS4) were both Blacklick creek stream sediments
17 mixed with radio-barite sludge at different ratios. All solid samples were homogenized with a
18 mixing paddle before packaging and shipment.
19
20
21
22
23
24
25
26
27
28
29
30

31 Each sample was sent to 15 labs and was received within 1-4 days after shipment. The
32 labs included eight academic, six commercial, and one government lab. Each lab was instructed
33 to use their own preparation and analytical methods to analyze the liquid samples for a suite of
34 cations and anions including Cl, Br, SO_4 , Li, B, Na, K, Mg, Ca, Sr, Ba, Al, Fe, Mn, S, Cr, Ni,
35 Cu, Zn, As, Cd, Pb, ^{226}Ra , and ^{228}Ra . Due to the analytical capabilities of participating labs and
36 the interest in technologically enhanced naturally occurring radioactive material (TENORM) in
37 oil and gas wastes, only ^{226}Ra and ^{228}Ra were measured for solid samples. Many labs did not
38 have the analytical equipment to measure all the cations or anions and were therefore asked to
39 only report analytes and values within their capabilities. An anonymous online portal was created
40 for data submission and reporting of sample preparation procedures (i.e., dilution factors,
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

precipitation or pre-concentration methods), analytical equipment and methods used for analyses, uncertainties, and calibration standards.

Data processing and statistical analysis. All submitted data were evaluated according to nonparametric statistical methods in Hoaglin et al. (1983)⁴⁴ that are commonly used in inter-laboratory comparisons by the United States Geological Survey (USGS)⁴⁵. This statistical approach is known to be resistant to outliers because the method is based on median, 25th percentile, and 75th percentile values rather than mean values in parametric statistics. All data were first trimmed to exclude values that were reported as zero or below detection limits. Thereafter, the 25th percentile (Q1), median, and 75th percentile (Q3) concentrations for all analytes in the three O&G wastewaters and four solid samples were calculated. $F_{\text{pseudosigma}}$ (mg/L), an approximation for standard deviation, was calculated for each analyte according to:

$$F_{\text{pseudosigma}} = \frac{Q3 - Q1}{1.349} \quad (\text{Equation 1}) \text{ where } 1.349 \text{ is the number}$$

of standard deviations encompassing 50% of the data (i.e., Q3-Q1)⁴⁴.

To perform all desired statistical processing tests, a full suite of data with a high number of total reported values (>7 reported values per analyte) and low $F_{\text{pseudosigma}}$ was required. For analytes with over seven reported values and with $F_{\text{pseudosigma}}$ values less than the median, the median value of all the data was reported as the most probable value (MPV) for the analyte concentration within the sample. In this study, $F_{\text{pseudosigma}}$ values for analytes with over seven reported values were never greater than the median. Thereafter, the performance of the labs were evaluated by calculating their z-score (dimensionless) according to:

$$z = \frac{\text{reported value} - \text{MPV}}{F_{\text{pseudosigma}}} \quad (\text{Equation 2}) \text{ Interpretation of the } z\text{-}$$

scores were as follows: $|z| \leq 2$ is an acceptable result, $2 < |z| \leq 3$ is a questionable result, and $|z| > 3$

1
2
3 is an unacceptable result⁴⁴. The range of acceptable results were compared to the MPV value for
4
5 a given analyte to determine the % difference (i.e., accuracy) of the measurements according to:
6

$$\% \text{ difference} = \left[\frac{MV - MPV}{MPV} \right] \times 100 \quad (\text{Equation 3})$$

7
8
9
10
11
12
13

14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32

measured value of an acceptable result.

14 In some cases, there were not enough reported values for specific analytes to do all the
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32

desired statistical tests. Therefore, the following modifications were made to the statistical processing methods above. When five or six values were reported for an analyte in a sample, the median and $F_{\text{pseudosigma}}$ values were reported with an asterisk (*) along with the 25th and 75th percentile concentrations. In this scenario, no z-scores or % difference calculations were performed. No summary statistics were calculated for analytes with <5 reported values. For these scenarios, the z-scores are represented as not calculable (n.c.) throughout the manuscript and are not included in data interpretations.

33 **Results and Discussion**

34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

Major cations, minor cations, and anions. Major cation (i.e., Na, K, Mg, Ca, Sr, and Ba), minor cation (i.e., Li, B, Al, Fe, and Mn), and anion (Br, Cl, SO₄) concentrations in the three O&G wastewaters were measured using a variety of methods, including inductively coupled plasma with optical emission spectrometry (ICP-OES), direct plasma spectrometry (DCP), inductively coupled plasma with mass spectrometry (ICP-MS), triple quadrupole inductively coupled plasma with mass spectrometry (ICP-MS/MS), neutron activation analysis (NAA), X-ray fluorescence (XRF), and ion chromatography (IC). A summary of the instruments used by participating labs for measuring particular analytes is included in the Supporting Information (Table S1).

Approximately 50% of all major and minor element analyses were performed using an ICP-OES (e.g., Perkin Elmer Optima 5300DV ICP-OES, Horiba Ultima Expert ICP-OES, Spectro ARCOS ICP-OES, Thermo Scientific iCAP 7400, and Thermo Scientific iCAP 6000). Prior to analyses, samples were diluted between 100-1000 times and measured in accordance with EPA method 200.7⁴⁶ using internal standards (i.e., Sc, In, Re, and Y), quality control samples, external standards [National Institute of Standards and Technology (NIST) 1640a, NIST 1643f, Ocean Scientific International Ltd (OSIL) seawater standard, USGS M-220, and NIST Standard Reference Material (SRM) 1640a], laboratory fortified blanks, matrix spikes, and/or laboratory reagent blanks to confirm the accuracy of the equipment. In one to three instances, labs using ICP-OES for major cation analyses switched to ICP-MS for Li, B, Ba, Al, Fe, or Mn measurements likely due to the lower concentrations of these cations relative to many of the major cations and lower detection limits of the ICP-MS (often less than 1 ppm after accounting for sample dilution). More complete descriptions of ICP-MS methods are included in the following section.

Table 1. The most probable value (MPV), 25th percentile (Q1), 75th percentile (Q3), and $F_{\text{pseudosigma}}$ (F) for major cation, minor cation, and anion concentrations in sample 1, 2, and 3. All values are represented in mg/L. When there were only 5 or 6 reported values submitted, summary statistics are noted with an asterisk (*). When there were less than 5 reported values for a given analyte, summary statistics were not calculable (n.c.).

Analyte	Sample 1			Sample 2			Sample 3		
	MPV	Q1-Q3	F	MPV	Q1-Q3	F	MPV	Q1-Q3	F
Br	746	652 - 773	90.4	1270	1180 - 1440	189	1890	1630 - 2060	320
Cl	65600	63900 - 68300	3300	117000	113000 - 120000	5470	176000	160000 - 180000	15000
SO ₄	n.c.	n.c.	n.c.	n.c.	n.c.	n.c.	170*	130 - 172*	33.0*
Na	27000	24900 - 28600	2710	47500	43600 - 49300	4260	66850	64600 - 68900	3170
K	336	276 - 383	79.3	716	621 - 765	107	2190	1770 - 2310	402
Mg	1230	1200 - 1300	69.3	2168	2100 - 2270	127	3100	2990 - 3130	104
Ca	10000	9280 - 10200	686	19800	18600 - 20600	1480	31400	30000 - 33200	2350
Sr	2160	2130 - 2200	49.7	3710	3580 - 3940	270	1540	1410 - 1620	156
Ba	659	641 - 690	37.2	1320	1280 - 1380	72.8	6.12	6.07 - 6.33	0.20
Li	32.1	30.3 - 34.3	3.00	50.3	48.0 - 51.0	2.19	71.7	68.0 - 74.2	4.60
B	5.00	3.95 - 5.09	0.85	7.00	6.76 - 8.05	0.95	15.3	14.7 - 16.0	0.99
Al	n.c.	n.c.	n.c.	n.c.	n.c.	n.c.	n.c.	n.c.	n.c.
Fe	64.8	58.7 - 69	7.61	94.9	85.8 - 98.5	9.44	169	158 - 181	17.0
Mn	6.10	5.75 - 6.7	0.70	14.4	13.7 - 14.9	0.93	47.8	41.5 - 48.3	5.06

1
2
3 Other methods for analyses included NAA, XRF, DCP, and IC. One lab used a neutron
4 activation analysis method for all analyses that consisted of drying samples into crystals,
5 irradiating the crystals in a nuclear reactor core, and then comparing the emitted gamma rays to
6 irradiated standard reference materials (i.e., Montana soil 2711 SRM and Buffalo River
7 sediments)^{47, 48} using a high purity germanium detector. Another lab used XRF for all analyses
8 but no details were provided on the method other than the sample analysis time (21 minutes) and
9 instrument manufacturer (i.e., SPECTRO XEPOS XRF Spectrometer). In one case, an IC
10 column (Dionex IonPac CS12A IC column with 15 mM methanesulfonic acid eluent) was used
11 to separate major cations (i.e. Ca, Mg, Na, K, and Sr) for analysis using a Dionex ICS2000 Ion
12 Chromatograph.
13
14
15
16
17
18
19
20
21
22
23
24
25

26 Over 80% of the labs used IC for anion analyses. A diversity of columns and methods
27 were referenced by participating labs, including AS11 HC, AS18, and AS19 columns with KOH
28 eluent. With the exception of one lab who reported greater than 10,000 times dilution, all labs
29 diluted samples approximately 100-1,000 times prior to IC analyses. Referenced standards
30 included the Dionex 7 Anion Standard II and a diluted OSIL seawater standard. Two other labs
31 used XRF or NAA for determining Cl and Br concentrations in the three samples.
32
33
34
35
36
37
38
39

40 All three O&G wastewaters had major cation, minor cation, and anion concentrations
41 (Table 1) that were within the 25th to 75th percentile concentrations for wastewaters from the
42 Appalachian Basin, U.S. (Table S2)⁴⁹. The samples were nearly 100% charge balanced by
43 chloride which had the highest concentration in sample 3 (MPV=176,000 mg/L Cl) and the
44 lowest concentration in sample 1 (MPV=65,600 mg/L Cl). With the exception of SO₄²⁻ and Al,
45 which had a low number of reported concentrations among the three samples (n < 5), summary
46 statistics were calculated for all major cation, minor cation, and anion concentrations according
47
48
49
50
51
52
53
54
55
56
57
58
59
60

1
2
3 to non-parametric statistics (Table 1)⁴⁴. $F_{\text{pseudosigma}}$ values for all these analytes were often orders
4
5 of magnitude lower than the MPV suggesting low variability among the reported results.
6

7
8 Greater than 80% of the reported values for major cation, minor cation, and anion
9
10 concentrations were of acceptable or questionable quality (Figure 1). For example, between all
11
12 three samples, a total of 433 values were reported (e.g., 14 analytes per sample x 3 samples x
13
14 number of values submitted by individual labs) and 365 of the values were determined to be of
15
16 acceptable or questionable quality. Of the remaining 68 reported values, 56 were of unacceptable
17
18 quality and 12 were not calculable because they were below method detection limits (e.g., Al and
19
20 SO_4^{2-} analyses). Unacceptable data quality was examined in more detail to determine if the data
21
22 quality was influenced by the methods used for analyses.
23
24
25

26
27 Figure 1. Data quality for major cation, minor cation, and anion concentrations reported in
28
29 sample 1, 2, and 3. Acceptable, questionable, and unacceptable quality were based on z-score
30
31 calculations when the number of values were ≥ 7 for a given analyte. When 5 or 6 values were
32
33 reported, no z score was calculated but is noted with an asterisk as a MPV and $F_{\text{pseudosigma}}$ were
34
35 still calculated (i.e., Table 1). When less than 5 values were reported, no statistics were
36
37 calculated.
38

39
40 Analyses of unacceptable quality data suggests that both the method and/or lab could
41
42 have an influence on the reported major and minor cation concentrations submitted in this study.
43
44 There were 48 total unacceptable quality values reported for major and minor cations (note that
45
46 an additional 8 anion results were unacceptable) among all three O&G wastewaters. When
47
48 grouped by method, the highest percent of unacceptable values were for XRF and NAA (e.g.,
49
50 52% of the XRF and 33% of the NAA) while only 9% of the ICP results were unacceptable.
51
52 NAA and XRF accounted for 40% of the total unacceptable values for all the submitted data. In
53
54 addition, these two methods were each used by one lab.
55
56

57
58 The high percentage of unacceptable values for NAA could be attributed to analyses of a
59
60 few cations. The NAA laboratory reported all detectable analytes, even though there was a strong

1
2
3 likelihood that elements with activation products that have short half-lives (less than several
4 days, e.g. ^{42}K and ^{82}Br) would be compromised by interference from the scattering of gamma
5 rays from ^{24}Na in the high purity germanium detector. A number of factors influence NAA
6 detection capabilities, including the isotopic abundance and neutron absorption cross-section of
7 the target isotope, the gamma ray intensity and gamma ray energy from the activated isotope,
8 and the presence of other elements in the sample. These last two factors are significant in the
9 high salinity O&G samples. The very high Na concentration in these samples produces a large
10 amount of ^{24}Na ($t_{1/2} = 14.997$ hours) during neutron irradiation. The high energy gamma rays
11 from ^{24}Na (1368.6 keV (99.99%) and 2754.0 keV (99.86%)) undergo Compton scattering in the
12 high purity germanium detector, creating a Compton plateau of increased counts at energies
13 below approximately $E_{\gamma} - 256$ keV ⁵⁰. These increased counts in the lower energy region of the
14 gamma ray spectrum can alter and even completely obscure the gamma ray peaks from activated
15 isotopes that emit lower energy gamma rays. Mainly because of this phenomenon, the most
16 accurate elemental determinations in these types of O&G samples are for elements whose
17 activation products have half-lives greater than several days, which allows for the full decay of
18 the ^{24}Na and the elimination of the ^{24}Na Compton plateaus. For example, by excluding data from
19 the shorter-lived isotopes (e.g. ^{42}K and ^{82}Br), the percentage of acceptable data points reported
20 by the NAA laboratory increases to 80%. Furthermore, it appears that three of the four remaining
21 outliers of unacceptable quality are from sample 3, which has the highest Na concentration of the
22 three samples; the exact reason for the concentration of outliers in sample 3 is not known, but the
23 high Na concentration could be the cause. Overall, NAA performs well for elements with longer-
24 lived activated isotopes such as Sr, Ba, Fe.
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

1
2
3 Other values reported by labs using ICP-OES suggests that the lab also has an influence
4 on the quality of data that was submitted. For instance, 17% and 27% of the reported values by
5 two labs using ICP-OES had unacceptable quality while each of the other six labs using ICP-
6 OES never had more than 4% of their data rejected due to unacceptable quality. As another
7 comparison, one lab using ICP-MS for all analyses had 40% of their reported values rejected for
8 data quality issues while another lab using ICP-MS had less than 6% rejected. These examples
9 illustrate that each of these ICP methods can likely be used to generate acceptable quality data
10 when measuring major and minor cation concentrations in O&G wastewaters and that a large
11 portion of the variability observed in the current study is likely a result of quality control issues
12 and internal lab protocols for specific analytical methods.
13
14
15
16
17
18
19
20
21
22
23
24
25

26 The only analytes that were particularly challenging for all participating labs were
27 SO_4 and Al. For instance, only five total detectable SO_4 concentrations and seven total detectable
28 Al concentrations were measured in the three O&G wastewaters (Figure 1). All the reported SO_4
29 values were for sample 3 which had a median value of 170 mg/L and $F_{\text{pseudostigma}}$ value of 33.0
30 mg/L. While the median value was 170 mg/L, seven labs reported that this was below their
31 detection (i.e., 200 to 500 mg/L) indicating that SO_4 analyses of O&G wastewaters are
32 challenging for labs when concentrations are below 200 to 500 mg/L. The reasons for the
33 challenges associated with measuring Al are unresolved as the number of reported values ($n = 2$
34 or 3 per sample) and large variations in detection limits (0.02 to 14 mg/L) prevent drawing any
35 conclusions from the data.
36
37
38
39
40
41
42
43
44
45
46
47
48

49 Major cation, minor cation, and anion concentrations in O&G wastewaters were within
50 $\pm 10\%$ of the MPV, with the exception of Br and K which sometimes exceeded $\pm 20\%$. These
51 accuracies are very similar to recent inter-laboratory comparisons of freshwaters where
52
53
54
55
56
57
58
59
60

1
2
3 acceptable quality data for major cations had $\pm 8.5\%$ difference from the MPV and minor cations
4 had up to $\pm 14.2\%$ difference (Table S3)⁴⁵. The range in the percent difference is based on
5
6 comparisons of the reported minimum and maximum concentrations of acceptable quality data to
7
8 the MPV. Results among the three samples indicate that the most deviation from the expected
9
10 MPV occurred for Br and K. If these differences were a result of dilution errors during sample
11
12 preparation, then similar % differences would be expected for analytes diluted to the same
13
14 dilution factors. This was not observed among the data submitted by several of the labs. For
15
16 instance, one lab diluted sample 2 by 50 times for K and Ca analyses by ICP-OES yet Ca
17
18 concentrations were within 5% of the MPV while K concentrations were 23% greater than the
19
20 MPV. Some of these differences could be attributed to the challenges of analyzing easily
21
22 ionizable cations such as K and Na that can have large relative standard deviations in analyses by
23
24 ICP⁵¹. In another case, one of the labs diluted sample 3 by 100 times and measured Cl
25
26 concentrations that were within 2% of the MPV while the bromide concentrations were 20%
27
28 greater than the MPV. All Br values reported with acceptable quality were measured using ion
29
30 chromatography, therefore, these differences are not necessarily instrument specific but could be
31
32 related to differences in calibration standards (e.g., use of certified standards versus standards
33
34 made from NaCl or NaBr salts, etc.), matrix-matching calibration standards (e.g., high Cl/Br
35
36 ratios in standards), or methods accounting for matrix interferences (e.g., peak overlap with
37
38 chloride or peak broadening by CO₂ or carbonate anions)⁵².
39
40
41
42
43
44
45
46

47 Figure 2. Range in accuracy of reported values with acceptable quality for major cation, minor
48 cation, and trace cation concentrations based on comparisons to the MPV. Values with a z score
49 that was between -2 and 2 were considered of acceptable quality. No accuracy calculations were
50 performed for SO₄ or Al due to the low number of detectable values and are represented as not
51 calculable (n.c.).
52
53
54
55
56
57
58
59
60

1
2
3 From a regulatory perspective, $\pm 10\%$ to 20% differences in any of the measured analytes
4 will not have a significant impact on the management or treatment of O&G wastewaters but
5 could influence geochemical interpretations made about O&G reservoirs based on wastewater
6 chemistry. For instance, some states that regulate the use of O&G wastewater spreading on roads
7 require the wastewaters to meet standards for Cl, Ca, Mg, Na, Ba, or Fe¹⁵. Other facilities that
8 treat these same wastewaters are also required to meet effluent discharge standards and permitted
9 total maximum daily loads for analytes; these standards often include Cl, Ba, and Fe⁵³. Based on
10 the results from this inter-laboratory comparison, academic, commercial, and government labs
11 can analyze each of these analytes with relatively high accuracy following a dilution step and the
12 $\pm 10\%$ differences in measured versus expected values will likely have very little influence on
13 how the wastewaters are managed. Other ions such as Br may have large percent differences
14 between measured and expected values. However, there are currently no surface water or
15 groundwater standards for Br despite evidence that it can lead to the formation of carcinogenic
16 disinfection byproducts in drinking water¹⁷. However, monitoring of Br loads from treatment
17 facility discharges may be required in future permits and therefore accurate Br measurements
18 should be a goal of every laboratory⁵⁴.

19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40 Differences in major and minor cations and anion concentrations between the measured
41 value and MPV will influence the calculation of elemental ratios, which are commonly used to
42 explain the origin of O&G wastewaters or are used as tracers for fingerprinting potential
43 contamination events^{55, 56}. For instance, Cl/Br ratios (mass/mass) for reported results with
44 acceptable quality ranged from 79 to 105 in sample 1 and 78 to 100 in sample 3 (Table S4).
45 O&G wastewaters throughout the Appalachian Basin are believed to originate from a common
46 ancient seawater source, however, the range in Cl/Br ratios (<50 to 110) reported in the literature
47
48
49
50
51
52
53
54
55
56
57
58
59
60

1
2
3 suggests that these fluids likely underwent varying degrees of evaporation (ranging from 20 -
4 40% evaporation)⁵⁶⁻⁵⁸. As a comparison, the range in Cl/Br ratios reported for any one of the
5 three samples in this study could be interpreted as a wastewater that originated from a seawater
6 evaporated by 27% to 39%. Therefore, some of the variability in Cl/Br ratios in existing
7 literature could be related to the challenges in measuring Br in these fluids. Other ratios
8 commonly used to trace O&G wastewaters in the environment (e.g., Sr/Ca and B/Cl)²³⁻²⁵ showed
9 much less variability (Table S4).

10
11
12
13
14
15
16
17
18
19 **Trace metal(loid) measurements.** Trace metal(loid)s (i.e., Cr, Ni, Cu, Zn, As, and Pb)
20 were measured using many of the same methods highlighted for major and minor cations.
21 However, the majority of analyses (60-75%) were performed using ICP-MS. ICP-MS equipment
22 included an ICP-MS Element2XR, VG PlasmaQuad3 ICP-MS, Agilent 7500 ICP-MS (n = 2),
23 Agilent 7900 ICP-MS, Thermo X series 2 ICP-MS, and Agilent 8800 ICP-MS/MS. Samples
24 prepared for the ICP-MS Element2XR were measured against a 2-point calibration curve and
25 with a In internal standard. Samples measured on the VG PlasmaQuad-3 ICP-MS were diluted
26 ~1,000 times prior to analyses. The equipment was calibrated with the NIST 1643e/1643f
27 standard, which was measured at varying concentrations before, after, and throughout sample
28 runs. Internal standards of In, Th, and Bi were spiked into all the samples prior to analyses.
29 Analyses on the Agilent 7500 ICP-MS were diluted 100 to 1,000 times prior to measurements.
30 The equipment was calibrated using NIST traceable standards and Sc, Ba, Ge, Rh, In, Pt, and Bi
31 were used as internal standards. All analyses on the Agilent 7900 ICP-MS were measured
32 according to EPA 200.8. Samples were diluted ~10 times prior to analyses. Calibration check
33 standards and laboratory control samples were measured before all samples and four internal
34 standards were used (Tb, Rh, Ge, and Sc) to account for instrument drift. All analyses on the
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

Thermo X series 2 ICP-MS were diluted approximately ~100 times prior to analyses. Mass interferences and matrix complications were accounted for by using internal standards (Sc, In, Re, Y) and high salinity, matrix-matched standards. Calibration curves for all analyses were verified by confirming <5% differences between measured and known metal(loid) concentrations in check standards (USGS M-220, USGS T-227, and SRM1640a). Lastly, analyses performed on the Agilent 8800 ICP-MS/MS were analyzed under a variety of conditions (i.e. no gas, He 5 mL, H₂, and O₂ gas). To account for instrumentation drift, a mix of internal standards including Sc, Ge, In, Lu, and Bi were run in a variety of acquisition modes. Dilution factors for all metal(loid)s measured by this method were approximately 70.

Table 2. The most probable value (MPV), 25th percentile (Q1), 75th percentile (Q3), and $F_{\text{pseudosigma}}$ (F) for trace metal(loid) concentrations in sample 1, 2, and 3. All values are represented in mg/L. When there were less than 5 reported values for a given analyte, summary statistics were not calculable (n.c.). When there were only 5 or 6 reported values submitted, summary statistics are noted with an asterisk (*). A Grubbs test was also performed on analytes with 5 or more reported values to remove any outliers⁵⁹.

Analyte	Sample 1			Sample 2			Sample 3		
	MPV	Q1-Q3	F	MPV	Q1-Q3	F	MPV	Q1-Q3	F
Ni	0.01*	0.01 - 0.35*	0.25*	0.03*	0.03 - 0.14*	0.08*	0.03*	0.03 - 0.17*	0.11*
Ni minus outliers	0.01*	0.01 - 0.35*	0.25*	0.03*	0.03*	0.00*	0.03*	0.030*	0.00*
Cu	n.c.	n.c.	n.c.	0.26*	0.12 - 0.69*	0.42*	1.53	1.34 - 1.92	0.43
Cu minus outliers	n.c.	n.c.	n.c.	0.26*	0.12 - 0.69*	0.42*	1.53	1.34 - 1.92	0.43
Zn	0.16*	0.11 - 0.36*	0.19*	0.33	0.18 - 0.55	0.27	1.86	1.43 - 1.97	0.41
Zn minus outliers	0.13*	0.10 - 0.19*	0.07*	0.28	0.16 - 0.35	0.14	1.83	1.36 - 1.93	0.42
As	n.c.	n.c.	n.c.	n.c.	n.c.	n.c.	0.07*	0.06 - 5.10*	3.75*
As minus outliers	n.c.	n.c.	n.c.	n.c.	n.c.	n.c.	0.07*	0.06 - 0.10*	0.03*
Pb	n.c.	n.c.	n.c.	n.c.	n.c.	n.c.	0.21	0.20 - 0.45	0.18
Pb minus outliers	n.c.	n.c.	n.c.	n.c.	n.c.	n.c.	0.20	0.20 - 0.21	0.01

Trace metal(loid) determinations in the O&G wastewaters were challenging for all laboratories (Table 2). There were only four analytes among the three wastewaters (Zn in sample 2, and Cu, Zn, and Pb in sample 3) that had sufficient data for performing non-parametric

1
2
3 statistics and calculating z-scores. The remaining analytes either had too little data to perform
4 any statistics ($n < 5$) or not enough data ($n = 5$ or 6) to perform all statistical analyses (Figure 3).
5
6 Even in samples where 5 or 6 values were reported, the 25th (Q1) to 75th (Q3) percentile ranges
7
8 were highly variable. For instance, Q1 to Q3 for Ni ranged from 0.009 to 0.345 mg/L and Zn
9
10 ranged from 0.108 to 0.358 mg/L in Sample 1 (Table 2). In every analyte with 5 or 6 values
11
12 reported, $F_{\text{pseudosigma}}$ was greater than the MPV indicating that there was a large amount of
13
14 variability among the data.
15
16
17
18

19 High method detection limits relative to the trace metal(loid) concentrations within the
20
21 wastewaters reduced the number of reported values. The reported MPVs for trace metal(loid)
22
23 measured in the three O&G wastewaters for this study (Table 2) are within the 25th to 75th
24
25 percentile concentrations for Appalachian Brines (Table S2). However, often greater than 50% of
26
27 the participating labs were unable to measure detectable concentrations within the samples
28
29 (Figure 3). Trace metal(loid) analyses are often required for certificates of analysis of O&G
30
31 wastewaters, but there are no federal trace metal(loid) standards that limit O&G wastewater
32
33 disposal. Therefore, trace metal(loid) concentrations in O&G wastewaters are often compared to
34
35 the drinking water standards²². Of the analyzed trace metal(loid), the most important to detect are
36
37 Cr, Cu, As, and Pb since they have primary drinking water standards of 0.1 mg/L, 1.3 mg/L, 0.01
38
39 mg/L, and 0.015 mg/L, respectively. While all the reported instrument detection limits (IDL's)
40
41 for labs using ICP-MS were below these standards, the labs diluted the samples 10 to 1,000 times
42
43 to reduce potential matrix effects from analyzing the high salinity brines, resulting in method
44
45 detection limits (MDLs) (e.g., dilution factor times instrument detection limit) that were
46
47 sometimes greater than the drinking water standards. Methods other than dilution, such as resins
48
49 or chelating agents, are often used to remove trace metals from high salinity solutions and
50
51
52
53
54
55
56
57
58
59
60

1
2
3 increase method detection limits⁶⁰. However, these methods are not necessary if the method
4
5 detection limits for analyzing O&G wastewaters are at or below the regulatory standards. ICP-
6
7 MS MDLs for these trace metal(loid)s were 0.05 to 0.6 mg/L for Cr, 0.01 to 2.76 mg/L for Cu,
8
9 0.01 to 0.1 mg/L for As, and 0.01 to 0.06 mg/L for Pb. Therefore, the MDLs were less than one-
10
11 to-six times above the drinking water standard for Cr, less than one-to-two times above for Cu,
12
13 one-to-ten times above for As, and one-to-seven times above for Pb. In other words, all labs were
14
15 able to achieve MDLs that were close to the primary drinking water standards, the concentrations
16
17 in the O&G wastewaters were simply low and challenging to detect after the samples were
18
19 diluted.
20
21
22
23

24 Figure 3. Data quality for trace metal(loid) concentrations reported in sample 1, 2, and 3.
25 Acceptable, questionable, and unacceptable designations were based on z-score calculations
26 when the number of reported values was ≥ 7 for a given analyte. When 5 or 6 values were
27 reported, no z score was calculated but is noted with an asterisk as a MPV and $F_{\text{pseudosigma}}$ were
28 still calculated (Table 2). When less than 5 values were reported, no statistics were calculated.
29
30

31 Only samples that had more than 0.2 mg/L of Pb or 1.5 mg/L Cu were detectable by more
32
33 than 50% of labs. Of the reported values for Pb in sample 3, five were of acceptable quality
34
35 while the other two values reported by labs using XRF or ICP-OES were determined to be of
36
37 questionable or unacceptable quality. The lab using ICP-OES performed no sample dilution.
38
39 Therefore, matrix interferences from the high salinity wastewater could have influenced their
40
41 reported Pb concentrations²⁶. All the reported values with acceptable quality were by labs using
42
43 ICP-MS with measured Pb concentrations ranging from 0.2 mg/L to 0.22 mg/L, approximately
44
45 10 times above the drinking water standard. Pb measurements by ICP-MS were accurate, only
46
47 deviating $\pm 5\%$ from the MPV (Figure 4). In comparison, other methods that produced
48
49 questionable or unacceptable quality values for sample 3 (i.e., XRF and ICP-OES) measured Pb
50
51 concentrations that were 200 to 11,000% different than the MPV. Therefore, we strongly
52
53
54
55
56
57
58
59
60

1
2
3 encourage using ICP-MS for Pb analyses of O&G wastewaters. This method might be limited by
4
5 MDLs, but appears to be accurate among five labs using ICP-MS at concentrations
6
7 approximately 10 times above the drinking water standard. Due to the low number of measured
8
9 Pb values in other samples, we could not assess the data quality and performance at lower Pb
10
11 concentrations.
12
13

14
15 Figure 4. Range in accuracy of reported values with acceptable quality for trace metal(loid)s
16 based on comparisons to the MPV. No accuracy calculations were performed for sample 1 due to
17 the low number of detectable concentrations. Other metal(loid)s where statistics were not
18 calculable (n.c.) due to the low number of detectable values ($n < 7$) are shown for sample 2 and
19
20 3.
21

22
23 Cu was the only other metal on the EPA's list of metals in drinking water that had a
24
25 sufficient number of reported values to assess the data quality. All of the reported Cu values in
26
27 sample 3 were determined to be of acceptable quality with concentrations ranging from 1.0 to 2.1
28
29 mg/L; values that are close to the EPA standard for drinking water quality (1.3 mg/L). These
30
31 measurements were also relatively accurate, ranging from $\pm 40\%$ difference in comparison to the
32
33 MPV (Figure 4). In other samples with Cu concentrations less than 1.5 mg/L, there was a high
34
35 amount of variability with $F_{\text{pseudosigma}}$ often greater than the median value (Table 2).
36
37

38
39 A significant amount of variability was observed in reported values for all other trace
40
41 metal(loid)s that could be related to the methods used by a few participating labs. For many of
42
43 the trace metal(loid)s, less than seven measured values were reported limiting our ability to use
44
45 the non-parametric statistics method (i.e., the z-score method by Hoaglin et al. (1983) and in
46
47 USGS inter-laboratory comparisons)^{44, 45} to identify unacceptable or questionable quality data.
48
49 Therefore, the Grubbs statistical test for identifying outliers⁵⁹ was performed on analytes with
50
51 five or more detectable values to determine if there were any statistically significant outliers ($p <$
52
53 0.05) in the trace metal data. When outliers were detected, the MPV, Q1 to Q3, and $F_{\text{pseudosigma}}$
54
55
56
57
58
59
60

1
2
3 values were recalculated (Table 2). For all trace metal(loid)s with five or more measured values,
4
5 10 outliers were identified out of the 66 total values reported for trace metal(loid)s. All outliers
6
7 came from results submitted by four labs who used ICP-OES, XRF, NAA, or ICP-MS. When
8
9 compared to the total number of trace metal(loid) values determined by each method, 57% of the
10
11 data submitted by XRF (4 outliers out of 7 measured values), 50% of the data submitted by ICP-
12
13 OES (3 outliers out of 6 measured values), and 33% of the data submitted by NAA methods (1
14
15 outlier out of 3 measured values) were outliers. For NAA, both reported Zn values were
16
17 acceptable, but the single As value was not. These NAA results are consistent with the
18
19 previously identified trend of longer-lived activated isotopes (^{65}Zn , $t_{1/2} = 243.93$ days) providing
20
21 more accurate data than shorter-lived activated isotopes (^{76}As , $t_{1/2} = 26.24$ hours), as the longer-
22
23 lived isotopes can be measured after the decay of ^{24}Na . In contrast, less than 4% of the data (2
24
25 out of 53) submitted by ICP-MS were considered outliers. After removing these outliers, the
26
27 recalculated Q1-Q3 values became smaller and the $F_{\text{pseudostigma}}$ values were reduced to below the
28
29 median values (Table 2).
30
31
32
33
34

35
36 Removing all ICP-OES, XRF, and NAA data from the measured values submitted for
37
38 sample 3 influenced interpretations of the submitted data. Therefore, we performed additional
39
40 calculations for sample 3 where all the reported values of Ni, Cu, Zn, As, and Pb by ICP-MS
41
42 were compared to the median values submitted by ICP-MS. After making these adjustments, the
43
44 % differences from the median were -5% to 30% for Ni, -34 to 38% for Cu, -30% to 65% for Zn,
45
46 -37% to 9% for As, and -1% to 9% for Pb. While we acknowledge that this is not a standard
47
48 method for statistical analyses, the example simply illustrates that after excluding methods other
49
50 than ICP-MS, most of the measured values deviated by $\pm 40\%$ from the median values. Similar %
51
52 differences were reported for acceptable quality data in recent inter-laboratory comparisons by
53
54
55
56
57
58
59
60

1
2
3 the USGS (e.g., up to 30% difference for trace metal(loid)s)⁴⁵. While the high percentage of
4 outliers in NAA, ICP-OES, or XRF could be attributed to lab protocols for each technique, we
5 encourage using ICP-MS for measuring trace metals in O&G wastewaters as there is some
6 evidence to suggest that ICP-MS measurements are accurate to within approximately $\pm 40\%$.
7
8
9

10
11
12 Analyzing trace metal concentrations in O&G wastewaters requires a dilution factor that
13 is enough to reduce potential matrix interferences without diluting analytes below their method
14 detection limits. Results from this inter-laboratory comparison suggest that most labs using ICP-
15 MS can detect metal(loid)s on the EPA's list of regulated metals in drinking water at
16 concentrations as low as 1 to 10 times above the primary standards. For instance, labs using ICP-
17 MS were able to measure Cu, As, and Pb concentrations to within $\pm 40\%$ difference when the
18 median values for these analytes were 1.5 mg/L, 0.06 mg/L, and 0.2 mg/L, respectively. Many
19 labs struggled to report values below these concentrations. From a regulatory perspective, the
20 question then becomes what is the method detection limit and accuracy that is needed for trace
21 metal determinations in O&G wastewaters and how necessary are these measurements since the
22 majority of these measurements appear to be below detection limits that are above the standards
23 set for trace metal concentrations in drinking water. If the goal of trace metal(loid) analyses is to
24 only identify wastewaters that may have trace concentrations approximately 1 to 100s of times
25 above the drinking water standard, then simply diluting the wastewaters and analyzing by ICP-
26 MS methods can result in accurate measurements (to within $\pm 40\%$ from the true value). If there
27 is a need to measure lower concentrations for regulatory purposes or to understand trace metal
28 geochemistry, then other methods that use resins or chelating agents to concentrate these metals
29 are likely required⁶¹.
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

Radium measurements in liquids. Participating labs (n=11) analyzed the O&G wastewaters for radium activity using a diversity of methods, including gamma ray spectroscopy, beta particle spectroscopy, Rn emanation counting in a scintillation cell, and alpha particle spectroscopy. A summary table with each of the methods used is included in the supporting information (Table S5). Gamma spectroscopy analyses were performed by the majority of the labs (70%) at geometries consistent with internal standards or certified reference materials. A common method for gamma spec analyses was to seal the samples in Marinelli beakers or polypropylene containers for 21 days to allow the ingrowth of ^{226}Ra daughter products (^{214}Pb or ^{214}Bi) that were measured at 295.2 keV, 351.9 keV, or 609.3 keV. In some cases, labs also analyzed the ^{226}Ra without ingrowth by direct measurements at 186.2 keV. One lab (Lab 7b; Table S5) also co-precipitated ^{226}Ra from the wastewaters along with a ^{133}Ba tracer to estimate Ra recoveries prior to analysis by gamma spectroscopy. Complete details of the method were not reported but similar methods have been reported previously⁶². This same lab also measured Ra directly in the samples using gamma spectroscopy (Lab 7a; Table S5).

Table 3. The most probable value (MPV), 25th percentile (Q1), 75th percentile (Q3), and $F_{\text{pseudostigma}}$ (F) for radium activities and isotope ratios in sample 1, 2, and 3. All values are represented in pCi/L except $^{228}\text{Ra}/^{226}\text{Ra}$ (dimensionless).

Analyte	Sample 1			Sample 2			Sample 3		
	MPV	Q1-Q3	F	MPV	Q1-Q3	F	MPV	Q1-Q3	F
^{226}Ra	676	513 - 916	299	1420	1170 - 1840	497	526	425 - 659	173
^{228}Ra	722	616 - 780	122	1520	1280 - 1630	256	928	765 - 998	173
$^{228}\text{Ra}/^{226}\text{Ra}$	0.86	0.75 - 1.39	0.47	0.82	0.74 - 1.45	0.52	1.41	1.32 - 2.17	0.63

Two labs used modified versions of EPA methods to pre-concentrate radium from the samples before analyses by alpha particle spectroscopy, Rn emanation counting in a scintillation cell, or beta particle spectroscopy (e.g., EPA Methods 903.0, 903.1, and 904.0, respectively). One lab added a ^{225}Ra tracer to the samples and then pre-concentrated radium using manganese oxide (MnO_2) and a Diphonix resin. Radioactivity measurements were performed by alpha

1
2
3 spectrometry and the ^{226}Ra activity was corrected for chemical yield based on the observed
4 activity of the alpha peak at 7.07 MeV (^{217}At , a progeny of ^{225}Ra). Complete details of the
5 method were not provided by the lab but similar methods have been included elsewhere³⁸.
6
7
8 Another lab used co-precipitation methods to remove and concentrate ^{226}Ra from the samples
9
10 according to EPA method 903.1. Radium was co-precipitated with barium-sulfate and the
11 precipitate was then dissolved with ethylenediaminetetraacetic acid (EDTA) and stored for
12
13 ingrowth of ^{222}Rn . ^{222}Rn alpha activity measured by scintillation counting was used to determine
14
15 the ^{226}Ra activity. These two labs also precipitated ^{228}Ra with barium and lead sulfate according
16
17 to EPA method 904.0. Lead sulfate precipitates were re-digested with EDTA and precipitated
18
19 with yttrium oxalate, which was then purified, and transferred to a planchet for gas proportional
20
21 counting of ^{228}Ac , a daughter of ^{228}Ra . One lab also noted that sub aliquots of the dissolved
22
23 precipitate were saved to determine the barium yield and estimate radium recovery from the
24
25 sample.
26
27
28
29
30
31
32

33 All but one of the participating labs were able to report detectable Ra concentrations in
34 the three oil and gas wastewaters (Figure 5). The only method that reported below detectable
35 concentrations was NAA; Ra is not considered a detectable element using NAA. The rest of the
36 values reported had ^{226}Ra and ^{228}Ra activities that were within the 25th to 75th percentiles for
37 O&G wastewaters from the Appalachian Basin and were generally of acceptable quality (Table
38 3; Figure 5); all ^{226}Ra results were considered to be acceptable quality while one ^{228}Ra value was
39 considered to be questionable quality along with another value that was of unacceptable quality.
40
41 Both ^{228}Ra values that were of questionable or unacceptable quality were from gamma ray
42 spectroscopy methods. Due to the large number of other acceptable quality analyses (n=7) by
43 gamma ray spectroscopy methods, the unacceptable or questionable Ra measurements do not
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

1
2
3 appear to be a result of using gamma ray spectroscopy and could instead be attributed to lab
4
5 specific methods or other potential sources of bias.
6

7
8 Results from this inter-laboratory comparison suggests that reported Ra activities in O&G
9
10 wastewaters could be within $\pm 50\%$ of the MPV (Figure 6). Comparisons of the reported values to
11
12 the MPV for radium activity in the three samples suggests that there is likely more inaccuracy in
13
14 ^{226}Ra measurements than ^{228}Ra measurements, as ^{226}Ra values were approximately $\pm 50\%$ from
15
16 the MPV while ^{228}Ra values were approximately $\pm 30\%$ from the MPV. As a comparison, $\pm 20\%$
17
18 accuracy has been estimated for ^{226}Ra in drinking water assessments⁶³. In another study, up to
19
20 $\pm 60\%$ accuracy for ^{226}Ra and $\pm 20\%$ for ^{228}Ra were reported in seawater samples⁶⁴.
21
22

23
24 Figure 5. Data quality for Ra concentrations reported in sample 1, 2, and 3. Acceptable,
25
26 questionable, and unacceptable quality were based on z-score calculations when the number of
27
28 values were ≥ 7 for a given analyte.

29
30 The differences in ^{226}Ra and ^{228}Ra activities measured by labs also influenced the
31
32 Raisotope ratios. The 25th to 75th percentile ratios for $^{228}\text{Ra}/^{226}\text{Ra}$ ranged from 0.8 - 1.5 in sample
33
34 1, 0.8 - 1.4 in sample 2, and 1.4 - 2.4 in sample 3 (Table 3). As a comparison, $^{228}\text{Ra}/^{226}\text{Ra}$ ratios
35
36 for all produced waters from the Appalachian Basin can range from 0 to 4⁶⁵. These ratios are
37
38 often used to fingerprint wastewaters produced from unconventional shale reservoirs compared
39
40 to conventional oil and gas reservoirs as the higher ^{238}U (parent isotope for ^{226}Ra) concentrations
41
42 in organic-rich shales relative to conventional sandstone formations can result in low $^{228}\text{Ra}/^{226}\text{Ra}$
43
44 ratios (e.g., median value for Marcellus Shale is 0.12)⁵⁸ that are traceable in suspected
45
46 contamination events^{7, 66}. None of the wastewaters analyzed in this study were from O&G wells
47
48 drilled into the Marcellus Shale, which was also reflective of the higher $^{228}\text{Ra}/^{226}\text{Ra}$ ratios (e.g.,
49
50 all MPVs greater than 0.9) measured by the participating labs. The range in $^{228}\text{Ra}/^{226}\text{Ra}$ ratios
51
52 reported by the labs did not influence the ability of this tracer to confirm that the fluids were not
53
54
55
56
57
58
59
60

1
2
3 from the Marcellus Shale. However, there could be instances where labs that under-reported
4 ^{226}Ra and over-reported ^{228}Ra activities (e.g., Lab 4, Lab 12, and Lab 14) in the three samples
5
6 could measure higher $^{228}\text{Ra}/^{226}\text{Ra}$ activities in a Marcellus Shale wastewater, which could be
7
8 interpreted as fluids from conventional oil and gas reservoirs. This variability in $^{228}\text{Ra}/^{226}\text{Ra}$
9
10 ratios and radium activities could have implications for how wastewaters are identified or
11
12 managed and it is therefore important to determine why these inaccuracies exist.
13
14
15

16
17 There are several factors that could influence the variability in the reported ^{226}Ra
18
19 activities including (1) Rn leakage, (2) gamma photon attenuation, or (3) calibration
20
21 inconsistencies^{37, 40-42}. Rn diffusion through storage containers and inconsistent preparation
22
23 procedures between samples and standards can result in inaccurate measurements of ^{226}Ra
24
25 daughter products⁴⁰. Potential concerns with losses of daughter products can be resolved by
26
27 measuring ^{226}Ra directly at 186 keV with gamma ray spectroscopy or at 4.8 MeV using alpha
28
29 particle spectroscopy. In this study, reported values by labs using either of these methods were
30
31 compared to determine if these indirect or direct counting techniques influenced the ^{226}Ra
32
33 activities. However, there was no consistency in the reported Ra activities by labs using either of
34
35 these methods. For instance, lab 13 measured ^{226}Ra activities using daughter products and had
36
37 average z-scores of -1.24 (-45% from MPV) for the three O&G wastewaters, while lab 3 also
38
39 measured ^{226}Ra using daughter products but had average z-scores of 0.67 (24% from MPV). In
40
41 other words, both labs used similar methods but values reported by lab 3 were often two times
42
43 higher than the values reported by lab 13. Interestingly, labs that measured ^{226}Ra directly also
44
45 showed significant variability despite being unaffected by potential biases from Rn leakage.
46
47
48
49 Among the labs that used direct measurements, average z-scores were -0.5 (-20% from MPV) for
50
51 Lab 11 and 14b, 0.2 (~5% from MPV) for lab 3, and 0.9 for Lab 7a (34% from MPV). Because
52
53
54
55
56
57
58
59
60

1
2
3 these z-scores span almost the entire range of calculated values, it does not appear that indirect
4 vs direct counting methods had a significant influence on the accuracy of the results. However,
5 an inter-laboratory comparison performed with a greater number of laboratories could examine
6 this possibility with greater statistical certainty.
7
8
9
10
11

12 Other potential sources of bias could occur by not accounting for photon attenuation in
13 samples relative to the O&G wastewaters^{41, 42}. Specifically, the attenuation of photons by
14 solutions with different densities or chemical matrixes relative to standard solutions can result in
15 negative bias (i.e., under-reporting of Ra activities). While attenuation effects are well known in
16 the literature, they are often unaccounted for in O&G wastewaters^{40,41}. In the current study, only
17 one lab (lab 7a) accounted for photon attenuation by using a high-salinity matrix-matched
18 radium standard to calibrate gamma ray spectroscopy equipment. Additionally, other wet-
19 chemical methods used by labs 8 and 9 were not affected by attenuation biases since Ra was
20 separated from solution prior to analysis. When grouped together, these labs (labs 7a, 8, and 9)
21 consistently reported ²²⁶Ra activities that were 20 to 50% higher than the MPV. It is possible that
22 these labs are closer to the true ²²⁶Ra activity of the wastewaters as they are likely unaffected by
23 attenuation bias or bias from Rn leakage. However, this is uncertain as other methods by lab 3
24 and lab 7b that were likely influenced by these potential sources of bias also over-reported Ra
25 activities by >20%.
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43

44 Figure 6. The % difference of measured Ra activities by individual labs based on comparisons to
45 the MPV. A summarized description of each labs methods is included in Table S5.
46
47

48 Regardless of the source and magnitude of these potential sources of bias, they appear to
49 have a consistent influence on the Ra activities reported by individual labs in this inter-laboratory
50 comparison. This is supported by the calculated z-scores for each of the labs which indicated that
51 if a lab reported high or low activity for one of the samples, they reported high or low activity for
52
53
54
55
56
57
58
59
60

1
2
3 all of the samples. For instance, calculated z-scores for lab 13 were -0.9 (-39% from MPV), -1.3
4 (-44% from MPV), and -1.5 (-52% from MPV) for sample 1, 2, and 3 respectively. In other
5
6 words, the similar z-scores for all samples analyzed by individual labs suggests that lab methods
7
8 were precise but inaccurate. The precision of the labs are encouraging in suggesting that the
9
10 inaccuracies in reported ^{226}Ra activities could be resolved by (1) confirming that the standards
11
12 used for calibrating equipment are accurate, (2) ensuring consistent Rn entrapment between
13
14 standards and samples, and (3) accounting for potential attenuation differences in standards and
15
16 samples. However, future work is needed to identify which of these factors has the most impact
17
18 on the reported activities in O&G wastewaters. We recommend that a high salinity solution with
19
20 certified Ra activities be developed (e.g., NIST standard) to help alleviate the potential sources
21
22 of bias from attenuation. Labs could also correct for potential negative bias from attenuation by
23
24 making their own high salinity, matrix matched Ra standards. We also recommend that labs
25
26 measuring ^{226}Ra activities in O&G wastewaters by ^{214}Bi or ^{214}Pb should perform simple quality
27
28 control metrics such as verifying potential bias from Rn leakages by confirming that
29
30 measurements using 186 keV or 352 keV, 609 keV, etc are comparable.
31
32
33
34
35
36

37 **Radium measurements in solids.** Most of the labs (9 of 10) measured radioactivity in the solid
38
39 samples by gamma spectroscopy. Of these nine labs, eight labs directly measured radioactivity
40
41 without chemically separating radium from the solids, i.e. radium activities were directly
42
43 measured on the solids as received. One lab did not describe their sample preparation, but stated
44
45 that they performed direct measurements using gamma spectroscopy. Because the study was
46
47 anonymous, only the sample preparation procedures described when the data was submitted
48
49 could be used for data interpretations. Radioactivity was determined in varying geometries that
50
51 were often incubated for >21 days prior to analysis, however, only two labs reported performing
52
53
54
55
56
57
58
59
60

a self-attenuation correction based on the Cutshall method or with any other attenuation method^{42, 67, 68}. ²²⁶Ra activity was often determined based on the average of the daughter products (²¹⁴Pb at 295.2 keV and 351.9 keV, ²¹⁴Bi at 609.3 keV) but also directly at 186.2 keV with a correction factor. ²²⁸Ra activity was determined based on its daughter product activity, ²²⁸Ac at 911.2 keV or at 463 keV. Detector efficiencies were determined using various standards, including ores from the Canadian Certified Reference Materials Project (CCRMP) (BL4a ore, DL1a ore, BL5 ore and Oka2 ore) and other traceable standards (IAEA-385 and NIST 4353a).

One lab did not perform their analysis by gamma spectroscopy. Instead, they digested 0.25 – 0.5 grams of solid using nitric acid, hydrogen peroxide, and hydrochloric acid according to EPA Method 3050B. Thereafter, ²²⁸Ra was pre-concentrated with barium/lead sulfate and then purified by precipitation from EDTA solution. After an ingrowth period for ²²⁸Ac from ²²⁸Ra, yttrium oxalate carried ²²⁸Ac, which was then purified, and measured for beta activity using a gas-flow proportional counting system according to EPA Method 904.0. Likewise, ²²⁶Ra was pre-concentrated with barium sulfate, sealed for ²²²Rn ingrowth, after which the ²²²Rn alpha activity was determined using alpha spectrometry (EPA method 903.1). A summary table with each of the methods used for determining the radium activities in the solids is included in the supporting information (Table S6).

Table 4. The most probable value (MPV), 25th percentile (Q1), 75th percentile (Q3), and $F_{\text{pseudostigma}}$ (F) for Ra activities and isotope ratios in solid samples 1, 2, 3, and 4. All values are represented as pCi/gram except ²²⁸Ra/²²⁶Ra (dimensionless).

Solid Sample	Analyte	MPV	Q1-Q3	F
SS1	²²⁶ Ra	1.82	1.67-1.97	0.22
	²²⁸ Ra	1.04	0.97-1.19	0.16
	²²⁸ Ra/ ²²⁶ Ra	0.59	0.53-0.66	0.09
SS2	²²⁶ Ra	10.3	10.2-11.8	1.21
	²²⁸ Ra	0.55	0.50-0.65	0.10
	²²⁸ Ra/ ²²⁶ Ra	0.05	0.05-0.06	0.01

SS3	^{226}Ra	6.50	6.20-7.22	0.75
	^{228}Ra	1.18	1.16-1.31	0.11
	$^{228}\text{Ra}/^{226}\text{Ra}$	0.19	0.16-0.21	0.04
SS4	^{226}Ra	3.00	2.95-3.36	0.30
	^{228}Ra	1.09	1.03-1.25	0.17
	$^{228}\text{Ra}/^{226}\text{Ra}$	0.36	0.33-0.40	0.05

All labs reported measurable activities of ^{226}Ra and ^{228}Ra in the solid samples (Table 4) that were generally of acceptable quality (Figure 7). Ra data quality was comparable to a previous inter-laboratory comparison performed by the International Atomic Energy Agency (IAEA) on a sea sediment⁶⁹. In our study, 14% (6 of 44) of the reported ^{226}Ra values were questionable or unacceptable which compares well to 18% from the IAEA study; while 25% (11 of 44) of the reported ^{228}Ra values were questionable or unacceptable, compared to 56.5% from the IAEA study⁶⁹.

Figure 7. Data quality for Ra activities reported in solid samples 1, 2, 3, and 4. Acceptable, questionable, and unacceptable designations were based on z-score calculations when the number of values were ≥ 7 for a given analyte.

All ^{226}Ra activities that were questionable or unacceptable were determined by gamma spectroscopy methods; three of these analyses were performed with 2 hours of counting time (and two of these analyses were performed in an unknown geometry), while the other three analyses were counted for over 16 hours. It is likely that these questionable or unacceptable measurements were because of lab specific methods (i.e., sample prep, counting time, and efficiency calibration), and not because of the use of gamma spectroscopy. For ^{228}Ra , eight of the eleven questionable or unacceptable data were determined by gamma spectroscopy. The other three were determined by beta counting after chemical separation. Amongst the questionable or unacceptable data determined by gamma spectroscopy, six analyses were likely performed after short counting times (< 24 hours).

1
2
3 The results from this inter-laboratory comparison suggest that the reported Raactivities of
4 O&G impacted solids could be within $\pm 20\%$ from the MPV (Figure 8). Variations in the reported
5 Ra measurements in the solid could be attributed to a number of factors, including (1) sample
6 geometry (fill height), (2) unintentional differences in Rn sealing between samples and
7 standards, (3) insufficient counting time, and (4) sample attenuation^{42, 68, 70}. All the reported
8 ²²⁶Ra activities in SS1 and SS3 were of acceptable or questionable quality. SS1 had the lowest
9 activity, while SS2 had the highest activity. Yet SS2 and SS4 both had reported values that were
10 unacceptable. There was therefore no reason to believe that the quality of the data was influenced
11 by the activity of the samples. Furthermore, the densities and matrix/chemical composition of
12 these solids were different, yet analysis of the z-scores showed no systematic influence on the
13 reported activities by sample type. Some labs over-estimated the radium activities in one solid
14 sample, but under-estimated it in another sample. As such, it was difficult to conclude if the
15 questionable or unaccepted data were solely due to density and matrix differences. However,
16 large % differences in the reported activities by labs that did not account for density or potential
17 matrix differences with attenuation corrections suggests that this was likely still an issue.

18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38 As with gamma spectroscopy measurements of liquid samples, another potential cause of
39 discrepancy could be whether Ra activity was determined directly at 186 keV, or indirectly from
40 the daughter products (²¹⁴Pb or ²¹⁴Bi). Direct measurement at 186 keV can result in erroneous
41 data, if there is U in the sample, as the gamma decay of ²³⁵U (185.7 keV) interferes with ²²⁶Ra
42 measurements at 186.2 keV. An interference correction must be performed if this is the case. If
43 the daughter products are used instead, then improper sealing of counting vessels will lead to
44 escape of Rn gas, which will result in inaccurate measurements of ²²⁶Ra decay products³⁷.

45
46
47
48
49
50
51
52
53
54 Figure 8. Range in the % difference of reported radium activities with acceptable quality based
55 on comparisons to the MPV.
56
57
58
59
60

1
2
3 Alpha spectrometry following chemical separation of Ra produced data of acceptable
4
5 quality for ^{226}Ra ; however, 3 out of 4 measurements for ^{228}Ra using beta particle counting were
6
7 of unacceptable quality. This suggested that beta counting by the gas-flow proportional counting
8
9 system following chemical separation was not a reliable method for determining the ^{228}Ra
10
11 activities of the solids.
12
13

14
15 Close inspection of the z-scores allows us to identify methods and labs that produced data
16
17 of consistently high quality. These labs reported values with low z-scores, indicating that the
18
19 measured activities were likely accurate, and none of the reported values were rejected across the
20
21 four solids samples. We were able to identify that for reliable Ra measurements, gamma
22
23 spectroscopy produced the most accurate results. In addition to this, labs that used ores from the
24
25 CCRMP reported values that were acceptable quality. The labs, lab 3 and lab 7, that also
26
27 accounted for attenuation using a point-source correction by the Cutshall technique, produced the
28
29 highest quality data. When these methods were used, the reported Ra activities were often within
30
31 $< \pm 5\%$ of the MPV. We therefore recommend gamma spectroscopy methods that incorporate
32
33 certified Ra standards, such as the ores from CCRMP, and account for the self-attenuation in
34
35 solid samples that result from density and matrix differences between the calibration standard
36
37 and the unknown sample. Furthermore, we recommend longer counting times for samples with
38
39 activities close to environmental background (> 24 hours), and a close attention to the sample
40
41 preparation concerning the geometry, fill height and Rn gas entrapment.
42
43
44
45
46

47 **Limitations of the inter-laboratory comparison**

48
49 There were several limitations of the current study that the authors would like to
50
51 acknowledge. First, none of the labs were required to analyze samples multiple times. Therefore,
52
53 there was no way to adequately assess how precise individual labs were in analyzing the O&G
54
55
56
57
58
59
60

1
2
3 wastewaters. We also explored several methods for analyzing the precision of the data; however,
4 these methods are heavily dependent on how outliers are excluded from the data. Therefore, we
5
6 relied on comparisons to the median (i.e., most probable value) to show how much agreement
7
8 there was among the reported values. Using the median as the MPV could influence our
9
10 interpretations of the accuracy of these measurements, however, this is a viable statistical method
11
12 that is commonly used in inter-laboratory studies⁴⁵. Testing the accuracy of each lab's
13
14 measurements could be resolved by requiring all labs to analyze certified standards for the
15
16 analytes in this study but the availability and cost of these standards prevented this comparison.
17
18 A well characterized check standard from the Spring 2018 USGS inter-laboratory study ⁷⁰ was
19
20 sent to participating labs for cation and anion analyses. However, not all of the labs analyzed the
21
22 sample. Because most labs did not report concentrations for the USGS sample, results for these
23
24 reference materials were not used to assess the accuracy of the labs. Another limitation of the
25
26 study was that statistical comparisons between various methods were not possible due to the
27
28 majority of labs performing one method of analysis. In some cases there were also not enough
29
30 reported values to determine the accuracy of the measurements (e.g., most of the trace
31
32 metal(loid)s) using the MPV method. Other potential factors that could influence the results,
33
34 such as dilution errors, were not explored but could be resolved by spiking internal standards into
35
36 all samples sent out for inter-laboratory comparisons and requiring labs to measure analytes
37
38 within the standard. Regardless of these limitations, there was relatively good agreement among
39
40 the reported values and we were able to comment on the accuracy of many of the methods used
41
42 for analyzing solid and liquid wastes from O&G development.
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

Conclusions and recommendations

Major cations, minor cations, and anions. The majority of laboratories that participated in this study reported values for major and minor cations and anions in the O&G wastewaters that were in good agreement with the MPVs. Accuracies for these cations and anions were similar to other inter-laboratory comparisons analyzing freshwaters. Depending on the detection limits of the analytical equipment, we recommend diluting samples approximately 10-1,000 times before analysis on an ICP-OES, ICP-MS, or IC, and using internal standards to correct for potential matrix interferences along with check standards to verify calibration curves. Combined major and minor cation and anion chemistry data supports the use of Sr/Ca and B/Cl ratios for tracing O&G wastewaters. However, the range in reported Cl/Br values in this inter-laboratory comparison indicate that geochemical interpretations using this ratio could have uncertainty and should be acknowledged when using data sets with Cl/Br ratios from multiple laboratories.

Trace metal(loid) measurements. In contrast to the major and minor cations, few reliable values were reported for trace metal(loid)s. The number of reported values were also limited by high method detection limits relative to the trace metal(loid) concentrations in the wastewaters. Reporting limits for trace metal(loid)s were often above or near drinking water standards, which could lead to difficulties regulating high salinity oil and gas wastewaters based on trace metal concentrations.

Radium measurements in liquids. The majority of laboratories were able to report values for Ra activities in high salinity brines, but values showed greater variability between laboratories than major and minor cations or anions. Compared to previous inter-laboratory studies of naturally occurring radioactivity in seawater and freshwater, the accuracy of reported values in this study were very similar, demonstrating that many participating laboratories using a

1
2
3 variety of methods for O&G wastewater analyses can produce acceptable quality data. However,
4
5 the range in values reported also suggests that individual laboratories are over-reporting or
6
7 under-reporting Ra activities by $\pm 50\%$ likely due to calibration inconsistencies among labs,
8
9 radon leakage, or self-attenuation. We recommend that a high salinity brine Ra standard be
10
11 developed to help eliminate these sources of bias.
12
13
14

15 **Radium measurements in solids.** Ra analyses of solid samples were more accurate than
16
17 liquid measurements, deviating by $\pm 20\%$ from the MPV but had less consistency in the %
18
19 differences reported by individual labs; i.e., labs over-estimated the Ra activities in one sample,
20
21 but under-estimated it in other samples. Some of this variability could be minimized by longer
22
23 counting times for samples with activities close to environmental background (> 24 hours),
24
25 correcting for gamma attenuation, and paying close attention to sample preparation procedures
26
27 (e.g., geometry, fill height, and radon gas entrapment).
28
29
30
31

32 **Acknowledgments**

33
34

35 The authors would also like to thank the ALS Life Sciences division in Fort Collins, CO and
36
37 Geochemical Testing in Somerset, PA for participating in this inter-laboratory comparison. All
38
39 authors participated equally in the measurements for this inter-laboratory study. Author order is
40
41 based on contributions to data processing, experimental design, and manuscript preparation.
42
43
44

45 **Author disclosure statement**

46
47

48 There are no competing financial interests.
49
50
51
52
53
54
55
56
57
58
59
60

References

1. De Gouw, J.; Parrish, D.; Frost, G.; Trainer, M., Reduced emissions of CO₂, NO_x, and SO₂ from US power plants owing to switch from coal to natural gas with combined cycle technology. *Earth's Future* **2014**, *2*, (2), 75-82.
2. Keranen, K. M.; Weingarten, M.; Abers, G. A.; Bekins, B. A.; Ge, S., Sharp increase in central Oklahoma seismicity since 2008 induced by massive wastewater injection. *Science* **2014**, *345*, (6195), 448-451.
3. Peischl, J.; Ryerson, T.; Aikin, K.; Gouw, J.; Gilman, J.; Holloway, J.; Lerner, B.; Nadkarni, R.; Neuman, J.; Nowak, J., Quantifying atmospheric methane emissions from the Haynesville, Fayetteville, and northeastern Marcellus shale gas production regions. *Journal of Geophysical Research: Atmospheres* **2015**, *120*, (5), 2119-2139.
4. Llewellyn, G. T.; Dorman, F.; Westland, J.; Yoxtheimer, D.; Grieve, P.; Sowers, T.; Humston-Fulmer, E.; Brantley, S. L., Evaluating a groundwater supply contamination incident attributed to Marcellus Shale gas development. *Proceedings of the National Academy of Sciences* **2015**, *112*, (20), 6325-6330.
5. Hildenbrand, Z. L.; Carlton Jr, D. D.; Fontenot, B. E.; Meik, J. M.; Walton, J. L.; Taylor, J. T.; Thacker, J. B.; Korlie, S.; Shelor, C. P.; Henderson, D., A comprehensive analysis of groundwater quality in the Barnett Shale region. *Environmental science & technology* **2015**, *49*, (13), 8254-8262.
6. Burgos, W. D.; Castillo-Meza, L.; Tasker, T. L.; Geeza, T. J.; Drohan, P. J.; Liu, X.; Landis, J. D.; Blotvogel, J.; McLaughlin, M.; Borch, T., Watershed-scale impacts from surface water disposal of oil and gas wastewater in western Pennsylvania. *Environmental Science & Technology* **2017**, *51*, (15), 8851-8860.
7. Alessi, D. S.; Zolfaghari, A.; Kletke, S.; Gehman, J.; Allen, D. M.; Goss, G. G., Comparative analysis of hydraulic fracturing wastewater practices in unconventional shale development: Water sourcing, treatment and disposal practices. *Canadian Water Resources Journal/Revue canadienne des ressources hydriques* **2017**, *42*, (2), 105-121.
8. Lutz, B. D.; Lewis, A. N.; Doyle, M. W., Generation, transport, and disposal of wastewater associated with Marcellus Shale gas development. *Water Resources Research* **2013**, *49*, (2), 647-656.
9. Mantell, M. E., Produced water reuse and recycling challenges and opportunities across major shale plays. In United States Environmental Protection Agency office of Research and Development, 2011: USEPA Technical Workshops for the Hydraulic Fracturing Study: Water Resources Management, Arlington, Va, 2011.
10. Vengosh, A.; Jackson, R. B.; Warner, N.; Darrah, T. H.; Kondash, A., A critical review of the risks to water resources from unconventional shale gas development and hydraulic fracturing in the United States. *Environmental science & technology* **2014**, *48*, (15), 8334-8348.

11. Shaffer, D. L.; Arias Chavez, L. H.; Ben-Sasson, M.; Romero-Vargas Castrillón, S.; Yip, N. Y.; Elimelech, M., Desalination and reuse of high-salinity shale gas produced water: drivers, technologies, and future directions. *Environmental science & technology* **2013**, 47, (17), 9569-9583.
12. Pichtel, J., Oil and gas production wastewater: Soil contamination and pollution prevention. *Applied and environmental soil science* **2016**, 2016.
13. Clark, C.; Veil, J. Produced water volumes and management practices in the United States. United States Department of Energy, Argonne National Laboratory: Argonne, IL, **2009**.
14. Tasker, T.; Burgos, W.; Piotrowski, P.; Castillo-Meza, L.; Blewett, T.; Ganow, K.; Stallworth, A.; Delompré, P.; Goss, G.; Fowler, L., Environmental and Human Health Impacts of Spreading Oil and Gas Wastewater on Roads. *Environmental science & technology* **2018**, 52, (12), 7081-7091.
15. Echchelh, A.; Hess, T.; Sakrabani, R., Reusing oil and gas produced water for irrigation of food crops in drylands. *Agricultural Water Management* **2018**, 206, 124-134.
16. Hladik, M. L.; Focazio, M. J.; Engle, M., Discharges of produced waters from oil and gas extraction via wastewater treatment plants are sources of disinfection by-products to receiving streams. *Science of the Total Environment* **2014**, 466, 1085-1093.
17. Skalak, K. J.; Engle, M. A.; Rowan, E. L.; Jolly, G. D.; Conko, K. M.; Benthem, A. J.; Kraemer, T. F., Surface disposal of produced waters in western and southwestern Pennsylvania: Potential for accumulation of alkali-earth elements in sediments. *International Journal of Coal Geology* **2014**, 126, 162-170.
18. Lauer, N. E.; Warner, N. R.; Vengosh, A., Sources of Radium Accumulation in Stream Sediments near Disposal Sites in Pennsylvania: Implications for Disposal of Conventional Oil and Gas Wastewater. *Environmental science & technology* **2018**, 52, (3), 955-962.
19. Kassotis, C. D.; Tillitt, D. E.; Davis, J. W.; Hormann, A. M.; Nagel, S. C., Estrogen and androgen receptor activities of hydraulic fracturing chemicals and surface and ground water in a drilling-dense region. *Endocrinology* **2014**, 155, (3), 897-907.
20. Elliott, E. G.; Ettinger, A. S.; Leaderer, B. P.; Bracken, M. B.; Deziel, N. C., A systematic evaluation of chemicals in hydraulic-fracturing fluids and wastewater for reproductive and developmental toxicity. *Journal of Exposure Science and Environmental Epidemiology* **2017**, 27, (1), 90.
21. Shih, J.-S.; Saiers, J. E.; Anisfeld, S. C.; Chu, Z.; Muehlenbachs, L. A.; Olmstead, S. M., Characterization and analysis of liquid waste from Marcellus Shale gas development. *Environmental science & technology* **2015**, 49, (16), 9557-9565.
22. Kolesar Kohl, C. A.; Capo, R. C.; Stewart, B. W.; Wall, A. J.; Schroeder, K. T.; Hammack, R. W.; Guthrie, G. D., Strontium isotopes test long-term zonal isolation of injected and

1
2
3 Marcellus formation water after hydraulic fracturing. *Environmental science & technology* **2014**,
4 48, (16), 9867-9873.
5

6
7 23. Stewart, B. W.; Chapman, E. C.; Capo, R. C.; Johnson, J. D.; Graney, J. R.; Kirby, C. S.;
8 Schroeder, K. T., Origin of brines, salts and carbonate from shales of the Marcellus Formation:
9 Evidence from geochemical and Sr isotope study of sequentially extracted fluids. *Applied*
10 *Geochemistry* **2015**, 60, 78-88.
11

12 24. Warner, N. R.; Jackson, R. B.; Darrah, T. H.; Osborn, S. G.; Down, A.; Zhao, K.; White, A.;
13 Vengosh, A., Geochemical evidence for possible natural migration of Marcellus Formation brine
14 to shallow aquifers in Pennsylvania. *Proceedings of the National Academy of Sciences* **2012**,
15 109, (30), 11961-11966.
16

17 25. Pancras, J. P.; Norris, G. A.; Landis, M. S.; Kovalcik, K. D.; McGee, J. K.; Kamal, A. S.,
18 Application of ICP-OES for evaluating energy extraction and production wastewater discharge
19 impacts on surface waters in Western Pennsylvania. *Science of the Total Environment* **2015**, 529,
20 21-29.
21
22

23 26. Morishige, Y.; Kimura, A., Ionization interference in inductively coupled plasma-optical
24 emission spectroscopy. SEI TECHNICAL REVIEW-ENGLISH EDITION **2008**, 66, 106.
25

26 27. Botto, R. I., Method for correcting for acid and salt matrix interferences in ICP-AES.
27 *Spectrochimica Acta Part B: Atomic Spectroscopy* **1985**, 40, (1-2), 397-412.
28

29 28. Dams, R. F.; Goossens, J.; Moens, L., Spectral and non-spectral interferences in inductively
30 coupled plasma mass-spectrometry. *Microchimica Acta* **1995**, 119, (3-4), 277-286.
31
32

33 29. Poehle, S.; Schmidt, K.; Koschinsky, A., Determination of Ti, Zr, Nb, V, W and Mo in
34 seawater by a new online-preconcentration method and subsequent ICP-MS analysis. *Deep Sea*
35 *Research Part I: Oceanographic Research Papers* **2015**, 98, 83-93.
36

37 30. Environmental Protection Agency. EPA Method 903.0: Alpha-Emitting Radium Isotopes in
38 Drinking Water. Available at [https://www.epa.gov/sites/production/files/2015-](https://www.epa.gov/sites/production/files/2015-08/documents/method_903-0_1980.pdf)
39 [08/documents/method_903-0_1980.pdf](https://www.epa.gov/sites/production/files/2015-08/documents/method_903-0_1980.pdf)
40
41

42 31. Environmental Protection Agency. EPA Radium 226 in drinking water: Radon Emanation
43 Technique Method 903.1. Available at [https://www.epa.gov/sites/production/files/2015-](https://www.epa.gov/sites/production/files/2015-06/documents/epa-903.1.pdf)
44 [06/documents/epa-903.1.pdf](https://www.epa.gov/sites/production/files/2015-06/documents/epa-903.1.pdf)
45

46 32. Environmental Protection Agency. EPA Gamma Emitting Radionuclides in drinking water:
47 Method 901.1. Available at [https://www.epa.gov/sites/production/files/2015-06/documents/epa-](https://www.epa.gov/sites/production/files/2015-06/documents/epa-901.1.pdf)
48 [901.1.pdf](https://www.epa.gov/sites/production/files/2015-06/documents/epa-901.1.pdf)
49

50 33. Environmental Protection Agency. EPA prescribed procedures for measurement of
51 radioactivity in drinking water. Available at
52 <https://nepis.epa.gov/Exe/ZyPDF.cgi/30000QHM.PDF?Dockey=30000QHM.PDF>
53
54
55
56
57
58
59
60

- 1
2
3 34. Zhang, T.; Bain, D.; Hammack, R.; Vidic, R. D., Analysis of radium-226 in high salinity
4 wastewater from unconventional gas extraction by inductively coupled plasma-mass
5 spectrometry. *Environmental Science & Technology* **2015**, 49, (5), 2969-2976.
6
7
8 35. Jia, G.; Jia, J., Determination of radium isotopes in environmental samples by gamma
9 spectrometry, liquid scintillation counting and alpha spectrometry: a review of analytical
10 methodology. *Journal of environmental radioactivity* **2012**, 106, 98-119.
11
12 36. Nelson, A. W.; May, D.; Knight, A. W.; Eitrheim, E. S.; Mehrhoff, M.; Shannon, R.; Litman,
13 R.; Schultz, M. K., Matrix complications in the determination of radium levels in hydraulic
14 fracturing flowback water from Marcellus Shale. *Environmental Science & Technology Letters*
15 **2014**, 1, (3), 204-208.
16
17 37. Purkl, S.; Eisenhauer, A., A rapid method for α -spectrometric analysis of radium isotopes in
18 natural waters using ion-selective membrane technology. *Applied radiation and isotopes* **2003**,
19 *59*, (4), 245-254.
20
21 38. Diab, H. M.; Abdellah, W. M., Validation of ²²⁶Ra and ²²⁸Ra measurements in water
22 samples using gamma spectrometric analysis. *Journal of Water Resource and Protection* **2013**,
23 *5*, (08), 53.
24
25 39. Rovenská, K.; Jiránek, M., Radon diffusion coefficient measurement in waterproofings—A
26 review of methods and an analysis of differences in results. *Applied Radiation and Isotopes*
27 **2012**, *70*, (4), 802-807.
28
29 40. Jodłowski, P., Self-absorption correction in gamma-ray spectrometry of environmental
30 samples-an overview of methods and correction values obtained for the selected geometries.
31 *Nukleonika* **2006**, *51*, 21-25.
32
33 41. Robu, E.; Giovani, C., Gamma-ray self-attenuation corrections in environmental samples.
34 *Romanian Reports in Physics* **2009**, *61*, (2), 295-300.
35
36 42. Semkow, T. M.; Mehmood, G.; Parekh, P. P.; Virgil, M., Coincidence summing in gamma-
37 ray spectroscopy. *Nuclear Instruments and Methods in Physics Research Section A:*
38 *Accelerators, Spectrometers, Detectors and Associated Equipment* **1990**, *290*, (2-3), 437-444.
39
40 43. Hoaglin, D. C.; Mosteller, F.; Tukey, J. W., Understanding robust and exploratory data
41 analysis. Wiley Series in Probability and Mathematical Statistics, New York: Wiley, 1983, edited
42 by Hoaglin, David C.; Mosteller, Frederick; Tukey, John W. 1983.
43
44 44. United States Geological Survey. Inter-laboratory comparison study results: Spring 2018.
45 Available at https://bqs.usgs.gov/srs_study/reports/index.php (2018).
46
47 45. Environmental Protection Agency. EPA Method 200.7: Determination of Metals and Trace
48 Elements in water and wastes by Inductively Coupled Plasma-Atomic Emission Spectrometry.
49 Available at [https://www.epa.gov/sites/production/files/2015-08/documents/method_200-](https://www.epa.gov/sites/production/files/2015-08/documents/method_200-7_rev_4-4_1994.pdf)
50 [7_rev_4-4_1994.pdf](https://www.epa.gov/sites/production/files/2015-08/documents/method_200-7_rev_4-4_1994.pdf)
51
52
53
54
55
56
57
58
59
60

- 1
2
3 46. National Institute of standards and technology. Certificate of analysis for standard reference
4 material 2711. Available at [https://clu-in.org/conf/tio/xrf_082808/cd/NIST-Standard-Reference-](https://clu-in.org/conf/tio/xrf_082808/cd/NIST-Standard-Reference-Materials/NIST_SRM_2711.pdf)
5 [Materials/NIST_SRM_2711.pdf](https://clu-in.org/conf/tio/xrf_082808/cd/NIST-Standard-Reference-Materials/NIST_SRM_2711.pdf) (2018).
6
7
8 47. Epstein, M. S.; Diamondstone, B. I.; Gills, T. E., A new river sediment standard reference
9 material. *Talanta* **1989**, 36, (1-2), 141-150.
10
11 48. Blondes, MS.; Gans, KD.; Thordsen, JJ.; Reidy, ME.; Thomas, B.; Engle, MA.; Kharaka,
12 YK.; Rowan, EL. US Geological Survey National Produced Waters Geochemical Database v2.3
13 (PROVISIONAL). *United States Geological Survey*. Available at
14 [https://energy.usgs.gov/EnvironmentalAspects/EnvironmentalAspectsofEnergyProductionandUs](https://energy.usgs.gov/EnvironmentalAspects/EnvironmentalAspectsofEnergyProductionandUse/ProducedWaters.aspx)
15 [e/ProducedWaters.aspx](https://energy.usgs.gov/EnvironmentalAspects/EnvironmentalAspectsofEnergyProductionandUse/ProducedWaters.aspx) (2014).
16
17
18 49. Knoll, G. F., Radiation detection and measurement. John Wiley & Sons: 2010.
19
20 50. Harris, D. C., Quantitative chemical analysis. Macmillan: 2010.
21
22 51. Novič, M.; Lečnik, B.; Hudnik, V.; Pihlar, B., Carbonate interferences by ion
23 chromatographic determination of anions in mineral waters. *Journal of Chromatography A* **1997**,
24 764, (2), 249-256.
25
26 52. Environmental Protection Agency. EPA Consent agreement for Pennsylvania Brine
27 Treatment. Available at [https://www.epa.gov/sites/production/files/2015-](https://www.epa.gov/sites/production/files/2015-06/documents/pennsylvania_cafa.pdf)
28 [06/documents/pennsylvania_cafa.pdf](https://www.epa.gov/sites/production/files/2015-06/documents/pennsylvania_cafa.pdf) (2018).
29
30
31 53. Good, K. D.; VanBriesen, J. M., Power Plant Bromide Discharges and Downstream Drinking
32 Water Systems in Pennsylvania. *Environmental Science & Technology* **2017**, 51, (20), 11829-
33 11838.
34
35 54. Johnson, B. M.; Kanagy, L. E.; Rodgers, J. H.; Castle, J. W., Chemical, physical, and risk
36 characterization of natural gas storage produced waters. *Water, air, and soil pollution* **2008**, 191,
37 (1-4), 33-54.
38
39 55. Dresel, P. E.; Rose, A. W., Chemistry and origin of oil and gas well brines in western
40 Pennsylvania. Open-File Report OFOG **2010**, 10, (01.00).
41
42
43 56. Barbot, E.; Vidic, N. S.; Gregory, K. B.; Vidic, R. D., Spatial and temporal correlation of
44 water quality parameters of produced waters from Devonian-age shale following hydraulic
45 fracturing. *Environmental science & technology* **2013**, 47, (6), 2562-2569.
46
47
48 57. Rowan, E. L.; Engle, M. A.; Kraemer, T. F.; Schroeder, K. T.; Hammack, R. W.; Doughten,
49 M. W., Geochemical and isotopic evolution of water produced from Middle Devonian Marcellus
50 shale gas wells, Appalachian basin, Pennsylvania. *Aapg Bulletin* **2015**, 99, (2), 181-206.
51
52 58. Miller, J.; Miller, J. C., Statistics and chemometrics for analytical chemistry. Pearson
53 Education: 2018.
54
55
56
57
58
59
60

- 1
2
3 59. Sohrin, Y.; Urushihara, S.; Nakatsuka, S.; Kono, T.; Higo, E.; Minami, T.; Norisuye, K.;
4 Umetani, S., Multielemental determination of GEOTRACES key trace metals in seawater by
5 ICPMS after preconcentration using an ethylenediaminetriacetic acid chelating resin. *Analytical*
6 *Chemistry* **2008**, 80, (16), 6267-6273.
7
8
9 60. Jackson, S. L.; Spence, J.; Janssen, D. J.; Ross, A.; Cullen, J., Determination of Mn, Fe, Ni,
10 Cu, Zn, Cd and Pb in seawater using offline extraction and triple quadrupole ICP-MS/MS.
11 *Journal of analytical atomic spectrometry* **2018**, 33, (2), 304-313.
12
13 61. Szabo, Z.; Vincent, T.; Fischer, J. M.; Kraemer, T. F.; Jacobsen, E., Occurrence and
14 geochemistry of radium in water from principal drinking-water aquifer systems of the United
15 States. *Applied geochemistry* **2012**, 27, (3), 729-752.
16
17 62. Eaton, A.; Cha, Y.; Geddes, L.; Morley, K. M., Evaluation of variability in radionuclide
18 measurements in drinking water. *Journal-American Water Works Association* **2011**, 103, (5),
19 119-134.
20
21 63. Charette, M. A.; Dulaiova, H.; Gonnee, M. E.; Henderson, P. B.; Moore, W. S.; Scholten, J.
22 C.; Pham, M. K., GEOTRACES radium isotopes interlaboratory comparison experiment.
23 *Limnology and Oceanography: Methods* **2012**, 10, (6), 451-463.
24
25 64. Rowan, E.; Engle, M.; Kirby, C.; Kraemer, T., Radium content of oil-and gas-field produced
26 waters in the Northern Appalachian Basin (USA): Summary and discussion of data. *US*
27 *Geological Survey Scientific Investigations Report* **2011**, 5135, (2011), 31.
28
29 65. Warner, N. R.; Kresse, T. M.; Hays, P. D.; Down, A.; Karr, J. D.; Jackson, R. B.; Vengosh,
30 A., Geochemical and isotopic variations in shallow groundwater in areas of the Fayetteville
31 Shale development, north-central Arkansas. *Applied Geochemistry* **2013**, 35, 207-220.
32
33 66. Fares, S., Measurements of natural radioactivity level in black sand and sediment samples of
34 the Temsah Lake beach in Suez Canal region in Egypt. *Journal of Radiation Research and*
35 *Applied Sciences* **2017**, 10, (3), 194-203.
36
37 67. Cutshall, N. H.; Larsen, I. L.; Olsen, C. R., Direct analysis of ²¹⁰Pb in sediment samples:
38 self-absorption corrections. *Nuclear Instruments and Methods in Physics Research* **1983**, 206,
39 (1-2), 309-312.
40
41 68. IAES. Report on worldwide intercomparisons exercise IAES-385: Radionuclides in Irish Sea
42 Sediment. Available at https://nucleus.iaea.org/rpst/Documents/IAEA_AL_151.pdf.
43 69. Bolivar, J.; Garcia-Leon, M.; Garcia-Tenorio, R., On self-attenuation corrections in gamma-ray
44 spectrometry. *Applied radiation and isotopes* **1997**, 48, (8), 1125-1126.
45
46 70. USGS. Inter-laboratory comparison study results. Available at
47 https://bqs.usgs.gov/srs_study/reports/index.php
48
49
50
51
52
53
54
55
56
57
58
59
60

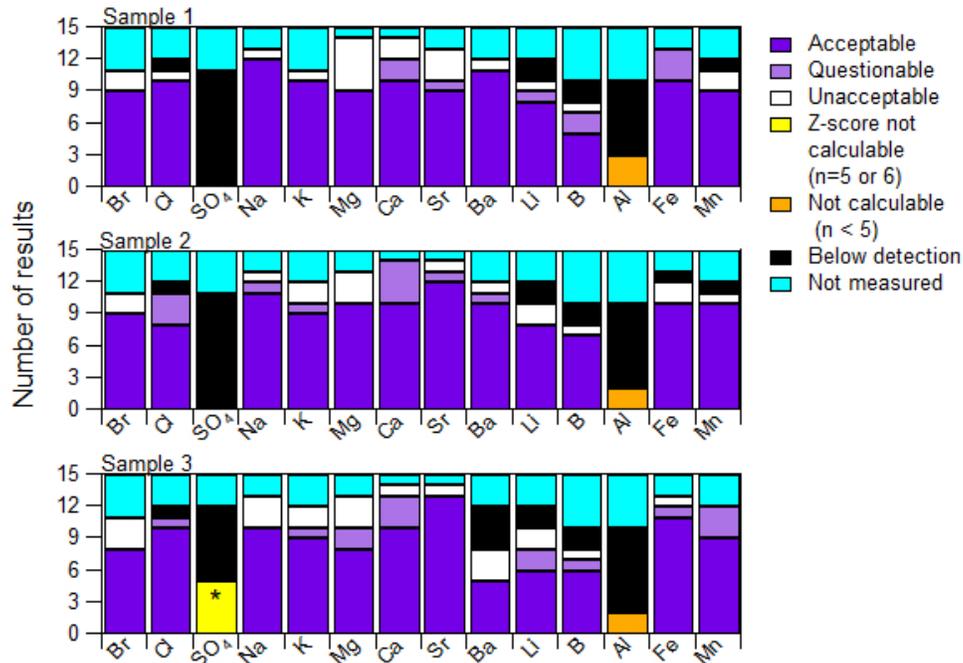


Figure 1. Data quality for major cation, minor cation, and anion concentrations reported in sample 1, 2, and 3. Acceptable, questionable, and unacceptable quality were based on z-score calculations when the number of values were ≥ 7 for a given analyte. When 5 or 6 values were reported, no z score was calculated but is noted with an asterisk as a MPV and Fpseudosigma were still calculated (i.e., Table 1). When less than 5 values were reported, no statistics were calculated.

158x110mm (96 x 96 DPI)

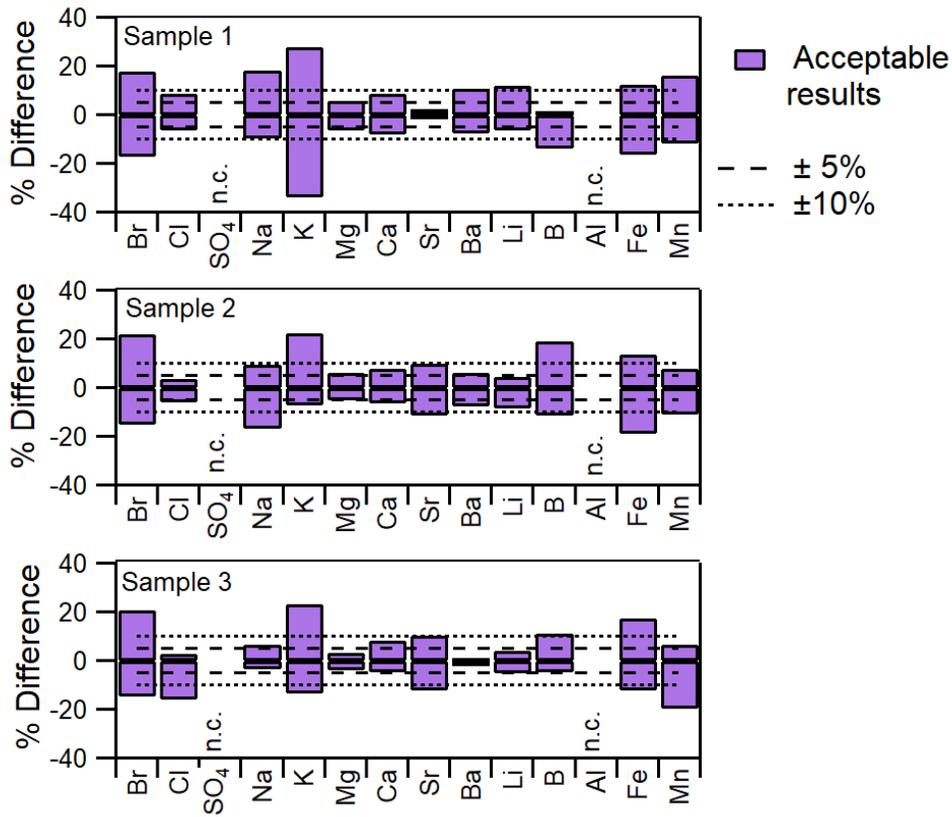


Figure 2. Range in accuracy of reported values with acceptable quality for major cation, minor cation, and trace cation concentrations based on comparisons to the MPV. Values with a z score that was between -2 and 2 were considered of acceptable quality. No accuracy calculations were performed for SO₄ or Al due to the low number of detectable values and are represented as not calculable (n.c.).

129x110mm (192 x 192 DPI)

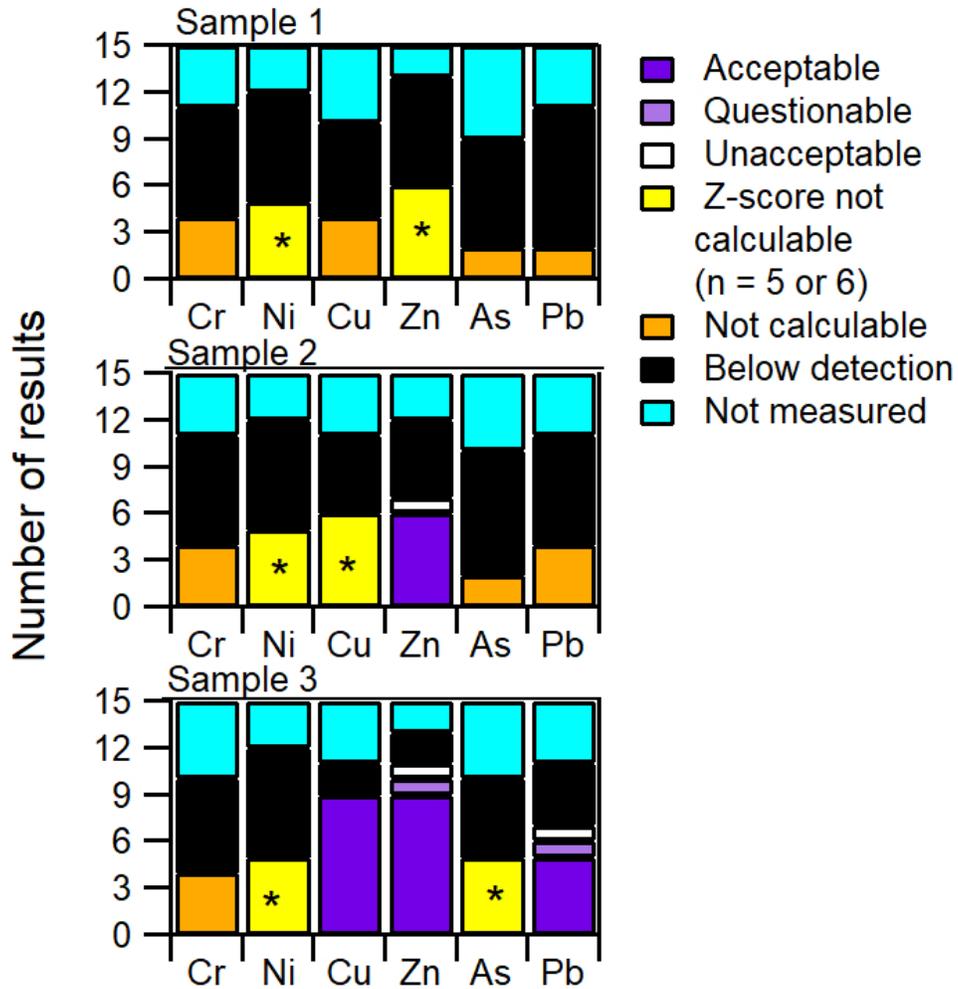


Figure 3. Data quality for trace metal(loid) concentrations reported in sample 1, 2, and 3. Acceptable, questionable, and unacceptable designations were based on z-score calculations when the number of reported values was ≥ 7 for a given analyte. When 5 or 6 values were reported, no z score was calculated but is noted with an asterisk as a MPV and Fpseudosigma were still calculated (Table 2). When less than 5 values were reported, no statistics were calculated.

95x98mm (192 x 192 DPI)

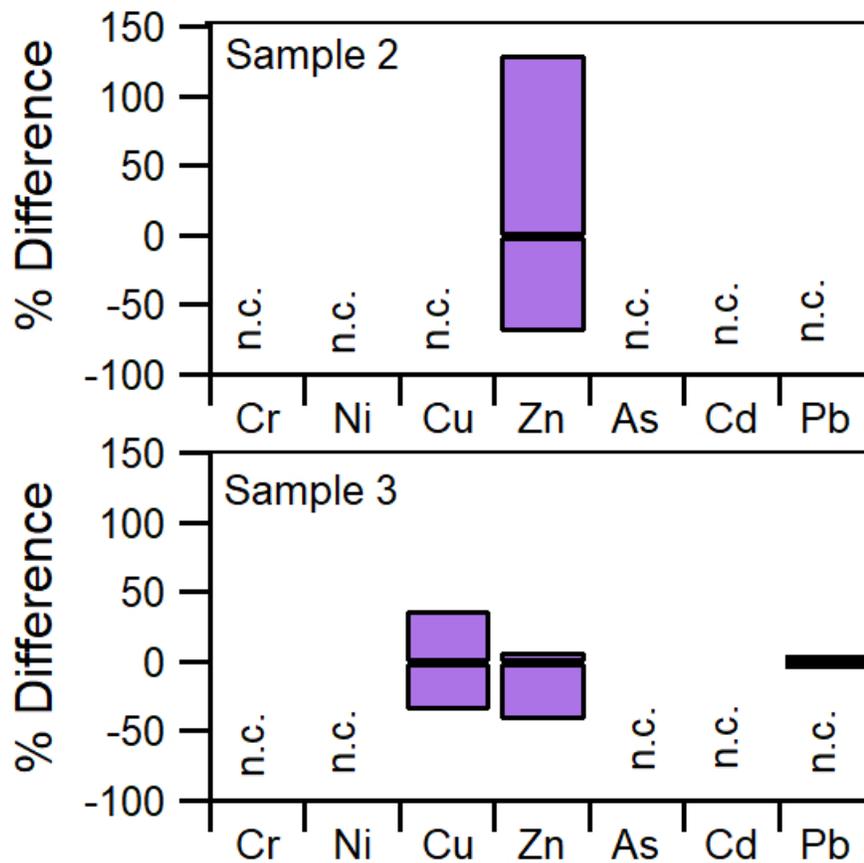


Figure 4. Range in accuracy of reported values with acceptable quality for trace metal(loid)s based on comparisons to the MPV. No accuracy calculations were performed for sample 1 due to the low number of detectable concentrations. Other metal(loid)s where statistics were not calculable (n.c.) due to the low number of detectable values ($n < 7$) are shown for sample 2 and 3.

82x81mm (192 x 192 DPI)

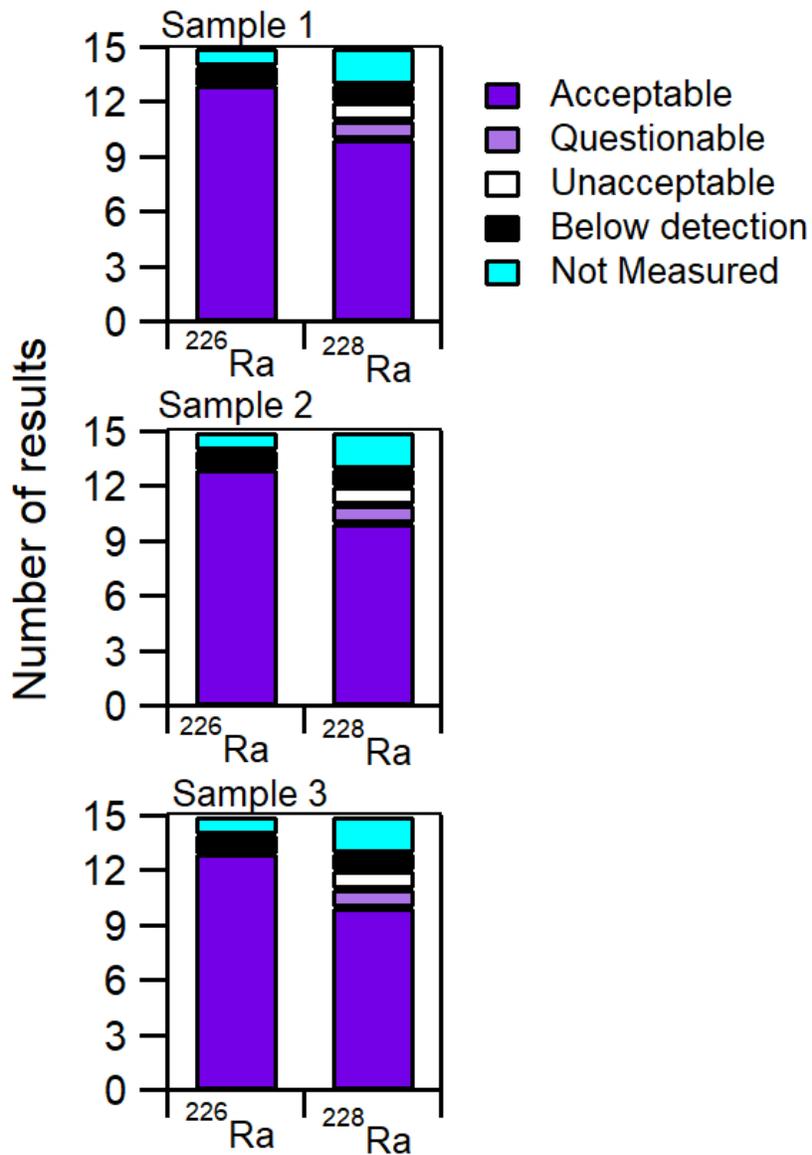


Figure 5. Data quality for Ra concentrations reported in sample 1, 2, and 3. Acceptable, questionable, and unacceptable quality were based on z-score calculations when the number of values were ≥ 7 for a given analyte.

80x110mm (192 x 192 DPI)

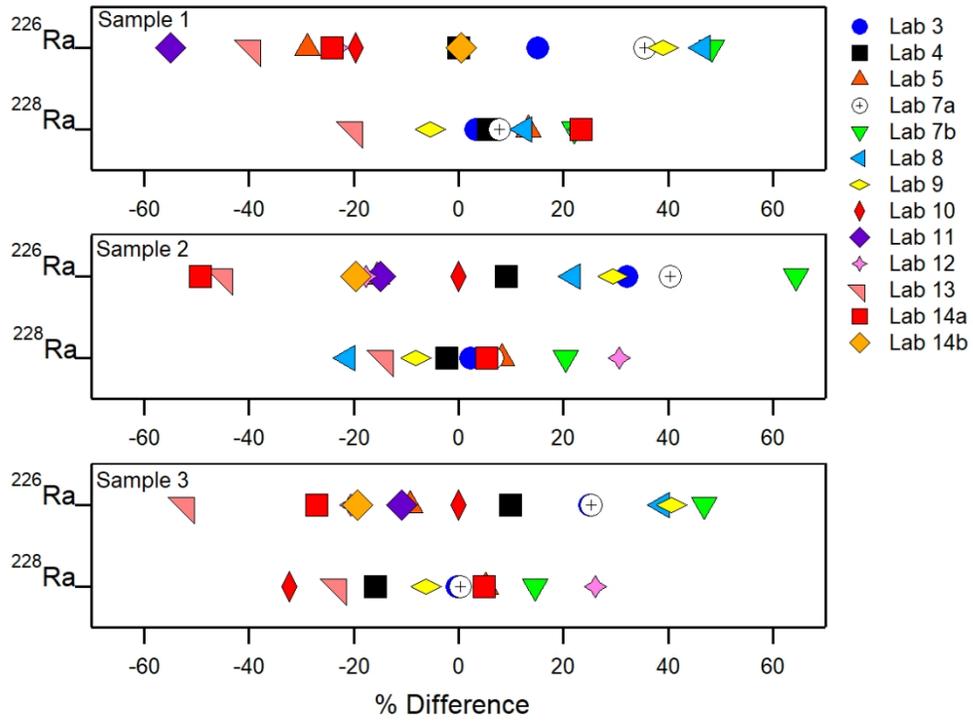


Figure 6. The % difference of measured Ra activities by individual labs based on comparisons to the MPV. A summarized description of each labs methods is included in Table S5.

154x118mm (192 x 192 DPI)

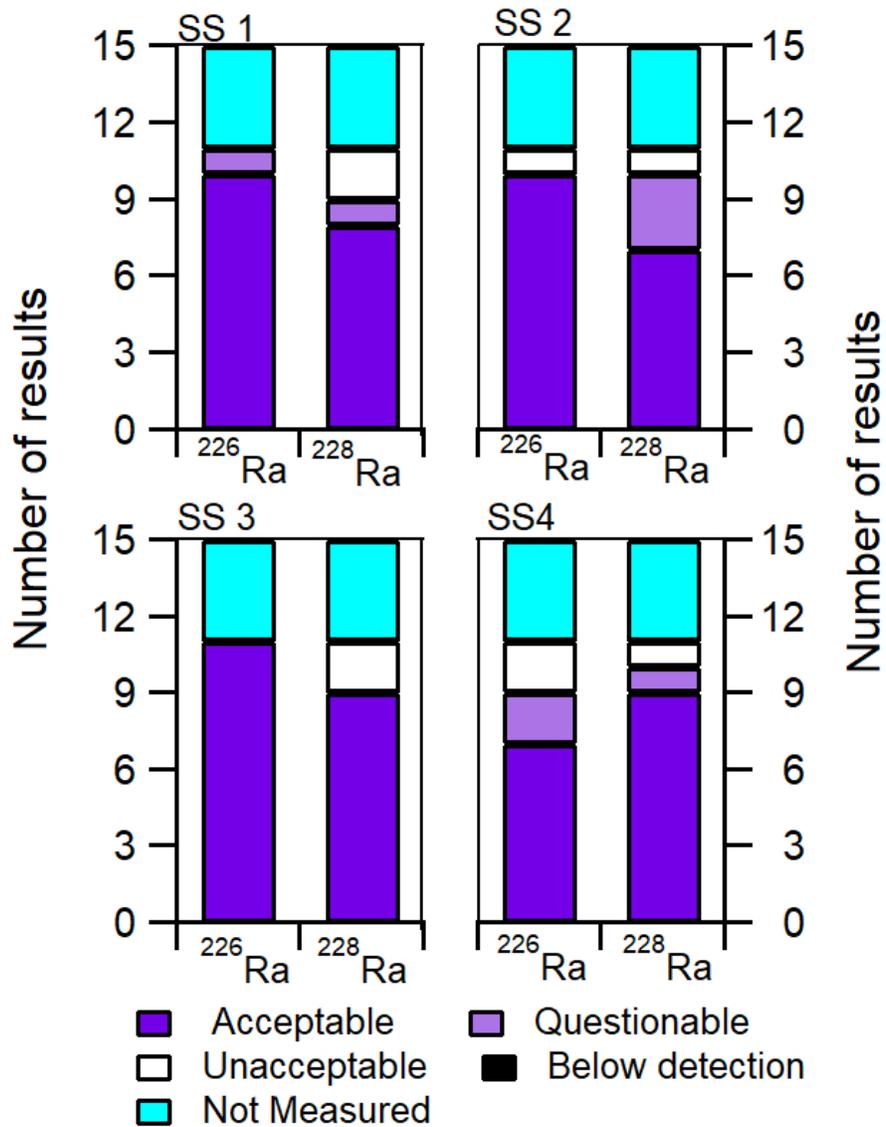


Figure 7. Data quality for Ra activities reported in solid samples 1, 2, 3, and 4. Acceptable, questionable, and unacceptable designations were based on z-score calculations when the number of values were ≥ 7 for a given analyte.

85x110mm (192 x 192 DPI)


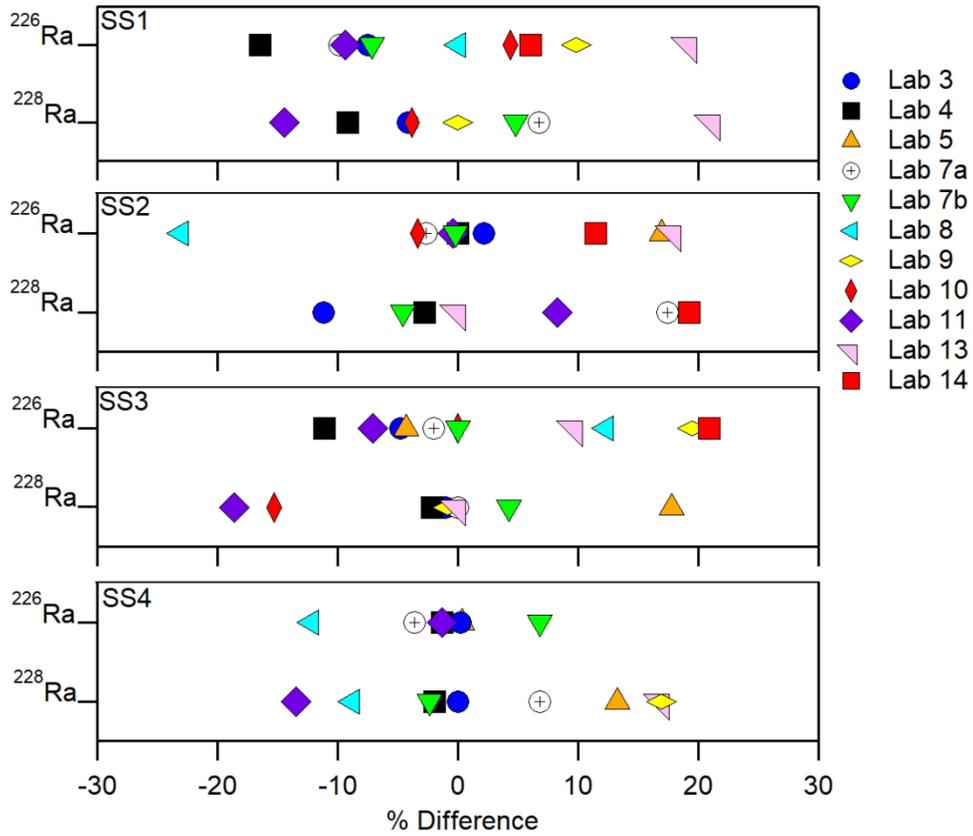


Figure 8. Range in the % difference of reported Ra activities with acceptable quality based on comparisons to the MPV.

157x134mm (192 x 192 DPI)

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

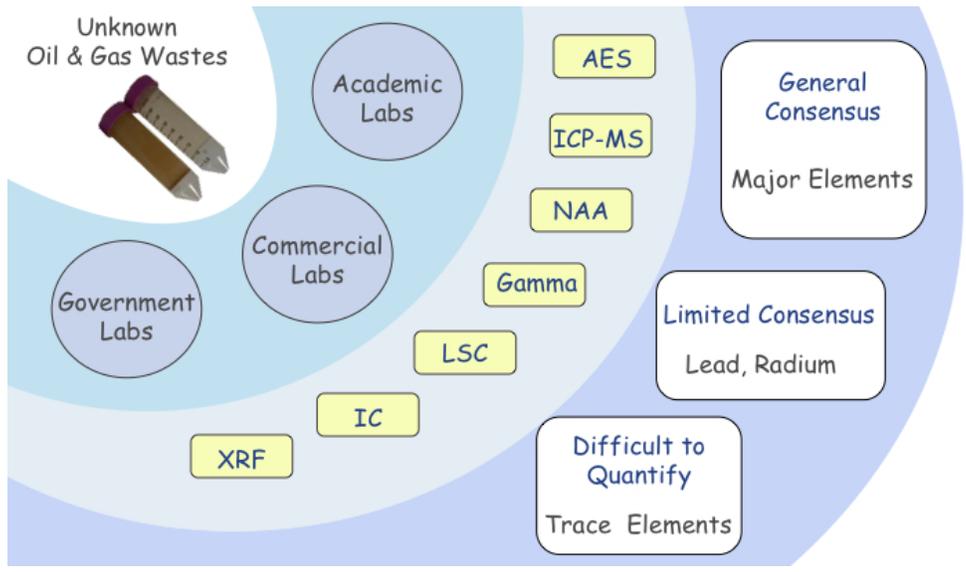

TOC art

254x142mm (72 x 72 DPI)