

RSC Advances



This is an *Accepted Manuscript*, which has been through the Royal Society of Chemistry peer review process and has been accepted for publication.

Accepted Manuscripts are published online shortly after acceptance, before technical editing, formatting and proof reading. Using this free service, authors can make their results available to the community, in citable form, before we publish the edited article. This *Accepted Manuscript* will be replaced by the edited, formatted and paginated article as soon as this is available.

You can find more information about *Accepted Manuscripts* in the [Information for Authors](#).

Please note that technical editing may introduce minor changes to the text and/or graphics, which may alter content. The journal's standard [Terms & Conditions](#) and the [Ethical guidelines](#) still apply. In no event shall the Royal Society of Chemistry be held responsible for any errors or omissions in this *Accepted Manuscript* or any consequences arising from the use of any information it contains.

ARTICLE

A Sensitive Electrochemical Sensor for Direct Phoxim Detection Based on Electrodeposited Reduced Graphene Oxide-Gold Nanocomposite

Cite this: DOI: 10.1039/x0xx00000x

Received 00th January 2012,
Accepted 00th January 2012

DOI: 10.1039/x0xx00000x

www.rsc.org/

Yuhong Zheng^b, Aiwu Wang^c, Haitao Lin^{a*}, Li Fu^{b*}, Wen Cai^c

The principal objective of this study was to develop a sensitive and selective electrochemical sensor for phoxim detection based on reduced graphene oxide-gold nanocomposite (RGO/Au) modified grassy carbon electrode (GCE). The proposed sensor was fabricated by pulsed electrodeposition of reduced graphene oxide followed by chronoamperometric deposition of Au nanoparticles, and applied for the electrochemical detection of phoxim. The modified electrode was characterized by SEM, UV-vis spectroscopy, Raman spectroscopy and XRD. The electrocatalytic activity of RGO/Au/GCE towards reduction of phoxim was evaluated using cyclic voltammetry and differential pulse voltammetry. The results showed that the RGO/Au nanocomposite could greatly enhance the electrochemical reduction of phoxim. Under the optimal conditions, the reduction peak current was proportional to phoxim concentration in a wide range between 0.01 and 10 μM , and the detection limit was 0.003 μM ($S/N = 3$). The proposed phoxim biosensor also exhibited excellent stability and reproducibility. In addition, the sensor was successfully employed for determining phoxim in a variety of food samples.

1. Introduction

Organophosphate pesticides have been widely used to control unwanted organisms in agricultural activity. They could be found in food products due to their overuse and accumulation in the food chain. They are well known as highly toxic compounds which can pose a risk to human neurological health. These neurotoxic compounds could irreversibly inhibit the enzyme acetylcholinesterase resulting in the buildup of the neurotransmitter acetylcholine which interferes with muscular responses and in vital organs produce serious symptoms and eventually death¹⁻³. Phoxim (phenylgloxynitrile oxime o,o-diethyl phosphorothionate, also known as Sebacil EC 50[®] and Byemite[®], Figure S1) is one of the most common organophosphate pesticides used for controlling a variety of ectoparasites in pigs, sheep and chicken⁴. Study showed that the phoxim can undergo photodegradation process and produce thiono-thiolo rearranged compound, o,o-diethyl-cyanobenzylideneamino-thiophosphonate (DCTP), a highly active acetylcholinesterase inhibitor, when exposed under natural sunlight⁵. Therefore, it is necessary to develop a highly sensitive, selective, rapid and reliable analytical method to determine phoxim for food quality control purpose. At present, some methods have been established for detection of phoxim such as high-performance liquid chromatogramraphy (HPLC)^{4, 6-9}, liquid chromatography-mass spectrometry¹⁰, enzymatic kinetic method¹¹, near-infrared

spectroscopy^{12, 13} and spectrophotometry¹¹. However, these reported methods require expensive and complicated instruments, time-consuming pretreatment steps and skilled operators. In order to avoid these problems, electrochemical method has attracted more attentions due to its sensitivity, accuracy, lower cost and simplicity¹⁴⁻¹⁸. Studies demonstrated acetylcholinesterase immobilized electrochemical sensors for phoxim determination^{19, 20}. However, enzyme based electrochemical sensors have some drawbacks, such as complicated and multi-step immobilization procedures, high cost and instability²¹⁻²³. Therefore, considerable attention has been paid on fabrication of non-enzymatic sensors for specific target molecules detection. So far, only two studies have been reported regarding the direct electrochemical detection of phoxim and development of a selective, sensitive and rapid electrochemical sensor still remains a challenge^{14, 24}.

Graphene, a two-dimensional one-atom-thick planar carbon sheets, has attracted a great deal of interest since it has been discovered in 2004 due to its extraordinary properties, such as excellent electronic conductivity and large specific surface area^{25, 26}. Therefore, graphene consider as an excellent candidate for electrode surface modification for specific target molecule detection. On the other hand, gold nanoparticles are widely used nanomaterials for the fabrication of electrochemical biosensors because they can provide suitable microenvironments for immobilization of biomolecules with

excellent electrocatalytic property²⁷⁻³⁰. Up to date, several examples for Au-graphene nanocomposites have been reported for electro-determination applications³¹⁻³³. For example, Liu and co-workers demonstrated the fabrication of a novel electrochemical DNA biosensor based on graphene-three dimensional nanostructure gold nanocomposite modified glassy carbon electrode³⁴. Sun and co-workers reported a three-dimensional macroporous gold nanoparticles/graphene composites for electrochemically sensitive detection of carcinoembryonic antigen in human serum³⁵. However, most of the graphene/Au composites were synthesized by in-situ method, only a small number of reports on growing Au nanoparticles on graphene surface by electrodeposition method³⁶.

The aim of this work was to develop a fast, simple, stabile and highly sensitive phoxim biosensor based on reduced graphene oxide-gold nanocomposite (RGO/Au) using pulsed electrodeposition combine with chronoamperometric deposition methods. The electrochemical behavior of phoxim at the RGO-Au nanocomposite modified grassy carbon electrode (GCE) was investigated. Several factors affecting the electrocatalytic performances of the proposed phoxim sensor were also further optimized. In addition, the proposed phoxim sensor was successfully employed for determination phoxim in a variety of food samples.

2. Experimental

2.1 Chemicals and materials

Phoxim, synthetic graphite (average particle diameter <20 μm), glutamic acid, ascorbic acid, uric acid, parathion, methyl parathion, malathion, methyl isofenphos, thimet, methamidophos and $\text{HAuCl}_4 \cdot 3\text{H}_2\text{O}$ were purchased from Sigma-Aldrich. All other chemicals used were analytical grade reagents without further purification. Milli-Q water (18.2 $\text{M}\Omega \text{ cm}$) was used throughout the experiments.

2.2 Electrodeposition of RGO/Au nanocomposite

Graphene oxide (GO) was prepared according to the modified Hummers method with little modifications^{37, 38}. The prepared GO was dispersed in to water (0.5 mg/mL) with the 0.25 M NaCl and then used for the following electrodeposition process. For electrodeposition of RGO film, a GCE (3 mm in diameter) was polished with alumina-water slurry followed by rinsing with ethanol and water. A platinum wire was used as the auxiliary electrode and an Ag/AgCl (3M KCl) as the reference electrode. The electrodeposition of RGO was carried out under pulsed electrodeposition technique of 500 cycles in the GO dispersion with N_2 bubbling (Figure S2). Next, electrochemical deposition of Au nanoparticles on RGO modified GCE was performed in 0.5 M H_2SO_4 solution containing 1% HAuCl_4 using chronoamperometry at an applied potential of -0.2 V for 60s.

2.3 Characterization

The morphology of as-synthesized nanocomposite was observed using a ZEISS, SUPRA 55 field emission scanning electron microscopy (FESEM) measurements. The optical analysis was obtained by UV-vis spectrophotometer (Perkin Elmer Lambda 950). Raman spectroscopy was performed at room temperature using a Raman Microprobe (Renishaw RM1000) with 514 nm laser light. The crystal phase information of sample was characterized from 5°

to 80° in 2θ by a XRD with Cu $\text{K}\alpha$ ($\lambda = 0.1546 \text{ nm}$) radiation (D8-Advanced, Bruker).

2.4 Real sample preparation

Food samples were purchased from the Carrefour supermarket. The pre-treatment of food samples are according to the literature with some modifications¹⁴. 50 g of each sample was cleaned by and homogenized using a grinder. The samples were then extracted with 100 mL of acetone. The supernatants were filtered to remove the solids and then evaporated to dryness. The residue was then dissolved and diluted to 50 mL with water.

3. Results and Discussion

3.1 Characterization of RGO/Au nanocomposite

The surface morphology of the resulting samples were observed by SEM. Figure 1A-C display the typical SEM images of electrodeposited RGO and RGO/Au nanocomposite. As shown in Figure 1A, electrodeposited RGO film displays a flake-like shape with many wrinkles. After chronoamperometric deposition of Au nanoparticles (Figure 1B), the surface and interlayers of RGO sheets have shown the decoration of many spherical Au nanoparticles with an average diameter of 35 nm (based on more than 200 Au nanoparticles). The uniformity of Au nanoparticles deposition was observed under high EHT voltage level. As shown in Figure 1C and Figure S3, the observation indicates our proposed method could uniformly deposit Au nanoparticles on the RGO film without aggregation.

Figure 1D displays the UV-vis spectra of GO, RGO and RGO/Au dispersions. The spectrum of GO exhibits a maximum absorption peak at 228 nm and a shoulder peak at about 302 nm, which assign to the $\pi-\pi^*$ transitions of aromatic C—C bonds and $n-\pi^*$ transitions of C=O bonds³⁹. After pulsed electrodeposition, the absorption peak at 226 nm shows a shift to 272 nm and the shoulder absorption peak disappears, suggesting the GO has been successfully reduced during the pulsed electrodeposition process. After chronoamperometric deposition of Au nanoparticles, the spectrum of the sample exhibits a new broad absorption peak centred at about 540 nm, corresponding to the surface plasmon absorption of Au nanoparticles, confirming the existence of Au nanoparticles in the sample⁴⁰.

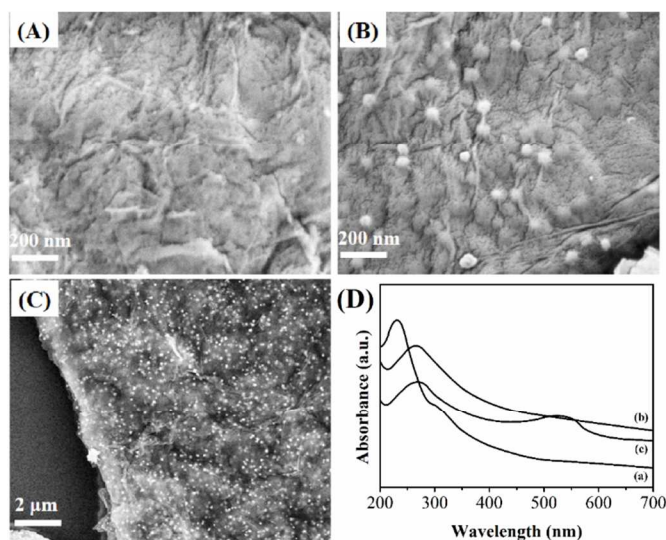


Figure 1. SEM images of (A) RGO and (B-C) RGO/Au nanocomposite. (D) UV-vis spectra of (a) GO, (b) RGO and (c) RGO-Au nanocomposite.

Raman scattering is a highly sensitive tool for the characterization of carbon based materials. Figure 2A shows the Raman spectra of the GO, RGO and RGO/Au nanocomposite. The spectrum of GO shows two characteristic bands at 1310 cm^{-1} (D band) and 1596 cm^{-1} (G band), which are corresponded to sp^3 and sp^2 carbon hybridization, respectively⁴¹. After the electrodeposition, the I_D/I_G ratio in RGO (1.31) shows a significant increase compared with the GO (0.91), indicating the increase in the average size of the sp^2 sites. According to literatures, it suggests the reduction reaction has taken place^{42,43}. The spectrum of RGO/Au nanocomposite shows a similar scattering profile with RGO, except the G band has a small upshift (from 1596 to 1601 cm^{-1}), which can be attributed to the doping of Au nanoparticles on RGO sheets^{44,45}.

The interlayer changes and crystalline structure of GO, RGO and RGO/Au nanocomposite were analyzed by XRD and depicted in Figure 2B. As expected, the XRD pattern of GO shows a characteristic (001) peak at 11.1° with a d -spacing value of 0.81 nm ⁴⁶. However, the RGO displays an almost featureless XRD pattern, suggesting the occurrence of reduction of GO. A small peak centred at 23.0° is due to the presence of stacked graphene layers of RGO⁴⁷. The XRD spectrum of In RGO/Au nanocomposite shows diffraction peaks located at 39.5° , 46.2° , 67.4° and 81.5° , which are assigned to (111), (200), (220) and (311) planes of face-centered-cubic (fcc) crystallographic structure of Au (JCPDS 4-0783), respectively, confirming the successful electrodeposition of Au nanoparticles.

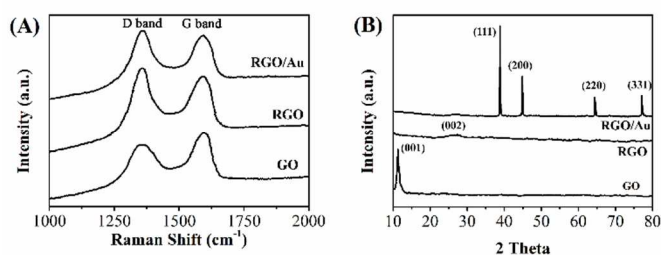


Figure 2. (A) Raman spectra and (B) XRD patterns of GO, RGO and RGO/Au nanocomposite.

3.2 Electrochemical behavior of phoxim at RGO/Au/GCE

Figure 3A shows the CV profiles of bare GCE and RGO/Au/GCE toward reduction of $10\text{ }\mu\text{M}$ phoxim at scan rate of 50 mV/s in the potential range of 0 to -1.2 V . It can be seen that a small peak is observed at the potential of -0.81 V with a peak current of $-6.53\text{ }\mu\text{A}$ in bare GCE, corresponding to the electro-reduction of phoxim (curve a). While at RGO/Au/GCE, a clear reduction peak with peak current about $-40.26\text{ }\mu\text{A}$ is observed at -0.69 V (curve c). Moreover, no reduction peak is observed on the CV of RGO/Au/GCE without phoxim (curve b), confirming the reduction peak in curve c is belonging to the reaction of phoxim. The enhancement of current response and lower the overpotential of phoxim reduction in RGO/Au/GCE could ascribe to the high specific surface area, the excellent electrocatalytic property of nanocomposite and the synergistic effect between RGO sheets and Au nanoparticles.

Figure 3B shows the CVs of $10\text{ }\mu\text{M}$ phoxim in a pH 7.0 PBS at the RGO/Au/GCE using different scan rates. The results show that the reduction peak current increases gradually with the increase of scan rate in the ranged from 40 to 230 mV/s . A linear relationship is obtained between the peak currents and the scan rates (Figure 3C), indicating the reduction of phoxim on RGO/Au/GCE is controlled by adsorption.¹⁴ The linear regression equation can be represented as: $I_{pa}(\text{ }\mu\text{A}) = -0.59657 v(\text{ mV/s}) - 10.24289$ ($R^2 = 0.997$). On the other hand, the reduction peak potential shifts negatively when the scan rate increases. E_{pc} shows a linear relationship with $\ln v$ (Figure 3D), indicating the electrochemical reaction is irreversible. The linear regression equation can be expressed as: $E_{pc}(\text{ V}) = -0.08548 \ln v(\text{ mV/s}) - 0.34717$ ($R^2 = 0.989$). Because the adsorbed phoxim is reduced in a totally irreversible one-step reaction, the following Laviron's equation^{48,49} can be used:

$$E_{pc} = E^0 + (RT / \alpha nF) \ln(RT k^0 / \alpha nF) + (RT / \alpha nF) \ln v$$

where R is the gas constant, α is the electron transfer coefficient, F the Faraday constant, k^0 is the standard heterogeneous rate constant of the reaction, T the Kelvin temperature, and n is the number of electron transferred. By combining the linear regression equation between reduction potential and $\ln v$, and Laviron's equation, we obtain the following:

$$-RT / \alpha nF = -0.08548$$

As the α exhibits the symmetry of energy barrier, lies between 0.3 and 0.7 in most systems, and is approximated as 0.5 ⁵⁰. The total number of electrons involved in the reduction of phoxim is found equal to 1 . A possible reaction mechanism of phoxim at the RGO/Au/GCE is represented in Figure S4¹⁴.

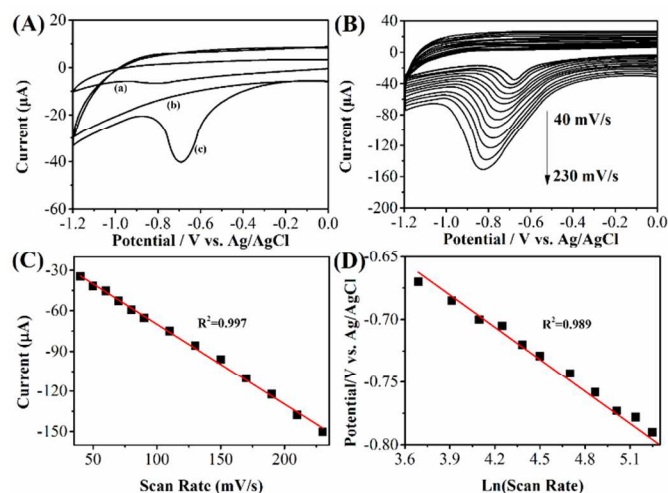


Figure 3. (A) CVs of bare (a) GCE, (b,c) RGO/Au/GCE in 0.1 M PBS (pH 7.0) with and without 10 μM phoxim. Scan rate: 50 mV/s. (B) CVs of RGO/Au/GCE in 10 μM phoxim at different scan rates (40, 50, 60, 70, 80, 90, 110, 130, 150, 170, 190, 210 and 230 mV/s). (C) The plot for the dependence of peak current on the scan rate. (D) The relationship between E_{pa} and $\ln v$.

It is a known fact that pH of the electrolyte has a significant effect on the electrochemical determination of target molecules. Figure 4A shows the current responses of reduction phoxim using RGO/Au/GCE at pH range from 4.0 to 9.0. It can be seen that the reduction peak current of phoxim increases gradually with increasing the pH up to 7.0, and then decreases in strongly alkaline conditions. Therefore, optimum pH for phoxim detection is 7.0.

Because the reduction of phoxim at RGO/Au/GCE is controlled by adsorption, accumulation may exert great influence on the analytic sensitivity and the intensity of peak current. Therefore, the reduction peak current of phoxim at different potentials was measured individually. As shown in Figure 4B, the peak current increases gradually with the increasing accumulation potential from -0.1 to -0.4 V and then decrease with further increasing potential. Figure 4C depicts the effect of accumulation time on the reduction peak current of 10 μM phoxim. As extending the accumulation time from 15 to 90 s, the reduction peak current of phoxim increases greatly, indicating that accumulation process could improve the determining sensitivity. When further prolonging the accumulation time from 90 to 150 s, the peak current remains unchanged. Therefore, the accumulation conditions of -0.4 V and 90 s were used in further measurements.

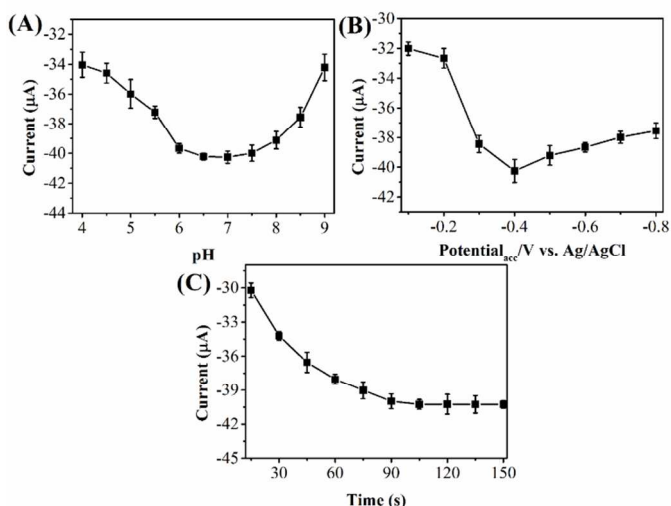


Figure 4. Effect of the (A) pH of PBS, (B) accumulation potential and (C) accumulation time on the current response of 10 μM phoxim at RGO/Au/GCE.

Differential pulse voltammetric (DPV) was employed for determining phoxim under the optimum experimental conditions. Figure 5 shows the DPV profiles of different concentrations of phoxim at RGO/Au/GCE. The reduction currents gradually increase along with the increasing of phoxim concentration from 0.01 to 10 μM. The insert of Figure 5 displays that the current response of RGO/Au/GCE has a linear relationship with the concentrations of phoxim. The obtained linear regression equation can be expressed as $I (\mu A) = -8.04894 (\mu M) - 5.49344$ ($R^2 = 0.994$). The detection limit for phoxim is estimated to be 0.003 μM based on a signal-to-noise ratio of 3. The analytical performance of this phoxim sensor was compared with that of other phoxim determination method reported previously as shown in Table S1.

Potential interference to the reduction current response of phoxim from many foreign species was investigated using DPV under optimal experimental conditions. Experimental results showed that 500-fold excess of Na^+ , Zn^{2+} , Fe^{3+} , Ca^{2+} , K^+ , Mg^{2+} , glutamic acid, glucose, ascorbic acid and uric acid have no influence on the signals of phoxim with the deviation below 5%. 100-fold excess of parathion, methyl parathion, malathion, methyl isofenphos, thimet, and methamidophos have also no influence on the signals of phoxim with the deviation below 4%. The results of the interference study were summarized in Table S2.

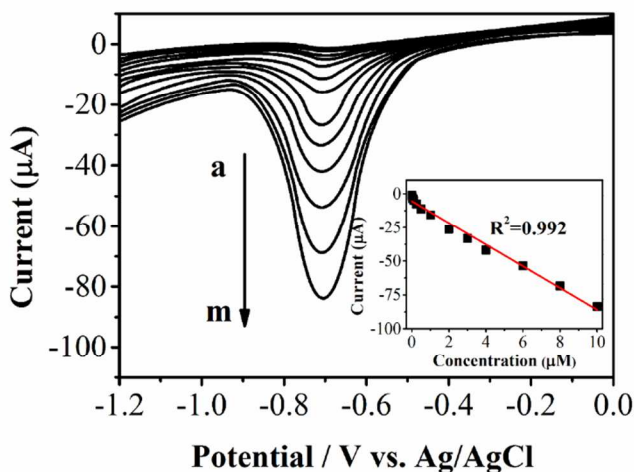


Figure 5. DPV curves for phoxim at RGO/Au/GCE with different concentrations of phoxim (from a to m: 0.008, 0.02, 0.05, 0.1, 0.25, 0.5, 1, 2, 3, 4, 6, 8, 10 μM).

3.3 Repeatability, stability and real sample analysis

In order to evaluate the repeatability of the RGO/Au/GCE, a 5 μM phoxim PBS solution was successively measured for 12 times using one RGO/Au/GCE. The RSD values were found to be 1.31%. On the other hand, five fresh fabricated RGO/Au/GCE were also used for determining 5 μM phoxim. The RSD was calculated to be 2.71 %. Therefore, our proposed phoxim electrochemical sensor has a satisfactory repeatability. The storage stability was tested by storing the RGO/Au/GCE in refrigerator for one month. The result showed that the reduction peak potential of phoxim had no shift and the current response only showed 3.21% decrease compared with the original test. Therefore, our proposed sensor also has a satisfactory stability. The robustness of the proposed phoxim sensor was investigated by studying the effect of small variations in PBS's pH (6.8-7.2), accumulation potential (-0.38 – -0.42 V) and accumulation time (88-92 s) on the recovery of phoxim. The results indicated no significant changes in the current response. The recovery for phoxim under variable conditions was in the range of 96.5%-101.1%. Therefore, the RGO/Au/GCE also exhibits very good robustness.

The proposed sensor was used for the determination of phoxim in broccoli, celery, egg, pork sausage and ham. DPV results showed no peak current of phoxim in all samples, indicating no phoxim is contained in these food. The standard addition method was then applied, by adding successive concentrations of phoxim. As shown in Table 1, the recovery for the determination of phoxim was in the range of 97.2–101.0%. In order to evaluate the accuracy, the contents of phoxim in these samples were also analyzed by GC-MS and listed in Table 1 as well. The results obtained by GC-MS and RGO/Au/GCE were in good agreement, confirming the proposed electrochemical sensor is capable for determining phoxim in various food samples.

Table 1 Determination results of phoxim in broccoli, celery, egg, pork sausage and ham using RGO/Au/GCE and GC-MS.

Sample	Added (μM)	Found (μM)	Recovery (%)	RSD(%)
Broccoli	—	Not found ^{*,#}	—	—
	0.1	0.0998 [*] , 0.0997 [#]	99.8 [*] , 99.7 [#]	1.98 [*] , 2.00 [#]
	1	0.9887 [*] , 1.0012 [#]	98.87 [*] , 100.12 [#]	2.15 [*] , 2.03 [#]
Celery	—	Not found ^{*,#}	—	—
	0.1	0.0996 [*] , 0.0963 [#]	99.6 [*] , 96.3 [#]	1.22 [*] , 2.21 [#]
	1	1.0099 [*] , 0.9721 [#]	100.99 [*] , 97.21 [#]	1.99 [*] , 1.02 [#]
Egg	—	Not found ^{*,#}	—	—
	0.05	0.0502 [*] , 0.0487 [#]	100.4 [*] , 97.4 [#]	2.28 [*] , 2.65 [#]
	2	2.0047 [*] , 1.9744 [#]	100.23 [*] , 98.72 [#]	3.01 [*] , 1.47 [#]
Pork sausage	—	Not found ^{*,#}	—	—
	0.05	0.0486 [*] , 0.0502 [#]	97.2 [*] , 100.4 [#]	1.92 [*] , 4.56 [#]
	2	1.9770 [*] , 2.0237 [#]	98.85 [*] , 101.19 [#]	0.74 [*] , 1.45 [#]
Ham	—	Not found ^{*,#}	—	—
	0.01	0.0101 [*] , 0.0089 [#]	101.0 [*] , 89.0 [#]	2.52 [*] , 3.07 [#]
	5	5.0336 [*] , 4.9881 [#]	100.67 [*] , 99.76 [#]	2.69 [*] , 3.99 [#]

^{*}Data collected from RGO/Au/GCE electrochemical sensor.

[#]Data collected from GC-MS.

4. Conclusions

In this study, a RGO/Au/GCE was successfully fabricated via sequential electrodeposition of RGO and Au nanoparticles on GCE. The synthesized RGO/Au nanocomposite was characterized by SEM, XRD, Raman spectroscopy and UV-vis spectroscopy, and then employed successfully in the sensitive electrochemical determination of phoxim. The RGO/Au/GCE displays a wide detection linear range (0.01 to 10 μM) and a low detection limit (0.003 μM) for phoxim sensing. In addition, the proposed sensor was successfully employed for deterring the content of phoxim in different types of food samples. The accuracy was confirmed by GC-MS.

Acknowledgments

Notes and references

^a Yunnan University of TCM, Kunming city, Yunnan, 650500 P. R. China

^b Institute of Botany, Jiangsu Province and Chinese Academy of Sciences, Nanjing Botanical Garden, Mem. Sun Yat-Sen, Nanjing 210014 P. R. China

^cDepartment of Physics and Materials Science, City University of Hong Kong, P. R. China

Corresponding author: Haitao Lin; email: haitaolinyutcm@yahoo.com

Li Fu; e-mail Address: lifugyt@gmail.com

Reference

- W. J. Donarski, D. P. Dumas, D. P. Heitmeyer, V. E. Lewis and F. M. Raushel, *Biochemistry*, 1989, **28**, 4650-4655.
- S. Chapalamadugu and G. R. Chaudhry, *Critical reviews in biotechnology*, 1992, **12**, 357-389.
- A. Mulchandani, W. Chen, P. Mulchandani, J. Wang and K. R. Rogers, *Biosensors and Bioelectronics*, 2001, **16**, 225-230.
- G. Hamscher, B. Prieß and H. Nau, *Analytica chimica acta*, 2007, **586**, 330-335.
- T. R. Roberts, D. H. Hutson, P. W. Lee, P. H. Nicholls and J. R. Plimmer, JSC International Ltd., Harrogate, UK, 1999, p. 447.
- P. Liang, L. Guo, Y. Liu, S. Liu and T.-z. Zhang, *Microchemical Journal*, 2005, **80**, 19-23.
- L. Guo, P. Liang, T. Zhang, Y. Liu and S. Liu, *Chroma*, 2005, **61**, 523-526.
- P. Liang, J. Xu, L. Guo and F. Song, *Journal of Separation Science*, 2006, **29**, 366-370.
- Z. Lv, L. Gao, H. Gao, Z. Hou and B. Zhang, *Journal of Food Science*, 2009, **74**, T37-T41.
- J. H. Lee, S. Park, W. Y. Jeong, H. J. Park, H. G. Kim, S.-J. Lee, J.-H. Shim, S. T. Kim, A. M. Abd El-Aty, M. H. Im, O. J. Choi and S. C. Shin, *Analytica chimica acta*, 2010, **674**, 64-70.
- Y. Ni, D. Cao and S. Kokot, *Analytica chimica acta*, 2007, **588**, 131-139.
- C. Gu, B. Xiang and J. Xu, *Spectrochimica Acta Part A: Molecular and Biomolecular Spectroscopy*, 2012, **97**, 594-599.
- F. Shen, Z.-k. Yan, Z.-z. Ye and Y.-b. Ying, *Spectroscopy and Spectral Analysis*, 2009, **29**, 2421-2424.
- M. Chao and M. Chen, *Food Anal. Methods*, 2014, **7**, 1729-1736.
- S. Chandran, L. Lonappan, D. Thomas, T. Jos and K. Girish Kumar, *Food Anal. Methods*, 2014, **7**, 741-746.
- T. Wang, D. Zhao, X. Guo, J. Correa, B. L. Riehl and W. R. Heineman, *Analytical Chemistry*, 2014, **86**, 4354-4361.
- L. Fu, W. Cai, A. Wang and Y. Zheng, *Materials Letters*, 2015, **142**, 201-203.
- L. Fu, A. Wang, Y. Zheng, W. Cai and Z. Fu, *Materials Letters*, 2015, **142**, 119-121.
- C. Zhang, J. Zhang, K. Wang and Z. Dai, *Acta Chimica Sinica*, 2012, **70**, 1008-1012.
- H. Yin, S. Ai, J. Xu, W. Shi and L. Zhu, *Journal of Electroanalytical Chemistry*, 2009, **637**, 21-27.
- S. Liu, B. Yu and T. Zhang, *Electrochimica Acta*, 2013, **102**, 104-107.
- L. Fu and Z. Fu, *Ceram Int*, 2015, **41**, 2492-2496.
- L. Fu, Y. Zheng, Q. Ren, A. Wang and B. Deng, *Journal of Ovonic Research*, 2015, **11**, 21-26.
- X. Lu, H. Bai, Q. Ruan, M. Yang, G. Yang, L. Tan and Y. Yang, *International Journal of Environmental Analytical Chemistry*, 2008, **88**, 813-824.
- K. S. Novoselov, A. K. Geim, S. V. Morozov, D. Jiang, Y. Zhang, S. V. Dubonos, I. V. Grigorieva and A. A. Firsov, *Science*, 2004, **306**, 666-669.
- X. Ma, M. Chao and Z. Wang, *Analytical Methods*, 2012, **4**, 1687-1692.
- C. Shan, H. Yang, D. Han, Q. Zhang, A. Ivaska and L. Niu, *Biosensors and Bioelectronics*, 2010, **25**, 1070-1074.
- J. M. Pingarrón, P. Yáñez-Sedeño and A. González-Cortés, *Electrochimica Acta*, 2008, **53**, 5848-5866.
- A. Afkhami, F. Soltani-Felehgari and T. Madrakian, *Talanta*, 2014, **128**, 203-210.
- X. Wang, Y. Wen, L. Lu, J. Xu, L. Zhang, Y. Yao and H. He, *Electroanalysis*, 2014, **26**, 648-655.
- F. Cui and X. Zhang, *Journal of Electroanalytical Chemistry*, 2012, **669**, 35-41.
- Y. Chen, Y. Li, D. Sun, D. Tian, J. Zhang and J.-J. Zhu, *Journal of Materials Chemistry*, 2011, **21**, 7604-7611.
- P. T. Do, P. Q. Do, H. B. Nguyen, V. C. Nguyen, D. L. Tran, T. H. Le, L. H. Nguyen, H. V. Pham, T. L. Nguyen and Q. H. Tran, *Journal of Molecular Liquids*, 2014, **198**, 307-312.
- A.-L. Liu, G.-X. Zhong, J.-Y. Chen, S.-H. Weng, H.-N. Huang, W. Chen, L.-Q. Lin, Y. Lei, F.-H. Fu, Z.-l. Sun, X.-H. Lin, J.-H. Lin and S.-Y. Yang, *Analytica chimica acta*, 2013, **767**, 50-58.
- G. Sun, J. Lu, S. Ge, X. Song, J. Yu, M. Yan and J. Huang, *Analytica chimica acta*, 2013, **775**, 85-92.
- Y. Hu, J. Jin, P. Wu, H. Zhang and C. Cai, *Electrochimica Acta*, 2010, **56**, 491-500.
- W. S. Hummers and R. E. Offeman, *Journal of the American Chemical Society*, 1958, **80**, 1339-1339.
- T. Gan and S. Hu, *Microchim Acta*, 2011, **175**, 1-19.
- J. I. Paredes, S. Villar-Rodil, A. Martínez-Alonso and J. M. D. Tascón, *Langmuir*, 2008, **24**, 10560-10564.
- X. C. Lv and J. Weng, *Scientific reports*, 2013, **3**.
- D. Graf, F. Molitor, K. Ensslin, C. Stampfer, A. Jungen, C. Hierold and L. Wirtz, *Nano Letters*, 2007, **7**, 238-242.
- X. Li, Q. Wang, Y. Zhao, W. Wu, J. Chen and H. Meng, *Journal of colloid and interface science*, 2013, **411**, 69-75.
- H. N. Tien, V. H. Luan, L. T. Hoa, N. T. Khoa, S. H. Hahn, J. S. Chung, E. W. Shin and S. H. Hur, *Chemical Engineering Journal*, 2013, **229**, 126-133.
- R. K. Shervedani and A. Amini, *Electrochimica Acta*, 2014, **121**, 376-385.
- J. Lee, K. S. Novoselov and H. S. Shin, *ACS Nano*, 2010, **5**, 608-612.
- T. Nakajima, A. Mabuchi and R. Hagiwara, *Carbon*, 1988, **26**, 357-361.
- D. Chen, L. Li and L. Guo, *Nanotechnology*, 2011, **22**.
- E. Laviron, *J. Electroanal. Chem.*, 1979, **101**, 19-28.
- E. Laviron, *J. Electroanal. Chem.*, 1974, **52**, 355-393.
- A. J. Bard and L. R. Faulkner, *Electrochemical Methods: Fundamentals and Applications*, 2nd Edition, Wiley, 1980.