

JAAS

Accepted Manuscript




This is an *Accepted Manuscript*, which has been through the Royal Society of Chemistry peer review process and has been accepted for publication.

Accepted Manuscripts are published online shortly after acceptance, before technical editing, formatting and proof reading. Using this free service, authors can make their results available to the community, in citable form, before we publish the edited article. We will replace this *Accepted Manuscript* with the edited and formatted *Advance Article* as soon as it is available.

You can find more information about *Accepted Manuscripts* in the [Information for Authors](#).

Please note that technical editing may introduce minor changes to the text and/or graphics, which may alter content. The journal's standard [Terms & Conditions](#) and the [Ethical guidelines](#) still apply. In no event shall the Royal Society of Chemistry be held responsible for any errors or omissions in this *Accepted Manuscript* or any consequences arising from the use of any information it contains.

Table of contents

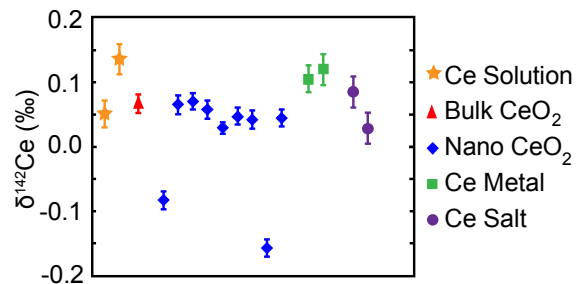

Stable $^{142}\text{Ce}/^{140}\text{Ce}$ isotope measurements of CeO_2 nanoparticles and purified materials for the purpose of stable isotope tracing.

1
2
3
4
5
6
7 **High precision $^{142}\text{Ce}/^{140}\text{Ce}$ stable isotope measurements**
8
9
10
11 **of purified materials**
12
13
14
15 **with a focus on CeO_2 nanoparticles**
16
17
18
19
20
21
22

23 Adam Laycock^{1*}, Barry Coles¹, Katharina Kreissig¹, Mark Rehkämper¹
24
25
26
27
28

29 ¹ Department of Earth Science & Engineering, Imperial College London, South Kensington,
30
31 London SW7 2AZ, England
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

Abstract

Engineered CeO₂ nanoparticles (NPs) are becoming increasingly prevalent in consumer products and this has raised concerns about the unknown behaviour and fate of such materials in the environment. Analytical limitations have hampered the detection of CeO₂ NPs in natural systems at environmentally relevant levels. This study presents data on the inherent stable isotope composition of commercially available purified Ce materials with a particular focus on CeO₂ NPs. The aim of this investigation is to determine whether CeO₂ NPs possess a distinct isotopic signature that may be exploited for their detection in natural systems. To achieve this, suitable stable isotope measurement protocols were developed for the precise determination of the ¹⁴²Ce/¹⁴⁰Ce isotope ratio by multiple collector ICP-MS using Ba for external normalisation of the instrumental mass bias. The data presented show that precisions of ±0.01‰ (2se) and ±0.04‰ (2sd) can be routinely achieved with these techniques. The results also demonstrate that commercially available CeO₂ NPs do not have a distinct Ce isotope composition that may be exploited for the purpose of stable isotope tracing.

1 Introduction

Engineered CeO₂ nanoparticles (NPs) are amongst the most extensively manufactured nanomaterials (NMs). They are widely used as a glass-polishing agent and, more recently, have been employed as an effective diesel fuel borne catalyst, significantly reducing emissions and increasing engine efficiency.¹⁻³ Even though engineered NPs are already used in a wide range and large number of consumer products, the toxicological properties and environmental fate of these materials are still relatively poorly understood.³⁻⁵ In particular, such investigations require methods that can detect small quantities of NPs in complex natural samples against the natural background levels of the elements present. One promising tracing approach is based on mass dependent differences in the stable isotope compositions of elements.

Mass dependent differences, or fractionations, in stable isotope compositions are generated by processes of physical (e.g., diffusion, adsorption), chemical (e.g., precipitation, redox change) or biological nature. Recent advances in mass spectrometry have allowed the resolution of such isotope effects for numerous metals. This includes the elements Ca, Ba, and U,⁷⁻⁹ which resemble Ce due to their refractory, lithophile nature and moderate to high atomic mass number. Such studies have shown that stable isotope fractionations are common in nature and recorded in many natural materials. Furthermore, industrial processes, such as partial evaporation and diffusion during smelting and purification, have been found to create distinct isotopic signatures for some metals, which have been exploited for tracing anthropogenic emissions to the environment.¹⁰

In contrast to many other elements, stable isotope variations for Ce have received only little attention to date, with results presented in just two recent studies.^{6, 11} Whilst the findings of these authors are limited to only a few samples from adsorption and precipitation experiments and 5 natural samples, they do reveal small but clearly resolvable variations in stable Ce isotope compositions. It is therefore conceivable that industrial processing and purification of Ce and the preparation of CeO₂ NPs is also associated with isotopic fractionation. If these effects are large enough they may result in an isotopic signature that is

1
2
3 sufficiently distinct from the natural background (e.g., soil, water, biological tissue) such that
4 isotopic tracing is feasible. For example, CeO₂ NPs that differ in their ¹⁴²Ce/¹⁴⁰Ce isotope
5 ratio from the background value by 10‰ may be suitable for tracing. In this case, detection
6 and quantification of as little as 0.5 mg kg⁻¹ of NP-derived Ce is already possible in a sample
7 with a natural Ce background of 50 mg kg⁻¹, if the isotopic measurements achieve a
8 precision of better than ±0.1‰.
9

10
11 This study investigates the feasibility of the stable isotope tracing approach for CeO₂
12 NPs. To this end, high-precision Ce stable isotope data were acquired by multiple collector
13 inductively coupled plasma mass spectrometry (MC-ICP-MS) for CeO₂ nano- and bulk-
14 particles and other purified Ce materials. These samples were chosen, to determine whether
15 the purification of Ce and NP synthesis might result in isotopic signatures that are distinct
16 from 'normal' Ce. A sufficiently distinct isotope composition would enable the tracing of CeO₂
17 NMs in natural systems by means of stable isotope measurements. Such an approach
18 would allow investigations into the behavior and fate of CeO₂ NPs in real world settings and
19 samples, thereby providing the improved understanding of environmental cycling. This
20 knowledge is needed to investigate whether the use and emission of engineered NMs pose
21 a threat to health or the environment and thus develop informed risk assessments.
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41

42 **2 Experimental**

43 *2.1 Samples*

44
45 Seven commercially available CeO₂ NP samples and three CeO₂ reference materials
46 (of which two are also in NP form), all provided as dry powders, were analysed in this study
47 (Table 1). The reference materials (JRC NM-211, NM-212, NM-213) are available from the
48 European Commission Joint Research Centre (JRC) whilst the commercial CeO₂ NPs were
49 sourced directly from the manufacturers.
50
51
52
53
54
55
56

57
58 Furthermore, three different Ce standard solutions were analysed, whereby the Alfa
59 Aesar Specpure solution was used as in-house Ce isotope reference material, relative to
60 which all other Ce isotope compositions were determined. The Ce solution that was

Table 1 Summary of Ce isotope data for nano- and bulk-sized CeO₂ particles, including several reference materials, and other purified Ce samples.

Sample type	Supplier / comments	Particle size (nm) ^a	n ^b	δ ¹⁴² Ce (‰) ^c	± 2sd (‰) ^d	± 2se (‰) ^e
Ce Solutions:						
	Alfa Aesar; In-house δ-zero reference material			±0		
	Sigma-Aldrich		11	+0.05	0.07	0.02
	Bristol Ce solution ^f		9	+0.14	0.07	0.02
Reference materials:						
	Bulk CeO ₂ ; JRC NM-213; Sigma-Aldrich	600 ± 400	11	+0.07	0.05	0.01
	CeO ₂ NPs; JRC NM-211; Antaria	13 ± 3	15	-0.08	0.06	0.01
	CeO ₂ NPs; JRC NM-212; Umicore	28 ± 10	10	+0.07	0.05	0.01
Commercial CeO ₂ NPs:						
	MKnano-CeO ₂ -070	70	11	+0.07	0.04	0.01
	Sky Spring nano 2110 CG	10 - 30	14	+0.06	0.05	0.01
	io-li-tec NO-0029-HP	15 - 30	6	+0.03	0.02	0.01
	io-li-tec NO-0017-HP	50 - 80	6	+0.05	0.03	0.01
	Sigma-Aldrich 544841-5G	<25	8	+0.04	0.04	0.01
	Alfa Aesar 44909	30	7	-0.16	0.04	0.01
	Energenics Europe Ltd ^g	-	11	+0.05	0.04	0.01
Ce metals (99.9% purity):						
	Piece 1; RGB Research, 99.9% purity		8	+0.11	0.06	0.02
	Piece 2; RGB Research, 99.9% purity		5	+0.12	0.05	0.02
Ce salts (99.99% purity):						
	Ammonium Ce(IV) nitrate; Sigma-Aldrich 431338		9	+0.09	0.07	0.02
	Ce(III) nitrate; Alfa Aesar 11330		8	+0.03	0.07	0.02

^a Particle size as reported by supplier. ^b Number of individual analyses. ^c All isotopic data are reported relative to the Alfa Aesar Specpure Ce standard solution, which served as in-house δ¹⁴²Ce = 0‰ reference material. ^d The quoted 2sd uncertainties are based on the reproducibility of n individual measurements. ^e The quoted 2se uncertainties (standard error of the mean) were calculated as 2se = 2sd/√n. ^f Bristol Ce solution from Willbold¹² ^g Supplied directly from Energenics Europe Ltd on request, no product code or particle size data provided.

1
2
3 prepared by Willbold¹² at the University of Bristol (termed 'Bristol Ce' hereafter) has also
4
5 been proposed as a Ce isotope reference material. Additional purified Ce based materials
6
7 analysed encompass two small chunks of Ce metal that were treated as distinct samples,
8
9 and the Ce salts ammonium Ce(IV) nitrate $(\text{NH}_4)_2\text{Ce}(\text{IV})(\text{NO}_3)_6$ and Ce(III) nitrate,
10
11 $\text{Ce}(\text{III})(\text{NO}_3)_3$ (Table 1).
12
13

14 15 16 *2.2 General procedures and reagents*

17
18 All sample preparation work was carried out in the ISO class VI clean room facility of
19
20 the MAGIC Research Centre at the Department of Earth Science and Engineering, Imperial
21
22 College London. For all blank sensitive procedures ISO class IV laminar flow hoods were
23
24 utilised. Concentrated 14.5 M HNO_3 and 6 M HCl were purified prior to use by sub-boiling
25
26 distillation in quartz stills, whilst water was from a Millipore Milli-Q Academic system that
27
28 produces $>18.2 \text{ M}\Omega \text{ cm}^{-1}$ water. Suprapur quality 30% H_2O_2 solution (Merck Millipore) and
29
30 99.5% purity NaBrO_3 (Alfa Aesar) were used as purchased.
31
32
33

34 35 36 *2.3 Sample preparation for stable isotope analysis*

37
38 Working stock solutions with Ce concentrations of $100 \mu\text{g mL}^{-1}$ in 0.1 M HNO_3 were
39
40 prepared from the CeO_2 powders and the purified Ce based materials (Table 1) as follows.
41
42 For the three Ce standard solutions, suitable aliquots were diluted with 0.1 M HNO_3 .
43
44 Solutions of the two Ce metal pieces were prepared at room temperature by dissolving
45
46 about 1 g of metal in 200 mL 2 M HNO_3 . The resulting solutions were diluted with 2 M HNO_3
47
48 to obtain concentrated Ce solutions of $1000 \mu\text{g mL}^{-1}$. Aliquots of these were further diluted to
49
50 obtain the working stock solutions. For the $\text{Ce}(\text{III})(\text{NO}_3)_3$ and $(\text{NH}_4)_2\text{Ce}(\text{IV})(\text{NO}_3)_6$ salts, about
51
52 10-15 mg of material were dissolved in 4 mL 4 M HNO_3 at room temperature. The resulting
53
54 solutions were evaporated to dryness and taken up in 0.1 M HNO_3 .
55
56

57
58 For the CeO_2 powders, 10-15 mg of material were weighed into 15 mL Teflon
59
60 beakers, 4 mL 14.5 M HNO_3 and 1 mL 30% H_2O_2 , to reduce Ce(IV) to Ce(III), were added
before placing the beakers on a hotplate at 80°C . Dissolution was allowed to proceed

overnight, whereupon the temperature was increased to 160°C. The beakers were again left on the hotplate overnight following which the samples were dried down. If complete digestion was not achieved before drying, the above procedure was repeated until CeO₂ powders were no longer visible in the solution. The samples were subsequently dried down three times with 100 µL 14.5 M HNO₃ at 100°C, before taking up in 0.1 M HNO₃.

2.4 Mass spectrometry

The Ce stable isotope measurements were performed with a Nu Instruments Nu Plasma HR MC-ICP-MS at the Imperial College MAGIC Laboratories. The instrument is fitted with a large capacity (80 L min⁻¹) rotary pump for enhanced evacuation of the expansion chamber to improve sensitivity. A Nu Instruments DSN and a CETAC Aridus I desolvation system were employed for sample introduction, both with glass nebulizers that provided solution uptake rates of about 100 µL min⁻¹. Normal instrumental operating parameters are summarised in Table 2.

Table 2 Instrumental operating parameters

Nu Plasma HR MC-ICP-MS		
RF Power (W)		1300
Acceleration potential (V)		~6000
Ar coolant gas flow (L min ⁻¹)		13
Ar auxiliary gas flow (L min ⁻¹)		1
Expansion chamber vacuum (mbar)		~0.75
Analyzer vacuum (mbar)		~2 x 10 ⁻⁹
Typical sample uptake (µL mL ⁻¹)		~100
Instrument performance		
Sensitivity (V/(µg mL ⁻¹)):	Ce	110 - 160
	Ba	130 - 180
Transmission efficiency (%):	Ce	0.10 - 0.14
	Ba	0.11 - 0.15

1
2
3 For isotopic analyses, the 100 $\mu\text{g mL}^{-1}$ stock solutions of the purified Ce samples and
4 the in-house standard (Table 1) were diluted with 0.1 M HNO_3 to prepare measuring
5 solutions with Ce concentrations of between 50 and 125 ng mL^{-1} . These Ce solutions were
6
7
8
9
10 doped with a 10 $\mu\text{g mL}^{-1}$ Ba stock solution (in 0.1 M HNO_3) to obtain Ba concentrations of 75
11
12 to 350 ng mL^{-1} and Ce/Ba ratios of between 1.5 and 3.5.

13
14 Data collection was carried out by static multiple collection with the Faraday cups of
15 the instrument, which are fitted with $10^{11} \Omega$ resistors. Each analysis consisted of 60
16
17 integrations of 5 seconds each, in 3 blocks of 20, where the ion beams of the atomic masses
18
19 135 (Ba – collector L3), 137 (Ba – L2), 139 (La - Axial), 140 (Ce, Nd – H1), 141 (Pr – H2),
20
21 142 (Ce – H3), and 145 (Nd – H5) were monitored. Prior to each block, baseline signals
22
23 were measured for 15 seconds, whilst the ion beam was deflected in the electrostatic
24
25 analyser. Analyses of mixed Ce-Ba solutions typically yielded sensitivities of about 110 to
26
27 160 $\text{V } \mu\text{g}^{-1} \text{ mL}^{-1}$ for Ce and 130 to 180 $\text{V } \mu\text{g}^{-1} \text{ mL}^{-1}$ for Ba during the course of the study,
28
29 equivalent to a transmission efficiency of about 0.10 to 0.15% for both elements (Table 2).
30
31 Each measurement was followed by a thorough (~2-3 min) washout of the sample
32
33 introduction system with 0.1 M HNO_3 , and this was generally sufficient to reduce the
34
35 measured signals to the baseline intensities.

36
37 To determine variations in the stable isotope composition of Ce, the analyses
38
39 focused on the two major Ce isotopes and determination of the $^{142}\text{Ce}/^{140}\text{Ce}$ isotope ratio.
40
41 The $^{135}\text{Ba}/^{137}\text{Ba}$ isotope ratio of the admixed Ba was monitored for mass bias correction with
42
43 the exponential law.¹³ Although only purified Ce materials were analysed, small amounts of
44
45 Nd were present in the samples and so the ^{145}Nd ion beam was measured for correction of
46
47 the isobaric interference of ^{142}Nd on ^{142}Ce using a ratio of $^{142}\text{Nd}/^{145}\text{Nd} = 3.27711$ ¹⁴. The
48
49 presence of the light rare earth elements (LREE) La and Pr was also monitored, using ^{139}La
50
51 and ^{141}Pr , even though interference corrections are not necessary. To assess the robustness
52
53 of the correction for isobaric ^{142}Nd , a series of Alfa Aesar Ce standard solutions were doped
54
55 with increasing amounts of Nd. This enabled determination of the maximum Nd/Ce ratios
56
57 that can be tolerated during analyses.
58
59
60

1
2
3 All sample measurements were bracketed with at least two analyses of the in-house
4 Alfa Aesar Ce isotope reference material. Differences between the corrected $^{142}\text{Ce}/^{140}\text{Ce}$
5 ratios of the samples and the reference material are reported in the form of $\delta^{142}\text{Ce}$ values,
6 which denote the relative deviation of the $^{142}\text{Ce}/^{140}\text{Ce}$ isotope ratio of a sample (R_{sam}) from
7 the in-house Alfa Aesar standard (R_{std}) in parts per 1000:
8
9
10
11
12

$$\delta^{142}\text{Ce} = ((R_{\text{sam}} - R_{\text{std}}) / R_{\text{std}}) \times 1000 \quad (1)$$

13
14
15
16
17
18

19 3 Results and discussion

20 3.1 Precision and accuracy of Ce stable isotope data for CeO_2 and purified Ce samples

21 The isotope data obtained for the CeO_2 powders and purified Ce samples (Table 1)
22 were acquired over a 9-month period that encompassed 11 separate analytical sessions.
23 Each single measurement consumed approximately 50 to 100 ng of Ce and the $\delta^{142}\text{Ce}$ data
24 for the samples feature 2sd reproducibilities, based on the results of 5 to 15 individual
25 measurements, of $\pm 0.02\text{‰}$ to $\pm 0.07\text{‰}$ (Table 1). Based on the multiple analyses, the mean
26 results have 2se uncertainties of only $\pm 0.01\text{‰}$ to $\pm 0.02\text{‰}$ (Table 1).
27
28
29
30
31
32
33
34
35

36 These performance characteristics are similar to that achieved in MC-ICP-MS stable
37 isotope analyses for elements of similar mass when normalised to a mass difference of 1
38 amu (comparison of 2sd/amu results). For example, typical 2sd/amu uncertainties of $\pm 0.01\text{‰}$
39 to $\pm 0.03\text{‰}$ were reported for MC-ICP-MS analyses of Cd and Mo standard solutions by
40 Abouchami *et al.*¹⁵ and Goldberg *et al.*¹⁶, respectively. Our data also compare favourably to
41 the Ce stable isotope results of Nakada *et al.*¹¹ and Ohno and Hirata⁶, who reported $\delta^{142}\text{Ce}$
42 uncertainties (2sd) of $\pm 0.06\text{‰}$ and $\pm 0.08\text{‰}$ for multiple analyses of Ce solutions. As in this
43 study, these authors also employed MC-ICP-MS but the samples were doped with Sm, and
44 $^{149}\text{Sm}/^{147}\text{Sm}$ was used for external normalisation of the instrumental mass bias.
45
46
47
48
49
50
51
52
53
54
55

56 As the analysed samples were purified Ce materials, it is unlikely that the accuracy of
57 the data is compromised by matrix effects and/or spectral interferences. The absence of the
58 former is confirmed by the observation that none of the samples displayed any unusual
59
60

mass bias behaviour of Ba during the analyses. In addition, it was observed that the use of two different sample introduction systems and variations in the Ce, Ba concentrations and Ce/Ba ratios between sample and the bracketing standard solutions of up to 460% and 230% respectively, had no discernible effect on the $\delta^{142}\text{Ce}$ data at the quoted level of precision.

The purity of the Ce solutions was, furthermore, assessed throughout the isotopic analyses by monitoring the LREEs La, Pr and Nd. These elements are likely to be the most prominent contaminants, as they are difficult to separate from Ce. However, only trace amounts of the LREEs were present, with typical LREE/Ce ratios of less than 10×10^{-5} and a maximum Nd/Ce of about 60×10^{-5} for a CeO_2 powder and the two metal samples (Table 3). Any Nd contamination is, however, of concern due to the isobaric interference of ^{142}Nd on ^{142}Ce , which was corrected during the analyses based on the monitoring of ^{145}Nd . Table 3 summarises the corrections that were applied to the $\delta^{142}\text{Ce}$ data of samples to account for the ^{142}Nd interference. The corrections were generally observed to be less than 0.2‰ but with maximum levels of up to 1.0 to 1.4‰ (Figure 1).

Table 3 REE/Ce ratios that were determined for the Ce standard and sample solutions and the corresponding correction to the $\delta^{142}\text{Ce}$ values.

	$\delta^{142}\text{Ce}$ correction (‰) ^a	Nd/Ce ($\times 10^{-5}$)	La/Ce ($\times 10^{-5}$)	Pr/Ce ($\times 10^{-5}$)
Purified Ce materials				
Alfa Aesar Ce Solution	0.2	8.3	3.2	5.7
Other Ce solutions	0.06 – 0.3	2.4 – 12	0.3– 3.5	0.3 – 2.8
CeO_2 powders	0.03 - 1.4	1.2 - 62	0.2 - 32	0.2 – 52
Ce metals	1	44	23	1.5
Ce salts	0.03 – 0.05	1.1 – 2.2	<0.01 – 0.8	<0.01 – 4.5

^a Change in $\delta^{142}\text{Ce}$ after correction for isobaric ^{142}Nd .

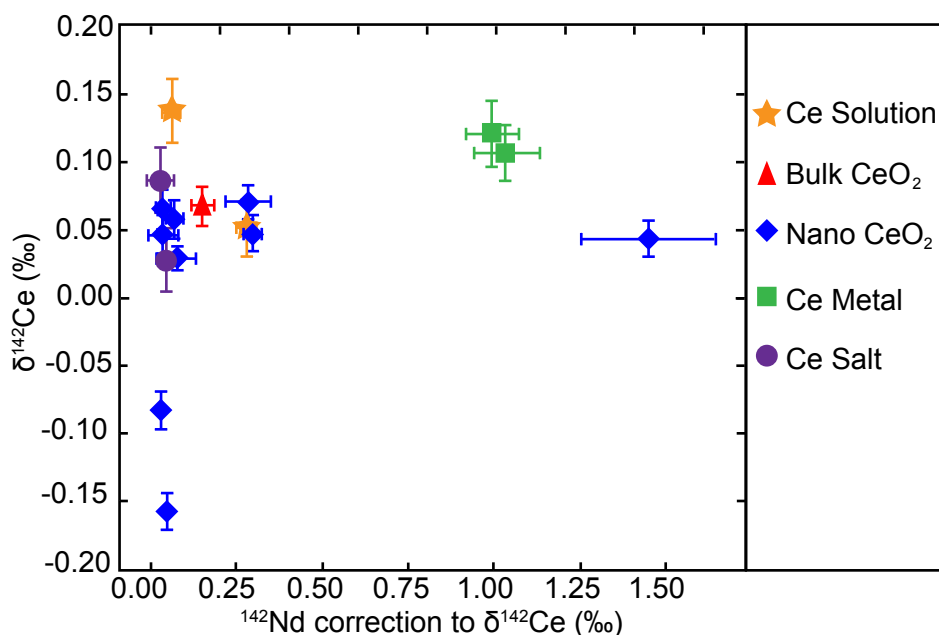


Figure 1 The $\delta^{142}\text{Ce}$ values of the purified Ce materials (Table 1) are plotted against the correction to the $\delta^{142}\text{Ce}$ values for the presence of isobaric ^{142}Nd (Table 3). The error bars associated with the x-axis denote the range of corrections applied to the $\delta^{142}\text{Ce}$ values for the presence of isobaric ^{142}Nd (Table 3), whereas the y-axis error bars denote the 2se uncertainties of the $\delta^{142}\text{Ce}$ values based on multiple analyses ($n = 5$ to 15; Table 1).

The controlled doping of the Alfa Aesar Ce standard solution with Nd was used to investigate the maximum Nd/Ce ratios that can be tolerated for reliable Ce isotope measurements. Our data demonstrate that correction of the ^{142}Nd interference on ^{142}Ce resulted in $^{142}\text{Ce}/^{140}\text{Ce}$ ratios that were identical, within 2sd uncertainty, to data for non-doped Alfa Aesar Ce solutions at Nd/Ce ratios of up to 0.01 (Figure 2). As all purified Ce materials analysed here were characterised by Nd/Ce of less than 0.001 (Table 3), the results obtained for these samples can be considered as accurate, as the presence of isobaric ^{142}Nd did not generate analytical artefacts. This conclusion is underlined by additional observations. First, a plot of $\delta^{142}\text{Ce}$ versus magnitude of the ^{142}Nd correction shows no obvious correlation (Figure 1). Second, seven of the nine CeO₂ powders are characterised by a very narrow range of $\delta^{142}\text{Ce}$ values, even though they feature variable levels of Nd. It is highly unlikely that the isotopic homogeneity of the CeO₂ powders is a fortuitous result of an inaccurate Nd correction. Third, the two isotopically distinct CeO₂ samples are subject to only relatively small $\delta^{142}\text{Ce}$ corrections of 0.03‰ and 0.05‰, which implies that the negative $\delta^{142}\text{Ce}$ values are unlikely to be an artefact. In summary, these

observations indicate, that the applied corrections on $\delta^{142}\text{Ce}$ for the presence of isobaric ^{142}Nd were accurate even at the highest observed Nd/Ce ratios of about 60×10^{-5} (Table 3).

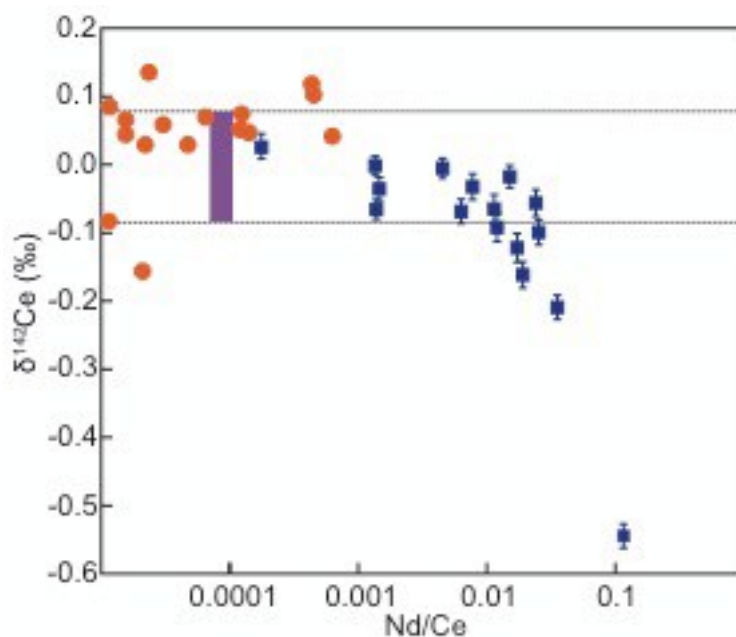


Figure 2 Plot of measured $\delta^{142}\text{Ce}$ values versus the Nd/Ce ratios of the sample solutions. The purple bar and dotted lines denote the 2sd uncertainty determined from multiple analyses of the Alfa Aesar Ce standard solution ($\pm 0.09\text{‰}$, $n = 25$). The data obtained for Alfa Aesar Ce standard solutions doped with varying levels of Nd (blue squares with internal 2sd uncertainties) demonstrate that accurate $\delta^{142}\text{Ce}$ values can be readily obtained at Nd/Ce ratios of up to 0.01. The orange circles represent the Ce samples that were analysed in this study.

3.2 Isotopic variability

The analysed CeO_2 NPs show a total variability in $\delta^{142}\text{Ce}$ of 0.23‰ , with values of between -0.16‰ and 0.07‰ . However, 7 of the 9 samples display a very narrow range of $\delta^{142}\text{Ce}$ values of 0.03‰ to 0.07‰ , whilst two outliers are characterised by $\delta^{142}\text{Ce}$ of -0.08‰ and -0.16‰ (Table 1, Figure 3). The CeO_2 bulk particles are essentially indistinguishable from most of the CeO_2 NP powders, with a $\delta^{142}\text{Ce}$ value of $0.07 \pm 0.01\text{‰}$ (2se). The remaining purified Ce samples also show only very limited variability in $\delta^{142}\text{Ce}$. The two Ce salts and the Sigma-Aldrich Ce standard solution are hereby isotopically identical, within the quoted 2se uncertainties of only 0.01 to 0.02‰ , to the CeO_2 particles. The two metal samples are slightly heavier with $\delta^{142}\text{Ce}$ values that are identical within uncertainty at 0.11‰ and 0.12‰ (Table 1, Figure 3).

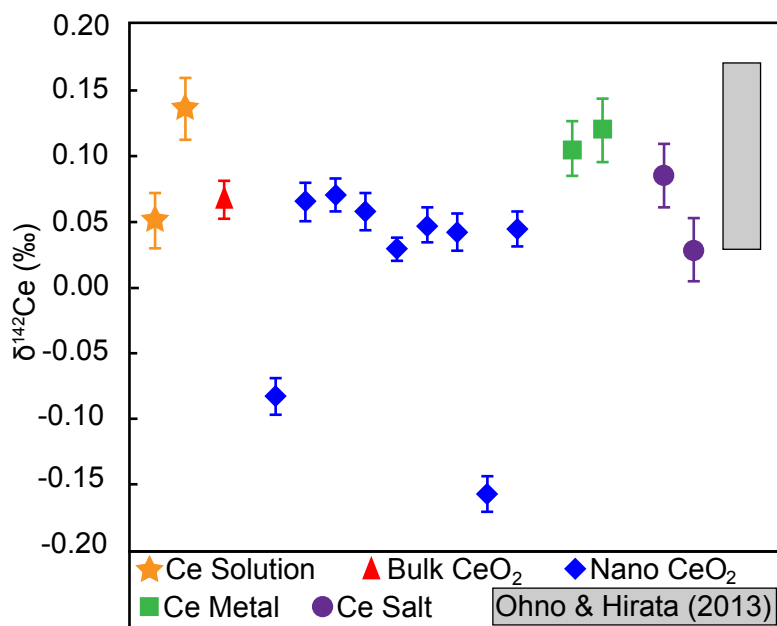


Figure 3 $\delta^{142}\text{Ce}$ data for the Ce samples analysed in this study. Error bars denote the 2 σ uncertainties that were calculated based on multiple analyses ($n = 5$ to 15; Table 1). The grey field denotes the range of $\delta^{142}\text{Ce}$ values determined by Ohno and Hirata⁶ for 5 rock samples. However, the position of this field in relation to our data may not be accurate, as a different Ce reference material were applied to define $\delta^{142}\text{Ce} = 0$.

No information was provided by the manufacturers on the provenance of the Ce or the methods that were used for element purification and NP synthesis. It is therefore conceivable that the limited isotopic variability observed here for various forms of purified Ce is simply a consequence of similar origin and similar production methods. It is notable, however, that our results appear to be in good accord with the Ce data published by Ohno and Hirata⁶. Even though the two investigations cannot be compared directly, as they are expressed relative to different $\delta^{142}\text{Ce} = 0$ reference materials, Ohno and Hirata⁶ also found only a limited range of $\delta^{142}\text{Ce}$ values of 0.14‰ for two igneous and three sedimentary rock samples (Figure 3). This may indicate that, even though some samples display resolvable isotopic differences, the overall variability of Ce stable isotope compositions may be quite limited for most terrestrial materials.

Considering the aims of our study, the observed 0.3‰ variability in $\delta^{142}\text{Ce}$ is too small to be exploitable for routine tracing purposes. This is demonstrated by a best-case scenario, which assumes that CeO₂ NPs have a $\delta^{142}\text{Ce}$ value that differs from a constant

1
2
3 natural background by 0.3‰. In this instance, an increase in the background Ce
4 concentration of 20%, from the addition of CeO₂ NPs, would result in a change of the δ¹⁴²Ce
5 value by 0.05‰. This example demonstrates that isotopic tracing methods for CeO₂ NPs
6 which are based on inherent differences in δ¹⁴²Ce are of no practical value because they do
7 not provide detection capabilities that are clearly superior to those offered by less costly and
8 less time consuming concentration measurements.
9
10
11
12
13
14
15
16
17

18 **4 Conclusions**

19
20 We present a robust and novel analytical protocol for the determination of ¹⁴²Ce/¹⁴⁰Ce
21 isotope ratios by MC-ICP-MS, which offer a reproducibility (2sd) of about ±0.05‰. The
22 techniques are, in principle, suitable for analyses of natural materials if used in conjunction
23 with an appropriate procedure for the separation and purification of Ce from the sample
24 matrix.
25
26
27
28
29
30

31 Our analyses show that commercially available CeO₂ NPs do not have a distinct isotope
32 signature and their detection in natural samples by stable isotope tracing is, therefore, not
33 feasible. However, the stable isotope tracing approach may still be successfully applied if an
34 enriched Ce isotope is used to produce isotopically labelled CeO₂ NPs.¹⁷
35
36
37
38
39
40
41

42 **Acknowledgements**

43
44 Two anonymous referees are thanked for their constructive comments. This research was
45 supported by funding from DEFRA and EPSRC and was carried out as part of PROSPECT,
46 a public–private partnership between DEFRA, EPSRC, TSB and the Nanotechnology
47 Industries Association (NIA Ltd.) and its members.
48
49
50
51
52
53
54
55
56
57
58
59
60

References

1. V. Arul Mozhi Selvan, R. B. Anand and M. Udayakumar, *ARPN Journal of Engineering and Applied Sciences*, 2009, **4**.
2. B. Park, P. Martin, C. Harris, R. Guest, A. Whittingham, P. Jenkinson and J. Handley, *Part Fibre Toxicol*, 2007, **4**, 12.
3. F. R. Cassee, E. C. van Balen, C. Singh, D. Green, H. Muijser, J. Weinstein and K. Dreher, *Crit Rev Toxicol*, 2011, **41**, 213-229.
4. R. D. Handy, R. Owen and E. Valsami-Jones, *Ecotoxicology*, 2008, **17**, 315-325.
5. K. Savolainen, L. Pylkkanen, H. Norppa, G. Falck, H. Lindberg, T. Tuomi, M. Vippola, H. Alenius, K. Hameri, J. Koivisto, D. Brouwer, D. Mark, D. Bard, M. Berges, E. Jankowska, M. Posniak, P. Farmer, R. Singh, F. Krombach, P. Bihari, G. Kasper and M. Seipenbusch, *Safety Sci*, 2010, **48**, 957-963.
6. T. Ohno and T. Hirata, *Anal Sci*, 2013, **29**, 47-53.
7. J. L. Druhan, C. I. Steefel, K. H. Williams and D. J. DePaolo, *Geochim Cosmochim Ac*, 2013, **119**, 93-116.
8. K. von Allmen, M. E. Bottcher, E. Samankassou and T. F. Nagler, *Chemical Geology*, 2010, **277**, 70-77.
9. G. A. Brennecka, L. E. Borg, I. D. Hutcheon, M. A. Sharp and A. D. Anbar, *Earth Planet Sc Lett*, 2010, **291**, 228-233.
10. A. E. Shiel, D. Weis and K. J. Orians, *Sci Total Environ*, 2010, **408**, 2357-2368.
11. R. Nakada, Y. Takahashi and M. Tanimizu, *Geochim Cosmochim Ac*, 2013, **103**, 49-62.
12. M. Willbold, *J Anal Atom Spectrom*, 2007, **22**, 1364-1372.
13. M. Rehkämper, M. Schönbachler and C. H. Stirling, *Geostandard Newslett*, 2001, **25**, 23-40.
14. J. K. Bohlke, J. R. de Laeter, P. De Bièvre, H. Hidaka, H. S. Peiser, K. J. R. Rosman and P. D. P. Taylor, *J Phys Chem Ref Data*, 2005, **34**, 57-67.
15. W. Abouchami, S. J. G. Galer, T. J. Horner, M. Rehkämper, F. Wombacher, Z. C. Xue, M. Lambelet, M. Gault-Ringold, C. H. Stirling, M. Schonbachler, A. E. Shiel, D. Weis and P. F. Holdship, *Geostand Geoanal Res*, 2013, **37**, 5-17.
16. T. Goldberg, G. Gordon, G. Izon, C. Archer, C. R. Pearce, J. McManus, A. D. Anbar and M. Rehkämper, *J Anal Atom Spectrom*, 2013, **28**, 724-735.
17. F. Larner and M. Rehkämper, *Environ Sci Technol*, 2012, **46**, 4149-4158.