


Journal of Materials Chemistry B

Materials for biology and medicine

rsc.li/materials-b

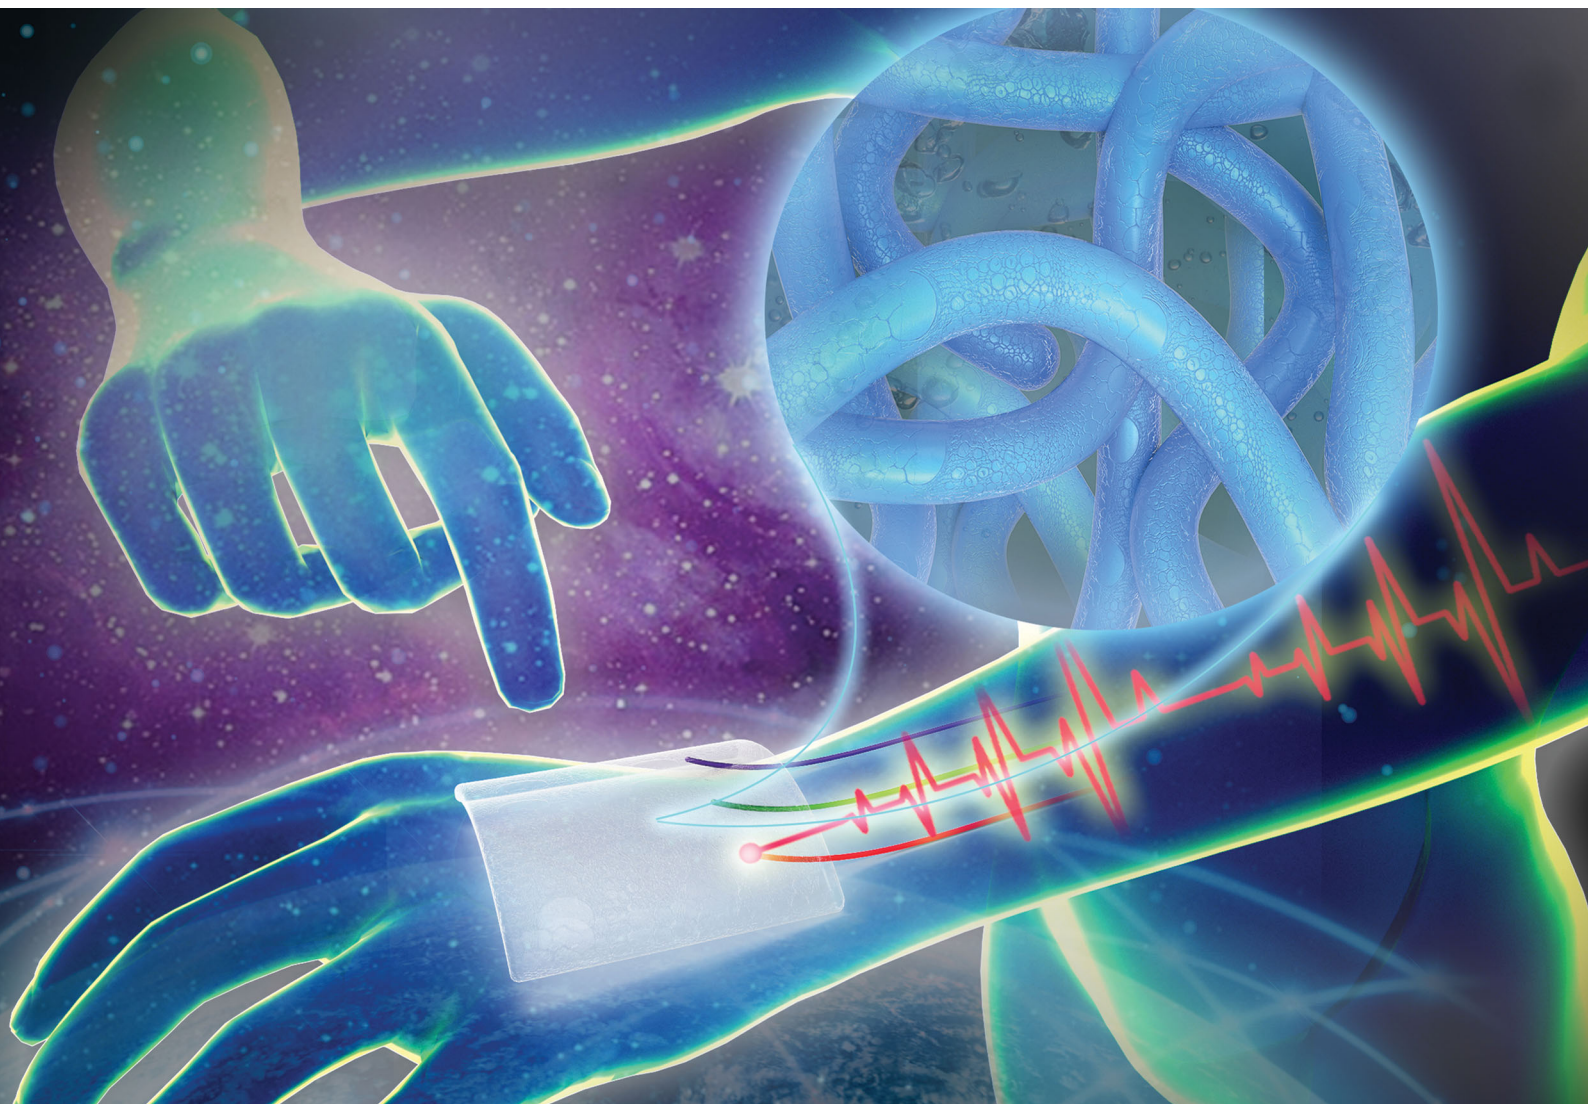

Themed issue: Biosensors

ISSN 2050-750X



ROYAL SOCIETY
OF CHEMISTRY

REVIEW ARTICLE

Jie Zheng *et al.*

From design to applications of stimuli-responsive hydrogel strain sensors

Indexed in
Medline!



Cite this: *J. Mater. Chem. B*, 2020, **8**, 3171

From design to applications of stimuli-responsive hydrogel strain sensors

Dong Zhang,^{†a} Baiping Ren,^{†a} Yanxian Zhang,^a Lijian Xu,^b Qinyuan Huang,^c Yi He,^d Xuefeng Li,^e Jiang Wu,^f Jintao Yang,^g Qiang Chen,^h Yung Changⁱ and Jie Zheng^{id}*^a

Stimuli-responsive hydrogel strain sensors that synergize the advantages of both soft-wet hydrogels and smart functional materials have attracted rapidly increasing interest for exploring the opportunities from material design principles to emerging applications in electronic skins, health monitors, and human-machine interfaces. Stimuli-responsive hydrogel strain sensors possess smart and on-demand ability to specifically recognize various external stimuli and convert them into strain-induced mechanical, thermal, optical, and electrical signals. This review presents an up-to-date summary over the past five years on hydrogel strain sensors from different aspects, including material designs, gelation/fabrication methods, stimuli-responsive principles, and sensing performance. Hydrogel strain sensors are classified into five major categories based on the nature of the stimuli, and representative examples from each category are carefully selected and discussed in terms of structures, response mechanisms, and potential medical applications. Finally, current challenges and future perspectives of hydrogel strain sensors are tentatively proposed to stimulate more and better research in this emerging field.

Received 27th November 2019,
Accepted 13th January 2020

DOI: 10.1039/c9tb02692d

rsc.li/materials-b

^a Department of Chemical, Biomolecular, and Corrosion Engineering, The University of Akron, Ohio 44325, USA. E-mail: zhengj@uakron.edu

^b Hunan Key Laboratory of Biomedical Nanomaterials and Devices, College of Life Science and Chemistry, Hunan University of Technology, Zhuzhou 412007, China

^c School of Automation and Information Engineering, Sichuan University of Science and Engineering, Zigong, Sichuan 643000, P. R. China

^d College of Chemical and Biological Engineering, Zhejiang University, Zheda Road 38, Hangzhou 310027, China

^e School of Material Science and Chemical Engineering, Hubei University of Technology, Wuhan 430068, P. R. China

^f School of Pharmaceutical Sciences, Wenzhou Medical University, Wenzhou, Zhejiang 325035, China

^g College of Materials Science & Engineering, Zhejiang University of Technology, Hangzhou 310014, China

^h School of Material Science and Engineering, Henan Polytechnic University, Jiaozuo, 454003, China

ⁱ Department of Chemical Engineering and R&D Center for Membrane Technology, Chung Yuan Christian University, Taoyuan 320, Taiwan

[†] These authors contribute equally to this work.



Dong Zhang

Dong Zhang is currently pursuing his PhD degree in the Department of Chemical, Biomolecular, and Corrosion Engineering at the University of Akron (UA) under the guidance of Prof. Jie Zheng. He received his BE (2016) and ME (2018) in Materials Science and Engineering at Zhejiang University of Technology, China. His current research focuses on the synthesis and characterization of biocompatible and functionalizable polymers for biomedical applications. He has published 26 peer-reviewed papers.




Baiping Ren

Dr Baiping Ren is currently an ORISE (Oak Ridge Institute for Science and Education) fellow in NCTR (National Center for Toxicological Research) of FDA and received her PhD of Chemical, Biomolecular, and Corrosion Engineering at the University of Akron (UA) from the Zheng lab in 2019. She has published 33 papers in several interdisciplinary research fields of smart polymers, anti-fouling materials, tough hydrogels, amyloid inhibitors, and anti-bacterial materials.

1. Introduction

Hydrogels, as classical soft-wet materials containing high water content in flexible 3D networks possess many structural and functional advantages such as hierarchical porous structures,

viscoelasticity, transparency, stretchability, and biocompatibility. Particularly, recent studies have pushed the potential applications and development of hydrogels from the traditional fields of cell/tissue scaffolds,^{1–4} drug/gene delivery carriers,^{5–7} wound dressings,^{8–11} and contact lenses^{12–14} to the emerging

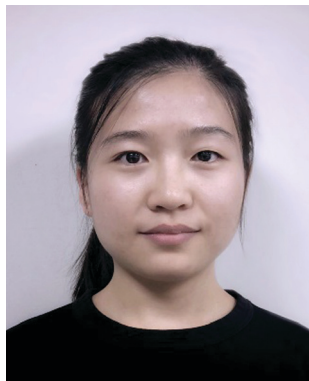

Yanxian Zhang

Yanxian Zhang is currently pursuing her PhD degree in the Department of Chemical, Biomolecular, and Corrosion Engineering at the University of Akron (UA) under the guidance of Prof. Jie Zheng. She received her BS (2014) and MS (2017) degree in Materials Science and Engineering at the University of Science and Technology Beijing, China. Her research interest mainly focuses on smart hydrogels, amyloid proteins, and antifouling materials, with 20+ papers published in these fields.




Lijian Xu

Dr Lijian Xu is a Professor of the College of Life Sciences and Chemistry at Hunan University of Technology, China. He earned his PhD in 2009 from the State Key Laboratory of Bioelectronics, Southeast University and later joined Hunan University of Technology in 2006. He has published more than 40 papers in the field of functional nanomaterials and biosensors for biomedical applications.



Qinyuan Huang

Dr Qinyuan Huang is an Assistant Professor at the School of Automation and Information Engineering at Sichuan University of Science and Engineering, China. He received his PhD in Mechatronic Engineering in 2016 at Sichuan University, China. His research interests include artificial intelligence, signal processing, evolutionary computation, and non-destructive testing of composite materials.

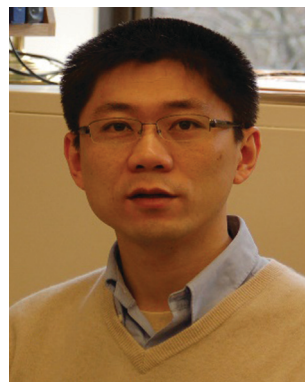

Yi He

Dr Yi He is an Associate Professor of College of Chemical and Biological Engineering at Zhejiang University and an Affiliate Associate Professor of Department of Chemical Engineering at University of Washington, Seattle. He earned his BS and PhD in Chemical Engineering at Zhejiang University, China (2000) and University of Washington (2008), respectively. His recent work has been primarily focused on developing new materials and technologies to improve human health and promote environmental sustainability without sacrificing economic viability and efficiency.



Xuefeng Li

Dr Xuefeng Li is a Professor of Polymer Materials Engineering at Hubei University of Technology (China). Li earned his BS and PhD in Polymer Materials Engineering at Hubei University of Technology (1995) and Huazhong University of Science and Technology (2005), respectively. His current research mainly focuses on the design, synthesis, and application of soft and wet polymer materials. He has authored over 100 peer-reviewed papers.




Jiang Wu

Dr Jiang Wu is currently an Associate Professor of Pharmaceutical Sciences at Wenzhou Medical University. She received her BS in Pharmaceutical Engineering (2009) and PhD in Applied Chemistry (2014) at Zhejiang University, China. She has special research interest in the design, synthesis, and engineering of bioinspired materials for wound regeneration, and has published 20+ papers in this field.

fields of wearable devices,^{15–17} electronic skins,^{18,19} soft robotics,^{20–22} and artificial intelligence sensors.²³ Among them, stimuli-responsive hydrogel strain sensors have attracted significant and continuous interest to be developed as a promising platform for disease diagnosis, health monitoring, damage/motion detection, water/food safety, and environmental monitoring^{24–28} because of their intelligent and programmable features capable of changing their shape/size/volume and probably other functional properties (e.g. conductivity, permeability, viscosity, and mechanics) in response to different stimuli. Different from dry sensors made of elastomers, polymer/inorganic composites, and carbon-based materials without water, the presence of a high water content enables hydrogel strain sensors to exhibit intrinsic swelling-induced viscoelastic, mechanical, self-recovery, self-healing properties,^{29–36} rendering them great potential to realize a variety of sensing actuations under different stimuli.³⁷ On the other hand, due to the high hydration nature of hydrogel sensors, all their stimuli-responsive polymers, crosslinkers, and incorporated entities need to be compatible with and

workable under wet and aqueous conditions. Another major difference is that the mismatched mechanics among polymer networks, additives, and crosslinkers with different swelling extents at polymer/water interfaces will create asymmetric forces that drive shape and volume changes of hydrogels even under subtle stimuli.

From a materials design viewpoint, all stimuli-responsive hydrogels can be potentially fabricated into hydrogel-based sensors. Several general design strategies have been proposed and demonstrated for the successful development of a wide variety of hydrogel sensors. Firstly, the most commonly used design is to directly fabricate stimuli-responsive materials into hydrogels, which are sensitive to external stimuli of temperature, pH, salt, light, and electric field. Several typical stimuli-responsive hydrogels include thermo-responsive poly(*N*-isopropylacrylamide) (polyNIPAM) and poly(vinyl methyl ether) (polyVME) hydrogels, pH-responsive carboxylated poly(2-hydroxyethyl methacrylate-ethylene glycol dimethacrylate) (poly(HEMA-EDMA)) hydrogels,³⁸ electronic-responsive conducting polymer-based (CPS) hydrogels,³⁹

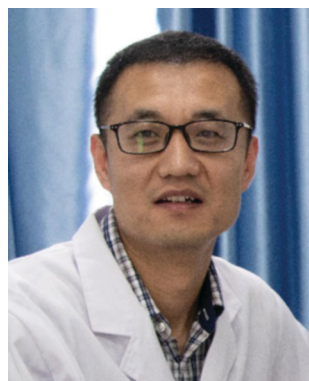

Jintao Yang

Dr Jintao Yang is a Professor of College of Materials Science and Technology, Zhejiang University of Technology. He received his BS and PhD in chemical engineering at China University of Petroleum (2000) and Zhejiang University (2005), respectively. His main research interests include polymer processing, polymer surfaces and interfaces, in particular smart materials based on zwitterionic polymers for biological and sensing applications. He has published over 70 peer reviewed papers.



Qiang Chen


Dr Qiang Chen is a Professor of Materials Science and Engineering at Henan Polytechnic University, China (HPU). Chen earned his BS and PhD in Chemistry and Polymer Chemistry and Physics at Henan University, China (2004) and Changchun Institute of Applied Chemistry, Chinese Academy of Sciences (2009), respectively. He joined HPU in 2009. His current research mainly focuses on tough hydrogels, adhesive hydrogels, and conductive hydrogels, and their functional applications. He has authored over 50+ peer-reviewed papers, with an h-index of 24 and citation of 1900+.



Yung Chang

Dr Yung Chang is a Distinguished Professor and the Director of the R&D center for Membrane Technology at Chung Yuan Christian University (CYCU), Taiwan. Chang earned his PhD in Chemical Engineering at National Taiwan University (2004). His current research mainly focuses on molecular design, technology development, and healthcare applications of bio-mimetic zwitterionic interfaces and membranes. He has authored over 200 peer-reviewed

papers and served on Editorial Boards and as an Editors in J. Polymer Research, and J. Taiwan Institute of Chemical Engineers.

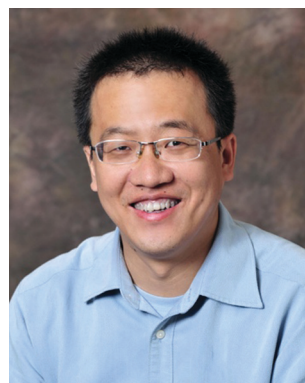

Jie Zheng

Dr Jie Zheng is a Professor of Chemical, Biomolecular, and Corrosion Engineering at University of Akron (UA). Zheng earned his BS and PhD in Chemical Engineering at Zhejiang University, China (1995) and University of Washington (2005), respectively. His current research mainly focuses on the design/engineering, synthesis, and application of better bio-functional and bio-mimetic soft materials. He has authored over 200 peer-reviewed papers, with an h-index of 54 and citation of 10 000+, and served on Editorial Boards and as an Editor in J. Materials Chemistry B, ACS Applied Bio Materials, PLoS One, and others.

light/force-sensitive poly(acrylamide (AAm)-*co*-methyl acrylate (MA))/spiropyran (SP) hydrogels,^{40,41} and salt-responsive poly([2-(methacryloyloxy)ethyl]-trimethylammonium chloride)-[*N*-(2-hydroxyethyl) acrylamide]/poly(3-(1-(4-vinylbenzyl)-1*H*-benzo[*d*]imidazol-3-ium-3-yl)-propane-1-sulfonate) (poly(METAC-HEAA)/polyVBIPS) and polyNIPAM/polyVBIPS hydrogels.^{42,43} Advances in chemical synthesis and gelation methods also allow the copolymerization or sequential polymerization of different stimuli-responsive monomers and crosslinkers to achieve dual or multiple stimuli-responsive properties embedded in hydrogel sensors, including polyAAM/poly(vinylalcohol)(PVA) humidity sensor,⁴⁴ poly(β -cyclodextrin (β -CD)-methacrylic acid (AAc)) hydrogels,⁴⁵ and Eu³⁺/Tb³⁺-polyNIPAM hydrogel.⁴⁶ In general, since hydrogels are typically isotropic materials, the use of pure polymer materials or simple polymer structures is unlikely to selectively trigger site-specific swelling or contraction, leading to shape adaptability and transformation in a controllable manner. To overcome this issue, another common design strategy is to incorporate stimuli-responsive entities (*i.e.* nanoparticles, nanoclay, nano-crystalline cellulose, and functional polymer chains) into hydrogel networks to create in-homogeneous structures, which in turn help to readily generate mismatch stress for a strain sensing under the desired stimuli. These stimuli-responsive entities can be either physically added to or chemically crosslinked with hydrogel networks, both of which require a controlled orientation and spatial distribution to achieve well-defined network architectures and to maximize the sensibility to external stimuli. However, the additional difficulty of snug-filling small entities into the porous structures of hydrogels needs to be addressed for preventing dead zones upon deformation.

From a structural design viewpoint, constructing hybrid network structures in hydrogel sensors, such as double-network structure, bilayer/multi-layer structure, interpenetrating structure, nanofilled structure, gradient structure, and other heterostructures, also allows the creation of mismatch stress in the polymer networks (*e.g.* softer *vs.* stiffer, swelling *vs.* non/less-swelling, and hydrophobic *vs.* hydrophilic) for achieving different sensing actuations in response to various external stimuli. Moreover, the network structure of hydrogel sensors can be cross-linked using either irreversible or reversible crosslinkers/additives.^{47,48} The incorporation of single or multiple reversible crosslinkers/additives, in most cases, enable different components or regions of hydrogels to undergo different extents of volume expansion/contraction in certain positions, directions, and even swelling rates, thus leading to programmable shape changes by bending, expanding, contracting, twisting, and fast buckling.

In all these designs, searching for new responsive sensing materials/components and constructing well-defined network structures are equally important for the rational design of highly sensitive and robust hydrogel sensors. However, although this sounds simple and straightforward, the appropriate integration of sensing materials and entities into hydrogel networks still remains a challenge mainly due to the incompatibility between materials, structures, and gelation methods. Moreover, on one hand, many hydrogel strain sensors exhibit a certain degree of reversible and multiple sensing ability due to their intrinsic stimuli-responsive nature; on the other hand, since the exposure of

hydrogels to external stimuli often damages their irreversible bonds and crosslinkers, hydrogel sensors also suffer from a loss in their original sensing ability. Thus, the introduction of self-healing functions in hydrogel sensors becomes necessary to rapidly recover their original network structure and to sustain their sensing ability through the dynamic reformation of reversible noncovalent interactions (*e.g.* hydrogen bonds, π - π stacking, hydrophobic interactions, host-guest interactions, and metal-coordination interactions) and/or reversible covalent bonds (*e.g.* imine bonds, disulfide bonds, acylhydrazone bonds, and boronate ester bonds).⁴⁹⁻⁵¹ Again, the cooperative and compatible fabrication of both self-healing and stimuli-responsive materials/entities in the same hydrogel may also face additional challenges. Similarly, hydrogel strain sensors must exhibit sensing-appropriate physical, mechanical, and biological properties. Generally, hydrogel strain sensors usually require high mechanical strength, toughness, and stretchability for transducing mechanical deformation into electrical/chemical/optical signals.⁵²⁻⁵⁵ Specifically, *in vivo* injectable hydrogel strain sensors must be biodegradable and biocompatible, and their degraded products also need to be biocompatible with minimal inflammatory responses.

All of these challenges from both materials and structural viewpoints highlight the importance of fabrication methods. Hydrogel strain sensors can be rationally designed and fabricated from a large dataset of stimuli-responsive monomers and crosslinkers *via* different polymerization methods, such as living cationic and anionic polymerization, reversible addition-fragmentation chain-transfer (RAFT) polymerization, atom-transfer radical polymerization (ATRP), self-assembly, microfabrication, and laser writing, all of which can well control the chemistry and structure in hydrogel networks.⁵⁶⁻⁶¹ In some cases, the polymer networks in hydrogel sensors can be readily functionalized with different stimuli-responsive pendent groups and additives even before gelation, and the resulting hydrogels can be directly used for sensing applications without the need for additional substrates and matrixes to serve as sensor platform.

As shown in Table 1 and Fig. 1, we summarized and classified some classical hydrogel sensors with different types of sensing ability. This review aims to highlight the most important and recent works on hydrogel sensors in the past five years, instead of a comprehensive review. Specifically, this review mainly covers the design principles and synthesis strategies of hydrogel sensors from both materials and structural viewpoints, selectively highlights some classical and interesting hydrogel sensors for different sensing purposes and applications, and finally presents some of the current scientific/technological barriers and the future research directions that should be undertaken to overcome these barriers.

2. General design strategy and categories of hydrogel strain sensors

To better understand the structure-function relationship of hydrogel strain sensors, here we classified hydrogel strain sensors into five basic groups of nanoparticle-incorporated, conducting polymer-incorporated, polyelectrolyte-incorporated,

Table 1 Summary and classification of the different types of hydrogel strain sensors

| Classification | Hydrogel | Signal | GF or LoD | Stretchability (%) | Other | Ref. |
|------------------------------------|---|-------------|---|--------------------|---|------|
| Conductive polymer-incorporated | PEDOT:PSS-polyAAm array | Electric | GF = ~20 | ~15 | Long-term sensing (~2 months), detect subtle force of 0.02–4.49 N | 62 |
| | PANI-poly(AAm-co-HEMA) | Electric | GF = 11 | ~300 | Detect wrist bending, speaking; biocompatible | 39 |
| | PANI/PSS-UPyMA | Electric | GF = 3.4 | ~300 | Self-healing (<30 s); detect pulse beating, speaking, finger bending | 63 |
| | polyNIPAAm/PANI | Electric | GF = 3.92 | ~200 | Stable performance (~350 cycles) | 64 |
| Polyelectrolyte-incorporated | ACC-polyAAc/sodium alginate (SA) | Capacitance | LoD = ~1 kPa | ~55 | Self-healing; detect speaking, blood pressure, and finger bending | 65 |
| | Poly(MAA-co-DMAPS) | Electric | LoD = 0.6–0.7% °C ⁻¹ | >10 000 | Self-healing; Temperature-responsive sensor (10–80 °C) | 66 |
| Nanoparticles-incorporated | Chitosan-AuNPs | Color | LoD = 2.4 μM of H ₂ O ₂ | — | Wide detection range (8.0 μM–15 mM) | 67 |
| | PNIPAM-AuNPs | Color | LoD = 0.2 °C | >100 | Color-temperature sensor range (25–40 °C); detecting time (~1 s) | 68 |
| | Fe ₃ O ₄ -poly(AAc-co-AAm) | Magnetic | LoD = 0.1 pH unit | — | Repeatable, reversible detection; detecting time (<60 min) | 69 |
| | Platinum nanoparticles (PtNPs)-PANI array | Electric | LoD = ~0.2 mM of glucose | — | High selectivity; signal-to-noise ratio of ~3 | 70 |
| | PtNPs-PANI | Electric | LoD = ~0.7 μM of glucose | — | High selectivity; detecting time (<3 s) | 71 |
| | AgNWs-polyAAm | Electric | GF = 0.71 | >22 000 | Wide working condition (–20 to 80 °C); detect breathing, speaking, and finger bending | 72 |
| | Nano barium ferrite (BaFe ₁₂ O ₁₉)-polyAAc | Electric | — | >40 | High ionic conductivity (1.22 × 10 ⁻² S cm ⁻¹); good self-recoverability | 73 |
| Inorganic electrolyte-incorporated | PDA-CNTs-poly(AAc-AAm) | Electric | — | ~700 | Self-adhesive; wide working condition (–20 to 60 °C); detect arm bending and wrist pulse | 74 |
| | MXene (Ti ₃ AlC ₂)-polyvinyl alcohol (PVA) | Electric | GF = 25 | >3400 | Self-healing; self-adhesive; detect human speaking, writing, and smiling | 75 |
| | PC/rGO-PVA | Electric | GF = 14.14 | >5000 | Self-healing (~3 s), detect finger bending, smiling, speaking, and wrist pulse | 76 |
| | F-SWCNT-polyPDA-PVA | Electric | — | >100 | Self-healing; self-adhesive; detect bending and relaxing of walking, chewing, and pulse | 77 |
| | SWCNT/PVA | Electric | GF = 1.51 | >1000 | Self-healing; detect bending and relaxing of knee/finger (>1000 cycles) | 78 |
| | TA/sodium alginate (SA)-polyAAm | Electric | GF = 2.0 | >2100 | Self-healing; detect smiling, finger bending, and wrist pulse | 79 |
| | KCl-(κ-carrageenan)/polyAAm | Electric | GF = 0.63 | ~1000 | Self-healing; detect finger bending | 80 |
| | Cu ²⁺ -polyAAm | Electric | LoD = ~0.005% strain | >1500 | Detect finger bending, speaking, and wrist pulse | 81 |
| | NaCl-gelatin/PVA | Electric | GF = ~0.4 | ~715 | Lower working condition (–20 °C); detect finger and elbow bending, speaking | 82 |
| | LiCl-poly(acrylated thymine-AAm) | Electric | — | ~2000 | Self-healing; self-adhesive; detect breathing, speaking and finger bending | 83 |
| Biomolecule-incorporated | NaCl-polyAAm | Capacitance | — | >590 | Detect finger bending (>4000 cycles) and location of touch | 84 |
| | LiCl-polyAAm | Capacitance | — | >1000 | Detect location of touch (work as smart screen) | 85 |
| | NaCl-SA/polyAAm | Electric | GF = 2.0 | ~3120 | Detect speaking, finger bending, and wrist pulse | 86 |
| | NaCl/SDS-regenerated silk fibroin(RSF)/HPAAm | Electric | GF = 2.0 | >1900 | Detect finger bending and location of touch | 87 |
| | LiCl-polyAAm | Capacitance | GF = 4.0 | >500 | Adhesive; stable performance (over 1500 cycles) | 88 |
| | PIL-BF ₄ /PEDGA | Electric | — | >1400 | Wide working condition (–75 °C to 340 °C); detect finger bending (>10 000 fatigue cycles) | 89 |
| | PVA/RSF/borax | Electric | — | ~5000 | Track leg, knee bending and different gestures | 90 |
| | Poly(AAm-co-aptamer) | Color | LoD = 0.0128HAU of H5N1 | — | <30 min detection time | 91 |
| | DNA-based | Cell | — | — | Detect live circulating tumor cells | 92 |

Note: Gauge Factor (GF) and Limit of Detection (LoD).

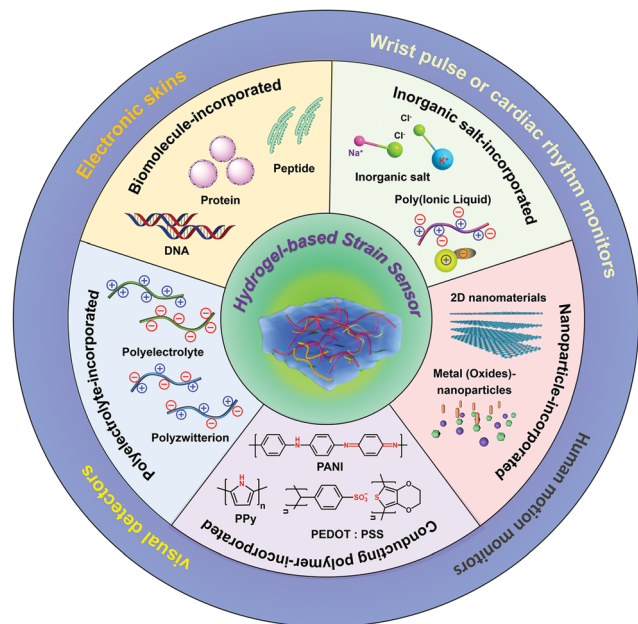


Fig. 1 Overview of the five typical types of hydrogel strain sensors.

inorganic salt-incorporated hydrogel, and biomolecule-incorporated hydrogel strain sensors, mainly depending on their structural-dependent network structures, gelation methods, and sensing mechanisms, not depending on the nature of the stimuli. Since these five types of hydrogel strain sensors possess anisotropic structures, a general working principle is to create non-uniform spatial stress in different regions/parts of the hydrogels to realize different stimuli-responsive sensing properties *via* strain-induced shape-adaptive actuations. On the other hand, while these five types of hydrogel strain sensors can achieve similar or the same stimuli-responsive sensing capacity (*i.e.* thermo, light, electric, and pH sensing capacity),⁹³ they are driven by different sensing mechanisms strongly depending on their network structures (Fig. 1). Inorganic nanofiller-incorporated hydrogel sensors are constructed by adding nanofillers or crosslinkers in polymer networks to create hybrid polymer/inorganic structures, where both materials contribute unique and beneficial properties to the hydrogel sensor, while the latter hydrogel sensors are likely constructed by different polymers to create an overall heterogeneous polymer/polymer structure. All these network structures allow the creation and maximizing the stress mismatch for strain-induced actuation upon external stimuli, and the sensing mechanics of these hydrogel sensors can further be tuned and optimized by changing the compositions in their hydrogel matrix, tailoring them for specific applications.

2.1. Nanoparticle-incorporated hydrogel sensors

Due to the unique and superior optical, conductive, and magnetic properties of nanoparticles (NPs), the physical incorporation or chemical crosslinking of nanoparticles into the polymer network enables the construction of hybrid inorganic NPs/polymer network structures, which help to translate the conformational change of the surface bound stimuli-responsive polymers into observable

optical property changes and improve their mechanical property, making them promising materials for desirable sensing applications.^{72,73,76,94} Several of the widely used one/two/three-dimensional NPs of gold nanoparticles (AuNPs), gold nanorods (AuNRs), silver nanoparticle (AgNPs), carbon nanotubes, graphene oxide, and MXenes, and magnetic nanoparticles (Fe_3O_4) have been incorporated into polyAAm, polyNIPAM, PVA, poly(NIPAM-*co*-AAm), and poly(AAc-*co*-AAm) to produce several representative strain sensors for pH, temperature, color and human movement.⁹⁵ As a typical example, AuNPs are often incorporated into a hydrogel matrix containing $-\text{SH}$, $-\text{CN}$ and $-\text{NH}_2$ groups *via* the formation of dynamic covalent bonds, which are responsive to different stimuli in different strain sensors. AuNPs were readily self-assembled on the amine-rich chitosan hydrogel matrix through horseradish peroxidase (HRP) immobilization, producing a AuNP-incorporated hydrogel biosensor,⁶⁷ which showed a wide range of response to H_2O_2 (8.0–15 μM), a low detection limit of 2.4 μM , and long-term sensing stability of up to 4 weeks. Moreover, AuNPs can also be modified by plasmonic nanostructures with different plasmonic materials, cluster structures, and geometries, and the modified AuNPs are used as real-time colorimetric indicators for hydrogel color sensors. As shown in Fig. 2a, combining plasmonic AuNPs with thermo-responsive polyNIPAM hydrogels, a smart colorimetric stretchable hydrogel biosensor was able to achieve rapid, reversible, and strain-insensitive color shifts between red and grayish violet in response to a temperature change from 25–40 $^\circ\text{C}$ within 1 s.⁶⁸ Besides the conventional AuNPs, AgNPs, and plasmonic nanoparticles, the incorporation of magnetic Fe_3O_4 nanoparticles into poly(AAc-*co*-AAm) hydrogels enabled the production of a pH sensor, which displayed a repeatable and reversible response to pH change, with a sufficient sensitivity to detect a 0.1 unit change in pH (Fig. 2b).⁶⁹

Carbon nanotubes (CNTs) and reduced graphene oxide (rGO) as typical two-dimensional carbon materials have been widely integrated and used as different electronic sensing devices made of elastomers, polymers, and organics due to their superior electronic properties of Fermi velocity, thermal conductivity, charge carrier mobility, and mechanical strength.^{96–99} However, the strong hydrophobicity and poor solubility of CNTs and rGO make it very challenging to directly incorporate them into highly hydrophilic hydrogels (70–90% water content) and to avoid their aggregation in the hydrogel matrix while still retaining their electronic sensing functions. To overcome this issue, a common strategy is to modify these hydrophobic carbon materials with hydrophilic/charge phenol hydroxyl, carboxylic acid, epoxide, and oxide groups to not only improve the dispersion of CNTs and strengthen their interfacial interactions with the polymer network, but also enhance their mechanical and electrical properties *via* electrostatic and π - π interactions, and hydrogen bonding. Consequently, different modified CNTs have been incorporated into polyAAm, polyAAc, polysaccharides, gelatin, collagen, and polyethylene glycol (PEG) hydrogels *via* hydrothermal and solvothermal reactions, cross-linking gelation, doping methods, and template-based synthesis. Among the different CNTs-incorporated hydrogel strain sensors, flexible and wearable strain sensors have

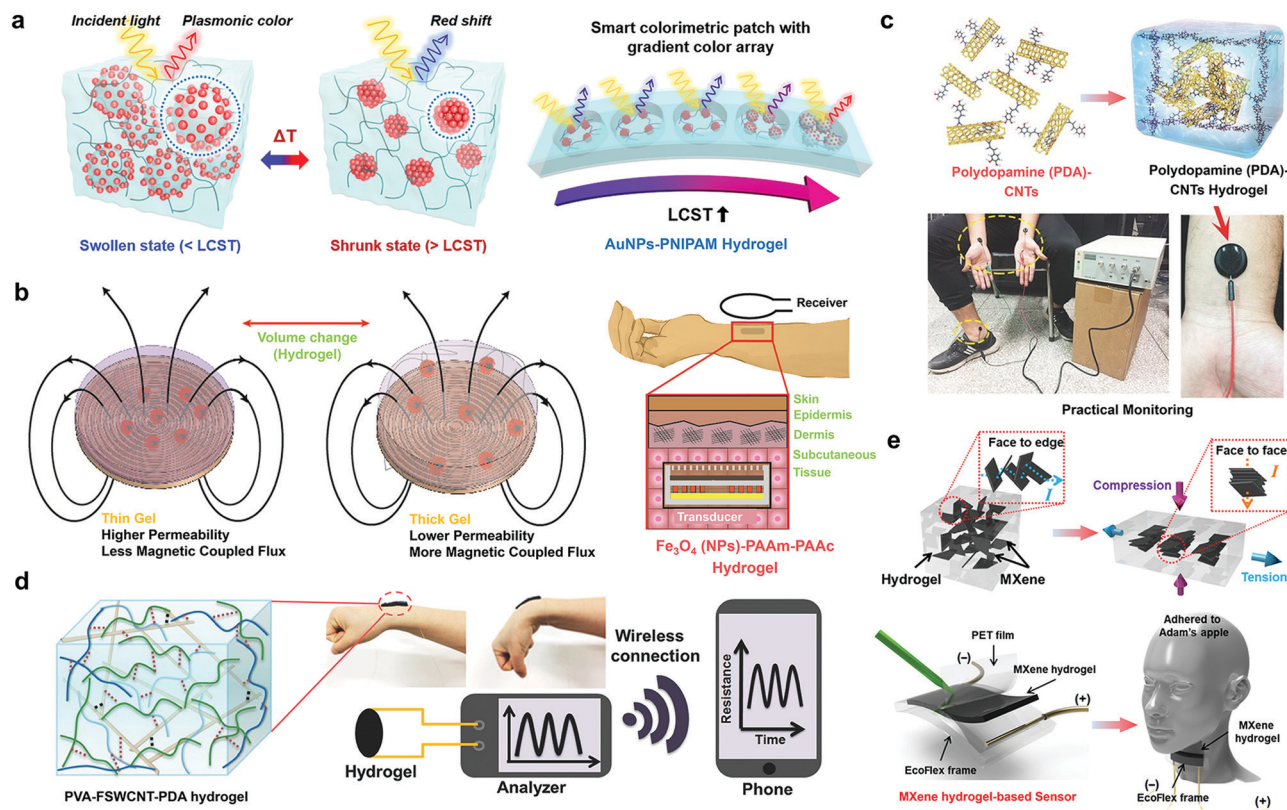


Fig. 2 Nanoparticle/polymer hydrogel sensors. (a) Thermo-responsive colorimetric plasmonic AuNPs-PNIPAM hydrogel sensors, exhibiting rapid and reversible color shifts from red to violet in response to a temperature change (25–40 °C) within 1 s. [Adapted with permission from ref. 68, Copyright 2018 Nature Publishing Group]. (b) Wireless iron oxide nanoparticle (Fe_3O_4NP)-embedded poly(AAc-co-AAm) hydrogel sensors that can detect subtle pH changes (0.1 unit) in response to a magnetic field. [Adapted with permission from ref. 69, Copyright 2014 Elsevier]. (c) Mussel-inspired PDA-CNTs-incorporated poly(AAm-AAc) hydrogels with highly adhesive, tough, and conductive properties for detecting human wrist pulse even at -20 °C. [Adapted with permission from ref. 74, Copyright 2018 Wiley-VCH]. (d) Automatable healable and adhesive PVA-FSWCNT-PDA hydrogel strain sensor for the real-time detection of human motions of finger bending and relaxing, walking, chewing, and pulse with fast self-healing ability (within 2 s) in response to external changes of stress or strain.⁷⁷ (e) MXene-PVA hydrogel sensors for monitoring electromechanical signal changes with a gauge factor of 25. [Adapted with permission from ref. 75, Copyright 2018 American Association for the Advancement of Science].

become immensely important for ultrasensitive human-machine interaction, healthcare monitoring, and human motions. As a classical example, conductive functionalized single-wall carbon nanotubes (FSWCNT), biocompatible polyvinyl alcohol (PVA), and polydopamine (PDA) were crosslinked to form a healable and adhesive PVA-FSWCNT-PDA hydrogel with dynamic supra-molecular structures, which exhibited fast self-healing ability (within 2 s), high self-healing efficiency (99%), and robust surface adhesion on different substrates (Fig. 2c). The PVA-FSWCNT-PDA hydrogel was further fabricated into a wearable soft strain sensor for the real-time detection of different human motions of finger bending and relaxing, walking, chewing, and pulse (Fig. 2d).⁷⁷ To expand this idea, single wall carbon nanotubes (SWCNT), GO, and silver nanowires (AgNWs) were separately incorporated into PVA hydrogels to produce different types of NP/PVA hydrogels as conductive strain sensors, all of which achieved fast and high self-healing efficiency (98%) of electric signals within ~ 3 s, sustained extreme elastic strain of 1000% with a gauge factor of 1.51, and effectively monitored and distinguished multifarious human motion of the finger, elbow, knee, and neck.⁷⁸

More impressively, MXene ($Ti_3C_2T_x$) as another 2D carbonitride/metal carbide was incorporated into the PVA hydrogel to obtain an MXene-based hydrogel strain sensor, which could detect various body motions (hand gestures and facial expressions) and monitor vital signals (human pulse and vocal sound) (Fig. 2e).⁷⁵ This high strain-induced electromechanical sensitivity is largely attributed to the 3D network structure of the MXene nanosheets embedded within the hydrogel matrix. Large deformation reduces the spacing between the nanosheets, but increases the surface contacts between the MXene nanosheets, and transforms the face-to-edge interconnections into face-to-face interconnections, all of which decrease the M-hydrogel resistance, and thus increase the detection sensitivity. It should be noted that besides the above-mentioned examples, most of nanoparticle/polymer hydrogel strain sensors can only be stretched to a strain of $\sim 200\%$, thus the breaking of the conducting contacts during deformation usually leads to a poor and irreversible detection sensitivity in these strain sensors. Thus, additional efforts should be made to increase the stretchability and self-healing properties of nanoparticle/polymer hydrogel strain sensors.

2.2. Conducting polymer-incorporated hydrogel strain sensors

Conducting polymers such as polypyrrole (PPy), polyaniline (PANI), and poly(3,4-ethylene-dioxythiophene) (PEDOT) are π -conjugated polymers with alternating single and double covalent bonds for conducting electrons.^{100–102} The use of conducting polymers to make hydrogel strain sensors possesses several intrinsic advantages as follows: (1) conductive polymers themselves are able to carry solvent ions for electrical conduction with fairly low resistance in the hydrogel networks. (2) In contrast to rigid NPs and metallic additives in polymer hydrogels to empower electronic conductivity, conductive polymer chains are very flexible and compatible with other polymers in the same hydrogel systems for empowering their high stretchability. Less structural disparity in network length scales can reduce the source of inhomogeneity in mechanical and electrical properties. (3) Obviously, conductive polymers can be simply fabricated with other elastomeric and polymer substrates into electronic sensors, and accordingly the conjugated polymers inside hydrogel networks possess high conductivity and thermal stability for piezoresistive strain sensors.^{64,103–105}

A general working mechanism for conducting hydrogel strain sensors is the delocalization of π -bonded electrons over the conjugated backbone structures. Thus, PANI, as firstly described in the mid-19th century by Henry Letheby, has been widely used for hydrogel bioelectronics.^{106,107} As an interesting example, a triplex biosensor made of nano-patterned PANI hydrogels and different enzymes was able to detect triglycerides, lactate, and glucose, with good selectivity and high sensitivity in both PBS and human serum samples.⁷⁰ The hydrophilic porous microstructure of the PANI hydrogel was favorable for the transportation of electrons generated from hydrogen peroxide in the enzymatic reactions. To enhance the electronic conductivity of hydrogel strain sensors, another common design strategy is to integrate conducting polymers with various ionic or organic dopants and nanoparticles. The incorporation of such dopants enables not only the creation of free radicals that can pair with the dopant to form polarons, but also oxidizes (p-doping) or reduces (n-doping) the conducting polymer at the π -bond sites by removing or donating electrons, both of which offer additional paths for charge carriers along the conducting polymer backbone.¹⁰⁸ Following this working principle, the incorporation of platinum nanoparticles (PtNPs) into the PANI hydrogel allowed the construction of a glucose sensor, with an ultrahigh low detection limit of 0.7 μ M glucose within 3 s (Fig. 3a).⁷¹ The significant increase in glucose detection ability of PtNPs/PANI hydrogel sensors is attributed to their enhanced electrocatalytic activity for oxidizing H_2O_2 . Similarly, polyAAm hydrogel doped with poly(3,4-ethylenedioxythiophene):polystyrene sulfonate (PEDOT:PSS) conductive polymers was used to create a classical piezoresistive tactile sensor (Fig. 3b).⁶² However, additional challenges still remain. Simple doping/mixing of additives into the conductive polymer network usually does not necessarily enhance mechanical strength, but instead make the hydrogels become more brittle due to the over-crosslinking effect.⁶³ To address this issue, the rational design of an interpenetrating

network (IPN) between conducting polymers and other polymers is a possible solution to minimize the potential trade-offs between mechanical and electrical properties *via in situ* polymerization or in-growth polymerization. Using this design strategy, several conducting hydrogels with IPN have been developed using polymerizing conducting polymers (*e.g.*, PEDOT:PSS and PANI) with other polymers (*e.g.* polyAAm, polyAAc, and gellan gum). All of these conductive IPN hydrogel sensors displayed enhanced mechanical properties compared to conductive hydrogel sensors without IPN, while still retaining high sensing ability (*e.g.* gauge factor = 11) (Fig. 3c).³⁹ Moreover, considering that the double-network (DN) structure is a special case of IPN, several recent attempts have fabricated two different polymers to form conductive hydrogels with a DN structure for imparting both high electronic conductivity and mechanical toughness, including PEDOT:PSS/PDMAAm DN hydrogels¹⁰⁹ and polyAAc/PEDOT:PSS DN hydrogel.¹¹⁰

2.3. Polyelectrolyte-incorporated hydrogel strain sensors

Polyelectrolytes (*e.g.* poly(2-acrylamido-2-methylpropane-1-sulfonic acid) [poly(AMPS)], polyAAc, and polyzwitterions) are among the most studied macro-ionic molecular systems. Considering the ionic nature of polyelectrolytes, polyelectrolyte hydrogels copolymerizing these electrolyte monomers into hydrogel networks possess intrinsic ionic groups and counterions, and thus they commonly undergo volume shrinking or swelling in response to pH and ionic changes.^{111–113} Compared to neutral polymer hydrogels, polyelectrolyte hydrogels usually exhibit “polyelectrolyte effect” behavior, *i.e.* the polyelectrolyte chains undergo fully stretching (swelling) conformation in water, but adopt a collapsed (shrinking) conformation in salt solution simply because the introduction of polyelectrolytes will screen the long-range electrostatic repulsions and short-range-excluded volume interactions between and within the polyelectrolyte chains, leading to ion/pH-responsive volume changes.^{114,115} Moreover, the strong binding of counterions to the polyelectrolyte chains creates additional cross-links in the hydrogel network, which influence the mechanical properties of polyelectrolyte hydrogels and even cause gel collapse in some cases. Moreover, the presence of charged groups allows the introduction of metal ion coordination and supramolecular interactions in the hydrogel networks, and thus to promote the hydroelectric separation and conductivity of the hydrogels.

Copolymerization of charged monomers [*e.g.* AMPS, AAC, 2-(methacryloyloxy)ethyl]dimethyl-(3-sulfopropyl) ammonium hydroxide (SBMA), 3-dimethyl (methacryloyloxyethyl) ammonium propanesulfonate (DMAPS) with neutral acrylamide monomers [*e.g.* AAm, NIPAM, HEMA]^{66,116–118} and the introduction of these charged monomers into the hydrogel network (*e.g.* PVA, P2VP, SA and polyAAm) to form IPN structures^{119–123} are two common strategies to construct polyelectrolyte hydrogel sensors. The copolymerization strategy can achieve poly(SBMA-*co*-HEMA) hydrogel sensor polyelectrolyte hydrogels with a high fracture elongation of 2000–10 000%, fracture strength of 0.2–0.6 MPa, and gauge factor of more than 1.5 (Fig. 4a). Another zwitterionic poly(MAA-*co*-DMAPS) hydrogel sensor with UCST and LCST characteristics displayed ultrastretchability of up to 10 000%,

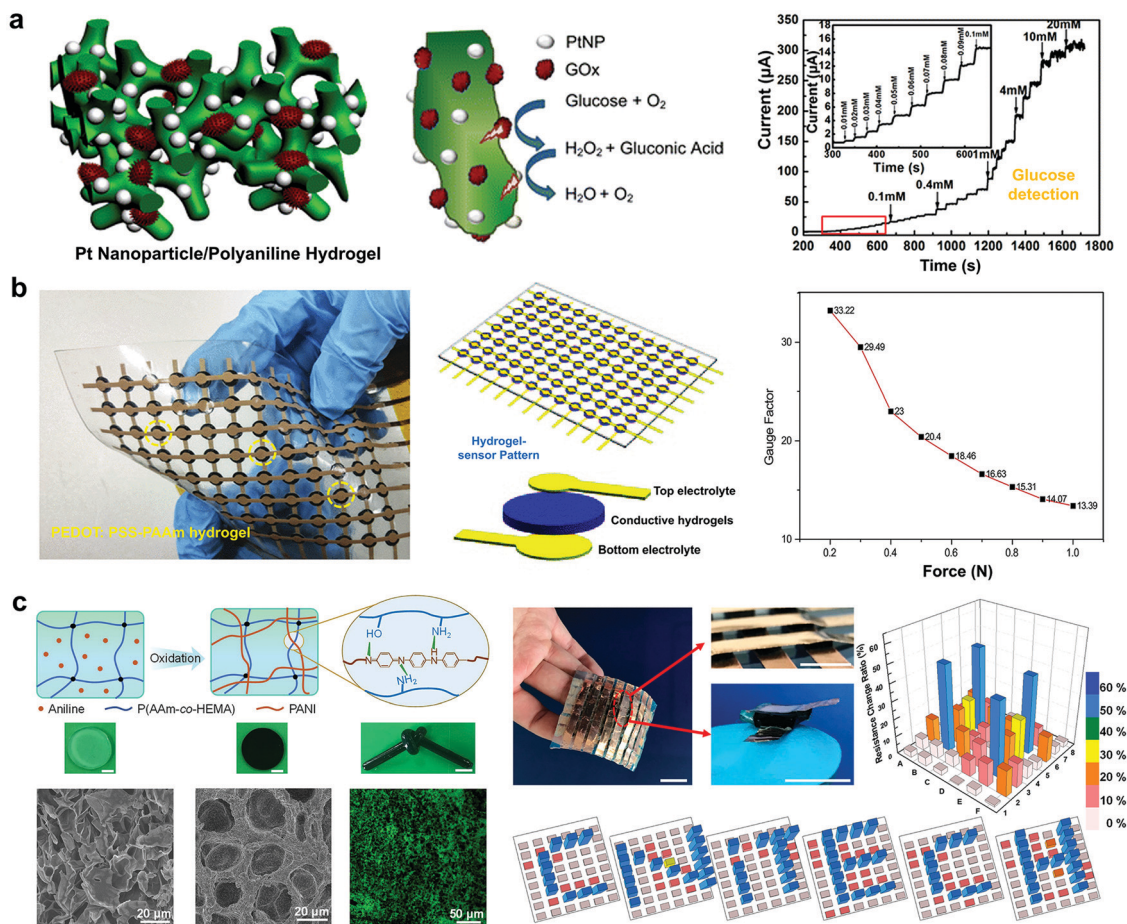


Fig. 3 Conductive polymer hydrogel strain sensors. (a) PtNPs/PANI hydrogels as a glucose sensor with high sensitivity of $96 \mu\text{A mM}^{-1} \text{cm}^{-2}$, low detection limit of $0.7 \mu\text{M}$, and fast response time of $\sim 3 \text{ s}$. Such unprecedented sensitivity is largely attributed to the synergistic integration of a PtNP catalyst into the 3D-microstructured PANI hydrogel matrix for promoting the electro-oxidation of hydrogen peroxide. [Adapted with permission from ref. 71, Copyright 2013 American Chemical Society]. (b) PolyAAM/PEDOT:PSS piezoresistive hydrogel sensors with a high gauge factor of 13–33 in response to a subtle force of 0.2–1.0 N. The blending of PEDOT:PSS in PAM hydrogels allows the output impedance ($k\Omega$) to be reduced to promote piezoresistive sensitivity. Adapted with permission from ref. 62, Copyright 2018 IEEE. (c) Conductive PANI-poly(AAm-co-HEMA) hydrogel sensors with high sensitivity ($\text{GF} = 11$) at low strain and outstanding linearity at high strain for detecting human motions of speaking, wrist pulse, and hand writing. [Adapted with permission from ref. 39, Copyright 2018 American Chemical Society].

which can converse forces to electrical signals for tracking human movements and perceiving changes in external temperature (Fig. 4b).⁶⁶ IPN structures can slightly enhance the tensile strength or sensitivity of hydrogel sensors by improving the integrity of the network structures. For instance, polyAAc/SA, polyAAc/PAAm, and polySBMA/PVA strain sensors exhibited 300–1000% stretchability, $\sim 0.6 \text{ MPa}$ tensile strength, and high detection capacity for multiple-time elbow/finger bending. Moreover, polyAAc/SA hydrogel sensors also exhibited high and sustainable sensitivity for detecting a wide range of pressure between 0.17–1000 kPa (Fig. 4c).⁶⁵

2.4. Inorganic salt-incorporated hydrogel strain sensors

Different from polyelectrolyte hydrogel strain sensors, electrolyte hydrogels are typically prepared *via* the direct physical or chemical doping of sodium chloride (NaCl), lithium chloride (LiCl), and cupric ions (Cu^{2+}) into polyAAM, HPAAM, and PVA hydrogels. Direct physical doping of NaCl, LiCl, and Cu^{2+} salts

into polyacrylamide (polyAAM) hydrogels provides a simple and straightforward route to form ion-doped electrolyte hydrogels.^{84,85} The resultant NaCl/polyAAM, LiCl/polyAAM, and Cu^{2+} /polyAAM hydrogel strain sensors are not only highly stretchable by up to 15-times of their original length and stable to sustain over 1000 pressure-capacitance cycles, but also detect any subtle human motion such as smiling, speaking, and finger bending. Moreover, these electrolyte hydrogels can also be fabricated into epidermal touch panels for use as human skin-machine interfaces for writing words, and playing games and a piano. (Fig. 5a). To enhance the mechanical properties, doping of different salts in the DN network structure produces different hydrogel strain sensors, including (i) κ -carrageenan/polyAAM DN hydrogel doped with KCl to achieve great strain sensitivity with a gauge factor of 0.63 at the strain of 1000%, elastic modulus of 280 kPa, and a fracture energy of 6150 J m^{-2} ;⁸⁰ (ii) PVA/gelatin doped with NaCl to achieve fracture stress of 1 MPa, fracture strain of 715%, elastic modulus of 157 kPa, and toughness of 3605 kJ m^{-3} ;⁸²

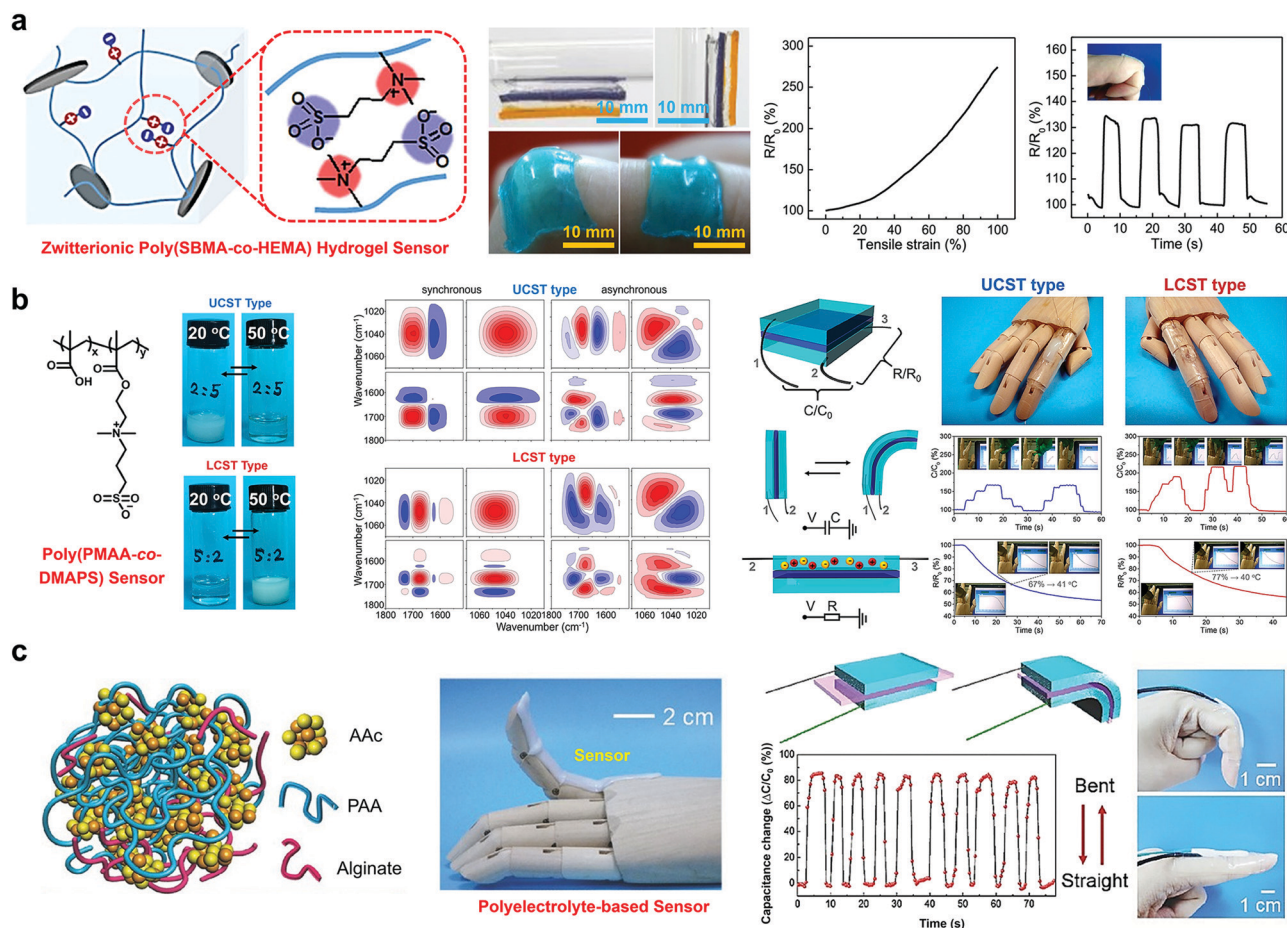


Fig. 4 Polyelectrolyte-incorporated hydrogel strain sensors. (a) Poly(SBMA-co-HEMA) hydrogel sensors with high strain conductivity and sensitivity (gauge factor = 1.8), high fracture toughness of 2.45 MJ m^{-3} , fracture strain of 2000%, fracture strength of 0.27 MPa, and compliant adhesion on different surfaces (hydrogels, skin, glass, silicone rubber, and nitrile rubber) [adapted with permission from ref. 116, Copyright 2019 American Chemical Society]. (b) Zwitterionic poly(MAA-co-DMAPS) hydrogel sensors to detect the movements of a wooden prosthetic finger and environmental temperature changes by tuning UCST and LCST for converting forces to electrical signals. [Adapted with permission from ref. 66, Copyright 2018 American Chemical Society]. (c) PolyAAc/SA hydrogels used as skin-mimic sensors for detecting subtle pressure changes as induced by a gentle finger touch, human motion, or small water droplets. [Adapted with permission from ref. 65, Copyright 2017 Wiley-VCH].

and (iii) SA/tannic acid (TA)/polyAAm hydrogel with ternary ionic multi-bond network with high sensitivity (GF of 2.0) (Fig. 5b).⁷⁹ All of these salt-doped hydrogels were fabricated into stretchable wearable strain sensors for the real-time monitoring of various human motions and physiological signals. However, although physical doping can achieve the regeneration of electrical conductivity by simple re-soaking methods, the strong dependence of salt concentration on ion-doped polyelectrolyte hydrogels will also affect the sensitivity and specificity of hydrogel sensors in real-world applications.

Different from direct physical doping, the chemical doping strategy helps to enhance the mechanical properties of hydrogels. Usually, the chemical doping strategy drives free salt ions to strongly bind to the polymer network *via* metallic ion coordination and supramolecular assembly. These interactions reduce the possibility of salting-out phenomena and blockage of the network channels of hydrogel sensors, both of which cause the failure of hydrogel sensors. Chemical doping of sodium dodecyl sulfate (SDS)/NaCl into the polyAAm or HPAAM

hydrogel network containing sodium alginate (SA) nanofibrils, regenerated silk fibroin (RSF), and cellulose derivatives improves the mechanical properties. NaCl/SA/polyAAm⁸⁶ and NaCl/SDS-RSF/HPAAm⁸⁷ hydrogel sensors (0.65–1.2 MPa) possessed 2–7 times higher tensile stress than pristine hydrogel sensors (0.1–0.2 MPa), with maximum stretchability of up to 1800–3100%. For the NaCl/SDS-RSF/HPAAm DN gel (Fig. 5c), SDS not only promoted the rapid formation of the first SDS-RSF network, but also formed SDS micelles to act as cross-linking points for a second HPAAM network. All of these tough electrolyte hydrogels can also be used as touchable or resistance-sensitive devices for sensing electronic signals.

Ionic liquids (ILs) are composed of cation–anion pairs of an organic ion and inorganic counterion. Different from inorganic salts, ILs are hydrophobic and difficult to add to hydrophilic hydrogels directly. Using click reaction and solvent exclusion methods, PIL-BF₄,⁸⁹ 1-butyl-3-methylimidazolium chloride (BMIMCl),¹²⁴ and [C16mim]⁺Cl⁻¹²⁵ were encased or cross-linked into PEDGA/PETA, xanthan gum, and bulk g-C₃N₄ hydrogels.

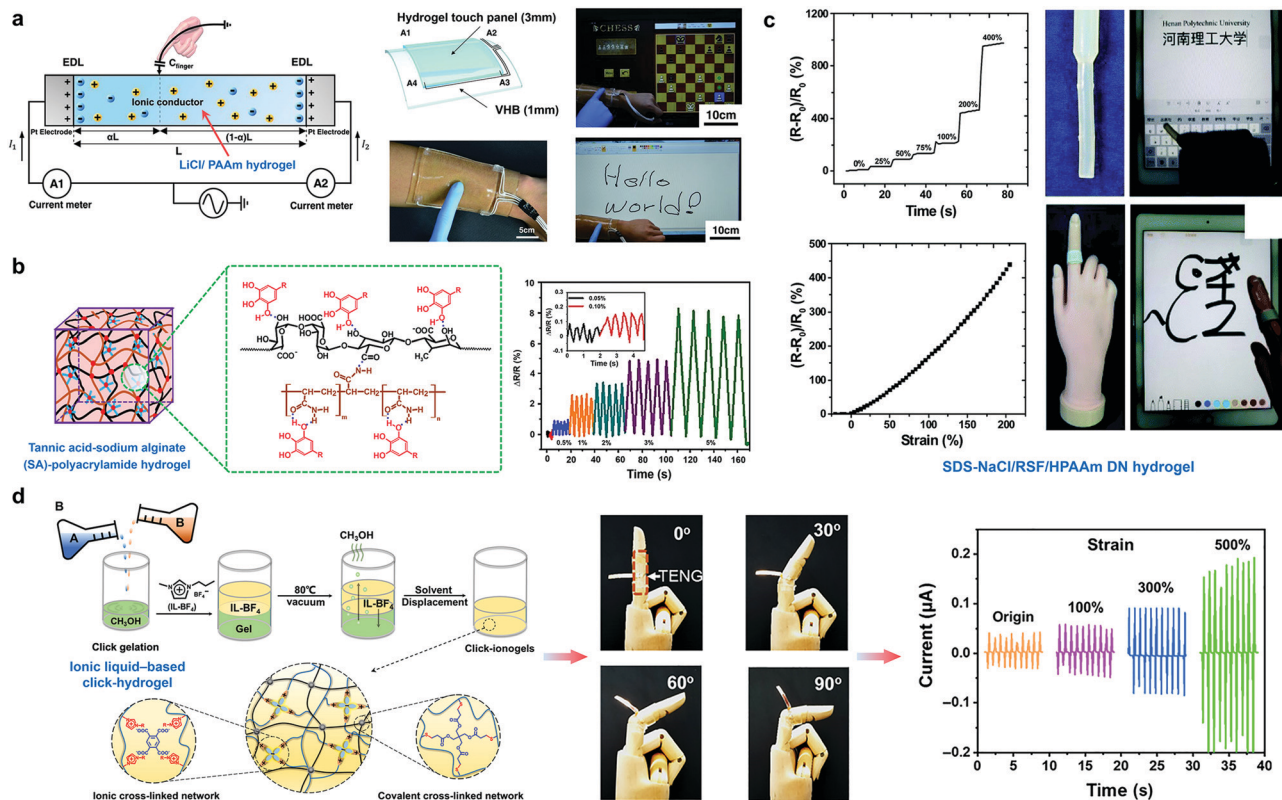


Fig. 5 Inorganic salt-incorporated hydrogel strain sensors. (a) LiCl–polyAAm hydrogel sensor with high stretchability and transmittance, which was further used as an ionic touch panel for writing words and playing games and a piano. [Adapted with permission from ref. 85, Copyright 2016 American Association for the Advancement of Science]. (b) SA/TA/polyAAm hydrogel sensor with a high gauge factor of 2–9 at a subtle (<100%) and large (2100%) strain for monitoring large limb motions of the human body (finger, knee, and elbow) and subtle muscle movements (smiling, chewing, and wrist pulse). Adapted with permission from ref. 79, Copyright 2019 American Chemical Society. (c) NaCl/SDS–RSF/HPAAm hydrogel sensor with high compression/tensile strength of 122/1.2 MPa, large extensibility of 19, high toughness of 1769 J m⁻², and high ionic conductivity of 0.012 S cm⁻¹. High ionic conductivity and strain sensitivity enable the RSF/HPAAm DN gel to be used as a touching screen pen and electronic skin. [Adapted with permission from ref. 87, Copyright 2019 Royal Society of Chemistry]. (d) Ionic liquid-based PIL–BF₄/PEDGA hydrogel strain sensor with high ionic conductivity (0.83 S m⁻¹ at room temperature) for detecting finger bending under a wide temperature range (–75 to 340 °C) over 10 000 fatigue cycles. [Adapted with permission from ref. 89, Copyright 2019 American Association for the Advancement of Science].

The resultant hydrogel sensors possessed high tensile strength of 1.5–2.2 MPa, stretchability of 1500% up to 10 000 fatigue cycles, and broad thermal responsive range of –75 to 340 °C. Due to the high ionic conductivity (0.83 S m⁻¹ at room temperature), hydrogel sensors can retain their high and stable electric sensitivity even at extremely low (–60 °C) and high (200 °C) temperatures (Fig. 5d). Furthermore, ILs are promising for preparing anti-freezing organogel and hydrogel sensors, which require further research efforts.

2.5. Biomolecule-incorporated hydrogel strain sensors

Hydrogels integrated with biomolecules (*e.g.* proteins, peptides, antibody, DNAs, and enzymes) present many general bio-related advantages of biodegradability, biocompatibility, and biostability, and specific bio-functionalities of drug/gene carriers, bioactivity, and bioimaging.^{126–128} From a fabrication viewpoint, biomolecule-based hydrogels are often fabricated *via* a variety of methods, including click chemistry, Michael addition of cysteine residues to vinyl sulfones or maleimides, UV-initiated cross-linking, native chemical ligation, nonspecific amine-carboxylic acid couplings,

and self-assembly.^{129–131} Functionally, biomolecule-based hydrogels achieve their specific functions *via* simple sequence design, but stimuli-responsive sensing properties from the coupling of functional biomolecules with the physical properties of polymers. The incorporation of biomolecules into synthetic polymer networks can also influence the swelling, structure, and mechanical properties of hydrogels. Practically, most biomolecule-based hydrogels are dominantly used for tissue engineering and extra-cellular matrix (ECM) mimics, but stimuli-responsive biomolecule-based hydrogels have attracted increasing interests for next-generation bioelectronic interfaces over the last decade due to their similarities to biological tissues and versatility in electrical, mechanical, and biofunctional engineering.

For protein/polymer hydrogels formed by native proteins (*e.g.* collagen, gelatin, silk fibroin, bovine serum albumin, β-lactoglobulin, YajC-CT, and ovalbumin) and synthetic polymers, they achieve stimuli-responsive properties mainly through conformational changes between native and denaturation states upon external simulation.¹³² For example, a series of PEG/protein hydrogels were synthesized with different proteins of soy protein,

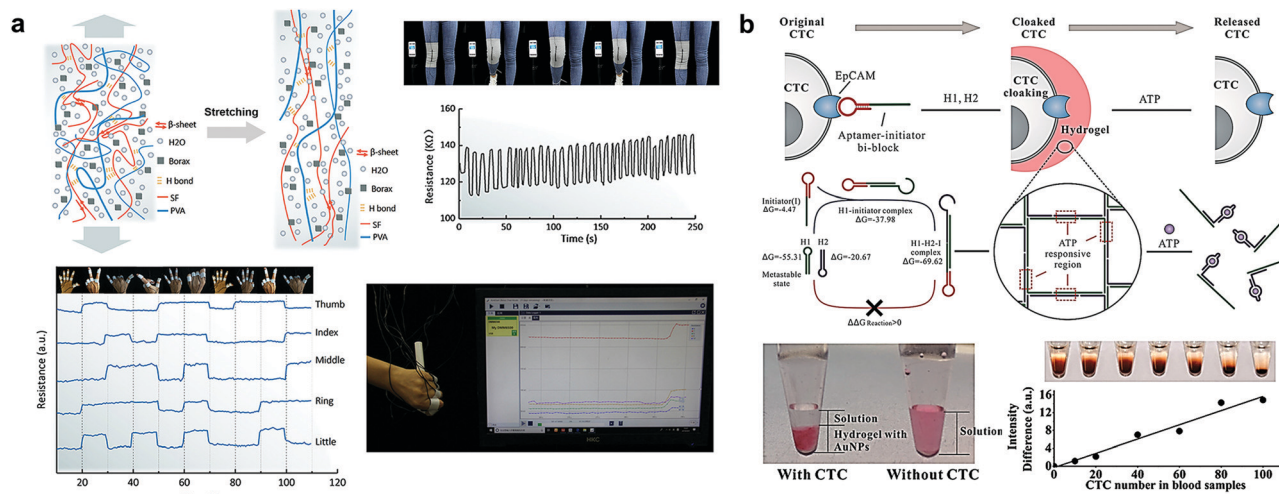


Fig. 6 Biomolecule-incorporated hydrogel strain sensors. (a) Protein-based PVA/RSF/borax hydrogel sensor with high stretchability, self-healing, and adhesion properties, which was integrated and used as a physical sensing platform for human motion detection [adapted with permission from ref. 90, Copyright 2019 American Chemical Society]. (b) ATP-aptamer-responsive DNA hydrogel sensor for capturing and releasing of circulating tumor cells with high cell viability. [Adapted with permission from ref. 92, Copyright 2019 American Chemical Society].

hydrolyzed soy protein, pea albumin, and casein.^{133–135} Due to the polyelectrolyte nature of proteins, the resultant PEG/protein hydrogels exhibited pH responsiveness for drug release, but their mechanical properties were weak. Besides PEG, other polymers including PVA, poly(propylene oxide) (PPO), polyAAc, and poly-HEMA have been used with RSF to produce polymer/RSF hybrid hydrogels, which can be regulated by heating, variation of pH,¹³⁶ alcohol, ions,⁹⁰ and shearing. RSF usually adopts β -sheet structures and favors the aggregation of these β -sheets into crystalline fibrous structures in polymer networks, and these hierarchical structures are the main contributors to the excellent mechanical properties of polymer/RSF hybrid hydrogels. Some PVA/RSF/borax hydrogels can also be used as a physical sensor to detect the bending and release of the leg, hand, and finger (Fig. 6a). However, the low stability and easy denaturation of proteins make protein/polymer hydrogels vulnerable in their sensing, mechanical, and biological properties. As an alternative, small peptides can mimic the main function of natural proteins, be facilely synthesized and precisely modified by simply controlling their sequences at large-scale and low-cost level *via* gene expression in bacteria, recombinant technology, and solid-phase peptide synthesis, and be easily incorporated with polymers *via* click chemistry. One design strategy to introduce stimuli-responsive properties for these peptides is to control their conformational changes *via* sol-to-gel transition by various environmental stimuli. For instance, an FEFEFKFK/polyNIPAAm and POG8/PEG hydrogel exhibited thermo-responsive properties, which could be tuned by the self-assembly of FEFEFKFK into β -sheet-rich fibers and POG8 into triple-helix fibers.^{137,138}

Compared to proteins and peptides, DNA possesses enhanced stability under intensive heating, pressure, and chemical processing. DNA-functionalized hydrogels are still a relatively new field. The most important property of DNA hydrogels is that nucleobases including adenine (A), thymine (T), guanine (G), cytosine (C), and uracil (U) serve as programmable microscopic motifs or crosslinkers

for constructing predictable secondary structural networks from the bottom up *via* base-pairing hybridization.¹³⁹ The hybridization of complementary DNA strands leads to the crosslinking of polymer chains and hydrogel formation with precise structural control and specific responses. DNA generally behaves like a long linear polymer and forms a hydrogel *via* physical entanglement or by chemical crosslinking of other polymers, composites, and small molecules. When nucleobases were independently introduced into polyacrylamide, DNA-polyAAm hydrogels exhibited a greatly enhanced elastic modulus of 0.43 MPa by several orders of magnitude,¹⁴⁰ and surface adhesion ($220\text{--}780\text{ N m}^{-1}$) on various solid materials, including polytetrafluoroethylene, plastics, glass, rubbers, metals, and wood.¹⁴¹ This mechanical enhancement in DNA (linear)-polyacrylamide hydrogels is largely attributed to their DNA-self-assembled supramolecular structures. Besides linear DNAs, DNA can also be precisely designed and self-assembled into different branched architectures of X, Y, T, and cross-shapes, which were further self-assembled into large-scale, three-dimensional hydrogel structures *via* efficient, ligase-mediated reactions, but these branched DNA hydrogels were very weak with a tensile modulus in the range of 1–50 kPa and tensile strain of 0.42–0.57.¹³⁹

Different from pure DNA hydrogels, due to the negatively charged nature of DNA, DNA is also used to form responsive complexes through physical interactions with cationic polyelectrolytes, nanocomposites and chemical grafting onto synthetic polymers.^{142,143} Physical DNA-polymer and DNA-composite hydrogels undergo reversible and switchable changes in their morphology, color, and size in response to external stimuli, and thus are often used as smart sensors and devices to monitor binding events. However, physical DNA-polymer hybrid hydrogels usually suffer from weak mechanical strength and poor sensitivity, presumably due to the lack of precise control to form ordered structures. Instead of using physical interactions,

DNA can be covalently grafted onto or crosslinked with polymers and proteins to construct programmable structures in hydrogel networks. For example, co-assembly with an octapeptide and DNA allowed the fabrication of DNA-inspired hydrogel sensors, which could selectively hybridize DNA and generate fluorescence, with a detection limit of 22 pM. DNA-poly(phenylenevinylene) hybrid hydrogels (DNA/SP-PPV) have been developed for monitoring drug release driven by the pH of the medium.¹⁴⁴ An ATP-responsive DNA hydrogel could achieve the controllable capture and release of cells by incorporating an ATP aptamer in the clamped HCR (aptamer-triggered clamped HCR, atHCR) (Fig. 6b).⁹² Overall, the unique properties of DNA-based hydrogels are particularly useful for biomolecule detection under biologically-relevant conditions, minimizing unwanted probe-probe interactions, and have the potential to hugely increase the analyte storage capacity of devices. In addition, unlike traditional reversible crosslinks such as DHEBA, DNA-crosslinks do not require the addition of an initiator-catalyst system to re-establish dissociated crosslinks.

3. Applications of hydrogel-based sensors

3.1. Hydrogel strain sensors as electronic skins

Human skin as a naturally evolved product combines multiple sensations and excellent mechanical properties, which offers a perfect example for developing biomimetic devices with stimuli-responsive properties for human-machine interactions. "Hydrogel electronic skins" are considered artificially intelligent skins, which marry the mutual advantages of hydrogels (*e.g.* high-water content, soft, biocompatibility, and high stretchability/toughness) and electronic devices (*e.g.* high electrical conductivity and stimuli-responsiveness).^{15,145,146} A transparent LiCl-polyAAM hydrogel sensor was designed as an electronic skin, which could sense a 0–1 kPa pressure change and subtle human movements up to more than 1000 times.⁸⁴ Following a similar design strategy, bioinspired mineral ACC/polyAAc/alginate hydrogel electronic skins were developed to sense gentle human motion (*e.g.* finger touch, speaking and laughing) with very high pressure sensitivity of up to 1 kPa.⁶⁵ Zwitterionic poly(MMA-co-DMAPS) hydrogel strain sensors by integrating a parallel-plate capacitor with an ionic resistor enabled the mechanoreceptor (detection for 10 000 strain change) and thermo-receptor in human skin to be mimicked (10–80 °C) due to temperature-sensitive transition between LCST and UCST.⁶⁶ However, challenges still remain, where most of hydrogel-based electronic skins still possess relatively unitary functions. Accordingly, more precise and multifunctional electronic skins, LiCl-PVA hydrogel strain sensors (>2000% of biaxial strain), combined with a flexible unit bearing power supply, control, readout and communication units, stretchable transducer batch, and printed circuit board was successfully constructed as an intelligence electronic skin.¹⁴⁷ This LiCl-PVA hydrogel electronic skin could real-time monitor and control the human body temperature, collect some health information (*e.g.* blood pressure and heart beat), and trigger drug release for

treatment whenever abnormal physiological signals were received. This electronic skin outperforms most of the current hydrogel electronic skins, which is worthy of further exploration for potential bioelectronic applications.

3.2. Hydrogel strain sensors as wrist pulse or cardiac rhythm monitors

Artery pulse in (pre)clinical practice is a significant indicator of arterial blood pressure, cardiac rhythm, and aged blood vessel, which often provides useful information for the real-time, non-invasive diagnosis of possible cardiovascular diseases.^{148,149} Due to the highly flexible and soft matrix of hydrogel strain sensors, hydrogel sensors enable closely fitting the curvature and surface of human skin with blood vessels underneath it to precisely detect three symbolic pulse waves as induced by wrist pulse, blood-pressure, and cardiac rhythm: percussion wave (P or P₁ wave), tidal wave (T or P₂ wave), and diastolic wave (D or P₃ wave), where the P₁/P₂ waves are the early/late systolic peak pressure and the P₃ wave is the diastolic pulse waveform.^{150,151} More interestingly, the P₁-wave/P₂-wave (radial artery augmentation index) and time delay between these two-wave peaks largely reflect the arterial stiffness level, which is highly related to the health condition of humans.¹⁵² For instance, several hydrogel-based wrist pulse/blood-pressure sensors made of PANI-poly(AAm-co-HEMA),³⁹ F-polyNIPAM/PANI,⁶⁴ AgNWs-polyAAM-PVP,⁷² SA/TA/polyAAM,⁷⁹ Cu²⁺/polyAAM,⁸¹ LiCl-PVA,⁸⁵ NaCl-SA/polyAAM,⁸⁶ PANI/PSS,⁶³ polySBMA/PVA,¹²³ Ca²⁺-SA-polyAAc,¹⁵³ agar/NaCl/polyAAM,¹⁵⁴ chitosan-PPy-polyAAc,¹⁵⁵ and SA-CNC/polyAAc¹⁵⁶ possessed high sensitivity with a gauge factor of 0.5–3, allowing the tracking of irregular pulses, waves, and intervals within 0.1 s. However, the shape, frequency, and amplitude of the pulse signals collected by these hydrogel sensors were still rough, and in some cases, they cannot accurately distinguish percussion (P₁), diastolic (P₂) and tidal (P₃) waves, limiting their further practical applications.

To overcome this detection sensitivity issue, the incorporation of nanoparticles into hydrogels, *i.e.* PDA-CNTs-poly(AAm-AAc),⁷⁴ MXene-PVA,⁷⁵ FSWCNT-PDA-PVA,⁷⁷ PDA-PPy-polyAAM,¹⁰⁵ CNTs-Egg white,¹⁵⁷ and SWCNT/polyAAM,¹⁵⁸ allows the gauge factor to be increased to 3–80 to distinguish different pulse waves under 10 kPa. Meanwhile, these wrist pulse/blood-pressure hydrogel sensors enable the transmission of wireless signals to smart phones. Besides hydrogel detection sensitivity (gauge factor), the specific contact area between hydrogel sensors and the human body is also important for wrist pulse or blood-pressure. A wireless pressure-sensing device incorporating Ca²⁺-SA¹⁵⁹ hydrogel microspheres could continuously detect and distinguish characteristic pulse waves from human skin (~25 Pa), consistent with the clinically used wrist pulse detectors. On the other hand, hydrogel strain sensors are still inferior to metal/organic-based (*e.g.* ZnO-, Pt-, CNT-, and Au nanowires-based) pulse sensors in terms of both detection sensitivity and specificity, presumably due to the irreversible fatigue and damage of the network structure in hydrogels. Thus, some reversible bonds or self-healable materials should be introduced in these hydrogel sensors.

3.3. Hydrogel strain sensors as visual sensors

Stimuli-responsive hydrogels (*e.g.* thermal-responsive, glucose-responsive, pH-responsive, and cocaine-responsive hydrogels) possess the general ability to induce volume/size changes (*i.e.* shrinking and swelling) upon external stimuli. Particularly, when incorporating photonic crystals (PCs) or nanoparticles (PNs) into a hydrogel network, it would alter the periodicity layout of PCs and PNs to trigger a transformation of bio-/physical-signals into colorimetric signals, eventually achieving optical changes.¹⁶⁰ Colorful poly(St-MMA-AAm) hydrogel sensor-embedded PCs were successfully designed to realize reversible color changes from transparent to violet, blue, cyan, green and red in response to different humidity conditions, and the color change almost covered the whole visible range.¹⁶¹ Such real-time, optical visual change was determined by expanding or contracting the crosslinked networks upon an increase or decrease of external humidity. Similarly, when incorporating PCs into the Si structure, poly(HEMA-*co*-MMA)-PCs hydrogel sensors could achieve color changes in response to temperature (25–50 °C) due to swelling/shrinking-induced viscoelastic deformation. A hybrid protein kinase A (PKA)/PCs hydrogel sensor enabled color changes for the label-free detection of kinase (PKA), as evidenced by a red shift, with the lowest detection limit of 2 U μL^{-1} for 2 h.¹⁶² Moreover, modified AuNPs with plasmonic nanostructures can also be incorporated into hydrogel sensors as real-time colorimetric visual detectors. A smart colorimetric stretchable plasmonic AuNPs-polyNIPAM hydrogel biosensor was able to achieve rapid, reversible, color changes between red and grayish violet in response to a temperature change from 25–40 °C within 1 s.⁶⁸ In general, PC/AuNP-incorporated hydrogel sensors hold great promise for wearable healthcare due to their visual signals by the naked eyes, without the need for any additional detection instruments. However, when applying these visual sensors to wearable healthcare devices, epidermal contortion and human activity often inevitably cause irreversible damage to the hydrogel networks and structures, which in turn compromise the performance of these hydrogel sensors. To overcome this issue, we propose the introduction of some pattern structures to minimize the stretching of PCs to protect their colorimetric response.

3.4. Hydrogel strain sensors as human motions

Like other strain sensors, hydrogel strain sensors enable different human motion activities to be captured or distinguished. Current commercial and representative organic/inorganic-based strain sensors made of a combination of CNT, GO, and other conductive materials with elastomeric substrates usually have limited stretchability of up to 200%, while hydrogel strain sensors tend to adopt more complex and considerable deformation detection due to their higher stretchability (300–10000%).^{163,164} Multi-scale strains of human motions include large-scale motions (*e.g.*, bending and twisting of hands, arms, and legs with minimal strain of >200%) and small-scale motions (*e.g.*, subtle movements of face, chest, and neck during emotional expression, breathing, and speaking with a minor strain of <50%). Both single-network hydrogel strain sensors (*e.g.* Cu²⁺-polyAAm⁸¹ and MXene-PVA⁷⁵) and double-network

hydrogel sensors (*e.g.* KCl- κ -carrageenan/polyAAm,⁸⁰ NaCl-SA/polyAAm,⁸⁶ NaCl/SDS-RSF/HPAAm,⁸⁷ and SA/TA/polyAAm⁷⁹) were able to detect these human motions. However, it is generally difficult for hydrogel networks to recover to their initial state immediately after undergoing large deformation, and thus re-calibration of signal baseline of many hydrogel sensors after several-round tests is required. Therefore, ultra-stretchable hydrogel sensors with good mechanical self-recovery are expected to improve the substantial detection ability for human motion. For instance, upon the incorporation of PVP-capped AgNWs into the polyAAm hydrogel, the resultant hydrogel sensor exhibited extremely high stretchability (>22000%), autonomous self-healing, mechanical compliance, and an ultrawide linear response range from a gauge factor of 0.15 at 0–430% tensile strain to 0.71 at 430–18100% tensile strain.⁷² Another typical MXene-PVA hydrogel sensor with 3400% stretchability and good self-recovery was designed to track facial expressions, hand gestures, finger bending, hand writing, and vocal motions. Due to its soft and sticky characteristics, the MXene-PVA sensor could readily adhere onto various positions of the human skin for stable and repeatable detection.⁷⁵ This sensor with great self-recovery can real-time and *in situ* track large body deformations, spatial gesture movements, and physiological signals for motion behaviors, and provide health evaluation without any calibration because the quick recovery of its cross-linked network will maintain the relatively stable signal baseline.

4. Conclusion and perspectives

This review provided an update on the current status and developments on hydrogel strain sensors, including their design strategies, preparation methods, functional properties, mechanical sensing mechanisms, and practical applications. However, despite the great advancements, functional hydrogel strain sensors with excellent electrical, magnetic, optical, and biocompatibility properties are still in their infancy. Current research still mainly focuses on the exploration of new stimuli-responsive hydrogel systems, but some fundamental issues need to be addressed.

Conventional hydrogels used for strain sensors usually possess limited mechanical strength and are prone to permanent breakage. This intrinsic mechanical weakness often renders hydrogel sensors vulnerable to damage under continuous and responsive actions, resulting in unstable sensitivity and specificity. Also, the lack of dynamic cues and mechanical strength within the hydrogels limit their sensing ability. To remedy this issue, on one hand, introducing self-healing properties to hydrogel sensors will repair structural damage, increase reusability and stability, and restore sensing ability to some extent. On the other hand, the use of tough hydrogels (*e.g.* double-network hydrogels and nanocomposite hydrogels) as a structural platform to integrate different sensing components is considered as alternative design strategy to enhance the sensing capacity of hydrogel sensors. However, it still remains a great challenge to design and construct self-healing hydrogel sensors, which combine several properties of

rapid autonomous self-healing ability, high-mechanical healing efficiency, and easily distinguishable response signals. Also, retaining the long-time self-healing of hydrogel sensors is another critical concern particularly under harsh conditions (e.g. underwater, freezing temperature, and salt/acidic solution). When applying hydrogel strain sensors to wearable devices, besides ultra-stretchability and high mechanical strength, additional robust adhesion to various solid surfaces (e.g. metal, glass, ceramic, and wood) and soft materials (e.g. rubber, skin, tissue, and organs) is required to maintain high strain sensitivity and stability to detect large human motions and tiny physiological signals. Another research direction is to apply hydrogel sensors for bio-applications, and in this regard, hydrogels themselves must be also nontoxic and biocompatible for hydrogel-based skin sensors, blood-pressure sensors, and implanted/injectable sensors. From an experimental viewpoint, it is always unstoppable motivation for material researchers to explore cutting-edge chemistries and fabrication technologies for designing and synthesizing novel hydrogels with desired properties towards specific sensing applications. In addition, beyond hydrogels, it is also interesting to develop and study organic gels prepared in or containing non-water solvents of varying polarity to understand the solvent effect on different aspects of organic gels, to reveal the differences and similarities in the gelation process, mechanical properties, toughening mechanisms, and network structures between hydrogels and organic gels, and to expand completely different gel systems for different applications.

In parallel, future efforts should be made to use computational modeling and machine learning technologies, together with polymer chemistry, synthesis, and gelation, to better understand the component-structure-performance relationship of hydrogel materials and to improve the structural-based design of hydrogel sensors and their interactions with target components and exogenous stimuli. Multi-scale simulations should study the deformation and recovery of hydrogels at the atomic, molecular, and macroscopic levels to clarify these issues since very little work has been done on this front.

Conflicts of interest

There are no conflicts to declare.

Acknowledgements

This review is particularly to thank all current and former collaborators who have been working on different aspects of smart hydrogel materials over years at the Zheng lab. We also thank Louisa Wang from Hathaway Brown School who has started to work in our lab. We also thank financial supports from NSF (1806138 and 1825122).

References

- J. L. Drury and D. J. Mooney, Hydrogels for tissue engineering: scaffold design variables and applications, *Biomaterials*, 2003, **24**(24), 4337–4351.
- P. X. Ma, Scaffolds for tissue fabrication, *Mater. Today*, 2004, **7**(5), 30–40.
- S. Sayyar, E. Murray, B. C. Thompson, J. Chung, D. L. Officer, S. Gambhir, G. M. Spinks and G. G. Wallace, Processable conducting graphene/chitosan hydrogels for tissue engineering, *J. Mater. Chem. B*, 2015, **3**(3), 481–490.
- B. A. Matthew, C. Jeannine, P. P. Benjamin, E. M. Jodie, P. M. Jessica, M. Benedetto, L. K. David and F. G. Omenetto, Laser-based three-dimensional multiscale micropatterning of biocompatible hydrogels for customized tissue engineering scaffolds, *Proc. Natl. Acad. Sci. U. S. A.*, 2015, **112**(39), 12052–12057.
- Y.-M. Kim, C.-H. Kim and S.-C. Song, Injectable Ternary Nanocomplex Hydrogel for Long-Term Chemical Drug/Gene Dual Delivery, *ACS Macro Lett.*, 2016, **5**(3), 297–300.
- V. Arti, V. Atul, Y. K. Guptac and S. Ahmad, Recent advances in hydrogel based drug delivery systems for the human body, *J. Mater. Chem. B*, 2014, **2**(2), 147–166.
- Q. Feng, J. Xu, K. Zhang, H. Yao, N. Zheng, L. Zheng, J. Wang, K. Wei, X. Xiao, L. Qin and L. Bian, Dynamic and Cell-Infiltratable Hydrogels as Injectable Carrier of Therapeutic Cells and Drugs for Treating Challenging Bone Defects, *ACS Cent. Sci.*, 2019, **5**(3), 440–450.
- H. He, Z. Xiao, Y. Zhou, A. Chen, X. Xuan, Y. Li, X. Guo, J. Zheng, J. Xiao and J. Wu, Zwitterionic poly(sulfobetaine methacrylate) hydrogels with optimal mechanical properties for improving wound healing in vivo, *J. Mater. Chem. B*, 2019, **7**(10), 1697–1707.
- M. di Luca, M. Curcio, E. Valli, G. Cirillo, F. Voli, M. E. Butini, A. Farfalla, E. Pantuso, A. Leggio, F. P. Nicoletta, A. Tavanti, F. Iemma and O. Vittorio, Combining antioxidant hydrogels with self-assembled microparticles for multifunctional wound dressings, *J. Mater. Chem. B*, 2019, **7**(27), 4361–4370.
- S. Li, S. Dong, W. Xu, S. Tu, L. Yan, C. Zhao, J. Ding and X. Chen, Antibacterial Hydrogels, *Adv. Sci.*, 2018, **5**(5), 1700527.
- L. Han, L. Yan, K. Wang, L. Fang, H. Zhang, Y. Tang, Y. Ding, L.-T. Weng, J. Xu, J. Weng, Y. Liu, F. Ren and X. Lu, Tough, self-healable and tissue-adhesive hydrogel with tunable multifunctionality, *NPG Asia Mater.*, 2017, **9**(4), e372.
- T. B. H. Schroeder, A. Guha, A. Lamoureux, G. VanRenterghem, D. Sept, M. Shtein, J. Yang and M. Mayer, An electric-eel-inspired soft power source from stacked hydrogels, *Nature*, 2017, **552**(7684), 214–218.
- J. Kim, M. Kim, M. S. Lee, K. Kim, S. Ji, Y. T. Kim, J. Park, K. Na, K. H. Bae, H. Kyun Kim, F. Bien, C. Young Lee and J. U. Park, Wearable smart sensor systems integrated on soft contact lenses for wireless ocular diagnostics, *Nat. Commun.*, 2017, **8**, 14997.
- J. F. Huang, J. Zhong, G. P. Chen, Z. T. Lin, Y. Deng, Y. L. Liu, P. Y. Cao, B. Wang, Y. Wei, T. Wu, J. Yuan and G. B. Jiang, A Hydrogel-Based Hybrid Theranostic Contact Lens for Fungal Keratitis, *ACS Nano*, 2016, **10**(7), 6464–6473.
- C. Yang and Z. Suo, Hydrogel iontronics, *Nat. Rev. Mater.*, 2018, **3**(6), 125–142.
- H. Li, T. Lv, H. Sun, G. Qian, N. Li, Y. Yao and T. Chen, Ultrastretchable and superior healable supercapacitors based on a double cross-linked hydrogel electrolyte, *Nat. Commun.*, 2019, **10**(1), 536.

- 17 S. Imani, A. J. Bandodkar, A. M. Mohan, R. Kumar, S. Yu, J. Wang and P. P. Mercier, A wearable chemical-electro-physiological hybrid biosensing system for real-time health and fitness monitoring, *Nat. Commun.*, 2016, 7, 11650.
- 18 Y. Cao, Y. J. Tan, S. Li, W. W. Lee, H. Guo, Y. Cai, C. Wang and B. C. K. Tee, Self-healing electronic skins for aquatic environments, *Nat. Electron.*, 2019, 2(2), 75–82.
- 19 Y. Yu, H. Yuk, G. A. Parada, Y. Wu, X. Liu, C. S. Nabzdyk, K. Youcef-Toumi, J. Zang and X. Zhao, Multifunctional “Hydrogel Skins” on Diverse Polymers with Arbitrary Shapes, *Adv. Mater.*, 2019, 31(7), e1807101.
- 20 Z. Zhao, C. Wang, H. Yan and Y. Liu, Soft Robotics Programmed with Double Crosslinking DNA Hydrogels, *Adv. Funct. Mater.*, 2019, 29(45), 1905911.
- 21 M. Cianchetti, C. Laschi, A. Menciassi and P. Dario, Biomedical applications of soft robotics. *Nature Reviews, Materials*, 2018, 3(6), 143–153.
- 22 M. Sitti, Miniature soft robots—road to the clinic, *Nat. Rev. Mater.*, 2018, 3(6), 74–75.
- 23 G. Ge, Y. Zhang, J. Shao, W. Wang, W. Si, W. Huang and X. Dong, Stretchable, Transparent, and Self-Patterned Hydrogel-Based Pressure Sensor for Human Motions Detection, *Adv. Funct. Mater.*, 2018, 28(32), 1802576.
- 24 X. Shuai, J. Arun and J. A. Rogers, Skin sensors are the future of health care, *Nature*, 2019, 571, 319–321.
- 25 X. Liu, C. Steiger, S. Lin, G. A. Parada, J. Liu, H. F. Chan, H. Yuk, N. V. Phan, J. Collins, S. Tamang, G. Traverso and X. Zhao, Ingestible hydrogel device, *Nat. Commun.*, 2019, 10(1), 493.
- 26 Y. Gao, J. Song, S. Li, C. Elowsky, Y. Zhou, S. Ducharme, Y. M. Chen, Q. Zhou and L. Tan, Hydrogel microphones for stealthy underwater listening, *Nat. Commun.*, 2016, 7, 12316.
- 27 L. Hyunjae, S. Changyeong, S. H. Yong, S. K. Min, R. C. Hye, K. Taegyung, S. Kwangsoo, H. C. Seung, H. Taeghwan and D.-H. Kim, Wearable/disposable sweat-based glucose monitoring device with multistage transdermal drug delivery module, *Sci. Adv.*, 2017, 3(3), e1601314.
- 28 P. Xiong, L. Mengmeng, C. Xiangyu, S. Jiangman, D. Chunhua, Z. Yang, Z. Junyi, H. Weiguang and Z. L. Wang, Ultrastretchable, transparent triboelectric nanogenerator as electronic skin for biomechanical energy harvesting and tactile sensing, *Sci. Adv.*, 2017, 3(5), e1700015.
- 29 P. Li, D. Zhang, Y. Zhang, W. Lu, W. Wang and T. Chen, Ultrafast and Efficient Detection of Formaldehyde in Aqueous Solutions Using Chitosan-based Fluorescent Polymers, *ACS Sens.*, 2018, 3(11), 2394–2401.
- 30 D. Zhang, Y. Fu, L. Huang, Y. Zhang, B. Ren, M. Zhong, J. Yang and J. Zheng, Integration of antifouling and antibacterial properties in salt-responsive hydrogels with surface regeneration capacity, *J. Mater. Chem. B*, 2018, 6(6), 950–960.
- 31 W. Lu, C. Ma, D. Zhang, X. Le, J. Zhang, Y. Huang, C.-F. Huang and T. Chen, Real-Time in Situ Investigation of Supramolecular Shape Memory Process by Fluorescence Switching, *J. Phys. Chem. C*, 2018, 122(17), 9499–9506.
- 32 M. D. Konieczynska, J. C. Villacamacho, C. Ghobril, M. Perezviloria, K. M. Tevis, W. A. Blessing, A. Nazarian, E. K. Rodriguez and M. W. Grinstaff, On-Demand Dissolution of a Dendritic Hydrogel-based Dressing for Second-Degree Burn Wounds through Thiol-Thioester Exchange Reaction, *Angew. Chem., Int. Ed.*, 2016, 55(34), 9984–9987.
- 33 N. Roy, N. Saha, T. Kitano and P. Saha, Development and Characterization of Novel Medicated Hydrogels for Wound Dressing, *Soft Materials*, 2010, 8(2), 130–148.
- 34 B. Mirani, E. Pagan, B. Currie, M. A. Siddiqui, R. Hosseinzadeh, P. Mostafalu, Y. S. Zhang, A. Ghahary and M. Akbari, An Advanced Multifunctional Hydrogel-Based Dressing for Wound Monitoring and Drug Delivery, *Adv. Healthcare Mater.*, 2017, 6(19), 1700718.
- 35 S. Sakai, M. Tsumura, M. Inoue, Y. Koga, K. Fukano and M. Taya, Polyvinyl alcohol-based hydrogel dressing gellable on-wound via a co-enzymatic reaction triggered by glucose in the wound exudate, *J. Mater. Chem. B*, 2013, 1(38), 5067–5075.
- 36 D. Zhang, Y. Zhang, W. Lu, X. Le, P. Li, L. Huang, J. Zhang, J. Yang, M. J. Serpe, D. Chen and T. Chen, Fluorescent Hydrogel-Coated Paper/Textile as Flexible Chemosensor for Visual and Wearable Mercury(II) Detection, *Adv. Mater. Technol.*, 2019, 4(1), 1800201.
- 37 T. S. Stashak, E. Farstvedt and A. Othic, Update on wound dressings: Indications and best use, *Clinical Techniques in Equine Practice*, 2004, 3(2), 148–163.
- 38 A. K. Yetisen, H. Butt, F. da Cruz Vasconcellos, Y. Montelongo, C. A. B. Davidson, J. Blyth, L. Chan, J. B. Carmody, S. Vignolini, U. Steiner, J. J. Baumberg, T. D. Wilkinson and C. R. Lowe, Light-Directed Writing of Chemically Tunable Narrow-Band Holographic Sensors, *Adv. Opt. Mater.*, 2014, 2(3), 250–254.
- 39 Z. Wang, J. Chen, Y. Cong, H. Zhang, T. Xu, L. Nie and J. Fu, Ultrastretchable Strain Sensors and Arrays with High Sensitivity and Linearity Based on Super Tough Conductive Hydrogels, *Chem. Mater.*, 2018, 30(21), 8062–8069.
- 40 H. Chen, F. Yang, Q. Chen and J. Zheng, A Novel Design of Multi-Mechanoresponsive and Mechanically Strong Hydrogels, *Adv. Mater.*, 2017, 29, 21.
- 41 Y. Zhang, B. Ren, F. Yang, Y. Cai, H. Chen, T. Wang, Z. Feng, J. Tang, J. Xu and J. Zheng, Micellar-incorporated hydrogels with highly tough, mechanoresponsive, and self-recovery properties for strain-induced color sensors, *J. Mater. Chem. C*, 2018, 6(43), 11536–11551.
- 42 S. Xiao, Y. Yang, M. Zhong, H. Chen, Y. Zhang, J. Yang and J. Zheng, Salt-Responsive Bilayer Hydrogels with Pseudo-Double-Network Structure Actuated by Polyelectrolyte and Antipolyelectrolyte Effects, *ACS Appl. Mater. Interfaces*, 2017, 9(24), 20843–20851.
- 43 S. Xiao, M. Zhang, X. He, L. Huang, Y. Zhang, B. Ren, M. Zhong, Y. Chang, J. Yang and J. Zheng, Dual Salt- and Thermoresponsive Programmable Bilayer Hydrogel Actuators with Pseudo-Interpenetrating Double-Network Structures, *ACS Appl. Mater. Interfaces*, 2018, 10(25), 21642–21653.
- 44 I. Naydenova, R. Jallapuram, V. Toal and S. Martin, A visual indication of environmental humidity using a color

- changing hologram recorded in a self-developing photopolymer, *Appl. Phys. Lett.*, 2008, **92**(3), 031109.
- 45 C. Ma, T. Li, Q. Zhao, X. Yang, J. Wu, Y. Luo and T. Xie, Supramolecular Lego assembly towards three-dimensional multi-responsive hydrogels, *Adv. Mater.*, 2014, **26**(32), 5665–5669.
- 46 S. Wei, W. Lu, X. Le, C. Ma, H. Lin, B. Wu, J. Zhang, P. Theato and T. Chen, Bioinspired Synergistic Fluorescence-Color-Switchable Polymeric Hydrogel Actuators, *Angew. Chem., Int. Ed.*, 2019, **58**(45), 16243–16251.
- 47 J. Zheng, P. Xiao, X. Le, W. Lu, P. Théato, C. Ma, B. Du, J. Zhang, Y. Huang and T. Chen, Mimosa inspired bilayer hydrogel actuator functioning in multi-environments, *J. Mater. Chem. C*, 2018, **6**(6), 1320–1327.
- 48 J. Wang, J. Wang, Z. Chen, S. Fang, Y. Zhu, R. H. Baughman and L. Jiang, Tunable, Fast, Robust Hydrogel Actuators Based on Evaporation-Programmed Heterogeneous Structures, *Chem. Mater.*, 2017, **29**(22), 9793–9801.
- 49 H. Wang, X. Ji, Z. Li and F. Huang, Fluorescent Supramolecular Polymeric Materials, *Adv. Mater.*, 2017, **29**(14), 1606117.
- 50 L. Voorhaar and R. Hoogenboom, Supramolecular polymer networks: hydrogels and bulk materials, *Chem. Soc. Rev.*, 2016, **45**(14), 4013–4031.
- 51 X. Ding and Y. Wang, Weak Bond-Based Injectable and Stimuli Responsive Hydrogels for Biomedical Applications, *J. Mater. Chem. B*, 2017, **5**(5), 887–906.
- 52 R. Moser, G. Kettlgruber, C. M. Siket, M. Drack, I. M. Graz, U. Cakmak, Z. Major, M. Kaltenbrunner and S. Bauer, From Playroom to Lab: Tough Stretchable Electronics Analyzed with a Tabletop Tensile Tester Made from Toy-Bricks, *Adv. Sci.*, 2016, **3**(4), 1500396.
- 53 X. Zhao, F. Chen, Y. Li, H. Lu, N. Zhang and M. Ma, Bioinspired ultra-stretchable and anti-freezing conductive hydrogel fibers with ordered and reversible polymer chain alignment, *Nat. Commun.*, 2018, **9**(1), 3579.
- 54 J. Zhang, W. Feng, H. Zhang, Z. Wang, H. A. Calcaterra, B. Yeom, P. A. Hu and N. A. Kotov, Multiscale deformations lead to high toughness and circularly polarized emission in helical nacre-like fibres, *Nat. Commun.*, 2016, **7**, 10701.
- 55 A. Chortos, J. Liu and Z. Bao, Pursuing prosthetic electronic skin, *Nat. Mater.*, 2016, **15**(9), 937–950.
- 56 Y. Shao, H. Jia, T. Cao and D. Liu, Supramolecular Hydrogels Based on DNA Self-Assembly, *Acc. Chem. Res.*, 2017, **50**(4), 659–668.
- 57 P. W. Frederix, G. G. Scott, Y. M. Abul-Haija, D. Kalafatovic, C. G. Pappas, N. Javid, N. T. Hunt, R. V. Ulijn and T. Tuttle, Exploring the sequence space for (tri-)peptide self-assembly to design and discover new hydrogels, *Nat. Chem.*, 2015, **7**(1), 30–37.
- 58 W. Lu, C. Huang, K. Hong, N.-G. Kang and J. W. Mays, Poly(1-adamantyl acrylate): Living Anionic Polymerization, Block Copolymerization, and Thermal Properties, *Macromolecules*, 2016, **49**(24), 9406–9414.
- 59 F. Luo, T. L. Sun, T. Nakajima, T. Kurokawa, Y. Zhao, K. Sato, A. B. Ihsan, X. Li, H. Guo and J. P. Gong, Oppositely charged polyelectrolytes form tough, self-healing, and rebuildable hydrogels, *Adv. Mater.*, 2015, **27**(17), 2722–2727.
- 60 K. Yue, G. Trujillo-de Santiago, M. M. Alvarez, A. Tamayol, N. Annabi and A. Khademhosseini, Synthesis, properties, and biomedical applications of gelatin methacryloyl (GelMA) hydrogels, *Biomaterials*, 2015, **73**, 254–271.
- 61 J. F. Xing, M. L. Zheng and X. M. Duan, Two-photon polymerization microfabrication of hydrogels: an advanced 3D printing technology for tissue engineering and drug delivery, *Chem. Soc. Rev.*, 2015, **44**(15), 5031–5039.
- 62 H. P. Tien, P. Hoa, N. C. Toan, N. T. Dat and C. H. Ryeol, A Highly Flexible, Stretchable and Ultra-thin Piezoresistive Tactile Sensor Array using PAM/PEDOT:PSS Hydrogel. 2017 14th International Conference on Ubiquitous Robots and Ambient Intelligence (URAI) 2017, 950–955.
- 63 J. Chen, Q. Peng, T. Thundat and H. Zeng, Stretchable, Injectable, and Self-Healing Conductive Hydrogel Enabled by Multiple Hydrogen Bonding toward Wearable Electronics, *Chem. Mater.*, 2019, **31**(12), 4553–4563.
- 64 Z. Wang, H. Zhou, W. Chen, Q. Li, B. Yan, X. Jin, A. Ma, H. Liu and W. Zhao, Dually Synergetic Network Hydrogels with Integrated Mechanical Stretchability, Thermal Responsiveness, and Electrical Conductivity for Strain Sensors and Temperature Alertors, *ACS Appl. Mater. Interfaces*, 2018, **10**(16), 14045–14054.
- 65 Z. Lei, Q. Wang, S. Sun, W. Zhu and P. Wu, A Bioinspired Mineral Hydrogel as a Self-Healable, Mechanically Adaptable Ionic Skin for Highly Sensitive Pressure Sensing, *Adv. Mater.*, 2017, **29**(22), 1700321.
- 66 Z. Lei and P. Wu, Zwitterionic Skins with a Wide Scope of Customizable Functionalities, *ACS Nano*, 2018, **12**(12), 12860–12868.
- 67 X. L. Luo, J. J. Xu, Q. Zhang, G. J. Yang and H. Y. Chen, Electrochemically deposited chitosan hydrogel for horseradish peroxidase immobilization through gold nanoparticles self-assembly, *Biosens. Bioelectron.*, 2005, **21**(1), 190–196.
- 68 A. Choe, J. Yeom, R. Shanker, M. P. Kim, S. Kang and H. Ko, Stretchable and wearable colorimetric patches based on thermoresponsive plasmonic microgels embedded in a hydrogel film. *NPG Asia, Materials*, 2018, **10**(9), 912–922.
- 69 S. H. Song, J. H. Park, G. Chitnis, R. A. Siegel and B. Ziaie, A wireless chemical sensor featuring iron oxide nanoparticle-embedded hydrogels, *Sens. Actuators, B*, 2014, **193**, 925–930.
- 70 L. Li, L. Pan, Z. Ma, K. Yan, W. Cheng, Y. Shi and G. Yu, All Inkjet-Printed Amperometric Multiplexed Biosensors Based on Nanostructured Conductive Hydrogel Electrodes, *Nano Lett.*, 2018, **18**(6), 3322–3327.
- 71 Z. Dongyuan, L. Borui, S. Yi, P. Lijia, W. Yaqun, L. Wenbo, Z. Rong and G. Yu, Highly Sensitive Glucose Sensor Based on Pt Nanoparticle/Polyaniline Hydrogel Heterostructures, *ACS Nano*, 2013, **7**, 3540–3546.
- 72 H. Zhang, W. Niu and S. Zhang, Extremely Stretchable and Self-Healable Electrical Skin with Mechanical Adaptability, an Ultrawide Linear Response Range, and Excellent Temperature Tolerance, *ACS Appl. Mater. Interfaces*, 2019, **11**(27), 24639–24647.
- 73 H. Gu, H. Zhang, C. Ma, H. Sun, C. Liu, K. Dai, J. Zhang, R. Wei, T. Ding and Z. Guo, Smart strain sensing organic–inorganic

- hybrid hydrogels with nano barium ferrite as the cross-linker, *J. Mater. Chem. C*, 2019, 7(8), 2353–2360.
- 74 L. Han, K. Liu, M. Wang, K. Wang, L. Fang, H. Chen, J. Zhou and X. Lu, Mussel-Inspired Adhesive and Conductive Hydrogel with Long-Lasting Moisture and Extreme Temperature Tolerance, *Adv. Funct. Mater.*, 2018, 28(3), 1704195.
- 75 Z. Yi-Zhou, H. L. Kang, H. A. Dalaver, S. Rachid, J. Qiu, K. Hyunho and H. N. Alshareef, MXenes stretch hydrogel sensor performance to new limits, *Sci. Adv.*, 2018, 4, eaat0098.
- 76 X. Pan, Q. Wang, P. He, K. Liu, Y. Ni, L. Chen, X. Ouyang, L. Huang, H. Wang and S. Xu, A bionic tactile plastic hydrogel-based electronic skin constructed by a nerve-like nanonetwork combining stretchable, compliant, and self-healing properties, *Chem. Eng. J.*, 2020, 379, 122271.
- 77 M. Liao, P. Wan, J. Wen, M. Gong, X. Wu, Y. Wang, R. Shi and L. Zhang, Wearable, Healable, and Adhesive Epidermal Sensors Assembled from Mussel-Inspired Conductive Hybrid Hydrogel Framework, *Adv. Funct. Mater.*, 2017, 27(48), 1703852.
- 78 G. Cai, J. Wang, K. Qian, J. Chen, S. Li and P. S. Lee, Extremely Stretchable Strain Sensors Based on Conductive Self-Healing Dynamic Cross-Links Hydrogels for Human-Motion Detection, *Adv. Sci.*, 2017, 4(2), 1600190.
- 79 H. Qiao, P. Qi, X. Zhang, L. Wang, Y. Tan, Z. Luan, Y. Xia, Y. Li and K. Sui, Multiple Weak H-Bonds Lead to Highly Sensitive, Stretchable, Self-Adhesive, and Self-Healing Ionic Sensors, *ACS Appl. Mater. Interfaces*, 2019, 11(8), 7755–7763.
- 80 S. Liu and L. Li, Ultrastretchable and Self-Healing Double-Network Hydrogel for 3D Printing and Strain Sensor, *ACS Appl. Mater. Interfaces*, 2017, 9(31), 26429–26437.
- 81 W. Fan, X. Zhang, H. Cui, C. Liu, Y. Li, Y. Xia and K. Sui, Direct Current-Powered High-Performance Ionic Hydrogel Strain Sensor Based on Electrochemical Redox Reaction, *ACS Appl. Mater. Interfaces*, 2019, 11(27), 24289–24297.
- 82 H. Chen, X. Ren and G. Gao, Skin-Inspired Gels with Toughness, Antifreezing, Conductivity, and Remoldability, *ACS Appl. Mater. Interfaces*, 2019, 11(31), 28336–28344.
- 83 Q. Zhang, X. Liu, L. Duan and G. Gao, Ultra-stretchable wearable strain sensors based on skin-inspired adhesive, tough and conductive hydrogels, *Chem. Eng. J.*, 2019, 365, 10–19.
- 84 J. Y. Sun, C. Keplinger, G. M. Whitesides and Z. Suo, Ionic skin, *Adv. Mater.*, 2014, 26(45), 7608–7614.
- 85 K. Chong-Chan, L. Hyun-Hee, H. O. Kyu and J.-Y. Sun, Highly stretchable, transparent ionic touch panel, *Science*, 2016, 353, 682–687.
- 86 X. Zhang, N. Sheng, L. Wang, Y. Tan, C. Liu, Y. Xia, Z. Nie and K. Sui, Supramolecular nanofibrillar hydrogels as highly stretchable, elastic and sensitive ionic sensors, *Mater. Horiz.*, 2019, 6(2), 326–333.
- 87 F. Chen, S. Lu, L. Zhu, Z. Tang, Q. Wang, G. Qin, J. Yang, G. Sun, Q. Zhang and Q. Chen, Conductive regenerated silk-fibroin-based hydrogels with integrated high mechanical performances, *J. Mater. Chem. B*, 2019, 7(10), 1708–1715.
- 88 S. Cheng, Y. S. Narang, C. Yang, Z. Suo and R. D. Howe, Stick-On Large-Strain Sensors for Soft Robots, *Adv. Mater. Interfaces*, 2019, 1900985.
- 89 Y. Ren, J. Guo, Z. Liu, Z. Sun, Y. Wu, L. Liu and F. Yan, Ionic liquid-based click-ionogels, *Sci. Adv.*, 2019, 5, 1–10.
- 90 N. Yang, P. Qi, J. Ren, H. Yu, S. Liu, J. Li, W. Chen, D. L. Kaplan and S. Ling, Polyvinyl Alcohol/Silk Fibroin/Borax Hydrogel Ionotronics: A Highly Stretchable, Self-Healable, and Biocompatible Sensing Platform, *ACS Appl. Mater. Interfaces*, 2019, 11(26), 23632–23638.
- 91 R. Wang and Y. Li, Hydrogel based QCM aptasensor for detection of avian influenza virus, *Biosens. Bioelectron.*, 2013, 42, 148–155.
- 92 P. Song, D. Ye, X. Zuo, J. Li, J. Wang, H. Liu, M. T. Hwang, J. Chao, S. Su, L. Wang, J. Shi, L. Wang, W. Huang, R. Lal and C. Fan, DNA Hydrogel with Aptamer-Toehold-Based Recognition, Cloaking, and Decloaking of Circulating Tumor Cells for Live Cell Analysis, *Nano Lett.*, 2017, 17(9), 5193–5198.
- 93 D. Buenger, F. Topuz and J. Groll, Hydrogels in sensing applications, *Prog. Polym. Sci.*, 2012, 37(12), 1678–1719.
- 94 J. Wu, Z. Wu, X. Lu, S. Han, B. R. Yang, X. Gui, K. Tao, J. Miao and C. Liu, Ultrastretchable and Stable Strain Sensors Based on Antifreezing and Self-Healing Ionic Organohydrogels for Human Motion Monitoring, *ACS Appl. Mater. Interfaces*, 2019, 11(9), 9405–9414.
- 95 D. Gan, Z. Huang, X. Wang, L. Jiang, C. Wang, M. Zhu, F. Ren, L. Fang, K. Wang, C. Xie and X. Lu, Graphene Oxide-Templated Conductive and Redox-Active Nanosheets Incorporated Hydrogels for Adhesive Bioelectronics, *Adv. Funct. Mater.*, 2019, 1907678.
- 96 C. Hou, H. Wang, Q. Zhang, Y. Li and M. Zhu, Highly conductive, flexible, and compressible all-graphene passive electronic skin for sensing human touch, *Adv. Mater.*, 2014, 26(29), 5018–5024.
- 97 H. S. Song, O. S. Kwon, J. H. Kim, J. Conde and N. Artzi, 3D hydrogel scaffold doped with 2D graphene materials for biosensors and bioelectronics, *Biosens. Bioelectron.*, 2017, 89(Pt 1), 187–200.
- 98 J. Wu, K. Tao, J. Zhang, Y. Guo, J. Miao and L. K. Norford, Chemically functionalized 3D graphene hydrogel for high performance gas sensing, *J. Mater. Chem. A*, 2016, 4(21), 8130–8140.
- 99 L. Han, X. Lu, M. Wang, D. Gan, W. Deng, K. Wang, L. Fang, K. Liu, C. W. Chan, Y. Tang, L. T. Weng and H. Yuan, A Mussel-Inspired Conductive, Self-Adhesive, and Self-Healable Tough Hydrogel as Cell Stimulators and Implantable Bioelectronics, *Small*, 2017, 13(2), 1601916.
- 100 Y.-Z. Long, M.-M. Li, C. Gu, M. Wan, J.-L. Duvail, Z. Liu and Z. Fan, Recent advances in synthesis, physical properties and applications of conducting polymer nanotubes and nanofibers, *Prog. Polym. Sci.*, 2011, 36(10), 1415–1442.
- 101 G. Lota, K. Fic and E. Frackowiak, Carbon nanotubes and their composites in electrochemical applications, *Energy Environ. Sci.*, 2011, 4(5), 1592–1605.
- 102 Y. He, Q. Gui, Y. Wang, Z. Wang, S. Liao and Y. Wang, A Polypyrrole Elastomer Based on Confined Polymerization in a Host Polymer Network for Highly Stretchable Temperature and Strain Sensors, *Small*, 2018, 14(19), e1800394.

- 103 A. D. Chowdhury, K. Takemura, T. C. Li, T. Suzuki and E. Y. Park, Electrical pulse-induced electrochemical biosensor for hepatitis E virus detection, *Nat. Commun.*, 2019, **10**(1), 3737.
- 104 B. W. An, S. Heo, S. Ji, F. Bien and J. U. Park, Transparent and flexible fingerprint sensor array with multiplexed detection of tactile pressure and skin temperature, *Nat. Commun.*, 2018, **9**(1), 2458.
- 105 L. Han, L. Yan, M. Wang, K. Wang, L. Fang, J. Zhou, J. Fang, F. Ren and X. Lu, Transparent, Adhesive, and Conductive Hydrogel for Soft Bioelectronics Based on Light-Transmitting Polydopamine-Doped Polypyrrole Nanofibrils, *Chem. Mater.*, 2018, **30**(16), 5561–5572.
- 106 P. Li, Z. Jin, L. Peng, F. Zhao, D. Xiao, Y. Jin and G. Yu, Stretchable All-Gel-State Fiber-Shaped Supercapacitors Enabled by Macromolecularly Interconnected 3D Graphene/Nanostructured Conductive Polymer Hydrogels, *Adv. Mater.*, 2018, **30**(18), e1800124.
- 107 Y. Shi, C. Ma, L. Peng and G. Yu, Conductive “Smart” Hybrid Hydrogels with PNIPAM and Nanostructured Conductive Polymers, *Adv. Funct. Mater.*, 2015, **25**(8), 1219–1225.
- 108 A. M. Bryan, L. M. Santino, Y. Lu, S. Acharya and J. M. D’Arcy, Conducting Polymers for Pseudocapacitive Energy Storage, *Chem. Mater.*, 2016, **28**(17), 5989–5998.
- 109 R. Kishi, K. Kubota, T. Miura, T. Yamaguchi, H. Okuzaki and Y. Osada, Mechanically tough double-network hydrogels with high electronic conductivity, *J. Mater. Chem. C*, 2014, **2**(4), 736–743.
- 110 T. Dai, X. Qing, Y. Lu and Y. Xia, Conducting hydrogels with enhanced mechanical strength, *Polymer*, 2009, **50**(22), 5236–5241.
- 111 J. You, S. Xie, J. Cao, H. Ge, M. Xu, L. Zhang and J. Zhou, Quaternized Chitosan/Poly(acrylic acid) Polyelectrolyte Complex Hydrogels with Tough, Self-Recovery, and Tunable Mechanical Properties, *Macromolecules*, 2016, **49**(3), 1049–1059.
- 112 Y. Huang, M. Zhong, F. Shi, X. Liu, Z. Tang, Y. Wang, Y. Huang, H. Hou, X. Xie and C. Zhi, An Intrinsically Stretchable and Compressible Supercapacitor Containing a Polyacrylamide Hydrogel Electrolyte, *Angew. Chem., Int. Ed.*, 2017, **56**(31), 9141–9145.
- 113 Z. Jia, Y. Zeng, P. Tang, D. Gan, W. Xing, Y. Hou, K. Wang, C. Xie and X. Lu, Conductive, Tough, Transparent, and Self-Healing Hydrogels Based on Catechol–Metal Ion Dual Self-Catalysis, *Chem. Mater.*, 2019, **31**(15), 5625–5632.
- 114 Q. Thiburce and A. J. Campbell, Low-Voltage Polyelectrolyte-Gated Polymer Field-Effect Transistors Gravure Printed at High Speed on Flexible Plastic Substrates, *Adv. Electron. Mater.*, 2017, **3**(2), 1600421.
- 115 S. Ali, M. Bleuel and V. M. Prabhu, Lower Critical Solution Temperature in Polyelectrolyte Complex Coacervates, *ACS Macro Lett.*, 2019, **8**(3), 289–293.
- 116 L. Wang, G. Gao, Y. Zhou, T. Xu, J. Chen, R. Wang, R. Zhang and J. Fu, Tough, Adhesive, Self-Healable, and Transparent Ionically Conductive Zwitterionic Nanocomposite Hydrogels as Skin Strain Sensors, *ACS Appl. Mater. Interfaces*, 2019, **11**(3), 3506–3515.
- 117 J. Kim, S. Nayak and L. A. Lyon, Bioresponsive hydrogel microlenses, *J. Am. Chem. Soc.*, 2005, **127**(26), 9588–9592.
- 118 Z. Lei and P. Wu, A supramolecular biomimetic skin combining a wide spectrum of mechanical properties and multiple sensory capabilities, *Nat. Commun.*, 2018, **9**(1), 1134.
- 119 S. Lin, C. Yuan, A. Ke and Z. Quan, Electrical response characterization of PVA-P(AA/AMPS) IPN hydrogels in aqueous Na₂SO₄ solution, *Sens. Actuators, B*, 2008, **134**(1), 281–286.
- 120 F. Liu and M. W. Urban, Recent advances and challenges in designing stimuli-responsive polymers, *Prog. Polym. Sci.*, 2010, **35**(1–2), 3–23.
- 121 P. Bouillot and B. Vincent, A comparison of the swelling behaviour of copolymer and interpenetrating network microgel particles, *Colloid Polym. Sci.*, 2000, **278**(1), 74–79.
- 122 Y. Xu, O. Ghag, M. Reimann, P. Sitterle, P. Chatterjee, E. Nofen, H. Yu, H. Jiang and L. L. Dai, Development of visible-light responsive and mechanically enhanced “smart” UCST interpenetrating network hydrogels, *Soft Matter*, 2017, **14**(1), 151–160.
- 123 Z. Wang, J. Chen, L. Wang, G. Gao, Y. Zhou, R. Wang, T. Xu, J. Yin and J. Fu, Flexible and wearable strain sensors based on tough and self-adhesive ion conducting hydrogels, *J. Mater. Chem. B*, 2019, **7**(1), 24–29.
- 124 H. Izawa and J.-i. Kadokawa, Preparation and characterizations of functional ionic liquid-gel and hydrogel materials of xanthan gum, *J. Mater. Chem.*, 2010, **20**(25), 5235.
- 125 J. Yan, M.-T. F. Rodrigues, Z. Song, H. Li, H. Xu, H. Liu, J. Wu, Y. Xu, Y. Song, Y. Liu, P. Yu, W. Yang, R. Vajtai, H. Li, S. Yuan and P. M. Ajayan, Reversible Formation of g-C₃N₄ 3D Hydrogels through Ionic Liquid Activation: Gelation Behavior and Room-Temperature Gas-Sensing Properties, *Adv. Funct. Mater.*, 2017, **27**(22), 1700653.
- 126 C. Wang, X. Liu, V. Wulf, M. Vazquez-Gonzalez, M. Fadeev and I. Willner, DNA-Based Hydrogels Loaded with Au Nanoparticles or Au Nanorods: Thermoresponsive Plasmonic Matrices for Shape-Memory, Self-Healing, Controlled Release, and Mechanical Applications, *ACS Nano*, 2019, **13**(3), 3424–3433.
- 127 Y. Li, Y. Ma, X. Jiao, T. Li, Z. Lv, C. J. Yang, X. Zhang and Y. Wen, Control of capillary behavior through target-responsive hydrogel permeability alteration for sensitive visual quantitative detection, *Nat. Commun.*, 2019, **10**(1), 1036.
- 128 S. Pahoff, C. Meinert, O. Bas, L. Nguyen, T. J. Klein and D. W. Huttmacher, Effect of gelatin source and photo-initiator type on chondrocyte redifferentiation in gelatin methacryloyl-based tissue-engineered cartilage constructs, *J. Mater. Chem. B*, 2019, **7**(10), 1761–1772.
- 129 J. C. Rose and L. De Laporte, Hierarchical Design of Tissue Regenerative Constructs, *Adv. Healthcare Mater.*, 2018, **7**(6), e1701067.
- 130 N. Masurier, J.-B. Tissot, D. Boukhriss, S. Jebors, C. Pinese, P. Verdié, M. Amblard, A. Mehdi, J. Martinez, V. Humblot and G. Subra, Site-specific grafting on titanium surfaces with hybrid temporin antibacterial peptides, *J. Mater. Chem. B*, 2018, **6**(12), 1782–1790.
- 131 Z. Li, G. Davidson-Rozenfeld, M. Vazquez-Gonzalez, M. Fadeev, J. Zhang, H. Tian and I. Willner, Multi-triggered

- Supramolecular DNA/Bipyridinium Dithienylethene Hydrogels Driven by Light, Redox, and Chemical Stimuli for Shape-Memory and Self-Healing Applications, *J. Am. Chem. Soc.*, 2018, **140**(50), 17691–17701.
- 132 W. Inthavong, T. Nicolai and C. Chassenieux, Polymer Probe Diffusion in Globular Protein Gels and Aggregate Suspensions, *J. Phys. Chem. B*, 2018, **122**(33), 8075–8081.
- 133 K. I. Shingel and M.-P. Faure, Structure-Property Relationships in Poly (ethylene glycol)-Protein Hydrogel Systems Made from Various Proteins, *Biomacromolecules*, 2005, **6**(3), 1635–1641.
- 134 A. R. Patel, Functional and Engineered Colloids from Edible Materials for Emerging Applications in Designing the Food of the Future, *Adv. Funct. Mater.*, 2018, 1806809.
- 135 X. Qin, C. Yu, J. Wei, L. Li, C. Zhang, Q. Wu, J. Liu, S. Q. Yao and W. Huang, Rational Design of Nanocarriers for Intracellular Protein Delivery, *Adv. Mater.*, 2019, **31**(46), e1902791.
- 136 H. Guo, J. Zhang, T. Xu, Z. Zhang, J. Yao and Z. Shao, The robust hydrogel hierarchically assembled from a pH sensitive peptide amphiphile based on silk fibroin, *Biomacromolecules*, 2013, **14**(8), 2733–2738.
- 137 A. Maslovskis, J. B. Guilbaud, I. Grillo, N. Hodson, A. F. Miller and A. Saiani, Self-assembling peptide/thermo-responsive polymer composite hydrogels: effect of peptide-polymer interactions on hydrogel properties, *Langmuir*, 2014, **30**(34), 10471–10480.
- 138 C. M. Rubert Perez, L. A. Rank and J. Chmielewski, Tuning the thermosensitive properties of hybrid collagen peptide-polymer hydrogels, *Chem. Commun.*, 2014, **50**(60), 8174–8176.
- 139 S. H. Um, J. B. Lee, N. Park, S. Y. Kwon, C. C. Umbach and D. Luo, Enzyme-catalysed assembly of DNA hydrogel, *Nat. Mater.*, 2006, **5**(10), 797–801.
- 140 D. C. Lin, B. Yurke and N. A. Langrana, Mechanical properties of a reversible, DNA-crosslinked polyacrylamide hydrogel, *J. Biomech. Eng.*, 2004, **126**(1), 104–110.
- 141 X. Liu, Q. Zhang and G. Gao, Bioinspired Adhesive Hydrogels Tackified by Nucleobases, *Adv. Funct. Mater.*, 2017, **27**(44), 1703132.
- 142 P. Zhang, J. Jiang, R. Yuan, Y. Zhuo and Y. Chai, Highly Ordered and Field-Free 3D DNA Nanostructure: The Next Generation of DNA Nanomachine for Rapid Single-Step Sensing, *J. Am. Chem. Soc.*, 2018, **140**(30), 9361–9364.
- 143 M. Li, H. Ding, M. Lin, F. Yin, L. Song, X. Mao, F. Li, Z. Ge, L. Wang, X. Zuo, Y. Ma and C. Fan, DNA Framework-Programmed Cell Capture via Topology-Engineered Receptor-Ligand Interactions, *J. Am. Chem. Soc.*, 2019, **141**(47), 18910–18915.
- 144 H. Tang, X. Duan, X. Feng, L. Liu, S. Wang, Y. Li and D. Zhu, Fluorescent DNA-poly(phenylenevinylene) hybrid hydrogels for monitoring drug release, *Chem. Commun.*, 2009, 641–643.
- 145 K. K. Kim, I. Ha, P. Won, D. G. Seo, K. J. Cho and S. H. Ko, Transparent wearable three-dimensional touch by self-generated multiscale structure, *Nat. Commun.*, 2019, **10**(1), 2582.
- 146 Y. Hong, F. Zhou, Y. Hua, X. Zhang, C. Ni, D. Pan, Y. Zhang, D. Jiang, L. Yang, Q. Lin, Y. Zou, D. Yu, D. E. Arnot, X. Zou, L. Zhu, S. Zhang and H. Ouyang, A strongly adhesive hemostatic hydrogel for the repair of arterial and heart bleeds, *Nat. Commun.*, 2019, **10**(1), 2060.
- 147 D. Wirthl, R. Pichler, M. Drack, G. Kettlguber, R. Moser, R. Gerstmayr, F. Hartmann, E. Bradt, R. Kaltseis, C. M. Siket, S. E. Schausberger, S. Hild, S. Bauer and M. Kaltenbrunner, Instant tough bonding of hydrogels for soft machines and electronics, *Sci. Adv.*, 2017, **3**(6), e1700053.
- 148 C. M. Boutry, L. Beker, Y. Kaizawa, C. Vassos, H. Tran, A. C. Hinckley, R. Pfattner, S. Niu, J. Li, J. Claverie, Z. Wang, J. Chang, P. M. Fox and Z. Bao, Biodegradable and flexible arterial-pulse sensor for the wireless monitoring of blood flow, *Nat. Biomed. Eng.*, 2019, **3**(1), 47–57.
- 149 S. Niu, N. Matsuhisa, L. Beker, J. Li, S. Wang, J. Wang, Y. Jiang, X. Yan, Y. Yun, W. Burnett, A. S. Y. Poon, J. B. H. Tok, X. Chen and Z. Bao, A wireless body area sensor network based on stretchable passive tags, *Nat. Electron.*, 2019, **2**(8), 361–368.
- 150 X. Li, Z. Yin, X. Zhang, Y. Wang, D. Wang, M. Gao, J. Meng, J. Wu and J. You, Epitaxial Liftoff of Wafer-Scale VO₂ Nanomembranes for Flexible, Ultrasensitive Tactile Sensors, *Adv. Mater. Technol.*, 2019, **4**(7), 1800695.
- 151 J. h. Li, J. h. Chen and F. Xu, Sensitive and Wearable Optical Microfiber Sensor for Human Health Monitoring, *Adv. Mater. Technol.*, 2018, **3**(12), 1800296.
- 152 X. Wang, Z. Liu and T. Zhang, Flexible Sensing Electronics for Wearable/Attachable Health Monitoring, *Small*, 2017, **13**(25), 1602790.
- 153 H. Liu, M. Li, C. Ouyang, T. J. Lu, F. Li and F. Xu, Biofriendly, Stretchable, and Reusable Hydrogel Electronics as Wearable Force Sensors, *Small*, 2018, **14**(36), e1801711.
- 154 W. Hou, N. Sheng, X. Zhang, Z. Luan, P. Qi, M. Lin, Y. Tan, Y. Xia, Y. Li and K. Sui, Design of injectable agar/NaCl/polyacrylamide ionic hydrogels for high performance strain sensors, *Carbohydr. Polym.*, 2019, **211**, 322–328.
- 155 M. A. Darabi, A. Khosrozadeh, R. Mbeleck, Y. Liu, Q. Chang, J. Jiang, J. Cai, Q. Wang, G. Luo and M. Xing, Skin-Inspired Multifunctional Autonomic-Intrinsic Conductive Self-Healing Hydrogels with Pressure Sensitivity, Stretchability, and 3D Printability, *Adv. Mater.*, 2017, **29**, 31.
- 156 C. Shao, M. Wang, L. Meng, H. Chang, B. Wang, F. Xu, J. Yang and P. Wan, Mussel-Inspired Cellulose Nanocomposite Tough Hydrogels with Synergistic Self-Healing, Adhesive, and Strain-Sensitive Properties, *Chem. Mater.*, 2018, **30**(9), 3110–3121.
- 157 Q. Chang, M. A. Darabi, Y. Liu, Y. He, W. Zhong, K. Mequanin, B. Li, F. Lu and M. M. Q. Xing, Hydrogels from natural egg white with extraordinary stretchability, direct-writing 3D printability and self-healing for fabrication of electronic sensors and actuators, *J. Mater. Chem. A*, 2019, **7**(42), 24626–24640.
- 158 T. H. Kang, H. Chang, D. Choi, S. Kim, J. Moon, J. A. Lim, K. Y. Lee and H. Yi, Hydrogel-Templated Transfer-Printing of Conductive Nanonetworks for Wearable Sensors on

- Topographic Flexible Substrates, *Nano Lett.*, 2019, **19**(6), 3684–3691.
- 159 Y. Tai and Z. Yang, Toward Flexible Wireless Pressure-Sensing Device via Ionic Hydrogel Microsphere for Continuously Mapping Human-Skin Signals, *Adv. Mater. Interfaces*, 2017, **4**(20), 1700496.
- 160 T. Wang, H. Yang, D. Qi, Z. Liu, P. Cai, H. Zhang and X. Chen, Mechano-Based Transductive Sensing for Wearable Healthcare, *Small*, 2018, **14**(11), e1702933.
- 161 E. Tian, J. Wang, Y. Zheng, Y. Song, L. Jiang and D. Zhu, Colorful humidity sensitive photonic crystal hydrogel, *J. Mater. Chem.*, 2008, **18**(10), 1116–1122.
- 162 K. I. MacConaghy, C. I. Geary, J. L. Kaar and M. P. Stoykovich, Photonic crystal kinase biosensor, *J. Am. Chem. Soc.*, 2014, **136**(19), 6896–6899.
- 163 L. Duan, D. R. D'Hooge and L. Cardon, Recent progress on flexible and stretchable piezoresistive strain sensors: from design to application, *Prog. Mater. Sci.*, 2019, 100617.
- 164 Y. O. Jin, S. Donghee, K. Toru, L. Yeongjun, K. Yeongin, L. Jeffrey, W. Hung-Chin, K. Jiheong, P. Joonsuk, G. Xiaodan, M. Jaewan, G.-J. W. Nathan, Y. Yikai, C. Wei, Y. Youngjun, B.-H. T. Jeffrey and Z. Bao, Stretchable self-healable semiconducting polymer film for active-matrix strain-sensing array, *Sci. Adv.*, 2019, **5**(11), eaav3097.