



Cite this: *Nanoscale*, 2023, **15**, 10776

# Activity-enhanced DNAzyme for design of label-free copper(II) biosensor†

William Etheridge,<sup>a,b</sup> Frederic Brossard,<sup>b</sup> Sitan Zheng,<sup>a</sup> Svenja Moench,<sup>c</sup> Suraj Pavagada,<sup>ib</sup>  <sup>a</sup> Róisín M. Owens  <sup>a</sup> and Ljiljana Fruk<sup>\*a</sup>

Metal ion-driven, DNA-cleaving DNAzymes are characterised by high selectivity and specificity. However, their use for metal ion sensing remains largely unexplored due to long reaction times and poor reaction yields relative to RNA-cleaving DNAzymes and other sensing strategies. Herein we present a study demonstrating a significant rate enhancement of a copper-selective DNA cleaving DNAzyme by both polydopamine (PDA) and gold (Au) nanoparticles (NPs). PDA NPs enhance the reaction through the production of hydrogen peroxide, while for AuNPs the enhancement is aided by the presence of citrate surface moieties, both of which drive the oxidative cleavage of the substrate. A 50-fold enhancement for PDA NPs makes the combination of PDA and DNAzyme suitable for a practical application as a sensitive biosensor for Cu(II) ions. Using DNAzyme deposition onto a gold electrode followed by Polydopamine Assisted DNA Immobilisation (PADII), we achieve a cost-effective, label-free and fast (within 15 min) electrochemical biosensor with a limit of detection of 180 nmol (11 ppm), thus opening a route for the rational design of a new generation of hybrid DNAzyme-based biosensors.

Received 10th May 2023,  
Accepted 4th June 2023

DOI: 10.1039/d3nr02169f

[rsc.li/nanoscale](https://rsc.li/nanoscale)

## 1. Introduction

DNAzymes are catalytically active sequences of single stranded DNA (ssDNA) exhibiting a range of functions such as DNA/RNA cleavage, ribonucleotide labelling and catalysis of click chemistry reactions.<sup>1,2</sup> Most DNAzyme mediated reactions require metal ion co-factors, and DNAzymes requiring Pb<sup>2+</sup>, Cu<sup>2+</sup>, Ag<sup>+</sup>, Hg<sup>2+</sup>, Mn<sup>2+</sup> and Zn<sup>2+</sup> ions have been identified through *in vitro* selection.<sup>3–8</sup> This dependency on metal ions has been exploited in the design of sensitive metal biosensors, mainly utilising RNA-cleaving DNAzymes, which generally exhibit high reaction rates due to the presence of a hydroxyl group within the RNA substrate. However, RNA degrades easily, limiting the application of such sensors in real-life settings such as environmental monitoring.

In contrast, despite their inherently higher stability, the use of DNA-cleaving DNAzymes remains largely underexplored due to their long reaction times and poor yields compared to RNA-

cleaving counterparts. Thus, to make DNA-cleaving DNAzymes more useful for metal ion sensing, DNAzymes with an improved kinetic profile need to be developed or new strategies enhancing their activity introduced. Herewith, we present a strategy to significantly enhance the activity of a Cu(II)-specific DNA-cleaving DNAzyme to develop a specific and more sensitive electrochemical platform for the detection of Cu(II) ions.

Although in low amounts Cu(II) is beneficial and acts as a metal cofactor of several enzyme classes,<sup>9</sup> accumulation of Cu(II) can have numerous detrimental effects. For example, increased amount of Cu(II) in plants due to soil contamination from mining, pesticide production and fossil fuel burning has been shown to have negative effects on germination, growth, and plant development, as well as the photosynthetic cycle.<sup>10–13</sup> High levels of Cu(II) in oceans stemming from pollutants such as marine paints and wastewater can lead to metabolic changes and developmental issues in plankton and algae, which are crucial for the health of the oceanic ecosystem.<sup>14,15</sup> In medicine, abnormalities in Cu(II) homeostasis have been implicated in an increased risk of developing neurological disorders such as Alzheimer's disease.<sup>16</sup> In addition, a genetic disorder known as Wilson's disease is directly related to the inability to process Cu(II) resulting in its accumulation in blood and tissue that can lead to severe tissue damage and death.<sup>17</sup> Finally, Cu(II) ingestion through tap water contamination has been linked to increased cases of liver cirrhosis and acute poisoning.<sup>18</sup>

<sup>a</sup>BioNano Engineering Group, Department of Chemical Engineering and Biotechnology, University of Cambridge, West Cambridge Site, Philippa Fawcett Drive CB3 0AS, Cambridge, UK. E-mail: lf389@cam.ac.uk

<sup>b</sup>Hitachi Cambridge Laboratory, Hitachi Europe Ltd, J. J. Thomson Avenue, Cambridge CB3 0HE, UK

<sup>c</sup>Karlsruhe Institute of Technology (KIT), Institute for Biological Interfaces (IBG 1), Hermann-von-Helmholtz-Platz, D-76344 Eggenstein-Leopoldshafen, Germany

† Electronic supplementary information (ESI) available. See DOI: <https://doi.org/10.1039/d3nr02169f>



Clearly, detection and quantification of Cu(II) in water and biological samples is important not only for environmental remediation but also in diagnostics and industrial process monitoring. Commonly, Cu(II) sensor design relies on ion interaction with organic dyes, which is measured by monitoring the resulting change in dye absorbance or emission.<sup>19</sup> However, such strategies often require extensive molecular design and the use of components that are often sensitive to environmental conditions.<sup>20,21</sup>

DNAzymes recently emerged as a suitable alternative to organic dyes, with two Cu-selective RNA-cleaving DNAzymes reported that exhibit a reaction kinetics and sensitivity suitable for point of care sensing.<sup>22</sup> These systems utilise fluorescence quenching phenomena and although a limit of detection for Cu(II) of 1.6 nM was achieved, reliance on the use of fluorescent dyes, quenchers, and unstable RNA substrates limits the long-term stability and storage of this sensor.

In addition to RNA-cleaving DNAzymes, six Cu(II) selective DNA-cleaving DNAzymes have been reported, with five of them requiring ascorbate ions alongside Cu(II) for substrate cleavage through the oxidative damage mechanism.<sup>23,24</sup> The remaining sixth DNAzyme, named F8, required the addition of Mn(II) ions and metal salts (Na<sup>+</sup> and K<sup>+</sup>), all of which resulted in a low reaction rate of DNA substrate cleavage with  $K_{\text{obs}} = 0.137 \text{ h}^{-1.25}$ .

Herewith, we present a simple route to significant improvement of the catalytic activity of Cu(II)-specific F8 DNAzyme by employing nanoparticles (NPs) as additives (Fig. 1a). We further exploit this enhancement to design a new class of sensitive electrochemical sensors for the rapid detection of Cu(II) ions in solution. This was achieved through the deposition of F8 and AuNPs followed by the production of a protective and activity-enhancing polydopamine (PDA) coating to improve the sensitivity, stability, and storage of the sensor (Fig. 1b). Not only does our biosensor results in fast readout and sensitivity,

but the use of a label-free electrochemical readout instead of fluorescent labels improves the cost-effectiveness and simplicity of the design. In addition, unlike other DNAzyme sensors, our design does not require complex electrode modification, covalent immobilisation,<sup>26</sup> or the use of mediators<sup>27</sup> to improve the electrochemical readout and sensitivity.

## 2. Materials and methods

### 2.1 DNA sequences

F8 DNAzyme	5' AG TGT TCC GTG GAT GGA GCA ATA GTC TCC CGG GTC CGT ATG GAT CGG CA 3'
F8 substrate	5' TGC CGA TCC ATA CTG CGG AAC ACT 3'
W8 non-enzyme DNA	5' AG TGT TCC GCA GTA TGG ATC GGC A 3'


DNAzyme, substrate and controls as well as Cy3-labelled DNAzyme were purchased from Integrated DNA Technologies with HPLC purification. Citrate coated gold (Au, 20 nm) and silver (Ag, 20 nm) nanoparticles, copper nano-powder (Cu, 25 nm) and iron oxide (Fe<sub>2</sub>O<sub>3</sub>/Fe<sub>3</sub>O<sub>4</sub>, 25 nm) were purchased from Sigma Aldrich. PDA NPs were made in house following the protocol in section 2.2. Fluorometric H<sub>2</sub>O<sub>2</sub> assay kit (MAK165-1KT) used to assess the production of H<sub>2</sub>O<sub>2</sub> from PDA NPs was obtained from Sigma Aldrich.

### 2.2 Synthesis of polydopamine nanoparticle (PDA NPs)

92 mg of dopamine hydrochloride (Sigma Aldrich) was dissolved in 1 mL ultra-pure water and added to 135 g of Tris Base (Sigma Aldrich) in 200 mL of ultra-pure water. The solution was then stirred at 300 rpm for 30 min and left overnight at room temperature. The solution was centrifuged at 25 000g, removing the supernatant and resuspending the pellet in water 3 times yielding the final polydopamine nanoparticles. The nanoparticles were characterised by zeta-potential and DLS measurements (both Malvern Zetasizer Nano ZS) giving a zeta potential of -43.8 mV and a polydispersity index of 0.185. SEM images (ESI, Fig. S1†) were taken and demonstrated a uniform and spherical morphology with an average diameter of 142.4 nm.

### 2.3 Screening of F8 DNAzyme activity in presence of nanoparticles

For all assays, 1 μM of both F8 and DNA substrate were annealed in 15 mM NaCl and 50 mM HEPES buffer (pH 7.0–7.6) by heating to 95 °C for 5 min and allowing to cool at room temperature for 30 min. The resulting F8-substrate complex was then exposed to 12.5 μM copper(II) chloride in the absence and presence of NPs (0.01 mg mL<sup>-1</sup> of 20 nm citrate capped Au and AgNPs, 25 nm CuNP, 140 nm PDA NPs and 30 nm Fe<sub>2</sub>O<sub>3</sub>/Fe<sub>3</sub>O<sub>4</sub>). All cleavage reactions were performed at 37 °C for 10 min and 1 hour. After incubation, the cleavage reaction was quenched using 8 M urea and results were analysed using 12% Urea PAGE Gel Electrophoresis at 45 V for 120 min. The resulting gels were imaged using a Syngene

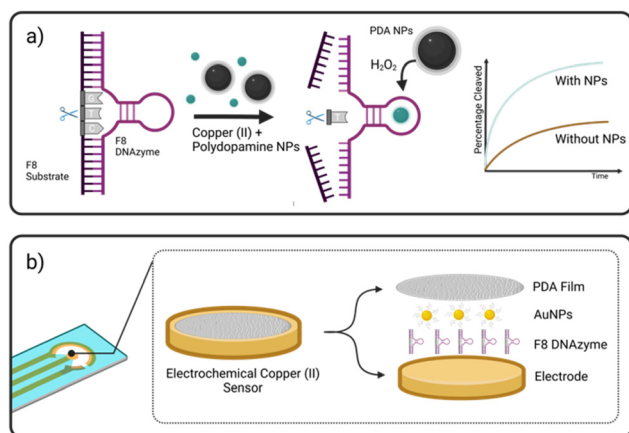

**Fig. 1** (a) DNA cleavage by DNAzyme (F8 DNAzyme) in the presence of copper(II) ions is enhanced in the presence of polydopamine nanoparticles (PDA NPs). Design of fast and efficient electrochemical sensor for Cu(II) based on the F8 DNAzyme exploiting both PDA and gold NP (Au NP) enhancement is shown in (b).



G-Box camera and quantified using ImageJ gel analysis software.

## 2.4 Electrochemical sensor design

Disposable screen-printed electrodes were purchased from Metrohm UK (DRP C220AT) consisting of a gold working electrode, a gold auxiliary electrode, and a silver reference electrode. They were first electrochemically cleaned by cyclic voltammetry from 0 to 1.5 V in 1 M sulphuric acid for 10 cycles and dried under nitrogen gas. Pre-annealed F8-substrate complex was added to 0.02 mg mL<sup>-1</sup> 20 nm citrate capped Au NPs and 10  $\mu$ L was drop cast onto the working electrode. The droplet was dried over 10 min under a light stream of nitrogen gas. 10  $\mu$ L of 5 mg mL<sup>-1</sup> dopamine hydrochloride in 10 mM Tris-buffer pH 8.5 was then drop casted onto the working electrode containing the dried Au NP-doped F8 complex. Dopamine was allowed to polymerise over 2 hours in 100% humidity to prevent drying, and then washed in PBS and water 3 times.

## 2.5 Electrochemical measurements

All electrochemical measurements were taken using a Palmsens 4 potentiostat in PBS. The sensor was clamped in position fully submerged in PBS and allowed to sit for 5 min in stirred solution (100 rpm). Three blank measurements were then taken to generate a stable baseline measurement. The solution was then adjusted to a desired Cu(II) concentration using 2 mM stock solution of CuCl<sub>2</sub> solution in ultra-pure water. Differential pulse voltammetry (DPV) measurements were then taken after 15 min. -0.5 V to +0.2 V was used for the voltage scan range with an increment of 0.01 V. The pulse width was 0.02 s with an amplitude of 0.2 V. Peak currents were calculated by subtracting baseline measurement at peak voltage.

# 3 Results and discussion

## 3.1 NP-mediated rate enhancement of F8 DNzyme

A screening assay was performed to investigate the effect of various classes of commercially available nanoparticles on the cleavage rate of F8 DNzyme. Initial motivation was to design solid platform for DNzyme immobilisation to ease the enzyme recovery from the solution. In short, 0.01 mg mL<sup>-1</sup> of copper (CuNP), iron oxide (Fe<sub>2</sub>O<sub>3</sub>/Fe<sub>3</sub>O<sub>4</sub> NP), polydopamine (PDA NPs), gold (AuNP), or silver (AgNP) nanoparticles were added to the solution of F8 DNzyme hybridised with F8 DNA sequence spiked with 12.5  $\mu$ M CuCl<sub>2</sub>. The reaction was stopped after 10 min and 60 min to assess the percentage of cleaved substrates using gel electrophoresis. Surprisingly, a significant amount of the cleaved substrate was observed already after 10 min in presence of PDA (67.3%), Au (44.9%), and Ag (13.5%) NPs when compared to the control that contain CuCl<sub>2</sub> only (1.3%) (Fig. 2). After 60 min, 100% substrate cleavage was obtained in the presence of PDA/AuNP, while control sample showed only 11% (Fig. 2 and complete PAGE gel image in Fig. S2†).



**Fig. 2** Nanoparticles explored for activity enhancement of F8DNzyme (a). The percentage of DNA substrate cleaved after 10 min in absence and the presence of NPs is shown in (b) and corresponding gel electrophoresis image (Urea PAGE 12%, F8 DNzyme labelled with Cy3-dye. F8 Substrate labelled with 6FAM-dye) in (c).

The rate enhancement of Au and Ag NPs is attributed to the citrate-coating, with citrate ions directly contributing to the improved cleavage rate as demonstrated by the effect of the citrate ions alone (ESI, Fig. S3 and S4†). On the other hand, we hypothesised that PDA NP-mediated enhancement stems from the direct generation of hydrogen peroxide (H<sub>2</sub>O<sub>2</sub>) by PDA NPs in solution. Previously, it was shown that the activity of F8 DNzyme can be increased by addition of H<sub>2</sub>O<sub>2</sub> to Cu(II) ions.<sup>25</sup> In addition, we knew from previous studies that PDA structures can generate H<sub>2</sub>O<sub>2</sub> from molecular oxygen present in water.<sup>28</sup> To test our hypothesis that indeed PDA-mediated production of H<sub>2</sub>O<sub>2</sub> impacts the oxidative cleavage of DNA substrate, we measured the concentration of H<sub>2</sub>O<sub>2</sub> generated by PDA NPs. Employing H<sub>2</sub>O<sub>2</sub> screening assay we found that 0.01 mg mL<sup>-1</sup> of PDA NPs, the amount used in DNzyme studies, generates 1.7  $\mu$ M H<sub>2</sub>O<sub>2</sub> (ESI, Fig. S5†). Due to the smaller enhancement rate, we did not look deeper into the mechanism of IONPs and CuNPs. However, as IONPs can generate H<sub>2</sub>O<sub>2</sub><sup>29</sup> this is a likely reason for observed cleavage enhancement, while in case of CuNPs, the enhancement effect could stem from increased concentration of Cu(II) available to the enzyme through a leaching effect.<sup>30</sup>

## 3.2 Design of the DNzyme-based Cu(II) sensor

Considering the remarkable enhancement of the Cu(II)-mediated DNA cleavage in the presence of NPs, we considered potential ways to exploit this effect in the design of an affordable and simple-to-fabricate biosensor for Cu(II) detection. In terms of sensing, electrochemical sensors have numerous advantages such as cost-effectiveness and ease of detection, and we aimed to focus on design of DNzyme based electrochemical sensing. One of the major challenges in design of electrochemical biosensors is ensuring the deposition and immobilisation of active elements onto electrode surface. To avoid complex immobilisation strategies that would involve additional DNzyme modifications, we decided to exploit PDA




and use it as a protective and activity-enhancing coating. Similar strategy was recently demonstrated in design of electrochemical  $\text{H}_2\text{O}_2$  biosensor using heme G-quadruplex DNAzyme, which was entrapped within PDA layer.<sup>31</sup>

Polydopamine assisted DNA immobilisation (PADI) is a simple and effective strategy that does not require any covalent attachment of DNAzymes onto the electrode. However, as PDA is an electrical insulator, it is crucial that the coating step is performed after drop casting of DNAzyme to ensure the current flow to the electrode.

As shown in Fig. 3, the fabrication of our biosensor consists of two steps: (i) drop-casting of DNAzyme/substrate complex onto a gold electrode followed by formation of PDA layer (PADI, ii). PADI proceeds through self-polymerisation of dopamine precursor on top of the deposited biomolecules and any rate-enhancing additives such as NPs.

To ensure that drop casting results in a homogenous and reproducible electrode coating, we investigated drop casting and drying using Cy3-labelled F8 DNAzyme. The coffee ring effect<sup>32</sup> was observed when the droplet of DNAzyme/substrate solution was allowed to dry on the electrode under atmospheric conditions causing most of the F8 DNAzyme complex to concentrate in a ring around the edge of the sensing electrode (ESI, Fig. S6a†). Such an effect impairs the reproducibility of the sensor production, and we explored different strategies to avoid it. Finally, homogenous deposition of DNAzyme was achieved by drying deposited solution under a steady stream of nitrogen for 60 seconds (ESI, Fig. S6b†). Such uniform layer of DNAzyme was coated with PDA by exposing the surface to a basic solution of dopamine (5 mg  $\text{mL}^{-1}$  Dopamine HCl, 10 mM Tris, pH 8.5).<sup>33,34</sup> Significant darkening of the surface was observed after 120 min, which is attributed to the successful formation of a polydopamine film (ESI, Fig. S7†).

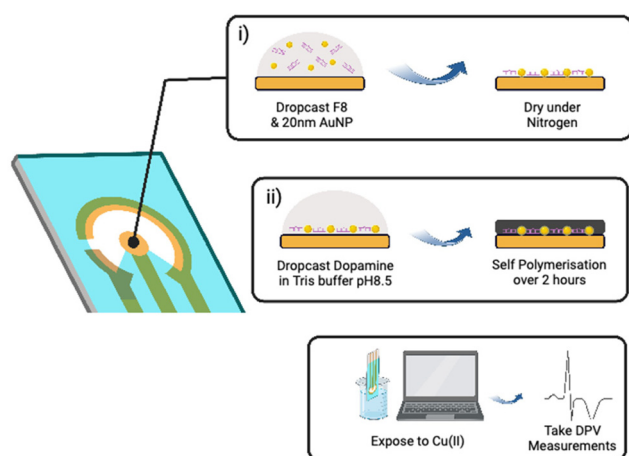


**Fig. 3** DNAzyme based electrochemical biosensor for  $\text{Cu(II)}$  is prepared by drop casting DNAzyme/substrate complex and rate enhancing Au NPs to the surface of electrode (i) followed by addition of dopamine and self-polymerisation resulting in PDA coating. (ii) Sensor is prepared within 2 hours after which  $\text{Cu(II)}$  detection can be performed using differential pulse voltammetry (DPV).

To confirm the formation of the coating, impedance spectroscopy measurements of the electrode were taken. Namely, PDA is known to be an electrical insulator and can cause the fouling of electrodes,<sup>35</sup> which results in increased impedance as observed with PDA-coated electrodes (ESI, Fig. S8†).

Once the deposition and coating were optimised, the electrochemical performance of the sensor was investigated using differential pulse voltammetry (DPV) before and 15 min after the exposure to  $\text{Cu(II)}$ . DPV was chosen as a read-out method due to its ability to perform fast measurements with high sensitivity.<sup>36</sup>

### 3.3 DNAzyme-based electrochemical detection of $\text{Cu(II)}$

The performance of the biosensor was first explored with F8 DNAzyme and two controls, using DPV measurements before and 15 min after exposure to 10  $\mu\text{M}$   $\text{Cu(II)}$  solution (Fig. 4a). The first control comprised of a non-enzymatic, linear strand W8, which was complementary to F8 substrate but did not contain DNAzyme features. The second control was simply an electrode coated with a PDA layer in the absence of F8

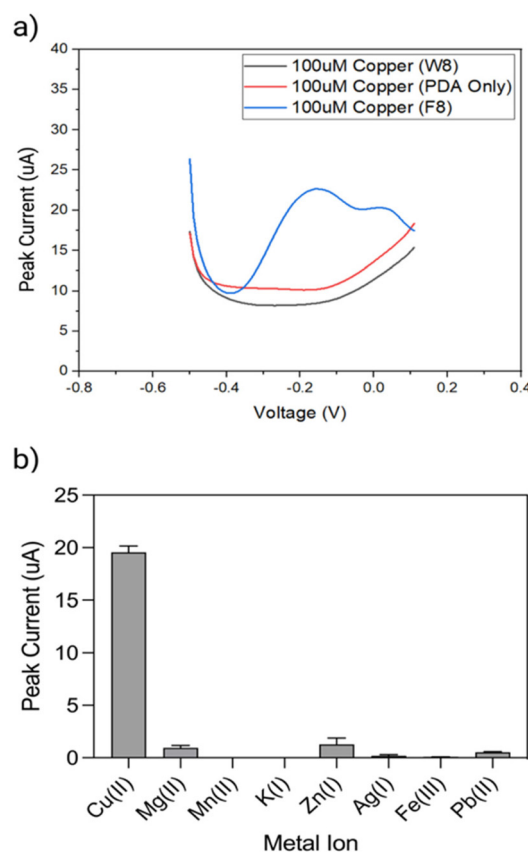

**Fig. 4** DPV response curves of polydopamine entrapped F8-DNAzyme electrode, polydopamine entrapped W8-DNA (non-enzymatic) electrode and polydopamine only electrode (a) in PBS with 10  $\mu\text{M}$   $\text{Cu(II)}$  after 15 min. (b) Peak current of DPV response curves for polydopamine entrapped F8-DNAzyme electrochemical sensor in 1 times PBS with 10  $\mu\text{M}$  of  $\text{Cu(II)}$ ,  $\text{Mg(II)}$ ,  $\text{Mn(II)}$ ,  $\text{K(I)}$ , and  $\text{Zn(II)}$ ,  $\text{Ag(I)}$ ,  $\text{Fe(III)}$ , and  $\text{Pb(II)}$  after 15 min.






DNAzyme. As it can be seen in Fig. 4a, two new cathodic current peaks are observed between  $-0.2$  to  $0$  V with DNAzyme coated electrode, which are not observed with control samples.

To explore the selectivity of F8-DNAzyme electrode towards  $\text{Cu(II)}$ , the electrode was exposed to solutions of other common ions such as  $\text{Mg(II)}$ ,  $\text{Mn(II)}$ ,  $\text{Zn(II)}$ , and  $\text{K(I)}$ , as well as the pollutants commonly found in soil and water such as  $\text{Fe(III)}$ ,  $\text{Pb(II)}$  and  $\text{Ag(I)}$  (Fig. 4b). No significant response was observed with those ions indicating high selectivity of our sensor towards  $\text{Cu(II)}$ .

Concerning the mechanism, we hypothesise that  $\text{Cu(II)}$  ions diffuse through the PDA layer into the active site of the DNAzyme (Fig. 5). The first cathodic peak can be attributed to the reduction of  $\text{Cu(II)}$  ions into  $\text{Cu(I)}$ , and the second one to  $\text{H}_2\text{O}_2$  produced by the PDA layer reacting with  $\text{Cu(I)}$  causing the cleavage of the substrate *via* an oxidative radical pathway. Such a mechanism is in line with the results presented here, although there is a possibility that other pathways might be involved.

In addition, the effect of Au NPs on the cleavage rate was evaluated first in the presence of small amount ( $0.01 \text{ mg mL}^{-1}$ ) of  $20 \text{ nm}$  Au NPs. DPV measurements employing PDA entrapped DNAzyme complex with and without citrate capped  $20 \text{ nm}$  Au NPs in  $\text{Cu(II)}$  solution are shown in ESI, Fig. S9.† It can be seen that inclusion of the Au NPs resulted in an increase of the peak current. In addition, there is no effect of Au NPs in absence of copper ions. This initial study clearly indicates that the addition of Au NPs to the DNAzyme solution further improves the performance of the sensor without impairing the  $\text{Cu(II)}$  selectivity. Current work is focused on exploiting this phenomenon further for the design of a sensitive  $\text{Cu(II)}$  sensor for blood screening.

Next, we investigated dependence of the peak current signal between the sensing range of  $-0.2$  to  $0.1 \text{ V}$  on the  $\text{Cu(II)}$  concentration. A clear increase in the peak current between a

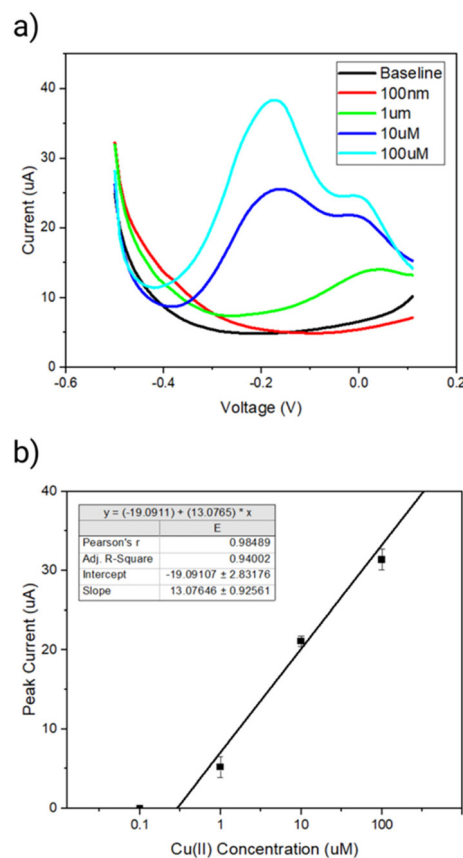


**Fig. 6** (a) DPV response curves for polydopamine entrapped F8 sensor in increasing concentrations of copper from  $0$  to  $100 \mu\text{M}$ . All measurements were taken in PBS after  $15 \text{ min}$  with stirring ( $100 \text{ rpm}$ ). (b) Peak current measured in sensing range of  $-0.4 \text{ V}$  to  $0.1 \text{ V}$  for different copper concentrations with a linear fit after subtracting a baseline taken in PBS only.

region of interest of  $-0.2$  to  $0.1 \text{ V}$  in presence of increasing concentration of  $\text{Cu(II)}$  was observed (Fig. 6a). The linear range of detection was found to be  $1 \mu\text{M}$  to  $100 \mu\text{M}$  copper over a sensing time of  $15 \text{ min}$  (Fig. 6b). The limit of detection was determined to be  $180 \text{ nM}$  ( $11 \text{ ppm}$ )  $\text{Cu(II)}$  using the slope of the concentration curve and a protocol reported by Armbruster *et al.*<sup>37</sup>

Finally, an often neglected but important factor when proposing a new biosensor device is its long-term stability. The stability of our PDA entrapped DNAzyme-based sensor was investigated over two months with the sensor stored under atmospheric conditions (ESI, Fig. S10†). A decay in the peak current was observed after two months, however, this could be improved by storage under dry and/or cold conditions and in the absence of light to minimise PDA and/or electrode degradation.

## 4. Conclusions

We have shown that the cleavage rate of a  $\text{Cu(II)}$ -specific DNA-cleaving DNAzyme can be significantly increased in the pres-

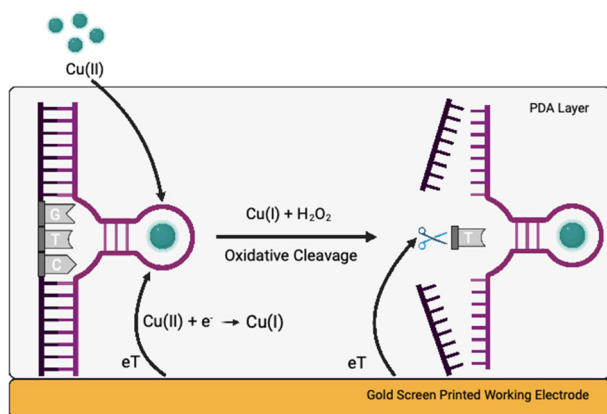

**Fig. 5** The proposed mechanism of action of the F8 DNAzyme-PDA electrode. Copper ions diffuse through PDA layer to the active site of F8 DNAzyme. Electron transfer occurs for the reduction reaction of  $\text{Cu(II)}$  to  $\text{Cu(I)}$ , which together with  $\text{H}_2\text{O}_2$  generated by PDA layer, results in oxidative cleavage of the substrate enabling further electron transfer to the electrode.



ence of citrate coated Au (5-fold enhancement in cleavage over 10 min) and polydopamine (PDA) nanoparticles (50-fold enhancement in cleavage over 10 min). Such an increase is directly related to the reducing potential of citrate ions in case the of Au NPs, and intrinsic H<sub>2</sub>O<sub>2</sub> production by PDA. Although their potential was acknowledged, DNazymes were generally considered too slow to have a huge practical value for metal sensor design. We have shown that nanoparticle additives have significant effect on the rate enhancement making DNazymes suitable for Cu(II) sensor design. Our electrochemical sensor is cost-effective and simple-to-make with Cu(II) limit of detection of 180 nM (11 ppm). The WHO guideline on the limit of Cu(II) in drinking water is given as 20 µM (1.3 mg ml<sup>-1</sup>) and the safe limit of copper in serum is regarded to be 2.4 µM.<sup>38</sup> As such, our sensor provides a cost effective and efficient alternative to other strategies for monitoring Cu(II) levels in drinking water and agricultural soil, as well as detection of Cu(II) in serum, and continuous monitoring of Cu(II) levels in large bioreactors.

## Author contributions

W. E. and L. F. contributed equally. They both conceptualised the project with the help of S. P. S. P. and W. E. performed research experiments. S. M., S. P. and S. Z. helped with experimental studies. F. B. and R. O. helped with critical comments, drafting, and revising the manuscript.

## Conflicts of interest

There are no conflicts to declare.

## Acknowledgements

This work was supported by EPSRC-Hitachi ICase PhD studentship Nr G105536 awarded to W. E. S. P. would like to thank EPSRC Sensor CDT and Cambridge International Trust and TRinity College-Henry Barlow Scholarship.

## References

- 1 N. Gan, *et al.*, DNzyme-Catalyzed Click Chemistry for Facilitated Immobilization of Redox Functionalities on Self-Assembled Monolayers, *J. Phys. Chem. C*, 2020, **124**, 19083–19090.
- 2 R. R. Breaker and G. F. Joyce, A DNA enzyme that cleaves RNA, *Chem. Biol.*, 1994, **1**, 223–229.
- 3 P.-J. J. Huang and J. Liu, An Ultrasensitive Light-up Cu<sup>2+</sup> Biosensor Using a New DNzyme Cleaving a Phosphorothioate-Modified Substrate, *Anal. Chem.*, 2016, **88**, 3341–3347.
- 4 K. Schlosser and Y. Li, Tracing Sequence Diversity Change of RNA-Cleaving Deoxyribozymes under Increasing Selection Pressure during in Vitro Selection, *Biochemistry*, 2004, **43**, 9695–9707.
- 5 R. Saran and J. Liu, A Silver DNzyme, *Anal. Chem.*, 2016, **88**, 4014–4020.
- 6 J. Li, In vitro selection and characterization of a highly efficient Zn(II)-dependent RNA-cleaving deoxyribozyme, *Nucleic Acids Res.*, 2000, **28**, 481–488.
- 7 R. R. Breaker and G. F. Joyce, A DNA enzyme with Mg<sup>2+</sup>-dependent RNA phosphoesterase activity, *Chem. Biol.*, 1995, **2**, 655–660.
- 8 A. K. Brown, J. Li, C. M.-B. Pavot and Y. Lu, A Lead-Dependent DNzyme with a Two-Step Mechanism, *Biochemistry*, 2003, **42**, 7152–7161.
- 9 R. Lontie, *Copper Proteins and Copper Enzymes*, CRC Press, 2018. DOI: [10.1201/9781351070911](https://doi.org/10.1201/9781351070911).
- 10 M. Jaishankar, T. Tseten, N. Anbalagan, B. B. Mathew and K. N. Beeregowda, Toxicity, mechanism and health effects of some heavy metals, *Interdiscip. Toxicol.*, 2014, **7**, 60–72.
- 11 H. Ali, E. Khan and M. A. Sajad, Phytoremediation of heavy metals—Concepts and applications, *Chemosphere*, 2013, **91**, 869–881.
- 12 Z. Shabbir, *et al.*, Copper uptake, essentiality, toxicity, detoxification and risk assessment in soil-plant environment, *Chemosphere*, 2020, **259**, 127436.
- 13 A. R. Mir, J. Pichtel and S. Hayat, Copper: uptake, toxicity and tolerance in plants and management of Cu-contaminated soil, *BioMetals*, 2021, **34**, 737–759.
- 14 L. Bat, S. Bilgin and A. Öztekin, Toxicity of copper on marine organisms from the Black Sea, *J. Coastal Life Med.*, 2017, **5**, 422–426.
- 15 G. W. Brian, The effects of heavy metals (other than mercury) on marine and estuarine organisms, *Proc. R. Soc. London, Ser. B*, 1971, **177**, 389–410.
- 16 Z. K. Mathys and A. R. White, Copper and Alzheimer's Disease, *Adv. Neurobiol.*, 2017, 199–216, DOI: [10.1007/978-3-319-60189-2\\_10](https://doi.org/10.1007/978-3-319-60189-2_10).
- 17 P. Ferenci, *et al.*, Diagnostic Value of Quantitative Hepatic Copper Determination in Patients With Wilson's Disease, *Clin. Gastroenterol. Hepatol.*, 2005, **3**, 811–818.
- 18 R. Eife, *et al.*, Chronic poisoning by copper in tap water: I. Copper intoxications with predominantly gastrointestinal symptoms, *Eur. J. Med. Res.*, 1999, **4**, 219–223.
- 19 M. Saleem, M. Rafiq, M. Hanif, M. A. Shaheen and S.-Y. Seo, A Brief Review on Fluorescent Copper Sensor Based on Conjugated Organic Dyes, *J. Fluoresc.*, 2018, **28**, 97–165.
- 20 L. Tang, X. Dai, X. Wen, D. Wu and Q. Zhang, A rhodamine-benzothiazole conjugated sensor for colorimetric, ratiometric and sequential recognition of copper(II) and sulfide in aqueous media, *Spectrochim. Acta, Part A*, 2015, **139**, 329–334.
- 21 X. Chen, *et al.*, New fluorescent and colorimetric chemosensors bearing rhodamine and binaphthyl groups for the detection of Cu<sup>2+</sup>, *Sens. Actuators, B*, 2009, **137**, 597–602.
- 22 P.-J. J. Huang and J. Liu, An Ultrasensitive Light-up Cu<sup>2+</sup> Biosensor Using a New DNzyme Cleaving a



- Phosphorothioate-Modified Substrate, *Anal. Chem.*, 2016, **88**, 3341–3347.
- 23 N. Carmi, L. A. Shultz and R. R. Breaker, In vitro selection of self-cleaving DNAs, *Chem. Biol.*, 1996, **3**, 1039–1046.
  - 24 R. Drouin, *et al.*, Cupric ion/ascorbate/hydrogen peroxide-induced DNA damage: DNA-bound copper ion primarily induces base modifications, *Free Radicals Biol. Med.*, 1996, **21**, 261–273.
  - 25 M. Wang, *et al.*, In vitro selection of DNA-cleaving deoxyribozyme with site-specific thymidine excision activity, *Nucleic Acids Res.*, 2014, **42**, 9262–9269.
  - 26 Y. Tan, *et al.*, An immobilization free DNAzyme based electrochemical biosensor for lead determination, *Analyst*, 2016, **141**, 1121–1126.
  - 27 K. Liu, K. S. Chen, D. Sen and H.-Z. Yu, Ultrasensitive detection of total copper with an electrochemical biosensor built on the in cis coupling of hexynyl CLICK-17 DNAzyme with azido self-assembled monolayers, *Electrochim. Acta*, 2021, **379**, 138125.
  - 28 A. Tyo, *et al.*, Development and Characterization of an Antimicrobial Polydopamine Coating for Conservation of Humpback Whales, *Front. Chem.*, 2019, **7**, 618.
  - 29 S. I. Nehme, L. Crocker and L. Fruk, Flavin-Conjugated Iron Oxide Nanoparticles as Enzyme-Inspired Photocatalysts for Azo Dye Degradation, *Catalysts*, 2020, **10**, 324.
  - 30 M. Raffi, *et al.*, Investigations into the antibacterial behavior of copper nanoparticles against Escherichia coli, *Ann. Microbiol.*, 2010, **60**, 75–80.
  - 31 A. Gao, Y.-R. Wang, X.-W. He and X.-B. Yin, An Electrochemical Hydrogen Peroxide Biosensor Based on Polydopamine-Entrapped G-Quadruplex-Hemin DNAzyme, *Chin. J. Anal. Chem.*, 2012, **40**, 1471–1476.
  - 32 R. D. Deegan, *et al.*, Capillary flow as the cause of ring stains from dried liquid drops, *Nature*, 1997, **389**, 827–829.
  - 33 A. B. Popov, *et al.*, Size-tuneable and immunocompatible polymer nanocarriers for drug delivery in pancreatic cancer, *Nanoscale*, 2022, **14**, 6656–6669.
  - 34 L. Crocker, *et al.*, Enzyme-inspired flavin–polydopamine as a biocompatible nanoparticle photocatalyst, *Nanoscale Horiz.*, 2019, **4**, 1318–1325.
  - 35 J. Szewczyk, D. Aguilar-Ferrer and E. Coy, Polydopamine films: Electrochemical growth and sensing applications, *Eur. Polym. J.*, 2022, **174**, 111346.
  - 36 B. J. Venton and D. J. DiScenza, Voltammetry, in *Electrochemistry for Bioanalysis*, Elsevier, 2020, pp. 27–50. DOI: [10.1016/B978-0-12-821203-5.00004-X](https://doi.org/10.1016/B978-0-12-821203-5.00004-X).
  - 37 D. A. Armbruster and T. Pry, Limit of blank, limit of detection and limit of quantitation, *Clin. Biochem. Rev.*, 2008, **29**(Suppl 1), S49–S52.
  - 38 G. J. Brewer, *Wilson's Disease*, Springer US, 2001. DOI: [10.1007/978-1-4615-1645-3](https://doi.org/10.1007/978-1-4615-1645-3).

