


JAAS

Journal of Analytical Atomic Spectrometry
rsc.li/jaas



ISSN 0267-9477

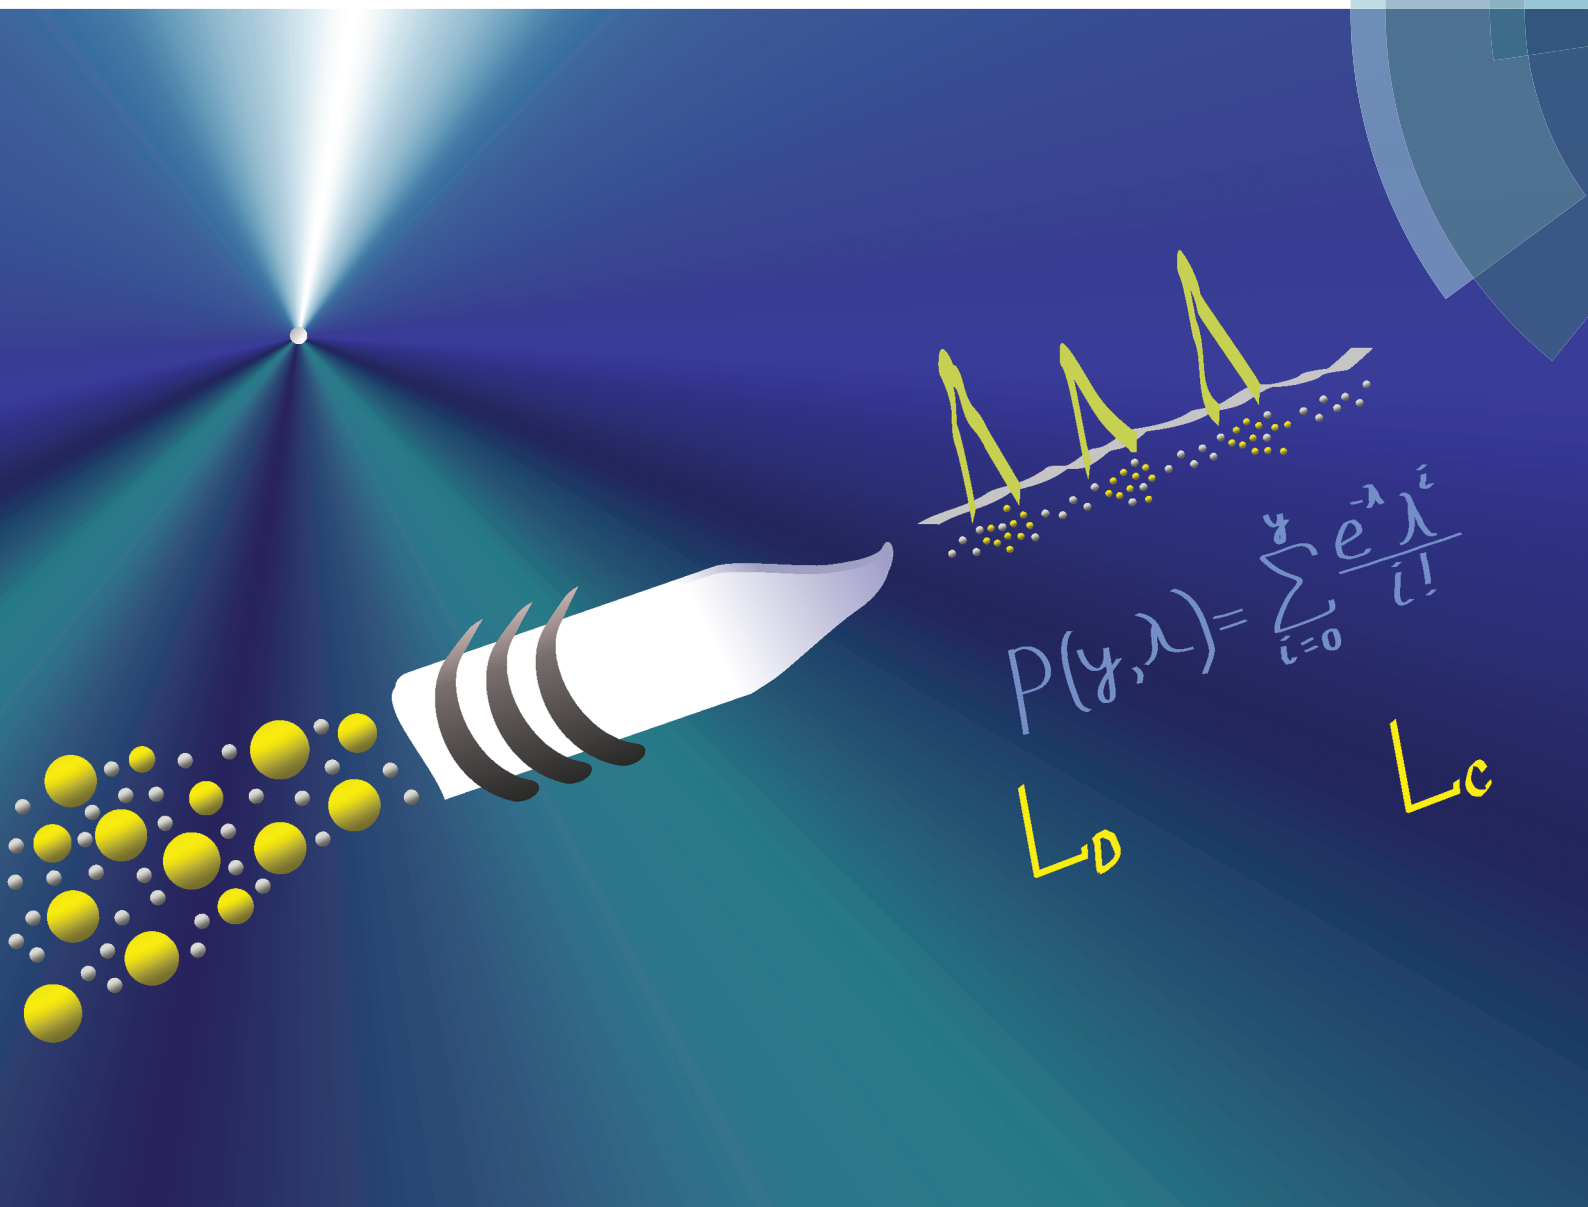

ROYAL SOCIETY
OF CHEMISTRY

Celebrating
IYPT 2019

PAPER

Darya Mozhayeva and Carsten Engelhard
A quantitative nanoparticle extraction method for
microsecond time resolved single-particle ICP-MS
data in the presence of a high background



Cite this: *J. Anal. At. Spectrom.*, 2019, **34**, 1571

A quantitative nanoparticle extraction method for microsecond time resolved single-particle ICP-MS data in the presence of a high background†‡

Darya Mozhayeva ^a and Carsten Engelhard ^{*ab}

The detection of nanoparticles (NPs) in the presence of a high background (BG) is challenging in single particle inductively coupled plasma mass spectrometry (SP-ICP-MS) and leads to inaccurate quantification. In this study, we report a data processing procedure for the deconvolution of SP-ICP-MS data and its application to quantification of both the Ag NP size distribution (20 to 100 nm Ag NPs) and the concentration of dissolved silver ions (Ag^+ up to $7.5 \mu\text{g L}^{-1}$) in mixtures using Poisson statistics to determine thresholds to identify the beginning and end of NP signal events. SP-ICP-MS with a microsecond time resolution data acquisition system (μsDAQ) and conventional pneumatic nebulization was used for the detection of Ag NPs in the presence of a significant concentration of ionic BG ($^{107}\text{Ag}^+$ up to 1 000 000 cps). In contrast to conventional three times standard deviation of the BG ($3 \times \text{SD}_{\text{BG}}$) decision criterion (normal distribution), our NP ion cloud extraction mechanism from the μsDAQ is based on setting thresholds to determine the beginning and the end of an ion cloud using Poisson statistics, which is suitable for the low count data. The algorithm was applied here for the flagging and detection of Ag NPs in the presence of Ag^+ . Critical level (false positive probability was set to 5%) and detection limit (false positive and false negative probabilities were set to 5%) based on Poisson distributions were implemented to determine the thresholds. A range of different sets of NP ion cloud extraction conditions were tested to verify the calculated thresholds and to obtain optimal extraction conditions at different BGs (Ag^+ concentration). The method can be universally applied for the detection of different elements with SP-ICP-MS.

Received 30th January 2019
Accepted 29th May 2019

DOI: 10.1039/c9ja00042a

rsc.li/jaas

Introduction

Manufactured nanomaterials (MNM)s are used increasingly in the modern society.¹ In the case of silver (Ag) NPs, the release of ionic silver (Ag^+) frequently leads to increased toxicity of this type of NP.^{2,3} However, even though a significant number of publications report on the mechanism of Ag NP toxicity, they might use NPs with different sizes, surface coatings and exposure media, and in different organisms/cell cultures; thus, it is still not clear to which degree toxicity stems from silver ions and NPs, respectively.⁴ Advanced analytical methods are required to assess the presence and the quantity of different silver species, especially at environmentally relevant concentrations. Centrifugal ultrafiltration and membrane filtration

require more detailed investigations and should be accounted for, the linear dynamic range of the pulse counting stage of the secondary electron multiplier (SEM) is limited, *etc.* Ideally, NPs can be distinguished from the BG as pulses, if the BG is low. Frequently, this is not the case, and BG increase hinders the detection of NPs, because of increased standard deviation (SD) of the BG; therefore, the detection limit (L_D) for NP size drastically deteriorates. Laborda *et al.* could detect Ag NPs of size from 40 to 80 nm (with a DT of 5 ms) in the presence of the Ag^+ BG below $1 \mu\text{g L}^{-1}$; however, the presence of already 300 ng L^{-1} of Ag^+ resulted in the increase of the calculated particle size L_D from 18 nm (in ultrapure water) to 32 nm (with 300 ng L^{-1} of Ag^+).¹² TiO_2 NPs could be distinguished from the continuous BG, where up to $0.5 \mu\text{g L}^{-1}$ of Ti(IV) was added.¹⁶ Schwertfeger *et al.* introduced an approach for NP and dissolved analyte quantification, where three dilutions were implemented for the detection of gold and silver NPs in the presence of the dissolved ions.¹⁷ First, the solution without any dilutions was measured to quantify the dissolved metal; afterwards, two dilutions were done for single NP measurements. Without the dilution, it was shown that the presence of already $1 \mu\text{g L}^{-1}$ of dissolved silver leads to errors (size overestimation and a lower number of particles detected) in the detection of 30 nm Ag NPs.

In conventional multi-elemental analysis with ICP quadrupole MS (ICP-Q-MS) a signal at a selected m/z is recorded for a certain DT (typically in the low to sub-millisecond range for NP detection and up to 1 s during homogeneous sample analysis). As NPs result in relatively short ion signal events in ICP-Q-MS (*e.g.* the ion signal duration for one 60 nm Ag NP was approximately 500 μs in our previous study),¹⁰ the choice of an appropriate DT is crucial to ensure a correct detection. The use of a DT on the microsecond time scale allows acquiring several data points per NP^{18–26} and helps to avoid incorrect detection, when *e.g.* one NP event is split between two DTs (split-particle event). An approach to use a 5 μs DT without a significant dead time (other than the SEM dead time) between consequent dwells was introduced by our group earlier.²⁶ When the prototype data acquisition system with 5 μs time resolution (μsDAQ) is used, the counts that would otherwise be counted in *e.g.* 3 ms are split into 600 dwells of 5 μs each; then, the counts detected per NP are summed up to get a signal reading per particle. This approach helps to minimize particle coincidence and split-particle events. Meanwhile, the BG is also split, and *e.g.* 100 000 cps of a constant BG signal would theoretically correspond to only 0.5 counts in 5 μs ; however, the counts that are recorded are positive integer numbers, so some of the readings would be 0 and others 1. This type of data should be described with a Poisson distribution, and not the Gaussian type. In this way, the low BG allows extending the concentration range of dissolved metals, in the presence of which NPs can still be detected and quantified. The data obtained with the μsDAQ are later processed to extract NPs with an optimized algorithm. In the algorithm, a NP event starts when a count value exceeds a certain threshold, and ends, when a second but lower threshold is reached.²⁶ However, there is a challenge: a high BG (*e.g.* 100 000 cps) can adversely influence the total counts per extracted NP ion cloud because

the BG is extracted together with the NPs and the extraction conditions (thresholds) have to be carefully selected. In addition, the ICP-MS user has to decide, which signal should still be counted as a signal from a NP and which signal should be counted as BG fluctuation when working at a low count level (a single 20 nm Ag

Experimental section

Sample preparation

Monodisperse spherical Ag NPs with nominal diameters of 20, 40, 60, and 100 nm with a citrate coating and an initial concentration of 0.020 g L^{-1} were bought from nanoComposix (San Diego, CA, USA). The diameters of the NPs determined by transmission electron microscopy (TEM) by the manufacturer were 18.5 ± 3.4 , 39 ± 4 , 62 ± 7 , and 98 ± 10 nm, respectively. The suspensions were preserved at 4°C in darkness before analyses and manually shaken for 30 s prior dilution. No data were provided by the manufacturer on the content of silver ions in the suspensions. Dilutions were done with bi-distilled deionized water directly prior the analyses to achieve a PNC of approximately $2.5 \times 10^5 \text{ NP mL}^{-1}$. Ag^+ solution ($999 \pm 5 \text{ mg L}^{-1}$, Inorganic Ventures, Christiansburg, VA, USA) was diluted for external calibration and added to NP suspensions with nine different concentrations from 10 ng L^{-1} to $7.5 \mu\text{g L}^{-1}$ (with experimental dilution uncertainty). NaNO_3 ($\geq 99\%$, analytical reagent grade, Carl Roth GmbH, Karlsruhe, Germany) and HNO_3 (70%, analytical reagent grade, Fisher Scientific, Loughborough, UK) were used for the matrix modification of bi-distilled water.

Instrumentation

All measurements were done on a model ICAP Qc (Thermo Fisher Scientific, Bremen, Germany) ICP-Q-MS instrument. The instrument was controlled by using Qtegra ISDS software (2.4.1800.192, Thermo Fisher Scientific). The ICP-Q-MS was equipped with a model ESI SC-2 DX autosampler (ESI Elemental Service & Instruments GmbH, Mainz, Germany), a model MicroFlow PFA-50 nebulizer (Thermo Fisher Scientific, Bremen, Germany) with a self-aspiration flow rate of around $65 \mu\text{L min}^{-1}$ at 1 L min^{-1} Ar (manufacturers' data), and a Peltier-cooled cyclonic quartz spray chamber held at 3°C . A second roughing pump (Sogevac SV40 BI, Leybold Vacuum Cologne, Germany) allowed achieving a lower interface pressure of $1.36 \pm 0.02 \text{ mbar}$, and together with a high sensitivity skimmer insert (insert "2.8", Glass Expansion, Melbourne, Australia), nickel cones helped to increase the sensitivity of the instrument. The main instrumental parameters of the ICP-MS are presented in Table 1.

Table 1 ICP-MS instrumental parameters

Parameter	Value
RF power	1450 W
Ar cooling gas flow	14 L min^{-1}
Ar auxiliary gas flow	0.8 L min^{-1}
Ar nebulizer flow	0.6 L min^{-1}
Sampling position	2 mm
Skimmer type	Ni (insert version)
Insert type	Skimmer cone insert "2.8"
Torch injector inner diameter	1 mm
Dwell time for the $\mu\text{sDAQ$	

number of NPs per 3 min run was always higher than 3500 for 40, 60, and 100 nm NPs. The number of detected NPs was considered to be sufficient to construct a size distribution with statistical significance (also because the determination of PNC was not the goal of the study). External size calibration was made daily with 20, 40, 60, and 100 nm Ag NPs without addition of dissolved silver. To have a starting point for the investigation of the influence of the extraction conditions on the calculated NP size external size calibration has been performed under $S = 5$, $T = 5$, and $E = 1$ extraction conditions (when 5 counts ($T = 5$) were detected in 25 μs ($S = 5$) an ion cloud starts and when there was only 1 count ($E = 1$) in 25 μs , the ion cloud ends). These values were calculated using the formulas from Table 2, when the average BG is low (see Table 3 and further sections for details). The BG was subtracted, and the linear fit resulted in $R^2 = 0.996 \pm 0.002$ based on the sizes provided by the manufacturer. A high correlation coefficient is the evidence of the stability of the NPs in the suspensions. After size calibration and BG subtraction, the size distribution diagrams were constructed by binning the data into 2 nm bins. Fitting of all obtained size distributions was performed with a Gaussian model. This allows us to easily compare the maxima of the distributions, which is not always straightforward with other fitting models (e.g. Poisson distribution). In this study, different criteria including the BG maximum, mean NP size, width of the size distribution, total number of detected NPs, and size starting from which the NP size distribution can be distinguished obtained from the constructed size distributions were used to compare different extraction conditions (see the ESI and Fig. S1†).

Results and discussion

Quantification of ionic silver in the presence of NPs with millisecond time resolution

The goal of this study is to develop a method that is capable of determining both the concentration of dissolved metal and the NP size. First, the possibility to quantify ionic silver in the presence of NPs was evaluated. The quantification of Ag^+ in solution was performed with ICP-Q-MS and 10 ms DT. L_D ($3.29 \times \text{SD}_{\text{BG}}$) calculated from ionic standard analysis was $16 \pm 2 \text{ ng L}^{-1}$, and the limit of quantification (L_Q) ($10 \times \text{SD}_{\text{BG}}$) was $47 \pm 6 \text{ ng L}^{-1}$. The data obtained with the μsDAQ could also be used for the quantification of the BG signal; however, the data processing would take a lot of time. Each 3 min measurement results in 3.6×10^7 data points, and this number of data points could not be visualized with the software available to us nowadays (limited to only a few millions of data points). Thus, data with millisecond time resolution were used to determine the BGs throughout this study. The BGs obtained with 10 ms DT in counts per second were recalculated to average BGs in 5 and 25 μs in order to be used in the further data evaluation. Computers with more computational power and software able to handle more input data will make the extraction of the average BG from the microsecond time resolution data much faster in the future.

Matrix effects in the plasma

In order to verify that the BG obtained in the presence of NPs corresponds to the concentration of Ag^+ in the suspension, the mean BG signal obtained with 10 ms DT for Ag^+ in the presence of Ag NPs of different diameters was compared with the mean BG signal obtained from Ag^+ calibration solutions at different concentrations (Fig. 1). The mean BG signal was found to be typically higher in the presence of NPs compared to the mean BG signal from a neat $\text{Ag}^$

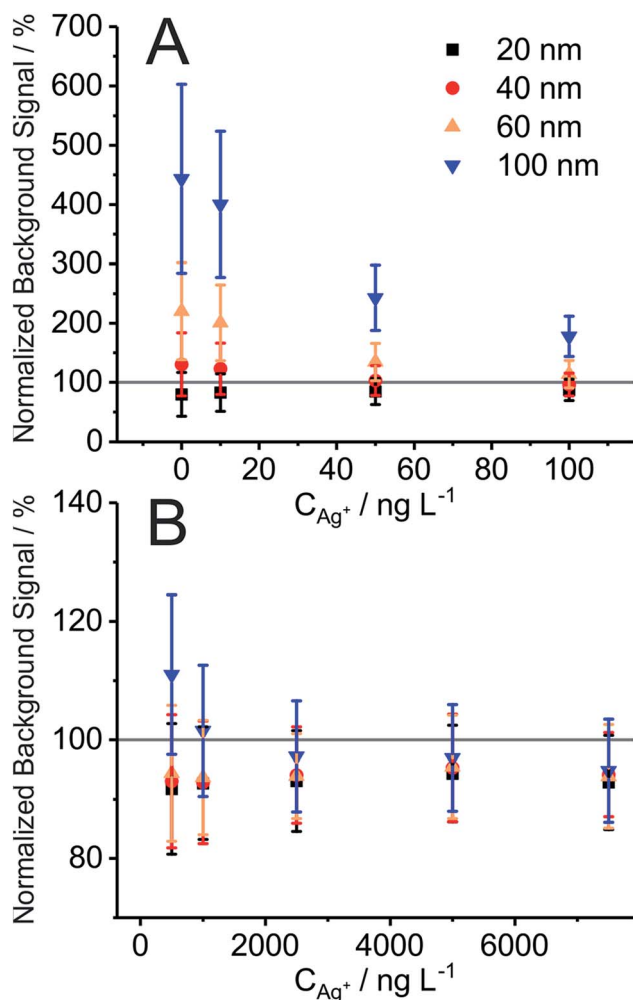


Fig. 1 Mean background (BG) signal (recorded with ICP-Q-MS at $^{107}\text{Ag}^+$, 10 ms DT) in the 20, 40, 60, and 100 nm Ag NP suspensions ($n = 3$, different sample measurements on three different days) after the addition of Ag^+ from 0 ng L^{-1} to 100 ng L^{-1} (A) and from 500 ng L^{-1} to 7.5 $\mu\text{g L}^{-1}$ (B) relative to the mean BG signal of Ag^+ calibration solutions without NPs. "Normalized background signal" represents the ratio of the mean BG signal, when Ag^+ was added to the NP suspension at different concentrations divided by the mean BG signal of Ag^+ calibration solutions of the same concentration but without NPs, in percent. A value of 100% would indicate that the BG counts obtained with and without NPs in solutions are equal.

BG signal were used below the saturation level of the used SEM. A future study on potential NP matrix effects in SP-ICP-MS with microsecond time resolution and a study on how to expand the upper level of the linear dynamic range in SP-ICP-MS are planned to further understand these observations in more detail.

BG correction for NP signals recorded with microsecond time resolution (μsDAQ)

As the total signal of an ion cloud is the sum of the extracted counts, it is important to compensate for any BG influence to achieve a more precise sizing. To avoid an artificial NP size increase, we propose a BG subtraction mechanism, where the BG is subtracted mathematically from each extracted ion cloud,

taking into the account the specific durations of each ion cloud with the following formula:

$$S_{\text{cor},i} = S_i - D_i \times \text{BG}_{5\ \mu\text{s}} \quad (1)$$

where $S_{\text{cor},i}$ is the corrected signal of an ion cloud, S_i is the non-corrected signal of an ion cloud, D_i is the duration of the ion cloud (expressed in number of extracted data points), and $\text{BG}_{5\ \mu\text{s}}$ is the BG per 5 μs . In this study, this BG value was recalculated from the BG obtained with the vendor software for the same measurement. The BG correction was implemented to all data used in this study.

After data processing with the BG subtraction (eqn (1)), the BG corrected Ag NP sizes in the presence of ionic silver were found to be in better agreement with Ag NP reference values (sizes obtained from suspensions without an

fluctuations. As it was not feasible in the current study to get an average BG from 5 μs resolved data due to a high number of data points and limitations in the software, the BG was obtained from data acquired with 10 ms DT and then recalculated (discussed above) to match shorter DTs. After a recalculation to 25 μs ($S = 5$), the BG is typically only between fractions of a count and 32 counts. In this case, a normal distribution, which was assumed for the conventional L_D formula derivation, does not apply anymore, and a Poisson distribution can be used instead.³⁴ Three main criteria determine the Poisson distribution:

- The values are positive integer numbers, which is the case for the μsDAQ .
- If a time interval tends to zero, then also the probability to get a count tends to zero, which is also true for the NP detection, as the detection occurs at discrete time intervals.
- A value x_n does not depend on the next value x_{n+1} . In order to achieve this condition, there should be only one data point detected per NP, which is not the case for the μsDAQ . As a NP represents a profile of data points, each data point is not independent.

In order to determine the L_D for an ion cloud, the ion cloud extraction process should be considered. To fulfil all three criteria of the Poisson distribution, especially the third criterion, we can consider only the beginning of an ion cloud,

namely the T threshold value (an ion cloud starts when the value is reached), so the decision for the detection of an ion cloud would depend only on the rising edge of the ion cloud count profile. Consequently, the L_D calculation for a low number of counts in the Poisson distribution has to be found. As in the ion cloud extraction process one of the conditions is that $T > E$ (when $T = E$, the algorithm would go to a loop), we propose to use L_C to determine the end of an ion cloud. Thus, the T parameter should be above L_D ($\alpha \leq 5\%$, $\beta \leq 5\%$), and the E parameter should be equal to L_C ($\alpha \leq 5\%$). Cases of a low number of counts are often found in radiochemistry; and Currie³⁴ treated the Poisson distribution under an assumption of a normal distribution, “if the number of counts is sufficiently large”. The L_D formulas for the Poisson distribution (with the assumption of a normal distribution) were determined for two cases: paired observations and well-known blank (where the deviations of the BG are neglected).³⁴ Later, the paper was extended³⁵ in order to address the issue of “very low-level counting data” below 5 counts. The initial paper and a more recent summary³⁶ presented a table based on the calculations using a cumulative exact Poisson distribution (without Gaussian approximation), a well-known blank; $\alpha \leq 5\%$ and $\beta \leq 5\%$ for L_D ($\alpha \leq 5\%$ for L_C). Formulae and example calculations for the exact Poisson distribution to determine L_D and L_C are presented in the ESI and Table S1.† It should be noted that for the Poisson distribution, L_Q should be above 100 counts; therefore, this parameter was not considered in the calculations.

For a user friendly calculation of L_D and L_C , we propose to use the formulas that are presented in Table 2 (Poisson distribution with the normal distribution approximation). The values obtained from the cumulative exact Poisson distributions were compared (Table 3) with the values obtained for the Poisson distribution with normality approximation, where only an average BG (μ_B) is sufficient to conduct the calculations (Table 2).³⁴ In the formula of paired

paired observations (Table 2) can be used as an approximation for the BG below 5 counts, and the “well-known” blank formula can be used for the BG above 5 counts. According to this approximation, the difference between the values obtained with the cumulative Poisson distribution and the normality approximated values was below 1 count (only two values of L_D differed less than 2 counts, with the higher values obtained for the normality approximation). In practice, false positives and false negatives can still be separated from the NP events, since the size distribution diagram is constructed, and the remaining BG can still be distinguished from the NPs by the $3.29 \times SD_{BG}$ criterion.

In order to get the ion cloud extraction parameters E and T , μ_B should be added to the obtained L_C and L_D to obtain the corresponding gross counts (y_C and y_D). It should be noted that only positive integer numbers are used in the ion cloud extraction, since only integer counts are detected; thus, the obtained non-integers can be rounded to the closest integer number to obtain the suitable ion cloud extraction conditions. In the next section, the hypothesis of using L_C and L_D for NP ion cloud extraction will be tested in detail.

Optimization of the ion cloud extraction conditions

Different ion cloud extraction conditions below and above L_C and L_D were chosen to study their effect on the obtained NP size distributions. It is noted here that 20 nm sized Ag NPs could only be partially separated from the BG in the count histogram. The size L_D was at least 16 nm ($S = 5$, $T = 5$, and $E = 1$) (Table S2†); therefore, 20 nm Ag NPs do not follow the same trends that were observed with 40, 60, and 100 nm sized Ag NPs (discussed below). All other tested NP size distributions could be separated from the BG even in the presence of ionic silver up to 1 000 000 cps, which is a significant improvement compared to the data obtained with 10 ms DT due to the high time resolution in SP-ICP-MS.

Fig. 2 and S2† show average calculated NP sizes (label B in Fig. S1†) obtained under different extraction conditions without an addition of dissolved silver (Fig. 2) and with the addition of $7.5 \mu\text{g L}^{-1}$ of Ag^+ (Fig. S2†). In general, the main trends are very similar, and the obtained sizes are more or less independent of the T parameter and change dependent on the E parameter. Lower E results in higher sizes, since more counts are added in the end of ion clouds and higher E results in lower sizes. No specific trends were found for the changes in the width of the NP size distributions (label C in Fig. S1†) under varying extraction conditions. The obtained NP sizes do not change to a large degree under the varied extraction conditions: maximum deviation is up to 4.7 nm for 40 nm, up to 2.1 nm for 60 nm, and up to 1.0 nm for 100 nm Ag NPs (Fig. 2 and S2†). Considering the trends from Fig. 2 and S2†, T and E parameters can be chosen from the proposed L_C and L_D calculations (Table 2).

The number of detected particles (label E in Fig. S1†) is an important parameter in quantitative SP-ICP-MS applications and was, therefore, used here to identify suitable ion cloud extraction conditions (Fig. S3 and S4†). It was found that there was a significant difference in the number of detected particles in the case of 20 nm sized Ag NPs with the change of extraction

conditions; however, this happens because they could not completely be separated from the BG. The trends are more difficult to follow (Fig. S3 and S4†), with the number of detected N

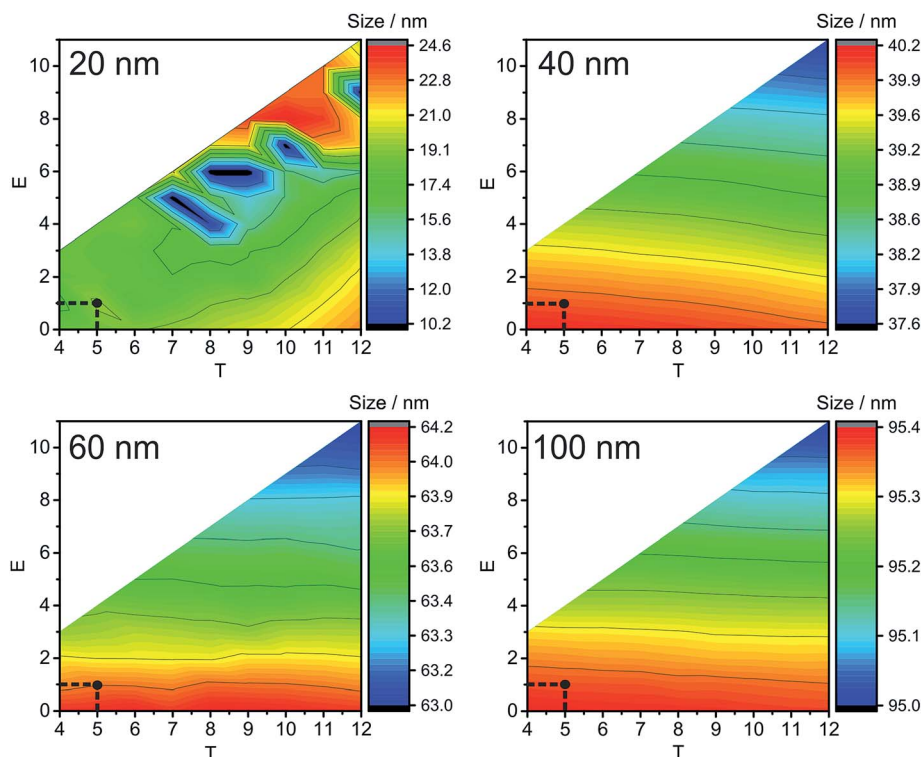


Fig. 2 Average sizes of 20, 40, 60, and 100 nm Ag NP size distributions (without addition of Ag^+ , $0 \mu\text{g L}^{-1}$, to the NP suspension) depending on different count thresholds during ion cloud extraction (T – number of counts required to flag ion cloud start and E – number of counts to define the end of ion cloud extraction). Optimal conditions ($S = 5$, $T = 5$, and $E = 1$) are highlighted with black dots. Note: the step size in size resolution is for illustrative purposes only and is a result of data processing. It does not represent the actual size resolution of the SP-ICP-MS method. Also, areas of white colour indicate extraction conditions, which were not tested.

beginning and end of NP signal events. Higher BG signals were not tested because of the use of the SEM in the counting mode. The principle of the data processing algorithm can be extended to different types of NPs, to the detection of different elements, or to NPs containing a high natural or instrumental BG. The method allows quantifying NPs in a wider range of the BG signal, compared to conventional SP-ICP-MS with a millisecond DT.

In order to determine the concentration of dissolved metal in the presence of NPs and to assess the NP size distribution the following steps are proposed:

- Perform a calibration with dissolved metal with a millisecond DT (*e.g.* 10 ms). This is done in order to ascertain the concentration of dissolved metal in the mixture, taking into account possible matrix effects.
- Construct the signal distribution after sample analysis to determine the average BG. It represents the dissolved metal concentration.
- In order to determine the NP size distribution, extract the NP ion clouds from the data obtained with the μsDAQ . This is done by setting thresholds (S , T , and E), and the threshold

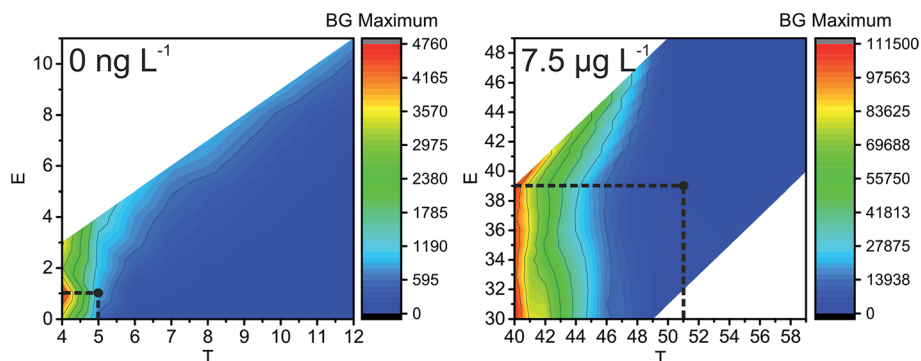


Fig. 3 Influence of ion cloud extraction conditions on the maximum of the number of BG events (BG count distribution maximum, see label A in Fig. S1†) during the analysis of 60 nm Ag NPs (left: without and right: with $7.5 \mu\text{g L}^{-1}$ Ag^+ added to the NP suspension). Optimal conditions are highlighted with black dots. Note: the step size in size resolution is for illustrative purposes only and a result of data processing. It does not represent the actual size resolution of the SP-ICP-MS method. Also, areas of white colour indicate extraction conditions, which were not tested.

typically increase with the increasing BG signal. The thresholds can be calculated using the average BG obtained from the vendor software from the cumulative Poisson distribution or with the normality approximation (Table 2). The ion cloud beginning threshold (T) may be increased by 4–5 counts to decrease the BG further.

- Subtract the average BG from each ion cloud to obtain more precise sizing information.
- Construct the size distribution based on the NP size calibration.

Conclusions

A data processing procedure was developed for SP-ICP-MS with microsecond time resolution (μ sDAQ) to determine both the concentration of dissolved metal and NP sizes in a mixture using Poisson statistics to determine thresholds to identify the beginning and end of NP signal events. Possible matrix effects were discussed, and a BG subtraction procedure was developed in order to obtain more precise quantitative information on the NPs. Data acquired with a millisecond DT were used to determine the average BG, which is related to the concentration of the dissolved ionic species. Data acquired with the μ sDAQ were used for the characterization of NPs. NPs were extracted based on thresholds, which were related to quantitative limits (L_C and L_D) for the Poisson distribution to get probability theory based NP ion cloud extraction from the raw data. Different extraction condition combinations were tested and used to verify the use of L_C and L_D for NP ion cloud extraction. The developed method is based on Ag NP detection, but it can be universally used with NPs containing elements detectable by ICP-MS, a high natural BG or high dissolved ion concentration; it can also be used for environmental samples or NP production quality control.

Conflicts of interest

There are no conflicts to declare. The manuscript was written through contributions of all authors. All authors have given approval to the final version of the manuscript. The authors declare no competing financial interest.

Acknowledgements

Funding within the project FENOMENO (Grant No. 03XP0005) is acknowledged. FENOMENO is funded in the FP7 ERA-NET on Nanosafety: Safe Implementation of Innovative Nanoscience and Nanotechnology (SIINN) (<http://www.siinn.eu/en/>). We also acknowledge the House of Young Talents of the University of Siegen for providing funding for Darya Mozhayeva. Ingo Strenge is gratefully acknowledged for his work on the prototype data acquisition system for ICP-MS and the extraction tool. Johannes Schmitt is gratefully acknowledged for the programming support. The machine shop team (especially Markus Rabe for help with the ICP-MS) in the Department of Chemistry and Biology of the University of Siegen is gratefully acknowledged.

References

- 1 S. P. Forster, S. Oliveira and S. Seeger, *Int. J. Nanotechnol.*, 2011, **8**, 592–613.
- 2 D. A. Notter, D. M. Mitrano and B. Nowack, *Environ. Toxicol. Chem.*, 2014, **33**, 2733–2739.
- 3 M. H. Shen, X. X. Zhou, X. Y. Yang, J. B. Chao, R. Liu and J. F. Liu, *Sci. Rep.*, 2015, **5**, 9674.
- 4 D. Mc

- 27 F. Laborda, J. Jiménez-Lamana, E. Bolea and J. R. Castillo, *J. Anal. At. Spectrom.*, 2013, **28**, 1220–1232.
- 28 G. Cornelis and M. Hassellöv, *J. Anal. At. Spectrom.*, 2014, **29**, 134–144.
- 29 A. Gundlach-Graham, L. Hendriks, K. Mehrabi and D. Günther, *Anal. Chem.*, 2018, **90**, 11847–11855.
- 30 S. Bazargan and H. Badii, Systems and methods for automated analysis of output in single particle inductively coupled plasma mass spectrometry and similar data sets, *US Pat.*, US9754774B2, 2017.
- 31 G. C. Y. Chan and G. M. Hieftje, *Spectrochim. Acta, Part B*, 2016, **121**, 55–66.
- 32 A. Murtazin, S. Groh and K. Niemax, *Spectrochim. Acta, Part B*, 2012, **67**, 3–16.
- 33 H. Kaiser, *Spectrochim. Acta*, 1947, **3**, 40–67.
- 34 L. A. Currie, *Anal. Chem.*, 1968, **40**, 586–593.
- 35 L. A. Currie, *IEEE Trans. Nucl. Sci.*, 1972, **19**, 119–126.
- 36 L. A. Currie, *J. Radioanal. Nucl. Chem.*, 2008, **276**, 285–297.

