

REVIEW

[View Article Online](#)
[View Journal](#) | [View Issue](#)

Cite this: *Mater. Adv.*, 2024,
5, 3563

Received 17th November 2023,
Accepted 19th March 2024

DOI: 10.1039/d3ma01019h

rsc.li/materials-advances

Paper-based sustainable biosensors

Anuj Kumar* and Pralay Maiti

Sustainability is the priority of the research community in designing and manufacturing value-added products, including biosensing devices. In this case, the utilization of paper and cellulose-based fibrous materials has been widely explored for developing biosensing devices in the past decade due to their high versatility, adaptability, biodegradability, and low cost. Recently, paper-based multifunctional biosensing devices have been developed for a sustainable future in a variety of applications such as the healthcare, agriculture, food safety and security, and environmental fields. However, there are still various technological and environmental issues that need to be overcome for manufacturing the desired biosensors. In this review, we provide the precise fundamentals of biosensing concepts, sustainable materials, and their utilization in developing paper-based sustainable biosensing devices for different healthcare, agriculture, food industry, environmental, and other applications. Moreover, the challenges, opportunities, and future perspectives regarding the use of these sustainable materials, together with their economic and advanced technological features are presented.

1. Introduction

Sensing devices are analytical tools employed to monitor analytes linked to environmental pollution, human diseases, food safety and security, and human-machine interactions. The

extensive research and utilization of these devices have remarkably increased in the past few decades^{1,2} owing to their simplicity, cheap reagents, and flexibility for on-site detection.^{3,4} Herein, compared to micro-materials, the use of nanoengineered materials can enhance the recognition of distinct analytes at a very low content due to their high surface area-to-volume ratio and specific functional mechanisms to facilitate the efficient recognition of chemical and/or biological species. Among the variety of available materials for developing sensing

School of Materials Science and Technology, Indian Institute of Technology (BHU), Varanasi 221005, Uttar Pradesh, India. E-mail: anuj.mst@itbhu.ac.in, anuj.budhera@gmail.com



Anuj Kumar

Anuj Kumar is a DBT-Ramalingaswami Faculty at the School of Materials Science and Technology, IIT-BHU, Varanasi (India) since April 2023. Prior to this position, he was an Assistant Professor (Polymers & Biomaterials), BK21 (Four)-participating Professor, and Postdoc at the School of Chemical Engineering at Yeungnam University (South Korea) and Assistant Professor (Chemistry) at DIT University (India). He received his PhD, MTech, and MSc from IIT Roorkee, IIT Delhi, and CCSU Meerut (India), respectively. His research interests are focused on polymers, biomaterials, 3D bioprinting, micro-fluidics, tissue engineering, drug delivery, cancer therapy, cultured meat production, flexible and wearable bioelectronics, etc.



Pralay Maiti

Pralay Maiti is a Senior Professor in the School of Materials Science and Technology, IIT-BHU, Varanasi (India). He received his PhD in Polymer from IACS (Jadavpur University) and MSc from IIT Kharagpur. Prior to this position, he was a Quick Hire Fellow at CLRI, Chennai, Visiting Scientist at Cornell University (USA), Postdoc at Toyota Technological Institute, and COE Researcher/Lecturer at Venture Business Laboratory, Hiroshima University (Japan). His current research interests include drug delivery vehicles, biomaterials and energy materials. He has published more than 230 papers in reputed journals, 29 patents, and 28 book chapters, with an h-index of 51 and more than 14 000 citations.



devices, great efforts have been devoted to employing natural polymers as substrates or even as components of the active layer in sensors^{5–8} to realize sustainable and/or biocompatible sensing devices by avoiding non-renewable and hazardous/toxic elements. In this case, cellulose materials and/or nanomaterials have been considered as potential components of sensors and biosensors. Therefore, the use of paper and nanopaper as substrates to fabricate electrodes and substituting conventional glass- or plastic-based materials with low-cost and disposable materials is highly desirable.

In this trend, standard paper has widely been utilized in the field of printed sensors, pursuing the upgrades advanced by the simple loading and delivery of reagents in the 3D cellulosic-network, ability to operate using very low volume of reagents and sample amounts, pores and channels of the substrate for avoiding interference of the components, and microfluidic patterns with no requirement of micropumps for flow initiation and avoiding bubble formation.^{9,10} Moreover, natural materials including nanocellulose materials provide interesting benefits in developing nanopaper-based sensors and biosensors, resulting in inexpensive, consistent, sustainable, disposable, and reagent-free tools for use in the monitoring of food quality and safety.^{9,11} Also, they provide the opportunity for the successful immobilization of various biological components to develop biocompatible and nontoxic biosensors.^{10–12} Moreover, paper (cellulose and nitrocellulose) is an appropriate substrate for a range of applications, including sensors for environmental and healthcare monitoring.¹³ Paper has been utilized passively in various analytical applications (*e.g.*, pH indicator strips, pregnancy tests, and rapid Covid-19 antigen tests).¹⁴ Accordingly, it has been utilized in many other applications including electronic and electrochemical devices due to its inexpensive nature, flexibility, fluid conduct (capillary action due to rough fibrous-network), significant sensitivity and easy disposal.^{15,16} Therefore, different electroactive elements can easily be detected by using paper-based sensor devices such as ions,¹⁷ dopamine,¹⁸ and biomarkers,¹⁹ together with their easily disposal. In this advancement, the fabrication of multifunctional paper-based biosensors to detect multiple parameters using only one physical input is highly desirable.

Presently, artificial intelligence (AI) and wearable sensors/biosensors have become two important areas to realize the tailoring of the best precision medicine therapies for individual patients. Therefore, the integration of AI and biosensing devices can potentially enable the better acquisition of patient data and enhance the design of wearable and implantable biosensing devices to monitor the fitness, health, and surroundings of patients. However, AI-biosensors with suitable practical characteristics encounter new opportunities and challenges. In this case, the innovations in materials, biorecognition components, signal acquisition and transport, data processing and intelligent decision system are the essential factors. Further, integration, slimness, miniaturization, and low energy utilization are the upcoming prospects of AI-biosensors for human healthcare. To this end, more technological advances are needed to detect low levels of specific

biomarkers in biofluids and the achieve system integration. Herein, biomarkers must channel the cavity between biophysical and biochemical markers to prepare all-inclusive prototypes for individuals. Moreover, great efforts need to be devoted to developing flexible electronic materials integrated with chip technology, the Internet of Things, huge data, and AI to accomplish the collective functioning of AI-biosensors, wherein the accumulated data is consumed by machine learning algorithms to monitor crucial signs, spot abnormalities and track therapies for further correlated interactions at the human-machine interface.²⁰

2. Biosensors

Sensors are devices that respond to stimuli and detect the events or changes in a specific environment and communicate the information to other interconnected technical devices (*e.g.*, computer system). Various physical and chemical characteristics (*e.g.*, odor, pressure, force, temperature, and pH) of any compound are measured and detected by these sensors and their associated interfaces in the presence of special chemical moieties. The moieties are solely sensitive to the targeted physical or chemical quantity for measurement (insensitive to all other parameters) and do not influence the characteristics of the input physical and/or chemical quantities. Therefore, important features such as selectivity, sensitivity, accuracy, calibration scope, resolution, repeatability, and cost-effectiveness are important factors in the selection of sensor systems.^{21,22} Moreover, sensors can be grouped broadly into two types, physical and chemical sensors. Physical sensor devices detect and/or quantify responses such as force, temperature, absorbance, refractive index, mass change, conductivity, and magnetic field.²³ Alternatively, chemical sensing devices have a chemically selective interface (layer) that responds selectively to a distinct analyte²⁴ and provides chemical reaction information (with analyte) or physical characteristic of the system being probed. For example, the content of certain constituents or probing the total composition (being transformed into signals such as changes in conductance, light, current, voltage, and sound effects). The operating principles of physical and chemical sensors are remarkably different. Most physical sensors are direct and only affected by a few parameters, whereas the signals from chemical sensors may be affected by various parameters. In this way, chemical sensors have attracted greater attention in broad commercial applications such as industrial, environmental, agricultural, and clinical fields.^{22,25}

Biosensors are sensors or a type of chemical sensor composed of a biological molecule as the recognition component. Therefore, biosensors are classified as analytical devices containing biological or biological-derived sensing components either unified within or closely linked with physicochemical transducers for the recognition of analytes.^{26,27} In the past, different biologically derived substances such as enzymes, nucleic acids, antigen-antibodies, cells, and microorganisms





Fig. 1 Schematic illustration of a biosensing device, which is comprised of a bioreceptor, transducer, and amplifier.⁴²

were included in various mechanical, electrochemical, optical, and acoustic detectors to develop biosensing devices with high selectivity and sensitivity.^{28,29} The first biosensor, as an amperometric oxygen electrochemical sensor, was originally established in 1962³⁰ using glucose oxidase to detect the content of glucose. However, the term “biosensor” was proposed in 1977 by Rechnitz *et al.*³¹ using an arginine selective electrode (living organisms) as the recognition element.

Biosensors should be highly responsive, free of physical constraints (*e.g.*, pH and temperature), and reusable. Biosensors are composed of three modules, as follows: (1) bioreceptor, (2) transducer, and (3) electric circuit (Fig. 1). In this case, the bioreceptor senses and responds to the analyte to generate a signal, the transducer transforms this biologically recognized action into an assessable signal, and then the electric circuit quantifies the transduced signal and collects it for display and examination, leading to diagnostic assessments.^{32–34} However, the lack of biorecognition elements impedes the development of diverse biosensors.³⁵ The transducer-based output signals include optical (*e.g.*, absorbance, luminescence, chemiluminescence, and surface plasmon),³⁶ mass (*e.g.*, piezoelectric and magnetoelastic),³⁷ thermometric,³⁸ and electrochemical signals.³⁹ Electrochemical biosensors can be categorized into amperometric, potentiometric, voltammetric, impedimetric/conductometric, and capacitive sensors.²² By using electronics and signal processors, biosensing and bioelectronic devices have been effectively utilized in several fields such as environmental monitoring, drug screening, clinical diagnostics, and governing of food quality. Recent research has mainly been focused on the miniaturization of biosensing and bioelectronic devices to enable the real-time, POC, and easy-to-use detection of analytes, especially in clinical and environmental trials.^{40,41}

Moreover, biosensor platforms are typically categorized into three ways, *i.e.*, dipstick tests, lateral flow assays (LFAs), and microfluidic paper-based analytical devices (μ PADs), among which, μ PADs are the most versatile owing to their pattern-paper made using hydrophobic polymers around designated areas in the paper. These barrier patterns are designed for accommodating small sample volumes for multiple reactions.

However, the techniques used to create these hydrophobic barrier patterns and layers in inexpensive μ PADs require a long manufacturing time and very expensive.

2.1. Materials used for sensing devices

Sensors or biosensor devices are products that respond to stimuli and utilized to detect and quantify light, temperature, sound, chemicals, motion, and biological elements. Based on the material type, design approaches, and fabrication technologies, the structures of these devices can be constructed into robust and sophisticated apparatus. There Various types of sensing devices are utilized based on their working principles (*e.g.*, force, temperature, gas, humidity, proximity, chemical, optical, motion, and imaging) and applications (*e.g.*, environmental monitoring, agriculture, health industry, pharma industries, medical imaging, space, paint and coating industry, and human-machine interfaces). Various types of materials have been utilized to develop and manufacture different types of sensors. The area of sensing materials utilized for sensing devices can be divided into two groups, as follows: (1) direct sensing devices (*i.e.*, a change in electrical signals) and (2) complex sensing devices (*i.e.*, no change in electrical features, need a conversion process).⁴³

Various types of materials have been used for fabricating these biosensing devices such as metals, metal oxides, metal organic frameworks (MOFs), sol-gel materials, graphene and carbon nanomaterials, synthetic polymers, and petroleum-based materials. However, there are still various challenges in the real-world applications of these devices, wherein these material types are associated with some difficulties owing to their bulkiness, lack of affinity between material and the substrate, vulnerability to oxidation, and shortcomings considering robustness and waste management (disposal).⁴⁴ In this regard, most of the sensors are comprised of petroleum-based materials from non-renewable resources and exhibit long-term stability in the soil (difficult to be degraded) when discarded, causing severe environmental pollution. Further, the application of these devices in the biological or biomedical field is limited due to various challenges including their



biocompatibility and biodegradability. Therefore, numerous research efforts have been devoted to searching for sustainable materials for the development of biocompatible, biodegradable, and renewable sensing and biosensing devices^{45–47} and still in progress for achieving the desired outcomes for their diverse applications in environmental pollution, agriculture, food industry, soft-robotics, human–machine interaction, bioelectronics, *etc.*

2.1.1. Use of renewable and sustainable materials for biosensing devices. The environmental issues caused by the massive quantity of non-degradable medical and electronic waste are the foremost concern in developing eco-friendly, biocompatible and biodegradable sensors. These sensors have emerged as appealing alternatives to traditional non-biodegradable sensors in both non-invasive and invasive health monitoring through wearable sensors, *in vivo* sensing, and in temporal body implants. Therefore, in recent years, sustainable (recyclable and disposable) sensors have widely been developed from nature-derived materials. Overall, these developed sensors can be categorized into two types, namely partially biodegradable and fully biodegradable sensors.⁴⁸ In this case, the biodegradable materials should be non-toxic and biocompatible with effective optical, mechanical, and electrical characteristics. These materials include polymers (natural, synthetic or their combination), copolymers, silicon based materials, proteins, plant-based polysaccharides, and metals. The physicochemical characteristics of polymers greatly influence their degree and rate of hydrolysis^{48–51} and play an important role in the degradation and stability of devices. Therefore, the choice of an appropriate substrate material to construct biodegradable devices with controlled operational times needs the careful consideration of parameters for stability and effective outcomes. In this regard, various biopolymers (*e.g.*, collagen, spider silk, silkworm silk, chitosan, gelatin, and cellulose)⁵² as substrate materials have widely been utilized to develop biodegradable devices owing to their remarkable biocompatibility, environmental sustainability, abundant nature, and flexibility.

Among the biopolymers, cellulose as the most abundant polysaccharide has been promisingly considered for the fabrication of biodegradable sensors with various potential applications due to their chemical distinctiveness, remarkable biocompatibility, appealing degradation profile under physiological conditions, high-temperature stability, transparency, flexibility, and easy processing. Also, cellulosic materials can be transformed into electronically conductive carbon materials with abundant pore networks and high specific surface areas using a straightforward carbonization process.⁵² However, it is difficult to control the mechanical properties and degradation rate of naturally derived substrates. Thus, biodegradable synthetic polymers with predictable and repeatable mechanical and degradable characteristics have been synthesized in controlled manner and utilized with or without biopolymers to fabricate sensor substrates.⁴⁸ Overall, renewable and sustainable materials have received significant attention over the past few years in basic research and real-world applications owing to their ability to minimize environmental, consumption, and cost-related

issues. In this way, these materials have widely been utilized in pristine form or a combination to manufacture sensing and biosensing devices for suitable and targeted utilization and outcomes with low cost, satisfactory biodegradability, high flexibility, and low-energy consumption.

The use of composite materials based on renewable resources has increased remarkably and continues in the development of new biosensing devices. In this case, various basic and technological methods have been applied to manufacture desired composite sensing and biosensing devices partially based on organic and renewable materials and their properties can be controlled by modifying the combination of components of renewable, inorganic, and organic nanomaterials. For example, different research groups developed various sensing devices by using different composite materials, for example, conductive paper was manufactured using carbonized paper for sensing human activity,⁵³ cellulose/CNT aerogels for gas sensing,⁵⁴ nanocellulose with silver nanowires (AgNWs)⁵⁵ and/or carbon nanotubes (CNTs),^{55–57} and bacterial cellulose/AgNPs/molybdenum trioxide (MoO₃) for gas sensing,⁵⁸ and for different applications including wearable sensing fibres, CNT/cellulose-based humidity sensor⁵⁹ and ammonia gas sensor,⁶⁰ leaves and wood,⁶¹ carbonized wood,⁶² wood cellulose fibres/barium titanate (BaTiO₃),⁶³ paper substrate/zinc oxide nanowires (ZnO NWs),⁶⁴ and sodium lignosulfonate/graphene.⁶⁵ Overall, renewable resources (*e.g.*, wood, plant, bio-based carbon, and cellulose) in various forms and from various origins have greatly established their significance by using them in combination with other materials to manufacture low-cost, biodegradable, and sustainable composites. Therefore, depending on their combination and fabrication process, these composite sensing materials can be manufactured into different forms such as films, fibres, paper, and aerogels for a variety of potential applications (*e.g.*, gas sensing, supercapacitors, photovoltaic cells, wearable and flexible sensing devices, and human–machine interface).⁶⁶ Throughout history, paper has been utilized in a broad variety of applications, and therefore, cellulose-based paper, which is a porous and green material, has been utilized to manufacture different biosensors owing to its low cost, flexibility, portability, biocompatibility, degradability and capillary force-assisting fluid transfer characteristics.⁶⁷

3. Paper-based biosensors

3.1. Paper and its properties

The use of paper as a flexible, porous, and degradable cellulosic material with an environment-friendly nature has shown great potential to be applied in sustainable biosensors, bioelectronics and other areas.^{68,69} Herein, paper-based devices provide multipurpose, inexpensive, and accurate systems for sensing humidity, gases, chemicals, strain, and biological species.^{10,69–72} However, it is difficult to simplify a set of characteristics of papers due to the differences in their material compositions, structures, and fabrication methods. For example, printing paper is composed of a high filler content, which can be either natural (*e.g.*, limestone, talc, and clay) or synthetic



alternatives (e.g., precipitated calcium carbonate, gypsum, and titanium dioxide) and distinguish the cost, thickness, structure, pore size, strength, and exterior form of the paper, and other characteristics based on its type and quantity.^{73–76} In addition, due to the highly hydrophilic nature of paper, the presence of moisture can soften the materials, thereby decreasing their elastic modulus with a poor thermal performance,⁷⁷ and therefore, it is processed under low-temperature conditions. Moreover, due to the flexible nature of paper, it has been broadly utilized as a substrate for actuators, sensors, and energy storage components^{78–83} despite the diverse set of characteristics across various types of paper.

In addition, smartphones have also been integrated with sensors (e.g., strips, chips, and hand-held detectors) for biochemical detection owing to their portability and global accessibility. Smartphones are often utilized as the controller, analyzer, and display for fast, real-time, and point-of-care monitoring, which can remarkably simplify the design and reduce the cost of detecting devices. Paper-based biosensors and bioelectronics integrated with smartphones have greatly emerged for portable and disposable devices that can be applied in environmental monitoring, healthcare diagnosis, and food safety.⁸⁴ The search for renewable and sustainable power sources is crucial for developing green electronics and sensor networks. For example, paper-based origami triboelectric nanogenerators (TENGs) with high flexibility, light weight, low cost, and recyclability were developed. These TENGs were efficient to harvest ambient mechanical energy from different types of human motions (e.g., stretching, lifting, and twisting) and could directly light LEDs. Additionally, these TENGs could also work as self-powered pressure sensors.⁸⁵ In a study, an inexpensive turnip tissue paper-based mediated amperometric H₂O₂ biosensing device was fabricated using screen-printed carbon electrodes (SPCEs). Herein, raw turnip peroxidase and potassium hexacyanoferrate(II) as a mediator were immobilized on a cellulose paper matrix. This device required a low amount of the sample (0.5 mL) for analysis and exhibited a linear detection range of 0.02–0.50 mM with an LOD of 4.1 mM H₂O₂. Moreover, the biosensing device maintained 70% of its activity after a storage period of 25 days at 4 °C.⁸⁶ Most recently, some innovative paper-based biosensors have been reported for renal surveillance in fingerprint blood,⁸⁷ visual detection of microbially contaminated food,⁸⁸ nucleic acid amplification-free and label-free detection of micro-RNA,⁸⁹ controlling the pandemic situation (e.g., Covid-19),⁹⁰ etc.

3.2. Processing and manufacturing of paper-based biosensing devices

A significant advancement in the development of portable and disposable paper-based biosensor (PBB) and microfluidic paper-based analytical devices (μ PADs) has recently been realized. In this case, paper, which is composed of cellulose microfibrils, provides both a huge microporous network for storing analytical elements and capillary force to drive liquid samples to a devoted reaction zone for the rapid detection of the desired analytes. Due to their inexpensive nature and ultra-

high sensitivity, these biosensors have shown great potential for medical emergencies, point-of-care health diagnosis, and wide early-detection of cancer compared to the conventional advanced analytical devices.¹⁰ Additionally, the development of inexpensive wearable flexible biosensing devices has attracted significant attention for the monitoring of health issues and chronic diseases in the human body. Herein, conventional wearable devices uninterruptedly record signals such as stress, pressure, and temperature for the real-time monitoring of human actions. However, the uninterrupted monitoring of different chemicals in body fluids and respired breath using wearable sensors still faces certain challenges such as accuracy, sensitivity, flexibility, and fitting of the sensor to human skin.^{91,92} Paper is a favorable substrate to manufacture POC *in-vitro* diagnostic devices due to its abundant availability, affordability, chemical stability, biodegradability, prominent porous fibrous network with high surface area for interactions, and natural capillary-driven mass transport of liquid samples.^{93–97} Various well-established technologies for the manufacture and processing of paper have been applied for the fabrication of paper-based microfluidic devices, including folding, cutting,^{98,99} masking,^{100,101} laser writing,¹⁰² and printing.^{103–105} However, paper can vary immensely based on its composition, internal structure, and wettability owing to its sources and manufacturing method,¹⁰⁶ for example, filter paper,^{107,108} chromatography paper,¹⁰⁹ common printer paper,¹¹⁰ and paper towels. The performance of diagnostic sensing devices for various target analytes is largely affected by the internal structure of paper. In this case, nanomaterials have shown a considerable prospect in developing paper-based sensors. In one study, CNT-based electrodes were fabricated for use in paper-based electrochemical sensing devices *via* a series of laser-cutting, drop-casting, and origami. Herein, a range of filter papers with varying porosities and different 3D cellulose networks was utilized with this process to analyze the effect of the cellulose scaffold on the ultimate CNT network and resulting electrochemical detection of glucose.¹¹¹ The synergistic blending of materials and interfaces is a decisive strategy in developing novel functional sensing devices for different potential applications, including inexpensive paper-based POC systems. Surface-functionalized polypyrrole (PPy) constructs were integrated monolithically into a 3D multilayered paper-based microfluidic biosensing device to monitor local humidity variations. The PPy constructs exhibited remarkable mechanical stability, which is relevant to flexible electronics and the electrical resistance connects with local relative humidity (RH) interior of the sealed microfluidic channels, and their sensing response was entirely reversible. In addition, the results showed that RH changes of 5–10% could affect the flow of the prolonged channels (> 5 cm) even when they were fully surrounded.¹¹²

4. Applications

Biosensors have been used in various fields, including food, environment, and medicine. These developed biosensor



devices are categorized into three types for human healthcare, as follows: (1) biosensors for *in vitro* diagnosis with urine, saliva, and blood samples, (2) continuous monitoring biosensors, and (3) wearable biosensors. Among them, *in vitro* diagnosis biosensors have received been widely developed *via* various approaches, and also used in integrated devices, such as lateral flow assays (LFAs) and microfluidic/electrochemical paper-based analytical devices (μ PADs/ePADs). Moreover, high-quality and inexpensive smartphone-based POC devices for basic healthcare monitoring can be developed using paper-based platforms. Exclusively, μ PADs have shown immense potential in using this inexpensive matrix for detecting blood glucose, urine metabolites, pH level, liver function, and infectious agents.¹¹³ Also, μ PADs have various benefits such as low cost, simple and rapid manufacturing, and disposability compared to the alternative traditional lab-on-chip devices.¹¹⁴ The integration of PADs with paper-microfluidics has empowered various studies for detecting different enzymatic and biological reactions with an electronic readout.⁸³ However, recently, continuous monitoring and wearable biosensors have attracted significant attention in terms of commercialization. A schematic illustration of these biosensors devices and their data processing and interpretation with the concept and implementation of artificial intelligence (AI) is provided in Fig. 2.¹¹⁵

4.1. Healthcare

Worldwide, human healthcare is the priority and requires sophisticated and affordable medical care products and devices. Among the various healthcare products and devices, paper-based biosensors are affordable diagnostic tools, but their wide utilization is impeded owing to the scarcity of

sensitive detection means to be implemented on paper substrates.

4.1.1. Medical diagnosis. Based on particular sensitivity and selectivity towards biomolecules, extensive studies have been performed for satisfactory outcomes. For example, rapid and sensitive cellulose-based strips (CBS) were prepared based on greenly synthesized, high-purity, and porous interpenetrated cellulose membranes immobilized with glucose oxidase (GOX) and horseradish peroxidase (HRP) *via* the periodate oxidation process. CBS exhibited an improved performance for the detection of a low concentration of glucose and demonstrated changes in color from colorless to blue within 5 min, while showing an LOD of 0.45 mM in the glucose range of 1 to 11 mM.¹¹⁶ In another study, glucose oxidase (GOX) was effectively implanted into the cellulosic fibre matrix of paper to prepare a paper-based amperometric glucose biosensing device based on PBB-modified SPCEs, which required a small content of sample (0.5 mL) as a glucose probe with a linear range of 0.25–200 mM and LOD of 0.01 mM, and it maintained its 72% of its activity after a storage period of 45 days.¹¹⁷

A paper-based cholesterol biosensing device was developed by modifying an electrode through electro-spraying using a nanocomposite of graphene (G), polyvinylpyrrolidone (PVP), and PANI (GPP). Herein, in this nanocomposite, the existence of a small quantity of PVP (2 mg mL⁻¹) enhanced the dispersibility of G and improved the electrochemical conductivity of the electrode, resulting in improved sensitivity in the biosensor. Compared to the unmodified electrode, a 3-times increased current signal was observed including remarkable electrocatalytic action to the oxidation of H₂O₂. Further, cholesterol oxidase was fixed to the GPP-modified electrode for the



Fig. 2 Schematic illustration of conceptual implementation of AI to process and interpret the received data. Reproduced with permission from ref. 115 Copyright 2022, Elsevier.



amperometric determination of cholesterol. Under the optimal situations, it exhibited a linear range of 50 μM to 10 mM for cholesterol with an LOD of 1 μM .¹¹⁸ In a study, a portable paper-based biosensor with a specific enzymatic calorimetric detection was developed for blood alcohol sensing (direct quantification of ethanol in whole blood) for on-site toxicological tests.¹¹⁹ Similarly, the detection of diverse biomarker types with zero background was achieved by using a paper-based electrochemical biosensor (paper functionalized with single molecule-labeled DNA and a screen-printed electrode along with target recognition solutions). It enabled high sensitivity and selectivity for the target *via* high specific target-triggered polymerization/nicking and DNAzyme-catalyzed signal amplification. These assays could be used to identify the target in spiked serum trials for the point-of-care analysis of clinical samples.¹²⁰

Paper-based microfluidic devices are portable, rapid, inexpensive, and disposable and only require small volumes of reagents and samples. The combination of these devices with the electrochemical detection mechanism extends the extra advantages of high selectivity, sensitivity, simplicity, and portability, and low-cost. In one study, an integrated paper-based screen-printed electrochemical biosensing device to detect and quantify a nerve agent contamination *in situ*. The strategy of this reagent-free method was the dual electrochemical analysis of butyrylcholinesterase (BChE) enzymatic action towards butyrylcholine with or without exposure to polluted samples, wherein the sensitivity was enhanced by using a nanocomposite of carbon black/Prussian Blue as a working electrode modifier. Herein, a nitrocellulose membrane strip was integrated with a paper-based test area holding a screen-printed electrode and BChE and detected paraoxon as a nerve agent stimulant linearly as low as 3 $\mu\text{g L}^{-1}$.¹²¹ In addition, a paper-based microfluidic electrochemical DNA biosensor was developed to detect EGFR mutations sensitively in patients using their saliva. In this study, oligonucleotides were functionalized on the surface of the electrodes and the outcome of the electrochemical signals were received by investigating the hybridization of DNA, where the indicator-labeled on DNA was recognized by horseradish peroxidase (HRP), showing a remarkable electrocatalytic response to H_2O_2 . Under the optimum situations, it exhibited a linear association between current value and the logarithm of the target DNA content (5–500.0 nM) with a limit of detection as low as 0.167 nM and showed satisfactory stability and high specificity in distinguishing the single nucleotide polymorphism of the target DNA.¹²² In the case of progesterone monitoring for *in vitro* fertilization therapy of dairy cows, it depends on antibodies, making this procedure expensive. Thus, an alternative transcription factor-based progesterone sensor was utilized with a portable and affordable paper fluidic arrangement, where fluorescent dye-labeled oligonucleotides were immobilized on nitrocellulose through a biotin–streptavidin interaction. In the absence and presence of progesterone, these oligonucleotides bind and unbind with the fluorescent transcription factor, respectively. Also, the LOD of the device was 27 nM, which is the clinically significant level of progesterone.³⁵

The use of nanomaterials in combination improves the efficiency of biosensors, for example, a disposable paper-based chemiresistive biosensor with manifold detection capability and microfluidic controls using single-walled carbon nanotubes (SWCNTs) was developed for label-free immunosensing. In this study, a stable water-based ink composed of pyrene carboxylic acid (PCA) and SWCNTs was synthesized and deposited on paper in a facile approach, which did not require extra covers or patterns. Specific antibodies were functionalized on the PCA/SWCNTs, and then human serum albumin (HSA) was rapidly, sensitively, and selectively detected and quantified with a limit of detection of 1 pM due to the porous-network of the paper surface, wherein more SWCNTs were accommodated and formed an electric network of SWCNTs.¹²³ Micro RNAs (miRNAs), which are 19–23 nucleotide-long non-coding RNA, have been identified as important biomarkers for various diseases including cancer. This type of biomarker (miRNA) was detected using a rapid, simple, ultrasensitive, greatly specific, and label-free paper-based SWCNT field-effect transistor (FET) biosensor, without nucleic acid amplification. This approach involved a two-step process, as follows: (1) direct hybridization of the targeted miRNA with a certain RNA probe immobilized on SWCNT system deposited on paper substrate to produce the first signal, and then (2) recognition of the resulting RNA/miRNA duplexes with the Carnation Italian ringspot virus p19 protein (p19) in a size-dependent mode to provide the second electrical response. For demonstration, the miRNA-122a biomarker (lowest detection: 0.1 aM and broad dynamic range: 0.1 aM–1 fM) was detected for the diagnosis of early-stage hepatocellular carcinoma in various samples, including human serum, phosphate buffer, and synthetic saliva. Overall, without any sample preparation, the biosensor successfully detected miRNA spiked in serum and artificial saliva.⁸⁹ In another study, multi-walled CNTs (MWCNTs) were coated on a paper substrate (15–20 nm average diameter) using stencil-free wax deposition and vacuum filtration to create hydrophilic and hydrophobic channels for the label-free, highly selective and sensitive detection of cholesterol owing to the high affinity of cholesterol oxidase towards MWCNTs through the electrostatic gating effect and direct electron transfer mechanism between cholesterol and MWCNTs. The disposable biosensor showed stability, reproducibility, and high specificity towards cholesterol (response to a concentration range of 10 nM–75 μM to 100 μM –8 mM and an LOD of 3.2 nM (3 S m^{-1})), while negligible interaction from interfering analytes.¹²⁴ In another study, a paper-based biosensor was developed *via* the electropolymerization of 5-amino-1,3,4-thiadiazole-2-thiol (ATT) on the surface of graphene oxide (GO) and showed high sensitivity by requiring only 200 μL of analyte solution for the cyclic voltammetry (CV) analysis. ATT showed good selectivity for specific binding with uric acid and the interference from nitrites in human blood and blood fluids could be prevented in the CV analysis owing to their different oxidation potentials.¹²⁵ In another study, a robust, user-friendly, and portable smartphone-aided biomimetic metal–organic framework (MOF) nanoreactor colorimetric paper (SBMCP) device was fabricated for the



on-demand POC recognition of endogenous biomolecules. In this study, the single/multiple enzyme constituents trapped within the micropores network of ZIF-8 (exoskeleton) facilitated the sensitive and selective detection of the target analyte, and then relocated the detection event to a visual color signal based on the cascade effect. In the SBMCP assay, only a small volume (5 μL) of sample was needed, and it provided the efficient and real-time colorimetric recognition of glucose and uric acid in diabetes and gout events.¹²⁶

Due to the changes in dietary habits and living standards, the occurrence of chronic kidney disease (CKD) is a rapidly rising global health concern. Thus, the early detection of CKD is critical in avoiding progression to final-stage renal disease and preventing expensive therapies. For this, a series of biomarkers, including blood urea nitrogen (BUN), has been proposed for this specific detection. Clinically, BUN is utilized as an indicator for renal function analysis and considered the gold standard for urea bioassay. However, the testing of BUN requires blood sampling, which is generally inconvenient, painful, time-utilizing, and expensive method. Therefore, inexpensive, simple, fast, and stable point-of-care biosensors are greatly desirable for evaluating the BUN levels with the minimum sample requirements. However, there are various challenges in developing novel sensing biosensing devices. In this regard, some biosensors such as origami paper-based sensors and smartphone-assisted paper-based biosensors have been developed for colorimetric readouts. Nevertheless, there are several challenges due to variations in camera quality and software,

and contamination issues. In this case, the demand for electrochemical point-of-care biosensors is increasing due to their inexpensive system, high sensitivity, robust miniaturization potential and ease of integration for the fabrication of compact devices. In 2023, Cheng *et al.* developed an inexpensive handheld optical biosensor with multilayer paper-based photochemical disposable test strips (Fig. 3), wherein these strips can help in separating and filtering whole blood samples and the colorimetric reaction uses urease immobilized on a membrane to hydrolyze urea into NH_3 , exhibiting intense color changes with a pH indicator. Further, this color change was detected using an optical reader *via* the reflection of light, and then BUN quantified *via* a unique photodetection algorithm. This process could be accomplished within 2 min using only 20 μL of fingertip blood sample for high accuracy and consistency with a broad concentration range (BUN: 2.46–38.14 mM) and LOD of 0.03 mM in different samples. Additionally, Bluetooth was employed in the reader and connected to a smartphone for active health monitoring or remote diagnosis for renal diseases.⁸⁷

In a study, an anthraquinone-labeled pyrrolidinyl peptide nucleic acid probe (AQ-PNA) and graphene-polyaniline (G-PANI)-functionalized electrode were utilized in developing a paper-based electrochemical DNA biosensing device to detect human papillomavirus (HPV) type 16 DNA (corresponding sequence of synthetic 14-base oligonucleotide target). Under the optimal conditions, the limit of detection of HPV type 16 DNA was observed to be 2.3 nM with a linear range of



Fig. 3 (A) Schematic illustration of a disposable photochemical test strip, (B) stacking of multilayer film strips with reflectance photometry, and (C) principle of enzymatic colorimetric response. Reproduced with permission from ref. 87 Copyright 2024, Elsevier.



10–200 nM. In addition, the real-time screening and monitoring of HPV-DNA type 16 were evaluated with the detection of PCR-intensified DNA samples from SiHa cells for the identification of the primary phases of cervical cancer.¹²⁷ In another study, a hand-operated paper-based rotational vertical-flow immunosensor (r-VFI) platform was designed, which required fewer pipetting steps, for the electrochemical detection of α -fetoprotein with numerous and time-progression steps without any interference from the convective factor of fluid motion. In this case, free transfer-switch-stop fluid flow could be achieved by rotating the paper disk. Overall, the assay duration was shortened to 9 min with the linear range (LR) of 0.01–500 ng mL⁻¹ and LOD of 1.65 pg mL⁻¹, and the sensitivity could be improved remarkably by switching off the sample cascade, which could extend the LR to 0.5 pg mL⁻¹ with LOD of 3.54 fg mL⁻¹. This is the lowest detectable level reported to date for paper-based sensors.¹²⁸

The rapid detection of deoxyribonuclease I (DNase I) activity as a biomarker based on the variations in the viscosity of DNA mucus was performed, exhibiting a linear range of 0.01–10 U mL⁻¹, remarkable sensitivity, specificity, and reproducibility. In addition, the limit of detection achieved was as low as 0.003 U mL⁻¹. This sensing device provided great potential in detecting DNase I and effective and rapid analysis of nucleic acid scavenger.¹²⁹ Further, in the case of investigating various biological actions and events of enantiomers, chiral examination is of crucial importance in different fields. For this, a paper-based chiral biosensor device was developed for detecting lactate enantiomers in human serum samples. For the purpose of achieving the sensitive and real-time detection of lactate enantiomers, an alginate hydrogel was utilized to construct enantiomer-selective sensing zones and dual enzyme (*i.e.*, lactate dehydrogenase (LDH) and glutamic pyruvic transaminase (GPT))-linked synergistic catalytic interactions with substrate recycling were used to improve the sensor response. The well-blended solutions including the components for gelation and sensing (*e.g.*, alginate, Ca²⁺, GPT, coenzymes, NAD⁺, L-Glu, L-LDH and D-LDH) were supplemented in the sensing domains. The fluorescence signals from nicotinamide adenine dinucleotide were acquired using a smartphone with color evaluation software. The results exhibited remarkable sensitivity with an LOD of 30.0 ± 0.7 μ M and 3.0 ± 0.2 μ M and broad linear range of detection of 0.1–3.0 mM and 0.01–0.5 mM for the concentrations of L-lactate and D-lactate, respectively, with reasonable accuracy.¹³⁰

A paper-based microfluidic electrochemical DNA biosensor was developed to detect EGFR mutations sensitively in patients with saliva. In this study, oligonucleotides were functionalized on the surface of electrodes and the outcome of the electrochemical signals were received by investigating the hybridization of DNA, where the indicator-labeled DNA was recognized by horseradish peroxidase (HRP), showing a remarkable electrocatalytic response to H₂O₂. Under the optimum conditions, it exhibited a linear association between current value and the logarithm of the target DNA content (5–500.0 nM) with a limit of detection as low as 0.167 nM and showed satisfactory

stability and high specificity in distinguishing single nucleotide polymorphism of target DNA.¹²² Bhattacharya *et al.* 2022 developed high-quality laser-induced graphene (LIG) electrodes, which were integrated into a paper-based electrochemical biosensor device for the detection of uric acid. Mechanistically, the enhanced charge-transfer kinetics in the paper-based two-electrode chronoamperometric biosensor led to improved functioning for sensing uric acid (*i.e.*, sensitivity: 24.35 1.55 μ A μ M⁻¹ and LOD: 41 nM).¹³¹ Further, the storage of very concentrated reagents and their release with high proficiency are vital in developing very sensitive biosensors, while the performance of the reservoirs in paper-based biosensors is restricted due to the intrinsic physicochemical characteristics of non-treated cellulose. Therefore, in a study, some polymeric water-soluble reservoirs (*e.g.*, carboxymethyl cellulose, chitosan, carrageenan, and poly(vinyl alcohol)) were created *via* the drop-casting method with nine different modifications to store and release enzymes and nanoparticles in paper-based biosensors. Exclusively, the release of the enzyme from the reservoir composed of carboxymethyl cellulose rapidly at a high concentration exhibited an ultralow LOD of 0.005 mM for colorimetric glucose sensing, while the reservoirs composed of polymer blends focused antibody-patterned nanoparticles and reduced the LOD of the model immunosensor by 10 times. Moreover, the pathogen *Klebsiella pneumoniae* in urine samples was detected rapidly with high specificity at the infectious dose threshold.¹³²

In a study, the polylactic acid (PLA) filament and wax filament were used to create hydrophobic patterns on paper for μ PADs using the 3D printing method and combined with a fluidic chip in a prototype biosensor, wherein the barrier patterns held cell-free reactions and the fluidic chip facilitated the sample delivery to the reactions in the device. Overall, this rapid prototyping device type could differentiate *Dengue virus* serotypes considering the differences in their small nucleotide sequences.¹³³ In another study, a CO₂ laser was used to generate etched grooves (a pitch of 0.75 mm) on paper to hasten the speed of the wicking channels in μ PADs. This study exhibited the influence of various adhesive sealed grooved channels on wicking, where tape sealing demonstrated faster wicking and use of lamination showed a negative effect on wicking. Moreover, this chemiresistive paper-based biosensor efficiently detected human serum albumin (15 mM) spiked in phosphate buffer, artificial urine, and artificial saliva.¹³⁴ A fullerene C₆₀-functionalized disposable graphite paper-based electrode was utilized to develop a highly sensitive electrochemical immunosensor for determining suppression of tumorigenicity 2 (ST2) in human serum. It showed remarkable repeatability and reproducibility with a broad detection range (0.1–100 fg mL⁻¹), low LOD (0.124 fg mL⁻¹), and limit of quantification (0.414 fg mL⁻¹).¹³⁵ In a study, an innovative phenylalanine electrochemical paper-based biosensor was manufactured using a hybrid of zinc oxide (ZnO) nanorods and gold (Au) nanoparticles together with the enzyme phenylalanine hydroxylase (from the extract of moss leaf-like tissue). The immobilization of the enzyme was performed by dropping



ZnO@Au hybrids and moss extract respectively onto a filter paper and the functionalized paper was positioned on the top of a graphite screen-printed electrode (GSPE). Further, it was effectively utilized in determining phenylalanine in a sample of human blood serum and exhibited the phenylalanine concentration in the range of 5.0 nM and 100 μ M with an LOD (S/N: 3) and quantification limit of 3.0 nM and 10.0 nM, respectively.¹³⁶ In another study, AuNPs were utilized to develop a colorimetric paper-based biosensor device to detect phenylalanine, wherein phenylalanine dehydrogenase enzyme reacted with phenylalanine selectively in the presence of NAD⁺ to form NADH, which reacts with MTT to form purple-colored formazan in the presence of diaphorase enzyme. Also, AuNPs interact with MTT as a cationic dye and increased the color intensity. Under the optimal circumstances, it exhibited a linear detection range of 0.8 to 33 mg dL⁻¹ and LOD of 0.57 mg dL⁻¹.¹³⁷

Recently, Covid-19 triggered by severe acute respiratory syndrome coronavirus 2 (SARS-CoV-2) appeared as a worldwide pandemic outbreak and in China. During the Covid-19 pandemic, the global demand for fast, inexpensive, broad distributable, and point-of-care nucleic acid diagnostic tools tremendously increased to stop widespread infections, preserve health/lives, and sustain economies.¹³⁸ For rapid and accurate testing, a paper-based electrochemical biosensor with a specific and sensitive immunosensor for the detection of immunoglobulins produced against SARS-CoV-2 was developed. Unlike other LFAs that involve multiple antibodies, this label-free paper-based electrochemical platform targeted SARS-CoV-2 antibodies without the definite obligation of an antibody. Additionally, this method was extended to detect an antigen (the spike protein of SARS-CoV-2) for the possible diagnosis of Covid-19 symptoms.¹³⁹ In another study, lyophilized cell-free protein synthesis (CFPS) and toehold switch riboregulators (TSRs) were used to develop a paper-based nucleic acid diagnostic template activated by only adding saliva. Herein, TSRs were engineered to express the bioluminescent reporter Nano-Luc upon reaction with the SARS-CoV-2 RNA sequences present in saliva tests. This biosensor system produced a visible signal within 7 min after administrating 15 μ L saliva and costed less than 0.50 USD roughly. However, additional research to reduce the LOD of this device is desirable for an effective outcome for society.¹³⁸

Nucleic acid amplification testing (NAAT) is a highly sensitive and specific technique, but it is not appropriate for rapid point-of-care testing. Thus, a 3D microfluidic paper-based electrochemical NAAT biosensor was developed using off-the-shelf gold plasma-coated threads (*i.e.*, electrodes) to combine electrochemical readouts *via* the *ex situ* construction of self-assembled monolayers on the threads. Then, movable stacks of filter papers were integrated with incubation, rinsing, and detection steps *via* a sandwich hybridization assay for time-sequenced responses (Fig. 4). This biosensor device utilized glass fibre substrates for loading the recombinase polymerase amplification components and conducting isothermal intensification. This paper-based biosensor device was used to detect

the toxic microalgae *Ostreopsis cf. ovata* and the detection of 1 ng μ L⁻¹ of *O. cf. ovata* genomic DNA was reported with an LOD of 0.06 pM for targeted synthetic DNA. Also, no significant cross-reactivity was observed from closely related microalgae species.¹⁴⁰

Pancreatic ductal adenocarcinoma is the leading neoplastic disease of the pancreas, which is fourth most common reason for death in cancer-related disease with only 8% survival rate after five years of the diagnosis. Therefore, an inexpensive office paper-based biosensor device was fabricated for detecting miRNA-492 for the early diagnosis of pancreatic ductal adenocarcinoma. In this design, an electrochemical sensor was screen-printed on paper using wax-printing, and then it was organized with highly specific peptide nucleic acid (PNA) as the biorecognition component. The construction of the PNA/miRNA-492 duplex was measured by monitoring the reaction between positively-charged ruthenium(III) hexamine with uncharged PNA and/or negatively-charged PNA/miRNA-492 complex. It showed a linear range of up to 100 nM with an LOD of 6 nM.¹⁴¹

Porcine pseudorabies, which is one of the most acute infectious diseases, influences the pig-breeding industry and causes massive losses, highlighting the vital requirement for developing clinical techniques for the exact and rapid diagnosis of wild-type PRV infection. PRV-gE antibodies are a notable indicator of PRV source only in the serum of infected individuals (wild-type PRV), not in injected PRV-gE-deleted vaccines, and enables the distinction of wild-type PRV infection from vaccine immunization. In this case, in 2021, Huang *et al.* developed a paper-based smartphone biosensing device based on an immunoassay for the distinct diagnosis of wild-type pseudorabies virus infection against vaccination immunization. The test of swine clinical samples exhibited the conformity of 98% between this system and the most commonly utilized commercial gE-ELISA kit. Overall, this biosensing device was fast (15 min), inexpensive, and easy-to-operate, and served as an on-site differential diagnosis method for PRV infection.¹⁴²

4.1.2. Physical health monitoring. Regular physical exercise is an important and established factor of human life for preventing and managing non-infectious diseases (*e.g.*, diabetes, heart disease, stroke, and various cancer types), as well as avoiding hypertension and maintaining body weight, mental health, quality of life and happiness. During physical activities, sweat as biological fluid is released from the body and can provide relevant physiological evidence towards the individual human health condition. Sweat includes various biomarkers such as biomolecules (*e.g.*, uric acid and ascorbic acid), metabolites (*e.g.*, urea, glucose, and lactate), electrolytes (*e.g.*, sodium, potassium, and chloride ions), and proteins.^{143–147} Herein, the concentration of glucose in human sweat is linked to the level of blood glucose,¹⁴⁶ while the amount of lactate discloses the metabolism and movement level of the body.¹⁴⁵ Therefore, the continuous and real-time monitoring of these biomarkers (*e.g.*, blood glucose and lactate concentration) in sweat is essential for the proper management of personal



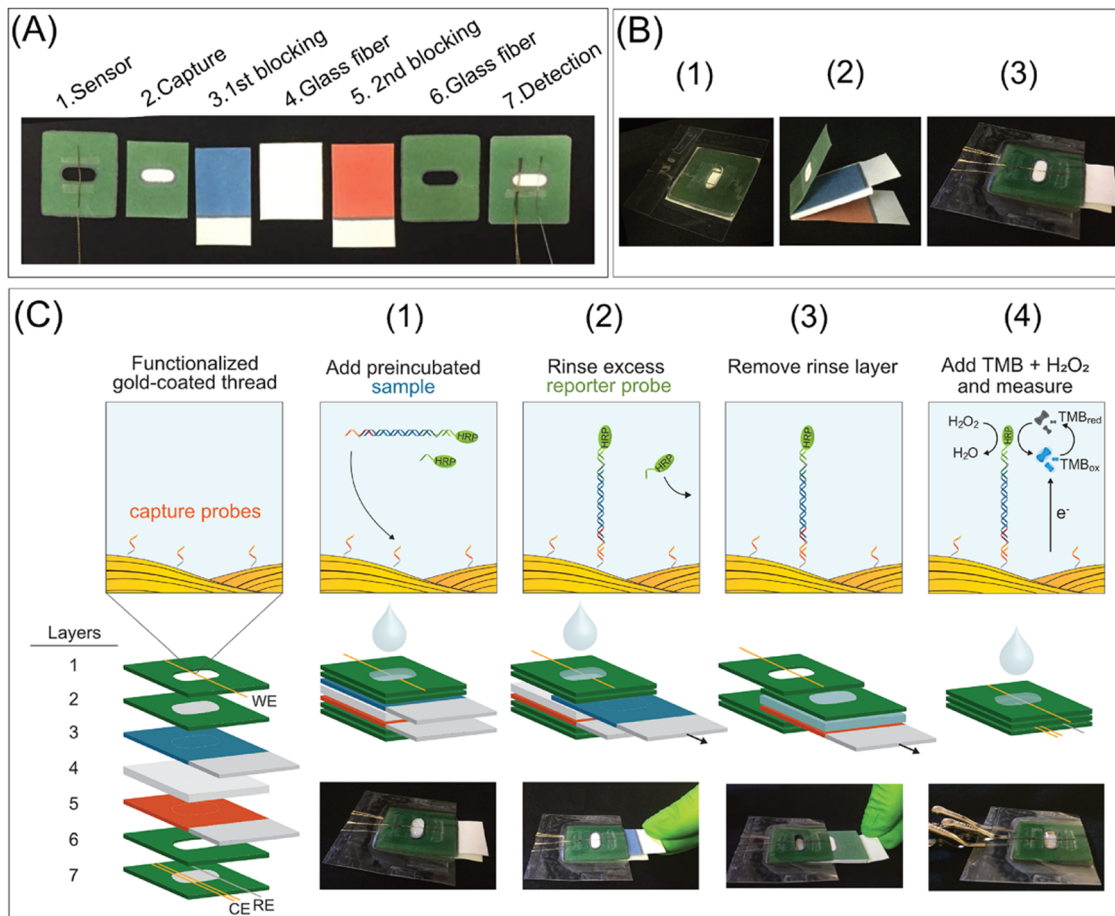


Fig. 4 Digital images and schematic representation of the elements, manufacturing, and operation of the device: (A) elements and functions, (B) manufacturing (1: detection, spacer, and sensor layers are aligned and laminated; 2: movable layers are created), 3: movable layers are incorporated between the laminated detection and space layers, and then the modified working electrode is employed in the detection layer, and (C) operational steps from sample incubation to chronoamperometric measurement. Reproduced with permission from ref. 140 Copyright 2021, the American Chemical Society.

health and offering awareness for related health issues such as blindness, cardiovascular and kidney diseases, stroke, and neuropathy.^{144,146,148} For this purpose, various sensing and biosensing devices have been designed and developed for selective, accurate, and real-time detection abilities.

Recently, in 2021, Li *et al.* developed an inexpensive, miniaturized, and greatly combined sensing paper using $\text{Ti}_3\text{C}_2\text{T}_x$ MXene and foldable layered wholly-paper substrates for the real-time monitoring of lactate and glucose in human sweat. In this study, the working were screen-printed carbon electrodes (SPCPes) and functionalized with $\text{Ti}_3\text{C}_2\text{T}_x$ MXene and methylene blue (MB), and the reference electrode was created using silver paste. Further, a drop of glucose oxidase was placed on the electrode surface for detecting glucose, whereas lactate oxidase was utilized for the detection of lactate. This device showed a linear chronoamperometric current response with a concentration in the range of 0.08–1.25 mM and LOD of 17.05 mM. At low and high contents, the approximate detection sensitivity of glucose was observed to be 2.4 nA mM⁻¹ and 1.0 nA mM⁻¹, respectively. Additionally, the amperometric

lactate response was also observed in the linear range of 0.3–20.3 mM with an LOD of 3.73 mM, including a sensitivity of 0.49 mA mM⁻¹. Moreover, in the presence of non-target metabolites and analytes, no obvious interference signals were recognized, the selectivity was good, and the response hardly altered after 14 days.¹⁴⁹ In another study, in 2022, Singh *et al.* developed a highly sensitive enzyme-free human sweat glucose sensor on a Whatman filter paper substrate by utilizing a dual-step pencil and pen strategy (Fig. 5). In this case, two pencil drawn electrodes (PDE) were made on the filter paper, with one of them as the working electrode was drawn with a sensitive layer of copper nanoparticle ink (CuNPs ink, 43.5%) pen and the second one as the reference electrode was drawn with silver conductive ink (Ag ink) pen. The developed CuNPs/PDE promoted rapid electron transfer during the electro-oxidation of glucose in a strong alkaline medium due to its highly conductive and crystalline nature and offered a rapid response time of ~1.5 s with a sensitivity of 2691.7 $\mu\text{A mM}^{-1} \text{ cm}^{-2}$ and LOD of 0.5 μM in a linear range of 1.2–40 μM . Moreover, the size of the sensor (25 mm × 10 mm) provides the opportunity to develop a





Fig. 5 (a) Schematic of the design and manufacture of two-electrode enzyme-free human sweat glucose sensor (i–ix) with the sensor dimensions and labelling, (b) secretion of sweat during treadmill exercise at room temperature, (c) filtration of sweat, and (d) set-up for developed sensor connected to a potentiostat with a computer system for detecting the level of sweat glucose in a human sweat sample. Reproduced with permission from ref. 150 Copyright 2022, Elsevier.

miniaturized and wearable electronic system for uninterrupted glucose monitoring.¹⁵⁰

In 2023, Fiore *et al.* developed a sustainable paper-based microfluidic device for the delivery of capillary-driven microfluidics for a reagent-free competitive magnetic-bead based immunosensor for cortisol determination in sweat samples. The presence of magnetic beads modified with monoclonal antibodies for recognizing cortisol in the reaction zone allowed the measurement of a specific analyte. The competitive interaction between the target cortisol and acetylcholinesterase enzyme-labeled cortisol demonstrated a reaction inversely proportional to the target cortisol (ranging from 10 to 140 ng mL⁻¹) by merely folding the pad loaded with the enzymatic substrate. Further, this paper-based microfluidic device was merged with a near-field communication wireless module to fabricate a flexible integrated wearable analytical device for detecting cortisol in sweat samples (Fig. 6).¹⁵¹

4.2. Agriculture

Agriculture generates food for the world and great revenue with technological innovations. In this case, to realize the better production of food and supplies, new effective strategies are required to identify the on-site yield limiting factors compared to conventional testing, which are mostly non-green, lack precision, and highly non-accessible to farmers. Therefore, biosensors for precision agriculture as a technology-assisted strategy can be applied as real-time, sensitive, and quantitative diagnostic devices when there is a high global food demand. Also, as POC devices, they can be utilized for the protection of crops, monitoring of soil health, and assessment of crop productivity.¹⁵²

Pesticides are utilized in agriculture to control pests, weeds, and diseases in plants with an excellent contribution to food security and availability.¹⁵³ However, the extensive use of pesticides in the atmosphere causes pollution, which has a negative impact on the ecosystem (*e.g.*, produced food, soil, and groundwater), and thereby human health.^{154,155} Thus, the extensive use of pesticides should be reduced to prevent or minimize the contamination of unwanted areas (other than targeted species). In this regard, effective electrochemical biosensors have been developed to detect and quantify the over-utilization of pesticides for precision agriculture with long-term food production efficiency and profitability, reducing the unwanted impact on wildlife and the atmosphere using real-time monitoring. Also, the usage of paper as a sustainable substrate reduces the environmental influence of these biosensors owing to its good biodegradability, porosity, and capillary forces.^{156,157} Recently, some paper-based sustainable biosensors have been developed to detect pesticides.^{158–160} For example, in 2019, Arduini *et al.* developed an origami paper-based enzymatic electrochemical biosensor for detecting three different types of pesticides in river water trials¹⁵⁸ and an origami wearable paper-based enzymatic biosensor to detect mustard agents in aerosol form.¹⁶¹ In addition, a flower-like origami paper-based enzymatic electrochemical biosensor was developed to detect three classes of analytes such as paraoxon (PX), 2,4-dichlorophenoxyacetic acid (DCPA) and glyphosate (GP) in the aerosol phase at the ppb level by quantifying their inhibitory action towards three different enzymes (*i.e.*, butyrylcholinesterase, alkaline phosphatase, and peroxidase), respectively, for precision agriculture. This integrated electrochemical biosensor was made of three office paper-based screen-printed





Fig. 6 Schematic illustration of monitoring cortisol by chasing the level of the subject during physical activity: (A) processing of samples and (B) assessing data and wireless transmission to a smartphone through NFC. Reproduced with permission from ref. 151 Copyright 2018, Elsevier.

electrodes and filter paper-based pads laden with enzymes and enzymatic substrates (Fig. 7). Herein, the percentage of inhibition in relation to the quantity of aerosolized pesticides was evaluated by using a smartphone-potentiostat (with initial and residual enzyme activity through chronoamperometric method).¹⁶²

A wide range of insecticides acts and initiates physiological responses when combined with nicotinic acetylcholine receptors (nAChRs), leading to paralysis and the death of pest organisms.^{163–166} Neonicotinoids is one of the most commonly utilized class of insecticides worldwide.^{167–169} The adverse effect of neonicotinoid pesticide residues on human health and the environment *via* contamination is a major concern, and thus sensitive, rapid, and on-site devices are highly desirable for detecting these residues for food security and sustainable development of environment. Various effective and highly sensitive methods have been developed and utilized for these purposes, but their usage is limited due to their high cost and time-consuming sample provision. Therefore, for food safety and public health, it is imperative to develop modest, fast, and low-cost diagnostic techniques for the real-time monitoring of these pesticides and insecticides. In this case, a paper-based surface-enhanced Raman scattering (SERS) intensified strategy was proposed by integrating multilayered plasmonic coupling using hybrids of 3D silver dendrite (SD), electropolymerized molecular identifier (EMI), and silver nanoparticles (AgNPs). Due to the distinct design of the multilayered coupling amplification approach, the SERS paper chips exhibited remarkable specificity and ultra-high sensitivity in detecting imidacloprid

(IMI), with a low limit of detection of $0.02811 \text{ ng mL}^{-1}$. Moreover, this approach showed good prospects for the automated screening of a diverse range of pollutants.¹⁷⁰ In another study, an eco-designed paper-based algal biosensor was developed for optical detection of nano-encapsulated-atrazine (a nanoformulated herbicide). In this study, a paper substrate soaked with an agar thin film was immobilized with a unicellular green photosynthetic algae *Chlamydomonas reinhardtii* and placed in a glass optical analysis. The detection of nano-encapsulated-atrazine demonstrated a range of 0.5 to 200 nM, demonstrating a relationship in reasonable dose-response curves and limit of detection of 4 pM. Further, the interference analyses showed a minor interference in the presence of 2 ppm copper and 10 ppb at safety bounds, a suitable recovery value of $96 \pm 5\%$ for 75 nM nano-encapsulated-atrazine, and good storage stability for up to 3 weeks.¹⁷¹

Soil pollution, caused by organophosphorus pesticides and their main metabolites, is a major concern worldwide. In this case, the on-site screening of these pollutants for determining soil bioavailability is still a challenge. Therefore, whole-cell biosensors are effective devices to distinguish the interaction mechanisms between pollutants and microbes. In this way, a novel, inexpensive and portable paper-strip biosensor was developed, which could precisely detect methyl parathion (MP) and its prime metabolite *p*-nitrophenol elements (Fig. 8). In this study, the *Escherichia coli* BL21/pNP-LacZ system was fixed to filter paper using an alginate biogel and polymyxin B sensitizer. The color intensity of this paper-strip biosensor recorded by a mobile app could provide the content of MP and





Fig. 7 Schematic representation of (A) flower-like origami paper-based electrochemical biosensor for detecting pesticides using smartphone-assisted potentiostat and (B) device composed of office paper-based screen-printed electrode and three filter pads (i), evaluation procedure of initial enzymatic activity in the absence of pesticide (ii), and residual enzymatic activity after exposure to pesticide solution (iii). Reproduced with permission from ref. 162 Copyright 2022, Elsevier.

p-nitrophenol. This method could detect and quantify the content of $10\text{--}10\,000\ \mu\text{g kg}^{-1}$ for *p*-nitrophenol and $25\text{--}7500\ \mu\text{g kg}^{-1}$ MP, wherein the investigation of soil samples showed the detection limit of $5.41\ \mu\text{g kg}^{-1}$ for *p*-nitrophenol and $9.57\ \mu\text{g kg}^{-1}$ for MP. Also, it could detect and quantify the content of $10\text{--}10\,000\ \mu\text{g kg}^{-1}$ for *p*-nitrophenol and $25\text{--}7500\ \mu\text{g kg}^{-1}$ MP. Moreover, this method could also be utilized to study the gene expression in complex environments.¹⁷²

Further, the extensive use of organophosphorus pesticides (OPs) in agriculture has reduced the possible threats of residue complications. Therefore, it is highly essential and desirable to develop operative diagnostic methods (e.g., rapid and reliable biosensor). In general, conventional biosensors majorly depend

on biorecognition components, which limit their real-world applications. Thus, to address these issues, nanozymes are broadly utilized in developing nanozyme-enabled biosensors owing to their inexpensive nature, remarkable stability, and promising catalytic action.¹⁷³ In this advancement, in 2022, Song *et al.* developed an AChE-nanozyme bioactive paper together with a 3D-printed system for the fast detection of different pesticides. After serially incorporating AChE, acetylcholine (ACh), and TMB, and H_2O_2 solutions *via* various syringes on the 3D printed system, the SAzyme (SACe-N-C) with peroxidase-like action exhibited continuous responses to AChE. However, OPs may impede the action of AChE and yield less or no choline (no reduction of blue oxTMB, oxidized by SACe-N-C)





Fig. 8 (I) Schematic illustration of manufacturing of paper-strip biosensor. (II) Diagram of whole-cell biosensor device for detecting MP and *p*-nitrophenol (*p*-NP): flow-diagram of the fabrication and utilization (A) and objective drawing (B) of whole-cell paper-strip biosensor. Reproduced with permission from ref. 172 Copyright 2023, Elsevier.

to the colorless redTMB successively, leading to the release of the action of SAcE-N-C and generation of the color of bioactive paper positively according to content of OPs. Moreover, this biosensing device could monitor the concentration of OP residues in fruits and vegetables within 30 min with an LOD of 55.83 ng mL^{-1} and 77.51 ng mL^{-1} for omethoate and methamidophos, respectively.¹⁷⁴

The occurrence of antibiotic-resistant bacteria due to the presence of antibiotics in environmental water is a serious issue. In this case, rapid and sensitive colorimetric paper-based biosensing devices can be utilized for detecting antibiotics the inhibit bacterial protein synthesis. By considering the concept of color change induced by β -galactosidase synthesis in real water samples without antibiotics, it exhibited the approximate limit of detection by the naked eye of 0.5, 2.1, 0.8, and 6.1 mg mL^{-1} for paromomycin, tetracycline, chloramphenicol, and erythromycin, respectively, by hampering the inhibition of β -galactosidase synthesis with antibiotics.¹⁷⁵

4.3. Food industry

Microorganisms such as bacteria, fungi, and viruses play a vital role in our life, wherein some microorganisms (e.g., *Penicillium* (2), *Saccharomyces* (1), and *Lactobacillus* (3)) are beneficial and broadly utilized in the food and medicinal industries. However, in many cases, the microbial contamination of food causes severe health problems, leading to significant economic loss annually. Therefore, the fast, sensitive, specific, and visual detection of microbes in food items is highly desirable. In this regard, various microbial detection devices have been developed, but they are complex and time-consuming methods, and are not effective in growing food testing demands. The climate change and increasing global population, which affect

agriculture and food safety, are major challenges worldwide, wherein the agricultural and food industries are the major support of our society and essential to be developed uninterruptedly to realize improved productivity and quality. For this purpose, fertilizers and pesticides have been extensively utilized in modern times for tremendous profits to agricultural productivity; however, the harmful impact of their residues in food products and environmental contamination cannot be ignored.¹⁷⁶ Some chemicals hazards (e.g., pesticides and veterinary drug residues), illegal or excessive additives, environmental impurities, natural toxins, and biological hazards (e.g., microbial impurities) can have adverse effects on human health even at low levels.^{177,178} Thus, suitable, effective, selective, and sensitive diagnostic devices are greatly desirable. In recent times, sensors as diagnostic devices showed an advantage of straightforward operation, high proficiency, and sensitivity. These devices include sensitive elements and conversion elements, which can quantify specific targets by converting them into usable signals according to certain laws.^{178,179} Herein, paper-based biosensors are very effective for the efficient and visual detection of microorganisms for food safety and environmental hygiene owing to their simple, low-cost, high speed, and all-in-one device.⁸⁸ In a study, an inexpensive and dual-step pen-on-paper strategy was used to fabricate a fully drawn fluidic patterned electrochemical paper-based biosensor for the amperometric enzymatic determination of glucose, wherein glucose oxidase and potassium ferricyanide (as the mediator) were immobilized in the test area. The results exhibited the limit of quantification of 0.08 mmol L^{-1} , reproducibility of $<12\%$ for 6 different devices, and the assay time of 120 s. This device was applied for the determination of glucose in food samples with 94–106% recovery.¹⁸⁰ Some paper-based



biosensing devices exhibited low sensitivity, and in this case, aptamers as bioreceptors are used to improve the selectivity and sensitivity of the sensors, specifically paper-based biosensors. Therefore, a paper-based electrochemical aptasensor was developed to detect ractopamine (RAC) with good sensitivity and selectively under the optimal conditions in the range of 0.001 μM to 100 mM (lower limit of quantification: 0.01 μM). Further, the monitoring of RAC in non-treated human plasma samples was observed with the lower limit of quantification of 0.01 μM and linear range of 0.01 μM –10 mM.¹⁸¹

Contamination of foods is the greatest concern to consumers,¹⁸² wherein food contamination occurs in various ways (e.g., physical, chemical, and biological processes). Among them, infectious microorganisms are the most serious contaminants of food, especially in packaged foods.¹⁸³ In this situation, the development of active and sensitive food packaging is highly desirable to protect and preserve foods or communicate between packaging foods and consumers.^{184,185} Therefore, the integration of biopolymer-based smart food packaging with biosensing entities has provided an attractive opportunity for the real-time monitoring of the microbial breakdown of packaged foods for food quality and safety.¹⁸⁶

The trustworthy detection of pathogenic bacteria in complex biological specimens using simple assays or sensing devices remains a key challenge. A simple colorimeter paper biosensing device was developed and used to detect *Helicobacter pylori* (*H. pylori*) specifically and sensitively. *H. pylori* is a pathogen intensely connected to gastric carcinoma, gastric ulcers, and duodenal ulcers in stool samples. The sensor device was designed based on the RNA-cleaving characteristic of the DNzyme, which is activated by a protein biomarker from *H. pylori*, enabling the sensitive and rapid detection of *H. pylori* in a human stool specimen within minutes. Moreover, the diagnostic device maintained its functionality under storage for at least 130 days at ambient temperature.¹⁸⁷ A multiplex lateral flow immunoassay (LFA) was developed to detect primary marine biotoxins (e.g., amnesic, paralytic, and diarrhetic shellfish poisoning toxins) with a single sample isolation method and diluted volume and showed no matrix effect on its detection performance.¹⁸⁸

Infections triggered by Gram-positive bacteria cause several severe diseases (e.g., bacteremia, sepsis, pneumonia, osteomyelitis, and endocarditis).^{189,190} Therefore, the rapid inspection of Gram-positive bacteria-contaminated food stuffs is highly required to prevent and control the epidemic situations induced by them.¹⁹¹ Compared to the lengthy traditional approach, nucleic acid-, immunological-, and biosensing-based strategies have been developed to reduce the time for detecting bacteria.^{192–194} However, the possible interference of a complex matrix on these approaches may generate false-positive or negative outcomes with no cultural supplementation. Thus, the development of pre-processing approaches to overcome matrix-linked inhibition and reach the low content of bacteria in foodstuffs is crucial to improve the accuracy of these approaches. Herein, an on-site colorimeter biosensing device was developed for ultrasensitive and fast recognition

by using polydopamine and polyethyleneimine (PDA-PEI)-functionalized papers (PDA-PEI@paper) for isolating bacteria and peptidoglycan-targeting carbon dots for the selective colorimetric recognition of Gram-positive bacteria. Moreover, this device could detect *S. aureus* up to 1 cfu mL⁻¹, *L. monocytogenes* up to 5 cfu mL⁻¹, and *B. subtilis* up to 9 cfu mL⁻¹ within 55 min. Also, the recognition of Gram-positive bacteria was performed in the samples of eggshell and sausage with recoveries in the range of 91.2–110%.¹⁹⁵ In another study, AuNPs were utilized in a paper-based DNA biosensing device for the visual detection of dairy products for their food authenticity, wherein species-specific DNA sequences were separated, intensified and recognized using specific DNA probes in the biosensing device. In this case, three species (e.g., cow, sheep, and goat) were analyzed as low as 1.6 fmol for cow and goat, and 3.1 fmol for sheep PCR result. In addition, contamination down to 0.01% could also be detected based on binary mixtures of milk yogurts of cow, goat, and sheep having 0.01% to 5% of cow yogurt in the yogurt of the sheep and goat, respectively. Overall, this biosensing device exhibited good specificity, reproducibility, and 10 fold detectability compared to other methods.¹⁹⁶

Salmonella causes millions of foodborne illnesses annually and result in higher death rates compared to other foodborne bacterial pathogens. A colorimeter paper-based analytical device (PAD) linked with immunomagnetic separation (IMS) was used for the specific detection of *Salmonella typhimurium* (*S. typhimurium*) without any interference from other pathogenic bacteria (e.g., *Escherichia coli*). The LOD for *S. typhimurium* was observed to be 102 CFU mL⁻¹, and also this device was utilized for inoculated Starling bird fecal and whole milk samples with an LOD of 105 CFU g⁻¹ and 103 CFU mL⁻¹, respectively.¹⁹⁷ The analysis of complex matrices in food samples is tedious due to the interference among them. In this case, optical biosensors with chemiluminescence and fluorescence detection mechanisms have been developed and applied over traditional methods due to their good sensitivity and selectivity. For example, phenolic compounds (PCs), which are key plant ingredients having redox characteristics responsible for antioxidant action, were detected by a paper-based chemiluminescence smartphone biosensing device. In this study, molasses, honey, and tea as food samples were analyzed and showed the LOD for PCs of 0.12, 0.28, 0.46, 0.85, and 1.23 $\mu\text{g mL}^{-1}$ for gallic acid, quercetin, catechin, kaempferol, and caffeic acid, respectively.¹⁹⁸ For the detection of procymidone in vegetables, three paper-based biosensor devices using a core biological immune scaffold (CBIS) were fabricated as time-resolved fluorescence immunochromatography strips with europium oxide (Eu-TRFICS). Herein, CBIS was designed using secondary fluorescent probes (of goat anti-mouse IgG and europium oxide time-resolved fluorescent microspheres) and procymidone monoclonal antibody (PCM-Ab). Three paper-based devices of Eu-TRFICS-1 (fixing of secondary fluorescent probes onto conjugated pad and mixing of PCM-Ab in a sample solution), Eu-TRFICS-2 (fixing of CBIS onto conjugate pad), and Eu-TRFICS-3 (direct mixing of CBIS with sample solution). These systems demonstrated multidimensional labeling and



directional-coupling (by resolving the difficulties of steric interruption of antibody labeling, inadequate exposure of antigen-recognition zone and easy loss of action in conventional methods). Among the three types, Eu-TRFICS-1 exhibited the best detection ability with the reduction of antibody usage by 25%, increased sensitivity by 3 times, detection of range of 1–800 ng mL⁻¹, and LOD of 0.12 ng mL⁻¹ with a visible LOD of 5 ng mL⁻¹.¹⁹⁹

The freshness of fresh meat can be evaluated by determining the Hx level (a metabolic product of ATP metabolism) and it can be utilized as a biomarker for detecting the early stage of spoilage.²⁰⁰ In a study, a pattern-free paper enzyme biosensing device was fabricated for one-step fish-freshness detection by indicating hypoxanthine (Hx). For this development, chitosan oligosaccharide lactate-functionalized nitrocellulose (NC) membranes were immobilized with a dual-enzyme system (xanthine oxidase and horseradish peroxidase) and showed a remarkable microfluidic accumulation effect. The as-developed biosensing device showed a color within 3 min and exhibited a linear response of 0.01–0.16 mmol L⁻¹ with an LOD of 8.22 μmol L⁻¹, and selective recognition of Hx with satisfactory recoveries of 96.13–103.11% for fish specimens. Herein, the biochemical signal of Hx level was converted to a colorimetric signal *via* a two-step enzymatic interaction for visual detection. Also, a remarkable color distinction between the negative specimen (colorless) and positive specimen (green) with the naked eyes could be observed by attaching it directly to the surface of fish meat. Also, quantitative analysis could be achieved using a smartphone.²⁰¹ Most recently, in 2024, Li *et al.* reported the fabrication of a pomegranate-structured film-based sensing device using PANI, multi-branched cellulose

nanofibers (MCNFs), and multi-walled carbon nanotubes (MWCNTs) for the detection of human-physiology and food spoilage gas signals for real-time monitoring by integrating it with a wireless heart-rate display and smart packaging censoring technique.²⁰²

4.4. Environmental pollutants

Various environmental pollutants pose a significant threat to human health and the global climate (atmosphere). Among them, the contamination of heavy metal ions in water is gaining considerable interest due to their serious harmful consequences to human health and adverse ecological effects. Mercury (Hg²⁺) and lead (Pb²⁺) are toxic metals present in water, posing a remarkable hazard to the environment and aquatic life *via* biological accumulation in the food chain, ultimately affecting human health. Exposure to even a trace amount of Hg²⁺ can trigger severe damage to human organs.²⁰³ Also, the accumulation of Pb²⁺ beyond a threshold value causes permanent damage.²⁰⁴ In this case, *in vitro* transcription (IVT) technology with an allosteric transcription factor (aTF)-based cell-free paper-based biosensor device was developed for the on-site detection of Hg²⁺ and Pb²⁺ simultaneously in a consistent and sensitive mode with just one drop of water (Fig. 9). It could detect Hg²⁺ and Pb²⁺ quantitatively in a linear range of 0.5–500 nM and 1–250 nM within a period of one hour, with an LOD of 0.5 nM and 0.1 nM for Hg²⁺ and Pb²⁺, respectively. Moreover, the recoveries ranged from 91.09% to 123.24% for the detection of real water models.²⁰⁵

Water-borne pathogens are also causing a remarkable increment in mortality rate due to issues such as poor sanitation, sewage sludge, and industrial effluents. Thus, to prevent this,



Fig. 9 (a) Schematic illustration of the development and application of paper-based biosensing device, (b) fluorescence output of paper-based biosensing device at different contents of Hg²⁺ and Pb²⁺, and (c) detection of real water models using this inexpensive and portable paper-based biosensing device. Reproduced with permission from ref. 205 Copyright 2021, Elsevier.

easy, sensitive, user-friendly, and rapid on-site biosensor devices for detecting pathogens are needed. In this advancement, an inexpensive, label-free, and eco-friendly paper-based screen-printed graphene oxide (GO)-functionalized electrochemical impedimetric biosensing device immobilized with lectin Concanavalin A (ConA) as the biorecognition unit was developed for the detection of a water-borne bacterial contamination, *Escherichia coli*, in water. Mechanistically, the high surface area and chemical action of GO on graphene led to the remarkably specific immobilization of ConA in bulk quantity onto the surface of GO owing to its active functional groups ($-\text{COOH}$) for site-specific reaction in the pH range of 4.5–6.0. This device achieved ultra-high sensitivity for detecting bacterial contamination over a wide linear range of 102–108 CFU mL^{-1} and ultra-low LOD of 0.1×10^2 CFU mL^{-1} without any chemical intensification.²⁰⁶ In another study, a 'turn-off' fluorescent biosensing device (mCherry L199C) for sensing Hg^{2+} was designed and developed *via* the direct modification of the chromophore environment of the fluorescent protein mCherry. The designed variant of mCherry L199C was expressed directly on the outer-membrane of *E. coli* cells *via* the cell surface display approach. The fluorescent biosensing device exhibited a favorable response to Hg^{2+} at the micromole level among other metal ions and over a wide pH range. The cells of this biosensor were incorporated in an alginate hydrogel to develop cell-alginate hydrogel-based paper. This system was simple and inexpensive, which could detect mercury pollution within 5 min and keep stable fluorescence and activity at 4 °C for 24 h.²⁰⁷

4.5. Other applications

There are various other mixed applications, wherein paper-based sustainable biosensing devices have been utilized for

desired outcomes as efficient diagnostic platforms. For example, a biosensor composed of a hydrophilic cellulosic paper disk with immobilized GOX placed on SPCE was developed and this biosensing device, using 0.1 M phosphate buffer solution (PBS, pH 7.0) and 10 mM soluble ferrocene monocarboxylic acid mediator, detected a low amount of glucose (5 μL) and showed a linear range of 1–5 mM glucose with an LOD of 0.18 mM, and maintained 98% of its activity after a period of 4 months. It was successfully utilized for the selective and sensitive assay of glucose in various commercial soda beverages.²⁰⁸ In another study, the level of glucose in beverages (*e.g.*, commercial orange juice) *via* potentiometric detection was monitored using a developed novel paper-based biosensor device. In this case, the electrodes were composed of platinized paper as a support and a biocompatible polymeric membrane composed of a blend of chitosan and poly(vinyl alcohol) holding glucose oxidase as the recognition layer. This biosensing device selectively and sensitively detected H_2O_2 produced by an enzymatic response. It exhibited rapid and accurate results, presenting the sensitivity of 119 ± 6.4 mV dec^{-1} in the range of 0.03–1.0 mM with an LOD of 0.02 mM.²⁰⁹ Presently, the use of volatile toxic complexes as chemical weapons as a large-scale destructive system has posed a new threat worldwide. In this case, the development of effective wearable sensing devices can be a good candidate for security monitoring. Therefore, a wearable electrochemical biosensor was fabricated for the rapid and on the spot detection of mustard agents directly in the aerosol phase. In this case, the electrodes were screen-printed onto a filter paper to create an origami-like and reagent-free device. The detection of mustard agents was conducted by monitoring their inhibitory effects *via* amperometric analysis of an enzymatic by-product (hydrogen peroxide, H_2O_2). In addition, the nanocomposite of carbon black/Prussian blue

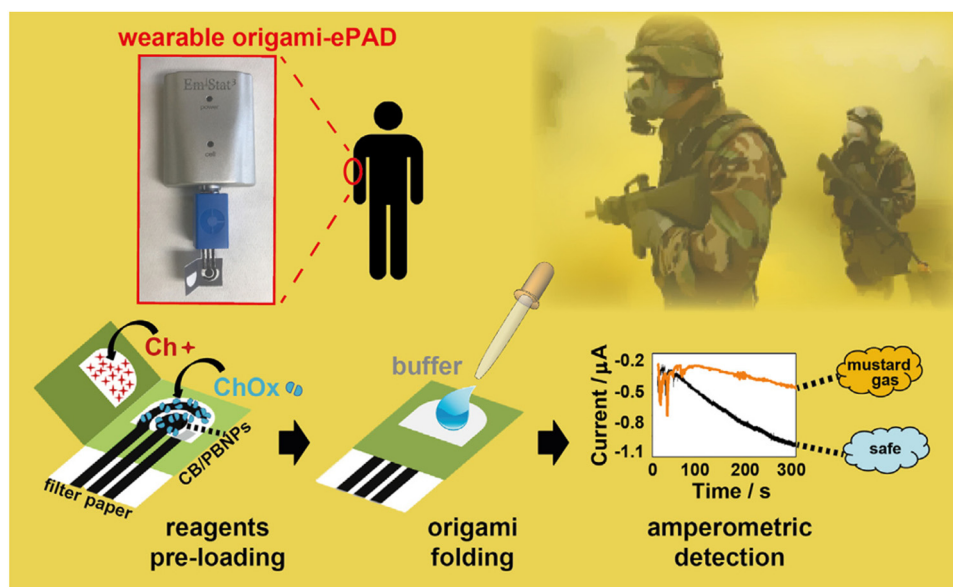


Fig. 10 Schematic of the working principle of the developed wearable origami-like ePAD. Reproduced with permission from ref. 161 Copyright 2019, Elsevier.



was utilized to modify the conductive graphite ink forming the working electrode for the electrocatalysis of H_2O_2 reduction. Moreover, after verification with a mustard agent, the developed origami-like biosensor was used to detect real sulfur mustard rapidly and in real time, demonstrating the LOD of 1 mM and $0.019 \text{ g min m}^{-3}$ for the liquid and aerosol phases, respectively (Fig. 10).¹⁶¹

5. Conclusion, challenges and future research directions

In this review, the fundamentals of sensing or biosensing devices and their utilized materials were precisely described. To guide the future research on the design of biosensors or bioelectronics, we focused on discussing the efficacy of the use of renewable and sustainable materials for biosensing devices as an alternative to petroleum-based polymers. Further, the recent advances in emerging paper-based sustainable materials and high-performance devices in biosensing, such as healthcare, agriculture, food industry, environmental pollutants, and others were discussed.

As discussed above, renewable and sustainable materials have received significant attention in the past few years in terms of basic research and real-world applications owing to their ability to minimize environmental, consumption, and cost-related issues. Accordingly, these materials have widely been utilized in pristine form or in combination to manufacture sensing and biosensing devices for suitable and targeted utilization and outcomes with low cost, satisfactory biodegradability, high flexibility, and low-energy consumption. Herein, paper is a workable alternative to traditional materials utilized in biosensing devices for various applications due to its inexpensive nature, flexibility, fluid conduct (capillary action due to rough fibrous-network), significant sensitivity and easy disposal. In addition, the combination of cellulose with a diverse range of additives (e.g., conductive polymers and nanomaterials) produces composite materials with remarkable electrical conductivity, while preserving the sustainability and biocompatibility of cellulose. Therefore, extensive research activities on paper- and cellulose-based biosensing devices have widely been reported and still on-going for effective utilization in various potential applications. However, there are still various challenges in using renewable materials in developing inexpensive sensing devices with satisfactory sensitivity, selectivity, response time, steadiness, and operational durability. Furthermore, they require an enhanced operational timing, low maintenance and installation cost, and data management.

For an independent measurement of environmental factors, calibrations, numerical corrections, and doping or coating methods are used for precise and effective operations. Further, with the development of communication technologies, high-frequency microprocessors, the Internet of things, real-time detection, and storage capacity, the successful integration of these technologies into the developed biosensing devices for on-spot real-time data is still another challenge. Various design

approaches and fabrication technologies should be used to enhance or convert renewable materials into value-added inexpensive products with desirable properties such as mechanical strength, flexibility, thermal stability, electrical characteristics, and recyclability. Significant functioning and advances in computer science with machine learning algorithms are beneficial in achieving optimal parameters and reduction in operational time and associated costs.^{210–212} In addition, artificial intelligence methods have provided a great opportunity in all sections of the world by allowing machines to mimic imagination, decision-making process, and manufacturing new materials.^{213,214} In this case, the use of microfabrication technologies (e.g., additive manufacturing) will decrease the time of manufacturing with anticipated structural design and reduction in wastage of materials, thereby decreasing the overall cost of the product.^{66,215} Moreover, the economic and technological challenges must be considered and encouraged by scientific research to convince decision-makers to develop the ideas for new sensing and biosensing devices.

Conflicts of interest

There are no conflicts to declare.

Acknowledgements

A. K. acknowledges the support from the Ramalingaswami Re-entry Fellowship (Ref: BT/HRD/35/02/2006) of Department of Biotechnology, Government of India.

References

- 1 H. Teymourian, M. Parrilla, J. R. Sempionatto, N. F. Montiel, A. Barfidokht, R. Van Echelpoel, K. De Wael and J. Wang, *ACS Sens.*, 2020, **5**, 2679–2700.
- 2 J. van der Zalm, S. Chen, W. Huang and A. Chen, *J. Electrochem. Soc.*, 2020, **167**, 037532.
- 3 D. Li, H. Duan, Y. Ma and W. Deng, *Anal. Chem.*, 2018, **90**, 5719–5727.
- 4 H. Nawaz, J. Zhang, W. Tian, K. Jin, R. Jia, T. Yang and J. Zhang, *J. Hazard. Mater.*, 2020, **387**, 121719.
- 5 A. Pavinatto, L. A. Mercante, C. S. Leandro, L. H. Mattoso and D. S. Correa, *J. Electroanal. Chem.*, 2015, **755**, 215–220.
- 6 J. Fan, S. Zhang, F. Li and J. Shi, *Cellulose*, 2020, **27**, 5477–5507.
- 7 G. Barandun, M. Soprani, S. Naficy, M. Grell, M. Kasimatis, K. L. Chiu, A. Ponzoni and F. Güder, *ACS sensors*, 2019, **4**, 1662–1669.
- 8 R. Prathapan, R. F. Tabor, G. Garnier and J. Hu, *ACS Appl. Bio Mater.*, 2020, **3**, 1828–1844.
- 9 F. Arduini, L. Micheli, V. Scognamiglio, V. Mazzaracchio and D. Moscone, *TrAC, Trends Anal. Chem.*, 2020, **128**, 115909.
- 10 K. Ratajczak and M. Stobiecka, *Carbohydr. Polym.*, 2020, **229**, 115463.



- 11 K. B. Teodoro, R. C. Sanfelice, F. L. Migliorini, A. Pavinatto, M. H. Facure and D. S. Correa, *ACS Sens.*, 2021, **6**, 2473–2496.
- 12 S. Kamel and T. A. Khattab, *Biosensors*, 2020, **10**, 67.
- 13 V. B. C. Lee, N. F. Mohd-Naim, E. Tamiya and M. U. Ahmed, *Anal. Sci.*, 2018, **34**, 7–18.
- 14 B. G. Andriyukov, *AIMS Microbiol.*, 2020, **6**, 280.
- 15 E. Solhi, M. Hasanzadeh and P. Babaie, *Anal. Methods*, 2020, **12**, 1398–1414.
- 16 A. Antonacci, V. Scognamiglio, V. Mazzaracchio, V. Caratelli, L. Fiore, D. Moscone and F. Arduini, *Front. Bioeng. Biotechnol.*, 2020, **8**, 339.
- 17 W.-J. Lan, X. U. Zou, M. M. Hamed, J. Hu, C. Parolo, E. J. Maxwell, P. Bühlmann and G. M. Whitesides, *Anal. Chem.*, 2014, **86**, 9548–9553.
- 18 N. F. Santos, S. O. Pereira, A. Moreira, A. V. Girão, A. F. Carvalho, A. J. Fernandes and F. M. Costa, *Adv. Mater. Technol.*, 2021, **6**, 2100007.
- 19 N. Nontawong, M. Amatatongchai, W. Wuepchaiyaphum, S. Chairam, S. Pimmongkol, S. Panich, S. Tamuang and P. Jarujamrus, *Int. J. Electrochem. Sci.*, 2018, **13**, 6940–6957.
- 20 X. Jin, C. Liu, T. Xu, L. Su and X. Zhang, *Biosens. Bioelectron.*, 2020, **165**, 112412.
- 21 P. Gründler, *Chemical Sensors: An Introduction for Scientists and Engineers*, Springer Science & Business Media, 2007.
- 22 A. A. Ensafi, *Electrochemical Biosensors*, Elsevier, 2019, pp. 1–10.
- 23 S. Li, Y. Zhang, Y. Wang, K. Xia, Z. Yin, H. Wang, M. Zhang, X. Liang, H. Lu and M. Zhu, *InfoMat*, 2020, **2**, 184–211.
- 24 J. Janata, *Principles of chemical sensors*, Springer Science & Business Media, 2010.
- 25 M. S. H. Ador, P. Bhattacharjee, S. Kabir, M. T. Ahmed, F. Ahmed and I. A. Choudhury, *Ref. Module Mater. Sci. Mater. Eng.*, 2023, DOI: [10.1016/B978-0-323-96020-5.00043-1](https://doi.org/10.1016/B978-0-323-96020-5.00043-1).
- 26 F.-G. Banica, *Chemical sensors and biosensors: fundamentals and applications*, John Wiley & Sons, 2012.
- 27 A. P. Turner, *Chem. Soc. Rev.*, 2013, **42**, 3184–3196.
- 28 A. Qureshi, Y. Gurbuz and J. H. Niazi, *Sens. Actuators, B*, 2012, **171**, 62–76.
- 29 S. Saha, M. Tomar and V. Gupta, *J. Appl. Phys.*, 2012, **111**, 102804.
- 30 L. C. Clark Jr and C. Lyons, *Ann. N. Y. Acad. Sci.*, 1962, **102**, 29–45.
- 31 G. A. Rechnitz, R. Kobos, S. Riechel and C. Gebauer, *Anal. Chim. Acta*, 1977, **94**, 357–365.
- 32 N. Bhattacharyya, S. Jain, S. Bhattacharyya, S. Pal, A. Jana and S. Mukherjee, *Ref. Module Mater. Sci. Mater. Eng.*, 2023, DOI: [10.1016/B978-0-323-96020-5.00058-3](https://doi.org/10.1016/B978-0-323-96020-5.00058-3).
- 33 D. G. Buerk, *Biosensors: Theory and applications*, CRC Press, 2014, DOI: [10.1201/9781498710770](https://doi.org/10.1201/9781498710770).
- 34 C. Karunakaran, K. Bhargava and R. Benjamin, *Biosensors and Bioelectronics*, Elsevier, 2015.
- 35 M. Zamani, J. Dupaty, R. Baer, U. Kuzmanovic, A. Fan, M. W. Grinstaff, J. E. Galagan and C. M. Klapperich, *ACS Omega*, 2022, **7**, 5804–5808.
- 36 F. S. Ligler and C. R. Taitt, *Optical biosensors: today and tomorrow*, Elsevier, 2011.
- 37 C. Steinem and A. Janshoff, *Piezoelectric Sensors*, Springer Science & Business Media, 2007.
- 38 S. Zhou, Y. Zhao, M. Mecklenburg, D. Yang and B. Xie, *Biosens. Bioelectron.*, 2013, **49**, 99–104.
- 39 S. Cosnier, *Electrochemical biosensors*, CRC Press, 2015.
- 40 O. Tokel, F. Inci and U. Demirci, *Chem. Rev.*, 2014, **114**, 5728–5752.
- 41 S. Sang, Q. Feng, X. Tang, T. Wang, X. Huang, A. Jian, Z. Ma and W. Zhang, *Microelectron. Eng.*, 2015, **134**, 33–37.
- 42 V. Naresh and N. Lee, *Sensors*, 2021, **21**, 1109.
- 43 S. Varshney, P. K. Rajput, A. Singhal and G. Varshney, *Mater. Today: Proc.*, 2022, **62**, 6679–6683.
- 44 G. Dandegaonkar, A. Ahmed, L. Sun, B. Adak and S. Mukhopadhyay, *Mater. Adv.*, 2022, **3**, 3766–3783.
- 45 H. Ma, Z. Cheng, X. Li, B. Li, Y. Fu and J. Jiang, *J. Bioresour. Bioprod.*, 2023, **8**, 15–32.
- 46 L. Wang, D. Chen, K. Jiang and G. Shen, *Chem. Soc. Rev.*, 2017, **46**, 6764–6815.
- 47 H. Zhu, W. Luo, P. N. Ciesielski, Z. Fang, J. Zhu, G. Henriksson, M. E. Himmel and L. Hu, *Chem. Rev.*, 2016, **116**, 9305–9374.
- 48 S. Sreejith, L. L. Joseph, S. Kollem, V. Vijumon and J. Ajayan, *Measurement*, 2023, 113261.
- 49 Q. Wang, T. Liu, X. Xu, H. Chen and S. Chen, *Int. J. Biol. Macromol.*, 2021, **169**, 60–66.
- 50 D. Molinnus, A. Drinic, H. Iken, N. Kröger, M. Zinser, R. Smeets, M. Köpf, A. Kopp and M. J. Schöning, *Biosens. Bioelectron.*, 2021, **183**, 113204.
- 51 J. Park, J.-K. Kim, S. A. Park and D.-W. Lee, *Microelectron. Eng.*, 2019, **206**, 1–5.
- 52 D. Zhao, Y. Zhu, W. Cheng, W. Chen, Y. Wu and H. Yu, *Adv. Mater.*, 2021, **33**, 2000619.
- 53 K. Xia, X. Chen, X. Shen, S. Li, Z. Yin, M. Zhang, X. Liang and Y. Zhang, *ACS Appl. Electron. Mater.*, 2019, **1**, 2415–2421.
- 54 H. Qi, J. Liu, J. Pionteck, P. Pötschke and E. Mäder, *Sens. Actuators, B*, 2015, **213**, 20–26.
- 55 H. Koga, M. Nogi, N. Komoda, T. T. Nge, T. Sugahara and K. Suganuma, *NPG Asia Mater.*, 2014, **6**, e93–e93.
- 56 R. K. Mishra, P. Mishra, K. Verma, A. Mondal, R. G. Chaudhary, M. M. Abolhasani and S. Loganathan, *Environ. Chem. Lett.*, 2019, **17**, 767–800.
- 57 S.-Y. Cho, H. Yu, J. Choi, H. Kang, S. Park, J.-S. Jang, H.-J. Hong, I.-D. Kim, S.-K. Lee and H. S. Jeong, *ACS Nano*, 2019, **13**, 9332–9341.
- 58 P. Sukhavattanukul and H. Manuspiya, *Carbohydr. Polym.*, 2020, **230**, 115566.
- 59 J.-W. Han, B. Kim, J. Li and M. Meyyappan, *J. Phys. Chem. C*, 2012, **116**, 22094–22097.
- 60 J.-W. Han, B. Kim, J. Li and M. Meyyappan, *Rsc Adv.*, 2014, **4**, 549–553.
- 61 T. S. D. Le, S. Park, J. An, P. S. Lee and Y. J. Kim, *Adv. Funct. Mater.*, 2019, **29**, 1902771.
- 62 S. Teng, G. Siegel, W. Wang and A. Tiwari, *ECS Solid State Lett.*, 2014, **3**, M25.



- 63 S. K. Mahadeva, K. Walus and B. Stoeber, *ACS Appl. Mater. Interfaces*, 2014, **6**, 7547–7553.
- 64 H. Koga, K. Nagashima, Y. Huang, G. Zhang, C. Wang, T. Takahashi, A. Inoue, H. Yan, M. Kanai and Y. He, *ACS Appl. Mater. Interfaces*, 2019, **11**, 15044–15050.
- 65 M. Niu, Y. Yao, Y. Shi, J. Luo, X. Duan, T. Liu and X. Guo, *Ind. Eng. Chem. Res.*, 2019, **58**, 10364–10372.
- 66 A. Nasri, M. Petrissans, V. Fierro and A. Celzard, *Mater. Sci. Semicond. Process.*, 2021, **128**, 105744.
- 67 R. Tang, M. Y. Xie, M. Li, L. Cao, S. Feng, Z. Li and F. Xu, *Appl. Mater. Today*, 2022, **26**, 101305.
- 68 A. Singh, D. Lantigua, A. Meka, S. Taing, M. Pandher and G. Camci-Unal, *Sensors*, 2018, **18**, 2838.
- 69 A. Kumar, K. Chen, T. Thundat and M. T. Swihart, *ACS Appl. Mater. Interfaces*, 2023, **15**, 5439–5448.
- 70 A. Quddious, S. Yang, M. M. Khan, F. A. Tahir, A. Shamim, K. N. Salama and H. M. Cheema, *Sensors*, 2016, **16**, 2073.
- 71 E. Noviana, D. B. Carrão, R. Pratiwi and C. S. Henry, *Anal. Chim. Acta*, 2020, **1116**, 70–90.
- 72 C.-M. Wang, C.-Y. Chen and W.-S. Liao, *Anal. Chim. Acta*, 2021, **1144**, 158–174.
- 73 M. A. Hubbe and R. A. Gill, *BioResources*, 2016, **11**, 2886–2963.
- 74 K. J. Hipolit, *Chemical Processing Aids in Papermaking: A Practical Guide*, Tappi press, 1992.
- 75 R. Bown, *Pap. Technol.*, 1998, **39**, 44–48.
- 76 R. Davidson, *Pap. Technol.*, 1965, **6**, 107–114.
- 77 N. L. Salmen, *Tappi*, 1980, **63**, 117–120.
- 78 F. Brunetti, A. Operamolla, S. Castro-Hermosa, G. Lucarelli, V. Manca, G. M. Farinola and T. M. Brown, *Adv. Funct. Mater.*, 2019, **29**, 1806798.
- 79 L. Chen, J. Lv, L. Ding, G. Yang, Z. Mao, B. Wang, X. Feng, S. Zapotoczny and X. Sui, *Chem. Eng. J.*, 2020, **400**, 125950.
- 80 J. H. Kim, D. Lee, Y. H. Lee, W. Chen and S. Y. Lee, *Adv. Mater.*, 2019, **31**, 1804826.
- 81 X. Zhao, W. Han, Y. Jiang, C. Zhao, X. Ji, F. Kong, W. Xu and X. Zhang, *Nanoscale*, 2019, **11**, 17725–17735.
- 82 Z. Wang, Y. H. Lee, S. W. Kim, J. Y. Seo, S. Y. Lee and L. Nyholm, *Adv. Mater.*, 2021, **33**, 2000892.
- 83 S. M. Khan, J. M. Nassar and M. M. Hussain, *ACS Appl. Electron. Mater.*, 2020, **3**, 30–52.
- 84 D. Zhang and Q. Liu, *Biosens. Bioelectron.*, 2016, **75**, 273–284.
- 85 P. K. Yang, Z. H. Lin, K. C. Pradel, L. Lin, X. Li, X. Wen, J. H. He and Z. L. Wang, *ACS Nano*, 2015, **9**, 901–907.
- 86 N. C. Sekar, L. Ge, S. A. M. Shaegh, S. H. Ng and S. N. Tan, *Sens. Actuators, B*, 2015, **210**, 336–342.
- 87 J. Cheng, Y. Fu, J. Guo and J. Guo, *Sens. Actuators, B*, 2023, **387**, 133795.
- 88 J. Li, K. Chen, Y. Su, L. Zhu, H. Zhang, W. Xu and X. Li, *Journal of Future Foods*, 2024, **4**, 61–70.
- 89 Y. Shen and A. Mulchandani, *Biosens. Bioelectron.: X*, 2023, 100364.
- 90 T. Pinheiro, A. R. Cardoso, C. E. Sousa, A. C. Marques, A. P. Tavares, A. M. Matos, M. T. Cruz, F. T. Moreira, R. Martins and E. Fortunato, *ACS Omega*, 2021, **6**, 29268–29290.
- 91 L. Xu, Z. Zhou, M. Fan and X. Fang, *Int. J. Electrochem. Sci.*, 2023, **18**, 13–19.
- 92 Z. Ouyang, S. Li, J. Liu, H.-Y. Yu, L. Peng, S. Zheng, D. Xu and K. C. Tam, *Nano Energy*, 2022, **104**, 107963.
- 93 M. Yence, A. Cetinkaya, S. I. Kaya, G. Ozcelikay and S. A. Ozkan, in *Recent Developments in Green Electrochemical Sensors: Design, Performance, and Applications*, ACS Publications, 2023, pp. 411–439.
- 94 K. Beaver, A. Dantanarayana and S. D. Minter, *J. Phys. Chem. B*, 2021, **125**, 11820–11834.
- 95 N. Postulka, T. Meckel and M. Biesalski, *Langmuir*, 2021, **37**, 8746–8752.
- 96 W. Heng, L. Weihua and K. Bachagha, *Carbohydr. Polym.*, 2023, 121306.
- 97 R. Gerulskis and S. D. Minter, *ECS Adv.*, 2023, **2**, 035501.
- 98 S. Selvaraj and D. R. Shankaran, *ChemistrySelect*, 2023, **8**, e202302027.
- 99 X. Li, H. Yang, S. Lu and R. Cai, *Adv. Mater. Technol.*, 2023, 2300079.
- 100 A. Uçar, G. A. Tiğ and E. Er, *TrAC, Trends Anal. Chem.*, 2023, 117027.
- 101 R. Moscoso, S. Abarca, C. Yáñez and J. Squella, *Electrochim. Acta*, 2023, **443**, 141984.
- 102 P. B. Deroco, D. Wachholz Junior and L. T. Kubota, *Electroanalysis*, 2023, **35**, e202200177.
- 103 S. R. Benjamin, F. de Lima, V. A. D. Nascimento, G. M. de Andrade and R. B. Oriá, *Biosensors*, 2023, **13**, 689.
- 104 T. S. Martins, S. A. Machado, O. N. Oliveira Jr and J. L. Bott-Neto, *Food Chem.*, 2023, **410**, 135429.
- 105 X. Ji, X. Zhao, Z. Zhang, Y. Si, W. Qian, H. Fu, Z. Chen, Z. Wang, H. Jin and Z. Yang, *Nano Res.*, 2023, 1–8.
- 106 H. Liu, J. Quan, J. Wang, Q. Hou, R. Wang, B. Cui, T. Lang, Y. Chen, H. Pan and J. Xu, *Cellulose*, 2023, **30**, 1225–1244.
- 107 H. Manisha, J. Sonia, S. Shashikiran, S. Yuvarajan, P. Rekha and K. S. Prasad, *Electrochem. Commun.*, 2022, **137**, 107259.
- 108 G. Maduraiveeran, *Curr. Anal. Chem.*, 2022, **18**, 509–517.
- 109 Y. Zheng, Y. Li, L. Fan, H. Yao and Z. Zhang, *Anal. Methods*, 2022, **14**, 1268–1278.
- 110 H. Zhang, X. Li, Q. Zhu and Z. Wang, *J. Electroanal. Chem.*, 2022, **909**, 116140.
- 111 C. J. Valentine, K. Takagishi, S. Umez, R. Daly and M. De Volder, *ACS Appl. Mater. Interfaces*, 2020, **12**, 30680–30685.
- 112 M. Santhiago, P. G. da Costa, M. P. Pereira, C. C. Correa, V. R. B. de Moraes and C. C. Bufon, *ACS Appl. Mater. Interfaces*, 2018, **10**, 35631–35638.
- 113 R. S. Khan, Z. Khurshid and F. Yahya Ibrahim Asiri, *Diagnostics*, 2017, **7**, 39.
- 114 L. Cai, C. Xu, S. Lin, J. Luo, M. Wu and F. Yang, *Biomicrofluidics*, 2014, **8**, 056504.
- 115 E. R. Kim, C. Joe, R. J. Mitchell and M. B. Gu, *Trends Biotechnol.*, 2023, **41**, 374–395.
- 116 X. Luo, J. Xia, X. Jiang, M. Yang and S. Liu, *Anal. Chem.*, 2019, **91**, 15461–15468.



- 117 N. C. Sekar, S. A. M. Shaegh, S. H. Ng, L. Ge and S. N. Tan, *Sens. Actuators, B*, 2014, **204**, 414–420.
- 118 N. Ruecha, R. Rangkupan, N. Rodthongkum and O. Chailapakul, *Biosens. Bioelectron.*, 2014, **52**, 13–19.
- 119 Y. Thepchuay, T. Sonsa-Ard, N. Ratanawimarnwong, S. Auparakkitanon, J. Sitanurak and D. Nacapricha, *Anal. Chim. Acta*, 2020, **1103**, 115–121.
- 120 X. Liu, X. Li, X. Gao, L. Ge, X. Sun and F. Li, *ACS Appl. Mater. Interfaces*, 2019, **11**, 15381–15388.
- 121 S. Cinti, C. Minotti, D. Moscone, G. Palleschi and F. Arduini, *Biosens. Bioelectron.*, 2017, **93**, 46–51.
- 122 T. Tian, H. Liu, L. Li, J. Yu, S. Ge, X. Song and M. Yan, *Sens. Actuators, B*, 2017, **251**, 440–445.
- 123 Y. Shen, T.-T. Tran, S. Modha, H. Tsutsui and A. Mulchandani, *Biosens. Bioelectron.*, 2019, **130**, 367–373.
- 124 S. Veeralingam and S. Badhulika, *J. Ind. Eng. Chem.*, 2022, **113**, 401–410.
- 125 Y.-J. Chang, M.-C. Lee and Y.-C. Chien, *SLAS Technol.*, 2022, **27**, 54–62.
- 126 X. Kou, L. Tong, Y. Shen, W. Zhu, L. Yin, S. Huang, F. Zhu, G. Chen and G. Ouyang, *Biosens. Bioelectron.*, 2020, **156**, 112095.
- 127 P. Teengam, W. Siangproh, A. Tuantranont, C. S. Henry, T. Vilaivan and O. Chailapakul, *Anal. Chim. Acta*, 2017, **952**, 32–40.
- 128 A. Yakoh, E. Mehmeti, K. Kalcher and S. Chaiyo, *Anal. Chem.*, 2022, **94**, 5893–5900.
- 129 X. Li, Q. Duan, M. Khan, D. Yang, Q. Liu, F. Yin, Q. Hu and L. Yu, *Talanta*, 2024, **266**, 124994.
- 130 J. Xu, M. Wang, M. Li, J. Yang and L. Yang, *Anal. Chim. Acta*, 2023, **1279**, 341834.
- 131 G. Bhattacharya, S. J. Fishlock, S. Hussain, S. Choudhury, A. Xiang, B. Kandola, A. Pritam, N. Soin, S. S. Roy and J. A. McLaughlin, *ACS Appl. Mater. Interfaces*, 2022, **14**, 31109–31120.
- 132 M. d M. G. del Campo, A. Alba-Patino, C. Palomino, M. Bauzá, E. Rojo-Molinero, A. Oliver, G. Turnes and R. de la Rica, *Sens. Actuators, B*, 2022, **354**, 131214.
- 133 R. Suvanasuthi, S. Chimmnaronk and C. Promptmas, *Talanta*, 2022, **237**, 122962.
- 134 S. Modha, Y. Shen, H. Chamouni, A. Mulchandani and H. Tsutsui, *Biosens. Bioelectron.*, 2021, **180**, 113090.
- 135 B. Demirbakan and M. K. Sezginürk, *Anal. Chim. Acta*, 2021, **1144**, 43–52.
- 136 M. Rahimi-Mohseni, J. B. Raoof, T. A. Aghajanzadeh and R. Ojani, *Microchem. J.*, 2021, **160**, 105739.
- 137 P. Jafari, S. M. Beigi, F. Yousefi, S. Aghabalazadeh, M. Mousavizadegan, M. Hosseini, S. Hosseinkhani and M. R. Ganjali, *Microchem. J.*, 2021, **163**, 105909.
- 138 J. P. Hunt, E. L. Zhao, T. J. Free, M. Soltani, C. A. Warr, A. B. Benedict, M. K. Takahashi, J. S. Griffiths, W. G. Pitt and B. C. Bundy, *New Biotechnol.*, 2022, **66**, 53–60.
- 139 A. Yakoh, U. Pimpitak, S. Rengpipat, N. Hirankarn, O. Chailapakul and S. Chaiyo, *Biosens. Bioelectron.*, 2021, **176**, 112912.
- 140 S. Khaliliazar, A. Toldrà, G. Chondrogiannis and M. M. Hamed, *Anal. Chem.*, 2021, **93**, 14187–14195.
- 141 M. Moccia, V. Caratelli, S. Cinti, B. Pede, C. Avitabile, M. Saviano, A. L. Imbriani, D. Moscone and F. Arduini, *Biosens. Bioelectron.*, 2020, **165**, 112371.
- 142 L. Huang, W. Xiao, T. Xu, H. Chen, Z. Jin, Z. Zhang, Q. Song and Y. Tang, *Sens. Actuators, B*, 2021, **327**, 128893.
- 143 J. Heikenfeld, A. Jajack, B. Feldman, S. W. Granger, S. Gaitonde, G. Begtrup and B. A. Katchman, *Nat. Biotechnol.*, 2019, **37**, 407–419.
- 144 Y. J. Hong, H. Lee, J. Kim, M. Lee, H. J. Choi, T. Hyeon and D. H. Kim, *Adv. Funct. Mater.*, 2018, **28**, 1805754.
- 145 P. J. Derbyshire, H. Barr, F. Davis and S. P. Higson, *J. Physiol. Sci.*, 2012, **62**, 429–440.
- 146 J. Moyer, D. Wilson, I. Finkelshtein, B. Wong and R. Potts, *Diabetes Technol. Ther.*, 2012, **14**, 398–402.
- 147 A. Alizadeh, A. Burns, R. Lenigk, R. Gettings, J. Ashe, A. Porter, M. McCaul, R. Barrett, D. Diamond and P. White, *Lab Chip*, 2018, **18**, 2632–2641.
- 148 A. Singh, A. Hazarika, C. Talukdar, M. Bhuyan, L. Dutta, M. Barthakur and K. Chakraborty, *IEEE Trans. Ind. Inf.*, 2021, **17**, 7546–7553.
- 149 M. Li, L. Wang, R. Liu, J. Li, Q. Zhang, G. Shi, Y. Li, C. Hou and H. Wang, *Biosens. Bioelectron.*, 2021, **174**, 112828.
- 150 A. Singh, A. Hazarika, L. Dutta, A. Bhuyan and M. Bhuyan, *Anal. Chim. Acta*, 2022, **1227**, 340257.
- 151 L. Fiore, V. Mazzaracchio, A. Serani, G. Fabiani, L. Fabiani, G. Volpe, D. Moscone, G. M. Bianco, C. Occhiuzzi and G. Marrocco, *Sens. Actuators, B*, 2023, **379**, 133258.
- 152 S. Mandal and G. C. Banik, *Chem. Sci. Rev. Lett.*, 2021, **10**, 116–112.
- 153 E.-C. Oerke, *J. Agric. Sci.*, 2006, **144**, 31–43.
- 154 P. Nicolopoulou-Stamati, S. Maipas, C. Kotampasi, P. Stamatis and L. Hens, *Public Health Front.*, 2016, **4**, 148.
- 155 M. A. Beketov, B. J. Kefford, R. B. Schäfer and M. Liess, *Proc. Natl. Acad. Sci. U. S. A.*, 2013, **110**, 11039–11043.
- 156 N. E. Pollok, C. Rabin, C. T. Walgama, L. Smith, I. Richards and R. M. Crooks, *ACS Sens.*, 2020, **5**, 853–860.
- 157 E. Noviana and C. S. Henry, *Curr. Opin. Electrochem.*, 2020, **23**, 1–6.
- 158 F. Arduini, S. Cinti, V. Caratelli, L. Amendola, G. Palleschi and D. Moscone, *Biosens. Bioelectron.*, 2019, **126**, 346–354.
- 159 A. Cioffi, M. Mancini, V. Gioia and S. Cinti, *Environ. Sci. Technol.*, 2021, **55**, 8859–8865.
- 160 X. Ruan, Y. Wang, E. Y. Kwon, L. Wang, N. Cheng, X. Niu, S. Ding, B. J. Van Wie, Y. Lin and D. Du, *Biosens. Bioelectron.*, 2021, **184**, 113238.
- 161 N. Colozza, K. Kehe, G. Dionisi, T. Popp, A. Tsoutsouloupoulos, D. Steinritz, D. Moscone and F. Arduini, *Biosens. Bioelectron.*, 2019, **129**, 15–23.
- 162 V. Caratelli, G. Fegatelli, D. Moscone and F. Arduini, *Biosens. Bioelectron.*, 2022, **205**, 114119.
- 163 C. Botías, A. David, J. Horwood, A. Abdul-Sada, E. Nicholls, E. Hill and D. Goulson, *Environ. Sci. Technol.*, 2015, **49**, 12731–12740.



- 164 F. Si, R. Zou, S. Jiao, X. Qiao, Y. Guo and G. Zhu, *Ecotoxicol. Environ. Saf.*, 2018, **148**, 862–868.
- 165 H. Li, R. Jin, D. Kong, X. Zhao, F. Liu, X. Yan, Y. Lin and G. Lu, *Sens. Actuators, B*, 2019, **283**, 207–214.
- 166 K.-L. Lee, M.-L. You, C.-H. Tsai, E.-H. Lin, S.-Y. Hsieh, M.-H. Ho, J.-C. Hsu and P.-K. Wei, *Biosens. Bioelectron.*, 2016, **75**, 88–95.
- 167 D. Englert, J. P. Zubrod, M. Link, S. Mertins, R. Schulz and M. Bundschuh, *Environ. Sci. Technol.*, 2017, **51**, 5793–5802.
- 168 C.-H. Chang, D. MacIntosh, B. Lemos, Q. Zhang and C. Lu, *J. Agric. Food Chem.*, 2018, **66**, 10097–10105.
- 169 T. Liu, D. Chen, Y. Li, X. Wang and F. Wang, *J. Agric. Food Chem.*, 2018, **66**, 4531–4540.
- 170 P. Zhao, H. Liu, L. Zhang, P. Zhu, S. Ge and J. Yu, *ACS Appl. Mater. Interfaces*, 2020, **12**, 8845–8854.
- 171 V. Scognamiglio, A. Antonacci, F. Arduini, D. Moscone, E. V. Campos, L. F. Fraceto and G. Palleschi, *J. Hazard. Mater.*, 2019, **373**, 483–492.
- 172 Z. Ma, Y. Li, C. Lu and M. Li, *J. Hazard. Mater.*, 2023, 131725.
- 173 F. Zhao, L. Wang, M. Li, M. Wang, G. Liu and J. Ping, *TrAC, Trends Anal. Chem.*, 2023, 117152.
- 174 G. Song, J. Zhang, H. Huang, X. Wang, X. He, Y. Luo, J.-C. Li, K. Huang and N. Cheng, *Food Chem.*, 2022, **387**, 132896.
- 175 T. T. M. Duyen, H. Matsuura, K. Ujiie, M. Muraoka, K. Harada and K. Hirata, *J. Biosci. Bioeng.*, 2017, **123**, 96–100.
- 176 X. Wang, Y. Luo, K. Huang and N. Cheng, *Adv. Agrochem*, 2022, **1**, 3–6.
- 177 G. Bayramoglu, M. Kilic and M. Y. Arica, *Food Chem.*, 2022, **382**, 132353.
- 178 Y. Li, Q. Wu, Z. Wu, Y. Zhuang, L. Sun, X. Fan, T. Zhao, L. Yi and Y. Gu, *Food Chem.*, 2023, **405**, 134974.
- 179 C. Griesche and A. J. Baeumner, *TrAC, Trends Anal. Chem.*, 2020, **128**, 115906.
- 180 V. Pagkali, D. Soulis, C. Kokkinos and A. Economou, *Sens. Actuators, B*, 2022, **358**, 131546.
- 181 H. K. Kordasht, A. Saadati and M. Hasanzadeh, *Food Chem.*, 2022, **373**, 131411.
- 182 C. Nerín, M. Aznar and D. Carrizo, *Trends Food Sci. Technol.*, 2016, **48**, 63–68.
- 183 B. Kuswandi, Y. Wicaksono, Jayus, A. Abdullah, L. Y. Heng and M. Ahmad, *Sens. Instrum. Food Qual. Saf.*, 2011, **5**, 137–146.
- 184 H.-z Chen, M. Zhang, B. Bhandari and C.-h Yang, *LWT*, 2019, **99**, 43–49.
- 185 S. Y. Lee, S. J. Lee, D. S. Choi and S. J. Hur, *J. Sci. Food Agric.*, 2015, **95**, 2799–2810.
- 186 A. Sobhan, K. Muthukumarappan and L. Wei, *Food Packag. Shelf Life*, 2021, **30**, 100745.
- 187 M. M. Ali, M. Wolfe, K. Tram, J. Gu, C. D. Filipe, Y. Li and J. D. Brennan, *Angew. Chem.*, 2019, **131**, 10012–10016.
- 188 C. Mills, M. J. Dillon, P. K. Kulabhusan, D. Senovilla-Herrero and K. Campbell, *Environ. Sci. Technol.*, 2022, **56**, 12210–12217.
- 189 S. K. Choi, A. Myc, J. E. Silpe, M. Sumit, P. T. Wong, K. McCarthy, A. M. Desai, T. P. Thomas, A. Kotlyar and M. M. B. Holl, *ACS Nano*, 2013, **7**, 214–228.
- 190 H. J. Chung, T. Reiner, G. Budin, C. Min, M. Liong, D. Issadore, H. Lee and R. Weissleder, *ACS Nano*, 2011, **5**, 8834–8841.
- 191 N. Verdoodt, C. R. Basso, B. F. Rossi and V. A. Pedrosa, *Food Chem.*, 2017, **221**, 1792–1796.
- 192 Y. Mao, X. Huang, S. Xiong, H. Xu, Z. P. Aguilar and Y. Xiong, *Food Control*, 2016, **59**, 601–608.
- 193 B. H. Park, S. J. Oh, J. H. Jung, G. Choi, J. H. Seo, E. Y. Lee and T. S. Seo, *Biosens. Bioelectron.*, 2017, **91**, 334–340.
- 194 T. Wang, P. Li, Q. Zhang, W. Zhang, Z. Zhang, T. Wang and T. He, *Sci. Rep.*, 2017, **7**, 4348.
- 195 L. Fu, S. Deng, Y. Luo, Q. Fu, Y. Fan and L. Jia, *Talanta*, 2023, **265**, 124920.
- 196 E. T. Bougadi and D. P. Kalogianni, *Food Chem.*, 2020, **322**, 126758.
- 197 M. Srisa-Art, K. E. Boehle, B. J. Geiss and C. S. Henry, *Anal. Chem.*, 2018, **90**, 1035–1043.
- 198 H. A. Al Lawati, J. Hassanzadeh, N. Bagheri and I. A. Lawati, *Talanta*, 2021, **234**, 122648.
- 199 G. Li, J. Sun, J. Li, Y. Zhang, J. Huang, F. Yue, H. Dong, F. Li, H. Xu and Y. Guo, *Talanta*, 2023, 124843.
- 200 P. K. Prabhakar, S. Vatsa, P. P. Srivastav and S. S. Pathak, *Food Res. Int.*, 2020, **133**, 109157.
- 201 X. Wang, Y. Wang, C. Guo, X. Zhang, Y. Wang, L. Lv, X. Wang and M. Wei, *Food Chem.*, 2023, **405**, 134811.
- 202 S. Li, S. Wang, B. Wu, M. Jiang, H.-Y. Yu, D. Ge, Y. Dong, W. Xu and K. C. Tam, *Nano Energy*, 2024, **120**, 109148.
- 203 O. Pourret and A. Hursthouse, *Int. J. Environ. Res. Public Health*, 2019, **16**, 4446.
- 204 S. Zhu, M. Xia, Y. Chu, M. A. Khan, W. Lei, F. Wang, T. Muhmood and A. Wang, *Appl. Clay Sci.*, 2019, **169**, 40–47.
- 205 Y. Zhang, C. Zhao, H. Bi, X. Zhang, B. Xue, C. Li, S. Wang, X. Yang, Z. Qiu and J. Wang, *J. Hazard. Mater.*, 2022, **438**, 129499.
- 206 S. Karuppiyah, N. C. Mishra, W.-C. Tsai, W.-S. Liao and C.-F. Chou, *ACS Sens.*, 2021, **6**, 3214–3223.
- 207 Y. Zheng, L. Wei, L. Duan, F. Yang, G. Huang, T. Xiao, M. Wei, Y. Liang, H. Yang and Z. Li, *J. Environ. Sci.*, 2021, **106**, 161–170.
- 208 C. S. K. Lawrence, S. N. Tan and C. Z. Floresca, *Sens. Actuators, B*, 2014, **193**, 536–541.
- 209 L. Guadarrama-Fernández, M. Novell, P. Blondeau and F. J. Andrade, *Food Chem.*, 2018, **265**, 64–69.
- 210 A. D. Clayton, A. M. Schweidtmann, G. Clemens, J. A. Manson, C. J. Taylor, C. G. Niño, T. W. Chamberlain, N. Kapur, A. J. Blacker and A. A. Lapkin, *Chem. Eng. J.*, 2020, **384**, 123340.
- 211 C. W. Coley, R. Barzilay, T. S. Jaakkola, W. H. Green and K. F. Jensen, *ACS Cent. Sci.*, 2017, **3**, 434–443.



- 212 G. H. Gu, J. Noh, I. Kim and Y. Jung, *J. Mater. Chem. A*, 2019, 7, 17096–17117.
- 213 W. Sha, Y. Guo, Q. Yuan, S. Tang, X. Zhang, S. Lu, X. Guo, Y.-C. Cao and S. Cheng, *Adv. Intell. Syst.*, 2020, 2, 1900143.
- 214 Z. Chen, Z. Chen, Z. Song, W. Ye and Z. Fan, *J. Semicond.*, 2019, 40, 111601.
- 215 C. Mendes-Felipe, J. Oliveira, I. Etxebarria, J. L. Vilas-Vilela and S. Lanceros-Mendez, *Adv. Mater. Technol.*, 2019, 4, 1800618.

