


 Cite this: *Chem. Commun.*, 2022, 58, 9790

 Received 6th June 2022,  
Accepted 2nd August 2022

DOI: 10.1039/d2cc03152c

rsc.li/chemcomm

## Two-photon polymerization lithography enabling the fabrication of PEDOT:PSS 3D structures for bioelectronic applications†

 Amedeo Ruggiero,<sup>‡</sup> Valeria Criscuolo,<sup>‡\*</sup> Sara Grasselli,<sup>a</sup> Ugo Bruno,<sup>ad</sup> Chiara Ausilio,<sup>a</sup> Claudia Latte Bovio,<sup>ad</sup> Ottavia Bettucci<sup>a</sup> and Francesca Santoro<sup>‡\*abc</sup>

**Conductive 3D platforms have gained increasing attention in bioelectronics thanks to the improvement in the cell-chip coupling. PEDOT:PSS is nowadays widely employed in bioelectronic applications thanks to its electrical and mechanical properties. In this work, an innovative fabrication method for the realization of PEDOT:PSS-based conductive micropillars and 3D cage-like structures is presented, combining two-photon lithography and electrodeposition techniques.**

Bioelectronic devices are electronic platforms that directly interact with biological systems, such as cells, tissues, or living systems, in order to monitor cellular electrical activity<sup>1</sup> or modulate cellular behavior<sup>2</sup> through the application of an external electrical field.<sup>3</sup> Here, a crucial role is played by the interface between cells and electrodes that determines the effectiveness of the electrical coupling. In particular, the presence of a cleft between the membrane and the electrode represents a major limitation in the transduction of electrical signals.<sup>4</sup> Several strategies have been developed to reduce the cleft at the interface, including the fabrication of protruding bioinspired microstructured electrodes featuring holes,<sup>5</sup> grooves<sup>6</sup> and pillars.<sup>7</sup> The topography-mediated rearrangement of the cell membrane and cytoskeletal machinery, promoting the engulfment of the electrode, have been shown to improve the cell-chip coupling.<sup>8</sup>

Interestingly, organic conductive materials have been widely employed in bioelectronic devices thanks to their physical-chemical properties compared to inorganic materials, ranging from a higher versatility in synthesis and functionalization

to fabrication and processability.<sup>9</sup> Nowadays, poly(3,4-ethylenedioxythiophene) polystyrene sulfonate (PEDOT:PSS) is one of the most widely used conjugated polymers in several bioelectronic applications.<sup>10</sup> It displays mechanical properties close to biological systems<sup>11</sup> and shows a mixed ionic/electronic conduction mechanism,<sup>10</sup> with hole conductivity above 1000 S cm<sup>-1</sup>,<sup>12</sup> which is fundamental for an efficient cell-chip communication.<sup>13</sup>

Combining the beneficial effects of 3D microelectrodes in reducing the cleft and improving cellular adhesion with the properties of PEDOT:PSS can provide a step forward in the development of next generation bioelectronic and biomedical devices. Indeed, recently 3D PEDOT:PSS-based microstructures have been successfully developed by means of inkjet printing,<sup>14</sup> 3D printing,<sup>15</sup> direct writing,<sup>16</sup> replica molding<sup>17</sup> and nanosphere lithography,<sup>18</sup> and with the support of photocurable hydrogels.<sup>19</sup> An interesting approach for the fabrication of 3D microelectrodes involves the fabrication of gold mushroom-like microstructures (with 1 μm in diameter) coated *via* electrodeposition of PEDOT:PSS precursors.<sup>20</sup> However, as the 3D processing of PEDOT:PSS remains challenging, there is still a need to develop versatile patterning procedures that allow the integration of the material with microscale devices adapting to different geometries.

In recent years, two-photon polymerization (2PP) lithography has emerged as an effective method for the fabrication of 3D microstructures for numerous cell-material interfacing applications<sup>21</sup> thanks to its high resolution (down to 100 nm)<sup>21</sup> and design flexibility that enables the fabrication of complex 3D architectures without any geometrical constraint.<sup>22</sup>

In this work, we propose an innovative approach for the fabrication of conductive micropillars and 3D cage-like scaffolds exploiting 2PP and electrodeposition of PEDOT:PSS *via* cyclic voltammetry (CV). The proposed technique allows for the fabrication of PEDOT:PSS-coated micropillars as well as complex 3D structures that can fulfill any geometrical requirement, paving the way towards the development of 3D organic-based

<sup>a</sup> *Tissue Electronics, Istituto Italiano di Tecnologia, 80125 Naples, Italy.*  
E-mail: valeria.criscuolo@iit.it

<sup>b</sup> *Faculty of Electrical Engineering and IT, RWTH Aachen, 52074, Germany*

<sup>c</sup> *Institute for Biological Information Processing-Bioelectronics, Forschungszentrum Juelich, 52428, Germany. E-mail: f.santoro@fz-juelich.de*


<sup>d</sup> *Dipartimento di Chimica, Materiali e Produzione Industriale, Università di Napoli Federico II, 80125 Naples, Italy*

† Electronic supplementary information (ESI) available: Experimental details and methods. See DOI: <https://doi.org/10.1039/d2cc03152c>

‡ These authors contributed equally to this work.






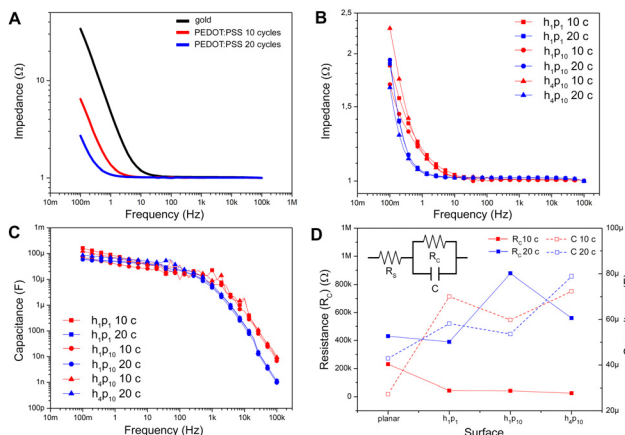

**Fig. 2** Electrochemical impedance spectroscopy characterization of PEDOT:PSS-coated pillar arrays. (A) Bode plots of planar gold film (black trace) and PEDOT:PSS films electrodeposited with 10 (red trace) and 20 (blue trace) CV cycles. (B) Bode plots of micropillar arrays coated with PEDOT:PSS films electrodeposited with 10 (red traces) and 20 (blue traces) CV cycles:  $h_1p_1$  (squares);  $h_1p_{10}$  (circles);  $h_4p_{10}$  (triangles). (C) Capacitance plots of pillar arrays coated with gold PEDOT:PSS films electrodeposited with 10 (red traces) and 20 (blue traces) CV cycles:  $h_1p_1$  (squares);  $h_1p_{10}$  (circles);  $h_4p_{10}$  (triangles). (D) Variation of the resistance  $R_c$  and capacitance  $C$  as a function of coated surfaces. The inset shows the equivalent circuit model used in this study.

Taken together, these findings suggest that the capacitance of microstructured electrodes is not linearly related to the thickness of the PEDOT:PSS film, whereas this linear relationship is maintained on planar substrates. In order to further confirm this hypothesis, EIS measurements were fitted with an electrical equivalent circuit shown in Fig. 2D (inset): here, the resistance  $R_s$  models the electrolyte resistance and other parasite contributions, while the parallel between  $R_c$  and  $C$  models the charge transfer resistance and the polymeric layer capacitance in PEDOT:PSS-coated micropillars.<sup>24</sup> The ideal capacitance is replaced by a constant phase element (CPE) that includes the non-idealities of conducting polymeric thin films.<sup>28</sup> Numerical data fitting extracted from planar electrodes (Table S1, ESI<sup>†</sup>) confirms that the equivalent PEDOT:PSS layer capacitance increases with the thickness.<sup>27</sup> The dependency of  $R_c$  and  $C$  on the shape of the micropillar arrays and PEDOT:PSS film thickness is shown in Fig. 2D (solid and dashed traces, respectively). In particular, PEDOT:PSS-coated micropillars are characterized by low values of resistance regardless of the height, density and number of CV applied cycles during the electrochemical deposition. Interestingly, the capacitance values of different micropillar arrays are comparable, showing no significant differences among electrodes with different PEDOT:PSS layer thickness, aspect ratios and spacings ( $h_1p_1$ ,  $h_1p_{10}$ ,  $h_4p_{10}$ ). Moreover, the electrochemical properties of the electrodeposited PEDOT:PSS films were also assessed by means of CV acquired in the range between  $-1.0$  to  $1.0$  V, using PBS as an electrolytic solution (Fig. S7, ESI<sup>†</sup>). The voltammograms showed the typical oxidation and reduction potentials of PEDOT:PSS, correlated to the PEDOT doped and de-doped state, and a reduction peak at  $+0.6$  V, in agreement with previous results.<sup>29</sup>

In conclusion, the electrochemical characterization supports the potential use of PEDOT:PSS-coated micropillars in bioelectronic

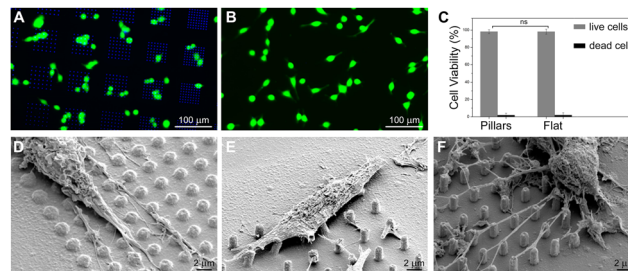


**Fig. 3** HT-22 cells cultured on PEDOT:PSS-coated micropillars. Fluorescence images of HT-22 cells showing live (green) and dead (blue) cells on (A) pillar arrays and (B) flat regions. (C) Percentage of live and dead cells reported as mean  $\pm$  SD ( $n = 3$ ). Scanning electron micrographs of HT22 cells on pillar arrays, coated with 10 applied CV cycles of PEDOT:PSS: (D)  $1 \mu\text{m}$  high and  $2 \mu\text{m}$  pitch, (E)  $4 \mu\text{m}$  high and  $6 \mu\text{m}$  pitch, and (F)  $4 \mu\text{m}$  high and  $3 \mu\text{m}$  pitch.

devices for both *in vitro* sensing and stimulation. Indeed, the impedance is lower than  $20 \text{ k}\Omega$  in the frequency range between  $1 \text{ Hz}$  and  $5 \text{ kHz}$ , which is usually considered the most relevant for extracellular neural electrophysiology.<sup>20</sup> Moreover, the electrodeposited PEDOT:PSS films do not show redox activity in the ranges of potential typically employed for stimulation of electrogenic cells.<sup>10</sup>

Furthermore, in order to evaluate the biocompatibility of PEDOT:PSS-coated micropillars, a live/dead assay was performed after 1 day *in vitro* (DIV 1, Experimental section, ESI<sup>†</sup>) on both HT-22 cells (Fig. 3A, B and Fig. S8, ESI<sup>†</sup>) and primary cortical neurons (Fig. S9A and B, ESI<sup>†</sup>). Here, live and dead cells were labelled with Calcein-AM (green fluorescence signal) and a Dead Cell Stain Kit (blue fluorescence signal), respectively. In agreement with previous works,<sup>30</sup> the PEDOT:PSS-coated micropillar arrays displayed high biocompatibility, with high percentages of live cells on both micropillars and flat regions ( $\sim 98\%$ , Fig. 3C and Fig. S9C, ESI<sup>†</sup>). Scanning electron micrographs showed that PEDOT:PSS-coated micropillars promote cellular adhesion and elongation of neurites (Fig. 3D–F), which suggests that different aspect ratios of micropillars might support the cell-chip coupling and eventually act as topographical guidance. As the native cellular environment is elaborate and cells organize in a three-dimensional manner, preliminary studies were performed fabricating more complex conductive 3D cage-like scaffolds featuring microtowers, channels and micropillars with dimensions and topographical arrangement similar to previous works<sup>31</sup> (details in the Experimental section and Fig. S10, ESI<sup>†</sup>). PEDOT:PSS was deposited applying 20 CV cycles to ensure a uniform and conformal coating. The scanning electron micrographs showed that, similar to what has been observed on micropillars, the PEDOT:PSS coating is conformal to the structure and the electrodeposition process did not affect the overall morphology of the designed structures (Fig. 4A). In addition, we investigated the thickness of the PEDOT:PSS film revealing the cross-section of the towers and the channels of the 3D cage-like structures *via* FIB cross sectioning (Fig. 4B and C). Interestingly, the overall PEDOT:PSS thickness reached a maximum of  $160 \text{ nm}$ , a value lower than the film thickness obtained on micropillar arrays (Fig. 4D). In particular, the towers featured with micropillars displayed a higher film thickness than the flat towers, with an average thickness of  $134 \pm 6 \text{ nm}$  and  $95 \pm 9 \text{ nm}$



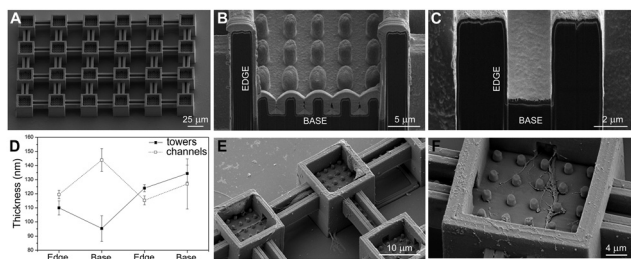

**Fig. 4** PEDOT:PSS-coated cage-like scaffold fabrication outcome, thickness analysis and cell-scaffold interaction. (A) Scanning electron micrograph of the 3D cage-like structures coated with 20 applied CV cycles. Scanning electron micrographs of cross-sections performed on different scaffold regions: (B) tower with pillars and (C) flat channel. (D) PEDOT:PSS thickness analysis on 3D structures: each graph shows the mean values and standard deviations depending on the cross-sectioned scaffold region. (E) Scanning electron micrograph of primary neurons cultured on 3D coated scaffolds and (F) close-up of a neurite wrapping around a pillar.

respectively. Conversely, the PEDOT:PSS film thickness on the flat channels was higher than the thickness on channels with pillars, with an average thickness of  $144 \pm 8$  nm and  $127 \pm 17$  nm, respectively. In addition, the high standard deviation indicates the lower reproducibility of the PEDOT:PSS deposition on such narrow elements, compared to the other substrate regions (Fig. 4D). Furthermore, the biocompatibility of the PEDOT:PSS-coated 3D cage-like structures was assessed (details in the Experimental section, ESI†). As expected, cell survival was high both for HT-22 cells and primary cortical neurons (Fig. S11A and B, respectively, ESI†), which suggests that the spatial arrangement and morphology of the substrate have no effect on cell viability. Finally, cellular adhesion and interaction with the 3D structures was investigated *via* SEM imaging (Fig. 4E and F). The substrates support cellular adhesion, confining and guiding neurite outgrowth throughout the entire scaffold. Moreover, the presence of micropillars provides anchorage points for the elongation and growth of neuronal processes, allowing for a close cell-chip coupling, fundamental for an effective bioelectronic device.

In conclusion, in this work, an innovative and versatile fabrication method for 3D PEDOT:PSS-coated microstructures combining 2PP and electrodeposition techniques is reported. This method was employed for the fabrication of conductive micropillar arrays with various aspect ratios and pitches as well as complex 3D cage-like structures to demonstrate the versatility of the proposed technique. First, the resulting thickness of PEDOT:PSS according to the applied CV cycles on the micropillars was characterized by means of FIB cross-sectioning and SEM imaging. Subsequently, the electrochemical properties of the coated micropillars were investigated by means of EIS revealing that the presence of the 3D structures mediates the capacitance of the PEDOT:PSS film and is not dependent on the thickness. These findings demonstrate that the PEDOT:PSS-coated micropillars are suitable as electrodes to be implemented in bioelectronic devices for both sensing and stimulation of neuronal tissues. Additionally, we assessed the cell viability of HT22 cells confirming the biocompatible nature of PEDOT:PSS. Furthermore, it was observed that micropillar arrays can act as topographical guidance and that cage-like scaffolds were

able to confine and guide neurite outgrowth. The results show that this fabrication method is suitable for the realization of conductive 3D structures of any kind of geometry, overcoming the limits of 2D cell cultures.

Francesca Santoro acknowledges the support of the European Research Council starting Grant BRAIN-ACT No. 949478. The authors acknowledge Dr Paschalis Gkoupidenis and Prof Roberto Centore for the scientific discussion corroborating the work.

## Conflicts of interest

There are no conflicts to declare.

## References

- 1 P. Mehrotra, *J. Oral Biol. Craniofacial Res.*, 2016, **6**, 153–159.
- 2 C. Chen, X. Bai, Y. Ding and I.-S. Lee, *Biomater. Res.*, 2019, **23**, 25.
- 3 M. Rolandi, A. Noy, S. Inal and J. Rivnay, *APL Mater.*, 2021, **9**, 070402.
- 4 A. Zhang and C. M. Lieber, *Chem. Rev.*, 2016, **116**, 215–257.
- 5 T. J. J. Hondrich, B. Lenyk, P. Shokohimehr, D. Kireev, V. Maybeck, D. Mayer and A. Offenhäusser, *ACS Appl. Mater. Interfaces*, 2019, **11**, 46451–46461.
- 6 P. Wijdenes, H. Ali, R. Armstrong, W. Zaidi, C. Dalton and N. I. Syed, *Sci. Rep.*, 2016, **6**, 34553.
- 7 Micha E. Spira and Aviad Hai, *Nat. Nanotechnol.*, 2013, **8**, 83–94.
- 8 A. Mariano, C. Lubrano, U. Bruno, C. Ausilio, N. B. Dinger and F. Santoro, *Chem. Rev.*, 2022, **122**, 4552–4580.
- 9 D. Ohayon and S. Inal, *Adv. Mater.*, 2020, **32**, 2001439.
- 10 Y. Liang, A. Offenhäusser, S. Ingebrandt and D. Mayer, *Adv. Healthcare Mater.*, 2021, **10**, 2100061.
- 11 L. V. Kayser and D. J. Lipomi, *Adv. Mater.*, 2019, **31**, 1806133.
- 12 J. Rivnay, S. Inal, B. A. Collins, M. Sessolo, E. Stavrinidou, X. Strakosas, C. Tassone, D. M. DeLongchamp and G. G. Malliaras, *Nat. Commun.*, 2016, **7**, 11287.
- 13 P. Zhang and J. Travas-Sejdic, *J. Mater. Chem. C*, 2021, **9**, 9730–9760.
- 14 I. Basak, G. Nowicki, B. Rutters, D. Desta, J. Prooth, M. Jose, S. Nagels, H.-G. Boyen, J. D'Haen, M. Buntinx and W. Deferme, *Polymers*, 2020, **12**, 2915.
- 15 H. Yuk, B. Lu, S. Lin, K. Qu, J. Xu, J. Luo and X. Zhao, *Nat. Commun.*, 2020, **11**, 1604.
- 16 P. Zhang, N. Aydemir, M. Alkaisi, D. E. Williams and J. Travas-Sejdic, *ACS Appl. Mater. Interfaces*, 2018, **10**(14), 11888–11895.
- 17 Y.-S. Hsiao, B.-C. Ho, H.-X. Yan, C.-W. Kuo, D.-Y. Chueh, H. Yu and P. Chen, *J. Mater. Chem. B*, 2015, **3**, 5103–5110.
- 18 S. So, H. W. M. Fung, K. Kartub, A. M. Maley and R. M. Corn, *J. Phys. Chem. Lett.*, 2017, **8**, 576–579.
- 19 D. N. Heo, S.-J. Lee, R. Timsina, X. Qiu, N. J. Castro and L. G. Zhang, *Mater. Sci. Eng.*, 2019, **99**, 582–590.
- 20 P. D. Jones, A. Moskalyuk, C. Barthold, K. Gutöhrlein, G. Heusel, B. Schröppel, R. Samba and M. Giugliano, *Front. Neurosci.*, 2020, **14**, 405.
- 21 C. Liao, A. Wuethrich and M. Trau, *Appl. Mater. Today*, 2020, **19**, 100635.
- 22 J. Harberts, C. Fendler, J. Teuber, M. Siegmund, A. Silva, N. Rieck, M. Wolpert, R. Zierold and R. H. Blick, *ACS Nano*, 2020, **14**, 13091–13102.
- 23 X. Strakosas, B. Wei, D. C. Martin and R. M. Owens, *J. Mater. Chem. B*, 2016, **4**, 4952–4968.
- 24 G. Dijk, H. J. Ruigrok and R. P. O'Connor, *Adv. Mater. Interfaces*, 2020, **7**, 2000675.
- 25 B. Rezaei, S. Saghir, J. Y. Pan, R. S. Davidsen and S. S. Keller, *Micromachines*, 2022, **13**, 371.
- 26 J. Wang, J. Zhang, X. Pei, S. Liu, F. Ning, Y. Li and C. Wang, *CrystEngComm*, 2020, **22**, 2361–2370.
- 27 D. A. Koutsouras, F. Torricelli, P. Gkoupidenis and P. W. M. Blom, *Adv. Mater. Technol.*, 2021, **6**, 2100732.
- 28 G. Inzelt and G. G. Láng, *Electropolymerization*, John Wiley & Sons, Ltd, 2010, pp. 51–76.
- 29 M. Marzocchi, I. Gualandi, M. Calienni, I. Zironi, E. Scavetta, G. Castellani and B. Fraboni, *ACS Appl. Mater. Interfaces*, 2015, **7**, 17993–18003.
- 30 H. He, L. Zhang, X. Guan, H. Cheng, X. Liu, S. Yu, J. Wei and J. Ouyang, *ACS Appl. Mater. Interfaces*, 2019, **11**, 26185–26193.
- 31 C. Fendler, C. Denker, J. Harberts, P. Bayat, R. Zierold, G. Loers, M. Münzenberg and R. H. Blick, *Adv. Biosys.*, 2019, **3**, 1800329.

