

Lab on a Chip

Devices and applications at the micro- and nanoscale

rsc.li/loc



ISSN 1473-0197



CRITICAL REVIEW

Jochen Kieninger *et al.*

Microsensor systems for cell metabolism – from 2D culture to organ-on-chip



Cite this: *Lab Chip*, 2018, 18, 1274

Microsensor systems for cell metabolism – from 2D culture to organ-on-chip

Jochen Kieninger, * Andreas Weltin,  Hubert Flamm and Gerald A. Urban

Microsensor systems for cell metabolism are essential tools for investigation and standardization in cell culture. Electrochemical and optical read-out schemes dominate, which enable the marker-free, continuous, online recording of transient effects and deliver information beyond microscopy and end-point tests. There has been much progress in microfluidics and microsensors, but the translation of both into standard cell culture procedures is still limited. Within this critical review, we discuss different cell culture formats ranging from standard culture vessels to dedicated microfluidic platforms. Key aspects are the appropriate supply of cells, mass transport of metabolites to the sensors and generation of stimuli. Microfluidics enable the transition from static to dynamic conditions in culture and measurement. We illustrate the parameters oxygen (respiration), pH (acidification), glucose and lactate (energy metabolism) as well as short-lived reactive species (ROS/RNS) from the perspective of microsensor integration in 2D and 3D cell culture. We discuss different sensor principles and types, along with their limitations, microfabrication technologies and materials. The state-of-the-art of microsensor platforms for cell culture is discussed with respect to sensor performance, the number of parameters and timescale of application. That includes the advances from 2D culture to the increasingly important 3D approaches, with specific requirements for organotypic micro-tissues, spheroids and solid matrix cultures. We conclude on the current progress, potential, benefits and limitations of cell culture monitoring systems from monolayer culture to organ-on-chip systems.

Received 1st September 2017,
Accepted 16th February 2018

DOI: 10.1039/c7lc00942a

rsc.li/loc

Introduction

The human body with its 10^{14} cells is a highly complex system often hindering the direct research on a specific organ

Laboratory for Sensors, IMTEK – Department of Microsystems Engineering, University of Freiburg, Germany. E-mail: kieninger@imtek.uni-freiburg.de; Tel: +49 761 203 7265



Jochen Kieninger

Dr.-Ing. Jochen Kieninger studied Microsystems Engineering at the University of Freiburg. In 2003, he received his diploma in engineering. Afterwards, he worked in the Laboratory for Sensors at the Department of Microsystems Engineering (IMTEK) and in the School of Soft Matter Research at the Freiburg Institute for Advanced Studies (FRIAS). In 2011, he completed his PhD on “Electrochemical microsensor system for cell culture monitoring”. In 2012, he was nominated as a lecturer and has since been working as a senior scientist in the Laboratory for Sensors. His research interests are electrochemical sensors, biosensors, micro-sensors for neurotechnology, cell culture monitoring, electrochemical methods for MEMS and microfabrication.



Andreas Weltin

Dr.-Ing. Andreas Weltin received his diploma (2008) and doctoral (2015) degrees in Microsystems Engineering from the University of Freiburg. Since 2015, he has been a group leader at the Laboratory for Sensors. In 2016, he received the nationwide 2nd Klee prize from DGBMT for his dissertation on in vivo sensors. He has developed and applied numerous microsensor platforms for 2D/3D cell culture metabolism. His research interests include the fabrication of (bio-)analytical microsystems, bio- and chemo-sensors, electrochemistry, microfluidics, and biomedical in vitro and in vivo applications in cancer research and neuroscience (presently, e.g., organ-on-chip systems in cancer therapy, characterization of neural interfaces).



A portrait of Dr. Michael J. Griffin, a man with dark hair and glasses, wearing a dark striped shirt. He is smiling slightly and looking directly at the camera.

Dr.-Ing. Hubert Flamm studied Microsystems Engineering and obtained his diploma degree from the University of Freiburg in 2009. From 2009 to 2017, he worked in the Laboratory for Sensors at the Department of Microsystems Engineering (IMTEK). In 2014, he received his doctoral degree studying about “Electrochemical Microsensors for Superoxide Monitoring in Cell Culture”. His research focuses on the



Prof. Dr. Gerald A. Urban received his Diploma in Physics at the Technical University Vienna. Afterwards, he became a research assistant at the Neurosurgical Department of University Hospital Vienna. He received his PhD in Electrical Engineering, was a co-founder of the company OSC, Cleveland, and became a scientific director of the Ludwig Boltzmann Institute for Biomedical Microengineering. In 1997, he became a full professor for

Pharmacodynamics studies, drug testing and compound screening are all applications in which the metabolic monitoring provides indicating parameters for specific pharmacological interactions. Results from *in vitro* cultivation of patient material in personalized medicine can benefit from microsensor readings, as within the very limited time frame of typical clinical scenarios a large quantity of information can be obtained. In all these different fields of application, the *in vitro* models in combination with microfluidics and sensors provide a rather simple possibility to parallelize the experiments in a reproducible manner. This allows both a

Monitoring systems can be separated into dynamic systems comprising microfluidics and static systems with stagnant medium following the routine procedure in cell culture. Depending on the field of application, either the culture system should provide results very fast, or micro-sensors should be able to measure for longer time, possibly without the need for recalibration. Another important aspect is the number of different sensing parameters provided by the system. In Fig. 1, we summarize the needs for the different fields of application. The fields are clustered depending on the desired measurement duration and on the number of measured parameters from single to multiparameter monitoring. Drug screening systems should be optimized for acquisition of results within minimal time, while standardization of cell culture typically addresses many cell cycles resulting in demands for stable sensors over weeks.

We do not comprehensively treat metabolic monitoring in bioreactors because of its different environment for sensors, resulting in completely different aspects for size, integration, stability and functionality. However, some works describing microsensors dedicated to bioreactors are applicable to mammalian cell culture and organ-on-chip systems as well and were therefore included. An overview of selected cell culture monitoring systems is given in Table 1.

Metabolic pathways – energy metabolism and relevant parameters

Keeping in mind that this is a severe abstraction, we focus on the simplified energy metabolism of glucose as illustrated in Fig. 2 for the discussion of the cell culture monitoring systems. In the first step, glycolysis, glucose is broken down into pyruvate molecules. Depending on oxygenation around the cell, pyruvate is further catabolized following an aerobic or an anaerobic pathway. Because of its overall higher efficiency (the amount of energy generated per glucose molecule), the aerobic pathway is preferred.

In the cytosol, glycolysis occurs, in which the six-carbon sugar glucose is broken down into two three-carbon sugars and converted further into two pyruvate ions. In the case of sufficient oxygen, pyruvate is oxidized within the mitochondria to acetyl-CoA releasing CO_2 . Acetyl-CoA is the starting point of the citric acid cycle, in which further energy is generated, with CO_2 and protons as by-products. Downstream of the citric acid cycle, in the oxidative phosphorylation, further energy is harvested by reduction of oxygen to water. If oxygenation is not sufficient, oxidative phosphorylation cannot occur, and the citric acid cycle stops, resulting in accumulation of pyruvate ions in the cytosol. In this case, the anaerobic pathway, the fermentation of pyruvate into lactate and release of a proton, sets in.

Cell culture monitoring using microsensors *per se* can measure extracellular substances only. Except for cultivating isolated mitochondria, only the substances marked green in

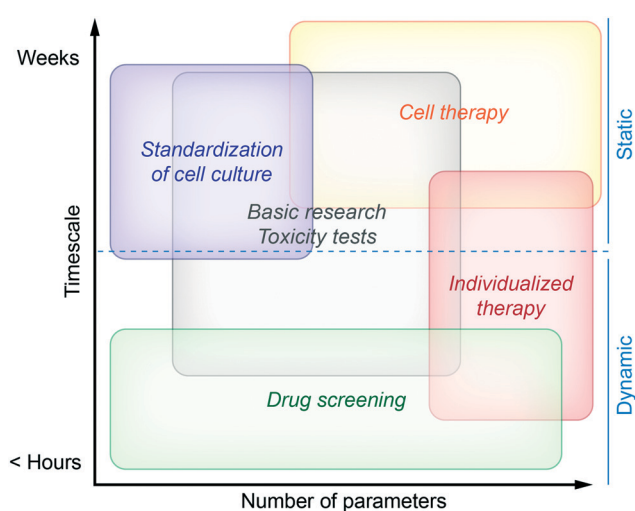


Fig. 1 Classification of cell culture monitoring systems by the needs of different fields of application.

Table 1 Overview of different cell culture monitoring systems. The selection was made to present typical representatives for each type of system rather than to be comprehensive

Name	Cell culture type	Material	Microfluidics	Parameters	Sensing principle	Notable features	Ref.
<i>Cytosensor</i>	2D, dynamic	Silicon	Yes	pH Oxygen Glucose, lactate	LAPS Amperometric (Pt) Amperometric biosensor (Pt)	Commercial	108 109, 110 110
<i>Sensing Cell Culture Flask</i>	2D, static	Glass	No	Oxygen pH Glucose, lactate Superoxide NO	Amperometric (Pt) Potentiometric (iridium oxide) Amperometric biosensor (Pt) Amperometric (Au) Differential pulse voltammetry (Au)	Standard culture vessel	28, 107 107 107 76 143
<i>Boero et al.</i>	2D, static	Silicon	Yes	Glucose, lactate	Amperometric biosensor (Au)	External biosensors	102
<i>Presens OxoDish</i>	2D, static	Polymer	No	Oxygen	Luminescence	Commercial, standard format	32
<i>Seahorse Bioscience</i>	2D/3D, static/dynamic	Polymer	No	Oxygen, pH	Fluorescence	Commercial, standard format, dip-in approach	55
<i>Bionas SC1000</i>	2D, dynamic	Silicon	Yes	pH Oxygen Adhesion	ISFET Amperometric (Pd) Impedance (IDES)	Commercial	56, 115
<i>MetaScreen</i>	2D, dynamic	Glass	Yes	Oxygen pH Glucose, lactate	Amperometric Potentiometric (iridium oxide) Amperometric biosensor	Downstream biosensors on-chip	57
<i>Misun et al.</i>	3D spheroid, dynamic	Glass	Yes	Glucose, lactate	Amperometric biosensor (Pt)	Hanging-drop network, <i>in situ</i> biosensors	19
<i>Bavli et al.</i>	3D spheroid, dynamic	Glass/PDMS	Yes	Oxygen Glucose, lactate	Luminescence (tissue embedded) Amperometric biosensor	Commercial, external downstream biosensors	133
<i>Zhang et al.</i>	3D spheroid, dynamic	Glass	Yes	pH Oxygen Immunosensors	Optical absorption Luminescence Cyclovoltammetric (Au)	Multiple sensor units, fluidic breadboard	135
<i>Weltin et al.</i>	3D spheroid, static	Polyimide	No	Oxygen Lactate	Amperometric (Pt) Amperometric biosensor (Pt)	Standard culture vessel, <i>in situ</i> biosensors, dip-in approach	18
<i>Domansky et al.</i>	3D, scaffold-based, dynamic	Polymer	Yes	Oxygen	Luminescence	On-chip pumps, dip-in approach	144

Fig. 2 can be accessed directly. The individual steps of the energy metabolism of glucose can only be seen indirectly.

Glucose as the major energy source in cell culture is available in the cell culture medium in high concentrations up to 10 mM or more. Physiological levels are typically lower (few mM), but glucose is not the sole energy source *in vivo*. In cell culture, glucose levels decrease depending on medium volume, cell density and metabolic activity and often reach values below the mM range before the medium is exchanged.

The concentration of dissolved **oxygen** is determinant for many different biological processes.³ Aerobic cell culture conditions (e.g. 5% CO₂, 95% air) result in dissolved oxygen concentrations in the range of 200 μ M. Depending on the type of culture, pericellular values are much lower because of the formation of diffusion gradients (see Fig. 3A). Typical oxygen concentrations in healthy tissue are between 20 and 150 μ M.

Pathologically low oxygen conditions (hypoxia) can be found, depending on the origin of the cells, at 25 μ M or lower.⁴ In cell culture, it is important to establish a well-defined pericellular oxygen concentration in order to ensure the reproducibility of the desired cellular state. In situations with limited medium volume or the possibility of formation of gradients, cellular respiration rates can be accessed. Typical rates are in the range of 200 fmol h⁻¹ per cell (T-47D breast cancer cell line).⁵ The aspect of oxygenation and oxygen control in cell culture has been discussed recently in more detail in this journal.^{6,7}

Lactate ions are the end product of the anaerobic pathway. Initially, the cell culture medium contains no or, in case serum was used to prepare the medium, up to a few mM lactate. Under typical culture conditions, lactate concentrations can rise up to few mM, usually not higher than half of the





Fig. 2 Simplified energy metabolism of glucose illustrated at the location where it takes place in a cell. Based on the availability of oxygen, an aerobic or an anaerobic pathway is possible. The substances highlighted in green can be observed in the extracellular space and are potential candidates for cell culture monitoring using microsensors.

initial glucose concentration in the medium. Taking into account the limitations of the simplified model described in Fig. 2, the fraction of twice the number of lactate molecules produced by the number of glucose molecules consumed can be used as a measure for the fraction of the anaerobic pathway. In a more detailed view, it should be considered that,

depending on the cell type, lactate can be used as an energy source or even metabolized to glucose, such as when liver cells convert lactate produced in the muscles back to glucose (Cori cycle).

Dissolved CO₂ gas and protons (pH) are interlinked by the dissolution of CO₂ and formation of bicarbonate ions (eqn (1)). Therefore, monitoring of pH is often preferred over measuring dissolved CO₂ gas in cell culture monitoring applications.



Additionally, the pH in a typical cell culture medium is stabilized by sodium bicarbonate and cultivating the cells in an incubator atmosphere containing CO₂ gas (e.g. 5%), which results in a strong buffer system following eqn (1). The pH of the typical cell culture medium is adjusted to 7.4, decreasing over time due to cell metabolism to values not much below pH 7 under appropriate culture conditions. In case cellular acidification should be accessed and measured as acidification rates with microsensors, a small total medium volume along with a weakly buffered medium is required.

Short-lived, reactive species

Along with the stable products of and educts for cellular metabolism, short-lived and reactive species play a role in cell metabolism, namely reactive oxygen (ROS) and reactive nitrogen species (RNS). ROS include both oxygen radicals as superoxide (O₂^{•−}) or hydroxyl radicals (OH[•]) and non-radical derivatives such as hydrogen peroxide (H₂O₂). The reactive nitrogen family includes nitrogen-derived radicals like the initial nitric oxide (NO[•]) and related products nitrogen dioxide (NO₂[•]) as well as the non-radical peroxyxynitrite (ONOO[−]). Among the ROS and RNS species, superoxide (O₂^{•−}) and nitric oxide (NO[•]) radicals are of primary interest. Besides their biological role, identification from cell/tissue release



Fig. 3 Concentration gradients in static 2D (A) and 3D cell culture (B), as well as dynamic cell culture monitoring with active transport (C). A: A monolayer of cells grows on the bottom of the culture vessel. A concentration gradient along the medium height occurs due to cellular production or consumption of substances. B: 3D cell agglomerates grow, often heterogeneously, in a 3D matrix or in medium. A radial concentration gradient occurs around the microtissues. Typically, there is an even stronger gradient inside the microtissues. C: A monolayer of cells grows inside a microfluidic microsensor system (microphysiometer). The small volume in the microchannel needs to be exchanged periodically using a pump to ensure cell survival. Large concentration changes of metabolites due to the small medium volume can be measured *in situ*, or metabolites are transported to downstream sensors by microfluidics.



spheroid size is in the range of several hundred micrometers. Gradients for metabolic reagents and products can be found in the matrix outside the spheroid. Additionally, and usually dominant, there are gradients which occur within the spheroids themselves, as illustrated in Fig. 3B. Oxygen, for example, depletes along the radius towards the center. Assuming appropriate culture conditions, it is possible to achieve neighboring layers with normoxic and hypoxic states, which are an essential model system in tumor research.¹⁴ Spheroids can be understood as an inverse model of the tumor geometry: in tissue, oxygen and nutrients' concentrations drop radially along the distance from a blood vessel in the center, whereas in a spheroid, the lowest oxygen and nutrients' concentrations can be found in its center. Especially for the method of hanging droplets, microfluidic systems have been applied to enable parallelization and enhance reproducibility.^{15–17} Access to metabolic parameters using microsensors is often limited to the medium surrounding the spheroid.^{18,19} Measurement of values or even tracing of gradients inside the spheroids can hardly be achieved by microsensors as typical sensor geometries are in the same size as the diameter. Although the penetration of the spheroid with sensors in the format of a microneedle is feasible,^{20–22} the results would strongly be influenced by the physical presence of the sensor.

Other 3D cell culture formats comprise cells growing **equally distributed in a 3D cell culture matrix** in a tissue-like manner, sometimes also comprising vessel-like structures to mimic vascularization.^{23,24} In such systems, sensors can be used to provide concentration readings at distinct points, *e.g.* outside the matrix and in the middle.

Microsensors can also be used to monitor **suspension cell culture**, however these systems typically relate to the field of bioreactors, which is not covered by this review.

Sensors and relevant parameters

Different metabolic parameters can be classified by the lifetime of the species and the presence or absence of strong gradients in the cell culture system. Both species with short lifetime (*e.g.* ROS, RNS) and substances with strong gradients, *i.e.* the source and sink within the cell culture (*e.g.* oxygen), require sensors located next to the cells (pericellular monitoring). Other parameters which are stable and consumed or produced by the cells only (such as glucose and lactate) are less critical regarding the spatial position of the sensor in relation to the cells. In a microfluidic system, these parameters could also be monitored downstream resulting in the same information about the cellular metabolism compared to readings from pericellular sensors. A summary of commonly used sensor types and relevant ranges for the major metabolic parameters can be found in Table 2.

It is important to know the absolute oxygen concentration because it is crucial for the aerobic or anaerobic pathways in

Potentiometric sensors with their inherent logarithmic transfer function (following the Nernst equation) would often fit better to the possible oxygen concentration ranges.³ However, to our knowledge, no potentiometric oxygen sensor has been applied successfully to monitor dissolved oxygen concentration in cell culture.

Acidification, pH

Potentiometric pH sensors, namely the pH glass electrode, are the most widely used sensors for proton activity. However, for application in cell culture, their size limits their usage during medium preparation. Only in bioreactors such electrodes are commonly applied. For cell culture monitoring, either light-addressable potentiometric sensors (LAPS), ion-selective field effect transistors (ISFET), metal oxide-based potentiometric sensors or optical sensors are used to monitor pH or the acidification rate (decrease of pH over time). The LAPS principle comprises a pH-sensitive insulation material like silicon oxynitride or Ta_2O_5 as the sensing element exposed to the electrolyte. Activation of charge carriers by LED or laser causes a photocurrent transducing the pH to an electrical quantity.³⁵ While early cell culture monitoring devices³⁶ measured acidification only using LAPS, this sensor principle was employed in recent multiparameter systems as well.^{37,38} ISFETs with a pH-sensitive gate material are among the smallest possible pH sensors employed in cell culture.^{39,40} Both LAPS and ISFET are limited to the availability of silicon as the substrate including CMOS circuits (see also the section on microfabrication and materials). Fanigliuolo *et al.* compared LAPS- and ISFET-based sensors to access cellular metabolism.⁴¹

Potentiometric pH sensors based on metal oxides, such as iridium oxide,^{42–46} tungsten oxide^{47–49} or ruthenium oxide,^{50–52} can also be used on transparent substrates and are often preferred because of their simple integration. However, the overall accuracy is also dependent on the stability of the reference electrode. Optical pH sensors are based on fluorescence quenching at alkaline pH, but usually need, in contrast to optical oxygen sensors, a second reference dye (dual lifetime referencing).⁵³

LAPSSs, ISFETs and potentiometric sensors have a logarithmic transfer function referring to the proton concentration

Parameter	Sensor types	Relevant range in cell culture	Analyte consumption
Oxygen	Direct amperometric sensor	0–200 μM	Yes
	Clark-type sensor	(0–20 kPa)	Depends on the principle
	Optical sensor (luminescence/fluorescence)		No
pH	Potentiometric sensor	5–8	No
	Optical sensor (luminescence/fluorescence)		No
Lactate	Electrochemical biosensor	0–15 mM	Yes
	Optical biosensor		Yes
Glucose	Electrochemical biosensor	0–25 mM	Yes
	Optical biosensor		Yes

Biosensors: glucose, lactate, glutamate, pyruvate

Sensors for short-lived species

The physiological concentration of NO is in the range of only pM to μ M during burst events.^{61,62} NO radicals show a typical diffusion of around 150–300 μ m within a 4–15 s range in biological media,^{63–67} whereas other sources report a diffusion of 10 μ m within 15 ms.⁶⁸

Under physiological conditions, the half-life of free superoxide radicals is very limited in the range of milliseconds to some few seconds. This short lifetime results in a low cellular basal concentration of some pM (ref. 69) and a free diffusion path length of around 40 μm under *in vivo* conditions.⁷⁰ The spontaneous decomposition rate of superoxide is strongly dependent on the local pH.

The short half-life and diffusion length of ROS and RNS arise from spontaneous or enzymatic decomposition and high reactivity with a bundle of different biomolecules, including membrane lipids, proteins, nucleic acids, other reactive species and transition metal ions. One example for a fast conversion is the reaction of NO* with O_2^{*-} to ONOO⁻ with an almost diffusion-controlled rate (the rate constant is $4\text{--}16 \times 10^9 \text{ mol}^{-1} \text{ L s}^{-1}$).⁷¹ As a consequence, the positioning of a sensor in the diffusion zone of ROS/RNS and the cellular microenvironment has tremendous influence on the signal height,⁶⁶ *e.g.* a complete signal loss at a position 1 mm away from single cell for NO measurement.⁶⁸ Also, Brovkovich *et al.* showed the direct influence of sensor tip distance on the NO signal in a single endothelial cell experiment.⁷² Lee *et al.* demonstrated the impact of electrode and sealing size at a needle-shaped NO microsensor setup.⁶⁵ It becomes obvious that a closer electrode cell distance (artificial synapse arrangement) increases the collection efficiency of the sensor. On the other hand, the diffusion of potential reaction partners like oxygen or arginine may be hindered by the sensor body, which leads to analyte accumulation.

In particular, in planar, chip-based sensor approaches with randomly growing cells, the complex hemispherical diffusion profiles for ROS and RNS can hardly be predicted. Further, the relationship between the diffusion profile/electrode overlap and electrode size may lead to a misinterpretation of the measured extracellular concentration when compared to an external calibration setup with homogeneously distributed analyte standards, even with correct sensor readings.

Microfabrication techniques allow for sensor design to measure within the expected area of occurrence and enable, along with appropriate electrochemical techniques, label-free measurement with sufficient spatial and time resolution. One approach to address the low concentration profiles of short-lived species might be the utilization of ultra-microelectrode (UME) arrays. A higher mass transfer rate, compared to millimetric electrodes, in terms of studying fast kinetics, and a better signal/noise ratio are the main aspects advocating their use, whereas smaller overall signals from lower electrode areas challenge the readout electronics' performance. Zhang *et al.* described an array of 2500 ultra-microelectrodes (carbon, 2 μm diameter) exploiting the effect of UME arrays for NO measurement.⁷³ This report demonstrated the occurrence of steady-state regimes and the

additivity of electrode currents. Later, the electrodes were coated with permselective membranes (Nafion and a commercial membrane from World Precision Instruments, USA) to enhance the selectivity towards NO, which can be detected by amperometry at 0.86 V *vs.* Ag/AgCl.

Parallel measurement of both ROS and RNS in stimulated adherent cell culture under static conditions was successfully demonstrated by Chang *et al.*⁷⁴ They used planar sputtered gold/cytochrome c electrodes for superoxide and screen-printed carbon electrodes with electrodeposited tetra-sulfonated nickel phthalocyanine (NiTSPc) for nitric oxide detection. The system consists of a full 24-well format sensor array and makes use of standard transwell inserts for cell culture pre-cultivation. The transwell is inserted into the measurement setup and avoids direct electrode/cell contact by the transfer membrane.

Another interesting approach by Isik *et al.* is the use of pyramid-shaped Pt tip electrodes on chip, to avoid direct cell-electrode contact and possible cell death upon electrical polarization.⁷⁵ The electrode tips are located between/above the cells, which enables a measurement of NO within its diffusion zone. The tips were modified with NiTSPc to improve their NO sensitivity and measurement with HUVEC cells was performed amperometrically at 0.75 V *vs.* Ag/AgCl. The study focused on adherent cell line cultivation under static conditions, but the 3D geometry of the electrodes might pave the way for measurement in tissue slices or 3D cell culture models.

Electrochemical measurement of ROS and RNS molecules makes use of specific redox potentials to discriminate between the main interfering substances, whereas the high oxidation potential especially for NO (>700 mV *vs.* Ag/AgCl) is not suitably specific. If high time resolution is required, fast-scan voltammetry and amperometric measurements are the methods of choice, but also with limited selectivity. Therefore, techniques like differential pulse voltammetry are a good compromise between acceptable time resolution and increased selectivity.

Alternative approaches to reduce cross-sensitivities use permselective membranes to cover the sensing electrodes, allowing only the analytes of interest to reach the electrode surface. Typical membrane materials in use are hydrogels, Nafion, polypyrrole, *o*-phenylenediamine or polymethylcellulose. In addition, we demonstrated selective and robust *in vitro* measurement of the superoxide radical by direct oxidation on a planar gold microelectrode covered with a polyethylenimine membrane.⁷⁶

Microfabrication and materials

Technology and substrate material

Early integrated cell culture monitoring systems used silicon as a substrate and were fabricated using (enhanced) CMOS technology.^{36,39,77–79} Silicon is essential in the case of LAPS and ISFETs, but also convenient for electrochemical sensors. An important possibility is to use the CMOS functionality to

integrate analog circuitry for amplification and multiplexing or even circuitry for digitalization directly into the sensor chip. Additionally, optical functionality like cameras^{80–82} could be integrated.

However, none of the described monitoring systems used integrated circuits to enhance signal performance or even eliminate external instrumentation. The sensor chip which is in direct contact with the cells should ideally be used once and therefore chips with integrated circuits generate unreasonably high costs. A critical disadvantage of silicon as a substrate is its opaqueness for visible light. Especially in the case of 2D cell culture, standard routines include optical inspection of the cells with through-light microscopy. Also, for 3D systems, optical access is beneficial. In the case of microfluidic systems, observation of bubbles simplifies successful measurements.

Approaches to introduce transparency by integration of a transparent window into the silicon chip⁷⁹ or small silicon chips into glass substrates³⁹ were mentioned. From today's perspective, the benefit of such approaches compared to the technological costs does not seem justifiable.

Glass substrates allow optical inspection of the cells as well as the possibility to use optical markers in the cell culture parallel to the microsensors. Thin-film processing for electrochemical sensors is possible using metals like platinum or gold along with silicon nitride or silicon oxide for passivation. Electrodes can be modified by electrodeposition of other metals onto the thin-film layers or coating with polymers similar to backend processes employed after CMOS fabrication in the case of silicon substrates.^{28,57}

Polymer-based systems can be flexible, such as dip-in microsensors based on polyimide,^{18,83} or used as stiff materials comparable to other cell culture labware, such as well plates with integrated optical sensors.³² Gas permeability is excellent in silicones, which can be employed for gas perfusion into the cell culture. Polydimethylsiloxane (PDMS) replicas are often used to form channels on top of glass chips in order to combine sensor chips with microfluidics.

Sensor functionalization

Electrochemical microsensors need (thin-film) electrodes based on metals or carbon. Depending on the sensor type, fully inert electrodes (*e.g.* glassy carbon), catalytically active but inert electrodes (*e.g.* platinum, gold) or redox-active electrodes (*e.g.* silver, copper) are employed. Often, the electrodes are covered with a diffusion-limiting membrane (*e.g.* pHEMA), which also prevents cells from sticking to the electrode surface. In the case of biosensors, the enzymes need to be immobilized directly on the electrode or dispersed in a membrane. All electrochemical sensors need a reference electrode, which is often silver/silver chloride with an appropriate membrane or coating, to avoid the adverse effect of dissolved silver ions on the cells.

Sensor functionalization for optical sensors is performed by application of the fluorescent dye dissolved in a



membrane material, typically made of silicone or similar gas-permeable polymeric material.

Material selection

All used materials need to be non-cytotoxic or be fully encapsulated. Additionally, the materials in direct contact with the cells should be optimized for the cells to adhere or, depending on the application, consist of cell-repelling material. Passivation layers from thin-film technology like silicon oxide and silicon nitride have shown to be well suited for culture cells, in the case of tumor cells even without additional coating.²⁸ Among the thick-film materials, the cytocompatibility of the epoxy-based polymer SU-8 is discussed controversially for different processing and cells.^{84–87} Coatings containing polyethylene glycol domains were suggested to render the material cell-repellent.⁸⁸ Because of the large variety of different cells used in culture, it is important to test all materials with respect to cytotoxicity and cytocompatibility for the specific cell type.

Sterilization

An important aspect is the selection of the appropriate sterilization method. Both the integrity of the material and the functionality of sensors have to be taken into account for choosing the procedure and dose. While for clinical application the employed sterilization method has to comply with regulatory demands, in research the importance of the topic is often neglected. In the case of microfabricated devices, the microbiological burden is typically low because of the clean room environment. This often allows applying disinfection using ethanol and culture media comprising antibiotics instead of sterilization.

For sensor systems fabricated in CMOS technology, gamma sterilization is often not preferred because of altered characteristics mainly due to generation of defects in the gate oxide. Elevated temperature (autoclaving) is often avoided because mechanical stress can cause failure in hybrid mounted sensor chips. Biosensors comprising enzymes rule out higher temperature at all, while ethanol should not come into contact with the enzyme membranes. For biosensors, gamma sterilization is often a good choice if enzyme stability is considered.

Systems for 2D cell culture – static conditions

The class of systems to monitor one or several parameters in 2D cell culture under static conditions typically replicates or enhances conventional culture vessel formats, like Petri dishes, well plates or tissue culture flasks. Depending on the desired parameter, fixed integration of the sensor points next to the cell layer is essential. Alternatively, dip-in approaches with sensors at defined positions using a motorized micro-stage can be applied.⁵

The majority of monitoring systems focusing on oxygen as the sole parameter employ optical oxygen sensors based on fluorescence quenching (Fig. 4A). Those works cover toxicity studies,³² evaluation of oxygen consumption rates,⁸⁹ investigation of hypoxia for cancer research⁹⁰ or in non-tumor cells,^{91–93} optimization of culture conditions,⁹⁴ stem cell differentiation,⁹⁵ and endocrinology.⁹⁶ Also, electrochemical oxygen sensors were used, mainly Clark-type²⁷ or direct amperometric sensors.²⁸ In our opinion, electrochemical sensors are only reasonable in the case of systems for multiparameter monitoring, especially in combination with biosensors, or if very low oxygen concentrations need to be measured.

Instead of integrating oxygen sensors into the bottom of the cell culture area, an approach was described using integrated sensor strips enabling measurements at different heights above the bottom of the cell culture.⁸³ This system is intended for determining oxygen gradients in stagnant medium above the cells in 2D culture, but would be an interesting approach to access oxygenation in 3D cell culture as well.

Another group of systems focuses on oxygen and pH as measurement parameters, for which mainly optical sensors are used.^{97,98} Further steps towards comprehensive multiparameter monitoring of cellular metabolism is the integration of biosensors into the sensor systems for static culture conditions. Systems were proposed using biosensors combined with microdialysis to measure glucose and lactate in static cell cultures (Fig. 4B).^{99–102} Glucose was also measured directly using a sensor chip dipped into a static cell culture.^{103,104}

A multiparameter system measuring oxygen, pH, glucose and lactate using silicon chips was described for static cell culture in wells (Fig. 4C).^{105,106} The *Sensing Cell Culture Flask* (Fig. 4D) was introduced as an electrochemical sensor platform on transparent glass chips, embedded into the bottom of conventional tissue culture flasks, with sensors for oxygen, pH, glucose and lactate.^{28,76,83,107}

Systems for 2D cell culture – dynamic conditions

In traditional 2D cell cultures, cells grow as an adherent monolayer at the bottom of relatively large vessels, *e.g.* flasks or microtiter plates. Total media volumes are in the range of 100 μ L to several mL. With typical handling, *i.e.* medium change every few days, strong gradients of metabolites develop slowly because diffusion is comparably slow (Fig. 3A). The aim of dynamic cell culture monitoring is to reduce liquid volume to a few microliters and therefore to generate fast concentration changes. To maintain appropriate culture conditions, this approach requires periodic exchange of medium to keep cells alive (Fig. 3C). By such periodic exchange through microfluidics in stop/flow protocols, metabolic rates can be measured repetitively within minutes by microsensors placed directly underneath the cells in the culture chamber or in the microfluidic outlet channels. Such systems for the





Fig. 4 Sensor systems for metabolic monitoring in 2D static culture. **A:** Optical monitoring system to measure oxygen at the bottom of cell culture wells³² (reprinted with permission from Elsevier). **B:** Microdialysis system to monitor glucose and lactate¹⁰² (reprinted with permission from Elsevier). **C:** Multiparameter monitoring on a silicon chip with oxygen, pH, glucose and lactate sensors¹⁰⁵ (reprinted from Pemberton *et al.*, 2016, DOI 10.3390/s141120519, under CC BY 4.0). **D:** *Sensing Cell Culture Flask*: a transparent sensor chip with different electrochemical sensors is embedded in the bottom of a tissue culture flask.¹⁰⁷

label-free, non-invasive monitoring of cell metabolism are called microphysiometers. Metabolic rates are accessible online, and changes upon substance exposure can be quantified. Suspended cells cannot attach properly to the chip surface under flow conditions to form 2D monolayers. Therefore, such systems are typically operated in an open configuration similar to a microtiter plate during a culture phase over up to a few days with a larger volume above the cells, during which the cells form adherent layers. For measurement, the systems are sealed with plugs, and the volume is reduced drastically for microfluidic operation.

The first microphysiometer (Fig. 5A) was based on a silicon chip with an integrated light-addressable potentiometric sensor (LAPS) for pH measurement.^{35,77} A sample of 10^4 to 10^6 cells was inserted onto a membrane. A plug with vertical in- and outflow channels was inserted for operation, reducing the chamber volume to 2.8 μL for measurement,¹⁰⁸ and a peristaltic pump was connected. The flow was stopped for around 30 s, during which extracellular acidification changed the pH in the range of 0.1 units. The system was later commercialized as the *Cytosensor*³⁶ and enhanced by other sensor types. By insertion of platinum wires into the sealing plug and subsequent polishing, microelectrodes were formed above the cell layer. Electrochemical biosensors for glucose and lactate and dissolved oxygen sensors were integrated.^{109–111} Newer implementations of the LAPS microphysiometry principle exist.^{37,38,112} With similar protocols, pH was also measured by means of ion-selective field effect transistors (ISFET) using CMOS technology on silicon chips.^{78,79,113} ISFETs also allowed the determination of dissolved oxygen by local pH changes.³⁰ More common is the direct amperometric measurement of oxygen by reduction at noble metal electrodes.^{57,110,114}

Another parameter of interest in such systems is cellular adhesion, which is measured by impedance analysis.^{78,79} Attachment and spreading of cells on interdigital electrode structures (IDES) is determined by capacitance changes. Adhesion can be monitored continuously during all phases of cell growth, and is mostly independent of flow. The combination of IDES-based impedance monitoring with ISFET-based pH sensing and amperometric oxygen measurement for drug and toxicology screening on a silicon chip was commercialized by Bionas (Fig. 5B).^{56,115} The key feature of microphysiometers, in comparison to traditional end-point tests, is the rapid determination of metabolic rates in a continuous, online measurement (Fig. 6A), which reveals transient recovery effects of cellular metabolism and allows the investigation of pharmacodynamics in drug screening (Fig. 6B) and cancer research.^{56,57,116}

Particularly for enzyme-based biosensors which produce hydrogen peroxide as an intermediary product, sensor placement outside the cell culture chamber is desirable to reduce oxidative stress. We demonstrated the placement of glucose and lactate biosensors in the outlet channel (Fig. 5C).^{57,117} Undiluted medium from the cell chamber was transported to the biosensor array and measured during the flow phase. Amperometric oxygen sensors based on platinum electrodes and potentiometric pH sensors based on iridium oxide electrodes were included in the cell culture chamber. In contrast to silicon-based devices, we integrated these electrochemical, multiparametric sensors on a transparent glass chip, which facilitates microscopy. Other groups focused on reduction of the volume to the sub-microliter range for glucose¹¹⁸ and lactate¹¹⁹ measurement or alternative fabrication methods such as screen- and inkjet-printing.¹²⁰

The method and systems commercialized by Seahorse Bioscience fall between static and dynamic monitoring.⁵⁵ Cells



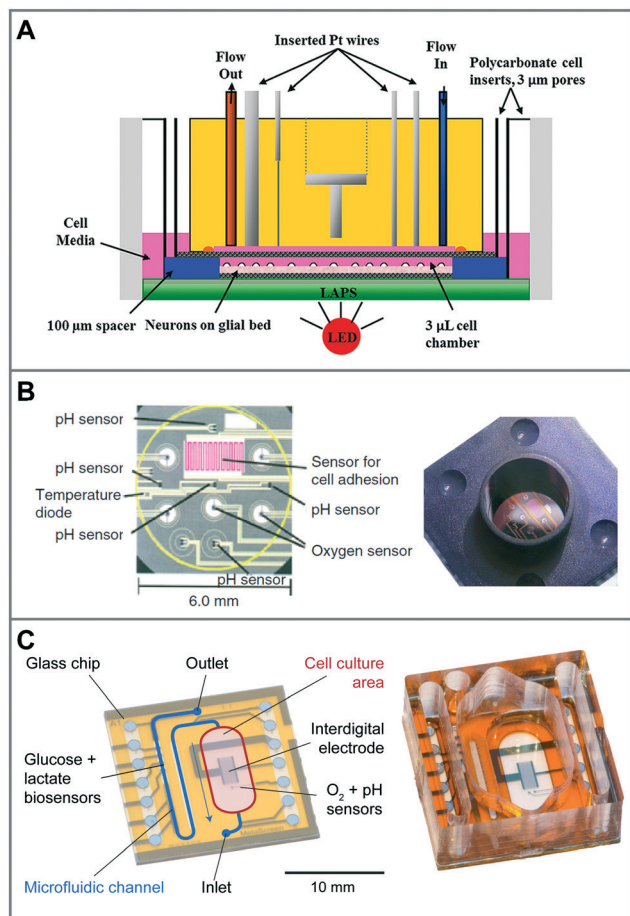


Fig. 5 Sensor systems for metabolic monitoring in 2D dynamic culture (microphysiometers). Cells are cultured directly on microsensor chips. For measurement, the medium volume is reduced to a few microliters and periodically exchanged by microfluidics. **A:** The Cytosensor microphysiometer based on a silicon chip, in which pH is measured with a light-addressable potentiometric sensor (LAPS). Amperometric microsensors are included by integrating wires in the cover.¹¹¹ (reprinted with permission, Copyright 2012 American Chemical Society). **B:** Silicon-based system with planar sensor integration for pH (ISFET), oxygen (amperometric) and cellular adhesion (interdigital electrode)^{56,115} (reprinted with permission from Elsevier). **C:** Glass-based system for better microscopy with *in situ* amperometric oxygen sensors (platinum), potentiometric pH sensors (iridium oxide) and an interdigital electrode, as well as amperometric glucose and lactate biosensors integrated in the downstream microfluidics.^{57,107}

are cultured in largely standard microtiter plates, into which a sensor probe is lowered, temporarily reducing the volume above the cells to around 2 µL. Oxygen and pH are measured using optical sensors. Pneumatic reservoirs above the medium enable the addition of test compounds, and the movement of the sensor tip mixes the medium. Metabolic rate determination within minutes is possible, but options for microfluidics and sensor placement are limited. The system allows parallel experiments in the entire plate with automated sequential readout. From an engineering standpoint, using microphysiometer systems seems straightforward. However, their operation with a combination of fluidics, sensors and cell handling is more complex than standard proce-



Fig. 6 Typical measurements from dynamic cell culture monitoring with microsensors. **A:** Extracellular acidification of 2D cells during the stop phase (pump off) in a microphysiometer system and return to the baseline during the flow phase (pump on)⁵⁶ (reprinted with permission from Elsevier). **B:** Metabolic rates for acidification, respiration and adhesion extracted from such an experiment. Rates change upon substance exposure, and continuous, online monitoring allows the measurement of pharmacodynamics and recovery effects in the drug screening application⁵⁶ (reprinted with permission from Elsevier). **C:** Biosensor measurement of lactate production from 3D microtissue spheroids in hanging droplets, including the blank signal, which shows lactate production and return to baseline depending on the flow profile¹⁹ (reprinted from Misun *et al.*, 2016, DOI 10.1038/micronano.2016.22, under CC BY 4.0).

dures in cell biology. The amount of data acquired is high compared to end-point tests and requires at least some basic data processing to obtain meaningful results. Valuable efforts to automate operation¹²¹ and parameterize data processing¹²² have been made. However, few novel concepts or parameters have emerged within the last decade, and many existing systems have faded away. Other systems never left



academia and might have suffered from reliability problems. Their complexity and their limited compatibility with true high-throughput screening are drawbacks which still persist even among the novel approaches for 3D cell cultures.

Systems for 3D cell culture and organ-on-chip

Regarding the access to cell metabolites, there are two main differences between 3D and monolayer cultures. First, cell numbers are usually lower in 3D culture¹² (10^3 in microtissues or spheroids vs. 10^4 – 10^6 in standard 2D monolayers), and cell aggregates are often distributed heterogeneously in space. Thus, concentration changes are smaller. Gradients are less homogeneous and multidirectional (Fig. 3B). Second, if cells are non-adherent, microfluidic protocols are not as easily applicable, because cells may be washed away. Measurements by impedance, which often rely on cell attachment and are used extensively in 2D, are also more difficult. If cells are in a solid matrix, there is not even direct fluidic access, and metabolite exchange relies on diffusion of metabolites through the matrix. Fluidic channels must be formed by microstructuring of the matrix.

Many microfluidic systems have been developed for the formation, trapping and culture of non-adherent microtissues, but very few include sensors to measure cell metabolites. Systems are often microfluidic channel networks fabricated from molded or thermoformed polymers with small wells to trap the microtissues, while the medium flows over or alongside the well.^{123–127} Paper has also been used for both fluidic compartments and cell scaffold.^{128,129} Supernatants and perfusion media are then transferred to external readers or analysed *in situ*. Measurement is often limited to viability testing by optical methods such as fluorimetric live/dead staining.^{16,130} As these systems often require periodic or constant perfusion, a strict differentiation between dynamic and static measurement is more difficult.

The straightforward, static dip-in approach is to measure metabolites directly in the stagnant supernatant in standard culture vessels, *i.e.* microtiter plates. Here, two difficulties arise: due to the low cell number, concentration changes are small, and medium exchange happens only every few days. This requires highly sensitive and long-term stable sensors since the fluid volume cannot be reduced indefinitely. We showed the direct measurement of lactate and oxygen using electrochemical microsensors in standard 96-well plates containing a single microtissue spheroid.^{18,131} Needle-type sensor strips¹³² with microelectrodes at the tip were dipped into and remained in the well over days. The integration of the sensor system into the standardized setup enables compatibility with standard handling procedures. Lactate production rates from 2000-cell spheroids in the range of $5 \mu\text{M h}^{-1}$ were measured over up to three days. Oxygen measurement in the direct vicinity of the spheroids also revealed no hypoxic conditions in the well even though assumingly anaerobic metabolic pathways were active. By measuring altered meta-

bolic rates under drug exposure, we demonstrated that metabolic access yields valuable information in drug screening, which complements and enhances microscopy or viability tests. Generally, electrochemical systems with electrode sizes in the micrometer range allow a highly localized measurement.

As in 2D systems, microfluidics can be utilized to reduce total media volumes and thus increase concentration changes. Collection and undiluted transport of media to downstream sensors enables the integral measurement over numerous microtissues. Such a system was realized for a multiwell bioreactor for hepatic spheroids (Fig. 7A).¹³³ Nine microtissues were kept in approx. $1.2 \mu\text{L}$ wells each, within a gas-tight bioreactor with constant perfusion. Sensors included *in situ* oxygen sensors composed of tissue-embedded phosphorescent beads and commercial amperometric biosensors for glucose and lactate off-chip, in a combined outlet channel.¹³⁴ Oxygen was measured continuously over 28 d and consumption rates were determined. After 4 d of adaptation, distinctly lower concentrations than air saturation were measured in the microwells. Glucose and lactate metabolism from all microtissues combined was measured from $40 \mu\text{L}$ medium extracted from the bioreactor. Microfluidic switching allowed frequent calibration of the biosensors with external solutions to account for drift of the sensors. A comparable concept for multi-organoid drug screening has been shown recently,¹³⁵ in which cardiac and



Fig. 7 Sensor systems for metabolic monitoring in 3D cell culture. **A:** 3D microtissue spheroids trapped in microwells within a perfused microbioreactor. Oxygen and pH are measured optically through nanoparticles embedded in the microtissues. Glucose and lactate are measured using downstream amperometric biosensors connected by a microfluidic switchboard¹³³ (copyright 2016 National Academy of Sciences). **B:** 3D microtissue spheroids cultured in interconnected hanging droplet networks. A glass-based sensor chip and microstructures allow fluidic connection between the drops and integration of *in situ* microsensors for, *e.g.* lactate, glucose or impedance¹⁹ (reprinted from Misun *et al.*, 2016, DOI 10.1038/micronano.2016.22, under CC BY 4.0).



Although a number of systems exist with promising new approaches, to date, in 3D cultures, the exact metabolic state and immediate microenvironment, *i.e.* nutrient and oxygen supply, of the microtissues have still been largely unknown and relied mainly on the controlled exchange of media and diffusion of metabolites. Especially for oxygen, measurement within the microtissue would be desirable, but current micro-sensors are typically not small enough to be inserted with sufficiently low tissue interference.

Potential and benefits of metabolic monitoring

The primary advantages of microfluidic systems are the reduction of media volume and thus faster concentration changes, the transport of undiluted medium to downstream sensors, as well as the possibility to repeatedly and efficiently generate a broad range of stimuli. The interplay between the state of the cells, microenvironment and sensing method is complex. Both the choice of a suitable measurement system and the obtained experimental findings must be critically evaluated for the aspects how cells are cultivated and supplied, how metabolites are transported to the sensors and how stimuli are generated. From the perspective of metabolic sensing, it is evident that even in simple, standard cell culture experiments, in which sometimes complex markers or pathways are investigated, basic metabolic parameters at the pericellular level are often unknown. Diffusion of metabolites in stagnant media or even solid matrices is comparably slow. If there is no flow, transport of metabolites to and from the cells will be governed by diffusion and thermal convection only. Therefore, nutrient or oxygen depletion can occur near the cells, even if those parameters seem globally well controlled. In 3D, the state and measurement of metabolites can be even more challenging. As a consequence, this may negatively affect the reproducibility or validity of findings in such experiments. At the moment, microsensors can therefore most likely still contribute more to standardization of cell culture experiments or help in basic physiological investigations, rather than replace classical high-throughput screening approaches.

Bringing sensors close to cells is important in order to obtain pericellular readings. In contrast, the physical presence of a sensor hinders a directly neighboring cell at the position of the sensor and slightly changes the diffusion profile next to the cell. In the case of single cell monitoring, this effect is crucial, and a trade-off has to be made. In 2D or 3D cell

cultures, the presence of the microsensor typically does not have much influence, compared to other boundary conditions of the culture itself.

In general, sensors without analyte consumption are preferred to minimize influence on the cellular microenvironment. An exception is the case of 2D cell culture with oxygen sensors positioned between the cells. Typically, cells cannot grow at the very same position of the sensor, thus causing spots in the cell layer without cellular respiration. Therefore, it is beneficial that such a microsensor shows analyte consumption in the range of the cellular respiration to avoid an anomaly in the diffusion profile next to the sensor.

The electrochemical measurement of short-lived reactive species concentration (ROS/RNS) and its spatial distribution is only possible in close vicinity to the releasing cell under stagnant conditions, which excludes downstream detection in microfluidic devices. Planar microdisc sensors in direct vicinity to adherent 2D cell cultures and needle-shaped electrodes, especially suited for 3D culture models, are the only way to address the fleeting existence of these substances. Needle-shaped sensors suffer from bad reproducibility, vibration sensitivity, fragile handling and low throughput due to (motorized) manual positioning under the microscope. Measurement results from planar microsensor platforms with randomly growing cells should be evaluated critically with respect to a particular system design/setup, whose influence on the findings might be underestimated.

Electrochemical, enzyme-based biosensors require frequent calibration because of sensitivity drift, and the enzymatic reaction may release harmful by-products. Placement outside the actual cell culture area addresses both aspects. For long-term application, schemes for recalibration should be considered.

The sometimes considerable complexity of fabrication technology and operation, as well as incompatibility with standard procedures, limits the widespread application of more advanced microfluidic systems. A simplification of microfluidic handling would often be desirable, which could mean the elimination of pumps and reliance on pipetting or passive flow for media exchange. Instrumentation for electrochemical sensors and optical sensors appears to be an expensive investment at first glance. However, upon closer look, the costs for instrumentation equipment are low compared to the typical installation costs for a cell laboratory. Still, there is a need for cost-effective parallelization in order to meet high-throughput screening demands.

Once standardization is established, it is unclear whether the measurement of basic metabolic parameters (O_2 , pH, glucose, lactate) will be equally important as other indicating parameters like gene expression *etc.* For 3D cell culture, in which major gradients occur within the microtissues, it is desirable to measure inside such structures with minimal invasion. Instead of sensors, embedded particles which could be read out from the outside are promising alternatives for some parameters and can also address the overall heterogeneity of such cultures.

Impact of microsensor systems on organ-on-chip and human-on-chip systems

In organ-on-chip systems, the cells as sub-units are linked together to model the functionality of a specific organ. Similarly, such organ-on-chip systems as sub-units can be linked together in order to model partial functionality of the human body and are therefore sometimes visionarily called body-on-chip or human-on-chip systems.^{141,142}

The basic requirements and challenges for microsensors are the same, independent of whether it is a 2D cell culture or an organ-on-chip system. Notably, the complexity increases from 2D to 3D. Once a system can be used in 3D cell culture models, it can be readily applied to organ-on-chip systems. From the point of view of cell culture monitoring, there is no difference between a 3D culture of cells without organotypic function and an organ-on-chip system. However, the impact of these systems changes from just reporting the metabolic state of the cells to providing insight into cell-cell interactions enabling the functionality of the organ by observing the metabolism of some representative cells within the model. Here, sensor readings can be linked to and provide input for computer models ("*in silico*"), which become more and more important with the increasing complexity from organ-on-chip to human-on-chip. In our understanding, a meaningful human-on-chip cellular model can hardly be described and accessed without microsensors reading the metabolic state at characteristic points in the system.

Conflicts of interest

There are no conflicts to declare.

Acknowledgements

The authors would like to thank all collaborators in the European Union projects EUROXY (FP6-LIFESCIHEALTH) and METOXIA (FP7-HEALTH-2007-B), namely Peter Ebbesen, Erik O. Pettersen, Joe A. Sandvik and Jan Villadsen, who shaped the authors' views on the relevance and limitation of microsensors for cell culture monitoring and its implications on cancer research.

References

- 1 D. Huh, Y. Torisawa, G. A. Hamilton, H. J. Kim and D. E. Ingber, *Lab Chip*, 2012, **12**, 2156–2164.
- 2 B. Zhang and M. Radisic, *Lab Chip*, 2017, **17**, 2395–2420.
- 3 P. Ebbesen, K.-U. Eckardt, F. Ciampor and E. O. Pettersen, *Acta Oncol.*, 2004, **43**, 598–600.
- 4 P. Ebbesen, E. O. Pettersen, J. Denekamp, B. Littband, J. Keski-Oja, A. Schousboe, U. Sonnewald, Ø. Åmellem and V. Zachar, *Acta Oncol.*, 2000, **39**, 247–248.
- 5 E. O. Pettersen, L. H. Larsen, N. B. Ramsing and P. Ebbesen, *Cell Proliferation*, 2005, **38**, 257–267.
- 6 M. D. Brennan, M. L. Rexius-Hall, L. J. Elgass and D. T. Eddington, *Lab Chip*, 2014, **14**, 4305–4318.



- 7 P. E. Oomen, M. D. Skolimowski and E. Verpoorte, *Lab Chip*, 2016, **16**, 3394–3414.
- 8 L. G. Griffith and M. A. Swartz, *Nat. Rev. Mol. Cell Biol.*, 2006, **7**, 211–224.
- 9 F. Pampaloni, E. G. Reynaud and E. H. K. Stelzer, *Nat. Rev. Mol. Cell Biol.*, 2007, **8**, 839–845.
- 10 M. Simian and M. J. Bissell, *J. Cell Biol.*, 2017, **216**, 31–40.
- 11 E. Fennema, N. Rivron, J. Rouwkema, C. van Blitterswijk and J. De Boer, *Trends Biotechnol.*, 2013, **31**, 108–115.
- 12 R. Z. Lin and H. Y. Chang, *Biotechnol. J.*, 2008, **3**, 1172–1184.
- 13 H. K. Kleinman and G. R. Martin, *Semin. Cancer Biol.*, 2005, **15**, 378–386.
- 14 D. R. Grimes, C. Kelly, K. Bloch and M. Partridge, *J. R. Soc., Interface*, 2014, **11**, 20131124–20131124.
- 15 S. Messner, I. Agarkova, W. Moritz and J. M. Kelm, *Arch. Toxicol.*, 2013, **87**, 209–213.
- 16 Y.-C. Tung, A. Y. Hsiao, S. G. Allen, Y. Torisawa, M. Ho and S. Takayama, *Analyst*, 2011, **136**, 473–478.
- 17 O. Frey, P. M. Misun, D. A. Fluri, J. G. Hengstler and A. Hierlemann, *Nat. Commun.*, 2014, **5**, 4250.
- 18 A. Weltin, S. Hammer, F. Noor, Y. Kaminski, J. Kieninger and G. A. Urban, *Biosens. Bioelectron.*, 2017, **87**, 941–948.
- 19 P. M. Misun, J. Rothe, Y. R. F. Schmid, A. Hierlemann and O. Frey, *Microsyst. Nanoeng.*, 2016, **2**, 16022.
- 20 J. Carlsson, C. G. Stålnacke, H. Acker, M. Haji-Karim, S. Nilsson and B. Larsson, *Int. J. Radiat. Oncol., Biol., Phys.*, 1979, **5**, 2011–2020.
- 21 R. M. Sutherland and W. F. Mueller-Klieser, *Cancer Res.*, 1982, **42**, 237–242.
- 22 W. F. Mueller-Klieser and R. M. Sutherland, *Br. J. Cancer*, 1982, **45**, 256–264.
- 23 H. Lee, M. Chung and N. L. Jeon, *MRS Bull.*, 2014, **39**, 51–59.
- 24 D. T. T. Phan, X. Wang, B. M. Craver, A. Sobrino, D. Zhao, J. C. Chen, L. Y. N. Lee, S. C. George, A. P. Lee and C. C. W. Hughes, *Lab Chip*, 2017, **17**, 511–520.
- 25 H. Suzuki, A. Sugama and N. Kojima, *Sens. Actuators, B*, 1990, **2**, 297–303.
- 26 G. Jobst, G. Urban, A. Jachimowicz and F. Kohl, *Biosens. Bioelectron.*, 1993, **8**, 123–128.
- 27 C. C. Wu, H. N. Luk, Y. T. T. Lin and C. Y. Yuan, *Talanta*, 2010, **81**, 228–234.
- 28 J. Kieninger, K. Aravindalochanan, J. A. Sandvik, E. O. Pettersen and G. A. Urban, *Cell Proliferation*, 2014, **47**, 180–188.
- 29 B.-K. Sohn and C.-S. Kim, *Sens. Actuators, B*, 1996, **34**, 435–440.
- 30 M. Lehmann, W. Baumann, M. Brischwein, H. Gahle, I. Freund, R. Ehret, S. Drechsler, H. Palzer, M. Kleintges, U. Sieben and B. Wolf, *Biosens. Bioelectron.*, 2001, **16**, 195–203.
- 31 I. Klimant and O. S. Wolfbeis, *Anal. Chem.*, 1995, **67**, 3160–3166.
- 32 S. Beckers, F. Noor, U. Müller-Vieira, M. Mayer, A. Strigun and E. Heinzle, *Toxicol. In Vitro*, 2010, **24**, 686–694.
- 33 C. J. Ochs, J. Kasuya, A. Pavesi and R. D. Kamm, *Lab Chip*, 2014, **14**, 459–462.
- 34 P. C. Thomas, M. Halter, A. Tona, S. R. Raghavan, A. L. Plant and S. P. Forry, *Anal. Chem.*, 2009, **81**, 9239–9246.
- 35 D. Hafeman, J. Parce and H. McConnell, *Science*, 1988, 1182–1185.
- 36 H. McConnell, J. Owicki, J. Parce, D. Miller, G. Baxter, H. Wada and S. Pitchford, *Science*, 1992, **257**, 1906–1912.
- 37 C. Wu, J. Zhou, N. Hu, D. Ha, X. Miao and P. Wang, *Sens. Actuators, A*, 2013, **199**, 136–142.
- 38 K. Su, J. Zhou, L. Zou, T. Wang, L. Zhuang, N. Hu and P. Wang, *Sens. Actuators, A*, 2014, **220**, 144–152.
- 39 W. H. Baumann, M. Lehmann, A. Schwinde, R. Ehret, M. Brischwein and B. Wolf, *Sens. Actuators, B*, 1999, **55**, 77–89.
- 40 P. Bergveld, *Sens. Actuators, B*, 2003, **88**, 1–20.
- 41 A. Fanigliulo, P. Accossato, M. Adami, M. Lanzi, S. Martinoia, S. Paddeu, M. T. Parodi, A. Rossi, M. Sartore, M. Grattarola and C. Nicolini, *Sens. Actuators, B*, 1996, **32**, 41–48.
- 42 W. Olthuis, M. A. M. Robben, P. Bergveld, M. Bos and W. E. van der Linden, *Sens. Actuators, B*, 1990, **2**, 247–256.
- 43 S. A. M. Marzouk, *Anal. Chem.*, 2003, **75**, 1258–1266.
- 44 I. A. Ges, B. L. Ivanov, D. K. Schaffer, E. A. Lima, A. A. Werdich and F. J. Baudenbacher, *Biosens. Bioelectron.*, 2005, **21**, 248–256.
- 45 I. A. Ges, B. L. Ivanov, A. A. Werdich and F. J. Baudenbacher, *Biosens. Bioelectron.*, 2007, **22**, 1303–1310.
- 46 T. Y. Kim and S. Yang, *Sens. Actuators, B*, 2014, **196**, 31–38.
- 47 K. Yamamoto, G. Shi, T. Zhou, F. Xu, M. Zhu, M. Liu, T. Kato, J. Y. Jin and L. Jin, *Anal. Chim. Acta*, 2003, **480**, 109–117.
- 48 P. Salazar, F. J. Garcia-Garcia, F. Yubero, J. Gil-Rostra and A. R. González-Elipe, *Electrochim. Acta*, 2016, **193**, 24–31.
- 49 Q. Guo, X. Wu, E. H. Han and W. Ke, *J. Electroanal. Chem.*, 2016, **782**, 91–97.
- 50 Y. H. Liao and J. C. Chou, *Sens. Actuators, B*, 2008, **128**, 603–612.
- 51 M. Brischwein, H. Grothe, J. Wiest, M. Zottmann, J. Ressler and B. Wolf, *Chem. Anal.*, 2009, **54**, 1193–1201.
- 52 A. Sardarinejad, D. K. Maurya and K. Alameh, *Sens. Actuators, A*, 2014, **214**, 15–19.
- 53 G. Liebsch, I. Klimant, C. Krause and O. S. Wolfbeis, *Anal. Chem.*, 2001, **73**, 4354–4363.
- 54 Y. Tian, B. R. Shumway, A. Cody Youngbull, Y. Li, A. K. Y. Jen, R. H. Johnson and D. R. Meldrum, *Sens. Actuators, B*, 2010, **147**, 714–722.
- 55 M. Wu, A. Neilson, A. L. Swift, R. Moran, J. Tamagnine, D. Parslow, S. Armistead, K. Lemire, J. Orrell, J. Teich, S. Chomicz and D. A. Ferrick, *Am. J. Physiol.*, 2006, **292**, C125–C136.
- 56 E. Thedinga, A. Kob, H. Holst, A. Keuer, S. Drechsler, R. Niendorf, W. Baumann, I. Freund, M. Lehmann and R. Ehret, *Toxicol. Appl. Pharmacol.*, 2007, **220**, 33–44.
- 57 A. Weltin, K. Slotwinski, J. Kieninger, I. Moser, G. Jobst, M. Wego, R. Ehret and G. A. Urban, *Lab Chip*, 2014, **14**, 138–146.
- 58 G. Jobst, I. Moser, M. Varahram, P. Svasek, E. Aschauer, Z. Trajanoski, P. Wach, P. Kotanko, F. Skrabal and G. Urban, *Anal. Chem.*, 1996, **68**, 3173–3179.



- 59 A. Weltin, J. Kieninger and G. A. Urban, *Anal. Bioanal. Chem.*, 2016, **408**, 4503–4521.
- 60 V. B. Koman, C. Santschi and O. J. F. Martin, *Biomed. Opt. Express*, 2015, **6**, 2353.
- 61 J. C. Toledo and O. Augusto, *Chem. Res. Toxicol.*, 2012, **25**, 975–989.
- 62 J. S. Stamler, D. I. Simon, J. A. Osborne, M. E. Mullins, O. Jaraki, T. Michel, D. J. Singel and J. Loscalzo, *Proc. Natl. Acad. Sci. U. S. A.*, 1992, **89**, 444–448.
- 63 C. Amatore, S. Arbault, M. Guille and F. Lemaître, *Chem. Rev.*, 2008, **108**, 2585–2621.
- 64 J. R. Lancaster, *Nitric Oxide*, 1997, **1**, 18–30.
- 65 Y. Lee, J. Yang, S. M. Rudich, R. J. Schreiner and M. E. Meyerhoff, *Anal. Chem.*, 2004, **76**, 545–551.
- 66 S. Isik, M. Etienne, J. Oni, A. Blöchl, S. Reiter and W. Schuhmann, *Anal. Chem.*, 2004, **76**, 6389–6394.
- 67 S. Isik and W. Schuhmann, *Angew. Chem., Int. Ed.*, 2006, **45**, 7451–7454.
- 68 D. M. Porterfield, J. D. Laskin, S. K. Jung, R. P. Malchow, B. Billack, P. J. Smith and D. E. Heck, *Am. J. Physiol.*, 2001, **281**, L904–L912.
- 69 X. J. Chen, A. C. West, D. M. Crokek and S. Banta, *Anal. Chem.*, 2008, **80**, 9622–9629.
- 70 M. Saran and W. Bors, *Chem.-Biol. Interact.*, 1994, **90**, 35–45.
- 71 G. Ferrer-Sueta and R. Radi, *ACS Chem. Biol.*, 2009, **4**, 161–177.
- 72 V. Brovkovich, E. Stolarczyk, J. Oman, P. Tomboulou and T. Malinski, *J. Pharm. Biomed. Anal.*, 1999, **19**, 135–143.
- 73 X. Zhang, J. Lin, L. Cardoso, M. Broderick and V. Darley-Usmar, *Electroanalysis*, 2002, **14**, 697–703.
- 74 S.-C. Chang, N. Pereira-Rodrigues, J. R. Henderson, A. Cole, F. Bedioui and C. J. McNeil, *Biosens. Bioelectron.*, 2005, **21**, 917–922.
- 75 S. Isik, L. Berdondini, J. Oni, A. Blöchl, M. Koudelka-Hep and W. Schuhmann, *Biosens. Bioelectron.*, 2005, **20**, 1566–1572.
- 76 H. Flamm, J. Kieninger, A. Weltin and G. A. Urban, *Biosens. Bioelectron.*, 2015, **65**, 354–359.
- 77 J. Owicki and J. W. Parce, *Biosens. Bioelectron.*, 1992, **7**, 255–272.
- 78 R. Ehret, W. Baumann, M. Brischwein, A. Schwinde, K. Stegbauer and B. Wolf, *Biosens. Bioelectron.*, 1997, **12**, 29–41.
- 79 B. Wolf, M. Brischwein, W. Baumann, R. Ehret and M. Kraus, *Biosens. Bioelectron.*, 1998, **13**, 501–509.
- 80 A. Ozcan and U. Demirci, *Lab Chip*, 2008, **8**, 98–106.
- 81 G. Zheng, S. A. Lee, Y. Antebi, M. B. Elowitz and C. Yang, *Proc. Natl. Acad. Sci. U. S. A.*, 2011, **108**, 16889–16894.
- 82 A. Greenbaum, W. Luo, T.-W. Su, Z. Göröcs, L. Xue, S. O. Isikman, A. F. Coskun, O. Mudanyali and A. Ozcan, *Nat. Methods*, 2012, **9**, 889–895.
- 83 P. Ebbesen, E. O. Pettersen, T. A. Gorr, G. Jobst, K. Williams, J. Kieninger, R. H. Wenger, S. Pastorekova, L. Dubois, P. Lambin, B. G. Wouters, T. Van Den Beucken, C. T. Supuran, L. Poellinger, P. Ratcliffe, A. Kanopka, A. Görlach, M. Gasmann, A. L. Harris, P. Maxwell and A. Scozzafava, *J. Enzyme Inhib. Med. Chem.*, 2009, **24**, 1–39.
- 84 Z.-Z. Wu, Y. Zhao and W. S. Kisaalita, *Colloids Surf., B*, 2006, **52**, 14–21.
- 85 V. N. Vernekar, D. K. Cullen, N. Fogleman, Y. Choi, A. J. Garcia, M. G. Allen, G. J. Brewer and M. C. LaPlaca, *J. Biomed. Mater. Res., Part A*, 2008, **89A**, 138–151.
- 86 K. V. Nemani, K. L. Moodie, J. B. Brennick, A. Su and B. Gim, *Mater. Sci. Eng., C*, 2013, **33**, 4453–4459.
- 87 A. Ajetunmobi, D. McAllister, N. Jain, O. Brazil, A. Corvin, Y. Volkov, D. Tropea and A. Prina-Mello, *J. Biomed. Mater. Res., Part A*, 2017, **105**, 2129–2138.
- 88 D. J. Kenan, E. B. Walsh, S. R. Meyers, G. A. O'Toole, E. G. Carruthers, W. K. Lee, S. Zauscher, C. A. H. Prata and M. W. Grinstaff, *Chem. Biol.*, 2006, **13**, 695–700.
- 89 R. R. Deshpande and E. Heinzle, *Biotechnol. Lett.*, 2004, **26**, 763–767.
- 90 A. Wouters, B. Pauwels, H. A. J. Lambrechts, G. G. O. Pattyn, J. Ides, M. Baay, P. Meijnders, S. Dewilde, J. B. Vermorken and F. Lardon, *Cancer Lett.*, 2009, **286**, 180–188.
- 91 N. Dehne, G. Hintereder and B. Brüne, *Exp. Cell Res.*, 2010, **316**, 1179–1189.
- 92 T. G. Fernandes, M. M. Diogo, A. Fernandes-Platzgummer, C. L. da Silva and J. M. S. Cabral, *Stem Cell Res.*, 2010, **5**, 76–89.
- 93 H. E. Abaci, R. Truitt, E. Luong, G. Drazer and S. Gerecht, *Am. J. Physiol.*, 2010, **298**, C1527–C1537.
- 94 R. R. Deshpande, C. Wittmann and E. Heinzle, *Cytotechnology*, 2004, **46**, 1–8.
- 95 S. M. Browne, H. Daud, W. G. Murphy and M. Al-Rubeai, *J. Biotechnol.*, 2014, **187**, 135–138.
- 96 W. Wang, L. Upshaw, D. M. Strong, R. P. Robertson and J. Reems, *J. Endocrinol.*, 2005, **185**, 445–455.
- 97 M. Naciri, D. Kuystermans and M. Al-Rubeai, *Cytotechnology*, 2008, **57**, 245–250.
- 98 S. Lee, B. L. Ibey, G. L. Coté and M. V. Pishko, *Sens. Actuators, B*, 2008, **128**, 388–398.
- 99 C. Boero, S. Carrara, G. Del Vecchio, L. Calzà and G. De Micheli, *IEEE Trans. Nanobiosci.*, 2011, **10**, 59–67.
- 100 J. Olivo, L. Foglia, M. A. Casulli, C. Boero, S. Carrara and G. De Micheli, *IEEE Trans. Biomed. Circuits Syst.*, 2014, 400–403.
- 101 C. Boero, J. Olivo, S. Carrara and G. De Micheli, *IEEE J. Emerg. Sel. Topic Circuits Syst.*, 2012, **2**, 658–671.
- 102 C. Boero, M. A. Casulli, J. Olivo, L. Foglia, E. Orso, M. Mazza, S. Carrara and G. De Micheli, *Biosens. Bioelectron.*, 2014, **61**, 251–259.
- 103 R. M. Pemberton, J. Xu, R. Pittson, N. Biddle, G. A. Drago, S. K. Jackson and J. P. Hart, *Anal. Biochem.*, 2009, **385**, 334–341.
- 104 R. M. Pemberton, J. Xu, R. Pittson, G. A. Drago, J. Griffiths, S. K. Jackson and J. P. Hart, *Biosens. Bioelectron.*, 2011, **26**, 2448–2453.
- 105 R. M. Pemberton, T. Cox, R. Tuffin, G. A. Drago, J. Griffiths, R. Pittson, G. Johnson, J. Xu, I. C. Sage, R. Davies, S. K. Jackson, G. Kenna, R. Luxton and J. P. Hart, *Sensors*, 2014, **14**, 20519–20532.
- 106 S. Mross, T. Zimmermann, N. Winkin, M. Kraft and H. Vogt, *Sens. Actuators, B*, 2016, **236**, 937–946.



- 107 E. O. Pettersen, P. Ebbesen, R. G. Gieling, K. J. Williams, L. Dubois, P. Lambin, C. Ward, J. Meehan, I. H. Kunkler, S. P. Langdon, A. H. Ree, K. Flatmark, H. Lyng, M. J. Calzada, L. Del Peso, M. O. Landazuri, A. Görlach, H. Flamm, J. Kieninger, G. Urban, A. Weltin, D. C. Singleton, S. Haider, F. M. Buffa, A. L. Harris, A. Scozzafava, C. T. Supuran, I. Moser, G. Jobst, M. Busk, K. Toustrup, J. Overgaard, J. Alsner, J. Pouyssegur, J. Chiche, N. Mazure, I. Marchiq, S. Parks, A. Ahmed, M. Ashcroft, S. Pastorekova, Y. Cao, K. M. Rouschop, B. G. Wouters, M. Koritzinsky, H. Mujcic and D. Cojocari, *J. Enzyme Inhib. Med. Chem.*, 2015, **30**, 689–721.
- 108 F. Hafner, *Biosens. Bioelectron.*, 2000, **15**, 149–158.
- 109 S. E. Eklund, D. E. Cliffl, E. Kozlov, A. Prokop, J. Wikswo and F. Baudenbacher, *Anal. Chim. Acta*, 2003, **496**, 93–101.
- 110 S. E. Eklund, D. Taylor, E. Kozlov, A. Prokop and D. E. Cliffl, *Anal. Chem.*, 2004, **76**, 519–527.
- 111 J. R. McKenzie, A. M. Palubinsky, J. E. Brown, B. McLaughlin and D. E. Cliffl, *ACS Chem. Neurosci.*, 2012, **3**, 510–518.
- 112 N. Hu, C. Wu, D. Ha, T. Wang, Q. Liu and P. Wang, *Biosens. Bioelectron.*, 2013, **40**, 167–173.
- 113 M. Lehmann, W. Baumann, M. Brischwein, R. Ehret, M. Kraus, A. Schwinde, M. Bitzenhofer, I. Freund and B. Wolf, *Biosens. Bioelectron.*, 2000, **15**, 117–124.
- 114 M. Brischwein, E. R. Motrescu, E. Cabala, A. M. Otto, H. Grothe and B. Wolf, *Lab Chip*, 2003, **3**, 234–240.
- 115 P. Mestres and A. Morguet, *Expert Opin. Drug Discovery*, 2009, **4**, 785–797.
- 116 H. Alborzinia, S. Can, P. Holenya, C. Scholl, E. Lederer, I. Kitanovic and S. Wölfl, *PLoS One*, 2011, **6**, e19714.
- 117 A. Weltin, J. Kieninger, G. Urban, I. Moser, G. Jobst, M. Wego and R. Ehret, *Proc. IEEE Sens.*, 2010, 2113–2116.
- 118 I. A. Ges and F. Baudenbacher, *Biosens. Bioelectron.*, 2010, **25**, 1019–1024.
- 119 I. A. Ges and F. Baudenbacher, *Biosens. Bioelectron.*, 2010, **26**, 828–833.
- 120 J. R. McKenzie, A. Cognata, A. N. Davis, J. P. Wikswo and D. E. Cliffl, *Anal. Chem.*, 2015, **87**, 7857–7864.
- 121 P. Wolf, M. Brischwein, R. Kleinhans, F. Demmel, T. Schwarzenberger, C. Pfister and B. Wolf, *Biosens. Bioelectron.*, 2013, **50**, 111–117.
- 122 J. Wiest, A. Namias, C. Pfister, P. Wolf, F. Demmel and M. Brischwein, *IEEE Trans. Biomed. Eng.*, 2016, **63**, 2368–2375.
- 123 M. H. Wu, S. B. Huang, Z. Cui, Z. Cui and G. B. Lee, *Sens. Actuators, B*, 2008, **129**, 231–240.
- 124 Y. Chen, D. Gao, H. Liu, S. Lin and Y. Jiang, *Anal. Chim. Acta*, 2015, **898**, 85–92.
- 125 C. Kim, J. H. Bang, Y. E. Kim, S. H. Lee and J. Y. Kang, *Lab Chip*, 2012, **12**, 4135–4142.
- 126 J. Ruppen, F. D. Wildhaber, C. Strub, S. Hall, T. Geiser, R. A. Schmid and O. T. Guenat, *Lab Chip*, 2015, **15**, 3076–3085.
- 127 E. J. Vrij, S. Espinoza, M. Heilig, A. Kolew, M. Schneider, C. A. van Blitterswijk, R. K. Truckenmüller and N. C. Rivron, *Lab Chip*, 2016, **16**, 734–742.
- 128 A. Mazzeo, E. Hong, D. E. Ingber and R. Derda, *Anal. Chem.*, 2013, **85**, 8085–8094.
- 129 K. A. Simon, B. Mosadegh, K. T. Minn, M. R. Lockett, M. R. Mohammady, D. M. Boucher, A. B. Hall, S. M. Hillier, T. Udagawa, B. K. Eustace and G. M. Whitesides, *Biomaterials*, 2016, **95**, 47–59.
- 130 K. Kwapiszewska, A. Michalczyk, M. Rybka, R. Kwapiszewski and Z. Brzózka, *Lab Chip*, 2014, **14**, 2096–2104.
- 131 S. Hammer, A. Weltin, Y. Kaminski, F. Noor, J. Kieninger and G. A. Urban, *Procedia Eng.*, 2015, **120**, 961–964.
- 132 A. Weltin, J. Kieninger, B. Enderle, A.-K. Gellner, B. Fritsch and G. A. Urban, *Biosens. Bioelectron.*, 2014, **61**, 192–199.
- 133 D. Bavli, S. Prill, E. Ezra, G. Levy, M. Cohen, M. Vinken, J. Vanfleteren, M. Jaeger and Y. Nahmias, *Proc. Natl. Acad. Sci. U. S. A.*, 2016, **113**, E2231–E2240.
- 134 S. Prill, M. S. Jaeger and C. Duschl, *Biomeicrofluidics*, 2014, **8**, 34102.
- 135 Y. S. Zhang, J. Aleman, S. R. Shin, T. Kilic, D. Kim, S. A. Mousavi Shaegh, S. Massa, R. Riahi, S. Chae, N. Hu, H. Avci, W. Zhang, A. Silvestri, A. Sanati Nezhad, A. Manbohi, F. De Ferrari, A. Polini, G. Calzone, N. Shaikh, P. Alerasool, E. Budina, J. Kang, N. Bhise, J. Ribas, A. Pourmand, A. Skardal, T. Shupe, C. E. Bishop, M. R. Dokmeci, A. Atala and A. Khademhosseini, *Proc. Natl. Acad. Sci. U. S. A.*, 2017, **114**, E2293–E2302.
- 136 S. A. M. Shaegh, F. De Ferrari, Y. S. Zhang, M. Nabavinia, N. B. Mohammad, J. Ryan, A. Pourmand, E. Laukaitis, R. B. Sadeghian, A. Nadjman, S. R. Shin, A. S. Nezhad, A. Khademhosseini and M. R. Dokmeci, *Biomeicrofluidics*, 2016, **10**, 44111.
- 137 R. Riahi, S. A. M. Shaegh, M. Ghaderi, Y. S. Zhang, S. R. Shin, J. Aleman, S. Massa, D. Kim, M. R. Dokmeci and A. Khademhosseini, *Sci. Rep.*, 2016, **6**, 24598.
- 138 J.-Y. Kim, D. A. Fluri, J. M. Kelm, A. Hierlemann and O. Frey, *J. Lab. Autom.*, 2015, **20**, 274–282.
- 139 T. E. de Groot, K. S. Vesperat, E. Berthier, D. J. Beebe and A. B. Theberge, *Lab Chip*, 2016, **16**, 334–344.
- 140 Y. R. F. Schmid, S. C. Bürgel, P. M. Misun, A. Hierlemann and O. Frey, *ACS Sens.*, 2016, **1**, 1028–1035.
- 141 C. Luni, E. Serena and N. Elvassore, *Curr. Opin. Biotechnol.*, 2014, **25**, 45–50.
- 142 C. Zhang, Z. Zhao, N. A. Abdul Rahim, D. van Noort and H. Yu, *Lab Chip*, 2009, **9**, 3185–3192.
- 143 K. Aravindalochanan, J. Kieninger, J. A. Sandvik, E. O. Pettersen and G. A. Urban, in *TRANSDUCERS 2009 - 15th International Conference on Solid-State Sensors, Actuators and Microsystems*, 2009, pp. 1003–1006.
- 144 K. Domansky, W. Inman, J. Serdy, A. Dash, M. H. M. Lim and L. G. Griffith, *Lab Chip*, 2010, **10**, 51–58.

