



Cite this: *Lab Chip*, 2018, 18, 3840

## Correlative light and electron microscopy for complex cellular structures on PDMS substrates with coded micro-patterns†

Rong Sun,<sup>ab</sup> Xi Chen,<sup>\*c</sup> Chun-Ying Yin,<sup>ab</sup> Lei Qi,<sup>b</sup> Pak-Ming Lau,<sup>b</sup> Hua Han<sup>c</sup> and Guo-Qiang Bi<sup>id \*abd</sup>

Fluorescence light microscopy (FLM) is commonly used for localizing specific cellular and subcellular targets. Electron microscopy (EM), on the other hand, can reveal ultrastructural details of cellular architectures beyond the limit of optical resolution. Correlative light and electron microscopy (CLEM) that combines the two techniques has proven valuable in various cell biological applications that require both specificity and resolution. Here, we report an efficient and easy-to-use CLEM system, and its applications in studying neuronal synapses. The system utilizes patterned symbols to encode coordinates on micro-fabricated polydimethylsiloxane (PDMS) substrates, on which dissociated primary hippocampal neurons grow and form synaptic connections. After imaging and localizing specifically labeled synapses with FLM, samples are embedded in resin blocks and sectioned for EM analysis. The patterned symbols on PDMS substrates provide coordinate information, allowing efficient co-registration between FLM and EM images with high precision. A custom-developed software package achieves automated EM image collection, FLM/EM alignment, and EM navigation. With this CLEM system, we have obtained high quality electron tomograms of fluorescently labeled synapses along dendrites of hippocampal neurons and analyzed docking statistics of synaptic vesicles (SVs) in different subtypes of excitatory synapses. This technique provides an efficient approach to combine functional studies with ultrastructural analysis of heterogeneous neuronal synapses, as well as other subcellular structures in general.

Received 6th July 2018,  
Accepted 18th October 2018

DOI: 10.1039/c8lc00703a

rscl/loc

### 1. Introduction

Electron microscopy (EM), especially electron tomography (ET), resolves 3D details of cellular architectures at nanometer resolution.<sup>1–4</sup> Although immuno-EM has been used to label certain proteins in biological samples with high resolution, it still suffers from relatively low labeling density and poor ultrastructure preservation.<sup>5,6</sup> On the other hand, the use of light microscopy (LM) to image fluorescently labeled molecules has revealed significant information regarding the organization and function of subcellular structures.<sup>7–9</sup> However, direct observation of ultrastructures is still limited by the res-

olution of light microscopy. To combine the advantages of LM and EM techniques, correlative light and electron microscopy (CLEM) has been developed.<sup>10–12</sup> As CLEM is a combination of two imaging modalities, a series of correlative methods have been developed based on varieties of LM and EM techniques, respectively,<sup>13–16</sup> and also based on different probes to correlate LM and EM images.<sup>17–19</sup> By such correlative methods, specific cellular features or components localized by fluorescence light microscopy (FLM) can then be examined by EM to achieve high resolution details in the same biological sample.

For complex cellular structures, however, such as processes and synapses of neuronal cells which form extensive networks in culture, it remains a challenge to efficiently and accurately target fluorescence in certain areas in EM with existing CLEM methods. Although commercial photoetched glass gridded coverslips for FLM/EM correlation have been applied in mammalian cell lines or yeast cells,<sup>20,21</sup> this kind of method would have low efficiency for long stretching neuropils and tiny synapses in cultured neurons inside each square of the coverslip. Custom micro-patterning substrates were reported to be adopted for correlative confocal microscopy and scanning electron microscopy (SEM) in the cultured

<sup>a</sup> Center for Integrative Imaging, National Laboratory for Physical Sciences at the Microscale, University of Science and Technology of China, Hefei, China

<sup>b</sup> CAS Key Laboratory of Brain Function and Disease, and School of Life Sciences, University of Science and Technology of China, No. 443 Huangshan Road, 230027, Hefei, Anhui, China. E-mail: gqbi@ustc.edu.cn

<sup>c</sup> Institute of Automation, Chinese Academy of Sciences, No. 95 Zhongguancun East Road, 100190, Beijing, China. E-mail: xi.chen@ia.ac.cn

<sup>d</sup> CAS Center for Excellence in Brain Science and Intelligence Technology, University of Science and Technology of China, Hefei, China

† Electronic supplementary information (ESI) available. See DOI: 10.1039/c8lc00703a



neuronal system.<sup>22</sup> However, the patterns themselves do not encode the coordinates, while the laser-cut alphabets on the substrates do. In addition, SEM could only provide surface information of samples. Another limitation of current CLEM methods concerns available software. Although several software solutions to CLEM workflows have been developed,<sup>19,23,24</sup> a software package that includes all aspects of the CLEM procedure in EM is still requisite.

To overcome these limitations, we developed a system of correlative light and electron microscopy. Our CLEM system is based on custom-designed coded micro-patterning PDMS substrates, on which dissociated primary hippocampal neurons grow and form synaptic connections. A CLEM software package has also been developed to achieve automated EM image collection, FLM/EM alignment, and EM navigation. With this CLEM system, including both hardware and software, we have obtained high quality electron tomograms of excitatory synapses along dendrites of hippocampal neurons and analyzed docking statistics of synaptic vesicles (SVs) in different subtypes of excitatory synapses.

## 2. Materials and methods


All animal experiments were approved and conducted according to protocols approved by the Animal Experiments Committee at the University of Science and Technology of China. All animal procedures were performed following the

guidelines of the Animal Experiment Committee at the University of Science and Technology of China. Low density cultures of dissociated embryonic rat hippocampal neurons were prepared according to a previously described protocol<sup>26</sup> with few modifications.

### 2.1. PDMS substrate fabrication and coded micro-patterning design


The patterned PDMS substrate was fabricated by conventional soft lithography according to a previously described protocol<sup>25</sup> with some modifications (Fig. 1a). SU-8 3005 photoresist (MicroChem) was spin-coated on a cleaned Si wafer. The coated wafer was baked on a hot plate at a temperature of 95 °C for 2 min. The SU-8 3005 photoresist was exposed to UV light under a photomask containing designed patterns. After UV exposure, the coated wafer was again baked on a hot plate at a temperature of 95 °C for 2 min. The exposed SU-8 photoresist was developed by a SU-8 developer, and the SU-8 mold on the Si wafer was completed. The mixture of the PDMS pre-polymer and curing agent (10:1 (w/w), Dow Corning Corp.) was poured on the SU-8 mold and cured on a hot plate at 80 °C for 40 min. After curing, the patterned PDMS was removed from the SU-8 mold.

The entire photomask consisted of 24 repeated elements (Fig. S1†). Each element represented one piece of PDMS substrate used for neuron culture, which is shown in Fig. 2a.

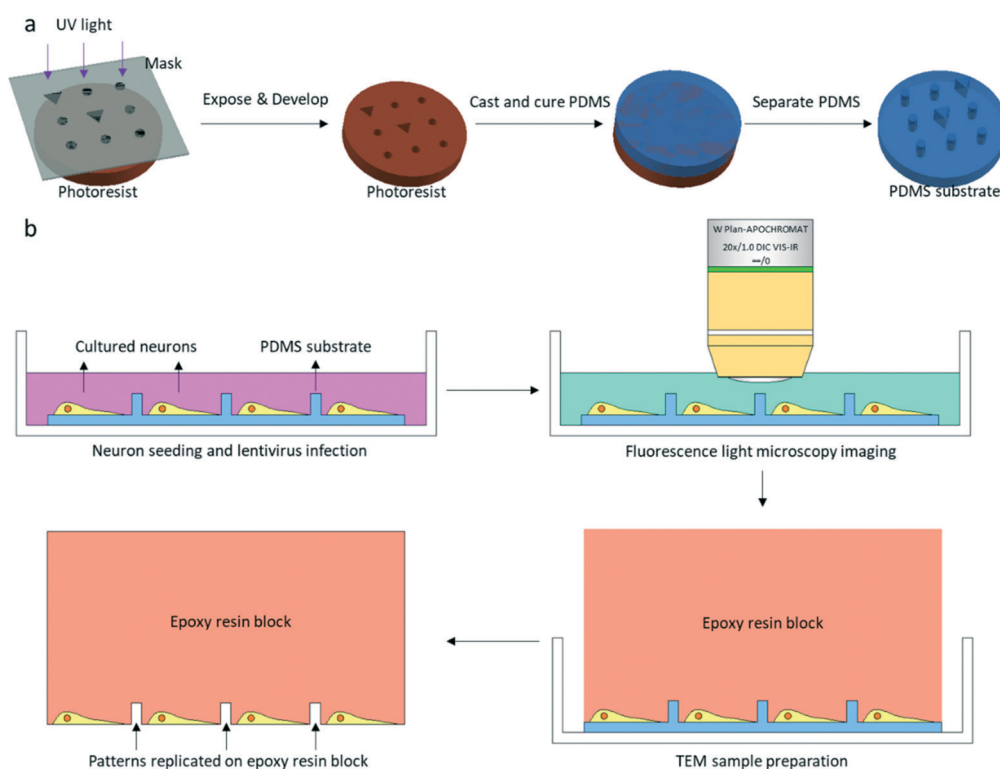

**Fig. 1** Schematic of PDMS substrate fabrication, fluorescence light microscopy imaging, and transmission electron microscopy (TEM) sample preparation. (a) The conventional soft lithography method is used for PDMS substrate fabrication, and the patterns are custom-designed for FLM and EM correlation. (b) FLM imaging and TEM sample preparation. After FLM imaging, the TEM sample is prepared in the dish. Patterns designed on PDMS are replicated on the epoxy resin block.



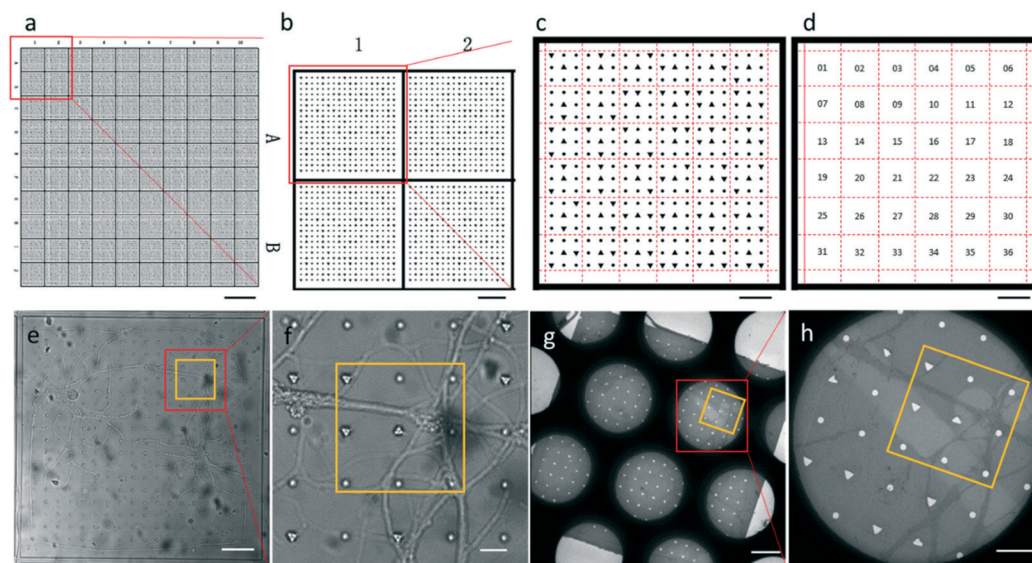

**Fig. 2** Patterned PDMS design and EM section with replicated patterns. (a–d) Design for the micro-fabricated PDMS substrate with a two-tier hierarchical coordinate system. (a and b) The square coordinates are defined by letters and digits along the sides of the PDMS substrate. (c and d) Each square is divided into 36 sets whose coordinates are encoded by  $3 \times 3$  geometrical symbols. (c) Shows geometrical symbols inside square A1, which is boxed in (b). (e–h) The PDMS substrate and EM section of a square. Set 11 is yellow-boxed. Dark circles in (g) and (h) are holes of the EM grid where the section was deposited. Scale bars: (a) 500  $\mu\text{m}$ , (b) 100  $\mu\text{m}$ , (c–e and g) 50  $\mu\text{m}$ , (f) 10  $\mu\text{m}$ , and (h) 20  $\mu\text{m}$ .

The PDMS substrate comprises a two-tier hierarchical coordinate system. The first-tier hierarchical coordinates were letters and digits along the left and top side of the substrate. These letters and digits encoded the coordinates of the squares (Fig. 2a and b). In this way, the patterned PDMS substrate constituted  $10 \times 10$  identical squares from A1 to J10. The secondary-tier hierarchical coordinates were patterned geometrical symbols, including circles and triangles, within each square. A square was divided into 36 symbol sets, each of which consisted of  $3 \times 3$  symbols (Fig. 2c and d). The set coordinate was defined according to the combination of symbols inside the symbol set: a triangle occupied the center site of the  $3 \times 3$  set of geometrical symbols. And the remaining eight sites were one reversed triangle and seven circles, or two reversed triangles and six circles. Thus, there were exactly  $\binom{8}{1} + \binom{8}{2}$  different sets from set 1 to set 36. These pattern-coded coordinates would allow rapid addressing in both the LM image and EM image (Fig. 2e–h), and further led to efficient LM/EM correlation.

## 2.2. Primary culture of hippocampal neurons and lentivirus infection

Low density cultures of dissociated embryonic rat hippocampal neurons were prepared according to a previously described protocol<sup>26</sup> with few modifications. Patterned PDMS substrates for cell culture were glow-discharged with  $\text{H}_2$  and  $\text{O}_2$  for 1 min by a Gatan plasma cleaning machine (Gatan, Inc.), and sterilized with UV light for 30 min. These PDMS substrates were coated with  $1 \text{ mg ml}^{-1}$  poly-L-lysine (Sigma) in sodium borate buffer for approximately 24 h, followed by washing with ddH<sub>2</sub>O for approximately another 24 h. Hippo-

campi were removed from embryonic day-18 (E18) rats and were treated with trypsin for 15 min at 37  $^\circ\text{C}$ , followed by washing and gentle trituration. The dissociated cells were plated on poly-L-lysine coated patterned PDMS substrates attached on the bottom of 35 mm Petri dishes with a density of 40 000–60 000 cells per ml.

The PSD95-EGFP construct was produced based on GW-PSD95-EGFP (a generous gift from Dr. Weidong Yao) and plentivirus-CaMKIIp-mKate2. Plasmids were packaged into lentivirus following a protocol from the laboratory of Dr. Karl Deisseroth.<sup>27</sup> For fluorescence light microscopy imaging, cultures were infected by lentivirus encoding PSD95-EGFP for 5–7 d *in vitro* (DIV). Twelve hours after the infection, half of the culture medium was replaced by fresh medium as previously described.<sup>28</sup>


## 2.3. Fluorescence light microscopy imaging

Cultures were used for FLM imaging at 16–18DIV. LM Imaging was performed with a 20 $\times$  water objective lens in a Zeiss 710 microscope (Fig. 1b). After replacing the culture medium with extracellular solution (ECS, containing 150 mM NaCl, 3 mM KCl, 3 mM CaCl<sub>2</sub>·2H<sub>2</sub>O, 10 mM HEPES and 5 mM glucose, pH 7.3), the dish was placed in the microscope. One bright field image and z-stack fluorescence images of the neurons were collected for one square of the PDMS substrate. The fluorescence image used for CLEM would be a z-projection image of the z-stack images. The cultured neurons were immediately fixed with 4% paraformaldehyde (PFA, SPI supplies) and 2.5% glutaraldehyde (GA, Alfa Aesar) in 0.1 M cacodylate buffer/HCl (Ted Pella) after fluorescence light microscopy imaging.







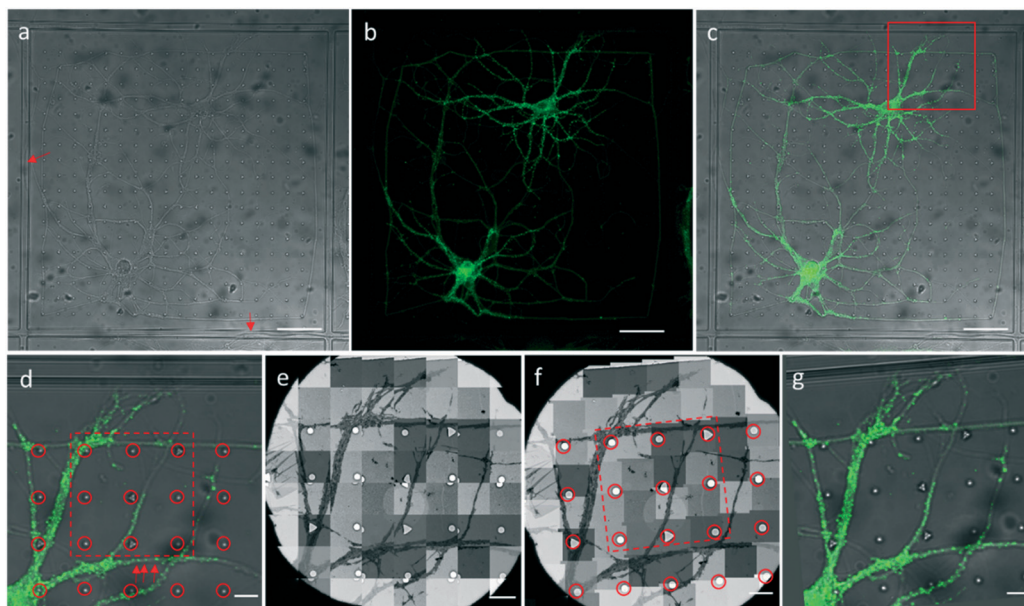

**Fig. 3** An example of optical imaging of cultured hippocampal neurons on the PDMS substrate and the CLEM procedure. (a–c) Bright field (a), fluorescence (b), and overlaid (c) images of cultured neurons expressing PSD95-EGFP on the PDMS substrate. Arrows indicate neurospits growing over the square bars. (d) Zoomed-in view of the boxed area in (c). Arrows indicate PSD95-EGFP puncta along the dendrite. (e) Sequential EM images taken by the CLEM software. Overlap between images is preset for montaging. (f) Montaged image of the sequential EM images. (g) Warped LM image to correlate the EM image (f) by the circled patterns in the EM (f) and LM (d) images. Scale bars: (a–c) 50  $\mu\text{m}$ , (d–g) 10  $\mu\text{m}$ .

appear as if they were trapped by the PDMS bars between squares. Meanwhile, some neurospits could grow over the square bars (arrows in Fig. 3a), indicating that neurons in different squares might form connections. These neurons labeled by PSD95-EGFP showed green fluorescent puncta at the processes, indicative of excitatory synapses (arrows in Fig. 3d). Moreover, the bright field image was taken to reveal the PDMS patterns by which we could perform the correlation procedure with EM images.

After FLM imaging, we prepared samples following the conventional TEM sample preparation protocols as described in Methods. After peeling off the PDMS from the resin block, the patterns were transferred onto the resin block along with the neurons. We cut samples into 200 nm sections, and loaded them into the electron microscope. Then, 3500 $\times$  EM images with overlap (Fig. 3e) were acquired to cover a hole of the 150 mesh EM grid automatically. We generated the navigation map (Fig. 3f) by montaging the acquired images using the CLEM software. The montaged navigation map offered a larger field of view with acceptable resolution compared with just one low magnification image, and provided adequate localization information to establish the correlation between the EM image and the LM image. Therefore, both neurospits and designed patterns could be clearly observed in the montaged navigation map. And the boxed area (set 30) in Fig. 3f would allow quick registration of the same set of symbols in the LM image (Fig. 3d). We correlated the montaged EM image and the LM image by selecting the corresponding symbols (circles in Fig. 3d and f). By aligning selected symbols, the light image was warped to the EM image (Fig. 3g) using non-linear transformation thin plate splines.<sup>30</sup> The accuracy

of the correlation could be improved with more corresponding points involved.


### 3.2. Electron tomography of identified excitatory synapses through CLEM

Through the CLEM procedure, we acquired the electron tomograms of excitatory synapses identified by PSD95-EGFP labeling. When we selected the PSD95-EGFP punctum (box 1 in Fig. 4e) in the optical image in the software, the EM stage moved to the actual position of the synapse in the EM section. In order to show the localization of the synapse clearly, it is also boxed in the contrast-adjusted image (Fig. 4c) of the navigation map and overlaid image (Fig. 4f) of the FLM/EM image.

After moving the EM stage to the selected synapse, we took a single projection image and a tilt-series. The single projection image at high magnification shows the typical ultrastructure of an excitatory synapse (Fig. 4g1). There was a population of SVs in the presynaptic compartment. The synaptic cleft, which was covered by an electron-dense area, was difficult to observe in the single projection image in this 200 nm section. In the 3D tomogram reconstructed based on the tilt series collected for the synapse (Fig. 4g2), individual SVs were distinguishable. Electron-dense areas in both presynaptic and postsynaptic compartments were recognized as the active zone (AZ) and postsynaptic density (PSD), respectively. A relatively uniform synaptic cleft appeared between the pre- and postsynaptic membrane. These results demonstrate that the high resolution electron tomograms of the excitatory synapses enable us to conduct quantitative analysis of the synaptic ultrastructure.





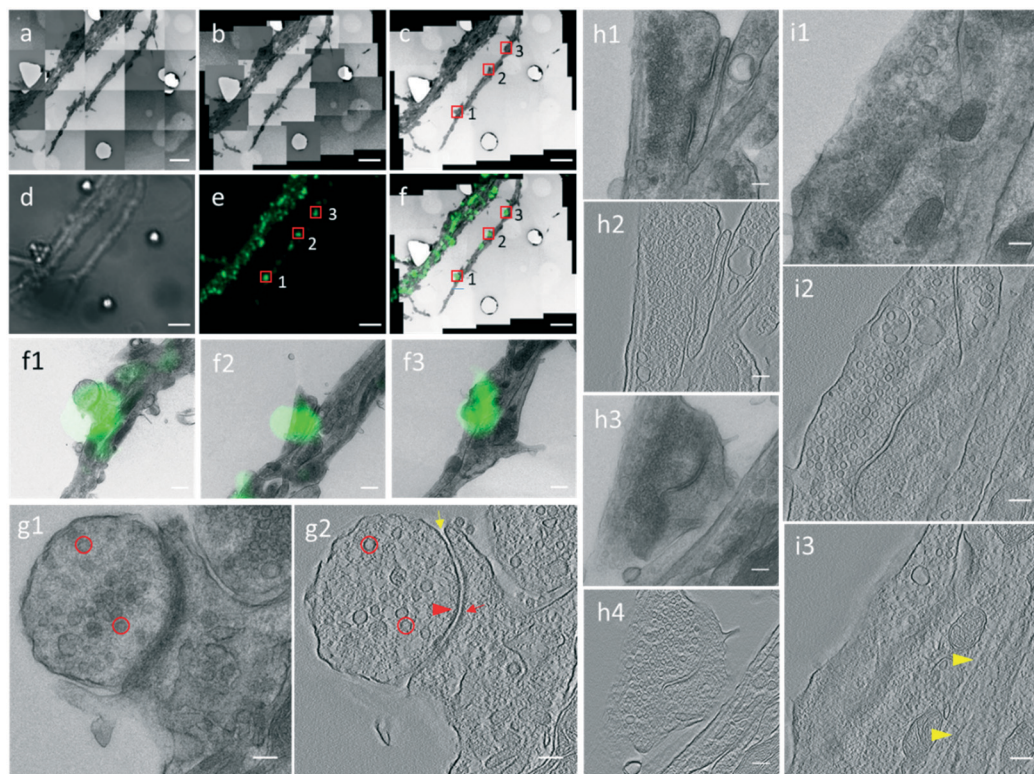

**Fig. 4** Electron tomogram of identified excitatory spine and shaft synapses. (a–c) Raw (a), montaged (b), and contrast-adjusted (c) images of sequential EM images. (d and e) Bright field (d) and fluorescence (e) images of the same view field with the EM image. (f) EM and LM images are correlated and merged by aligning designed PDMS patterns. (f1–f3) Zoomed-in views of boxed synapses in (f) from area 1–3. (g1 and g2) A single projection image and a tomographic slice of the same synapse boxed in area 1 in (c), (e), and (f). (h1–h4) Single projection images and tomographic slices on two serial EM sections showing the same spine synapse boxed in area 2 in (c), (e), and (f). (i1–i3) A single projection image and two tomographic slices showing the same shaft synapse boxed in area 3 in (c), (e), and (f). Red circle, SV; red arrowhead, AZ; red arrow, PSD; yellow arrow, synaptic cleft; yellow arrowhead, microtubule. Scale bars: (a–f) 5  $\mu\text{m}$ , (f1–f3) 100  $\mu\text{m}$ , (g1–i3) 100 nm.

By this CLEM routine, we generated a data set containing 42 electron tomographic reconstructions of excitatory synapses. Among these synapses, in most cases, whether it was a spine or shaft synapse could be determined in a single projection image of one EM section. For example, the synapse in Fig. 4g1 was a typical spine synapse and the synapse in Fig. S4† was a typical shaft synapse as the synapse formed directly on the dendritic shaft, with microtubules readily visible in the postsynaptic compartment.

However, in some cases, a spine or shaft synapse was difficult to distinguish in the single projection image because the postsynaptic compartment was too dense to observe microtubules or the postsynaptic compartment was cut too small in a single EM ultrathin section. By our CLEM system, two excitatory synapses were detected in the same dendrite in the PSD95-EGFP labeled cultured neurons (boxes 2 and 3 in Fig. 4e), and whether they were spine or shaft synapses was determined by information in multiple serial EM sections or by information in multiple tomographic slices of the 3D tomograms. For the synapse boxed in area 2 in Fig. 4e, the single projection image (Fig. 4h1) or the tomogram (Fig. 4h2) in one EM section only reveals a very small postsynaptic compartment, from which it is unable to determine whether or not it is a spine. We then performed the CLEM procedure on

the neighboring EM section and localized the same synapse indicated by the same fluorescent punctum (Fig. S5†). Next, a high resolution single projection image and an electron tomogram of the synapse were acquired, which clearly contained a dendritic spine without microtubules as the postsynaptic compartment (Fig. 4h3 and h4). Thus, according to the synaptic structure in the two serial sections, we verified the presence of a spine synapse. Regarding the synapse boxed in area 3 in Fig. 4e, although microtubules were not visible in the single projection image (Fig. 4i1), the 3D reconstructed tomogram presented a typical presynaptic ultrastructure, including SVs and a synaptic cleft in one tomographic slice (Fig. 4i2), and microtubules along the postsynaptic dendrite in another tomographic slice (Fig. 4i3), showing that it was a shaft synapse. According to the above described process, the 42 excitatory synapses were subdivided into 27 spine synapses and 15 shaft synapses.

### 3.3. Quantitative analysis of docked SVs in identified excitatory spine and shaft synapses

High resolution electron tomograms allowed us to detect SV docking (Fig. 5), a preceding step of SV fusion upon  $\text{Ca}^{2+}$  stimulation.<sup>31</sup> SVs that were in direct physical contact with




the presynaptic membrane in the AZ were considered to be docked (Fig. 5e). In contrast, some SVs appeared linked to the presynaptic membrane by short filaments, and these SVs were termed tethered SVs (Fig. 5f). In our analysis, these tethered SVs were not considered docked. Fused SVs (Fig. 5g) were excluded from the analysis, as well.

With structural differences between spine and shaft synapses in their postsynaptic compartments, the number of docked SVs might also differ in these two subtypes of synapses. Thus, we analyzed the number of docked vesicles in 27 excitatory spine synapses and 15 excitatory shaft synapses obtained by our CLEM system (Fig. 5h). We noted that every

synapse analyzed here was just a part of the intact synapse. More docked SVs were found in excitatory spine synapses ( $5.3 \pm 0.7$  (Mean  $\pm$  SEM),  $n = 27$  in excitatory spine synapses and  $3.3 \pm 0.7$  (Mean  $\pm$  SEM),  $n = 15$  in excitatory shaft synapses;  $p < 0.05$ , two-sample  $t$ -test). This ultrastructural difference implies different sizes of the readily releasable pool between excitatory spine and shaft synapses.

### 3.4. Discussion

CLEM methods are applied as a powerful tool to connect ultrastructure information and functional study in cell biology.

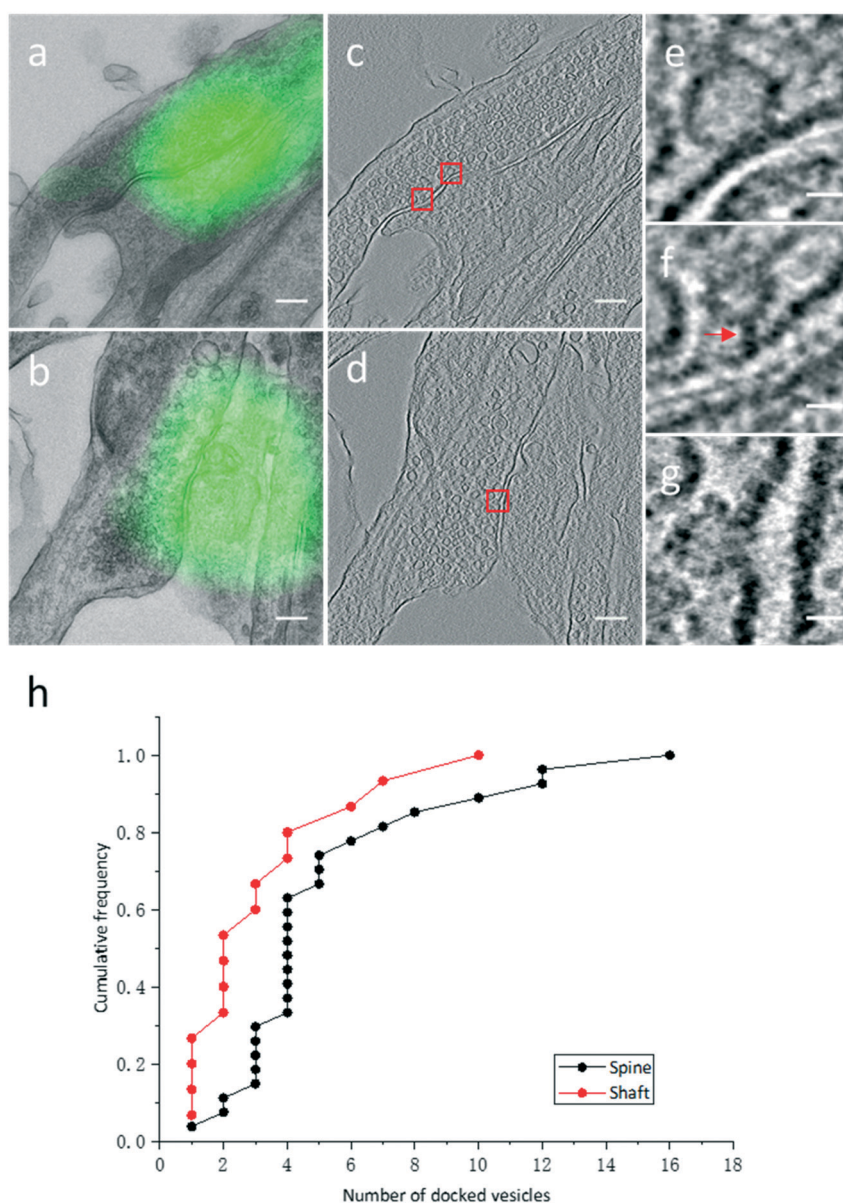

**Fig. 5** Quantitative analysis of docked vesicles in excitatory spine and shaft synapses. (a and b) Single projection images of two excitatory synapses co-localized with PSD95-EGFP puncta. (c) A tomographic slice showing the same synapse in (a). (d) A tomographic slice showing the same synapse in (b). (e–g) Vesicles fixed at multiple stages of exocytosis boxed in (c) and (d). (e) Vesicle directly in contact with the AZ. (f) Vesicle tethered to the AZ membrane by filaments (arrow). (g) Vesicle fused to the AZ membrane. (h) Cumulative frequency of the number of docked vesicles in excitatory spine and shaft synapses. Scale bars: (a–d) 200 nm, (e–g) 20 nm.





Combining multiple forms of LM and EM methods, a series of hybrid correlative approaches show great potential in neuroscience study.<sup>12,32</sup> However, some limitations to resolve the ultrastructure of crowded synapses still remain. For example, the CLEM method, by preserving fluorescence in the resin-embedded sample, which often requires reduced or no osmium tetroxide during sample preparation, leads to poor ultrastructure in EM.<sup>33,34</sup> The CLEM method using anatomical landmarks, such as vessels or cell bodies,<sup>35</sup> which are randomly distributed, is incapable of providing efficient and accurate correlative probes for the neuronal culture system.

In this article, we describe an automated CLEM system based on the micro-patterning coded PDMS and a custom-developed software package. With this hardware and software together, we utilize this CLEM system for the observation of excitatory synapses in cultured hippocampal neurons. PDMS is a suitable substrate for culturing mammalian cells, and possesses the characteristic of being able to be made into different shapes and sizes by the conventional soft lithography method.<sup>36–38</sup> Thus, this kind of PDMS substrate offers a series of advantages for CLEM in cultured neuronal networks. First, cultured neurons grow very well on PDMS substrates after proper treatment. Second, compared to the laser-etched gridded glass coverslip, PDMS is inexpensive, can be rapidly produced, and is very easy to separate from the EM resin block without other operations. Third, our micro-patterning PDMS substrate is coded by a two-tier hierarchical coordinate system, which provides high resolution information for the LM/EM correlation.

The CLEM software constitutes another major advantage of our system. The reported software solutions covered only parts of the CLEM procedure, while our software package offers a high integration level, including the functions of automatic scanning, navigation and LM/EM correlation, which greatly improves the efficiency of CLEM experiments. The image capture program was developed using AutoIt,<sup>39</sup> a BASIC-like scripting language which can simulate keystrokes and mouse movement. This means that the acquiring software is not restricted by the API from electron microscope manufacturers and can be adopted by other microscopes easily, because it just fills in input boxes and clicks buttons in the control software of the electron microscope. We also provide the source code of the image capture program with the CLEM software so that the other laboratories could adjust the code to accord with their EM control GUI easily.

Using the CLEM system, we have successfully obtained a batch of identified excitatory synaptic tomograms. Although the majority of excitatory synapses are spine synapses, excitatory terminals make synaptic contacts on dendritic shafts.<sup>6,40,41</sup> The hypothesis that shaft synapses represent immature excitatory synapses and eventually become spine synapses was proposed because of the downregulation of excitatory shaft synapses and the increase of excitatory spine synapses during development.<sup>40,42,43</sup> We analyze the number of docked SVs and find more docked SVs in excitatory spine synapses than those in excitatory shaft synapses. As the num-

ber of docked vesicles is changing during synaptic maturation,<sup>44</sup> our result may imply that the two subtypes of excitatory synapses are in different developmental stages. By our CLEM system, we use PSD95-EGFP labeled FLM to exclude inhibitory synapses and high resolution 3D tomograms to detect docked vesicles specifically, confirming the power of our CLEM method.

In conclusion, our CLEM system, which is highly integrative, efficient and easy-to-use, provides an overall solution for ultrastructural studies guided by fluorescence imaging in a cultured neuronal system and other culture cell systems.

## Author contributions

R. S., X. C., P.-M. L., H. H. and G.-Q. B. designed the research; R. S., C.-Y. Y. and L. Q. performed the experiments; X. C. developed the CLEM software; R. S. and X. C. analyzed the data; R. S., X. C., H. H. and G.-Q. B. wrote the paper.

## Conflicts of interest

There are no conflicts of interest to declare.

## Acknowledgements

This work was supported in part by grants from the National Key R&D Program of China (No. 2016YFA0400900), CAS (No. XDB02050000), and the National Natural Science Foundation of China (No. 31630030). We acknowledge the use of instruments at the Center for Integrative Imaging of the Hefei National Laboratory for Physical Sciences at the Microscale. We thank Chang-Lu Tao and Yun-Tao Liu for technical advice on imaging and data processing. We thank Fang Xu for assistance in setting up the soft lithography platform.

## References

- 1 W. Baumeister, *Curr. Opin. Struct. Biol.*, 2002, **12**, 679–684.
- 2 A. Hoenger and J. R. McIntosh, *Curr. Opin. Cell Biol.*, 2009, **21**, 89–96.
- 3 S. Watanabe, B. R. Rost, M. Camacho-Perez, M. W. Davis, B. Sohl-Kielczynski, C. Rosenmund and E. M. Jorgensen, *Nature*, 2013, **504**, 242–247.
- 4 C. Imig, S. W. Min, S. Krinner, M. Arancillo, C. Rosenmund, T. C. Sudhof, J. Rhee, N. Brose and B. H. Cooper, *Neuron*, 2014, **84**, 416–431.
- 5 M. Megias, Z. Emri, T. F. Freund and A. I. Gulyas, *Neuroscience*, 2001, **102**, 527–540.
- 6 K. M. Harris and R. J. Weinberg, *Cold Spring Harbor Perspect. Biol.*, 2012, **4**, 30.
- 7 B. N. G. Giepmans, S. R. Adams, M. H. Ellisman and R. Y. Tsien, *Science*, 2006, **312**, 217–224.
- 8 J. W. Lichtman and J. A. Conchello, *Nat. Methods*, 2005, **2**, 910–919.
- 9 D. J. Stephens and V. J. Allan, *Science*, 2003, **300**, 82–86.
- 10 J. Caplan, M. Niethammer, R. M. Taylor, 2nd and K. J. Czymmek, *Curr. Opin. Struct. Biol.*, 2011, **21**, 686–693.





- 11 D. S. Lidke and K. A. Lidke, *J. Cell Sci.*, 2012, **125**, 2571–2580.
- 12 I. Begemann and M. Galic, *Front. Synaptic Neurosci.*, 2016, **8**, 28.
- 13 W. Kukulski, M. Schorb, M. Kaksonen and J. A. G. Briggs, *Cell*, 2012, **150**, 508–520.
- 14 E. Johnson, E. Seiradake, E. Y. Jones, I. Davis, K. Grunewald and R. Kaufmann, *Sci. Rep.*, 2015, **5**, 9583.
- 15 V. Lucic, A. H. Kossel, T. Yang, T. Bonhoeffer, W. Baumeister and A. Sartori, *J. Struct. Biol.*, 2007, **160**, 146–156.
- 16 Y.-W. Chang, S. Chen, E. I. Tocheva, A. Treuner-Lange, S. Loebach, L. Sogaard-Andersen and G. J. Jensen, *Nat. Methods*, 2014, **11**, 737–739.
- 17 M. Grabenbauer, W. J. C. Geerts, J. Fernandez-Rodriguez, A. Hoenger, A. J. Koster and T. Nilsson, *Nat. Methods*, 2005, **2**, 857–862.
- 18 D. Bishop, I. Nikic, M. Brinkoetter, S. Knecht, S. Potz, M. Kerschensteiner and T. Misgeld, *Nat. Methods*, 2011, **8**, 568–570.
- 19 M. Schorb and J. A. G. Briggs, *Ultramicroscopy*, 2014, **143**, 24–32.
- 20 L. E. Reddick and N. M. Alto, *J. Visualized Exp.*, 2012, e3650.
- 21 H. Asakawa, Y. Hiraoka and T. Haraguchi, *Micron*, 2014, **61**, 53–61.
- 22 L. Benedetti, E. Sogne, S. Rodighiero, D. Marchesi, P. Milani and M. Francolini, *Sci. Rep.*, 2014, **4**, 7033.
- 23 P. Paul-Gilloteaux, X. Heiligenstein, M. Belle, M. C. Domart, B. Larijani, L. Collinson, G. Raposo and J. Salamero, *Nat. Methods*, 2017, **14**, 102–103.
- 24 W. Kukulski, M. Schorb, S. Welsch, A. Picco, M. Kaksonen and J. A. G. Briggs, *J. Cell Biol.*, 2011, **192**, 111–119.
- 25 Y. C. Li, R. Sun, B. Zhang, Y. C. Wang and H. Y. Li, *PLoS One*, 2015, **10**, 15.
- 26 G. Q. Bi and M. M. Poo, *J. Neurosci.*, 1998, **18**, 10464–10472.
- 27 F. Zhang, V. Gradinaru, A. R. Adamantidis, R. Durand, R. D. Airan, L. de Lecea and K. Deisseroth, *Nat. Protoc.*, 2010, **5**, 439–456.
- 28 C.-L. Tao, Y.-T. Liu, R. Sun, B. Zhang, L. Qi, S. Shivakoti, C.-L. Tian, P. Zhang, P.-M. Lau, Z. H. Zhou and G.-Q. Bi, *J. Neurosci.*, 2018, **38**, 1493–1510.
- 29 J. R. Kremer, D. N. Mastronarde and J. R. McIntosh, *J. Struct. Biol.*, 1996, **116**, 71–76.
- 30 F. L. Bookstein, *IEEE Trans. Pattern Anal. Mach. Intell.*, 1989, **11**, 567–585.
- 31 T. C. Südhof, *Neuron*, 2013, **80**, 675–690.
- 32 S. Wang, S. Li, G. Ji, X. Huang and F. Sun, *Biophys. Rep.*, 2017, **3**, 8–16.
- 33 O. Avinoam, M. Schorb, C. J. Beese, J. A. G. Briggs and M. Kaksonen, *Science*, 2015, **348**, 1369–1372.
- 34 S. Watanabe, J. Richards, G. Hollopeter, R. J. Hobson, W. M. Davis and E. M. Jorgensen, *J. Visualized Exp.*, 2013, e3995.
- 35 W. C. Lee, V. Bonin, M. Reed, B. J. Graham, G. Hood, K. Glattfelder and R. C. Reid, *Nature*, 2016, **532**, 370–374.
- 36 J. N. Lee, X. Jiang, D. Ryan and G. M. Whitesides, *Langmuir*, 2004, **20**, 11684–11691.
- 37 D. B. Weibel, W. R. DiLuzio and G. M. Whitesides, *Nat. Rev. Microbiol.*, 2007, **5**, 209–218.
- 38 A. Vishwanathan, G. Q. Bi and H. C. Zeringue, *Lab Chip*, 2011, **11**, 1081–1088.
- 39 A. Flesner, *AutoIt v3: Your Quick Guide*, O'Reilly Media, 2007.
- 40 J. C. Fiala, M. Feinberg, V. Popov and K. M. Harris, *J. Neurosci.*, 1998, **18**, 8900–8911.
- 41 J. C. Anderson and K. A. C. Martin, *J. Comp. Neurol.*, 2006, **495**, 709–721.
- 42 C. Boyer, T. Schikorski and C. F. Stevens, *J. Neurosci.*, 1998, **18**, 5294–5300.
- 43 I. M. Ethell and E. B. Pasquale, *Prog. Neurobiol.*, 2005, **75**, 161–205.
- 44 M. G. Mozhayeva, Y. Sara, X. R. Liu and E. T. Kavalali, *J. Neurosci.*, 2002, **22**, 654–665.

